



US 20160166135A1

(19) **United States**

(12) **Patent Application Publication**
Fiset

(10) **Pub. No.: US 2016/0166135 A1**

(43) **Pub. Date: Jun. 16, 2016**

(54) **CLEANING DEVICE FOR CLEANING A SCOPE, LAPAROSCOPE OR MICROSCOPE USED IN SURGERY OR OTHER MEDICAL PROCEDURES AND A METHOD OF USING THE DEVICE DURING SURGICAL OR OTHER MEDICAL PROCEDURES**

Publication Classification

(51) **Int. Cl.**
A61B 1/12 (2006.01)
A61B 17/34 (2006.01)
(52) **U.S. Cl.**
CPC *A61B 1/126* (2013.01); *A61B 1/127* (2013.01); *A61B 17/3417* (2013.01)

(71) Applicant: **Medix3d LLC**, Santa Monica, CA (US)

(72) Inventor: **Claude Fiset**, Ojai, CA (US)

(21) Appl. No.: **14/966,622**


(22) Filed: **Dec. 11, 2015**

Related U.S. Application Data

(60) Provisional application No. 62/091,466, filed on Dec. 12, 2014.

(57) **ABSTRACT**

A device and method for cleaning or defogging a surgical scope during minimally invasive surgery, including a casing which houses a sponge and a heating element configured to be accessible to the surgical scope and the casing is configured to removably attach to a trocar during a surgical procedure.

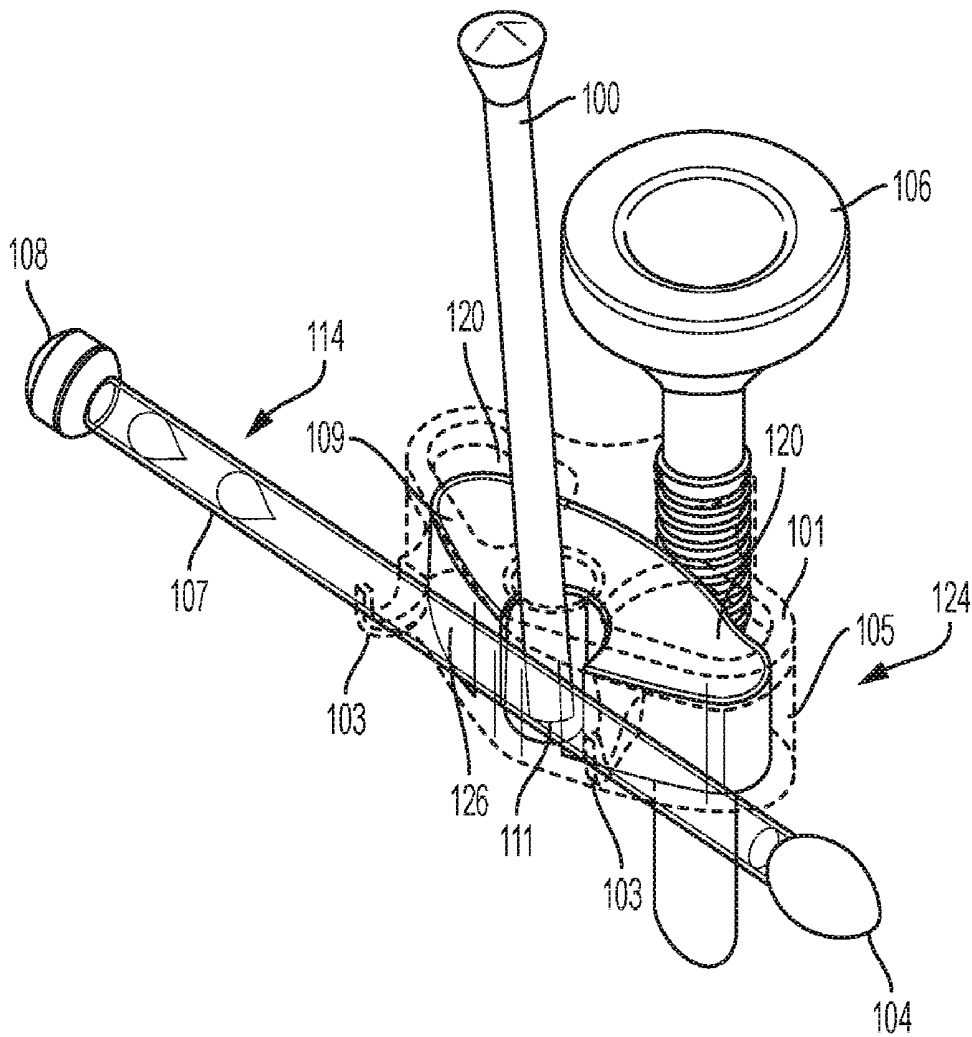

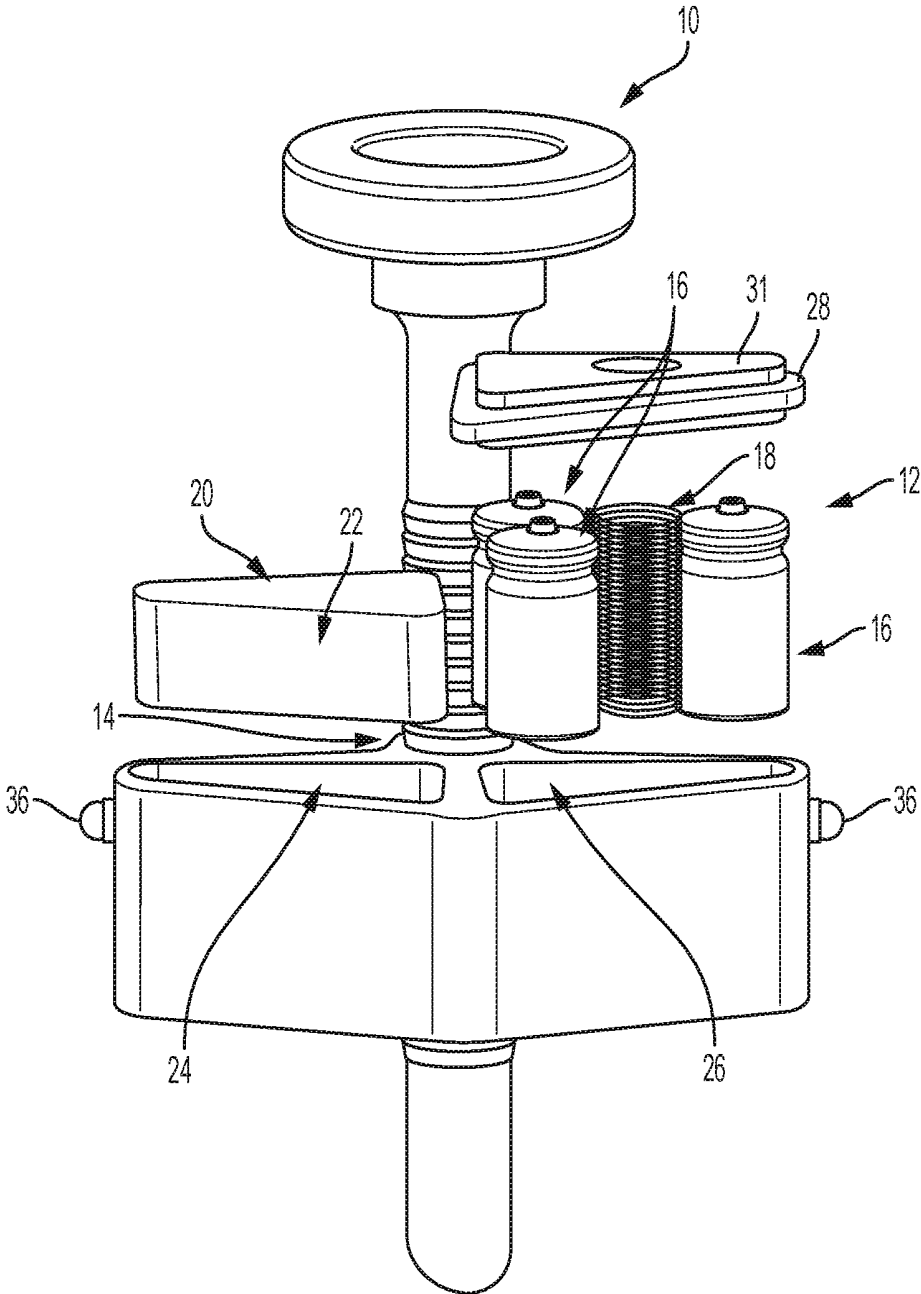


FIG. 1

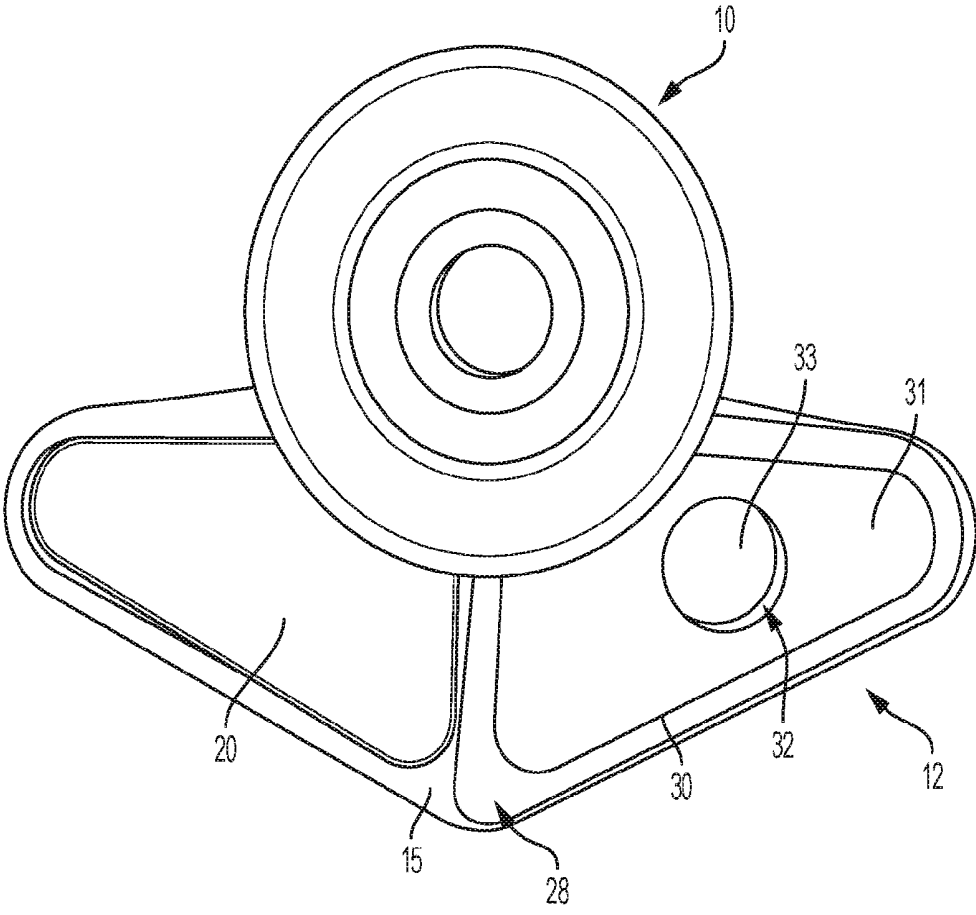


FIG. 2

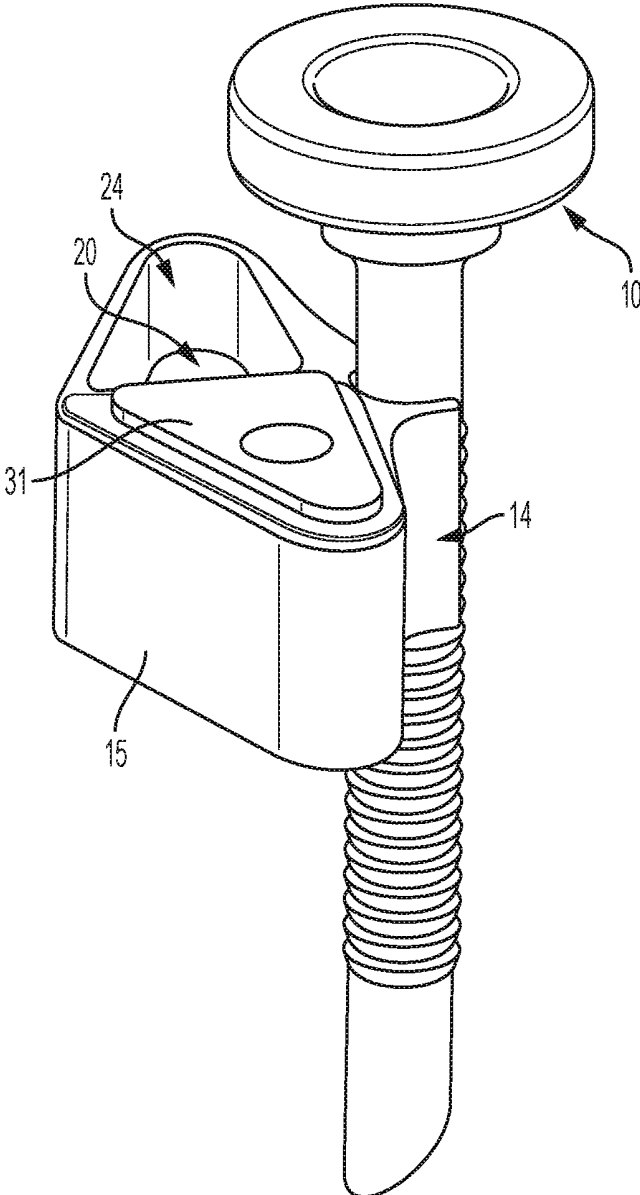


FIG. 3



FIG. 4

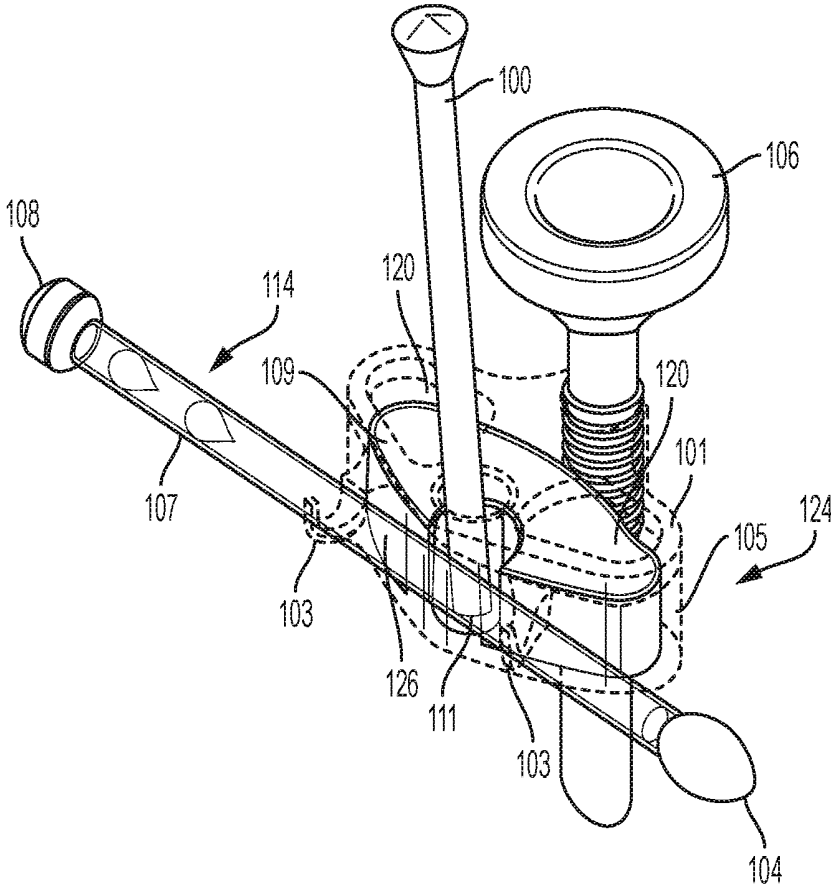


FIG. 6

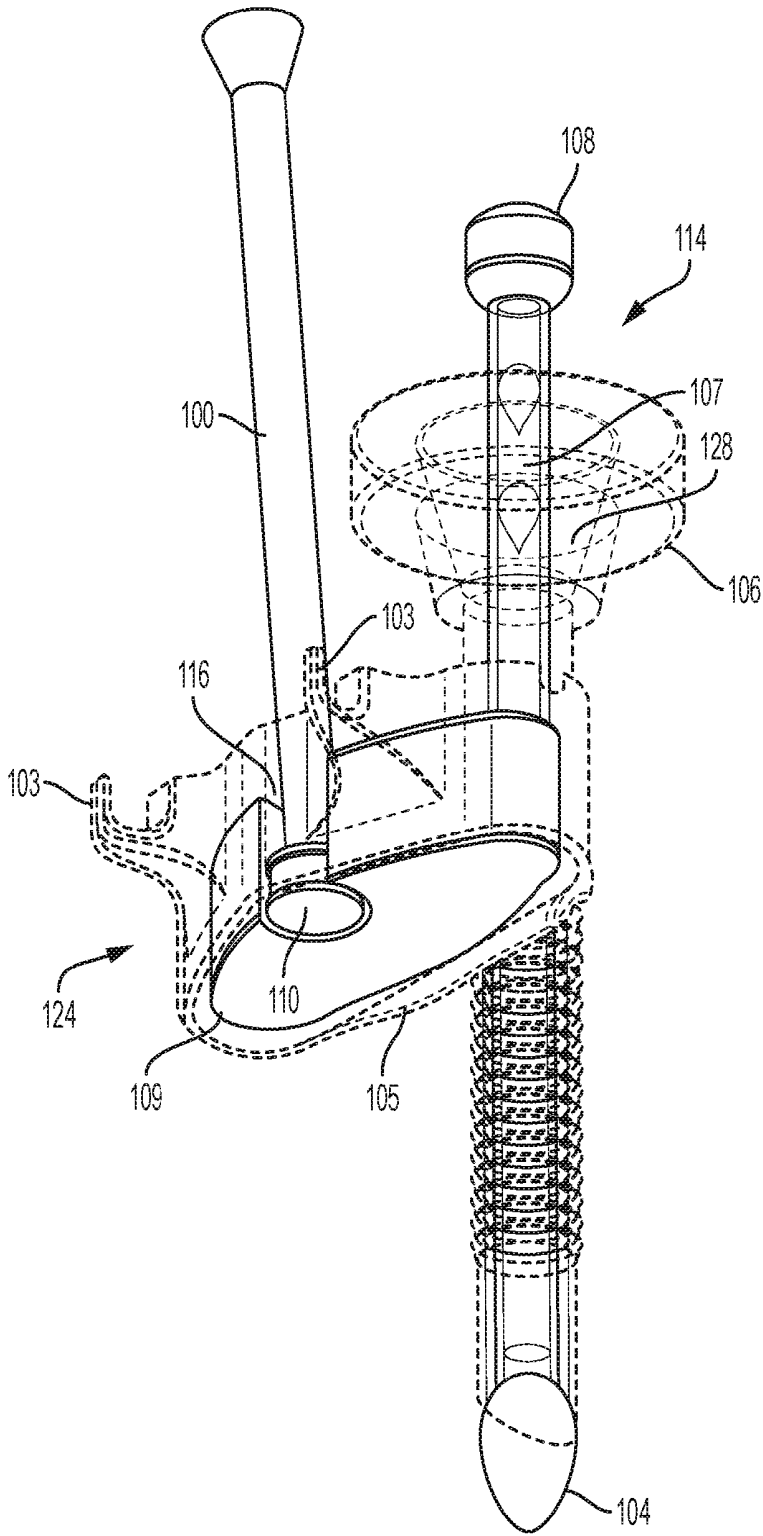


FIG. 7

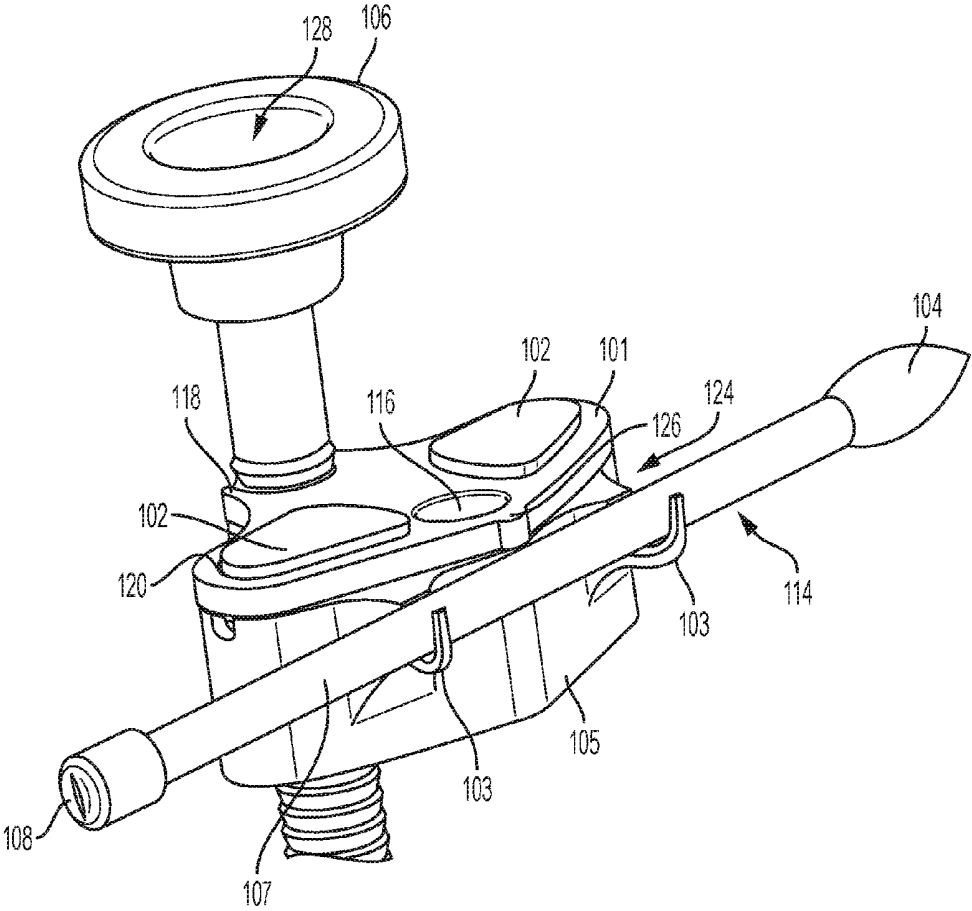


FIG. 8

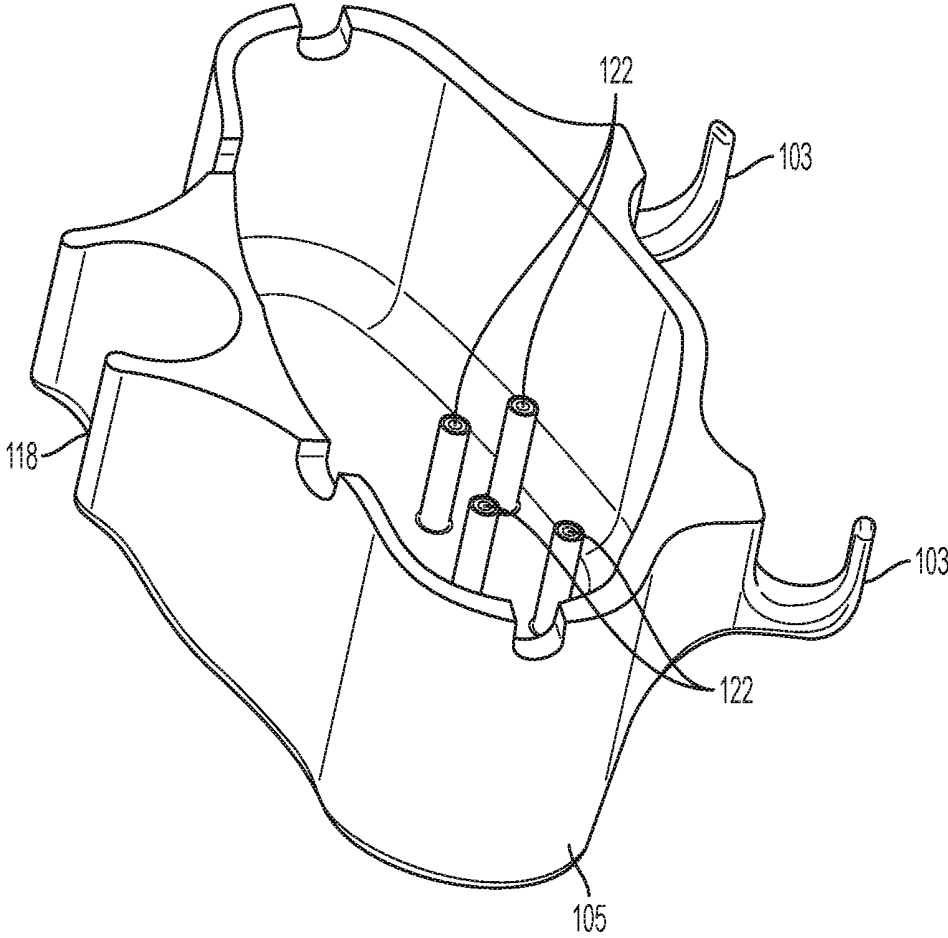


FIG. 9

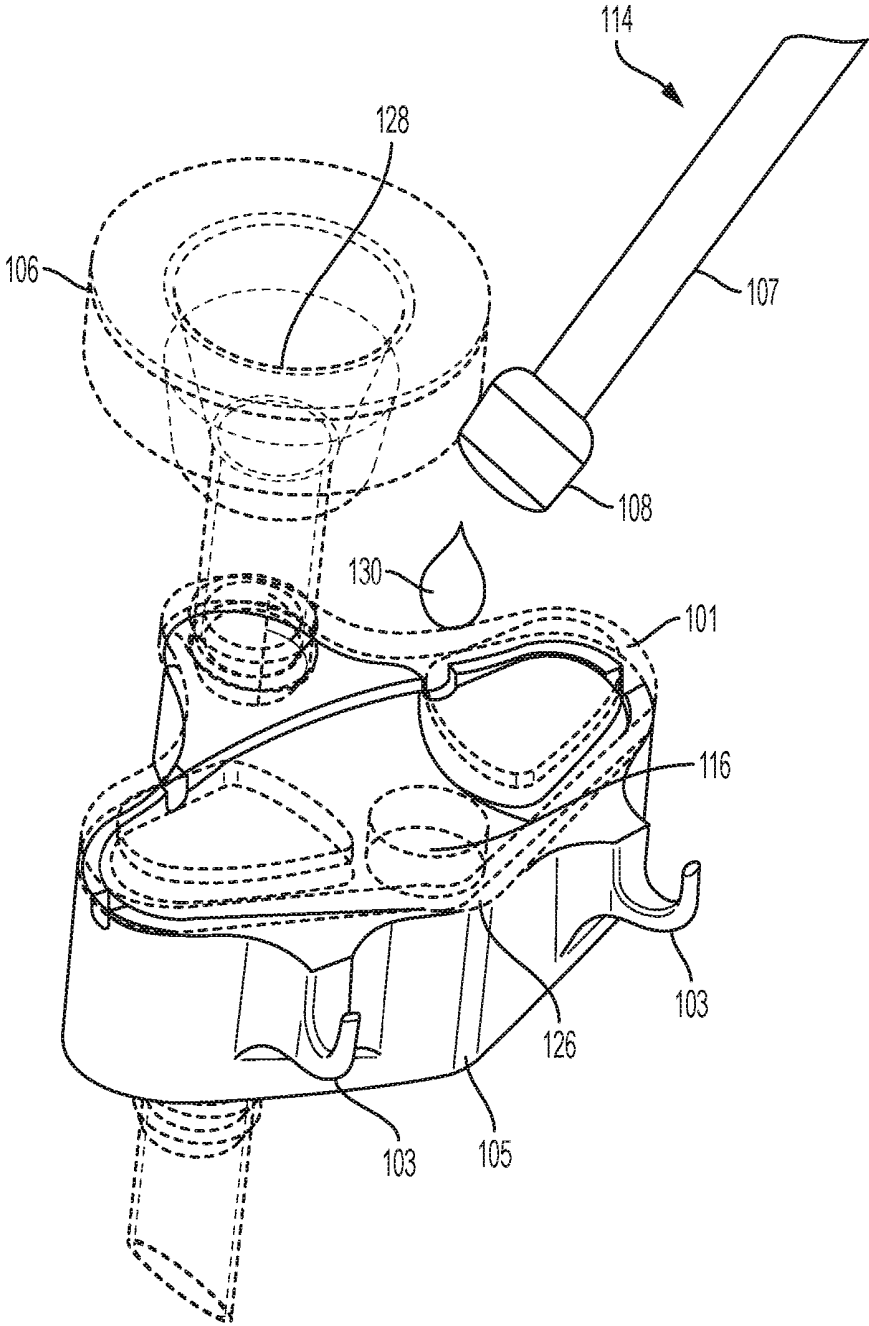


FIG. 10

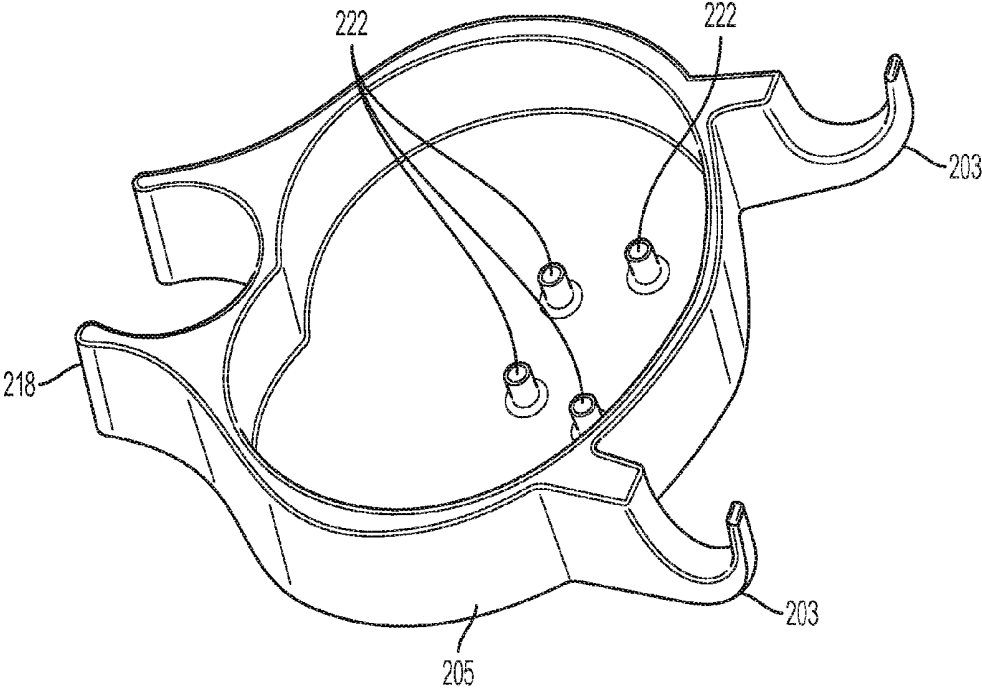


FIG. 12

**CLEANING DEVICE FOR CLEANING A
SCOPE, LAPAROSCOPE OR MICROSCOPE
USED IN SURGERY OR OTHER MEDICAL
PROCEDURES AND A METHOD OF USING
THE DEVICE DURING SURGICAL OR
OTHER MEDICAL PROCEDURES**

CROSS REFERENCE TO RELATED
APPLICATIONS

[0001] The present application claims priority to U.S. Provisional Patent Application No. 62/091,466, filed on Dec. 12, 2014, entitled “CLEANING DEVICE FOR CLEANING A SCOPE, LAPAROSCOPE OR MICROSCOPE USED IN SURGERY OR OTHER MEDICAL PROCEDURES AND A METHOD OF USING THE DEVICE DURING SURGICAL OR OTHER MEDICAL PROCEDURES”, which is hereby incorporated by reference in its entirety.

BACKGROUND OF THE INVENTION

Field of the Invention

[0002] The present application relates to a cleaning device for cleaning a scope, laparoscope, or microscope used in surgery or other medical procedures and a method of using the device during surgical or other medical procedures. The present application further relates to a cleaning kit for cleaning a trocar and a scope, laparoscope, or microscope, used in surgery or other medical procedures, and a method of using the kit during surgical or other medical procedures.

[0003] The following patents and patent publications are hereby incorporated by reference: U.S. Patent Application Publication No. 2012/0184897, having the title “INTEGRATED SYSTEMS AND METHODS FOR MAINTENANCE AND MANAGEMENT OF AN INTRA-ABDOMINAL GAS ENVIRONMENT DURING LAPAROSCOPIC SURGERY,” published Jul. 19, 2012; U.S. Patent Application Publication No. 2012/0197084, having the title “SYSTEMS AND METHODS FOR OPTIMIZING AND MAINTAINING VISUALIZATION OF A SURGICAL FIELD DURING THE USE OF SURGICAL SCOPES,” published Aug. 2, 2012; U.S. Patent Application Publication No. 2013/0060086, having the title “IMAGING SENSOR PROVIDING IMPROVED VISUALIZATION FOR SURGICAL SCOPES,” published on Mar. 7, 2013; U.S. Patent Application Publication No. 2010/0168520, having the title “VIEW OPTIMIZER AND STABILIZER FOR USE WITH SURGICAL SCOPES,” published Jul. 1, 2010; U.S. Pat. No. 8,535,220, having the title “LAPAROSCOPE CLEANING SYSTEM,” issued Sep. 17, 2013; U.S. Pat. No. 4,392,485, having the title “ENDOSCOPE,” issued on Jul. 12, 1983; U.S. Pat. No. 8,152,717, entitled “DEVICE FOR WHITE BALANCING AND APPLYING AN ANTI-FOG AGENT TO MEDICAL VIDEOSCOPIES PRIOR TO MEDICAL PROCEDURES,” issued on Apr. 10, 2012; U.S. Pat. No. 7,803,109, entitled “METHOD AND APPARATUS FOR PROTECTING THE DISTAL LENS OF ENDOSCOPES,” issued on Sep. 28, 2010; U.S. Pat. No. 7,311,660, entitled “METHOD AND APPARATUS FOR HEATING AND APPLYING WARM ANTIFOG SOLUTION TO ENDOSCOPES AS WELL AS A DISTAL LENS PROTECTOR,” issued on Dec. 25, 2007; U.S. Pat. No. 7,080,641, entitled “METHOD AND APPARATUS FOR HEATING STERILE SOLUTIONS DURING MEDICAL PROCEDURES,” issued on Jul. 25,

2006; U.S. Pat. No. 8,870,752, entitled “MEDICAL DEVICE SHEATH,” issued on Oct. 28, 2014; U.S. Pat. No. 8,727,969, entitled “ENDOSCOPE,” issued on May 20, 2014; U.S. Pat. No. 8,696,552, entitled “SELF-CONTAINED STERILIZABLE SURGICAL SYSTEM,” issued on Apr. 15, 2014; U.S. Pat. No. 8,540,745, entitled “BALLOON DISSECTOR WITH CANNULA,” issued on Sep. 24, 2013; U.S. Pat. No. 8,517,918, entitled “OPTICAL TROCAR WITH SCOPE HOLDING ASSEMBLY,” issued on Aug. 27, 2013; U.S. Pat. No. 8,467,589, entitled “HYBRID REGISTRATION METHOD,” issued on Jun. 18, 2013; U.S. Pat. No. 8,454,645, entitled “BALLOON DISSECTOR WITH CANNULA,” issued on Jun. 4, 2013; U.S. Pat. No. 8,452,068, entitled “HYBRID REGISTRATION METHOD,” issued on May 28, 2013; U.S. Pat. No. 7,955,330, entitled “MULTI-PORT SIDE-FIRE COAGULATOR,” issued Jun. 7, 2011; and U.S. Pat. No. 7,927,330, entitled “MULTI-PORT SIDE-FIRE COAGULATOR,” issued Apr. 19, 2011.

[0004] During minimally invasive surgeries, such as laparoscopic surgery, trocars are used to permit access into a patient’s body. Trocars are medical devices or instruments that comprise hollow tubes or hollow portions. During surgery, such as laparoscopic surgery, a trocar may be inserted through an incision into a patient’s body, such as into the abdominal or pelvic cavity of a patient. The trocar acts as a passageway for other surgical tools or devices, such as scopes, laparoscopes, microscopes, knives, graspers, scissors, staplers, and more, to enter the body for use during surgery.

[0005] During such surgical procedures, the lenses of viewing devices inserted into the body through the trocar, such as scopes, laparoscopes, and/or microscopes, may become clouded or the view therethrough may become partially or completely obscured. The view can be obscured, either partially or completely, if the lenses are smeared with bodily fluids or the like, or if the lenses become clouded or fogged over due to the humidity within the body of the patient. In addition, the interior of the trocars should also be kept clean.

[0006] An object of the present application may be to provide a cleaning device for a trocar and surgical scopes, which cleaning device may be utilized during surgery. The cleaning device also may be used to defog lenses or optics of a surgical scope.

SUMMARY OF THE INVENTION

[0007] When minimally invasive surgeries are performed using trocars, the scopes and/or microscopes used during surgery, which often are inserted into the body of the patient, may become smeared with bodily fluids or the like. This may cause the lens of the scope or microscope to become obscured or clouded because of smearing and/or the humidity or moisture within the body of the patient. Embodiments of the cleaning device and method described herein address these problems. There may be other applications for the scope or microscope which create the same problems as with minimally invasive surgery, and embodiments of the device and method described below may be appropriate to address those problems as well.

[0008] An embodiment of the cleaning device according to the present application may be configured for cleaning a surgical scope during minimally invasive surgery. The cleaning device may comprise a casing which houses a sponge and a heating element, and an attachment element connected to an

outer surface of the casing and configured to removably attach the casing to the trocar, wherein the casing is configured to allow a lens of the surgical scope to access the sponge and the heating element. In an embodiment, the casing may comprise a first depression formed in an upper surface of the casing and configured to receive the sponge therein and a second depression formed in an upper surface of the casing and configured to receive the heating element therein. In an embodiment the sponge may be impregnated with a cleaning medium. In an embodiment, the cleaning device may include a snap member that is configured to removably attach the casing to the trocar.

[0009] In an embodiment, the heating element may be comprised of a heating coil and at least one battery operatively connected to the heating coil, wherein the heating coil is configured to warm the lens of the surgical scope when the surgical scope is positioned in proximity to the heating coil. In an embodiment, the cleaning device may further comprise at least one light operatively connected to the at least one battery.

[0010] In an embodiment, the heating element may be comprised of a chemical pack.

[0011] An embodiment of the cleaning device described herein may comprise a cover and a wiping element, wherein the cover is disposed over the second depression, wherein the cover comprises a first hole, wherein a wiping element comprises a second hole, and wherein the wiping element is disposed over the cover so that the first hole and the second hole are oriented to allow the surgical scope to access the heating element. In an embodiment, the wiping element may be comprised of a microfiber material.

[0012] Another embodiment disclosed herein is a cleaning kit for use during minimally invasive surgery, comprising a container housing a sponge and configured to removably attach to the trocar, a cover comprising a scope access hole configured to permit a surgical scope to access the sponge, the cover positioned on an upper surface of the container; and a cannula cleaner comprising an elongated body having a first end having a cleaning tip disposed thereon and a second end, the cannula cleaner configured to be removably supported by at least one of the container and cover when not in use, wherein the cannula cleaner is configured for insertion in a cannula of a trocar and the cleaning tip is configured to contact the cannula when the cannula cleaner is inserted into the cannula. An embodiment of the cleaning kit may include a cannula cleaner wherein the elongated body further comprises a solution container configured to receive a cleaning medium, and a valve disposed on the second end of the elongated body, wherein the valve is configured to dispense the cleaning medium during surgery. In an embodiment the cleaning kit may comprise at least one wiping element disposed on the cover, wherein the at least one wiping element is configured to allow the surgical scope to access the sponge through the scope access hole. In an embodiment, the cleaning kit may further comprise a snap member configured to attach the container to the trocar.

[0013] In an embodiment, the cleaning kit may further comprise a heater disposed in the container, wherein the heater is configured to warm the surgical scope inserted through the scope access hole. In an embodiment, the heater is configured to border a substantial portion of a perimeter of the sponge. In an embodiment, the heater comprises a heating coil and at least one battery operatively connected to the heating coil, and the heating coil is configured to warm the

lens of the surgical scope during surgery. In an embodiment, the heater may comprise a chemical pack.

[0014] In an embodiment, the cleaning kit may further comprise one or more lights operatively connected to at least one battery.

[0015] Another embodiment is directed to a method of cleaning a surgical scope during minimally invasive surgery comprising inserting a trocar into a patient, attaching a cleaning device according to claim 3 to the trocar, heating a heating element of the cleaning device to a desired temperature, inserting the surgical scope into the trocar, removing the surgical scope from the trocar, wiping the lens of the surgical scope on the wiping element, and heating the lens of the surgical scope with the heating element. In an embodiment, this method further may comprise wiping the lens on the sponge.

[0016] One feature or aspect of an embodiment is using a cleaning device for cleaning laparoscopes used in a medical procedure, the cleaning device comprising a body with a snap device attached to the body, which snap device is configured to attach to a trocar. The body comprises an isosceles triangular shape with a longer side connecting the equal sides of the isosceles triangle with the snap device being attached to the middle of said longer side of the isosceles triangle, and the body comprising two hollowed out portions, one of said hollowed out portions being disposed on each side of said snap arrangement. A first hollowed out portion being configured to house a sponge impregnated with a cleaning solution, which cleaning solution is configured to clean off the tip portion of a laparoscope, where a lens is disposed, which tip portion is configured to be inserted into the trocar and into the body of the patient. A second hollowed out portion being configured to house a heating arrangement, which heating arrangement comprises a chemical heat pack and/or a battery-operated electric heating arrangement and a cover for the heating arrangement being disposed to form a closing side of said second hollowed out portion and being configured to provide an enclosure for the heating arrangement disposed in said second hollowed out portion. The cover comprising at least one of: a heat chamber cover, a microfiber holder, and a microfiber covering layer. The cover further comprises a hole therein being configured to receive a tip of a laparoscope. The procedure comprising: wetting said sponge by impregnating said sponge with cleaning solution, and disposing said impregnated sponge in said first hollowed out portion of said cleaning device; inserting said heating arrangement in said second hollowed out portion of said cleaning device; snapping said cleaning device onto the trocar and orienting said cleaning device toward a surgeon such that the apex of said isosceles triangle is disposed towards the surgeon or in some other direction than the apex being disposed towards said surgeon; heating the heating arrangement to a predetermined temperature; initially inserting a laparoscope into the trocar and into the body of a patient; proceeding with surgery until the lens portion of the laparoscope at its tip becomes smeared with the patient's bodily components or until the lens of the laparoscope is unusable because of condensation on the lens; removing the laparoscope from the trocar and wiping the lens on said impregnated sponge until the bodily components or condensate has been removed; inserting the tip of the laparoscope with its lens through said hole in said heat chamber cover; raising the temperature of the laparoscope tip sufficiently to minimize condensation on the laparoscope lens during a next phase of the surgical procedure; removing the

tip of the laparoscope from said heating chamber and inserting the tip of the laparoscope into the trocar; continuing the surgical procedure with a cleaned laparoscope; and repeating the above cleaning operation when required.

[0017] Another feature or aspect of an embodiment is a cleaning device for cleaning laparoscopes during a medical procedure for performing laparoscopic surgery, said cleaning device comprising: a body with a snap device attached to said body, which snap device is configured to attach to a trocar. The body comprises an isosceles triangular shape with a longer side connecting the equal sides of the isosceles triangle with the snap device being attached to the middle of said longer side of the isosceles triangle and the body comprising two hollowed out portions, one of said hollowed out portions being disposed on each side of said snap arrangement. A first hollowed out portion being configured to house a sponge impregnated with a cleaning solution, which cleaning solution is configured to clean off the tip portion of a laparoscope, where a lens is disposed, which tip portion is configured to be inserted into the trocar and into the body of the patient. A second hollowed out portion being configured to house a heating arrangement, which heating arrangement comprises a chemical heat pack and/or a battery-operated electric heating arrangement and a cover for the heating arrangement being disposed to form a closing side of said second hollowed out portion and being configured to provide an enclosure for the heating arrangement disposed in said second hollowed out portion. The cover comprising at least one of: a heat chamber cover, a microfiber holder, and a microfiber covering layer. The cover further comprises a hole therein being configured to receive a tip of a laparoscope.

[0018] For purposes of the description hereinafter, the spatial orientation terms and derivatives thereof shall relate to the embodiment as it is oriented in the drawing figures. However, it is to be understood that the invention may assume various alternative variations, except where expressly specified to the contrary. It is also to be understood that the specific devices illustrated in the attached drawings, and described in the following specification, are simply exemplary embodiments. Hence, specific dimensions and other physical characteristics related to the embodiments disclosed herein are not to be considered as limiting.

[0019] These and other features and characteristics of the present invention, as well as the methods of operation and functions of the related elements of structures and the combination of parts and economies of manufacture, will become more apparent upon consideration of the following description and the appended claims with reference to the accompanying drawings, all of which form a part of this specification, wherein like reference numerals designate corresponding parts in the various figures. As used in the specification and the claims, the singular form of "a", "an", and "the" include plural referents unless the context clearly dictates otherwise.

[0020] The above-discussed embodiments of the present invention will be described further herein below.

BRIEF DESCRIPTION OF THE DRAWING(S)

[0021] FIG. 1 shows an exploded front view of an embodiment of a cleaning device and a trocar used in at least minimally invasive surgery;

[0022] FIG. 2 is a top view of an embodiment of a cleaning device attached to a trocar;

[0023] FIG. 3 shows a perspective view of an embodiment of a cleaning device attached to a trocar by a snap member;

[0024] FIG. 4 shows a perspective view of an embodiment of a cleaning device and trocar;

[0025] FIG. 5 shows an exploded view of an embodiment of a cleaning device;

[0026] FIG. 6 shows a partially transparent perspective view of an embodiment of a cleaning kit attached to a trocar or cannula;

[0027] FIG. 7 shows another view of an embodiment of the cleaning kit shown in FIG. 6;

[0028] FIG. 8 shows another view of an embodiment of the cleaning kit shown in FIG. 6;

[0029] FIG. 9 shows a view of a container of an embodiment of the cleaning kit shown in FIG. 6;

[0030] FIG. 10 shows another view of the embodiment of the cleaning kit shown in FIG. 6, with a cannula cleaner being used to dispense cleaning medium;

[0031] FIG. 11 shows an embodiment of a cleaning kit; and

[0032] FIG. 12 shows a view of a container of an embodiment of the cleaning kit shown in FIG. 11.

DESCRIPTION OF THE INVENTION

[0033] FIG. 1 shows a trocar 10 used in minimally invasive surgery. The trocar 10 has a cleaning device 12 removably connected thereto. The cleaning device 12 as shown is snapped onto the trocar 10 using a snap member 14. However, this is not to be construed as limiting the present disclosure as any suitable attachment element, such as a hook-and-loop fabric, buckles, clips, tape, etc., configured to securely and removably attach the cleaning device 12 to the trocar 10 may be utilized.

[0034] An embodiment of cleaning device 12 is depicted in FIG. 1 in an exploded view. The cleaning device 12 comprises a casing 15 having the snap member 14 attached to an outside rear surface thereof. A first depression 24 may be formed in an upper surface of the casing 15 of cleaning device 12 to receive a sponge 20. In one example, the sponge 20 may be impregnated with a cleaning medium 22. The casing 15 may further include a second depression 26 formed in an upper surface thereof and disposed opposite the first depression 24. The second depression 26 may be configured to receive a heating element therein. In one example, the heating element can comprise batteries 16 and a heating coil 18 operatively connected to the batteries 16. The heating coil 18 may be configured to warm a microscope, laparoscope, or other surgical scope (not shown) so that the scope is ready for reinsertion in the trocar 10 and ready for reinsertion into the body of the patient being operated upon. Instead of batteries 16 and heating coil 18, a chemical pack housing chemicals that combine in an exothermic reaction, such as is used by skiers in their gloves to keep their hands warm while skiing, may be used as the heating element.

[0035] In one exemplary use of the cleaning device 12, the scope being utilized in a surgical procedure is removed from the trocar 10. It is first wiped off on the sponge 20, thereby to remove matter from the patient which has built up during the surgical procedure or which has condensed upon the scope during the surgical procedure. The heating element is then used to heat the front of the scope, thereby heating the front of the scope above the temperature of the patient to discourage the formation of condensate on the front of the scope when the scope is within the body of the patient. One or more lights 36, such as light emitting diode (LED), may be positioned on casing 15 and used to provide illumination for the trocar 10

and the site where the trocar **10** is inserted into a patient. The lights may be operatively connected to batteries **16**.

[0036] FIG. 2 shows a top view of cleaning device **12** attached to trocar **10**. The second depression **26** may further include a heating chamber cover **28** positioned over the top thereof to provide protection for the heating element. The heating chamber cover **28** may further include a microfiber holder **30** formed therein configured to hold a microfiber cover **31**. The heating chamber cover **28** and the microfiber cover **31** may be configured with at least one scope access hole **32** which permit the microscope or other scope to be inserted into heating chamber **33** to be warmed by heating coil **18**, a heating pack, or some other manner known in the art. Microfiber cover **31** may be used by surgical staff to wipe debris and/or fluids from a scope in order to clean the optics thereof prior to inserting the scope into the scope access hole **32** to be heated. In an embodiment, microfiber cover **31** may be disposed on heating chamber cover **28** within the holder **30** in order to provide easy access to surgical staff.

[0037] With further reference to FIG. 2, in one example, casing **15** may have a substantially isosceles triangular shape when viewed from above, with the two sides of the triangle that are not of equal length not adjacent to the trocar **10**. Such a configuration may have the benefit of optimizing placement of the heating coil **18** and batteries **16** in casing **15** next to sponge **20**. This configuration also may have the benefit of providing easy access to cleaning device **12** while minimizing interference of the device with access to the surgical site while the cleaning device **12** is attached to the trocar **10** during a surgical procedure.

[0038] In FIG. 3, the trocar **10** is shown again with the cleaning device **12** attached thereto by snap member **14**. An advantage of such an embodiment is that it places cleaning device **12** in close proximity to trocar **10**, and thereby provides easy access to surgical staff. Such an embodiment also has the advantage that cleaning device **12** does not need to be set on a separate tray.

[0039] With reference to FIGS. 3 and 4, sponge **20** is shown in its installed position in first depression **24** in casing **15**. Sponge **20** may be comprised of any material known in the art. Sponge **20** may be used for cleaning debris and/or fluid from a scope. Sponge **20** also may be impregnated with cleaning medium **22**, such as a cleaning and/or defogging fluid. In an embodiment, cleaning medium **22** and or sponge **20** may be sterile.

[0040] FIG. 4 shows the trocar **10** with an embodiment of cleaning device **12** from a different angle than the previous figures. Holes in microfiber cover **31** and heating chamber cover **28** create the scope access hole **32**, which allows a scope to access heating chamber **33** in second depression **26**, where heating coil **18** may warm and aid in defogging a scope. Debris may be wiped from a scope's optical components by surgical staff on microfiber cover **31** and/or sponge **20**, which may be impregnated with cleaning medium **22**.

[0041] FIG. 5 is another exploded view of the cleaning device **12** having the casing **15**. The casing **15** comprises an attaching mechanism, such as snap member **14**, which is configured to attach to a trocar. Snap member **14** is configured to removably attach to trocar **10**. Other embodiments of casing **15** may be configured to attach to trocar **10** with tape, a friction fit, or through another mechanism otherwise known in the art.

[0042] The casing **15** also comprises a first depression **24**, which is configured to hold a sponge **20**. The sponge **20** may

be at least partially moistened with cleaning medium **22**. The casing **15** also comprises second depression **26** which is configured to hold batteries **16** and heating coil **18** or a defogger, and forms heating chamber **33**. Second depression **26** may hold one or more batteries **16**, which in an embodiment includes three lithium batteries. In other embodiments, other types of batteries **16** may be used or adapted for use, and other numbers of batteries may be used. In another embodiment, another heating source other than an electrical or battery-powered heating source could be utilized, such as a chemical heat source or chemical heat pack, which would avoid the use and ultimate disposal of batteries, which can present challenges due to the potential environmental impact of battery waste.

[0043] The second depression **26** and heating chamber **33** of the casing **15** may be at least partially covered by heating chamber cover **28**. The heating chamber cover **28** may comprise the microfiber holder **30** and scope access hole **32**. A scope or microscope may be inserted into the scope access hole **32** and through the heating coil **18** or defogger. The scope or microscope may be wiped on the microfiber cover **31** disposed in the holder **30** before or after insertion into the scope access hole **32**.

[0044] In at least one possible embodiment, a structure or material, such as double-sided adhesive tape, could be connected or attached to the casing **15**, such as the side or underside, to allow the casing **15** to be connected or attached to a support structure.

[0045] FIG. 6 shows a partially transparent view of an embodiment of a cleaning kit **124** attached to a trocar **106**. The kit **124** includes a container **105** that may house a sponge **110**, which may be impregnated with a cleaning solution, and a heater **109**. A cover **101** is located on top of the container **105**. The cover **101** has an opening therein into which can be inserted a surgical viewing device **100**, such as a scope, laparoscope, or microscope, such that the scope lens **111** is inside the container **105**. In an embodiment, cover **101** may include one or more recesses **120**, at least one of which contains a microfiber wipe or cleaner **102**. Also shown is a cannula cleaner **114**, which is held by two cannula cleaner tube holders **103**. Holders **103** may removably secure the cannula cleaner **114** to the container **105** when it is not in use during a surgical procedure. Cannula cleaner **114** may be secured by a friction fit, or in some other manner otherwise known in the art. In addition, the cover **101** may have one or more projections **126** that project out above the cannula cleaner **114** to further secure the cannula cleaner **114** in place in a secured position on container **105**.

[0046] An embodiment of cannula cleaner **114** may include an elongated body with a cleaning tip **104** disposed at one end. In an embodiment, the body of the cannula cleaner **114** may comprise a tube that also functions as a solution container **107**. On the end opposite the cleaning tip **104** is located a solution dispensing valve **108**. Either the valve **108** or the solution container **107** may be squeezed or pinched or pressed in to cause an amount of a cleaning or defogging solution, or some other liquid known in the art, to be dispensed. The solution may be dispensed into the container **105**. By containing the solution in the cannula cleaner **114**, a supply of cleaning solution is readily available to be dispensed into the container **105**, and is in easy reach for a user of the trocar **106** and cleaning kit **124**, such as by a surgeon or other medical professional. By mounting the cannula cleaner **114** on the container **105**, the cannula cleaner **114** is easy to reach for use

in cleaning or clearing out the trocar **106**. The design of the cannula cleaner **114** therefore combines a cleaning device with a cleaning solution supply, so as to facilitate keeping the trocar **106** and viewing instruments clean during a surgical procedure. However, it should be understood that other embodiments of cannula cleaner **114** may exist, such as an embodiment that does not hold solution and lacks a solution dispensing valve **108**. Another embodiment may include cleaning tips **104** at both ends of the cleaning device **114**. In such an embodiment, the cleaning tips **104** may be of the same size or of different sizes. Cannula cleaning tip **104** may be comprised of a sponge, foam, microfiber, or some material otherwise known in the art.

[0047] FIG. 7 shows another view of the cleaning kit **124** shown in FIG. 6. In FIG. 7, container **105** is shown as transparent in order to demonstrate how scope **100** may be inserted through scope access hole **116**, so that the optics thereof may contact sponge **110**. However, it should be understood that not all embodiments of container **105** need be transparent. FIG. 7 also depicts how scope **100** may interact with an embodiment of heater **109**. In an embodiment, heater **109** may be configured to surround or partially surround scope **100**, and may substantially border the perimeter or part of the perimeter of sponge **110**. Heater **109** and sponge **110** may be configured to create a substantially cylindrical space, where the lens **111** of a scope **100** may be inserted for cleaning and/or defogging, which may be preferable to engage embodiments of scopes **100** that are substantially cylindrically-shaped. In an embodiment, sponge **110** may be configured to maximize efficient contact with lens **111** of scope **100**. In an embodiment, sponge **110** may be substantially circular in shape. Embodiments of heater **109** may comprise other shapes. Embodiments of heater **109** may use electrical or chemical processes to generate heat, or may do so using another manner known in the art.

[0048] With further reference to FIG. 7, cannula cleaner **114** may be inserted into a cannula **128** of trocar **106** to clean the cannula **128** of fluids, condensates, and/or debris. In an embodiment, cannula cleaning tip **104** may be inserted into cannula **128**. In an embodiment, cannula cleaning tip **104** may have a diameter that is substantially the same or larger than the diameter of the cannula **128**. Cannula cleaning tip **104** may be comprised of a deformable material, and deform to fit into cannula **128** while contacting the walls of the cannula **128**. Cannula cleaning tip **104** may be sufficiently absorptive to absorb fluids and/or condensate present in trocar **106**. Trocar **106** is shown as transparent in order to better illustrate the insertion of cannula cleaner **114** therein; however, it should be understood that embodiments of trocar **106** need not be transparent.

[0049] FIG. 8 shows a perspective view of the cleaning kit **124** depicted in FIG. 6. Cannula cleaner **114** is shown disposed on cannula holders **103**, which are configured to contain cannula cleaning device **114** against container **105** during a surgical procedure when cannula cleaner **114** is not in use. In an embodiment, cover **101** of cleaning kit **124** may include projection **126** that is configured to further constrain cannula cleaner **114** when not in use. Cover **101** may include one or more microfiber wipes **102** disposed thereon to further aid in cleaning debris or condensate from a scope **100**. While the embodiment shown in FIG. 8 shows a configuration wherein two microfiber wipes **102** are positioned on cover **101** roughly on either side of scope access hole **116**, it should be understood that other configurations or numbers of wipes **102**

may be used. It also should be understood that embodiments of cover **101** need not include microfiber wipes **102**, and that other materials or wiping elements otherwise known in the art may be used to wipe debris from the lens **111** of a scope **100**. Wipes **102** may be disposed in one or more recesses **120** in cover **101**. Cleaning kit **124** may removably attach to trocar **106** by a snap member **118**, or another manner known in the art.

[0050] FIG. 9 shows a perspective view of a portion of the container **105** of the cleaning kit **124** shown in FIG. 6. An embodiment of container **105** may be integrally molded with snap member **118** and/or one or more cannula cleaning device holder **103**. The interior of container **105** may comprise a single chamber, or multiple chambers. The at least one chamber may include one or more support posts **122**. Support posts **122** may provide support for cover **101**, and may provide support for configurations of heater **109**. In embodiments of heater **109**, posts **122** may support configurations of batteries, a heating coil, chemical packs, or other components of a heater **109** otherwise known in the art.

[0051] FIG. 10 shows another view of the cleaning kit **124**. In an embodiment, cannula cleaner **114** may be used to dispense cleaning and/or defogging solution into container **105** through scope access hole **116**. In an embodiment, solution may exit solution container **107** of cannula cleaner **114** through solution dispensing valve **108**. When solution—represented by a droplet of cleaning solution **130**—enters through scope access hole **116**, it may contact and be absorbed by sponge **110**. A scope may then be inserted into container **105** through scope access hole **116** and contact impregnated sponge **110**, which may aid in cleaning and/or defogging the scope **100**.

[0052] With reference to FIGS. 11 and 12, an alternative embodiment of a cleaning kit **224** is illustrated. Cleaning kit **224** is configured to clean lens **211** of a scope **200** and may include a container **205** that is shorter or thinner than the embodiment of the container **105** shown in FIG. 6. In the example in FIG. 11, no batteries are utilized, so a shorter or thinner container **205** can be utilized. In an embodiment, the kit may use no heating device or heating medium. In another embodiment, a chemical heating medium or chemical heating pack may be used which takes up less space than batteries. Cover **201** also may include a microfiber wipe or cleaner **202** that spans most or all of the surface area of cover **201**. FIG. 11 depicts two cannula cleaners **214** in order to demonstrate both insertion into trocar **206**, and placement in cleaner tube holders **203**. However, it should be understood that not all embodiments of cleaning kit **224** require more than one cannula cleaner **214**. Each of the cannula cleaners may include a cannula cleaning tip **204** at a first end thereof, a solution container **207** extending between the first end and second end thereof, and a solution dispensing valve **208** positioned at the second.

[0053] FIG. 12 shows a view of container **205** of the embodiment of the cleaning kit **224** shown in FIG. 11. In an embodiment, snap member **218** and one or more cannula cleaner holders **203** may be integrally molded with container **205**. The container **205** may comprise a chamber, and may include one or more internal supports **222**. In one example, internal supports **222** may be used to support cover **201**, or constrain a heater and/or sponge.

[0054] It is to be understood that the invention may assume various alternative variations, except where expressly specified to the contrary. It is also to be understood that the specific

devices illustrated in the attached drawings, and described in the specification, are simply exemplary embodiments of the invention. Although the invention has been described in detail for the purpose of illustration based on what is currently considered to be the most practical and preferred embodiments, it is to be understood that such detail is solely for that purpose and that the invention is not limited to the disclosed embodiments, but, on the contrary, is intended to cover modifications and equivalent arrangements that are within the spirit and scope thereof. For example, it is to be understood that the present invention contemplates that, to the extent possible, one or more features of any embodiment can be combined with one or more features of any other embodiment. The embodiments of the invention described herein above in the context of the preferred embodiments are not to be taken as limiting the embodiments of the invention to all of the provided details thereof, since modifications and variations thereof may be made without departing from the spirit and scope of the embodiments of the invention.

The invention claimed is:

1. A cleaning device configured for cleaning a surgical scope during minimally invasive surgery comprising:
 - a casing housing a sponge and a heating element; and
 - an attachment element connected to an outer surface of the casing and configured to removably attach the casing to a trocar,
 wherein the casing is configured to allow a lens of the surgical scope to access the sponge and the heating element.
2. The cleaning device of claim 1, wherein:
 - the casing comprises a first depression formed in an upper surface of the casing and configured to receive the sponge therein and a second depression formed in an upper surface of the casing and configured to receive the heating element therein.
3. The cleaning device of claim 2, further comprising:
 - a cover and a wiping element,
 wherein the cover is disposed over the second depression, wherein the cover comprises a first hole;
 - wherein the wiping element comprises a second hole; and
 - wherein the wiping element is disposed over the cover so that the first hole and the second hole are oriented to allow the surgical scope to access the heating element.
4. The cleaning device of claim 3, wherein the wiping element is comprised of a microfiber material.
5. The cleaning device of claim 1, wherein the sponge is impregnated with a cleaning medium.
6. The cleaning device of claim 1, wherein:
 - the heating element is comprised of a heating coil and at least one battery operatively connected to the heating coil,
 - wherein the heating coil is configured to warm the lens of the surgical scope when the surgical scope is positioned in proximity to the heating coil.
7. The cleaning device of claim 6, further comprising one or more lights operatively connected to the at least one battery.
8. The cleaning device of claim 1, wherein the heating element is comprised of a chemical pack.
9. The cleaning device of claim 1, wherein the attachment element is a snap member, the snap member being configured to removably attach the casing to the trocar.
10. A cleaning kit for use during minimally invasive surgery comprising:
 - a container housing a sponge configured to removably attach to a trocar;
 - a cover comprising a scope access hole configured to permit a surgical scope to access the sponge, the cover positioned on an upper surface of the container; and
 - a cannula cleaner comprising an elongated body having a first end having a cleaning tip disposed thereon and a second end, the cannula cleaner configured to be removably supported by at least one of the container and the cover when not in use,
 wherein the cannula cleaner is configured for insertion in a cannula of the trocar and the cleaning tip is configured to contact the cannula when the cannula cleaner is inserted into the cannula.
11. The cleaning kit of claim 10, wherein the elongated body of the cannula cleaner further comprises:
 - a solution container configured to receive a cleaning medium; and
 - a valve disposed on the second end of the elongated body, wherein the valve is configured to dispense the cleaning medium during surgery.
12. The cleaning kit of claim 10, further comprising:
 - at least one wiping element disposed on the cover,
 - wherein the at least one wiping element is configured to allow the surgical scope to access the sponge through the scope access hole.
13. The cleaning kit of claim 10, further comprising:
 - a heater disposed in the container,
 - wherein the heater is configured to warm the surgical scope inserted through the scope access hole.
14. The cleaning kit of claim 13, wherein the heater is configured to border a substantial portion of a perimeter of the sponge.
15. The cleaning kit of claim 13, wherein the heater comprises a heating coil and at least one battery operatively connected to the heating coil, and
 - wherein the heating coil is configured to warm a lens of the surgical scope during surgery.
16. The cleaning kit of claim 15, further comprising one or more lights operatively connected to the at least one battery.
17. The cleaning kit of claim 13, wherein the heater comprises a chemical pack.
18. The cleaning kit of claim 10, further comprising a snap member configured to attach the container to the trocar.
19. A method of cleaning a surgical scope during minimally invasive surgery comprising:
 - inserting a trocar into a patient;
 - attaching a cleaning device according to claim 3 to the trocar;
 - heating a heating element of the cleaning device to a desired temperature;
 - inserting the surgical scope into the trocar;
 - removing the surgical scope from the trocar;
 - wiping a lens of the surgical scope on the wiping element; and
 - heating the lens of the surgical scope with the heating element.
20. The method of claim 19, further comprising wiping the lens on the sponge.

专利名称(译)	用于外科手术或其他医疗程序的范围，腹腔镜或显微镜的清洁装置以及在外科手术或其他医疗程序中使用该装置的方法		
公开(公告)号	US20160166135A1	公开(公告)日	2016-06-16
申请号	US14/966622	申请日	2015-12-11
[标]申请(专利权)人(译)	MEDIX3D		
申请(专利权)人(译)	MEDIX3D LLC		
当前申请(专利权)人(译)	MEDIX3D LLC		
[标]发明人	FISSET CLAUDE		
发明人	FISSET, CLAUDE		
IPC分类号	A61B1/12 A61B17/34		
CPC分类号	A61B1/126 A61B17/3417 A61B1/127 A61B1/0014 A61B1/313 A61B1/121 A61B2090/701		
优先权	62/091466 2014-12-12 US		
其他公开文献	US10080488		
外部链接	Espacenet	USPTO	

摘要(译)

一种用于在微创手术期间清洁或除去手术镜的装置和方法，包括容纳海绵的壳体和被配置成可接近手术镜和壳体的加热元件，其构造成在外科手术过程中可移除地连接到套管针上。

