



US007665647B2

(12) **United States Patent**
Shelton, IV et al.

(10) **Patent No.:** **US 7,665,647 B2**
 (45) **Date of Patent:** **Feb. 23, 2010**

(54) **SURGICAL CUTTING AND STAPLING
 DEVICE WITH CLOSURE APPARATUS FOR
 LIMITING MAXIMUM TISSUE
 COMPRESSION FORCE**

4,317,451 A 3/1982 Cerwin et al.

(Continued)

FOREIGN PATENT DOCUMENTS

(75) Inventors: **Frederick E. Shelton, IV**, New Vienna,
 OH (US); **Jeffrey S. Swayze**, Hamilton,
 OH (US)

CA 2458946 A1 3/2003

(Continued)

(73) Assignee: **Ethicon Endo-Surgery, Inc.**, Cincinnati,
 OH (US)

OTHER PUBLICATIONS

(*) Notice: Subject to any disclaimer, the term of this
 patent is extended or adjusted under 35
 U.S.C. 154(b) by 0 days.

Disclosed Anonymously, "Motor-Driven Surgical Stapler Improve-
 ments," Research Disclosure Database No. 526041, Published: Feb.
 2008.

(Continued)

(21) Appl. No.: **11/541,151**

Primary Examiner—Rinaldi I. Rada

Assistant Examiner—Gloria R. Weeks

(22) Filed: **Sep. 29, 2006**

(57) **ABSTRACT**

(65) **Prior Publication Data**

US 2008/0078801 A1 Apr. 3, 2008

(51) **Int. Cl.**
A61B 17/068 (2006.01)

(52) **U.S. Cl.** **227/177.1; 227/175.1; 227/181.1**

(58) **Field of Classification Search** **227/175.1,**
227/177.1, 181.1

See application file for complete search history.


(56) **References Cited**

U.S. PATENT DOCUMENTS

2,037,727 A	4/1936	Chapelle
2,853,074 A	9/1958	Olson
3,490,675 A	1/1970	Green et al.
3,551,987 A	1/1971	Wilkinson
3,643,851 A	2/1972	Green et al.
3,662,939 A	5/1972	Bryan
3,717,294 A	2/1973	Green
3,819,100 A	6/1974	Noiles et al.
3,894,174 A	7/1975	Cartun
3,940,844 A	3/1976	Colby et al.

A surgical instrument for being endoscopically or laparo-
 scopically inserted into a surgical site for simultaneous stap-
 ling and severing of tissue includes an elongate channel that
 is configured to operably support a staple cartridge therein.
 An anvil is operably coupled to the elongate channel and is
 selectively movable between open and closed positions. A
 closure tube assembly interfaces with the anvil to selectively
 apply a closing force thereto in response to a closing motion
 applied to the closure tube assembly. At least one force lim-
 iting member interacts with the closure tube assembly to limit
 an amount of the closing force applied to the anvil by the
 closure tube assembly in response to a resistive force experi-
 enced by the anvil when clamping tissue between the anvil
 and the elongate channel. The force limiting member may
 comprise one or more spring sections in the closure tube
 assembly or at least one leaf spring in the distal end of the
 closure tube assembly. Other embodiments may include steps
 formed in a ramp portion of the anvil for engaging the distal
 end of the closure tube assembly.

12 Claims, 116 Drawing Sheets

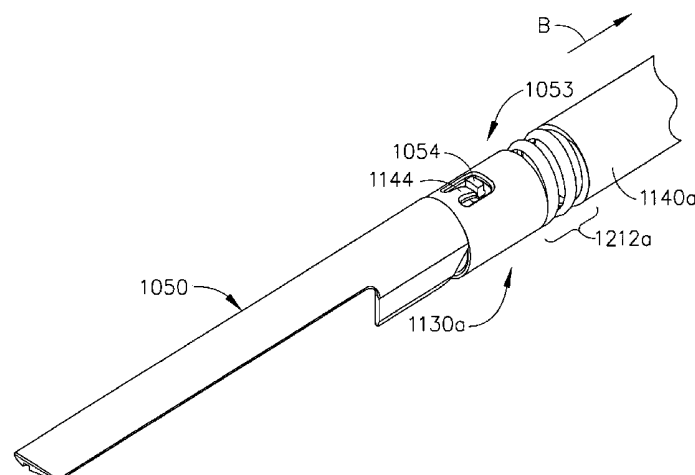

U.S. PATENT DOCUMENTS					
4,321,002 A	3/1982	Froehlich	5,156,315 A	10/1992	Green et al.
4,331,277 A	5/1982	Green	5,158,567 A	10/1992	Green
4,379,457 A	4/1983	Gravener et al.	5,197,648 A	3/1993	Gingold
4,380,312 A	4/1983	Landrus	5,205,459 A	4/1993	Brinkerhoff et al.
4,383,634 A	5/1983	Green	5,211,649 A	5/1993	Kohler et al.
4,396,139 A	8/1983	Hall et al.	5,219,111 A	6/1993	Bilotti et al.
4,402,445 A	9/1983	Green	5,221,036 A	6/1993	Takase
4,415,112 A	11/1983	Green	5,222,963 A	6/1993	Brinkerhoff et al.
4,428,376 A	1/1984	Mericle	5,222,975 A	6/1993	Crainich
4,429,695 A	2/1984	Green	5,222,976 A	6/1993	Yoon
4,442,964 A	4/1984	Becht	5,242,457 A	9/1993	Akopov et al.
4,475,679 A	10/1984	Fleury, Jr.	5,246,156 A	9/1993	Rothfuss et al.
4,485,816 A	12/1984	Krumme	5,246,443 A	9/1993	Mai
4,500,024 A	2/1985	DiGiovanni et al.	5,253,793 A	10/1993	Green et al.
4,505,273 A	3/1985	Braun et al.	5,258,009 A	11/1993	Connors
4,506,671 A	3/1985	Green	5,263,629 A	11/1993	Trumbull et al.
4,520,817 A	6/1985	Green	5,271,544 A	12/1993	Fox et al.
4,522,327 A	6/1985	Korthoff et al.	RE34,519 E	1/1994	Fox et al.
4,526,174 A	7/1985	Froehlich	5,275,323 A	1/1994	Schulze et al.
4,530,453 A	7/1985	Green	5,282,806 A	2/1994	Haber et al.
4,548,202 A	10/1985	Duncan	5,282,829 A	2/1994	Hermes
4,566,620 A	1/1986	Green et al.	5,304,204 A	4/1994	Bregen
4,573,622 A	3/1986	Green et al.	5,307,976 A	5/1994	Olson et al.
4,580,712 A	4/1986	Green	5,309,927 A	5/1994	Welch
4,589,416 A	5/1986	Green	5,318,221 A	6/1994	Green et al.
4,605,001 A	8/1986	Rothfuss et al.	5,342,395 A	8/1994	Jarrett et al.
4,606,343 A	8/1986	Conta et al.	5,342,396 A	8/1994	Cook
4,610,250 A	9/1986	Green	5,344,060 A	9/1994	Gravener et al.
4,610,383 A	9/1986	Rothfuss et al.	5,350,400 A	9/1994	Esposito et al.
4,619,262 A	10/1986	Taylor	5,352,238 A	10/1994	Green et al.
4,629,107 A	12/1986	Fedotov et al.	5,358,510 A	10/1994	Luscombe et al.
4,633,874 A	1/1987	Chow et al.	5,366,134 A	11/1994	Green et al.
4,655,222 A	4/1987	Florez et al.	5,366,479 A	11/1994	McGarry et al.
4,664,305 A	5/1987	Blake, III et al.	5,379,933 A	1/1995	Green et al.
4,667,674 A	5/1987	Korthoff et al.	5,383,880 A	1/1995	Hooven
4,671,445 A	6/1987	Barker et al.	5,389,098 A	2/1995	Tsuruta et al.
4,709,120 A	11/1987	Pearson	5,392,979 A	2/1995	Green et al.
4,715,520 A	12/1987	Roehr, Jr. et al.	5,395,030 A	3/1995	Kuramoto et al.
4,719,917 A	1/1988	Barrows et al.	5,395,033 A	3/1995	Byrne et al.
4,728,020 A	3/1988	Green et al.	5,397,046 A	3/1995	Savage et al.
4,741,336 A	5/1988	Failla et al.	5,397,324 A	3/1995	Carroll et al.
4,754,909 A	7/1988	Barker et al.	5,403,312 A	4/1995	Yates et al.
4,767,044 A	8/1988	Green	5,411,508 A	5/1995	Bessler et al.
4,805,617 A	2/1989	Bedi et al.	5,413,267 A	5/1995	Solyntjes et al.
4,805,823 A	2/1989	Rothfuss	5,413,268 A	5/1995	Green et al.
4,809,695 A	3/1989	Gwathmey et al.	5,415,334 A	5/1995	Williamson, IV et al.
4,817,847 A	4/1989	Redtenbacher et al.	5,415,335 A	5/1995	Knodell, Jr.
4,821,939 A	4/1989	Green	5,425,745 A	6/1995	Green et al.
4,869,414 A	9/1989	Green et al.	5,431,322 A	7/1995	Green et al.
4,869,415 A	9/1989	Fox	5,433,721 A	7/1995	Hooven et al.
4,892,244 A	1/1990	Fox et al.	5,441,193 A	8/1995	Gravener
4,915,100 A	4/1990	Green	5,445,304 A	8/1995	Plyley et al.
4,941,623 A	7/1990	Pruitt	5,445,644 A	8/1995	Pietrafitta et al.
4,944,443 A	7/1990	Odds et al.	5,456,401 A	10/1995	Green et al.
4,955,959 A	9/1990	Tompkins et al.	5,462,215 A	10/1995	Viola et al.
4,978,049 A	12/1990	Green	5,465,895 A	11/1995	Knodel et al.
5,009,661 A	4/1991	Michelson	5,465,896 A	11/1995	Allen et al.
5,027,834 A	7/1991	Pruitt	5,470,006 A	11/1995	Rodak
5,031,814 A	7/1991	Tompkins et al.	5,472,132 A	12/1995	Savage et al.
5,040,715 A	8/1991	Green et al.	5,474,566 A	12/1995	Alesi et al.
5,062,563 A	11/1991	Green et al.	5,478,354 A	12/1995	Tovey et al.
5,065,929 A	11/1991	Schulze et al.	5,480,089 A	1/1996	Blewett
5,071,430 A	12/1991	de Salis et al.	5,482,197 A	1/1996	Green et al.
5,080,556 A	1/1992	Carreno	5,484,095 A	1/1996	Green et al.
5,104,025 A	4/1992	Main et al.	5,484,451 A	1/1996	Akopov et al.
5,106,008 A	4/1992	Tompkins et al.	5,485,947 A	1/1996	Olson et al.
5,111,987 A	5/1992	Moeinzadeh et al.	5,485,952 A	1/1996	Fontayne
5,116,349 A	5/1992	Aranyi	5,487,499 A	1/1996	Sorrentino et al.
5,129,570 A	7/1992	Schulze et al.	5,487,500 A	1/1996	Knodel et al.
5,137,198 A	8/1992	Nobis et al.	5,489,058 A	2/1996	Plyley et al.
5,139,513 A	8/1992	Segato	5,497,933 A	3/1996	DeFonzo et al.
			5,503,320 A	4/1996	Webster et al.
			5,503,635 A	4/1996	Sauer et al.

5,503,638 A	4/1996	Cooper et al.	5,680,983 A	10/1997	Plyley et al.
5,509,596 A	4/1996	Green et al.	5,685,474 A	11/1997	Seeber
5,518,163 A	5/1996	Hooven	5,688,270 A	11/1997	Yates et al.
5,518,164 A	5/1996	Hooven	5,690,269 A	11/1997	Bolanos et al.
5,522,817 A	6/1996	Sander et al.	5,692,668 A	12/1997	Schulze et al.
5,529,235 A	6/1996	Boiarski et al.	5,697,543 A	12/1997	Burdorff
5,535,934 A	7/1996	Boiarski et al.	5,697,943 A	12/1997	Sauer et al.
5,535,935 A	7/1996	Vidal et al.	5,702,408 A	12/1997	Wales et al.
5,535,937 A	7/1996	Boiarski et al.	5,704,534 A	1/1998	Huitema et al.
5,540,375 A	7/1996	Bolanos et al.	5,706,997 A	1/1998	Green et al.
5,542,594 A	8/1996	McKean et al.	5,709,680 A	1/1998	Yates et al.
5,547,117 A	8/1996	Hamblin et al.	5,711,472 A	1/1998	Bryan
5,549,628 A	8/1996	Cooper et al.	5,713,505 A	2/1998	Huitema
5,553,765 A	9/1996	Knodel et al.	5,715,987 A	2/1998	Kelley et al.
5,554,169 A	9/1996	Green et al.	5,715,988 A	2/1998	Palmer
5,560,532 A	10/1996	DeFonzo et al.	5,716,366 A	2/1998	Yates
5,562,239 A	10/1996	Boiarski et al.	5,718,359 A	2/1998	Palmer et al.
5,562,241 A	10/1996	Knodel et al.	5,725,536 A	3/1998	Oberlin et al.
5,562,682 A	10/1996	Oberlin et al.	5,725,554 A	3/1998	Simon et al.
5,564,615 A	10/1996	Bishop et al.	5,732,871 A	3/1998	Clark et al.
5,571,090 A	11/1996	Sherts	5,735,445 A	4/1998	Vidal et al.
5,571,116 A	11/1996	Bolanos et al.	5,738,474 A	4/1998	Blewett
5,573,543 A	11/1996	Akopov et al.	5,743,456 A	4/1998	Jones et al.
5,575,799 A	11/1996	Bolanos et al.	5,752,644 A	5/1998	Bolanos et al.
5,575,803 A	11/1996	Cooper et al.	5,752,965 A	5/1998	Francis et al.
5,577,654 A	11/1996	Bishop	5,758,814 A	6/1998	Gallagher et al.
5,580,067 A	12/1996	Hamblin et al.	5,762,255 A	6/1998	Chrisman et al.
5,582,611 A	12/1996	Tsuruta et al.	5,762,256 A	6/1998	Mastri et al.
5,584,425 A	12/1996	Savage et al.	5,766,188 A	6/1998	Igaki
5,586,711 A	12/1996	Plyley et al.	5,779,130 A	7/1998	Alesi et al.
5,588,579 A	12/1996	Schnut et al.	5,779,132 A	7/1998	Knodel et al.
5,588,580 A	12/1996	Paul et al.	5,782,396 A	7/1998	Mastri et al.
5,588,581 A	12/1996	Conlon et al.	5,782,397 A	7/1998	Koukline
5,597,107 A	1/1997	Knodel et al.	5,785,232 A	7/1998	Vidal et al.
5,601,224 A	2/1997	Bishop et al.	5,794,834 A	8/1998	Hamblin et al.
5,603,443 A	2/1997	Clark et al.	5,797,536 A	8/1998	Smith et al.
5,605,272 A	2/1997	Witt et al.	5,797,537 A	8/1998	Oberlin et al.
5,605,273 A	2/1997	Hamblin et al.	5,797,538 A	8/1998	Heaton et al.
5,607,094 A	3/1997	Clark et al.	5,799,857 A	9/1998	Robertson et al.
5,607,095 A	3/1997	Smith et al.	5,820,009 A	10/1998	Melling et al.
5,609,285 A	3/1997	Grant et al.	5,823,066 A	10/1998	Huitema et al.
5,624,452 A	4/1997	Yates	5,826,776 A	10/1998	Schulze et al.
5,628,446 A	5/1997	Geiste et al.	5,829,662 A	11/1998	Allen et al.
5,630,539 A	5/1997	Plyley et al.	5,833,690 A	11/1998	Yates et al.
5,630,540 A	5/1997	Blewett	5,833,695 A	11/1998	Yoon
5,632,432 A	5/1997	Schulze et al.	5,836,503 A	11/1998	Ehrenfels et al.
5,632,433 A	5/1997	Grant et al.	5,839,639 A	11/1998	Sauer et al.
5,634,584 A	6/1997	Okorocha et al.	5,846,254 A	12/1998	Schulze et al.
5,636,779 A	6/1997	Palmer	5,855,311 A	1/1999	Hamblin et al.
5,636,780 A	6/1997	Green et al.	5,865,361 A	2/1999	Milliman et al.
5,639,008 A	6/1997	Gallagher et al.	5,868,760 A	2/1999	McGuckin, Jr.
5,645,209 A	7/1997	Green et al.	5,871,135 A	2/1999	Williamson, IV et al.
5,647,526 A	7/1997	Green et al.	5,878,937 A	3/1999	Green et al.
5,649,937 A	7/1997	Bito et al.	5,878,938 A	3/1999	Bittner et al.
5,651,491 A	7/1997	Heaton et al.	5,891,160 A	4/1999	Williamson, IV et al.
5,653,373 A	8/1997	Green et al.	5,893,506 A	4/1999	Powell
5,653,374 A	8/1997	Young et al.	5,894,979 A	4/1999	Powell
5,653,721 A	8/1997	Knodel et al.	5,897,562 A	4/1999	Bolanos et al.
5,655,698 A	8/1997	Yoon	5,901,895 A	5/1999	Heaton et al.
5,657,921 A	8/1997	Young et al.	5,902,312 A	5/1999	Frater et al.
5,658,300 A	8/1997	Bito et al.	5,906,625 A	5/1999	Bito et al.
5,662,258 A	9/1997	Knodel et al.	5,911,353 A	6/1999	Bolanos et al.
5,662,260 A	9/1997	Yoon	5,915,616 A	6/1999	Viola et al.
5,662,662 A	9/1997	Bishop et al.	5,918,791 A	7/1999	Sorrentino et al.
5,667,517 A	9/1997	Hooven	5,919,198 A	7/1999	Graves, Jr. et al.
5,667,527 A	9/1997	Cook	5,941,442 A	8/1999	Geiste et al.
5,669,544 A	9/1997	Schulze et al.	5,954,259 A	9/1999	Viola et al.
5,673,840 A	10/1997	Schulze et al.	5,988,479 A	11/1999	Palmer
5,673,841 A	10/1997	Schulze et al.	6,010,054 A	1/2000	Johnson et al.
5,673,842 A	10/1997	Bittner et al.	6,017,356 A	1/2000	Frederick et al.
5,678,748 A	10/1997	Plyley et al.	6,022,352 A	2/2000	Vandewalle
5,680,981 A	10/1997	Mililli et al.	6,024,748 A	2/2000	Manzo et al.
5,680,982 A	10/1997	Schulze et al.	6,032,849 A	3/2000	Mastri et al.

US 7,665,647 B2

Page 4

6,045,560	A	4/2000	McKean et al.	6,846,307	B2	1/2005	Whitman et al.
6,050,472	A	4/2000	Shibata	6,846,308	B2	1/2005	Whitman et al.
6,079,606	A	6/2000	Milliman et al.	6,846,309	B2	1/2005	Whitman et al.
6,083,234	A	7/2000	Nicholas et al.	6,849,071	B2	2/2005	Whitman et al.
6,083,242	A	7/2000	Cook	RE38,708	E	3/2005	Bolanos et al.
6,086,600	A	7/2000	Kortenbach	6,872,214	B2	3/2005	Sonnenschein et al.
6,099,537	A	8/2000	Sugai et al.	6,877,647	B2	4/2005	Green et al.
6,102,271	A	8/2000	Longo et al.	6,905,057	B2	6/2005	Swayze et al.
6,109,500	A	8/2000	Alli et al.	6,913,608	B2	7/2005	Liddicoat et al.
6,119,913	A	9/2000	Adams et al.	6,939,358	B2	9/2005	Palacios et al.
H1904	H	10/2000	Yates et al.	6,945,444	B2	9/2005	Gresham et al.
6,126,058	A	10/2000	Adams et al.	6,953,138	B1	10/2005	Dworak et al.
6,131,789	A	10/2000	Schulze et al.	6,953,139	B2	10/2005	Milliman et al.
6,155,473	A	12/2000	Tompkins et al.	6,959,852	B2	11/2005	Shelton, IV et al.
6,171,316	B1	1/2001	Kovac et al.	6,960,220	B2	11/2005	Marino et al.
6,171,330	B1	1/2001	Benchetrit	6,964,363	B2	11/2005	Wales et al.
6,202,914	B1	3/2001	Geiste et al.	6,974,462	B2	12/2005	Sater
6,241,139	B1	6/2001	Milliman et al.	6,978,921	B2	12/2005	Shelton, IV et al.
6,250,532	B1	6/2001	Green et al.	6,978,922	B2	12/2005	Bilotti et al.
6,258,107	B1	7/2001	Balázs et al.	6,981,628	B2	1/2006	Wales
6,264,086	B1	7/2001	McGuckin, Jr.	6,981,941	B2	1/2006	Whitman et al.
6,264,087	B1	7/2001	Whitman	6,986,451	B1	1/2006	Mastri et al.
6,273,897	B1	8/2001	Dalessandro et al.	6,988,649	B2	1/2006	Shelton, IV et al.
6,302,311	B1	10/2001	Adams et al.	6,988,650	B2	1/2006	Schwemberger et al.
6,315,184	B1	11/2001	Whitman	7,000,818	B2	2/2006	Shelton, IV et al.
6,320,123	B1	11/2001	Reimers	7,000,819	B2	2/2006	Swayze et al.
6,325,810	B1	12/2001	Hamilton et al.	7,008,435	B2	3/2006	Cummins
6,330,965	B1	12/2001	Milliman et al.	7,032,798	B2	4/2006	Whitman et al.
6,358,224	B1	3/2002	Tims et al.	7,032,799	B2	4/2006	Viola et al.
6,387,113	B1	5/2002	Hawkins et al.	7,044,352	B2	5/2006	Shelton, IV et al.
6,387,114	B2	5/2002	Adams	7,044,353	B2	5/2006	Mastri et al.
6,398,797	B2	6/2002	Bombard et al.	7,055,730	B2	6/2006	Ehrenfels et al.
6,416,486	B1	7/2002	Wampler	7,055,731	B2	6/2006	Shelton, IV et al.
RE37,814	E	8/2002	Allgeyer	7,056,330	B2	6/2006	Gayton
6,436,107	B1	8/2002	Wang et al.	7,059,508	B2	6/2006	Shelton, IV et al.
6,440,146	B2	8/2002	Nicholas et al.	7,063,712	B2	6/2006	Vargas et al.
6,443,973	B1	9/2002	Whitman	7,066,944	B2	6/2006	Laufer et al.
6,488,197	B1	12/2002	Whitman	7,070,083	B2	7/2006	Jankowski
6,491,201	B1	12/2002	Whitman	7,077,856	B2	7/2006	Whitman
6,503,257	B2	1/2003	Grant et al.	7,083,075	B2	8/2006	Swayze et al.
6,503,259	B2	1/2003	Huxel et al.	7,090,673	B2	8/2006	Dycus et al.
6,505,768	B2	1/2003	Whitman	7,090,684	B2	8/2006	McGuckin, Jr. et al.
6,517,565	B1	2/2003	Whitman et al.	7,097,089	B2	8/2006	Marczyk
6,522,101	B2	2/2003	Malackowski	7,114,642	B2	10/2006	Whitman
6,551,333	B2	4/2003	Kuhns et al.	7,118,582	B1	10/2006	Wang et al.
6,578,751	B2	6/2003	Hartwick	7,128,253	B2	10/2006	Mastri et al.
6,592,597	B2	7/2003	Grant et al.	7,128,254	B2	10/2006	Shelton, IV et al.
6,601,749	B2	8/2003	Sullivan et al.	7,140,527	B2	11/2006	Ehrenfels et al.
6,616,686	B2	9/2003	Coleman et al.	7,143,924	B2	12/2006	Scirica et al.
6,619,529	B2	9/2003	Green et al.	7,143,925	B2	12/2006	Shelton, IV et al.
6,629,988	B2	10/2003	Weadock	7,143,926	B2	12/2006	Shelton, IV et al.
6,644,532	B2	11/2003	Green et al.	7,159,750	B2	1/2007	Racenet et al.
6,656,193	B2	12/2003	Grant et al.	7,168,604	B2	1/2007	Milliman et al.
6,669,073	B2	12/2003	Milliman et al.	7,188,758	B2	3/2007	Viola et al.
6,681,978	B2	1/2004	Geiste et al.	7,207,471	B2	4/2007	Heinrich et al.
6,681,979	B2	1/2004	Whitman	7,207,472	B2	4/2007	Wukusick et al.
6,682,528	B2	1/2004	Frazier et al.	7,210,609	B2 *	5/2007	Leiboff et al. 227/180.1
6,695,199	B2	2/2004	Whitman	7,225,964	B2	6/2007	Mastri et al.
6,698,643	B2	3/2004	Whitman	7,246,734	B2	7/2007	Shelton, IV
6,704,210	B1	3/2004	Myers	7,258,262	B2	8/2007	Mastri et al.
6,716,223	B2	4/2004	Leopold et al.	7,296,724	B2	11/2007	Green et al.
6,716,233	B1	4/2004	Whitman	7,328,829	B2	2/2008	Arad et al.
6,747,121	B2	6/2004	Gogolewski	7,398,908	B2	7/2008	Holsten et al.
6,755,338	B2	6/2004	Hahnen et al.	7,431,188	B1	10/2008	Marczyk
6,767,356	B2	7/2004	Kanner et al.	7,490,749	B2	2/2009	Schall et al.
6,773,438	B1	8/2004	Knodel et al.	7,494,039	B2	2/2009	Racenet et al.
6,786,382	B1	9/2004	Hoffman	7,506,790	B2	3/2009	Shelton, IV
6,793,652	B1	9/2004	Whitman et al.	7,510,107	B2	3/2009	Timm et al.
6,805,273	B2	10/2004	Bilotti et al.	2002/0117534	A1	8/2002	Green et al.
6,817,508	B1	11/2004	Racenet et al.	2002/0165541	A1	11/2002	Whitman
6,817,509	B2	11/2004	Geiste et al.	2003/0216778	A1	11/2003	Weadock
6,830,174	B2	12/2004	Hillstead et al.	2003/0220660	A1	11/2003	Kortenbach et al.
6,843,403	B2	1/2005	Whitman	2004/0002726	A1	1/2004	Nunez et al.

US 7,665,647 B2

Page 5

2004/0006372	A1	1/2004	Racenet et al.	2006/0291981	A1	12/2006	Viola et al.
2004/0028502	A1	2/2004	Cummins	2007/0023477	A1	2/2007	Whitman et al.
2004/0034357	A1	2/2004	Beane et al.	2007/0034666	A1	2/2007	Holsten et al.
2004/0034369	A1	2/2004	Sauer et al.	2007/0034668	A1	2/2007	Holsten et al.
2004/0044364	A1	3/2004	DeVries et al.	2007/0045379	A1	3/2007	Shelton, IV
2004/0094597	A1	5/2004	Whitman et al.	2007/0073340	A1	3/2007	Shelton, IV et al.
2004/0097987	A1	5/2004	Pugsley et al.	2007/0075114	A1	4/2007	Shelton, IV et al.
2004/0101822	A1	5/2004	Wiesner et al.	2007/0083234	A1	4/2007	Shelton, IV et al.
2004/0108357	A1	6/2004	Milliman et al.	2007/0084897	A1	4/2007	Shelton, IV et al.
2004/0111081	A1	6/2004	Whitman et al.	2007/0102452	A1	5/2007	Shelton, IV et al.
2004/0122471	A1	6/2004	Toby et al.	2007/0102453	A1	5/2007	Morgan et al.
2004/0164123	A1	8/2004	Racenet et al.	2007/0102472	A1	5/2007	Shelton, IV
2004/0167572	A1	8/2004	Roth et al.	2007/0102473	A1	5/2007	Shelton, IV et al.
2004/0173659	A1	9/2004	Green et al.	2007/0102474	A1	5/2007	Shelton, IV et al.
2004/0222268	A1	11/2004	Bilotti et al.	2007/0102475	A1	5/2007	Ortiz et al.
2004/0232199	A1	11/2004	Shelton, IV et al.	2007/0102476	A1	5/2007	Shelton, IV et al.
2004/0232201	A1	11/2004	Wenchell et al.	2007/0106317	A1	5/2007	Shelton, IV et al.
2004/0243151	A1	12/2004	Demmy et al.	2007/0114261	A1	5/2007	Ortiz et al.
2004/0243176	A1	12/2004	Hahnen et al.	2007/0158385	A1	7/2007	Hueil et al.
2004/0254608	A1	12/2004	Huitema et al.	2007/0170225	A1	7/2007	Shelton, IV et al.
2005/0006434	A1	1/2005	Wales et al.	2007/0175949	A1	8/2007	Shelton, IV et al.
2005/0021026	A1	1/2005	Baily	2007/0175950	A1	8/2007	Shelton, IV et al.
2005/0023324	A1	2/2005	Doll et al.	2007/0175951	A1	8/2007	Shelton, IV et al.
2005/0059997	A1	3/2005	Bauman et al.	2007/0175952	A1	8/2007	Shelton, IV et al.
2005/0070929	A1	3/2005	Dalessandro et al.	2007/0175953	A1	8/2007	Shelton, IV et al.
2005/0070958	A1	3/2005	Swayze et al.	2007/0175955	A1	8/2007	Shelton, IV et al.
2005/0072827	A1	4/2005	Mollenauer	2007/0175956	A1	8/2007	Swayze et al.
2005/0080454	A1	4/2005	Drews et al.	2007/0175957	A1	8/2007	Shelton, IV et al.
2005/0103819	A1	5/2005	Racenet et al.	2007/0175958	A1	8/2007	Shelton, IV et al.
2005/0107824	A1	5/2005	Hillstead et al.	2007/0175959	A1	8/2007	Shelton, IV et al.
2005/0119669	A1	6/2005	Demmy	2007/0175960	A1	8/2007	Shelton, IV et al.
2005/0125009	A1	6/2005	Perry et al.	2007/0175961	A1	8/2007	Shelton, IV et al.
2005/0131390	A1	6/2005	Heinrich et al.	2007/0175962	A1	8/2007	Shelton, IV et al.
2005/0143759	A1	6/2005	Kelly	2007/0175964	A1	8/2007	Shelton, IV et al.
2005/0145671	A1	7/2005	Viola	2007/0179476	A1	8/2007	Shelton, IV et al.
2005/0165415	A1	7/2005	Wales	2007/0181632	A1	8/2007	Milliman
2005/0169974	A1	8/2005	Tenerz et al.	2007/0194079	A1	8/2007	Hueil et al.
2005/0173490	A1	8/2005	Shelton, IV	2007/0194080	A1	8/2007	Swayze et al.
2005/0184121	A1	8/2005	Heinrich	2007/0194081	A1	8/2007	Hueil et al.
2005/0187576	A1	8/2005	Whitman et al.	2007/0194082	A1	8/2007	Morgan et al.
2005/0189397	A1	9/2005	Jankowski	2007/0213750	A1	9/2007	Weadock
2005/0203550	A1	9/2005	Laufer et al.	2007/0233053	A1	10/2007	Shelton, IV et al.
2005/0216055	A1	9/2005	Scirica et al.	2007/0262116	A1	11/2007	Hueil et al.
2005/0230453	A1	10/2005	Viola	2007/0295780	A1	12/2007	Shelton et al.
2005/0245965	A1	11/2005	Orban, III et al.	2008/0029570	A1	2/2008	Shelton et al.
2005/0263562	A1	12/2005	Shelton, IV et al.	2008/0029571	A1	2/2008	Shelton et al.
2005/0263563	A1	12/2005	Racenet et al.	2008/0029572	A1	2/2008	Shelton et al.
2005/0274768	A1	12/2005	Cummins et al.	2008/0029573	A1	2/2008	Shelton et al.
2006/0011699	A1	1/2006	Olson et al.	2008/0029574	A1	2/2008	Shelton et al.
2006/0025813	A1	2/2006	Shelton et al.	2008/0029575	A1	2/2008	Shelton et al.
2006/0025816	A1	2/2006	Shelton	2008/0029576	A1	2/2008	Shelton et al.
2006/0047307	A1	3/2006	Ortiz et al.	2008/0029577	A1	2/2008	Shelton et al.
2006/0047308	A1	3/2006	Ortiz et al.	2008/0035701	A1	2/2008	Racenet et al.
2006/0049229	A1	3/2006	Milliman et al.	2008/0041917	A1	2/2008	Racenet et al.
2006/0052825	A1	3/2006	Ransick et al.	2008/0078800	A1	4/2008	Hess et al.
2006/0060630	A1	3/2006	Shelton, IV et al.	2008/0078802	A1	4/2008	Hess et al.
2006/0085033	A1	4/2006	Criscuolo et al.	2008/0078803	A1	4/2008	Shelton et al.
2006/0097026	A1	5/2006	Shelton, IV	2008/0078804	A1	4/2008	Shelton et al.
2006/0100643	A1	5/2006	Laufer et al.	2008/0078805	A1	4/2008	Omaits et al.
2006/0108393	A1	5/2006	Heinrich et al.	2008/0078806	A1	4/2008	Omaits et al.
2006/0122636	A1	6/2006	Bailley et al.	2008/0078807	A1	4/2008	Hess et al.
2006/0142772	A1	6/2006	Ralph et al.	2008/0078808	A1	4/2008	Hess et al.
2006/0151567	A1	7/2006	Roy	2008/0082115	A1	4/2008	Morgan et al.
2006/0173470	A1	8/2006	Oray et al.	2008/0082124	A1	4/2008	Hess et al.
2006/0180634	A1	8/2006	Shelton, IV et al.	2008/0082125	A1	4/2008	Murray et al.
2006/0183246	A1	8/2006	Wiesner et al.	2008/0082126	A1	4/2008	Murray et al.
2006/0190028	A1	8/2006	Wales et al.	2008/0083813	A1	4/2008	Zemlok et al.
2006/0226196	A1	10/2006	Hueil et al.	2008/0164296	A1	7/2008	Shelton et al.
2006/0245971	A1	11/2006	Burns et al.	2008/0167522	A1	7/2008	Giordano et al.
2006/0273135	A1	12/2006	Beetel	2008/0167644	A1	7/2008	Shelton et al.
2006/0278680	A1	12/2006	Viola et al.	2008/0167670	A1	7/2008	Shelton et al.
2006/0278681	A1	12/2006	Viola et al.	2008/0167671	A1	7/2008	Giordano et al.
2006/0289602	A1	12/2006	Wales et al.	2008/0167672	A1	7/2008	Giordano et al.

2008/0167736	A1	7/2008	Swayze et al.	EP	0484677	B2	6/1996
2008/0169327	A1	7/2008	Shelton et al.	EP	0541987	B1	7/1996
2008/0169328	A1	7/2008	Shelton	EP	0667119	B1	7/1996
2008/0169329	A1	7/2008	Shelton et al.	EP	0770355	A1	5/1997
2008/0169330	A1	7/2008	Shelton et al.	EP	0503662	B1	6/1997
2008/0169331	A1	7/2008	Shelton et al.	EP	0625335	B1	11/1997
2008/0169332	A1	7/2008	Shelton et al.	EP	0552423	B1	1/1998
2008/0169333	A1	7/2008	Shelton et al.	EP	0592244	B1	1/1998
2008/0210738	A1	9/2008	Shelton et al.	EP	0648476	B1	1/1998
2008/0237296	A1	10/2008	Boudreaux et al.	EP	0603472	B1	11/1998
2008/0237298	A1	10/2008	Schall et al.	EP	0605351	B1	11/1998
2008/0296343	A1	12/2008	Schall et al.	EP	0878169	A1	11/1998
2008/0296345	A1	12/2008	Shelton, IV et al.	EP	0879742	A1	11/1998
2008/0296346	A1	12/2008	Shelton, IV et al.	EP	0760230	B1	2/1999
2008/0296347	A1	12/2008	Shelton, IV et al.	EP	0537572	B1	6/1999
2008/0300579	A1	12/2008	Broehl et al.	EP	0552050	B1	5/2000
2008/0300580	A1	12/2008	Shelton, IV et al.	EP	1090592	A1	4/2001
2008/0300613	A1	12/2008	Shelton, IV et al.	EP	1256318	B1	5/2001
2008/0308601	A1	12/2008	Timm et al.	EP	0908152	B1	1/2002
2008/0308602	A1	12/2008	Timm et al.	EP	0872213	B1	5/2002
2008/0308603	A1	12/2008	Shelton, IV et al.	EP	1238634	A2	9/2002
2008/0308604	A1	12/2008	Timm et al.	EP	0656188	B1	1/2003
2008/0308606	A1	12/2008	Timm et al.	EP	0829235	B1	6/2003
2008/0308607	A1	12/2008	Timm et al.	EP	0813843	B1	10/2003
2008/0314954	A1	12/2008	Boudreaux	EP	0741996	B1	2/2004
2008/0314955	A1	12/2008	Boudreaux et al.	EP	0705570	B1	4/2004
2008/0314956	A1	12/2008	Boudreaux	EP	1086713	B1	5/2004
2008/0314957	A1	12/2008	Boudreaux	EP	1426012	A1	6/2004
2008/0314961	A1	12/2008	Boudreaux et al.	EP	0888749	B1	9/2004
2008/0314962	A1	12/2008	Boudreaux	EP	1477119	A1	11/2004
2009/0001121	A1	1/2009	Hess et al.	EP	1479345	A1	11/2004
2009/0001123	A1	1/2009	Morgan et al.	EP	1479347	A1	11/2004
2009/0001124	A1	1/2009	Hess et al.	EP	1479348	A1	11/2004
2009/0001125	A1	1/2009	Hess et al.	EP	1520521	A1	4/2005
2009/0001126	A1	1/2009	Hess et al.	EP	1520523	A1	4/2005
2009/0001128	A1	1/2009	Weisenburgh, II et al.	EP	1520525	A1	4/2005
2009/0001130	A1	1/2009	Hess et al.	EP	1522264	A1	4/2005
2009/0005807	A1	1/2009	Hess et al.	EP	1550408	A1	7/2005
2009/0005808	A1	1/2009	Hess et al.	EP	1557129	A1	7/2005
2009/0005809	A1	1/2009	Hess et al.	EP	1064883	B1	8/2005
2009/0012556	A1	1/2009	Boudreaux et al.	EP	1157666	B1	9/2005
2009/0076534	A1	3/2009	Shelton, IV et al.	EP	1621138	A2	2/2006
2009/0200355	A1	8/2009	Baxter, III et al.	EP	1621141	A2	2/2006

FOREIGN PATENT DOCUMENTS

CA	2512960	A1	1/2006	EP	1382303	B1	6/2006
CA	2514274	A1	1/2006	EP	1045672	B1	8/2006
DE	273689	C	5/1914	EP	1617768	B1	8/2006
DE	1775926	A	1/1972	EP	1702567	A2	9/2006
DE	9412228	U	9/1994	EP	1129665	B1	11/2006
DE	19924311	A1	11/2000	EP	1256317	B1	12/2006
DE	69328576	T2	1/2001	EP	1728473	A1	12/2006
DE	20112837	U1	10/2001	EP	1728475	A2	12/2006
DE	20121753	U1	4/2003	EP	1479346	B1	1/2007
DE	10314072	A1	10/2004	EP	1484024	B1	1/2007
EP	0122046	A1	10/1984	EP	1754445	A2	2/2007
EP	0033548	B1	5/1986	EP	1759812	A1	3/2007
EP	0276104	A2	7/1988	EP	1300117	B1	8/2007
EP	0639349	A2	2/1994	EP	1813199	A1	8/2007
EP	0593920	A1	4/1994	EP	1813207	A1	8/2007
EP	0600182	A2	6/1994	EP	1872727	A1	1/2008
EP	0630612	A1	12/1994	EP	1839596	A2	2/2008
EP	0634144	A1	1/1995	EP	1897502	A1	3/2008
EP	0646356	A2	4/1995	EP	1749486	B1	3/2009
EP	0646357	A1	4/1995	FR	999646	A	2/1952
EP	0669104	A1	8/1995	FR	1112936	A	3/1956
EP	0679367	A2	11/1995	FR	2765794	A	1/1999
EP	0392547	B1	12/1995	GB	939929	A	10/1963
EP	0685204	A1	12/1995	GB	2336214	A	10/1999
EP	0699418	A1	3/1996	JP	6007357	A	1/1994
EP	0702937	A1	3/1996	JP	7051273	A	2/1995
EP	0705571	A1	4/1996	JP	8033641	A	2/1996
				JP	8229050	A	9/1996

JP	2000287987	A	10/2000	WO	WO 03/077769	A1	9/2003
JP	2001286477	A	10/2001	WO	WO 03/082126	A1	10/2003
JP	2002369820	A	12/2002	WO	WO 03/088845	A2	10/2003
JP	2005505322	T	2/2005	WO	WO 03/090630	A2	11/2003
JP	2005103293	A	4/2005	WO	WO 03/094743	A1	11/2003
RU	2187249	C2	8/2002	WO	WO 03/094745	A1	11/2003
RU	2225170	C2	3/2004	WO	WO 03/094746	A1	11/2003
SU	1377053	A1	2/1988	WO	WO 03/094747	A1	11/2003
SU	1561964	A1	5/1990	WO	WO 03/101313	A1	12/2003
SU	1722476	A1	3/1992	WO	WO 03/105698	A2	12/2003
WO	WO 93/08755	A1	5/1993	WO	WO 03/105702	A2	12/2003
WO	WO 95/18572	A1	7/1995	WO	WO 2004/006980	A2	1/2004
WO	WO 95/23557	A1	9/1995	WO	WO 2004/028585	A2	4/2004
WO	WO 95/29639	A1	11/1995	WO	WO 2004/032754	A2	4/2004
WO	WO 96/35464	A1	11/1996	WO	WO 2004/032760	A2	4/2004
WO	WO 97/34533	A1	9/1997	WO	WO 2004/032762	A1	4/2004
WO	WO 98/30153	A1	7/1998	WO	WO 2004/032763		4/2004
WO	WO 99/12483	A1	3/1999	WO	WO 2004/047653	A2	6/2004
WO	WO 99/15086	A1	4/1999	WO	WO 2004/049956	A2	6/2004
WO	WO 99/34744	A1	7/1999	WO	WO 2004/086987	A1	10/2004
WO	WO 99/45849	A1	9/1999	WO	WO 2004/096057	A2	11/2004
WO	WO 00/57796	A1	10/2000	WO	WO 2004/112618	A2	12/2004
WO	WO 00/64365	A1	11/2000	WO	WO 2004/112652	A2	12/2004
WO	WO 00/72762	A1	12/2000	WO	WO 2005/027983	A2	3/2005
WO	WO 00/72765	A1	12/2000	WO	WO 2005/037329	A2	4/2005
WO	WO 01/05702	A1	1/2001	WO	WO 2005/096954	A2	10/2005
WO	WO 01/10482	A1	2/2001	WO	WO 2005/115251	A2	12/2005
WO	WO 01/54594	A1	8/2001	WO	WO 2006/044490	A2	4/2006
WO	WO 01/62158	A2	8/2001	WO	WO 2006/044581	A2	4/2006
WO	WO 01/62162	A1	8/2001	WO	WO 2006/044810	A2	4/2006
WO	WO 01/62164	A2	8/2001	WO	WO 2006/083748	A1	8/2006
WO	WO 01/91646	A1	12/2001	WO	WO 2006/132992	A1	12/2006
WO	WO 02/07618	A1	1/2002	WO	WO 2007/016290	A2	2/2007
WO	WO 02/17799	A1	3/2002	WO	WO 2007/121579	A1	11/2007
WO	WO 02/19920	A1	3/2002	WO	WO 2007/142625	A2	12/2007
WO	WO 02/30297	A2	4/2002	WO	WO 2008/045383	A2	4/2008
WO	WO 02/32322	A2	4/2002				
WO	WO 02/43571	A2	6/2002				
WO	WO 02/058568	A1	8/2002				
WO	WO 02/067785	A2	9/2002				
WO	WO 02/098302	A1	12/2002				
WO	WO 03/000138	A2	1/2003				
WO	WO 03/001329	A2	1/2003				
WO	WO 03/013363	A1	2/2003				
WO	WO 03/020106	A2	3/2003				
WO	WO 03/079909	A3	3/2003				
WO	WO 03/030743	A2	4/2003				
WO	WO 03/037193	A1	5/2003				
WO	WO 03/047436	A3	6/2003				
WO	WO 03/057048	A1	7/2003				
WO	WO 03/057058	A1	7/2003				
WO	WO 03/063694	A1	8/2003				

OTHER PUBLICATIONS

C.C. Thompson et al., "Peroral Endoscopic Reduction of Dilated Gastrojejunal Anastomosis After Roux-en-Y Gastric Bypass: A Possible New Option for Patients with Weight Regain," *Surg Endosc* (2006) vol. 20, pp. 1744-1748.

B.R. Coolman, DVM, MS et al., "Comparison of Skin Staples With Sutures for Anastomosis of the Small Intestine in Dogs," Abstract; <http://www.blackwell-synergy.com/doi/abs/10.1053/jvet.2000.7539?cookieSet=1&journalCode=vsu> which redirects to <http://www3.interscience.wiley.com/journal/119040681/abstract?CRETRY=1&SRETRY=0>; [online] accessed: Sep. 22, 2008 (2 pages).

* cited by examiner

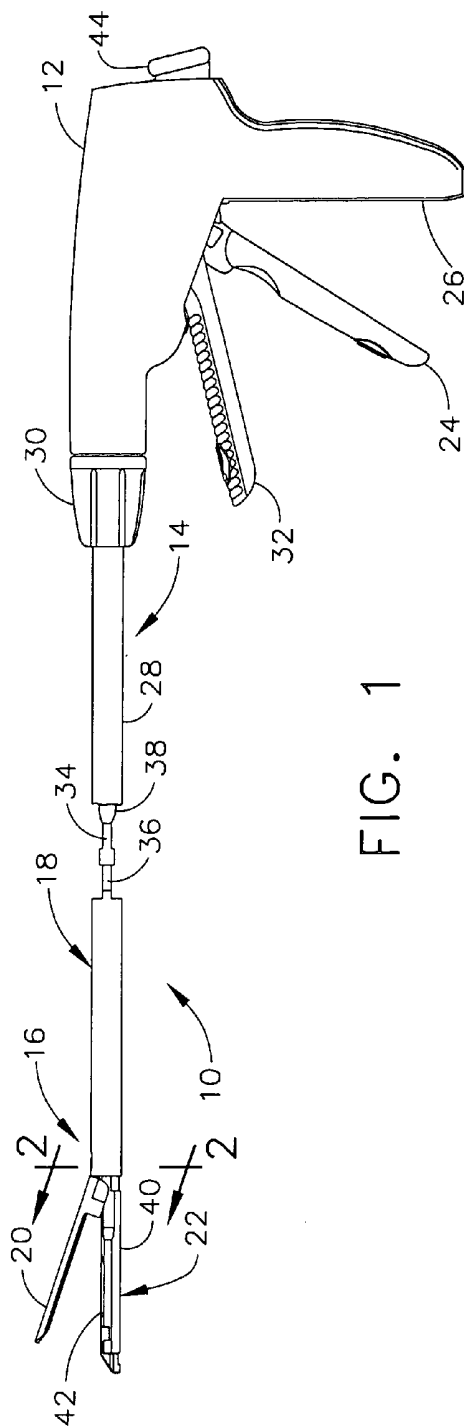


FIG. 1

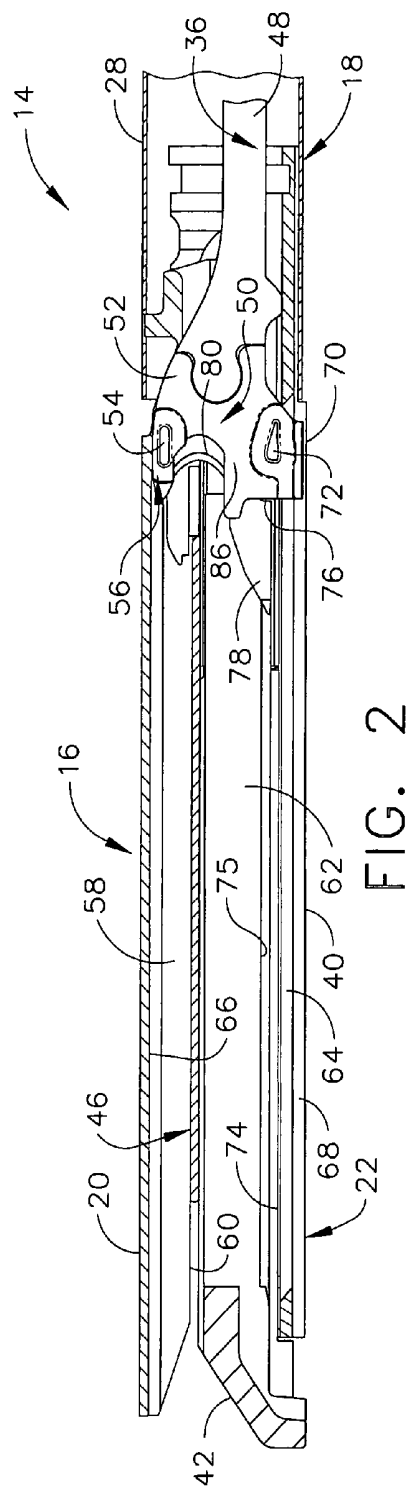


FIG. 2

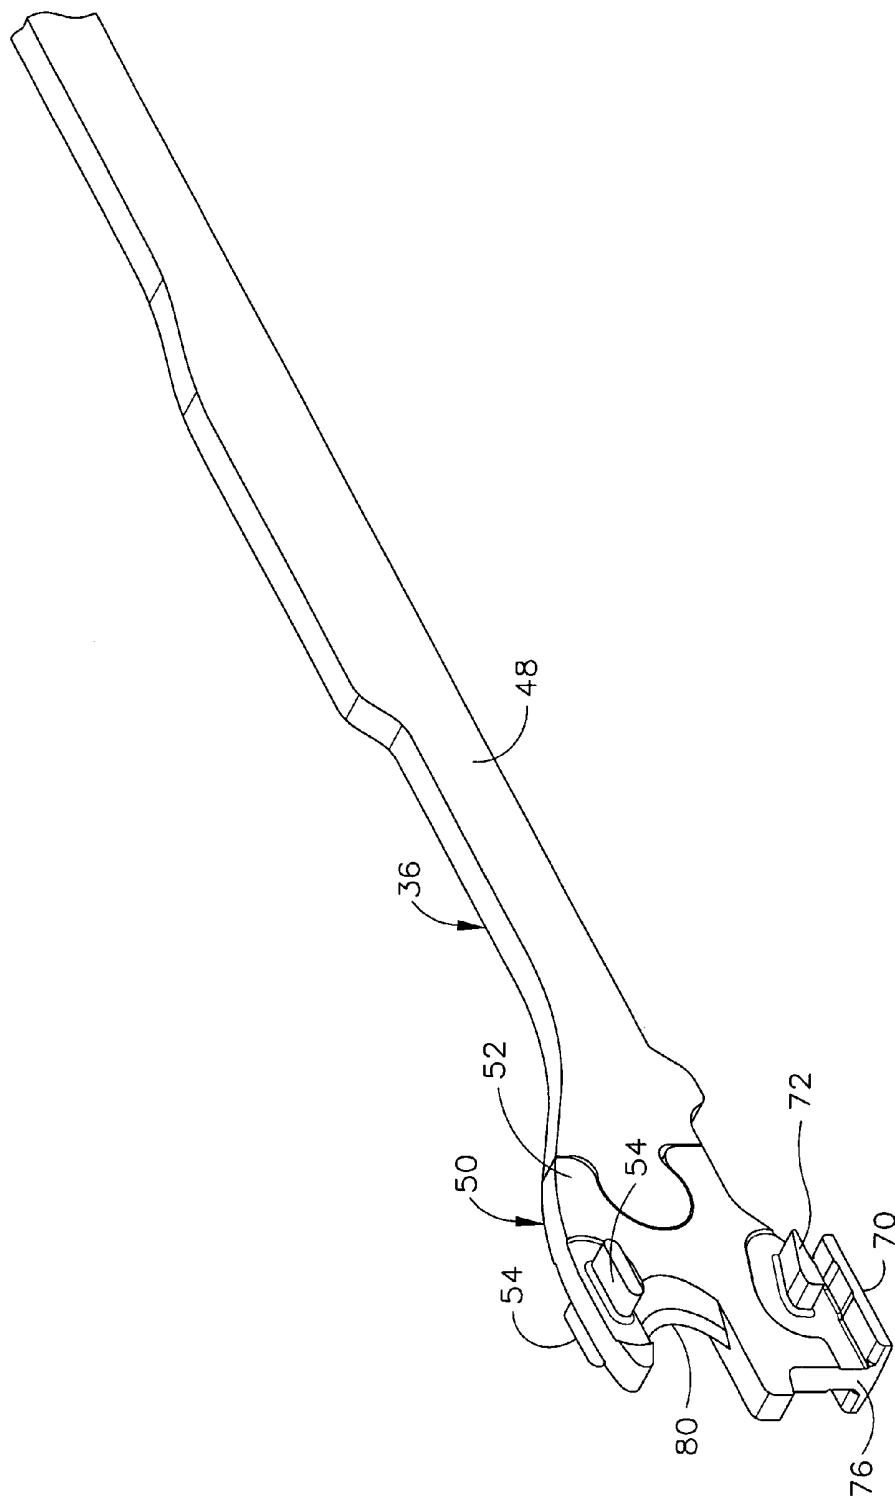


FIG. 3

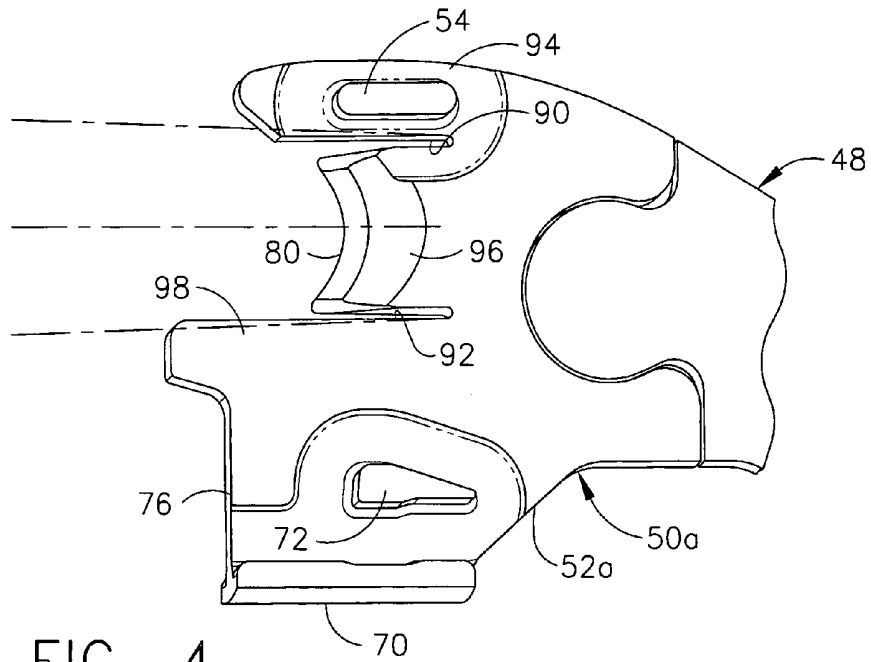


FIG. 4

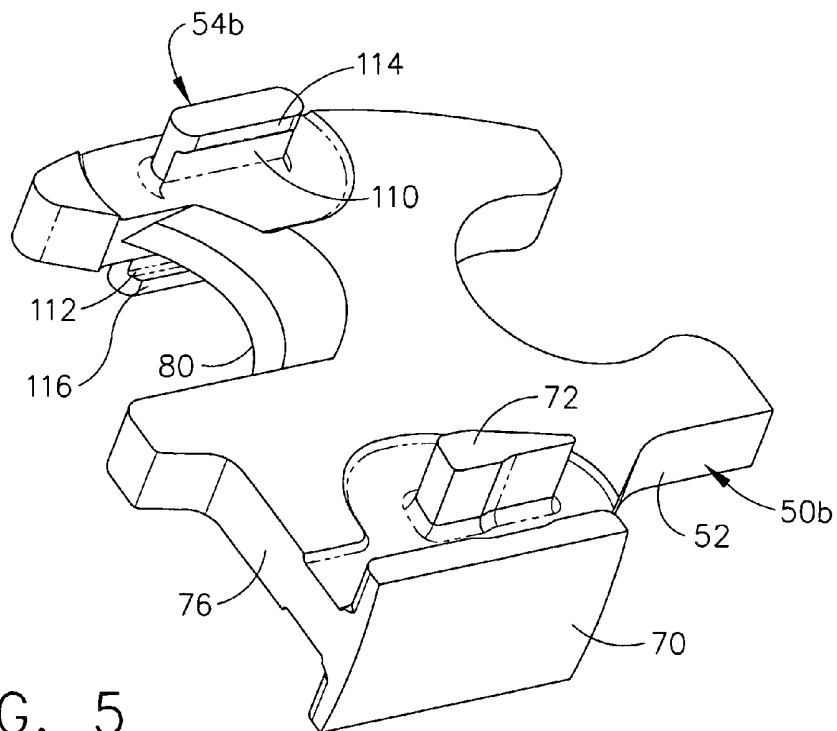


FIG. 5

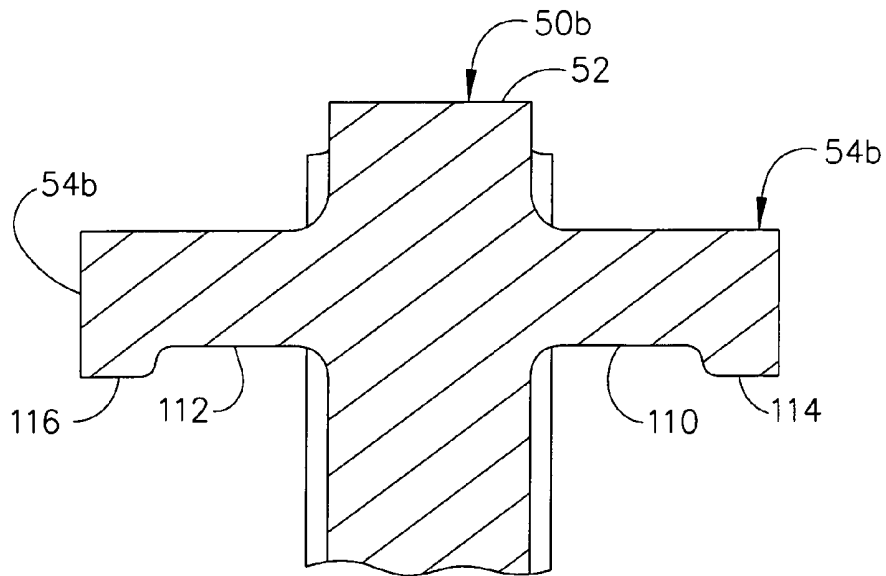


FIG. 6

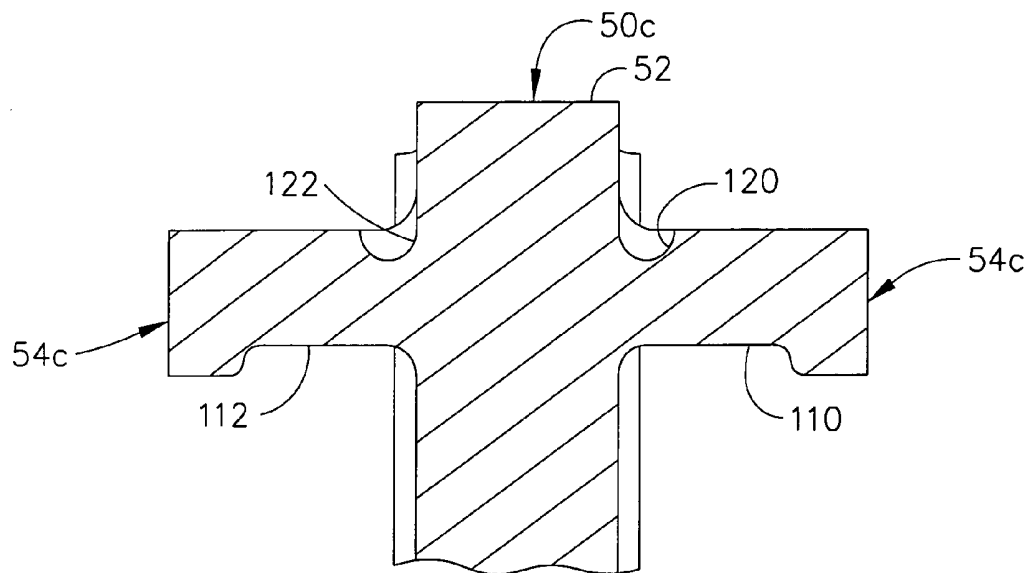


FIG. 7

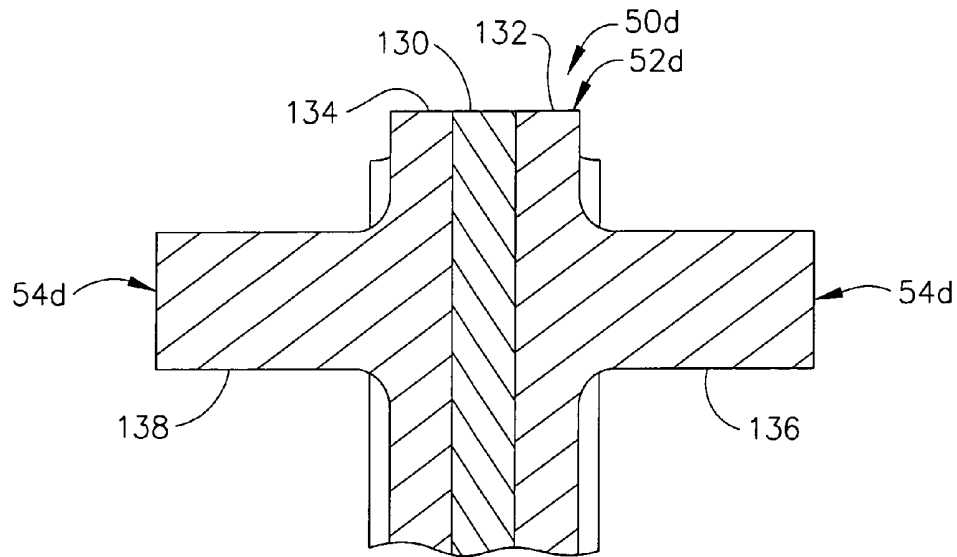


FIG. 8

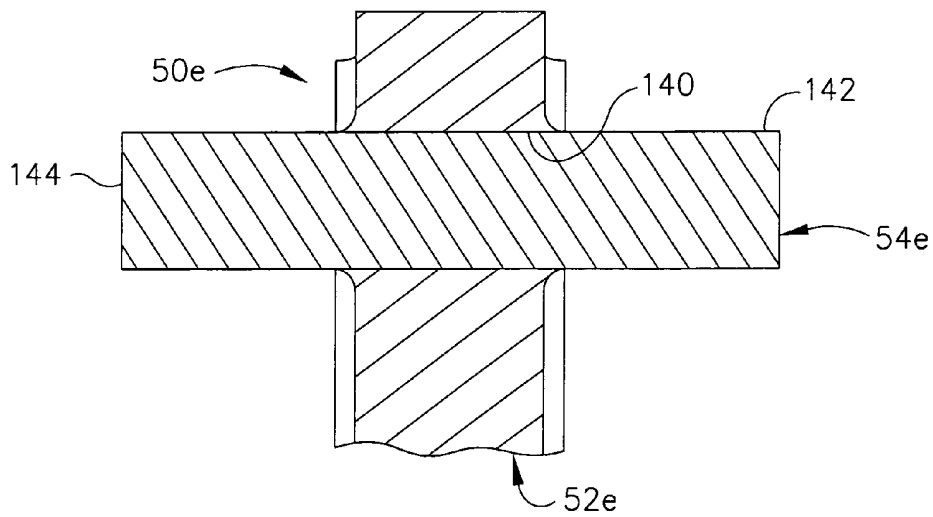


FIG. 9

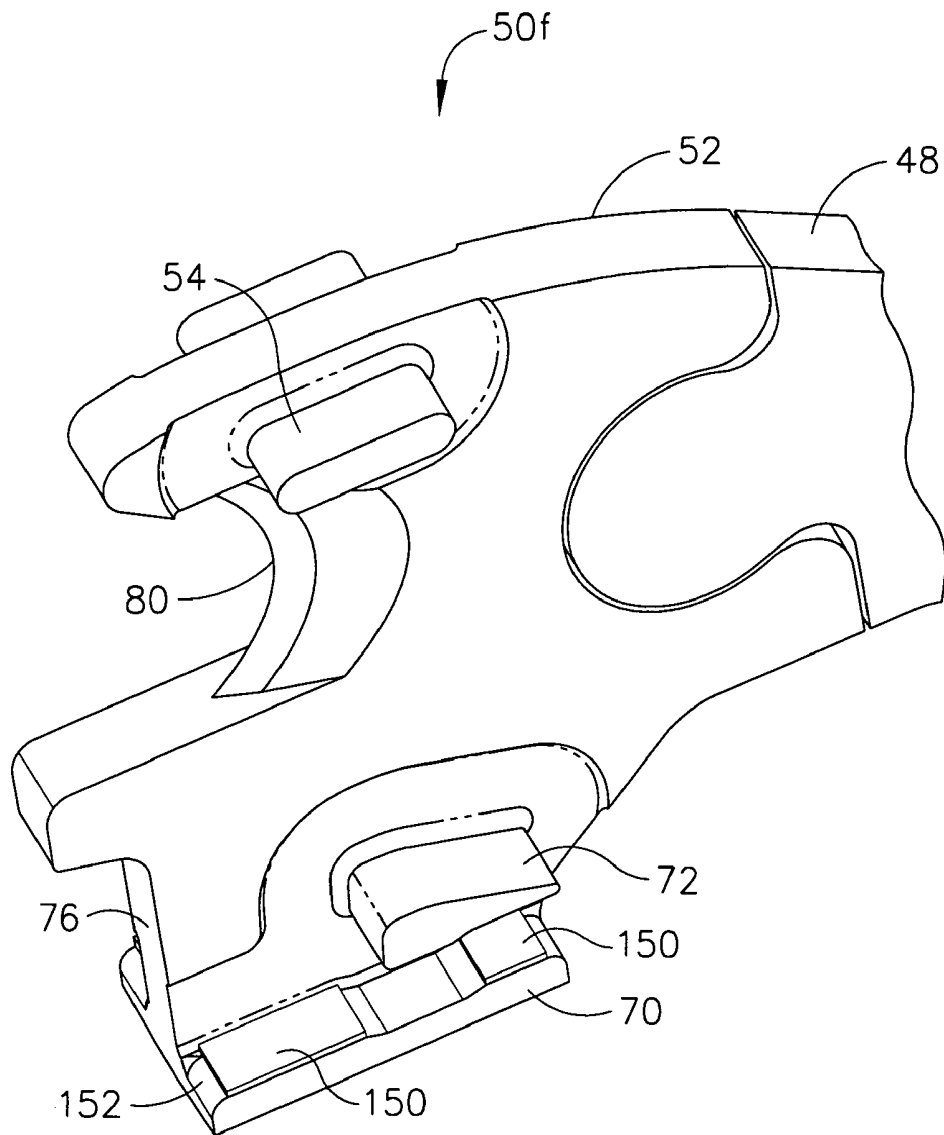


FIG. 10

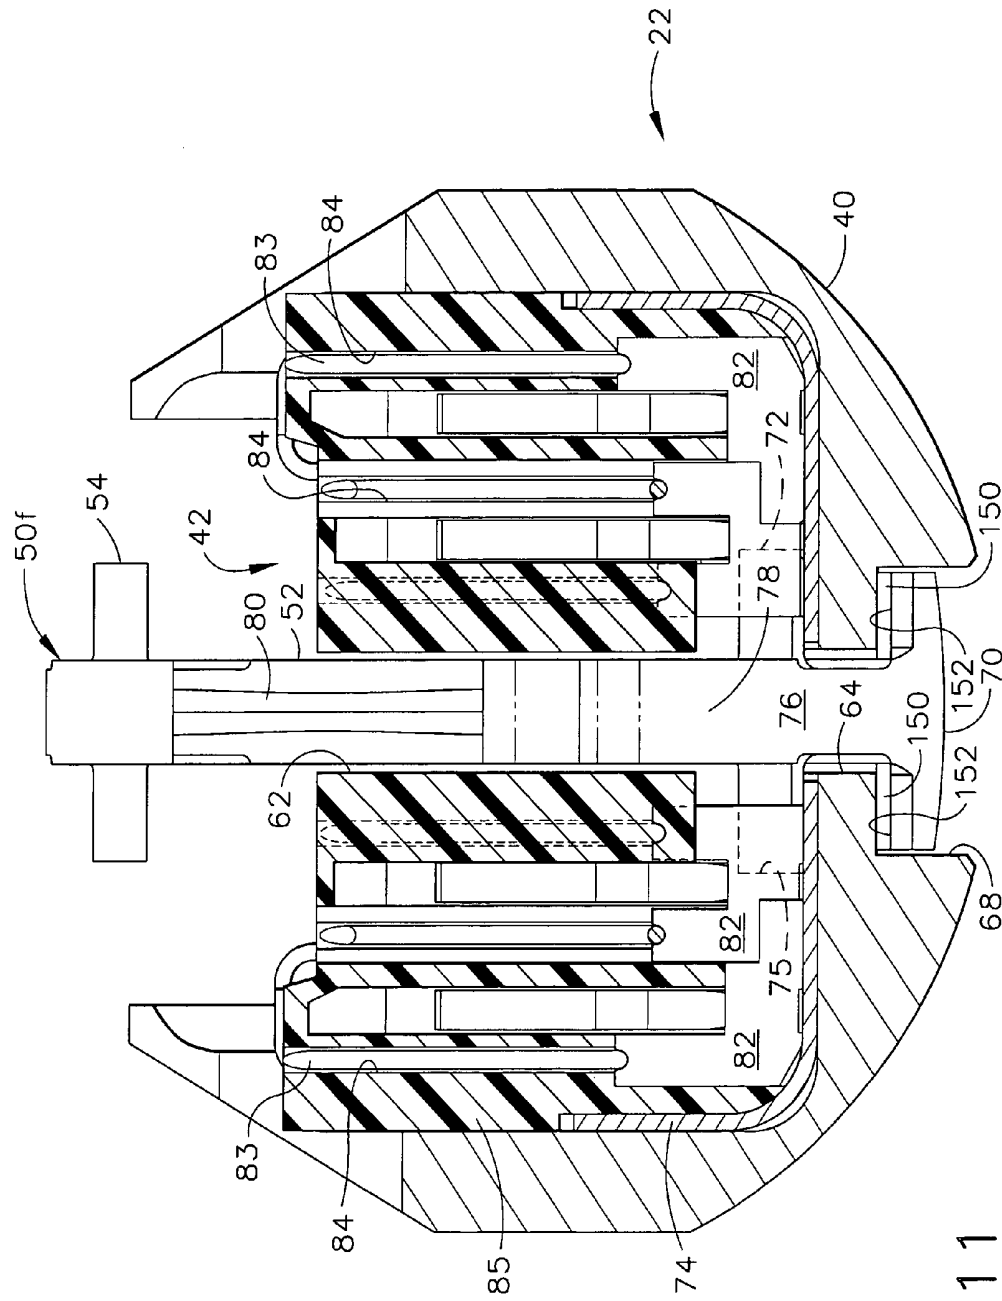


FIG. 11

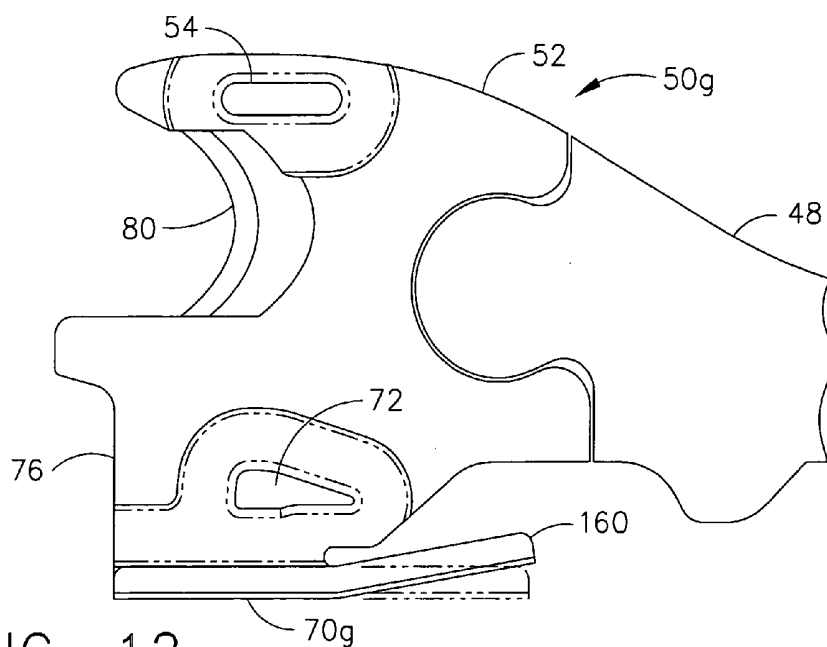


FIG. 12

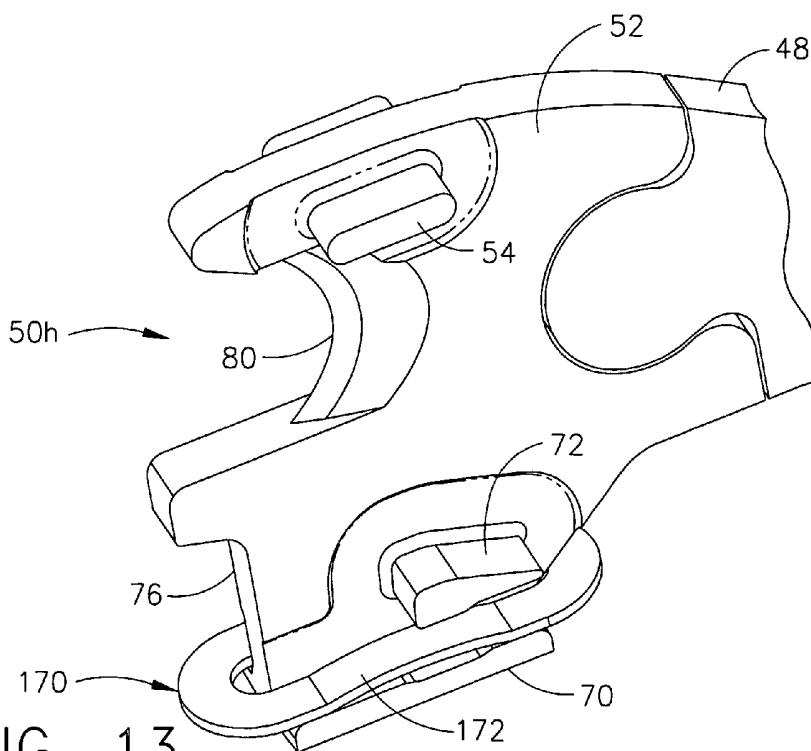


FIG. 13

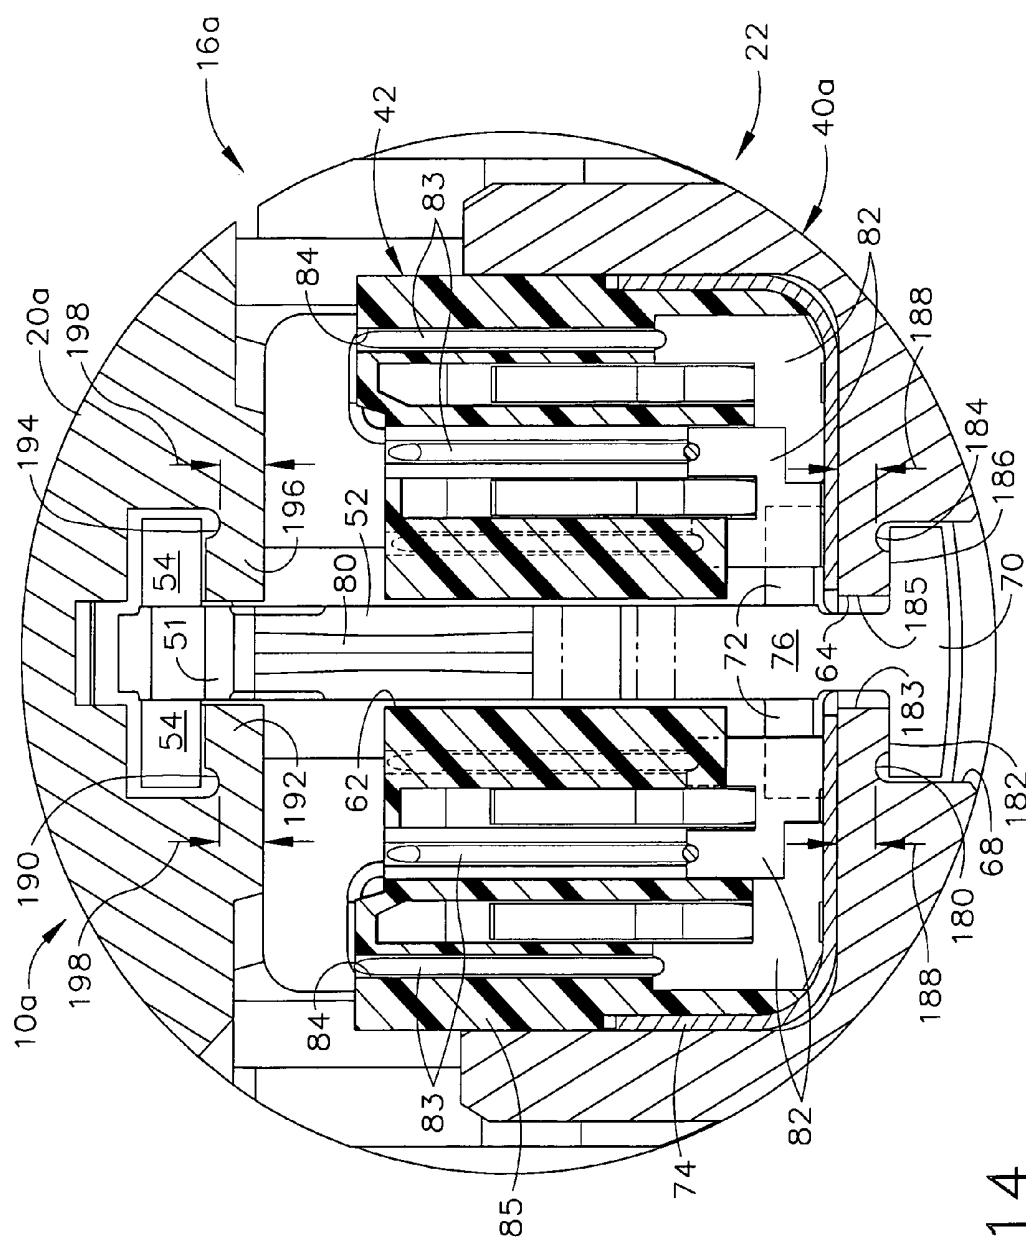


FIG. 14

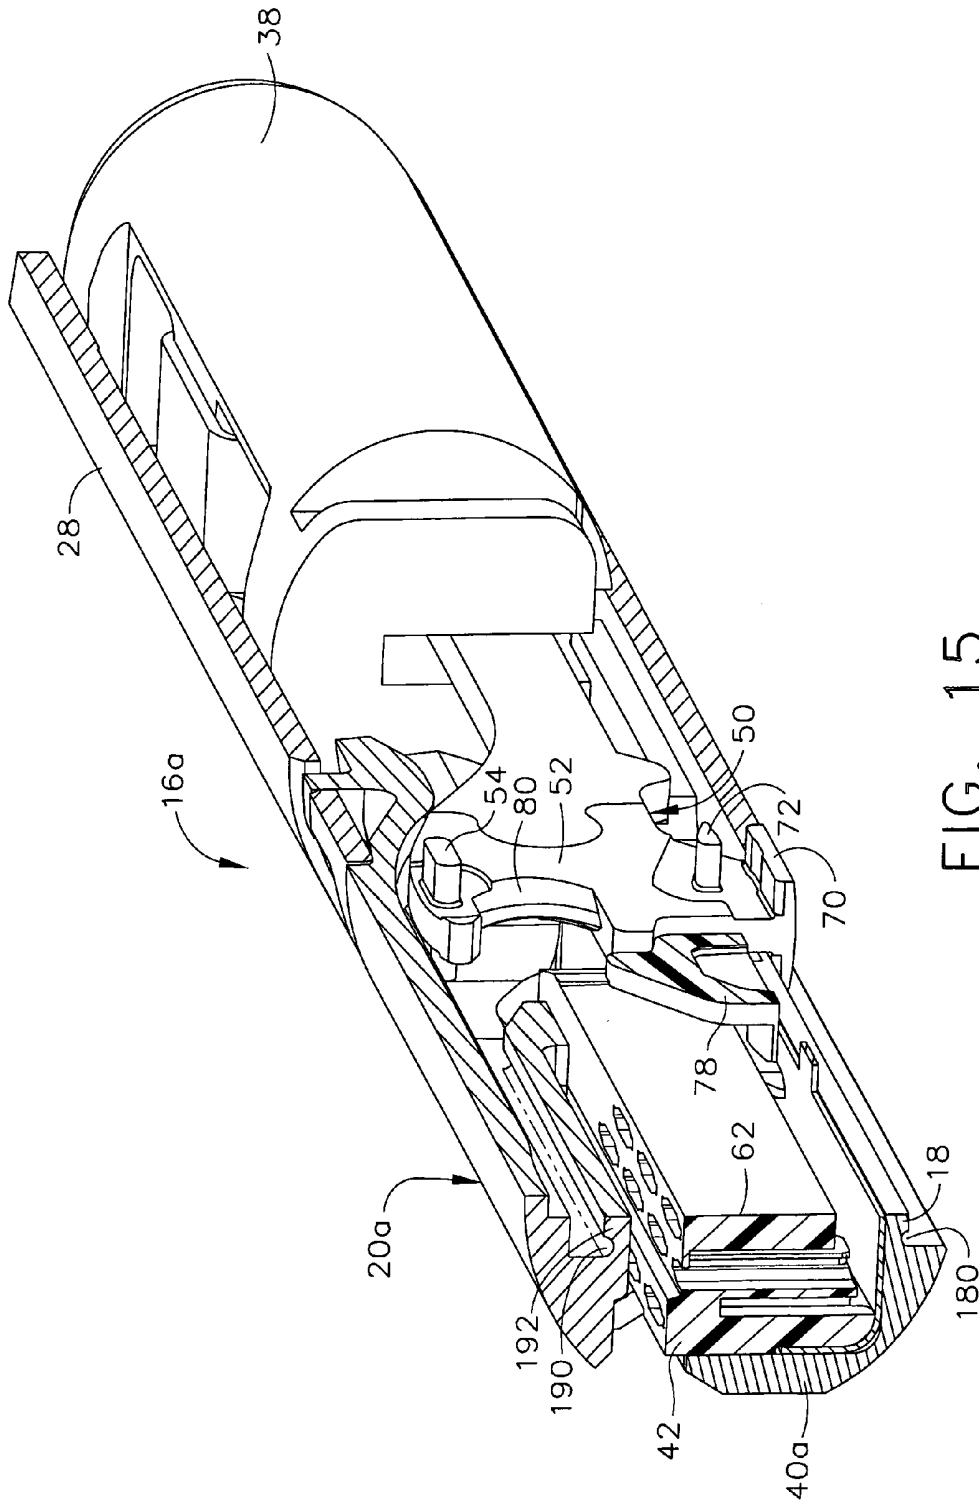


FIG. 15

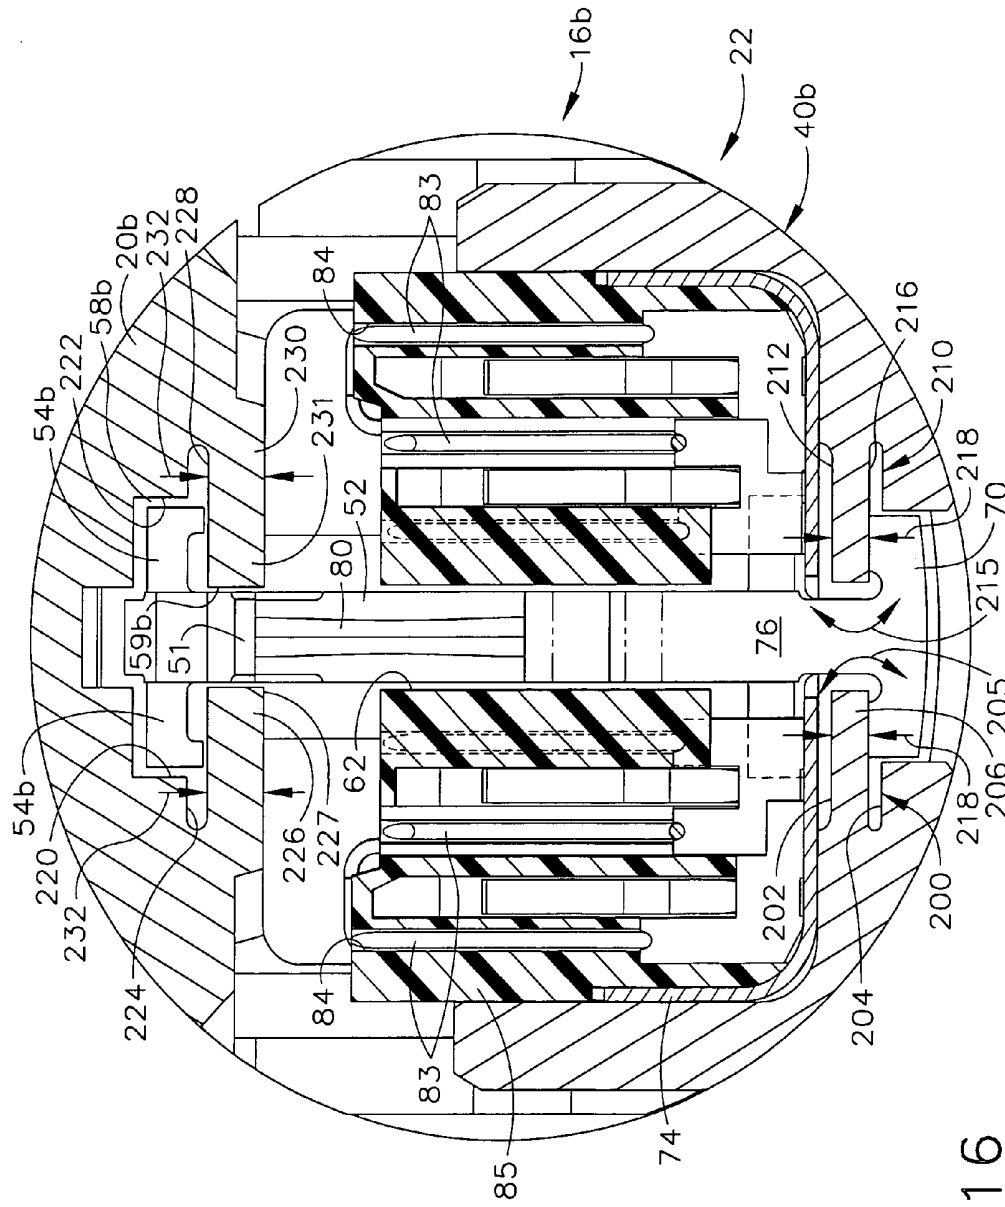


FIG. 16

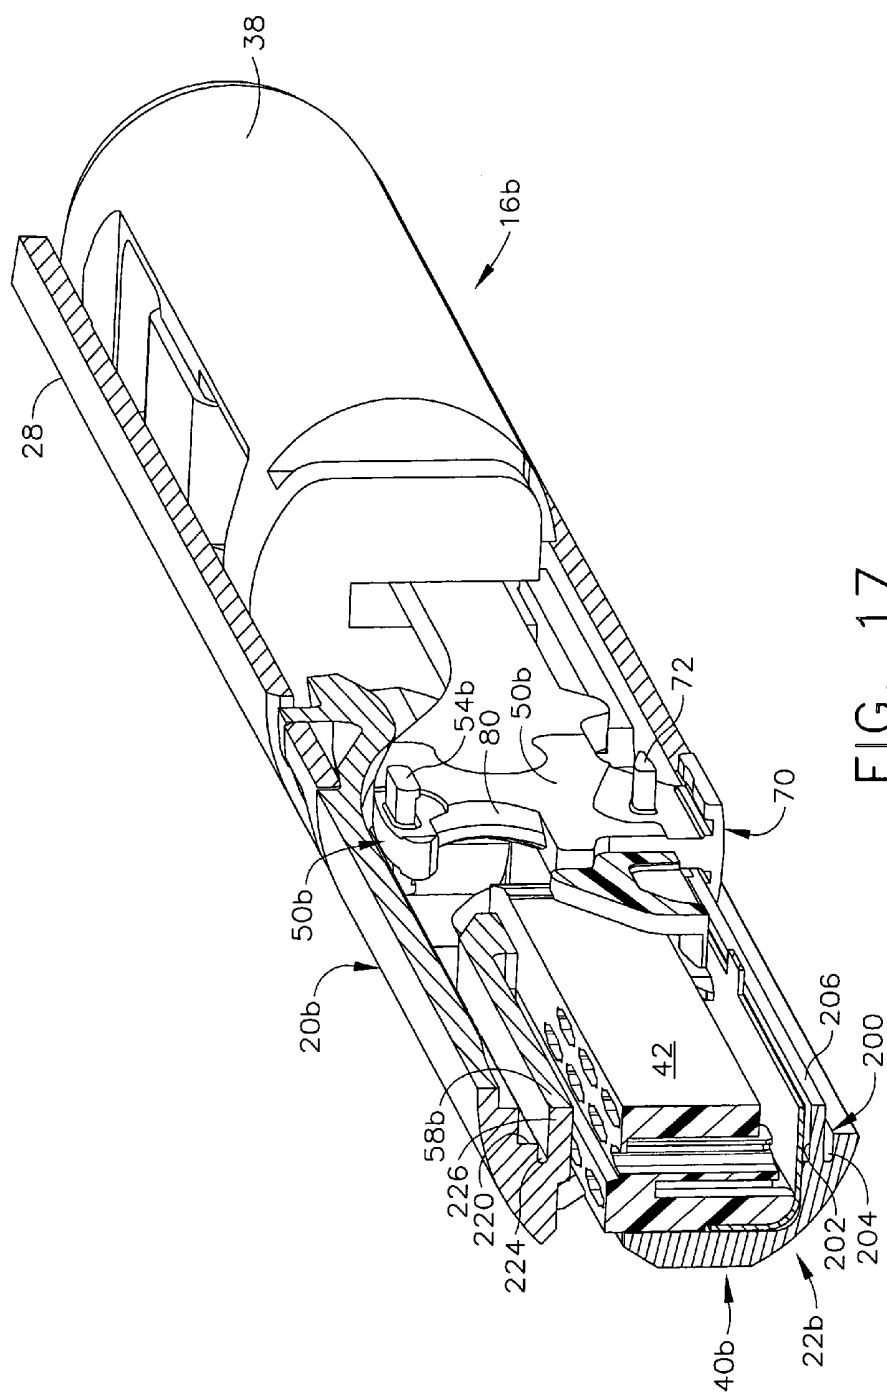


FIG. 17

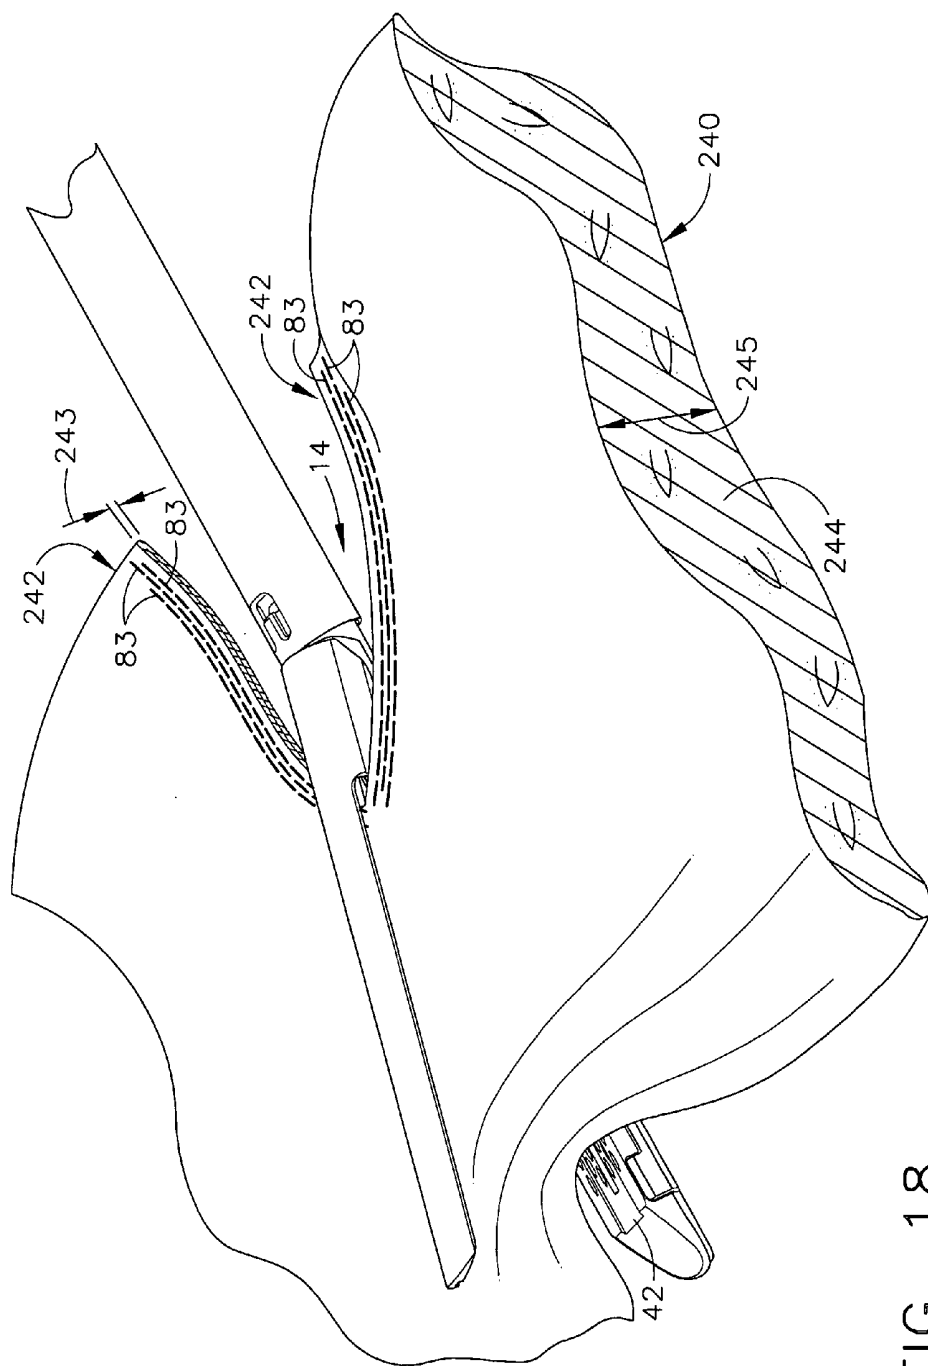


FIG. 18

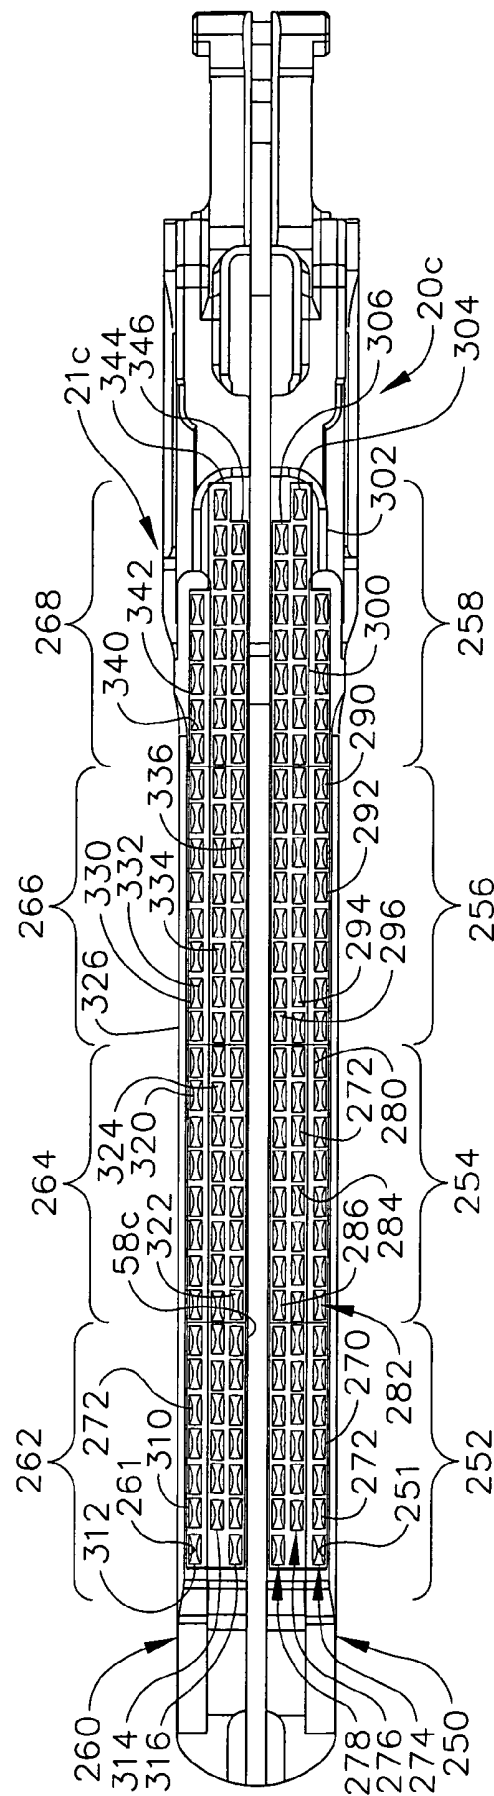


FIG. 19

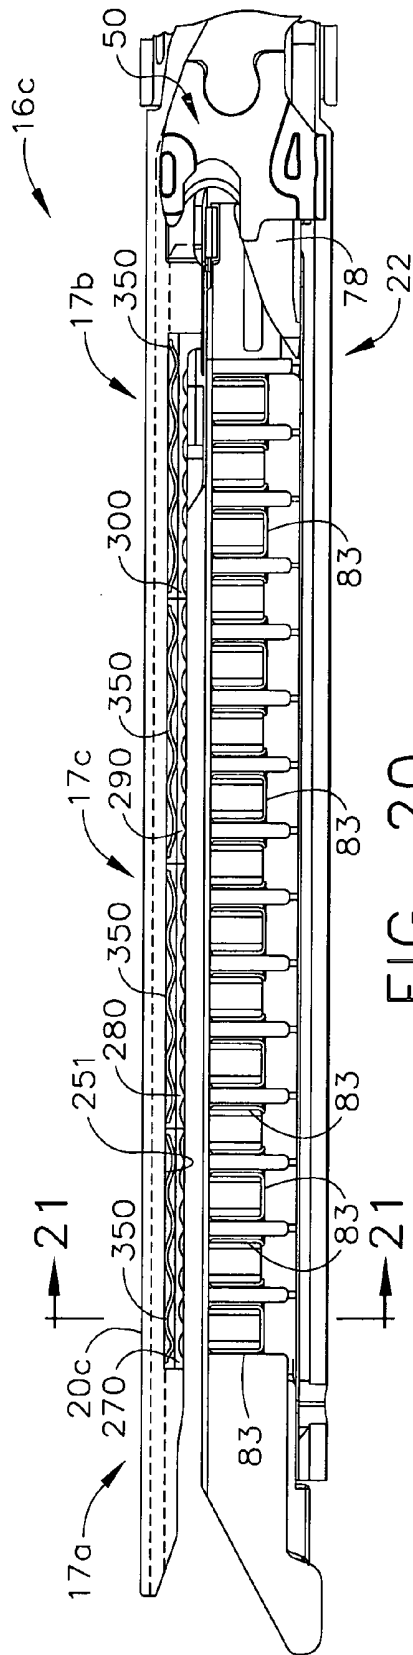


FIG. 20

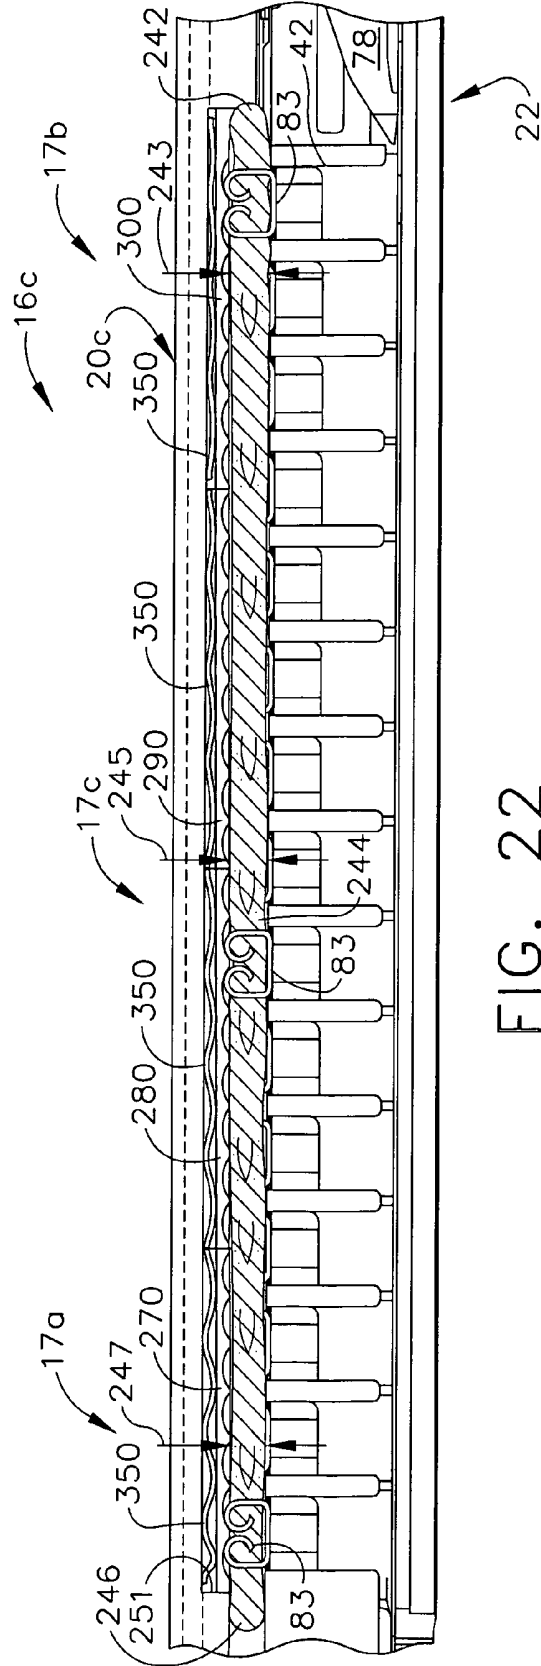


FIG. 22

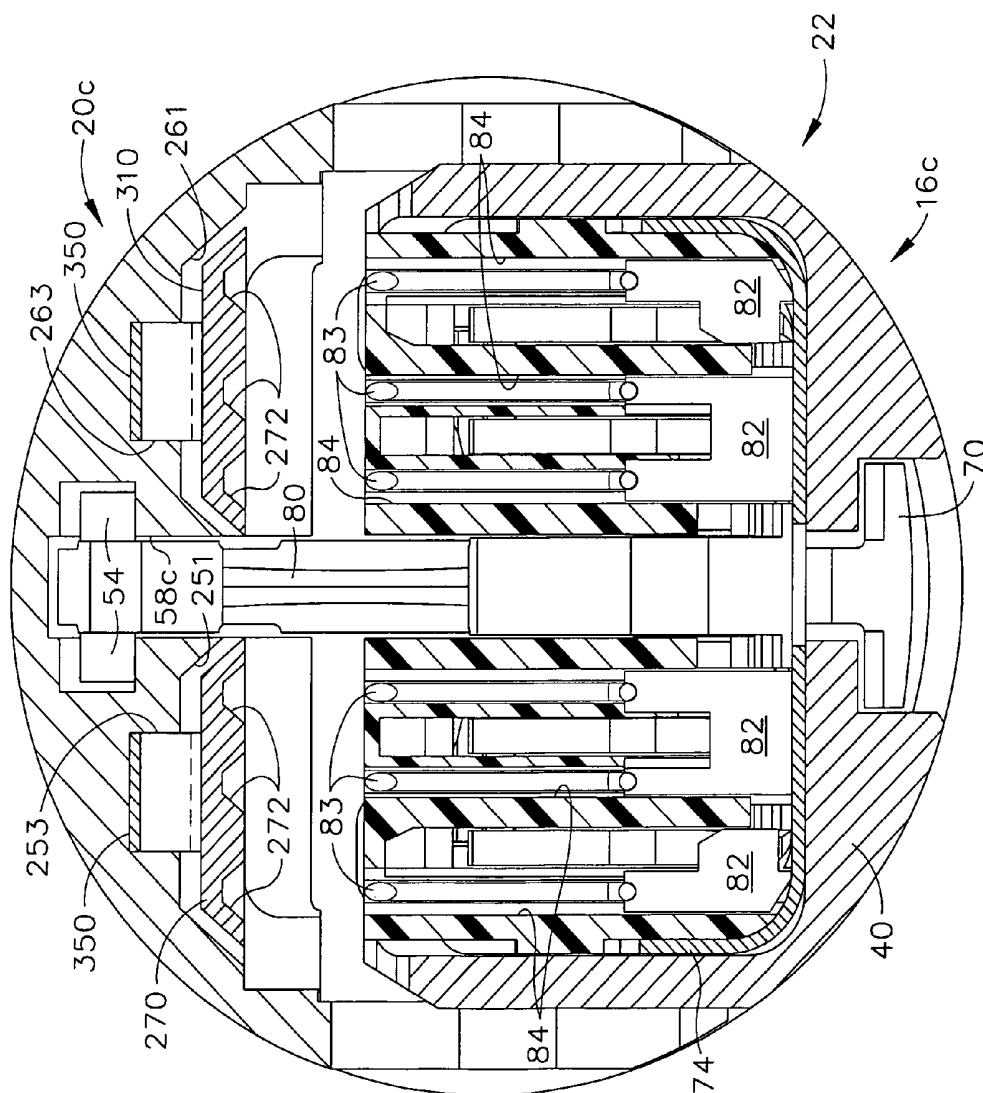


FIG. 21

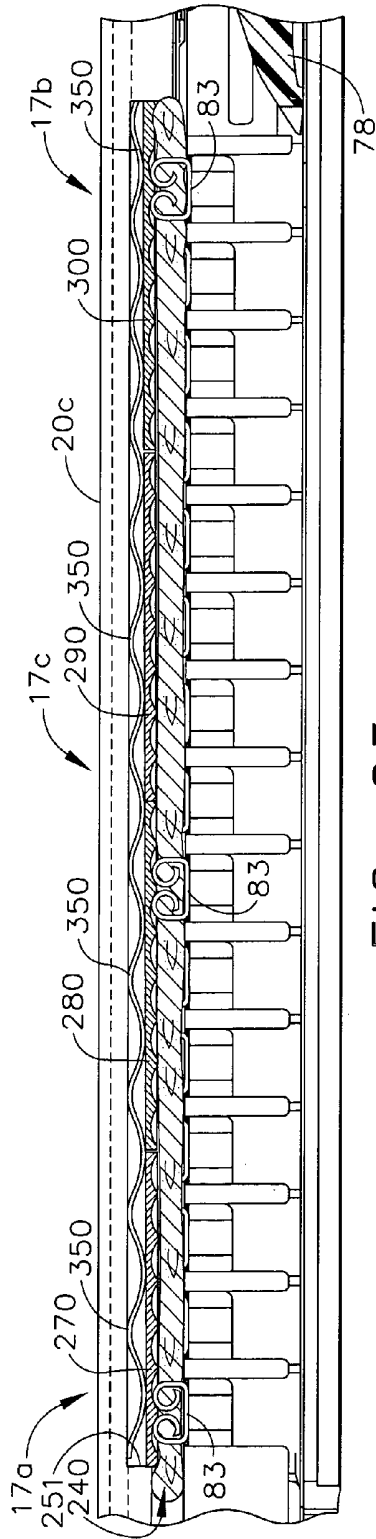


FIG. 23

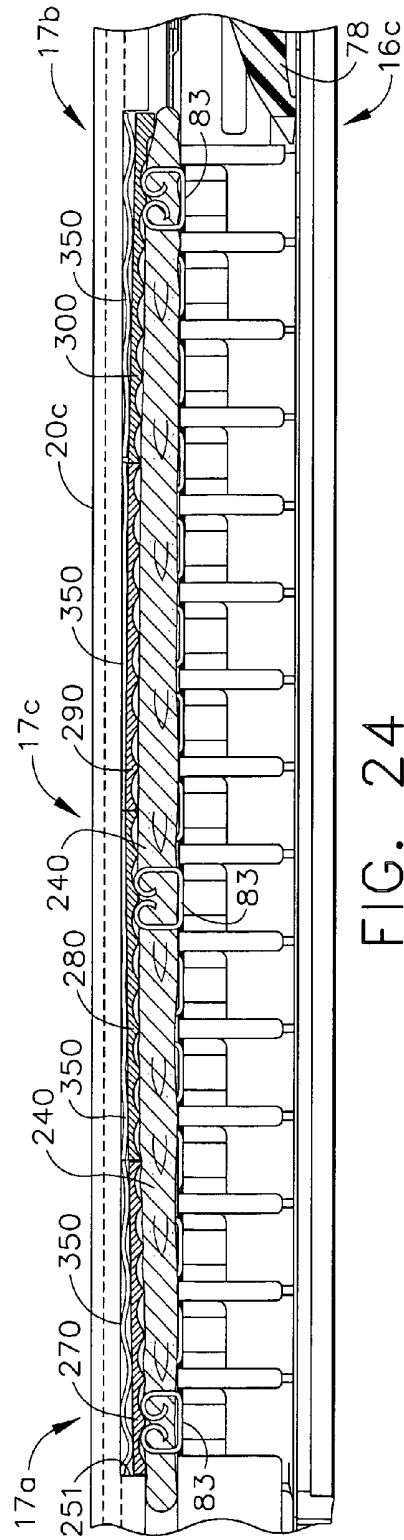


FIG. 24

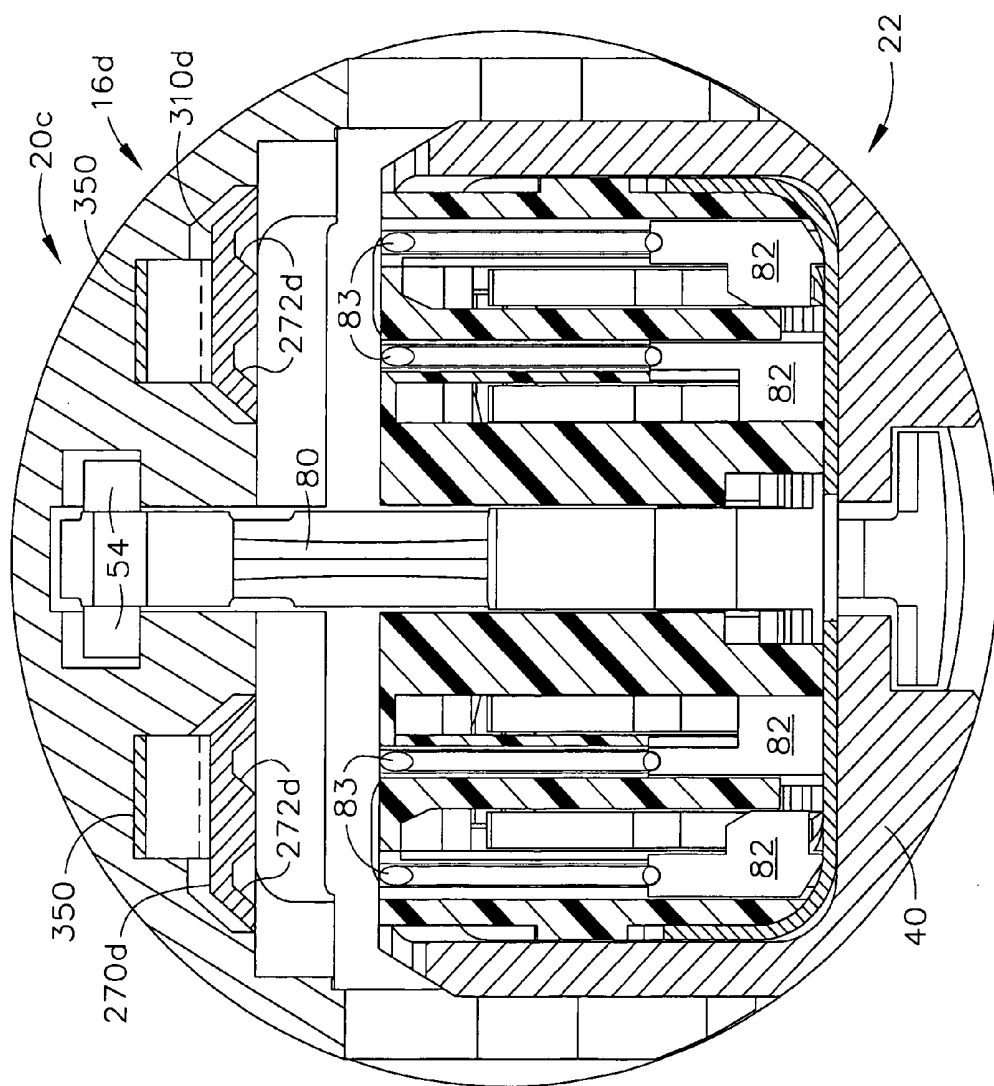


FIG. 25

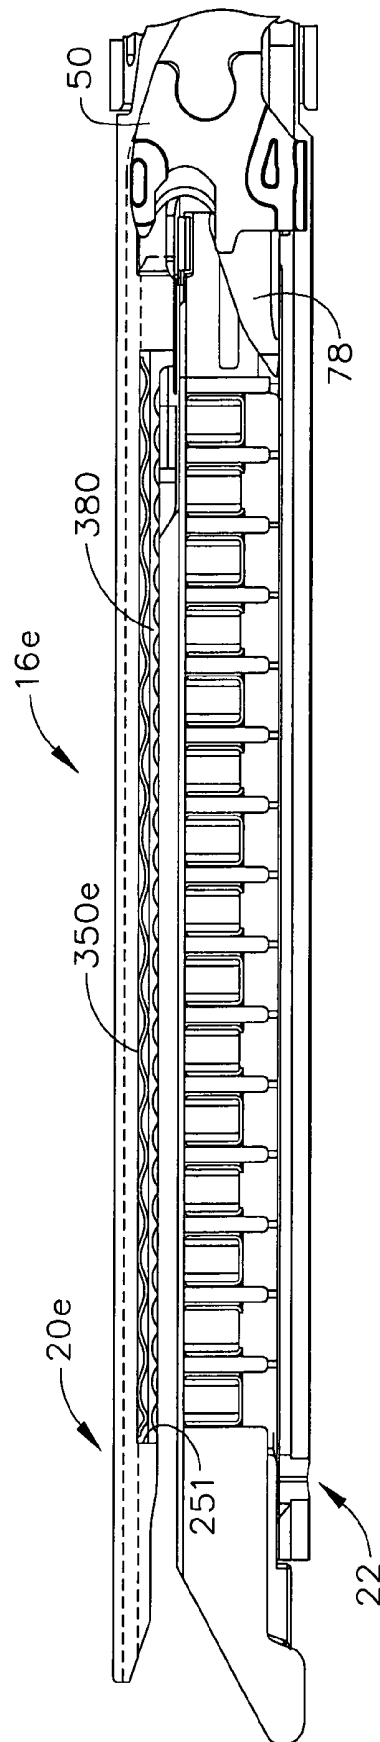


FIG. 26

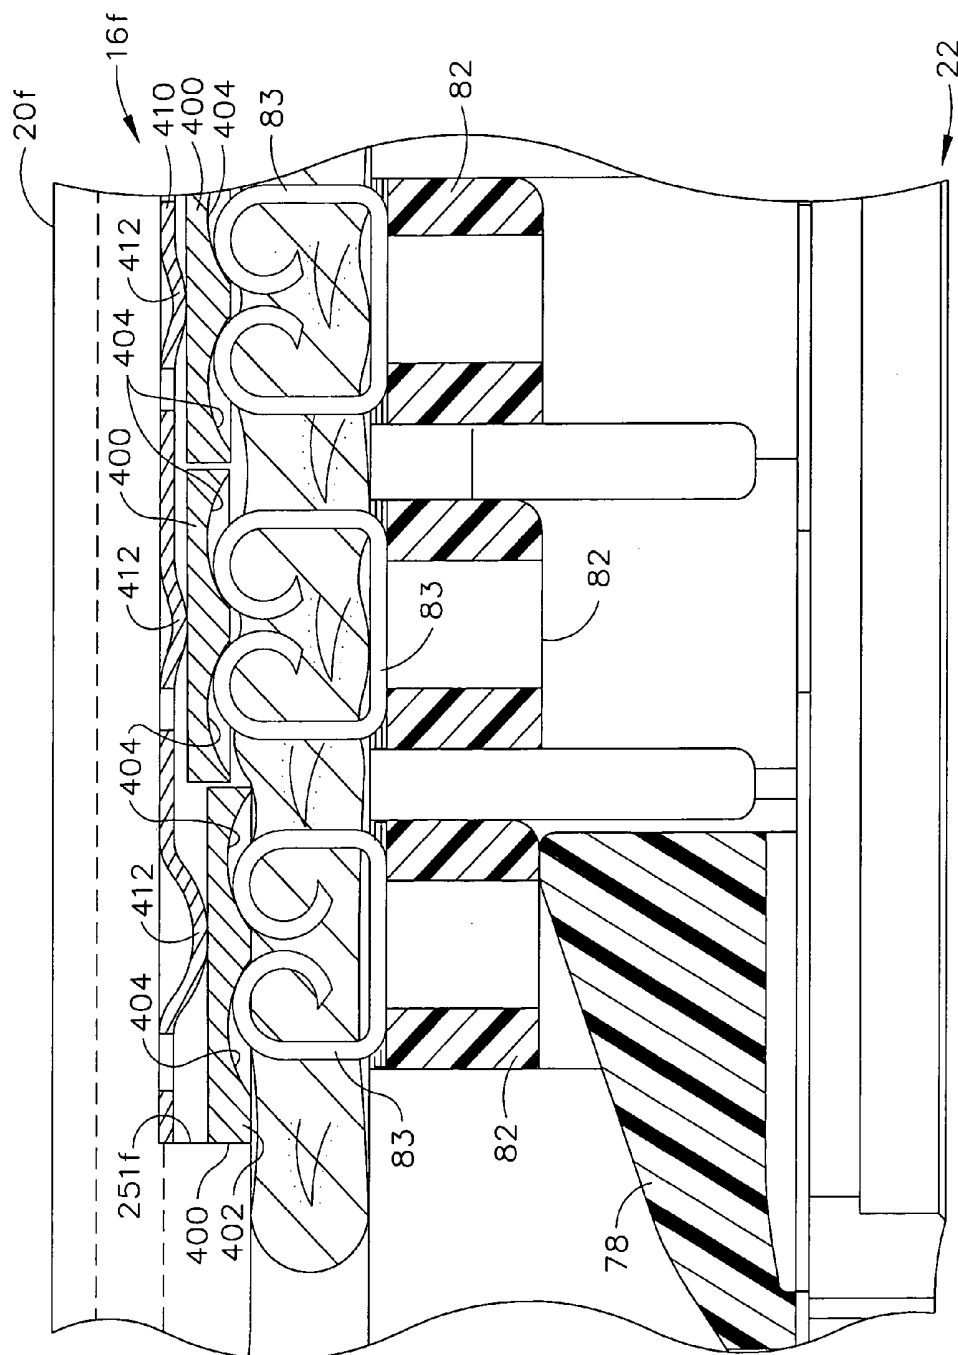


FIG. 27

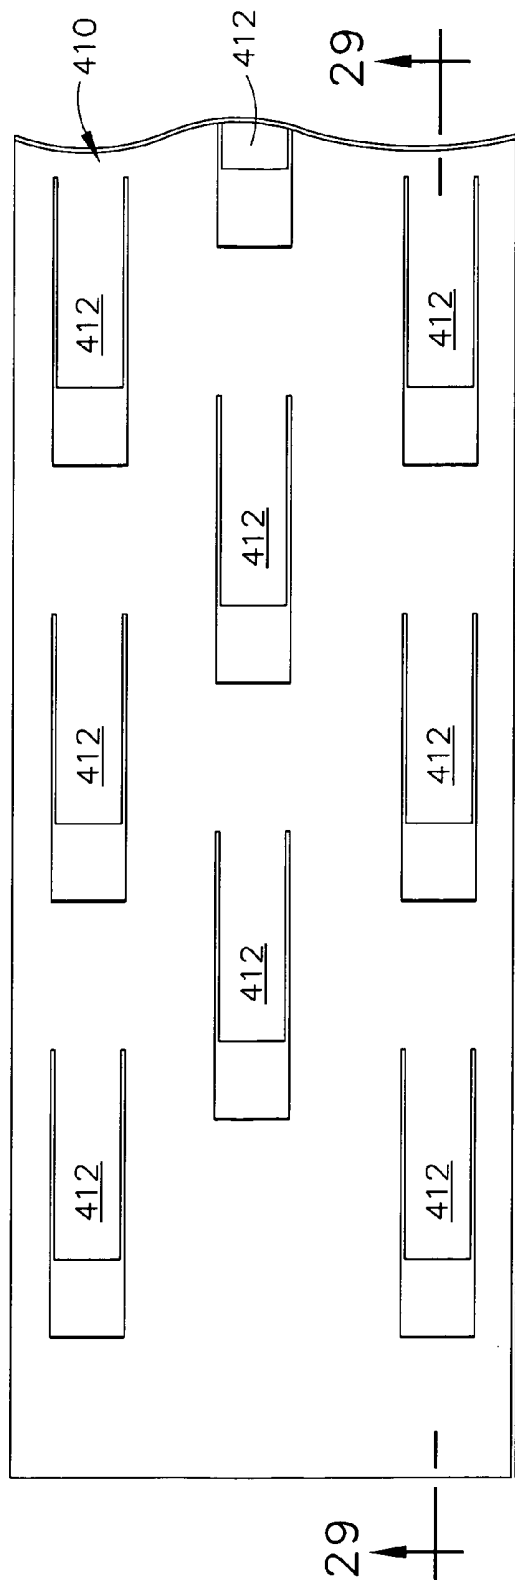


FIG. 28

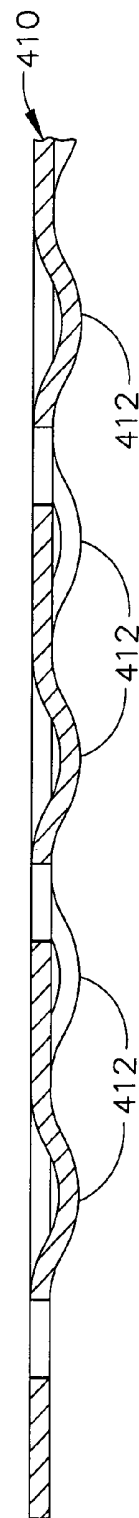


FIG. 29

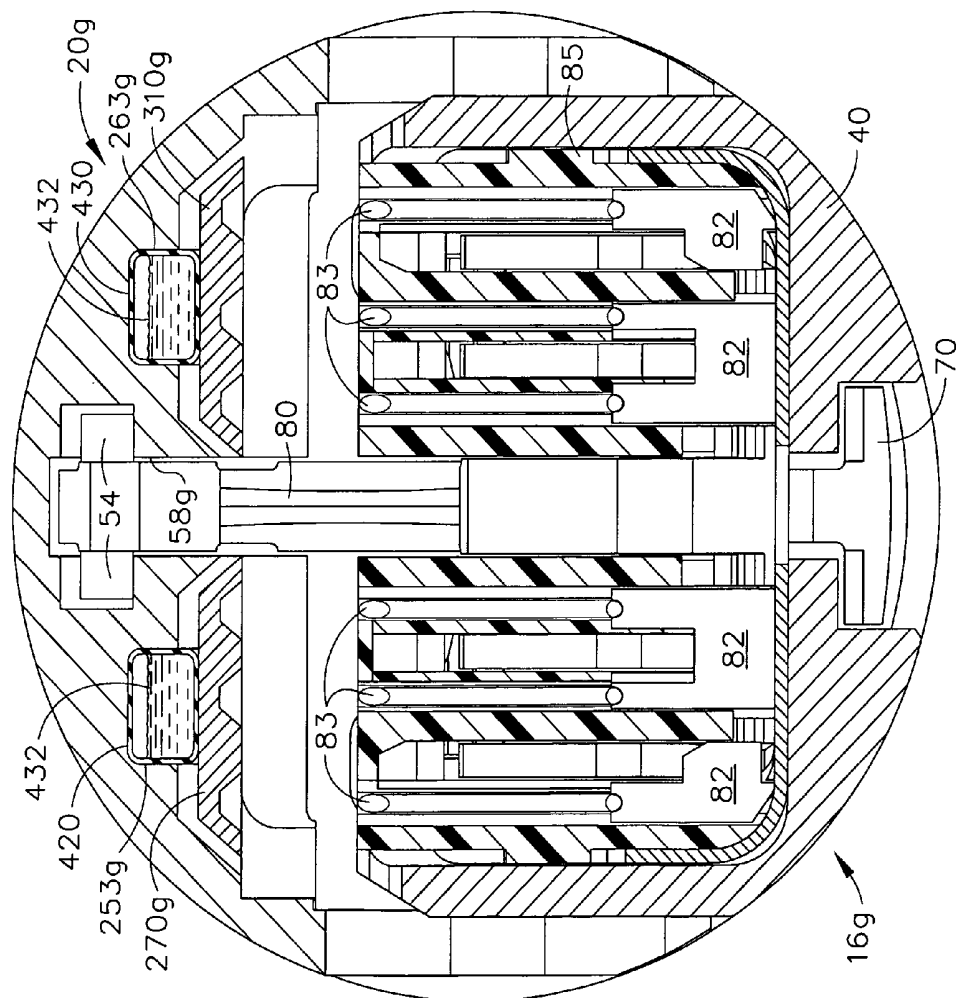


FIG. 30

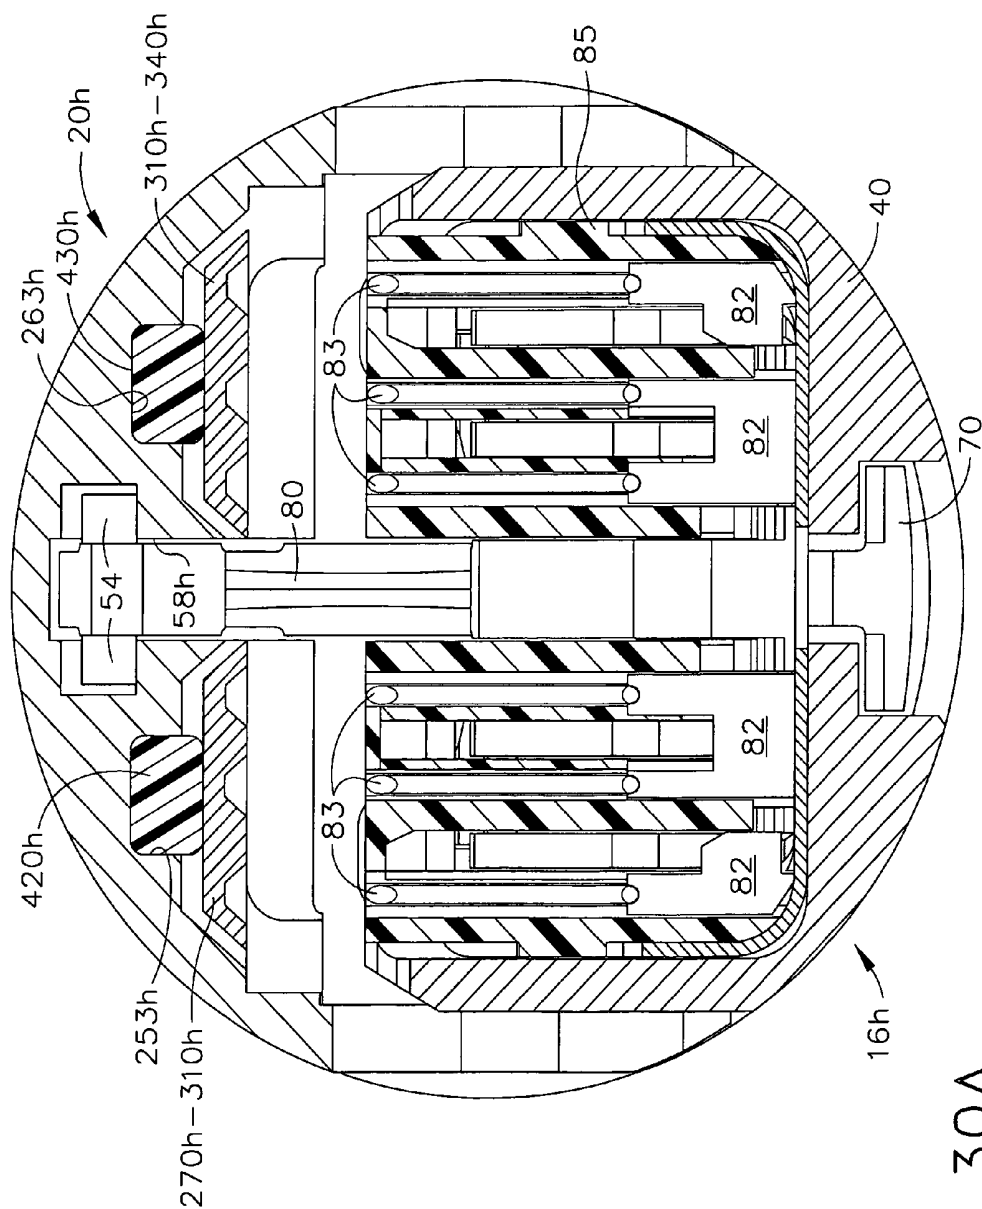
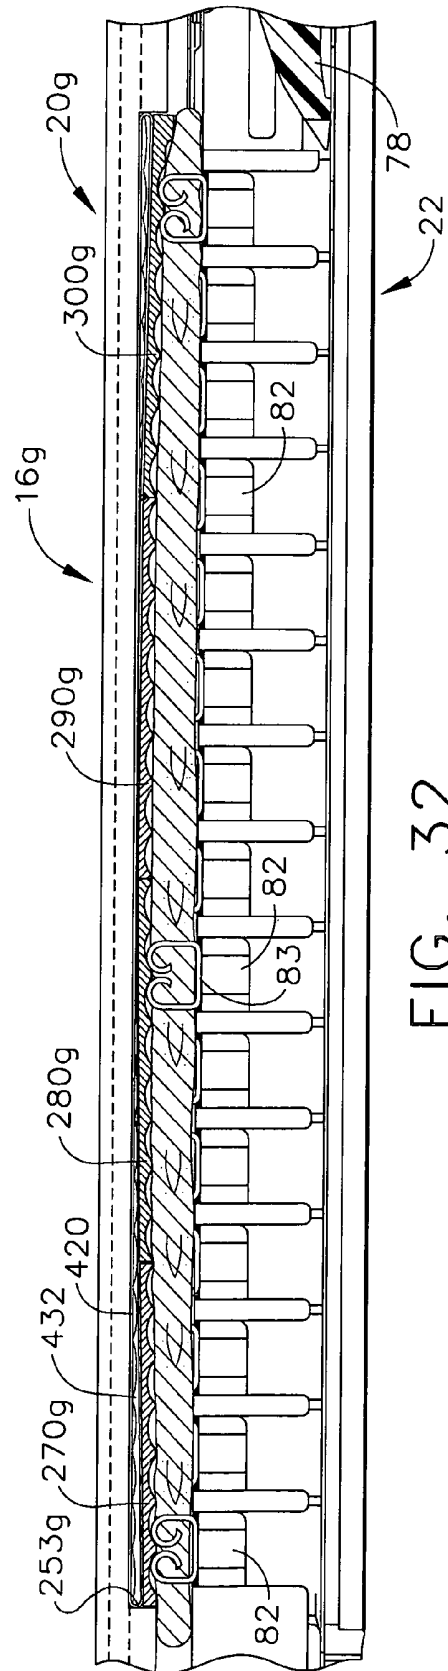
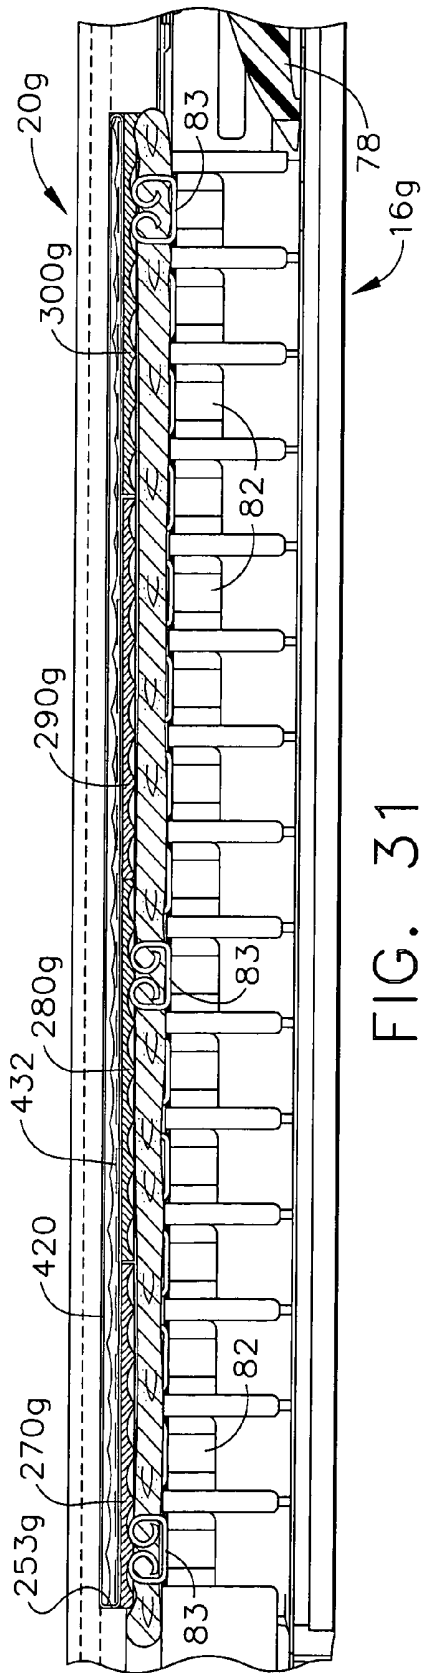


FIG. 30A



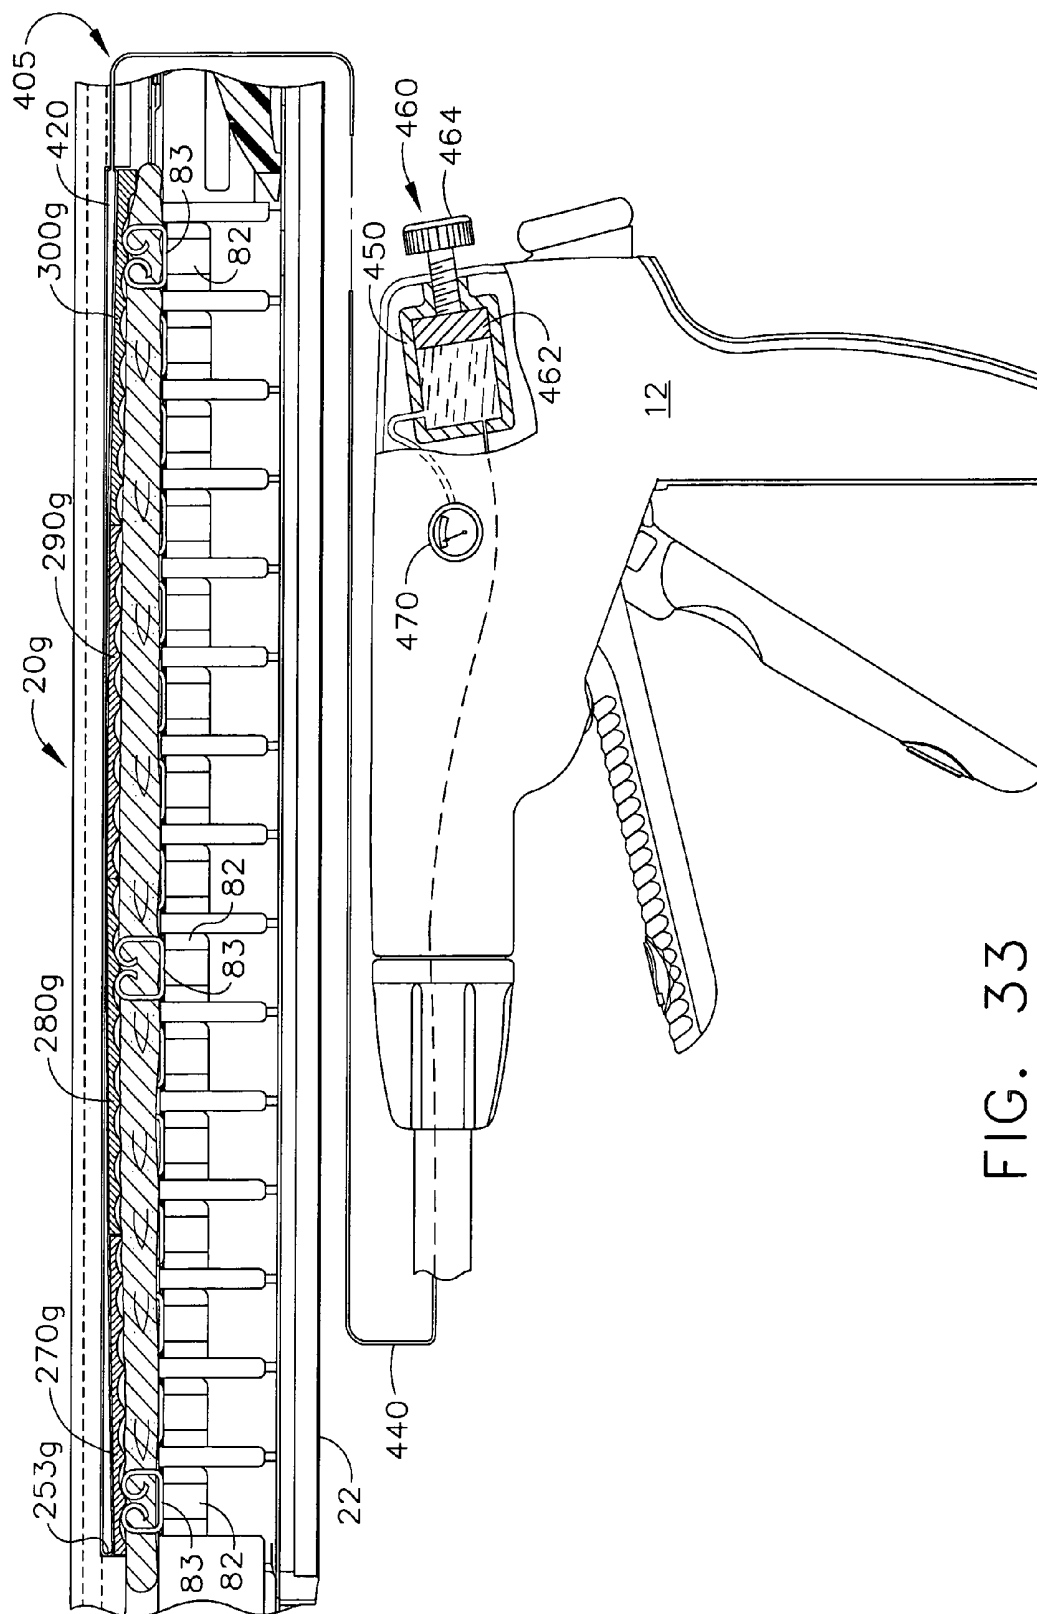
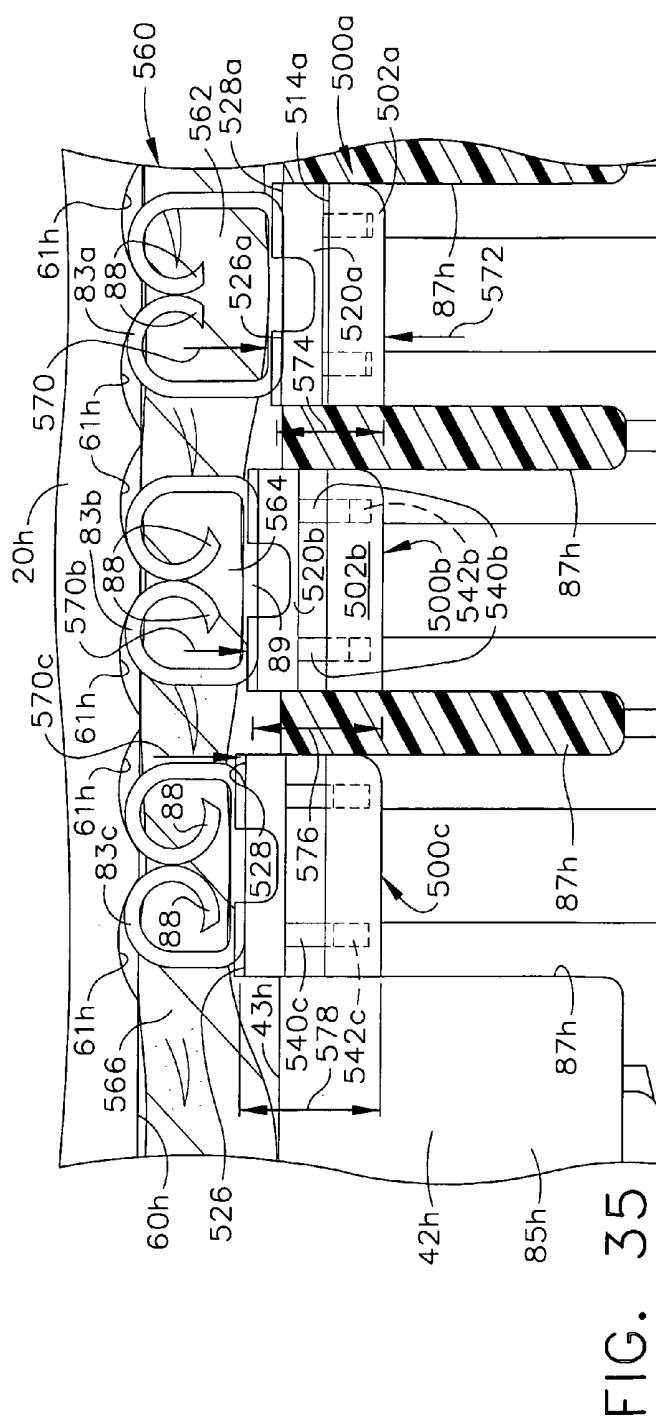
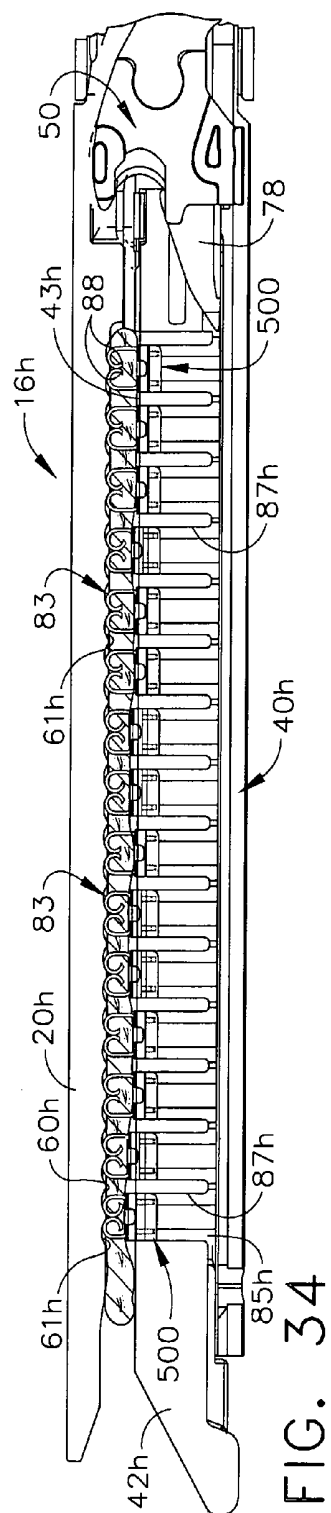
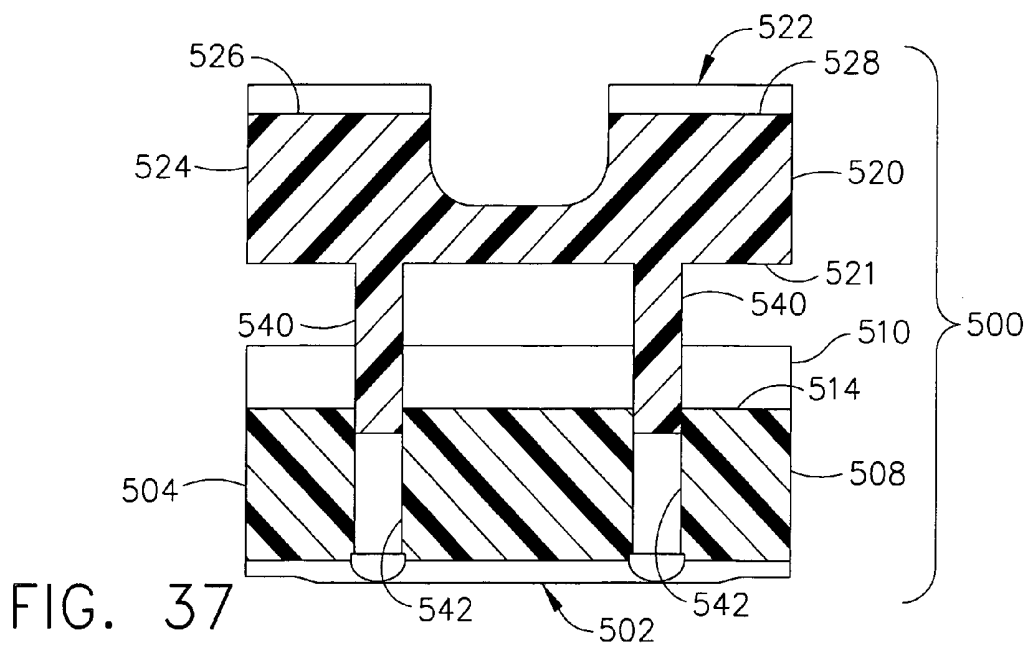
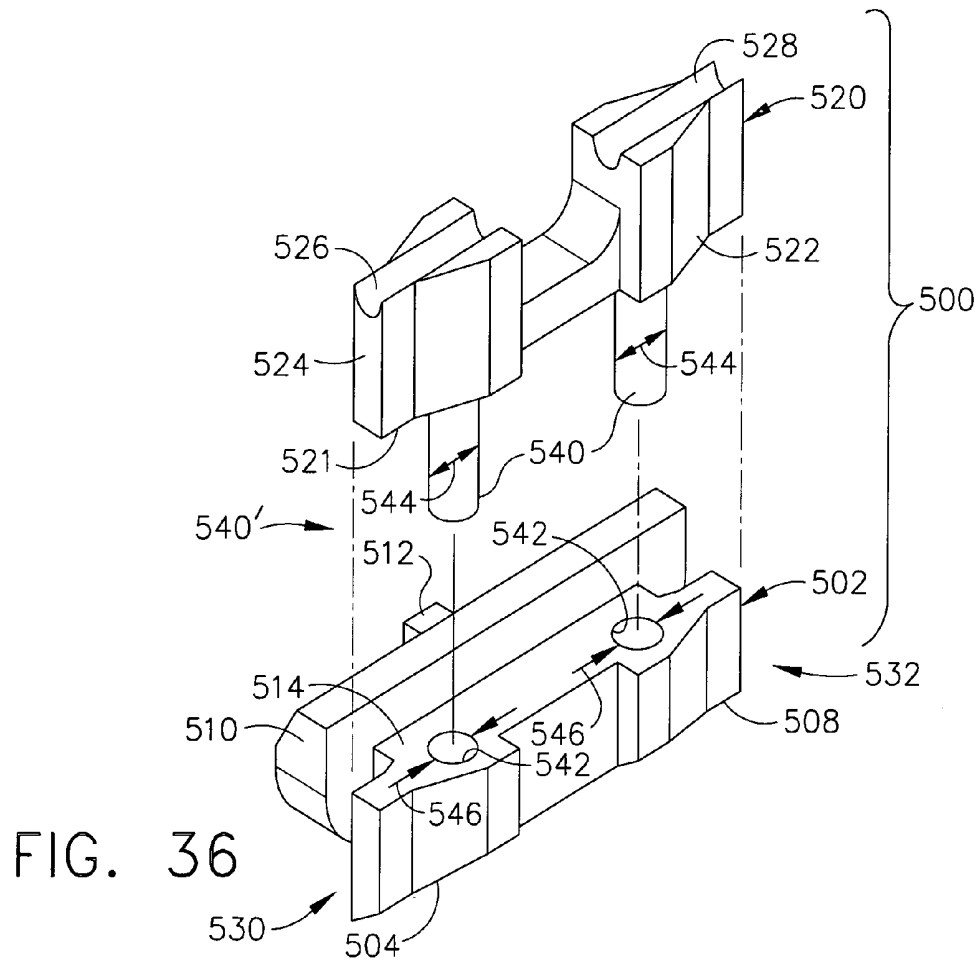
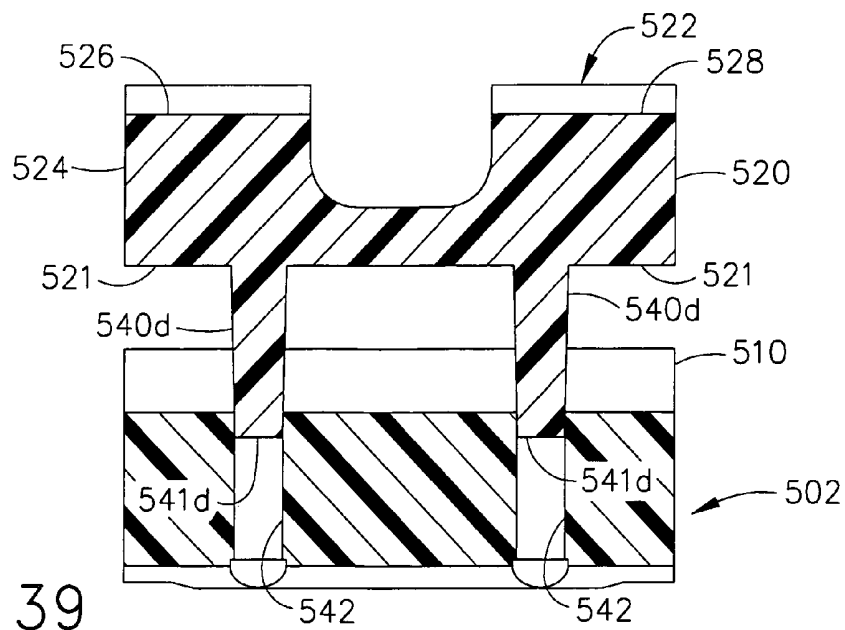
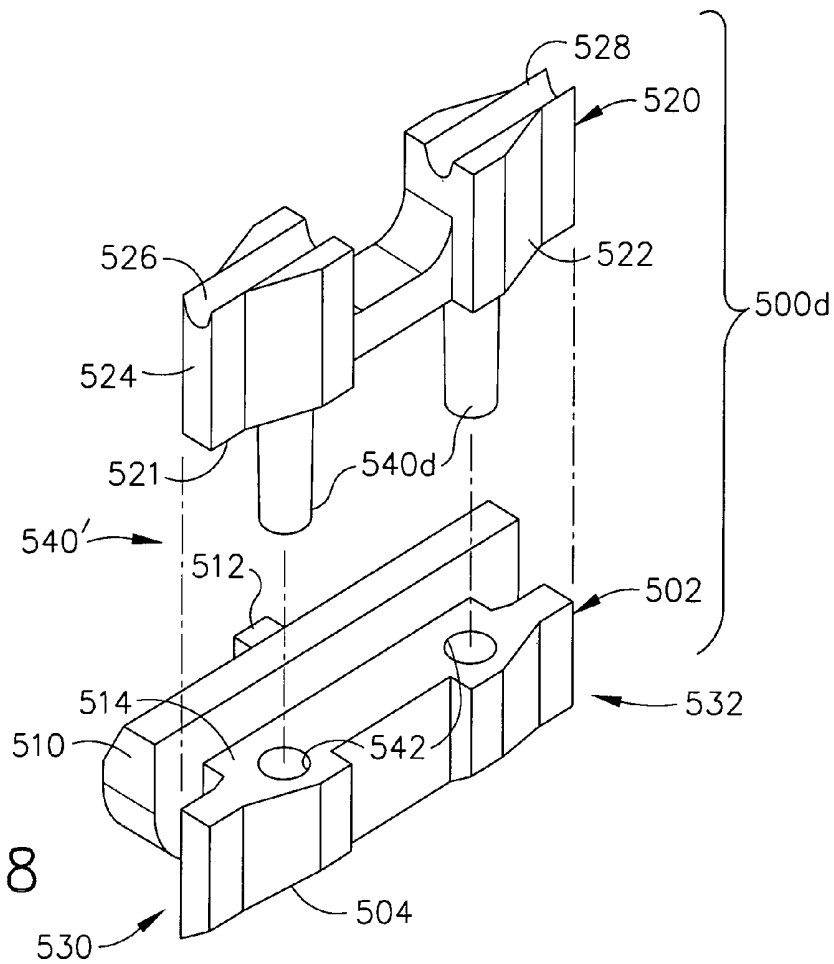
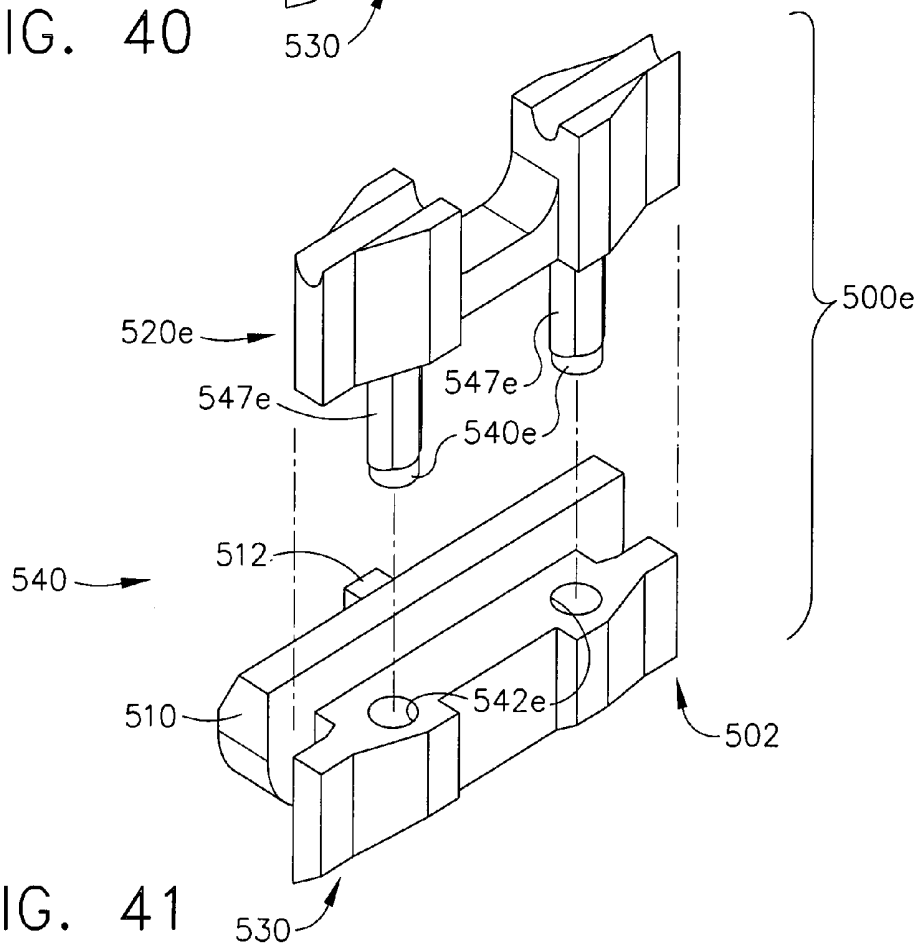
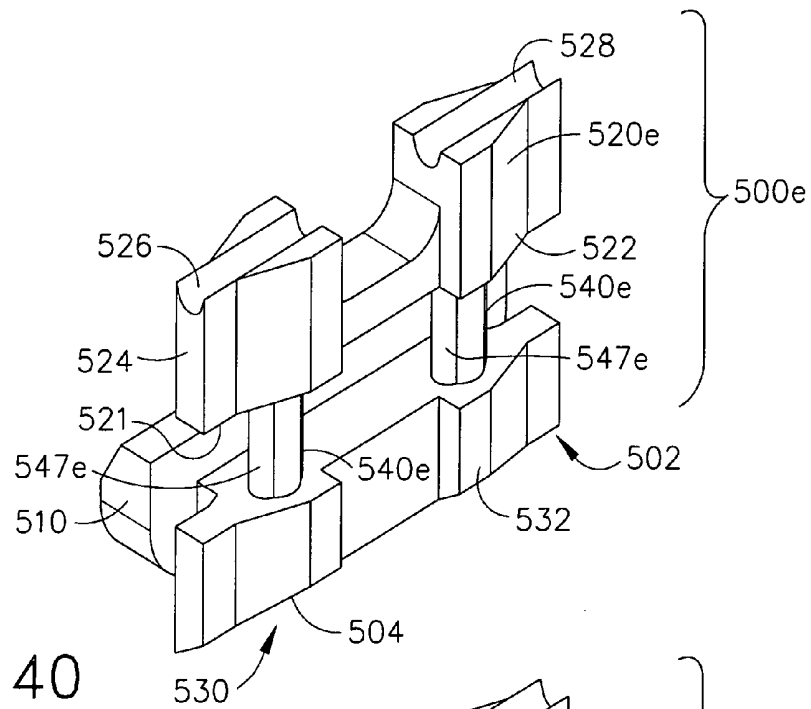


FIG. 33









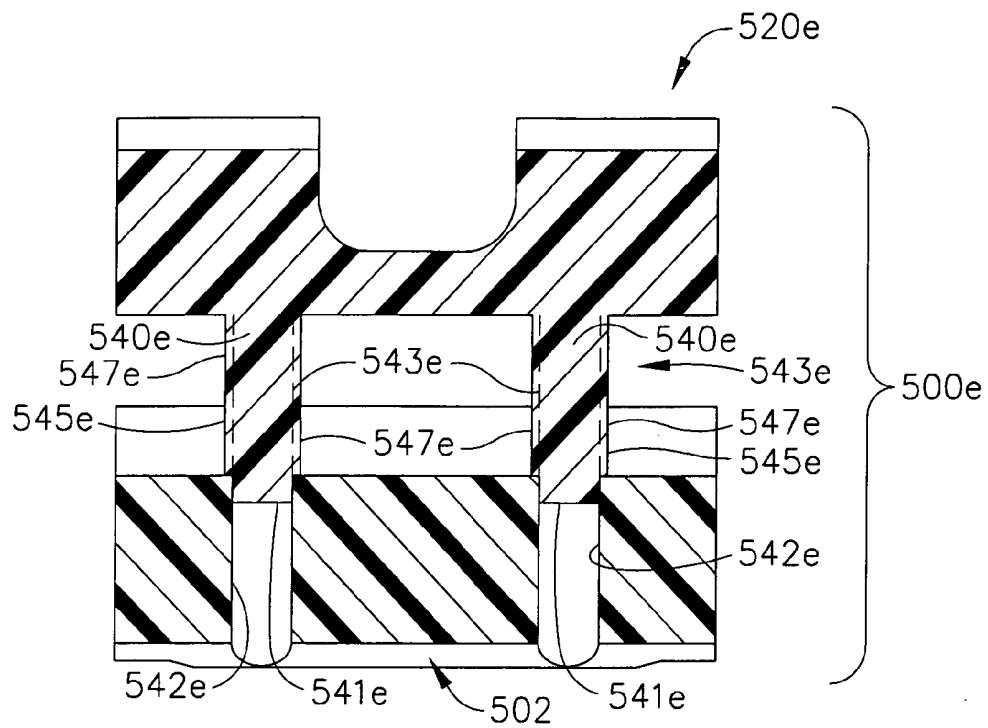


FIG. 42

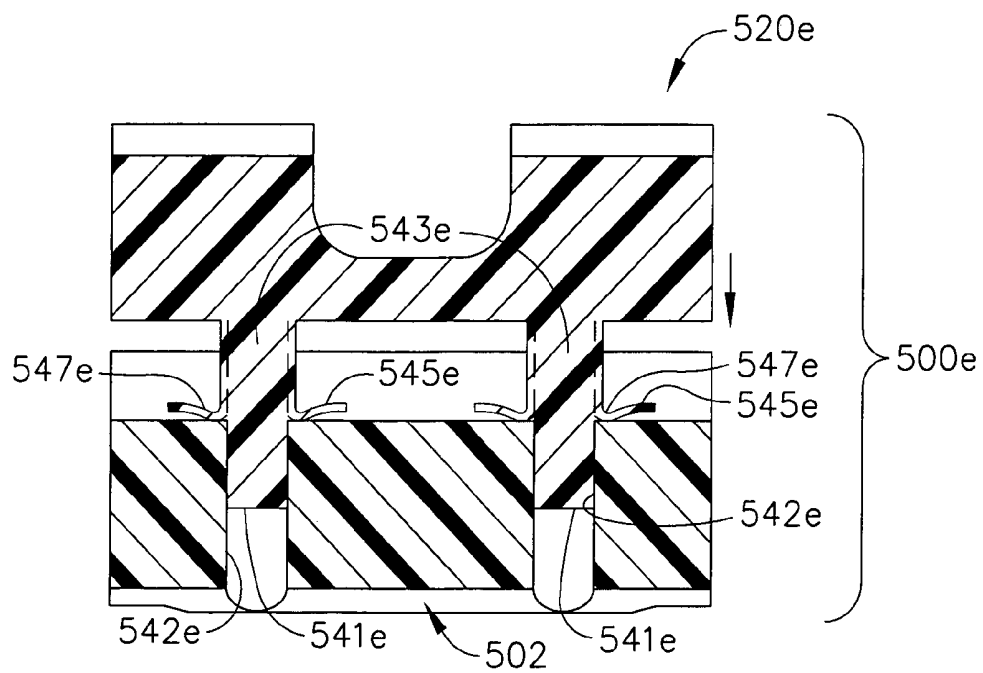


FIG. 43

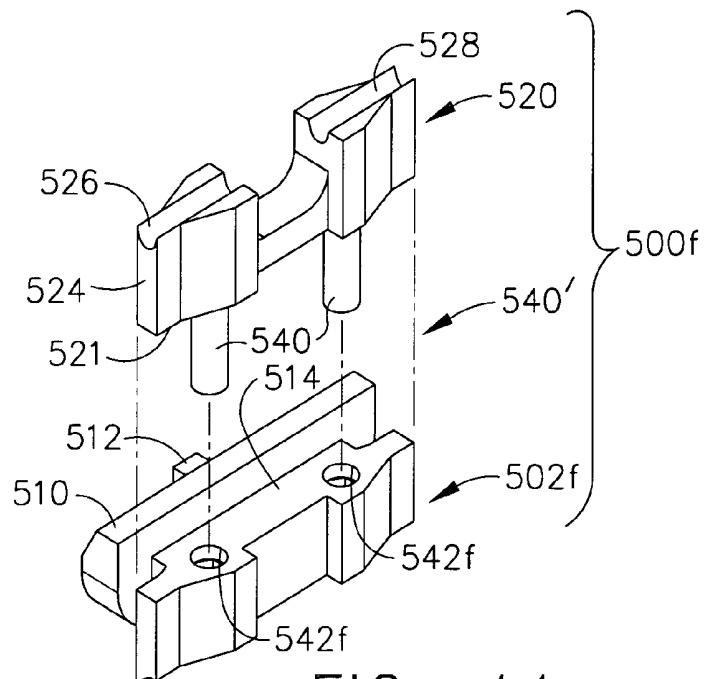


FIG. 44

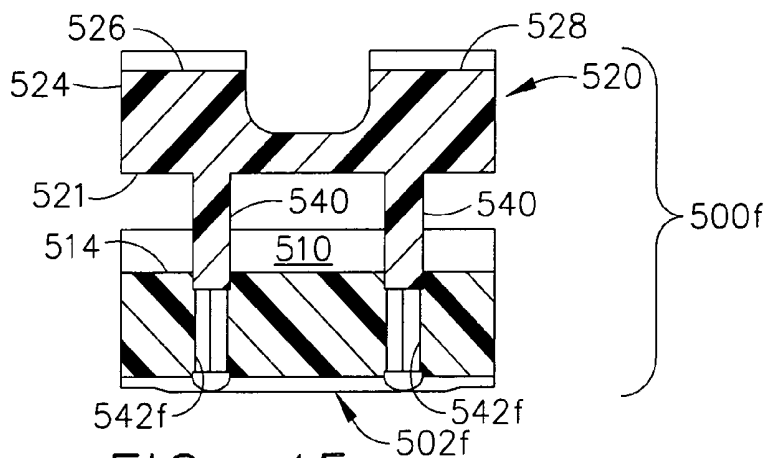


FIG. 45

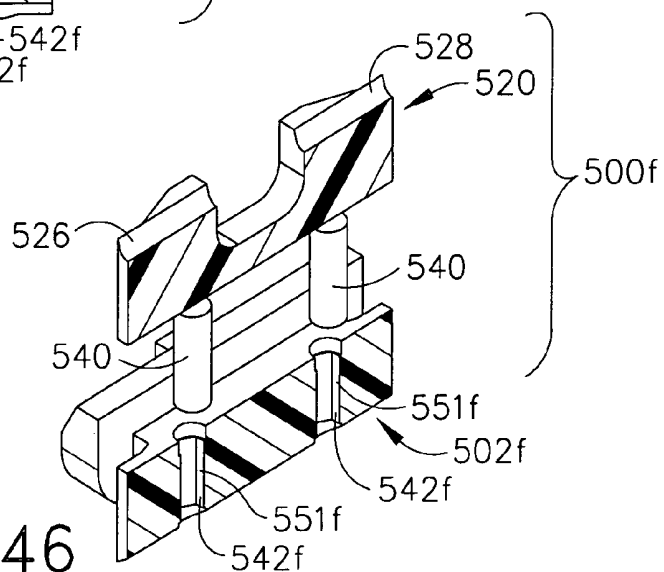


FIG. 46

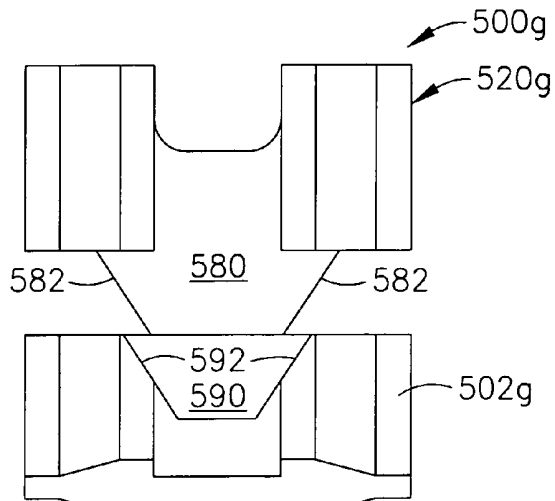


FIG. 47

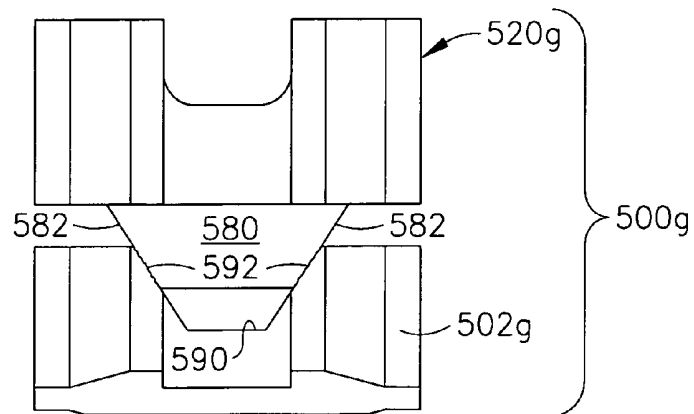


FIG. 48

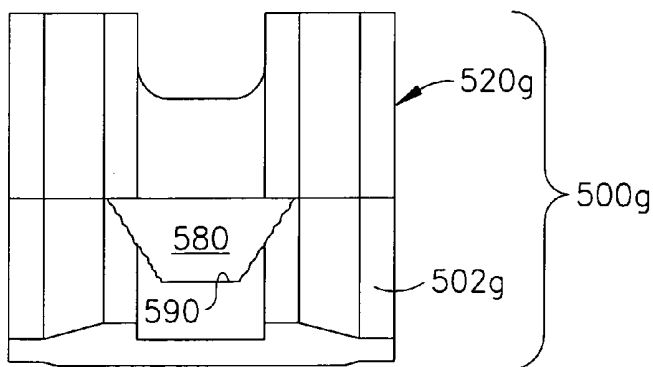
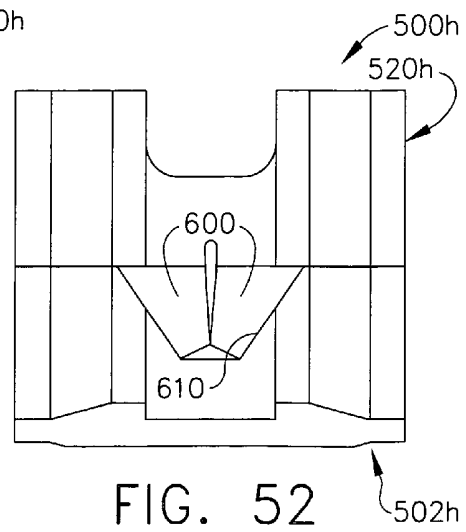
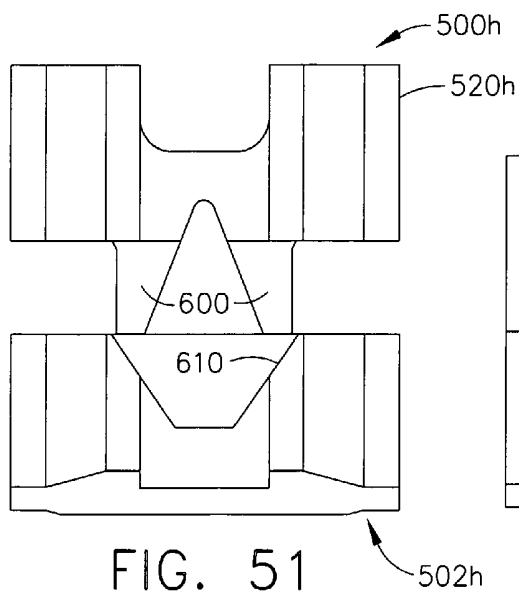
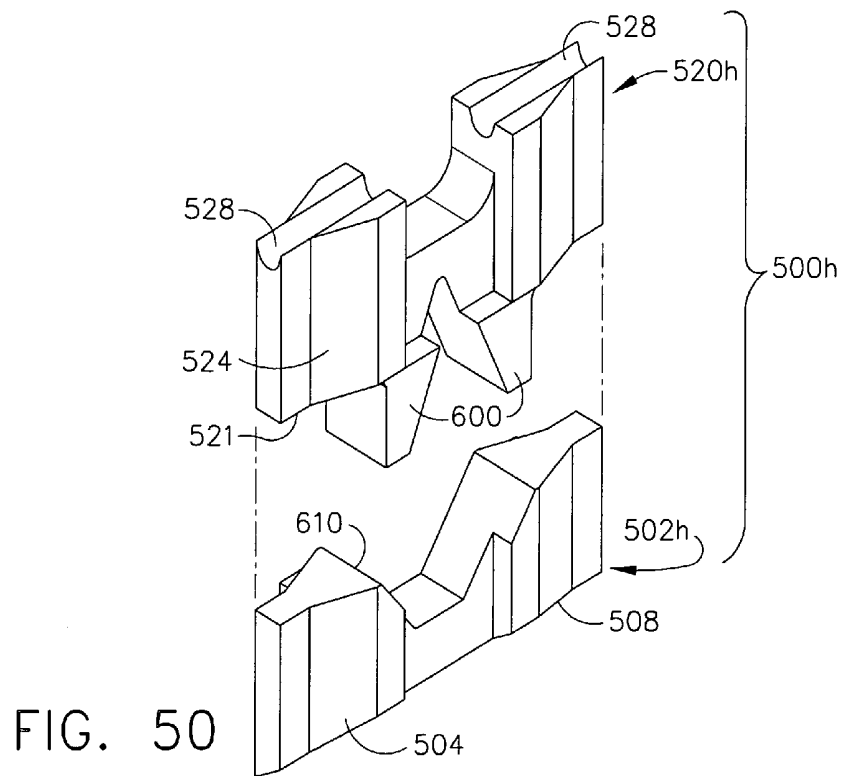
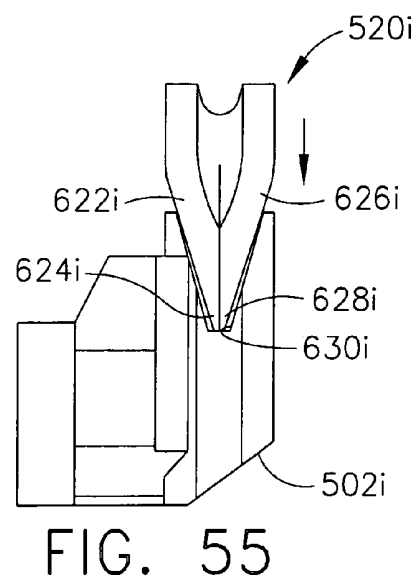
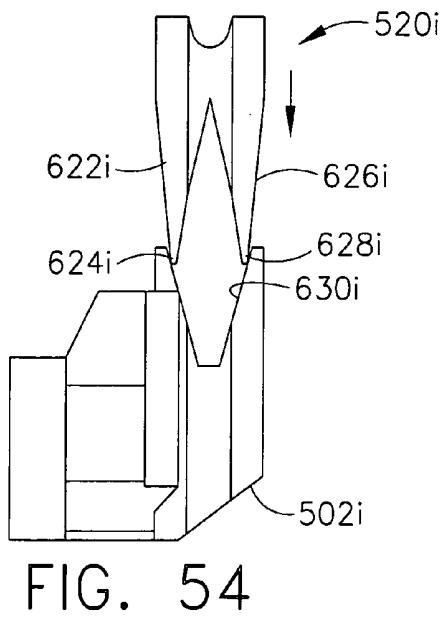
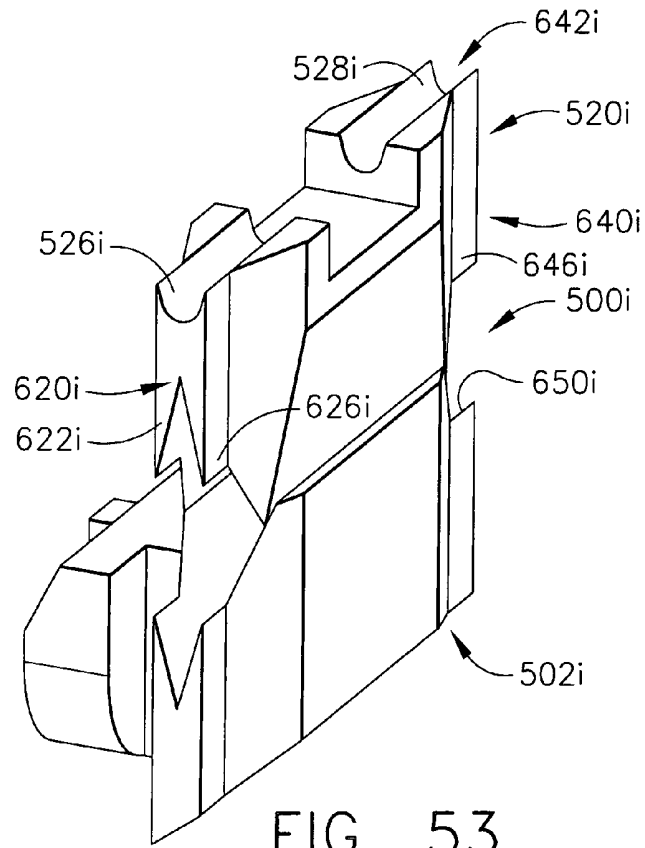


FIG. 49





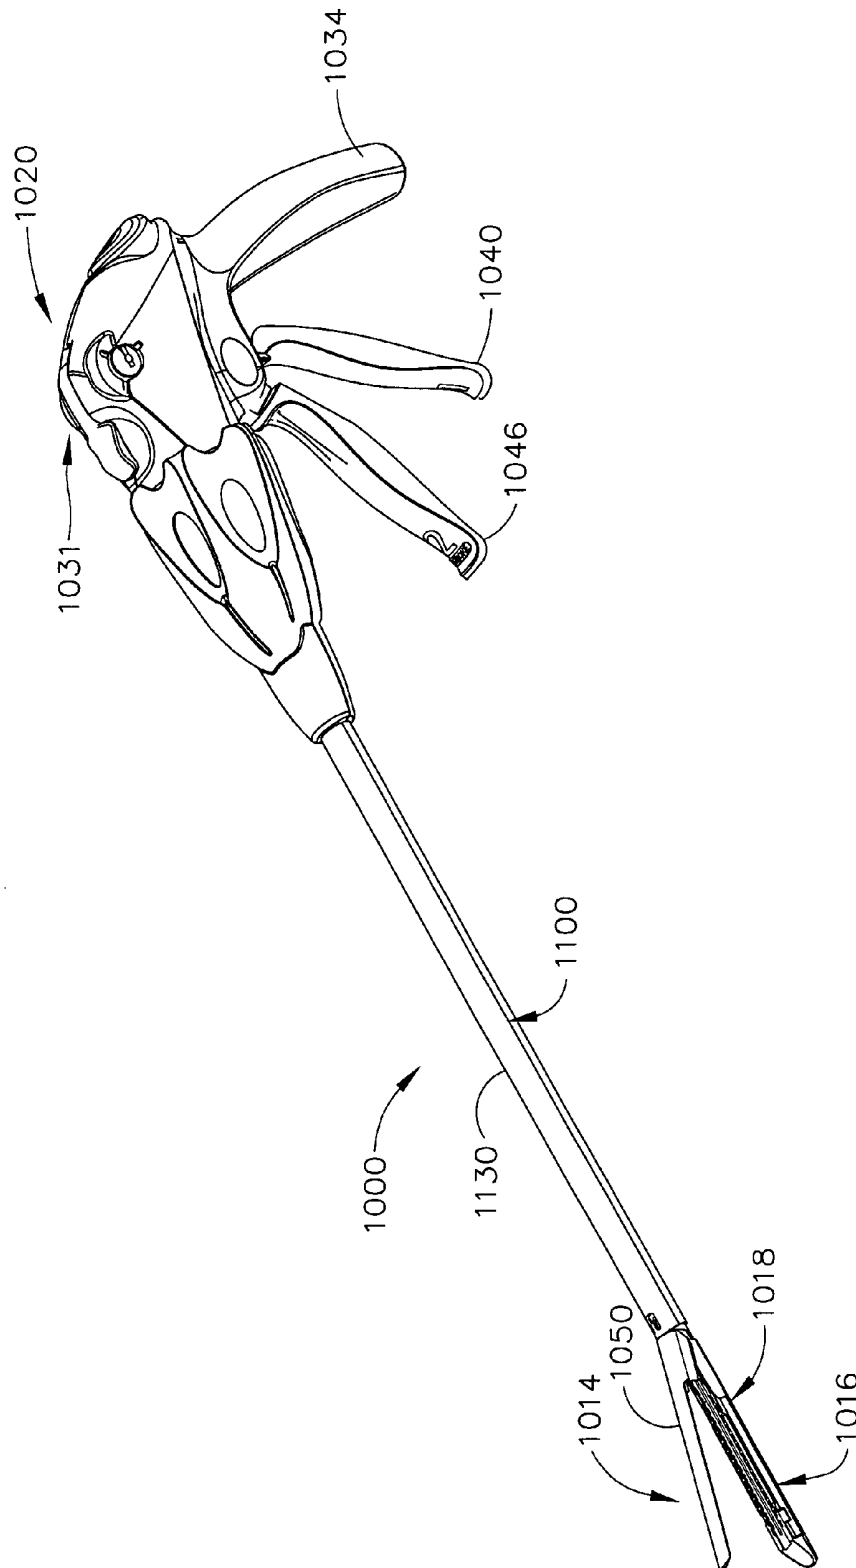
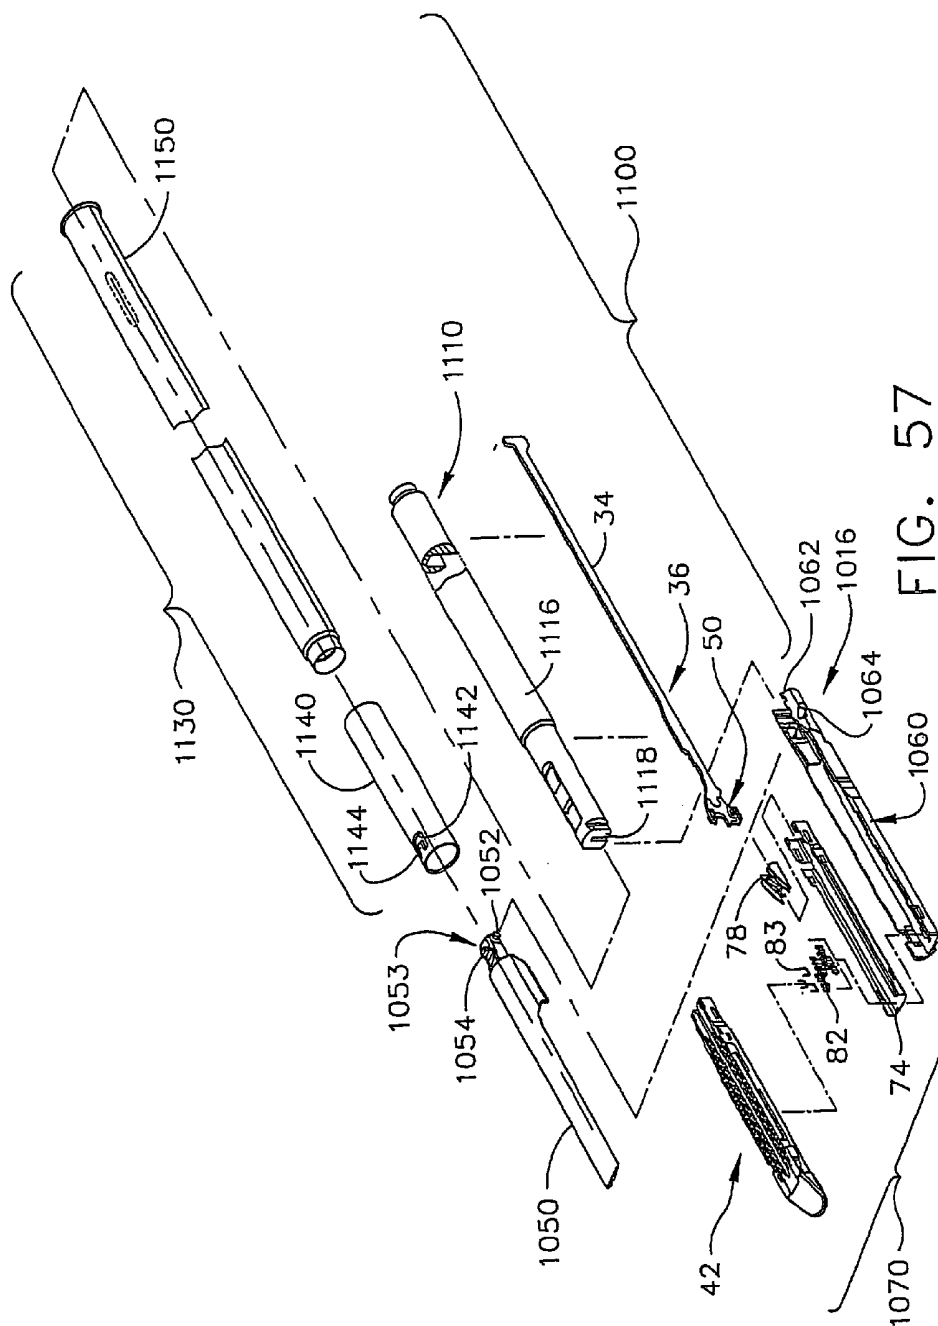


FIG. 56



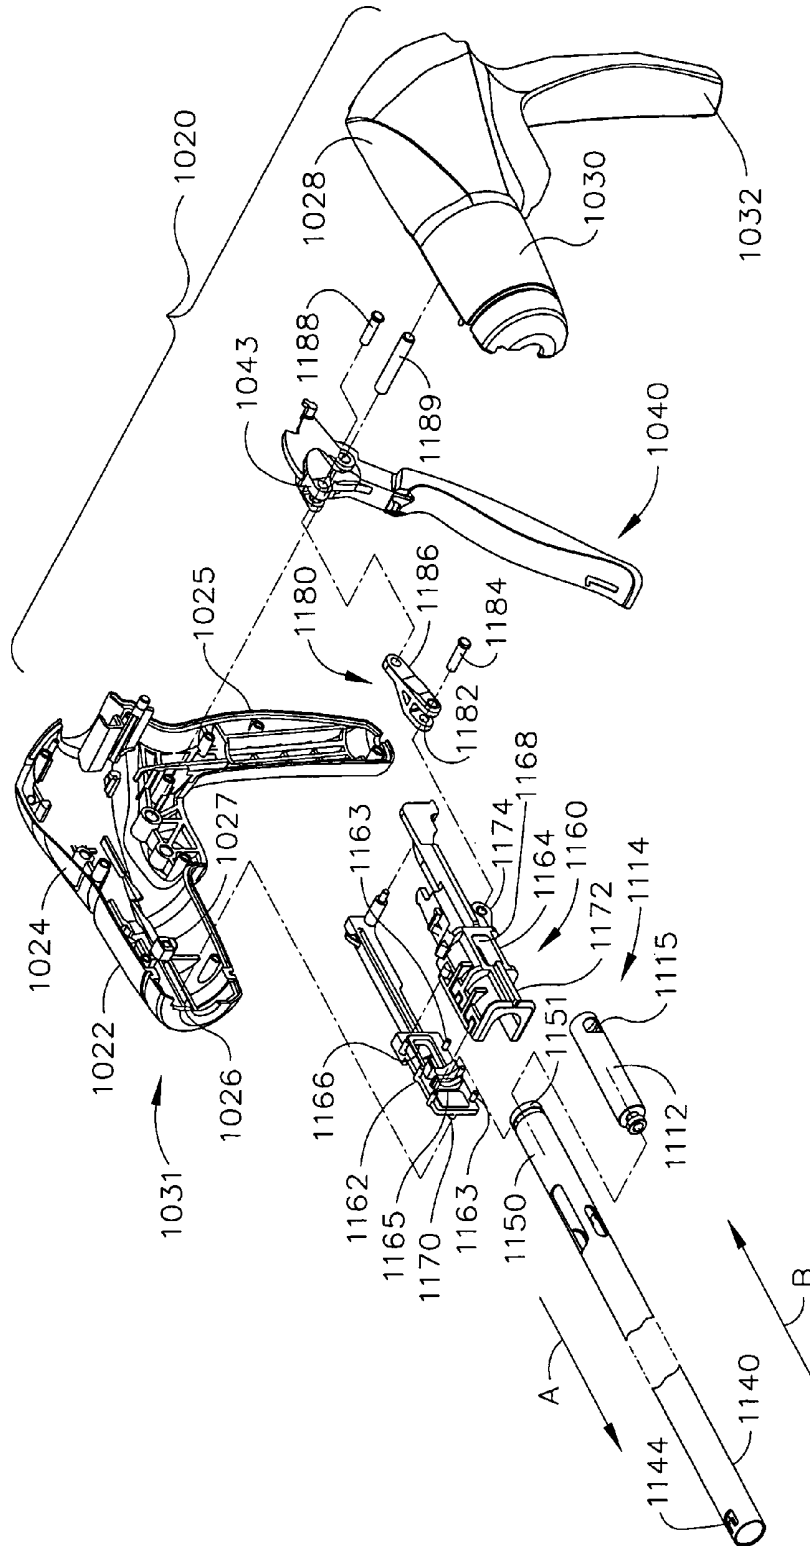


FIG. 58

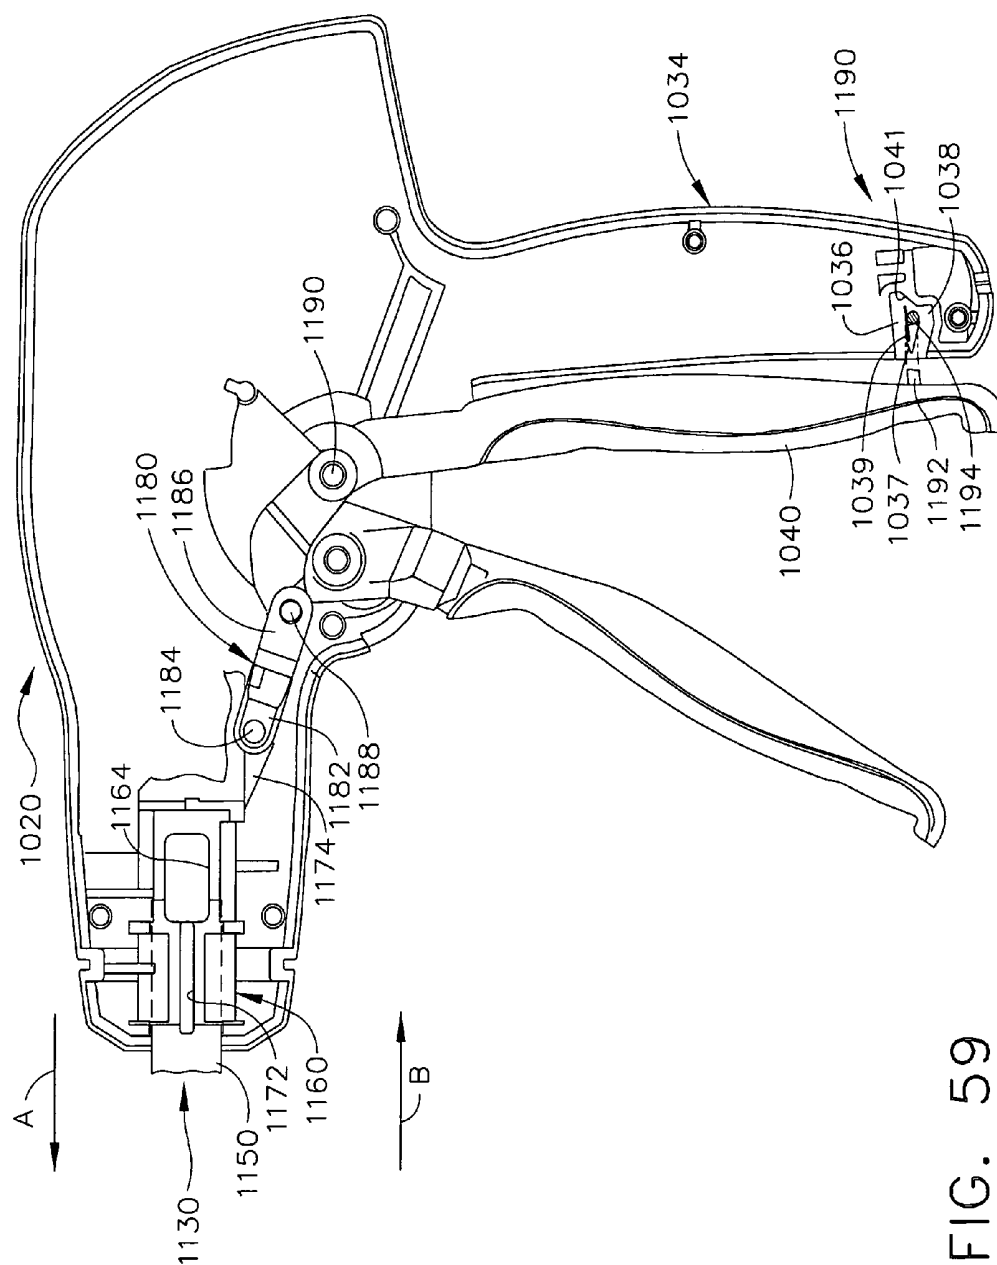


FIG. 59

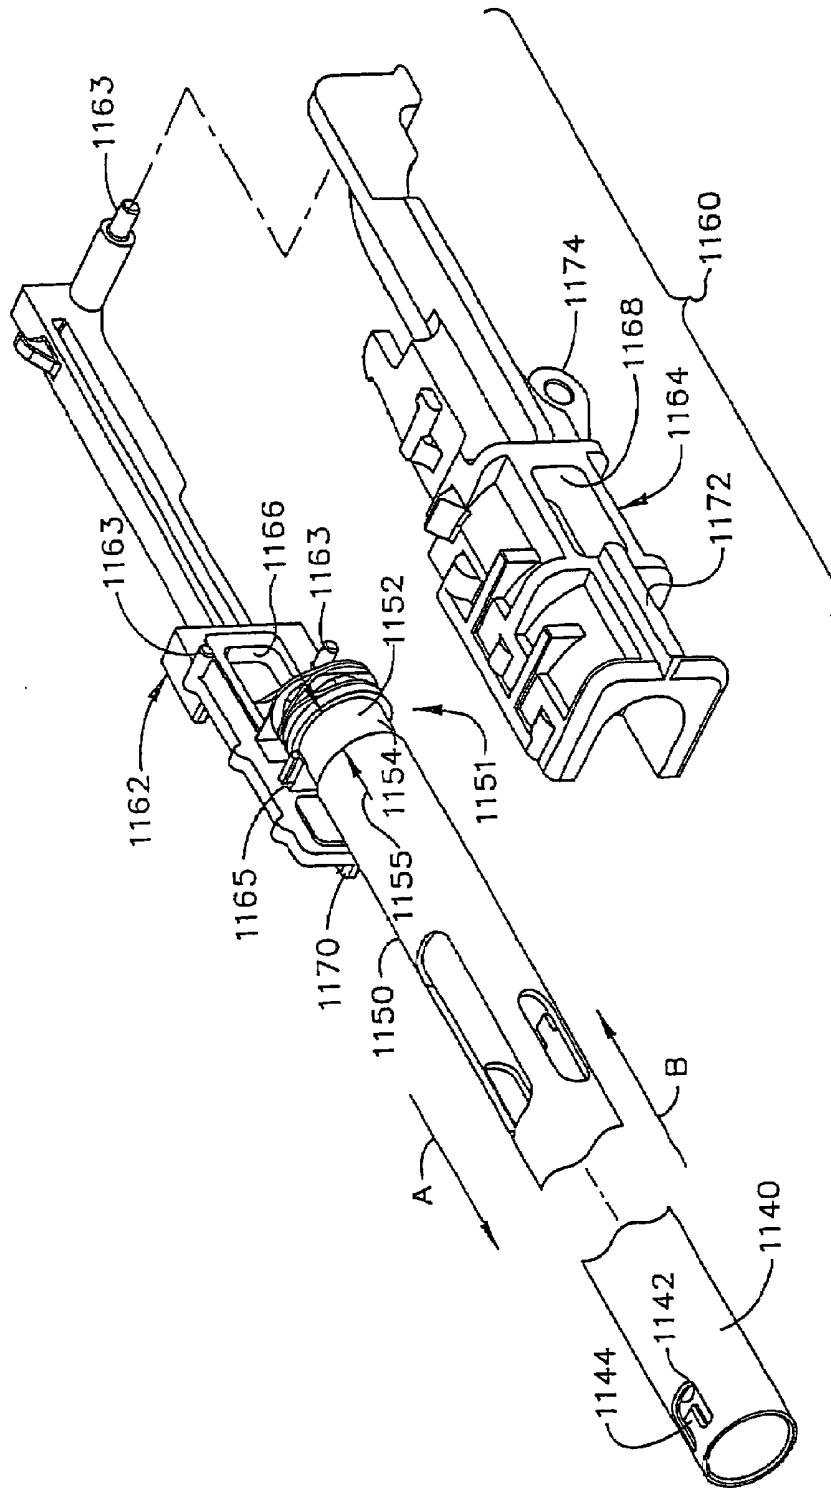


FIG. 60

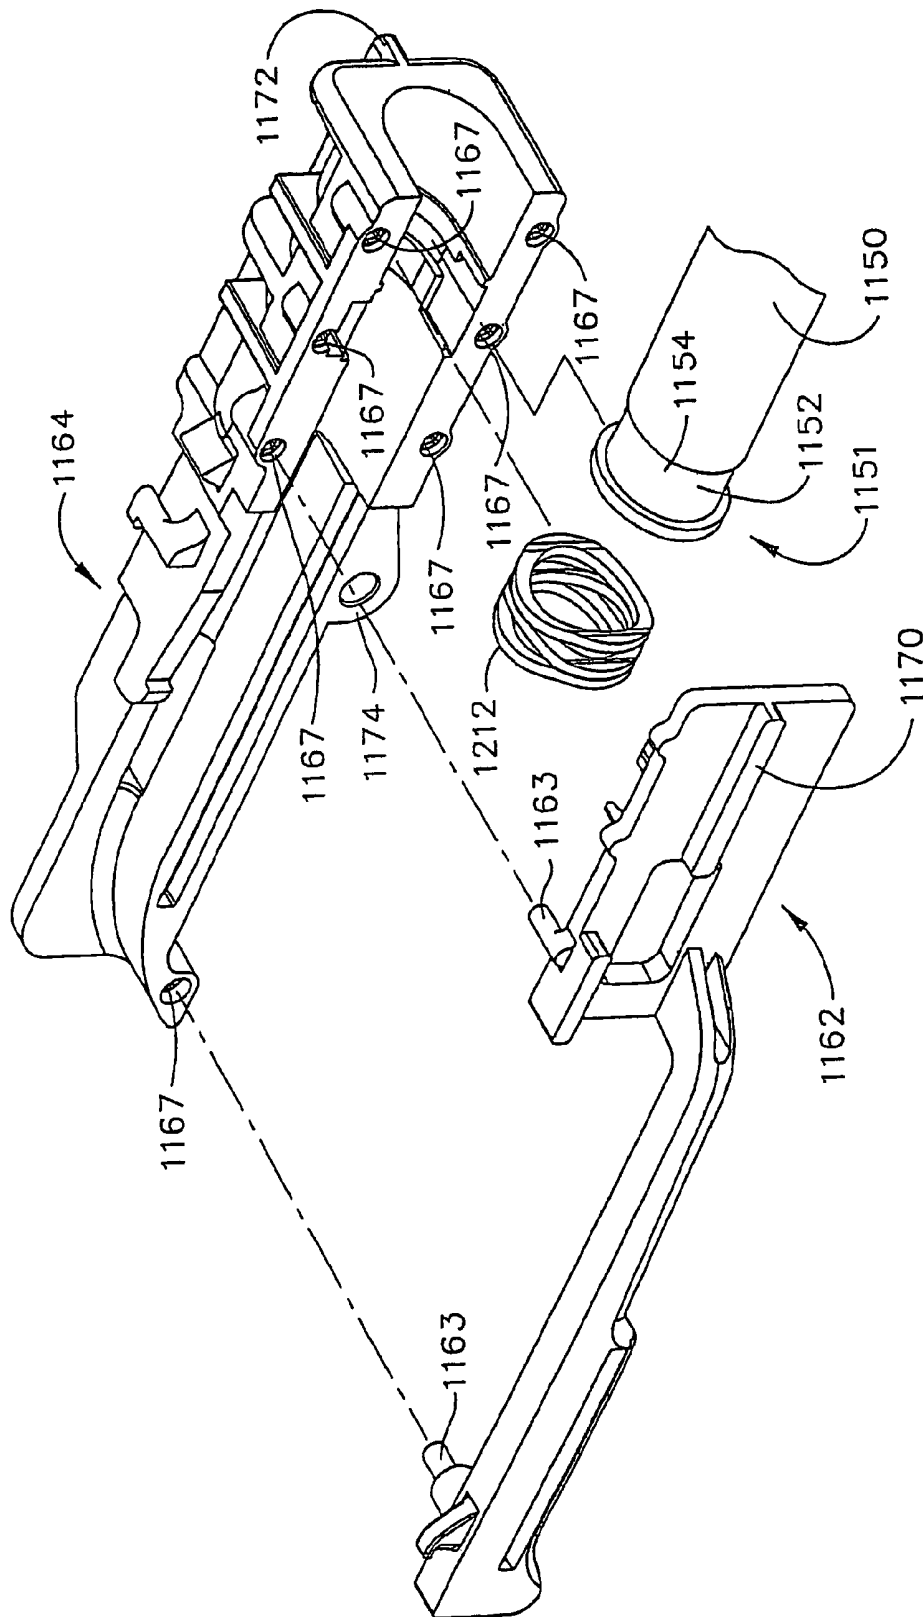


FIG. 61

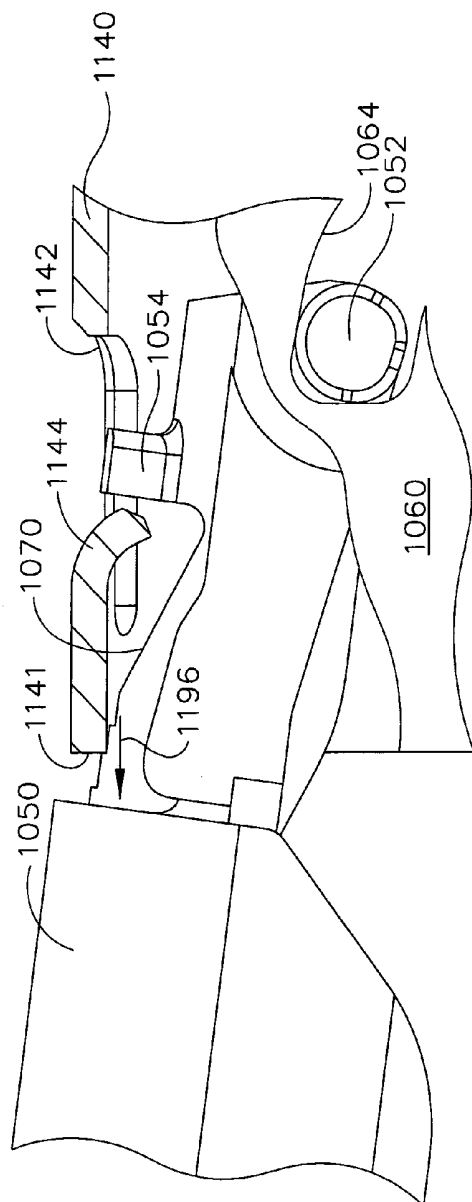


FIG. 62

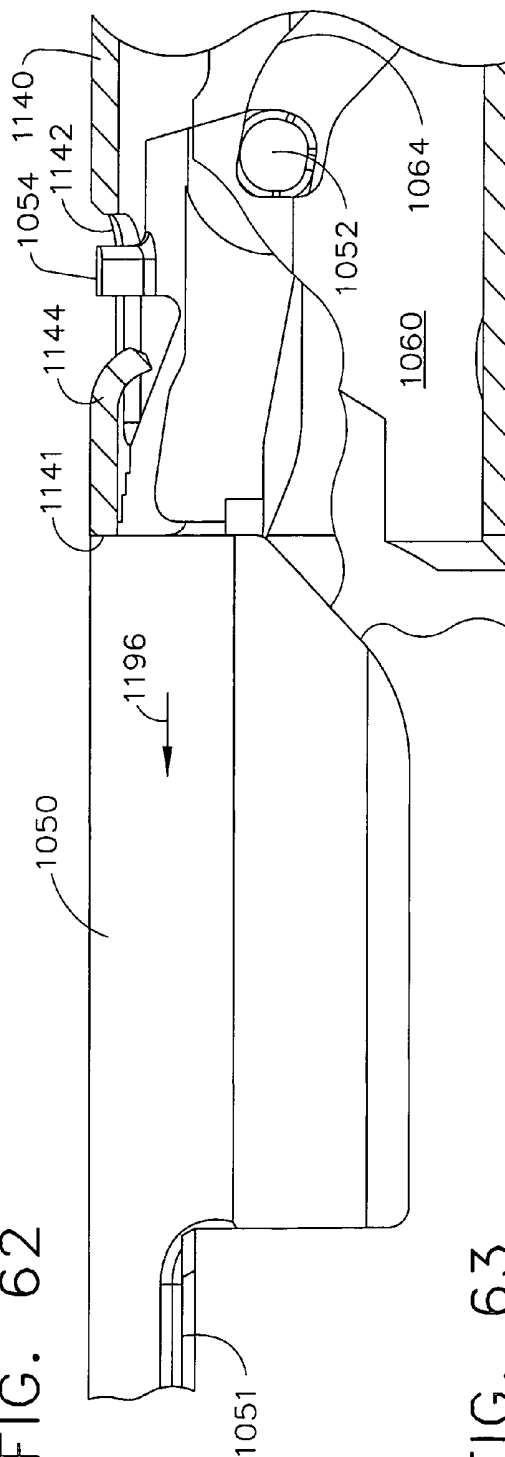


FIG. 63

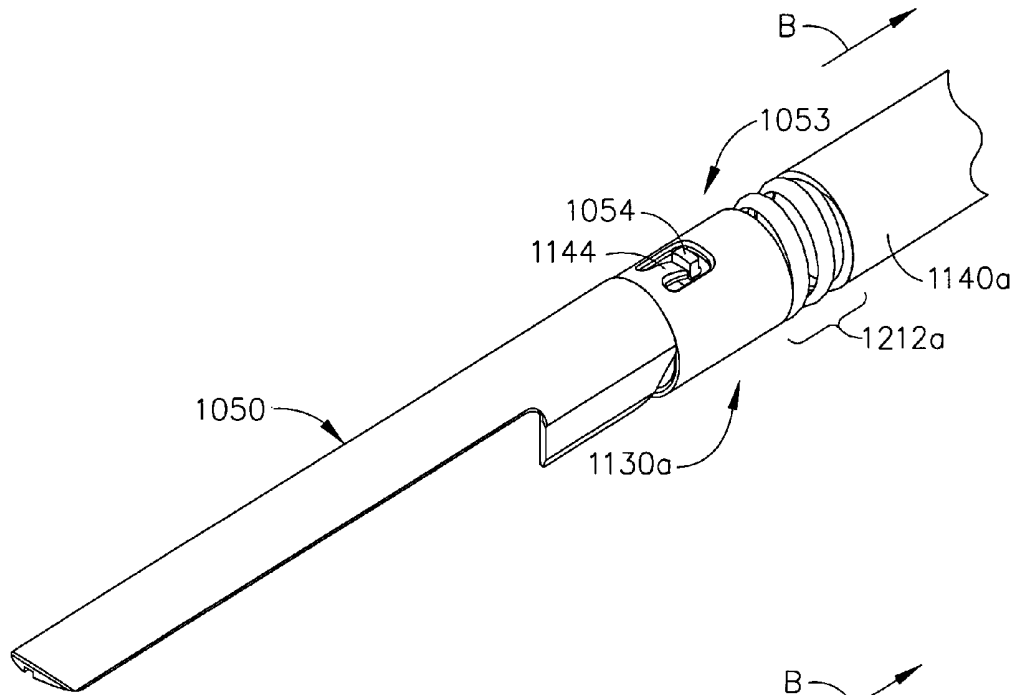


FIG. 64

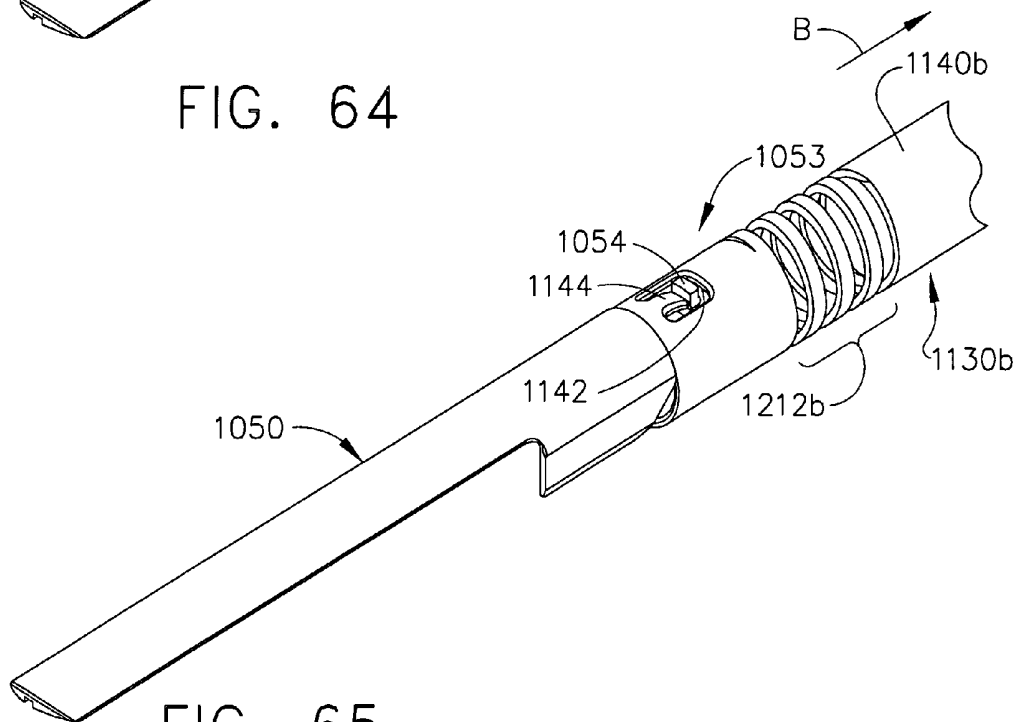


FIG. 65

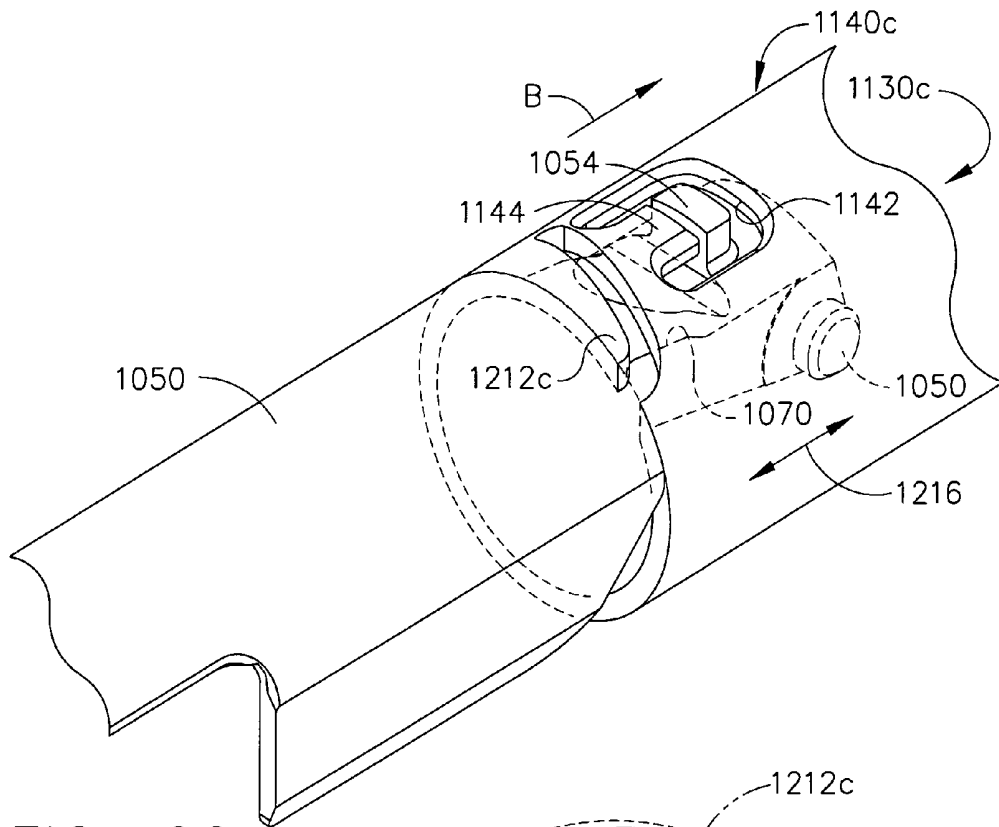


FIG. 66

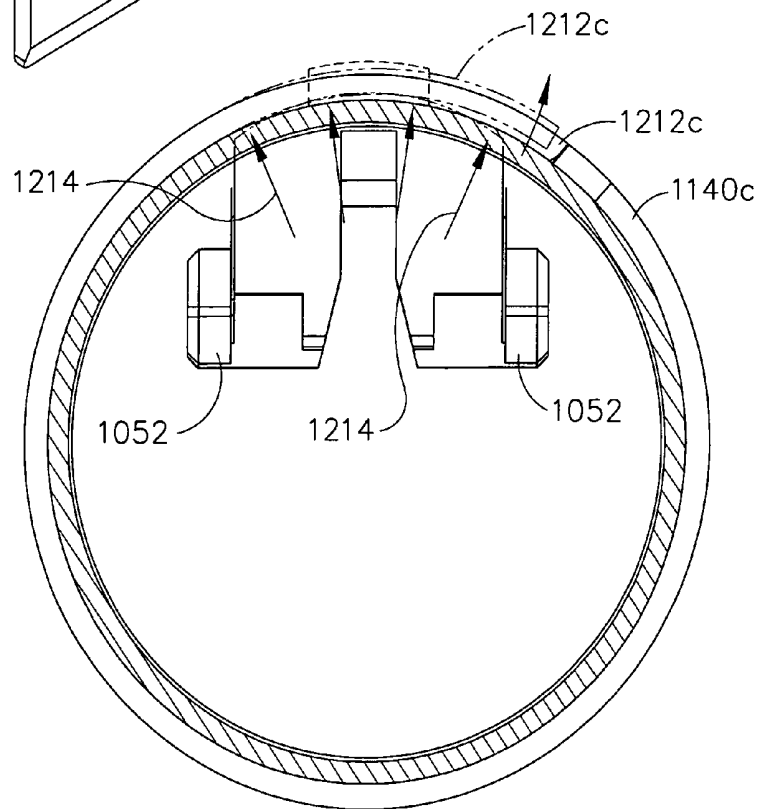
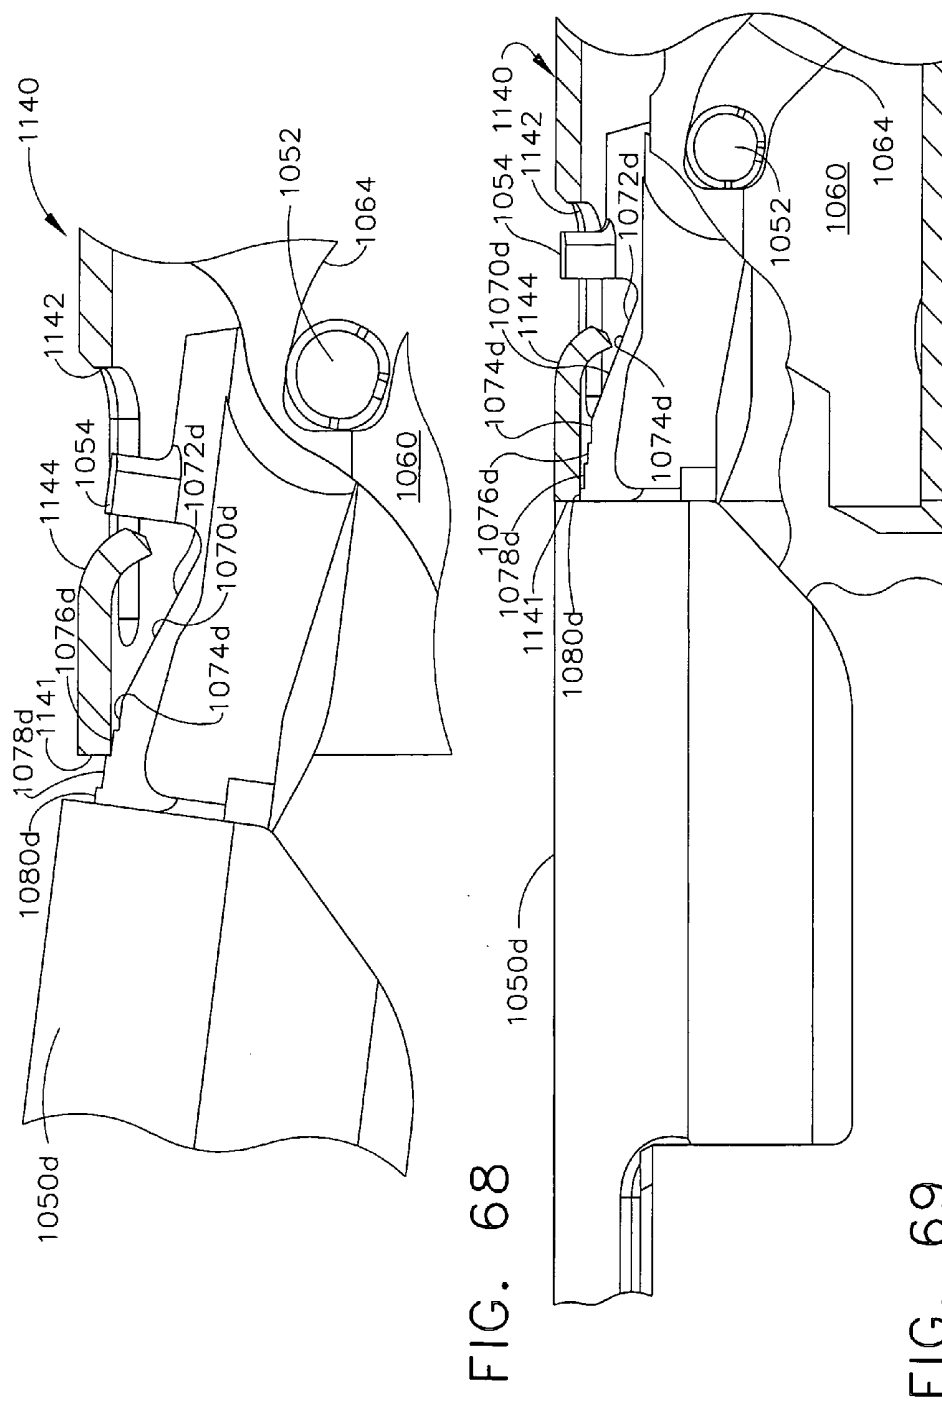


FIG. 67



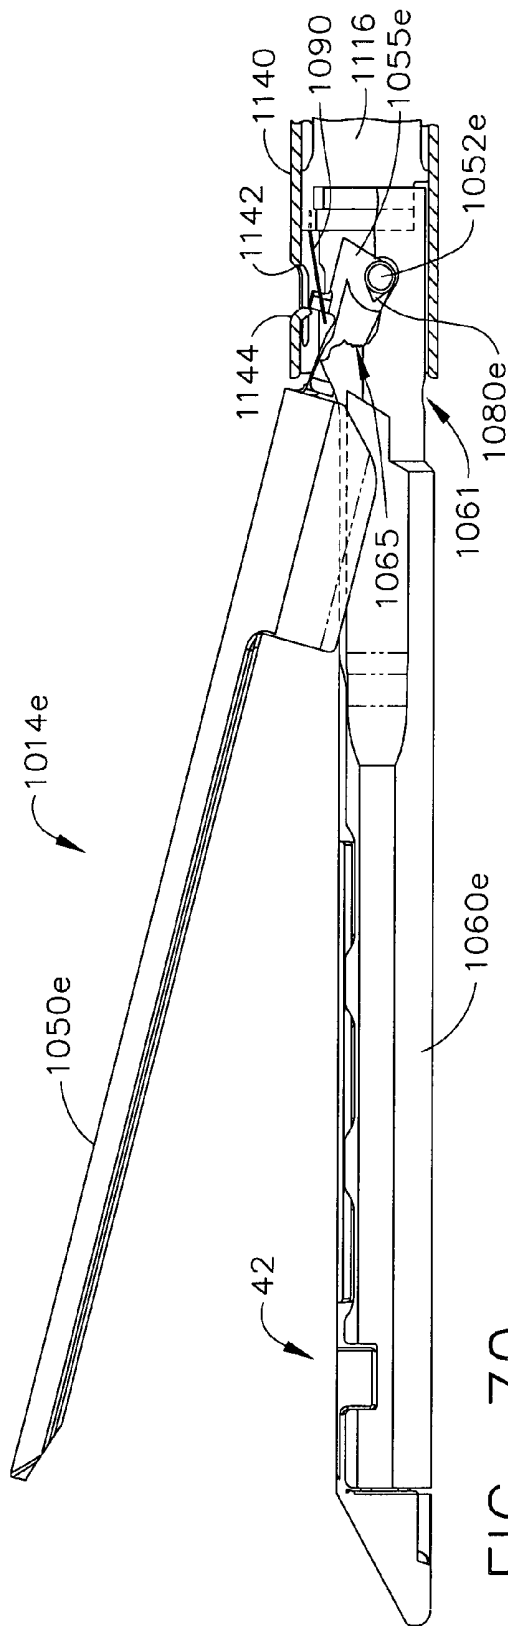


FIG. 70

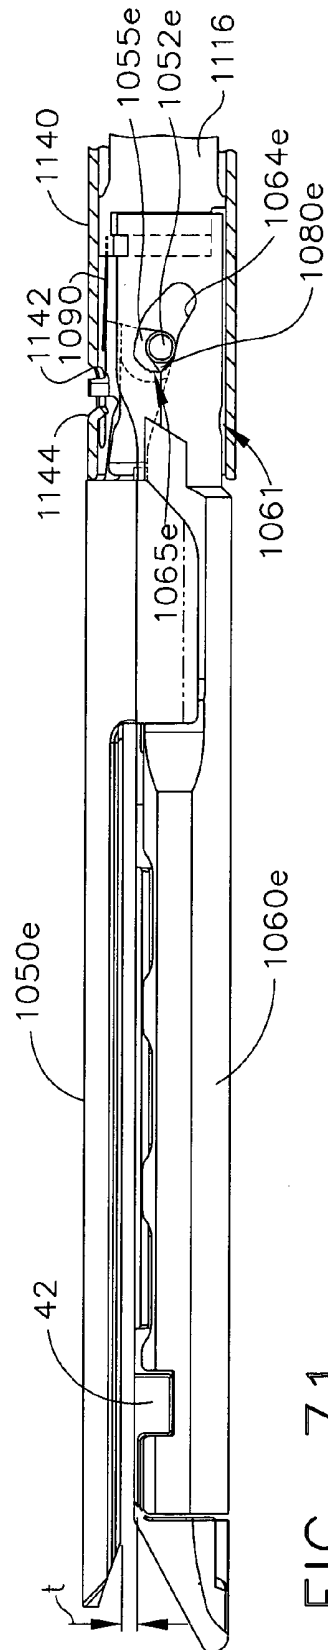


FIG. 71

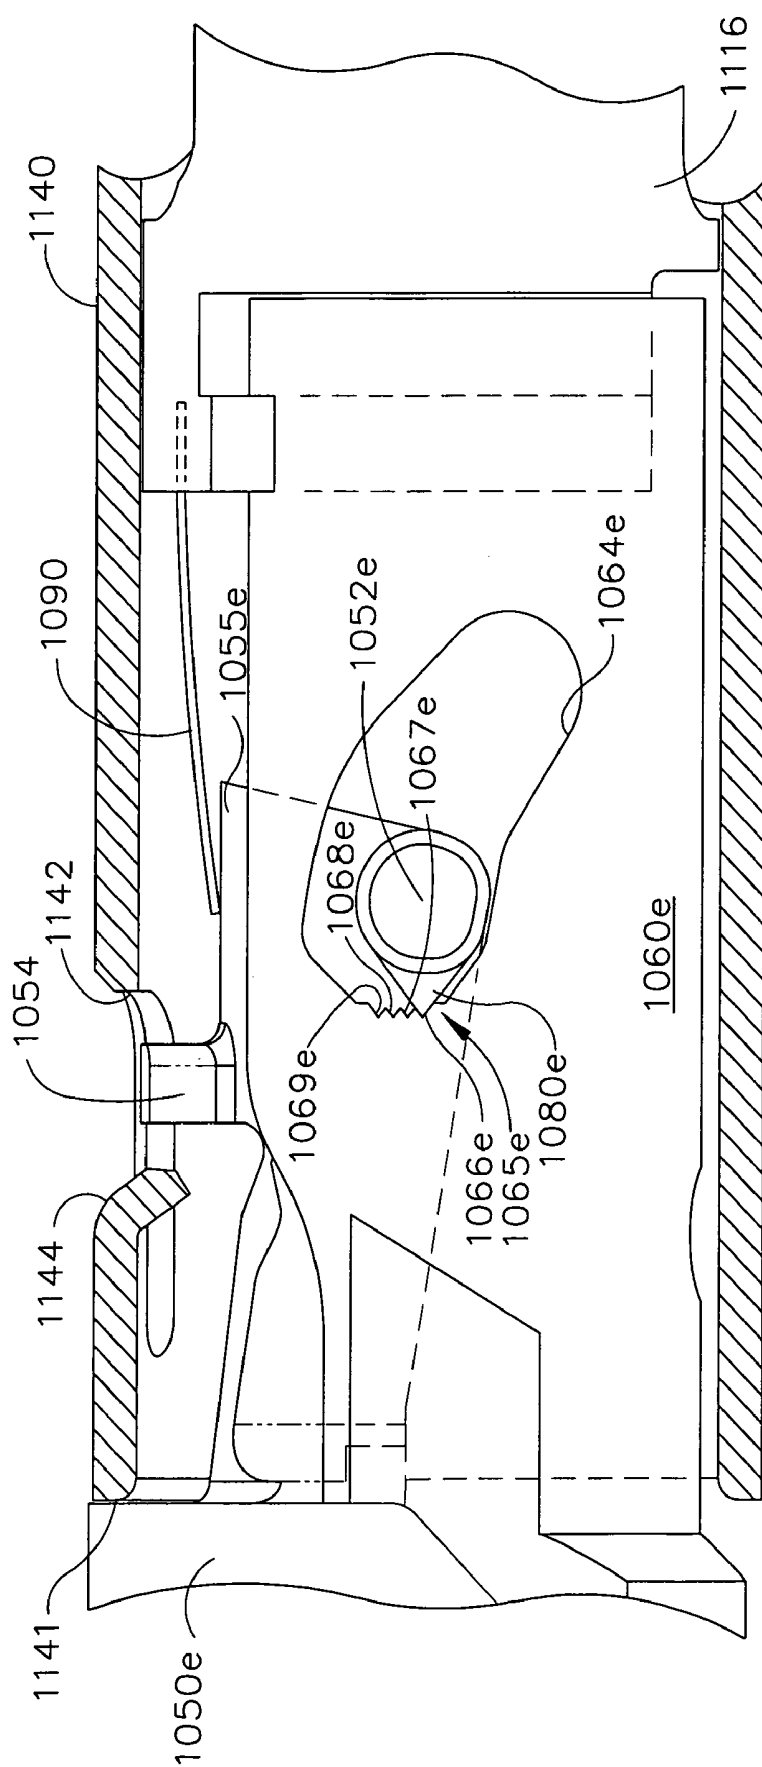


FIG. 72

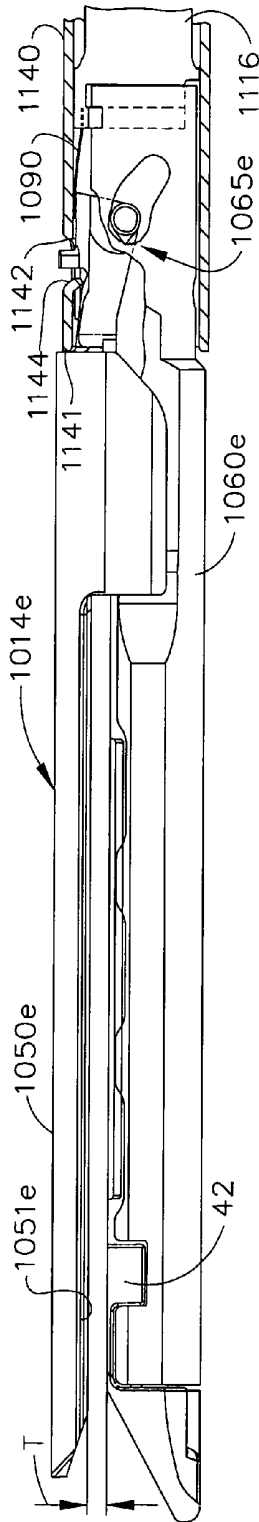


FIG. 73

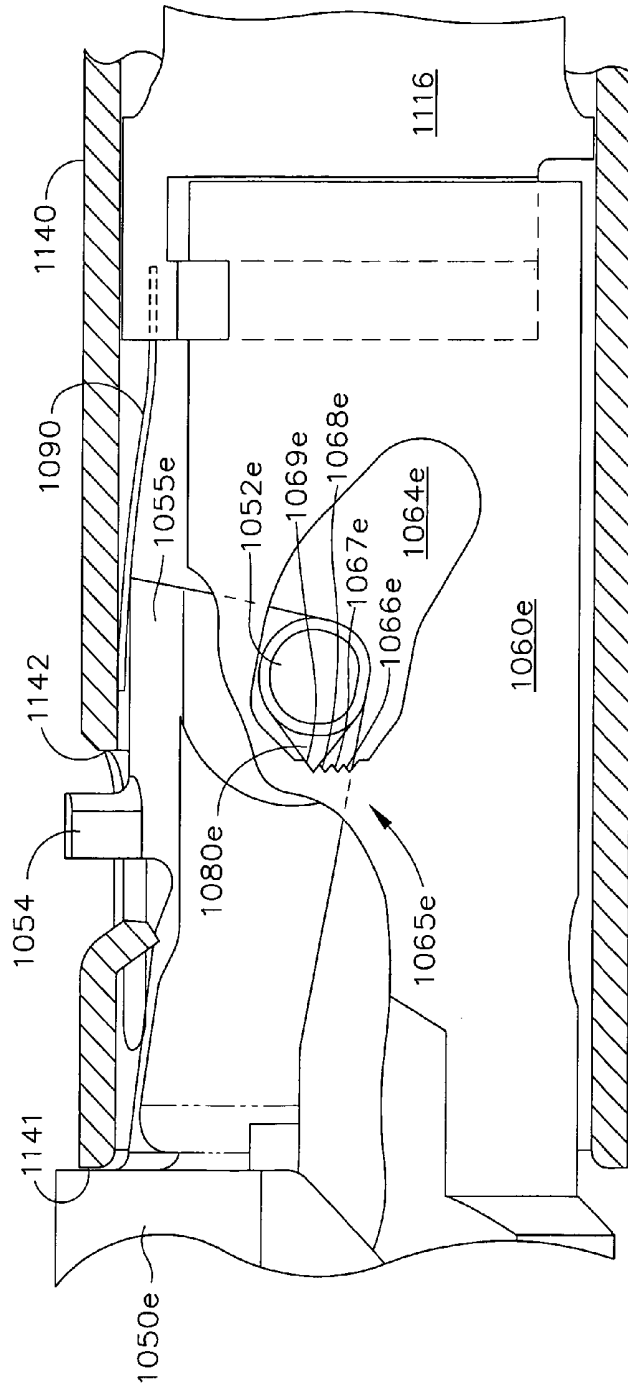


FIG. 74

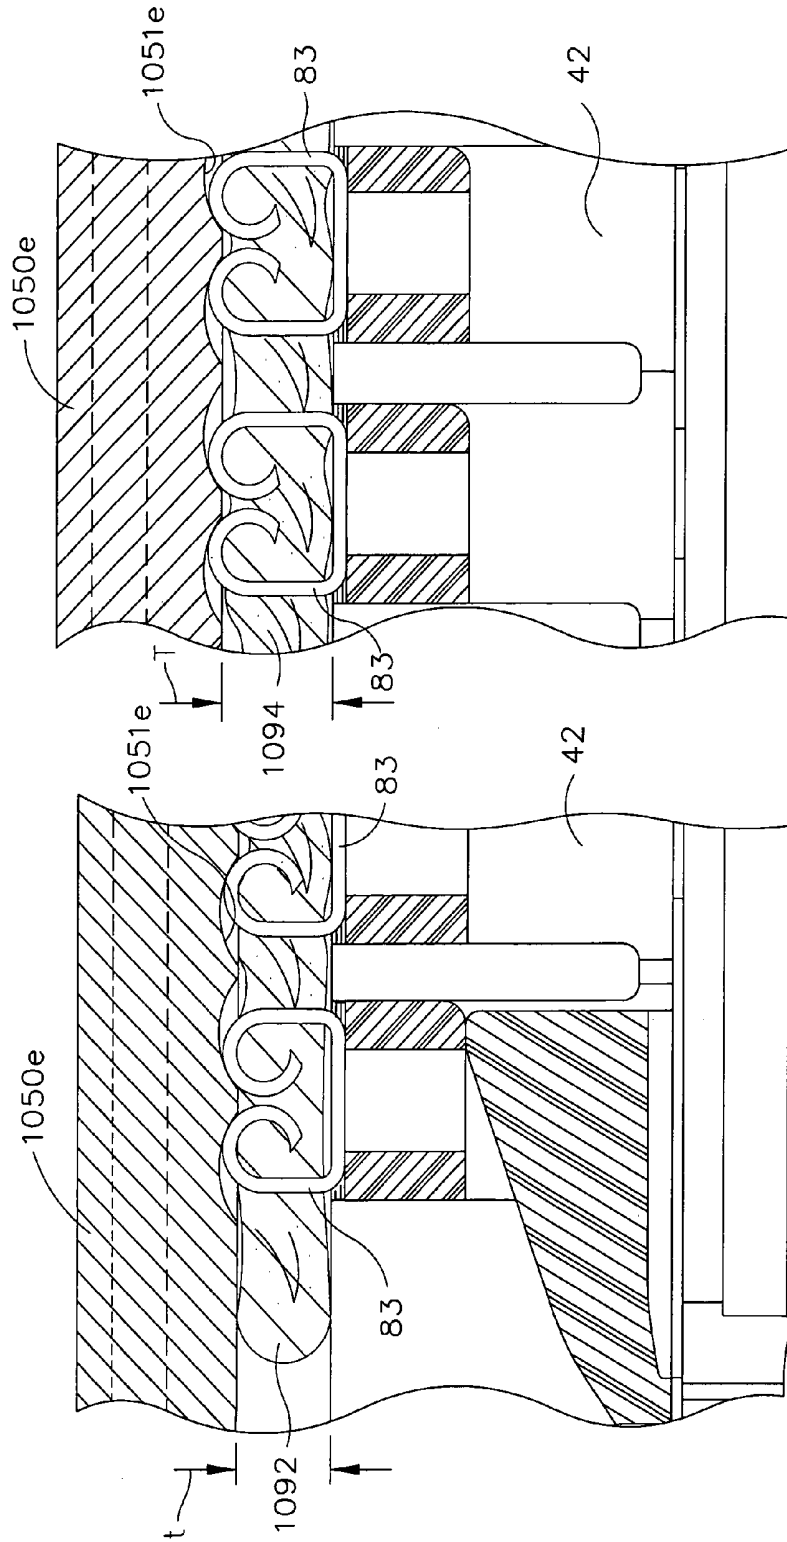


FIG. 75

FIG. 76

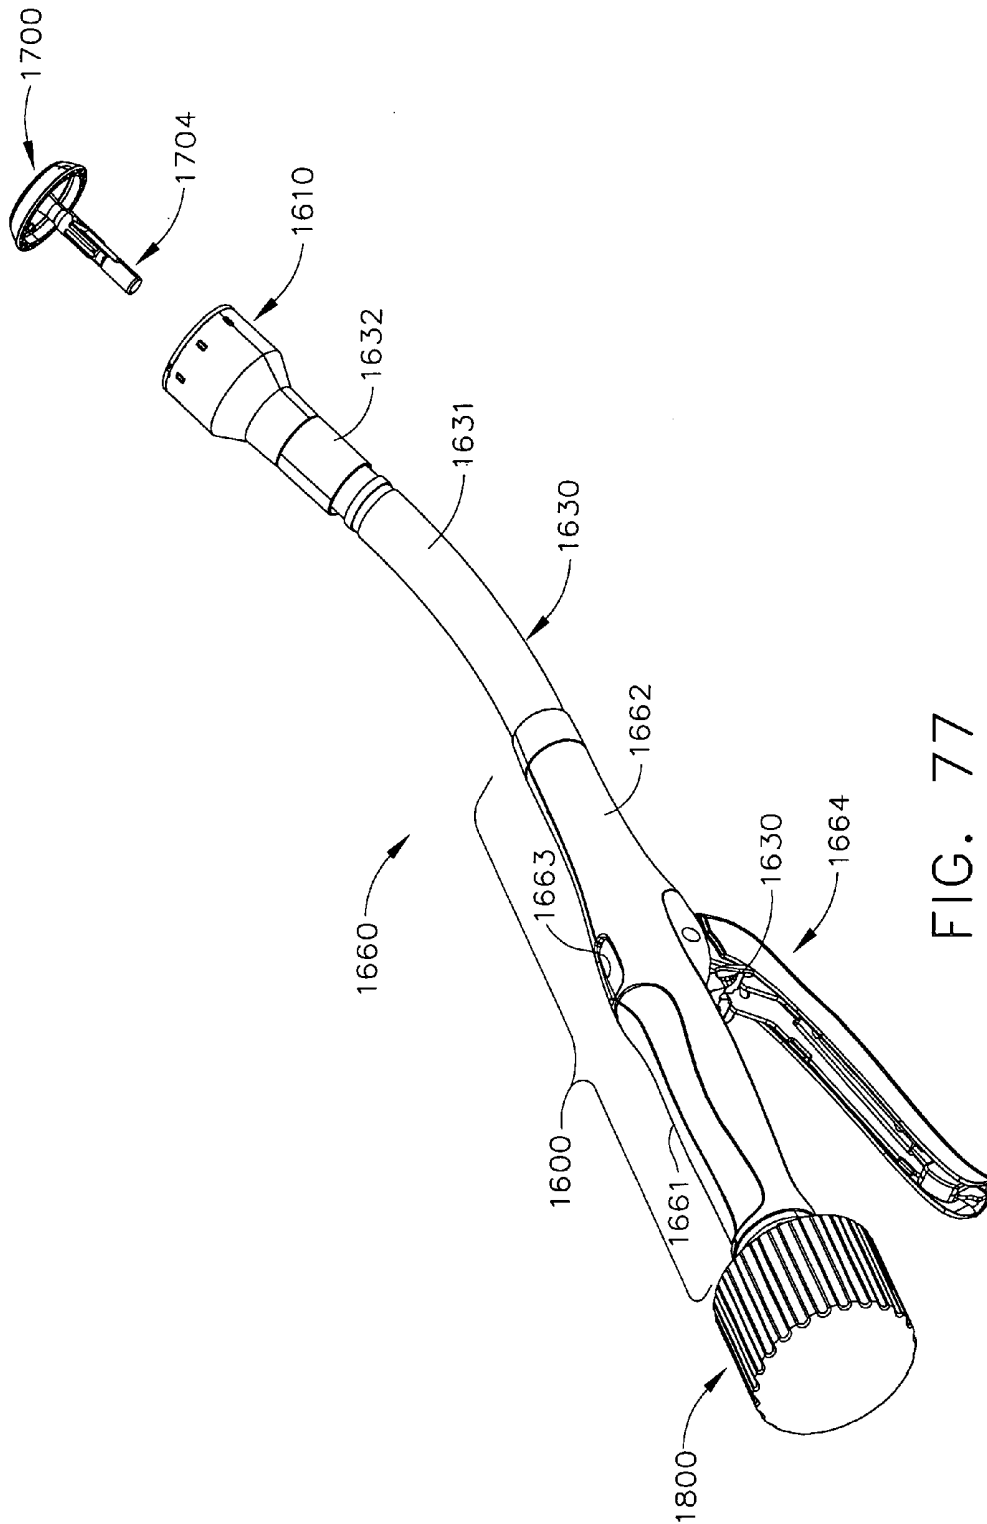


FIG. 77

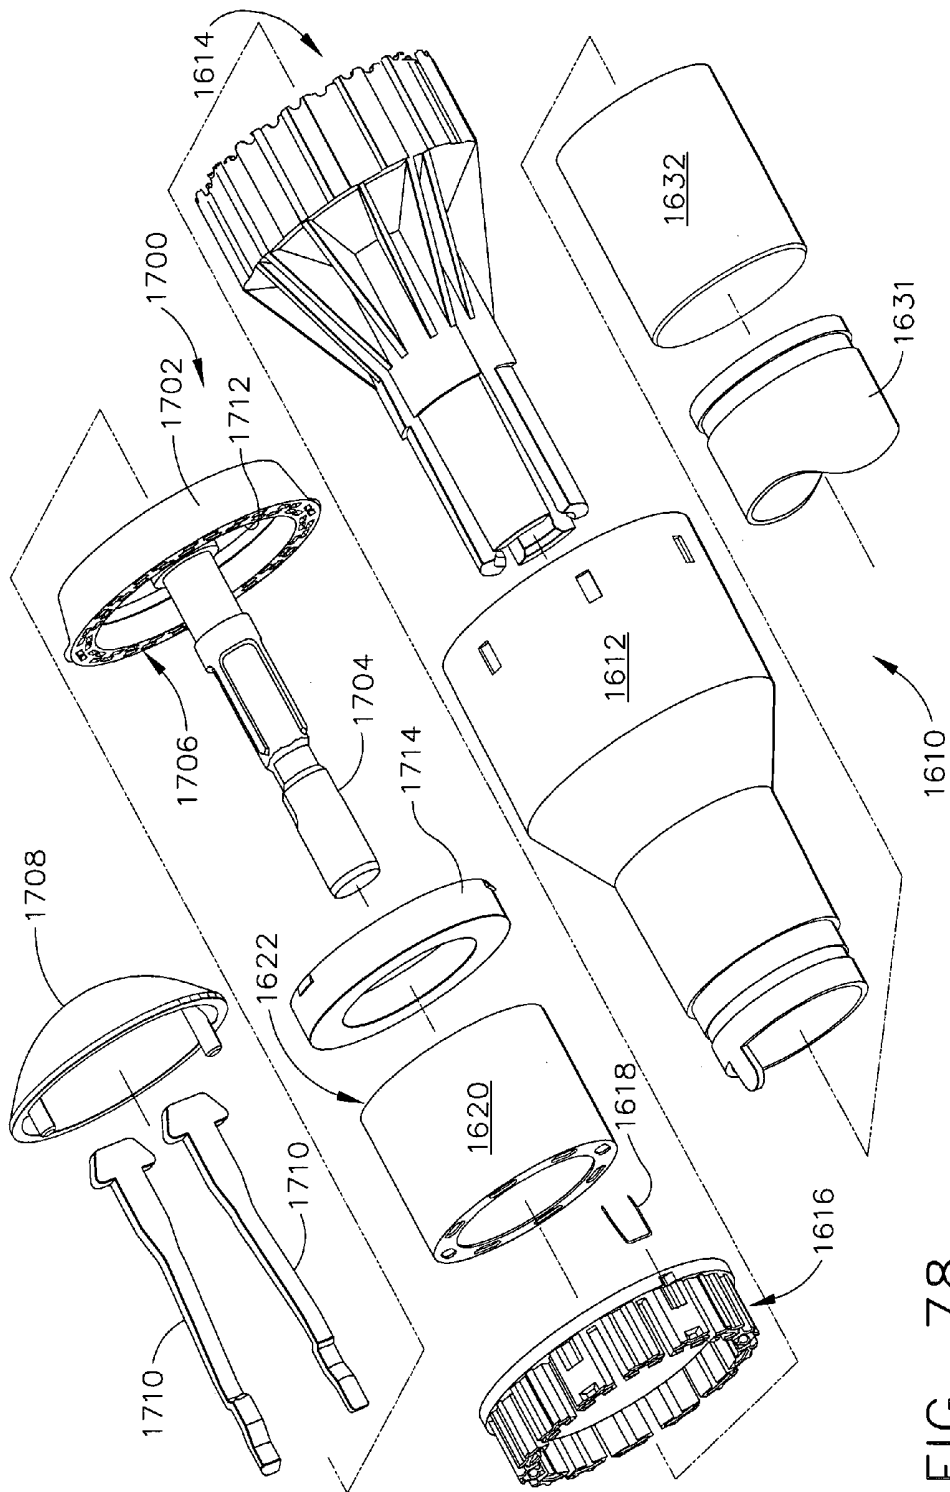
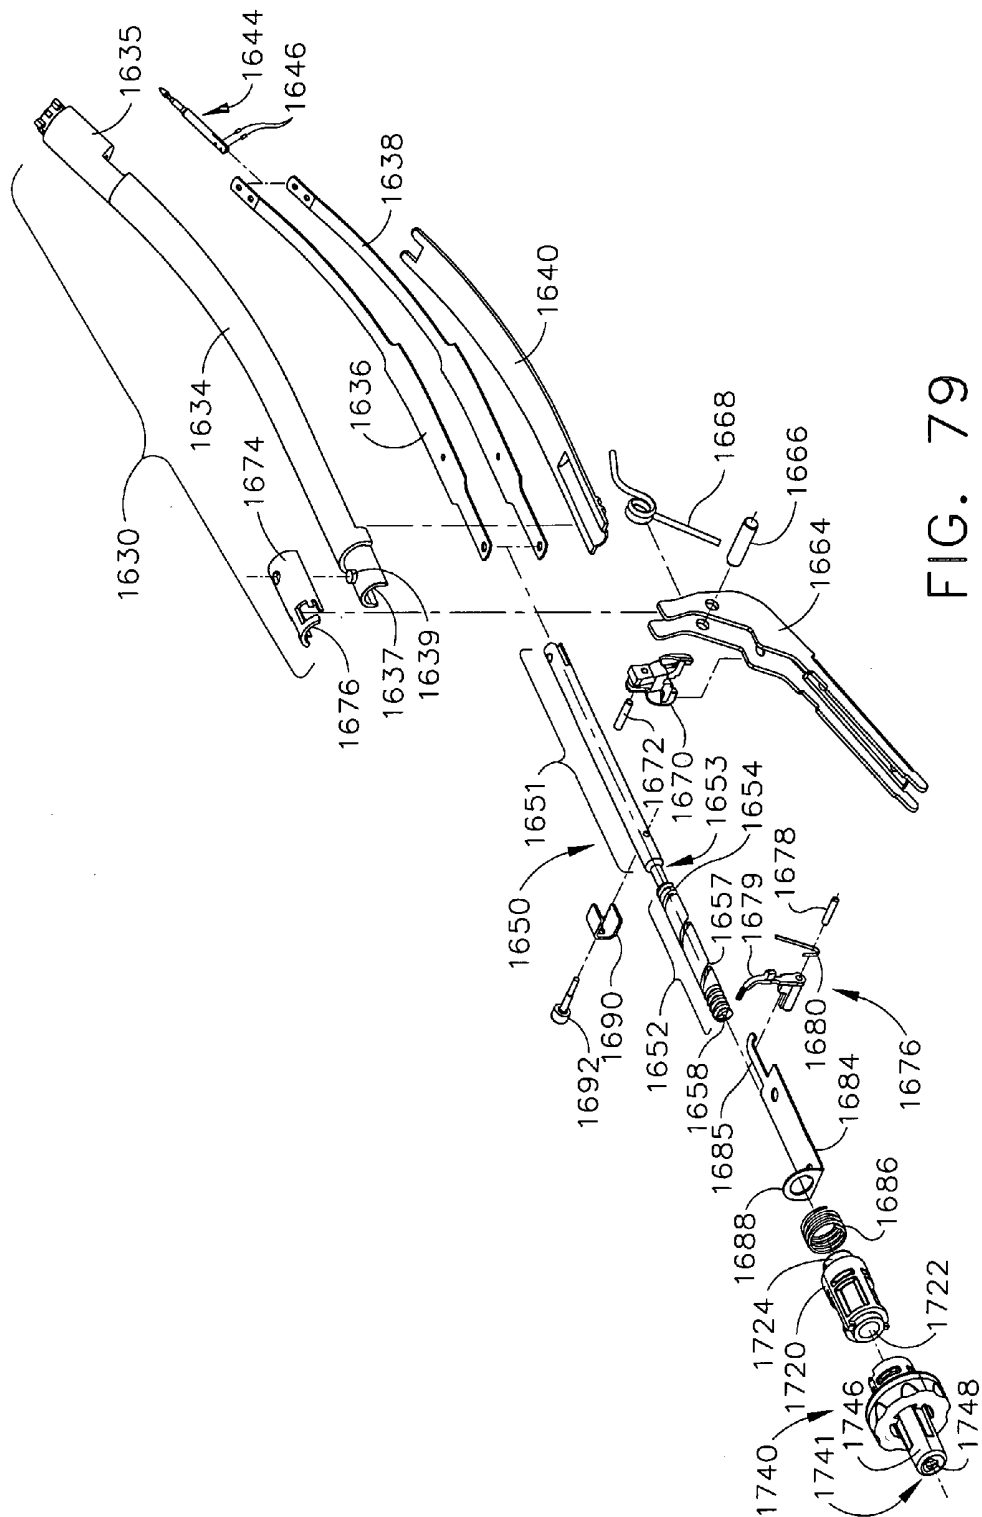


FIG. 78



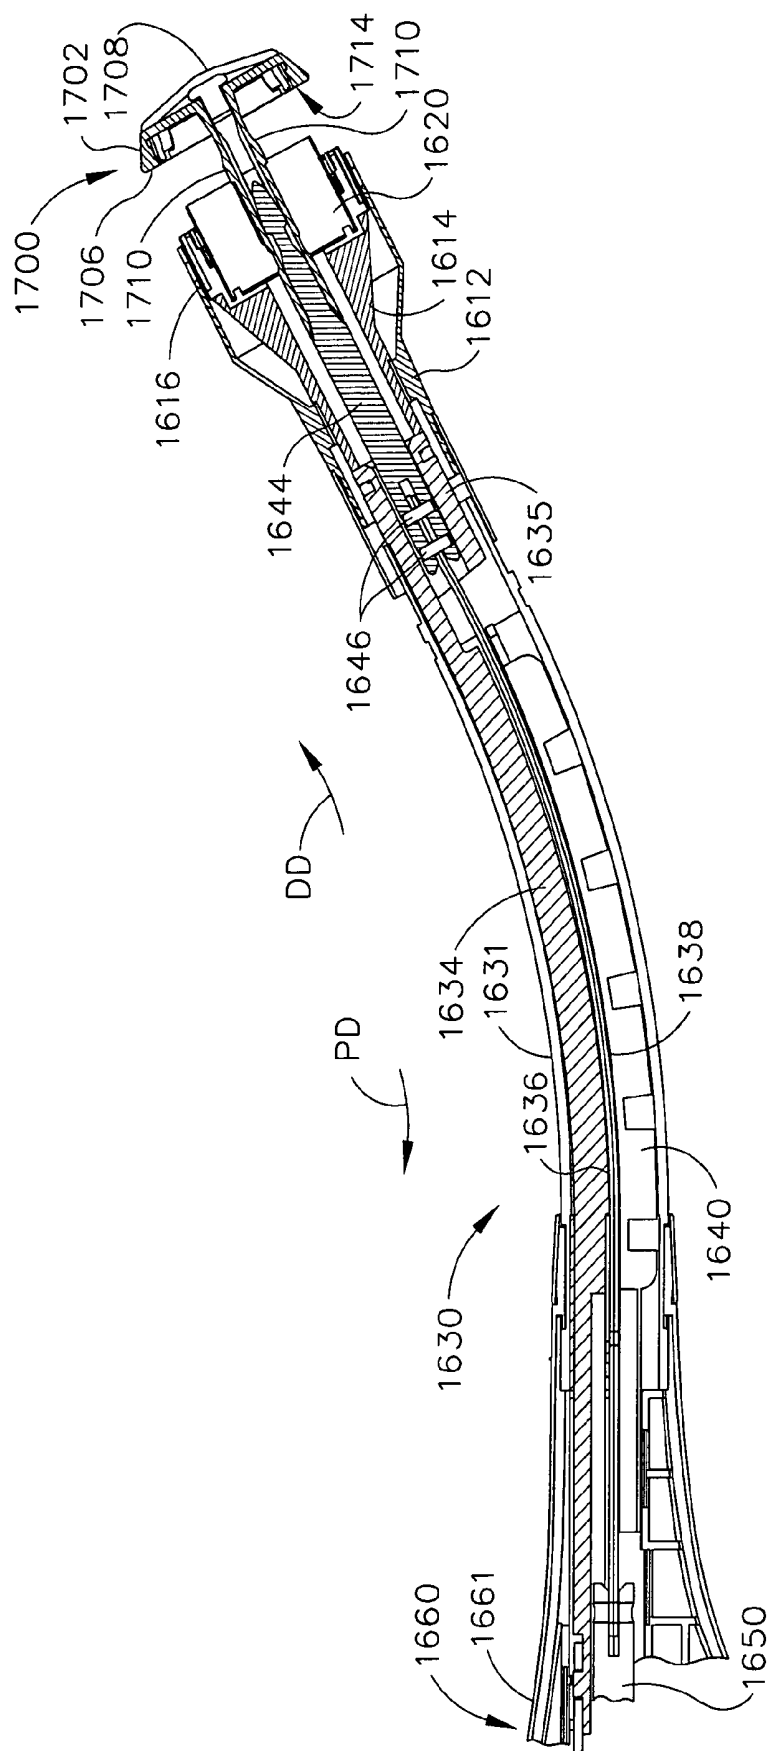


FIG. 80

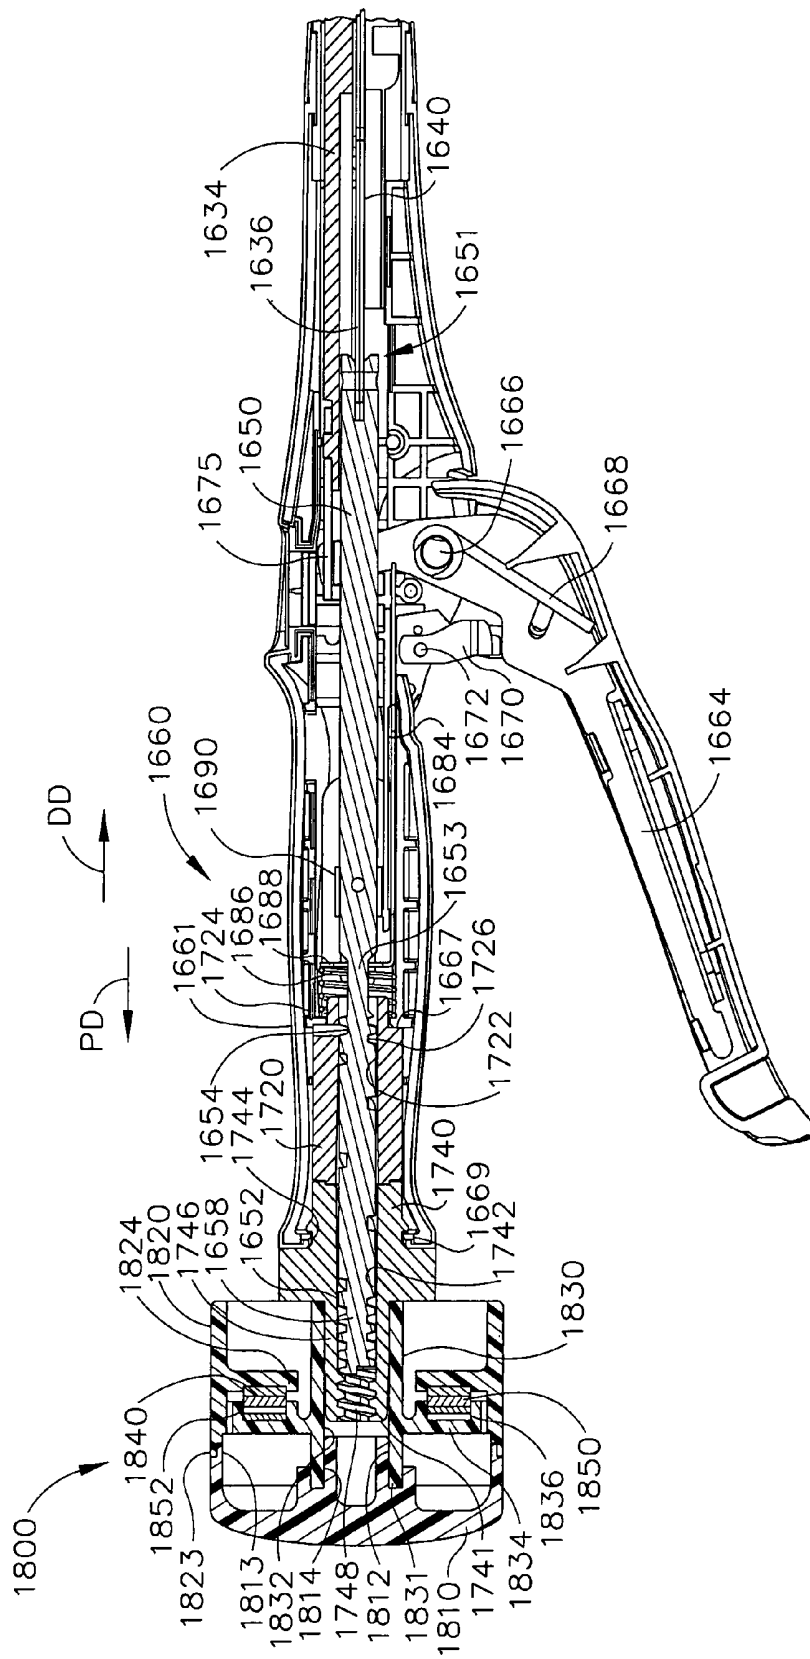


FIG. 81

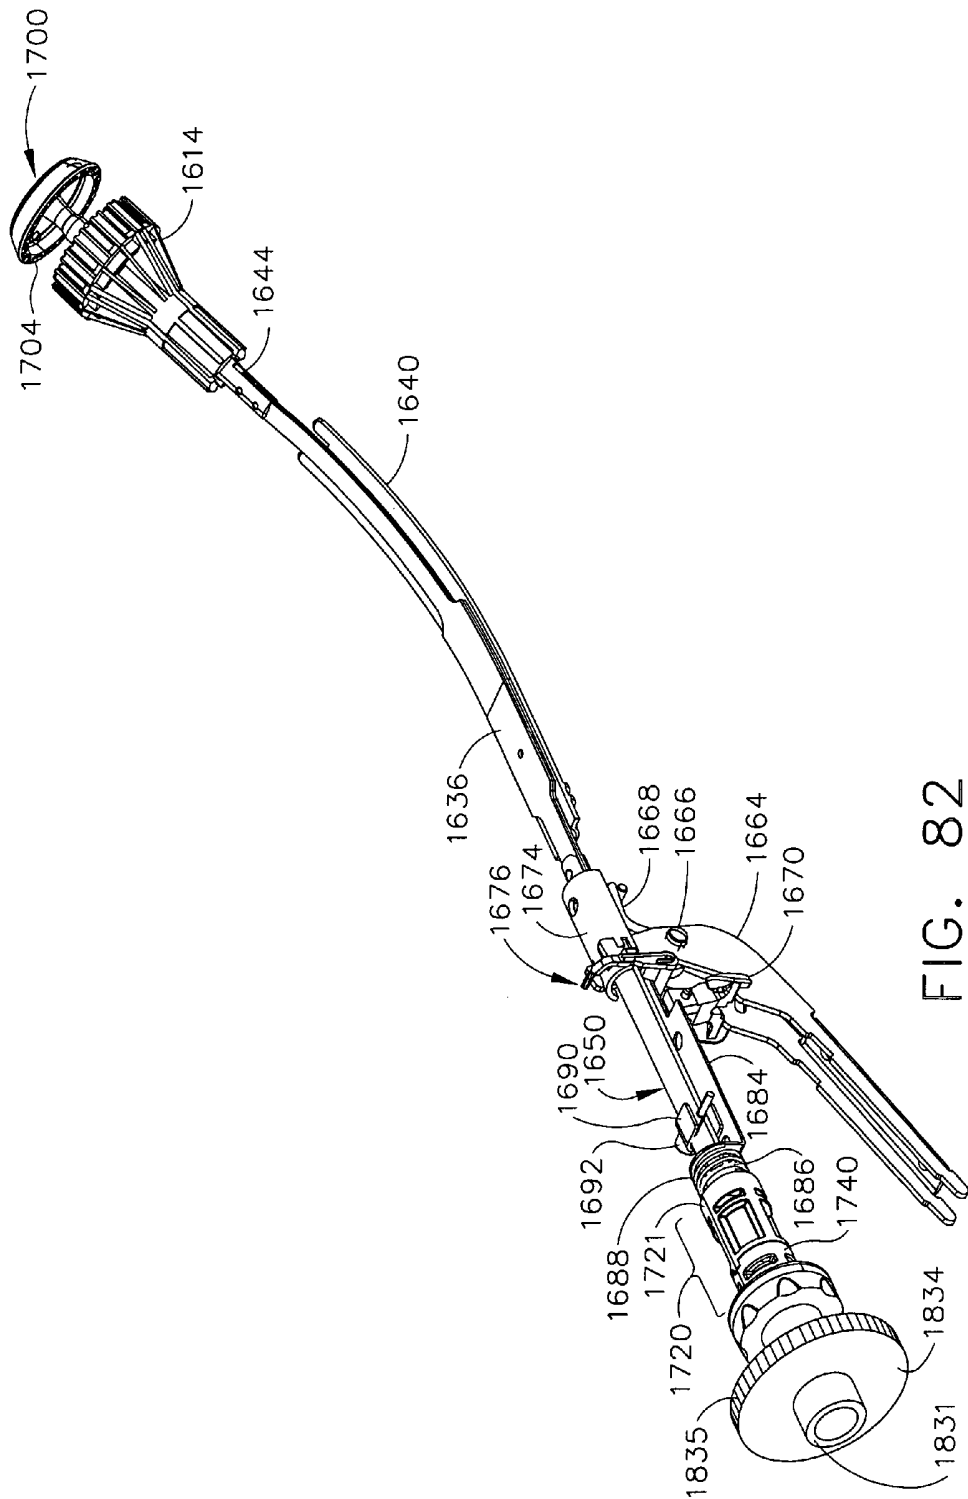


FIG. 82

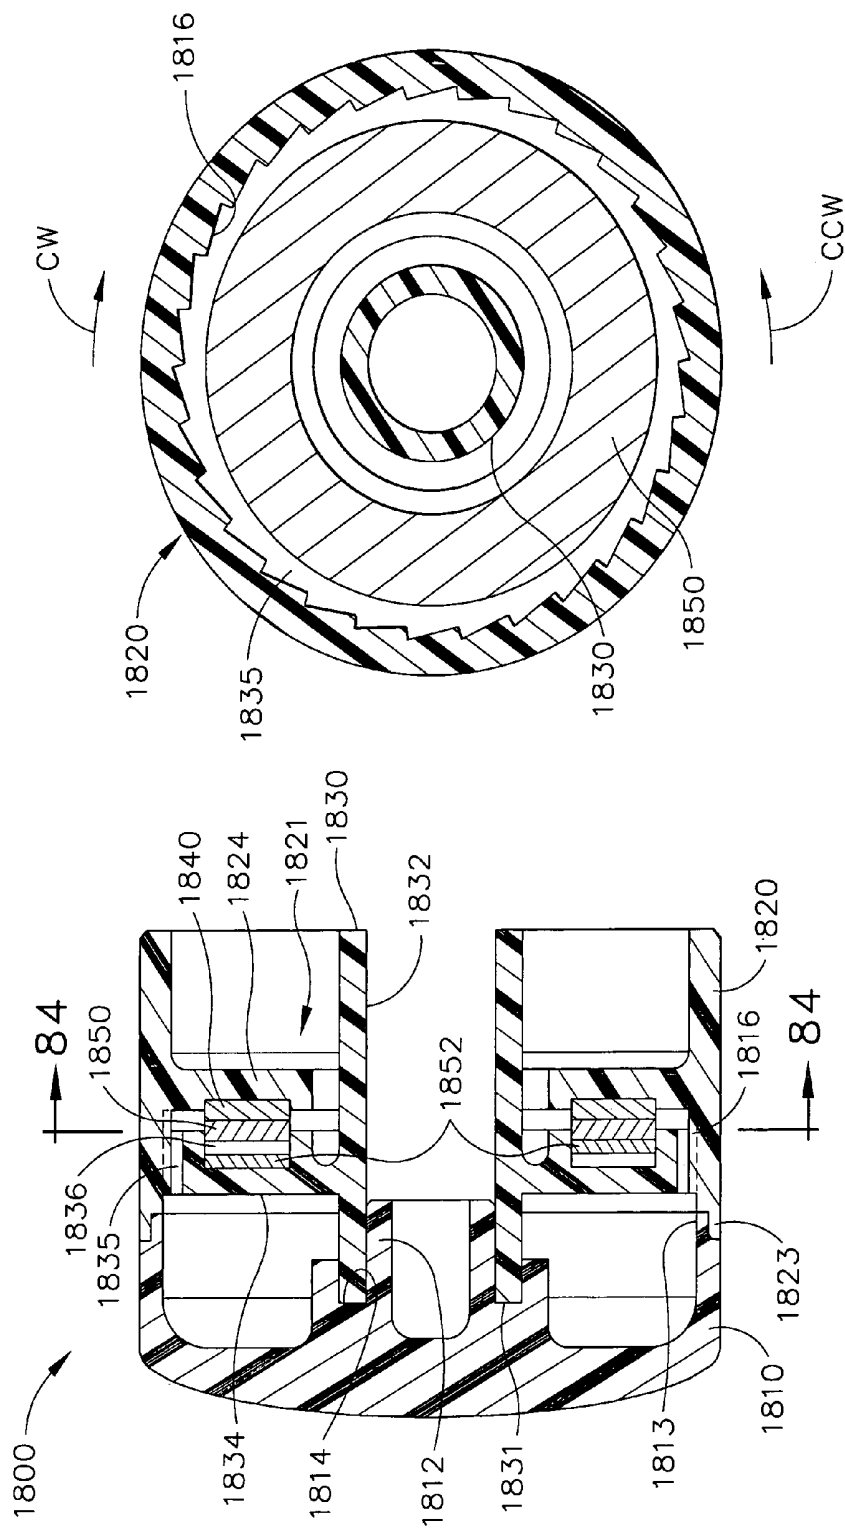


FIG. 84

FIG. 83

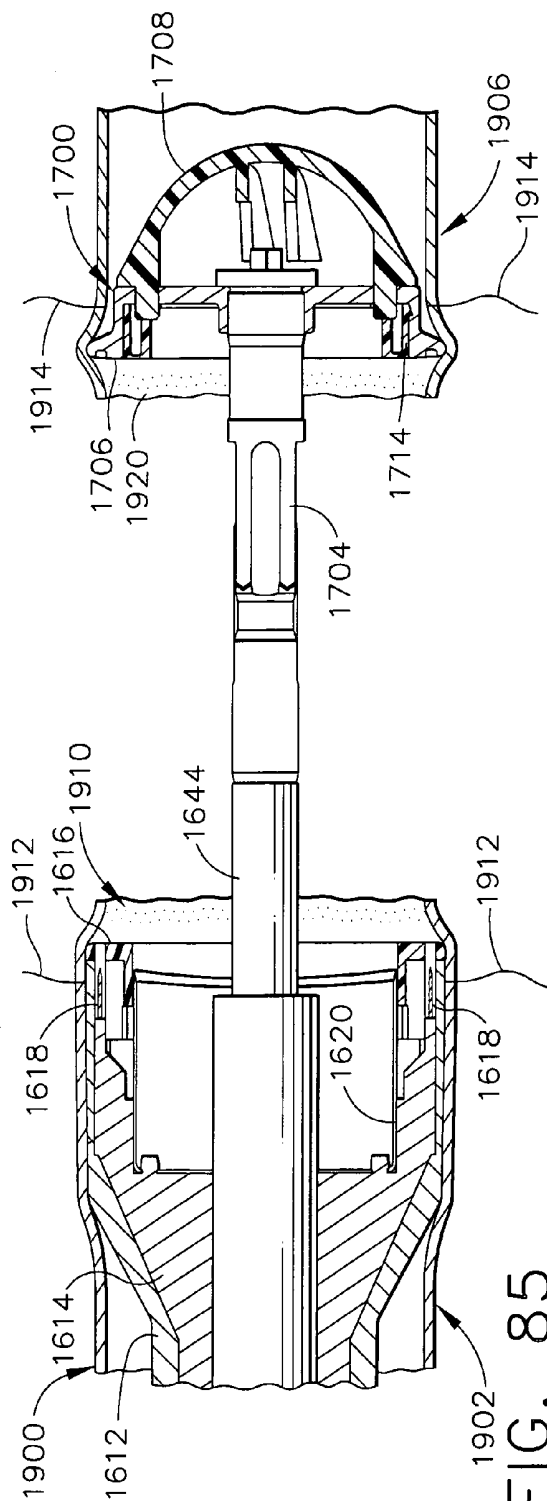


FIG. 58

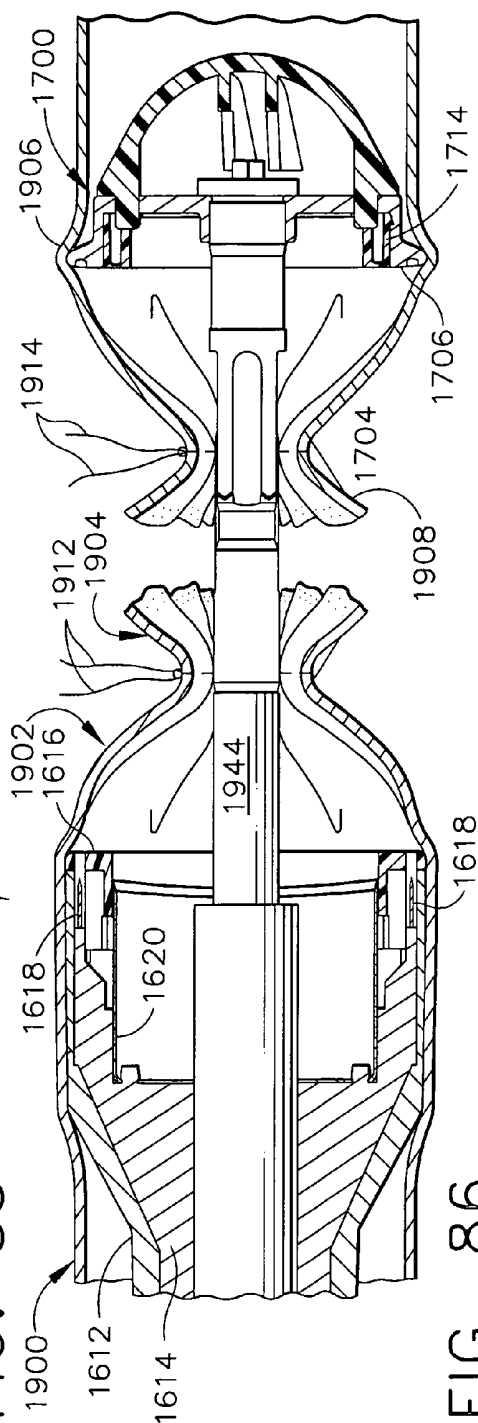


FIG. 68

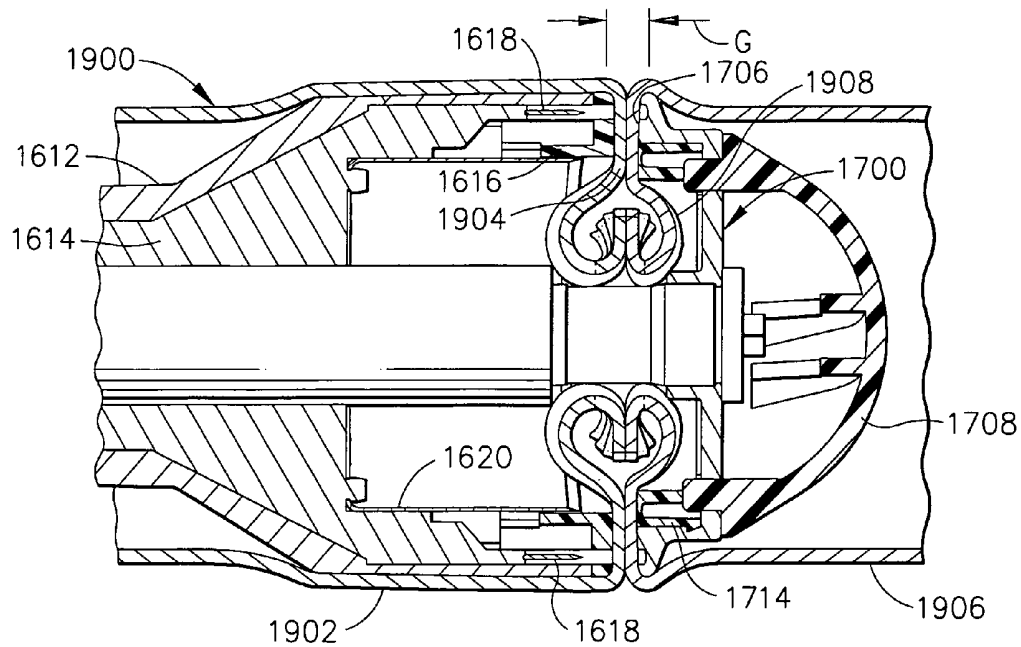


FIG. 87

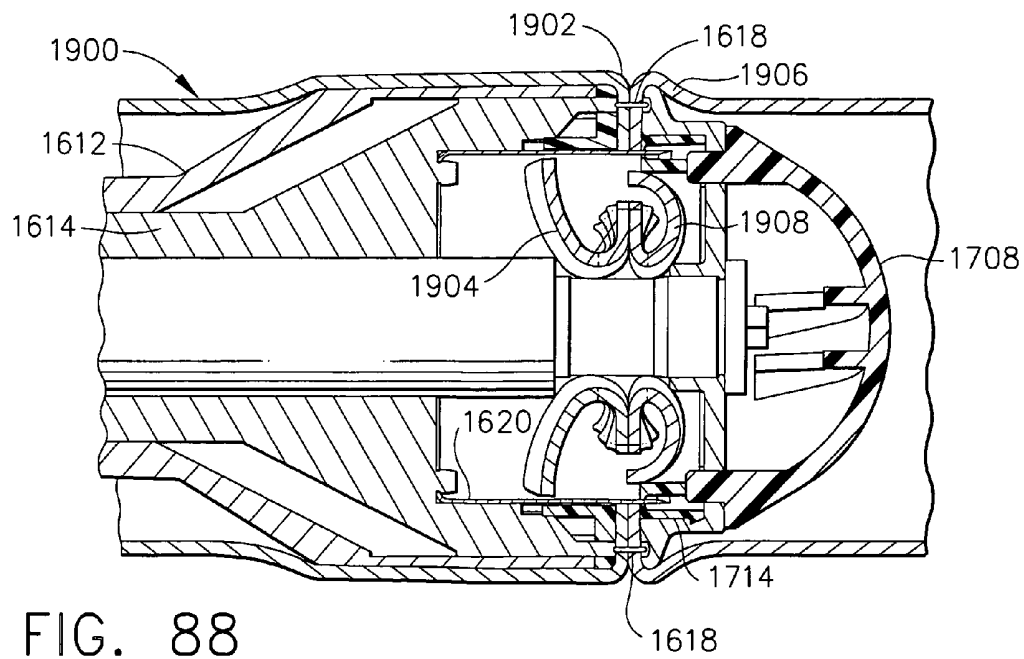


FIG. 88

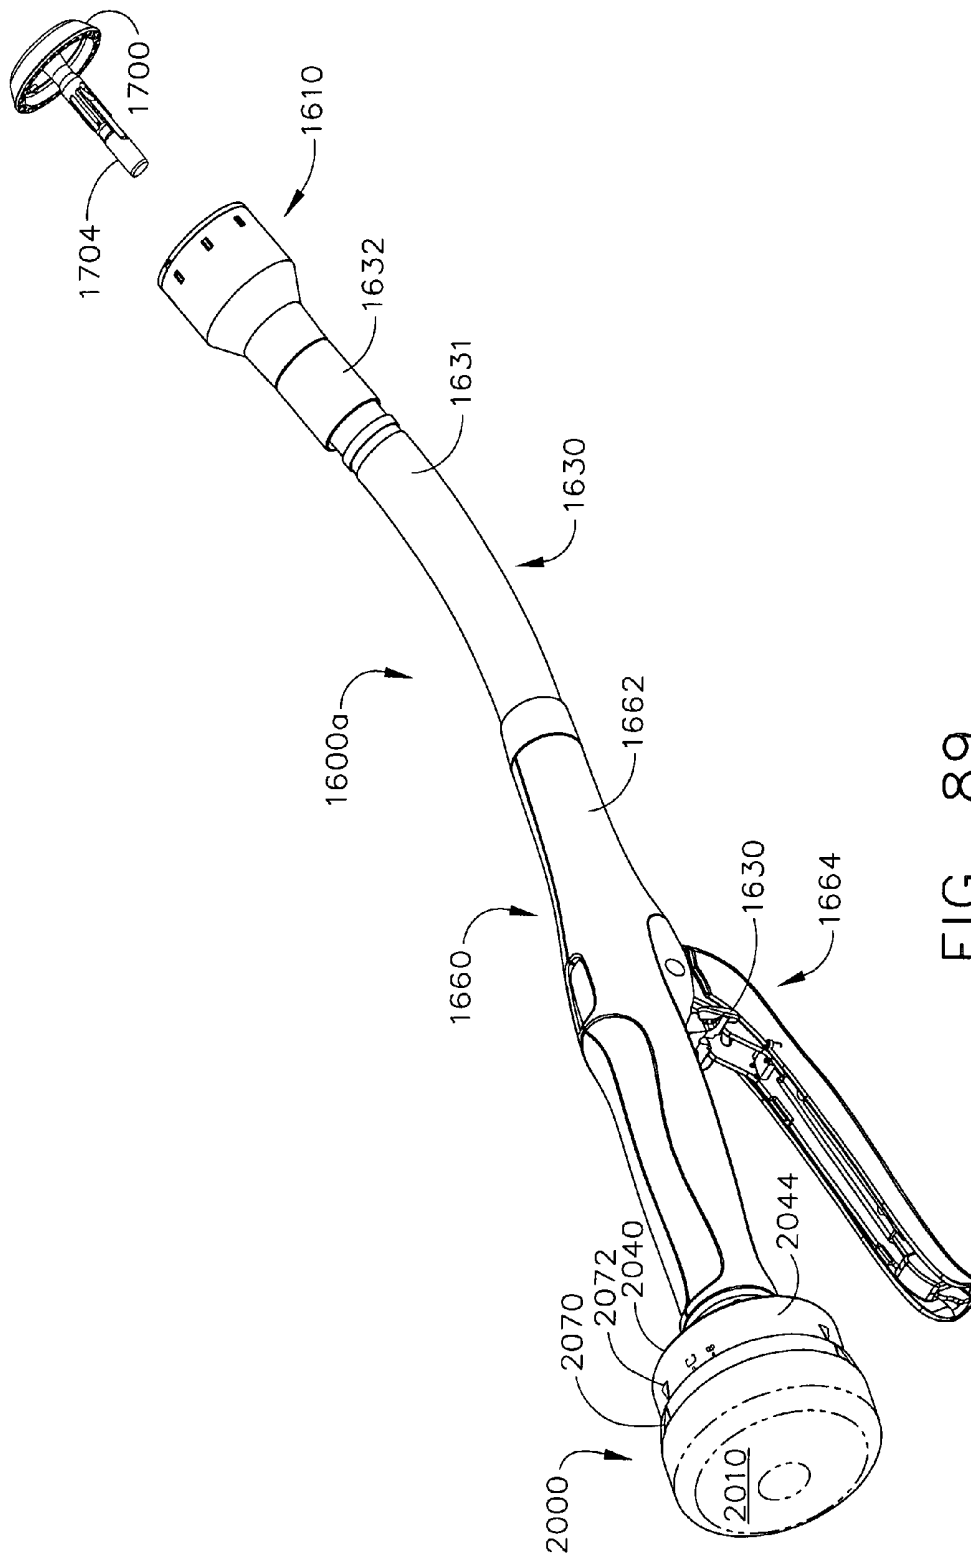


FIG. 89

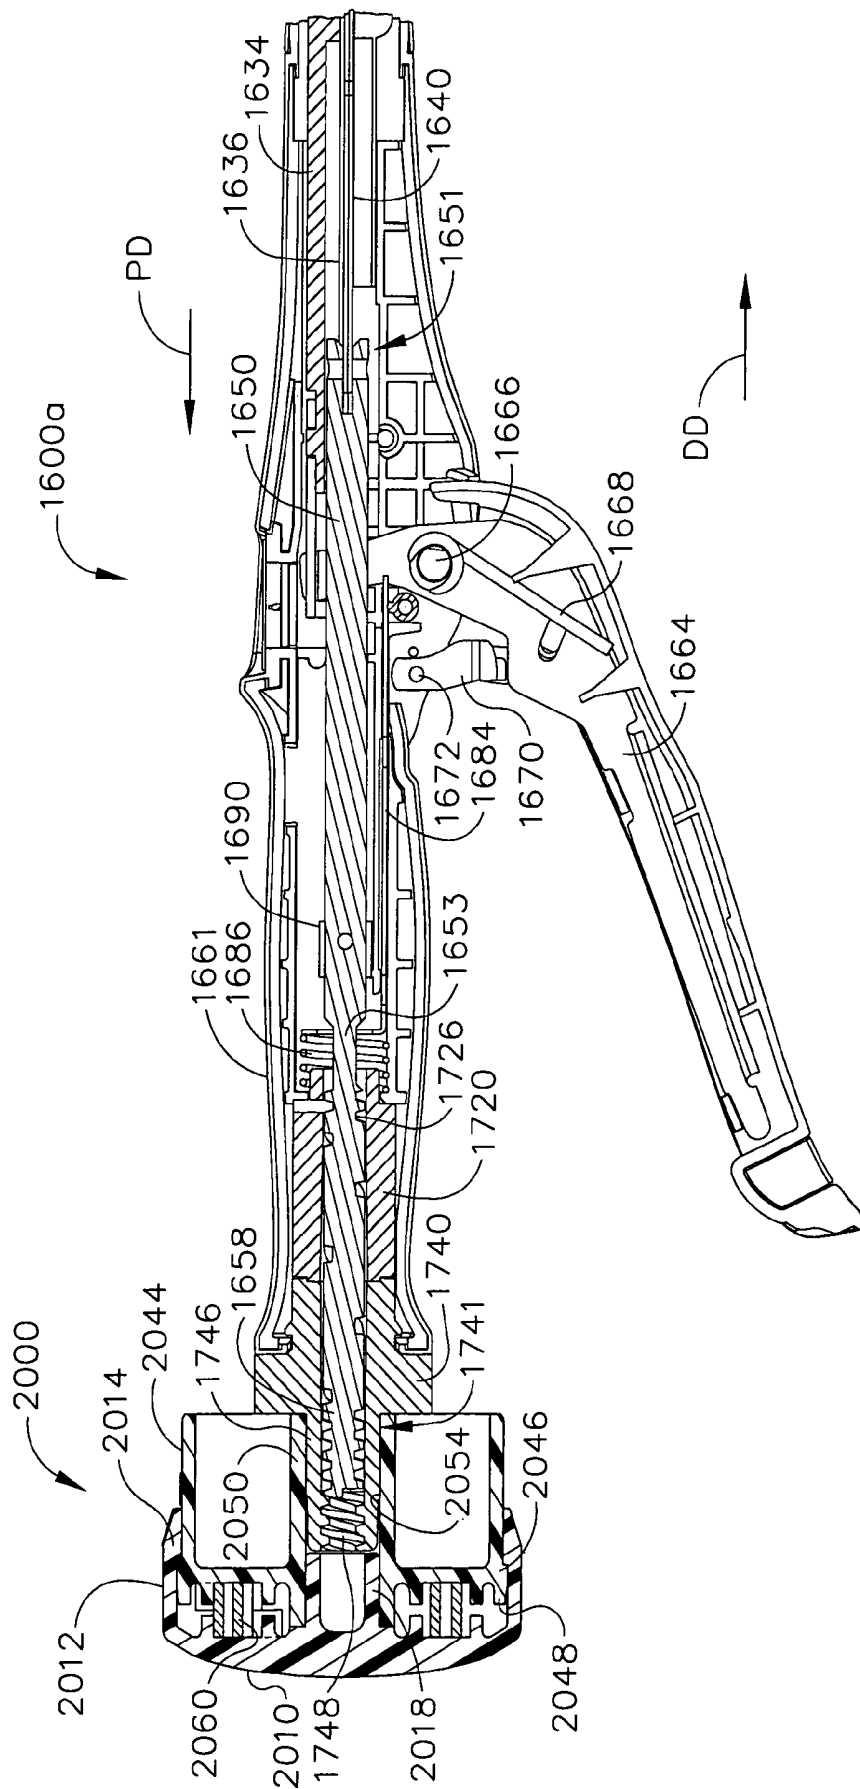


FIG. 90

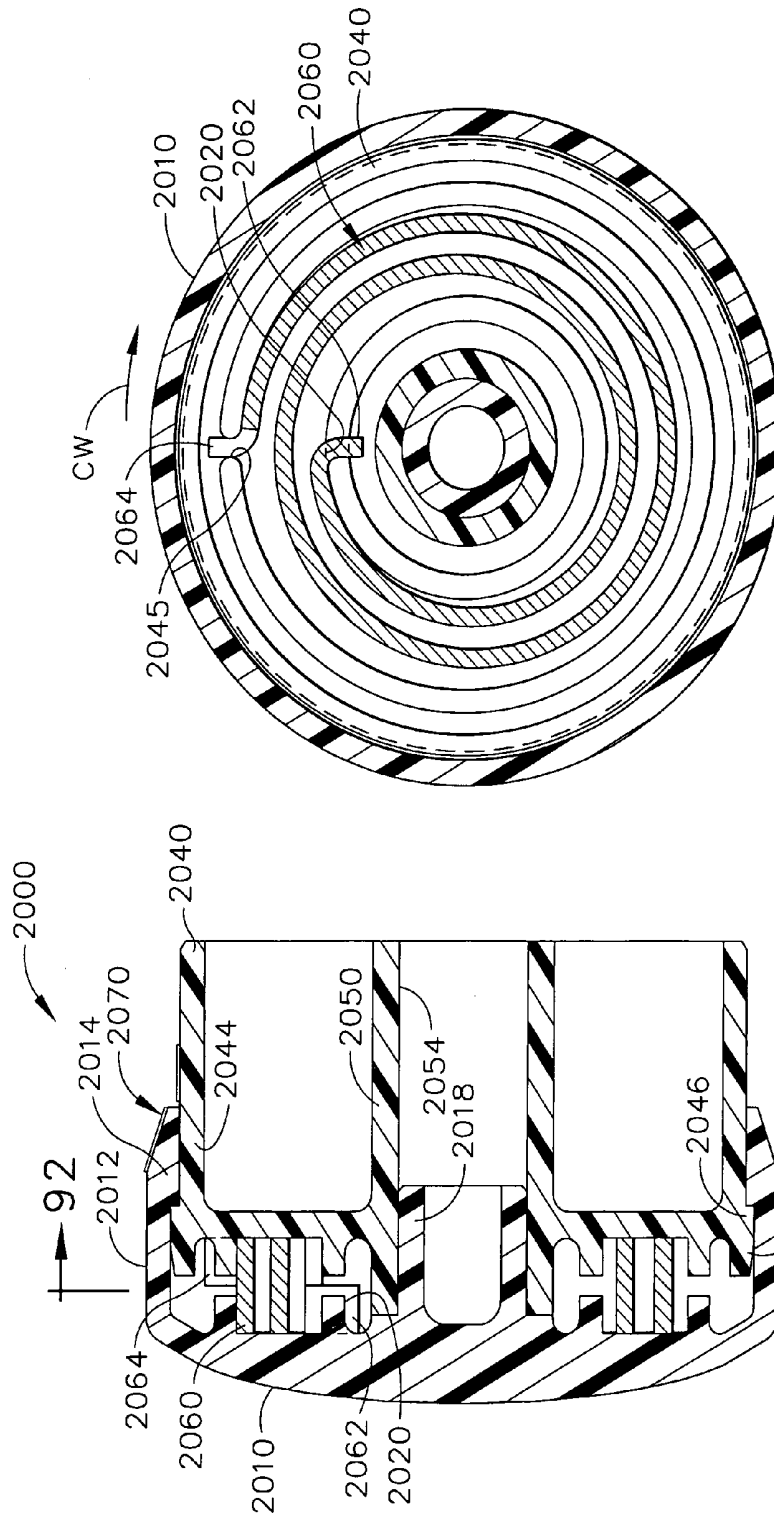


FIG. 92

FIG. 91

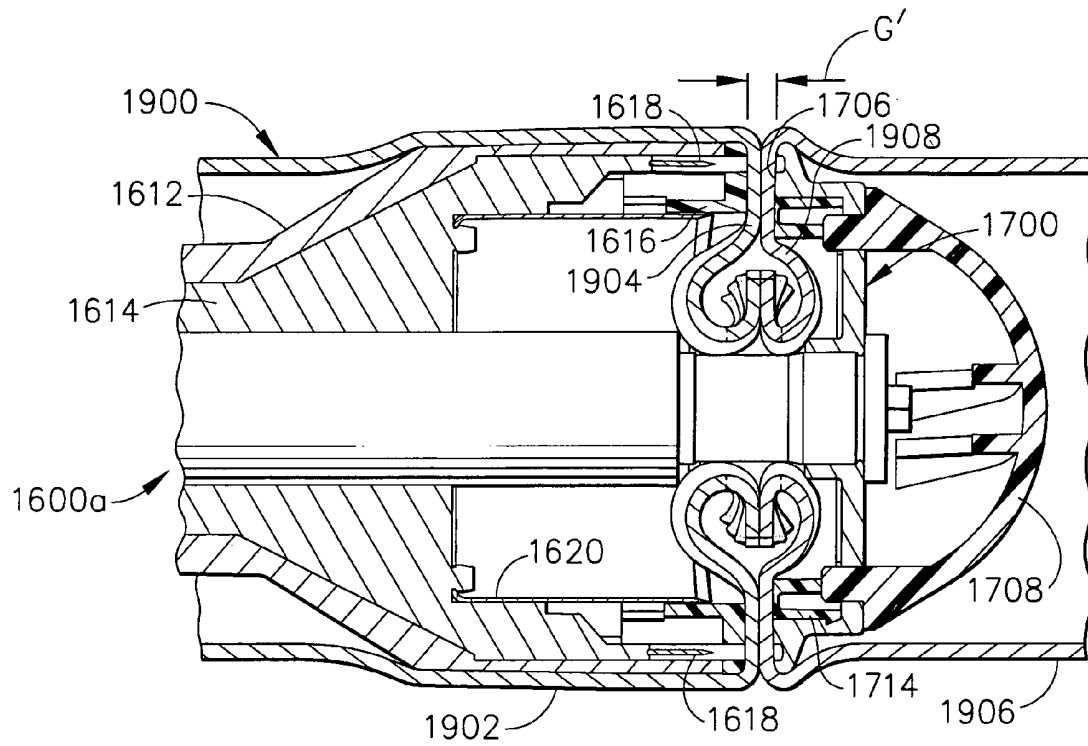


FIG. 93

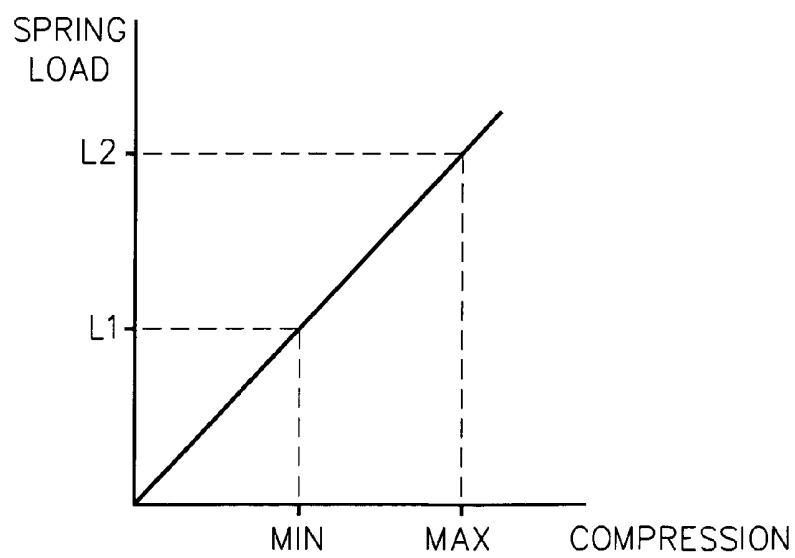


FIG. 94

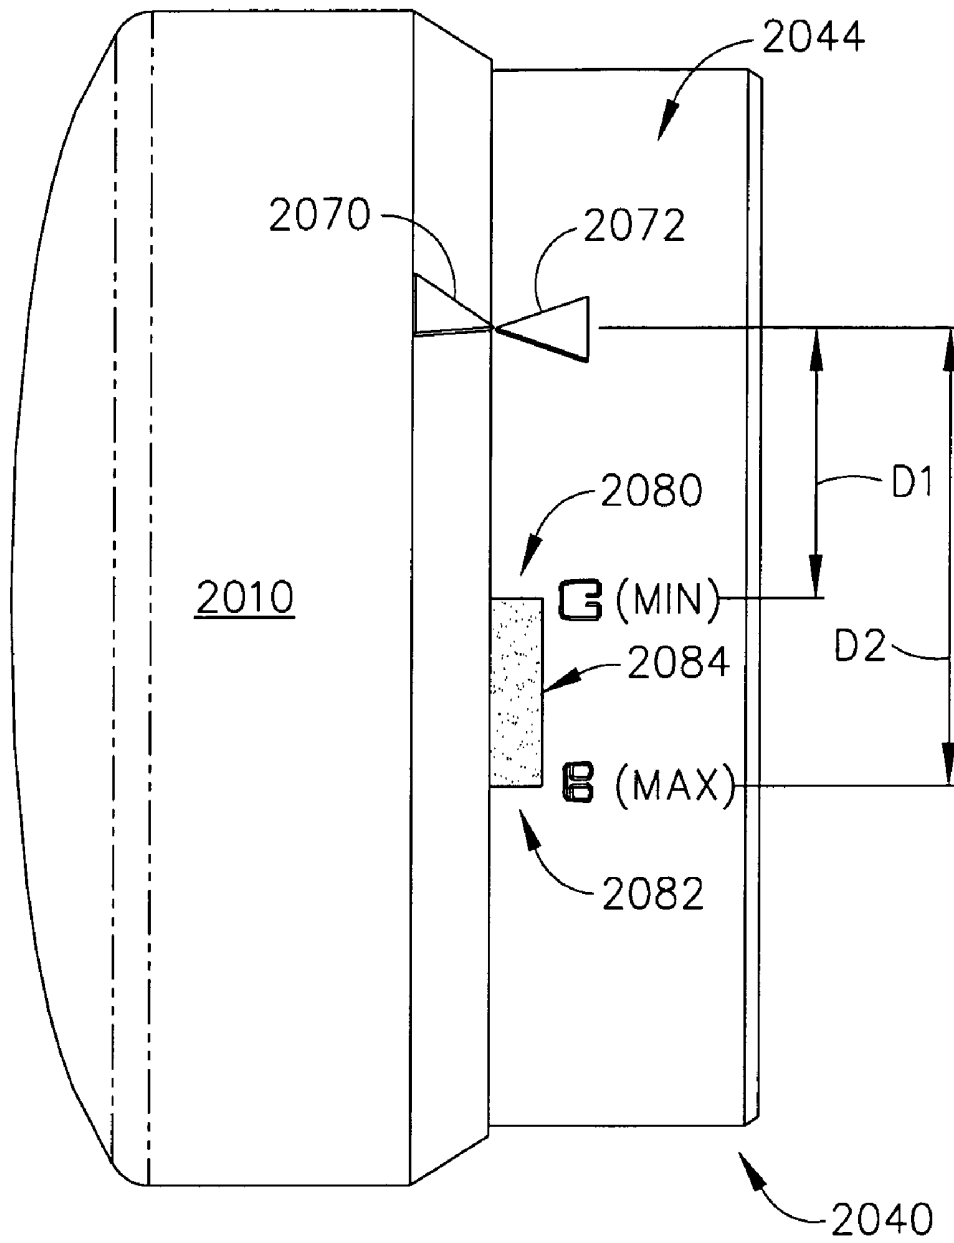


FIG. 95

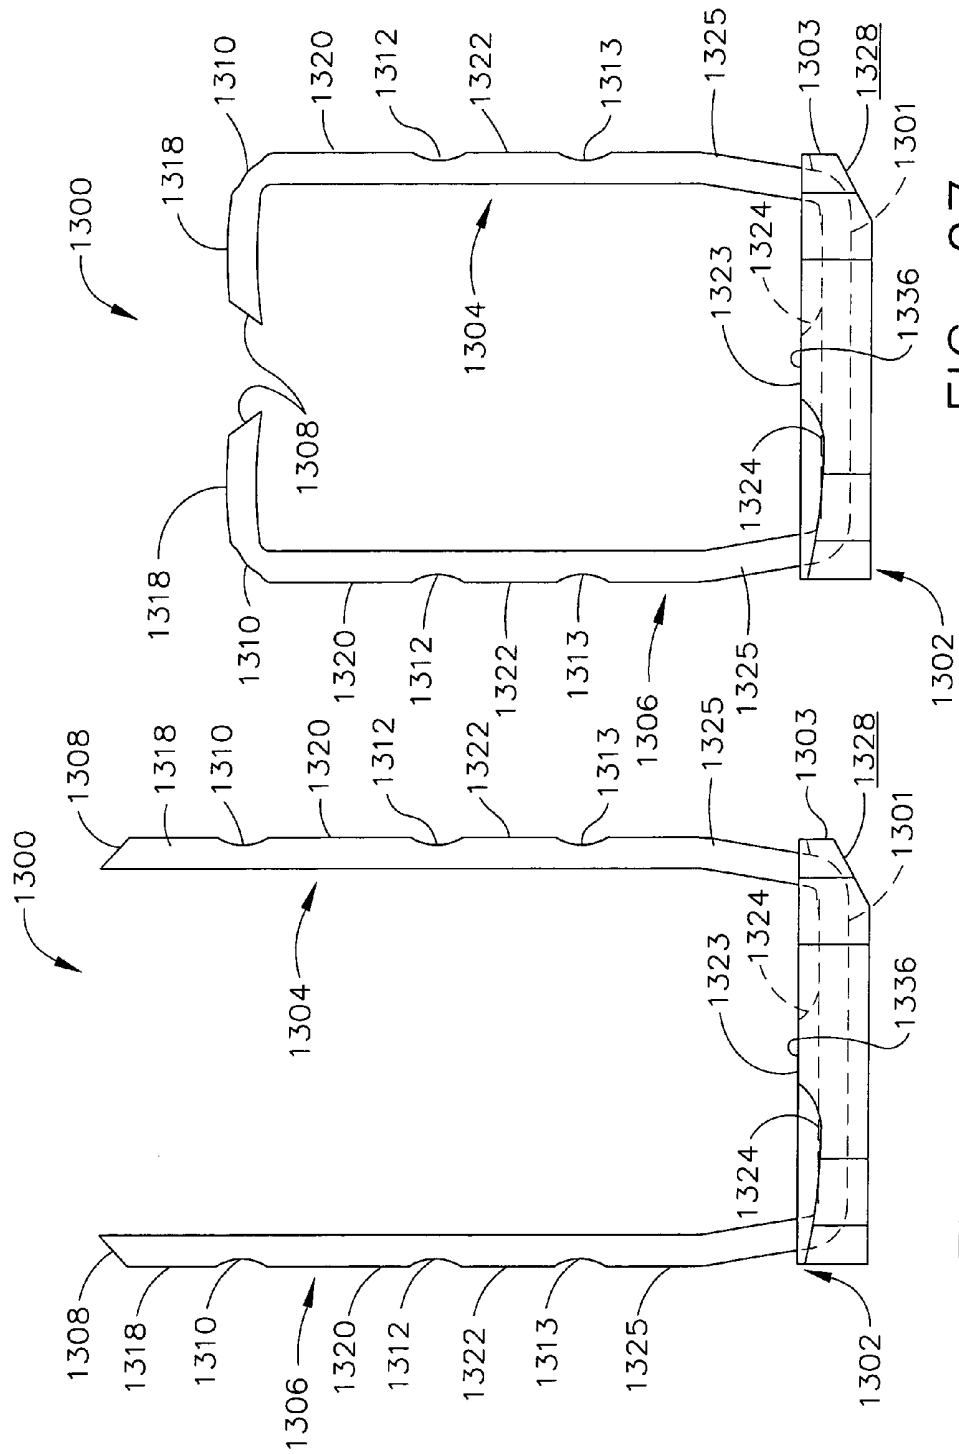


FIG. 97

FIG. 96

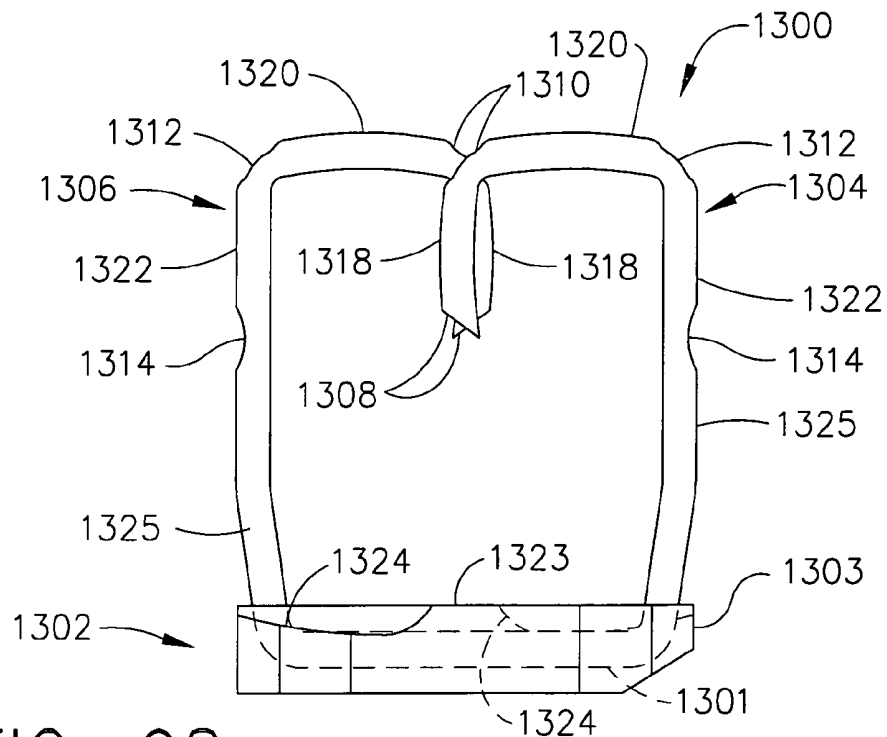


FIG. 98

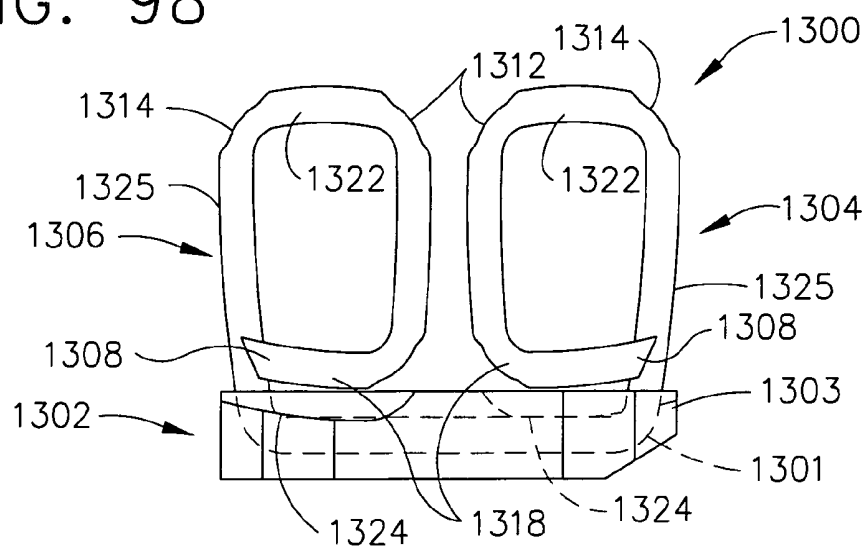


FIG. 99

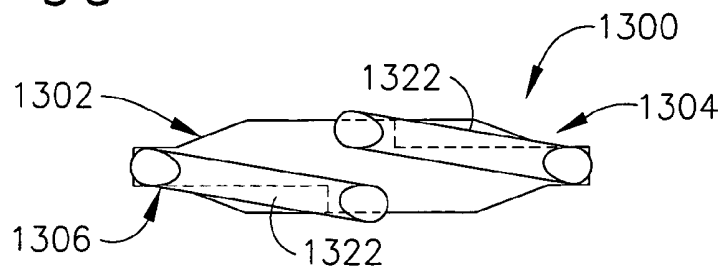


FIG. 100

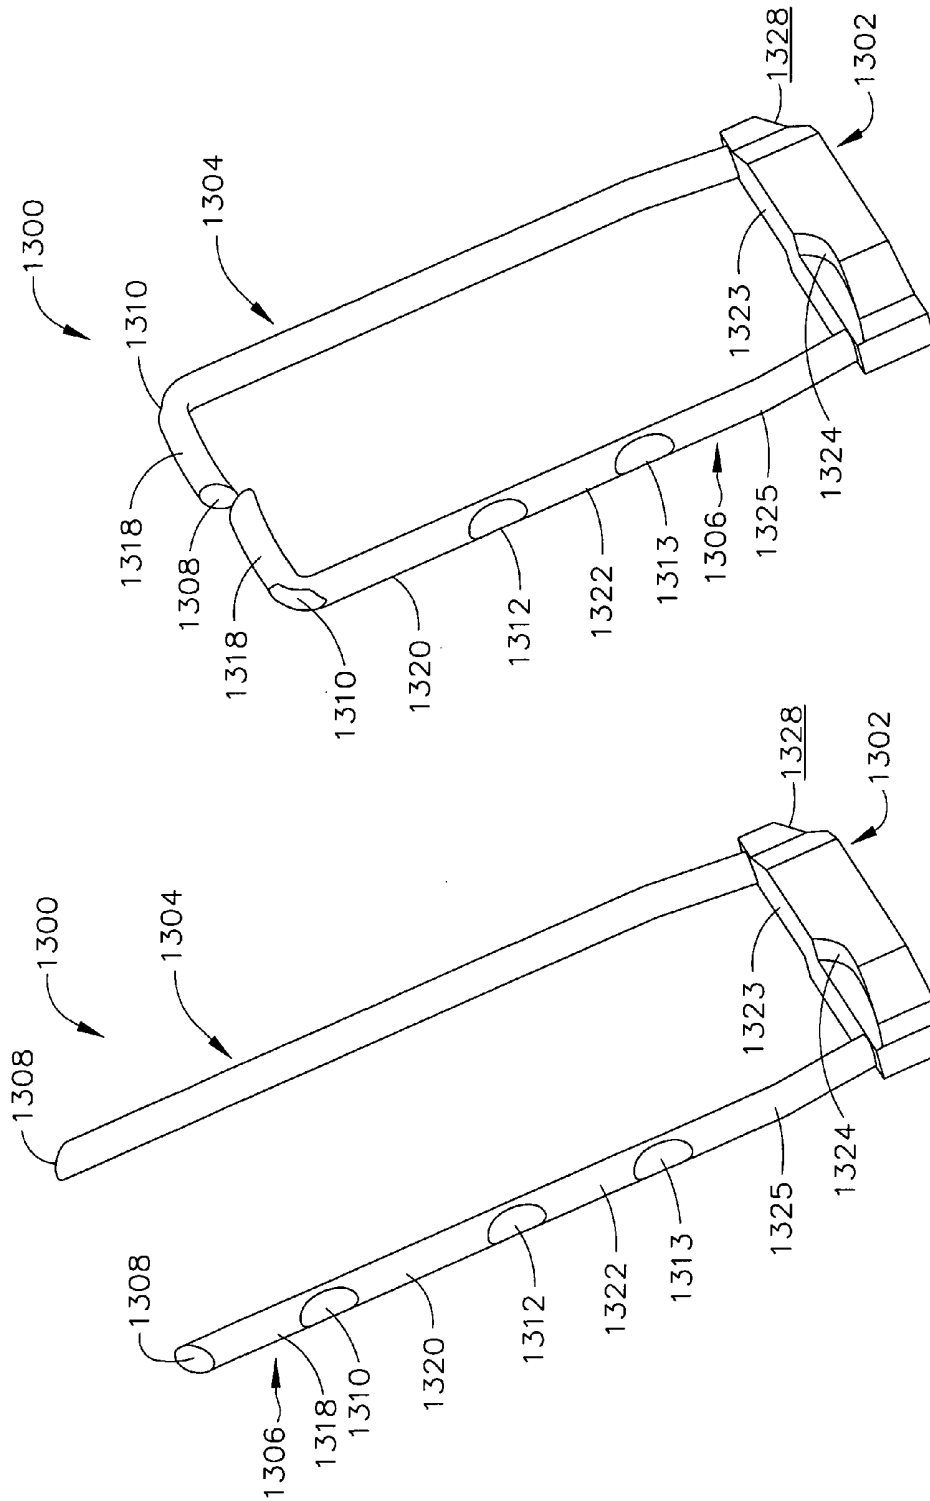


FIG. 102

FIG. 101

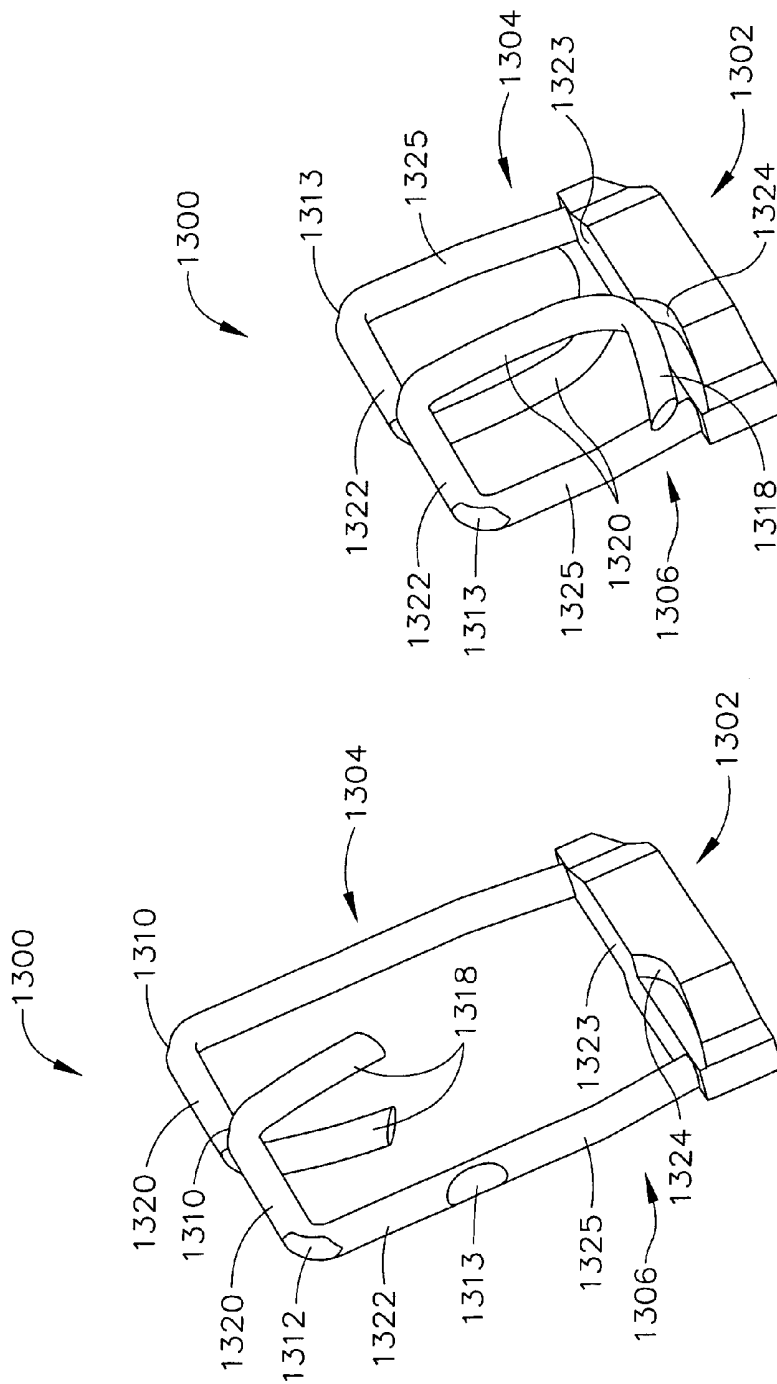


FIG. 103

FIG. 104

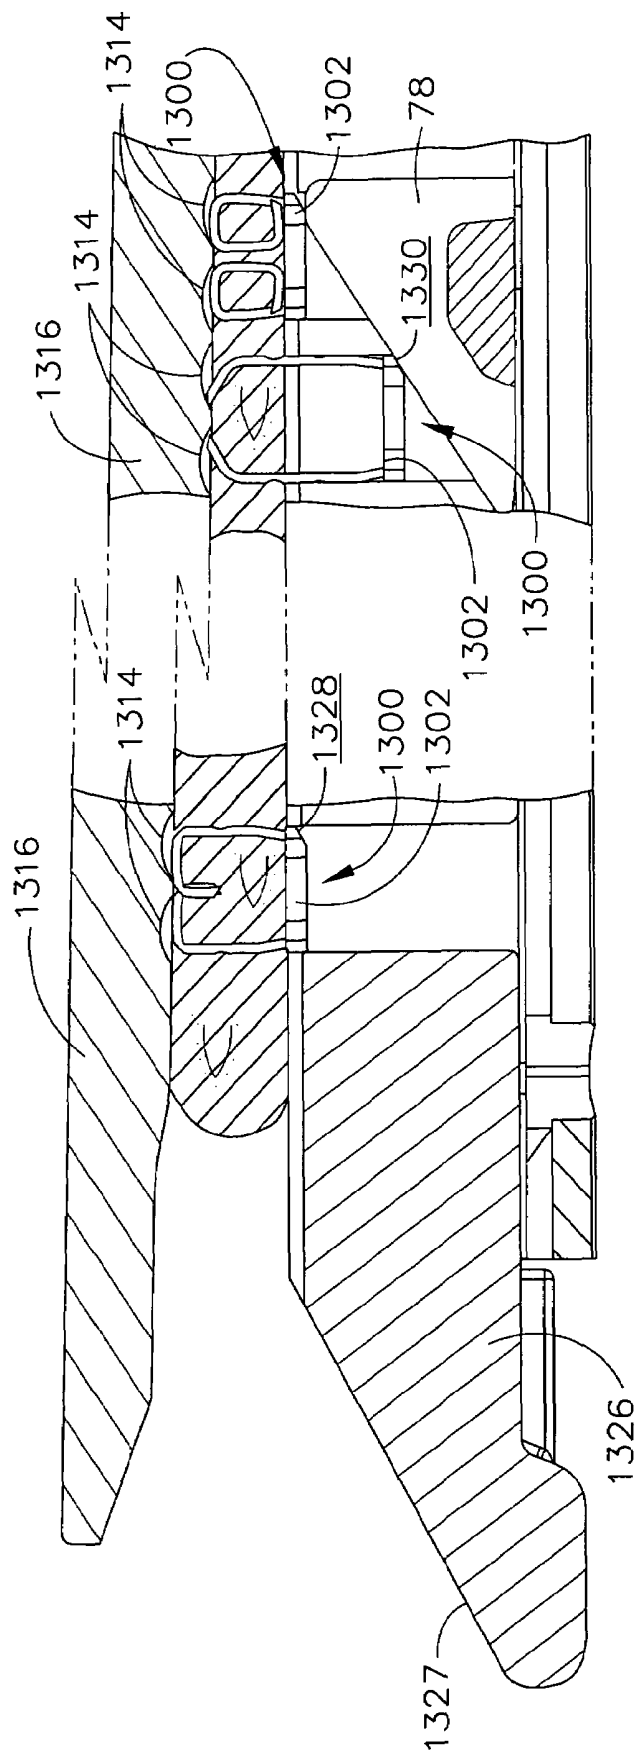


FIG. 105

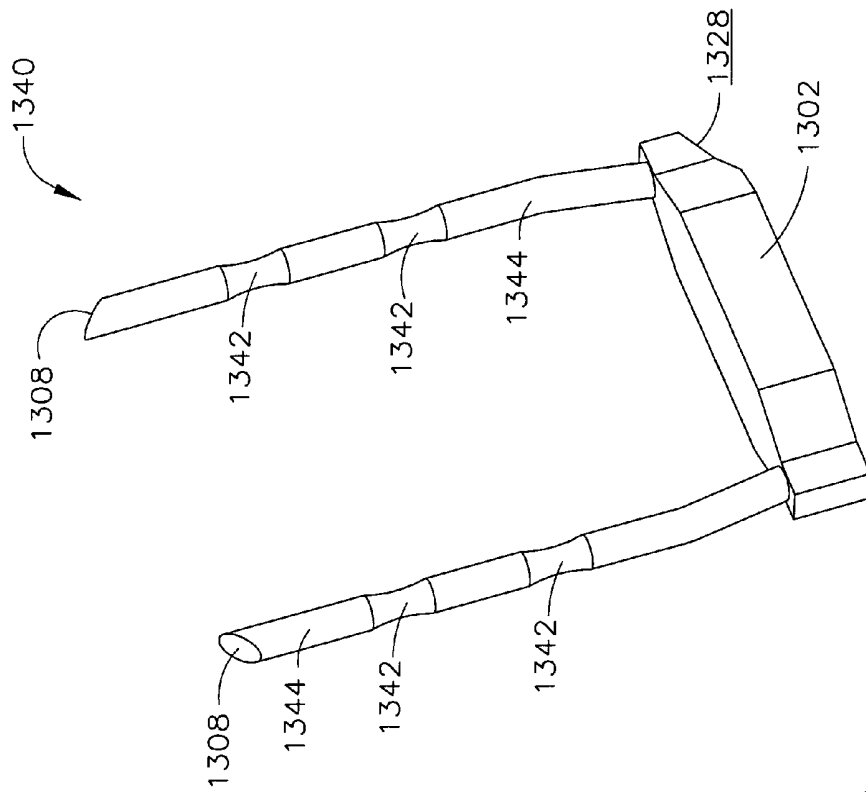


FIG. 107

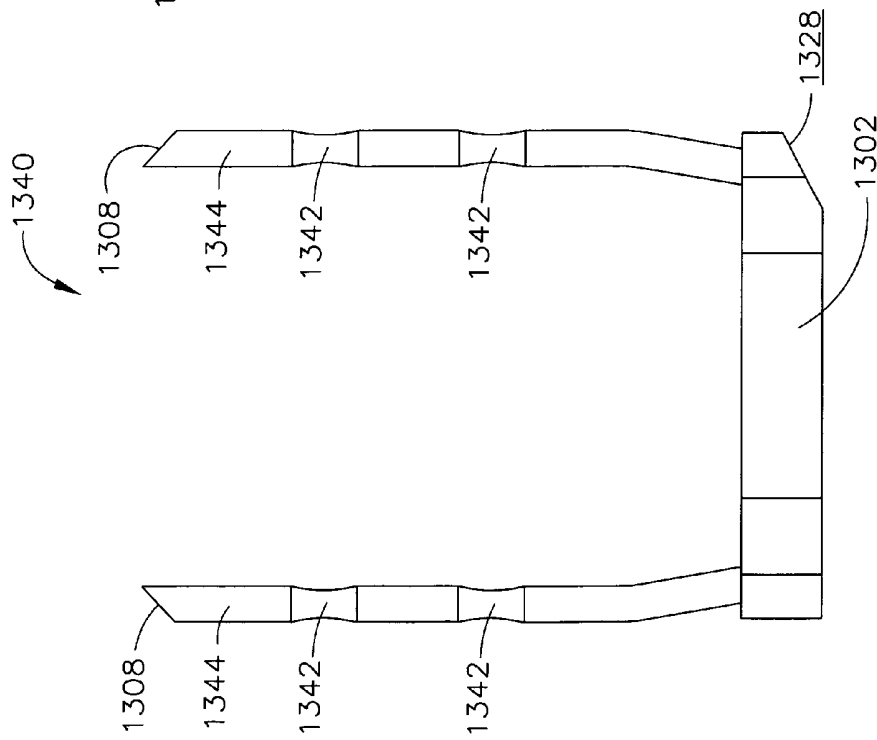


FIG. 106

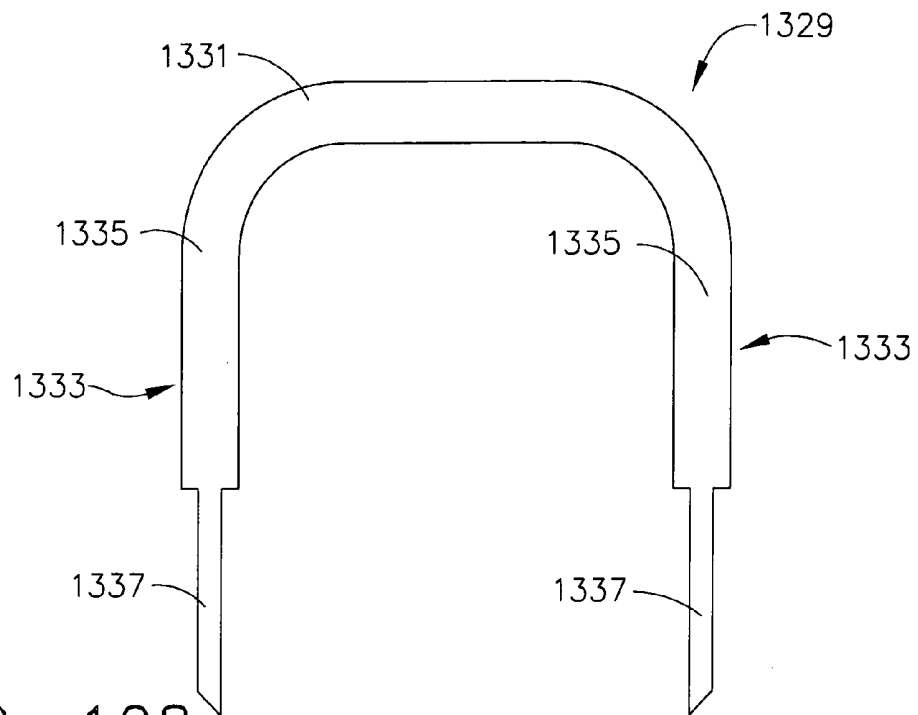


FIG. 108

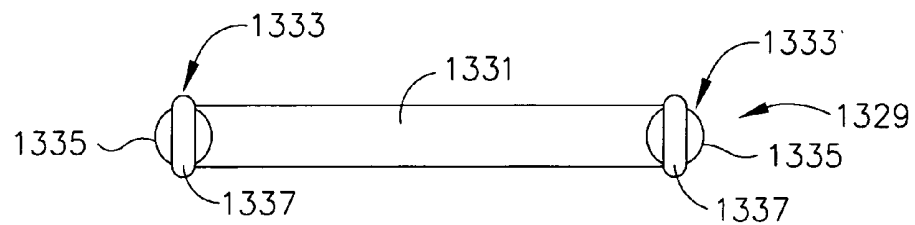


FIG. 109

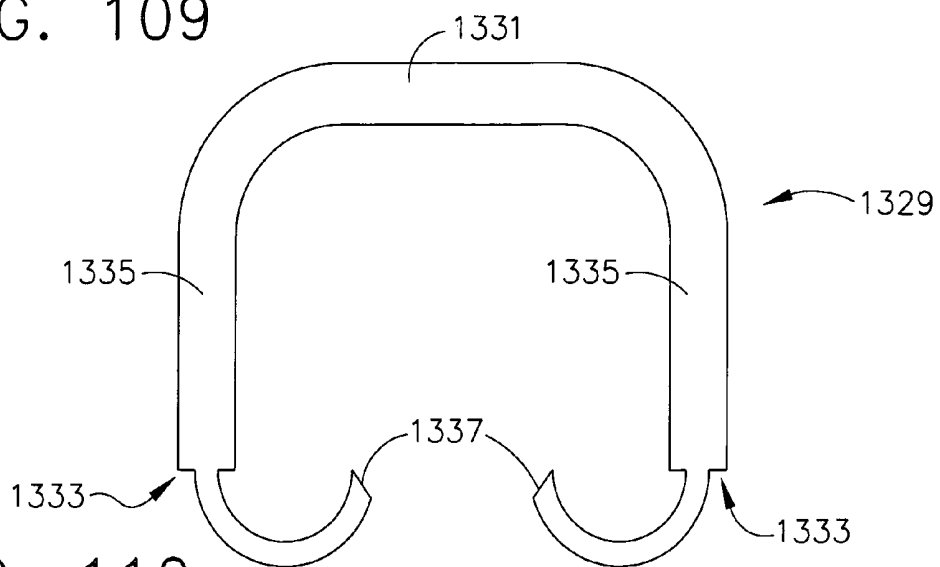


FIG. 110

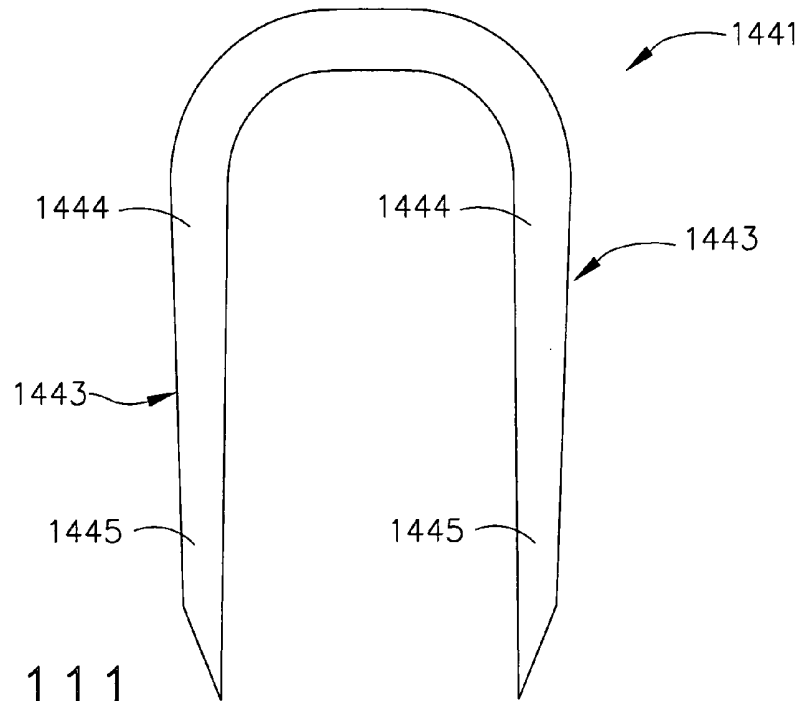


FIG. 111

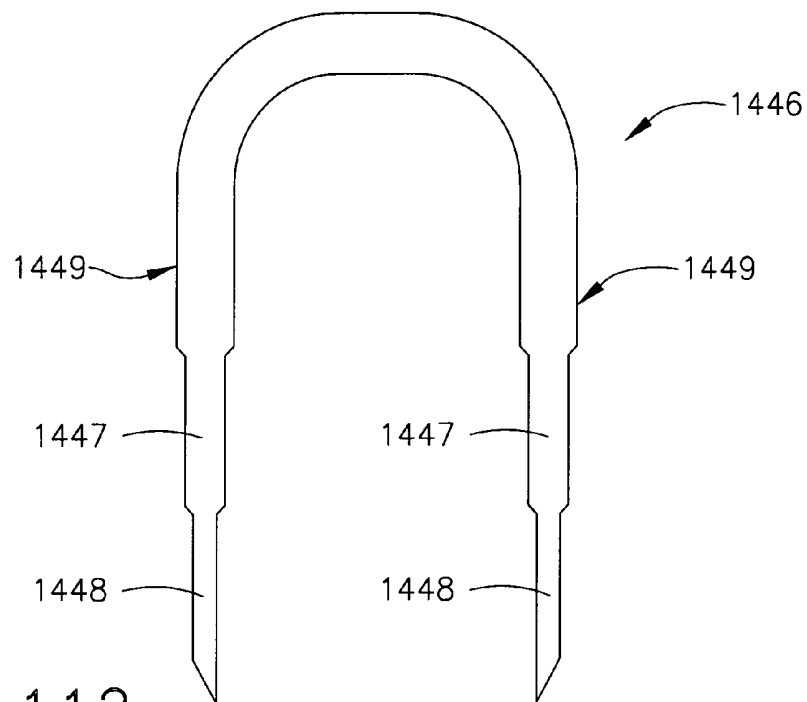


FIG. 112

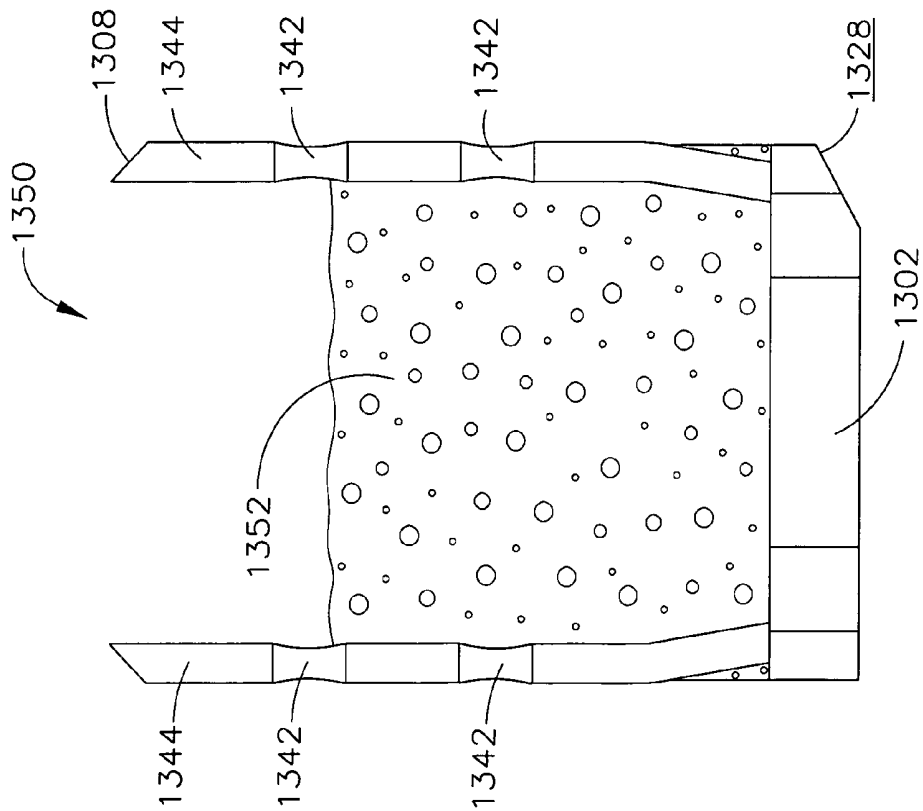


FIG. 113

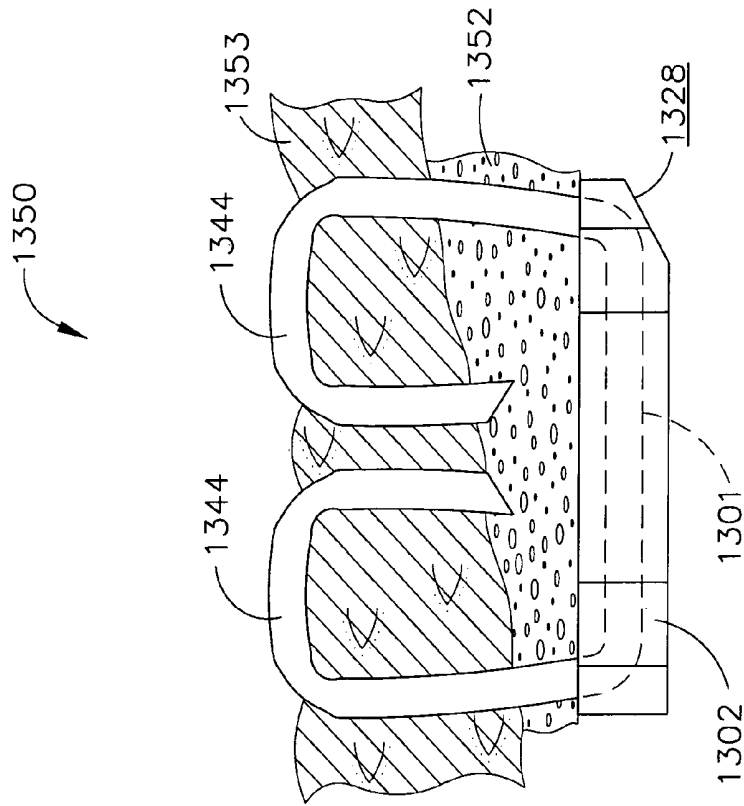


FIG. 114

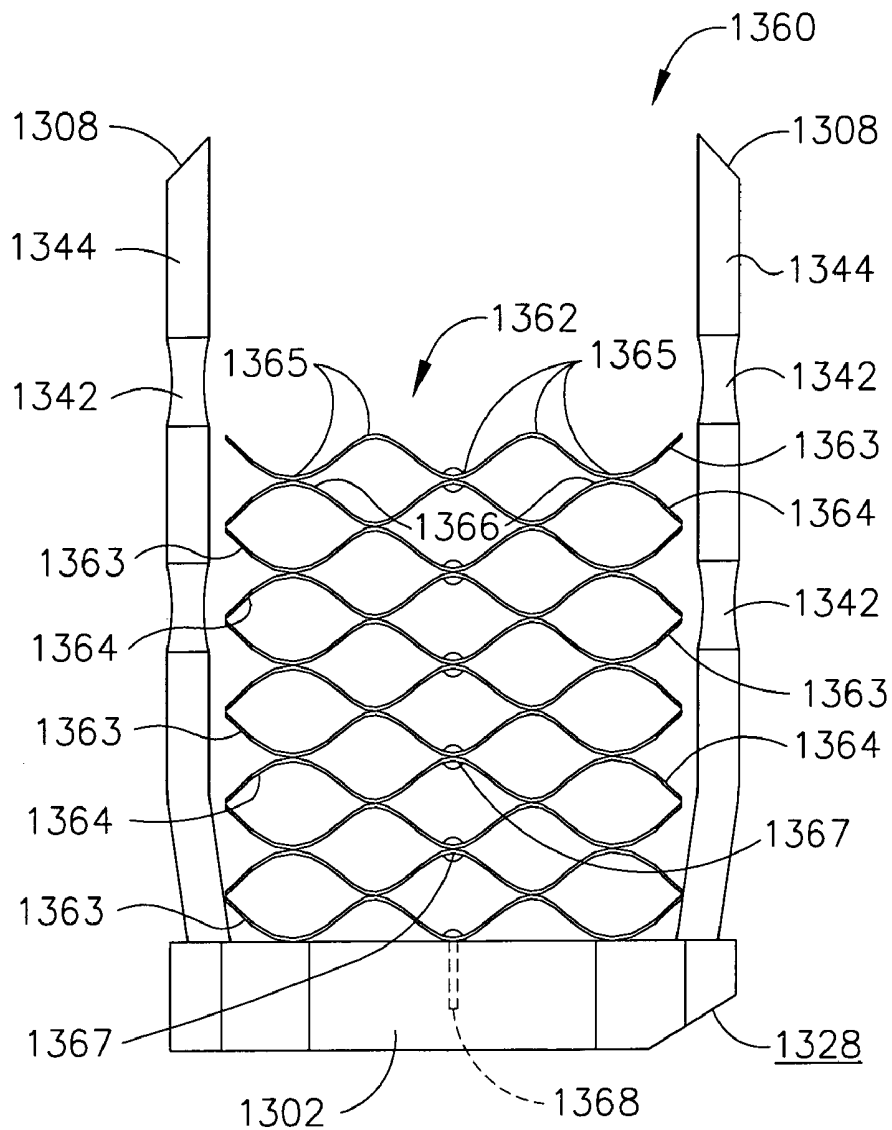


FIG. 115

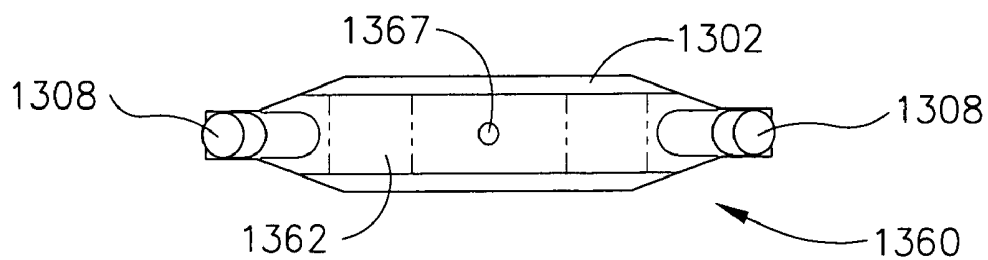


FIG. 116

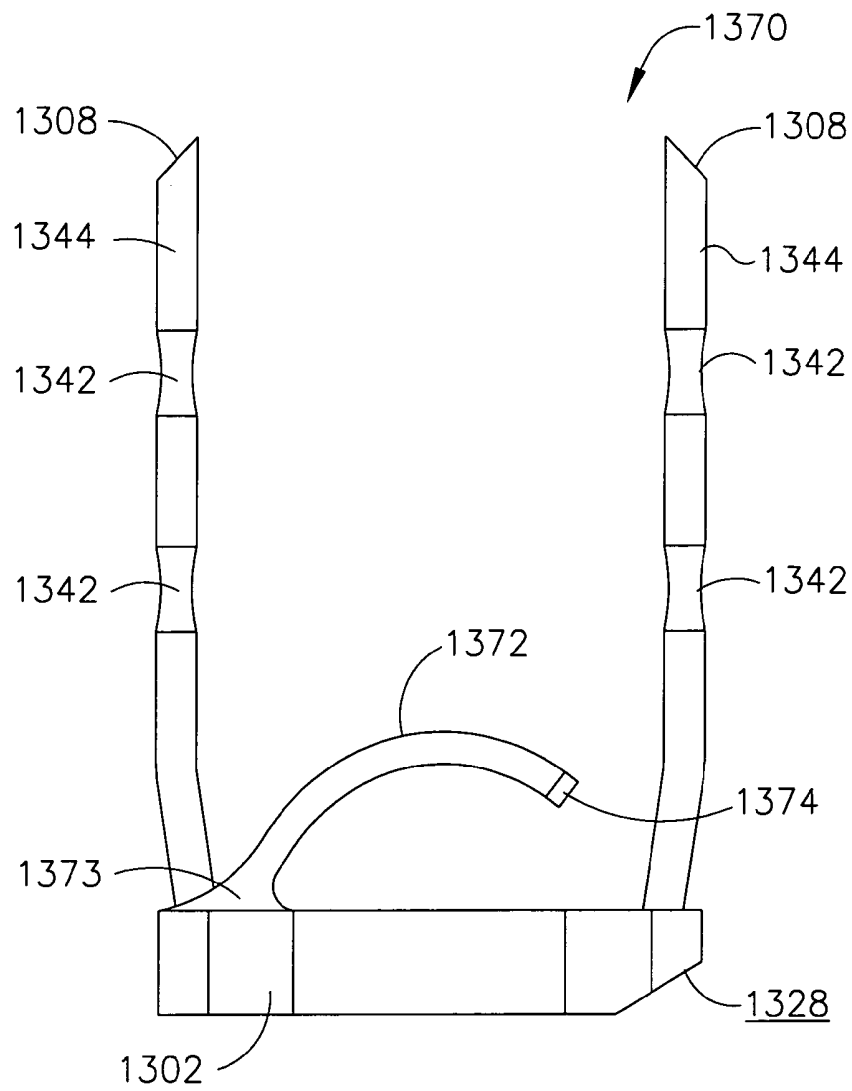


FIG. 117

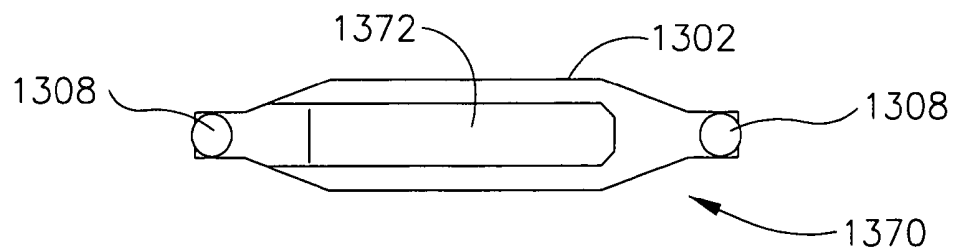


FIG. 118

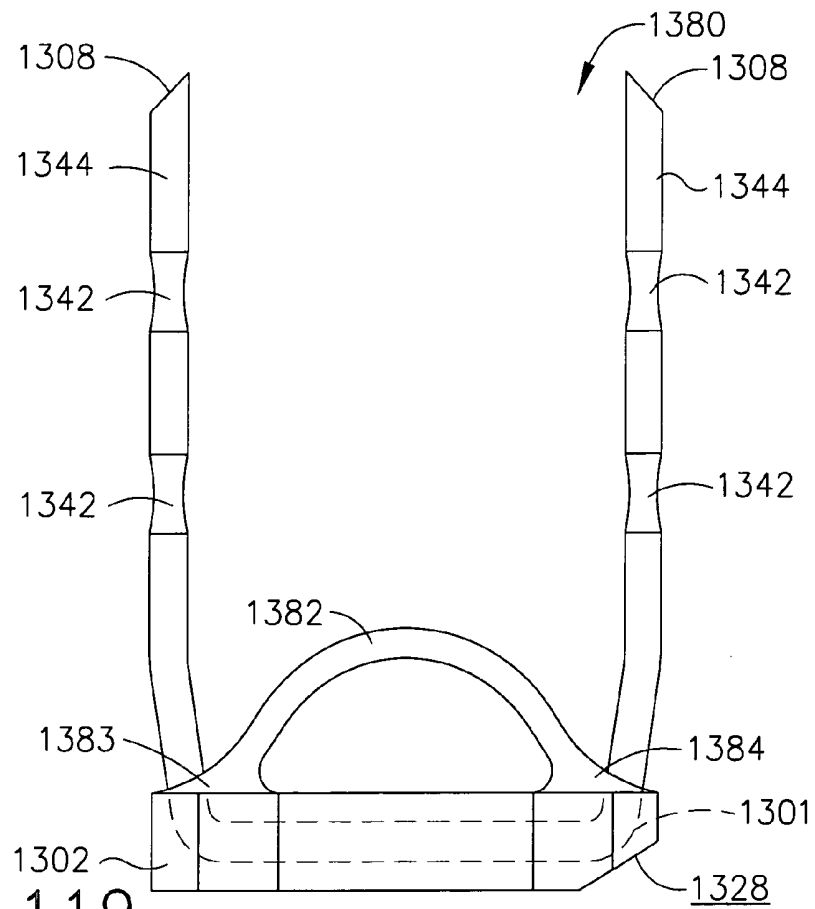


FIG. 119

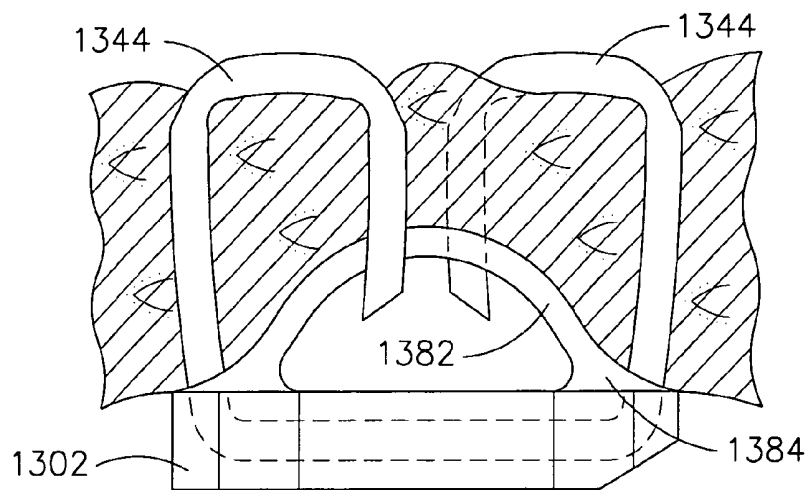


FIG. 120

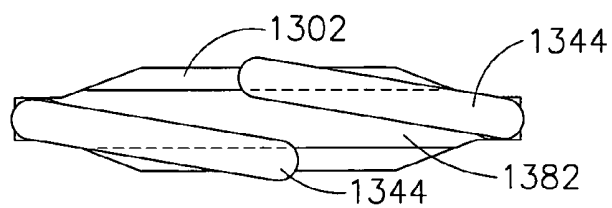
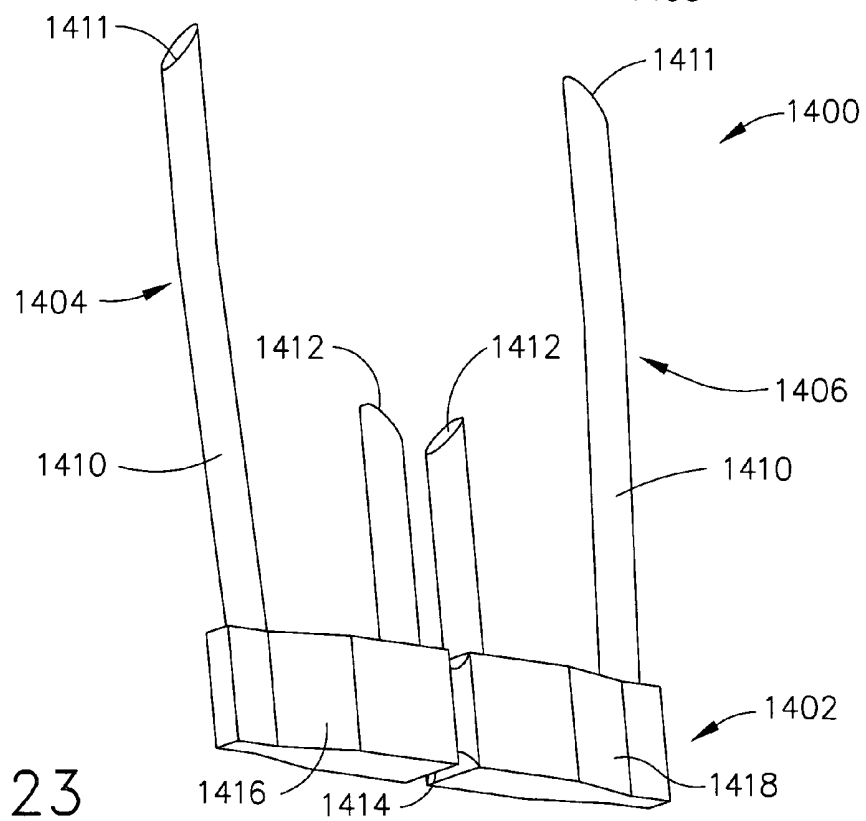
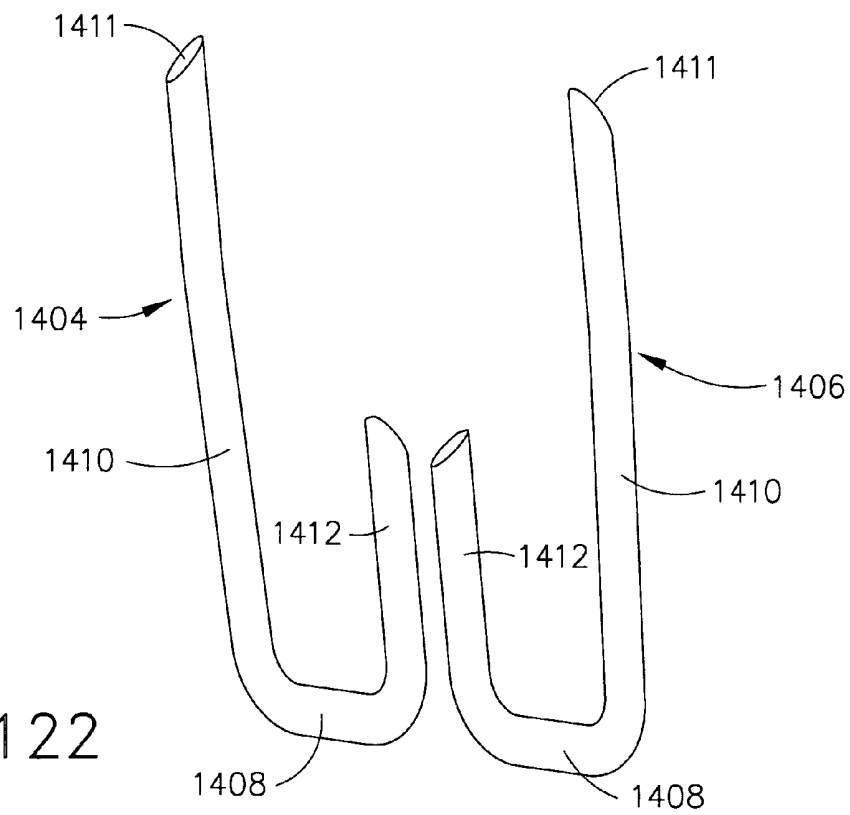


FIG. 121



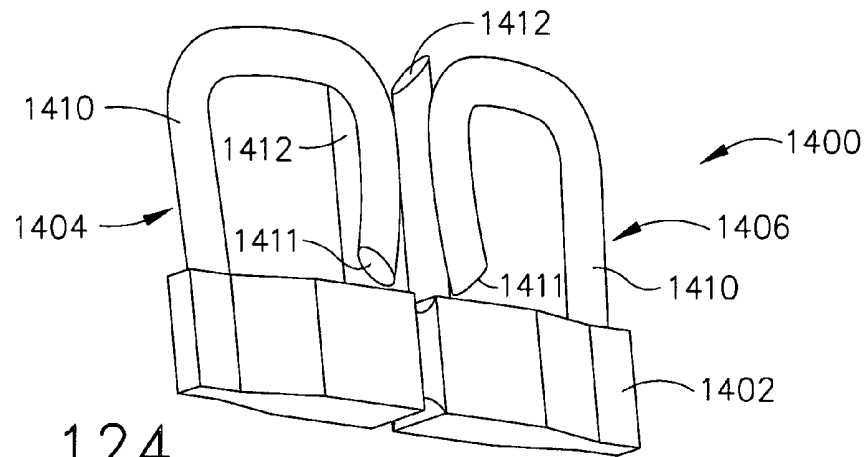


FIG. 124

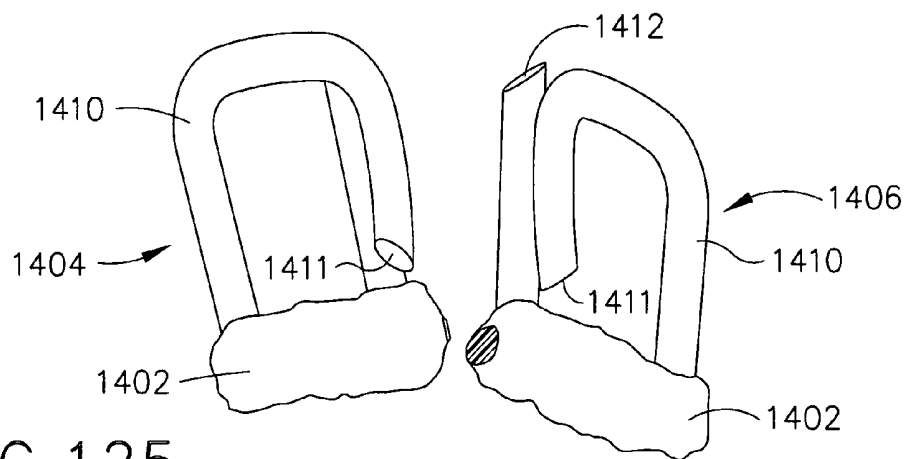


FIG. 125

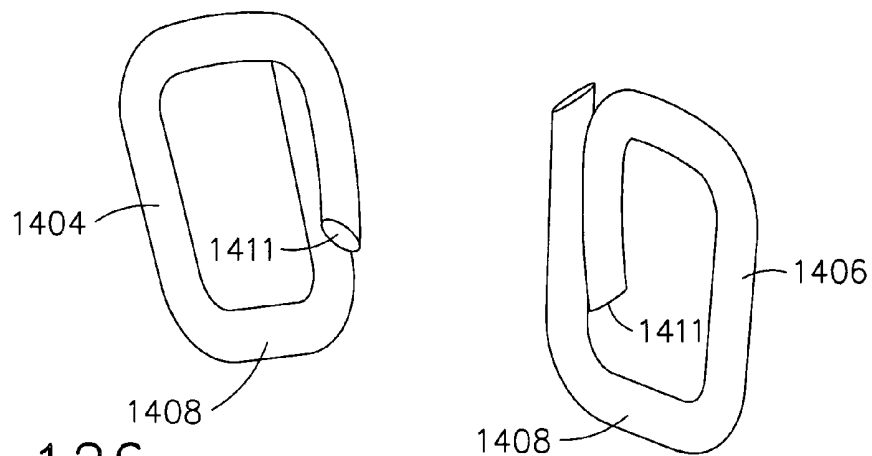


FIG. 126

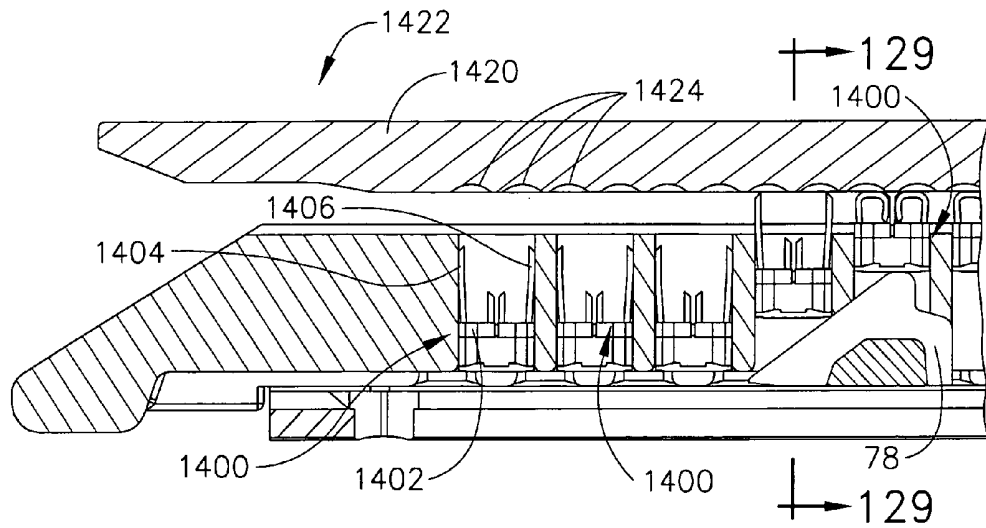


FIG. 127

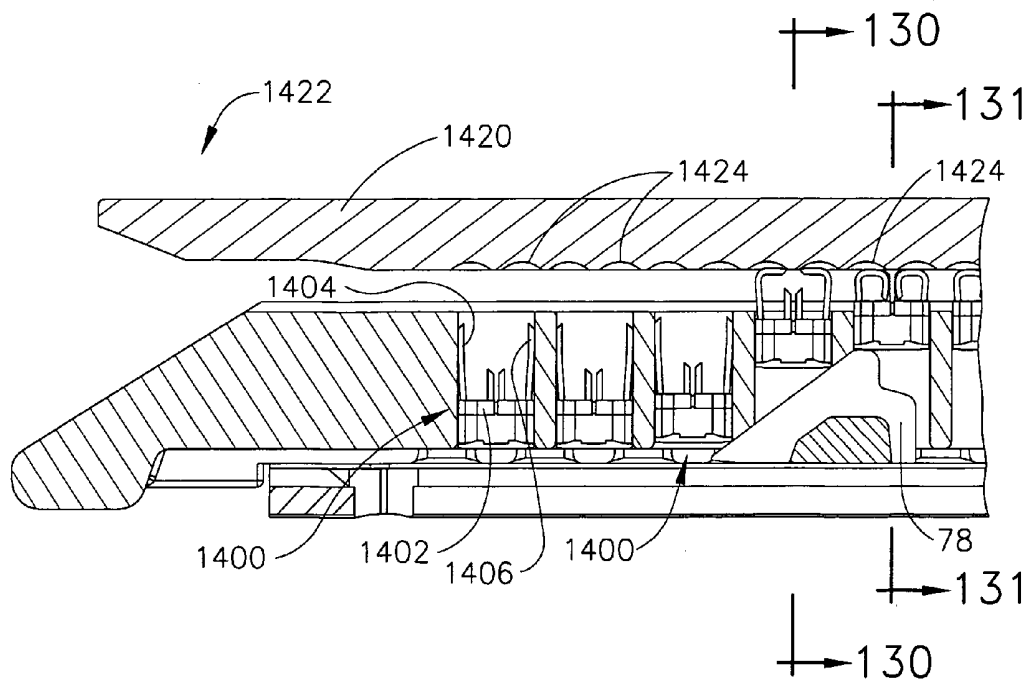


FIG. 128

FIG. 129A

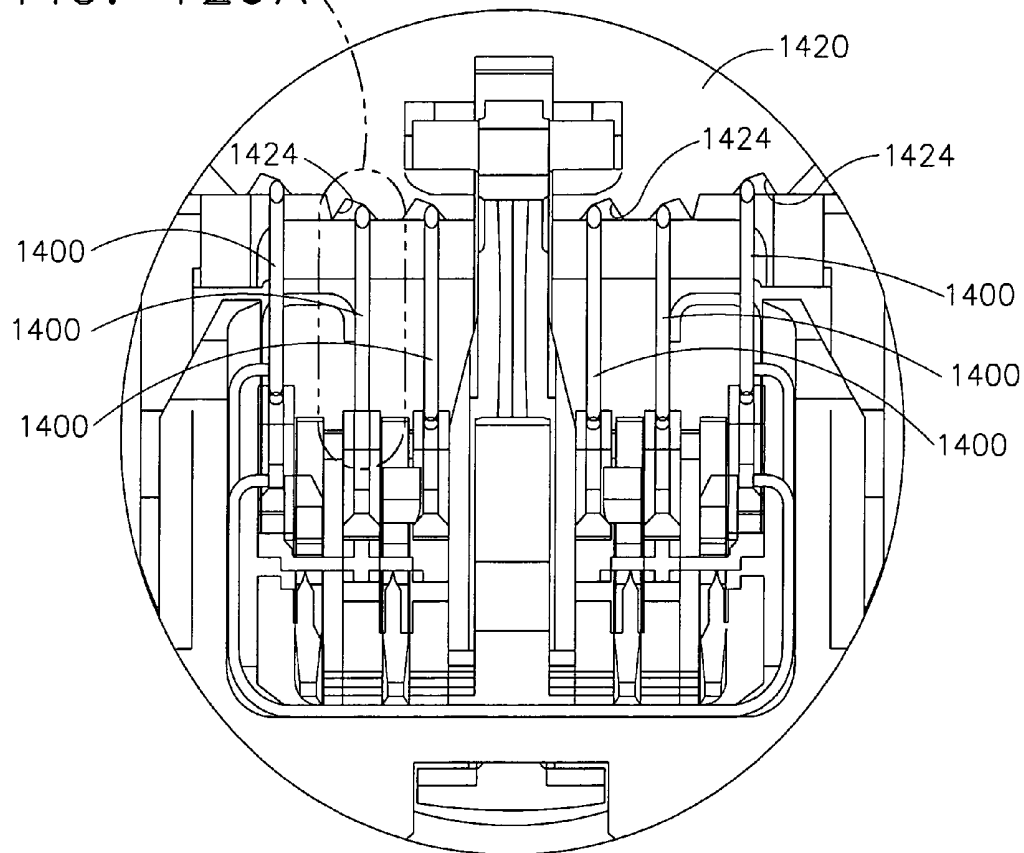


FIG. 129

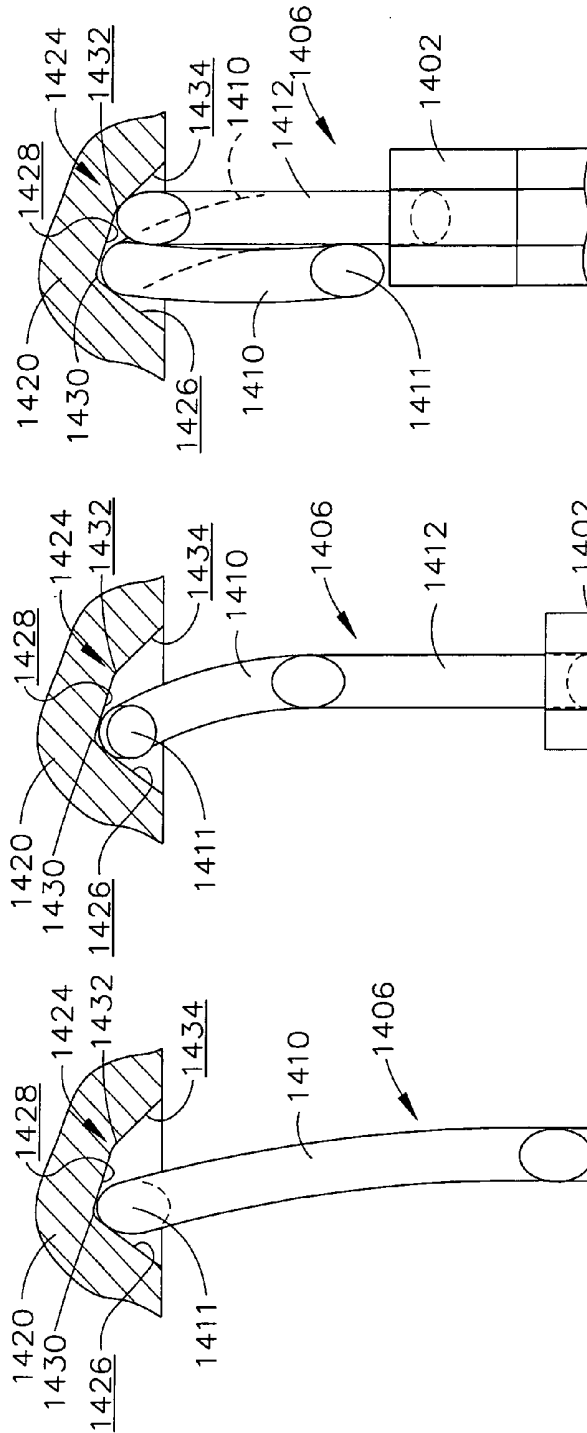


FIG. 129A

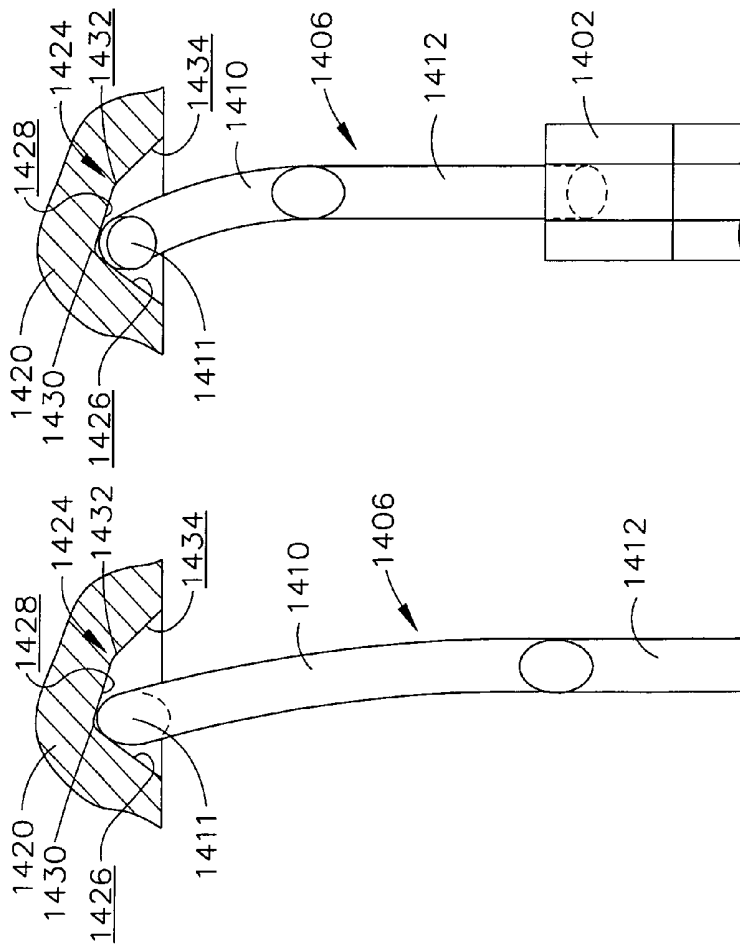


FIG. 130

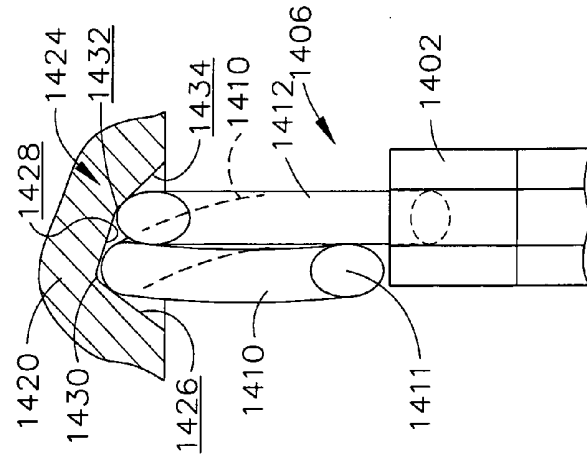


FIG. 131

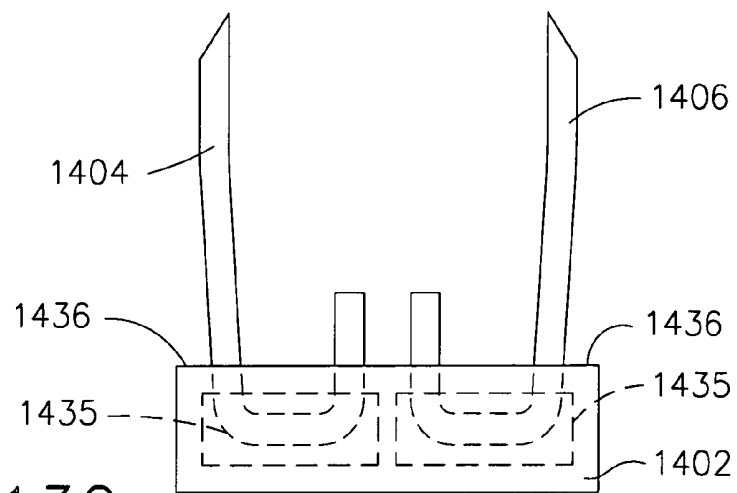


FIG. 132

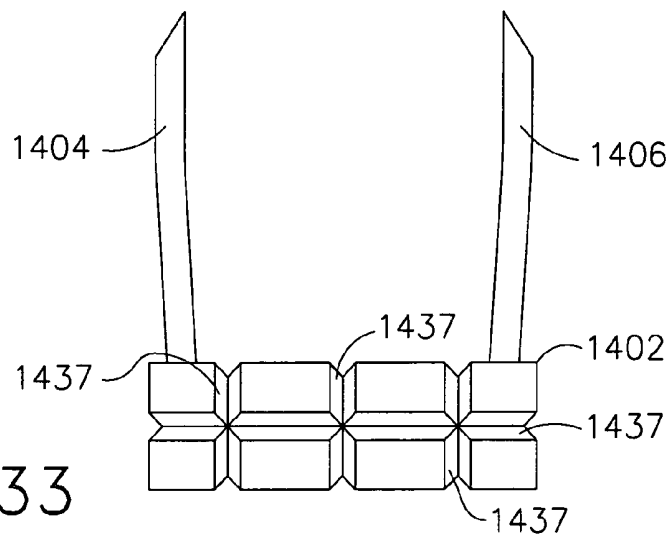


FIG. 133

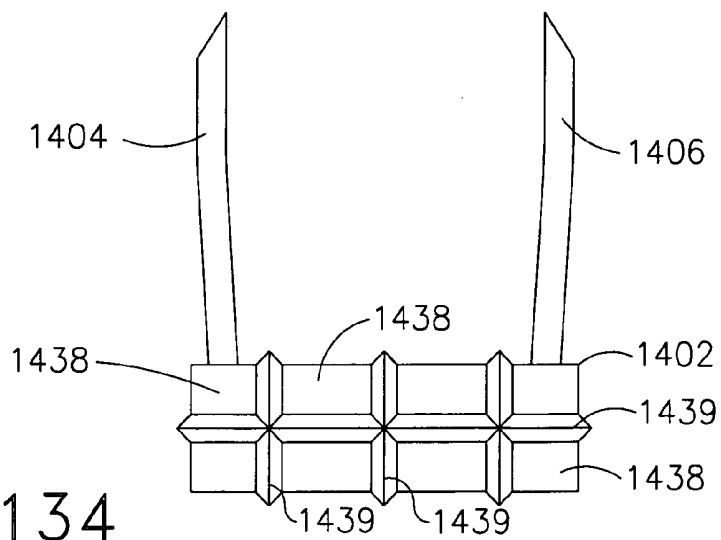


FIG. 134

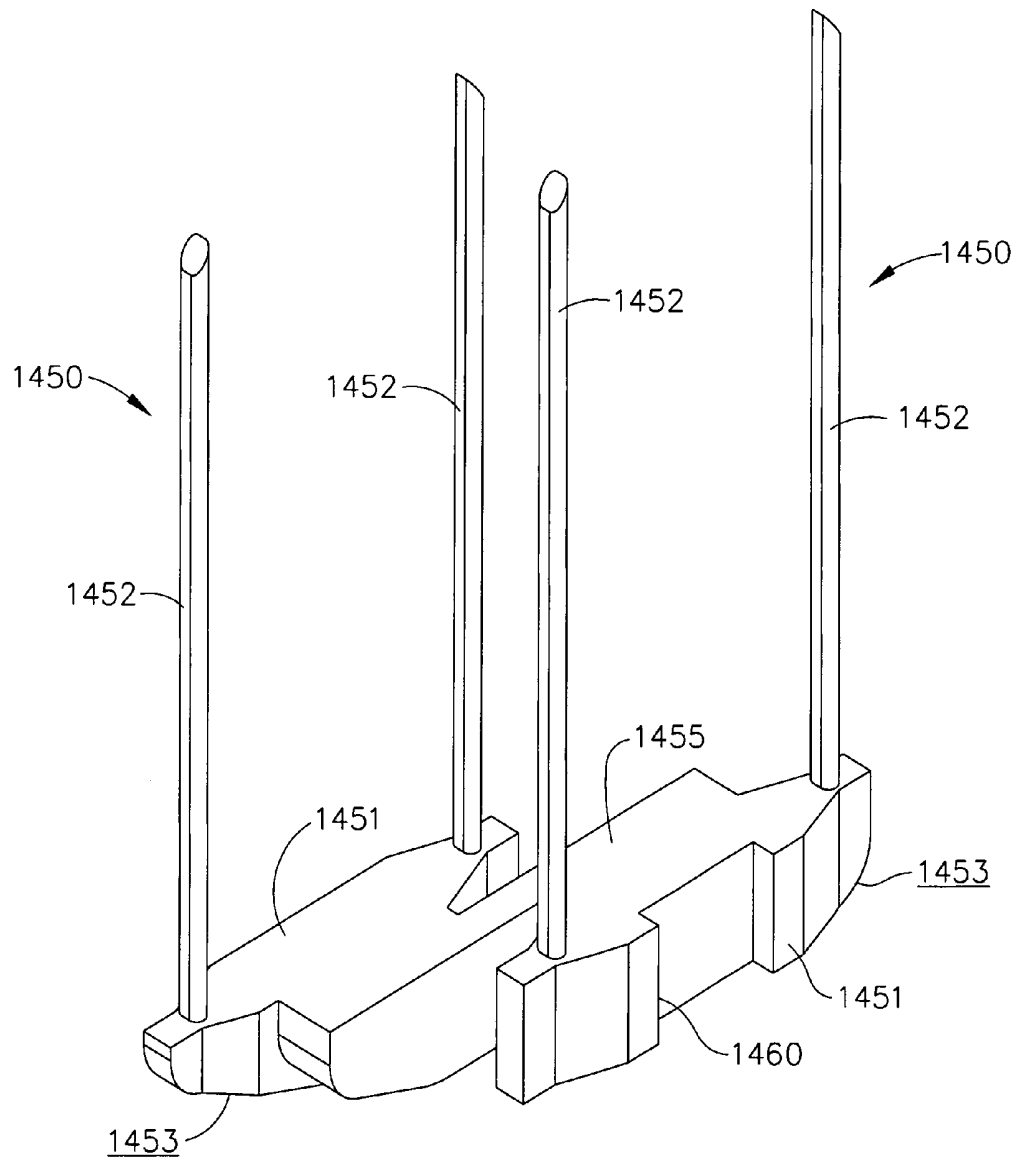


FIG. 135

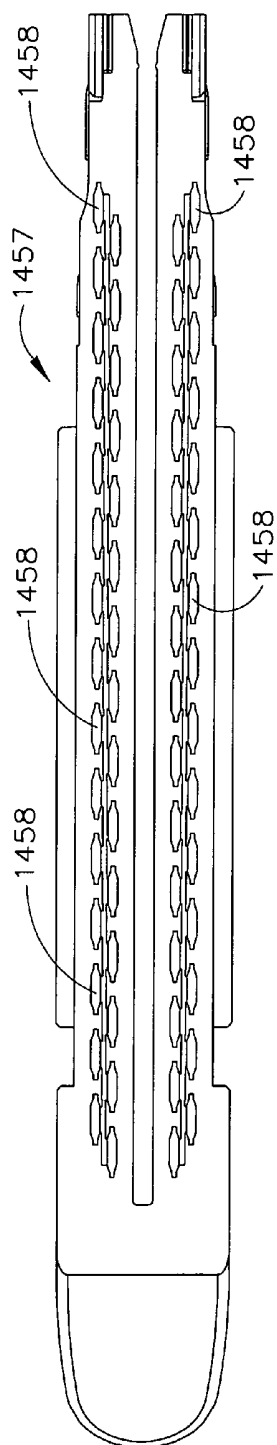


FIG. 136

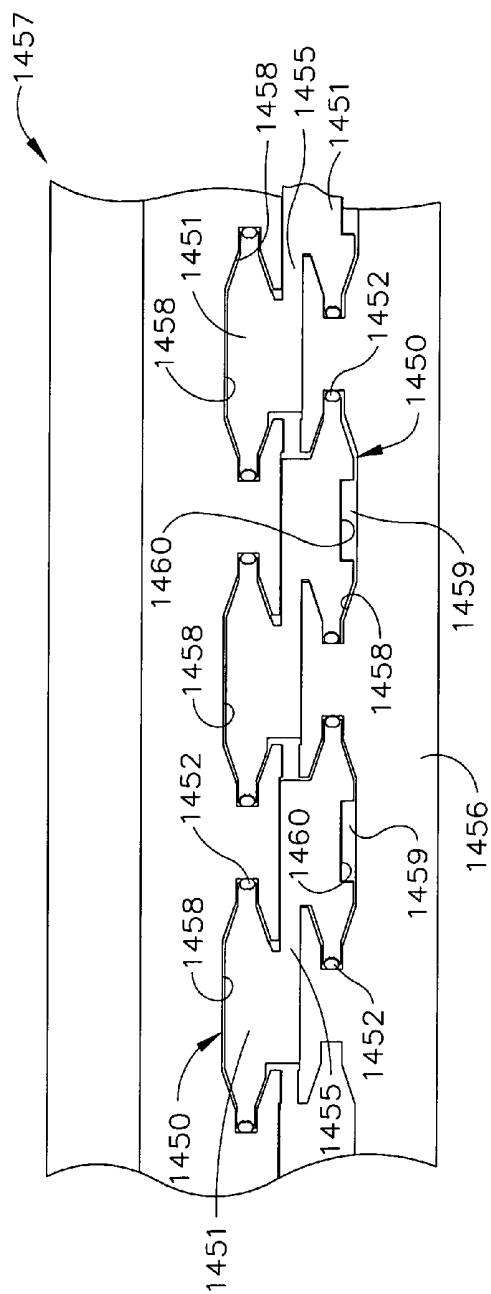


FIG. 137

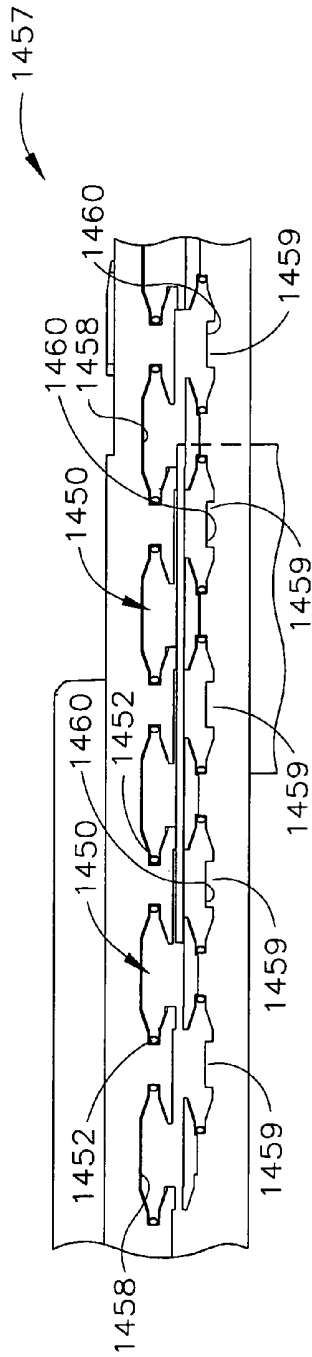


FIG. 138

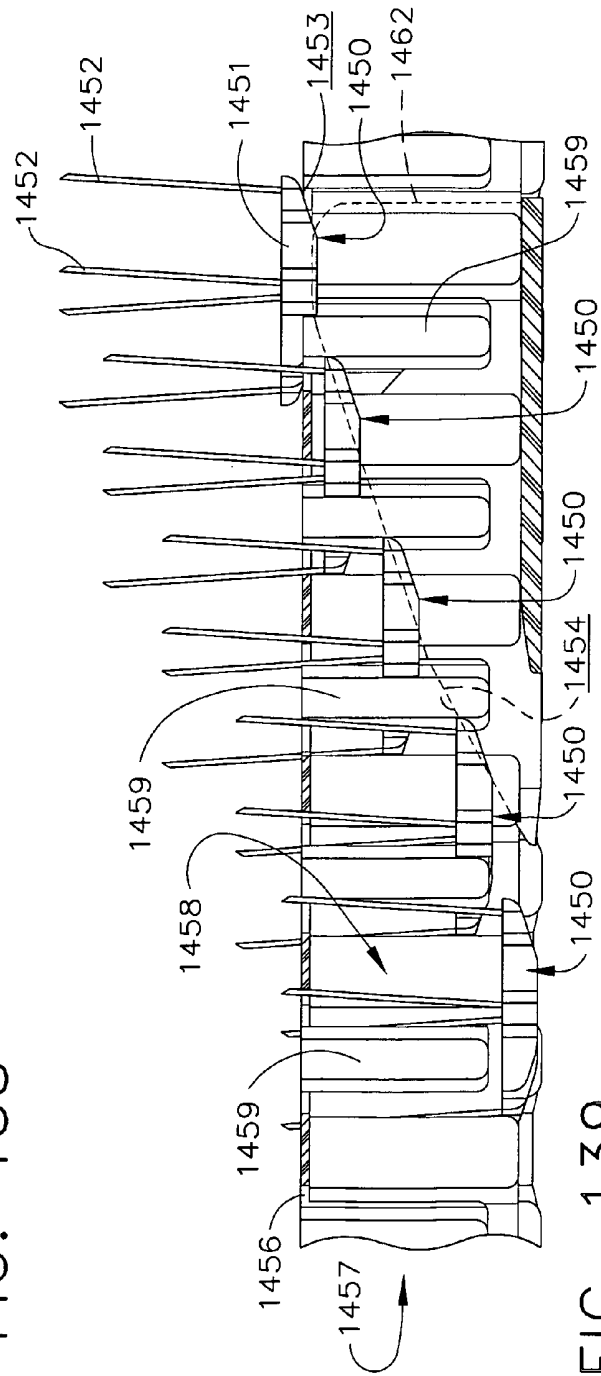


FIG. 139

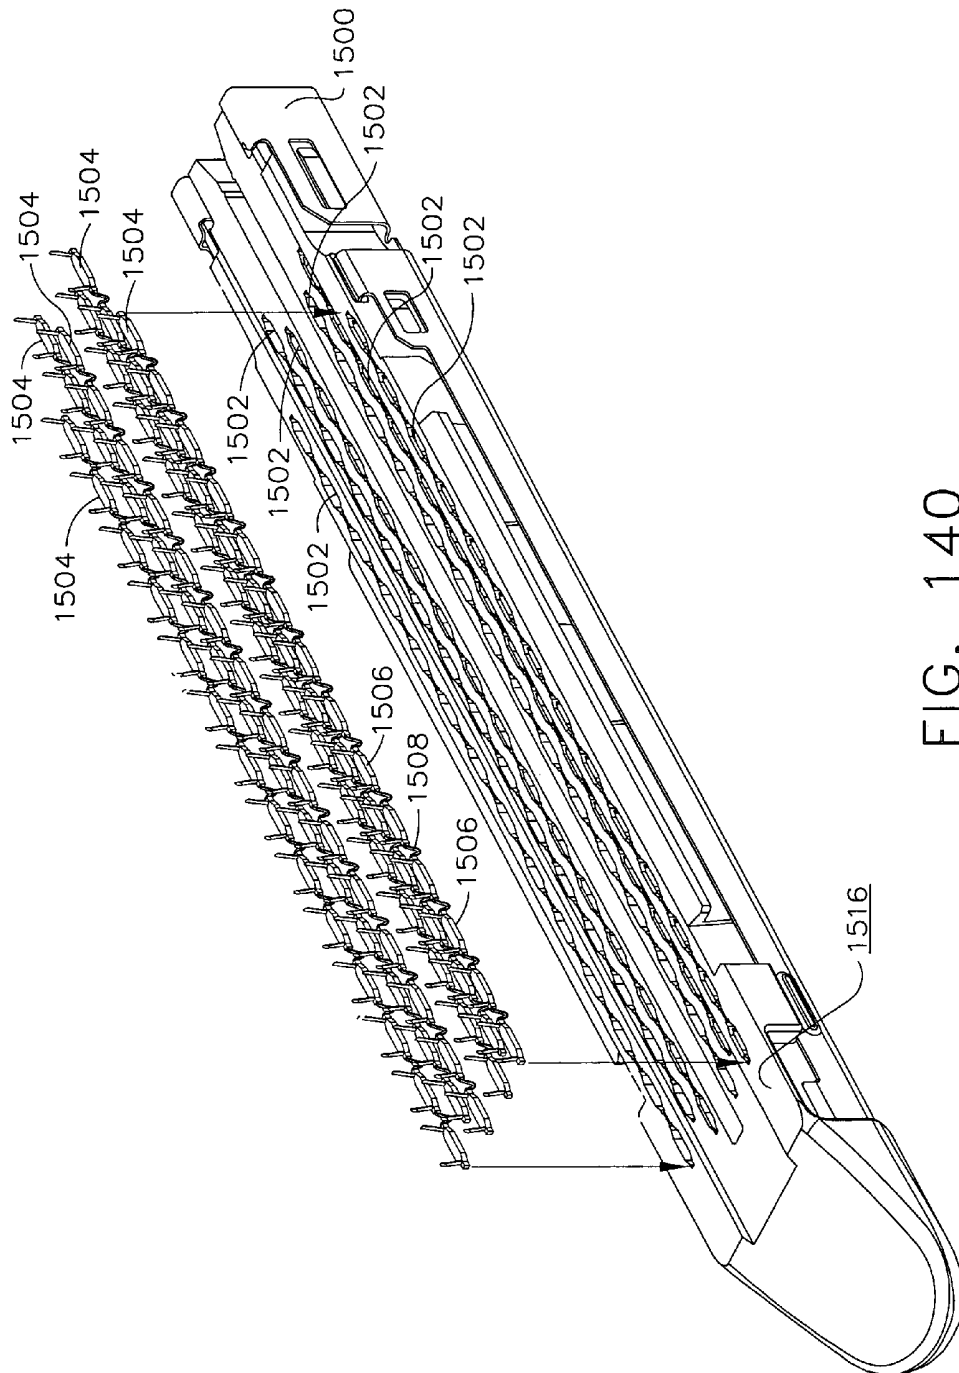


FIG. 140

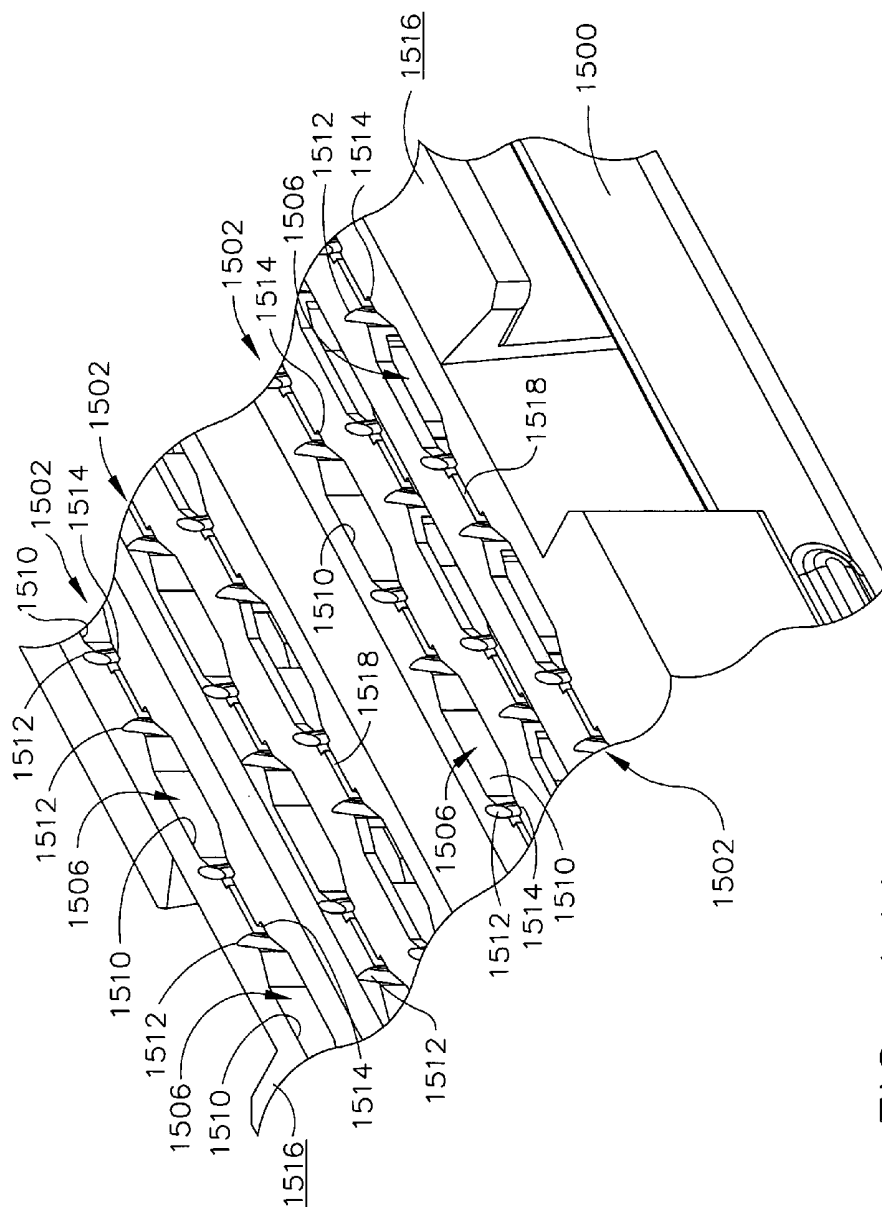


FIG. 141

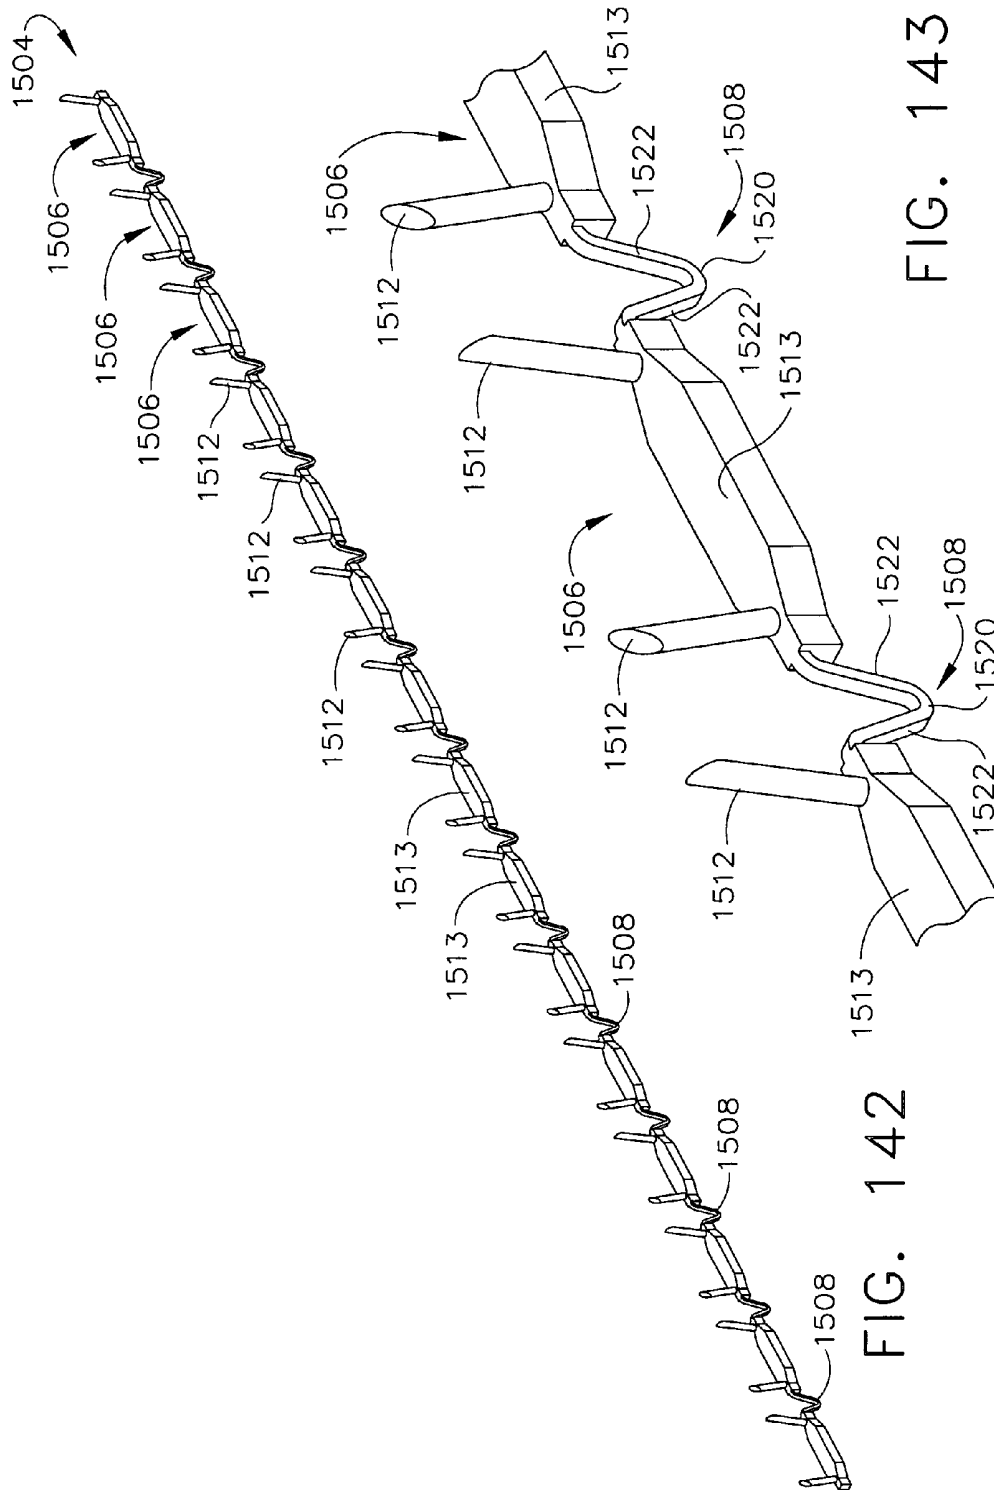


FIG. 143

FIG. 142

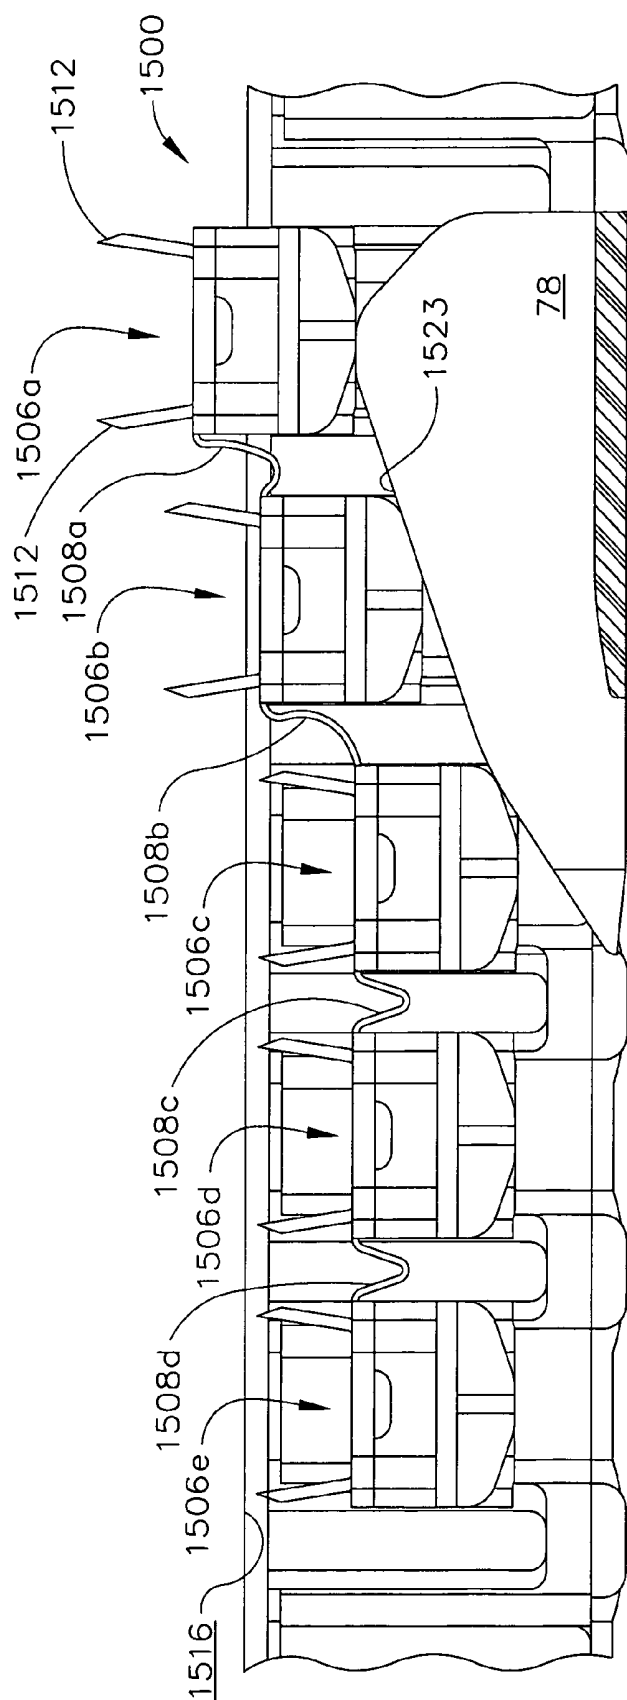


FIG. 144

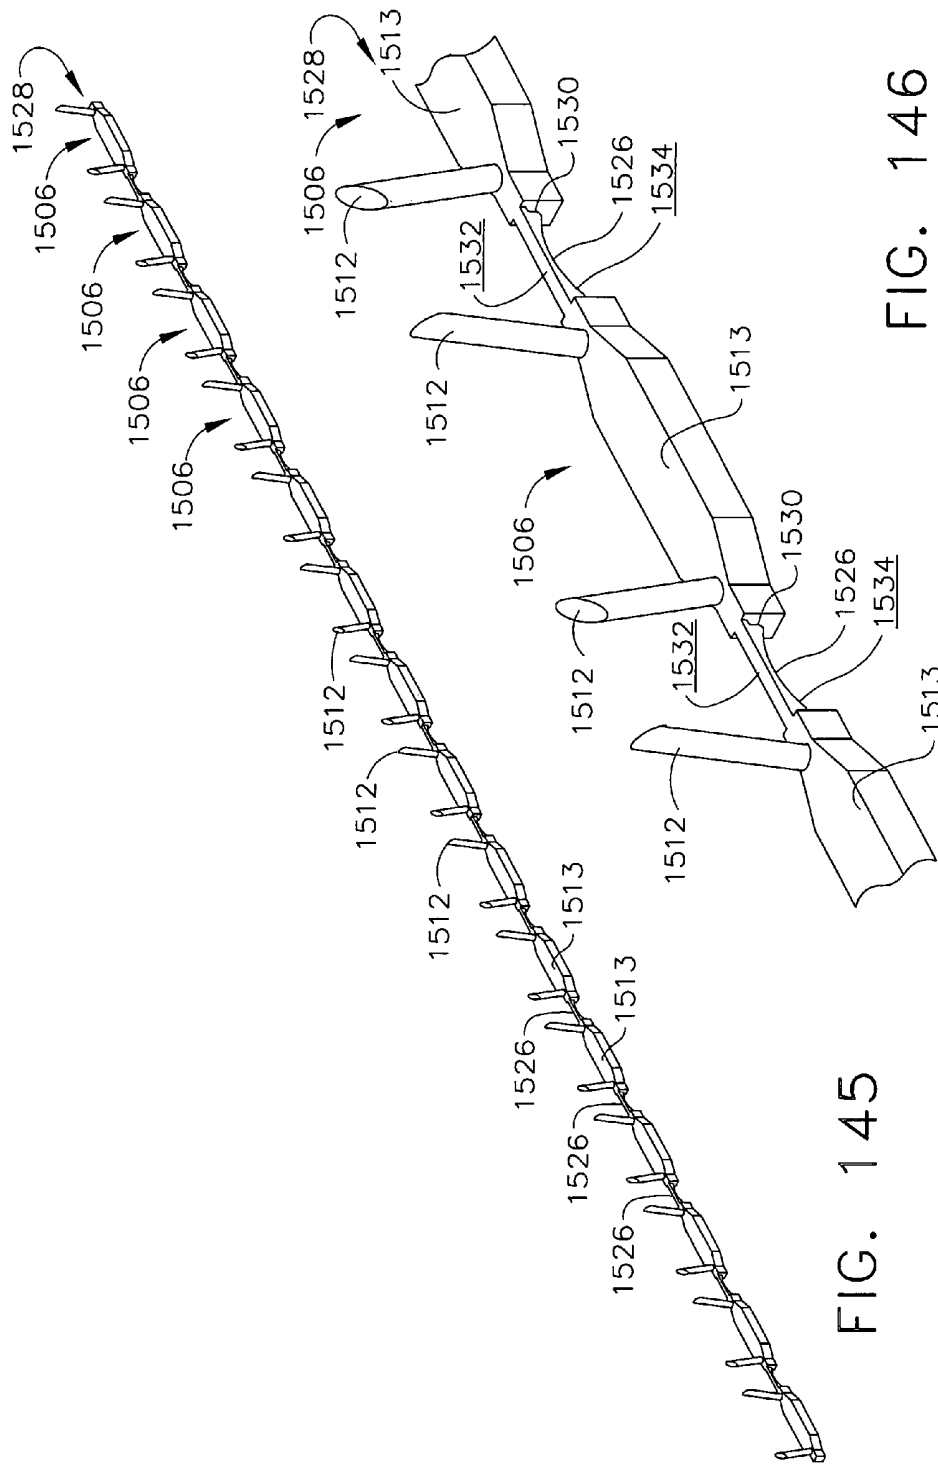


FIG. 145

FIG. 146

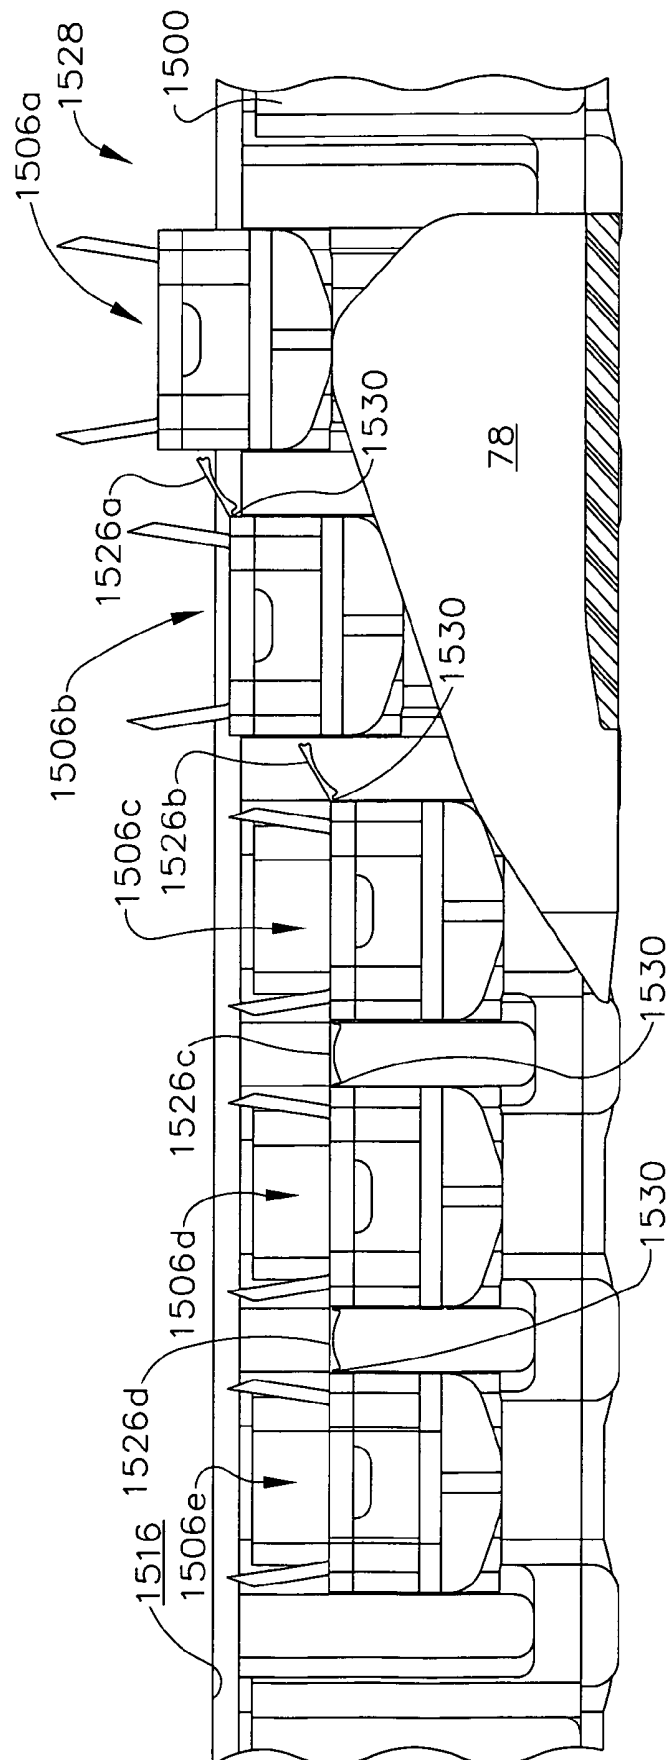


FIG. 147

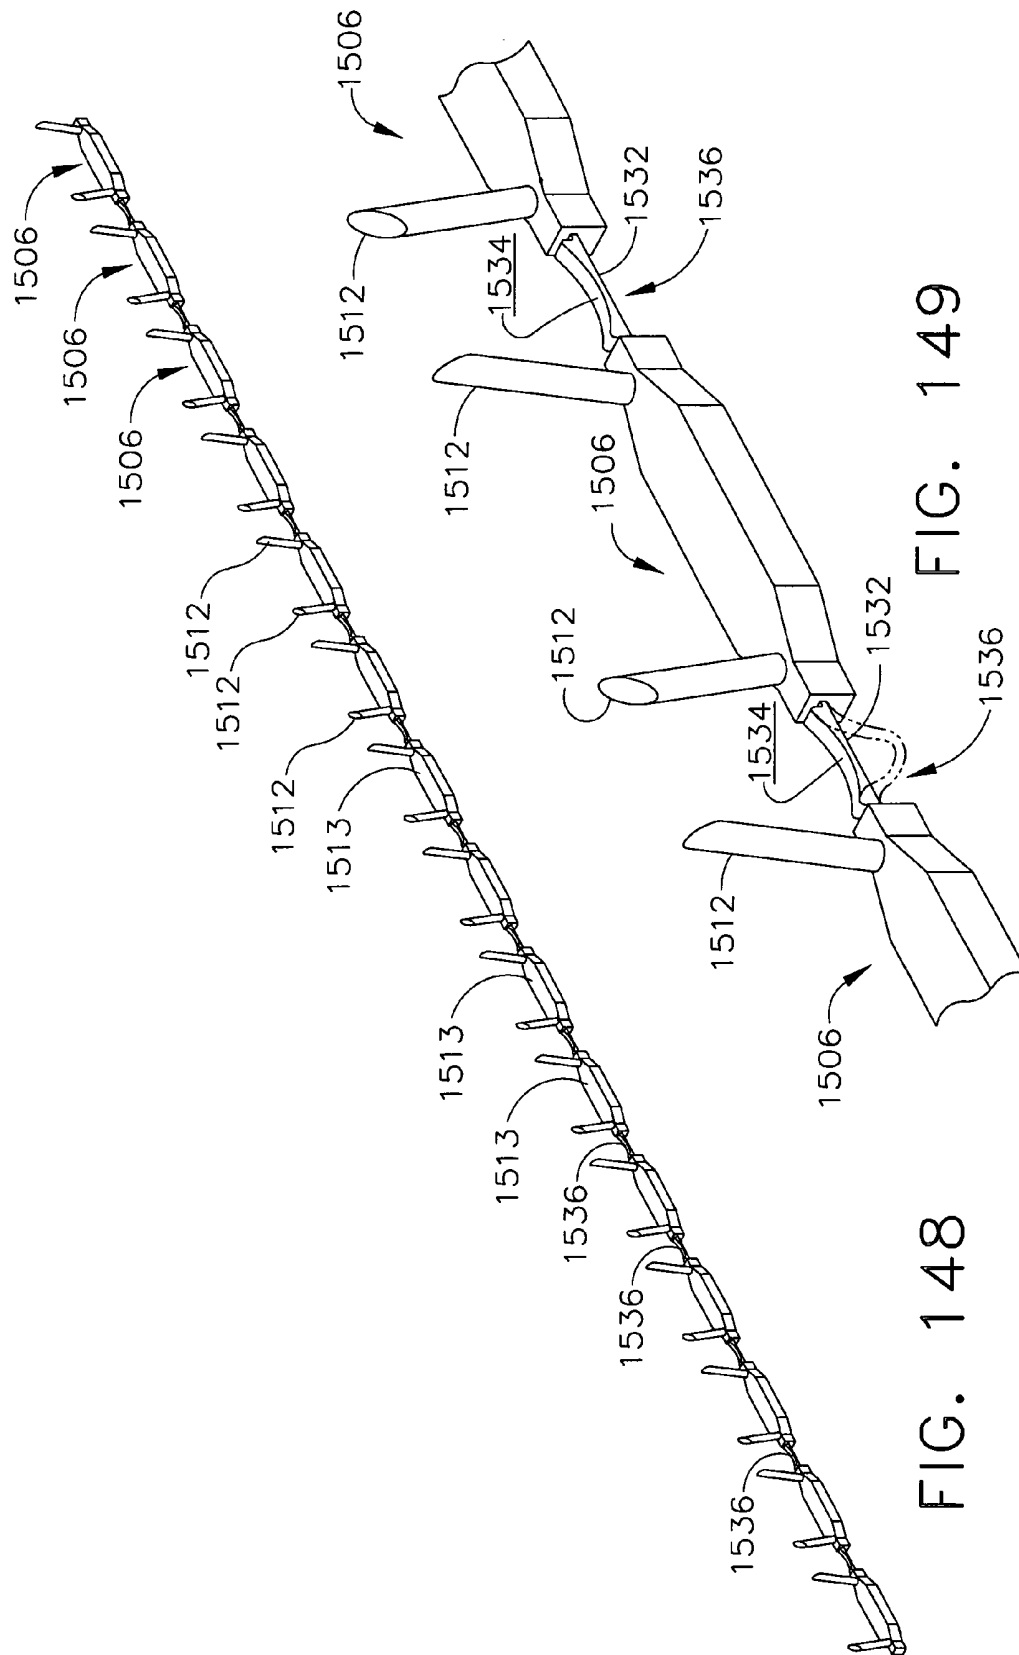


FIG. 149

FIG. 148

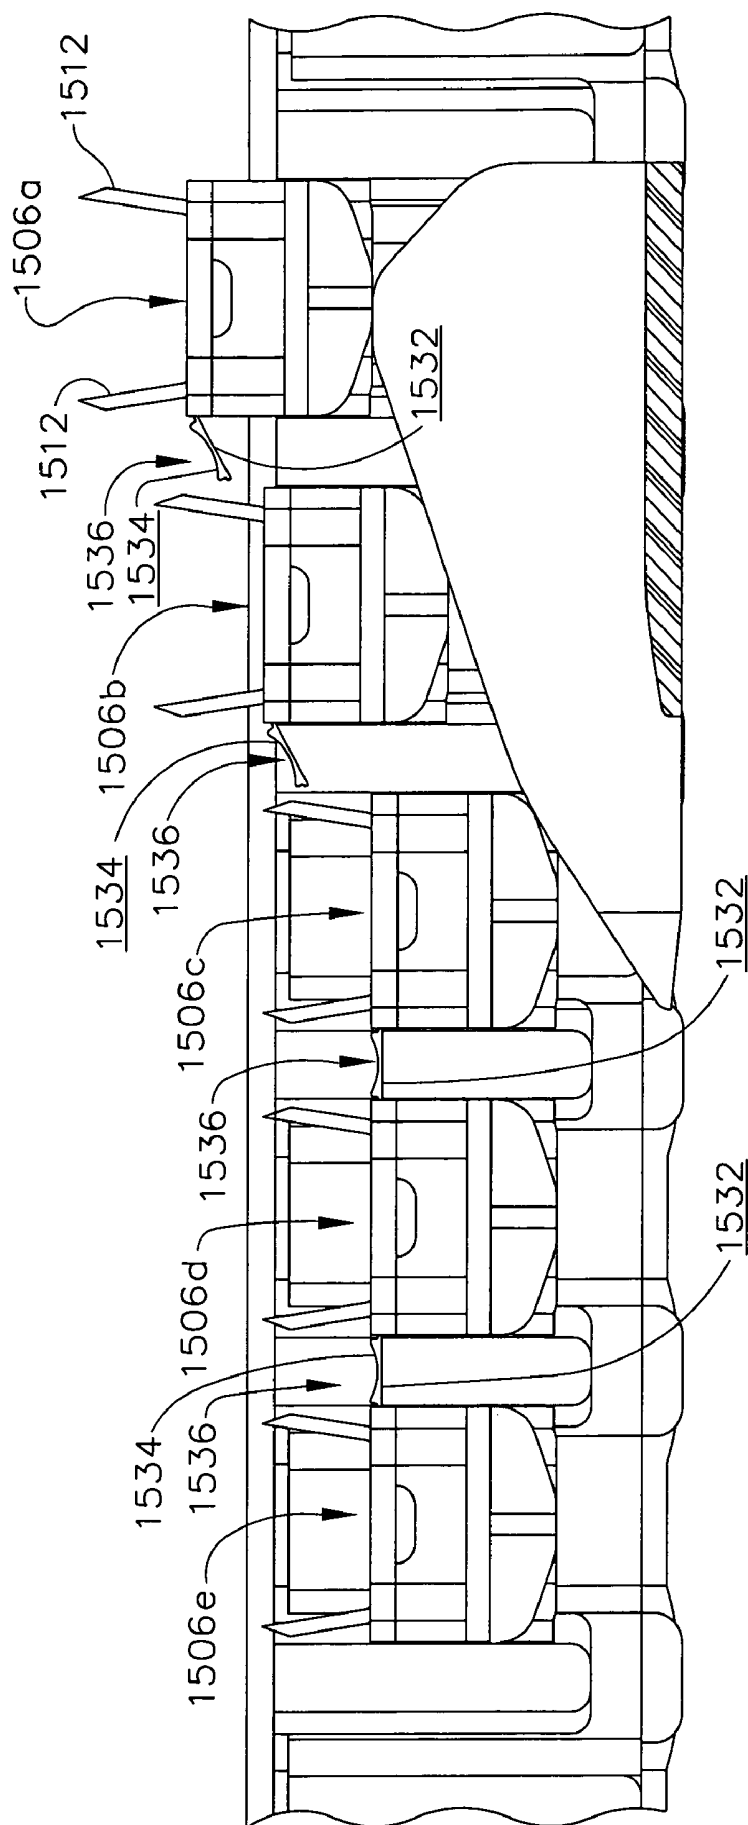


FIG. 150

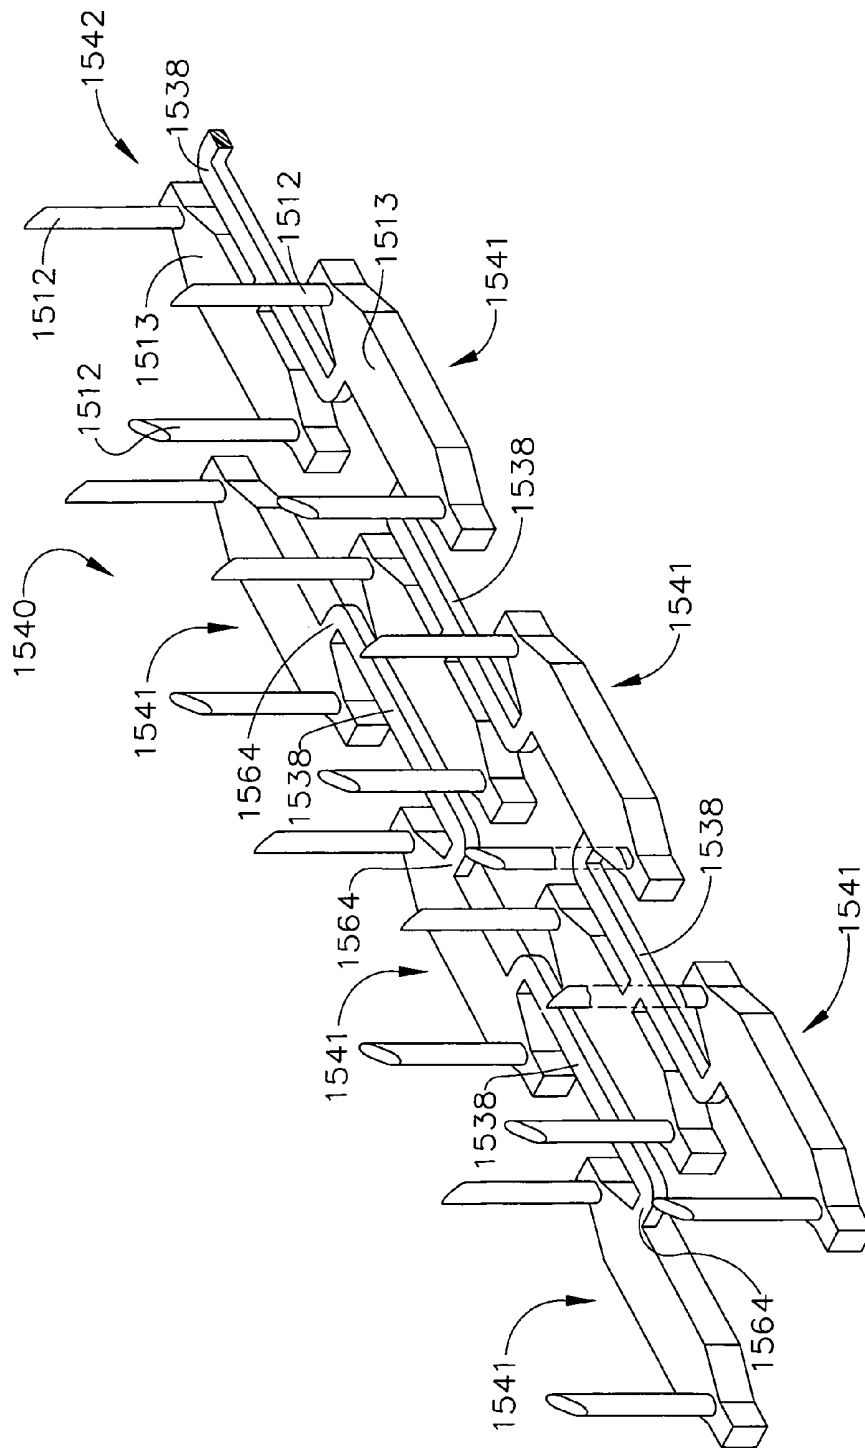


FIG. 151

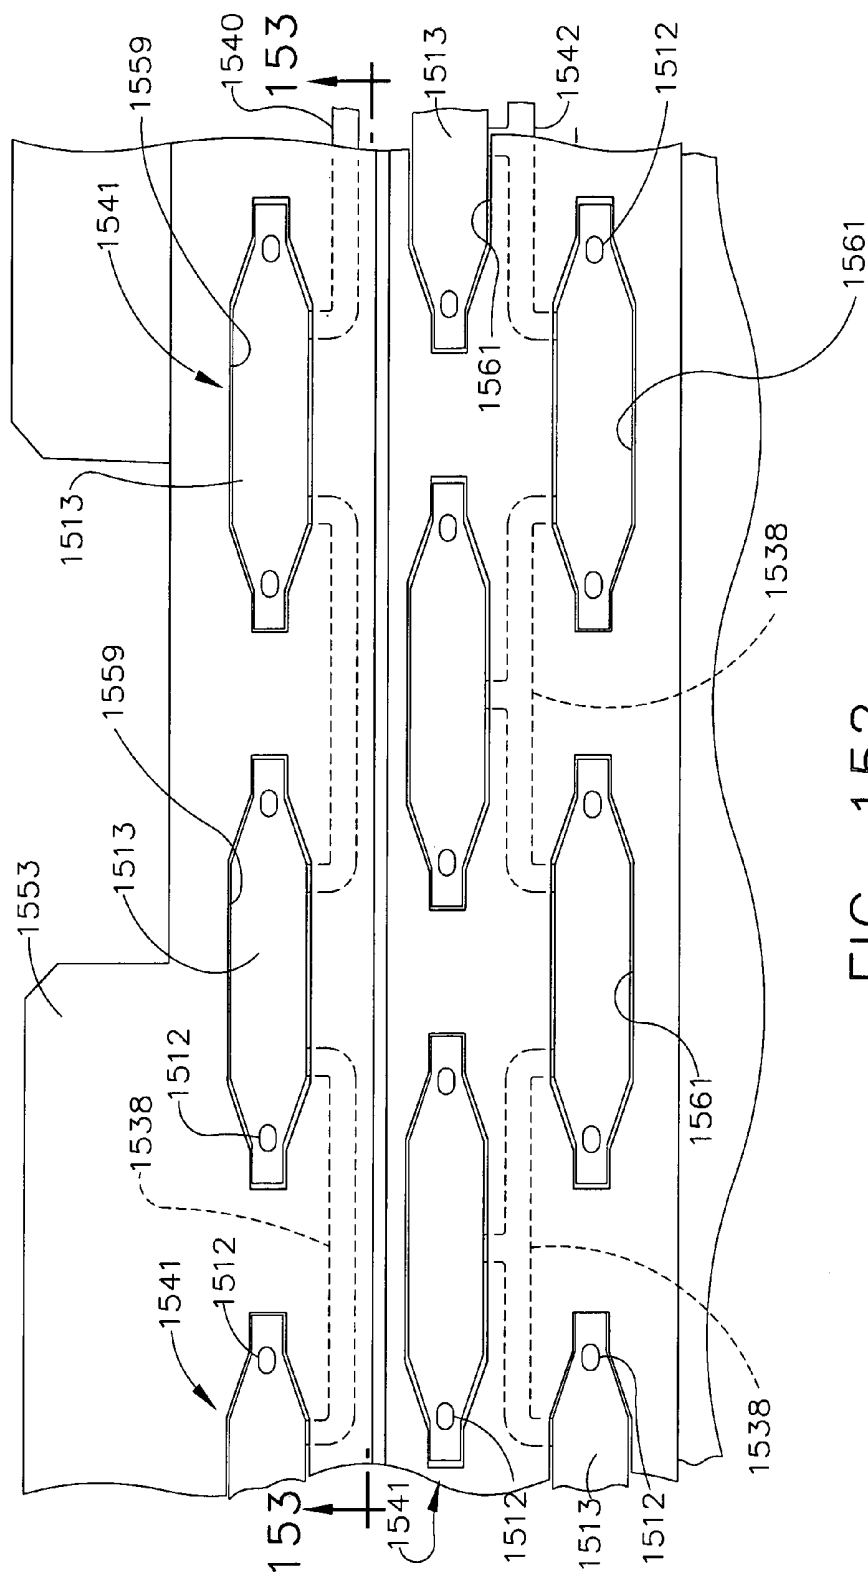


FIG. 152

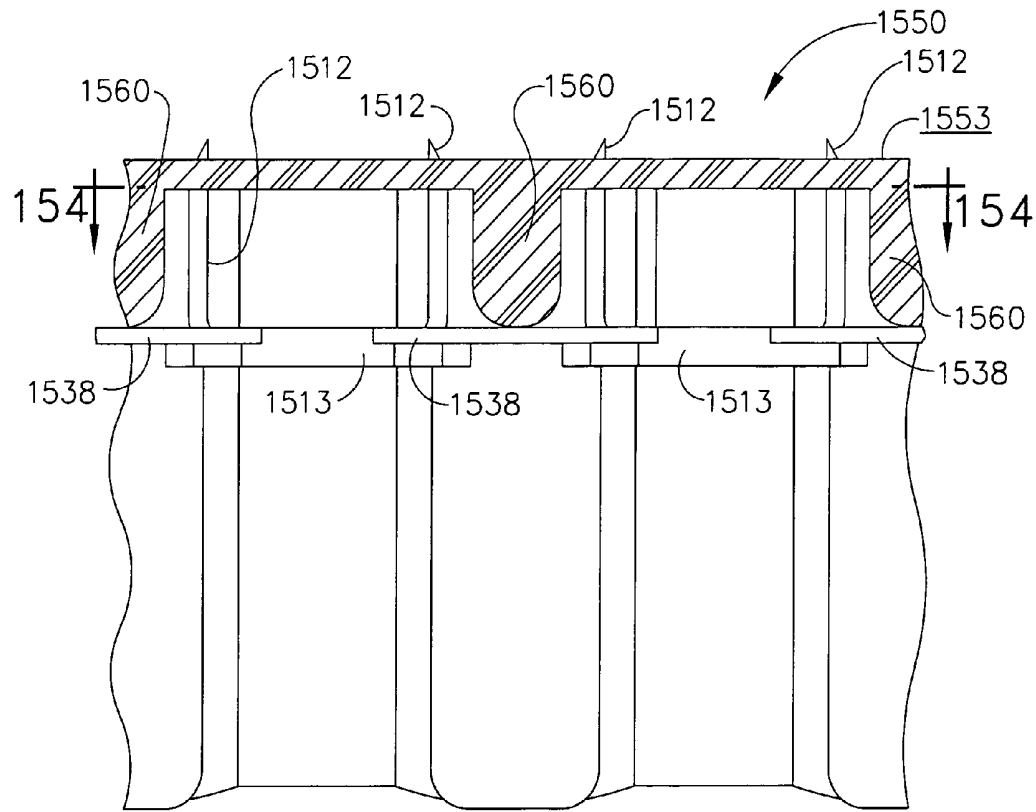


FIG. 153

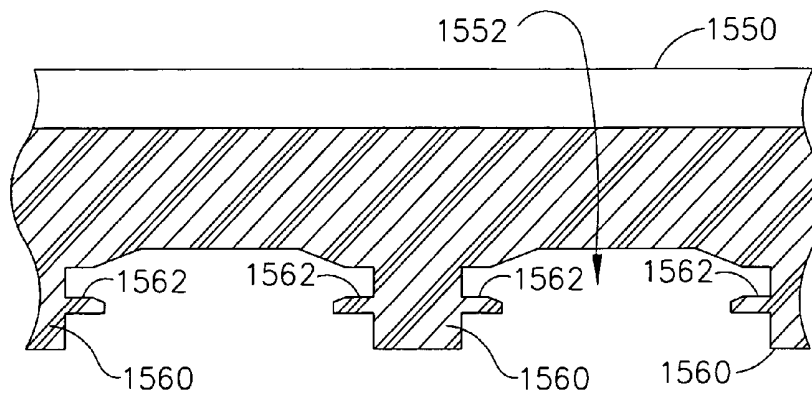


FIG. 154

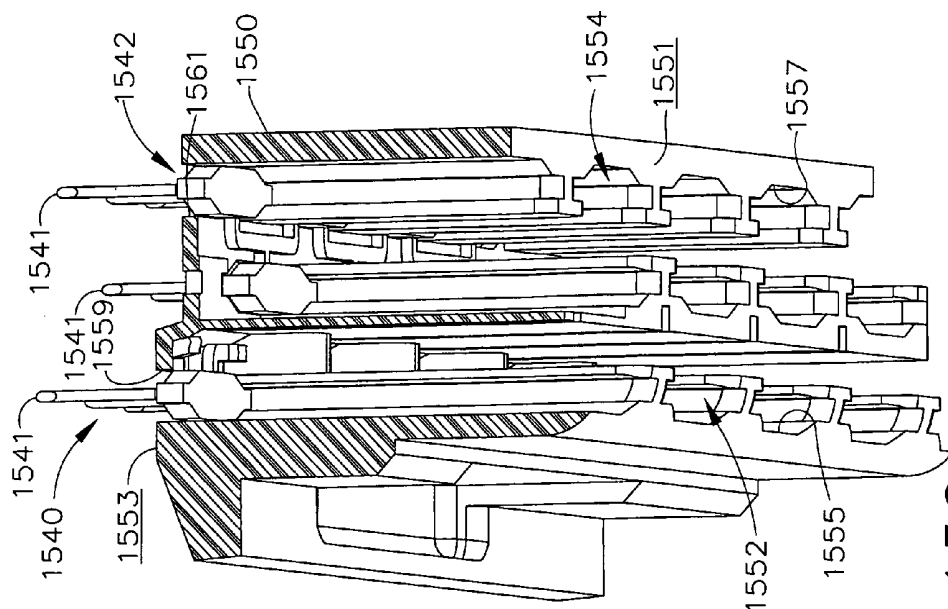


FIG. 156

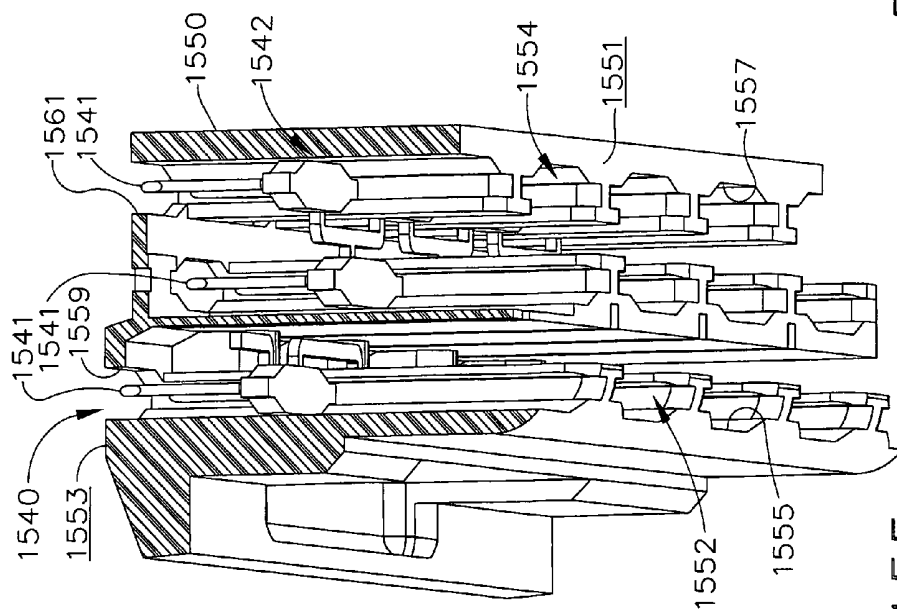


FIG. 155

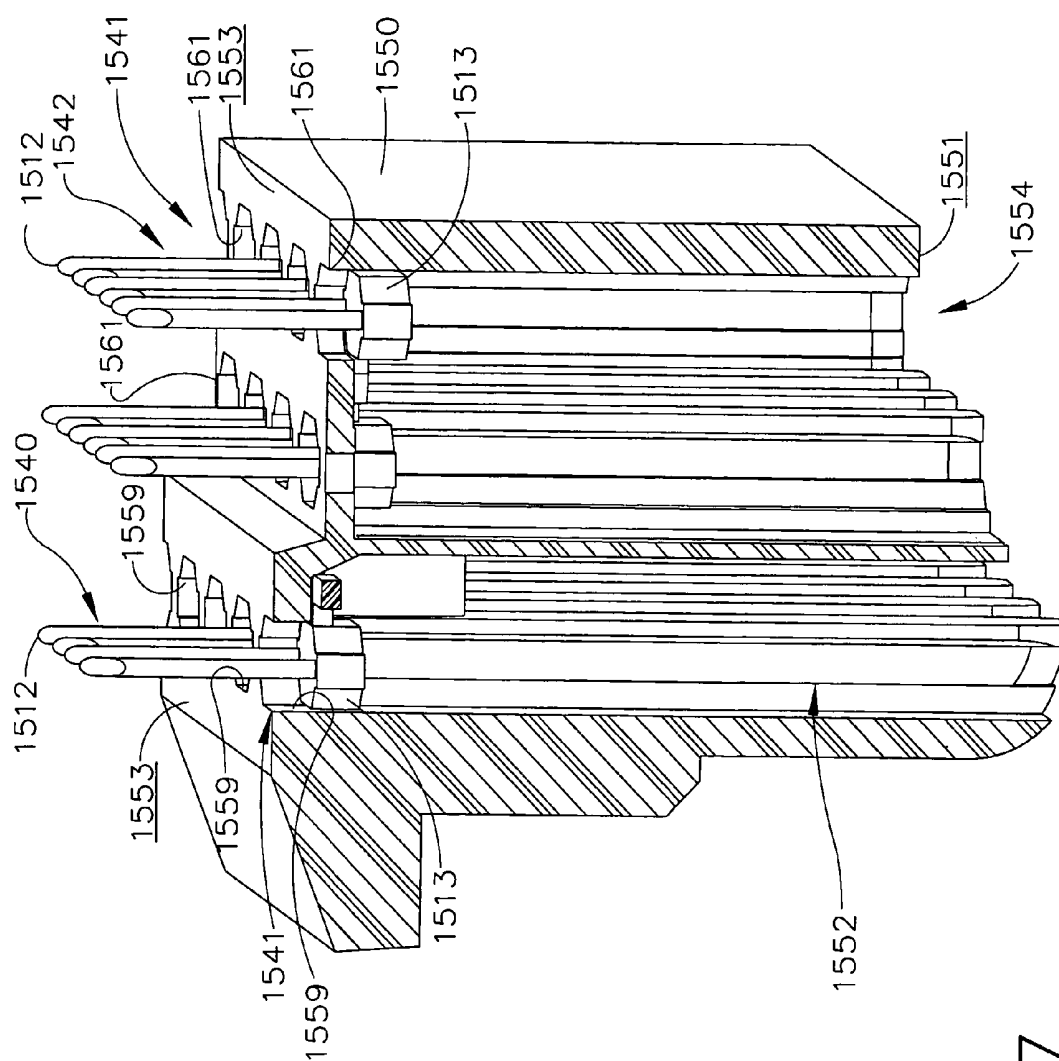


FIG. 157

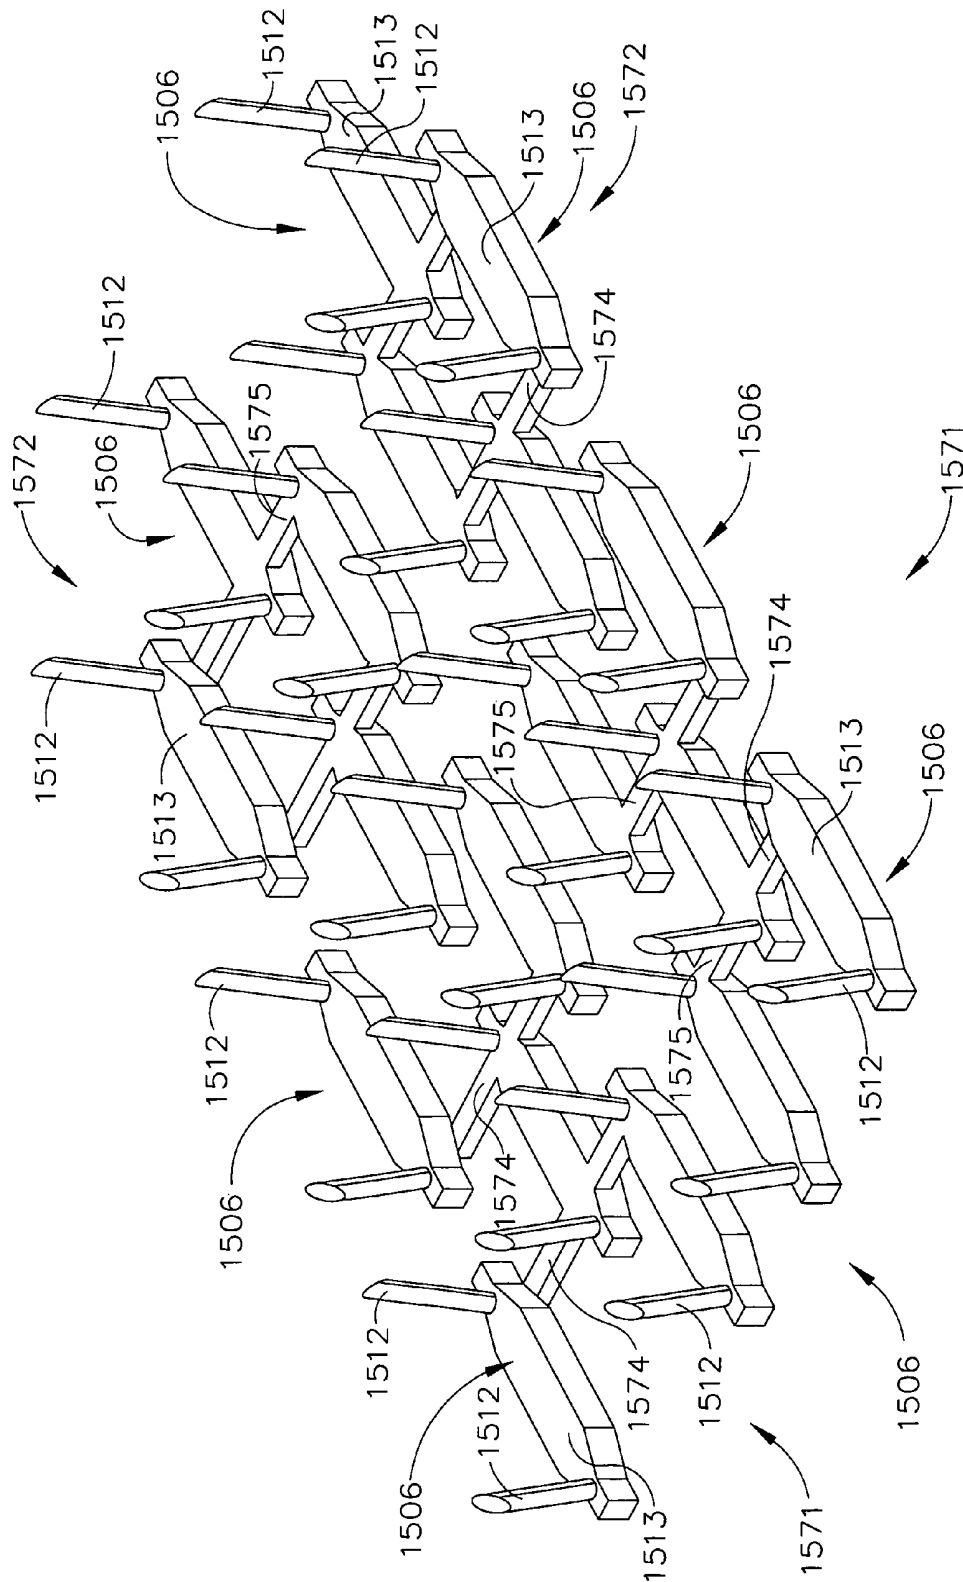


FIG. 158

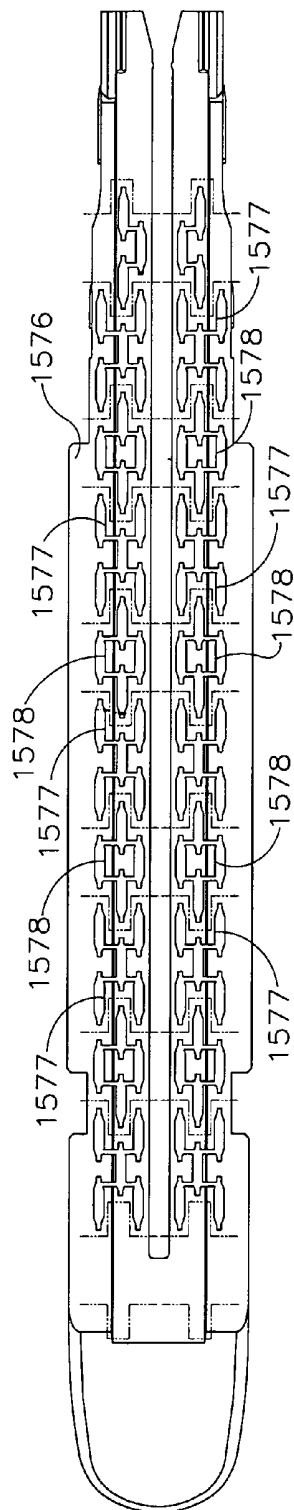


FIG. 159

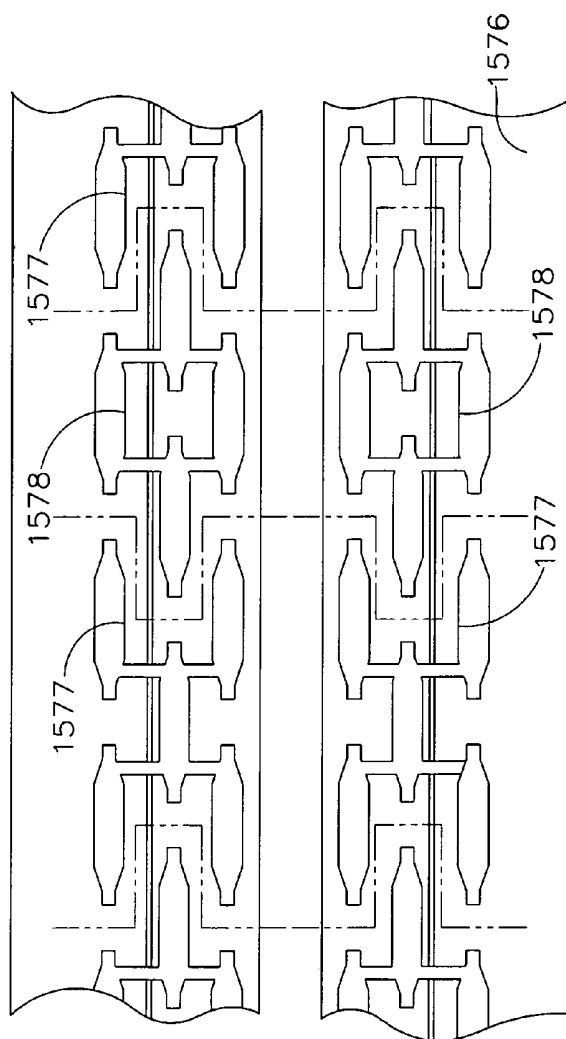


FIG. 159A

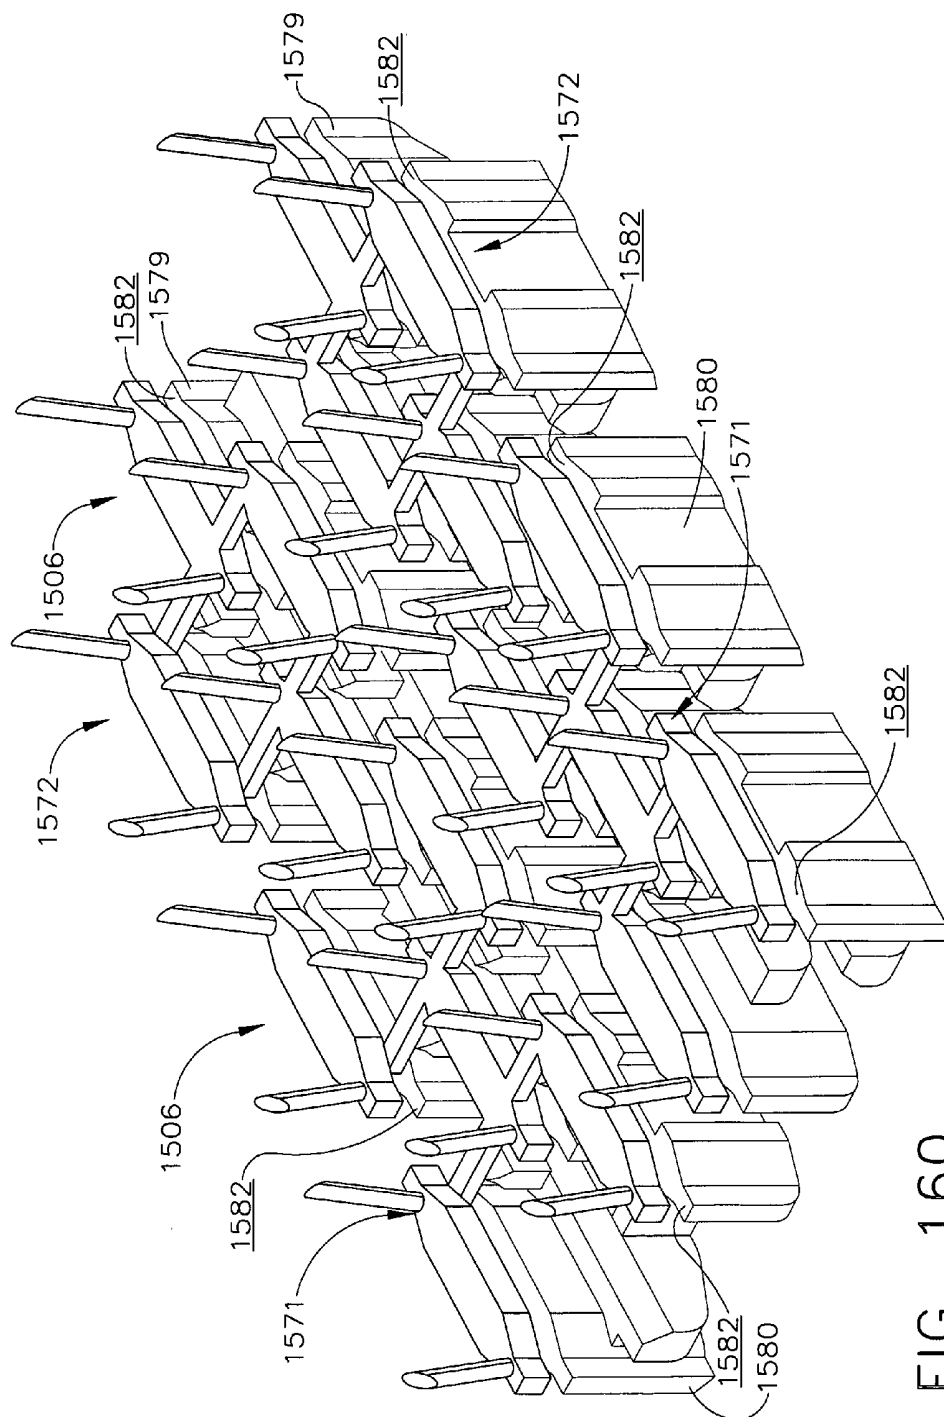


FIG. 160

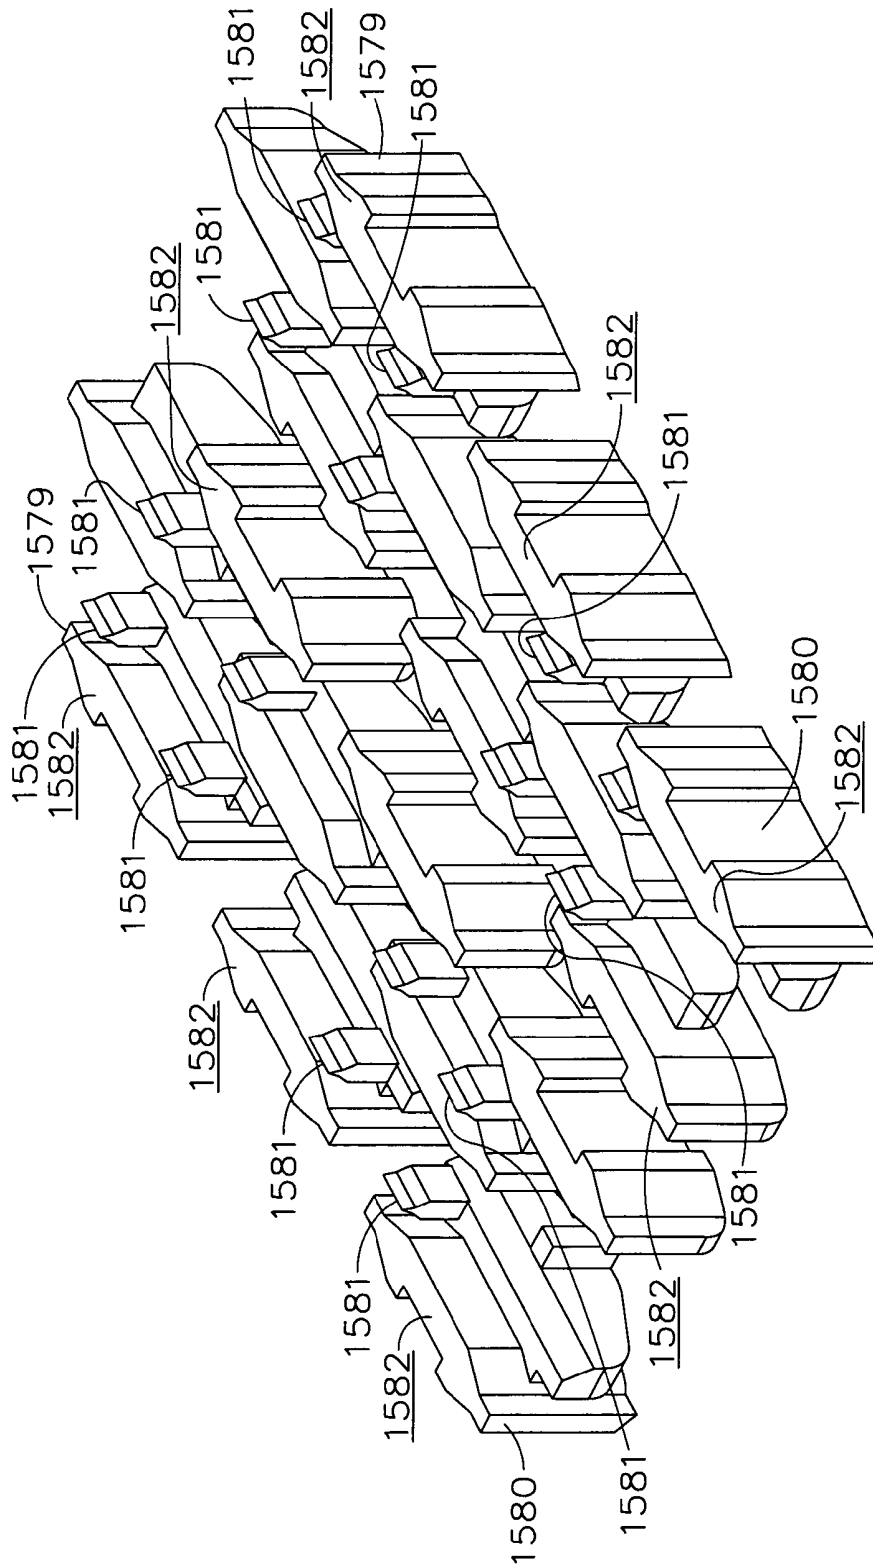


FIG. 161

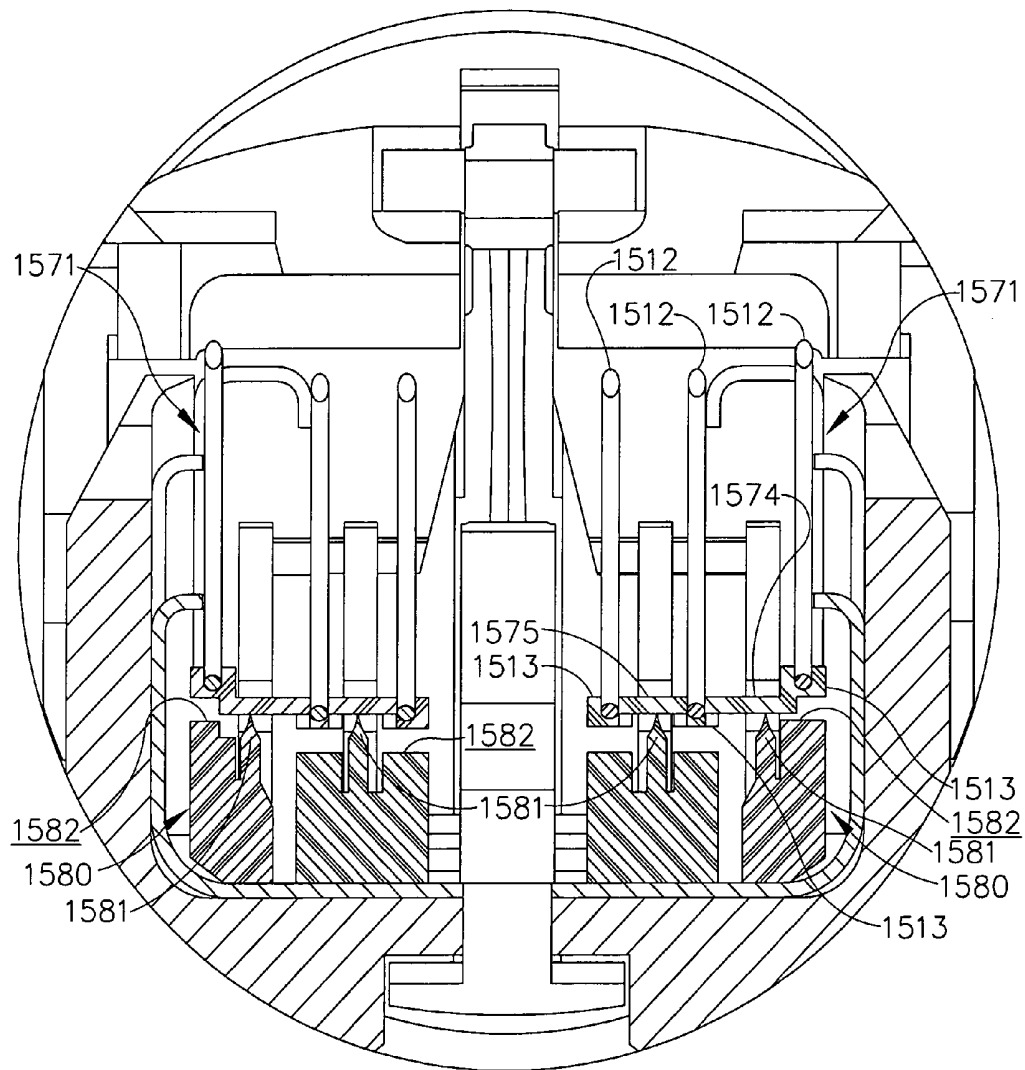


FIG. 162

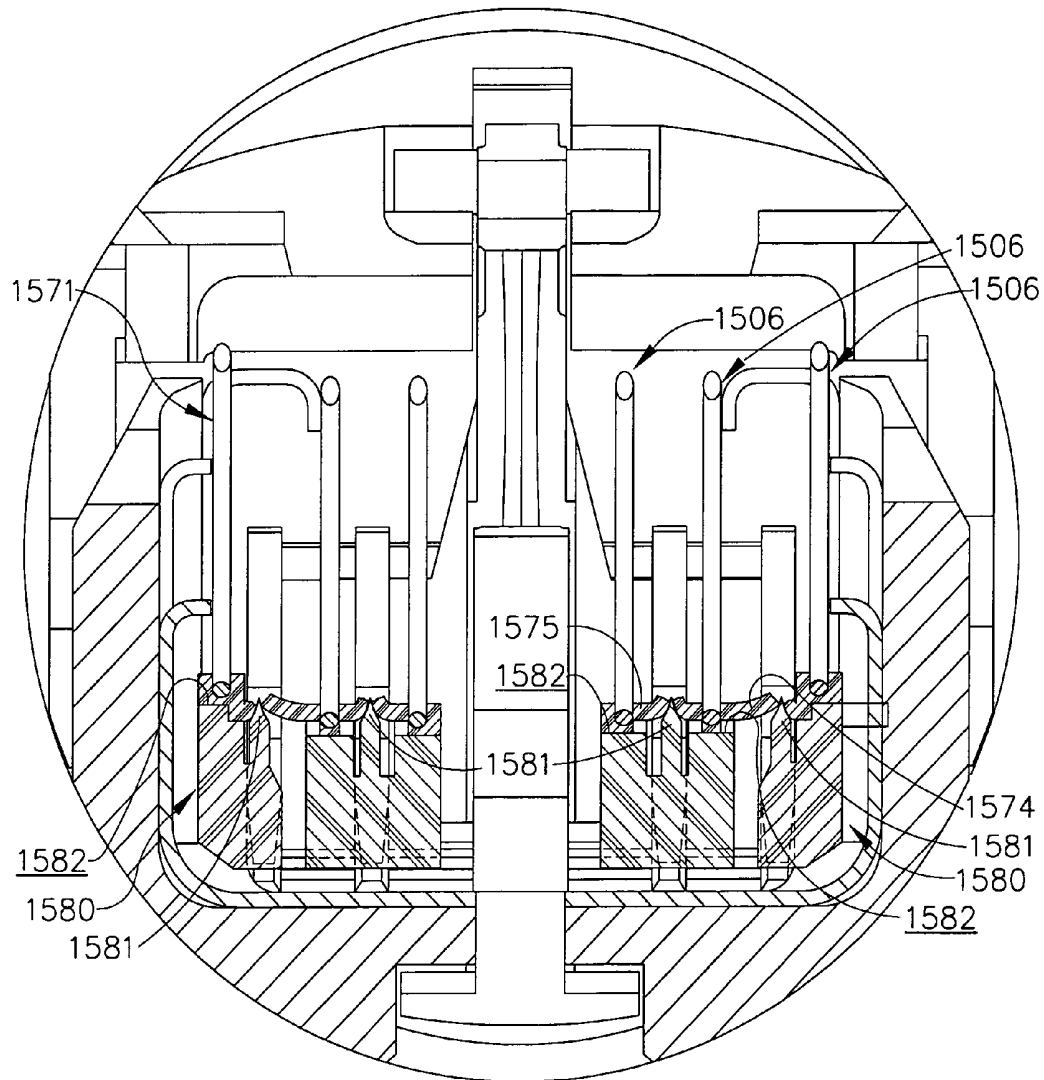
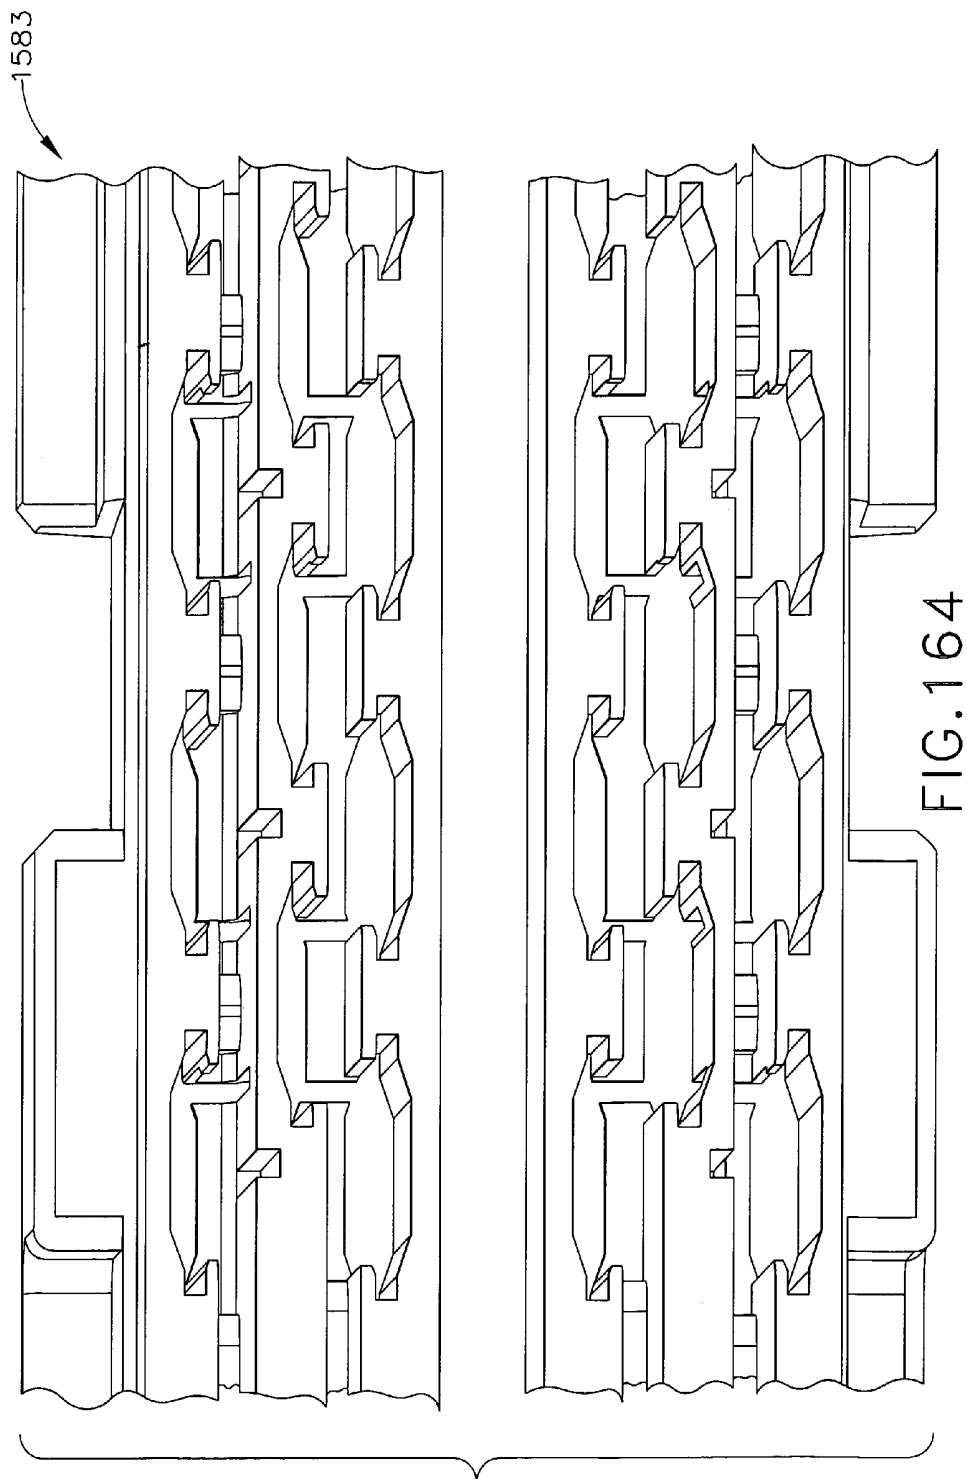


FIG. 163



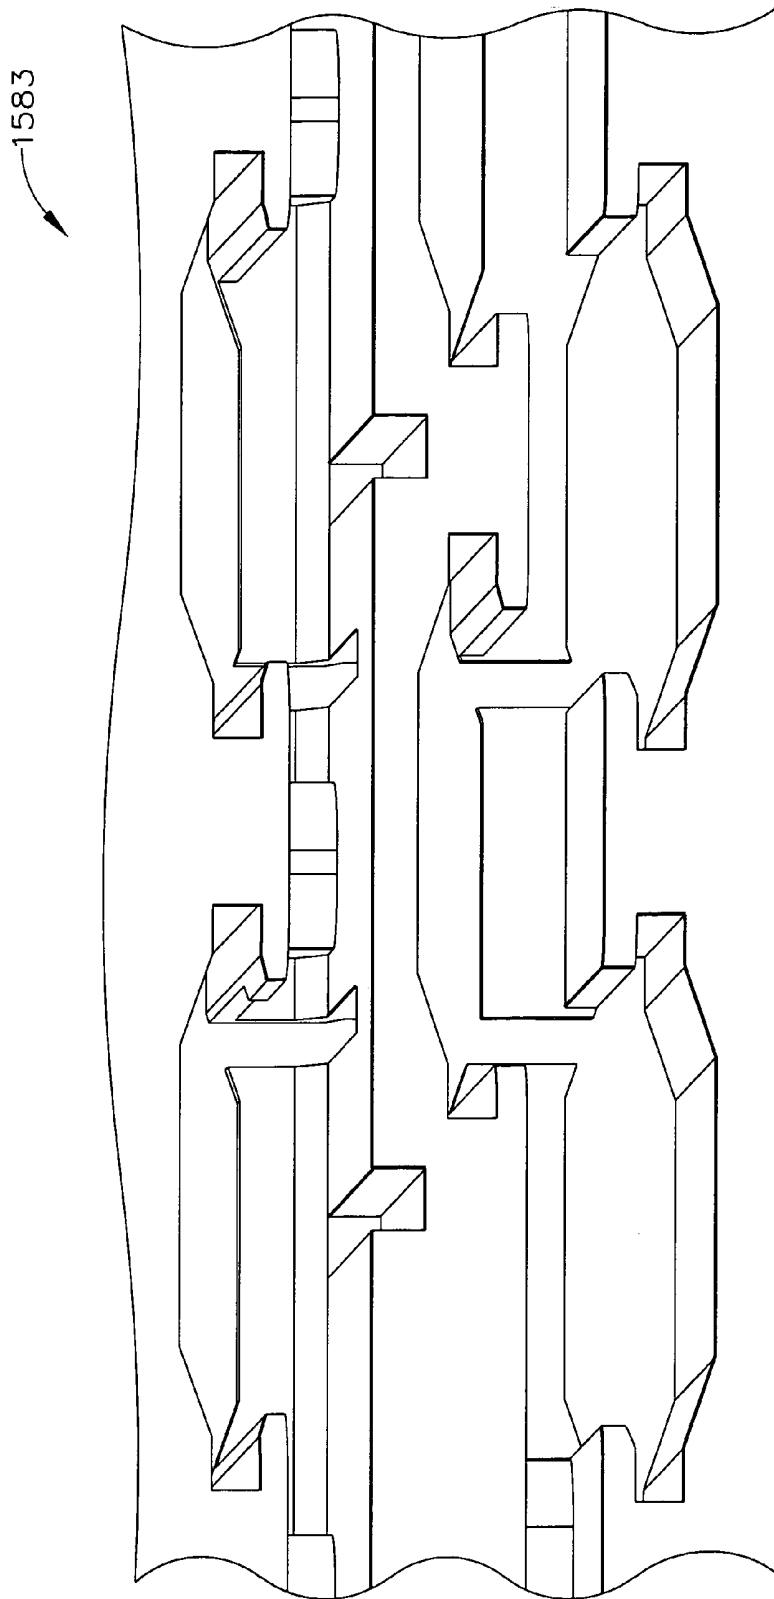


FIG. 164A

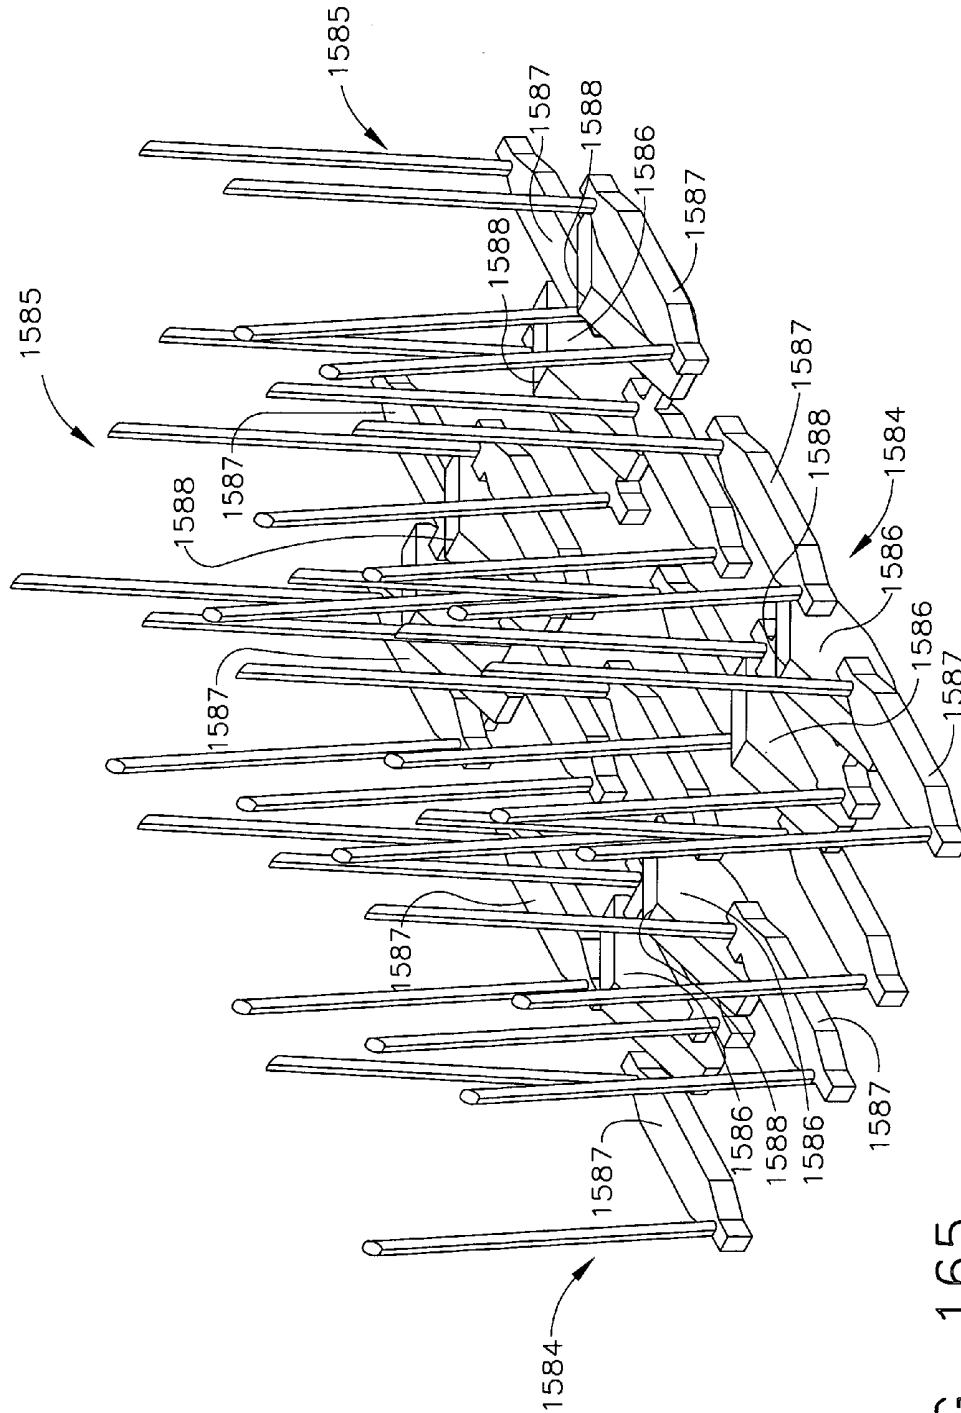


FIG. 165

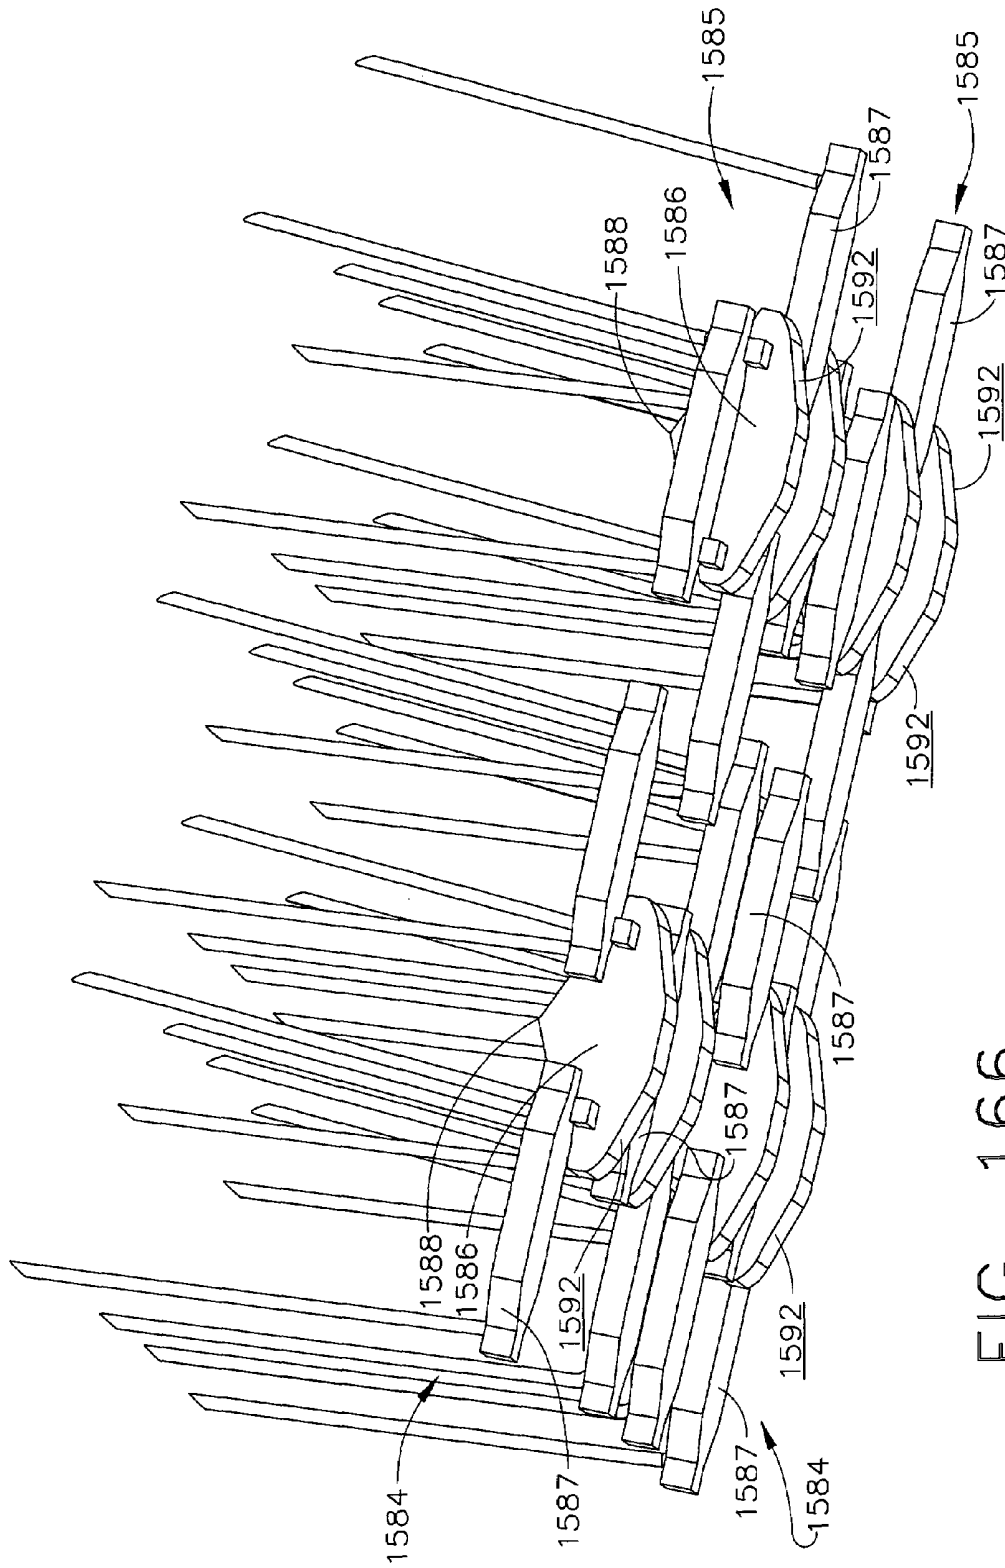


FIG. 166

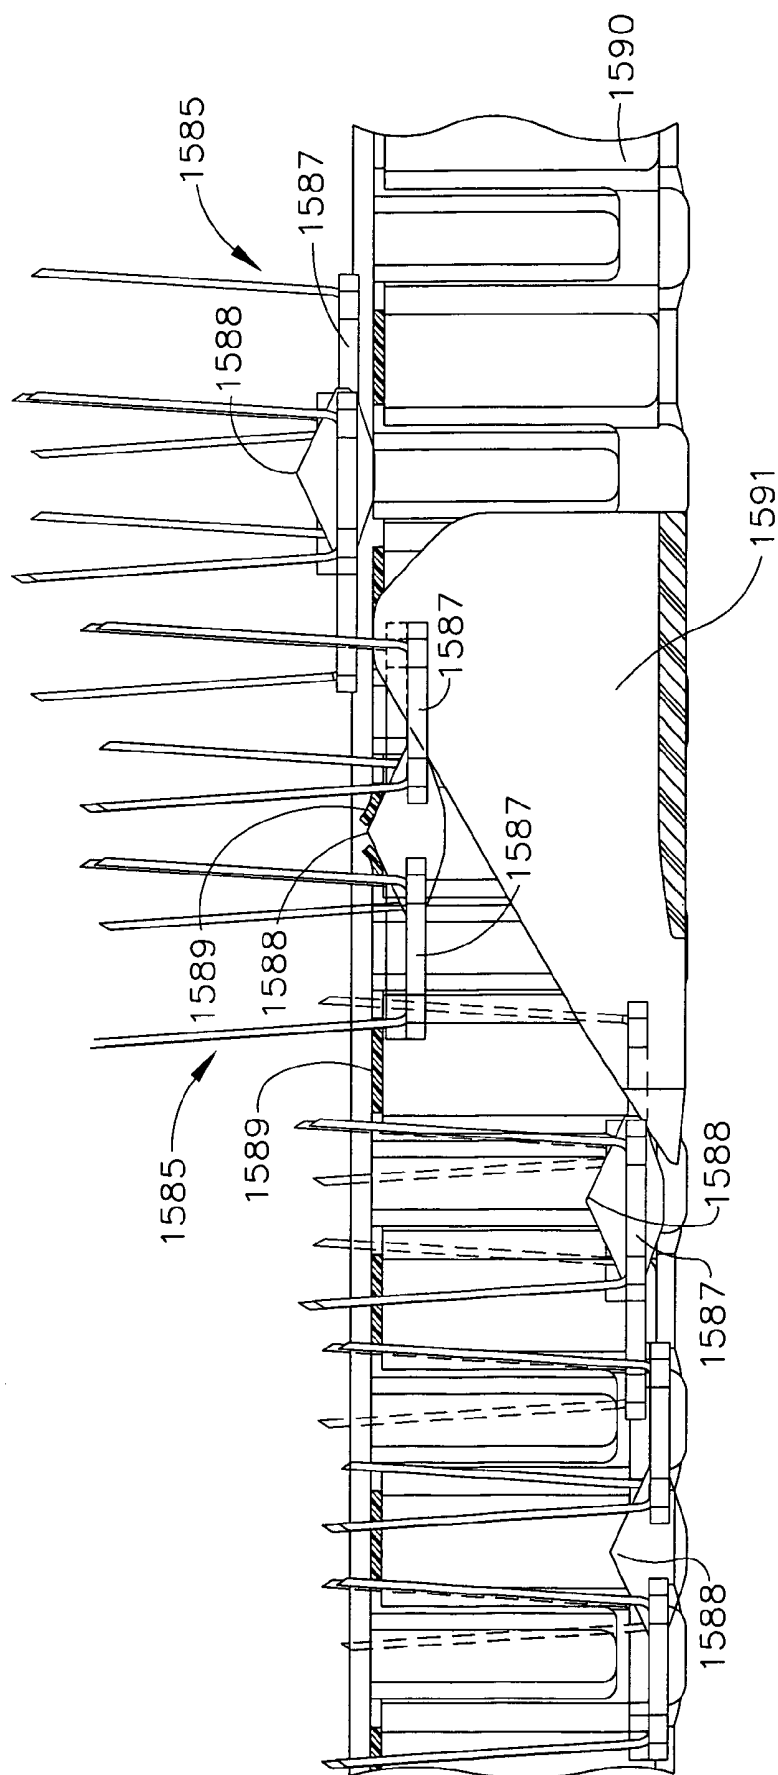


FIG. 167

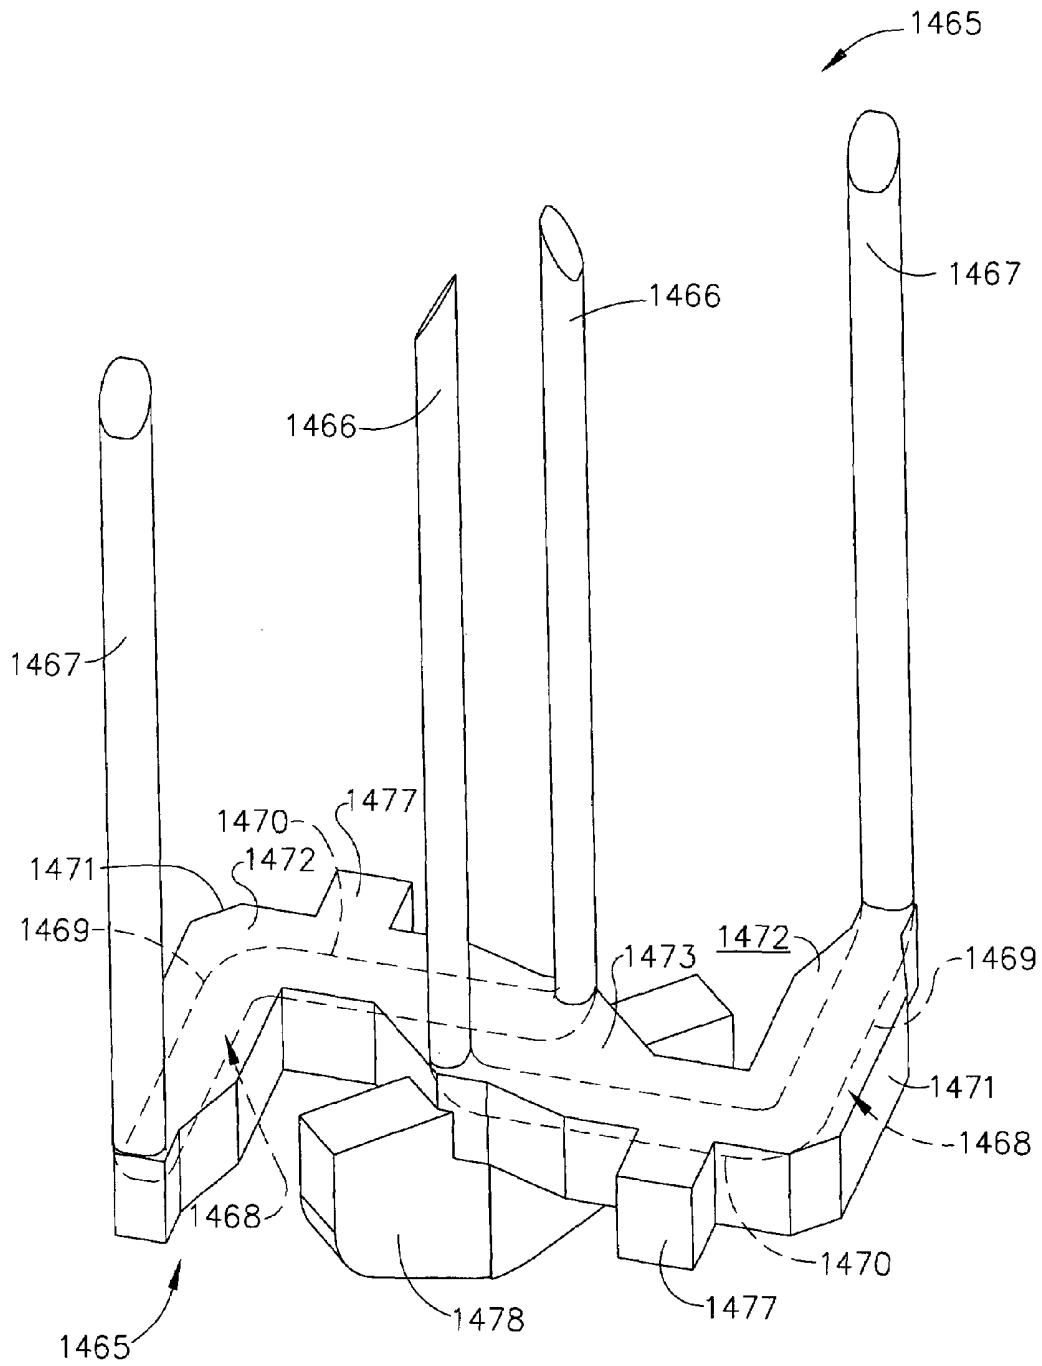


FIG. 168

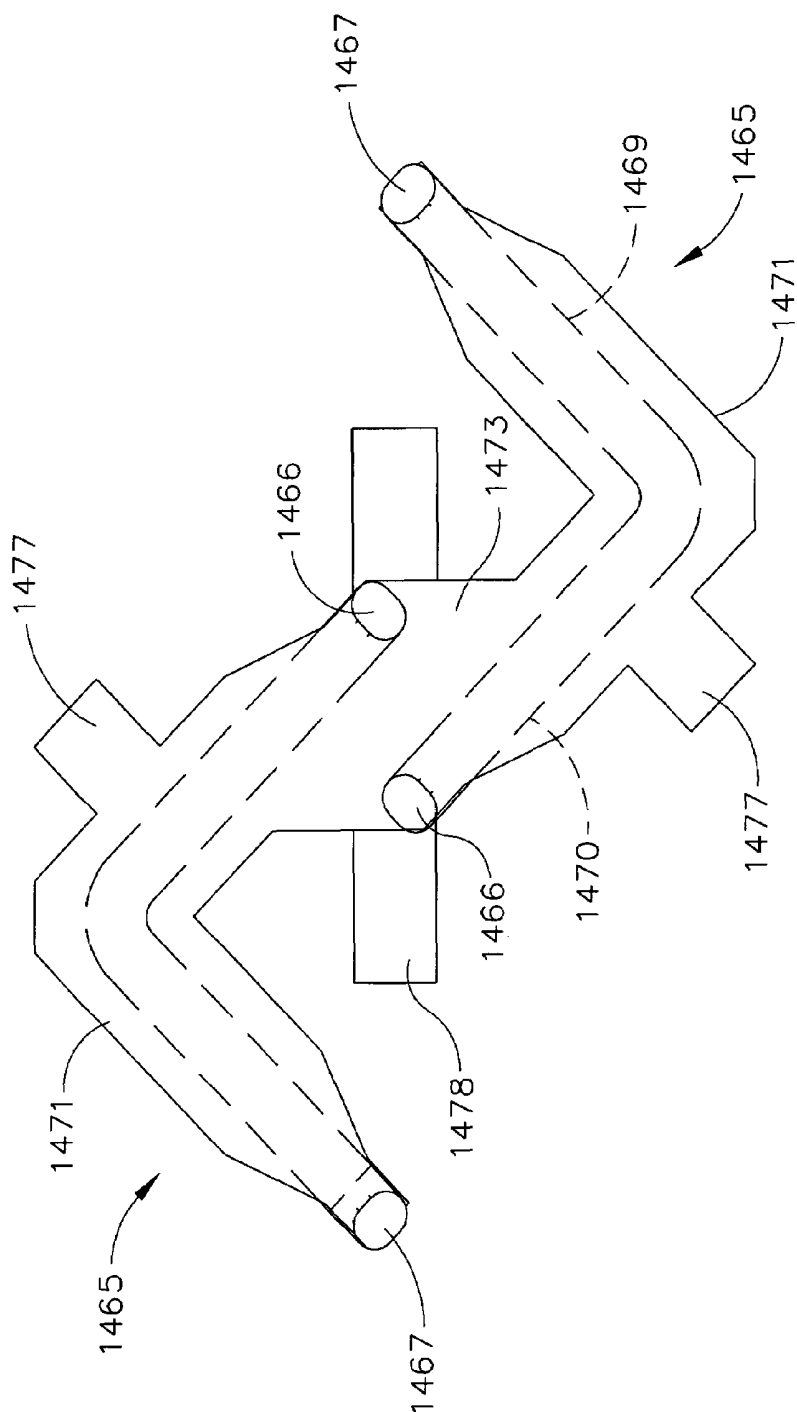
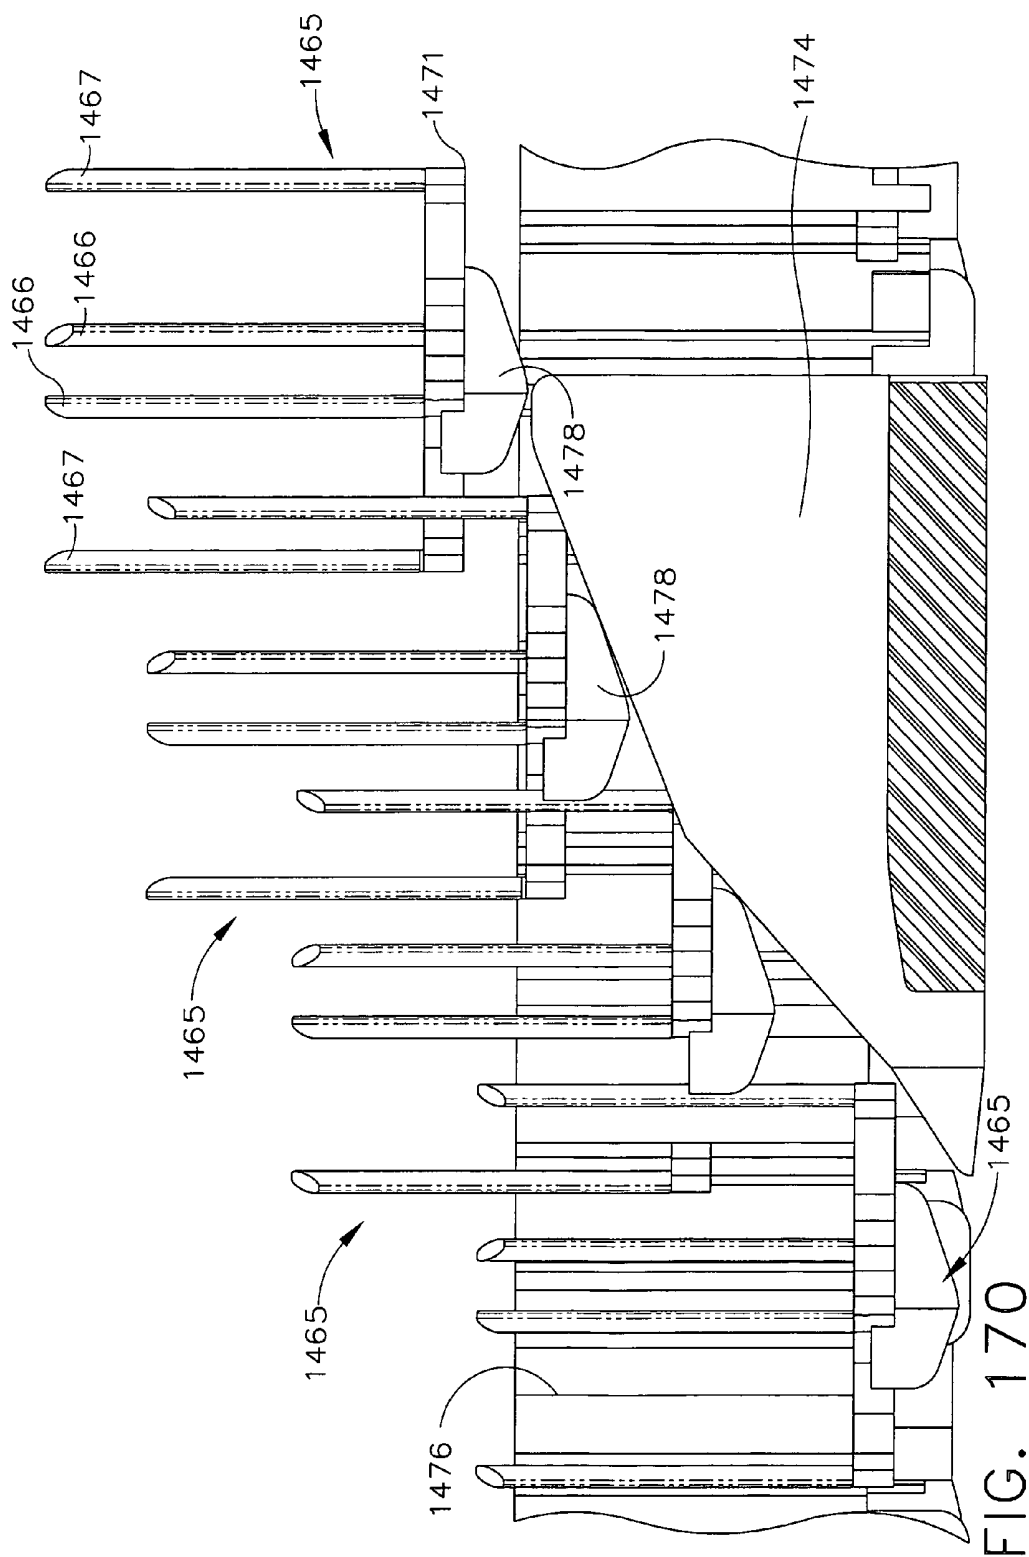


FIG. 169.



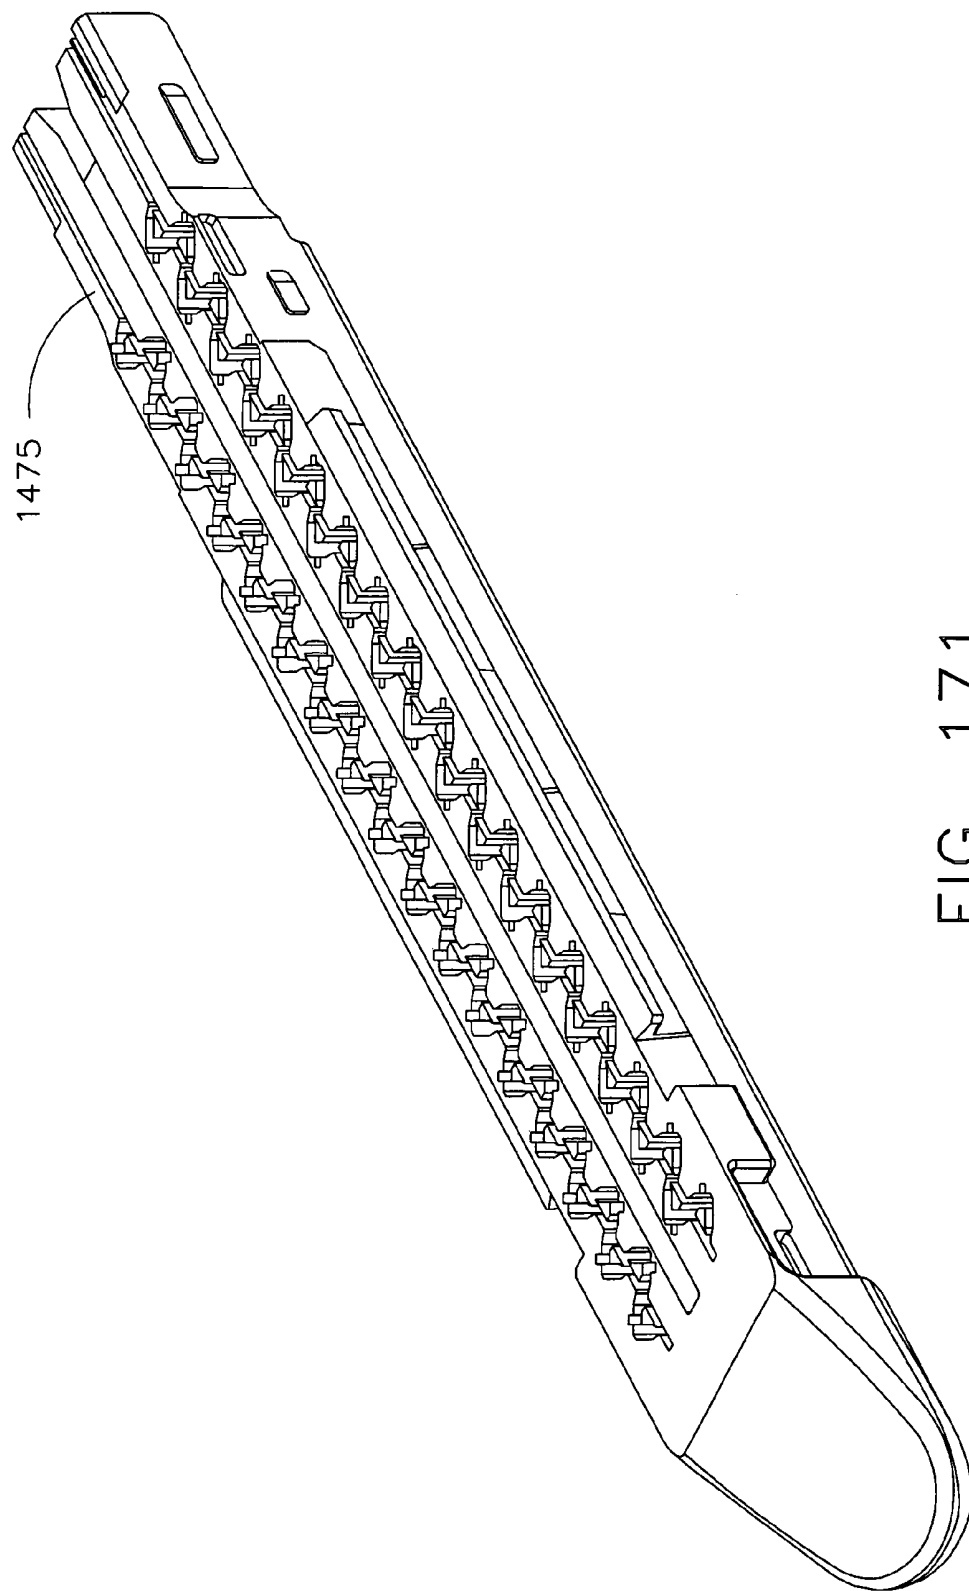


FIG. 171

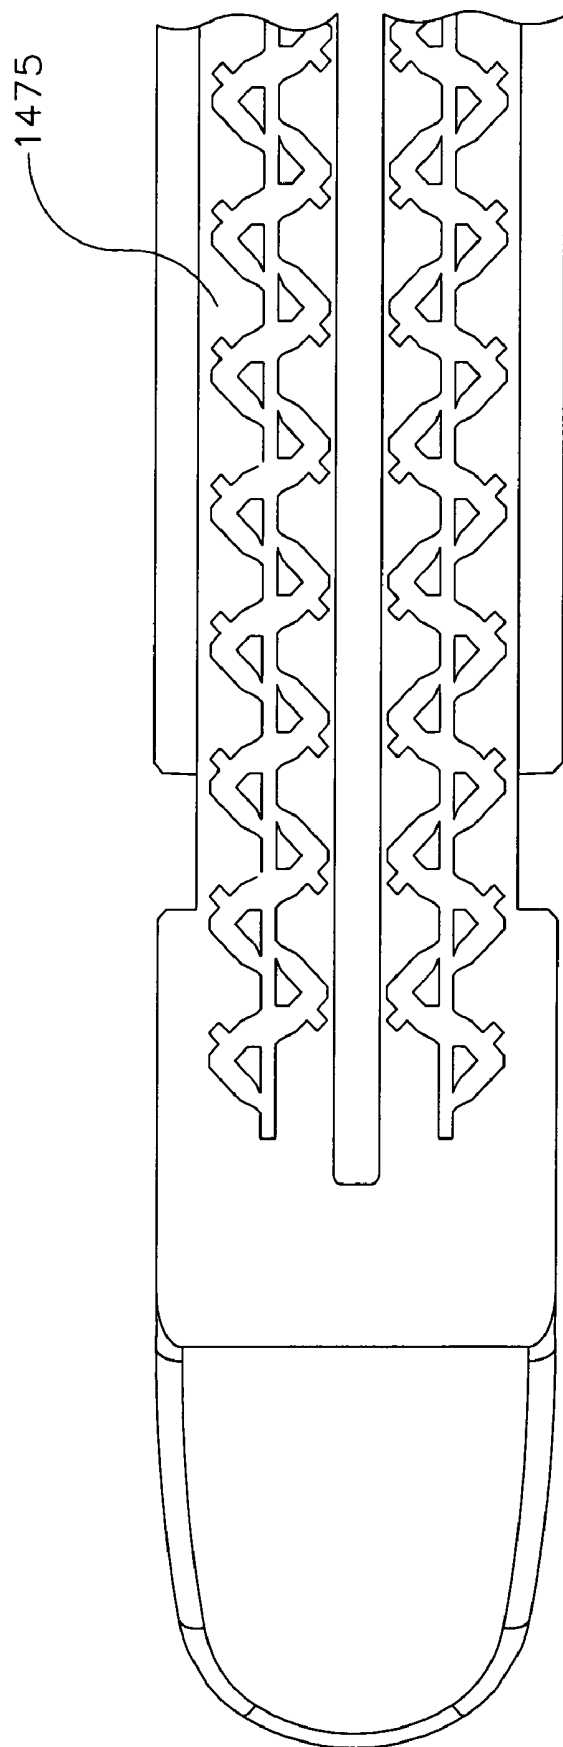


FIG. 172

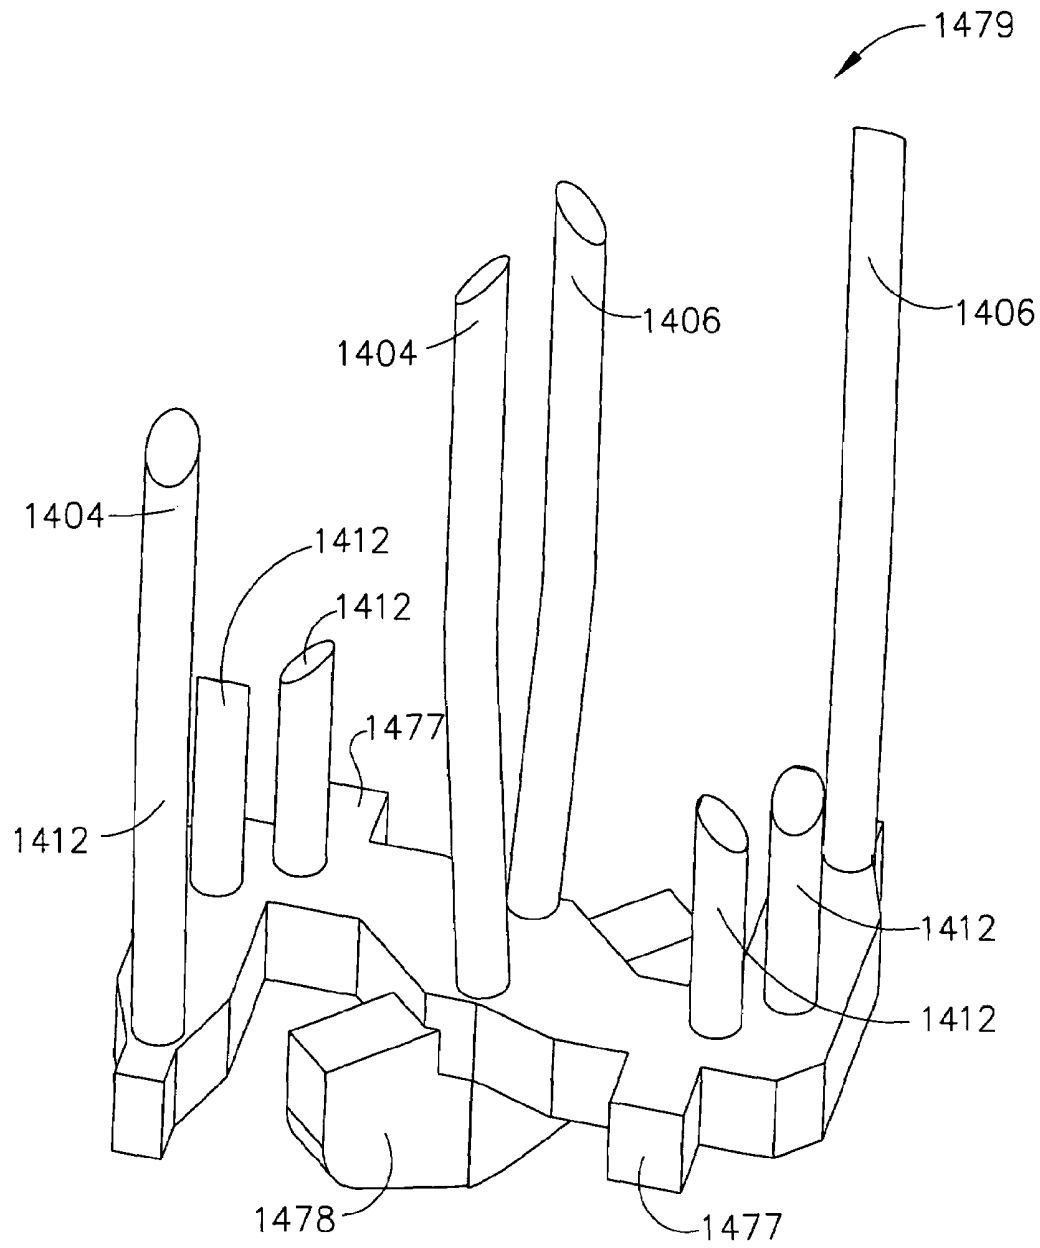


FIG. 173

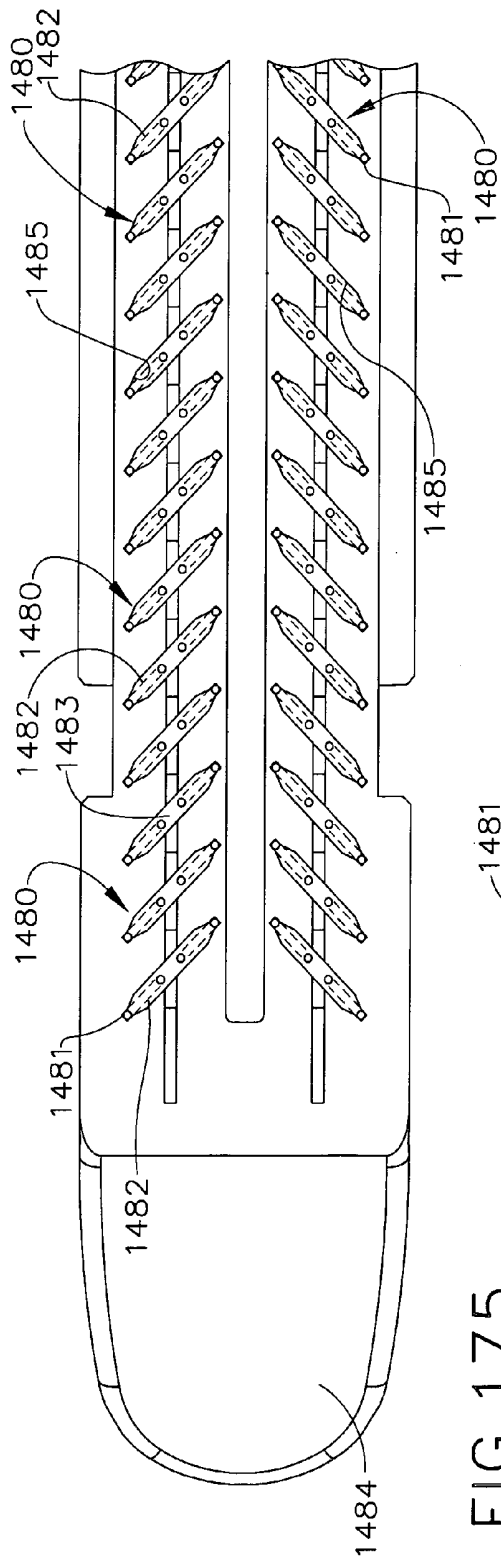


FIG. 175

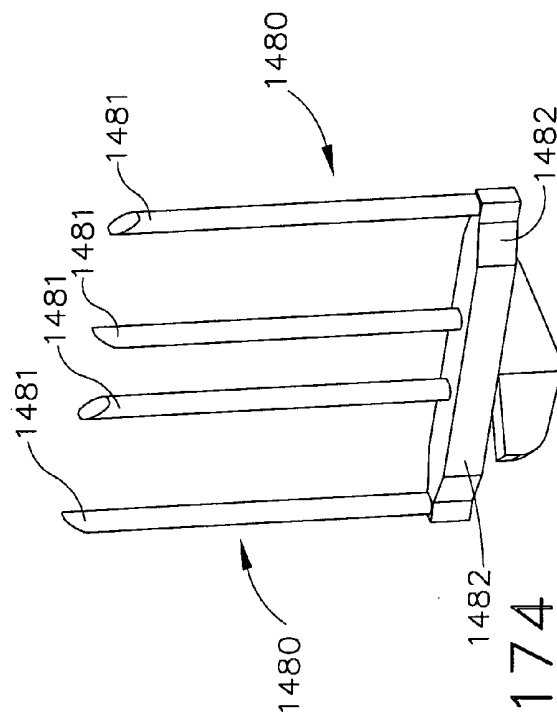
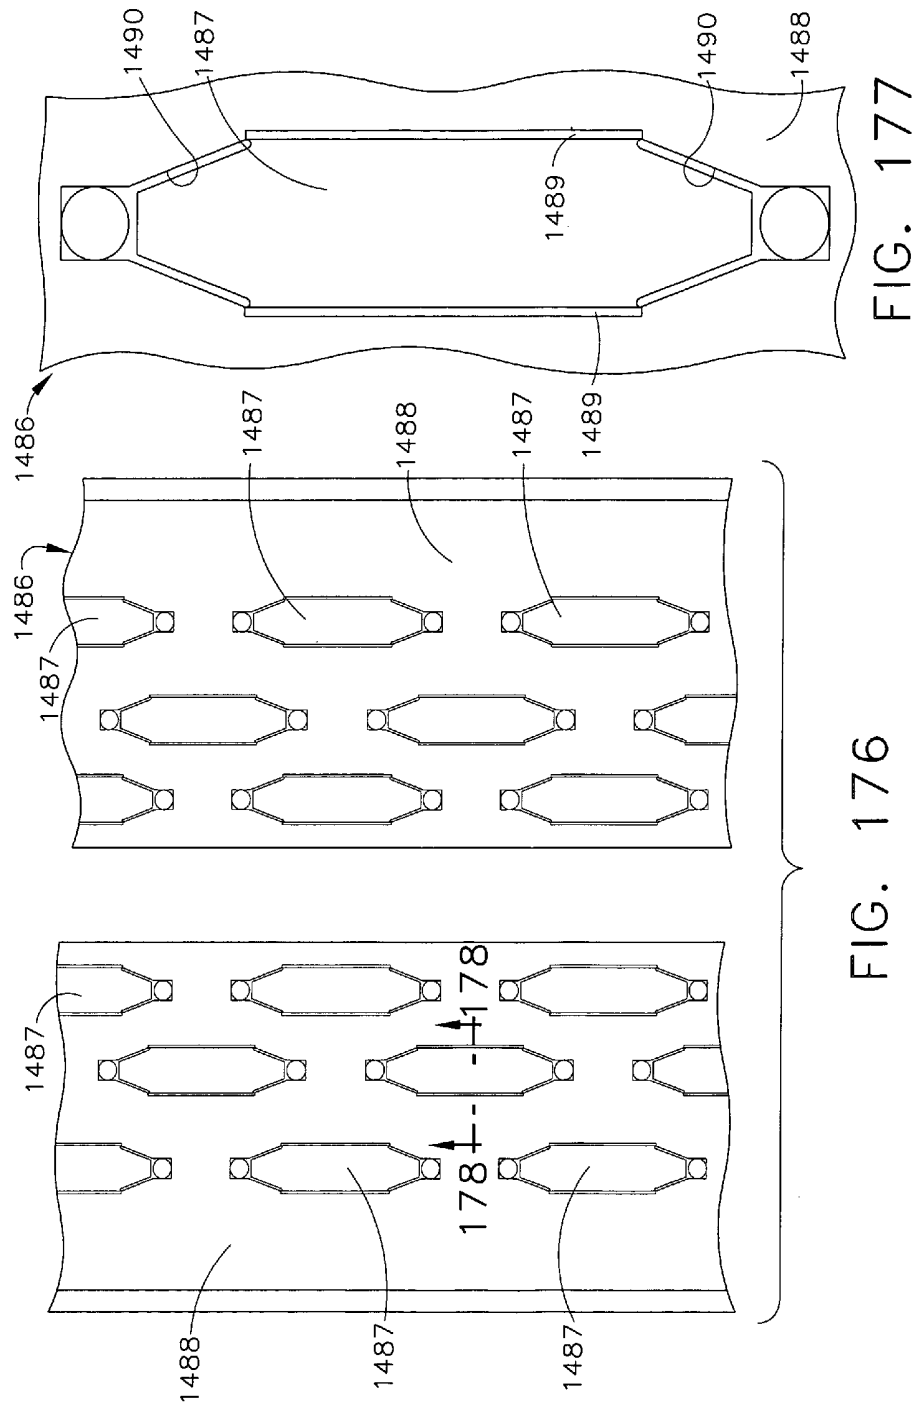


FIG. 174



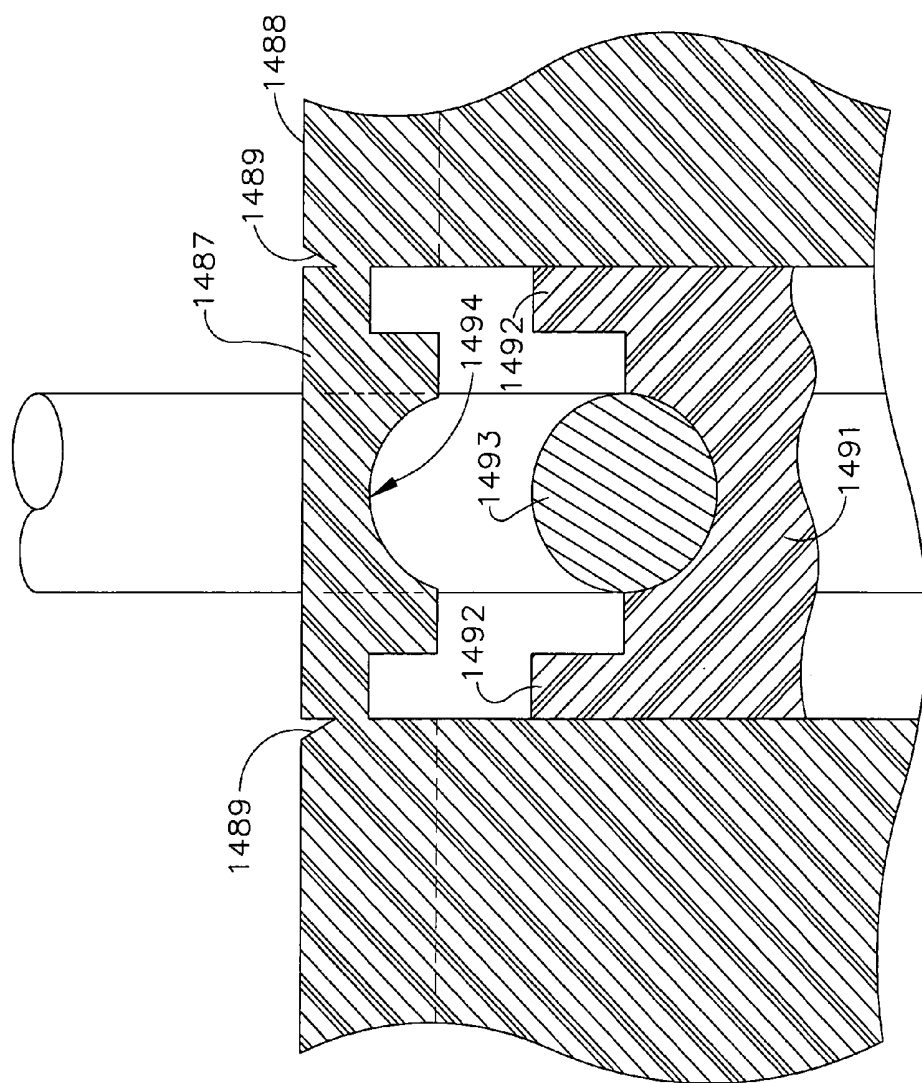


FIG. 178

**SURGICAL CUTTING AND STAPLING
DEVICE WITH CLOSURE APPARATUS FOR
LIMITING MAXIMUM TISSUE
COMPRESSION FORCE**

**CROSS REFERENCE TO RELATED
APPLICATIONS**

The subject application is related to eleven co-pending and commonly-owned applications filed on even date herewith, the disclosure of each is hereby incorporated by reference in their entirety, these eleven applications being respectively entitled:

(1) Surgical Stapling Instruments Having Flexible Channel and Anvil Features For Adjustable Staple Heights to Frederick E. Shelton, IV, Jerome R. Morgan, Michael A. Murray, Richard W. Timm, James T. Spivey, James W. Voegelé, Leslie M. Fugikawa, and Eugene L. Timperman, U.S. application Ser. No. 11/540,735;

(2) Surgical Stapling Instruments With Collapsible Features For Controlling Staple Height to Frederick E. Shelton, IV, Jeffrey S. Swayze, Leslie M. Fugikawa, and Eugene L. Timperman, U.S. application Ser. No. 11/540,734;

(3) Surgical Cutting and Stapling Instrument With Self Adjusting Anvil to Frederick E. Shelton, IV and Joshua Uth, U.S. application Ser. No. 11/541,050;

(4) Surgical Stapling Instrument With Mechanical Indicator To Show Levels of Tissue Compression to Todd Phillip Omaitis, Bennie Thompson, Frederick E. Shelton, IV, and Eugene L. Timperman, U.S. application Ser. No. 11/529,879;

(5) Surgical Stapling Instrument With Mechanical Mechanism For Limiting Maximum Tissue Compression to Todd Phillip Omaitis, Bennie Thompson, Frederick E. Shelton, IV and Eugene L. Timperman, U.S. application Ser. No. 11/541,164;

(6) Surgical Stapling Instruments and Staples to Christopher J. Hess, William B. Weisenburgh, II, Jerome R. Morgan, James W. Voegelé, Frederick E. Shelton, IV and Joshua Uth, U.S. application Ser. No. 11/529,904;

(7) Surgical Staples Having Dissolvable, Bioabsorbable or Biofragmentable Portions and Stapling Instruments For Deploying The Same to Christopher J. Hess, Michael A. Murray, Jerome R. Morgan, James W. Voegelé, Robert Gill, and Michael Clem, U.S. application Ser. No. 11/541,374;

(8) Connected Surgical Staples and Stapling Instruments For Deploying The Same to Christopher J. Hess, William B. Weisenburgh, II, Jerome R. Morgan, Frederick E. Shelton, IV, Leslie M. Fugikawa, and Eugene L. Timperman, U.S. application Ser. No. 11/541,098;

(9) Surgical Staples Having Attached Drivers and Stapling Instruments For Deploying The Same to Christopher J. Hess, Jerome R. Morgan, Michael Clem, Frederick E. Shelton, IV, and William B. Weisenburgh, II, U.S. application Ser. No. 11/529,935;

(10) Surgical Staples and Stapling Instruments to Christopher J. Hess, William B. Weisenburgh, II, Jerome R. Morgan, Frederick E. Shelton, IV, and Darrel Powell, U.S. application Ser. No. 11/541,182; and

(11) Surgical Staples Having Compressible or Crushable Members For Securing Tissue Therein and Stapling Instruments For Deploying The Same to Christopher J. Hess, Jerome R. Morgan, William B. Weisenburgh, II, James W. Voegelé, Carl Shurtleff, Mark Ortiz, Michael Stokes, Frederick E. Shelton, IV, and Jeffrey S. Swayze, U.S. application Ser. No. 11/541,123.

FIELD OF THE INVENTION

The present invention generally relates to endoscopic and open surgical instrumentation, and more particularly, to surgical staples, surgical staplers and cutters including, but not limited to, open surgical stapling devices, laparoscopic surgical stapling devices, endoscopic and intraluminal surgical stapling devices.

BACKGROUND

Endoscopic and laparoscopic surgical instruments are often preferred over traditional open surgical devices since a smaller incision tends to reduce the post-operative recovery time and complications. The use of laparoscopic and endoscopic surgical procedures has been relatively popular and has provided additional incentive to develop the procedures further. In laparoscopic procedures, surgery is performed in the interior of the abdomen through a small incision. Similarly, in endoscopic procedures, surgery is performed in any hollow viscus of the body through narrow endoscopic tubes inserted through small entrance wounds in the skin.

Laparoscopic and endoscopic procedures generally require that the surgical region be insufflated. Accordingly, any instrumentation inserted into the body must be sealed to ensure that gases do not enter or exit the body through the incision. Moreover, laparoscopic and endoscopic procedures often require the surgeon to act on organs, tissues and/or vessels far removed from the incision. Thus, instruments used in such procedures are typically long and narrow while being functionally controllable from a proximal end of the instrument.

Significant development has gone into a range of endoscopic surgical instruments that are suitable for precise placement of a distal end effector at a desired surgical site through a cannula of a trocar. These distal end effectors engage the tissue in a number of ways to achieve a diagnostic or therapeutic effect (e.g., endocutter, grasper, cutter, staplers, clip applicator, access device, drug/gene therapy delivery device, and energy device using ultrasound, RF, laser, etc.).

Known surgical staplers include an end effector that simultaneously makes a longitudinal incision in tissue and applies lines of staples on opposing sides of the incision. The end effector includes a pair of cooperating jaw members that, if the instrument is intended for endoscopic or laparoscopic applications, are capable of passing through a cannula passageway. One of the jaw members receives a staple cartridge having at least two laterally spaced rows of staples. The other jaw member defines an anvil having staple-forming pockets aligned with the rows of staples in the cartridge. The instrument includes a plurality of reciprocating wedges which, when driven distally, pass through openings in the staple cartridge and engage drivers supporting the staples to effect the firing of the staples toward the anvil.

Recently, an improved "E-beam" firing bar was described for a surgical stapling and severing instrument that advantageously included a top pin that slides within an internal slot formed in the upper jaw (anvil) and has a middle pin and bottom foot that slides on opposite sides of a lower jaw of an end effector, or more particularly a staple applying assembly. Distal to the middle pin, a contacting surface actuates a staple cartridge held within an elongate staple channel that forms the lower jaw. Between the contacting surface and the top pin, a cutting surface, or knife, severs tissue clamped between the anvil and the staple cartridge of the lower jaw. Since both jaws are thus engaged by the E-beam, the E-beam maintains a desired spacing between the jaws to ensure proper staple

formation. Thus, if a lesser amount of tissue is clamped, the E-beam holds up the anvil to ensure sufficient spacing for the staples to properly form against an undersurface of the anvil. In addition, if a greater amount of tissue is clamped, the E-beam draws down the anvil to ensure that the spacing does not exceed the length of the staple such that the ends of each staple are not sufficiently bent to achieve a desired degree of retention. Such an E-beam firing bar is described in U.S. patent application Ser. No. 10/443,617, entitled "Surgical Stapling Instrument Incorporating an E-Beam Firing Mechanism", filed on May 20, 2003, now U.S. Pat. No. 6,978,921, issued Dec. 27, 2005, the disclosure of which is hereby incorporated by reference in its entirety.

While an E-beam firing bar has many advantages for a surgical stapling and severing instrument, often it is desirable to sever and staple tissue of various thicknesses. A thin layer of tissue may result in staples that only form loosely, perhaps requiring the need for bolstering material. A thick layer of tissue may result in formed staples that exert a strong compressive force on the captured tissue, perhaps resulting in necrosis, bleeding or poor staple formation/retention. Rather than limiting the range of tissue thicknesses that are appropriate for a given surgical stapling and severing instrument, it would be desirable to accommodate a wider range of tissue thickness with the same surgical stapling and severing instrument.

Consequently, a significant need exists for an improved surgical stapling and severing instrument that incorporates a staple applying assembly (end effector) that adjusts to the amount of tissue that is clamped.

In addition, the staple drivers that are commonly employed in existing staple applying assemblies are traditionally made as stiff as possible to assure proper "B" form staple height. Because of this stiff construction, these drivers do not provide any flexibility for adjusting the formed height of the staple to a particular thickness of tissue clamped within the assembly.

Thus, another significant need exists for staple drivers that are able to facilitate the adjustment of the formed height of the staples in response to variations in tissue thickness.

In various types of endocutter arrangements, the anvil is opened and closed by axially actuating a closure tube assembly that serves to interface with closure features on the proximal end of the anvil. The anvil is commonly formed with trunnions that are received in somewhat elongated slots in the proximal end of the channel. The trunnions serve to pivotally support the staple cartridge and permit the anvil to move into axial alignment while pivoting to a closed position. Unfortunately, however, this arrangement lacks means for limiting or adjusting the amount of clamping forces applied to the anvil during the clamping process. Thus, the same amount of clamping forces generated by the closure tube assembly are applied to the anvil regardless of the thickness of the tissue to be clamped therein. Such arrangement can result in thinner tissues being over clamped which could lead to excessive bleeding and possibly damage or even destroy the tissue.

Thus, there is another need for a closure system that includes means for limiting or adjusting the amount of closure forces applied to the anvil based on the thickness of the tissue to be clamped between the anvil and the staple cartridge.

In certain types of surgical procedures the use of surgical staples has become the preferred method of joining tissue, and, specially configured surgical staplers have been developed for these applications. For example, intra-luminal or circular staplers have been developed for use in a surgical procedure known as an anastomosis. Circular staplers useful to perform an anastomosis are disclosed, for example, in U.S.

Pat. No. 5,104,025 and U.S. Pat. No. 5,309,927 which are each herein incorporated by reference.

An anastomosis is a surgical procedure wherein sections of intestine are joined together after a connecting section has been excised. The procedure requires joining the ends of two tubular sections together to form a continuous tubular pathway. Previously, this surgical procedure was a laborious and time consuming operation. The surgeon had to precisely cut and align the ends of the intestine and maintain the alignment while joining the ends with numerous suture stitches. The development of circular staplers has greatly simplified the anastomosis procedure and also decreased the time required to perform an anastomosis.

In general, a conventional circular stapler typically consists of an elongated shaft having a proximal actuating mechanism and a distal stapling mechanism mounted to the shaft. The distal stapling mechanism typically consists of a fixed stapling cartridge containing a plurality of staples configured in a concentric circular array. A round cutting knife is concentrically mounted in the cartridge interior to the staples. The knife is moveable in an axial, distal direction. Extending axially from the center of the cartridge is a trocar shaft. The trocar shaft is moveable, axially, with respect to the cartridge and elongated shaft. An anvil member is mounted to the trocar shaft. The anvil member has a conventional staple anvil mounted to it for forming the ends of the staples. The distance between the distal face of the staple cartridge and the staple anvil is controlled by an adjustment mechanism mounted to the proximal end of the stapler shaft. Tissue contained between the staple cartridge and the staple anvil is simultaneously stapled and cut when the actuating mechanism is engaged by the surgeon.

When performing an anastomosis using a circular stapler, typically, the intestine is stapled using a conventional surgical stapler with double rows of staples being emplaced on either side of a target section (i.e., specimen) of intestine. The target section is typically simultaneously cut as the section is stapled. Next, after removing the specimen, the surgeon typically inserts the anvil into the proximal end of the lumen, proximal of the staple line. This is done by inserting the anvil head into an entry port cut into the proximal lumen by the surgeon. On occasion, the anvil can be placed transanally, by placing the anvil head on the distal end of the stapler and inserting the instrument through the rectum. Typically the distal end of the stapler is inserted transanally. The surgeon then ties the proximal end of the intestine to the anvil shaft using a suture or other conventional tying device. Next, the surgeon cuts excess tissue adjacent to the tie and the surgeon attaches the anvil to the trocar shaft of the stapler. The surgeon then closes the gap between the anvil and cartridge, thereby engaging the proximal and distal ends of the intestine in the gap. The surgeon next actuates the stapler causing several rows of staples to be driven through both ends of the intestine and formed, thereby joining the ends and forming a tubular pathway. Simultaneously, as the staples are driven and formed, a concentric circular blade is driven through the intestinal tissue ends, cutting the ends adjacent to the inner row of staples. The surgeon then withdraws the stapler from the intestine and the anastomosis is complete.

During the stapling process, however, the surgeon must be careful not to over compress the material that is being stapled to avoid killing or detrimentally damaging that tissue. While some prior staplers are fitted with an indicator mechanism for providing the surgeon with some indication of the spacing between the anvil and the staple cartridge, it is desirable for the stapler to include a mechanism that provides a means for avoiding over compression of the tissue.

BRIEF SUMMARY

The invention overcomes the above-noted and other deficiencies of the prior art by providing a surgical instrument that incorporates a cartridge supporting assembly that is configured to operably support a staple cartridge therein. An anvil is operably coupled to the cartridge supporting assembly and is selectively movable between open and closed positions. A closure member interfaces with the anvil to selectively apply a closing force thereto in response to a closing motion applied to the closure member. The closure member may also be configured to apply an opening force to the anvil in response to an opening motion applied to the closure member. At least one force limiting member interacts with the closure member to limit an amount of the closing force applied to the anvil by the closure member in response to a resistive force experienced by the anvil when clamping tissue between the anvil and the staple cartridge supported in the cartridge supporting assembly.

In another aspect of the invention, a surgical instrument has a handle assembly and an elongate spine that is coupled to the handle assembly. An elongate channel is distally coupled to the elongate spine and is configured to support a staple cartridge therein. An anvil is operably coupled to the elongate channel and is selectively movable between open and closed positions. A closure tube assembly is movably received on the elongate spine and has a distal end portion that is oriented to selectively interact with the anvil to cause the anvil to move between the open and closed positions. A closure drive is operably supported within the handle assembly and movably supports a proximal end portion of the closure tube assembly therein. The closure drive is operable to selectively apply opening and closing motions to the closure tube assembly such that upon application of the closure motion to the closure tube assembly, the closure tube assembly applies a closing force to the anvil. At least one force limiting member interacts with the closure tube assembly to limit an amount of the closing force applied to the anvil by the closure tube assembly in response to a resistive force experienced by the anvil when clamping tissue between the anvil and the elongate channel.

These and other objects and advantages of the present invention shall be made apparent from the accompanying drawings and the description thereof.

BRIEF DESCRIPTION OF THE FIGURES

The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate embodiments of the invention, and, together with the general description of the invention given above, and the detailed description of the embodiments given below, serve to explain the principles of the present invention.

FIG. 1 is a left side view in elevation of a surgical stapling and severing instrument with an open end effector (staple applying assembly) with a shaft partially cut away to expose a firing member of a proximal firing rod and distal firing bar guided by a frame ground and encompassed by a closure sleeve.

FIG. 2 is a left side view of a closed end effector (staple applying assembly) with a retracted force adjusted height firing bar consistent with the present invention of the surgical stapling and severing instrument of FIG. 1 taken in longitudinal vertical cross section along lines 2-2.

FIG. 3 is a left isometric view of the force adjusted (compliant) height firing bar of FIG. 2.

FIG. 4 is a left side view of a distal portion ("E-beam") of a first version of the force adjusted height firing bar of FIG. 2

having horizontal slits formed respectively between the top pin and cutting surface and between the middle pin and the cutting surface to enhance vertical flexure.

FIG. 5 is a lower left isometric view of a distal portion ("E-beam") of a second version of the force adjusted firing bar of FIG. 2 having a relieved lower area of an upper pin to enhance vertical flexure.

FIG. 6 is a front view in elevation of an upper portion of the E-beam of FIG. 5 taken in vertical and transverse cross section through the upper pin along lines 6-6.

FIG. 7 is a front view of an upper portion of a third version of the E-beam of FIG. 5 taken in vertical and transverse cross section along lines 6-6 but further including relieved upper root attachments of the top pin for enhanced vertical flexure.

FIG. 8 is a front view of an upper portion of a fourth version of the E-beam of FIG. 5 taken in vertical and transverse cross section along lines 6-6 but including a resilient inner vertical laminate layer instead of a relieved undersurface of the top pin for enhanced vertical flexure.

FIG. 9 is a front view of an upper portion of a fifth version of the E-beam of FIG. 5 taken in vertical and transverse cross section along lines 6-6 but including an upper pin formed of a resilient material instead of a relieved undersurface of the upper pin for enhanced vertical flexure.

FIG. 10 is an upper left isometric view of a distal portion ("E-beam") of a sixth version of the force adjusted firing bar of FIG. 2 having resilient material upon a bottom foot to enhance vertical flexure.

FIG. 11 is a front view in elevation taken in vertical and transverse cross section through the padded lower foot of the end effector (staple applying assembly) of the surgical stapling and severing instrument of FIG. 1.

FIG. 12 is a left view in elevation of a distal portion ("E-beam") of a seventh version of the force adjusted firing bar of FIG. 2 having a proximally and upwardly extended spring arm attached to a lower foot to enhance vertical flexure.

FIG. 13 is a left top isometric view of a distal portion ("E-beam") of an eighth version of the force adjusted firing bar of FIG. 2 having a spring washer encompassing a lower foot to enhance vertical flexure.

FIG. 14 is a cross-sectional end view of another staple applying assembly or end effector of the present invention in a clamped or closed position.

FIG. 15 is a partial perspective view of the staple applying assembly of FIG. 14 with some of the elements thereof shown in cross-section.

FIG. 16 is a cross-sectional end view of another staple applying assembly or end effector of the present invention in a clamped or closed position.

FIG. 17 is a partial perspective view of the staple applying assembly of FIG. 16 with some of the elements thereof shown in cross-section.

FIG. 18 is a partial perspective of a staple applying assembly of the present invention clamping a piece of tissue that has been partially cut and stapled.

FIG. 19 is a bottom view of an anvil embodiment of the present invention.

FIG. 20 is a longitudinal cross-sectional view of a staple applying assembly employing the anvil embodiment depicted in FIG. 19.

FIG. 21 is a cross-sectional end view of the staple applying assembly of FIG. 20 taken along line 21-21 in FIG. 20, with some elements shown in solid form for clarity.

FIG. 22 is another longitudinal cross-sectional view of the staple applying assembly of FIGS. 20 and 21 clamping a piece of tissue therein, wherein the tissue has varying cross-sectional thicknesses.

FIG. 23 is another partial longitudinal cross-sectional view of the staple applying assembly of FIGS. 20-22 clamping another piece of tissue therein.

FIG. 24 is another partial longitudinal cross-sectional of the staple applying assembly of FIGS. 20-23 clamping another piece of tissue therein.

FIG. 25 is an end cross-sectional view of another staple applying assembly of the present invention in a clamped position.

FIG. 26 is longitudinal cross-sectional view of another staple applying assembly of the present invention.

FIG. 27 is a cross-sectional view of a portion of another staple applying assembly of the present invention with a piece of tissue clamped and stapled therein.

FIG. 28 is a top view of a portion of a biasing plate embodiment of the present invention.

FIG. 29 is a cross-sectional view of a portion of the biasing plate of FIG. 28 taken along line 29-29 in FIG. 28.

FIG. 30 is an end cross-sectional view of the staple applying assembly of FIG. 27 with some elements shown in solid form for clarity.

FIG. 30A is an end cross-sectional view of another staple applying assembly of the present invention with some elements shown in solid form for clarity.

FIG. 31 is a longitudinal cross-sectional view of the staple applying assembly of FIGS. 27 and 30 with tissue clamped and stapled therein.

FIG. 32 is another longitudinal cross-sectional view of the staple applying assembly of FIG. 31 with another portion of tissue clamped and stapled therein.

FIG. 33 is another longitudinal cross-sectional view of the staple applying assembly of FIGS. 30-32 fluidically coupled to a fluid reservoir supported by a handle assembly of various embodiments of the present invention.

FIG. 34 is a longitudinal cross-sectional view of a staple applying assembly of other embodiments of the present invention wherein tissue of varying thickness is clamped therein.

FIG. 35 is an enlarged cross-sectional view of a portion of the staple applying assembly of FIG. 34.

FIG. 36 is an exploded perspective view of a collapsible staple driver embodiment of the present invention in a first (uncollapsed) position.

FIG. 37 is a cross-sectional view of the collapsible staple driver embodiment of FIG. 36.

FIG. 38 is an exploded perspective view of another collapsible staple driver embodiment of the present invention in a first (uncollapsed) position.

FIG. 39 is a cross-sectional view of the collapsible staple driver embodiment of FIG. 38.

FIG. 40 is a perspective view of another collapsible staple driver embodiment of the present invention.

FIG. 41 is an exploded perspective view of the collapsible staple driver embodiment of FIG. 40.

FIG. 42 is a cross-sectional view of the collapsible staple driver embodiment of FIGS. 40 and 41 in a first (uncollapsed) position.

FIG. 43 is another cross-sectional view of the collapsible staple driver embodiment of FIGS. 40-42 after compression forces have been applied thereto.

FIG. 44 is an exploded perspective view of another collapsible staple driver embodiment of the present invention.

FIG. 45 is a cross-sectional view of the collapsible staple driver embodiment of FIG. 44 in a first (uncollapsed) position.

FIG. 46 is an exploded perspective view of the collapsible staple driver embodiment of FIGS. 44 and 45 with some of the elements thereof shown in cross-section.

FIG. 47 is an exploded front view of another collapsible staple driver embodiment of the present invention.

FIG. 48 is another front view of the collapsible staple driver of FIG. 47 in a first (uncollapsed) position.

FIG. 49 is another front view of the staple driver of FIGS. 47 and 48 after it has been compressed to a fully collapsed position.

FIG. 50 is an exploded assembly view of another collapsible staple driver embodiment of the present invention.

FIG. 51 is an exploded front view of the collapsible staple driver embodiment of FIG. 50.

FIG. 52 is another front view of the collapsible staple driver embodiment of FIGS. 50 and 51 after being compressed into a fully collapsed position.

FIG. 53 is a perspective view of another collapsible staple driver embodiment of the present invention.

FIG. 54 is a side elevational view of the collapsible staple driver of FIG. 53 in a first (uncollapsed) position.

FIG. 55 is another side elevational view of the collapsible staple driver of FIGS. 53 and 54 after being compressed to a fully collapsed position.

FIG. 56 is a perspective view of a surgical cutting and staple instrument of various embodiments of the present invention.

FIG. 57 is an exploded assembly view of an end effector and elongate shaft assembly of various embodiments of the present invention.

FIG. 58 is an exploded assembly view of a handle assembly and closure shuttle arrangements of various embodiments of the present invention, with the firing system components omitted for clarity.

FIG. 59 is a cross-sectional side view of the handle assembly depicted in FIG. 58 with the closure trigger thereof in a locked position.

FIG. 60 is a left side exploded assembly view of a closure shuttle and closure tube assembly of various embodiments of the present invention.

FIG. 61 is a right side exploded assembly view of a closure shuttle and closure tube assembly of various embodiments of the present invention.

FIG. 62 is a partially enlarged view of a distal end of a closure tube assembly interacting with a partially closed anvil with some of the components shown in cross-section for clarity.

FIG. 63 is another partially enlarged view of the closure tube and anvil of FIG. 62 with the anvil illustrated in a fully closed position and some elements shown in cross-section for clarity.

FIG. 64 is a partial perspective view of a closure tube assembly and anvil of various embodiments of the present invention.

FIG. 65 is a partial perspective view of another closure tube assembly and anvil of various embodiments of the present invention.

FIG. 66 is a partial perspective view of another closure tube assembly and anvil of various embodiments of the present invention with the anvil in a fully closed position.

FIG. 67 is cross-sectional end view of the closure tube and anvil arrangement of FIG. 66 with the elongate channel omitted for clarity.

FIG. 68 is a partially enlarged view of a closure tube and anvil arrangement of other various embodiments of the present invention with the anvil in a partially closed position.

FIG. 69 is another partially enlarged view of the closure tube and anvil arrangement of FIG. 68 with the anvil in a fully closed position.

FIG. 70 is a cross-sectional view of another endocutter embodiment of the present invention with the anvil thereof in an open position and some components shown in solid form for clarity.

FIG. 71 is another cross-sectional view of the endocutter embodiment of FIG. 70 with the anvil in a fully closed position and some components shown in solid form for clarity.

FIG. 72 is an enlarged cross-sectional view of a portion of the anvil and the closure tube assembly of the embodiments depicted in FIGS. 70 and 71 with the anvil in its fully closed position.

FIG. 73 is another cross-sectional view of the endocutter embodiment of FIG. 70 with the anvil in a maximum clamping position with some components shown in solid form for clarity.

FIG. 74 is an enlarged cross-sectional view of a portion of the anvil and the closure tube assembly of the embodiments depicted in FIG. 73 with the anvil in its maximum clamping position.

FIG. 75 is an enlarged cross-sectional view of a portion of the endocutter depicted in FIGS. 70-74 clamping a thin piece of tissue.

FIG. 76 is another enlarged cross-sectional view of a portion of the endocutter depicted in FIGS. 70-75 clamping a thicker piece of tissue.

FIG. 77 is a perspective view of another stapling instrument of various embodiments of the present invention.

FIG. 78 is an exploded perspective assembly view of an anvil and head arrangement that may be employed with various stapler embodiments of the type depicted in FIG. 77.

FIG. 79 is an exploded perspective assembly view of a shaft and trigger assembly that may be employed with various embodiments of the stapler depicted in FIG. 77.

FIG. 80 is a partial cross-sectional view of a shaft assembly and head assembly embodiment of the present invention with the anvil attached to the shaft assembly.

FIG. 81 is a cross-sectional view of the handle assembly and closure knob assembly of various embodiments of the present invention.

FIG. 82 is a perspective view of the shaft assembly, trigger assembly, staple driver, anvil and closure knob assembly with the handle housing, head casing and outer tubular shroud removed wherefrom.

FIG. 83 is a cross-sectional view of a knob assembly embodiment of the present invention.

FIG. 84 is a cross-sectional view of the knob assembly of FIG. 83 taken along line 84-84 in FIG. 83.

FIG. 85 is a partial cross-sectional view of a stapler embodiment of the present invention inserted into separated portions of intestine.

FIG. 86 is another cross-sectional view of the staple and intestine arrangement of FIG. 85 with the proximal and distal ends of the intestine being sutured around the anvil shaft.

FIG. 87 is another cross-sectional view of the stapler and intestine arrangement of FIGS. 85 and 86 with the anvil retracted to a fully compressed position and prior to firing the stapler.

FIG. 88 is another cross-sectional view of the stapler and intestine arrangement of FIGS. 85-87 after the staples have been fired and the knife has severed the portions of sutured intestine.

FIG. 89 is a perspective view of another stapler embodiment of the present invention.

FIG. 90 is partial cross-sectional view of a portion of the stapler of FIG. 89.

FIG. 91 is cross-sectional view of a closure actuator that may be employed with the stapler of FIGS. 89 and 90.

FIG. 92 is a cross-sectional view of the closure actuator of FIG. 91 taken along line 92-92 in FIG. 91.

FIG. 93 is a cross-sectional view of a portion of the stapler of FIGS. 89-92 inserted in a portion of an intestine with the stapler anvil retracted to a fully compressed position and prior to firing the stapler.

FIG. 94 is a graph illustrating the relationship between a compression force and resistive load generated by a variable force generator that may be used in connection with various embodiments of the present invention.

FIG. 95 is another view of the closure actuator of FIGS. 91 and 92.

FIG. 96 is a side view of a surgical staple in an undeployed shape in accordance with an embodiment of the present invention.

FIG. 97 is a side view of the staple of FIG. 96 in a first deformed shape.

FIG. 98 is a side view of the staple of FIG. 96 in a second deformed shape.

FIG. 99 is a side view of the staple of FIG. 96 in a third deformed shape.

FIG. 100 is a top view of the staple of FIG. 99.

FIG. 101 is a perspective view of the staple of FIG. 96.

FIG. 102 is a perspective view of the staple of FIG. 97.

FIG. 103 is a perspective view of the staple of FIG. 98.

FIG. 104 is a perspective view of the staple of FIG. 99.

FIG. 105 is a partial cross-sectional view of a surgical stapler, and surgical staples illustrated in various deformed shapes in accordance with an embodiment of the present invention.

FIG. 106 is a side view of a surgical staple in accordance with an alternative embodiment of the present invention.

FIG. 107 is a perspective view of the staple of FIG. 106.

FIG. 108 is a side view of a staple in accordance with an alternative embodiment of the present invention.

FIG. 109 is a top view of the staple of FIG. 108.

FIG. 110 is a side view of the staple of FIG. 108 in a deformed shape.

FIG. 111 is a side view of a staple in accordance with an alternative embodiment of the present invention.

FIG. 112 is a side view of a staple in accordance with an alternative embodiment of the present invention.

FIG. 113 is a side view of a surgical staple in accordance with an embodiment of the present invention including a crushable member.

FIG. 114 is a side view of the staple of FIG. 113 in a deformed shape.

FIG. 115 is a side view of a surgical staple in accordance with an embodiment of the present invention including a spring having a first elastic member and a second elastic member.

FIG. 116 is a top view of the staple of FIG. 115.

FIG. 117 is a side view of a surgical staple in accordance with an embodiment of the present invention including a cantilever spring.

FIG. 118 is a top view of the staple of FIG. 117.

FIG. 119 is a side view of a surgical staple in accordance with an embodiment of the present invention including a spring.

FIG. 120 is a side view of the staple of FIG. 119 in a deformed shape.

FIG. 121 is a top view of the staple of FIG. 120.

11

FIG. 122 is a perspective view of first and second deformable members of a staple in accordance with an embodiment of the present invention.

FIG. 123 is a perspective view of a dissolvable, or bioabsorbable, material overmolded onto the deformable members of FIG. 122.

FIG. 124 is a perspective view of the staple of FIG. 123 in a deformed shape.

FIG. 125 is a perspective view of the staple of FIG. 124 where a portion of the dissolvable material has been dissolved and the first and second deformable members have moved relative to one another.

FIG. 126 is a perspective view of the staple of FIG. 125 after the dissolvable material has completely dissolved.

FIG. 127 is a partial cross-sectional view of a surgical stapler having an anvil, and a staple cartridge for removably storing staples in accordance with an embodiment of the present invention.

FIG. 128 is a partial cross-sectional view of the stapler of FIG. 127 illustrating several staples in various deformed shapes.

FIG. 129 is a partial cross-sectional view of the stapler of FIG. 127 taken along line 129-129 in FIG. 127.

FIG. 129A is a detail view of a staple in FIG. 129.

FIG. 130 is a detail view of the staple of FIG. 129A in a first deformed shape.

FIG. 131 is a detail view of the staple of FIG. 129A in a second deformed shape.

FIG. 132 is a side view of a staple in accordance with an alternative embodiment of the present invention having two materials overmolded onto the deformable members.

FIG. 133 is a detail view of a staple in accordance with an alternative embodiment of the present invention.

FIG. 134 is a detail view of a staple in accordance with an alternative embodiment of the present invention.

FIG. 135 is a perspective view of staples in accordance with an embodiment of the present invention.

FIG. 136 is a top view of a staple cartridge configured to accommodate the staples of FIG. 135.

FIG. 137 is a detail view of the staple cartridge of FIG. 136.

FIG. 138 is a second detail view of the staple cartridge of FIG. 136.

FIG. 139 is a cross-sectional view of the staple cartridge of FIG. 136 having the staples of FIG. 135 therein.

FIG. 140 is a perspective view of staples and a staple cartridge of a stapler in accordance with an embodiment of the present invention.

FIG. 141 is a detail view of the staple cartridge of FIG. 140.

FIG. 142 is a perspective view of a strip of the staples of FIG. 140.

FIG. 143 is a detail view of the staples of FIG. 142.

FIG. 144 is a side cross-sectional view of the staples and staple cartridge of FIG. 140.

FIG. 145 is a perspective view of a strip of staples in accordance with an alternative embodiment of the present invention.

FIG. 146 is a detail view of the staples of FIG. 145.

FIG. 147 is a side cross-sectional view of a stapler deploying the staples of FIG. 145.

FIG. 148 is a perspective view of a strip of staples in accordance with an alternative embodiment of the present invention.

FIG. 149 is a detail view of the staples of FIG. 148.

FIG. 150 is a side cross-sectional view of a stapler deploying the staples of FIG. 149.

12

FIG. 151 is a perspective view of a strip of staples in accordance with an alternative embodiment of the present invention.

FIG. 152 is a view of the staple strip of FIG. 151 stored within a staple cartridge.

FIG. 153 is a cross-sectional view of the staple cartridge of FIG. 152 taken along line 153-153 in FIG. 152.

FIG. 154 is a cross-sectional view of the staple cartridge of FIG. 152 taken along line 154-154 in FIG. 153.

FIG. 155 is a cross-sectional perspective view of the staple cartridge of FIG. 152 with staples positioned in a first position.

FIG. 156 is a cross-sectional perspective view of the staple cartridge of FIG. 152 with the staples positioned in a second position.

FIG. 157 is an additional cross-sectional perspective view of the staple cartridge of FIG. 152.

FIG. 158 is a perspective view of staples in accordance with an embodiment of the present invention connected in a "puck" configuration.

FIG. 159 is a bottom view of a staple cartridge in accordance with an alternative embodiment of the present invention configured to receive the staples of FIG. 158.

FIG. 159A is a detail view of the staple cartridge of FIG. 159.

FIG. 160 is a perspective of the staples of FIG. 158 positioned over drivers of the staple cartridge of FIG. 159.

FIG. 161 is a perspective view of the drivers of FIG. 160.

FIG. 162 is a cross-sectional view of the staple cartridge of FIG. 159.

FIG. 163 is a second cross-sectional view of the staple cartridge of FIG. 159.

FIG. 164 is a bottom view of a staple cartridge in accordance with an alternative embodiment of the present invention.

FIG. 164A is a detail view of the staple cartridge of FIG. 164.

FIG. 165 is a perspective view of staples in accordance with an alternative embodiment of the present invention.

FIG. 166 is a second perspective view of the staples of FIG. 165.

FIG. 167 is a cross-sectional view of the staples of FIG. 165 being deployed by a stapler in accordance with an embodiment of the present invention.

FIG. 168 is a perspective view of a staple assembly in accordance with an embodiment of the present invention.

FIG. 169 is a top view of the staple assembly of FIG. 168.

FIG. 170 is a perspective view of a staple cartridge configured to receive the staple assembly of FIG. 169.

FIG. 171 is a top view of the staple cartridge of FIG. 170.

FIG. 172 is a cross-sectional view of the staples of FIG. 168 and the staple cartridge of FIG. 170.

FIG. 173 is a perspective view of a staple assembly in accordance with an alternative embodiment of the present invention.

FIG. 174 is a perspective view of a staple assembly in accordance with an alternative embodiment of the present invention for forming non-parallel staple patterns.

FIG. 175 is a top view of the staple of FIG. 174 positioned within a staple cartridge in accordance with an embodiment of the present invention.

FIG. 176 is a top view of staples and a staple cartridge in accordance with an embodiment of the present invention.

FIG. 177 is a detail view of the staple cartridge of FIG. 176.

FIG. 178 is a cross-sectional view illustrating the shearable deck of the staple cartridge of FIG. 176.

DETAILED DESCRIPTION

Turning to the Drawings, wherein like numerals denote like components throughout the several views, in FIG. 1, a surgical stapling and severing instrument 10 includes a handle portion 12 that is manipulated to position an implement portion 14 including a fastening end effector, depicted as a staple applying assembly 16, distally attached to an elongate shaft 18. The implement portion 14 is sized for insertion through a cannula of a trocar (not shown) for an endoscopic or laparoscopic surgical procedure with an upper jaw (anvil) 20 and a lower jaw 22 of the staple applying assembly 16 closed by depression of a closure trigger 24 toward a pistol grip 26 of the handle portion 12, which advances an outer closure sleeve 28 of the elongate shaft 18 to pivot shut the anvil 20.

Once inserted into an insufflated body cavity or lumen, the surgeon may rotate the implement portion 14 about its longitudinal axis by twisting a shaft rotation knob 30 that engages across a distal end of the handle 12 and a proximal end of the elongate shaft 18. Thus positioned, the closure trigger 24 may be released, opening the anvil 20 so that tissue may be grasped and positioned. Once satisfied with the tissue held in the staple applying assembly 16, the surgeon depresses the closure trigger 24 until locked against the pistol grip 26, clamping tissue inside of the staple applying assembly 16.

Then a firing trigger 32 is depressed, drawn toward the closure trigger 24 and pistol grip 26, thereby applying a firing force or motion thereto to distally advance a firing member from an unfired position. The firing member is depicted as including a proximal firing rod 34 attached to a distal firing bar 36, that is supported within a frame ground 38 that connects the handle portion 12 to the staple applying assembly 16. During the staple firing motion, the firing bar 36 engages an elongate staple channel 40 and actuates a staple cartridge 42 contained therein, both forming the lower jaw 22. The firing bar 36 also engages the closed anvil 20. After releasing the firing trigger 32 to apply a retraction force or motion to the firing bar 36, depression of a closure release button 44 unclamps the closure trigger 24 so that the closure sleeve 28 may be retracted to pivot and open the anvil 20 to release the severed and stapled tissue from the staple applying assembly 16.

It should be appreciated that spatial terms such as vertical, horizontal, right, left etc., are given herein with reference to the figures assuming that the longitudinal axis of the surgical instrument 10 is co-axial to the central axis of the elongate shaft 18, with the triggers 24, 32 extending downwardly at an acute angle from the bottom of the handle assembly 12. In actual practice, however, the surgical instrument 10 may be oriented at various angles and, as such, these spatial terms are used relative to the surgical instrument 10 itself. Further, "proximal" is used to denote a perspective of a clinician who is behind the handle assembly 12 who places the implement portion 14 distal, or away from him or herself. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

In FIG. 2, the staple applying assembly 16 is closed upon compressed tissue 46. In FIGS. 2-3, the firing bar 36 has a proximal portion 48 that is attached to a distal E-beam 50 that translates within the staple applying assembly 16. As depicted with the firing bar 36 retracted, a vertical portion 52 of the E-beam 50 resides essentially aft of the staple cartridge 42, as

after a new staple cartridge 42 has been inserted into the elongate staple channel 40. An upper pin 54 that extends laterally from an upper portion of the vertical portion 52 of the E-beam 50 initially resides within an anvil pocket 56 recessed near a proximal pivoting end of the anvil 20. As the E-beam 50 is distally advanced during the staple firing motion, the vertical portion 52 passes through a narrow longitudinal anvil slot 58 (FIGS. 1, 11) formed in a staple forming undersurface 60 of the anvil 20, a proximally open vertical slot 62 formed in cartridge 42 and an underlying longitudinal channel slot 64 formed in the elongate staple channel 40.

In FIGS. 2, 11, the narrow longitudinal anvil slot 58 (FIG. 2) communicates upwardly to a laterally widened longitudinal anvil channel 66 sized to slidably receive the upper pin 54. The longitudinal channel slot 64 communicates downwardly to a laterally widened longitudinal channel track 68 that receives a lower foot 70, which is sized to slide therein and is attached at a bottom of the vertical portion 52 of the E-beam 50. A laterally widened middle pin 72 extending from the vertical portion 52 of the E-beam 50 is positioned to slide along a top surface of a bottom tray 74 of the staple cartridge 42, which in turn rests upon the elongate staple channel 40. A longitudinal firing recess 75 formed in the staple cartridge 42 above the bottom tray 74 is sized to allow the middle pin 72 to translate through the staple cartridge 42.

A distal driving surface 76 of the vertical portion 52 of the E-beam 50 is positioned to translate through the proximally open vertical slot 62 of the staple cartridge 42 and distally drive a wedge sled 78 proximally positioned in the staple cartridge 42. The vertical portion 52 of the E-beam 50 includes a cutting surface 80 along a distal edge above the distal driving surface 76 and below the upper pin 54 that severs the clamped tissue 46 simultaneously with this stapling.

With particular reference to FIG. 11, it should be appreciated that the wedge sled 78 drives upwardly staple drivers 82 that in turn drive upwardly staples 83 out of staple apertures 84 formed in a staple body 85 of the staple cartridge 42 to form against the undersurface 60 of the anvil 20 which is in confronting relationship relative to an upper surface 43 of staple cartridge 42 (FIG. 2).

In FIGS. 2, 11, advantageously, the illustrative spacing, denoted by arrow 86 (FIG. 2), between the upper pin 54 is compliantly biased toward a compressed state wherein 0.015 inches of compressed tissue 46 is contained in the staple applying assembly 16. However, a larger amount of compressed tissue 46 up to about 0.025 inches is allowed by an inherent flexure of the E-beam 50. Excessive flexure, of perhaps up to 0.030 inches, is avoided should the length of staples be insufficient to form with the additional height. It should be appreciated that these dimensions are illustrative for a staple height of 0.036 inches. The same would be true for each category of staple, however.

In FIG. 4 a first version of a compliant E-beam 50a includes top and bottom horizontal slits 90, 92 from a distal edge of the vertical portion 52a, perhaps formed by electro drilling machine (EDM). The vertical portion 52a thus contains a vertically compliant top distally projecting arm 94 containing the upper pin 54, a knife flange 96 containing the cutting surface 80, and a lower vertical portion 98 containing the distal driving surface 76, middle pin 72 and lower foot 70. The horizontal slits 90, 92 allow a compliant vertical spacing by allowing the top distally arm 94 to pivot upwardly to adjust to increased force from compressed tissue 46 (not shown).

In FIGS. 5-6, a second version of a compliant E-beam 50b includes left and right lower relieved areas 110, 112 formed into an upper pin 54b to each side of the vertical portion 52,

15

leaving left and right lower bearing points **114**, **116** respectively. The outboard position of the bearing points **114**, **116** provides a long moment arm to exert the force to flex. It should be appreciated given the benefit of the present disclosure that the dimensions of the relieved areas **110**, **112** and the choice of materials for the compliant E-beam **50b** may be selected for a desired degree of flexure, given the staple size and other considerations.

In FIG. 7, a third version of a compliant E-beam **50c** is as described above in FIGS. 5-6 with further flexure provided by left and right upper narrow relieved areas **120**, **122** formed into opposite top root surfaces of an upper pin **54c** proximate to the vertical portion **52**.

In FIG. 8, a fourth version of a compliant E-beam **50d** is as described for FIGS. 2-3 with an added feature of a composite/laminate vertical portion **52d** that includes a central resilient vertical layer **130** sandwiched between left and right vertical layers **132**, **134** that support respectively left and right portions **136**, **138** of an upper pin **54d**. As the left and right portions **136**, **138** are flexed either up or down, the resulting bowing of the left and right vertical layers **132**, **134** are accommodated by a corresponding compression or expansion of the central resilient vertical layer **130**.

In FIG. 9, a fifth version of a compliant E-beam **50e** is as described for FIGS. 2-3 with an added feature of a discrete upper pin **54e** formed of a more flexible material that is inserted through a horizontal aperture **140** through a vertical portion **52e**. Thus, left and right outer ends **142**, **144** of the discrete upper pin **54e** flex in accordance with loading forces.

Alternatively or in addition to incorporating flexure into an upper pin **54**, in FIGS. 10-11, a sixth version of a compliant E-beam **50f** as described for FIGS. 2-3 further includes resilient pads **150** that are attached to upper surfaces **152** of the bottom foot **70**. The resilient pads **150** adjust the spacing of the upper pin **54** in accordance to the compression force experienced at the bottom foot **70**.

In FIG. 12, a seventh version of a compliant E-beam **50g** is as described above for FIGS. 2-3 with the added feature of a bottom foot (shoe) **70g** having an upwardly aft extended spring finger **160** that resiliently urges the E-beam **50g** downwardly to adjust vertical spacing in accordance with loading force.

In FIG. 13, an eighth version of a compliant E-beam **50h** is as described above in FIGS. 2-3 with the added feature of an oval spring washer **170** resting upon the bottom foot **70** encircling the vertical portion **52** and having an upwardly bowed central portion **172** that resiliently urges the E-beam **50h** downwardly to adjust vertical spacing in accordance with loading force.

For another example, a compliant E-beam consistent with aspects of the present invention may include engagement to an anvil similar to the engagement in the illustrative versions of two structures that slide against opposite sides of the elongate staple channel. Similarly, a compliant E-beam may engage a lower jaw by having a laterally widened portion that slides internally within a channel formed in a lower jaw structure.

As yet an additional example, in the illustrative version, the staple cartridge **42** is replaceable so that the other portions of the staple applying assembly **16** may be reused. It should be appreciated given the benefit of the present disclosure that applications consistent with the present invention may include a larger disposable portion, such as a distal portion of an elongate shaft and the upper and lower jaws with a staple cartridge permanently engaged as part of the lower jaw.

As yet another example, the illustrative E-beam advantageously affirmatively spaces the upper and lower jaws from

16

each other. Thus, the E-beam has inwardly engaging surfaces that pull the jaws together during firing in instances where a larger amount of compressed tissue tends to spread the jaws. Thereby the E-beam prevents malformation of staples due to exceeding their effective length. In addition, the E-beam has outwardly engaging surfaces that push the jaws apart during firing in stances where a small amount of tissue or other structure attributes of the instrument tend to pinch the jaws together that may result in staple malformation. Either or both functions may be enhanced by applications consistent with aspects of the invention wherein inherent flexure in the E-beam adjusts to force to allow a degree of closing of the jaws or of opening of the jaws.

FIG. 14 is an end cross-sectional view of a surgical instrument **10a** that has a staple applying assembly **16a** of another embodiment of the present invention wherein like reference numerals are used to designate like elements and which employs an elongate channel **40a** for supporting a staple cartridge **42** therein. In various embodiments, the channel **40a** has resilient or flexible features configured to enable the staple applying assembly **40a** to effectively accommodate different thicknesses of tissue. FIG. 15 is a partial perspective view of the staple applying assembly **16a** with some components shown in cross-section for clarity. As can be seen in FIG. 14, in this embodiment, a first longitudinally extending relief area **180** and a second longitudinally extending relief area **184** are provided in the longitudinal channel **40a**. The first longitudinally extending relief area **180** defines a first resilient or flexible channel ledge portion **182** and the second longitudinally extending relief area **184** defines a second resilient or flexible channel ledge portion **186**. The elongate channel slot **64** through which the upper end **51** of the vertical portion **52** of the firing member in the form of E-beam **50** extends is formed between the free ends **183**, **185** of the flexible ledges **182**, **186**, respectively. As can be further seen in FIG. 14, such arrangement permits the lower foot **70** of the E-beam **50** to bear upon the flexible ledge portions **182**, **186** to accommodate differences in the thickness of the tissue clamped between the anvil **20** and the lower jaw **22** as the E-beam **50** transverses therethrough. It will be understood that the thickness **188** of the ledge portions **182**, **186** may be selected to provided the desired amount of flexure to those portions of the elongate channel **40a**. Also, the choice of materials for the elongate channel **40a** may be selected for a desired degree of flexure, in view of the staple size and other considerations.

The elongate channel **40a** as described above may be used in connection with a staple applying assembly that employs a conventional anvil **20**. That is, the longitudinally extending anvil slot **58** may essentially have a "T" shape that is sized to accommodate the upper pins **54** and an upper end **51** of the vertical portion **52** of the E-beam **50**. The embodiment depicted in FIGS. 14 and 15 employs an anvil **20a** that has resilient or flexible features for further accommodating differences in tissue thicknesses clamped between the anvil **20a** and the lower jaw **22**. In particular, as can be seen in FIG. 14, a third longitudinally extending relief area **190** and a fourth longitudinally extending relief area **194** may be provided in the anvil **20a** as shown. The third longitudinally extending relief area **190** defines a first anvil ledge portion **192** and the fourth longitudinally extending relief area **194** defines a second anvil ledge portion **196** upon which the upper pins **54** of the E-beam **50** may bear. Such arrangement provides a degree of flexure to the anvil **20a** to accommodate differences in tissue thickness clamped between the anvil **20a** and the lower jaw **22**. It will be understood that the thickness **198** of the ledge portions **192**, **196** may be selected to provide the

desired amount of flexure to those portions of the anvil **20a**. Also, the choice of materials for the anvil **20a** may be selected for a desired degree of flexure, in view of the staple size and other considerations. Anvil **20a** may be used in connection with the above-described channel arrangement as shown in FIGS. **14** and **15** or it may be employed with conventional channel arrangements without departing from the spirit and scope of the present invention.

The person of ordinary skill in the art will also appreciate that the anvil **20a** and/or the channel **40a** may be successfully employed with a conventional E-beam arrangement or any of the E-beam arrangements depicted herein. The E-beams disclosed herein may be reciprocatingly driven by control arrangements housed within the handle assembly. Examples of such control arrangements are disclosed in U.S. Pat. No. 6,978,921, issued Dec. 27, 2005, which has been herein incorporated by reference. Other known firing member configurations and control arrangements for applying firing and retraction forces or motions thereto could conceivably be employed without departing from the spirit and scope of the present invention.

FIGS. **16** and **17** illustrate a staple applying assembly **16b** that employs another version of a channel **40b** and an anvil **20b** that each have resilient or flexible portions to accommodate differences in tissue thicknesses clamped between the anvil **20b** and the lower jaw **22b**. As can be seen in those Figures, a first pair **200** of upper and lower longitudinally extending relieved or undercut areas **202**, **204** are provided in the channel **40b** to define a first cantilever-type support ledge **206** and a second pair **210** of relieved or undercut areas **212**, **214** are provided in the channel **40b** to define a second cantilever-type support ledge **216**. The first pair relieved areas **202**, **204** provide a degree of flexure to the first support ledge **206** to enable it to flex as illustrated by arrow **205**. Likewise, the second pair **210** of relieved areas **212**, **214** provide a degree of flexure to the second support ledge **216** to enable it to flex as illustrated by arrow **215**. As with the above described embodiments, the thickness **208** of the support ledges **206** and **216** may be selected to provide the desired amount of flexure to those portions of the elongate channel **40b** to accommodate different thicknesses of tissue. Also, the choice of materials for the elongate channel **40b** may be selected for a desired degree of flexure, in view of the staple size and other considerations.

FIGS. **16** and **17** further illustrate an anvil **20b** that has a T-shaped slot **58b** that defines a first lateral wall portion **220** and a second lateral wall portion **222**. In various embodiments, a first longitudinally extending undercut area **224** is provided in the first lateral wall portion **220** to define a resilient or flexible first ledge **226**. Similarly, in various embodiments, a second longitudinally extending undercut area **228** is provided in the second lateral wall portion **222** to define a resilient or flexible second ledge **230**. As can be seen in FIG. **16**, the ends **227**, **231** of the first and second ledges **226**, **230**, respectively serve to define a portion **59b** of anvil set slot **58b** through which an upper end portion **51** of E-beam **50b** extends. Such arrangement permits the upper pins **54b** of the E-beam **50b** may bear upon the first resilient ledge **226** and the second resilient ledge **230** to provide a degree of flexure to the anvil **20b** to accommodate differences in tissue thickness clamped between the anvil **20b** and the lower jaw **22b**. It will be understood that the thickness **232** of the ledges **226**, **230** may be selected to provide the anvil **20b** with a desired amount of flexure to accommodate different tissue thicknesses. Also, the choice of materials for the anvil **20b** may be selected for a desired degree of flexure, in view of the staple size and other considerations. Anvil **20b** may be used in

connection with the above-described channel **40b** shown in FIGS. **16** and **17** or it may be employed with a conventional channel arrangement. The skilled artisan will also appreciate that the anvil **20a** and/or the channel **40b** may be successfully employed with a conventional E-beam arrangement or any of the B-beams described herein.

FIG. **18** illustrates the cutting and stapling of tissue **240** with any one of the various surgical cutting and stapling instrument embodiments of the present invention. A portion **242** of the tissue **240** illustrated in FIG. **18** has already been cut and stapled. After the clinician has cut and stapled the first portion **242**, the instrument would be withdrawn to enable new staple cartridge **42** to be installed. FIG. **18** illustrates the position of the implement portion **14** prior to commencing the second cutting and stapling process. As can be seen in that Figure, the portion **242** of the tissue **240** that has been stapled has a thickness **243** that is less than the thickness **245** of other portions **244** of the tissue **240**.

FIG. **19** is a view of the underside of an anvil **20c** that may be employed with a staple applying assembly **16c** of various embodiments of the present invention. The anvil **20c** includes an anvil body **21c** that supports movable staple forming pockets that define different staple zones. In the embodiment depicted in FIG. **19**, four left staple zones **252**, **254**, **256**, **258** are provided on a left side **250** of the anvil slot **58c** and four right staple zones **262**, **264**, **266**, **268** are provided on a right side **260** of the anvil slot **58c** within the anvil body **21c**. The first left staple zone **252** is defined by a first left staple forming insert member **270** that has a series of staple forming pockets **272** therein. In this embodiment, three rows **274**, **276**, **278** of staple forming pockets **272** are provided in the insert **270**. As can be seen in FIG. **19**, the central row **276** of pockets **272** are slightly longitudinally offset from the outer two rows **274**, **278** of pockets **272** and correspond to the arrangement of the corresponding staple apertures **84** in corresponding staple cartridges **42**. Those of ordinary skill in the art will appreciate that such arrangement serves to result in the application of the staples **83** in a staggered manner as illustrated in FIG. **18**.

Similarly, the second left staple zone **254** may be defined by a second left staple forming insert **280** that may have three rows **282**, **284**, **286** of staple forming pockets **272** therein. The third left staple zone **256** may be defined by a third left staple forming insert **290** that may have three rows **292**, **294**, **296** of staple forming pockets **272** therein. The fourth left staple zone **258** may be defined by a fourth left staple forming insert **300** that may have three rows **302**, **304**, **306** of staple forming pockets **272** therein. The first, second, third and fourth left staple forming inserts **270**, **280**, **290**, **300** are longitudinally aligned in a left side cavity **251** provided in the anvil **20c** on the left side **250** of the anvil slot **58**.

The first right staple zone **262** may be defined by a first right staple forming insert member **310** that has a series of staple forming pockets **272** therein. In this embodiment, three rows **312**, **314**, **316** of staple forming pockets **272** are provided in the insert **310**. As can be seen in FIG. **19**, the central row **314** of staple forming pockets **272** are slightly longitudinally offset from the outer two rows **312**, **316** and correspond to the arrangement of the corresponding staple apertures **84** in corresponding staple cartridges **42**. Such arrangement serves to result in the application of the staples **83** in a staggered manner on the right side of the tissue cut line. The second right staple zone **264** may be defined by a second right insert **320** that may have three rows **322**, **324**, **326** of staple forming pockets **272** therein. The third right staple zone **266** may be defined by a third right staple forming insert **330** that may have three rows **332**, **334**, **336** of staple forming pockets **272** therein. The fourth right staple zone **268**

may be defined by a fourth right staple forming insert **340** that may have three rows **342, 344, 346** of staple forming pockets **272** therein. The first, second, third, and fourth right staple forming inserts **310, 320, 330, 340** are longitudinally aligned in a right side cavity **261** provided in the anvil **20c** on the right side **260** of the anvil slot **58**. In various embodiments, the staple forming inserts may be fabricated from stainless steel or other suitable materials that are harder than the material from which the staples are fabricated. For example, the inserts may be successfully fabricated from other materials such as cobalt chromium, aluminum, 17-4 stainless steel, 300 series stainless steel, 400 series stainless steel, other precipitant hardened stainless steels, etc.

At least one biasing member or compliant member in the form of a wave spring **350** or other suitable biasing or compliant medium or member corresponding to each of the staple forming inserts **270, 280, 290, 300, 310, 320, 330, 340** is provided between the respective left staple forming inserts **270, 280, 290, 300** and the bottom of the left side cavity **251** as shown in FIGS. **20-23**. Wave springs **350** or other suitable biasing or compliant medium or member is also provided between each of the right staple forming inserts **310, 320, 330, 340** and the bottom surface of the right side cavity **261**. The wave springs **350** on the left side of the anvil slot **58c** may be received in a corresponding spring cavity **253** and the wave springs **350** on the right side of the anvil cavity **58c** may be received in a corresponding spring cavity **263**. To biasingly retain each insert **270, 280, 290, 300, 310, 320, 330, 340** in the anvil **20c**, each insert **270, 280, 290, 300, 310, 320, 330, 340** may be attached to its corresponding spring **350** or biasing member by, for example, adhesive or other fastener arrangements. In addition, each spring **350** may be attached to the anvil **20c** by, for example, adhesive or other mechanical fastener arrangements to retain a portion of the wave spring **350** within its respective spring cavity **253** or **263**. Such spring/biasing member arrangements serve to bias the inserts **270, 280, 290, 300, 310, 320, 330, 340** toward the tissue **240** and staples and essentially act as resilient "shock absorbers" to accommodate differences in tissue thicknesses. This advantage is illustrated in FIGS. **22-24**.

In particular, as can be seen in FIG. **22**, the portion **242** of the tissue **240** clamped in the proximal end **17b** of the staple applying assembly **16c** has a first thickness (arrow **243**) that is thicker than the thickness (arrow **245**) of the portion **244** of tissue **240** clamped in the central portion **17c** of the staple applying assembly **16c**. The thickness **245** of tissue portion **244** is greater than the thickness (arrow **247**) of the portion **246** of tissue **240** that is clamped in the distal end **17a** of the staple applying assembly **16c**. Thus, the staples **83** formed in the distal portion **17a** of the staple applying assembly **16c** are more tightly formed than the staples **83** formed in the central portion **17c** of the staple applying assembly **16c** which are more tightly formed than those staples **83** formed in the proximal end **17b** of the staple applying assembly **16c** due to the differences in tissue thicknesses. FIG. **23** further illustrates the variations in staple formation heights based upon the variations in the thicknesses of the tissue clamped within the staple applying assembly **16c**. FIG. **24** illustrates a condition wherein the tissue **240** clamped in the central portion **17c** of the staple applying assembly **16c** is thicker than the portions of tissue clamped in the distal and proximal ends of the staple applying assembly **16c**. Thus, the formation heights of the staples in the central portion **17c** will be higher than the staple formation heights of the staples associated with the proximal end **17b** and distal end **17a** of the staple applying assembly **16c**.

Those of ordinary skill in the art will understand that the unique and novel features of the embodiments depicted in FIGS. **19-24** may also be employed in connection with a staple applying assembly that is essentially identical in construction and operation to staple applying assembly **16c** described above, except that the staple forming inserts **270, 280, 290, 300, 310, 320, 330, 340** may have just one row of staple formation pockets **272** therein or two rows of staple formation pockets **272** therein. For example, FIG. **25** illustrates an embodiment that only applies two rows of staples on each side of the tissue cut line. Shown in that Figure are staple forming inserts **270d** and **310d** that only have two rows of staple forming pockets **272d** each.

The skilled artisan will further understand that the number of staple forming inserts employed on each side of the anvil slot **58** may vary. For example a single longitudinally extending insert may be used on each side of the anvil slot **58**. FIG. **26** illustrates another staple applying assembly **16e** of the present invention that only employs one staple forming insert on each side of the anvil slot. FIG. **26** depicts a cross-sectional view of the left side of an anvil **20e** that supports a single left staple forming insert **380** that is attached to a single wave spring **350e**. Other biasing members or multiple wave springs or biasing members may also be employed. The biasing member or members **350e** are supported in the left side cavity **251e** and attached to the anvil **20e** in one of the various manners described above. A similar right side insert (not shown) would be employed on the right side of the anvil slot **58**. Furthermore, although FIGS. **19-24** depict use of four staple forming inserts on each side of the anvil slot greater numbers of staple forming inserts may be employed.

FIGS. **27-29** illustrate another staple applying assembly **16f** of the present invention wherein a separate movable staple forming insert is provided for each staple **83**. In particular, as can be seen in FIG. **27**, a single staple forming insert **400** is provided for each staple **83**. Each staple forming insert **400** may have staple forming pockets **404** formed on its underside **402** thereof for forming the ends of the corresponding staple **83**. As with various embodiments described above, each insert **400** has a biasing member **412** associated therewith. In the example depicted in FIGS. **27-29**, the biasing members **412** comprise stamped portions of a biasing plate **410**. The biasing plate **410** may comprise a piece of metal or other suitable material wherein each biasing member **412** is stamped or otherwise cut and formed to correspond with a staple forming insert **400**. The biasing plate **410** may comprise a single plate that is supported within a cavity **251f** in the anvil **20f** or multiple plates **410** may be employed on each side of the anvil slot. It will be understood that a similar arrangement may be employed on the right side of the anvil slot. Each staple forming insert **400** may be attached to its corresponding biasing member **412** by adhesive or other suitable fastener arrangement. Thus, it will be appreciated that a variety of different numbers and arrangements of movable staple forming inserts may be employed without departing from the spirit and scope of the present invention. In particular, at least one movable staple forming insert may be employed on each side of the anvil slot.

FIGS. **30-32** illustrate another staple applying assembly **16g** of other embodiments of the present invention wherein the biasing or compliant medium between the staple forming inserts and the anvil comprises at least one fluid bladder. More specifically, as can be seen in FIG. **30**, a left bladder **420** is positioned within a left side cavity **253g** on the left side of the anvil slot **58g** in the anvil **20g**. Likewise, a right side bladder **430** is positioned with a right side cavity **263** in the anvil **20g**. The series of left side staple forming inserts **270g, 280g,**

290g, 300g may be attached to the left side bladder 430 by a suitable adhesive or other fastener arrangement. Likewise the right side staple forming inserts (not shown) may be attached to the right side bladder 430 by adhesive or other suitable fastener arrangements. In one embodiment, each bladder 420, 430 is sealed and partially filled with a liquid 432 such as, for example, glycerin oil or saline solution. Those of ordinary skill in the art will appreciate that such arrangement will permit the staple forming inserts to move to better accommodate variations in the thickness of the tissue clamped within the staple applying assembly 16g. For example, for tissues that have a relatively constant thickness, the liquid 432 will be relatively evenly distributed within each of the bladders 420, 430 to provide a relatively even support arrangement for the staple forming inserts. See FIG. 31. However, when a thicker portion of tissue is encountered, those staple forming inserts corresponding to the thicker tissue will be compressed into their respective anvil cavity thereby forcing the liquid in that part of the bladder to the portions of the bladder corresponding to the thinner tissue portions. See FIG. 32.

In some applications, it may be desirable for the clinician to be able to control the amount of pressure within the bladders 420, 430. For example, less pressure may be desirable when cutting and stapling more delicate tissues such as lung tissue and the like. More pressure may be desirable when cutting and stapling thicker tissues such as, for example, stomach tissue, intestine tissue, kidney tissue, etc. To provide the clinician with this additional flexibility, the bladders 420, 430 may each be fluidically coupled by a supply line 440 or conduit to a fluid reservoir 450 supported by the handle portion 12 of the instrument. In the embodiment illustrated in FIG. 33, the clinician can increase or decrease the amount of fluid within the bladders 420, 430 and resulting pressure therein by means of an adjustment mechanism 460 mounted to the fluid reservoir 450. In various embodiments, the adjustment mechanism 460 may comprise a piston 462 that is attached to an adjustment screw 464. By adjusting the adjustment screw 464 inward, the piston 462 forces fluid out of the reservoir 450 to the bladders 420, 430. Conversely, by reversing the adjustment screw 464, the piston 462 permits more fluid 432 to return or remain within the reservoir 450. To assist the clinician in determining the amount of pressure within that hydraulic system, generally designated as 405, a pressure gauge 470 may be employed as shown. Thus, for those tissues requiring a higher amount of pressure, the clinician can preset the pressure in the bladders 420, 430 to a pressure that is conducive to successfully clamp and staple that particular type of tissue. While a piston/screw arrangement has been described for controlling the pressure in the hydraulic system, the skilled artisan will understand that other control mechanisms could successfully be employed without departing from the spirit and scope of the present invention.

FIG. 30A illustrates another staple applying assembly 16h of other embodiments of the present invention wherein the biasing or compliant medium between the staple forming inserts and the anvil comprises at least one compressible polymer member. More specifically, as can be seen in FIG. 30A, a left compressible polymer member 420h is positioned within a left side cavity 253h on the left side of the anvil slot 58h in the anvil 20h. Likewise, a right side compressible polymer member 430h is positioned with a right side cavity 263h in the anvil 20h. The series of left side staple forming inserts 270h-300h may be attached to the left compressible polymer member 420h by a suitable adhesive or other fastener arrangement. Likewise the right side staple forming

inserts 310h-340h may be attached to the right side compressible polymer member 430h by adhesive or other suitable fastener arrangements.

FIGS. 34-37 depict a unique and novel collapsible or compressible staple driver arrangement that enables the various staple drivers to accommodate different tissue thicknesses by collapsing or compressing in response to compression forces that the driver encounters during the firing process. As used herein, the term "firing process" refers to the process of driving the staple drivers towards the staple forming undersurface of the anvil. As was mentioned above, prior staple drivers were fabricated from stiff/rigid material designed to resist deflection and deformation when encountering compression forces during the firing process. A variety of such driver configurations are known. For example, some staple drivers are configured to support a single staple and others are designed to support multiple staples. A discussion of single and double staple drivers and how they may be operably supported and fired within a staple cartridge is found in U.S. patent application Ser. No. 11/216,562, filed Sep. 9, 2005, entitled Staple Cartridges For Forming Staples Having Differing Formed Staple Heights to Frederick E. Shelton, IV, the disclosure of which is herein incorporated by reference.

FIG. 34 depicts a staple applying assembly 16h that includes an elongate channel 40h that has an anvil 20h pivotally coupled thereto in a known manner. The elongate channel 40h is configured to operably support a staple cartridge 42h therein. The anvil 20h has a staple forming undersurface 60h thereon that is adapted to confront the upper surface 43h of the staple cartridge 42h when the anvil 20h is pivoted to the closed position shown in FIG. 34. The staples 83 are each supported on a corresponding staple driver 500, the construction of which will be discussed in further detail below.

Each staple driver 500 may be movably supported within a corresponding staple channel 87h provided in the cartridge body 85h as shown in FIGS. 34 and 35. Also operably supported within the cartridge body 85h is a driving member or wedge sled 78 that is oriented for engagement by the E-beam firing member 50 during the firing process. See FIG. 34. As the E-beam firing member 50 and wedge sled 78 are driven distally through the elongate channel 40h and staple cartridge 42 in a known manner, the wedge sled 78 drives the staple drivers 500 upwardly within the cartridge body 85h. As the staple drivers 500 are driven upwardly toward the staple forming undersurface 60h of the anvil 20h, they carry with them their respective staple 83 or staples which are driven into forming engagement with the corresponding staple forming pockets 61h in the staple forming undersurface 60h of the anvil 20h. As the ends 88 of the staple 83 contact the forming pockets 61h, they are bent over thus providing the staple 83 with a shape that somewhat resembles a "B". While the various embodiments of the present invention have been described herein in connection with E-beam firing members, it is conceivable that these various embodiments may also be successfully employed with a variety of different firing member and driving member arrangements without departing from the spirit and scope of the present invention.

One collapsible staple driver embodiment of the present invention is depicted in FIGS. 36 and 37. As can be seen in those Figures, the collapsible or compressible staple driver 500 includes a base portion 502 and a staple supporting portion 520 that is movable from a first uncollapsed position relative to the base portion 502 in response to compression forces generated during the firing process. In various embodiments, the base portion 502 may have a forward support column segment 504 and a rearward support column segment 508 that is spaced from the forward support column segment

504 and is substantially integrally formed therewith. The base portion 502 may also have an upstanding side portion 510 that has a rib 512 protruding from a backside thereof. The upstanding side portion 510 serves to define a receiving ledge 514 in the base portion 502 for receiving the staple supporting portion 520 thereon. Those of ordinary skill in the art will understand that when the staple supporting portion 520 is received on the ledge 514, the staple driver 500 is unable to collapse or compress any further.

The staple supporting portion 520 of the staple driver 500 may similarly include a forward support column segment 522 and rearward support column segment 524 that is spaced from the forward support column segment 522. When the staple supporting portion 520 is received on the base portion 502, the forward support column segments 504, 522 serve to form a forward column portion 530 and the rearward column segments 508, 524 form a rearward column portion 532. A forward staple receiving groove 526 is formed in the forward support column segment 522 and a rearward staple receiving groove 528 is formed in the rearward support column segment 524. The forward staple receiving groove 526 and the rearward staple receiving groove 528 serve to support a staple 83 therein as illustrated in FIG. 35. The rib 512 and the forward column 530 and rearward column 532 may cooperate with corresponding channels (not shown) in the staple cartridge body 85 to provide lateral support to the staple driver 500 while permitting the driver to be driven upward within the cartridge body 85 during the firing process.

In various embodiments, a resistive attachment structure, generally designated as 540' is provided to support the staple supporting portion 520 in a first uncompressed or uncollapsed orientation relative to the base portion (FIG. 37) prior to encountering any compressive forces during the firing operation and to permit the staple supporting portion 520 and the base portion to move towards each other (collapse or compress) in response to the magnitude of the compression forces applied to the staple supporting portion 520 and base portion 520 during the staple firing operation. As can be seen in FIGS. 36 and 37, the resistive attachment structure 540' in various embodiments may comprise a pair of attachment rods 540 that protrude from the bottom 521 of the staple supporting portion 520 and correspond to holes or apertures 542 in the base portion 502. The rods 540 are sized and shaped relative to the holes 542 to establish an interference fit or "light press fit" (i.e., an interference of approximately 0.001 inches) therebetween such that when the staple supporting portion 520 and base driver portion 502 are compressed together during the staple firing operation as will be discussed in further detail below, the staple supporting portion 520 and the base portion 502 can compress toward each other to reduce the overall height of the staple driver 500 in relation to the amount of compression force encountered during the firing process. In various embodiments, for example, the staple supporting portion 520 and base portion 520 may be fabricated from the same material such as, for example, plastic material such as ULTEM®. In other embodiments, the base portion 502 and the staple supporting portion 520 may be fabricated from different materials. For example, staple supporting portion 520 may be fabricated from ULTEM® and base portion 502 may be fabricated from glass or mineral filled ULTEM®. However, other materials could also be employed. For example, the base portion 502 could be fabricated from Nylon 6/6 or Nylon 6/12.

In various embodiments, a frictional or an interference fit of approximately 0.001 inch may be established between the attachment rods 540 and their corresponding holes 542. However, other degrees of interference fit may be employed to

attain the desired amount and rate of driver compression in proportion to the magnitude of compression forces encountered when stapling a particular type/thickness of tissue. For example, in one embodiment, the degree of interference fit between the attachment rods 540 and their respective holes 542 may be approximately 0.002 to 0.005 inches for stapling tissues wherein it is anticipated that compression forces on the order of 2-5 pounds may be generated during the firing operation.

FIG. 35 illustrates various ranges of travel and compression that the staple drivers 500 may experience when encountering tissues of varying thicknesses. More specifically, FIG. 35 illustrates a portion of tissue 560 clamped between the upper surface 43h of the staple cartridge 42h and the staple forming undersurface 60h of the anvil 20h. As illustrated in FIG. 35, the tissue 560 has three thicknesses. The thickest portion of tissue is designated as 562 and comprises the portion of tissue that is on the right side of the Figure. The next thickness portion of tissue is designated as 564 and the thinnest portion of tissue 560 is designated as 566 and is on the left side of the Figure. For the purposes of this explanation, the staple driver associated with tissue portion 562 is designated as staple driver 500a. The staple driver associated with tissue portion 564 is designated as staple driver 500b and the staple driver associated with tissue portion 566 is designated as 500c. It will be understood that staple drivers 500a, 500b, 500c, may be identical in construction to staple driver 500 as described above.

Turning to staple driver 500a first, as the staple driver 500a is driven upwardly towards the staple forming undersurface 60h of the anvil 20h by the wedge sled (not shown in FIG. 35), it encounters the thick tissue portion 562 which resists the upward movement of the staple driver 500a. Such resistive force (represented by arrow 570) opposes the drive force (represented by arrow 572) generated by the wedge sled and serves to overcome the amount of interference established between the attachment rods 540 and their respective holes 542 and forces the rods 540 deeper into their respective holes 542 to thereby permit the staple supporting portion 520a of the staple driver 500a and base portion 502a to move toward each other. This movement of the staple supporting portion 520a and base portion 502a towards each other under a compressive force generated during the staple firing operation is referred to herein as "collapsing" or "compressing". When in the completely compressed position wherein the staple supporting portion 520a is received on the ledge 514a of the base portion 502a, the staple supporting ledges 526a, 528a on the staple supporting portion 520a may preferably support the bottom cross member 89 of the staple 83 above the upper surface 43h of the staple cartridge 42h to avoid catching the staple 83 on the staple cartridge 42h when the staple applying assembly 16h is withdrawn. The compressed height of the staple driver 500a is designated by arrow 574 in FIG. 35.

Turning next to staple driver 500b which corresponds to tissue portion 564, because the tissue portion 564 is not as thick as tissue portion 562, the resistive force 570b encountered by the staple driver 500b during the firing operation is not as great as resistive force 570. Therefore, the attachment pins 540b of staple driver 500b are not advanced into their respective holes 542b as far as the pins 540 of staple driver 500a were advanced into their respective holes 542. Thus, the compressed height 576 of staple driver 500b is greater than the compressed height 574 of staple driver 500a. As can also be seen in FIG. 35, the bottom portion 89 of the staple 83 supported in staple driver 500b is supported above the upper surface 43h of the staple cartridge 42h.

Staple driver 500c is associated with the thinnest tissue portion 566. Thus, the resistive force 570c encountered by the staple driver 500c during the staple firing operation is less than the resistive force 570b that was encountered by staple driver 500b. Thus, the pins 540c of staple driver 500c are not advanced into their respective holes 542c as far as the pins 540b of staple driver 500b were advanced into their respective holes 542b. Thus, the compressed height 578 of staple driver 500c is greater than the compressed height 576 of staple driver 500b.

As can be further seen in FIG. 35, because the compressed height 578 of staple driver 500c is greater than the compressed height 576 of staple driver 500b, the staple 83c supported by staple driver 500c was compressed to a greater extent than the staple 83b that was supported by staple driver 500b. Thus, the formed height of staple 83c is less than the formed height of staple 83b which is less than the formed height of staple 83a as illustrated in FIG. 35.

Those of ordinary skill in the art will appreciate that the number, shape, composition and size of the attachment rods and their respective holes can vary from embodiment to embodiment without departing from the spirit and scope of the present invention. Such interrelationship between the attachment rods and their respective holes serves to establish an amount of frictional interference therebetween which can be overcome in relation to various compression forces encountered when clamping/stapling different thicknesses of tissue. In an alternative version, the attachment to rods 540 may be formed on the base portion 502 and the holes provided in the staple supporting portion 520.

FIGS. 38 and 39 illustrate another staple driver 500d embodiment of the present invention that may be substantially identical in construction and operation to the staple drivers 500 described above, except that the attachment rods 540d are somewhat tapered or frusto-conically shaped. In various embodiments, for example, the ends 541d of the attachment rods 540d may be sized relative to holes 542 such that a light press fit is established therebetween when in the first uncollapsed state depicted in FIG. 39. The degree of taper of the attachment rods 540d may be tailored to attain the desired amount of staple driver compression in relation to the magnitude of compression forces encountered during the staple firing process. Thus, in these embodiments, the magnitude of the interference fit between the attachment rods 540d and the holes 542 increases as the staple driver 500d encounters greater compression forces which drive the attachment rods 540d deeper into their respective holes 542d. In alternative embodiments, the attachment rods 540 may have a round shape and the holes 542 may be tapered to attain the desired amount and rate of staple driver compression in proportion to the amount of anticipated compression forces applied thereto during the firing operation. In an alternative version, the attachment rods 540d may be formed on the base portion 502 and the holes 542 may be formed in the staple supporting portion 520.

FIGS. 40-43 illustrate another staple driver 500e embodiment of the present invention that may be substantially identical in construction and operation to the staple drivers 500 described above, except that the attachment rods 540e are configured or shaped to include an additional amount of material oriented to be sheared off of the remaining portion of the rods as the staple driver 500e encounters compression forces during the firing operation. More specifically and with reference to FIG. 42, the attachment rods 540e have a tip portion 541e that is received within the corresponding hole 542e. The tip portion 541e may be sized relative to the hole 542e such that a sliding fit is achieved therebetween or, in

other embodiments, a small interference fit may be established between those components when in the first uncollapsed position. The remaining portion 543e of each attachment rod 540e may be provided or formed with an additional amount of material 545e that is designed to be sheared therefrom as the staple driver 500e encounters the anticipated compression forces during the firing operation. See FIG. 43. The additional material 545e may extend completely around the circumference of the portion 543e of each attachment rod 540e or the material 543e may comprise one or more segments oriented around the circumference of the attachment rod 540e. For example, in the embodiment depicted in FIGS. 40-43, two segments 547e of material 543e are diametrically opposed on each attachment rod 540e as shown. In various embodiments, the diametric distance between the segments may be somewhat larger than the diameter of the holes 542e to cause the segments 547e to be sheared or removed from at least a portion of the rods 540e as the staple driver 500e encounters the anticipated compression forces during the firing operation.

The portions of additional material 543e may comprise an integral portion of the attachment rod 540e or the additional material 543e may comprise a second material applied to the attachment rod 540e and designed to shear off therefrom when the staple driver 500e encounters the anticipated compression forces. In various embodiments, the base portion 502 may be fabricated from a material that is more rigid than the material from which attachment rods 540e and/or the additional material 543e are fabricated such that the base portion 502 facilitates the shearing off of additional material 543e as the staple support portion 520e and base portion 502e are compressed together during the staple firing operation. In an alternative version, the attachment rods 540e may be formed on the base portion 502 and the holes 542e can be provided in the staple supporting portion 520e.

FIGS. 44-46 illustrate another staple driver 500f of the present invention that may be substantially identical in construction and operation to the staple drivers 500 described above, except that the holes 542f in the base portion 502f may be hexagonally shaped or may have one or more surfaces therein designed to establish an interference fit with the attached rods 540 or to otherwise resist further entry of the attachment rods 540 into the holes 542f. For example, the holes 542f shown have a pair of flat surfaces 551f formed therein that serve to establish an interference fit or a degree of frictional resistance between the attachment rods 540f and the holes 542f which can be overcome by the various compression forces encountered when clamping/stapling different thicknesses of tissue. In the embodiment depicted in FIGS. 44-46, the attachment rods 540 have a substantially circular cross-sectional shape and the holes 542f have flat surfaces 551 formed therein. In alternative embodiments, however, the holes 542 may be round and the flat surfaces may be formed on the attachment rods 540. In an alternative version, the attachment rods 540 may be provided on the base portion 502f and the holes 542f can be provided in the staple supporting portion 520.

FIGS. 47-49 illustrate another staple driver 500g of the present invention that comprises a base portion 502g and a staple supporting portion 520g. The staple supporting portion 520g has staple supporting grooves (not shown) formed therein and a downwardly protruding tang 580 protruding from its undersurface 521g. The tang 580 has two tapered surfaces 582 and is shaped to be received in a corresponding cavity 590 formed in the base portion 502g. The cavity 590 is formed with tapered sides 592 and is sized to receive the tang 580 therein in the following manner. As the driver staple 500g

encounters the compression forces generated during the firing operation, the tang 580 is forced into the cavity 590. FIG. 49 illustrates the staple driver 500g in a fully collapsed or compressed position. The staple supporting portion 520g and/or tang 580 may be fabricated from a material that is somewhat more compliant than the material from which the base portion 502g is formed so that the tang 580 can be forced into the cavity 590 in the base portion 502g without substantially distorting the base portion 502g to the extent that it would hamper the ability of the staple driver 500g to be fully driven to a final firing position. For example, the staple supporting portion and/or the tang 580 may be fabricated from ULTEM® and the base portion 502g may be fabricated from glass filled Nylon to achieve the desired amount of driver compression when encountering the anticipated compression forces during the firing operation. In an alternative version, the tang 580 may be provided on the base portion 502g and the hole 590 can be provided in the staple supporting portion 520g.

FIGS. 50-52 illustrate another staple driver 500h embodiment of the present invention that may be substantially identical in construction and operation to the staple drivers 500 described above, except that, instead of attachment rods, the staple supporting portion 520h has two tapered tangs 600 protruding therefrom designed to be compressed into a V-shaped cavity 610 formed in the base portion 502h. Prior to commencement of the firing operation, the staple supporting portion 520h is supported on the base portion 502h within the staple cartridge. As the staple supporting portion 520h and the base portion 502h are compressed together during the firing operation, the tapered tangs 600 are forced inwardly as shown in FIG. 52. The degree to which the tangs 600 are compressed into the V-shaped cavity 610 is dependent upon the magnitude of the compression forces encountered during the firing operation.

The staple supporting portion 500h and/or tangs 600 may be fabricated from a material that is somewhat more compliant than the material from which the base portion 502h is formed so that the tangs 600 can be forced into the V-shaped cavity 610 in the base portion 502h without substantially distorting the base portion 502h to the extent that it would hamper the ability of the staple driver 500h to be fully driven to a final firing position. For example, the staple supporting portion and/or the tangs 600 may be fabricated from Nylon with no fill and the base portion 502h may be fabricated from ULTEM® with a glass or mineral fill to achieve the desired amount of staple driver compression when encountering the anticipated compression forces during the firing operation. In an alternative version, the tangs 600 may be provided on the base portion 502h and the cavity 610 may be provided in the staple supporting portion 520h.

FIGS. 53-55 illustrate yet another staple driver 500i embodiment of the present invention that includes a staple supporting portion 520i that has V-shaped staple supporting grooves 630i, 650i therein. In this embodiment, the staple supporting portion 520i has a first pair 620i of two tapered tangs 622i, 626i protruding therefrom oriented to be compressed into the first V-shaped groove or cavity 630i and a second pair 640i of two tapered tangs 642i, 646i oriented to be compressed into the second V-shaped groove or cavity 650i. More specifically and with reference to FIG. 54, the first tang 622i has an end 624i that is spaced from an end 628i of the second tang 626i prior to commencement of the staple firing operation. When in the position illustrated in FIG. 54, the ends 624i, 628i are biased outwardly into frictional contact with the upper side walls of the first V-shaped groove 630i to retain the staple supporting portion 520i in the uncollapsed position shown in FIG. 54. Although not shown, the second

pair 640i of tangs 642i, 646i are also similarly configured as tangs 622i, 626i and serve to engage the second V-shaped groove 650i in the same manner.

As the staple supporting portion 520i and the base portion 502i are compressed together during the firing operation, the ends 624i, 628i of the first tangs 622i, 626i and the ends of the second tangs 642i, 646i are biased toward each other to permit the tangs to be driven deeper into their respective grooves 630i, 650i. FIG. 55 illustrates the first pair 620i of tangs 622i, 626i in their fully compressed state which also corresponds to the fully compressed state of the driver 500i. The degree to which the tangs are compressed into their respective V-shaped grooves is dependent upon the magnitude of the compression forces encountered during the firing operation.

The staple supporting portion 500i and/or tangs 622i, 626i, 642i, 646i may be fabricated from a material that is somewhat more compliant than the material from which the base portion 502i is formed so that the tangs 622i, 626i, 642i, 646i can be forced into their respective V-shaped grooves in the base portion 502i without substantially distorting the base portion 502i to the extent that it would hamper the ability of the driver 500i to be fully driven to a final firing position. For example, the staple supporting portion 520i and/or the tangs 622i, 626i, 642i, 646i may be fabricated from ULTEM® and the base portion 502i may be fabricated from Nylon with a glass or mineral fill to achieve the desired amount of driver compression when encountering the anticipated compression forces during the firing operation. In an alternative version, the tangs 622i, 626i, 642i, 646i may be provided on the base portion 502i and the V-shaped grooves 630i, 650i may be provided in the staple supporting portion 520i.

The various embodiments of the present invention described above and their respective equivalent structures represent vast improvements over prior staple applying assemblies and end effectors. Various embodiments of the present invention provide anvils and/or channels with flexible portions that permit the overall staple height to increase as the compression within the assembly increases due to tissue thickness. Other embodiments employ anvil arrangements that have flexible forming pockets that can be compressed away from the staple cartridge in response to variations in tissue thickness. In doing so, the inherent gap between the forming pocket and the cartridge increases which serves to increase the formed height of the staple. Such advantages can result in improved staple line consistency and provide better clinical outcomes.

FIGS. 56-63 illustrate another surgical stapling and severing instrument 1000 of the present invention. As can be seen in FIG. 56, the instrument 1000 includes a handle assembly 1020 that is manipulated to position an implement portion 1014 including a fastening end effector, depicted as a staple applying assembly 1016, distally attached to an elongate shaft assembly 1100. The implement portion 1014 is sized for insertion through a cannula of a trocar (not shown) for an endoscopic or laparoscopic surgical procedure with an upper jaw (anvil) 1050 and a lower jaw 1018 of the staple applying assembly 1016 closed by depression of a closure trigger 1040 toward a pistol grip 1034 of the handle assembly 1020, which advances an outer closure tube assembly 1130 of the elongate shaft assembly 1100 to pivot the anvil 1050 to a closed position as will be discussed in further detail below.

Once inserted into an insufflated body cavity or lumen, the closure trigger 1040 may be released, opening the anvil 1050 so that tissue may be grasped and positioned. Once satisfied with the tissue held in the staple applying assembly 1016, the surgeon depresses the closure trigger 1040 until locked against the pistol grip 1034, clamping tissue inside of the

staple applying assembly **1016**. Then a firing trigger **1046** is drawn toward the closure trigger **1040** and pistol grip **1034**, thereby applying a firing force or motion thereto to distally advance a firing member supported with in the implement **1014** from an unfired position. As the firing member advances through the implement or end effector **1014** in a known manner, it severs the tissue clamped within the end effector **1014** and fires or drives the staples contained with the staple cartridge **42** supported therein.

As depicted in FIG. **57**, this embodiment may employ the firing bar **36** and E-Beam **50** arrangements described above. In other alternative embodiments, the E-Beam arrangements described in U.S. patent application Ser. No. 11/231,456, filed Sep. 21, 2005 and entitled "Surgical Stapling Instrument Having Force Controlled Spacing End Effector", the disclosure of which is herein incorporated by reference may also be employed. In addition, as the present Detailed Description proceeds, those of ordinary skill in the art will appreciate that the advantages provided by these embodiments of the present invention may be effectively attained when used in connection with other known non-E beam firing bar configurations. Thus, these embodiments of the present invention should not be limited solely to use in connection with E-beam type firing and cutting arrangements.

FIG. **57** depicts the firing bar **36** as including a proximal firing rod **34**, that is supported within a "frame ground" or spine assembly **1110** that connects the handle assembly **1020** to the staple applying assembly **1016**. During the staple firing motion, the firing bar **36** engages an elongate staple channel **1060** and actuates a staple cartridge **42** contained therein, both forming the lowerjaw **1018** in the various manners described above.

A variety of different firing arrangements for applying an actuation force to the firing bar **36** to cause the firing bar to linearly advance and retract through the staple applying assembly **1016** are known. Such firing motions may be manually generated such as through use of the various firing system arrangements disclosed in U.S. Patent application Ser. No. 11/475,412, filed Jun. 27, 2006, entitled "Manually Driven Surgical Cutting and Fastening Instrument" to Frederick E. Shelton, IV, et al., the disclosure of which is herein incorporated by reference. Still other actuation systems, such as the pneumatically powered actuation systems disclosed in U.S. patent application Ser. No. 11/497,898 filed Aug. 2, 2006, entitled "Pneumatically Powered Surgical Cutting and Fastening Instrument With a Variable Control of the Actuating Rate of Firing With Mechanical Power Assist" to Frederick B. Shelton, IV et al., the disclosure of which is herein incorporated by reference may be successfully employed. Other embodiments may include, for example, the electrical motor driven actuation systems disclosed in U.S. patent application Ser. No. 11/343,562, filed Jan. 31, 2006, entitled "Motor-Driven Surgical Cutting and Fastening Instrument With Articlatable End Effector" to Frederick E. Shelton, IV et al., the disclosure of which is also herein incorporated by reference. Still other embodiments may include other known mechanically, electrically, hydraulically and/or pneumatically powered firing systems without departing from the spirit and scope of the present invention.

In various embodiments, the elongate shaft assembly **1100** consists of a closure tube assembly **1130** that is received on the spine assembly **1110**. See FIG. **57**. The spine assembly **1110** may comprise a single member or it may comprise multiple segments with an articulation joint (not shown) mounted therein. Such articulation joints are known in the art and may, for example, be mechanically, electrically, hydraulically or pneumatically controlled. In the embodiment

depicted in FIGS. **57** and **58**, the spine assembly **1110** includes a proximal portion **1112** (FIG. **58**) and a distal portion **1116** (FIG. **57**). As will be discussed below, the proximal portion **1112** is attached to the handle assembly **1020** such that the closure tube assembly **1130** may be axially moved thereon to cause the anvil **1050** to pivot between open and closed positions. As can be seen in FIG. **57**, the elongate channel **1060** has proximally placed attachment cavities **1062** that each receive a corresponding channel anchoring member **1118** formed on the distal end of the distal spine portion **1116**. The elongate channel **1060** also has elongated anvil cam slots **1064** that movably receive a corresponding anvil trunnion **1052** on the anvil **1050** as will be discussed in further detail below.

The closure tube assembly **1130** may comprise a distal closure tube portion **1140** and a proximal closure tube portion **1150**. The distal closure tube portion **1140** and the proximal closure tube portion **1150** may be fabricated from a polymer or other suitable material. The distal closure tube portion **1140** and the proximal closure tube portion **1150** are each hollow for receiving a corresponding portion of the spine assembly **1110** therein. The closure tube assembly **1130** is depicted as comprising two separate portions **1140** and **1150** for ease of assembly of the entire elongate shaft assembly **1100**. Those portions **1140** and **1150** may be attached together after assembly by adhesive or other suitable fastening means. It is conceivable, however, that the closure tube assembly **1130** may be fabricated as one piece. In addition, as was mentioned above, the spine assembly of various embodiments of the present invention may have an articulation joint mounted therein. For those embodiments, a double pivot closure joint (not shown) may be employed in the closure tube assembly **1130**. Examples of such double pivot closure arrangements are disclosed in U.S. patent application Ser. No. 11/497,898, which has been herein incorporated by reference.

In use, the closure tube assembly **1130** is translated distally to close the anvil **1050**, for example, in response to the actuation of the closure trigger **1040**. The anvil **1050** is closed by distally translating the closure tube assembly **1130** on the spine assembly **1110**, causing the back of a horseshoe aperture **1142** in the distal closure tube portion **1140** to strike a closure feature **1053** in the form of an open/closing tab **1052** on the anvil **1050** and cause it to pivot to the closed position. See FIG. **57**. To open the anvil **1050**, the closure tube assembly **1130** is axially moved in the proximal direction on the spine assembly **1110** causing a tab **1144** on the distal closure tube portion **1140** to contact and push against the open/closing tab **1054** on the anvil **1050** to pivot the anvil **1050** to the opened position.

FIG. **58** illustrates an exploded assembly view of a non-limiting handle assembly **1020** of various embodiments of the present invention wherein the various firing system components have been omitted for clarity. In the embodiment depicted in FIG. **58**, the handle assembly **1020** has a "pistol grip" configuration and is formed from a right hand case member **1022** and a left handed case member **1028** that are molded or otherwise fabricated from a polymer or other suitable material and are designed to mate together. Such case members **1022** and **1028** may be attached together by snap features, pegs and sockets molded or otherwise formed therein and/or by adhesive, screws, bolts, clips, etc. The upper portion **1024** of the right hand case member **1022** mates with a corresponding upper portion **1030** of the left hand case member **1028** to form a primary housing portion designated as **1031**. Similarly, the lower grip portion **1025** of the right hand case member **1022** mates with the lower grip portion

1032 of the left hand case member 1028 to form a grip portion generally designated as 1034. See FIG. 56. Those of ordinary skill in the art will readily appreciate, however, that the handle assembly 1020 may be provided in a variety of different shapes and sizes.

For the purposes of clarity, FIG. 58 only illustrates the components employed to control the axial movement of the closure tube assembly 1130 which ultimately controls the opening and closing of the anvil 1050. As can be seen in that Figure, a closure shuttle 1160 that is coupled to the closure trigger 1040 by a linkage assembly 1180 is supported within the primary housing portion 1031. Closure shuttle 1160 may also be fabricated in two pieces 1162, 1164 that are molded or otherwise fabricated from a polymer or other suitable material and are designed to mate together. For example, in the embodiment illustrated in FIGS. 58, 60, and 61, the right hand portion 1162 may be provided with fastener posts 1163 that are designed to be received within corresponding sockets 1167 (FIG. 61) in the left hand portion 1164. The right and left hand portions 1162, 1164 may be otherwise retained together by snap members and/or adhesive and/or bolts, screws, clips, etc. As can be seen in those Figures, a retention groove 1152 is provided in the proximal end 1151 of the proximal closure tube portion 1150. The right hand portion 1162 of the closure shuttle 1160 has a right retention flange 1165 (FIG. 60) that is adapted to cooperate with a left hand portion 1164 of the closure shuttle 1160 such that the retention flange 1165 extends into the retention groove 1151 in the proximal closure tube portion 1150. The retention flange 1165 serves to affix the closure tube assembly 1130 to the closure shuttle 1160 while facilitating its limited axial movement relative thereto as will be discussed in further detail below.

As can also be seen in FIG. 58, a right spine assembly retention peg 1027 protrudes inward from the right hand case member 1024. Such peg 1027 protrudes into an elongated slot or window 1166 in the right hand portion 1162 of the closure shuttle 1160. A similar closure shuttle retention peg (not shown) protrudes inward from the left hand case member 1164 to be received in another window or slot 1168 provided in the left hand side portion 1164 of the closure shuttle 1160. The retention pegs are configured to extend into a hole 1115 in the proximal end 1114 of the proximal spine portion 1110 to non-movably affix the spine portion 1110 to the handle assembly 1020 while permitting the closure shuttle 1160 to move axially relative thereto. See FIG. 58. The retention pegs may be mechanically attached to the proximal end 1114 of the proximal spine portion 1112 by, for example, bolts, screws, adhesive, snap features, etc. In addition, the closure shuttle 1160 is provided with laterally extending guide rails 1170, 1172. Rail 1170 is configured to be slidably received within rail guide 1026 in the right hand case member 1024 and rail 1172 is configured to be slidably received within a rail guide (not shown) in left hand case member 1028. See FIG. 58.

Axial movement of the closure shuttle 1160 and closure tube assembly 1130 in the distal direction (arrow "A") is created by moving the closure trigger 1040 toward the grip portion 1034 of the handle assembly 1020 and axial movement of the closure shuttle 1160 in the proximal direction (arrow "B") is created by moving the closure trigger 1040 away from the grip portion 1034. In various embodiments, the closure shuttle 1160 is provided with a connector tab 1174 that facilitates the attachment of the closure linkage assembly 1180 thereto. See FIGS. 58 and 59. The closure linkage assembly 1180 includes a yoke portion 1182 that is pivotally pinned to the connector tab 1174 by a pin 1184. The closure linkage assembly 1180 further has a closure arm 1186 that is pivotally pinned to a yoke assembly 1043 formed on the

closure trigger 1042 by a closure pin 1188 as illustrated in FIG. 58. The closure trigger 1140 is pivotally mounted within the handle assembly 1020 by a pivot pin 11890 that extends between the right hand case member 1024 and the left hand case member 1028.

When the clinician desires to close the anvil 1050 to clamp tissue within the end effector 1014, the clinician draws the closure trigger 1040 toward the pistol grip portion 1034. As the clinician draws the closure trigger 1040 toward the pistol grip portion 1034, the closure linkage assembly 1180 moves the closure shuttle 1160 in the distal "A" direction until the closure linkage assembly 1180 moves into the locked position illustrated in FIG. 59. When in that position, the closure linkage assembly 1180 will tend to retain the closure shuttle 1160 in that locked position.

In various embodiments, to further retain the closure shuttle 1160 in the closed position, the closure trigger 1040 may be provided with a releasable locking mechanism 1190 that is adapted to engage the pistol grip portion 1034 and releasably retain the closure trigger 1040 in the locked position. Other locking devices may also be used to releasably retain the closure shuttle 1160 in the locked position.

In the embodiment depicted in FIG. 59, the closure trigger 1040 includes a flexible longitudinal arm 1192 that includes a lateral pin 1194 extending therefrom. The arm 1192 and pin 1194 may be made from molded plastic, for example. The pistol grip portion 1034 of the handle assembly 1020 includes an opening 1036 with a laterally extending wedge 1037 disposed therein. When the closure trigger 1040 is retracted, the pin 1194 engages the wedge 1037, and the pin 1194 is forced downward (i.e., the arm 1192 is rotated clockwise) by the lower surface of the wedge 1037. When the pin 1194 fully passes the lower surface, the clockwise force on the arm 1192 is removed, and the pin 1194 is rotated counterclockwise such that the pin 1194 comes to rest in a notch 1038 behind the wedge 1037 thereby locking the closure trigger 1040. The pin 1194 is further held in place in the locked position by a flexible stop 1039 extending from the wedge 1037. trigger 1040, causing the pin 1194 to engage a sloped back wall 1041 of the opening 1036,

To unlock the closure trigger 1040, the operator may further squeeze the closure trigger 1040, causing the pin 1194 to engage a sloped back wall 1041 of the opening 1036, forcing the pin 1194 upward past the flexible stop 1039. The pin 1194 is then free to travel out of the opening 1036 such that the closure trigger 1040 is no longer locked to the pistol grip portion 1034. Further details of such arrangement may be found in U.S. patent application Ser. No. 11/344,020, filed Jan. 31, 2006 and entitled "Surgical Instrument Having A Removable Battery" to Shelton, IV et al., the relevant portions of which are herein incorporated by reference. Other releasable locking arrangements could also be employed.

As the closure shuttle 1160 is moved to the locked position, the closure tube assembly 1130 is moved distally on the spine assembly 1110 causing the closure/opening tab 1054 on the anvil 1050 to be contacted by the proximal end of the horse-shoe aperture 1142 in the distal closure tube portion 1140 to thereby pivot the anvil 1050 to the closed (clamped) position. Thus, the clamping forces attained by the anvil 1050 during the clamping process are ultimately dependant upon the closure forces generated by the closure tube assembly (represented by arrow 1196 in FIGS. 62 and 63) as it contacts the tab 1054 on the anvil 1050. As was discussed above, prior closure tube arrangements lack means for limiting the amount of actuation force applied to the closure/opening tab 1054 of the anvil 1050.

Various embodiments of the present invention address such shortcomings of prior closure tube arrangements by including a force limiting member generally designated as **1200** for limiting the amount of closure force or load applied by the closure tube assembly to the closure/opening tab **1054** of the anvil. For example, in one embodiment, the force limiting member **1200** may comprise a cushioning member **1210** oriented adjacent to the proximal end **1151** of the proximal closure tube portion **1150**. More specifically and with reference to FIGS. **60** and **61**, the cushioning member **1210** comprises a wave spring assembly **1212** that may be supported in a cavity **1169** formed in the closure shuttle **1160**. The wave spring assembly **1212** may be supported between an attachment post **1163** and the proximal end **1151** of the proximal closure tube portion **1150**. In various embodiments, the wave spring assembly **1212** may be fabricated from spring steel in the form depicted in the Figures. However, other cushioning arrangements or compliant member arrangements such as, for example, members fabricated from rubber, elastomer, polymer, foam rubber, etc. could be successfully employed to provided the closure tube assembly **1130** with some freedom to axially move in the proximal direction to reduce the clamping force ultimately applied to the anvil **1050** during the anvil closing process which will be discussed in further detail below.

As can also be seen in FIGS. **60** and **61**, the retention groove **1152** in the proximal closure tube portion **1150** comprises an area **1154** that has a diameter that is less than the outer diameter of the proximal closure tube portion **1150**. The area **1154** is axially elongated to provide the closure tube assembly **1130** to move axially and distally relative to the closure shuttle **1160** a distance that is defined by the axial length (arrow **1155** in FIG. **60**) of the retention groove **1152**.

In this embodiment, as the closure trigger **1040** is moved toward the pistol grip portion **1032**, the closure shuttle **1160** is advanced in the distal direction (arrow A). As the closure shuttle **1160** moves distally, the closure tube assembly **1130** is also forced distally. As can be seen in FIGS. **62** and **63**, distal end **1141** of the distal closure tube portion **1140** is oriented to move axially up a ramp portion **1070** of the anvil **1050**. As the distal end **1141** contacts the anvil ramp **1070** and continues to move distally up the ramp, it imparts a closure force to the anvil **1050**. The anvil trunnions **1052** are received in corresponding "kidney-shaped" slots **1064** in the proximal end of the elongate staple channel **1060** and serve to guide the anvil **1050** in a desired closure path which results in the clamping of the tissue between the staple forming undersurface of the anvil **1051** and the upper surface of the staple cartridge **42**. As the anvil **1050** contacts the tissue, a resulting resistive force is transferred to the anvil **1050** and ultimately to the distal end **1141** of the distal closure tube portion **1140**. The magnitude of such resistive force is effected by the thickness of the tissue being clamped. Thinner tissues will exert less resistive forces than thicker tissues. However, as the resistive forces are encountered, the cushioning member **1210** enables the closure tube assembly **1130** to move proximally to ultimately limit the amount of closure force applied to the anvil **1050** by the closure tube assembly **1130**.

The magnitudes of the resistive forces for various thicknesses and types of tissues may be determined and the wave spring **1212** sized accordingly such that the desired amount of clamping force is applied to the tissue between the anvil **1050** and the staple cartridge **42**. The wave spring **1212** may be sized and oriented such that when the anvil **1050** is at a fully compressed position, the wave spring **1212** is not fully compressed or "bottomed out".

FIGS. **64** and **65** illustrate other versions of closure tube assemblies that may be employed to limit closure forces applied to the anvil **1050**. As can be seen in those Figures, the force limiting members **1200a**, **1200b** comprise spring sections **1212a**, **1212b** actually formed into the distal closure tube portion **1140a**, **1140b**, respectively. While the spring sections **1140a**, **1140b** are depicted as being somewhat helical in nature and formed in the distal closure tube portions **1140a**, **1140b**, those of ordinary skill in the art will understand that the spring sections **1212a**, **1212b** may be provided in any portion of the closure tube assemblies **1130a**, **1130b** and could conceivably be provided in different configurations. Those of ordinary skill in the art will understand that in these embodiments, the retention groove **1152** in the proximal closure tube portion may not be elongated such that the closure tube assembly **1130a**, **1130b** is essentially not axially movable relative to the closure shuttle **1160**. In addition, while only one spring section is shown as being provided in the closure tube assembly, it is conceivable that more than one spring section may be formed in a single closure tube assembly. As with the above-described versions, as the resistive forces are encountered during clamping, the spring members **1212a**, **1212b** enable their respective closure tube assembly **1130a**, **1130b** to move proximally to ultimately limit the amount of closure force applied to the anvil **1050**.

FIGS. **66** and **67** illustrate another closure tube assembly of various embodiments of the present invention that may be employed to limit closure forces applied to the anvil **1050**. As can be seen in those Figures, the force limiting member **1200c** comprises a leaf spring **1212c** formed in the distal end **1141** of the distal closure tube portion **1140c**. When the closure tube assembly **1130c** is actuated to move distally to close the anvil **1050**, the leaf spring **1212c** rides up the anvil ramp **1070** and is free to move radially (arrows **1214** in FIG. **66**) and axially (arrow **1216** in FIG.). As with the above-described versions, as the resistive forces are encountered during clamping, the leaf spring **1212c** enables the closure tube assembly **1130c** to move proximally (arrow B) to ultimately limit the amount of closure force applied to the anvil **1050**.

FIGS. **68** and **69** illustrate another embodiment of the present invention that may be employed to limit closure forces applied to the anvil **1050** by the closure tube assembly **1130**. As can be seen in those Figures, this embodiment employs an anvil **1050d** that has a stepped ramp **1070** that is configured to be engaged by the distal end **1141** of the distal closure tube portion **1140**. In particular, the anvil **1050d** depicted in those Figures has a series of steps **1074d**, **1076d**, **1078d**, **1080d** formed therein. As the closure tube assembly **1130** is moved distally, the distal end **1141** starts to ride up the smooth portion **1072d** of the ramp **1070** until it contacts the first step **1074d**. The closure tube assembly **1130** will not advance further up the ramp **1070d** to apply a higher amount of closure force to the anvil until the actuation force applied to the closure tube assembly **1130** attains a sufficient magnitude to cause the distal end **1141** to bump up over the first step **1074d** and proceed to engage the next step **1076d**. The closure tube assembly **1130** will not advance further up the ramp **1070d** until the actuation force attains a sufficient magnitude to cause the distal end **1141** to bump up over the second step **1076d** at which time it will engage the next step **1078d** and so on. Thus, the stepped anvil **1050d** cooperates with the closure tube assembly **1130** to provide a means for relating the amount of clamping forces ultimately applied to the tissue between the anvil **1050d** and the staple cartridge **42** based on the amount of resistive forces generated thereby and encountered by the closure tube assembly **1130** during clamping. While four such steps have been disclosed, other numbers of

steps may be employed. For example, only one such step may be used or 2, 3, or more than 4 steps could conceivably be employed.

FIGS. 70-76 illustrate another unique and novel endocutter implement portion 1014e of various embodiments of the present invention that includes an elongate channel 1060e and an anvil arrangement 1050e that are "self adjusting" with respect to tissue thickness. In various embodiments, the proximal end of the anvil 1050e is pivotally attached to the proximal end of the elongate channel 1060e by mounting members which may comprise trunnions 1052e movably received in corresponding elongate slots 1064e formed in the proximal end 1061e of the elongate channel 1060e. As can be seen in FIGS. 70-74, at least one of the slots 1064e on each side of the elongate channel 1060e (only one slot 1064e is illustrated in FIGS. 70-74) and preferably both of the slots 1064e each have an end wall 1065e that has a discrete number of predetermined locations in the form of detents or pivot nests 1066e, 1067e, 1068e, 1069e formed therein. As can be seen in these Figures, the detents 1066e, 1067e, 1068e, 1069e may each comprise a V-shaped notch that is adapted to seatingly receive the pointed end of a pawl 1080e formed on the corresponding trunnion 1052e. It is conceivable that other detent and pawl configurations may be successfully employed. As can also be seen in FIGS. 70-74, this embodiment may further include a leaf spring 1090 or other suitable biasing member for applying a downward biasing force to the proximal end 1055e of the anvil 1050e. In various embodiments, the leaf spring 1090 may be attached to the distal portion 1116 of the spine assembly 1110 and oriented to bear upon the proximal end 1055e of the anvil 1050e.

As can be seen in FIG. 74, the slot 1064e is sized relative to the trunnion 1052e to permit the trunnion 1052e to find different clamped heights in response to the thickness of the tissue clamped between the anvil 1050e and the cartridge 42 and the application of the closing motion to the anvil 1050e. The leaf spring 1090 serves to bias the pawl 1080e into a slightly upward position wherein it can be received in any one of the notches 1066e, 1067e, 1068e, 1069e. As the anvil 1050e is closed onto the tissue by means of distally advancing the closure tube assembly 1130 in the above-described manner, the tissue thickness itself may dictate which of the notches 1066e, 1067e, 1068e, 1069e that the pawl 1080e ultimately seatingly engages. Because the leaf spring 1090 biases the pointed pawl upwardly, the pawl 1080e would find the uppermost notch 1069e when no tissue is between the anvil 1050e and the cartridge 42 which would clamp the end effector 1014e to its most closed position. See FIGS. 71 and 74. However, if during the clamping process, the anvil 1050e and channel 1060e encounter resistance, the leaf spring 1090 would be compressed and the anvil trunnions 1052e would find a lower pivot notch which would ultimately result in a larger gap between the anvil 1050e and the cartridge 42.

FIG. 70 illustrates the anvil 1050e in an open position. FIG. 71 illustrates the anvil 1050e in its most closed position. The tissue clamping space or distance between the underside 1051e of the anvil 1050e and the cartridge 42 is designated as "t". FIG. 75 also illustrates the position of the anvil 1050e relative to the staple cartridge 42 and tissue 1092 that has a thickness "t". Similarly, FIG. 73 illustrates the anvil 1050e in its uppermost clamped position wherein the distance between the underside 1051e of the anvil 1050e and the cartridge 42 is designated as "T". FIG. 76 also illustrates the anvil 1050e relative to the staple cartridge 42 and tissue 1094 that has a thickness "T". As can be seen in FIGS. 75 and 76, the staples 83 in the thinner tissue 1092 are more tightly formed than the staples 83 extending through the thicker tissue 1094.

FIGS. 77-88 illustrate another embodiment of the present invention that may be employed in connection with a circular stapler 1600 that includes a unique and novel apparatus for limiting the amount of compression force that can be generated between the anvil and the staple cartridge to avoid over compressing and possibly destroying the tissue to be stapled. A variety of different circular staplers are known in the art. FIGS. 77-88 illustrate an exemplary circular stapler arrangement that may employ the benefits of various aspects of the subject invention. It is conceivable, however, that the various embodiments of the present invention may be successfully employed with other stapler constructions without departing from the spirit and scope of the present invention.

As seen in FIG. 77, there is disclosed the circular stapler 1600 including a head 1610, an anvil 1700, an adjustment knob assembly 1800, and trigger 1664. The head 1610 is coupled to a handle assembly 1660 by an arcuate shaft assembly 1630. The trigger 1664 is pivotally supported by the handle assembly 1660 and acts to operate the stapler 1600 when a safety mechanism 1670 is released. As will be discussed in further detail below, when the trigger 1664 is activated, a firing mechanism (not shown in FIG. 77) operates within the shaft assembly 1630 so that staples 1618 are expelled from the head 1610 into forming contact with the anvil 1700. Simultaneously, a knife 1620 operably supported within the head 1610 acts to cut tissue held within the circumference of the stapled tissue. The stapler 1600 is then pulled through the tissue leaving stapled tissue in its place.

FIG. 78 illustrates one form of anvil 1700 and head 1610 that may be employed in connection with various embodiments of the subject invention. As can be seen in that Figure, the anvil 1700 may have a circular body portion 1702 that has an anvil shaft for attaching a trocar thereto. The anvil body 1702 has a staple forming undersurface 1706 thereon and may also have a shroud 1708 attached to the distal end thereof. The anvil 1700 may be further provided with a pair of trocar retaining clips or leaf-type springs 1710 that serve to releasably retain a trocar 1644 in retaining engagement with the anvil shaft 1704 as will be discussed in further detail below. In the embodiment depicted in FIG. 78, a plastic knife board 1714 may be fitted into a cavity 1712 in the anvil body 1702.

As can also be seen in FIG. 78, the head 1610 may comprise a casing member 1612 that supports a cartridge supporting assembly in the form of a circular staple driver assembly 1614 therein that is adapted to interface with a circular staple cartridge 1616 and drive staples 1618 supported therein into forming contact with the staple forming undersurface 1706 of anvil 1700. A circular knife member 1620 is also centrally disposed within the staple driver assembly 1614. The proximal end of the casing member 1612 may be coupled to an outer tubular shroud 1631 of the arcuate shaft assembly 1630 by a distal ferrule member 1632.

FIGS. 79-82 illustrate one form of arcuate shaft assembly 1630 that may be employed with various embodiments of the present invention. As can be seen in FIGS. 79 and 80, the arcuate shaft assembly 1630 may include a compression shaft 1634, a distal compression shaft portion 1635, a top tension band 1636, a bottom tension band 1638 and a spacer band 1640 that are assembled within the outer tubular shroud 1631 (FIG. 80). A trocar tip 1644 may be attached to the top tension band 1636 and bottom tension band 1638 by fasteners 1646. The proximal ends of the top tension band 1636 and bottom tension band 1638 may be attached to a distal end of an adjustment shaft 1650. As can be seen in FIG. 80, the trocar tip 1644 may be inserted into the anvil shaft 1704 of the anvil 1700 and retained in engagement by trocar retaining clips 1710.

As can be seen in FIG. 80, the distal compression shaft portion 1635 is coupled to the staple driver assembly 1614. Thus, axial movement of the compression shaft 1634 within the outer tubular shroud 1631 causes the staple driver assembly 1614 to move axially within the casing member 1612. As will be discussed below, actuation of the firing trigger 1664 will cause the compression shaft 1634 to move in the distal direction (arrow "DD") thereby driving the staple driver assembly 1614 distally to fire the staples 1618 into forming contact with the staple forming undersurface 1706 of the anvil 1700. As the staple driver assembly 1614 is driven distally, it also drives the distal end 1622 of the knife 1620 through the tissue held within the circumference of the stapled tissue into the knife board 1714 mounted in the anvil 1700. The knife board 1714 may be fabricated from plastic or other suitable material that will permit the sharp distal end 1622 of the knife 1620 to penetrate and achieve a desirable cutting action through the clamped tissue.

In various embodiments, the adjusting shaft 1650 is axially movably supported within a handle assembly 1660 that may comprise two handle casing segments 1661, 1662 that are interconnected together by suitable fastener arrangements for ease of assembly. The trigger 1664 is pivotally attached to the handle assembly 1660 by a pivot pin 1666. A spring 1668 is supported on pivot pin 1666 and serves to bias the trigger 1664 away from the handle assembly 1660 to an unactuated position. A safety yoke 1670 is pivotally coupled to the trigger assembly 1664 by pin 1672 such that it can be pivoted between a safe position wherein the trigger 1664 cannot be depressed towards the handle 1660 and an off position wherein the safety yoke 1670 does not inhibit pivotal travel of the trigger assembly 1664 toward the handle assembly 1660. As can be seen in FIG. 79, the trigger 1664 may have a pair of fins 1665 that are sized to be received in slots 1676 in a firing clip 1674 that is attached to the proximal end 1637 of compression shaft 1634 by a protrusion 1639 or other suitable fastener arrangements. Such arrangement permits the distal axial movement (arrow "DD") and the proximal axial movement (arrow "PD") of the compression shaft 1634 by pivoting the trigger 1664 as will be further discussed below. The trigger 1664, the compression shaft portions 1634, 1635 and the firing cap 1674 and other related components may comprise a firing assembly generally designated as 1675.

As can be seen in FIGS. 79 and 81, the adjustment shaft 1650 has a distal portion 1651 that is attached to the top and bottom tension bands 1636, 1638 and a proximal portion 1652 that is adjoined to the distal portion 1651 by a reduced diameter segment 1653. The proximal portion 1652 is axially received within an axial passage 1722 in the distal closure nut 1720 that is keyed onto or otherwise attached to a proximal closure nut 1740 to form a closure nut assembly generally designated as 1721 such that the distal closure nut 1720 and the proximal closure nut 1740 may rotate together. The distal closure nut 1720 may further have a distally extending hub portion 1724 that abuts an inwardly extending retainer flange 1667 formed inside the handle assembly 1660. See FIG. 81. Such arrangement permits the distal closure nut 1720 to freely rotate within the handle assembly 1660, but is unable to move axially therewithin. Likewise, the proximal end portion 1652 of the adjustment shaft 1650 is axially received within an axial passage 1742 within the proximal closure nut 1740. A circumferentially extending groove 1744 may be provided in the outer surface of the proximal closure nut 1740 for receiving an inwardly protruding proximal retainer flange 1669 formed on the proximal end of the handle assembly

1660. Such arrangement serves to permit the proximal closure nut 1740 to freely rotate relative to the handle assembly 1660.

Also in various embodiments, the closure knob assembly 1800 is attached to the proximal end 1741 of the proximal closure nut 1740. In one embodiment for example, the proximal end 1741 of the proximal closure nut 1740 may be formed with a proximally extending tapered hub portion 1746 that is adapted to be nonrotatably received in an axial passage 1832 in a clutch hub portion 1830. See FIG. 81. The tapered hub portion 1746 can also be formed with a key or spline arrangement to non-rotatably affix the hub portion 1746 with the clutch hub portion 1830. Other fastener arrangements and methods may be employed to non-movably attach the hub portion 1746 of the proximal closure nut 1740 to the clutch hub portion 1830. Thus, rotation of the clutch hub portion 1830 will cause the proximal closure nut 1740 and distal closure nut 1720 to also rotate.

As can also be seen in FIGS. 81, 83, and 84, the knob assembly 1800 may further include a proximal cap portion 1810 and a distal cap portion 1820. The proximal end 1831 of the clutch hub portion may be received in a circular slot 1814 formed in a distal end of the proximal cap portion 1810. The slot 1814 may be sized to permit the proximal cap portion 1810 to rotate about the proximal end 1831 of the clutch hub portion 1830. In addition, the proximal cap portion 1810 may have a protrusion 1812 that rotatably extends into the axial passage 1832 in the clutch hub portion 1830. Also in various embodiments, the closure knob assembly 1800 may comprise a distal cap portion 1820 that is rigidly and non-rotatably coupled to the proximal cap portion 1810. Those of ordinary skill in the art will understand that the closure knob assembly 1800 may be fabricated in multiple parts for ease of assembly of various components of the instrument. In various embodiments, the mating ends of the proximal cap portion 1810 and distal cap portion 1820 may be configured with complementary flanged portions 1813, 1823, respectively as shown in FIGS. 81 and 83, that are interconnected by adhesive, welding, etc. or other fastener arrangements may be employed. Thus, when fastened together, the proximal cap portion 1810 and the distal cap portion 1820 rotate together as a unit.

As can further be seen in FIGS. 81 and 83, various embodiments may comprise a slip clutch assembly generally designated as 1821. The slip clutch assembly 1821 may take various forms that are supported by or are integrally formed in the adjustment knob assembly 1800. In one embodiment, for example, the distal cap portion 1820 may be provided with an inwardly extending cap flange 1824 that is in confronting orientation with an outwardly extending clutch flange 1834 formed on the clutch hub portion 1830. A first friction pad 1840 is non-rotatably affixed to the inwardly extending cap flange 1824. A pad cavity 1836 may be formed within the clutch flange 1834 for movably receiving a second friction pad 1850 and a wave spring 1852 therein. The second friction pad 1850 may be provided with splines or keys (not shown) to prevent rotation thereof in the cavity 1836, but facilitate some axial travel thereof within the cavity 1836. In various embodiments, the first and second friction pads 1840, 1850 may be fabricated from, for example, liquid crystal polymer, Nylon, ULTEM®, polycarbonate, aluminum, etc.

In various embodiments, the proximal portion 1652 of the adjustment shaft 1650 has a low pitch thread segment 1654 formed therein that communicates with a higher pitched threaded segment 1657. See FIG. 79. As can be seen in FIG. 81, a drive pin 1726 protrudes inwardly into the axial passage 1722 for "driving" engagement with the threaded segments 1654, 1657 in the adjustment shaft 1650. In addition, the

proximal end 1652 of the adjustment shaft 1650 has a threaded section 1658 adapted for threaded engagement with a threaded cavity 1748 in the tapered hub portion 1746 of the proximal closure nut 1740. In various embodiments, the drive pin 1726 is oriented in the distal closure nut 1720 such that when the drive pin 1726 is still engaged with the low pitched distal thread segment 1654 of the adjustment shaft 1650, the threaded end 1658 of the adjustment shaft 1650 has sufficiently threadably engaged the threaded cavity 1748 in the tapered hub portion 1746 of the proximal closure nut 1740 for threaded travel therein as the closure knob assembly 1800 is rotated. In particular, as the closure knob assembly 1800 is rotated in the counterclockwise ("CC") direction, the adjustment shaft 1650 is moved in the distal direction "DD" by virtue of the engagement of the drive pin 1726 with the threaded segments 1654 and 1657 formed in the adjustment shaft 1650. Those of ordinary skill in the art will appreciate that rotation of the distal closure nut 1720 when the drive pin 1726 is engaged with the distal threaded segment 1654 will result in fastener axial movement of the adjustment shaft 1650 than when the drive rod 1726 is engaged with the threaded segment 1567 which has a larger pitch than the threaded segment 1564. Axial movement of the adjustment shaft 1650 moves the top and bottom tension bands 1636, 1638, the trocar tip 1644 and the anvil 1700 (when attached to the trocar tip 1644) in the distal "DD" direction away from the head 1610.

To close the anvil 1700 or move it toward the head 1610 and staple cartridge 1616 supported therein in the "PD" direction, the surgeon begins to turn the closure knob assembly 1800 in the clockwise ("CW") direction. The frictional forces generated between the first and second friction pads 1840, 1850 serves to retain the closure knob assembly 1800 in frictional engagement with the clutch hub 1830 which is non-rotatably attached to the proximal closure nut 1740. Because the proximal closure nut 1740 is non-rotatably affixed to the distal closure nut 1720, the distal closure nut 1720 is also rotated in the clockwise direction. Rotation of the distal closure nut 1720 results in the driving engagement of the drive pin 1726 with either of the thread segments 1654, 1657 (depending upon the position of the adjustment shaft 1650 relative thereto) and causes the adjustment shaft 1650 to be drawn in the proximal direction ("PD"). As the adjustment shaft 1650 is drawn in the proximal direction, the threaded end 1658 of the adjustment shaft 1650 threadably engages the threaded cavity 1748 of the tapered threaded hub portion 1746 of the proximal closure nut 1740 and reduced diameter segment 1653 moves adjacent to the drive pin such that the drive pin is no longer in driving engagement with the adjustment shaft 1650. Now, the threaded end 1652 is in full threaded engagement with the threaded hole 1748 in the proximal closure nut 1740. Further rotation of the closure knob assembly 1800 in the clockwise direction continues to draw the adjustment shaft 1650 in the proximal direction "PD". As the adjustment shaft 1650 is drawn in the proximal direction, the anvil 1700 is moved towards the cartridge 1616 supported in the staple driver assembly 1614 to clamp an amount of tissue therebetween. As the anvil 1700 continues to move toward the staple cartridge 1616, the tissue is compressed therebetween and resists further travel of the anvil 1700 in the proximal direction.

In various embodiments, to prevent the tissue from being over compressed which could result in damaging or killing the tissue to be stapled, the composition of the first and second friction pads 1840, 1850 and the size of the spring 1852 are selected such that when a predetermined amount of tissue compression is attained, the friction pads 1840, 1850 begin to

slip to prevent further rotation of the closure knob assembly 1800 from being transferred to the clutch hub 1830. Thus, even if the surgeon continues to rotate the closure knob assembly 1800 after the tissue has been adequately compressed, such further rotation will not result in continued movement of the adjustment shaft 1650 (and anvil 1700) in the proximal direction to avoid over compressing the tissue. For example, in various embodiments, the instrument may be constructed such that the maximum amount of compression forces that may be applied to the tissue between the anvil 1700 and the cartridge 1616 may be approximately 150 pounds per square inch. For such applications, the first and second friction pads 1840, 1850 and the wave spring 1852 may be so configured to permit slippage between the first and second friction pads 1840, 1850 if the closure knob assembly 1800 continues to be rotated after that maximum amount of compression force has been attained. In such example, the rotation of the closure knob assembly 1800 may generate an approximate amount of torque of, for example, 15 inch pounds which overcomes the frictional forces that are established when the maximum amount of desirable compression has been attained (which serves to retain the first and second friction pads 1840, 1850 in frictional engagement with each other) and permit the desired slippage between the first and second friction pads. In various embodiments, to ensure that the adjustment shaft 1650 is moved distally when the closure knob assembly 1800 is rotated in a counterclockwise direction, a series of circumferentially extending ratchet teeth 1816 may be formed in the interior of the closure knob assembly 1800 for engagement with circumferentially extending engagement teeth 1835 formed on the circumference of the clutch flange 1834. See FIGS. 83 and 84. The teeth 1816, 1835 may be configured such that when the closure knob assembly 1800 is rotated in the clockwise direction to move the anvil 1700 toward the cartridge 1616, the teeth 1816 on the closure knob assembly 1800 slip over the teeth 1835 formed on the clutch flange 1834. However, when the closure knob assembly 1800 is rotated in the counterclockwise direction, the teeth 1816 engage teeth 1845 on the clutch flange 1834 to cause the clutch hub 1830 and the proximal and distal closure nuts 1720, 1740 to rotate therewith to move the anvil 1700 away from the cartridge 1616.

As indicated above, various embodiments may be provided with a safety yoke 1670 that prevents actuation of the trigger assembly 1664 when the safety yoke 1670 is in a "safe" or engaged position. In various embodiments, a safety spring 1686 may be journaled on the adjustment shaft 1650 and be received on the hub portion 1724 of the distal closure nut 1720. The spring 1686 may be oriented between the distal closure nut 1720 and an upstanding end wall portion 1688 of the safety release 1684. See FIG. 81. The safety spring 1686 serves to bias the safety release 1684 in the distal direction and into contact with the safety yoke 1670 to prevent the safety yoke from being pivoted to an off position wherein the trigger 1664 may be actuated. Also in these variations, a rod clip 1690 may be attached to the adjustment shaft 1650 by and adjusting screw 1692 that extends through a slot (not shown) in the rod clip 1690. The rod clip 1690 may be so located on the adjustment shaft 1650 such that when the adjustment shaft 1650 has been axially positioned in its most proximal position which results in the maximum amount of desirable compression being applied to the tissue or in a position wherein the anvil 1700 has begun to clamp the tissue, but has not yet attained the predetermined maximum amount of compression force, the rod clip 1690 has contacted the upstanding end wall 1688 and moved it proximally a sufficient distance to move the distal end 1685 of the safety release 1684 out of

retaining engagement with the safety yoke **1670**. The surgeon may then pivot the safety yoke **1670** to the off position thereby enabling the trigger **1664** to be depressed.

Various embodiments of the invention may also be fitted with a staple form indicator **1676** that may be pivotally mounted within the handle assembly **1660** by a pivot pin **1678**. The staple form indicator **1676** may have a pointer end portion **1679** that is viewable through a viewing window **1663** (FIG. 77) formed in the handle assembly **1660**. The end portion **1679** may be biased in the distal direction by an indicator spring **1680**. As can be seen in FIG. 79, the staple form indicator **1676** may be formed with a tab **1682** that is oriented for engagement by a hooked end **1685** of a safety release **1684**. As the safety release **1684** is moved proximally in connection with the proximal movement of the adjustment shaft **1650**, the hooked end **1685** causes the staple form indicator **1676** to pivot in the proximal direction. An indicator plate (not shown) may be positioned within the window **1663** and so calibrated such the indicator **1676** cooperates with the indicator plate to indicate the amount of distance between the anvil **1700** and the cartridge **1616**.

One exemplary method of using the circular stapler **1600** will now be described with reference to FIGS. 85-88. When performing an anastomosis using a circular stapler, the intestine **1900** may be stapled using a conventional surgical stapler with multiple rows of staples being emplaced on either side of a target section (i.e., specimen) of intestine **1900**. FIG. 85 illustrates the liner staple lines **1910**, **1920**. The target section is typically simultaneously cut as the section is stapled. The target section has already been removed in FIG. 85. Next, after removing the target specimen, the surgeon inserts the anvil **1700** into the proximal portion **1902** of the intestine **1900**, proximal of the staple line **1910**. This is done by inserting the anvil head **1700** into an entry port cut into the proximal intestine portion **1902** or the anvil **1700** can be placed transanally, by placing the anvil **1700** on the distal end of the stapler **1600** and inserting the instrument through the rectum. Next, the surgeon attaches the anvil **1700** to the trocar tip **1644** of the stapler **1600** and inserts the anvil **1700** into the distal portion **1906** of the intestine **1900**. The surgeon may then tie the distal end **1904** of the proximal section **1902** of the intestine **1900** to the anvil shaft **1704** using a suture **1912** or other conventional tying device and also tie the proximal end **1908** of the distal intestine portion **1906** around the anvil shaft using another suture **1914**. See FIG. 86. The surgeon then begins to rotate the closure knob assembly **1800** in the clockwise direction to draw the anvil **1700** toward the cartridge **1616** supported in the staple driver **1614** to close the gap between the anvil **1700** and cartridge **1616** and thereby engage the proximal end **1908** of the distal intestine portion **1906** with the distal end **1904** of the proximal intestine portion **1902** in the gap "G" therebetween. See FIG. 87. The surgeon continues to rotate the closure knob assembly **1800** until the first and second friction pads **1840**, **1850** slip and the desired amount of compression (the desired gap G) is attained. When in that position, the surgeon may then pivot the safety yoke **1670** to the off position and fire the stapler **1600** by depressing the firing trigger **1664**. Depressing the trigger **1664** causes the compression shaft **1634** to drive the staple driver **1614** distally to drive the staples **1618** to be driven through both ends **1904**, **1908** of the intestine **1900**, thereby joining the portions **1902** and **1906** and forming a tubular pathway. Simultaneously, as the staples **1618** are driven and formed, the knife **1620** is driven through the intestinal tissue ends **1904** and **1908**, cutting the ends adjacent to

the inner row of staples **1618**. The surgeon then withdraws the stapler **1600** from the intestine and the anastomosis is complete.

FIGS. 89-95 illustrate another stapler embodiment **1600a** of the present invention. Stapler **1600a** may essentially employ the same components described above with respect to stapler **1600** except for the changes that will be discussed in detail below. For example, in this embodiment, a slip clutch assembly may not be employed. However, this embodiment may employ a closure actuator assembly **2000** that includes a proximal cap portion **2010** and a distal cap portion **2040** that are rotatably retained together.

More specifically, as shown in FIGS. 90 and 91, in various embodiments, the proximal cap portion **2010** may have a sleeve portion **2012** that is sized to extend over the outer wall portion **2044** of the distal cap portion **2040** and be retained thereon by virtue of an inwardly extending flange **2014** formed on the sleeve portion **2012**. Flange **2014** may be snapped over an outwardly protruding rim **2046** formed on the circumference of the wall portion **2044** of the distal cap portion **2040**. Such arrangement serves to attach the proximal cap portion **2010** to the distal cap portion **2040** while facilitating its rotation relative thereto. To facilitate ease of attachment, a beveled edge **2048** may be provided on the end **2041** of the wall portion **2044**.

As can also be seen in FIGS. 90 and 91, the distal cap portion **2040** may further have a cap hub portion **2050** that has a proximal end **2052** that may be rotatably received in a circular slot **2016** formed in the proximal cap portion **2010**. The slot **2016** may be sized relative to the cap hub portion **2050** such that the proximal cap portion **2010** can freely rotate around the cap hub portion **2050**. In addition, the proximal cap portion **2010** may have a protrusion **2018** that rotatably extends into an axial passage **2054** in the cap hub portion **2050** to provide additional rotational support to the closure knob assembly **2000**. As can be seen in FIG. 90, the proximal end **1741** of the proximal closure nut **1740** may be formed with a proximally extending tapered hub portion **1746** that is adapted to be nonrotatably received in the axial passage **2054** in the cap hub portion **2050**. The tapered hub portion **1746** may also be formed with a key or spline arrangement to non-rotatably affix the hub portion **1746** with the cap hub portion **2050**. Other fastener arrangements and methods may be employed to non-movably attach the hub portion **1746** of the proximal closure nut **1740** to the cap hub portion **2050**. Thus, rotation of the cap hub portion **2050** will cause the proximal closure nut **1740** and distal closure nut **1720** to also rotate in the manners described above and axially advance the adjustment shaft **1650** distally or proximally depending upon the direction in which the proximal and distal closure nuts are rotated.

Rotation of the proximal and distal closure nuts **1740**, **1720** is attained by rotating the proximal cap portion **2010** relative to the distal cap portion **2040**. The interaction between the proximal cap portion **2010** and the distal cap portion **2040** may be controlled by a variable force generating member **2060** that interconnects those components and serves to apply a resistive force to the proximal cap portion **2010** in relation to the amount of compression experienced by the tissue compressed between the anvil **1700** and the staple cartridge **1616**. In various embodiments, for example, the variable force generating member may comprise a spiral spring **2060**. In some embodiments, the innermost end **2062** of the spiral spring **2060** may be configured as shown in FIG. 92 and inserted into a retaining slot **2020** in the proximal cap portion **2010**. End **2062** of spring **2060** may also be attached to the proximal cap portion **2010** by other fastener arrangements. Likewise, the

outer end **2064** of the spring **2060** may be configured as shown in FIG. **92** and received in a retention slot **2045** formed in the distal cap portion **2040**. However, the outer end **2064** of spring **2060** may be attached to the distal cap portion **2040** by other suitable fastener arrangements.

In various embodiments, a reference indicator mark **2070** may be provided on the proximal cap portion **2010** such that it aligns with a corresponding initial mark **2072** on the outer wall **2044** of the distal cap portion **2040** when the stapler **1600a** is in the unadvanced or neutral position. See FIGS. **89** and **95**. When in that aligned position, the spiral spring **2060** may essentially be unloaded or it may be under a relatively small amount of load necessary to retain the proximal cap portion **2010** in that starting position. Rotation of the proximal cap portion **2010** in the clockwise "CW" direction will be transferred to the distal cap portion **2040** through the spring **2060** and to the proximal closure nut **1740** attached to the distal cap portion **2040**. Rotation of the proximal closure nut **1740** also causes the distal closure nut **1720** to rotate and axially draw the adjustment shaft in the proximal "PD" direction. When the adjustment shaft **1650** is drawn proximally, is also causes the anvil **1700** to move towards the cartridge because it is attached to the trocar tip **1644** which is attached to the adjustment shaft **1650** by means of the top and bottom tension bands **1636**, **1638** as was discussed above. As the anvil **1700** moves closer to the staple cartridge **1616** supported in the head **1610**, the tissue **1904**, **1908** clamped therebetween begins to compress and resist further travel of the anvil **1700** to the cartridge. See FIG. **93**. Such resistive compressive force also must be overcome by the spring load to enable the anvil **1700** to further compress the tissue **1904**, **1908** between the anvil **1700** and the cartridge **1616**.

In various embodiments, the amount of spring load ("L1") necessary to attain a minimum amount of tissue compression ("Min") may be determined as well as the amount of spring load ("L2") required to attain a maximum amount of tissue compression ("Max") may also be determined. In addition, the distance "D1" that the proximal cap portion **2010** must be rotated from the neutral position to generate spring load "L1" and the distance "D2" that the proximal cap portion **2010** must be rotated to generate spring load "L2" may be determined. The graph depicted in FIG. **94** illustrates an example of a relationship between these parameters. Those of ordinary skill in the art will appreciate that such relationships may change depending upon the spring used and various other factors such as, for example, frictional forces encountered by the moving components of the device.

As can be seen in FIG. **95**, a second indicator mark or indicia **2080** corresponding to the position of the proximal cap portion **2010** when it has been rotated to generate the minimum amount of compression force "Min" is provided on the outer wall **2044** of the distal cap portion **2040** such that the second indicia **2080** coincides with the reference indicator **2070** on the proximal cap portion **2010**. Likewise a third indicator mark or indicia **2082** may be provided on the outer wall **2044** of the distal cap portion **2040** such that the third indicia **2082** coincides with the reference indicator **2070** on the proximal cap portion **2010** when the proximal cap portion **2010** has been rotated to that position which generates the maximum amount of compression force "Max". See FIG. **95**. Those of ordinary skill in the art will recognize that a variety of different indicia arrangements may be employed without departing from the spirit and scope of the present invention. For example, the area **2084** on the outer wall **2044** of the distal cap portion **2040** between the second indicia member **2080** and the third indicia member **2082** may be painted or otherwise colored green to indicate to the surgeon that if the ref-

erence indicator **2070** is located in that region and acceptable amount of compression force may be attained.

Thus, in these embodiments, the spring **2060** provides a means for interrelating the amount of compression experienced by the tissue located between the anvil **1700** and the staple cartridge **1616** and the distance that the proximal cap portion **2010** must be rotated to attain that amount of compression. Such arrangement permits the use of reference indicators and indicia on the proximal and distal cap portions **2010**, **2040** to enable the surgeon to accurately determine when the anvil has been located in a position that will result in acceptable staple formation. These reference indicators and indicia can be so oriented to inform the surgeon when the anvil has been moved to a position that will result in a minimum amount of compression being applied to the tissue while still facilitating the formation of sealing staples. Likewise, such reference indicators and indicia may be so oriented to inform the surgeon that the anvil has been moved to a position that will result in a maximum amount of compression being applied to the tissue while still facilitating the formation of sealing staples.

As known in the art, surgical staples can be used to hold several layers of tissue together after the tissue has been resected, for example. Often, as described above, a surgical stapler is used to deform the staples from an undeployed shape into a deployed, i.e., deformed, shape. Referring to FIG. **27**, the staples, such as staples **83**, for example, include a base, or crown, and deformable legs extending therefrom. In use, the deformable legs are typically deformed toward the crown by an anvil in the surgical stapler. Referring to FIG. **27**, the amount of this deformation is usually dependent upon the thickness of the tissue being stapled. More particularly, if the tissue is thinner, the anvil is brought closer to the staple cartridge before the anvil contacts the tissue and, as a result, the staples will have less distance to be deployed before they are deformed against the anvil. For example, the legs of the staple on the left in FIG. **27** are inserted through thinner tissue while the legs of the staple on the right are inserted through thicker tissue and, as a result, the legs of the staple on the left are deformed more than the legs of the staple on the right. As a result of the foregoing, a common staple design can be readily adapted to various tissues having different thicknesses.

As described above, referring to FIG. **27**, the legs of staples **83** are bent toward the base, or crown, of the staple. More particularly, the ends of the legs are curled by the anvil of the stapler until the desired deformation is achieved. Stated another way, when the ends of the legs contact the anvil of the stapler, the ends are guided by the anvil such that the legs are continuously bent into an arcuate configuration until the staple is deformed into a "B" shape, for example. In embodiments where the staple has long legs, and/or embodiments where the staples are used in very thin tissue, the legs may be curled significantly such that their ends project outwardly from the staple. In these embodiments, the ends may be sharp and may impinge on surrounding tissue causing discomfort to the patient. To ameliorate this problem, the present invention includes staple **1300** which can be bent in segments, as opposed to a continuous arcuate shape as described above.

Similar to the above, referring to FIG. **96**, staple **1300** includes crown **1302** and deformable legs **1304** and **1306** extending therefrom. Legs **1304** and **1306** include first notches **1310**, second notches **1312**, and third notches **1313** therein. In use, referring to FIG. **105**, when ends **1308** of legs **1304** and **1306** contact pockets **1314** of anvil **1316**, ends **1308** can be guided toward each other, for example. As the staple is further driven toward anvil **1316** by sled driver **78**, referring to

staple **1300b**, legs **1304** and **1306** may bend significantly at first notches **1310**. Referring to FIG. 97, owing to the reduced cross-section of legs **1304** and **1306** at first notches **1310**, legs **1304** and **1306** are more susceptible to deformation at this location. For example, when legs **1304** and **1306** are bent at notches **1310**, first segments **1318** may bend at an approximately 90 degree angle, for example, with respect to second segments **1320** of legs **1304** and **1306**. In other embodiments, first segments **1318** may be bent at any suitable angle with respect to second segments **1320**.

Further to the above, referring to FIG. 98, second notches **1312** in legs **1304** and **1306** permit second segments **1320** to bend with respect to third segments **1322** at an approximately 90 degree angle, for example. In other embodiments, second segments **1320** may be bent at any other suitable angle with respect to third segments **1322**. Similar to the above, notches **1313** permit third segments **1322** to bend with respect to fourth segments **1325**. As a result of notches **1310**, **1312**, and **1313**, legs **1304** and **1306** may not be bent into a continuous curl as described above; rather, they can be bent into a segmented, rectangular configuration. As a result of the above, staples having long legs **1304** and **1306** may be deformed in a manner such that the ends of the deformable members do not extend outwardly from the staple, rather, they can be positioned intermediate legs **1304** and **1306** as illustrated in FIG. 99. While the legs of the illustrated staples in FIGS. 96-105 have three notches and four segments, various embodiments are envisioned which have additional, or less, notches and segments. Furthermore, while the segments of the staple legs described above are substantially straight, various embodiments are envisioned in which the segments are curved, curvilinear, or other otherwise suitably configured to achieve a desired shape.

To facilitate the bending of third segments **1322** with respect to fourth segments **1325**, for example, crown **1302** may include a forming surface, or anvil, for guiding and/or deforming legs **1304** and **1306** when they contact crown **1302**. More particularly, referring to FIGS. 99 and 101-104, as legs **1304** and **1306** are being deformed from the shape illustrated in FIG. 98 to the shape illustrated in FIG. 99, ends **1308** of deformable members **1304** and **1306** may contact crown **1302**. To guide ends **1308**, anvil **1323** of crown **1302** includes recesses **1324** which can direct ends **1308** to move outwardly as illustrated in FIG. 99 or in any other suitable direction. In various embodiments, recesses **1324** may not deform legs **1304** and **1306** significantly, however, in the illustrated embodiment, recesses **1324** are configured to deform legs **1304** and **1306** at an approximately 90 degree angle. In various embodiments, anvil **1316** of the stapler and anvil **1323** in crown **1302** can co-operate to deform staple **1300** into the shape illustrated in FIG. 99, for example, or any other suitable shape.

In various embodiments, although not illustrated, a forming surface, or anvil, can be included in staple cartridge **1326** in addition to, or in lieu of, anvil **1323** in crown **1302**. In these embodiments, anvil **1316** deforms legs **1304** and **1306** such that ends **1308** contact the recesses in stapler cartridge **1326**. Similar to the above, the staple cartridge recesses can be configured to guide and/or deform legs **1304** and **1306** when they contact stapler cartridge **1326**. In various embodiments, anvils on both crown **1302** and stapler cartridge **1326** can be utilized to deform and/or guide the staple. In the illustrated embodiment, crown **1302** includes material **1303** overmolded onto base **1301**. As discussed in greater detail below, material **1303** can be comprised of a plastic material, for example, a bioabsorbable material, and/or a non-bioabsorbable material. In at least one of these embodiments, the material **1303** is

formed around a single continuous wire comprising base **1301** and deformable members **1304** and **1306**. In other embodiments, deformable members **1304** and **1306** can include separate deformable members embedded in plastic material **1303**. Further, in various embodiments, the wire comprising base **1301** can be deformed to provide the recesses and anvils described above.

Referring to FIGS. 106 and 107, similar to the above, the staple, in various embodiments, can include several necked down sections in the staple legs which can be configured to cause the staple legs to deform and/or buckle at the necked down sections. More specifically, staple **1340** can include several necked-down or tapered sections **1342** which allow staple legs **1344** to deform in segments as described above. Tapered sections **1342**, similar to notches **1310**, **1312**, and **1313**, provide a stress concentration area. Stress concentration areas are typically locations in which a loaded member, for example, will fail. Stated another way, stress concentration areas may magnify the stress in a particular area of a loaded member causing the loaded member to yield, or plastically strain, at the stress concentration area before the remainder of the loaded member plastically strains. As used herein, the term "yield" generally refers to the point of maximum stress and/or strain above which a material will no longer behave in a completely elastic manner. However, various embodiments are envisioned in which the materials used herein do not have a traditional yield point, for example. These materials can include materials which strain plastically as soon as they are stressed and/or super-elastic materials which do not have a discernable yield point. These materials can include shape memory alloys, such as Nitinol, for example, that allow for large strain deformations during the above-described forming processes. Typically, engineers are charged with eliminating stress concentration areas to achieve a desired goal; however, according to the teachings of the present invention, stress concentration areas can be utilized to achieve the above-described goals.

In various embodiments, referring to FIGS. 108-110, staple **1329** includes base portion **1331** and two deformable legs **1333** extending therefrom. Legs **1333** can each include a first portion **1335** having a substantially round cross-section and a second portion **1337** having a substantially flat cross-section. In at least one embodiment, legs **1333** and base **1331** are comprised of a metal wire that is coined, or formed, on its ends to create substantially flat portions **1337**. As known in the art, coining, or forming, a metal wire may be performed with a stamping press before and/or after, the wire is bent into the "U" shape illustrated in FIG. 108. Referring to FIG. 110, legs **1333** are configured such that flat portions **1337** can be bent to secure tissue within the staple while round portions **1335** can remain substantially unbent. In use, as a result, staple **1329** can be used to secure thicker tissues. More specifically, owing to substantially unbent portions **1335**, thicker tissues can be accommodated between portions **1335** while flat portions **1337** can be bent to retain the tissue therebetween. The amount in which flat portions **1337** are deformed is typically dependent upon the thickness of the tissue captured in the staple.

In various embodiments, referring to FIG. 111, staple **1441** can include deformable legs **1443** which have a tapered configuration. More particularly, staple legs **1443** can include a base portion **1444** that has a larger cross-section than the cross-section of tip portion **1445**. In use, similar to the above, staple **1441** can accommodate thicker tissues as, owing to the thicker cross-section of base portions **1444**, base portions **1444** may remain substantially unbent while tip portions **1445** are bent to retain the tissue in the staple. In other various

embodiments, referring to FIG. 112, staple 1446 can include several stepped portions 1447 and 1448 which allow some portions of legs 1449 to be bent, some portions to be only partially bent, and other portions to remain substantially unbent. The suitable amount and configurations of the stepped portions may be selected to accommodate the type and/or thickness of the tissue being secured.

Referring to FIGS. 113 and 114, staple 1350, similar to staple 1340, includes crown 1302 and deformable legs 1344. Staple 1340, as described above, in at least one embodiment, is configured to compress tissue between deformable legs 1344 and crown 1302. However, in applications in which the tissue is very thin, for example, sufficient compression of the tissue between deformable legs 1344 and crown 1302 may be difficult to achieve and a gap between the tissue and legs 1344, for example, may exist. For these applications, it may be desirable to include an additional member intermediate the tissue and the deformable members and/or crown which not only fills the gap, but compresses the tissue against at least one of the crown and/or deformable members.

Staple 1350, referring to FIGS. 113 and 114, can include, in various embodiments, deformable, or compressible, member 1352. As described above, referring to FIG. 114, compressible member 1352 can bias tissue 1353 against deformable legs 1344. As a result of this compression, the lumens, or vessels, in tissue 1353 can be compressed and thereby slow the flow of blood therethrough. In at least one embodiment, compressible member 1352 is entirely elastic after it has been compressed, i.e., the addition of, or the removal of, any stress onto compressible member 1352 will result in a linearly corresponding increase, or decrease, in strain thereof. Stated in another way, in these elastic embodiments, compressible member 1352 can substantially act like a spring. However, in at least one embodiment, compressible member 1352 can be crushable, i.e., after it has been compressed, at least a portion, if not all, of compressible member 1352 is permanently deformed and the addition of, or removal of, any stress onto compressible member 1352 does not necessarily result in a linearly corresponding strain. In various embodiments, compressible member 1352 can be comprised of foam. The foam can be absorbable or non-absorbable. The foam can be comprised of synthetic materials and/or mammalian-derived materials including, but not limited to, polyglycolide trimethylene carbonate copolymer, polyglycolic acid, caprolactone/glycolide, EPTFE, and bovine pericardium. Further, in at least one embodiment, compressible member 1352 may include a first portion which is elastically deformable and a second portion which is plastically deformable.

Referring to FIGS. 115 and 116, staple 1360 can include collapsible spring member 1362. Collapsible spring member 1362 can include a plurality of first elastic members 1363 and second elastic members 1364. Each first elastic member 1363 can include an arcuate profile which includes projections 1365 extending therefrom which are sized and configured to contact corresponding projections 1366 extending from each second elastic member 1364. More specifically, first elastic members 1363 and second elastic members 1364 are configured such that they can be stacked upon each other and, when a compressive load is applied to such a stack, the first and elastic members can flatten and thereby "collapse" the stack of elastic members. In the illustrated embodiment, collapsible spring member 1362 further includes fasteners 1367 and 1368. Referring to FIG. 115, fasteners 1367 can connect the central portions of adjacent first elastic members 1363 and second elastic members 1364 to prevent the elastic members from becoming dislodged or misaligned with respect to each other. Similarly, fastener 1368 can prevent collapsible spring

member 1362 from becoming dislodged with respect to crown 1302. In use, collapsible spring member 1362 can provide a compressive load to tissue in between said deformable members and said crown.

Referring to FIGS. 117 and 118, staple 1370 can include cantilever spring 1372. Cantilever spring 1372 includes first end 1373 attached to crown 1302 and second end 1374 which is free to move with respect to first end 1373. In use, when tissue is compressed between spring 1372 and deformable legs 1344, spring 1372 can apply an upwardly-directed biasing, or compressive, force against the tissue. More particularly, as deformable legs 1344 are deformed and pushed against the tissue, second end 1374 of spring 1372 can move downwardly with respect to first end 1373. As a result of this deflection, spring member 1372 stores potential energy and acts to release this potential energy by applying an upward force against the tissue, thereby compressing the tissue between spring member 1372 and deformable legs 1344. In an alternative embodiment, referring to FIGS. 119-121, spring member 1382 of staple 1380 can have first and second ends, 1382 and 1384, respectively, attached to crown 1302. In at least one embodiment, springs 1372 and 1382, for example, can be integrally molded with crown 1302. In these embodiments, springs 1372 and 1382 can be comprised of a dissolvable, bioabsorbable, or biofragmentable material such that, as the material dissolves, the biasing force of springs 1372 and 1382 can decrease throughout the healing process. As a result, a larger compressive force can be applied during the initial healing stages when the restriction of blood loss is important and a smaller compressive force can be applied during the later healing stages when tissue regeneration is important wherein the smaller force permits expansion and growth of the tissue within the staple.

In other various embodiments, although not illustrated, the tissue can be positioned, and compressed between, the compressible member and the crown of the staple. In these embodiments, the deformable members are deformed against the compressible member which, as a result, is compressed between the deformable legs and the tissue.

Referring to FIGS. 122 and 123, staple 1400 includes crown 1402, first deformable member 1404, and second deformable member 1406. Deformable members 1404 and 1406 each include a base 1408, a deformable leg 1410, and a second leg 1412 which, in the illustrated embodiment, are comprised of a single continuous wire. In other various embodiments, staples 1400 may be configured in any other suitable manner to achieve the goals of the invention described herein. In the illustrated embodiment, members 1404 and 1406 are connected together by a material that is overmolded onto the bases 1408 of members 1404 and 1406. In various embodiments, the material can include a dissolvable, bioabsorbable, or biofragmentable material such as Vicryl and PDS from Ethicon, Inc., for example. As used herein, the terms dissolvable, bioabsorbable, and biofragmentable all generally refer to materials that can be at least partially assimilated by the body after being implanted into a patient, for example.

In use, staple 1400 can be inserted into the soft tissue of a person, for example, via a stapler and can be deformed into the configuration illustrated in FIG. 124. More particularly, in the illustrated embodiment, deformable members 1404 and 1406 can be deformed by the anvil of the stapler such that ends 1411 of legs 1410 are brought into close proximity to crown 1402. Once staple 1400 is implanted into the tissue, crown 1402 may begin to break down, dissolve and weaken. More particularly, referring to FIG. 125, the bioabsorbable material of crown 1402 may deteriorate to the point where

first member **1404** and second deformable member **1406** become disconnected from each other as illustrated in FIG. **126**. Once first member **1404** and second member **1406** have become disconnected, they can move relative to one another. The time required for crown **1402** to sufficiently dissolve may depend on the material used and/or the size of crown **1402**. Polyglatin **910** material, sold under the trade name Vicryl, for example, may dissolve in 7-14 days.

In various embodiments, dissolvable crown **1402** may provide several therapeutic advantages. For example, when staple **1400** is initially deployed, deformable members **1404** and **1406** may significantly compress the tissue within the staple against crown **1402**. In some applications, this compression may be desirable to limit bleeding from the tissue. As crown **1402** deteriorates, the gap between the deformed members **1404** and **1406** and crown **1402** may increase thereby relaxing the compressive forces acting on the tissue. In some applications, relaxing the compression forces during the healing process may allow the tissue to slowly expand and return to its normal thickness over a period of time. In some embodiments, crown **1402** can be coated with a hydrophilic material that initially expands to compress the tissue captured within the staple before dissolving away thereafter. In these embodiments, the hydrophilic material expands by absorbing water from the surrounding tissue and fluids. In addition to the above, staple **1400**, when it is inserted into the tissue, may be very stiff and, if several staples are inserted into the tissue, the tissue may not be permitted to move and expand during the healing process. However, after crowns **1402** of staples **1400** have dissolved, the deformable members **1404** and **1406** of the staples may be able to move relative to each other while still holding the underlying tissue together.

In various embodiments, deformable members **1404** and **1406** may be comprised of a substantially non-dissolvable or non-bioabsorbable material. In other embodiments, at least one of deformable members **1404** and **1406** may be comprised of a dissolvable, bioabsorbable, or biofragmentable material such as magnesium or iron, for example. In at least one embodiment, the iron is pure iron. In either event, the dissolvable material of members **1404** and **1406** can be selected such that they dissolve at the same rate as, slower than, or faster than the dissolvable material of crown **1402**. For example, the material of crown **1402** can be selected such that it completely dissolves away while deformable members **1404** and **1406** are still holding tissue together. Further, in various embodiments, the material of first deformable member **1404** can be selected such that it dissolves faster than the material of second deformable member **1406**. Accordingly, the deformable members of these embodiments may allow for a staggered release of the tissue. Further, in various embodiments, at least two adjacent staples **1400**, as described in greater detail below, can be connected by a bridge before and/or after the staples have been deployed into the tissue. In these embodiments, a first staple can be comprised of bioabsorbable materials that dissolve away at a faster rate than the materials of a second staple attached thereto. Similarly, the bridge connecting the staples can be comprised of materials that dissolve away at the same rate, and/or a different rate, than the first and second staples. In these embodiments, the first staples can dissolve away before the second staples allowing for a staggered release of the tissue.

The staples described above can be used to approximate tissue, i.e., the staples can secure resected or damaged tissue such that the strength of the resected or damaged tissue approximates that of healthy tissue. To this end, a method of approximating tissue can include suturing tissue with a surgical staple comprised of a dissolvable material and a non-

dissolvable material to approximate tissue in a first state, and dissolving the dissolvable material to cause the remaining non-dissolvable material to approximate the tissue in a second state. In at least one embodiment, the tissue approximation in the second state is more flexible than in the first state.

In addition to the above, referring to FIG. **132**, crown **1402** may be comprised of at least two overmolded or co-molded materials. More particularly, crown **1402** may be comprised of a first material **1435** overmolded onto deformable members **1404** and **1406** and a second material **1436** overmolded onto second material **1436**, for example. In this embodiment, second material **1436** can be configured to dissolve away quickly thereby allowing deformable members **1404** and **1406** to separate from each other early on in the healing process. However, first material **1435** can be selected to dissolve at a slower rate than second material **1436** in order for crown **1302** to continue to provide a compressive force on the tissue even after second material **1436** has completely dissolved away. In at least one embodiment, first material **1435** can be injection molded onto deformable members **1404** and **1406** and then permitted to cure, and/or substantially solidify, before second material **1436** is injection molded onto first material **1435**. In other various embodiments, first material **1435** and second material **1436** can be injection molded onto deformable members **1404** and **1406** at substantially the same time or in rapid succession. In these embodiments, the first and second materials can chemically bond together to provide sufficient strength therebetween so that the staple may be handled without the first and second materials separating from one another. In other embodiments, the first and second materials can form mechanically interlocking features to accomplish the same result.

In the embodiment illustrated in FIG. **123**, crown **1402** may include reduced cross-section **1414** intermediate portions **1416** and **1418**. In use, intermediate section **1414**, as it has a smaller cross-section than portions **1416** and **1418**, may completely dissolve away before sections **1416** and **1418** thereby allowing first member **1404** to become unconnected from second member **1406** before the entirety of crown **1402** has dissolved (FIG. **125**). In at least one embodiment, the cross-sections of sections **1414**, **1416**, and **1418** can be selected such that deformable members **1404** and **1406** become unconnected at a desired stage in the healing process. In at least one embodiment, referring to FIG. **133**, crown **1402** can include score marks **1437** which reduce the thickness of crown **1402** in the scored areas. In these embodiments, the score marks may be formed when crowns **1402** are overmolded onto deformable members **1404** and **1406** or formed by a cutting tool thereafter. As a result of score marks **1437**, crown **1402**, as it dissolves, can break up into several small pieces which are, in some circumstances, more easily absorbable by the body. In at least one embodiment, referring to FIG. **134**, crown **1402** may include a plurality of pockets **1438** intermediate raised portions **1439**. In use, the material intermediate raised portions **1439** may dissolve away leaving behind a lattice, or grid, of raised portions **1439** intermediate deformable members **1404** and **1406**.

In at least one embodiment, crown **1402** is also comprised of at least one therapeutic drug. In these embodiments, as the dissolvable material deteriorates, the therapeutic drug can be absorbed by the surrounding tissue. In some embodiments, the drug is dispersed throughout the dissolvable material such that the drug is steadily released during the healing process, however, in other embodiments, the therapeutic drug may be unevenly dispersed throughout the dissolvable material, or layered within and/or on the material to provide an increased dosage of the drug at a particular stage in the healing process.

In at least one embodiment, having an absorbable staple with an absorbable insulator reduces the possibility of arcing along a row of staples when an electrocautery device is used in situ, for example. The absorbable insulators, or crowns, on the staples substantially prevent an electrical current from jumping between staples as the top of each staple is not electrically conductive under normal operating conditions. As a result, the possibility of damaging tissue is reduced.

In use, as described above, and referring to FIGS. 127 and 128, deformable members 1404 and 1406 of staple 1400 are deformed by anvil 1420 of stapler 1422. More particularly, ends 1411 of members 1404 and 1406 are received within recesses 1424 in anvil 1420 and are guided toward crown 1402 as members 1404 and 1406 are deformed by anvil 1420. Referring to FIGS. 129 and 129A, recesses 1424 can include a configuration which causes the ends of members 1404 and 1406 to bend out of plane with members 1412 and bases 1408. More particularly, referring to FIGS. 130 and 131, each recess 1424 includes several planar surfaces oriented to initially deflect end 1411 laterally, and then downwardly, to curl the top portion of deformable leg 1410 alongside the bottom portion of deformable leg 1410 as illustrated in FIG. 131. Referring to FIGS. 130 and 131, recess 1424 includes surfaces 1426 and 1428 which form vertex 1430 therebetween. Surfaces 1426 and 1428, and vertex 1430, are configured to receive end 1411 of deformable member 1406, for example. After sufficient pressure is applied by anvil 1420, leg 1410 of deformable member 1406 is curled within vertex 1430. Thereafter, as leg 1410 is further deformed, leg 1410 also contacts vertex 1432 which is intermediate surfaces 1428 and 1434 of recess 1424. As illustrated in FIG. 131, vertex 1432 assists in deforming member 1406 into a desired shape. While the above anvils are described in connection with staples 1400, these anvils can be used to deform other differently-configured staples including the suitable staples disclosed in this application.

Referring to FIGS. 96 and 97, staple 1300 includes an integral staple crown and driver. More particularly, referring to FIG. 105, crown 1302 is configured to be directly driven by cam sled 78. In use, as described in detail above, cam sled 78 is progressed through staple cartridge 1326 from the position illustrated in FIG. 105 toward distal end 1327 of staple cartridge 1326. As cam sled 78 is moved in this direction, staples 1300 are successively lifted by cam sled 78 toward anvil 1316. In previous surgical staplers, a separate driver was positioned intermediate the cam sled and the staple. However, the present invention simplifies these previous systems by including features in crown 1302 which allow staples 1300 to be directly lifted by cam sled 78. More particularly, referring to FIGS. 96 and 97, crown 1302 includes beveled surfaces 1328 which are configured to co-operate with angled surface 1330 of cam sled 78 such that crowns 1302 slide up cam surface 1330. In the illustrated embodiment, both beveled surfaces 1328 and cam surface 1330 are oriented at an approximately 30 degree angle with respect to the horizontal. As a result, in the present embodiment, beveled surface 1328 may sit flushly on cam surface 1330, however, embodiments are envisioned in which beveled surfaces 1328 and cam surface 1330 are not oriented at the same angle. Furthermore, the present invention is not limited to embodiments having 30 degree angles. On the contrary, any suitable angle, or angles, can be used.

Referring to FIGS. 96 and 97, base 1301 of staple 1300, in the illustrated embodiment, is embedded in crown 1302. More particularly, crown 1302 can be overmolded onto base 1301 such that crown 1302 tightly surrounds base 1301 and wherein, in the present embodiment, base 1301 is enveloped

or enclosed by crown 1302. In other various embodiments, crown 1302 may be separately manufactured and then assembled to base 1301. In either event, base 1301 and/or deformable members 1304 and 1306 can be at least partially embedded into crown-driver 1302. As a result, staple 1300 can include larger deformable members 1304 and 1306 than in previous designs. In these embodiments, as a result of the above, staple 1300 may accommodate larger tissues intermediate the deformable members and tissue-contacting surface 1336 of crown 1302. In one embodiment, crown-driver 1302 may be comprised of a dissolvable or bioabsorbable material, as described above, that, as it dissolves, allows the tissue compressed within staple 1300 to expand and grow. In various embodiments, as described above, crown-driver 1302 may be comprised of, or coated by, a hydrophilic material that expands when exposed to water in the body to further compress the tissue in the staple. Further, similar to the above, crown-driver 1302 may be configured to increase the contact area between crown 1302 and the tissue. In some embodiments, increasing this contact area reduces the localized stress on the tissue surface which may reduce the possibility of tissue necrosis, for example.

As indicated above, an integral staple crown and driver may reduce the quantity of components needed to deploy the staples. As a result, embodiments in accordance with the present invention may reduce the cost and/or manufacturing time to produce the stapling systems. Further, eliminating the separate driver components may reduce the possibility of misalignment between the staples and the cam sled.

In an alternative embodiment of the present invention, referring to FIG. 135, staples 1450 can each include a crown 1451 and two deformable legs 1452 extending therefrom. Referring to FIG. 135, the crowns of staples 1450 can be connected together by bridge 1455. Similar to the above, crowns 1451 and bridge 1455 can be integrally molded onto staple legs 1452. Also similar to the above, crowns 1451 can include beveled surfaces 1453 which, referring to FIG. 139, can be configured to cooperate with angled surface 1454 of cam driver 1462. As above, cam driver 1462 is configured to successively raise staples 1450 toward an anvil positioned opposite deck 1456 of staple cartridge 1457. As discussed in greater detail below, bridges 1455 can be configured to connect staples 1450 even after they have been deployed or, alternatively, staple cartridge 1457 can include shears which break bridges 1455 and separate staples 1450 when they are deployed.

Staple cartridge 1457, referring to FIGS. 136-138, further includes cavities 1458 configured to receive staples 1450. In at least one embodiment, cavities 1458 include keys 1459 which are sized and configured to fit within slots 1460 in crowns 1451. More particularly, slots 1460 and keys 1459, in the present embodiment, are configured to substantially limit the motion of staples 1450 with respect to staple cartridge 1457 to a substantially linear motion, i.e., in the present embodiment, an upwardly and/or downwardly motion. As a result of these features, the possibility of staples 1450 becoming bound within or misaligned with respect to cavities 1458 can be reduced. In alternative embodiments, cavities 1458 can include slots and staples 1450 can have keys.

Although surfaces 1453 have been described herein as being beveled, surfaces 1453 are not limited to flat surfaces. On the contrary, various embodiments are envisioned in which surfaces 1453 are curved, radiused, curvilinear, and/or include several sections having various configurations. In either event, surfaces 1453 are configured to co-operate with cam sled 1462 such that staples 1450 are deployed as described above. Similarly, surface 1454 of cam sled 1462 is

not limited to a flat surface. On the contrary, surface 1454 can be curved, radiused, curvilinear, and/or have any other suitable configuration.

Staple cartridge 1500, referring to FIG. 140, includes recesses 1502 for receiving staple strips 1504. Referring to FIGS. 140 and 141, staple strips 1504 include several staples 1506 connected together by bridges 1508. Recesses 1502 include several pockets 1510 which are sized and configured for receiving staples 1506 therein. In at least one embodiment, staples 1506 include deformable members 1512 which are sized and configured to be biased against the sidewalls of notches 1514 in recesses 1502. More particularly, deformable members 1512 can be configured to create a press-fit between staples 1506 and pockets 1510 such that staple strips 1504 remain seated within recesses 1502 under normal usage conditions. However, in the present embodiment, staple strips 1504 can be removed from recesses 1502 with a moderate application of force.

As illustrated in FIG. 140, recesses 1502 open to top surface 1516 of staple cartridge 1500 such that staple strips 1504 can be inserted into staple cartridge 1500 by aligning strips 1504 with recesses 1502 in top surface 1516 and pressing them into the position illustrated in FIG. 141. Referring to FIG. 141, recesses 1502 further include recess portions 1518 intermediate adjacent pockets 1510 which are sized and configured for receiving bridges 1508. In the embodiment illustrated in FIGS. 140-143, bridges 1508 are configured such that adjacent staples 1506 can move with respect to each other when being inserted into pockets 1510. Accordingly, bridges 1508 can accommodate dimensional differences, and/or manufacturing tolerances, in the alignment of strips 1504 with recesses 1502. More particularly, each bridge 1508 can include a curved portion 1520 configured to allow portions 1522 of bridge 1508 to move with respect to each other.

In the illustrated embodiments, the deformable members of each staple 1506 comprise a single continuous wire that can be bent into a "U" and/or "V" shape. Crowns 1513, in the present embodiment, can be overmolded onto a portion of these wires such that the wires are embedded into and supported by crown 1513. In addition, as illustrated in FIG. 143, bridges 1508 can be integrally molded with crowns 1513 when crowns 1513 are overmolded onto the wire. As a result, bridges 1508 and crowns 1513, in the present embodiment, can comprise an integral, continuous body of plastic, for example. Although not illustrated, bridges 1508 and crowns 1513, in various embodiments, may be molded as a separate component, or components, that are attached to the staples. In these embodiments, the wires of the staples can be press-fit and/or glued into recesses in the separately molded components, for example.

In use, referring to FIG. 144, as sled 78 is moved forward, sled 78 lifts staples 1506 upwardly toward an anvil positioned opposite top surface 1516. Owing to the angled orientation of surface 1523 of sled 78, staples 1506a-1506e, for example, are incrementally lifted in successive order. More particularly, staples 1506a and 1506b, while they are being lifted by sled 78, may be lifted to different relative heights with respect to surface 1516 at any given moment. To accommodate this difference in relative position, bridge 1508a can be flexible such that it does not break as staple 1506a is being deployed. Bridge 1508a, in the embodiment illustrated in FIG. 144, can be configured such that it remains attached to staples 1506a and 1506b during the deployment thereof and, in addition, during the initial healing process of the patient.

In other various embodiments, referring to FIGS. 145-147, staples 1506 can be connected together by bridges 1526 to form staple strips 1528. Similar to bridges 1508, bridges 1526

can be integrally formed with crowns 1513 when crowns 1513 are overmolded onto deformable members 1512 as described above. However, bridges 1526, unlike bridges 1508, can be configured such that they break away from at least one of the two adjacent staples 1506 that they connect. More particularly, referring to FIGS. 146 and 147, bridges 1526 can include notches 1530 therein which are configured to reduce the cross-sectional thickness, and strength, of bridges 1526. In use, referring to FIG. 147, as staple 1506a is lifted upwardly with respect to staple 1506b, bridge 1526a can break away from staple 1506a. Stated another way, when staple 1506a is lifted upwardly, the stress created within bridge 1526a by pulling staple 1506a away from staple 1506b may cause bridge 1526a to break, especially in the portion of bridge 1526a having notch 1530 therein.

In the illustrated embodiment, bridge 1526a may remain attached to staple 1506b after it has been deployed. In other embodiments, bridge 1526a may remain attached to staple 1506a. In either event, notches 1530 can be designed such that bridges 1526 remain attached to a desired staple. In other embodiments, bridges 1526 may separate from both adjacent staples 1506 and fall into a cavity (not illustrated) within staple cartridge 1500, and/or sled 78. In these embodiments, the separated bridges 1526 may be removed from the stapler by removing the staple cartridge and/or removing them through an access panel in either the staple cartridge and/or the sled. In various embodiments, notches 1530 are not included in every bridge 1526. In these embodiments, several staples may remain attached to each other after being deployed while other staples may be detached. In these embodiments, the stiffness of the row of staples, when inserted into the tissue, can be controlled by selectively alternating whether the staples are attached or detached.

Referring to FIG. 146, bridges 1526 may include a substantially flat top surface 1532 which is substantially flush with top surfaces of crowns 1513. Bridges 1526 may further include a substantially arcuate surface, or lobe, 1534 in the bottom of bridges 1526 such that the thickest portions of bridges 1526 are adjacent to staples 1506. As a result of this configuration, the overall deflection of staple strip 1528 may be reduced making staple strip 1528 easier to insert into the staple cartridge. In other embodiments, referring to FIGS. 148-150, bridges 1536 may have lobes 1534 which face upward, i.e., in the opposite direction that they face on bridges 1526. In lieu of the configurations of bridges 1526 and 1536 which have a flat surface 1532, the bridges may comprise an arcuate configuration on both sides of the bridge. In these embodiments, similar to the embodiment in FIGS. 142 and 143, the bridges may deflect to permit some relative movement between adjacent staples 1506.

In various other embodiments, referring to FIGS. 151-157, the staple strips may be loaded into the staple cartridge from the bottom of the staple cartridge. For example, referring to FIGS. 155-157, staple cartridge 1550 includes cavities 1552 and 1554 which are sized and configured for receiving staple strips 1540 and 1542, respectively. In use, staple strips 1540 and 1542 are aligned with openings 1555 and 1557 in bottom surface 1551 and are inserted into cavities 1552 and 1554, respectively. In various embodiments, staple strips 1540 and 1542 may be configured such that they are press fit into cavities 1552 and 1554. In these embodiments, similar to the above, deformable members 1512 could engage the sidewalls of the cavities to retain staple strips 1540 and 1542 in staple cartridge 1550. In various embodiments, crowns 1513 and/or bridges 1538 of staple strips 1540 and 1542 can be dimensioned such that they engage the sidewalls of cavities 1552 and 1554 in a friction-fit manner. In other embodiments,

staple cartridge 1550 and staple strips 1540 and 1542 may include co-operating detent features which retain the staple strips in the staple cartridge. Once inserted into the cavities, staples 1541 of staple strips 1540 and 1542 can be positioned such that a portion of their deformable members 1512 extend through openings 1559 and 1561 in top surface 1553. Deformable members 1512 of staples 1541, as illustrated in FIG. 151, can extend substantially perpendicularly from crowns 1513.

Similar to the above, referring to FIGS. 155 and 156, staple strips 1540 and 1542 can be advanced upward through cavities 1552 and 1554 toward an anvil positioned opposite top surface 1553 from a first position illustrated in FIG. 155 to a second position illustrated in FIG. 156. When staple strips 1540 and 1542 are advanced into the position illustrated in FIG. 153, bridges 1538 may be pressed against shears 1560 of staple cartridge 1550. Thereafter, the staple strips may be pushed further upward causing shears 1560 to break bridges 1538 away from one or more of staples 1541, as described above. Referring to FIG. 154, shears 1560 in cavity 1552 include projections 1562 which extend therefrom and are configured to break bridges 1538 away from crowns 1531 at locations 1564 (FIG. 151).

In any of the embodiments described herein, the material overmolded onto the staples to form crowns 1513 and bridges 1526, and/or bridges 1508, may be comprised of a dissolvable, bioabsorbable or biofragmentable material. Further, similar to the above, in various embodiments, the bioabsorbable material may include at least one therapeutic drug mixed therein or coated thereon, for example. Similar to the above, in various embodiments, drivers may be connected to, and/or integrally molded with, the crowns of the staples.

In alternative embodiments, the staples may be connected in "puck" configurations in lieu of strips, for example. In various embodiments, referring to FIG. 158, staple pucks 1571 and 1572 include staples 1506 which are interconnected by bridges 1574 and 1575. Staple pucks 1571 have five staples 1506 which are interconnected by two bridges 1574 and two bridges 1575. As illustrated in FIG. 158, bridges 1575 connect adjacent staples 1506 such that the tops of their crowns 1513 are substantially flush with each other, however, bridges 1574 connect adjacent staples 1506 such that the top of their crowns 1513 are vertically offset from each other. Similarly, staple pucks 1572 include four staples 1506 which are interconnected by two bridges 1574 and two bridges 1575.

Referring to FIGS. 159 and 159A, staple cartridge 1576 includes cavities 1577 which are sized and configured for receiving staple pucks 1571, and cavities 1578 which are sized and configured for receiving staple pucks 1572. Referring to FIG. 160, staple cartridge 1576 further includes drivers 1579 and 1580 which are sized and configured for supporting staple pucks 1571 and 1572, respectively, thereon. More specifically, referring to FIGS. 161-163, drivers 1579 and 1580 can include shears 1581 upon which staples pucks 1571 and 1572 are supported. After being inserted into cavities 1577 and 1578, referring to FIG. 163, bridges 1574 and 1575 are positioned over shears 1581. In use, as described above, drivers 1579 and 1580 are lifted toward deck 1582 of staple cartridge 1576 by a cam sled. However, referring to FIG. 163, once drivers 1579 and 1580 contact bridges 1574 and 1575, and the upward movement of staple pucks 1571 and 1572 is prohibited by staple cartridge 1576, further upward movement of drivers 1579 and 1580 causes shears 1581 to break bridges 1574 and 1575, thereby separating staples 1306. Once bridges 1574 and 1575 have been broken, support surfaces 1582 of drivers 1579 and 1580 are configured to push

staples 1306 upwardly toward an anvil, as described above. Referring to FIGS. 164 and 164A, an alternative staple cartridge 1583 is illustrated having recesses sized and configured for receiving alternate configurations of the staple pucks.

In at least one alternative embodiment of the present invention, referring to FIGS. 165 and 166, staple pucks 1584 and 1585 can be configured such that bridges 1586 interconnecting staples 1587, for example, include shears 1588 extending therefrom. In the present embodiment, referring to FIG. 167, shears 1588 can be configured to dissect deck 1589 of staple cartridge 1590. More particularly, as staple pucks 1585 are raised by cam sled 1591, for example, shears 1588 can break through deck 1589 such that pucks 1585 can be raised above deck 1589 when deployed. As a result, staples 1587 can be completely deployed from staple cartridge 1590 before staple cartridge 1590 is removed from the surgical site. In alternative embodiments, although not illustrated, the staple cartridge can also include shears which detach staples 1587 from bridges 1586, and/or shears 1588, after shears 1588 have dissected staple cartridge deck 1589. Similar to the above, bridges 1589 can include beveled surfaces 1592 which are configured to co-operate with cam sled 1591.

Referring to FIG. 168, staples 1465 can each include a first deformable leg 1466, a second deformable leg 1467, and a base 1468 connecting deformable legs 1466 and 1467. Unlike previous staples which have a base that is substantially coplanar with its legs, base 1468 can extend in at least one direction that is transverse to a plane defined by legs 1466 and 1467. More particularly, base 1468 can include first portion 1469 and second portion 1470 which extend laterally from legs 1466 and 1467 and form an angle therebetween. In the present embodiment, referring to FIG. 169, first portion 1469 forms an approximately 90 degree angle with respect to second portion 1470. However, the present invention is not limited to 90 degree angles; rather, any suitable angle may be used. More particularly, the angle between first portion 1469 and second portion 1470 may, in some embodiments, be greater than 90 degrees and may, in other embodiments, be less than 90 degrees. Furthermore, in other embodiments, base 1468 may include several substantially linear segments and/or curved sections.

Staple 1465 can further include crown 1471 overmolded onto base 1468. More particularly, owing to the configuration of base 1468 as described above, crown 1471 can also extend transversely with respect to the plane defined between legs 1466 and 1467. Referring to FIGS. 168 and 169, crown 1471 can include tissue-contacting surface 1472 which is sized and configured for supporting tissue thereon. Tissue-contacting surface 1472, owing to the configuration of crown 1471, can be larger than the tissue contacting surfaces of previous staples. Accordingly, the larger contact surface can reduce the localized pressure acting on the tissue captured within the staple. As known in the art, reducing this localized pressure can reduce the possibility of tissue necrosis without reducing the compressive force acting on the tissue. Stated another way, the pressure acting on the tissue is a function of the force acting on the tissue divided by the area in which it acts. Increasing the area can reduce the localized pressure while not reducing the clamping force applied by the staple.

Further, owing to the configurations of base 1468 and crown 1471, the larger surface area of crown 1471 can improve the stability of crown 1471, and the surrounding tissue, after the staple has been deployed into the tissue. More particularly, after previous staples are deployed, the relatively-narrow crowns of these previous staples may not prevent the staples from rocking with respect to the tissue or straining the tissue surrounding the staple. Staples 1465,

owing to the configuration of crown **1471**, can reduce, and possibly eliminate, these previous problems. More specifically, owing to larger contact surface **1472**, crown **1471** is more stable, i.e., it is less likely to rotate with respect to the tissue. Furthermore, the crowns of previous staples, owing to their narrower configurations, may cut through the underlying tissue. Staple **1465**, owing to the larger configuration of crown **1471**, may reduce, or even eliminate, this possibility. In an alternative embodiment, referring to FIG. **173**, staple assembly **1479** can include several of the "J" deformable members of staple **1400** (FIGS. **122** and **123**).

To further improve the stability of staples **1465**, two adjacent staples **1465**, for example, may be connected together by bridge **1473**. More specifically, referring to FIGS. **168** and **169**, the base **1468**, and crown **1471**, of the first staple may be laterally disposed in one direction and the base **1468**, and crown **1471**, of the second staple may be laterally disposed in the opposite direction. These oppositely disposed features may improve the stability of the staples by providing stabilizing surfaces on opposite sides of the assembly. The two staples, referring to FIG. **172**, may be deployed from staple cartridge **1475** by cam sled **1474** at the same time. To facilitate the deployment of the staples, staple cartridge **1475** may include, similar to the above, slots **1476** sized and configured for receiving keys **1477** extending from crowns **1471** of staples **1465**. More particularly, keys **1477** and slots **1476** can be configured to limit the movement of staples **1465** with respect to staple cartridge **1475** to a substantially linear upward motion. In addition, similar to the above, each bridge **1473** can include an integral driver **1478** which is configured to co-operate with cam sled **1474**. In at least one embodiment, crowns **1471**, bridge **1473** and driver **1478** can be comprised of a dissolvable or bioabsorbable material.

As known in the art, staples can be deployed into tissue such that staples are aligned in a row. However, in the past, staples configured in diagonal patterns have been disincantized owing to potential leak paths between the staples. The staples of the present invention can overcome these previous problems. Referring to FIGS. **174** and **175**, staples **1480** each include two deformable members **1481** extending from a crown **1482** and bridge **1483** connecting crowns **1482**. When staples **1480** are inserted into tissue, as described above, the tissue is compressed between crowns **1482** and deformable members **1481**. However, in the embodiments in which bridges **1483** are inserted into the body along with staples **1480**, bridges **1483** can also compress the tissue and close off any leak paths therebetween. Referring to FIG. **175**, staple cartridge **1484** includes recesses **1485** therein which are configured to receive staples **1480** in a diagonal pattern such that staples **1480** can be deployed into the tissue as described above.

In an alternative embodiment, a portion of the staple cartridge can be broken away therefrom during the deployment of the staple. This portion can be configured to be positioned intermediate the base of the staple and the tissue captured within the staple. More particularly, referring to FIGS. **176-178**, a surgical stapling system can include staple cartridge **1486** having staple pads **1487** integrally molded into deck **1488** of staple cartridge **1486**. Staple cartridge **1486** can include score marks **1489** and slots **1490** surrounding staple pads **1487** such that staple pads **1487** can be easily separated from deck **1488**. More particularly, referring to FIG. **178**, the stapling system can include drivers **1491** having shears **1492** which are configured to press against staple pads **1487** when base **1493** is brought in close proximity to staple saddle **1494** and "punch-out" staple pads **1487**. In at least one embodiment, after they have been punched out, the staple pads can be

positioned intermediate base **1493** and the tissue captured within the staple. As a result, staple pads **1487** can be configured to act as the crown of the staple or, in alternative embodiments, act as a buttressing member intermediate the staple and the tissue. In at least one embodiment, similar to the above, staple pads **1487** can be comprised of a bioabsorbable material.

The staples described above can be used in various surgical techniques. For example, one surgical technique can include a method of transecting tissue or a hollow organ by positioning a surgical stapling system adjacent tissues to be transected, the surgical stapling system including at least one of the staples described above, actuating the surgical stapling system to compress the tissues together, actuating the surgical stapling system to fasten and divide the tissue with said staple, and removing the surgical stapling system from the operative site. In at least one embodiment, the surgical technique can include the anastomosis of two hollow organs and/or the fixation of at least two tissues.

While the present invention has been illustrated by description of several embodiments and while the illustrative embodiments have been described in considerable detail, it is not the intention of the applicant to restrict or in any way limit the scope of the appended claims to such detail. Additional advantages and modifications may readily appear to those skilled in the art. For example, while various manually operated surgical instruments have been depicted for clarity, it should be appreciated that such devices may also be robotically manipulated. In addition, those skilled in the art will appreciate that the embodiments, features and improvements disclosed herein may be readily employed in connection with a variety of other known surgical cutter/staplers, staplers, etc. that may have application in open, laparoscopic, endoscopic and/or intraluminal surgical procedures. In particular, such unique and novel features may be practiced in connection with linear staplers, cutters, contour cutters, etc. Thus, the scope and protection afforded to the various embodiments disclosed herein should not be limited solely to endocutter-type surgical staplers.

While several embodiments of the invention have been described, it should be apparent, however, that various modifications, alterations and adaptations to those embodiments may occur to persons skilled in the art with the attainment of some or all of the advantages of the invention. For example, according to various embodiments, a single component may be replaced by multiple components, and multiple components may be replaced by a single component, to perform a given function or functions. This application is therefore intended to cover all such modifications, alterations and adaptations without departing from the scope and spirit of the disclosed invention as defined by the appended claims.

The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include a combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those of ordinary skill in the art will appreciate that the reconditioning of a device can utilize a variety of different techniques for disassembly, cleaning/replacement, and reassembly. Use of such

techniques, and the resulting reconditioned device, are all within the scope of the present application.

Preferably, the invention described herein will be processed before surgery. First a new or used instrument is obtained and, if necessary, cleaned. The instrument can then be sterilized. In one sterilization technique, the instrument is placed in a closed and sealed container, such as a plastic or TYVEK® bag. The container and instrument are then placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or higher energy electrons. The radiation kills bacteria on the instrument and in the container. The sterilized instrument can then be stored in the sterile container. The sealed container keeps the instrument sterile until it is opened in the medical facility.

As used herein, the term "fluidically coupled" means that the elements are coupled together with an appropriate line or other means to permit the passage of pressurized gas therebetween. As used herein, the term "line" as used in "supply line" or "return line" refers to an appropriate passage formed from rigid or flexible conduit, pipe, tubing, etc. for transporting fluid from one component to another.

Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

The invention which is intended to be protected is not to be construed as limited to the particular embodiments disclosed. The embodiments are therefore to be regarded as illustrative rather than restrictive. Variations and changes may be made by others without departing from the spirit of the present invention. Accordingly, it is expressly intended that all such equivalents, variations and changes which fall within the spirit and scope of the present invention as defined in the claims be embraced thereby.

What is claimed is:

1. A surgical instrument comprising:

a cartridge supporting assembly configured to operably support a staple cartridge therein;

an anvil operably coupled to said cartridge supporting assembly and being selectively movable between open and closed positions;

a closure member interfacing with said anvil to selectively apply a closing force thereto in response to a closing motion applied to said closure member and an opening force thereto in response to an opening motion applied to said closure member; and

a ramp portion formed on a proximal end of said anvil for selective contact by a distal end of said closure member; and

at least two steps sequentially formed in said ramp portion in a distal direction for selective engagement by said distal end of said closure member as said closure member is advanced in the distal direction on said ramp to limit an amount of the closing force applied to said anvil by said closure member.

2. The surgical instrument of claim 1 further comprising:

a handle assembly operably supporting said closure drive; and

a closure trigger operably supported by said handle assembly and interacting with said closure drive such that activation of said closure trigger in a closing direction causes closure drive to apply said closure motion to said closure member and activation of said closure trigger in an opening direction causes said closure drive to apply said opening motion to said closure member.

3. A surgical instrument, comprising:

a handle assembly;

an elongate spine coupled to said handle assembly;

an elongate channel distally coupled to said elongate spine and configured to support a staple cartridge therein;

an anvil operably coupled to said elongate channel and selectively movable between open and closed positions;

a closure tube assembly defining a closure axis and movably received on said elongate spine, said closure tube assembly having a distal end portion oriented to selectively interact with said anvil to cause said anvil to move between said open and closed positions;

a closure drive operably supported within said handle assembly movably supporting a proximal end portion of said closure tube assembly therein and being operable to selectively apply opening and closing motions to said closure tube assembly such that upon application of said closure motion to said closure tube assembly, said closure tube assembly applies a closing force to said anvil; and

at least one force limiting member supported by said closure drive for travel therewith for interacting with said closure tube assembly to limit an amount of the closing force applied to said anvil by said closure tube assembly in response to a resistive force experienced by said anvil when clamping tissue between said anvil and said elongate channel, wherein said force limiting member defines a compression axis that is substantially parallel with the closure axis defined by said closure tube assembly.

4. The surgical instrument of claim 3 wherein said anvil is pivotally coupled to said elongate channel by a pair of trunnions formed on said anvil and received in corresponding elongated slots in said elongate channel member.

5. A surgical instrument comprising:

a cartridge supporting assembly configured to operably support a staple cartridge therein;

an anvil operably coupled to said cartridge supporting assembly and being selectively movable between open and closed positions; and

a variable length closure member defining a closure axis and supported for selective contact with said anvil to selectively apply a closing force thereto in response to a closing motion applied to said closure member and an opening force thereto in response to an opening motion applied to said closure member, said closure member having a resilient portion therein configured to enable the length of said closure member to change in response to a resistive force experienced by said anvil when clamping tissue between said anvil and a staple cartridge supported in said cartridge supporting assembly, wherein said resilient portion defines a compression axis that is substantially parallel with the closure axis defined by said closure member.

61

6. The surgical instrument of claim 5 wherein said resilient portion comprises a leaf spring formed in a distal end of said closure member and oriented for selective contact with a portion of said anvil during the application of said closing force to said anvil.

7. The surgical instrument of claim 5 wherein said anvil is pivotally coupled to said cartridge supporting assembly.

8. The surgical instrument of claim 5 wherein a magnitude of said resistive force is dependent upon a thickness of the tissue clamped between said anvil and the cartridge supported in said cartridge supporting assembly.

9. A method for processing an instrument for surgery, said method comprising:

obtaining said surgical instrument of claim 5;

sterilizing said surgical instrument; and

storing said instrument in a sterile container.

10. The surgical instrument of claim 5 wherein said resilient portion comprises at least one spring segment formed in said closure member.

62

11. The surgical instrument of claim 10 wherein said at least one spring segment comprises a helical spring section integrally formed in said closure member.

12. A surgical instrument comprising:

a cartridge supporting assembly configured to operably support a staple cartridge therein;

an anvil operably coupled to said cartridge supporting assembly and being selectively movable between open and closed positions; and

closure means for selectively apply a closing force to said anvil and an opening force to said anvil, wherein said closure means defines a closure axis; and

force limiting means for interacting with said closure means to limit an amount of the closing force applied to said anvil by said closure means in response to a resistive force experienced by said anvil when clamping tissue between said anvil and said elongate channel, wherein said force limiting means defines a compression axis that is substantially parallel with the closure axis defined by said closure means.

* * * * *

专利名称(译)	具有封闭装置的外科切割和缝合装置，用于限制最大组织压缩力		
公开(公告)号	US7665647	公开(公告)日	2010-02-23
申请号	US11/541151	申请日	2006-09-29
[标]申请(专利权)人(译)	谢尔顿检基ê 斯韦兹JEFFREY小号		
申请(专利权)人(译)	谢尔顿检基ê 斯韦兹JEFFREY小号		
当前申请(专利权)人(译)	爱惜康内镜手术，INC.		
[标]发明人	SHELTON IV FREDERICK E SWAYZE JEFFREY S		
发明人	SHELTON, IV, FREDERICK E. SWAYZE, JEFFREY S.		
IPC分类号	A61B17/068		
CPC分类号	A61B17/07207 A61B19/30 A61B2017/00831 A61B2017/07228 A61B2017/07242 A61B2017/07264 A61B2017/07271 A61B2017/07278 A61B2017/07285 A61B2019/302 A61B17/064 A61B17/0644 A61B17/068 A61B17/072 A61B17/07292 A61B17/105 A61B17/11 A61B17/1114 A61B17/115 A61B17/ /1155 A61B17/34 A61B90/03 A61B2017/00004 A61B2017/00128 A61B2017/00539 A61B2017/00862 A61B2017/0641 A61B2017/0725 A61B2017/2932 A61B2017/2943 A61B2017/320052 A61B2018 /00666 A61B2019/306 A61B2019/4857 A61B2090/032 A61B2090/036 A61B2090/065 A61B2090/0811 A61B2017/07257		
其他公开文献	US20080078801A1		
外部链接	Espacenet USPTO		

摘要(译)

用于内窥镜或腹腔镜插入手术部位以同时缝合和切断组织的手术器械包括细长通道，该细长通道构造成可操作地将钉仓支撑在其中。砧座可操作地连接到细长通道并且可在打开和关闭位置之间选择性地移动。闭合管组件与砧座接合，以响应于施加到闭合管组件的闭合运动而选择性地向其施加闭合力。至少一个力限制构件与闭合管组件相互作用，以限制闭合管组件施加到砧座上的闭合力的量，以响应砧座在砧座和细长通道之间夹紧组织时所经受的阻力。力限制构件可包括闭合管组件中的一个或多个弹簧部分或闭合管组件的远端中的至少一个片簧。其他实施例可包括形成在砧座的斜坡部分中的台阶，用于接合闭合管组件的远端。

