



US007824424B2

(12) **United States Patent**
Jensen et al.

(10) **Patent No.:** **US 7,824,424 B2**
(45) **Date of Patent:** ***Nov. 2, 2010**

(54) **SYSTEM AND METHOD FOR RELEASABLY HOLDING A SURGICAL INSTRUMENT**

(75) Inventors: **Joel F. Jensen**, Redwood City, CA (US);
Philip S. Green, Palo Alto, CA (US)

(73) Assignee: **SRI International**, Menlo Park, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1491 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **11/195,494**

(22) Filed: **Aug. 1, 2005**

(65) **Prior Publication Data**

US 2005/0283140 A1 Dec. 22, 2005

Related U.S. Application Data

(60) Continuation of application No. 10/265,285, filed on Oct. 4, 2002, now Pat. No. 7,204,844, which is a continuation of application No. 09/521,253, filed on Mar. 8, 2000, now Pat. No. 6,461,372, which is a division of application No. 09/105,706, filed on Jun. 26, 1998, now Pat. No. 6,080,181, which is a division of application No. 08/848,934, filed on May 1, 1997, now Pat. No. 5,810,880, which is a division of application No. 08/485,587, filed on Jun. 7, 1995, now Pat. No. 5,649,956.

(51) **Int. Cl.**
A61B 17/28 (2006.01)

(52) **U.S. Cl.** **606/205**

(58) **Field of Classification Search** 606/130,
606/131, 205-210, 170, 174, 180; 901/18,
901/21, 23, 34, 64; 414/1

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,418,184 A	5/1922	Trunick
1,664,210 A	3/1928	Hall

(Continued)

FOREIGN PATENT DOCUMENTS

CH	482 439	1/1970
DE	28 19 976	5/1978

(Continued)

OTHER PUBLICATIONS

Vertut, Jean and Coeffet, Philippe Coiffet; "Robot Technology; Volume 3A Teleoperation and Robotics Evolution and Development"; 1986; Prentice-Hall, Inc; Englewood Cliffs, N.J.


(Continued)

Primary Examiner—Kevin T Truong

(57) **ABSTRACT**

The invention is directed to a system and method for releasably holding a surgical instrument (14), such as an endoscopic instrument configured for delivery through a small percutaneous penetration in a patient. The instrument comprises an elongate shaft (100) with a pair of mounting pins (116) laterally extending from the shaft between its proximal and distal ends. An instrument holder comprises a support having a central bore (202) and an axially extending slot (204) for receiving the instrument shaft and the mounting pins. A pair of locking slots (206) are cut into the support transversely to and in communication with the axial slot so that the mounting pins can be rotated within the locking slots. The instrument support further includes a latch assembly for automatically locking the mounting pins within the locking slots to releasably couple the instrument to the instrument holder. With this twist-lock motion, the surgeon can rapidly engage and disengage various instruments from the holder during a surgical procedure, such as open surgery, laparoscopy or thoracoscopy.

18 Claims, 10 Drawing Sheets

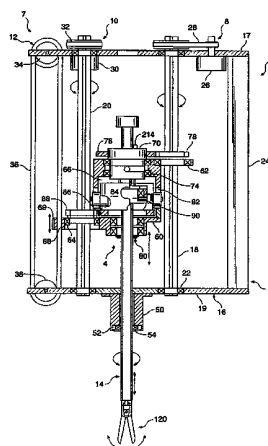

U.S. PATENT DOCUMENTS					
2,815,697 A	12/1957	Saunders-Singer	4,947,702 A	8/1990	Kato
2,901,258 A	8/1959	Brandafi	4,954,952 A	9/1990	Ubhayakar et al.
3,145,333 A *	8/1964	Pardini et al. 901/34	4,979,933 A	12/1990	Runge
3,171,549 A	3/1965	Orloff	4,979,949 A	12/1990	Matsen, III et al.
3,463,329 A	8/1969	Gartner	4,980,626 A	12/1990	Hess et al.
3,818,125 A	6/1974	Butterfield	4,989,253 A	1/1991	Liang et al.
3,921,445 A	11/1975	Hill et al.	4,996,975 A	3/1991	Nakamura
3,923,166 A	12/1975	Fletcher et al.	5,002,418 A	3/1991	McCown et al.
3,934,201 A	1/1976	Majefski	5,020,001 A	5/1991	Yamamoto et al.
4,058,001 A	11/1977	Waxman	5,020,933 A	6/1991	Salvestro et al.
4,113,115 A	9/1978	Yoshio	5,024,236 A	6/1991	Shapiro
4,150,326 A	4/1979	Engelberg et al.	5,036,463 A	7/1991	Abela et al.
4,221,997 A	9/1980	Flemming	5,045,936 A	9/1991	Lobb et al.
4,260,319 A	4/1981	Motoda et al.	5,046,022 A	9/1991	Conway et al.
4,264,266 A	4/1981	Trechsel	5,050,608 A	9/1991	Watanabe et al.
4,349,837 A	9/1982	Hinds	5,053,975 A	10/1991	Tsuchihashi et al.
4,367,998 A	1/1983	Causer	5,056,031 A	10/1991	Nakano et al.
4,419,041 A	12/1983	Rose	5,060,532 A	10/1991	Barker
4,436,684 A	3/1984	White	5,062,761 A	11/1991	Glachet
4,456,961 A	6/1984	Price	5,065,741 A	11/1991	Uchiyama et al.
4,474,174 A	10/1984	Petruzzi	5,077,506 A	12/1991	Krause
4,490,022 A	12/1984	Reynolds	5,078,140 A	1/1992	Kwoh
4,503,854 A	3/1985	Jako	5,078,142 A	1/1992	Siczek et al.
4,506,393 A	3/1985	Murphy	5,086,401 A	2/1992	Glassman et al.
4,510,574 A	4/1985	Guittet et al.	5,090,401 A	2/1992	Schwieker
4,517,963 A	5/1985	Michel	5,096,236 A	3/1992	Thöny
4,562,463 A	12/1985	Lipton	5,097,839 A	3/1992	Allen
4,563,567 A	1/1986	Geffroy et al.	5,098,426 A	3/1992	Sklar et al.
4,582,067 A	4/1986	Silverstein et al.	5,125,888 A	6/1992	Howard et al.
4,583,117 A	4/1986	Lipton et al.	5,141,519 A	8/1992	Smith et al.
4,601,000 A	7/1986	Montabert	5,142,930 A	9/1992	Allen et al.
4,636,138 A	1/1987	Gorman	5,145,227 A	9/1992	Monford, Jr.
4,638,799 A	1/1987	Moore	5,154,717 A	10/1992	Matsen, III et al.
4,651,201 A	3/1987	Schoolman	5,170,347 A	12/1992	Tuy et al.
4,655,257 A	4/1987	Iwashita	5,182,641 A	1/1993	Dienr et al.
4,672,963 A	6/1987	Barken	5,184,601 A	2/1993	Putman
4,676,243 A	6/1987	Clayman	5,187,574 A	2/1993	Kosemura et al.
4,722,056 A	1/1988	Roberts et al.	5,187,796 A	2/1993	Wang et al.
4,728,974 A	3/1988	Nio et al.	5,188,111 A	2/1993	Yates et al.
4,744,363 A	5/1988	Hasson	5,201,325 A	4/1993	McEwen et al.
4,750,475 A	6/1988	Yoshihashi	5,201,743 A	4/1993	Haber et al.
4,750,487 A	6/1988	Zanetti	5,209,747 A	5/1993	Knoepfler
4,751,925 A	6/1988	Tontarra	5,216,596 A	6/1993	Weinstein
4,762,455 A	8/1988	Coughlan et al.	5,217,003 A	6/1993	Wilk
4,764,944 A	8/1988	Finlayson	5,219,351 A	6/1993	Teubner et al.
4,788,482 A	11/1988	Tachibana et al.	5,221,283 A	6/1993	Chang
4,791,588 A	12/1988	Onda et al.	5,222,499 A	6/1993	Allen et al.
4,791,934 A	12/1988	Brunnett	5,228,429 A	7/1993	Hatano
4,794,912 A	1/1989	Lia	5,230,338 A	7/1993	Allen et al.
4,806,066 A	2/1989	Rhodes et al.	5,235,510 A	8/1993	Yamada et al.
4,808,898 A	2/1989	Pearson	5,236,432 A	8/1993	Matsen, III et al.
4,815,006 A	3/1989	Andersson et al.	5,240,011 A	8/1993	Assa
4,826,392 A	5/1989	Hayati	5,251,127 A	10/1993	Raab
4,833,383 A	5/1989	Skarr et al.	5,253,706 A	10/1993	Reid
4,837,703 A	6/1989	Kakazu et al.	5,257,203 A	10/1993	Riley et al.
4,837,734 A	6/1989	Ichikawa et al.	5,257,998 A	11/1993	Ota et al.
4,853,874 A	8/1989	Iwamoto et al.	5,260,319 A	11/1993	Effland et al.
4,854,301 A	8/1989	Nakajima	5,261,404 A	11/1993	Mick et al.
4,855,822 A	8/1989	Narendra et al.	5,264,266 A	11/1993	Yokoyama et al.
4,860,215 A	8/1989	Seraji	5,271,384 A	12/1993	McEwen et al.
4,862,873 A	9/1989	Yajima et al.	5,273,039 A	12/1993	Fujiwara et al.
4,863,133 A	9/1989	Bonnell	5,273,309 A	12/1993	Lau et al.
4,873,572 A	10/1989	Miyazaki et al.	5,279,309 A	1/1994	Taylor et al.
4,883,400 A	11/1989	Kuban et al.	5,280,427 A	1/1994	Magnusson et al.
4,899,730 A	2/1990	Stennert et al.	5,281,220 A	1/1994	Blake, III
4,921,393 A	5/1990	Andeen et al.	5,282,606 A	2/1994	Praiss
4,922,338 A	5/1990	Arpino	5,284,130 A	2/1994	Ratliff
4,930,494 A	6/1990	Takehana et al.	5,289,273 A	2/1994	Lang
4,941,106 A	7/1990	Krieger	5,299,288 A	3/1994	Glassman et al.
4,942,539 A	7/1990	McGee et al.	5,313,306 A	5/1994	Kuban et al.
4,943,296 A	7/1990	Funakubo et al.	5,325,866 A	7/1994	Krzyzanowski
			5,339,799 A	8/1994	Kami et al.
			5,343,391 A	8/1994	Mushabac

5,357,962	A	10/1994	Green	
5,368,015	A	11/1994	Wilk	
5,368,428	A	11/1994	Hussey et al.	
5,371,536	A	12/1994	Yamaguchi	
5,377,310	A	12/1994	Jain et al.	
5,377,683	A	1/1995	Barken	
5,382,885	A	1/1995	Salcudean et al.	
5,396,685	A	3/1995	Wilk et al.	
5,397,323	A	3/1995	Taylor et al.	
5,398,685	A	3/1995	Wilk et al.	
5,402,801	A	4/1995	Taylor	
5,417,210	A	5/1995	Funda et al.	
5,425,528	A	6/1995	Rains et al.	
5,441,505	A	8/1995	Nakamura	
5,445,166	A	8/1995	Taylor	
5,452,733	A	9/1995	Sterman et al.	
5,458,574	A	10/1995	MacHold et al.	
5,474,566	A	12/1995	Alesi et al.	
5,480,409	A	1/1996	Riza	
5,515,478	A	5/1996	Wang	
5,524,180	A	6/1996	Wang et al.	
5,553,198	A	9/1996	Wang et al.	
5,571,110	A	11/1996	Matsen, III et al.	
5,572,999	A	11/1996	Funda et al.	
5,619,992	A	4/1997	Guthrie et al.	
5,629,594	A	5/1997	Jacobus et al.	
5,630,431	A	5/1997	Taylor	
5,631,973	A	5/1997	Green	
5,636,138	A	6/1997	Gilbert et al.	
5,645,520	A	7/1997	Nakamura et al.	
5,649,956	A *	7/1997	Jensen et al.	606/205
5,657,429	A	8/1997	Wang et al.	
5,695,501	A *	12/1997	Carol et al.	606/130
5,735,290	A	4/1998	Sterman et al.	
5,754,741	A	5/1998	Wang et al.	
5,762,458	A	6/1998	Wang et al.	
5,779,623	A	7/1998	Bonnell	
5,807,378	A *	9/1998	Jensen et al.	606/1
5,808,665	A	9/1998	Green	
5,810,686	A	9/1998	de Jong et al.	
5,810,880	A *	9/1998	Jensen et al.	606/205
5,815,640	A	9/1998	Wang et al.	
5,817,084	A	10/1998	Jensen	
5,841,950	A	11/1998	Wang et al.	
5,855,583	A	1/1999	Wang et al.	
5,876,325	A	3/1999	Mizuno et al.	
5,878,193	A	3/1999	Wang et al.	
5,907,664	A	5/1999	Wang et al.	
5,911,036	A	6/1999	Wright et al.	
5,931,832	A	8/1999	Jensen	
5,954,746	A	9/1999	Holthaus et al.	
5,971,976	A	10/1999	Wang et al.	
6,001,108	A	12/1999	Wang	
6,017,358	A	1/2000	Yoon et al.	
6,042,599	A	3/2000	Huttner et al.	
6,063,095	A	5/2000	Wang	
6,080,181	A *	6/2000	Jensen et al.	606/205
6,413,264	B1 *	7/2002	Jensen et al.	606/130
7,204,844	B2 *	4/2007	Jensen et al.	606/205
2001/0031983	A1	10/2001	Brock et al.	
2002/0087048	A1	7/2002	Brock et al.	
2002/0120252	A1	8/2002	Brock et al.	
2002/0143319	A1	10/2002	Brock et al.	

FOREIGN PATENT DOCUMENTS

DE	9204116	3/1992
DE	4213426	10/1992
DE	3806190	9/1998
EP	0239409	9/1987
EP	0291292	11/1988
EP	0595291	5/1994
EP	0776738	6/1997

FR	2460762	1/1961
FR	2593106	7/1987
GB	2040134	8/1980
GB	2117732	10/1983
GB	494943	8/1995
JP	59-146770	8/1984
JP	62-29198	6/1987
JP	02-15349	4/1990
JP	7059788 A2	3/1995
JP	7136173 A2	5/1995
WO	WO 91/04711	4/1991
WO	WO 92/16141	10/1992
WO	WO 93/13916	7/1993
WO	WO 94/03113	2/1994
WO	WO 94/18881	9/1994
WO	WO 94/26167	11/1994
WO	WO 95/01757	1/1995

OTHER PUBLICATIONS

"Introduction to a New Project for the National Research and Development Program (Large Scale Project) in FY 1991—Macromachine Technology", Ministry of International Trade and Industry, Japan, (Apr. 1991) pp. 1-11.

Abstracts and Video Catalogue, 3.sup.rd World Congress of Endoscopic Surgery Abstracts, Surgical Laparoscopy & Endoscopy, vol. 3, No. 3, (1993) pp. 248-275.

Alexander, III, "Impacts of Telemation on Modern Society", 1st CISM-IFTO MM Symposium, vol. 2, pp. 122-136.

Altamuro, V.M., "Automatic Guided Vehicles and Robots," Mark's Standard Handbook for Mechanical Engineers, Ninth Edition, McGraw-Hill Book Company, New York, 1987.

Asada et al., "Development of a Direct-Drive Arm Using High torque Brushless Motors," Chapter 7, pp. 583-599.

Askew, et al., "Ground Control Testbed for Space Station Freedom Robot Manipulators", Proceedings of the IEEE Virtual Reality Annual International Symposium, Seattle, Washington, USA, (Sep. 18-22, 1993), Institute of Electrical and Electronics Engineers, pp. 69-75.

Bejczy et al., "Controlling Remote Manipulators Through Kinesthetic Coupling", Computers in Mechanical Engineering, 1983, pp. 48-60.

Bergamasco et al., "Advanced interfaces for teleoperated biomedical robots" IEEE Engineering in Medicine and Biology Society 11th Annual International Conference, (1989) pp. 0912-0913.

Besant et al., "Camera control for laparoscopic surgery by speech-recognizing robot: Constant attention and better use of personnel" 3.sup.rd World Congress of Endoscopic surgery, vol. 3, No. 3, (1993) pp. 271.

Blue Cross, "Another Pair of Hands for Surgeon?" The Blue Cross Magazine Perspective, 1972, p. 27.

Bose et al., "Tremor Compensation for Robotics Assisted Microsurgery," Proc. Ann. Int'l Conf. IEEE Engineering in Medicine and Biology Society, 14(3):1067-1068 (Oct. 1992).

Bowersox et al., "Vascular applications of telepresence surgery: Initial feasibility studies in swine" Journal of Vascular Surgery (1996) vol. 23, No. 2, pp. 281-287.

Charles, "Design of a surgeon-machine interface for teleoperated microsurgery" IEEE IEEE Engineering in Medicine and Biology Society 11th Annual International Conference, (1989) pp. 0883-0884.

Clement et al., "An Overview of CAT [Computer Assisted Telemanipulator] Control in Nuclear Services," 1985 IEEE Conference on Robotics and Automation, pp. 713-717.

Colgate, "Power and Impedance scaling in bilateral manipulation" Proceedings of 1991 IEEE International Conference on Robotics and Automation (Apr. 1991) pp. 2292-2297.

Computer Motion, Inc. advertisement entitled "AESOP Automated Endoscopic System for Optimal Positioning" 1 page total.

Corcoran, "Robots for the operating room," The New York Times, Sunday (Jul. 1992) 4 pages total.

Das et al., "Kinematic control and visual display of redundant teleoperators," IEEE (1989) pp. 1072-1077.

- Davies et al., "A surgeon robot for prostatectomies" IEEE (1991) pp. 870-877.
- Dolan et al., "A robot in an operating room: A bull in china shop?" IEEE (1987) pp. 289-291.
- Finlay et al., "Controlling the movement of a surgical laparoscope" IEEE (May/Jun. 1995) pp. 289-291.
- Finlay et al., "Results of a feasibility study into applications for advanced medical robots," National Research Council Canada/Join Coordinating Forum for the International Advanced Robotics Programme (1988) pp. 2.1-2.6.
- Fisher et al., "Virtual Interface Environment", Proceedings IEEE/AIAA 7th Digital Avionics Systems, Conference, 1986, pp. 346-350.
- Fisher, S.S., "Telepresence Master Glove Controller for Dexterous Robotic End-Effectors," SPIE, vol. 726, Intelligent Robots and Computer Vision: Fifth in a Series, pp. 396-401, 1986.
- Flatau, "Compact servo master-slave manipulator with optimized communication links" Proceedings of 17th conference on remote systems technology (Nov. 1969) pp. 154-164.
- Fu et al., "Robotics: Control, Sensing, Vision and Intelligence," McGraw-Hill Book Company, 1987.
- Funda et al., "Constrained Cartesian motion control for teleoperated surgical robots" IEEE (1996) vol. 12, No. 3, pp. 453-465.
- Galloway, Jr., et al., "A New Device for Interactive, Image-guided Surgery", Proceedings of SPIE Conference on Medical Imaging (Feb. 24-26, 1991), pp. 9-18.
- Gayed et al., "An advanced control micromanipulator for surgical applications" Systems Science (1987) vol. 13, No. 1-2, pp. 123-134.
- Glauser et al., "Conception of a robot dedicated to neurosurgical operations" IEEE (1991) pp. 898-907.
- Green et al., "Telepresence Surgery" IEEE Engineering in Medicine and Biology (May/Jun. 1995) pp. 324-329.
- Green et al., "Telepresence: Advanced teleoperator technology for minimally invasive surgery" 3rd World Congress of Endoscopic Surgery (Jun. 1992) p. 49, abstract 704.
- Guerrouad et al., "S.M.O.S.: Stereotaxical Microtelamanipulator for Ocular Surgery," IEEE Engineering in Medicine & Biology Society, 11.sup.th Annual International Conference, 1989, Medical Applications of Robotics, Track 16: Biorobotics, pp. 879-880.
- Guinot et al., "Analysis of a robot wrist device for mechanical decoupling of end-effector position and orientation" Six CISM-IFTOMM symposium on theory and practice of robots and manipulators (Sep. 1986) pp. 42-53.
- Hannaford et al., "Performance Evaluation of Six-Axis Generalized Force-Reflecting Teleoperator" 21/3 IEEE Transactions on Systems, Man and Cybernetics, vol. 21, No. 3 (May/Jun. 1991) at 621, col. 2.
- Hayati, et al., "Remote Surface Inspection System", Robotics and Autonomous Systems, (1993) Elsevier Science Publs. 11:1:45-59.
- Held et al., "Telepresence, Time Delay and Adaptation", Spatial Displays and Spatial Instruments Proceedings of a Conference sponsored by NASA Ames Research Center and the School of Optometry, Univ. of California, pp. 28-1 through 28-16.
- Hill et al., "Telepresence surgery demonstration system" IEEE (1994) pp. 2302-2307.
- Holler et al., "An ATM-based local communication system for telesurgery" Interactive technology and the new paradigm for healthcare (1995) pp. 137-146.
- Hunter et al., "Manipulation and dynamic mechanical testing of microscopic objects using a tele-microrobot system" (1989) pp. 1553-1558.
- Hunter et al., "Manipulation and dynamic mechanical testing of microscopic objects using a tele-microrobot system" IEEE Control Systems, Magazine (Feb. 1990) vol. 10, No. 2, pp. 3-9.
- Hunter et al., "Ophthalmic Microsurgical Robot and Associated Virtual Environment," Computer Biol. Med. 125(2):173-182 (1995).
- Hurteau, et al., "Laparoscopic Surgery Assisted by a Robotic Cameraman: Concept and Experimental Results", Proceedings of IEEE Int'l Conference on Robotics and Automation, San Diego, California, USA, (May 8-13, 1994) pp. 2286-2289.
- Inoue et al., "Six-axis bilateral control of an articulated slave manipulator using a Cartesian master manipulator" Advanced Robotics, (1990) vol. 4, No. 2, pp. 139-150.
- Intuitive Surgical, "The da Vinci.TM. Endoscopic Instrument Control System User Manual," Intuitive Surgical, Inc., 1999.
- Jau, "Anthropomorphic Remoter Manipulator", NASA Tech Briefs, 1991, p. 92.
- Kavoussei et al., "Telerobotic assisted laparoscopic surgery: Initial laboratory and clinical experience" Urology (Jul. 1994) vol. 44, No. 1, pp. 15-19.
- Kazerooni et al., "The dynamics and control of a haptic interface device" IEEE Transactions on Robotics and Automation (Aug. 1994) vol. 10, No. 4, pp. 453-464.
- Kazerooni, "Design and Analysis of the Statically Balanced Direct-Drive Robot Manipulator," Robotics & Computer-Integrated Manufacturing, 1989, vol. 6, No. 4, pp. 287-293.
- Kazerooni, "Human/robot interaction via the transfer of power and information signals/Part I: Dynamics and control analysis" IEEE (1989) pp. 1632-1640.
- Kazerooni, "Human/robot interaction via the transfer of power and information signals/Part II: An experimental analysis" IEEE (1989) pp. 1641-1647.
- Kim et al., "A Helmet Mounted Display for Telerobotics", 33 IEEE Computer Society International Conference, California, 1988, pp. 543-547.
- Krishnan et al., "Design considerations of a new generation endoscope using robotics and computer vision technology" Abstract No. 276, session CL 25/2, 1 page, Jun. 1992.
- Lavallee, "A New System for Computer Assisted Neurosurgery", IEEE Engineering in Medicine & Biology Society 11th Annual International Conference, Nov. 1989, vol. 3, pp. 926-927.
- Mair, "Industrial robotics" Prentice Hall Publishers, New York, pp. 41-54, 203-209.
- Majima et al., "On a micro-manipulator for medical application-stability consideration of its bilateral controller" Mechatronics (1991) vol. 1, No. 3, pp. 293-309.
- Matsushima, "Servo Micro Manipulator Tiny Micro Mark-1", 4th Symposium on Theory and Practice of Robots and Manipulators, 1982, pp. 193-201.
- Ng et al., "Robotic Surgery, A First-Hand Experience in Transurethral Resection of the Prostate," IEEE Engineering in Medicine and Biology, (Mar. 1993) pp. 120-125.
- Preisig et al., "A Literature Review: Robots in Medicine", IEEE Engineering in Medicine & Biology magazine, vol. 10, Issue 2 (Jun. 1991), pp. 13-22.
- Rasor et al., "Endocorporeal Surger Using Remote Manipulators," Remotely Manned Systems, Proceedings of the First National Conference, California Institute of Technology, Pasadena, CA, Sep. 13-15, 1972, pp. 483-492.
- Richter, "Telesurgery may Bridge Future Gaps", Times Tribune, Sunday, Jan. 24, 1988, pp. A-1 and A-16.
- Sabatini et al., "Force Feedback-Based Telemicromanipulation for Robot Surgery on Soft-Tissues" IEEE Engineering in Medicine Biology Society, 11.sup.th Annual International Conference (1989) vol. 3 pp. 890-891.
- Sabatini et al., "Force Feedback-Based Telemicromanipulation for Robot Surgery on Soft Tissues", IEEE Engineering in Medicine & Biology Society 11th Annual International Conference, Nov. 1989, vol. 3, pp. 912-913.
- Soto et al., "The safety assessment of human-robot systems, (Architectonic principles of hazard-control systems)," JSME International Journal (Mar. 1989) vol. 32, No. 1, pp. 67-74.
- Spain, "Stereo Advantage for a Peg-In-Hole Task Using Force-Feedback Manipulator", Stereoscopic Displays and Applications, 1990, pp. 244-254.
- Statutory Declaration of Dr. Phillip S. Green, European Patent Convention in the Matter of EP-B-653922 Mathys & Squire, 100 Gray's Inn Road, London WC1X 8AL, United Kingdom, Ref. IK/1-12053.
- Tachi et al., "Tele-existence Master Slave System for Remote Manipulation", 1990, Proceedings of the 29th Conference on Decision and Control, vol. 1 of 6, pp. 85-90.
- Taubes, "Surgery in Cyberspace," Discover, Dec. 1994, pp. 85-92.
- Taylor et al., "A telerobotic assistant for laparoscopic surgery," Computer Science (Feb. 1994) pp. 1-24.
- Taylor et al., "Taming the bull: Safety in a precise surgical robot" IEEE (1991) pp. 865-873.
- Taylor et al., "A Telerobotic Assistant for Laparoscopic Surgery," Engineering in Medicine and Biology, May-Jun. 1995, pp. 279-288.

Tejima et al., "A new microsurgical robot system for corneal transplantation" Precision Machinery (1988) vol. 2, pp. 1-9.

Tendick et al., "Analysis of the surgeon's grasp for telerobotic surgical manipulation" IEEE Engineering in Medicine and Biology Society 11th Annual International Conference (1989) pp. 0914-0915.

Thring, "Robots and telechairs: Manipulators with memory; remote manipulators; machine limbs for the handicapped" Ellis Horwood Series in Engineering Science, pp. 9-11, Chapter 5: pp. 122-131, Chapter 7: pp. 194-195, Chapter 8: pp. 236-278, Chapter 9: p. 279.

Trevelyan et al., "Motion Control for a Sheep Shearing Robot," IEEE Robotics Research Conference, the 1st International Symposium, Carroll, NH, USA, Conference Date: Aug. 25, 1983, Conference No. 05357, Publication by MIT Press, pp. 175-190.

Trevelyan, "Skills for a shearing robot: Dexterity and sensing" Robotics Research/Second International Symposium (1985) pp. 272-282.

Trivedi et al., "Developing telerobotics systems using virtual reality concepts" IEEE (Jul. 1993) pp. 352-359.

Vertut et al., "Sensor aided and/or computer-aided bilateral teloperation system (SCATS)," Fifth CISM-IFTOMM Symposium, Theory and Practice of Robots and Manipulators, Proceedings of RoManSy '84, part 4. MIT Press, Cambridge, Massachusetts, 1985.

Vibet, "Properties of master-slave robots," Motor-Con (Apr. 1987) pp. 309-316.

Videotape: "Telepresence: Advanced Teleoperator Technology for Enhanced Minimally Invasive Surgery," Phil Green (Apr. 1992).

* cited by examiner

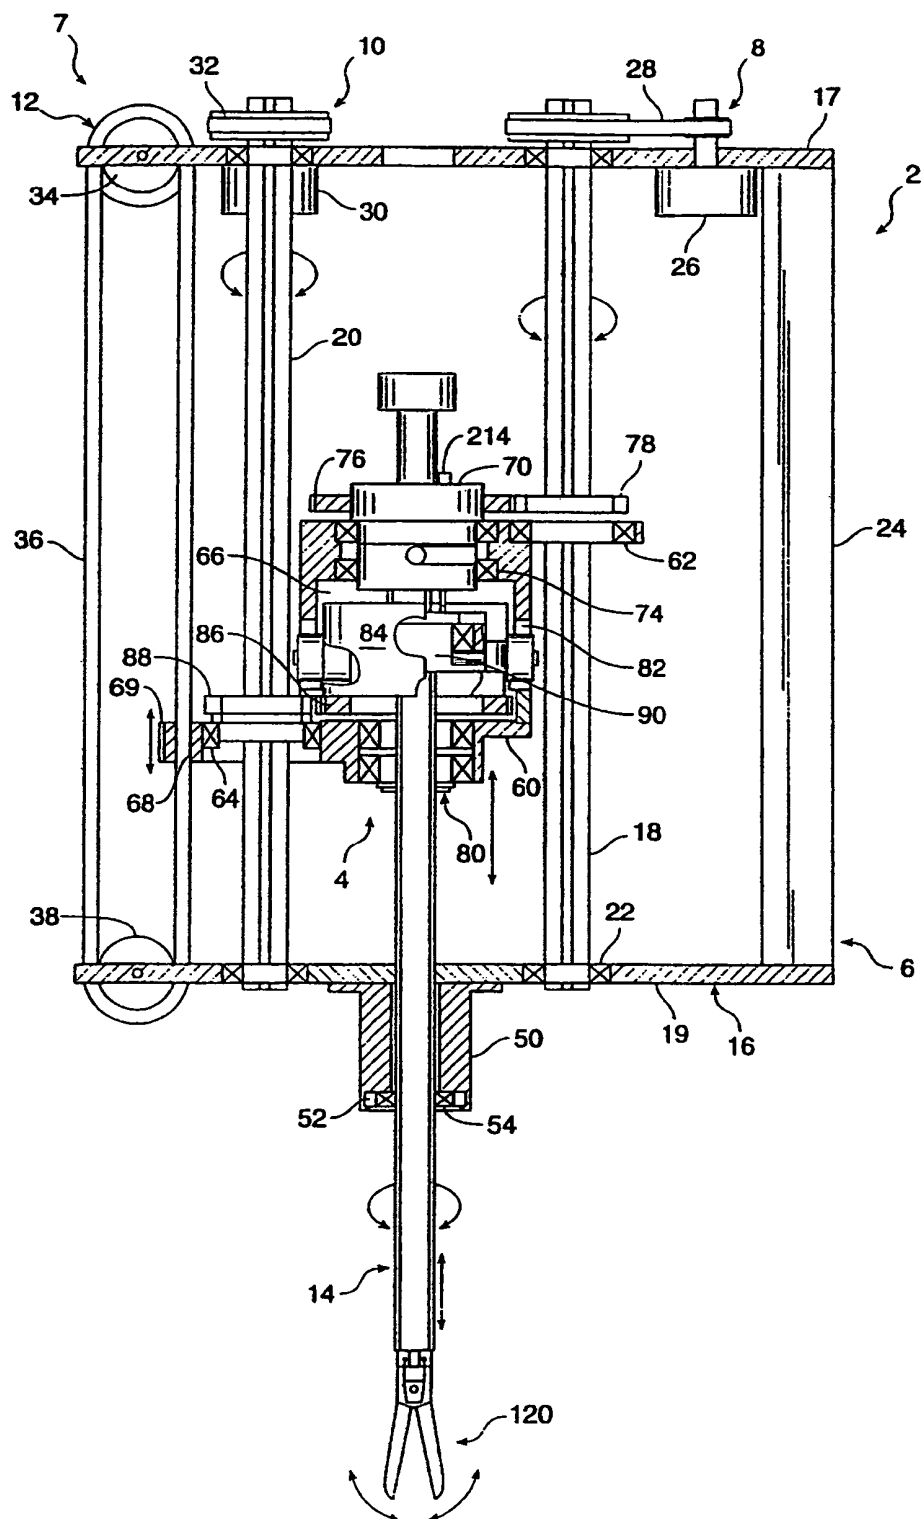


FIG. 1

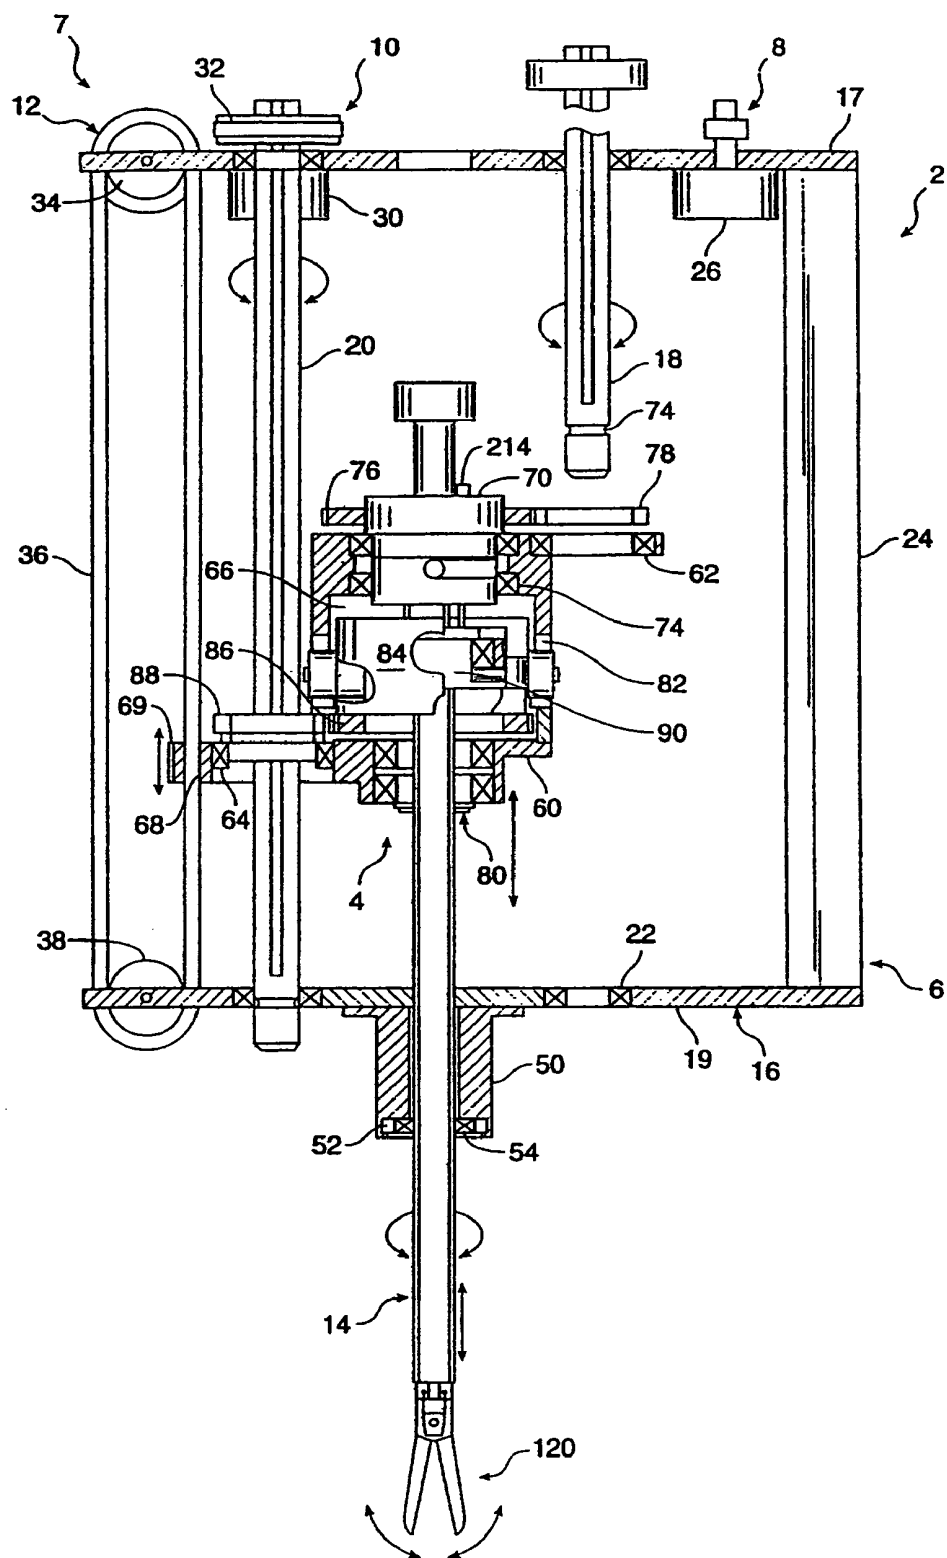


FIG. 1A

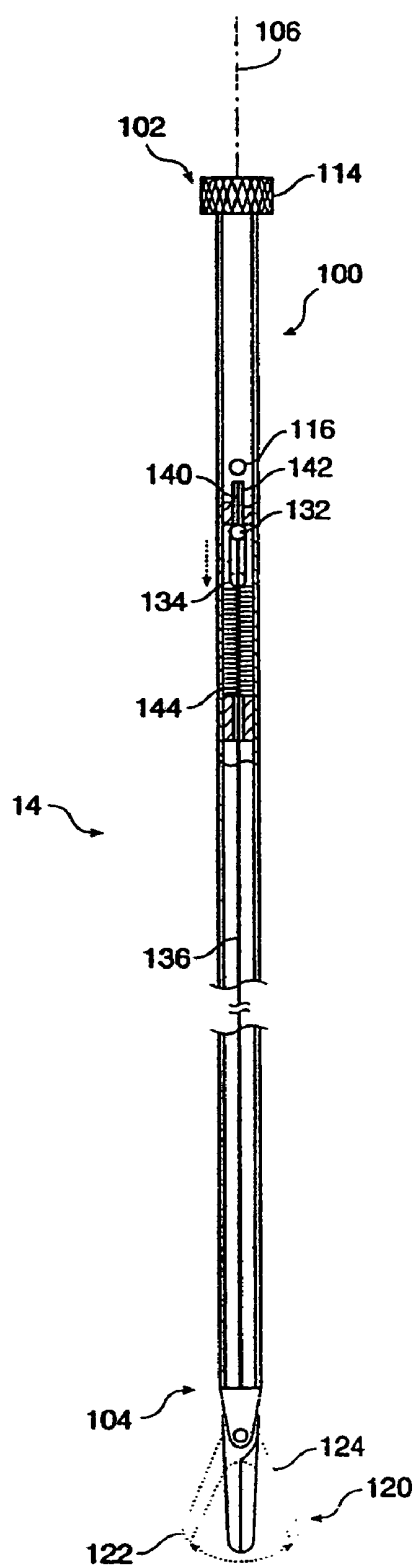


FIG. 2A

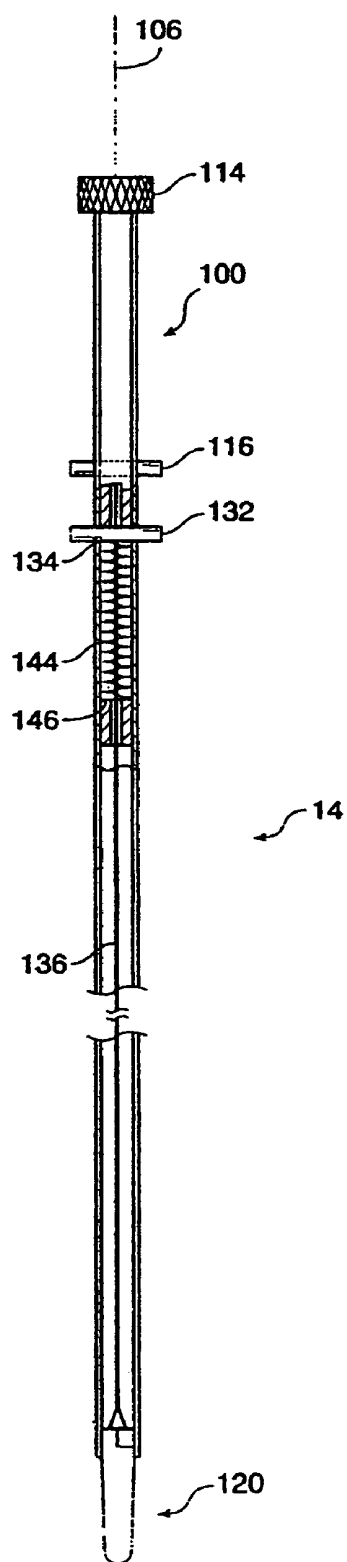


FIG. 2B

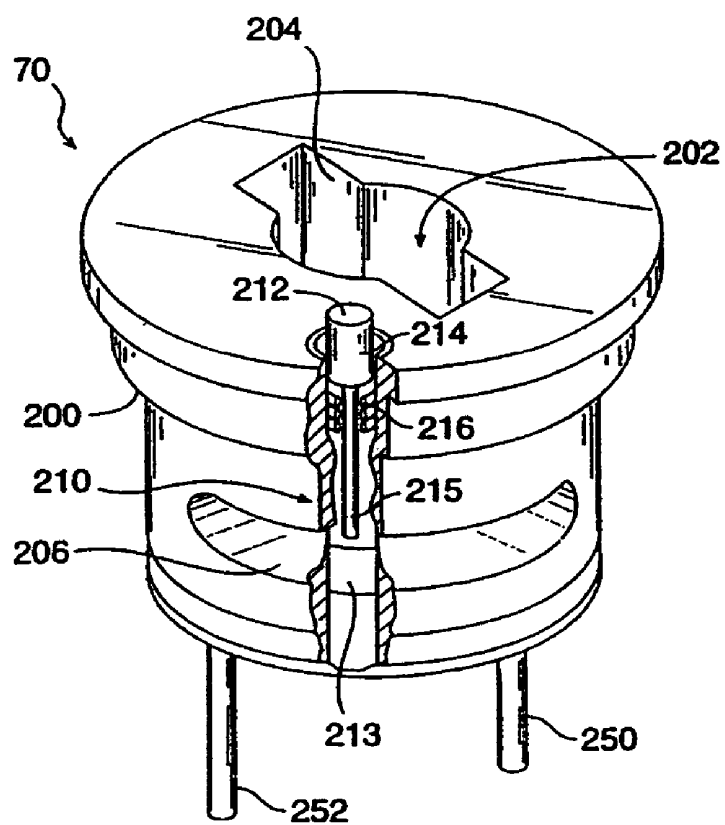


FIG. 3A

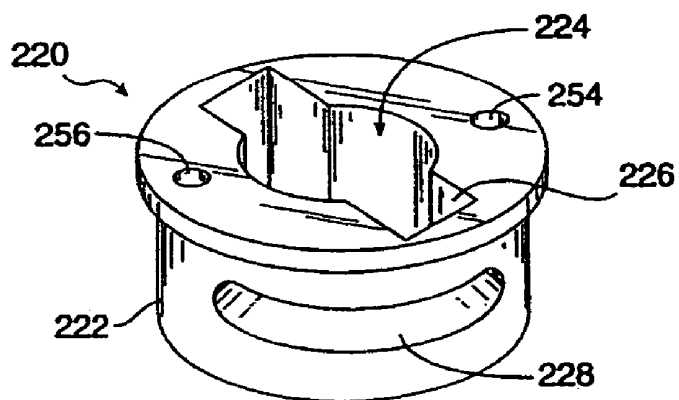


FIG. 3B

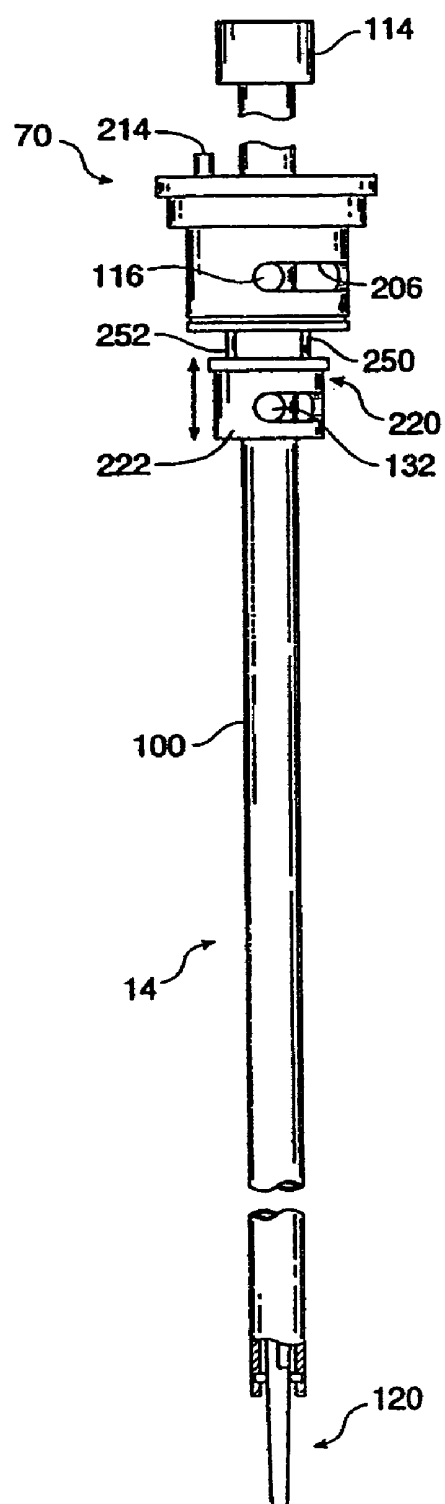


FIG. 4

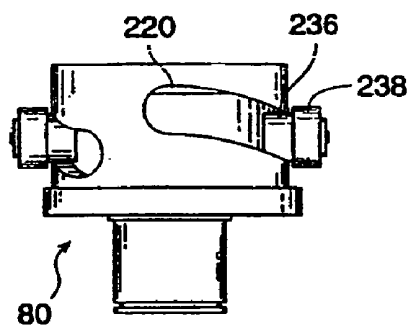


FIG. 5

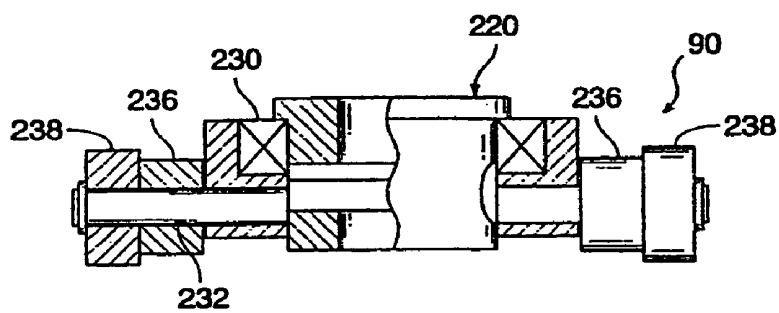


FIG. 6A

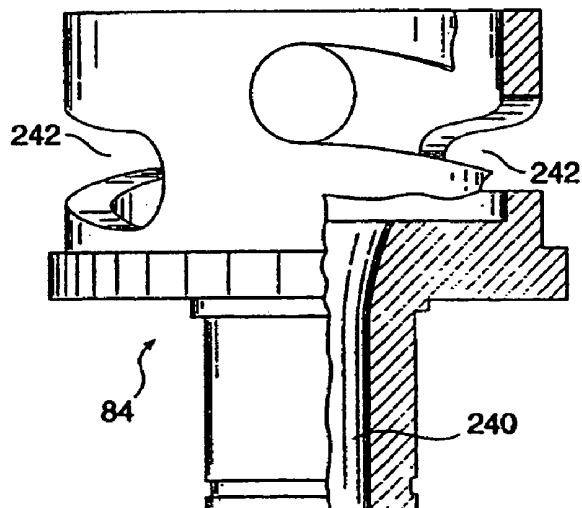


FIG. 6B

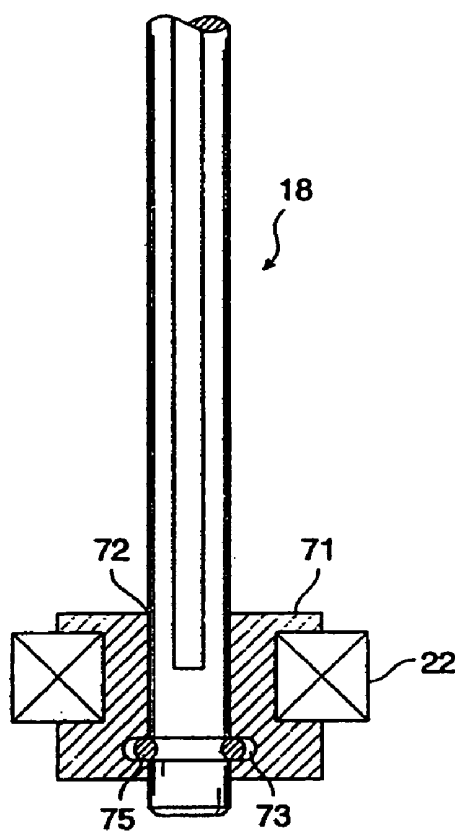


FIG. 7

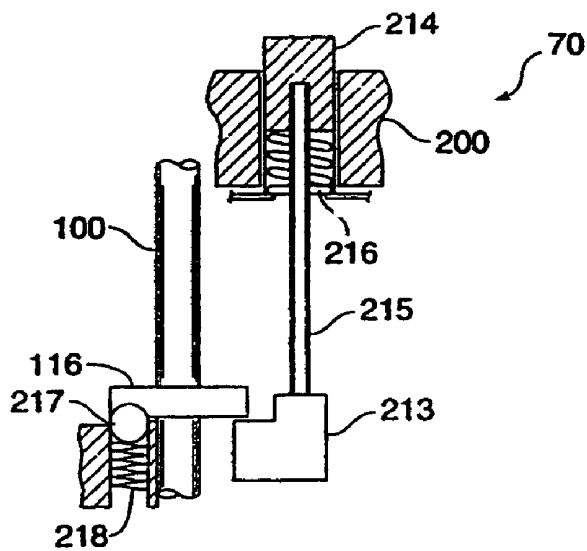


FIG. 8

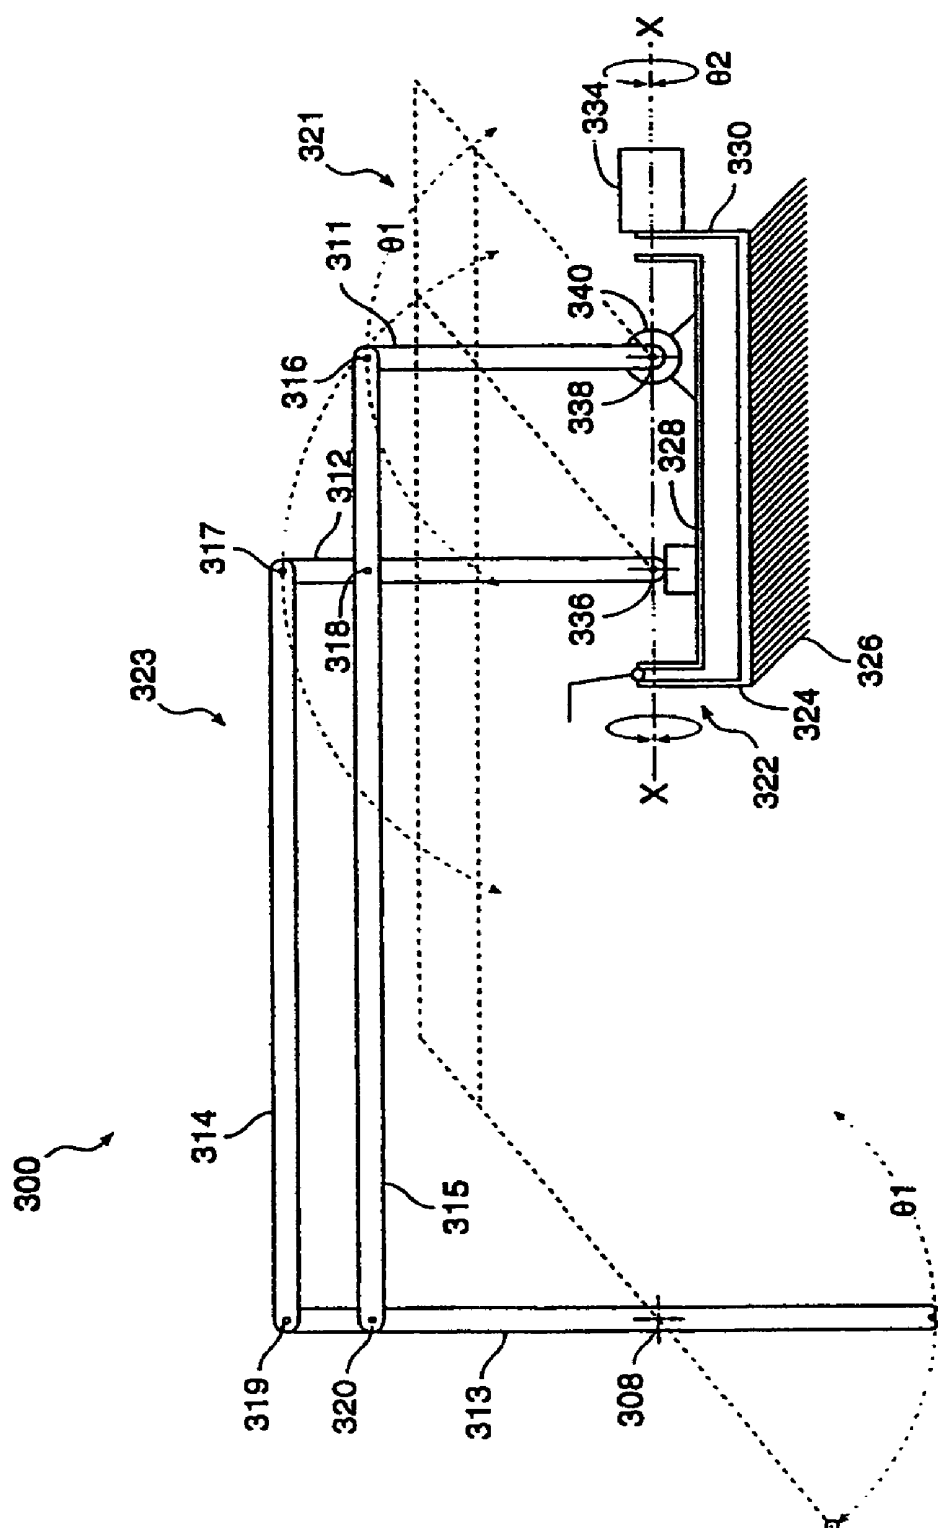


FIG. 9

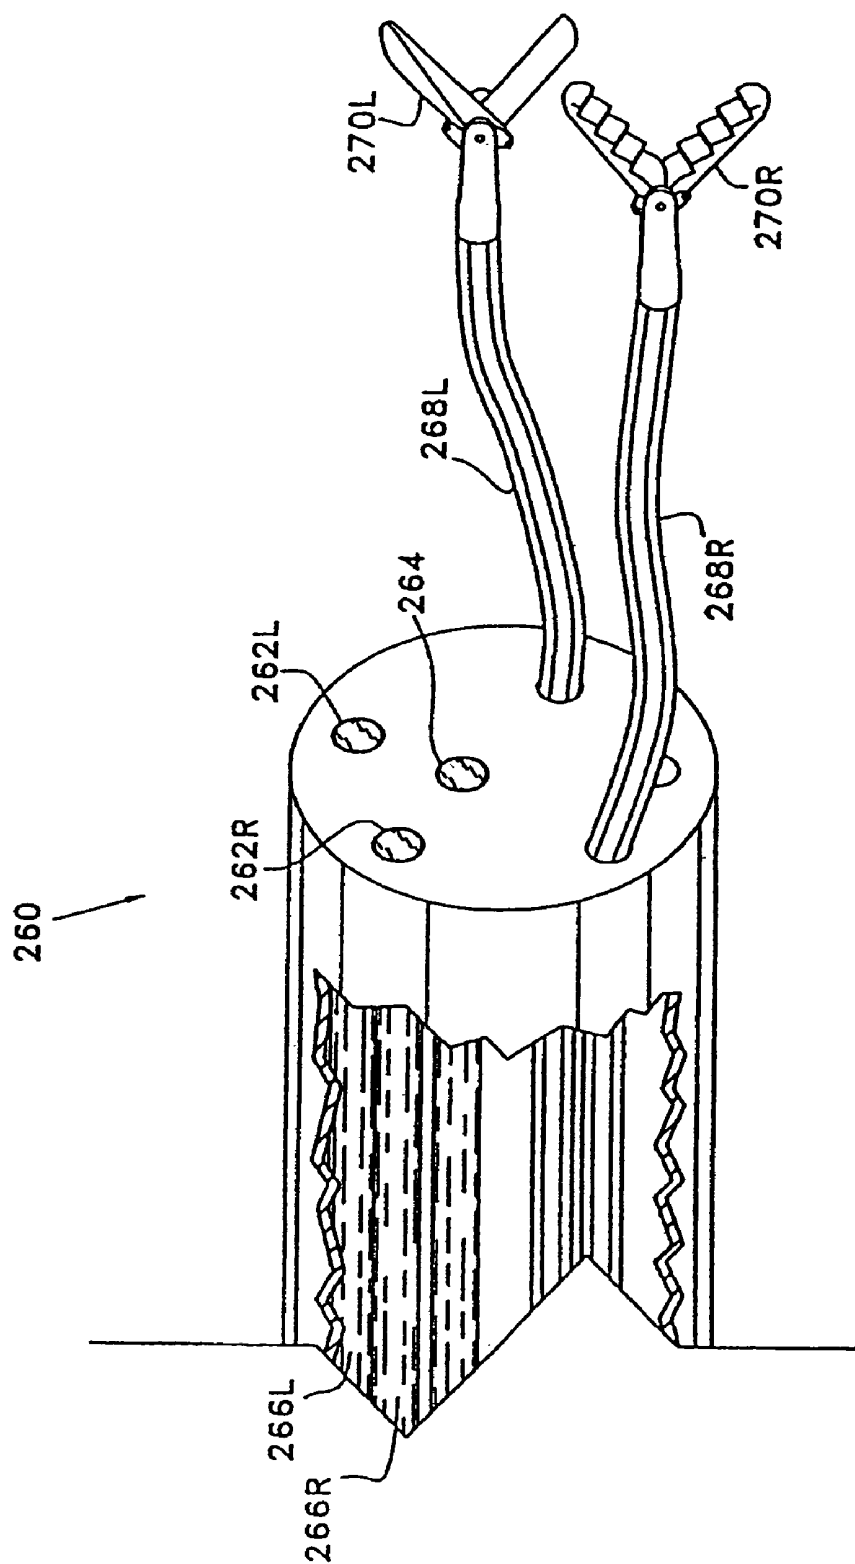


FIG. 10

SYSTEM AND METHOD FOR RELEASABLY HOLDING A SURGICAL INSTRUMENT

CROSS-REFERENCES TO RELATED APPLICATIONS

This application is a continuation of U.S. application Ser. No. 10/265,285 filed Oct. 4, 2002, which is a continuation of U.S. application Ser. No. 09/521,253 filed on Mar. 8, 2000, now U.S. Pat. No. 6,461,372, which is a continuation of U.S. application Ser. No. 09/105,706 filed on Jun. 26, 1998, now U.S. Pat. No. 6,080,181, which is a division of U.S. application Ser. No. 08/848,934, filed on May 1, 1997, now U.S. Pat. No. 5,810,880, which is a division of application Ser. No. 08/485,587, filed on Jun. 7, 1995, now U.S. Pat. No. 5,649,956, all of which are incorporated herein by reference.

STATEMENT AS TO RIGHTS TO INVENTIONS MADE UNDER FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

This invention was made with Government support under contract awarded by the National Institute for Health (NIH) under grant number 5 R01GM-44902-02. The Government has certain rights in this invention.

REFERENCE TO A "SEQUENCE LISTING," A TABLE, OR A COMPUTER PROGRAM LISTING APPENDIX SUBMITTED ON A COMPACT DISK

NOT APPLICABLE

BACKGROUND OF THE INVENTION

This invention relates to surgical manipulators and more particularly to robotic assisted apparatus for use in surgery.

In standard laparoscopic surgery, a patient's abdomen is insufflated with gas, and trocar sleeves are passed through small (approximately ½ inch) incisions to provide entry ports for laparoscopic surgical instruments. The laparoscopic surgical instruments generally include a laparoscope for viewing the surgical field, and working tools such as clamps, graspers, scissors, staplers, and needle holders. The working tools are similar to those used in conventional (open) surgery, except that the working end of each tool is separated from its handle by an approximately 12 inch long extension tube. To perform surgical procedures, the surgeon passes instruments through the trocar sleeves and manipulates them inside the abdomen by sliding them in and out through the sleeves, rotating them in the sleeves, levering (e.g., pivoting) the sleeves in the abdominal wall, and actuating end effectors on the distal end of the instruments.

In robotically-assisted and telerobotic surgery (both open surgery and endoscopic procedures), the position of the surgical instruments is controlled by servo motors rather than directly by hand or with fixed clamps. The servo motors follow the motions of a surgeon's hands as he/she manipulates input control devices at a location that may be remote from the patient. Position, force, and tactile feedback sensors may be employed to transmit position, force, and tactile sensations from the surgical instrument back to the surgeon's hands as he/she operates the telerobotic system.

The servo motors are typically part of an electromechanical device that supports and controls the surgical instruments that have been introduced directly into an open surgical site or through trocar sleeves into the patient's abdomen becomes a body cavity. During the operation, the electromechanical

device or instrument holder provides mechanical actuation and control of a variety of surgical instruments, such as tissue graspers, needle drivers, etc., that each perform various functions for the surgeon, i.e., holding or driving a needle, grasping a blood vessel or dissecting tissue.

This new method of performing telesurgery through remote manipulation will create many new challenges. One such challenge is that different surgical instruments will be attached and detached from the same instrument holder a number of times during an operation. In laparoscopic procedures, for example, the number of entry ports into the patient's abdomen is generally limited during the operation because of space constraints as well as a desire to avoid unnecessary incisions in the patient. Thus, a number of different surgical instruments will typically be introduced through the same trocar sleeve during the operation. Likewise, in open surgery, there is typically not enough room around the surgical site to position more than one or two surgical manipulators, and so the surgeon's assistant will be compelled to frequently remove instruments from the holder and exchange them with other surgical tools.

What is needed, therefore, is an improved system and method for releasably coupling a surgical instrument to an instrument holder. The system should be configured to quickly and easily engage and disengage the instrument from the holder to minimize the instrument exchange time during endoscopic surgery. Preferably, the system is part of an electromechanical device that can be coupled to a controller mechanism to form a telerobotic system for operating the surgical instrument by remote control.

BRIEF SUMMARY OF THE INVENTION

According to the invention, a system and method provide for releasably holding a surgical instrument during conventional open surgery or endoscopic procedures, such as laparoscopy. The instrument comprises an elongate shaft with proximal and distal ends and a mounting means having a protrusion extending radially from the shaft between the proximal and distal ends. An instrument holder comprises a support having a body with an axial passage for receiving the instrument shaft and a first hole in communication with the axial passage for receiving the protrusion. A second hole is cut into the body transversely to and in communication with the first hole so that the protrusion can be rotated within the second hole. To prevent the instrument from being accidentally twisted and thereby disengaged from the instrument holder during surgery, the holder further includes a locking means coupled to the body for automatically locking the protrusion within the second hole thereby releasably locking the instrument to the instrument holder.

In a preferred configuration, the protrusion of the mounting means comprises a pair of opposing arms, such as mounting pins, extending outward from the instrument shaft. The first hole is an axially extending slot for receiving the mounting pins and the second hole is a perpendicular locking slot having a first portion aligned with the axial slot and a second portion extending circumferentially around the body of the instrument support. With this configuration, the mounting pins can be slid through the axial slot and rotated into the locking slot to attach the instrument to the holder. The instrument can be removed by performing the same two steps in reverse order. With this twist-lock motion, the surgeon can rapidly engage and disengage various instruments from the instrument holder during a surgical procedure.

The locking means preferably comprises a releasable latch assembly for locking the mounting pins to the instrument

holder. The latch assembly includes a spring-loaded plunger coupled to a latch that normally locks the instrument in place by capturing the mounting pin in the locking slot. The plunger has a button extending outward from the instrument holder for moving the latch away from the locking slot. The button can be depressed manually or automatically to release the mounting pins and allow instrument exchange when the instrument is easily accessible to the surgeon.

The invention is particularly useful for releasably holding an endoscopic instrument configured for introduction through a small percutaneous penetration into a body cavity, e.g., the abdominal or thoracic cavity. To that end, the instrument preferably includes an end effector, such as a pair of jaws, coupled to the distal end for engaging a tissue structure within the body cavity. To actuate the end effector, the instrument has a second pair of arms, such as actuator pins, laterally extending from the shaft and operatively coupled to the end effector. Preferably, the actuator pins are axially displaceable with respect to the shaft to actuate the end effector (e.g., open and close the jaws). The instrument holder further includes an actuator driver releasably coupled to the actuator arms and to an external driver for actuating the end effector. The actuator driver preferably includes a twist-lock interface having transverse slots similar to that described for the instrument support so that the instrument can be simultaneously engaged or disengaged from both the instrument support and the actuator driver.

Other features and advantages of the invention will appear from the following description in which the preferred embodiment has been set forth in detail in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a partial sectional elevational view of a robotic endoscopic surgical instrument mounted to a manipulator assembly according to the present invention;

FIG. 1A is a partial sectional elevational view of the manipulator assembly of FIG. 1 illustrating the removal of an instrument holder from the rest of the assembly;

FIGS. 2A and 2B are enlarged side and front cross-sectional views, respectively, of the surgical instrument of FIG. 1;

FIGS. 3A and 3B are perspective views of an instrument support and an actuator pin catch, respectively, for releasably mounting the surgical instrument to the manipulator assembly;

FIG. 4 is a front elevational view of the surgical instrument mounted within the instrument support and actuator pin catch of FIGS. 3A and 3B;

FIG. 5 is a front elevational view of an actuator driver for providing axial movement of the actuator pin catch of FIG. 3B;

FIGS. 6A and 6B are enlarged cross-sectional views of an actuator carriage assembly and a helical actuator of the actuator driver of FIG. 5;

FIG. 7 is an enlarged detail of a portion of the frame of the manipulator assembly of FIG. 1 illustrating a coupling mechanism for removing the shafts from the frame;

FIG. 8 is a partial cross-sectional view of the instrument support of FIG. 3A illustrating a locking mechanism for a twist lock interface according to the present invention; and

FIG. 9 is an elevational view of a remote center positioner for holding the manipulator assembly of FIG. 1.

FIG. 10 shows a fragmentary portion of the insertion portion of an endoscope for use with the present invention.

DETAILED DESCRIPTION OF THE INVENTION

Referring to the drawings in detail, wherein like numerals indicate like elements, a manipulator assembly 2 is illustrated according to the principles of the invention. Manipulator assembly 2 generally includes an instrument holder 4 removably mounted to a base 6 and a drive assembly 7 for manipulating a surgical instrument 14 releasably coupled to instrument holder 4.

Referring to FIG. 1, base 6 comprises a frame 16 having proximal and distal elongate support members 17, 19 and first and second ball-spline shafts 18, 20 rotatably coupled to support members 17, 19 via bearings 22. Frame 16 further includes a support bracket 24 for attaching manipulator assembly 2 to a remote center positioner 300, as discussed in more detail below (see FIG. 9). Drive assembly 7 comprises first, second and third drives 8, 10, 12, which are mounted to frame 16 and configured to provide three degrees of freedom to surgical instrument 14. In the preferred embodiment, first drive 8 rotates instrument 14 around its own axis, second drive 10 actuates an end effector 120 on the distal end of instrument 14 and third drive 12 axially displaces instrument 14 with respect to frame 16. Of course, it will be readily recognized by those skilled in the art that other configurations are possible. For example, assembly 2 may include additional drives for providing additional degrees of freedom to surgical instrument 14, such as rotation and flexion of an instrument wrist.

First drive 8 comprises a rotation drive motor 26 fixed to frame 16 and coupled to first shaft 18 by a drive belt 28 for rotating first shaft 18 with respect to frame 16. Second drive 10 comprises a gripper drive motor 30 fixed to frame 16, and coupled to second shaft 20 by a drive belt 32 for rotating second shaft 20 with respect to frame 16. Third drive 12 comprises a vertical drive motor 34 coupled to instrument holder 4 via a drive belt 36 and two pulleys 38 for axially displacing instrument holder 4 with respect to frame 16. Drive motors 26, 30, 34 are preferably coupled to a controller mechanism via servo-control electronics (not shown) to form a telerobotic system for operating surgical instrument 14 by remote control. The drive motors follow the motions of a surgeon's hands as he/she manipulates input control devices at a location that may be remote from the patient. A suitable telerobotic system for controlling the drive motors is described in commonly assigned co-pending application Ser. No. 08/623,932 filed Jan. 21, 1992 TELEOPERATOR SYSTEM AND METHOD WITH TELEPRESENCE, which is incorporated herein by reference.

The above described telerobotic servo system preferably has a servo bandwidth with a 3 dB cut off frequency of at least 10 hz so that the system can quickly and accurately respond to the rapid hand motions used by the surgeon. To operate effectively with this system, instrument holder 4 has a relatively low inertia and drive motors 26, 30, 34 have relatively low ratio gear or pulley couplings.

In a specific embodiment, surgical instrument 14 is an endoscopic instrument configured for introduction through a percutaneous penetration into a body cavity, such as the abdominal or thoracic cavity. In this embodiment, manipulator assembly 2 supports a cannula 50 on distal support member 19 of frame 16 for placement in the entry incision during an endoscopic surgical procedure (note that cannula 50 is illustrated schematically in FIG. 1 and will typically be much longer). Cannula 50 is preferably a conventional gas sealing trocar sleeve adapted for laparoscopic surgery, such as colon resection and Nissen fundoplication.

As shown in FIG. 1, cannula 50 preferably includes a force sensing element 52, such as a strain gauge or force-sensing resistor, mounted to an annular bearing 54 within cannula 50. Bearing 54 supports instrument 14 during surgery, allowing the instrument to rotate and move axially through the central bore of bearing 54. Bearing 54 transmits lateral forces exerted by the instrument 14 to force sensing element 52, which is operably connected to the controller mechanism for transmitting these forces to the input control devices (not shown) held by the surgeon in the telerobotic system. In this manner, forces acting on instrument 14 can be detected without disturbances from forces acting on cannula 50, such as the tissue surrounding the surgical incision, or by gravity and inertial forces acting on manipulator assembly 2. This facilitates the use of manipulator assembly in a robotic system because the surgeon will directly sense the forces acting against the end of instrument 14. Of course, the gravitational forces acting on the distal end of instrument 14 will also be detected by force sensing element 52. However, these forces would also be sensed by the surgeon during direct manipulation of the instrument.

As shown in FIG. 1, instrument holder 4 comprises a chassis 60 mounted on shafts 18, 20 via ball-spline bearings 62, 64 so that chassis 60 may move axially with respect to shafts 18, 20, but is prevented from rotating with shafts 18, 20. Chassis 60 is preferably constructed of a material that will withstand exposure to high temperature sterilization processes, such as stainless steel, so that chassis 60 can be sterilized after a surgical procedure. Chassis 60 includes a central cavity 66 for receiving surgical instrument 14 and an arm 68 laterally extending from chassis 60. Arm 68 is fixed to drive belt 36 so that rotation of drive belt 36 moves instrument holder 4 in the axial direction along shafts 18; 20.

Instrument holder 4 is removably coupled to base 6 and the drive motors so that the entire holder 4 can be removed and sterilized by conventional methods, such as steam, heat and pressure, chemicals, etc. In the preferred configuration, arm 68 includes a toggle switch 69 that can be rotated to release arm 68 from drive belt 36 (FIG. 1). In addition, shafts 18, 20 are removably coupled to bearings 22 so that the shafts can be axially withdrawn from support members 17, 19 of frame 16, as shown in FIG. 1A. To this end, the distal bearings 22 preferably include a coupling mechanism for allowing the removal of shafts 18, 20. As shown in FIG. 7, distal support member 19 includes a support collar 71 within each distal bearing 22 having an inner bore 72 for passage of one of the shafts 18, 20. Each support collar 71 has an internal groove 73 and shafts 18, 20 each have an annular groove 74 (see FIG. 1A) near their lower ends that is aligned with internal grooves 73 when the shafts are suitably mounted within frame 16 (FIG. 1). A spring clip 75 is positioned within each internal groove 73 to hold each shaft 18, 20 within the respective support collar 71. Spring clip 74 has a discontinuity (not shown) to allow removal of shafts 18, 20 upon the application of a threshold axial force on the shafts.

To remove instrument holder 4 from base 6, the operator rotates toggle switch 69 to release arm 68 from drive belt 36 and removes drive belts 28, 32 from drives 8, 10. As shown in FIG. 1A, the operator holds instrument holder 4 and pulls shafts 18, 20 upwards, providing enough force to release spring clips 75. Shafts 18, 20 will disengage from distal bearings 22 and slide through ball-spline bearings 62, 64 so that instrument holder 4 is disconnected from base 6. It should be understood that the invention is not limited to the above described means for removably coupling instrument holder 4 to base 6 and drive assembly 7. For example, distal support member 19 may be removably coupled to the rest of frame 16

so that the surgeon simply removes member 19 and slides holder down and off shafts 18, 20. Proximal support member 17 may be removably coupled to frame 16 in a similar manner. Alternatively, the drive motors may be housed in a separate servo-box (not shown) that is removably attached to base 6. In this configuration, the servo-box would be removed from base 6 so that the entire base 6, together with holder 4, can be sterilized.

The lower portion of base 6 (including distal support member 19) may also be sterilized to decontaminate those parts that come into contact with holder 4 or instrument 14 (e.g., by dipping the lower portion of base 6 into a sterilizing bath). To facilitate this type of sterilization, shafts 18, 20 will preferably be somewhat longer than shown in FIG. 1 so that the upper portion of base 6, including drive assembly 7, is disposed sufficiently away from holder 4 and instrument 14. In this manner, the surgical manipulator can be easily sterilized after a surgical procedure without damaging the drive motors or the electrical connections required for the telerobotic system.

Instrument holder 4 further includes an instrument support 70 (see detail in FIG. 3A), for releasably coupling surgical instrument 14 to the manipulator assembly. Instrument support 70 is rotatably mounted within chassis 60 via mounting bearings 74 so that support 70 and the instrument can be rotated therein. As shown in FIG. 1, support 70 is circumscribed by an annular ring gear 76 having teeth that mesh with the teeth of a drive gear 78 mounted to first shaft 18. Drive gear 78 is configured around first shaft 18 such that it will rotate with first shaft 18, thereby rotating instrument support 70 and the surgical instrument therewith. Drive gear 78 is also configured to move axially with respect to first shaft 18 to allow axial movement of instrument holder 4 with respect to frame 16.

Instrument holder 4 further includes an actuator driver 80 (see detail in FIG. 5) movably mounted within axial guide slots 82 on either side of chassis 60. Actuator driver 80 comprises a helical actuator 84 (see detail in FIG. 6B) having a ring gear 86 that meshes with a gripper drive gear 88 mounted to second shaft 20. Rotation of second shaft 20 causes rotation of gripper drive gear 88, thereby rotating ring gear 86 and helical actuator 84 within chassis 60. Actuator driver 80 further includes an actuator carriage assembly 90 (see detail in FIG. 6A) for releasably coupling an end effector actuator of surgical instrument 14 to instrument holder 4 (see FIG. 2). Carriage assembly 90 is mounted within helical actuator 84 and chassis 60 such that rotation of helical actuator 84 causes a corresponding axial movement of carriage assembly 90 with respect to chassis 60, as discussed in greater detail below.

FIGS. 2A and 2B illustrate a specific embodiment of an endoscopic surgical instrument 14 capable of being operated by a motorized manipulator, such as manipulator assembly 2, for telerobotic surgery. Surgical instrument 14 can be a variety of conventional endoscopic instruments adapted for delivery through a percutaneous penetration into a body cavity, such as tissue graspers, needle drivers, microscissors, electrocautery dissectors, etc. In the preferred embodiment, instrument 14 is a tissue grasper comprising a shaft 100 having a proximal end 102, a distal end 104 and a longitudinal axis 106 therebetween. A knurled handle 114 is attached to proximal end 102 of shaft 100 to facilitate manipulation of instrument 14.

Shaft 100 is preferably a stainless steel tube having an outer diameter in the range of 2-10 mm, usually 4-8 mm, so as to fit within a cannula having an internal diameter in the range of 2-15 mm. Shaft 100 can also be introduced directly through a

percutaneous incision in the patient. Shaft **100** has a length selected to reach a target site in a body cavity, such as the abdomen, and to extend sufficiently out of the body cavity to facilitate easy manipulation of surgical instrument **14**. Thus, shaft **100** should be at least between 10 cm and 40 cm and is preferably between 17 cm and 30 cm. It should be noted that although shaft **100** is shown as having a circular cross-sectional shape in the drawings, shaft **100** could alternatively have a rectangular, triangular, oval or channel cross-sectional shape.

In a specific configuration, shaft **100** includes a mounting means for releasably coupling surgical instrument **14** to instrument support **70** and first drive **8** of manipulator assembly **2**. In the preferred embodiment, mounting means comprises a pair of opposed mounting pins **116** extending laterally outward from shaft **100**. Mounting pins **116** are rigidly connected to shaft **100** and are adapted for engaging a twist-lock interface on instrument support **70**, as discussed in detail below. It should be understood that the invention is not limited to a pair of opposing pins and mounting means can include a single mounting pin or a plurality of pins extending circumferentially around shaft. Alternatively, pins **116** may have a variety of other shapes, such as spherical or annular, if desired.

Instrument **14** includes an end effector **120** extending from distal end **104** for engaging a tissue structure on the patient, such as the abdomen during laparoscopic surgery. In the preferred embodiment, end effector **120** comprises a pair of jaws **122**, **124** that are movable between open and closed positions for grasping a blood vessel, holding a suture, etc. Jaws **122**, **124** preferably have transverse grooves or other textural features (not shown) on opposing surfaces to facilitate gripping of the tissue structure. To avoid the possibility of damaging the tissue to which jaws **122**, **124** are applied, the jaws may also include atraumatic means (not shown), such as elastomeric sleeves made of rubber, foam or surgical gauze wrapped around jaws **122**, **124**.

To move jaws **122**, **124** between the open and closed positions, instrument **14** includes an end effector actuator releasably coupled to actuator driver **80** and second drive **10** of manipulation assembly **2** (see FIG. 4). In the preferred embodiment, end effector actuator comprises a pair of opposed actuator pins **132** laterally protruding from axially extending slots **134** in shaft **100**. Actuator pins **132** are coupled to an elongate rod **136** slidably disposed within an inner lumen **138** of shaft **100**. Actuator pins **132** are slidable within slots **134** so that rod **136** is axially movable with respect to shaft **100** and mounting pins **116** to open and close jaws **122**, **124**, as is conventional in the art. Elongate rod **136** has a proximal portion **140** that is disposed within an inner lumen **142** within shaft **100** to prevent actuator pins **132** from moving in the laterally direction and to ensure that rod **136** remains generally centered within shaft **100** during a surgical procedure.

Jaws **122**, **124** are preferably biased into the closed position by an annular compression spring **144** positioned within shaft **100** between actuator pins **132** and an annular disc **146** fixed to the inside surface of shaft **100**. During endoscopic procedures, this allows the surgical team to introduce jaws **122**, **124** through cannula **50** (or any other type of percutaneous penetration) and into the body cavity without getting stuck within cannula **50** or damaging surrounding tissue.

FIGS. 3A, 3B and 4 illustrate a twist lock mechanism for releasably connecting surgical instrument **14** to manipulator assembly **2** so that different instruments may be rapidly changed during an endoscopic surgical procedure. As shown

in FIG. 3A, instrument support **70** comprises an annular collar **200** defining a central bore **202** for receiving shaft **100** of surgical instrument **14**. Collar **200** further defines an axially extending slot **204** in communication with bore **202** and sized to allow mounting and actuator pins **116**, **132** of instrument **14** to slide therethrough (see FIG. 4). Two locking slots **206** are cut into annular collar **200** at a transverse angle, preferably about 90°, to axially extending slot **204** (note that only one of the locking slots are shown in FIG. 3A). Locking slots **206** intersect slot **204** near the center of annular collar **200** and extend circumferentially around bore **202**, preferably about 90°, to allow rotation of both mounting pins **116** therethrough, as discussed below.

As shown in FIGS. 3A and 8, instrument support **70** further comprises means for locking mounting pins **116** into locking slots **206** so that the instrument cannot be accidentally twisted and thereby disengaged from instrument support **70** during surgery. Preferably, the locking means comprises a latch assembly having a plunger **210** slidably disposed within a hole **212** in collar **200**, as shown in FIG. 3A. Plunger **210** comprises an L-shaped latch **213** coupled to a release button **214** by a rod **215** extending through hole **212**. Plunger **210** is movable between a first position, where latch **213** is not disposed within locking slots **206** so that mounting pins **116** are free to rotate therethrough, and a second position, where latch **213** is at least partially disposed within one of the locking slots **206** so as to prevent rotation of mounting pins **116**. Latch **213** is preferably biased into the second or locked position by a compression spring **216**.

Button **214** is disposed on the upper surface of support **70** for manual actuation by the surgeon or automatic actuation by base **6**. Preferably, when instrument holder **4** is moved to its most proximal position (see FIG. 1), proximal support member **17** of frame **16** depresses release switch **214** to move latch **213** into the first or open position. With this configuration, instruments can be exchanged only when the instrument holder **4** is in the most proximal position, where shaft **100** of instrument **14** is easily accessible. In addition, this prevents the accidental release of the instrument when its distal end has penetrated cannula **50** and is disposed within the body cavity.

The intersecting axial and locking slots **204**, **206** form an interface for releasably coupling mounting pins **116** of surgical instrument **14** to instrument holder **4**. To insert instrument **14**, the surgeon aligns mounting pins **116** with axial slot **204** and slides the instrument through bore **202** of annular collar **200** until mounting pins **116** are aligned with locking slots **206**, as shown in FIG. 4. The instrument is then rotated a sufficient distance, preferably about a ¼ turn, through locking slots **206** so that the pins are no longer aligned with axial slot **204**. When instrument **14** is moved distally, switch **214** is released (FIG. 1) and latch **213** moves into locking slots **206** to prevent mounting pins **116** from rotating back into alignment with axial slot **204** so that instrument **14** is secured to instrument support **70**. It should be noted that a single mounting pin may be utilized with the above described configuration to lock the surgical instrument to the support. However, two opposing pins are preferred because this configuration reduces torsional forces on the inner surface of locking slots **206**.

As shown in FIG. 8, the locking means preferably includes a ball detent **217** disposed within collar **200**. Ball detent **217** is biased upward into one of the locking slots **206** by a spring **218**. Ball detent **217** serves to temporarily capture mounting pins **116** in a position rotated about 90° from alignment with axial slot **204**. This ensures that the mounting pins will be completely rotated into the proper position (i.e., out of the way of latch **213**) when instrument **14** is twisted into instru-

ment holder. Otherwise, when switch **214** is released, latch **213** could become engaged with mounting pins **216** so that the latch is unable to move completely into the locked position, thereby potentially causing the accidental release of instrument **14** during surgery.

As shown in FIGS. **3B**, **4** and **5**, actuator driver **80** of instrument holder **4** further comprises an actuator pin catch **220** for releasably holding and moving actuator pins **132** of instrument **14**. Actuator pin catch **220** is constructed similarly to instrument support **70** (FIG. **3A**), comprising an annular collar **222** that defines a bore **224** for receiving shaft **100** and an axially extending slot **226** for receiving actuator pins **132**. A locking slot **228** is cut into actuator pin catch **220** at a 90° angle so that actuator pins can be rotated into the lock slot to couple actuator pins **132** to actuator driver **66**, as discussed above in reference to the mounting pins. It should be noted that slot **226** need not extend completely through collar **222** since actuator pins **132** are located distally of mounting pins **116** (the instrument is preferably inserted jaws first). Of course, actuator and mounting pins **132**, **116** may be reversed so that the mounting pins are distal to the actuator pins, if desired.

Referring to FIG. **6A**, actuator pin catch **220** is rotatably mounted on a ball bearing **230** in actuator carriage assembly **90**. Bearing **230** allows the pin catch **220** to rotate freely in carriage assembly **90** while preventing relative axial motion. Therefore, when instrument **14** is rotated by first drive **8**, actuator pins **132** will rotate within carriage assembly **90**. Carriage assembly **90** further comprises two sets of axles **232** for rotatably supporting a pair of inner rollers **236** and a pair of outer rollers **238**. As shown in FIG. **1**, outer rollers **238** are slidably disposed within axial guide slots **82** of chassis **60** to prevent rotation of carriage assembly **90** with respect to chassis **60**. Inner and outer rollers **236**, **238** cooperate with helical actuator **84** and chassis **60** of instrument holder **4** to move axially with respect to the holder, thereby axially moving pin catch **220** and actuator pins **132** therewith relative to shaft **100** of instrument **14** (which actuates jaws **122**, **124**, as discussed above).

As shown in FIG. **6B**, helical actuator **84** includes a central bore **240** for receiving carriage assembly **90** and surgical instrument **14** and two opposing helical tracks **242**, **244** each extending circumferentially around helical actuator **84** (preferably slightly less than 180°) for receiving inner rollers **236** of carriage assembly **90**, as shown in FIG. **5**. With outer rollers **238** constrained in axial guide slots **82** of chassis **60**, rotation of helical actuator **84** causes carriage assembly **90** (and actuator pin catch **220**) to move up or down, depending on the sense of the rotation. Because of the symmetrical design of helical actuator **84**, the actuation force applied by second driver **10** will not generate any effective side loads on instrument **14**, which avoids frictional coupling with other degrees of freedom such as axial (third driver **12**) and rotation (first driver **8**). In the preferred embodiment, helical tracks **242**, **244** have a pitch selected such that the mechanism can be easily back-driven, allowing grip forces to be sensed in a position-served teleoperation system.

As shown in FIGS. **3A** and **3B**, instrument holder **4** further includes a pair of axial guide pins **250**, **252** fixed to instrument support **70**. Actuator pin catch **220** has a pair of openings **254**, **256** for receiving guide pins **250**, **252**. Guide pins **250**, **252** prevent relative rotation between pin catch **220** and support **70** (so that actuator and mounting pins **116**, **132** can both rotate with the instrument) and allow axial movement relative to each other (so that end effector **120** can be actuated by axial movement of actuator pins **132**).

FIG. **9** is an elevational view of a remote center positioner **300** which can be used to support manipulator assembly **2** above the patient (note that support manipulator **2** is not shown in FIG. **8**). Remote center positioner **300** provides two degrees of freedom for positioning manipulator assembly **2**, constraining it to rotate about a point **308** coincident with the entry incision. Preferably, point **308** will be approximately the center of bearing **54** in cannula **50** (FIG. **1**). A more complete description of remote center positioner **300** is described in commonly assigned co-pending application Ser. No. 08/062,404 filed May 14, 1993 REMOTE CENTER POSITIONER, which is incorporated herein by reference.

A first linkage means is indicated generally by the numeral **321** and a second linkage in the form of a parallelogram is indicated by the numeral **323**. The first linkage means is pivotally mounted on a base plate for rotation about an x-x axis. The second linkage means is pivotally connected to the first linkage means and is adapted to move in a plane parallel to the first linkage. Five link members (including extensions thereof), **311**, **312**, **313**, **314**, and **315** are connected together with pivot joints **316-320**. A portion of element **313** extends beyond pivot **320** of the parallelogram linkage. The parallelogram linkage has an operating end at link member **313** and a driving end at link member **312**. The elongated element **313** may, as desired later, carry a surgical instrument or other device, such as support bracket **24** of manipulator assembly **2**. The pivot joints allow relative motion of the link members only in the plane containing them.

A parallelogram linkage is formed by corresponding link members **314**, **315** and link members **312** and **313**. The portions of link members **314** and **315** of the parallelogram are of equal length as are the portions of members **312** and **313** of the parallelogram. These members are connected together in a parallelogram for relative movement only in the plane formed by the members. A rotatable joint generally indicated by the numeral **322** is connected to a suitable base **324**. The rotatable joint **322** is mounted on a base plate **326** adapted to be fixedly mounted to the base support means **324**. A pivot plate **328** is pivotally mounted to base plate **326** by suitable means at, such as, pivots **330**, **332**. Thus pivot plate **328** may be rotated about axis x-x through a desired angle **62**. This may be accomplished manually or by a suitable pivot drive motor **334**.

A first linkage is pivotally mounted on the pivot plate **328** of the rotatable joint **322**. The linkage elements **311**, **312** and the link members are relatively stiff or inflexible so that they may adequately support an instrument used in surgical operations. Rods made of aluminum or other metal are useful as such links. The linkage elements **311** and **312** are pivotally mounted on base plate **328** for rotation with respect to the rotatable joint by pivots **336** and **338**. At least one of the pivots **336**, **338** is positioned so that its axis of rotation is normal to and intersects the x-x axis. Movement may occur manually or may occur using a linkage drive motor **340**. The first linkage is also shaped in the form of a parallelogram formed by linkage elements **311**, and **312**; the portion of link member **315** connected thereto by pivots **316**, **318**; and base plate **328**. One of the link members **315** is thus utilized in both the first **321** and second **323** linkage means. Linkage element **312** also forms a common link of both the first linkage means **321** and the second linkage means **323**. In accordance with the invention, a remote center of spherical rotation **308** is provided by the above described embodiment of apparatus when the linkage element **311** is rotated and/or when pivot plate **328** is rotated about axis x-x. Thus, the end of element **313** can be

moved through desired angles **81** and **92** or rotated about its own axis, while the remote center of rotation remains at the same location.

FIG. **9** also shows an inclinometer **350** attached to the base of remote center positioner **300**. The remote center positioner may be mounted at an arbitrary orientation with respect to vertical depending on the particular surgery to be performed, and inclinometer **350** can be used to measure this orientation. The measured orientation can be used to calculate and implement servo control signals necessary to control the telerobotic system so as to prevent gravitational forces acting on the system mechanisms from being felt by the surgeon.

Reference now is made to FIG. **10** wherein the distal end portion or tip, **260** of the insertion section of an endoscope is shown which is a substantially the same type as shown in the above-mentioned publication entitled "Introduction to a New Project for National Research and Development Program (Large-Scale Project) in FY 1991" which endoscope may be used in the practice of the present invention. The insertion end of the endoscope includes a pair of spaced viewing windows **262R** and **262L** and an illumination source **264** for viewing and illuminating a workspace to be observed. Light received at the windows is focused by objective lens means, not shown, and transmitted through fiber-optic bundles to a pair of cameras at he operating end of the endoscope, now shown. The camera outputs are converted to a three-dimensional image of the workspace which image is located adjacent hand-operated means at the operator's station, now shown. Right and left steerable catheters **268R** and **268L** pass through accessory channels in the endoscope body, which catheters are adapted for extension from the distal end portion, as illustrated. End effectors **270R** and **270L** are provided at the ends of the catheters which may comprise conventional endoscopic instruments. Force sensors, not shown, also are inserted through the endoscope channels. Steerable catheters which include control wires for controlling bending of the catheters and operation of an end effector suitable for use with this invention are well known. Control motors for operation of the control wires are provided at the operating end of the endoscope, which motors are included in a servomechanism of a type described in U.S. patent application Ser. No. 07/823,932 for operation of the steerable catheters and associated end effectors from a remote operator's station. As with the other embodiments described in U.S. patent application Ser. No. 07/823,932, the interfacing computer in the servomechanism system remaps the operator's hand motion into the coordinate system of the end effectors, and images of the end effectors are viewable adjacent the hand-operated controllers. With this embodiment, the operator has the sensation of reaching through the endoscope to put his hands directly on the end effectors for control thereof. Endoscopes of different types may be employed in this embodiment of the invention so long as they include one or more accessory channels for use in control of end effectors means, and suitable viewing means for use in providing a visual display of the workspace. For example, gastric, colonscopic, and like type, endoscopes may be employed.

Variations and changes may be made by others without departing from the spirit of the present invention. For example, it should be understood that the present invention is not limited to endoscopic surgery. In fact, instrument holder **4**, along with a telerobotic control mechanism, would be particularly useful during open surgical procedures, allowing a surgeon to perform an operation from a remote location, such as a different room or a completely different hospital.

What is claimed is:

1. A manipulator assembly comprising:

a base,
an instrument holder removably mounted on the base,
a surgical instrument releasably coupled to the instrument holder, and
a drive assembly for manipulating the surgical instrument through the instrument holder, and for manipulating the instrument holder relative to the base in at least one degree of freedom; wherein the surgical instrument comprises:
an elongate shaft with one or more mounting pins laterally extending from the shaft;
the instrument holder comprising a support having a central bore, an axially extending slot for receiving the elongate shaft and the one or more mounting pins of the surgical instrument, and one or more locking slots cut into the support transversely to and in communication with the axial slot so that the one or more mounting pins can be rotated within corresponding of the one or more locking slots when received therein.

2. The manipulator assembly according to claim **1**, wherein the support further has a latch assembly for automatically locking the one or more mounting pins with the corresponding one or more locking slots to releasably couple the surgical instrument to the instrument holder.

3. The manipulator assembly according to claim **2**, wherein the latch assembly includes a latch element that is at least partially disposed within at least one of the locking slots so as to prevent rotation of the mounting pin received therein when the latch element is in a biased position, and is not disposed within any one the locking slots so that the one or more mounting pins received therein are free to rotate therethrough when latch element is in a release position.

4. The manipulator assembly according to claim **3**, wherein the latch element is maintained in the biased position by a compression spring and moved into the release position by compressing the compression spring.

5. The manipulator assembly according to claim **1**, wherein the surgical instrument comprises a shaft having a proximal end and a distal end, and a longitudinal axis defined therebetween; and the drive assembly comprises a first drive for rotating the surgical instrument around the longitudinal axis, a second drive for actuating an end effector on the distal end of the surgical instrument, and a third drive for displacing the surgical instrument along the longitudinal axis.

6. The manipulator assembly according to claim **5**, wherein the first drive, second drive and third drive are coupled to a controller mechanism via servo-control electronics for form a telerobotic system for operating the surgical instrument by remote control.

7. The manipulator assembly according to claim **5**, wherein the base comprises a frame; and the first drive comprises a rotation drive motor fixed to the frame and coupled to a first shaft by a first drive belt for rotating the first shaft with respect to the frame.

8. The manipulator assembly according to claim **7**, wherein the second drive comprises a gripper drive motor fixed to the frame and coupled to a second shaft by a second drive belt for rotating the second shaft with respect to the frame.

9. The manipulator assembly according to claim **8**, wherein the third drive comprises a vertical drive motor coupled to the instrument holder via a third drive belt and at least one pulley for axially displacing the instrument holder with respect to the frame.

10. The manipulator assembly according to claim **9**, wherein the instrument holder comprises a chassis mounted

13

on the first shaft and the second shaft respectively via first bearings and second bearings so that the chassis may move axially with respect to the first shaft and the second shaft, but is prevented from rotating with the first shaft and the second shaft.

11. The manipulator assembly according to claim 10, wherein the chassis includes a central cavity for receiving the surgical instrument, and a chassis arm laterally extending from the chassis and coupled to the third drive belt so that rotation of the third drive belt moves the instrument holder in the axial direction along the first shaft and the second shaft.

12. The manipulator assembly according to claim 11, wherein the chassis arm includes a toggle switch that can be rotated to release the chassis arm from the third drive belt.

13. The manipulator assembly according to claim 12, wherein the first bearings includes a first coupling mechanism for coupling and decoupling of the first shaft from the first bearings, and the second bearings includes a second coupling mechanism for coupling and decoupling of the second shaft from the second bearings.

14. The manipulator assembly according to claim 13, wherein the first coupling mechanism includes a first spring clip inserted between an annular groove formed on a distal end of the first shaft and an internal groove formed in a first support collar of the first bearings so as to hold the first shaft within the first support collar, and the second coupling mechanism includes a second spring clip inserted between an annular groove formed on a distal end of the second shaft and an internal groove formed in a second support collar of the second bearings so as to hold the second shaft within the second support collar.

14

15. A manipulator assembly comprising:

a surgical instrument,
an instrument holder releasably coupled through a twist lock mechanism to the surgical instrument, and
a drive assembly coupled to the surgical instrument through the instrument holder for manipulating the surgical instrument;

wherein the surgical instrument comprises an elongate shaft with one or more mounting pins laterally extending from the shaft; and the instrument holder comprises a support having a central bore, an axially extending slot for receiving the elongate shaft and the one or more mounting pins of the surgical instrument, and one or more locking slots cut into the support transversely to and in communication with the axial slot so that the one or more mounting pins can be rotated within corresponding of the one or more locking slots when received therein.

16. The manipulator assembly according to claim 15, wherein the support further has a latch assembly for automatically locking the one or more mounting pins with the corresponding one or more locking slots to releasably couple the surgical instrument to the instrument holder.

17. The manipulator assembly according to claim 16, wherein the latch assembly includes a latch element that is at least partially disposed within at least one of the locking slots so as to prevent rotation of the mounting pin received therein when the latch element is in a biased position, and is not disposed within any one of the locking slots so that the one or more mounting pins received therein are free to rotate there-through when latch element is in a release position.

18. The manipulator assembly according to claim 17, wherein the latch element is maintained in the biased position by a compression spring and moved into the release position by compressing the compression spring.

* * * * *

专利名称(译)	用于可释放地保持手术器械的系统和方法		
公开(公告)号	US7824424	公开(公告)日	2010-11-02
申请号	US11/195494	申请日	2005-08-01
[标]申请(专利权)人(译)	斯坦福研究院		
申请(专利权)人(译)	SRI国际公司		
当前申请(专利权)人(译)	SRI国际公司		
[标]发明人	JENSEN JOEL F GREEN PHILIP S		
发明人	JENSEN, JOEL F. GREEN, PHILIP S.		
IPC分类号	A61B17/28 A61B17/00 A61B19/00 B25J9/10 B25J15/04 B25J18/04		
CPC分类号	B25J9/1065 B25J15/04 B25J18/04 A61B19/22 A61B17/29 Y10T403/581 A61B2017/00464 A61B2017/2932 A61B2019/223 A61B2019/2234 A61B2019/2242 A61B2019/2292 A61B2019/265 A61B2017/00477 Y10T403/587 A61B34/35 A61B34/70 A61B34/71 A61B34/76 A61B2034/305 A61B2090/506		
其他公开文献	US20050283140A1		
外部链接	Espacenet USPTO		

摘要(译)

本发明涉及一种用于可释放地保持外科器械 (14) 的系统和方法, 所述外科器械 (14) 例如是内窥镜器械, 其配置成通过患者体内的小的经皮穿透来递送。该器械包括细长轴 (100), 该细长轴具有一对安装销 (116), 所述安装销 (116) 在其近端和远端之间从轴横向延伸。仪器支架包括支撑件, 该支撑件具有中心孔 (202) 和轴向延伸的槽 (204), 用于接收器械轴和安装销。一对锁定槽 (206) 横向于轴向槽切入支撑件并与轴向槽连通, 使得安装销可在锁定槽内旋转。器械支撑件还包括门锁组件, 用于自动地将安装销锁定在锁定槽内, 以将器械可释放地连接到器械保持器。通过这种扭锁操作, 外科医生可以在外科手术过程中快速地接合和脱离各种器械, 例如开放手术, 腹腔镜检查或胸腔镜检查。

