



US010335024B2

(12) **United States Patent**
Rentschler et al.

(10) **Patent No.:** **US 10,335,024 B2**
(45) **Date of Patent:** **Jul. 2, 2019**

(54) **MEDICAL INFLATION, ATTACHMENT AND DELIVERY DEVICES AND RELATED METHODS**

1/32; A61B 2017/00876; A61B 2017/00345; A61B 19/26; A61B 2019/2253; A61B 2019/2249; A61B 2017/00292; A61B 2017/00349; A61M 29/02

(71) Applicant: **Board of Regents of the University of Nebraska**, Lincoln, NE (US)

USPC 606/108, 191, 198, 200, 192; 600/123, 600/139, 37, 204-209; 623/1.11, 1.12; 604/528-532

(72) Inventors: **Mark Rentschler**, Boulder, CO (US); **Shane Farritor**, Lincoln, NE (US)

See application file for complete search history.

(73) Assignee: **Board of Regents of the University of Nebraska**, Lincoln, NE (US)

(56) **References Cited**

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 207 days.

U.S. PATENT DOCUMENTS

3,870,264 A 3/1975 Robinson
3,989,952 A 11/1976 Timberlake et al.
(Continued)

(21) Appl. No.: **15/018,530**

FOREIGN PATENT DOCUMENTS

(22) Filed: **Feb. 8, 2016**

CN 1082821918 12/2012
DE 102010040405 3/2012
(Continued)

(65) **Prior Publication Data**

US 2016/0157709 A1 Jun. 9, 2016

Related U.S. Application Data

OTHER PUBLICATIONS

(63) Continuation of application No. 12/192,663, filed on Aug. 15, 2008, now abandoned.
(Continued)

International Preliminary Report on Patentability from related case PCT/US2007/014567, dated Jan. 8, 2009, 11 pp.
(Continued)

(51) **Int. Cl.**
A61M 29/00 (2006.01)
A61B 1/313 (2006.01)
(Continued)

Primary Examiner — Amy R Weisberg
(74) *Attorney, Agent, or Firm* — Davis, Brown, Koehn, Shors & Roberts, P.C.; Sean D. Solberg


(52) **U.S. Cl.**
CPC *A61B 1/3132* (2013.01); *A61B 17/0218* (2013.01); *A61B 17/0281* (2013.01);
(Continued)

(57) **ABSTRACT**

The various embodiments disclosed herein relate to procedural space maintenance devices, medical device positioning devices, and devices that provide both procedural space maintenance and device positioning. Further embodiments relate to medical device insertion and/or retraction devices.

(58) **Field of Classification Search**
CPC A61B 17/0281; A61B 17/0218; A61B 2017/00283; A61B 2019/2215; A61B 2017/00557; A61B 2017/0042; A61B

20 Claims, 16 Drawing Sheets

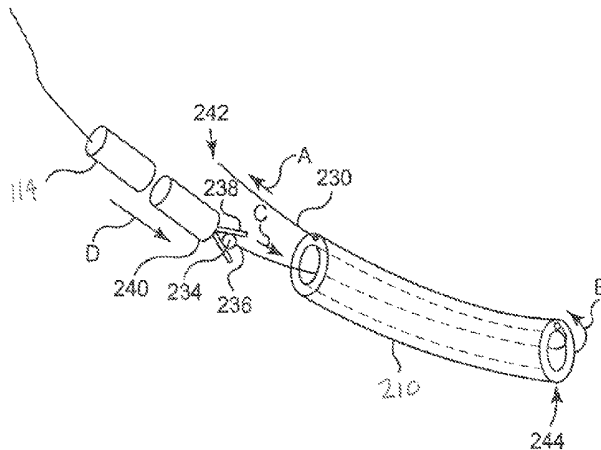

Related U.S. Application Data

		5,515,478 A	5/1996	Wang
		5,524,180 A	6/1996	Wang et al.
		5,553,198 A	9/1996	Wang et al.
(60)	Provisional application No. 60/956,032, filed on Aug. 15, 2007, provisional application No. 60/990,062, filed on Nov. 26, 2007, provisional application No. 60/990,470, filed on Nov. 27, 2007.	5,562,448 A	10/1996	Mushabac
		5,588,442 A	12/1996	Scovil et al.
		5,620,417 A	4/1997	Jang et al.
		5,623,582 A	4/1997	Rosenberg
		5,624,380 A	4/1997	Shuichi et al.
(51)	Int. Cl.	5,624,398 A	4/1997	Smith et al.
	<i>A61B 17/02</i> (2006.01)	5,632,761 A	5/1997	Smith et al.
	<i>A61B 34/00</i> (2016.01)	5,645,520 A	7/1997	Nakamura et al.
	<i>A61B 17/34</i> (2006.01)	5,657,429 A	8/1997	Wang et al.
	<i>A61B 1/32</i> (2006.01)	5,657,584 A	8/1997	Hamlin
	<i>A61B 17/00</i> (2006.01)	5,672,168 A	9/1997	de la Torre et al.
	<i>A61B 34/30</i> (2016.01)	5,674,030 A	10/1997	Sigel
	<i>A61B 90/50</i> (2016.01)	5,728,599 A	3/1998	Rosteker et al.
(52)	U.S. Cl.	5,736,821 A	4/1998	Suyama et al.
	CPC <i>A61B 17/3468</i> (2013.01); <i>A61B 34/30</i> (2016.02); <i>A61B 34/72</i> (2016.02); <i>A61B 34/73</i> (2016.02); <i>A61B 1/32</i> (2013.01); <i>A61B 90/50</i> (2016.02); <i>A61B 2017/0042</i> (2013.01); <i>A61B 2017/00283</i> (2013.01); <i>A61B 2017/00292</i> (2013.01); <i>A61B 2017/00345</i> (2013.01); <i>A61B 2017/00349</i> (2013.01); <i>A61B 2017/00557</i> (2013.01); <i>A61B 2017/00876</i> (2013.01); <i>A61B 2017/0225</i> (2013.01); <i>A61B 2034/301</i> (2016.02); <i>A61B 2034/302</i> (2016.02)	5,754,741 A	5/1998	Wang et al.
		5,762,458 A	6/1998	Wang et al.
		5,769,640 A	6/1998	Jacobus et al.
		5,791,231 A	8/1998	Cohn et al.
		5,792,135 A	8/1998	Madhani et al.
		5,797,538 A	8/1998	Heaton et al.
		5,797,900 A	8/1998	Madhani et al.
		5,807,377 A	9/1998	Madhani et al.
		5,808,665 A	9/1998	Green
		5,815,640 A	9/1998	Wang et al.
		5,825,982 A	10/1998	Wright et al.
		5,841,950 A	11/1998	Wang et al.
		5,845,646 A	12/1998	Lemelson
		5,855,583 A	1/1999	Wang et al.
		5,876,325 A	3/1999	Mizuno et al.
(56)	References Cited	5,878,193 A	3/1999	Wang et al.
	U.S. PATENT DOCUMENTS	5,878,783 A	3/1999	Smart
		5,895,417 A *	4/1999	Pomeranz A61B 17/00234 606/41

4,246,661 A	1/1981	Pinson	5,906,591 A	5/1999	Dario et al.
4,258,716 A	3/1981	Sutherland	5,907,664 A	5/1999	Wang et al.
4,278,077 A	7/1981	Mizumoto	5,910,129 A	6/1999	Koblish et al.
4,538,594 A	9/1985	Boebel et al.	5,911,036 A	6/1999	Wright et al.
4,568,311 A	2/1986	Miyaki	5,971,976 A	10/1999	Wang et al.
4,623,183 A	11/1986	Amori	5,993,467 A	11/1999	Yoon
4,736,645 A	4/1988	Zimmer	6,001,108 A	12/1999	Wang et al.
4,771,652 A	9/1988	Zimmer	6,007,550 A	12/1999	Wang et al.
4,852,391 A	8/1989	Ruch et al.	6,030,365 A	2/2000	Laufer
4,896,015 A	1/1990	Taboada et al.	6,031,371 A	2/2000	Smart
4,897,014 A	1/1990	Tietze	6,058,323 A	5/2000	Lemelson
4,922,755 A	5/1990	Oshiro et al.	6,063,095 A	5/2000	Wang et al.
4,922,782 A	5/1990	Kawai	6,066,090 A	5/2000	Yoon
4,990,050 A	2/1991	Tsuge et al.	6,102,850 A	8/2000	Wang et al.
5,019,968 A	5/1991	Wang et al.	6,107,795 A	8/2000	Smart
5,108,140 A	4/1992	Bartholet	6,132,368 A	10/2000	Cooper
5,172,639 A	12/1992	Wiesman et al.	6,132,441 A	10/2000	Grace
5,176,649 A	1/1993	Wakabayashi	6,139,563 A	10/2000	Cosgrove, III et al.
5,178,032 A	1/1993	Zona et al.	6,156,006 A	12/2000	Brosens et al.
5,187,032 A	2/1993	Sasaki et al.	6,159,146 A	12/2000	El Gazayerli
5,187,796 A	2/1993	Wang et al.	6,162,171 A	12/2000	Ng et al.
5,195,388 A	3/1993	Zona et al.	D438,617 S	3/2001	Cooper et al.
5,201,325 A	4/1993	McEwen et al.	6,206,903 B1	3/2001	Ramans
5,217,003 A	6/1993	Wilk	D441,076 S	4/2001	Cooper et al.
5,263,382 A	11/1993	Brooks et al.	6,223,100 B1	4/2001	Green
5,271,384 A	12/1993	McEwen et al.	D441,862 S	5/2001	Cooper et al.
5,284,096 A	2/1994	Pelrine et al.	6,238,415 B1	5/2001	Sepetka et al.
5,297,443 A	3/1994	Wentz	6,240,312 B1	5/2001	Alfano et al.
5,297,536 A	3/1994	Wilk	6,241,730 B1	6/2001	Alby
5,304,899 A	4/1994	Sasaki et al.	6,244,809 B1	6/2001	Wang et al.
5,307,447 A	4/1994	Asano et al.	6,246,200 B1	6/2001	Blumenkranz et al.
5,353,807 A	10/1994	DeMarco	D444,555 S	7/2001	Cooper et al.
5,363,935 A	11/1994	Schempf et al.	6,286,514 B1	9/2001	Lemelson
5,382,885 A	1/1995	Salcudean et al.	6,292,678 B1	9/2001	Hall et al.
5,388,528 A	2/1995	Pelrine et al.	6,293,282 B1	9/2001	Lemelson
5,411,550 A *	5/1995	Herweck A61F 2/06 600/36	6,296,635 B1	10/2001	Smith et al.
			6,309,397 B1	10/2001	Julian et al.
5,436,542 A	7/1995	Petelin et al.	6,309,403 B1	10/2001	Minaret et al.
5,441,494 A	8/1995	Ortiz	6,312,435 B1	11/2001	Wallace et al.
5,458,131 A	10/1995	Wilk	6,321,106 B1	11/2001	Lemelson
5,458,583 A	10/1995	McNeely et al.	6,327,492 B1	12/2001	Lemelson
5,458,598 A	10/1995	Feinberg et al.	6,331,181 B1	12/2001	Tiemey et al.
5,471,515 A	11/1995	Fossum et al.	6,346,072 B1	2/2002	Cooper

(56)

References Cited

U.S. PATENT DOCUMENTS

6,352,503	B1	3/2002	Matsui et al.	6,799,088	B2	9/2004	Wang et al.
6,364,888	B1	4/2002	Niemeyer et al.	6,801,325	B2	10/2004	Farr et al.
6,371,952	B1	4/2002	Madhani et al.	6,804,581	B2	10/2004	Wang et al.
6,394,998	B1	5/2002	Wallace et al.	6,810,281	B2	10/2004	Brock et al.
6,398,726	B1	6/2002	Ramans et al.	6,817,972	B2	11/2004	Snow
6,400,980	B1	6/2002	Lemelson	6,817,974	B2	11/2004	Cooper et al.
6,408,224	B1	6/2002	Lemelson	6,817,975	B1	11/2004	Farr et al.
6,424,885	B1	7/2002	Niemeyer et al.	6,820,653	B1	11/2004	Schempf et al.
6,432,112	B2	8/2002	Brock et al.	6,824,508	B2	11/2004	Kim et al.
6,436,107	B1	8/2002	Wang et al.	6,824,510	B2	11/2004	Kim et al.
6,441,577	B2	8/2002	Blumenkranz et al.	6,832,988	B2	12/2004	Sprout
6,450,104	B1	9/2002	Grant et al.	6,832,996	B2	12/2004	Woloszko et al.
6,451,027	B1	9/2002	Cooper et al.	6,836,703	B2	12/2004	Wang et al.
6,454,758	B1	9/2002	Thompson et al.	6,837,846	B2	1/2005	Jaffe et al.
6,459,926	B1	10/2002	Nowlin et al.	6,837,883	B2	1/2005	Moll et al.
6,463,361	B1	10/2002	Wang et al.	6,839,612	B2	1/2005	Sanchez et al.
6,468,203	B2	10/2002	Belson	6,840,938	B1	1/2005	Morley et al.
6,468,265	B1	10/2002	Evans et al.	6,852,107	B2	2/2005	Wang et al.
6,470,236	B2	10/2002	Ohtsuki	6,858,003	B2	2/2005	Evans et al.
6,491,691	B1	12/2002	Morley et al.	6,860,346	B2	3/2005	Burt et al.
6,491,701	B2	12/2002	Nemeyer et al.	6,860,877	B1	3/2005	Sanchez et al.
6,493,608	B1	12/2002	Niemeyer et al.	6,866,671	B2	3/2005	Tiemey et al.
6,496,099	B2	12/2002	Wang et al.	6,870,343	B2	3/2005	Borenstein et al.
6,508,413	B2	1/2003	Bauer et al.	6,871,117	B2	3/2005	Wang et al.
6,512,345	B2	1/2003	Borenstein	6,871,563	B2	3/2005	Choset et al.
6,522,906	B1	2/2003	Salisbury, Jr. et al.	6,879,880	B2	4/2005	Nowlin et al.
6,544,276	B1	4/2003	Azizi	6,892,112	B2	5/2005	Wang et al.
6,548,982	B1	4/2003	Papanikolopoulos et al.	6,899,705	B2	5/2005	Niemeyer
6,554,790	B1	4/2003	Moll	6,902,560	B1	6/2005	Morley et al.
6,565,554	B1	5/2003	Niemeyer	6,905,460	B2	6/2005	Wang et al.
6,574,355	B2	6/2003	Green	6,905,491	B1	6/2005	Wang et al.
6,587,750	B2	7/2003	Gerbi et al.	6,911,916	B1	6/2005	Wang et al.
6,591,239	B1	7/2003	McCall et al.	6,917,176	B2	7/2005	Schempf et al.
6,594,552	B1	7/2003	Nowlin et al.	6,933,695	B2	8/2005	Blumenkranz
6,610,007	B2	8/2003	Belson	6,936,001	B1	8/2005	Snow
6,620,173	B2	9/2003	Gerbi et al.	6,936,003	B2	8/2005	Iddan
6,642,836	B1	11/2003	Wang et al.	6,936,042	B2	8/2005	Wallace et al.
6,645,196	B1	11/2003	Nixon et al.	6,943,663	B2	9/2005	Wang et al.
6,646,541	B1	11/2003	Wang et al.	6,949,096	B2	9/2005	Davison et al.
6,648,814	B2	11/2003	Kim et al.	6,951,535	B2	10/2005	Ghodoussi et al.
6,659,939	B2	12/2003	Moll et al.	6,965,812	B2	11/2005	Wang et al.
6,661,571	B1	12/2003	Shioda et al.	6,974,411	B2	12/2005	Belson
6,671,581	B2	12/2003	Niemeyer et al.	6,974,449	B2	12/2005	Niemeyer
6,676,684	B1	1/2004	Morley et al.	6,979,423	B2	12/2005	Moll
6,684,129	B2	1/2004	Salisbury, Jr. et al.	6,984,203	B2	1/2006	Tartaglia et al.
6,685,648	B2	2/2004	Flaherty et al.	6,984,205	B2	1/2006	Gazdzinski
6,685,698	B2	2/2004	Morley et al.	6,991,627	B2	1/2006	Madhani et al.
6,687,571	B1	2/2004	Byrne et al.	6,993,413	B2	1/2006	Sunaoshi
6,692,485	B1	2/2004	Brock et al.	6,994,703	B2	2/2006	Wang et al.
6,699,177	B1	3/2004	Wang et al.	6,994,708	B2	2/2006	Manzo
6,699,235	B2	3/2004	Wallace et al.	6,997,908	B2	2/2006	Carrillo, Jr. et al.
6,702,734	B2	3/2004	Kim et al.	7,025,064	B2	4/2006	Wang et al.
6,702,805	B1	3/2004	Stuart	7,027,892	B2	4/2006	Wang et al.
6,714,839	B2	3/2004	Salisbury, Jr. et al.	7,033,344	B2	4/2006	Imran
6,714,841	B1	3/2004	Wright et al.	7,039,453	B2	5/2006	Mullick
6,719,684	B2	4/2004	Kim et al.	7,042,184	B2	5/2006	Oleynikov et al.
6,720,988	B1	4/2004	Gere et al.	7,048,745	B2	5/2006	Tierney et al.
6,726,699	B1	4/2004	Wright et al.	7,053,752	B2	5/2006	Wang et al.
6,728,599	B2	4/2004	Wright et al.	7,063,682	B1	6/2006	Whayne et al.
6,730,021	B2	5/2004	Vassiliades, Jr. et al.	7,066,879	B2	6/2006	Fowler et al.
6,731,988	B1	5/2004	Green	7,066,926	B2	6/2006	Wallace et al.
6,746,443	B1	6/2004	Morley et al.	7,074,179	B2	7/2006	Wang et al.
6,764,441	B2	7/2004	Chiel et al.	7,077,446	B2	7/2006	Kameda et al.
6,764,445	B2	7/2004	Ramans et al.	7,083,571	B2	8/2006	Wang et al.
6,766,204	B2	7/2004	Niemeyer et al.	7,083,615	B2	8/2006	Peterson et al.
6,770,081	B1	8/2004	Cooper et al.	7,087,049	B2	8/2006	Nowlin et al.
6,774,597	B1	8/2004	Borenstein	7,090,683	B2	8/2006	Brock et al.
6,776,165	B2	8/2004	Jin	7,097,640	B2	8/2006	Wang et al.
6,780,184	B2	8/2004	Tanrisever	7,105,000	B2	9/2006	McBrayer
6,783,524	B2	8/2004	Anderson et al.	7,107,090	B2	9/2006	Salisbury, Jr. et al.
6,785,593	B2	8/2004	Wang et al.	7,109,678	B2	9/2006	Kraus et al.
6,788,018	B1	9/2004	Blumenkranz	7,118,582	B1	10/2006	Wang et al.
6,792,663	B2	9/2004	Krzyzanowski	7,121,781	B2	10/2006	Sanchez et al.
6,793,653	B2	9/2004	Sanchez et al.	7,125,403	B2	10/2006	Julian et al.
6,799,065	B1	9/2004	Niemeyer	7,126,303	B2	10/2006	Farritor et al.
				7,147,650	B2	12/2006	Lee
				7,155,315	B2	12/2006	Niemeyer et al.
				7,169,141	B2	1/2007	Brock et al.
				7,182,025	B2	2/2007	Ghorbel et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,182,089	B2	2/2007	Ries	2004/0034302	A1	2/2004	Abovitz et al.
7,199,545	B2	4/2007	Oleynikov et al.	2004/0050394	A1	3/2004	Jin
7,206,626	B2	4/2007	Quaid, III	2004/0070822	A1	4/2004	Shioda et al.
7,206,627	B2	4/2007	Abovitz et al.	2004/0099175	A1	5/2004	Perrot et al.
7,210,364	B2	5/2007	Ghorbel et al.	2004/0102772	A1	5/2004	Baxter et al.
7,214,230	B2	5/2007	Brock et al.	2004/0106916	A1	6/2004	Quaid et al.
7,217,240	B2	5/2007	Snow	2004/0111113	A1	6/2004	Nakamura et al.
7,239,940	B2	7/2007	Wang et al.	2004/0138525	A1	7/2004	Saadat
7,250,028	B2	7/2007	Julian et al.	2004/0138552	A1	7/2004	Harel et al.
7,259,652	B2	8/2007	Wang et al.	2004/0140786	A1	7/2004	Borenstein
7,273,488	B2	9/2007	Nakamura et al.	2004/0153057	A1	8/2004	Davison
7,311,107	B2	12/2007	Harel et al.	2004/0173116	A1	9/2004	Ghorbel et al.
7,339,341	B2	3/2008	Oleynikov et al.	2004/0176664	A1	9/2004	Iddan
7,372,229	B2	5/2008	Farritor et al.	2004/0215331	A1	10/2004	Chew et al.
7,447,537	B1	11/2008	Funda et al.	2004/0225229	A1	11/2004	Viola
7,492,116	B2	2/2009	Oleynikov et al.	2004/0254680	A1	12/2004	Sunaoshi
7,566,300	B2	7/2009	Devierre et al.	2004/0267326	A1	12/2004	Ocel et al.
7,574,250	B2	8/2009	Niemeyer	2005/0014994	A1	1/2005	Fowler et al.
7,637,905	B2	12/2009	Saadat et al.	2005/0021069	A1	1/2005	Feuer et al.
7,645,230	B2	1/2010	Mikkaichi et al.	2005/0029978	A1	2/2005	Oleynikov et al.
7,655,004	B2	2/2010	Long	2005/0043583	A1	2/2005	Killmann et al.
7,670,329	B2	3/2010	Flaherty et al.	2005/0049462	A1	3/2005	Kanazawa
7,731,727	B2	6/2010	Sauer	2005/0054901	A1	3/2005	Yoshino
7,762,825	B2	7/2010	Burbank et al.	2005/0054902	A1	3/2005	Konno
7,772,796	B2	8/2010	Farritor et al.	2005/0064378	A1	3/2005	Toly
7,785,251	B2	8/2010	Wilk	2005/0065400	A1	3/2005	Banik et al.
7,785,333	B2	8/2010	Miyamoto et al.	2005/0083460	A1	4/2005	Hattori et al.
7,789,825	B2	9/2010	Nobis et al.	2005/0095650	A1	5/2005	Khalili et al.
7,794,494	B2	9/2010	Sahatjian et al.	2005/0096502	A1	5/2005	Khalili
7,865,266	B2	1/2011	Moll et al.	2005/0143644	A1	6/2005	Gilad et al.
7,960,935	B2	6/2011	Farritor et al.	2005/0154376	A1	7/2005	Riviere et al.
8,021,358	B2	9/2011	Doyle et al.	2005/0165449	A1	7/2005	Cadeddu et al.
8,179,073	B2	5/2012	Farritor et al.	2005/0283137	A1	12/2005	Doyle et al.
8,353,897	B2	1/2013	Doyle et al.	2005/0288555	A1	12/2005	Binmoeller
9,089,353	B2	7/2015	Farritor	2005/0288665	A1	12/2005	Woloszko
2001/0018591	A1	8/2001	Brock et al.	2006/0020272	A1	1/2006	Gildenberg
2001/0049497	A1	12/2001	Kaloo et al.	2006/0046226	A1	3/2006	Bergler et al.
2002/0003173	A1	1/2002	Bauer et al.	2006/0119304	A1	6/2006	Farritor et al.
2002/0013601	A1	1/2002	Nobles et al.	2006/0149135	A1	7/2006	Paz
2002/0026186	A1	2/2002	Woloszka et al.	2006/0152591	A1	7/2006	Lin
2002/0038077	A1	3/2002	de la Torre et al.	2006/0155263	A1	7/2006	Lipow
2002/0065507	A1	5/2002	Azizi	2006/0195015	A1	8/2006	Mullick et al.
2002/0091374	A1	7/2002	Cooper	2006/0196301	A1	9/2006	Oleynikov et al.
2002/0103417	A1	8/2002	Gazdzinski	2006/0198619	A1	9/2006	Oleynikov et al.
2002/0111535	A1	8/2002	Kim et al.	2006/0241570	A1	10/2006	Wilk
2002/0120254	A1	8/2002	Julien et al.	2006/0241732	A1	10/2006	Denker
2002/0128552	A1	9/2002	Nowlin et al.	2006/0253109	A1	11/2006	Chu
2002/0140392	A1	10/2002	Borenstein et al.	2006/0258954	A1	11/2006	Timberlake et al.
2002/0147487	A1	10/2002	Sundquist et al.	2007/0032701	A1	2/2007	Fowler et al.
2002/0151906	A1	10/2002	Demarais et al.	2007/0043397	A1	2/2007	Ocel et al.
2002/0156347	A1	10/2002	Kim et al.	2007/0055342	A1	3/2007	Wu et al.
2002/0171385	A1	11/2002	Kim et al.	2007/0080658	A1	4/2007	Farritor et al.
2002/0173700	A1	11/2002	Kim et al.	2007/0106113	A1	5/2007	Ravo
2002/0190682	A1	12/2002	Schempf et al.	2007/0123748	A1	5/2007	Meglan
2003/0020810	A1	1/2003	Takizawa et al.	2007/0142725	A1	6/2007	Hardin et al.
2003/0045888	A1	3/2003	Brock et al.	2007/0156019	A1	7/2007	Larkin et al.
2003/0065250	A1	4/2003	Chiel et al.	2007/0156211	A1	7/2007	Ferren et al.
2003/0089267	A1	5/2003	Ghorbel et al.	2007/0167955	A1	7/2007	De La Menardiere et al.
2003/0092964	A1	5/2003	Kim et al.	2007/0225633	A1	9/2007	Ferren et al.
2003/0097129	A1	5/2003	Davison et al.	2007/0225634	A1	9/2007	Ferren et al.
2003/0100817	A1	5/2003	Wang et al.	2007/0241714	A1	10/2007	Okeynikov et al.
2003/0114731	A1	6/2003	Cadeddu et al.	2007/0244520	A1	10/2007	Ferren et al.
2003/0135203	A1	7/2003	Wang et al.	2007/0250064	A1	10/2007	Darois et al.
2003/0139742	A1	7/2003	Wampler et al.	2007/0255273	A1	11/2007	Fernandez et al.
2003/0144656	A1	7/2003	Ocel et al.	2008/0004634	A1	1/2008	Farritor et al.
2003/0167000	A1	9/2003	Mullick	2008/0015565	A1	1/2008	Davison
2003/0172871	A1	9/2003	Scherer	2008/0015566	A1	1/2008	Livneh
2003/0179308	A1	9/2003	Zamorano et al.	2008/0033569	A1	2/2008	Ferren et al.
2003/0181788	A1	9/2003	Yokoi et al.	2008/0045803	A1	2/2008	Williams
2003/0229268	A1	12/2003	Uchiyama et al.	2008/0058835	A1	3/2008	Farritor et al.
2003/0230372	A1	12/2003	Schmidt	2008/0058989	A1	3/2008	Oleynikov et al.
2004/0117032	A1	1/2004	Roth et al.	2008/0103440	A1	5/2008	Ferren et al.
2004/0024311	A1	2/2004	Quaid	2008/0109014	A1	5/2008	de la Pena
2004/0034282	A1	2/2004	Quaid	2008/0111513	A1	5/2008	Farritor et al.
2004/0034283	A1	2/2004	Quaid	2008/0119870	A1	5/2008	Williams et al.
				2008/0132890	A1	6/2008	Woloszko et al.
				2008/0161804	A1	7/2008	Rioux et al.
				2008/0164079	A1	7/2008	Ferren et al.
				2008/0183033	A1	7/2008	Bern et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0221591 A1 9/2008 Farritor et al.
 2008/0269557 A1 10/2008 Marescaux et al.
 2008/0269562 A1 10/2008 Marescaux et al.
 2009/0020724 A1 1/2009 Paffrath
 2009/0024142 A1 1/2009 Ruiz Morales
 2009/0048612 A1 2/2009 Farritor et al.
 2009/0054909 A1 2/2009 Farritor et al.
 2009/0069821 A1 3/2009 Farritor et al.
 2009/0076536 A1 3/2009 Rentschler et al.
 2009/0137952 A1 5/2009 Ramamurthy et al.
 2009/0143787 A9 6/2009 De La Pena
 2009/0163929 A1 6/2009 Yeung et al.
 2009/0171373 A1 7/2009 Farritor et al.
 2009/0234369 A1 9/2009 Bax et al.
 2009/0236400 A1 9/2009 Cole et al.
 2009/0240246 A1 9/2009 Devill et al.
 2009/0247821 A1 10/2009 Rogers
 2009/0248038 A1 10/2009 Blumenkranz et al.
 2009/0281377 A1 11/2009 Newell et al.
 2009/0305210 A1 12/2009 Guru et al.
 2010/0010294 A1 1/2010 Conlon et al.
 2010/0016659 A1 1/2010 Weitzner et al.
 2010/0016853 A1 1/2010 Burbank
 2010/0042097 A1 2/2010 Newton et al.
 2010/0056863 A1 3/2010 Dejima et al.
 2010/0069710 A1 3/2010 Yamatani et al.
 2010/0069940 A1 3/2010 Miller et al.
 2010/0081875 A1 4/2010 Fowler et al.
 2010/0139436 A1 6/2010 Kawashima et al.
 2010/0198231 A1 8/2010 Manzo et al.
 2010/0204713 A1 8/2010 Ruiz
 2010/0245549 A1 9/2010 Allen et al.
 2010/0262162 A1 10/2010 Omori
 2010/0292691 A1 11/2010 Brogna
 2010/0318059 A1 12/2010 Farritor et al.
 2011/0015569 A1 1/2011 Kirschenman et al.
 2011/0020779 A1 1/2011 Hannaford et al.
 2011/0071347 A1 3/2011 Rogers et al.
 2011/0071544 A1 3/2011 Steger et al.
 2011/0077478 A1 3/2011 Freeman et al.
 2011/0098529 A1 4/2011 Ostrovsky et al.
 2011/0152615 A1 6/2011 Schostek et al.
 2011/0224605 A1 9/2011 Farritor et al.
 2011/0230894 A1 9/2011 Simaan et al.
 2011/0237890 A1 9/2011 Farritor et al.
 2011/0238080 A1 9/2011 Ranjit et al.
 2011/0264078 A1 10/2011 Lipow
 2011/0270443 A1 11/2011 Kamiya et al.
 2012/0035582 A1 2/2012 Nelson et al.
 2012/0109150 A1 5/2012 Quaid et al.
 2012/0116362 A1 5/2012 Kieturakis
 2012/0179168 A1 7/2012 Farritor
 2012/0253515 A1 10/2012 Coste-Maniere et al.
 2013/0041360 A1 2/2013 Farritor
 2013/0131695 A1 5/2013 Scarfogliero et al.
 2013/0345717 A1 5/2013 Scarfogliero et al.
 2014/0039515 A1 2/2014 Mondry et al.
 2014/0046340 A1 2/2014 Wilson et al.
 2014/0058205 A1 2/2014 Frederick et al.
 2014/0303434 A1 10/2014 Farritor et al.
 2015/0051446 A1 2/2015 Farritor et al.

FOREIGN PATENT DOCUMENTS

EP 1354670 10/2003
 EP 2286756 2/2011
 EP 2286756 A1 2/2011
 EP 2329787 8/2011
 EP 2563261 3/2013
 JP 2004144533 5/1990
 JP 5115425 5/1993
 JP 200716235 6/1993
 JP 2006507809 9/1994
 JP 07 136173 5/1995
 JP 7306155 11/1995

JP 08-224248 9/1996
 JP 2001500510 1/2001
 JP 2001505810 5/2001
 JP 2003220065 8/2003
 JP 2004322310 6/2004
 JP 2004180781 7/2004
 JP 2004329292 11/2004
 JP 2006508049 3/2006
 JP 2009-106606 5/2009
 JP 2010-533045 10/2010
 JP 2010-536436 12/2010
 JP 2011-504794 2/2011
 JP 2011-045500 3/2011
 JP 2011-115591 6/2011
 WO WO 1992/21291 5/1991
 WO WO 0189405 11/2001
 WO WO 2002/082979 10/2002
 WO WO 2002/100256 12/2002
 WO WO 2005/009211 7/2004
 WO WO 2005044095 5/2005
 WO WO 2006/052927 8/2005
 WO WO 2006 005075 1/2006
 WO WO 2006/079108 1/2006
 WO WO2006079108 7/2006
 WO WO 2007011654 1/2007
 WO WO 2007/111571 10/2007
 WO WO 2007/149559 12/2007
 WO WO 2009023851 A1 8/2008
 WO WO 2009/144729 12/2009
 WO WO2010/042611 4/2010
 WO WO2010/046823 4/2010
 WO WO201050771 A2 5/2010
 WO WO 2011/118646 A1 9/2011
 WO WO 2011/135503 A1 11/2011
 WO WO 2011135503 11/2011
 WO WO 2011075693 7/2012
 WO WO 2013009887 1/2013
 WO WO 2014011238 1/2014

OTHER PUBLICATIONS

International Search report and Written Opinion from international application No. PCT/US2012/41911, dated Mar. 13, 2013.
 International Search Report and Written Opinion from international application No. PCT/US12/46274, dated Sep. 25, 2012.
 International Search Report and Written Opinion from international application No. PCT/US2007/089191, dated Nov. 10, 2008, 20 pp.
 "International Search Report and Written Opinion from international application No. PCT/US07/14567, dated Apr. 28, 2008, 19 pp."
 International Search Report and Written Opinion of international application No. PCT/US2008/069822, dated Aug. 5, 2009, 12 pp.
 International Search Report and Written Opinion of international application No. PCT/US2008/073334, dated Jan. 12, 2009, 11 pp.
 International Search Report and Written Opinion of international application No. PCT/US2008/073369, dated Nov. 12, 2008, 12 pp.
 International Search Report and Written Opinion issued in PCT/US11/46809, dated Dec. 8, 2011.
 Ishiyama et al., "Spiral-type Micro-machine for Medical Applications," 2000 International Symposium on Micromechatronics and Human Science, 2000: 65-69.
 Jagannath et al., "Peroral transgastric endoscopic ligation of fallopian tubes with long-term survival in a porcine model," *Gastrointestinal Endoscopy*, 2005; 61(3): 449-453.
 Kalloo et al., "Flexible transgastric peritoneoscopy: a novel approach to diagnostic and therapeutic interventions in the peritoneal cavity," *Gastrointestinal Endoscopy*, 2004; 60(1): 114-117.
 Kang et al., "Robotic Assistants Aid Surgeons During Minimally Invasive Procedures," *IEEE Engineering in Medicine and Biology*, Jan.-Feb. 2001; pp. 94-104.
 Kantsevov et al., "Endoscopic gastrojejunostomy with survival in a porcine model," *Gastrointestinal Endoscopy*, 2005; 62(2): 287-292.
 Kantsevov et al., "Transgastric endoscopic splenectomy," *Surgical Endoscopy*, 2006; 20: 522-525.

(56)

References Cited

OTHER PUBLICATIONS

- Kazemier et al. (1998), "Vascular Injuries During Laparoscopy," *J. Am. Coli. Surg.* 186(5): 604-5.
- Kim, "Early Experience with Telesurgical Robot-Assisted Laparoscopic Cholecystectomy Using da Vinci," *Surgical Laparoscopy, Endoscopy & Percutaneous Techniques*, 2002; 12(1):33-40.
- Ko et al., "Per-Oral transgastric abdominal surgery," *Chinese Journal of Digestive Diseases*, 2006; 7: 67-70.
- Lafullarde et al., "Laparoscopic Nissen Fundoplication: Five-year Results and Beyond," *Arch/Surg*, Feb. 2001; 136:180-184.
- Leffett et al. (2002), "Aortic injury during laparoscopic fundoplication," *Surg. Endoscopy* 16(2): 362.
- Li et al. (2000), "Microvascular Anastomoses Performed in Rats Using a Microsurgical Telesurgical Manipulator," *Comp. Aid. Surg.* 5: 326-332.
- Liem et al., "Comparison of Conventional Anterior Surgery and Laparoscopic Surgery for Inguinal-hernia Repair," *New England Journal of Medicine*, 1997; 336 (22): 1541-1547.
- MacFarlane et al., "Force-Feedback Grasper Helps Restore the Sense of Touch in Minimally Invasive Surgery," *Journal of Gastrointestinal Surgery*, 1999; 3: 278-285.
- Mack et al., "Present Role of Thoracoscopy in the Diagnosis and Treatment of Diseases of the Chest," *Ann Thorac Surgery*, 1992; 54: 403-409.
- Mack, "Minimally Invasive and Robotic Surgery," *JAMA*, Feb. 2001; 285(5): 568-572.
- Mei et al., "Wireless Drive and Control of a Swimming Microrobot," *Proceedings of the 2002 IEEE International Conference on Robotics & Automation*, May 2002: 1131-1136.
- Melvin et al., "Computer-Enhanced vs. Standard Laparoscopic Antireflux Surgery," *J Gastrointest Surg* 2002; 6: 11-16.
- Menciassi et al., "Locomotion of a Leffed Capsule in the Gastrointestinal Tract: Theoretical Study and Preliminary Technological Results," *IEEE Int. Conf. on Engineering in Medicine and Biology*, San Francisco, CA, pp. 2767-2770, Sep. 2004.
- Menciassi et al., "Robotic Solutions and Mechanisms for a Semi-Autonomous Endoscope," *Proceedings of the 2002 IEEE/RSJ Intl. Conference on Intelligent Robots and Systems*, Oct. 2002; 1379-1384.
- Menciassi et al., "Shape memory alloy clamping devices of a capsule for monitoring tasks in the gastrointestinal tract," *J. Micromech. Microeng.* 2005, 15: 2045-2055.
- Meron, "The development of the swallowable video capsule (M2A)," *Gastrointestinal Endoscopy* 2000; 52 6: 817-819.
- Micron, <http://www.micron.com>, 2006, 1/4-inch VGA NTSC/PAL CMOS Digital Image Sensor, 98 pp.
- Midday Jeff et al., "Material Handling System for Robotic natural Orifice Surgery", *Proceedings of the 2011 Design of medical Devices Conference*, Apr. 12-14, 2011, Minneapolis, MN, 4 pages.
- Miller, Ph.D., et al., "In-Vivo Stereoscopic Imaging System with 5 Degrees-of-Freedom for Minimal Access Surgery," *Dept. of Computer Science and Dept. of Surgery, Columbia University*, New York, NY, 7 pp.
- Munro (2002), "Laparoscopic access: complications, technologies, and techniques," *Curro Opin. Obstet. Gynecol.*, 14(4): 365-74.
- Nio et al., "Efficiency of manual vs robotical (Zeus) assisted laparoscopic surgery in the performance of standardized tasks," *Surg Endosc*, 2002; 16: 412-415.
- Office Action dated Apr. 17, 2007, received in related case U.S. Appl. No. 11/552,379, 5 pp.
- Office Action dated Apr. 3, 2009, received in related case U.S. Appl. No. 11/932,516, 43 pp.
- Office Action dated Aug. 18, 2006, received in related case U.S. Appl. No. 11/398,174, 6 pp.
- Office Action dated Aug. 21, 2006, received in related case U.S. Appl. No. 11/403,756, 6 pp.
- Office Action dated Oct. 29, 2007, received in related case U.S. Appl. No. 11/695,944, 6 pp.
- Office Action dated Oct. 9, 2008, received in related case U.S. Appl. No. 11/932,441, 4 pp.
- Oleynikov et al., "In Vivo Camera Robots Provide Improved Vision for Laparoscopic Surgery," *Computer Assisted Radiology and Surgery (CARS)*, Chicago, IL, Jun. 23-26, 2004b.
- Oleynikov et al., "In Vivo Robotic Laparoscopy," *Surgical Innovation*, Jun. 2005, 12(2): 177-181.
- Oleynikov et al., "Miniature Robots Can Assist in Laparoscopic Cholecystectomy," *Journal of Surgical Endoscopy*, 19-4: 473-476, 2005.
- O'Neill, "Surgeon takes new route to gallbladder," *The Oregonian*, Jun. 2007, 2 pp.
- Orlando et al., (2003), "Needle and Trocar Injuries in Diagnostic Laparoscopy under Local Anesthesia: What Is the True Incidence of These Complications?" *Journal of Laparoendoscopic & Advanced Surgical Techniques* 13(3): 181-184.
- Park et al., "Trocar-less Instrumentation for Laparoscopy: Magnetic Positioning of Intra-abdominal Camera and Retractor," *Ann Surg*, Mar. 2007; 245(3): 379-384.
- Park et al., "Experimental studies of transgastric gallbladder surgery: cholecystectomy and cholecystogastric anastomosis (vid-eos)," *Gastrointestinal Endoscopy*, 2005; 61(4): 601-606.
- Palm, William, "Rapid Prototyping Primer" May 1998 (revised Jul. 30, 2002) (<http://www.me.psu.edu/lamancusa/rapidpro/primer/chapter2.htm>).
- Patronik et al., "Development of a Tethered Epicardial Crawler for Minimally Invasive Cardiac Therapies," *IEEE*, pp. 239-240.
- Patronik et al., "Crawling on the Heart: A Mobile Robotic Device for Minimally Invasive Cardiac Interventions," *MICCAI*, 2004, pp. 9-16.
- Patronik et al., "Preliminary evaluation of a mobile robotic device for navigation and intervention on the beating heart," *Computer Aided Surgery*, 10(4): 225-232, Jul. 2005.
- Peirs et al., "A miniature manipulator for integration in a self-propelling endoscope," *Sensors and Actuators A*, 2001, 92: 343-349.
- Peters, "Minimally Invasive Colectomy: Are the Potential Benefits Realized?" *Dis Colon Rectum* 1993; 36: 751-756.
- Phoe et al., "Analysis and Development of Locomotion Devices for the Gastrointestinal Tract," *IEEE Transaction on Biomedical Engineering*, vol. 49, No. 6, Jun. 2002, pp. 613-616.
- Phoe et al., "Development of Microbotic Devices for Locomotion in the Human Gastrointestinal Tract," *International Conference on Computational Intelligence, Robotics and Autonomous Systems (CIRAS 2001)*, Nov. 28-30, (2001), Singapore.
- Platt et al., "In Vivo Robotic Cameras can Enhance Imaging Capability During Laparoscopic Surgery," in the *Proceedings of the Society of American Gastrointestinal Endoscopic Surgeons (SAGES) Scientific Conference*, Ft. Lauderdale, FL, Apr. 13-16, 2005, 1 pg.
- Preliminary Amendment filed Apr. 11, 2007, in related case U.S. Appl. No. 11/403,756, 7 pp.
- Preliminary Amendment filed Jul. 30, 2008, in related case U.S. Appl. No. 12/171,413, 4 pp.
- RCE and Amendment filed Jun. 13, 2007, in related case U.S. Appl. No. 11/403,756, 8 pp.
- Rentschler et al., "Mobile In Vivo Biopsy and Camera Robot," *Studies in Health and Infonnatics Medicine Meets Reality*, vol. 119., pp. 449-454, IOS Press, Long Beach, CA, 2006e.
- Rentschler et al., *Mobile in Vivo Biopsy Robot*, *IEEE International Conference on Robotics and Automation*, Orlando, Florida, May 2006, pp. 4155-4160.
- Rentschler et al., "Miniature in vivo Robots for Remote and Harsh Environments," *IEEE Transactions on Information Technology in Biomedicine*, Jan. 2006; 12(1): 66-75.
- Rentschler et al., "An In Vivo Mobile Robot for Surgical Vision and Task Assistance," *Journal of Medical Devices*, Mar. 2007, vol. 1: 23-29.
- Rentschler et al., "In vivo Mobile Surgical Robotic Task Assistance," 1 pg.
- Rentschler et al., "In vivo Robotics during the NEEMO 9 Mission," *Medicine Meets Virtual Reality*, Feb. 2007, 1 pg.
- Rentschler et al., "In Vivo Robots for Laparoscopic Surgery," *Studies in Health Technology and Infonnatics—Medicine Meets Virtual Reality*, ISO Press, Newport Beach, CA, 2004a, 98: 316-322.

(56)

References Cited

OTHER PUBLICATIONS

- Rentschler et al., "Mechanical Design of Robotic In Vivo Wheeled Mobility," ASME Journal of Mechanical Design, 2006a, pp. I-II.
- Rentschler et al., "Mobile In Vivo Camera Robots Provide Sole Visual Feedback for Abdominal Exploration and Cholecystectomy," Journal of Surgical Endoscopy, 20-I: 135-138, 2006b.
- Rentschler et al., "Mobile In Vivo Robots Can Assist in Abdominal Exploration," from the Proceedings of the Society of American Gastrointestinal Endoscopic Surgeons (SAGES) Scientific Conference, Ft. Lauderdale, FL, Apr. 13-16, 2005b.
- Rentschler et al., "Modeling, Analysis, and Experimental Study of In Vivo Wheeled Robotic Mobility," IEEE Transactions on Robotics, 22 (2): 308-321, 2005c.
- Rentschler et al., "Natural Orifice Surgery with an Endoluminal Mobile Robot," The Society of American Gastrointestinal Endoscopic Surgeons, Dallas, TX, Apr. 2006d, 14 pp.
- Rentschler et al., "Theoretical and Experimental Analysis of In Vivo Wheeled Mobility," ASME Design Engineering Technical Conferences: 28th Biennial Mechanisms and Robotics Conference, Salt Lake City, Utah, Sep. 28-Oct. 2, 2004, pp. 1-9.
- Rentschler et al., "Toward In Vivo Mobility," Studies in Health Technology and Informatics—Medicine Meets Virtual Reality, ISO Press, Long Beach, CA, 2005a, III: 397-403.
- Response to Rule 312 Amendment in related case U.S. Appl. No. 11/695,944, dated Jan. 12, 2009, 2 pp.
- Riviere et al., "Toward Active Tremor Canceling in Handheld Microsurgical Instruments," IEEE Transactions on Robotics and Automation, Oct. 2003, 19(5): 793-800.
- Rosen et al., "Force Controlled and Teleoperated Endoscopic, Grasper for Minimally Invasive Surgery—Experimental Performance Evaluation," IEEE Transactions of Biomedical Engineering, Oct. 1999; 46(10): 1212-1221.
- Rosen et al., "Objective Laparoscopic Skills Assessments of Surgical Residents Using Hidden Markov Models Based on Haptic Information and Tool/Tissue Interactions," Studies in Health Technology and Informatics—Medicine Meets Virtual Reality, Jan. 2001, 7 pp.
- Rosen et al., "Spherical Mechanism Analysis of a Surgical Robot for Minimally Invasive Surgery—Analytical and Experimental Approaches," Studies in Health Technology and Informatics—Medicine Meets Virtual Reality, pp. 442-448, Jan. 2005.
- Rosen et al., "Task Decomposition of Laparoscopic Surgery for Objective Evaluation of Surgical Residents' Learning Curve Using Hidden Markov Model," Computer Aided Surgery, vol. 7, pp. 49-61, 2002.
- Rosen et al., "The Blue Dragon—A System of Measuring the Kinematics and the Dynamics of Minimally Invasive Surgical Tools In-Vivo," Proc. of the 2002 IEEE International Conference on Robotics and Automation, Washington, DC, pp. 1876-1881, May 2002.
- Ruurda et al., "Robot-Assisted surgical systems: a new era in laparoscopic surgery," Ann R. Coll Surg Engl., 2002; 84: 223-226.
- Ruurda et al., "Feasibility of Robot-Assisted Laparoscopic Surgery," Surgical Laparoscopy, Endoscopy & Percutaneous Techniques, 2002; 12(1):41-45.
- Sackier et al., "Robotically assisted laparoscopic surgery," Surgical Endoscopy, 1994; 8: 63-66.
- Salky, "What is the Penetration of Endoscopic Techniques into Surgical Practice?" Digestive Surgery, 2000; 17:422-426.
- Satava, "Surgical Robotics: The Early Chronicles," Surgical Laparoscopy, Endoscopy & Percutaneous Techniques, 2002; 12(1): 6-16.
- Schippers et al., (1996) "Requirements and Possibilities of Computer-Assisted Endoscopic Surgery," In: Computer Integrated Surgery: Technology and Clinical Applications, pp. 561-565.
- Schurr et al., "Robotics and Telem Manipulation Technologies for Endoscopic Surgery," Surgical Endoscopy, 2000; 14: 375-381.
- Schwartz, "In the Lab: Robots that Slink and Squirm," The New York Times, Mar. 27, 2007, 4 pp.
- Sharp LL-151-3D, <http://www.sharp3d.com>, 2006, 2 pp.
- Slatkin et al., "The Development of a Robotic Endoscope," Proceedings of the 1995 IEEE International Conference on Robotics and Automation, pp. 162-171, 1995.
- Smart Pill "Fastastic Voyage: Smart Pill to Expand Testing," <http://www.smartpilldiagnostics.com>, Apr. 13, 2005, 1 pg.
- Southern Surgeons Club (1991), "A prospective analysis of 1518 laparoscopic cholecystectomies," N. Eng. J. Med. 324 (16): 1073-1078.
- Stefanini et al., "Modeling and Experiments on a Legged Microrobot Locomoting in a Tubular Compliant and Slippery Environment," Int. Journal of Robotics Research, vol. 25, No. 5-6, pp. 551-560, May-Jun. 2006.
- Stiff et al., "Long-term Pain: Less Common After Laparoscopic than Open Cholecystectomy," British Journal of Surgery, 1994; 81: 1368-1370.
- Strong, et al., "Efficacy of Novel Robotic Camera vs. a Standard Laparoscopic Camera," Surgical Innovation vol. 12, No. 4, Dec. 2005, Westminster Publications, Inc., pp. 315-318.
- Suzumori et al., "Development of Flexible Microactuator and its Applications to Robotics Mechanisms," Proceedings of the IEEE International Conference on Robotics and Automation, 1991: 1622-1627.
- Taylor et al., "A Telerobotic Assistant for Laparoscopic Surgery," IEEE Eng Med Biol, 1995; 279-287.
- Tendick et al. (1993), "Sensing and Manipulation Problems in Endoscopic Surgery: Experiment, Analysis, and Observation," Presence 2(1): 66-81.
- Abbott et al., "Design of an Endoluminal NOTES Robotic System," from the Proceedings of the 2007 IEEE/RSJ Int'l Conf. on Intelligent Robot Systems, San Diego, CA, Oct. 29-Nov. 2, 2007, pp. 410-416.
- Allendorf et al., "Postoperative Immune Function Varies Inversely with the Degree of Surgical Trauma in a Murine Model," Surgical Endoscopy 1997; 11:427-430.
- Ang, "Active Tremor Compensation in Handheld Instrument for Microsurgery," Doctoral Dissertation, tech report CMU-RI-TR-04-28, Robotics Institute, Carnegie Mellon University, May 2004, 167pp.
- Applicant Amendment after Notice of Allowance under Rule 312, filed Aug. 25, 2008, in related case U.S. Appl. No. 11/695,944, 6pp.
- Applicant Response to Office Action dated Apr. 17, 2007, in related case U.S. Appl. No. 11/552,379, filed Aug. 8, 2007, 7 pp.
- Applicant Response to Office Action dated Aug. 18, 2006, in related case U.S. Appl. No. 11/398,174, filed Nov. 7, 2006, 8pp.
- Applicant Response to Office Action dated Aug. 21, 2006, in related case U.S. Appl. No. 11/403,756, filed Nov. 21, 2006, 52pp.
- Applicant Response to Office Action dated Oct. 29, 2007, in related case U.S. Appl. No. 11/695,944, filed Jan. 22, 2008, 6pp.
- Atmel 8005X2 Core, <http://www.atmel.com>, 2006, 186pp.
- Bailey et al., "Complications of Laparoscopic Surgery," Quality Medical Publishers, Inc., 1995, 25pp.
- Ballantyne, "Robotic Surgery, Telerobotic Surgery, Telepresence, and Telementoring," Surgical Endoscopy, 2002; 16: 1389-1402.
- Bauer et al., "Case Report: Remote Percutaneous Renal Percutaneous Renal Access Using a New Automated Telesurgical Robotic System," Telemedicine Journal and e-Health 2001; (4): 341-347.
- Begos et al., "Laparoscopic Cholecystectomy: From Gimmick to Gold Standard," J Clin Gastroenterol, 1994; 19(4): 325-330.
- Berg et al., "Surgery with Cooperative Robots," Medicine Meets Virtual Reality, Feb. 2007, 1 pg.
- Breda et al., "Future developments and perspectives in laparoscopy," Eur. Urology 2001; 40(1): 84-91.
- Breedveld et al., "Design of Steerable Endoscopes to Improve the Visual Perception of Depth During Laparoscopic Surgery," ASME, Jan. 2004; vol. 126, pp. 1-5.
- Breedveld et al., "Locomotion through the Intestine by means of Rolling Stents," Proceedings of the ASME Design Engineering Technical Conferences, 2004, pp. 1-7.
- Calafiore et al., "Multiple Arterial Conduits Without Cardiopulmonary Bypass: Early Angiographic Results," Ann Thorac Surg, 1999; 67: 450-456.
- Camarillo et al., "Robotic Technology in Surgery: Past, Present and Future," The American Journal of Surgery, 2004; 188: 2S-15.

(56)

References Cited

OTHER PUBLICATIONS

- Cavusoglu et al., "Telesurgery and Surgical Simulation: Haptic Interfaces to Real and Virtual Surgical Environments," In McLaughlin, M.L., Hespanha, J.P., and Sukhatme, G., editors. Touch in virtual environments, IMSC Series in Multimedia 2001, 28pp.
- Cavusoglu et al., "Robotics for Telesurgery: Second Generation Berkeley/UCSF Laparoscopic Telesurgical Workstation and Looking Towards the Future Applications," *Industrial Robot: An International Journal*, 2003; 30(1): 22-29.
- Chanthasopephan et al., (2003), "Measuring Forces in Liver Cutting: New Equipment and Experimental Results," *Annals of Biomedical Engineering* 31: 1372-1382.
- Choi et al., "Flexure-based Manipulator for Active Handheld Microsurgical Instrument," Proceedings of the 27th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBS), Sep. 2005, 4pp.
- Cuschieri, "Technology for Minimal Access Surgery," *BMJ*, 1999, 319: 1-6.
- Dakin et al., "Comparison of laparoscopic skills performance between standard instruments and two surgical robotic systems," *Surg Endosc.*, 2003; 17: 574-579.
- Dumpert et al., "Improving in Vivo Robot Vision Quality," from the Proceedings of Medicine Meets Virtual Reality, Long Beach, CA, Jan. 26-29, 2005. 1 pg.
- Dumpert et al., "Stereoscopic In Vivo Surgical Robots," *IEEE Sensors Special Issue on In Vivo Sensors for Medicine*, Jan. 2007, 10 pp.
- Examiner Interview Summary dated Aug. 6 and Aug. 12, 2008, in related case U.S. Appl. No. 11/695,944, 1 pg.
- Examiner Interview Summary dated May 9, 2008, in related case U.S. Appl. No. 11/695,944, 1 pg.
- Examiner Interview Summary dated Nov. 30, 2006, in related case U.S. Appl. No. 11/398,174, 2pp.
- Falcone et al., "Robotic Surgery," *Clin. Obstet. Gynecol.* 2003, 46(1): 37-43.
- Faraz et al., "Engineering Approaches to Mechanical and Robotic Design for Minimally Invasive Surgery (MIS)," Kluwer Academic Publishers (Boston), 2000, 13pp.
- Fearing et al., "Wing Transmission for a Micromechanical Flying Insect," Proceedings of the 2000 IEEE International Conference to Robotics & Automation, Apr. 2000; 1509-1516.
- Fireman et al., "Diagnosing small bowel Crohn's disease with wireless capsule endoscopy," *Gut* 2003; 52: 390-392.
- Flynn et al., "Tomorrow's Surgery: micromotors and microbots for minimally invasive procedures," *Minimally Invasive Surgery & Allied Technologies*.
- Franklin et al., "Prospective Comparison of Open vs. Laparoscopic Colon Surgery for Carcinoma: Five-Year Results," *Dis Colon Rectum*, 1996; 39: S35-S46.
- Fraulob et al., "Miniature assistance module for robot-assisted heart surgery," *Biomed. Tech.* 2002, 47 Suppl. 1, Pt. 1: 12-15.
- Fukuda et al., "Mechanism and Swimming Experiment of Micro Mobile Robot in Water," Proceedings of the 1994 IEEE International Conference on Robotics and Automation, 1994: 814-819.
- Fukuda et al., "Micro Active Catheter System with Multi Degrees of Freedom," Proceedings of the IEEE International Conference on Robotics and Automation, May, 1994, pp. 2290-2295.
- Fuller et al., "Laparoscopic Trocar Injuries: A Report from a U.S. Food and Drug Administration (FDA) Center for Devices and Radiological Health (CDRH) Systematic Technology Assessment of Medical Products (STAMP) Committee," U.S. Food and Drug Administration, available at <http://www.fda.gov/oc>, Finalized: Nov. 7, 2003; Updated: Jun. 24, 2005, 11 pp.
- Grady, "Doctors Try New Surgery for Gallbladder Removal," *The New York Times*, Apr. 20, 2007, 3 pp.
- Tendick et al., "Applications of Micromechatronics in Minimally Invasive Surgery," *IEEE/ASME Transactions on Mechatronics*, 1998; 3(1): 34-42.
- Thomann et al., "The Design of a new type of Micro Robot for the Intestinal Inspection," Proceedings of the 2002 IEEE Intl. Conference on Intelligent Robots and Systems, Oct. 2002: 1385-1390.
- U.S. Appl. No. 60/180,960, filed Feb. 2000.
- U.S. Appl. No. 60/956,032, filed Aug. 15, 2007.
- U.S. Appl. No. 60/983,445, filed Oct. 29, 2007.
- U.S. Appl. No. 60/990,062, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,076, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,086, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,106, filed Nov. 26, 2007.
- U.S. Appl. No. 60/990,470, filed Nov. 27, 2007.
- U.S. Appl. No. 61/025,346, filed Feb. 1, 2008.
- U.S. Appl. No. 61/030,588, filed Feb. 22, 2008.
- U.S. Appl. No. 61/030,617, filed Feb. 22, 2008.
- Way et al., (editors), "Fundamentals of Laparoscopic Surgery," Churchill Livingstone Inc., 1995, 14 pp.
- Wolfe et al., "Endoscopic Cholecystectomy: An analysis of Complications," *Arch. Surg.* Oct. 1991; 126: 1192-1196.
- Worn et al., "Espirit Project No. 33915: Miniaturised Robot for Micro Manipulation (MINIMAN)," Nov. 1998; <http://www.ipr.ira.ujka.de/-microbot/miniman>.
- Yu et al., "Microbotic Cell Injection," Proceedings of the 2001 IEEE International Conference on Robotics and Automation, May 2001; 620-625.
- Yu, BSN, RN, "M2ATM Capsule Endoscopy a Breakthrough Diagnostic Tool for Small Intestine Imaging," vol. 25, No. 1, *Gastroenterology Nursing*, pp. 24-27.
- International Search Report and Written Opinion of international application No. PCT/US2010/061137, dated Feb. 11, 2011, 10 pp.
- Abbou et al., "Laparoscopic Radical Prostatectomy with a Remote Controlled Robot," *The Journal of Urology*, Jun. 2001, 165: 1964-1966.
- Glukhovskiy et al., "The development and application of wireless capsule endoscopy," *Int. J. Med. Robot. Comput. Assist. Surgery*, 2004; 1(1): 114-123.
- Gong et al., *Wireless endoscopy, Gastrointestinal Endoscopy* 2000; 51(6): 725-729.
- Hanly et al., "Value of the SAGES Learning Center in introducing new technology," *Surgical Endoscopy*, 2004; 19 (4):477-483.
- Hanly et al., "Robotic Abdominal Surgery," *The American Journal of Surgery* 188 (Suppl. to Oct. 1994): 19S-26S, 2004.
- Heikkinen et al., "Comparison of laparoscopic and open Nissen fundoplication two years after operation: A prospective randomized trial," *Surgical Endoscopy*, 2000; 14: 1019-1023.
- Hissink, "Olympus Medical develops capsule camera technology," Dec. 2004, accessed Aug. 29, 2007, <http://www.letsgodigital.org>, 3 pp.
- Horgan et al., "Technical Report: Robots in Laparoscopic Surgery," *Journal of Laparoendoscopic & Advanced Surgical Techniques*, 2001; 11(6): 415-419.
- Stoianovici et al., "Robotic Tools for Minimally Invasive Urologic Surgery," Jan. 1, 2002, pp. 1-17.
- Cleary et al., "State of the Art in Surgical Robotics: Clinical Applications and Technology Challenges," *Computer Aided Surgery*, Jan. 1, 2002, pp. 312-328, vol. 6.
- Green, "Telepresence Surgery," Jan. 1, 1995, Publisher: IEEE Engineering in Medicine and Biology.
- Franzino, "The Laprotek Surgical System and the Next Generation of Robotics," *Surg Clin North Am*, 2003 83(6): 1317-1320.
- Guber et al., "Miniaturized Instrument Systems for Minimally Invasive Diagnosis and Therapy," *Biomedizinische Technic*. 2002, Band 47, Ergänzungsband 1: 198-201.

* cited by examiner

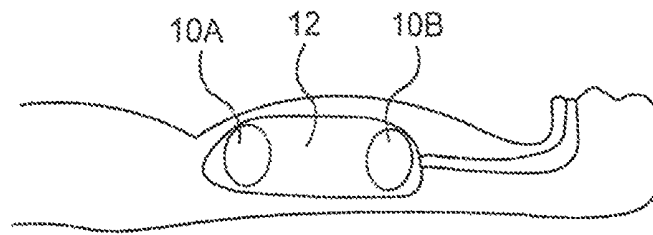


Fig. 1A

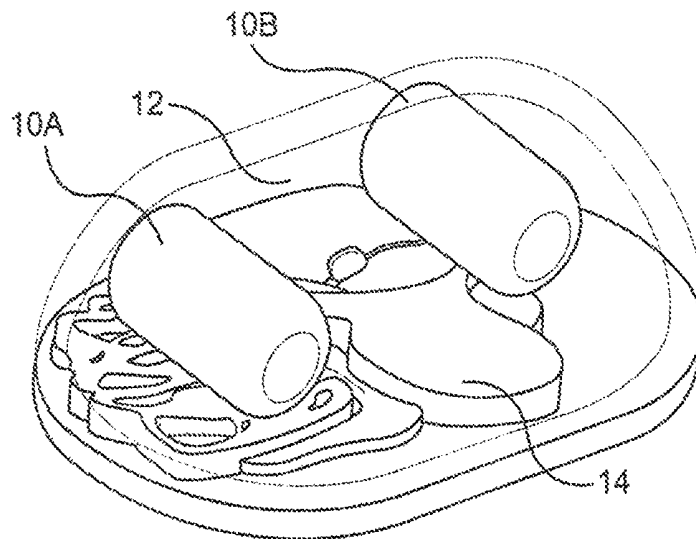


Fig. 1B

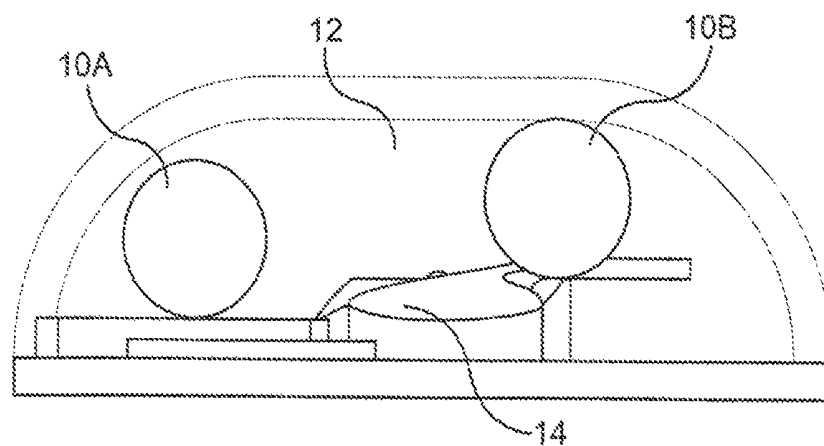


Fig. 1C

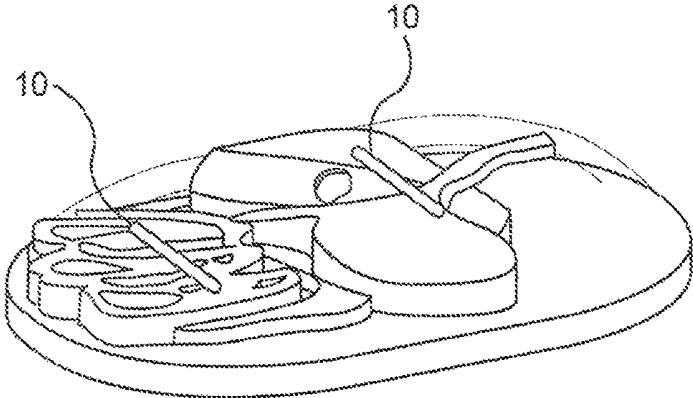


Fig. 1D

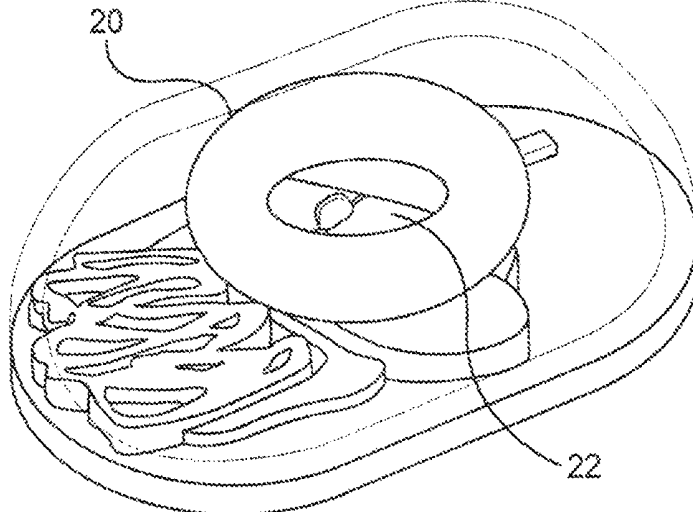


Fig. 2A

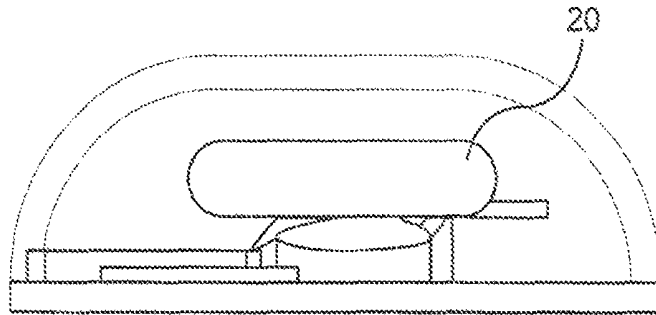


Fig. 2B

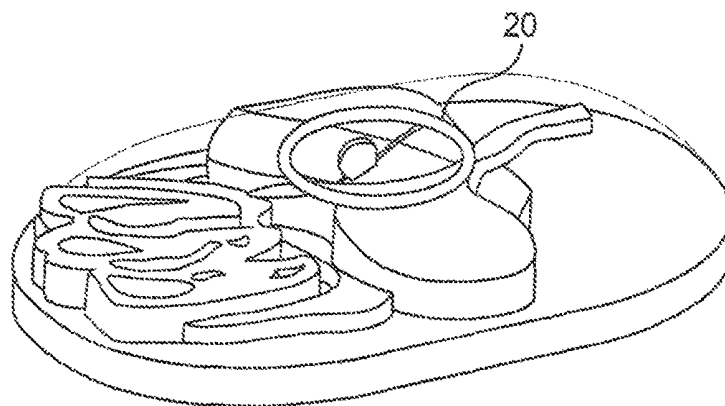


Fig. 2C

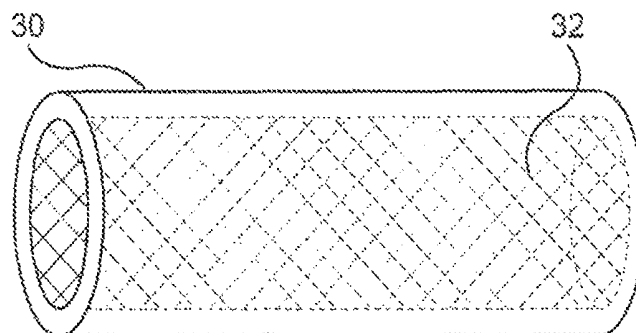


Fig. 3

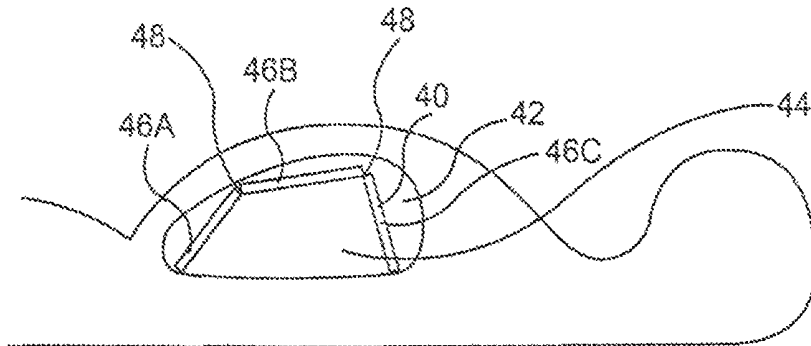


Fig. 4A

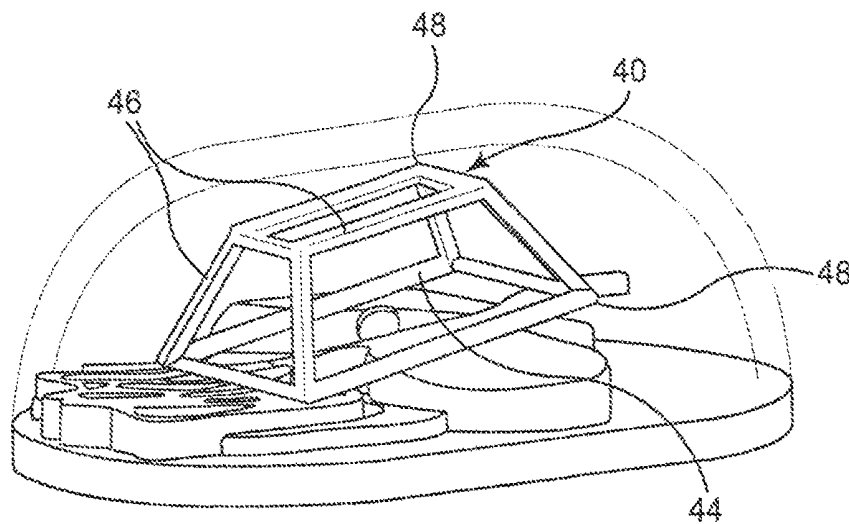


Fig. 4B

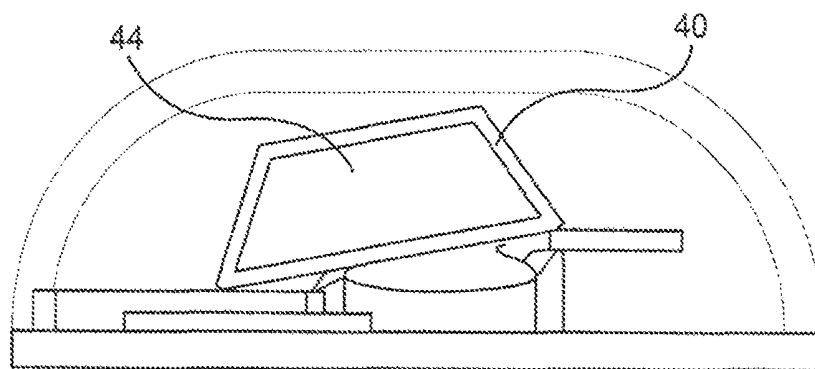


Fig. 4C

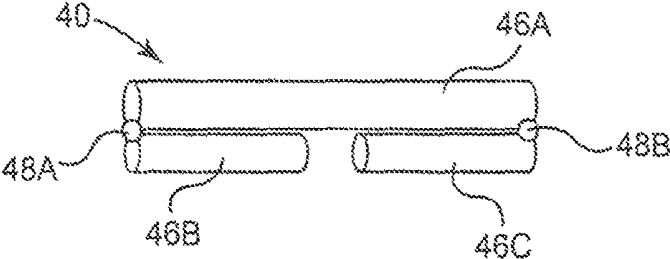


Fig. 4D

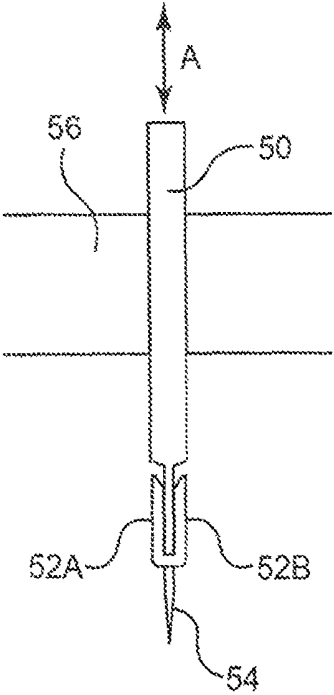


Fig. 5A

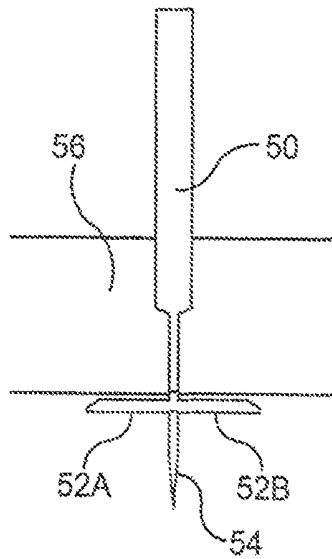


Fig. 5B

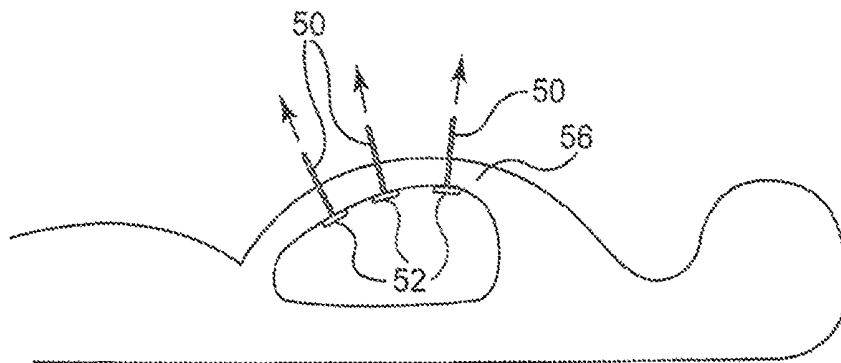


Fig. 5C

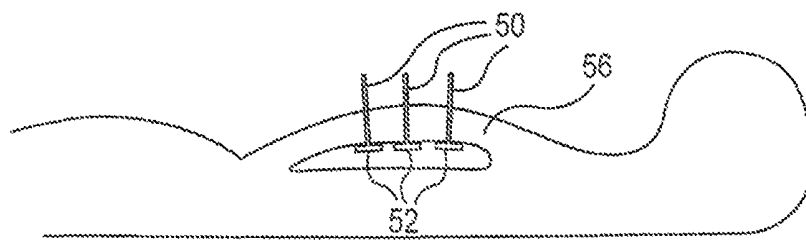


Fig. 5D

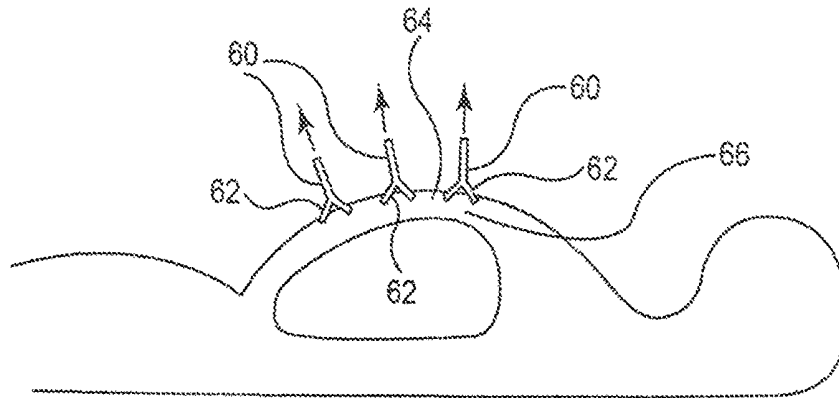


Fig. 6A

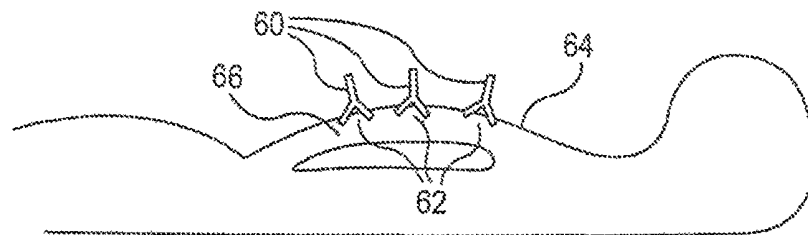


Fig. 6B

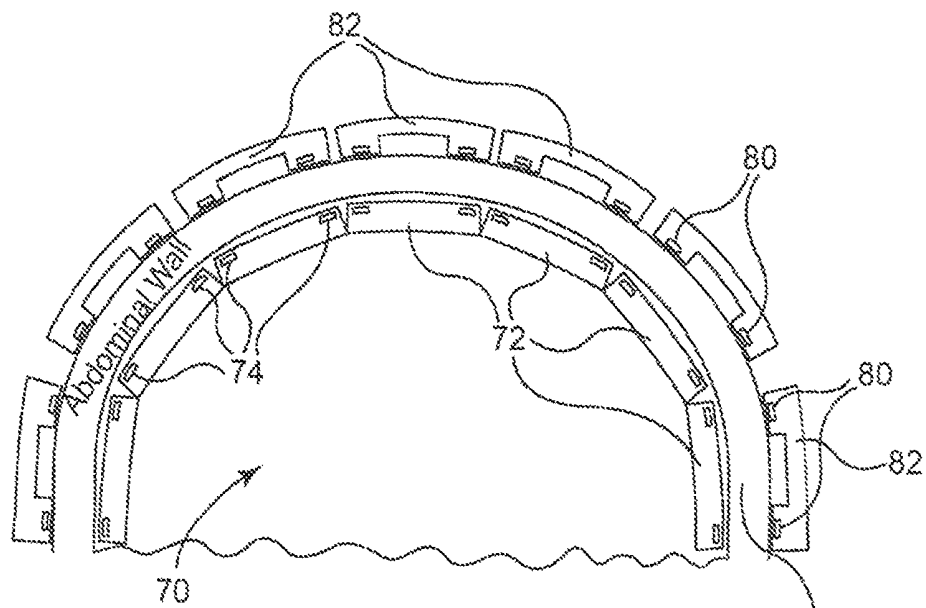


Fig. 7A

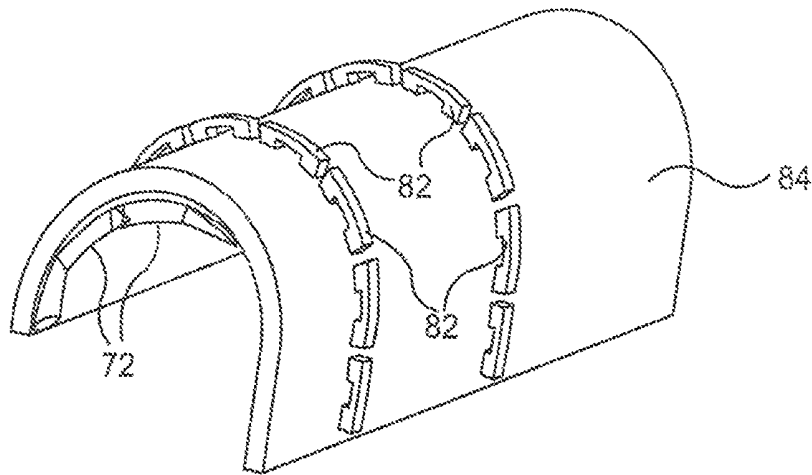


Fig. 7B

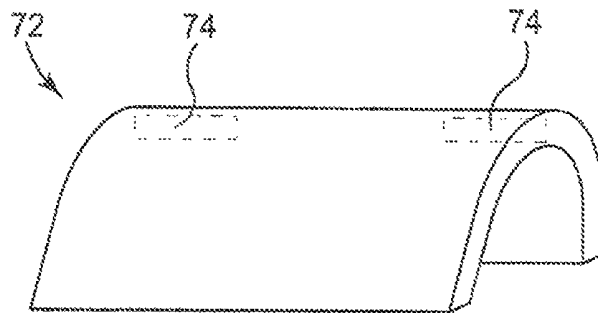


Fig. 7C

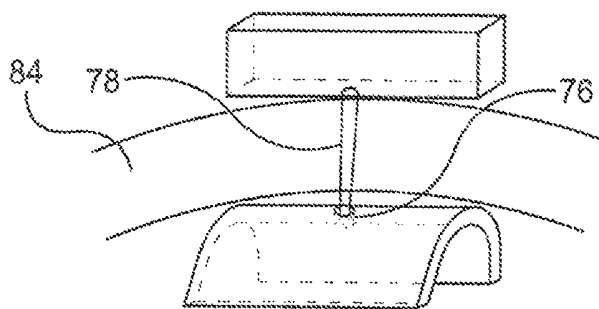


Fig. 7D

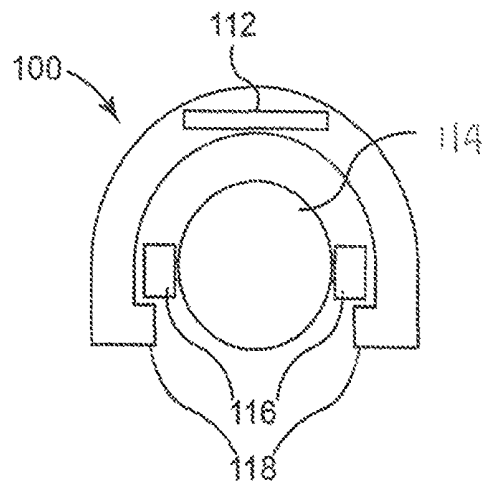


Fig. 8A

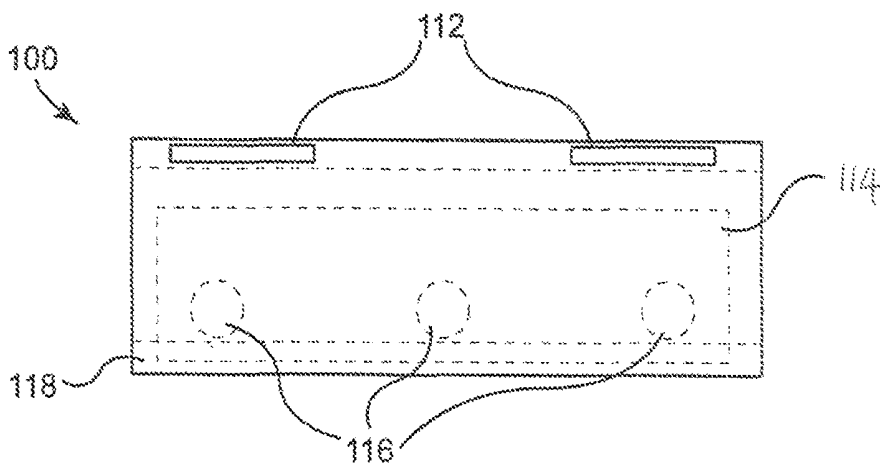


Fig. 8B

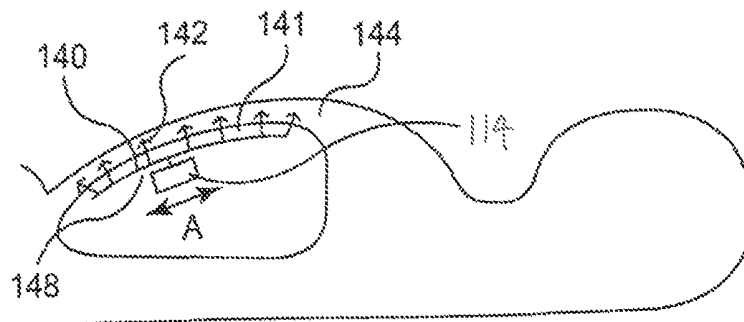


Fig. 9

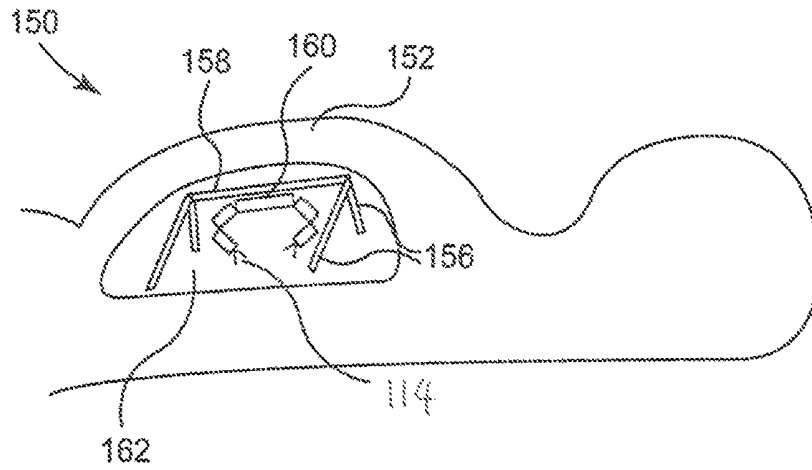


Fig. 10

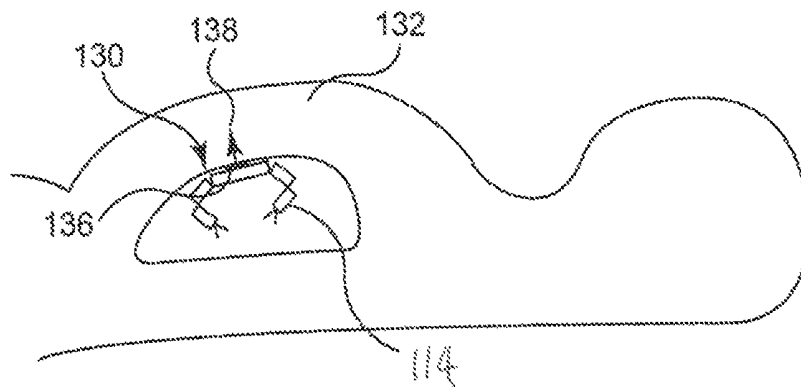


Fig. 11

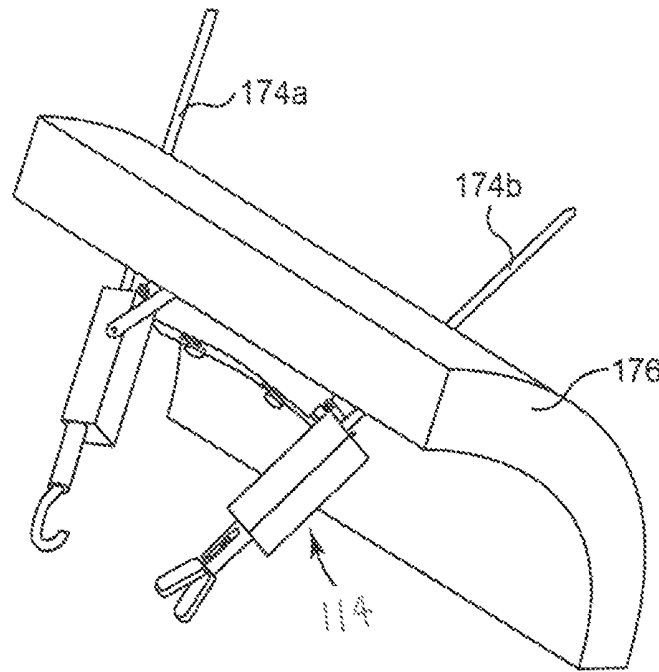


Fig. 12

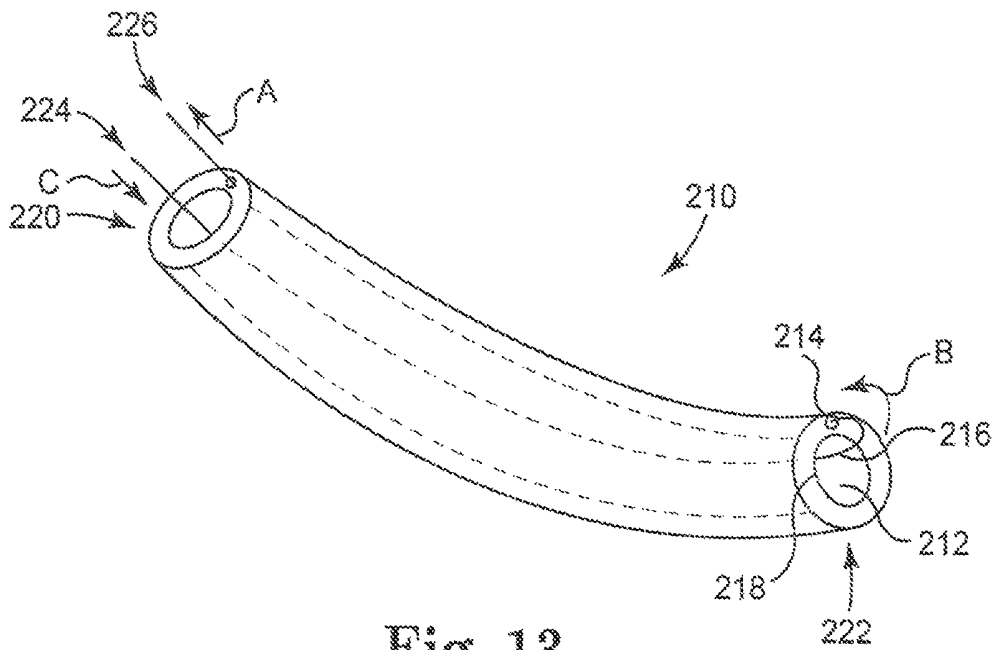


Fig. 13

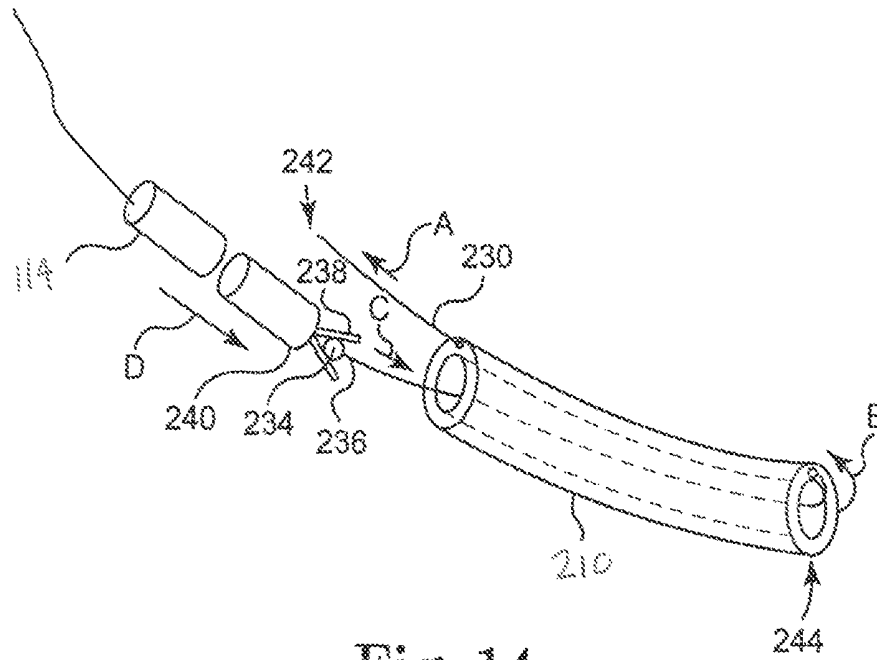


Fig. 14

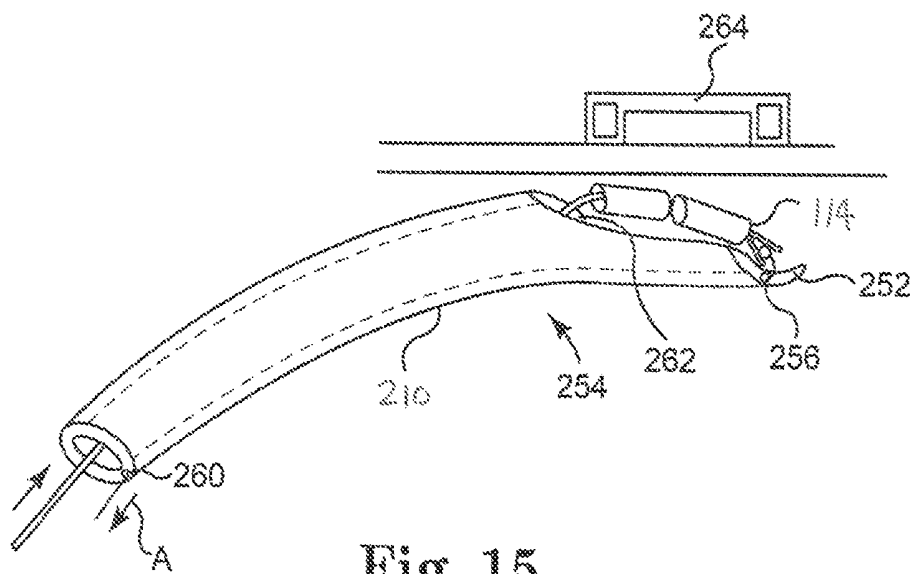


Fig. 15

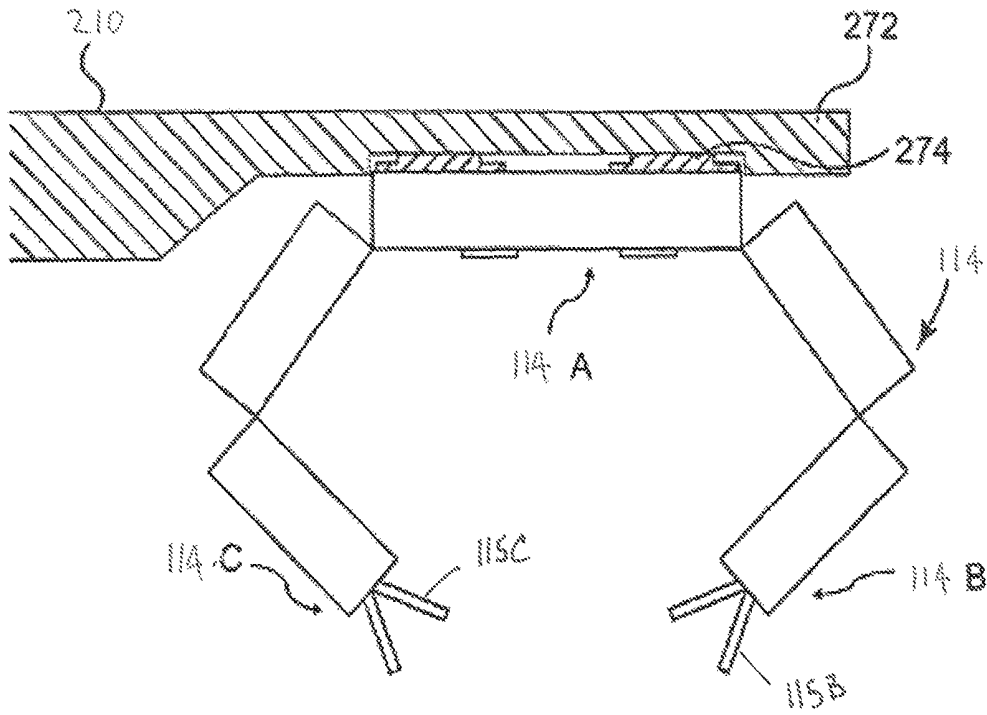


Fig. 16

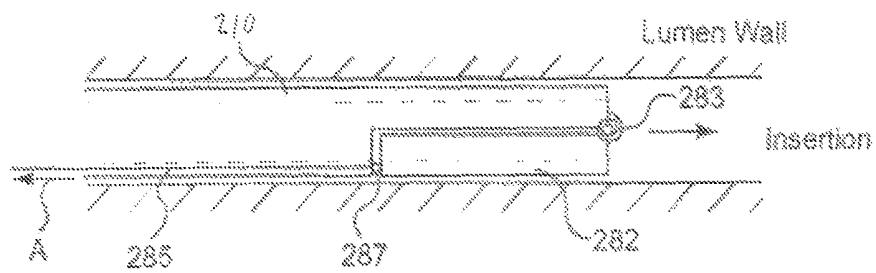


Fig. 17A

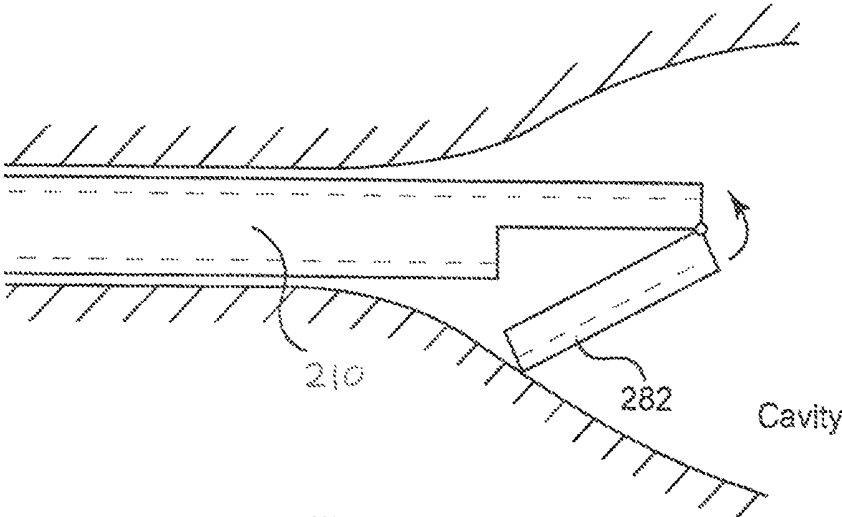


Fig. 17B

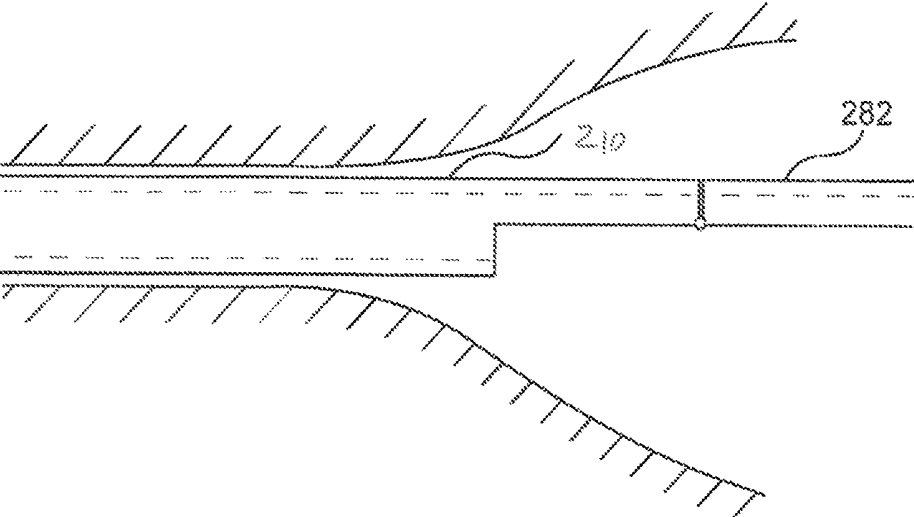


Fig. 17C

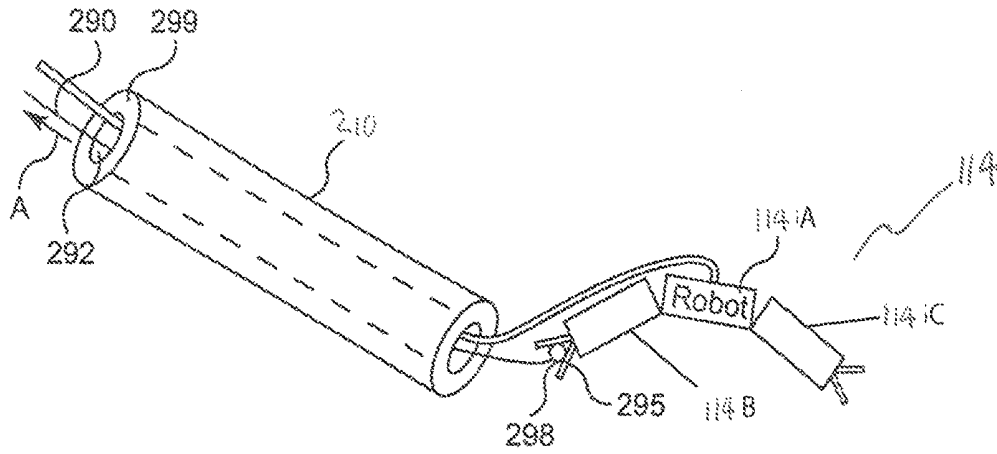


Fig. 18




Fig. 19A




Fig. 19B




Fig. 19C

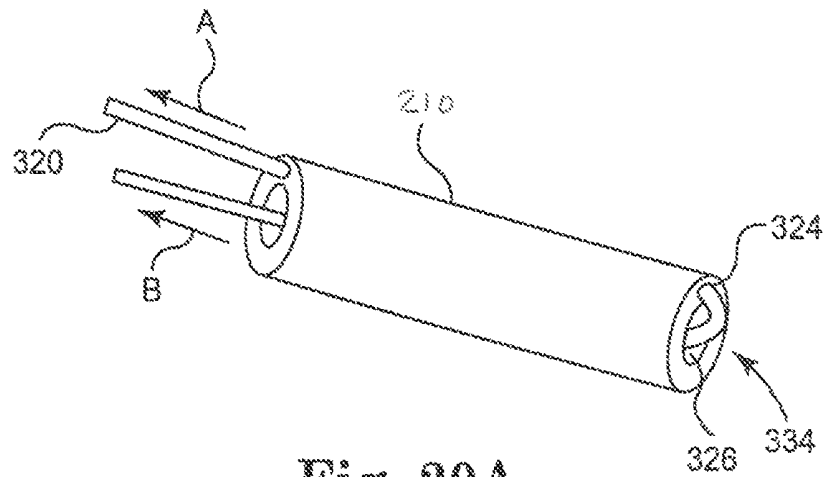


Fig. 20A

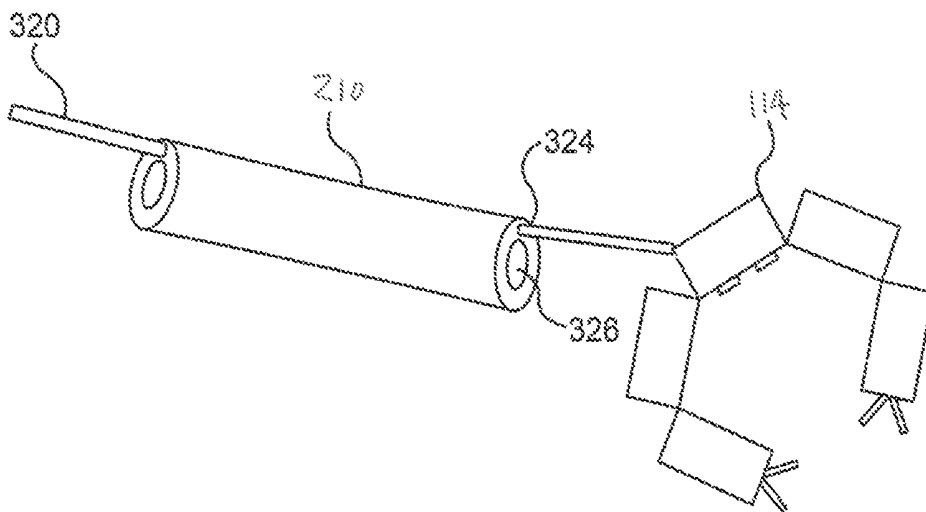


Fig. 20B

MEDICAL INFLATION, ATTACHMENT AND DELIVERY DEVICES AND RELATED METHODS

CROSS-REFERENCE TO RELATED APPLICATIONS

This is a continuation-in-part of U.S. application Ser. No. 12/192,663, filed Aug. 15, 2008 and entitled "Medical Inflation, Attachment, and Delivery Devices and Related Methods," which claims priority to Provisional Application No. 60/956,032, filed Aug. 15, 2007; Provisional Application No. 60/990,062, filed Nov. 26, 2007; and Provisional Application No. 60/990,470, filed Nov. 27, 2007; all of which are hereby incorporated herein by reference in their entireties.

GOVERNMENT SUPPORT

This invention was made with government support under Grant No. WSIXWH-08-02-0043 awarded by the U.S. Army Medical Research and Materiel Command within the Department of Defense. Accordingly, the government has certain rights in this invention.

TECHNICAL FIELD

The embodiments disclosed herein relate to various medical devices and related components, including robotic and/or in vivo medical devices and related components, along with related procedures and methods. Certain embodiments include various cavity inflation or structural retention system embodiments, including inflatable devices, scaffold-like devices, and externally-supported wall retention devices. Further embodiments include various medical device attachment and control components, including attachment pin devices and magnetic attachment devices. Additional embodiments include various medical device delivery devices that can be used to deliver various types of medical devices, including in vivo devices, to target medical treatment areas, including tubular devices with operational distal ends that provide for simple delivery, control, and retrieval of various medical devices.

BACKGROUND

Invasive surgical procedures are essential for addressing various medical conditions. When possible, minimally invasive procedures such as laparoscopy are preferred.

However, known minimally invasive technologies such as laparoscopy are limited in scope and complexity due in part to 1) mobility restrictions resulting from using rigid tools inserted through access ports, and 2) limited visual feedback. Known robotic systems such as the da Vinci® Surgical System (available from Intuitive Surgical, Inc., located in Sunnyvale, Calif.) are also restricted by the access ports, as well as having the additional disadvantages of being very large, very expensive, unavailable in most hospitals, and having limited sensory and mobility capabilities.

There is a need in the art for improved surgical methods, systems, and devices.

SUMMARY

One embodiment disclosed herein relates to a body cavity spatial support device having an inflatable body and an inflation mechanism. In one embodiment, the body has a

generally cylindrical shape, while in another embodiment it has a generally donut shape. Alternatively, the device can have two or more inflatable bodies.

Another embodiment disclosed herein relates to a collapsible body cavity spatial support device. The device has at least three links hingedly coupled to each other and is configured to have a collapsed configuration and a deployed configuration.

A further embodiment disclosed herein relates to a pin having a needle tip and a retention component. The pin can be configured to be inserted through a cavity wall and be urged away from the cavity to maintain a procedural space in the cavity. According to one implementation, two or more pins are used cooperatively to maintain the procedural space.

Yet another embodiment disclosed herein relates to a pin having a grasping component configured to attach to an outer portion of the cavity wall. In one embodiment, two or more of these pins can be used cooperatively to maintain the procedural space.

One further embodiment disclosed herein relates to a procedural space maintenance system having at least two modular components that are coupled to each other and configured to be positioned inside a cavity of a patient. In one embodiment, the components each have at least one magnet. The system further comprises at least one external magnet configured to urge the at least two modular components away from the cavity and thereby maintain a procedural space in the cavity. In an alternative embodiment, the at least two modular components each have a mating or coupling component configured to couple with a medical device.

Another embodiment disclosed herein relates to a device positioning system having at least two modular components that are coupled to each other and configured to be positioned inside a cavity of a patient and attached to an interior cavity wall. The components are configured to couple together to create an attachment component along which a medical device can be positioned. Alternatively, the modular components have at least two legs to allow the system to be positioned in the cavity (instead of the attachment components for attaching to the interior wall).

A further embodiment disclosed herein relates to a device positioning and control system having at least one pin that is inserted through the cavity wall and coupled to an arm of a medical device positioned inside the body cavity. The pin can be used to maintain the position of the device and, according to a further embodiment, assist with the operation of the arm.

Yet another embodiment disclosed herein relates to a delivery or removal device having a tubular body, a device lumen, a wire lumen, and a wire disposed through the device and wire lumens. In accordance with one embodiment, the wire has an attachment component. In another embodiment, the tubular body has a protrusion at a distal end of the body. In a further embodiment, the protrusion is a deployable protrusion. In yet another embodiment, the protrusion has a device receiving component.

While multiple embodiments are disclosed, still other embodiments of the present invention will become apparent to those skilled in the art from the following detailed description, which shows and describes illustrative embodiments of the invention. As will be realized, the invention is capable of modifications in various obvious aspects, all without departing from the spirit and scope of the present invention. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1A is a side cutaway view depicting an inflatable device for maintaining procedural space in a body cavity, according to one embodiment.

FIG. 1B is a perspective cutaway view of the device of FIG. 1A.

FIG. 1C depicts another side cutaway view of the device of FIG. 1A.

FIG. 1D shows a perspective cutaway view of the uninflated device of FIG. 1A.

FIG. 2A is a perspective cutaway view of an inflatable device for maintaining procedural space in a body cavity, according to another embodiment.

FIG. 2B is a side cutaway view of the device of FIG. 2A.

FIG. 2C is a side cutaway view of the uninflated device of FIG. 2A.

FIG. 3 is a schematic depiction of an inflatable balloon having an inner skeleton, according to one embodiment.

FIG. 4A is a side cutaway view depicting a device for maintaining procedural space in a body cavity, according to one embodiment.

FIG. 4B is a perspective cutaway view of the device of FIG. 4A.

FIG. 4C is another side cutaway view of the device of FIG. 4A.

FIG. 4D is a schematic depiction of the device of FIG. 4A in a collapsed configuration.

FIG. 5A is a side view of a wall retention pin having a retention component in the collapsed configuration, according to one embodiment.

FIG. 5B is a side view the wall retention pin of FIG. 5A in which the retention component is in the deployed configuration.

FIG. 5C is a side cutaway view of three wall retention pins similar to that of FIG. 5A in use, according to one embodiment.

FIG. 5D is another side cutaway view of the three wall retention pins of FIG. 5C in a relaxed configuration in which the cavity wall is not being urged away from the cavity.

FIG. 6A is a side cutaway view of three wall retention pins, each having an attachment component, according to another embodiment.

FIG. 6B is another side cutaway view of the three wall retention pins of FIG. 6A in a relaxed configuration in which the cavity wall is not being urged away from the cavity.

FIG. 7A is a side cutaway view of a wall retention system, according to one embodiment.

FIG. 7B is a perspective cutaway view of the wall retention system of FIG. 7A.

FIG. 7C is a perspective view of one modular component of a wall retention system, according to one embodiment.

FIG. 7D is a perspective cutaway view of another modular component of a wall retention system, according to another embodiment.

FIG. 8A is an end view of a modular component of a wall retention system, according to a further embodiment.

FIG. 8B is a side view of the modular component of FIG. 8A.

FIG. 9 is a side cutaway view of a device support system, according to one embodiment.

FIG. 10 is a side cutaway view of another device support system, according to another embodiment.

FIG. 11 is a side cutaway view of yet another device support system, according to a further embodiment.

FIG. 12 is a perspective cutaway view of a device support and control system, according to another embodiment.

FIG. 13 is a perspective view of a procedural delivery device, according to one embodiment.

FIG. 14 is a perspective view of another delivery device, according to another embodiment.

FIG. 15 is a side cutaway view of another delivery device, according to a further embodiment.

FIG. 16 is a side view of another delivery device component, according to another embodiment.

FIG. 17A is a side cutaway view of another delivery device, according to another embodiment.

FIG. 17B is another side cutaway view of the delivery device of FIG. 17A.

FIG. 17C is another side cutaway view of the delivery device of FIG. 17A.

FIG. 18 is a perspective view of a retraction device, according to one embodiment.

FIG. 19A is a cross-sectional depiction of an insertion device, according to one embodiment.

FIG. 19B is a cross-sectional depiction of another insertion device, according to one embodiment.

FIG. 19C is a cross-sectional depiction of a further insertion device, according to one embodiment.

FIG. 20A is a perspective view of an insertion and retraction device, according to one embodiment.

FIG. 20B is another perspective view of the device of FIG. 20A.

DETAILED DESCRIPTION

The various systems and devices disclosed herein relate to devices for use in medical procedures and systems. More specifically, the various embodiments relate to various cavity inflation or structural retention system embodiments, various medical device attachment and control components, and various medical device delivery, control, and retrieval devices, all of which can be used in various procedural devices and systems.

It is understood that the various embodiments of cavity structural retention systems, device attachment components, and device delivery, control, and retrieval systems and other types of devices disclosed herein can be incorporated into or used with any known medical devices, including, but not limited to, robotic or in vivo devices as defined herein.

For example, the various embodiments disclosed herein can be incorporated into or used with any of the medical devices disclosed in copending U.S. application Ser. No. 11/932,441 (filed on Oct. 31, 2007 and entitled "Robot for Surgical Applications"), Ser. No. 11/695,944 (filed on Apr. 3, 2007 and entitled "Robot for Surgical Applications"), Ser. No. 11/947,097 (filed on Nov. 27, 2007 and entitled "Robotic Devices with Agent Delivery Components and Related Methods"), Ser. No. 11/932,516 (filed on Oct. 31, 2007 and entitled "Robot for Surgical Applications"), Ser. No. 11/766,683 (filed on Jun. 21, 2007 and entitled "Magnetically Coupleable Robotic Devices and Related Methods"), Ser. No. 11/766,720 (filed on Jun. 21, 2007 and entitled "Magnetically Coupleable Surgical Robotic Devices and Related Methods"), Ser. No. 11/966,741 (filed on Dec. 28, 2007 and entitled "Methods, Systems, and Devices for Surgical Visualization and Device Manipulation"), Ser. No. 12/171,413 (filed on Jul. 11, 2008 and entitled "Methods and Systems of Actuation in Robotic Devices"), 60/956,032 (filed Aug. 15, 2007), 60/990,062 (filed on Nov. 26, 2007), 60/990,076 (filed Nov. 26, 2007), 60/990,086 (filed on Nov. 26, 2007), 60/990,106 (filed on Nov. 26, 2007), 60/990,470 (filed on Nov. 27, 2007), 61/030,588 (filed on Feb. 22,

2008), and 61/030,617 (filed on Feb. 22, 2008), all of which are hereby incorporated herein by reference in their entireties.

In an exemplary embodiment, any of the various embodiments disclosed herein can be incorporated into or used with a natural orifice transluminal endoscopic surgical device, such as a NOTES device. Those skilled in the art will appreciate and understand that various combinations of features are available including the features disclosed herein together with features known in the art.

Certain device implementations disclosed in the applications listed above can be positioned within a body cavity of a patient, including certain devices that can be positioned against or substantially adjacent to an interior cavity wall, and related systems. An “in vivo device” as used herein means any device that can be positioned, operated, or controlled at least in part by a user while being positioned within a body cavity of a patient, including any device that is positioned substantially against or adjacent to a wall of a body cavity of a patient, further including any such device that is internally actuated (having no external source of motive force), and additionally including any device that may be used laparoscopically or endoscopically during a surgical procedure. As used herein, the terms “robot,” and “robotic device” shall refer to any device that can perform a task either automatically or in response to a command.

Certain implementations disclosed herein relate to cavity inflation or cavity structural retention devices or systems that are configured to provide space within the cavity of a patient for purposes of operating various medical devices and components within the cavity to perform one or more of various medical procedures, including, for example, the various medical devices and procedures disclosed in the various applications listed above and incorporated herein.

FIGS. 1A-1D, 2A-2C, and 3 depict various embodiments of inflatable devices that can be used to provide or create procedural space in a body cavity.

FIGS. 1A-1D depict one example of an inflatable cavity inflation system 10A, 10B, according to one embodiment. In this embodiment, the system 10A, 10B has two inflatable components 10A, 10B, which can also be referred to herein as “balloons.” The two balloons 10A, 10B can be inserted into and positioned in a body cavity as best shown in FIGS. 1A-1C such that they create or provide space within the cavity that allows a user (such as a doctor or surgeon) to operate various devices and/or perform various procedures within the space in the cavity. The two balloons 10A, 10B can be positioned in any fashion within the cavity to maintain the surgical space in the cavity. Alternatively, one inflation balloon or more than two inflation balloons can be positioned in the body cavity.

According to one embodiment, the body cavity is the abdominal cavity 12 as shown best in FIGS. 1A-1C. In such an embodiment, the balloons 10A, 10B are positioned on or adjacent to the various organs and tissues 14 in the cavity 12. Alternatively, the cavity can be any known body cavity.

In one implementation, the inflatable components 10A, 10B are made of polyethylene terephthalate (“PET”), which is manufactured by Advanced Polymers, Inc. of Salem, N.H. Alternatively, the components 10A, 10B can be made of nylon. In a further alternative, the components 10A, 10B are made of polyurethane. In yet another alternative, the components 10A, 10B can be made of any known expandable, durable, biocompatible material that can be used in medical devices.

The inflatable components 10A, 10B in one embodiment have tubing (not shown) or any other such connection

attached to the components 10A, 10B that can couple the components to an external pump (not shown) that can be used to inflate the balloons 10A, 10B. Alternatively, the inflatable components 10A, 10B each have an inflation device (not shown) disposed somewhere within or on each balloon 10A, 10B that can be used to inflate each balloon 10A, 10B. According to one embodiment, the inflation device is a robotic device with a pressurized cavity that is opened for “self” inflation of the balloon.

In an alternative embodiment as shown in FIGS. 2A-2C, a single inflatable component 20 is provided that is shaped like a donut or hoop. In this embodiment, the single component 20 can provide sufficient space within the patient’s cavity to allow a user to operate a medical device and/or perform a medical procedure. According to one implementation, the donut-shaped balloon 20 can be positioned over the target procedural site such that the open portion in the center of the balloon 22 forms or maintains a procedural cavity space for purposes of the procedure.

It is understood that such a donut-shaped balloon 20 can be made of the same material as the balloons 10A, 10B discussed above.

In use, any of the balloons 10A, 10B, 20 can be utilized in the following manner. The un-inflated balloon(s) can be positioned inside the cavity as shown for example in FIGS. 1D and 2C. Once positioned, the balloon (or balloons) is inflated to provide or create procedural space within the cavity. At the conclusion of the procedure, the balloon(s) can be deflated or the pressurized gas can be sucked out by an external pump, and then the balloon(s) can be removed.

In a further alternative, any configuration of the balloons 10A, 10B, 20 can include internal structural members such as a series of pins or linkages inside of the balloons. FIG. 3 provides a schematic depiction of one embodiment of a balloon 30 having a skeleton or inner structure 32 disposed within the balloon 30. In the embodiment of FIG. 3, the skeleton 32 is a wire mesh similar to a stent. Alternatively, the skeleton 32 can be any structure configured to provide some deployable rigidity or structure to the balloon 30.

In use, the balloon 30 can be inserted in a deflated or undeployed state and, once positioned as desired, the inner structure 32 is triggered to expand into the deployed position as shown in FIG. 3 to provide or maintain a procedural space within a body cavity. According to one implementation, the inner skeleton 32 deploys in a fashion similar to a vascular stent, in which a tool of some kind is used to actuate the skeleton 32 to deploy. According to a further embodiment, the skeleton 32 locks into place upon deployment.

It is understood that many different medical devices, components, and procedures can be used in conjunction with the various inflatable device embodiments as shown in FIGS. 1A-1D, 2A-2C, and 3, including the positionable in vivo devices and various robotic devices and procedures described in the various applications disclosed and incorporated by reference above. That is, the various inflatable device embodiments can be used to provide and/or maintain procedural space in a body cavity such that any type procedure or related device for use in a body cavity can be used in the space, including the various devices and procedures disclosed and incorporated by reference above.

FIGS. 4A-4D depict a different support device 40 for providing or creating procedural space in a body cavity, according to one embodiment. This device 40 can be a scaffold-like structure intended to be expandable or deployable within the body cavity.

As shown best in FIGS. 4A-4C, the support device 40 operates to hold the upper cavity wall up in a tent-like

fashion. That is, the device **40** can be positioned within a body cavity such as an abdominal cavity **42** to provide a procedural space **44**. The device **40** has a plurality of arms **46** (also referred to as “linkages”) as shown in FIGS. **4A** and **4B**. In one embodiment, the arms **46** are all mechanically coupled to each other such that they can be converted between a collapsed configuration as depicted in FIG. **4D** and the deployed configuration as shown in FIGS. **4A-4C**. The device **40** is deployed by actuating the arms **46** into the configuration as shown. In one embodiment, the device **40** is deployed automatically through the use of springs or inflatable balloons that are attached at or otherwise positioned in the hinges **48** of the device **40**. Alternatively, the device **40** has motors or hydraulics that can be used to mechanically deploy the device **40**. In a further alternative, any known component that can urge the device **40** from the collapsed configuration to the deployed configuration can be coupled or otherwise associated with the hinges of the device **40**.

The arms **46** of the device **40** can be made of any biocompatible polymers. Alternatively, the arms **46** can be made of stainless steel. In a further alternative, the arms **46** can be made of any known substantially rigid, biocompatible material.

It is understood that the arms **46** of the device **40** are coupled at joints **48**, as best shown in FIGS. **4B** and **4D**, or other similar known connection components. It is further understood that these joints **48** can be any known pivot or hinge joints. Alternatively, the joints **48** can be universal joints with rotation in two planes.

In accordance with another implementation, externally-supported wall retention systems and devices are provided to create and/or maintain a procedural space in a body cavity.

It is understood that many different medical devices, components, and procedures can be used in conjunction with the various support device embodiments as shown in FIGS. **4A-4D**, including the positionable in vivo devices and various robotic devices and procedures described in the various applications incorporated by reference above. That is, the various support device embodiments can be used to provide and/or maintain procedural space in a body cavity such that any type procedure or related device for use in a body cavity can be used in the space, including the various devices and procedures disclosed and incorporated by reference above.

FIGS. **5A-5D** depict one embodiment of an externally-supported wall retention system. In this embodiment, the system relates to at least two retention pins similar to the pin **50** depicted in FIGS. **5A** and **5B** that can be inserted through the cavity wall, attached to the wall, and subsequently urged away from the cavity to create a procedural space within the cavity.

As shown in FIGS. **5A** and **5B**, each pin **50** (also referred to herein as a “needle”) has a distal end having a needle tip **54** and two leaves or toggle-like components **52A**, **52B** that are each pivotally attached to the pin **50** such that the leaves **52A**, **52B** can move between a collapsed position as shown in FIG. **5A** and a deployed position as shown in FIG. **5B**. In the collapsed position depicted in FIG. **5A**, each of the leaves **52A**, **52B** are disposed in a position parallel to the length of the pin **50**. In the deployed position depicted in FIG. **5B**, each of the leaves **52A**, **52B** are disposed in a position perpendicular to the length of the pin **50**.

In an alternative embodiment, any known toggle-like or attachment component can be provided near the distal end of the pin **50** to allow for insertion of the pin **50** through the cavity wall **56** and then capture of the interior portion of the

wall while the pin **50** is being urged away from the cavity to create space within the cavity.

In use as best shown in FIGS. **5C** and **5D**, at least two pins or needles **50** are positioned in the cavity wall **56** such that the pins **50** are attached to the wall **56** and then can be urged away from the cavity **58** in the direction of the arrows in FIG. **5A** to provide procedural space within the cavity **58**. In one embodiment, each pin or needle **50** is inserted into the cavity wall **56** along the axis indicated by the letter A in FIG. **5C** while the leaves **52A**, **52B** are in the collapsed position. Once the leaves **52A**, **52B** are inserted through the wall **56** and into the body cavity, the leaves **52A**, **52B** are moved into the deployed position as shown in FIG. **5B** (and in FIGS. **5C** and **5D**). Each pin **50** can then be urged or moved in an outward direction (away from the patient) until the leaves **52A**, **52B** are in contact with the wall **56**. According to one embodiment, sufficient force is applied to the pin **50** such that the leaves **52A**, **52B** can support the wall **56** and maintain an open cavity configuration, wherein the cavity wall **56** is urged away from the organs within the cavity, as shown in FIG. **5C**.

In one embodiment, the force applied to the pin **50** or pins **50** is a manual force applied by the surgeon or assistant pulling on the pins with her or his hands. Alternatively, the force applied is a mechanical force provided by a device or by attaching the pins **50** to a stationary device.

An alternative embodiment of an externally-supported wall retention system is provided in FIGS. **6A** and **6B**. In this embodiment, each of the pins **60** operate in a similar fashion as the pins **50** shown in FIGS. **5A-5D**. That is, the pins **60** are attached to the cavity wall and urged to pull the wall away from the cavity to provide procedural space within the cavity. However, in contrast to the pins **50** described above, each pin **60** of FIGS. **6A** and **6B** is not inserted into the cavity and attached to the inner wall of the cavity. Instead, each pin **60** has an attachment component **62** that can be attached to an external portion of the patient outside the body cavity. That is, the attachment component **62** can attach to an external portion **64** of the cavity wall.

In one embodiment, the attachment component **62** is a “grasper” that attaches to the external portion **64** of the cavity wall **66** by grasping the external portion **64**. Alternatively, the attachment component **62** has barbs or other components that can be inserted partially into the external portion **64** of the wall **66**. In a further alternative, the attachment component **62** has an adhesive that is used to attach the component **62** to the wall **66**. In use, once the attachment component **62** is attached to the wall **66** as shown in FIG. **6B**, each pin **60** is urged away from the patient in the same fashion described above such that the pins **60** urge the wall **64** away from the body and thereby maintain an open cavity space as shown in FIG. **6A**.

It is understood that many different medical devices, components, and procedures can be used in conjunction with the various externally-supported wall retention embodiments as shown in FIGS. **5A-5D** and **6A-6B**, including the positionable in vivo devices and various robotic devices and procedures described in the various applications incorporated by reference above. That is, the various wall retention device embodiments can be used to provide and/or maintain procedural space in a body cavity such that any type procedure or related device for use in a body cavity can be used in the space, including the various devices and procedures disclosed and incorporated by reference above.

FIGS. **7A-8B** depict further exemplary implementations of externally-supported wall retention and device positioning systems and devices that create and/or maintain a

procedural space in a body cavity while also providing for positioning one or more medical devices within the body cavity.

FIGS. 7A-7D depict an embodiment of an externally-supported wall retention and device positioning system that provides for both maintaining the open configuration of the surgical cavity and for positioning a medical device within the cavity. In one implementation, the system as depicted provides for positioning one or more medical devices along an interior wall of the cavity. As shown in FIG. 7A, the device or system 70 has two or more modular components 72 (also referred to herein as “rail modules”) that are hingedly coupled to each other. According to one embodiment, each of the modular components 72 has at least one magnet 74 disposed therein, as best shown in FIGS. 7A and 7C. Alternatively, each of the modular components 72 has at least one attachment point 76 to which a pin or needle 78 can attach, as best shown in FIG. 7D.

The device 70 as shown in FIG. 7A is configured such that each of the modular components 72 can be inserted through a small incision or a trocar-like tube into the surgical cavity. That is, the device 70 can be configured in an elongate shape such that its profile is small enough to be inserted through such an incision or tube.

After insertion, the modular components 72 of the device 70 are positioned against the interior of the cavity wall 84. In one embodiment, the device 70 is positioned against the wall 84 using exterior magnets 80 positioned outside the cavity as shown in FIGS. 7A and 7B. In one embodiment as shown, the magnets 80 are positioned in handles 82. This approach could provide a method for non-insufflating NOTES procedures if multiple devices 70 are positioned along the cavity wall 84. That is, it is possible to use this embodiment to create and/or maintain a procedural space in a body cavity without insufflation. The use of multiple modules 72 allows for the implementation of multiple magnets or needles for attachment to the cavity wall. This provides for a stronger attachment because the force applied by the multiple magnets to create a procedural space is greater than that created by one or two magnets.

Alternatively, the device 70 is positioned against the wall using exterior pins or needles 78, as shown in FIG. 7D.

According to one alternative embodiment, a modular component 100 similar to those disclosed in FIGS. 7A-7D is shown in FIGS. 8A-8B that is configured to receive one or more medical devices along track or mating components in the modular components. Each module 100 in this embodiment has at least one attachment magnet 112 and one or more tracks or mating components 118 with which a robotic device 114 can moveably mate using a set of wheels or cogs 116 and along which the robotic device 114 can move. Thus, two or more modular components 100 can be connected to each other to create a “railway” that one or more medical devices can traverse to move around the procedural cavity (similar to the set of modules as shown in FIG. 7A).

Each module 100 as shown in FIG. 8A has at least one magnet 112 associated with or disposed within the module 100. Further, each module 100 has a mating component 118 associated with or defined by the module 100. A medical device 114 can be coupled with the rail module 100 by the mating component 116 on the device 114. In one embodiment as shown, the mating component 116 on the device 114 is a wheel or cog that can couple with the rail 118 on the module 100. In one embodiment, the device 114 can be maintained in a substantially fixed position such that the device 114 can move along the rail module 100 relative to the cavity. This module 100 can be positioned transversely

or sagittally along the cavity wall. Alternatively, the module 100 can be positioned in any known fashion within the cavity to allow for transporting a medical device along a predetermined path. In a further embodiment, more than one module 100 is positioned within the cavity and coupled together (in a fashion similar to FIG. 7A) and the device 114 can be positioned within the coupled modules 100 so that the device 114 can traverse along the length of the coupled modules 100. Alternatively, more than one device can be placed along the coupled modules 100 or more than one set of coupled modules 100 can be positioned in the cavity.

One advantage of the multiple modules with multiple magnets is that the weight of the attached device can be distributed across multiple attachment points. Furthermore, if the device includes arms, this approach provides a more stabilized and distributed base for tissue manipulation forces.

It is understood that many different medical devices, components, and procedures can be used in conjunction with the various externally-supported wall retention and device positioning systems and device embodiments as shown in FIGS. 7A-8B, including the positionable in vivo devices and various robotic devices and procedures described in the various applications incorporated by reference above. That is, the various wall retention and device positioning embodiments can be used to provide and/or maintain procedural space in a body cavity while also providing for the positioning and/or attachment of one or more medical devices, such that any type of procedure or related device for use in a body cavity can be used and positioned in the space, including the various devices and procedures disclosed and incorporated by reference above.

FIGS. 9-12 depict exemplary implementations of device positioning systems and devices that provide for positioning one or more medical devices within the body cavity.

FIG. 9 depicts one embodiment of a modular “railed” device 140. In this embodiment, each module 141 has a hook or attachment component 142 that can attach to the cavity wall 144. In one embodiment as shown, each module 141 is attached to the wall 144 with a hook or similar attachment component 142 that penetrates the wall 144. Alternatively, each module 141 is attached to the wall using an adhesive. In a further alternative, each module 141 is attached to the wall by any known attachment method or device.

Each module 141 also has a track or mating component 148 that is capable of coupling with one or more medical devices. The coupling of each module 141 to each other or positioning of the modules 141 adjacent to each other creates a positioning device 140 along which a medical device 114 can move or be positioned.

FIG. 10 depicts another embodiment of a positioning device 150. Instead of attaching with an attachment component to a cavity wall 152, this device 150 is supported in the cavity 162 using at least two legs or links 156 that are positioned along a bottom portion of the cavity to support the rail 158. In the embodiment depicted in FIG. 10, the device attachment component is a rail 158 along which the medical device 114 can move or be positioned. Alternatively, the device attachment component can be any such component along which the one or more medical devices 114 can be positioned. In the embodiment depicted in FIG. 10, the device 150 has four legs 156 that create a swing-set-like structure. A medical device 114 can be moveably attached to the rail 158 such that the medical device 114 can move back and forth along the rail 158.

In one alternative implementation, the railed device 150 can have robotic, or otherwise actuated, components. For

example, the legs **156** can have actuators (not shown) that actuate the legs **156** to move such that the device **114** can be raised or lowered. In a further embodiment, the attachment point **160** where the medical device **114** is coupled to the rail **158** can be coupled to an actuator (not shown) such that the actuator can operate to move the device **114** along the rail **158**.

In accordance with another implementation, the railed device **150** can support a medical device **114** as shown and described above while also providing cavity space maintenance. That is, the device **150** can also provide support to hold the upper cavity wall away from the lower cavity wall and therefore maintain the procedural cavity space.

FIG. **11** depicts another embodiment of a medical device positioning or attachment device **130**. The device **130** has a wall attachment component **138** and a device attachment component **136**. The wall attachment component **138** as shown in FIG. **11** is a hook that attaches to the cavity wall **132**. Alternatively, the wall attachment component **138** can utilize an adhesive. In a further alternative, the wall attachment component **138** can be any known component for attaching to the cavity wall. Further, according to another implementation, attachment device **130** is made of a degradable material and thus need not be removed from the cavity wall after the procedure is completed.

The device attachment component **136** provides for removable attachment to a medical device **114**. In one embodiment, the device attachment component **136** is a magnet that removably couples to the medical device **114**. Alternatively, the attachment component **136** provides for a mechanical coupling with the medical device **114**. In a further alternative, the attachment component **136** provides for any type of attachment method or device to attach to the medical device **114** such that the device **114** can be removed. In one implementation, the device **114** can be removed and a second device can be attached. In a further implementation, more than one medical device **114** can be attached.

Another embodiment of a medical device attachment or positioning device is depicted in FIG. **12**. In this embodiment, the medical device **114** is positioned against an interior cavity wall using two pins **174A**, **174B** inserted through the cavity wall and coupled to the device **114**. In one embodiment, these pins **174A**, **174B** are thin needles that require no suturing or recovery time. According to one implementation, the pins **174** can be known needles currently used for amniocentesis and chorionic villi sampling. Alternatively, each pin **174A**, **174B** can be any pin-like or needle-like component capable of being inserted into the patient's body and coupled to the medical device **114** disposed within the patient's body. After insertion, the needles **174** are attached to the in vivo device **114**. In one embodiment, only one pin is attached, thereby allowing the device **114** to rotate about the single attachment point. Alternatively, two pins are inserted to hold the robot in position, with additional needles inserted as needed to move the robot to a different orientation. In another implementation, these attachment pins can also be used in conjunction with magnets to position and/or attach the device.

The use of attachment pins provides a stable attachment of the medical device to or near the cavity wall. In those embodiments in which the medical device is controlled by some form of exterior component, the pins can assist in ensuring the medical device is positioned near or adjacent to the exterior handle or other exterior component. Alternatively, the pin length is controlled or manipulated to provide a vertical degree-of-freedom that would allow the medical device to move up and down relative to the pin and/or the

body cavity. Attachment or coupling of the pins to the device includes self-assembly techniques that include magnets at the pin tips or semi-autonomous connection with the medical device. Alternatively, the pins are attached through surgeon assistance in vivo using endoscopic tools or other medical devices.

In one method, the pin or pins are inserted into the patient's body and then the medical device or devices are coupled to the pin(s). In another embodiment, the medical device is positioned against the cavity wall prior to insertion of the pin(s), and the pin (or pins) is inserted such that the pin couples to the device during insertion. Alternatively, the pin (or pins) is first inserted and then the medical device is coupled to the pin.

According to one embodiment, the pins **174** described herein can be used to assist with the attachment or positioning of one or more medical devices within a body cavity of an obese patient in which the cavity wall **176** has a thickness that makes it difficult or impossible to use magnetic attachment devices or methods.

It is understood that many different medical devices, components, and procedures can be used in conjunction with the various device positioning embodiments as shown in FIGS. **9-12**, including the positionable in vivo devices and various robotic devices and procedures described in the various applications incorporated by reference above. That is, the various device positioning embodiments can be used to provide for the positioning and/or attachment of one or more medical devices, such that any type of procedure or related device for use in a body cavity can be used and positioned in the space, including the various devices and procedures disclosed and incorporated by reference above.

FIGS. **13-20B** depict exemplary implementations of medical device **114** insertion and retraction devices.

FIG. **13** depicts an overtube **210**, according to one embodiment, for use in inserting a medical device into a patient's body and retracting the device (shown, for example, at **114** in FIGS. **14-16** and **18**) from the body through the overtube **210**. It is understood that the term "overtube" as used herein is intended to mean any medical procedural tube that is inserted into a patient and positioned such that further procedural devices can be inserted through the tube into the patient, retrieved through the tube from the patient, and/or such that the further procedural devices can be operated inside the patient through the tube. Thus, "overtube" includes any tube that is inserted down the patient's esophagus or through any incision or into any cavity and positioned such that other devices or instruments can be inserted into the patient's body.

The overtube **210** as shown in FIG. **13** defines a device lumen **212** through which a medical device, such as a robotic device, can be passed. In addition, the overtube **210** also defines a wire lumen **214** through which an insertion wire **216** can be passed. In the embodiment depicted in FIG. **13**, the wire lumen **214** is defined in the outer wall **218** of the overtube **210** and has a diameter that is smaller than the device lumen **212**.

In use, the overtube **210** allows a user to pull a medical device **114** through the overtube **210** from the proximal end **220** to the distal end **222** of the overtube **210**. That is, according to one implementation, the insertion wire **216** is inserted through the device lumen **212** and also inserted through the wire lumen **214** as depicted in FIG. **13**, such that the proximal end **224** of the wire **216** and the distal end **226** of the wire **216** both extend from the proximal end **220** of the overtube **210**.

The proximal end **224** of the wire **216** is then attached to the device (not shown) to be pulled through the overtube **210**. Alternatively, the wire **216** is attached to the device prior to positioning the wire **216** in the tube **210**. The distal end **226** of the wire **216** is then pulled by the user such that the wire moves in the direction indicated by the arrows A, B, and C, thereby resulting in the device being pulled toward the distal end **222** of the overtube **210**.

In one implementation, the wire **216** is a braided metal cable. Alternatively, the wire **216** is a nylon string. In yet another alternative, the wire can be any such wire, tether, thread, cord, or any other type of elongate flexible material that can be used in medical procedures such as the methods described herein.

According to one embodiment, the overtube **210** is a flexible polyethylene tube. Alternatively, the overtube can be any tube, cannula, or other type of hollow elongate object having a lumen that can be used for insertion of devices into, or use of devices within, a patient's body.

FIG. **14** depicts one method and device for attachment of a wire **230** to a medical device **114** for device insertion. In this embodiment, the wire **230** has an attachment component **234** in the form of a ball coupled to the proximal end **236** of the wire **230**. In use, the clamp **238** on the distal end **240** of the device **114** is clamped onto or otherwise coupled with the ball **234** on the wire **230**. Upon attachment of the device **114** to the wire **230** via attachment of the clamp **238** to the ball **234**, the user can pull the distal end **242** of the wire **230** to move the wire **230** as shown by the arrows A, B, and C to thereby pull the device **114** toward the distal end **244** of the overtube **210**, which is the direction depicted by arrow D. Once the device **114** has reached the desired position, the user can operate the clamp **238** to release the ball **234** such that the device **114** can then be used to perform the intended procedure.

According to the embodiment depicted in FIG. **14** and discussed above, the attachment component **234** is a ball. Alternatively, the attachment component is a hook that can hook to a portion or component of the medical device. In another embodiment, the attachment component is a loop-shaped portion of string or cable that can be looped or otherwise coupled with an appropriate mating component on the medical device. Alternatively, the component **234** can be any shape or any component that allows for easy attachment to the medical device **114**. In a further alternative, the attachment component **234** is a magnet that can magnetically couple with the device **114**. In yet another alternative, the attachment component can be any component that can be used to removably attach the wire **230** to a medical device **114**.

FIG. **15** depicts an alternative embodiment of an overtube **210** for insertion or delivery of a medical device. In this implementation, the overtube **210** has a protrusion **252** that protrudes or extends from the distal end **254** of the tube **210**. The term "protrusion" shall encompass, for purposes of this application, any portion or component of the overtube **210**, or a separate component, such as a lip or an extension, that protrudes or extends from the distal end **254** of the tube **210**. According to one embodiment, the wire lumen **256** is defined in the protrusion **252** as shown in FIG. **15** and has a diameter that is smaller than the device lumen **262**.

In use, the protrusion **252** as shown in FIG. **15** facilitates positioning of the medical device **114**, which can be a robotic device according to one embodiment. That is, as the wire **260** is pulled as shown by arrow A, the wire **260** pulls the device **114** toward the protrusion **252** on the distal end **254** of the tube **210**. Because the protrusion **252** extends

beyond the distal end **254** of the tube, the device **114** exits from the device lumen **262** as it approaches the protrusion **252** and thus is pulled into or positioned in the target or procedural site in the patient's body. In an alternative step, a magnetic handle **264** or other magnetic component can be positioned externally to the body cavity and used to further position the device **114**. Alternatively, any external positioning component can be utilized in conjunction with the overtube **210** to facilitate positioning the device as desired and/or with precision.

A further alternative implementation is depicted in FIG. **16**, in which the overtube **210** has a protrusion **272** having an indentation or device receiving component (also referred to as a "docking component") **274** that is configured to receive a medical device **114** such that the device **114** can couple with or "dock" to the protrusion **272** or to the end of the overtube **210** for final positioning or even during the entire or a significant portion of the medical procedure. In this implementation, the coupling can be accomplished with magnets or mechanical attachment components such as claims or screws. In yet another embodiment, the medical device docks to the protrusion or to the overtube itself to charge onboard batteries, or to store a biopsy sample, or to exchange end-effectors. As shown, the device has a device body **114A** with two arms **114B**, **114C**, each with an end-effector **115B**, **115C**.

Alternatively, the protrusion can be a deployable protrusion. For example, one embodiment of a deployable protrusion **282** is depicted in FIGS. **17A** and **17B**. In this embodiment, the protrusion **282** is movably coupled to the overtube **210** and can unfold using a spring **283**, such as a torsional spring. FIG. **17A** depicts the protrusion **282** in the undeployed position in which the torsional spring **283** is configured to urge the protrusion **282** into the deployed position but is retained in the undeployed or closed position by retention component **287**. The retention component **287** can be a hook, latch, or any other actuatable retention component that can be actuated to release the protrusion **282** from the undeployed position. FIG. **17B** depicts the protrusion **282** at a position between the undeployed position and the deployed position and FIG. **17C** depicts the protrusion **282** in the fully deployed position.

In use, the protrusion **282** can be maintained in the undeployed position during insertion. That is, according to one embodiment, the protrusion **282** is not be deployed until the overtube **210** is inserted into the patient. At this point, the protrusion **282** can then be deployed through a series of actuators or cables. For example, according to one embodiment as shown in FIG. **17A**, the overtube **210** has a wire or cable **285** coupled to the retention component **287** such that the wire or cable **285** can be pulled in the direction of arrow A to actuate the retention component **287** to release the protrusion **282**. Once released, the force applied to the protrusion **282** by the torsional spring **283** causes the protrusion **282** to move toward the deployed position as shown in FIG. **17B**. FIG. **17C** depicts the protrusion **282** after it has reached the deployed position.

Alternatively, the overtube **210** can have any other kind of overtube positioning component at its distal end. That is, any component that facilitates exit of the device from the device lumen and/or positioning of the device at the target area can be used with the overtube. For example, it is understood that the concept of this positioning component shall encompass any hole or gap defined in the tube that provides for positioning of the device in the same fashion that the protrusion accomplishes such positioning.

In another embodiment, FIG. 18 depicts a method and device for retracting a device from an interior portion of a patient's body. More specifically, FIG. 18 depicts a retraction wire 290 that can be inserted through the device lumen 292 of the overtube 210 and into the procedural site. In use, the user can operate the clamp 295 or some other type of attachment component of the medical device 114 to attach to the wire attachment component 298, which in this embodiment is a ball. In the embodiment shown, the device 114 has a device body 114A with two arms 114B, 114C. Alternatively, the wire attachment component 298 can be any such attachment component as described above, including a magnet or any other component that provides for attachment of the wire 290 and the device 114. Once the device 114 is attached to the wire 290, the user pulls the wire 290 toward the proximal end 299 of the tube 294 (in the direction indicated by arrow A), thereby retracting the device 114 from the procedural site.

FIGS. 19A, 19B, and 19C depict profiles of three different over tubes 210A, 210B, and 210C, according to three different embodiments. Each overtube has an orientation component 306, 308, and 310 that cooperates with the device to be inserted through the overtube 210A, 210B, or 210C to orient the device. More specifically, according to the embodiments depicted in FIGS. 19A, 19B, and 19C, the orientation component in each figure is configured to mate or couple with the body of the device being inserted through the overtube 210A, 210B, or 210C such that the device is forced to be oriented in a particular fashion as it passes through the overtube 210A, 210B, 210C, thereby facilitating the proper orientation of the device during insertion and/or positioning.

It is understood that FIGS. 19A, 19B, and 19C are merely exemplary, and that any orientation component configuration can be provided so long as it results in mating with the device to be inserted such that the device can be provided with the proper orientation.

FIGS. 20A and 20B depict another method and device for inserting and retracting a medical device, according to one embodiment. In this embodiment, the connection component 320 (also referred to as a "tether") connecting the medical device 114 to the external controller (not shown) is disposed through the wire lumen 324 and the device lumen 326 of the overtube 210 as shown in FIG. 20A and performs in the same fashion as the embodiments of the insertion wires described above. That is, in use, the tether 320 can be pulled as indicated by the arrow A in FIG. 20A such that the device (not shown) attached to the opposite end (not shown) of the tether 320 is urged toward the distal end 330 of the overtube 210 until it exits the device lumen 326 of the overtube 210 and is positioned at the procedural site, as depicted in FIG. 20B.

In this implementation as shown in FIGS. 20A and 20B, the tether 320 can be electrical cabling, hydraulic or pneumatic lines, or suction and irrigation lines, any of which can supply further power or actuation to the device 114.

It is understood that in certain embodiments, the overtube is a relatively stiff tube that exhibits some flexibility for facilitating insertion into the patient. In alternative embodiments, the overtube is designed to be stiff enough to provide sufficient rigidity perpendicular to the primary axis of the tube for operation of hydraulics or pneumatic lines. Furthermore, it is understood that positioning the tether in a wire lumen or tether lumen in the overtube helps keep the overtube inner lumen free from tethers, thereby facilitating insertion of various devices through the overtube.

It is understood that many different medical devices, components, and procedures can be used in conjunction with the various device insertion, positioning, and retraction embodiments as shown in FIGS. 13-20B, including the positionable in vivo devices and various robotic devices and procedures described in the various applications incorporated by reference above. That is, the various device insertion, positioning, and retraction embodiments can be used to provide for the insertion, positioning, and/or retraction of one or more medical devices, such that any type of procedure or related device for use in a body cavity can be inserted into, positioned within, and/or retracted from the space, including the various devices and procedures disclosed and incorporated by reference above.

Although the present invention has been described with reference to preferred embodiments, persons skilled in the art will recognize that changes may be made in form and detail without departing from the spirit and scope of the invention.

What is claimed is:

1. A delivery or removal device for delivering or moving a robotic medical device for laparoscopic surgery, the device comprising:

a. a robotic medical device comprising a first arm and second arm;

b. an overtube comprising:

i. an elongate body having a wall, a first end and a second end;

ii. a device lumen disposed within the body and extending from the first end to the second end; and

iii. a wire lumen disposed within the wall of the elongate body and extending from the first end to the second end, wherein the device lumen is configured to accommodate the passage of the robotic medical device comprising a first arm and a second arm; and

c. a retraction wire configured to be disposed within the wire lumen and device lumen so as to urge the robotic medical device comprising a first arm and a second arm through the device lumen.

2. The device of claim 1, wherein the overtube is sized to be positionable through a laparoscopic port or natural orifice.

3. The device of claim 1, wherein the overtube comprises a protrusion at the second end, wherein the protrusion further defines the wire lumen.

4. The device of claim 3, wherein the protrusion further comprises a robotic medical device receiving component configured to receive the robotic medical device.

5. The device of claim 4, wherein the medical device receiving component comprises at least one magnet configured to magnetically couple to the robotic medical device comprising the first arm and second arm, whereby the robotic medical device comprising a first arm and a second arm releasably couples to the medical device receiving component.

6. The device of claim 5, wherein a portion of the protrusion is defined by a portion of a wall of the device lumen.

7. A delivery or removal device, comprising:

a. a robotic laparoscopic medical device comprising a first arm and second arm;

b. a tubular body having a proximal end and distal end, the tubular body comprising:

i. a device lumen defined by the inner surface wall of the tubular body, the device lumen being sized to receive the robotic laparoscopic medical device, the device lumen comprising a proximal device opening

- at a proximal end of the tubular body and a distal device opening at a distal end of the tubular body; and
 - ii. a wire lumen disposed within the wall of the tubular body, wherein the wire lumen is not coaxial with the device lumen, the wire lumen comprising a proximal wire opening at a proximal end of the tubular body wall and a distal wire opening at a distal end of the tubular body wall, wherein the wire lumen has a smaller diameter than the device lumen; and
 - e. a wire disposed within the wire lumen and device lumen so as to urge the robotic medical device comprising the first arm and second arm through the device lumen.
8. The device of claim 7, wherein the overtube is sized to be positionable through a laparoscopic port or natural orifice.
9. The device of claim 7, wherein the tubular body comprises a protrusion at a distal end of the tubular body, wherein the protrusion further defines the wire lumen.
10. The device of claim 7, wherein the robotic laparoscopic medical device comprising the first arm and second arm further comprises an attachment component disposed on at least one of the first arm or second arm.
11. The device of claim 7, wherein the robotic laparoscopic medical device comprising the first arm and second arm is in vivo device.
12. The device of claim 7, wherein the robotic laparoscopic medical device comprising the first arm and second arm further comprises at least one end effector.
13. The device of claim 12, wherein the at least one end effector is an attachment component.
14. The device of claim 7, wherein the tubular body comprises a protrusion at the distal end, wherein the protrusion further defines the wire lumen.
15. The device of claim 14, wherein the protrusion further comprises a robotic medical device receiving component configured to receive the robotic laparoscopic medical device comprising the first arm and a second arm.
16. The device of claim 15, wherein the medical device receiving component comprises at least one magnet configured to magnetically couple to the robotic medical device comprising the first arm and a second arm, whereby the

- robotic medical device comprising the first arm and a second arm releasably couples to the medical device receiving component.
17. A delivery or removal device for introducing a robotic laparoscopic medical device comprising a first arm and a second arm into a patient, comprising:
- a. a robotic laparoscopic medical device comprising a first arm and a second arm;
 - b. a tubular body having a proximal end and a distal end and comprising a protrusion at a distal end of the tubular body;
 - c. a device lumen coextensive with the inner surface of an interior wall of the tubular body, the device lumen being configured to receive the robotic laparoscopic medical device comprising a first arm and a second arm, wherein a portion of the protrusion is defined by a portion of a wall of the device lumen, wherein the device lumen comprises a proximal device opening at a proximal end of the tubular body and a distal device opening at a distal end of the tubular body;
 - d. a wire lumen disposed within the wall of the tubular body, the wire lumen comprising a proximal wire opening at a proximal end of the tubular body and a distal wire opening at a distal end of the tubular body, wherein the wire lumen has a smaller diameter than the device lumen; and
 - e. a moveable wire disposed through the device lumen and the wire lumen, the moveable wire comprising an attachment component disposed at or near an end of the moveable wire, wherein the attachment component is configured to be removably attachable to the robotic laparoscopic medical device comprising a first arm and a second arm.
18. The device of claim 17, wherein the tubular body is sized to be positionable through a laparoscopic port or natural orifice.
19. The device of claim 17, wherein the robotic laparoscopic medical device comprising the first arm and a second arm is in vivo device.
20. The device of claim 17, wherein the robotic laparoscopic medical device comprising the first arm and a second arm further comprises at least one end effector.

* * * * *

专利名称(译)	医疗通胀，附着和输送装置以及相关方法		
公开(公告)号	US10335024	公开(公告)日	2019-07-02
申请号	US15/018530	申请日	2016-02-08
申请(专利权)人(译)	板内布拉斯加大学校董		
当前申请(专利权)人(译)	板内布拉斯加大学校董		
[标]发明人	RENTSCHLER MARK FARRITOR SHANE		
发明人	RENTSCHLER, MARK FARRITOR, SHANE		
IPC分类号	A61M29/00 A61B34/00 A61B17/34 A61B17/02 A61B1/313 A61B17/00 A61B34/30 A61B1/32 A61B90/50		
CPC分类号	A61B1/3132 A61B17/0281 A61B17/3468 A61B34/30 A61B34/72 A61B34/73 A61B17/0218 A61B2034/302 A61B1/32 A61B90/50 A61B2017/0042 A61B2017/00283 A61B2017/00292 A61B2017/00345 A61B2017/00349 A61B2017/00557 A61B2017/00876 A61B2017/0225 A61B2034/301		
优先权	60/956032 2007-08-15 US 60/990062 2007-11-26 US 60/990470 2007-11-27 US		
其他公开文献	US20160157709A1		
外部链接	Espacenet		

摘要(译)

这里公开的各种实施例涉及程序空间维护设备，医疗设备定位设备，以及提供程序空间维护和设备定位的设备。进一步的实施例涉及医疗装置插入和/或缩回装置。

