



(11)

EP 3 616 631 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
04.03.2020 Bulletin 2020/10

(51) Int Cl.:
A61B 17/32^(2006.01)

(21) Application number: 19187882.6

(22) Date of filing: 10.03.2014

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR

(30) Priority: 15.03.2013 US 201313834248

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
14719402.1 / 2 967 626

(71) Applicant: Ethicon LLC
Guaynabo 00969 (PR)

(72) Inventors:

- MESSERLEY, Jeffrey D.
Cincinnati, OH Ohio 45244 (US)
- WITT, David A.
Maineville, OH Ohio 45039 (US)

- STULEN, Foster B.
Mason, OH Ohio 45040 (US)
- PAPA, Christopher A.
Cincinnati, OH Ohio 45242 (US)
- BATTAGLIA, Vincent P., Jr.
Lebanon, OH Ohio 45036 (US)

(74) Representative: Bettridge, Paul Sebastian
Carpmaels & Ransford LLP
One Southampton Row
London WC1B 5HA (GB)

Remarks:

- This application was filed on 230719 as a divisional application to the application mentioned under INID code 62.
- Claims filed after the date of receipt of the divisional application (Rule 68(4) EPC).

(54) ULTRASONIC SURGICAL SHEARS WITH CLAMPING FEATURE

(57) An apparatus for operating on tissue comprises a shaft, an acoustic waveguide, and an end effector. The acoustic waveguide extends along the shaft and is configured to transmit ultrasonic vibration. The end effector comprises an ultrasonic blade and a clamp arm. The ultrasonic blade is in acoustic communication with the acoustic waveguide. The clamp arm is pivotable toward

the ultrasonic blade. The end effector defines a first longitudinal region and a second longitudinal region. The end effector is configured to clamp tissue between the clamp arm and the ultrasonic blade in the first longitudinal region. The end effector is configured to sever tissue with the ultrasonic blade in the second longitudinal region.

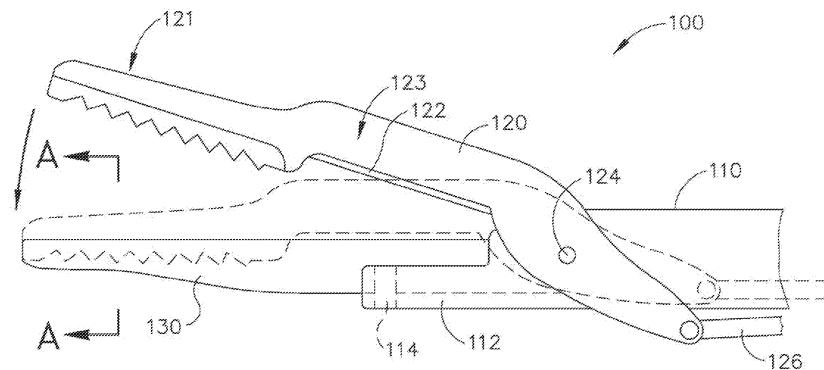


Fig.2

Description

BACKGROUND

[0001] A variety of surgical instruments include an end effector having a blade element that vibrates at ultrasonic frequencies to cut and/or seal tissue (e.g., by denaturing proteins in tissue cells). These instruments include piezoelectric elements that convert electrical power into ultrasonic vibrations, which are communicated along an acoustic waveguide to the blade element. Examples of such ultrasonic surgical instruments include the HARMONIC ACE® Ultrasonic Shears, the HARMONIC WAVE® Ultrasonic Shears, the HARMONIC FOCUS® Ultrasonic Shears, and the HARMONIC SYNERGY® Ultrasonic Blades, all by Ethicon Endo-Surgery, Inc. of Cincinnati, Ohio. Further examples of such devices and related concepts are disclosed in U.S. Pat. No. 5,322,055, entitled "Clamp Coagulator/Cutting System for Ultrasonic Surgical Instruments," issued June 21, 1994, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 5,873,873, entitled "Ultrasonic Clamp Coagulator Apparatus Having Improved Clamp Mechanism," issued February 23, 1999, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 5,980,510, entitled "Ultrasonic Clamp Coagulator Apparatus Having Improved Clamp Arm Pivot Mount," filed October 10, 1997, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 6,325,811, entitled "Blades with Functional Balance Asymmetries for use with Ultrasonic Surgical Instruments," issued December 4, 2001, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 6,783,524, entitled "Robotic Surgical Tool with Ultrasound Cauterizing and Cutting Instrument," issued August 31, 2004, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2006/0079874, entitled "Tissue Pad for Use with an Ultrasonic Surgical Instrument," published April 13, 2006, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2007/0191713, entitled "Ultrasonic Device for Cutting and Coagulating," published August 16, 2007, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2007/0282333, entitled "Ultrasonic Waveguide and Blade," published December 6, 2007, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2008/0200940, entitled "Ultrasonic Device for Cutting and Coagulating," published August 21, 2008, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2010/0069940, entitled "Ultrasonic Device for Fingertip Control," published March 18, 2010, the disclosure of which is incorporated by reference herein; and U.S. Pub. No. 2011/0015660, entitled "Rotating Transducer Mount for Ultrasonic Surgical Instruments," published January 20, 2011, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0029546, entitled "Ultrasonic Surgical Instrument Blades," published February 2, 2012, the disclosure of which is incorporated by

reference herein; U.S. Pat. App. No. 13/538,588, filed June 29, 2012, entitled "Surgical Instruments with Articulating Shafts," the disclosure of which is incorporated by reference herein; and U.S. Pat. App. No. 13/657,553, filed October 22, 2012, entitled "Flexible Harmonic Waveguides/Blades for Surgical Instruments," the disclosure of which is incorporated by reference herein.

[0002] Additionally, some of the foregoing surgical tools may include a cordless transducer such as that disclosed in U.S. Pub. No. 2012/0112687, entitled "Recharge System for Medical Devices," published May 10, 2012, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2012/0116265, entitled "Surgical Instrument with Charging Devices," published May 10, 2012, the disclosure of which is incorporated by reference herein; and/or U.S. Pat. App. No. 61/410,603, filed November 5, 2010, entitled "Energy-Based Surgical Instruments," the disclosure of which is incorporated by reference herein.

[0003] While several surgical instruments and systems have been made and used, it is believed that no one prior to the inventors has made or used the invention described in the appended claims.

25 BRIEF DESCRIPTION OF THE DRAWINGS

[0004] While the specification concludes with claims which particularly point out and distinctly claim this technology, it is believed this technology will be better understood from the following description of certain examples taken in conjunction with the accompanying drawings, in which like reference numerals identify the same elements and in which:

35 FIG. 1 depicts a side elevational view of an exemplary ultrasonic surgical instrument;

40 FIG. 2 depicts a partial side elevational view of an exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

45 FIG. 3 depicts a partial side elevational view of the end effector of FIG. 2, with a harmonic wave superimposed to show exemplary nodal positioning;

50 FIG. 4 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

55 FIG. 5 depicts an end view of an exemplary cross-sectional configuration of an end effector, taken along line A-A of FIG. 2, clamping tissue;

FIG. 6 depicts an end view of another exemplary cross-sectional configuration of an end effector, taken along line A-A of FIG. 2, clamping tissue;

FIG. 7 depicts an end view of another exemplary

cross-sectional configuration of an end effector, taken along line A-A of FIG. 2, clamping tissue;

FIG. 8 depicts an end view of another exemplary cross-sectional configuration of an end effector, taken along line A-A of FIG. 2, clamping tissue;

FIG. 9 depicts an end view of another exemplary cross-sectional configuration of an end effector, taken along line A-A of FIG. 2, clamping tissue;

FIG. 10 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

FIG. 11 depicts a cross-sectional view of the end effector of FIG. 10, taken along line 11-11 of FIG. 10;

FIG. 12 depicts a cross-sectional view of the end effector of FIG. 10, taken along line 12-12 of FIG. 10;

FIG. 13 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

FIG. 14 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

FIG. 15 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

FIG. 16 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

FIG. 17 depicts a partial side elevational view of the end effector of FIG. 16, with a harmonic wave superimposed to show exemplary nodal positioning;

FIG. 18 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1;

FIG. 19 depicts a partial side elevational view of an exemplary alternative ultrasonic blade suitable for incorporation in any of the end effectors referred to herein;

FIG. 20 depicts a partial side elevational view of another exemplary alternative ultrasonic blade suitable for incorporation in any of the end effectors referred to herein;

FIG. 21 depicts a partial top plan view of another exemplary alternative ultrasonic blade suitable for incorporation in any of the end effectors referred to

herein;

FIG. 22 depicts a partial side elevational view of the ultrasonic blade of FIG. 21;

FIG. 23 depicts a partial top plan view of another exemplary alternative ultrasonic blade suitable for incorporation in any of the end effectors referred to herein;

FIG. 24 depicts a partial side elevational view of the ultrasonic blade of FIG. 23;

FIG. 25 depicts a partial top plan view of another exemplary alternative ultrasonic blade suitable for incorporation in any of the end effectors referred to herein;

FIG. 26 depicts a partial top plan view of another exemplary alternative ultrasonic blade suitable for incorporation in any of the end effectors referred to herein;

FIG. 27 depicts a partial side elevational view of another exemplary alternative end effector suitable for incorporation in the instrument of FIG. 1, with a clamp arm in an open position and with an ultrasonic blade in a home position in relation to a tube extension pad;

FIG. 28 depicts a partial side elevational view of the end effector of FIG. 27, with the clamp arm in a closed position and with the ultrasonic blade deflected into engagement with the tube extension pad;

FIG. 29 depicts a partial side elevational view of the end effector of FIG. 27, with the clamp arm in an open position and with the ultrasonic blade deflected further away from the tube extension pad;

FIG. 30 depicts a front elevational view of the end effector of FIG. 27, with the features positioned as shown in FIG. 27;

FIG. 31 depicts a front elevational view of the end effector of FIG. 27, with the features positioned as shown in FIG. 28; and

FIG. 32 depicts a front elevational view of the end effector of FIG. 27, with the features positioned as shown in FIG. 29.

[0005] The drawings are not intended to be limiting in any way, and it is contemplated that various embodiments of the technology may be carried out in a variety of other ways, including those not necessarily depicted in the drawings. The accompanying drawings incorporated in and forming a part of the specification illustrate several aspects of the present technology, and together

with the description serve to explain the principles of the technology; it being understood, however, that this technology is not limited to the precise arrangements shown.

DETAILED DESCRIPTION

[0006] The following description of certain examples of the technology should not be used to limit its scope. Other examples, features, aspects, embodiments, and advantages of the technology will become apparent to those skilled in the art from the following description, which is by way of illustration, one of the best modes contemplated for carrying out the technology. As will be realized, the technology described herein is capable of other different and obvious aspects, all without departing from the technology. Accordingly, the drawings and descriptions should be regarded as illustrative in nature and not restrictive.

[0007] It is further understood that any one or more of the teachings, expressions, embodiments, examples, etc. described herein may be combined with any one or more of the other teachings, expressions, embodiments, examples, etc. that are described herein. The following-described teachings, expressions, embodiments, examples, etc. should therefore not be viewed in isolation relative to each other. Various suitable ways in which the teachings herein may be combined will be readily apparent to those of ordinary skill in the art in view of the teachings herein. Such modifications and variations are intended to be included within the scope of the claims.

[0008] For clarity of disclosure, the terms "proximal" and "distal" are defined herein relative to a robotic surgical driver comprising a proximal housing having an interface that mechanically and electrically couples with a surgical instrument having a distal surgical end effector. The term "proximal" refers to the position of an element closer to the robotic surgical driver housing and the term "distal" refers to the position of an element closer to the surgical end effector of the surgical instrument and further away from the housing.

I. Exemplary Ultrasonic Surgical Instrument

[0009] FIG. 1 illustrates an exemplary ultrasonic surgical instrument (10). At least part of instrument (10) may be constructed and operable in accordance with at least some of the teachings of U.S. Pat. No. 5,322,055; U.S. Pat. No. 5,873,873; U.S. Pat. No. 5,980,510; U.S. Pat. No. 6,325,811; U.S. Pat. No. 6,783,524; U.S. Pub. No. 2006/0079874; U.S. Pub. No. 2007/0191713; U.S. Pub. No. 2007/0282333; U.S. Pub. No. 2008/0200940; U.S. Pub. No. 2010/0069940; U.S. Pub. No. 2011/0015660; U.S. Pub. No. 2012/0112687; U.S. Pub. No. 2012/0116265; U.S. Pat. App. No. 13/538,588; U.S. Pat. App. No. 13/657,553; and/or U.S. Pat. App. No. 61/410,603. The disclosures of each of the foregoing patents, publications, and applications are incorporated by reference herein. As described therein and as will be de-

scribed in greater detail below, instrument (10) is operable to cut tissue and seal or weld tissue (e.g., a blood vessel, etc.) substantially simultaneously. In other words, instrument (10) operates similar to an endocutter type of stapler, except that instrument (10) provides tissue welding through application of ultrasonic vibrational energy instead of providing lines of staples to join tissue. This same ultrasonic vibrational energy also separates tissue similar to severing of tissue by a translating knife member. It should also be understood that instrument (10) may have various structural and functional similarities with the HARMONIC ACE® Ultrasonic Shears, the HARMONIC WAVE® Ultrasonic Shears, the HARMONIC FOCUS® Ultrasonic Shears, and/or the HARMONIC SYNERGY® Ultrasonic Blades. Furthermore, instrument (10) may have various structural and functional similarities with the devices taught in any of the other references that are cited and incorporated by reference herein.

[0010] To the extent that there is some degree of overlap between the teachings of the references cited herein, the HARMONIC ACE® Ultrasonic Shears, the HARMONIC WAVE® Ultrasonic Shears, the HARMONIC FOCUS® Ultrasonic Shears, and/or the HARMONIC SYNERGY® Ultrasonic Blades, and the following teachings relating to instrument (10), there is no intent for any of the description herein to be presumed as admitted prior art. Several teachings herein will in fact go beyond the scope of the teachings of the references cited herein and the HARMONIC ACE® Ultrasonic Shears, the HARMONIC WAVE® Ultrasonic Shears, the HARMONIC FOCUS® Ultrasonic Shears, and the HARMONIC SYNERGY® Ultrasonic Blades.

[0011] Instrument (10) of the present example comprises a handpiece (20), a shaft assembly (30), and an end effector (40). Handpiece (20) comprises a body (22) including a finger grip (24) and a pair of buttons (26). Handpiece (20) also includes a trigger (28) that is pivotable toward and away from body (22). Trigger (28) and finger grip (24) together provide a scissor grip type of configuration. It should be understood, however, that various other suitable configurations may be used, including but not limited to a pistol grip configuration. End effector (40) includes an ultrasonic blade (42) and a pivoting clamp arm (44). Clamp arm (44) is coupled with trigger (28) such that clamp arm (44) is pivotable toward ultrasonic blade (42) in response to pivoting of trigger (28) toward body (22); and such that clamp arm (44) is pivotable away from ultrasonic blade (42) in response to pivoting of trigger (28) away from body (22). Various suitable ways in which clamp arm (44) may be coupled with trigger (28) will be apparent to those of ordinary skill in the art in view of the teachings herein. In some versions, one or more resilient members are used to bias clamp arm (44) and/or trigger (28) to the open position shown in FIG. 1.

[0012] An ultrasonic transducer assembly (12) extends proximally from body (22) of handpiece (20). Transducer assembly (12) is coupled with a generator (16) via a cable (14). Transducer assembly (12) receives electrical power

from generator (16) and converts that power into ultrasonic vibrations through piezoelectric principles. Generator (16) may include a power source and control module that is configured to provide a power profile to transducer assembly (12) that is particularly suited for the generation of ultrasonic vibrations through transducer assembly (12). By way of example only, generator (16) may comprise a GEN 300 sold by Ethicon Endo-Surgery, Inc. of Cincinnati, Ohio. In addition or in the alternative, generator (16) may be constructed in accordance with at least some of the teachings of U.S. Pub. No. 2011/0087212, entitled "Surgical Generator for Ultrasonic and Electrosurgical Devices," published April 14, 2011, the disclosure of which is incorporated by reference herein. It should also be understood that at least some of the functionality of generator (16) may be integrated into handpiece (20), and that handpiece (20) may even include a battery or other on-board power source such that cable (14) is omitted. Still other suitable forms that generator (16) may take, as well as various features and operabilities that generator (300) may provide, will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0013] Ultrasonic vibrations that are generated by transducer assembly (12) are communicated along an acoustic waveguide (not shown), which extends through shaft assembly (30) to reach ultrasonic blade (42). Blade (42) is thus operable to effectively cut through and seal tissue, particularly when the tissue is being clamped between clamp arm (44) and blade (42). It should be understood that the waveguide may be configured to amplify mechanical vibrations transmitted through the waveguide. Furthermore, either the waveguide may include features operable to control the gain of the longitudinal vibrations along the waveguide and/or features to tune the waveguide to the resonant frequency of the system. Buttons (26) are operable to selectively activate transducer assembly (12), to thereby activate ultrasonic blade (42). In the present example, two buttons (26) are provided - one for activating ultrasonic blade (42) at a low power and another for activating ultrasonic blade (42) at a high power. However, it should be understood that any other suitable number of buttons and/or otherwise selectable power levels may be provided.

[0014] In the present example, the distal end of ultrasonic blade (42) is located at a position corresponding to an anti-node associated with resonant ultrasonic vibrations communicated through the waveguide, in order to tune the acoustic assembly to a preferred resonant frequency f_o when the acoustic assembly is not loaded by tissue. When transducer assembly (12) is energized, the distal end of ultrasonic blade (42) is configured to move longitudinally in the range of, for example, approximately 10 to 500 microns peak-to-peak, and in some instances in the range of about 20 to about 200 microns at a predetermined vibratory frequency f_o of, for example, 55.5 kHz. When transducer assembly (12) of the present example is activated, these mechanical oscillations are

transmitted through the waveguide to reach ultrasonic blade (42), thereby providing oscillation of ultrasonic blade (42) at the resonant ultrasonic frequency. Thus, when tissue is secured between ultrasonic blade (42) and clamp arm (44), the ultrasonic oscillation of ultrasonic blade (42) may simultaneously sever the tissue and denature the proteins in adjacent tissue cells, thereby providing a coagulative effect with relatively little thermal spread. In some versions, an electrical current may also be provided through ultrasonic blade (42) and clamp arm (44) to also cauterize the tissue. While some configurations for an acoustic transmission assembly and transducer assembly (12) have been described, still other suitable configurations for an acoustic transmission assembly and transducer assembly (12) will be apparent to one or ordinary skill in the art in view of the teachings herein. Similarly, other suitable configurations for end effector (40) will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0015] In the present example, shaft assembly (30) is configured to selectively couple with transducer assembly (12). To assist in proper coupling, a torque wrench (32) is included about shaft assembly (30). Torque wrench (32) is configured to facilitate gripping of shaft assembly (30) as shaft assembly (30) is rotated relative to transducer assembly (12) during coupling. In addition, torque wrench (32) is configured to provide audible and/or tactile feedback once the appropriate amount of torque as been achieved to provide a coupling of transducer assembly (12) and shaft assembly (30) at the appropriate tightness. For instance, torque wrench (32) may provide a pair of audible and tactile clicks once the appropriate level of torque/tightness has been achieved. Other variations of torque wrench (32) will be apparent to those of ordinary skill in the art in view of the teachings herein. Furthermore, it should be understood that torque wrench (32) may simply be omitted, if desired.

[0016] In some versions, shaft assembly (30) includes an articulation section enabling end effector (40) to be angularly deflected laterally away from the longitudinal axis defined by shaft assembly (30). By way of example only, such an articulation section may be configured in accordance with one or more teachings of U.S. Pub. No. 2012/0078247, the disclosure of which is incorporated by reference herein. As another merely illustrative example, such an articulation section may be configured in accordance with one or more teachings of U.S. Pat. App. No. 13/538,588 and/or U.S. Pat. App. No. 13/657,553, the disclosures of which are incorporated by reference herein. Of course, some versions of shaft assembly (30) may simply lack articulation altogether.

[0017] The foregoing components and operabilities of instrument (10) are merely illustrative. Instrument (10) may be configured in numerous other ways as will be apparent to those of ordinary skill in the art in view of the teachings herein. By way of example only, at least part of instrument (10) may be constructed and/or operable in accordance with at least some of the teachings of any

of the following, the disclosures of which are all incorporated by reference herein: U.S. Pat. No. 5,322,055; U.S. Pat. No. 5,873,873; U.S. Pat. No. 5,980,510; U.S. Pat. No. 6,325,811; U.S. Pat. No. 6,783,524; U.S. Pub. No. 2006/0079874; U.S. Pub. No. 2007/0191713; U.S. Pub. No. 2007/0282333; U.S. Pub. No. 2008/0200940; U.S. Pub. No. 2010/0069940; U.S. Pub. No. 2011/0015660; U.S. Pub. No. 2012/0112687; U.S. Pub. No. 2012/0116265; U.S. Pat. App. No. 13/538,588; and/or U.S. Pat. App. No. 13/657,553. Additional variations for instrument (10) will be described in greater detail below. It should be understood that the below described variations may be readily applied to any of the instruments referred to in any of the references that are cited herein, among others.

II. Exemplary Alternative Ultrasonic End Effector with Dual Modes

[0018] In some instances, the operation of an ultrasonic surgical instrument provides tradeoffs between tissue cutting speed and tissue sealing effectiveness. For instance, the region of an ultrasonic blade closest to an anti-node associated with resonant ultrasonic vibrations communicated through the blade may provide the fastest tissue cutting speed; yet may be less effective at sealing tissue (e.g., particularly thick tissue). The region of an ultrasonic blade closest to a node associated with resonant ultrasonic vibrations communicated through the blade may provide the most effective tissue sealing (e.g., particularly thick tissue) by providing a uniform pressure profile and a uniform displacement profile; yet may provide a relatively slow tissue cutting speed. It may therefore be desirable to facilitate easy selection between these capabilities through a single variation of instrument (10). This may be done by establishing clearly demarcated regions in an end effector to enable the operator to readily recognize and select from the appropriate blade regions based on the particular surgical task and context at hand. Merely illustrative examples of such end effectors are shown in FIGS. 2-12 and are described in greater detail below; while other variations will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0019] In the examples described below, an end effector provides a first region that is more effective for sealing tissue (e.g., through clamping between a clamp pad and an ultrasonic blade); and a second region that is more effective for cutting tissue (e.g., through a shearing action between a clamp arm and the ultrasonic blade). It should be understood, however, that the first region may still effectively cut tissue and the second region may still effectively seal tissue. In these examples, the separate regions are provided through different clamp arm configurations, while the configuration of the ultrasonic blade does not change between the separate regions. In some other versions, however, the configuration of the ultrasonic blade may in fact change between the separate

regions. In either case, the ultrasonic blade may be viewed as having a working/active length that extends along both regions. In other words, the working/active length of the ultrasonic blade may be defined as the length of the first region plus the length of the second region. In some versions, the working length is approximately 4 cm. Alternatively, any other suitable working/active length may be provided.

[0020] FIG. 2 shows an exemplary alternative end effector (100) that may be used in place of end effector (40) described above, such that end effector (100) may be readily incorporated into instrument (10). End effector (100) of this example comprises a clamp arm (120) and an ultrasonic blade (130). Ultrasonic blade (130) is substantially similar to ultrasonic blade (42) described above. Clamp arm (120) is pivotally coupled with an outer tube (110) at a pivot coupling (124). Outer tube (110) may be provided as a component of shaft assembly (30). A rod (126) is pivotally coupled with clamp arm (120) and is translatable to selectively pivot clamp arm (120) toward and away from ultrasonic blade (130). Rod (126) may be actuated by trigger (28) and/or any other suitable user input feature. Rod (126) may also be substituted with a cable, beam, and/or any other suitable structure. Various other ways in which clamp arm (120) may be actuated to selectively pivot toward and away from ultrasonic blade (130) will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0021] Outer tube (110) includes a distally projecting tongue (112), which further includes a blade support (114). Blade support (114) comprises a pad that engages ultrasonic blade (130) at a position corresponding to a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (130). This is illustrated in FIG. 3, which shows a wave (W) depicting the resonant ultrasonic vibrations communicated through ultrasonic blade (130), with a node (N) being at the same longitudinal position as blade support (114). The rest of tongue (112) does not contact ultrasonic blade (130); yet tongue (112) extends around a substantial portion of the underside exterior of ultrasonic blade (130). Tongue (112) thus serves as a partial shield, preventing tissue from contacting the shielded portion of ultrasonic blade (130).

[0022] Clamp arm (120) includes a fast cutting region (121) and a slow cutting region (123), which is proximal to fast cutting region (121). In the present example, fast cutting region (121) is more effective for cutting tissue (through a shearing action); while slow cutting region (123) is more effective for sealing tissue (through a clamping action). Slow cutting region (123) includes a tissue pad (122), which extends along the full length of slow cutting region (123) and thus serves to demarcate slow cutting region (123). By way of example only, tissue pad (122) may comprise polytetrafluoroethylene and/or any other suitable material(s); and/or may be configured in accordance with at least some of the teachings of U.S. Pub. No. 2006/0079874, the disclosure of which is incor-

porated by reference herein. In the present example, tissue pad (122) is configured such that tissue will be clamped along a horizontal plane between tissue pad (122) and ultrasonic blade (130), without pad (122) or blade (130) passing through that horizontal plane. However, and as will be described in greater detail below in reference to FIGS. 5-9, fast cutting region (121) is configured such that tissue will be clamped obliquely between fast cutting region (121) and ultrasonic blade (130), with fast cutting region and ultrasonic blade (130) passing through the same horizontal plane in a cross-bite type of arrangement to provide oblique shearing of tissue.

[0023] As can be seen in FIG. 2, blade support (114) is at a longitudinal position corresponding to the longitudinal center of slow cutting region (123) when clamp arm (120) is pivoted to a closed position against ultrasonic blade (130). It should therefore be understood that slow cutting region (123) is centered about a node (N) associated with resonant ultrasonic vibrations communicated through ultrasonic blade (130). In some other versions, the node (N) is proximal to slow cutting region. For instance, the node (N) may be located proximal to pivotal coupling (124). As yet another merely illustrative variation, a first node (N) may be located at the proximal end of slow cutting region (123), with a second node (N) being located at the distal end of slow cutting region (123) (i.e., at the transition between regions (121, 123)).

[0024] In the present example, and as best seen in FIG. 3, the distal tip of ultrasonic blade (130) is located at a longitudinal position corresponding to an anti-node (AN) associated with resonant ultrasonic vibrations communicated through ultrasonic blade (130). Clamp arm (120) distally terminates at approximately the same longitudinal position as ultrasonic blade (130) when clamp arm (120) is pivoted to a closed position against ultrasonic blade (130). It should therefore be understood that fast cutting region (121) is located in a region closest to anti-node (AN) associated with resonant ultrasonic vibrations communicated through ultrasonic blade (130). When using end effector (100) to sever and seal tissue, the operator may position the tissue between slow cutting region (123) and ultrasonic blade (130) if the tissue is relatively thick; or between fast cutting region (121) and ultrasonic blade (130) if the tissue is relatively thin and the operator wishes to provide a relatively fast cutting speed.

[0025] FIG. 4 shows another exemplary alternative end effector (200) that may be used in place of end effector (40) described above, such that end effector (200) may be readily incorporated into instrument (10). End effector (200) of this example comprises a clamp arm (220) and an ultrasonic blade (230). Ultrasonic blade (230) is substantially similar to ultrasonic blades (42, 130) described above. Clamp arm (220) is substantially similar to clamp arm (120) described above. In particular, clamp arm (220) includes a fast cutting region (221), a slow cutting region (223), a tissue pad (222), a pivotal coupling

(224), and a rod (226). These components are substantially similar to fast cutting region (121), slow cutting region (123), tissue pad (122), pivotal coupling (124), and rod (126), respectively, as described above. Outer tube (210) of this example is also similar to outer tube (110) described above, except that tongue (212) of outer tube (210) projects further distally than tongue (112) of outer tube (110). In particular, tongue (212) extends to a longitudinal position corresponding to the distal tip of ultrasonic blade (230). This simply provides additional shielding to the underside of ultrasonic blade (230). Tongue (212) also includes a blade support (214), though this is substantially similar to blade support (113) described above. In some instances, at least part of tongue (212) is configured in accordance with at least some of the teachings of U.S. Pub. No. 2012/0029546, the disclosure of which is incorporated by reference herein.

[0026] FIGS. 5-9 show exemplary alternative forms that the fast cutting sections (121, 221) of end effectors (100, 200) may take. In particular, FIG. 5 shows a clamp arm (300) and ultrasonic blade (310) clamping tissue (2) along a non-horizontal path. Clamp arm (300) and ultrasonic blade (310) are not centered along a common vertical axis in this example; yet they pass through a common horizontal plane in this example. Clamp arm (300) includes a substantially vertical portion (302) and a substantially transverse portion (304), which projects laterally to cross a vertical plane that is interposed between vertical portion (302) and ultrasonic blade (310). Transverse portion (304) is positioned above substantially vertical portion (302) in this example. Ultrasonic blade (310) has a substantially vertical face (312) and a rounded face (314), such that ultrasonic blade (310) has a reverse D-shaped cross-sectional profile. When tissue (2) is clamped between clamp arm (300) and ultrasonic blade (310), tissue (2) is captured between substantially vertical portion (302) of clamp arm (300) and substantially vertical face (312) of ultrasonic blade (310). Tissue (2) is also captured between substantially transverse portion (304) of clamp arm (300) and the upper region of rounded face (314). Clamp arm (300) and ultrasonic blade (310) may cooperate to provide a shearing action against tissue (2) as clamp arm (300) is pivoted toward ultrasonic blade (310).

[0027] FIG. 6 shows another clamp arm (320) and ultrasonic blade (330) clamping tissue (2) along a non-horizontal path. Clamp arm (320) and ultrasonic blade (330) are not centered along a common vertical axis in this example; yet they pass through a common horizontal plane in this example. Clamp arm (320) includes a substantially vertical portion (322) and a substantially transverse portion (324), which projects laterally to cross a vertical plane that is interposed between vertical portion (322) and ultrasonic blade (330). Transverse portion (324) is positioned below substantially vertical portion (322) in this example. Ultrasonic blade (330) has a substantially vertical face (332), a substantially horizontal face (334), and an oblique face (336), such that ultrasonic

blade (330) has a cross-sectional profile similar to a right triangle. When tissue (2) is clamped between clamp arm (320) and ultrasonic blade (330), tissue (2) is captured between transverse portion (324) of clamp arm (320) and oblique face (336) of ultrasonic blade (330). Clamp arm (320) and ultrasonic blade (330) may cooperate to provide a shearing action against tissue (2) as clamp arm (320) is pivoted toward ultrasonic blade (330).

[0028] FIG. 7 shows another clamp arm (340) and ultrasonic blade (350) clamping tissue (2), this time along a horizontal path. Clamp arm (340) and ultrasonic blade (350) are both centered along a common vertical axis in this example. Clamp arm (340) includes a tissue pad (342) similar to tissue pads (122, 222) described above. Tissue pad (342) is positioned below clamp arm (340) such that tissue pad (342) includes a downwardly presented surface. Clamp arm (340) and tissue pad (342) together define a generally elliptical cross-sectional profile. Ultrasonic blade (350) has a generally rectangular cross-sectional profile, with a notch (352) extending along a lower corner. When tissue (2) is clamped between clamp arm (340) and ultrasonic blade (350), tissue (2) is captured between tissue pad (342) and the upper surface of ultrasonic blade (350).

[0029] FIG. 8 shows another clamp arm (360) and ultrasonic blade (370) clamping tissue (2) along a non-horizontal path. Clamp arm (360) and ultrasonic blade (370) are not centered along a common vertical axis in this example; yet they pass through a common horizontal plane in this example. Clamp arm (360) includes a tissue pad (362) similar to tissue pads (122, 222) described above. Tissue pad (362) is positioned on a lateral side of clamp arm (360), such that tissue pad (362) presents an oblique exposed contact surface associated with the lower left-hand quadrant of clamp arm (360). Ultrasonic blade (370) includes a rounded surface (372) and an oblique surface (374), such that ultrasonic blade (370) has an angled D-shaped cross-sectional profile. When tissue (2) is clamped between clamp arm (360) and ultrasonic blade (370), tissue (2) is captured between the oblique exposed surface of tissue pad (362) and oblique surface (374) of ultrasonic blade (370). Clamp arm (360) and ultrasonic blade (370) may cooperate to provide a shearing action against tissue (2) as clamp arm (360) is pivoted toward ultrasonic blade (370).

[0030] FIG. 9 shows another clamp arm (380) and ultrasonic blade (390) clamping tissue (2) along a non-horizontal path. Clamp arm (380) and ultrasonic blade (390) are not centered along a common vertical axis in this example; yet they pass through a common horizontal plane in this example. Clamp arm (380) includes a spine portion (382) and a pad sleeve (384) encompassing spine portion (382). Clamp arm (380) has a generally round cross-sectional configuration. Ultrasonic blade (390) has a generally rectangular cross-sectional configuration. When tissue (2) is clamped between clamp arm (380) and ultrasonic blade (390), tissue (2) is captured between an upper corner of ultrasonic blade (390) and

clamp arm (380). Clamp arm (380) and ultrasonic blade (390) may cooperate to provide a shearing action against tissue (2) as clamp arm (380) is pivoted toward ultrasonic blade (390).

[0031] While FIGS. 5-9 have been described above as showing exemplary alternative forms that the fast cutting sections (121, 221) of end effectors (100, 200) may take, it should be understood that slow cutting sections (123, 223) of end effectors (100, 200) may also take any of the various forms shown in FIGS. 5-9. Furthermore, the forms shown FIGS. 4-9 may be readily varied in numerous ways. Other suitable configurations for fast cutting sections (121, 221) and/or slow cutting sections (123, 223) will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0032] FIGS. 10-12 show yet another exemplary alternative end effector (1200) that may be used in place of end effector (40) described above, such that end effector (1200) may be readily incorporated into instrument (10).

End effector (1200) of this example comprises an outer tube (1210), a pivoting clamp arm (1220), and an ultrasonic blade (1230). Ultrasonic blade (1230) is substantially similar to ultrasonic blades (42, 130) described above. Clamp arm (1220) is substantially similar to clamp arm (120) described above. In particular, clamp arm (1220) includes a fast cutting region (1221), a slow cutting region (1223), a tissue pad (1222), and a pivotal coupling (1224). However, in this example the longitudinal positioning of fast cutting region (1221) and a slow cutting region (1223) is reversed compared to the longitudinal positioning of fast cutting region (121) and a slow cutting region (123). In particular, fast cutting region (1221) is positioned proximal to slow cutting region (1223) in this example. This may provide a configuration that is roughly similar to the configuration provided by a Foster-Gilles needle holder. The configuration may thus provide some degree of familiarity to some operators.

[0033] As shown in FIG. 11, the portion of clamp arm (1220) extending through slow cutting region (1223) is substantially flat and generally symmetric about a vertical plane that extends along the longitudinal axis of end effector (1200). Tissue pad (1222) is fitted in clamp arm (1220) by a rail (1223), though it should be understood that numerous other relationships may be used. By way of example only, tissue pad (1222) may comprise polytetrafluoroethylene and/or any other suitable material(s); and/or may be configured in accordance with at least some of the teachings of U.S. Pub. No. 2006/0079874, the disclosure of which is incorporated by reference herein. In the present example, tissue pad (1222) is configured such that tissue will be clamped along a horizontal plane between tissue pad (1222) and ultrasonic blade (1230), without pad (1222) or blade (1230) passing through that horizontal plane.

[0034] As shown in FIG. 12, the portion of clamp arm (1220) extending through fast cutting region (1221) is generally L-shaped and asymmetric about a vertical plane that extends along the longitudinal axis of end effector (1200).

factor (1200). In particular, this portion of clamp arm (1220) includes a horizontally extending portion (1230) positioned above ultrasonic blade (1230) and a vertically extending portion (1240) positioned lateral to ultrasonic blade (1230). Horizontally extending portion (1230) crosses over a vertical plane that extends along the longitudinal axis of end effector (1200); while vertically extending portion (1240) is positioned lateral to that same vertical plane. When tissue is clamped between the portion of clamp arm (1220) extending through fast cutting region (1221) and ultrasonic blade (1230), clamp arm (1220) and ultrasonic blade (1230) may cooperate to provide a shearing action against the tissue as clamp arm (1220) is pivoted toward ultrasonic blade (1230).

[0035] Ultrasonic blade (1230) is coupled with outer tube (1210) at a blade support (1214) located proximal to pivotal coupling (1224). Blade support (1214) is at a longitudinal position corresponding to a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (1230). In the present example, the distal end of end effector (1200) terminates at a longitudinal position corresponding to an anti-node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (1230). In some versions, there are no nodes positioned anywhere along the length of ultrasonic blade (1230) between blade support (1214) and the distal tip of end effector (1200). In some other versions, clamp arm (1220) is configured such that a node is located at the transition between fast cutting region (1221) and slow cutting region (1223), in addition to having a separate node at blade support (1214). As yet another merely illustrative example, clamp arm (1220) may be configured such that a node is located at the center of slow cutting region (1223), in addition to having a separate node at blade support (1214). Still other suitable configurations and relationships between features of end effector (1200) and the waveform of resonant ultrasonic vibrations communicated through ultrasonic blade (1230) will be apparent to those of ordinary skill in the art in view of the teachings herein.

III. Exemplary Alternative Ultrasonic End Effector with Heat Generating Pad Insert

[0036] It should be understood that the degree of longitudinal displacement in an ultrasonically vibrating blade will vary along the length of the blade, with the displacement being the greatest at a position corresponding to an anti-node; and with the displacement being reduced to zero at a position corresponding to a node. The active length of an ultrasonic blade, such as ultrasonic blade (42), may be defined from the distal tip of the blade (which may be associated with an anti-node) to the point on the blade where the longitudinal displacement (through ultrasonic vibrations) decreases to 50%. This active length may represent a length corresponding to less than a quarter of a wavelength associated with ultrasonic vibrations being communicated along the blade. Thus, the region

of length around a position corresponding to a node associated with ultrasonic vibrations being communicated long the blade may be viewed as an acoustic cold spot or a nodal gap where it is difficult for the blade to quickly develop heat to cut and coagulate tissue. It may therefore be desirable to avoid such cold spots (i.e., bridge the nodal gap), to thereby effectively extend the active length of the ultrasonic blade. Merely illustrative examples of end effectors that effectively extend the effective length of an ultrasonic blade are shown in FIGS. 13-15 and are described in greater detail below; while other variations will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0037] At least some of the examples described below rely on the property of absolute or dynamic viscosity, which is observed in a mechanical system where a moving plate slides across a stationary plate with a lubricant between the two. The value for absolute viscosity can be expressed as $\eta = Fh/Av$; where η is the absolute viscosity; F is the friction force between the moving plate and the lubricant; h is the distance between the moving plate and the stationary plate; A is the contact area between the moving plate and the lubricant; and v is the velocity of the moving plate. The temperature increase between the two plates is a function of the absolute viscosity η . In the context of an ultrasonic surgical instrument (10), ultrasonic blade (42) may serve as the moving plate, clamp arm (40) may serve as the stationary plate, and the tissue between blade (42) and arm (40) may serve as the lubricant. The nodal gap could be bridged by keeping absolute viscosity η constant along the desired working length of ultrasonic blade (42), thereby keeping a substantially constant temperature along the desired working length of ultrasonic blade (42) to effectively eliminate what would otherwise be an acoustic cold spot. In a conventional version of instrument (10), the velocity v decreases in the nodal gap associated with the acoustic cold spot referred to above. Thus, in order to maintain a constant absolute viscosity η across the nodal gap (to thereby eliminate the acoustic cold spot and provide uniform heating of tissue), it may be desirable to affect one or more of the other variables to effectively compensate for the reduction in velocity v . One or more of the examples described below may effectively compensate for the reduction in velocity v by effectively increasing the contact area A as described below. One or more of the examples described below may effectively compensate for the reduction in velocity v by effectively decreasing the tissue height as described below. One or more of the examples described below may effectively compensate for the reduction in velocity v by increasing the friction F by increasing the coefficient of friction in the tissue pad at the nodal region.

[0038] FIG. 13 shows an exemplary alternative end effector (400) that may be used in place of end effector (40) described above, such that end effector (400) may be readily incorporated into instrument (10). End effector (400) of this example comprises an ultrasonic blade (420)

extending distally from a shaft assembly (410). Ultrasonic blade (420) and shaft assembly (410) are substantially identical to ultrasonic blade (42) and shaft assembly (30) described above. End effector (400) also includes a clamp arm (430), which is selectively pivotable toward and away from ultrasonic blade (420) similar to clamp arm (44) described above. Clamp arm (430) includes a metallic arm (432) section, a pair of polytetrafluoroethylene pads (434), and a polyimide pad (436) positioned between polytetrafluoroethylene pads (434). Polyimide pad (436) is located at a position along clamp arm (430) that corresponds to the location (422) of a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (420). Polyimide is provided as an exemplary material for pad (436) because polyimide has a higher melting temperature and higher coefficient of friction than polytetrafluoroethylene. It should be understood, however, that numerous other suitable materials may be used for pad (436), including any suitable material that has a higher melting temperature and/or higher coefficient of friction than polytetrafluoroethylene.

[0039] Due to the differences in the material properties of polytetrafluoroethylene and polyimide, polyimide pad (436) may tend to generate higher heat when forced against an active ultrasonic blade (420). Thus, when tissue is clamped between clamp arm (430) and ultrasonic blade (420), and ultrasonic blade (420) is activated, the ultrasonic vibrations communicated by blade (420) immediately adjacent to the nodal location (422) may be more effectively carried by polyimide pad (436) than they would otherwise be carried by a polytetrafluoroethylene pad that would otherwise extend across the nodal location (422). In other words, due to the material properties and location of polyimide pad (436), polyimide pad (436) may effectively bridge the nodal gap and effectively eliminate the acoustic cold spot by providing substantially constant heating along the length of clamp arm (430).

[0040] FIG. 14 shows another exemplary alternative end effector (500) that may be used in place of end effector (40) described above, such that end effector (500) may be readily incorporated into instrument (10). End effector (500) of this example comprises an ultrasonic blade (520) extending distally from a shaft assembly (510). Ultrasonic blade (520) and shaft assembly (510) are substantially identical to ultrasonic blade (42) and shaft assembly (30) described above. End effector (500) also includes a clamp arm (530), which is selectively pivotable toward and away from ultrasonic blade (520) similar to clamp arm (44) described above. Clamp arm (530) includes a metallic arm section (532), a polytetrafluoroethylene pad (534), and a polyimide pad (536) positioned on polytetrafluoroethylene pad (534). Polyimide pad (536) is located at a position along clamp arm (530) that corresponds to the location (522) of a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (520). Polyimide is provided as an exemplary material for pad (536) because polyimide has a higher melting temperature and higher coefficient

of friction than polytetrafluoroethylene. It should be understood, however, that numerous other suitable materials may be used for pad (536), including any suitable material that has a higher melting temperature and/or higher coefficient of friction than polytetrafluoroethylene.

[0041] The configuration of clamp arm (530) is similar to the configuration of clamp arm (530) as described above, such that the material properties and location of polyimide pad (536) may result in polyimide pad (536) effectively bridging the nodal gap and effectively eliminating an acoustic cold spot by providing substantially constant heating along the length of clamp arm (530). However, in this example, polyimide pad (536) is raised relative to polytetrafluoroethylene pad (534). This creates additional interference against tissue when tissue is clamped between clamp arm (530) and ultrasonic blade (520). This additional interference may provide enhanced heating of the tissue, thereby further bridging the nodal gap.

[0042] FIG. 15 shows another exemplary alternative end effector (600) that may be used in place of end effector (40) described above, such that end effector (600) may be readily incorporated into instrument (10). End effector (600) of this example comprises an ultrasonic blade (620) extending distally from a shaft assembly (610). Ultrasonic blade (620) and shaft assembly (610) are substantially identical to ultrasonic blade (42) and shaft assembly (30) described above. End effector (600) also includes a clamp arm (630), which is selectively pivotable toward and away from ultrasonic blade (620) similar to clamp arm (44) described above. Clamp arm (630) includes a metallic arm (632) section, a pair of polytetrafluoroethylene pads (634), and a polyimide pad (636) positioned between polytetrafluoroethylene pads (634). Polyimide pad (636) is located at a position along clamp arm (630) that is slightly offset from the location (622) of a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (620). Polyimide is provided as an exemplary material for pad (636) because polyimide has a higher melting temperature and higher coefficient of friction than polytetrafluoroethylene. It should be understood, however, that numerous other suitable materials may be used for pad (636), including any suitable material that has a higher melting temperature and/or higher coefficient of friction than polytetrafluoroethylene. The offset of polyimide pad (636) in this example may provide a more desirable closing of the nodal gap than the version shown in FIG. 13. For instance, in some settings, it may be desirable to substantially close the nodal gap but not to close it completely uniformly. Various suitable lengths, widths, thicknesses, stand-off heights, nodal offsets, and materials that may be used for polyimide pads (436, 536, 636) will be apparent to those of ordinary skill in the art in view of the teachings herein.

IV. Exemplary Alternative Ultrasonic End Effector with Scalpel Extension

[0043] In some instances, an operator may wish to clamp tissue between a clamp arm and an ultrasonic blade to provide simultaneous severing and sealing of the clamped tissue. In some other instances, an operator may wish to use an ultrasonic blade like a scalpel, simultaneously severing and sealing tissue (or just spot sealing tissue) without clamping on the tissue with a clamp arm. Conventional instrumentation may require use of separate instruments to perform clamping operations and scalpel operations. However, the examples below provide both kinds of operations in a single instrument. It should be understood that the below examples are mere examples, and that numerous variations will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0044] FIG. 16 shows another exemplary alternative end effector (700) that may be used in place of end effector (40) described above, such that end effector (700) may be readily incorporated into instrument (10). End effector (700) of this example comprises a clamp arm (720) and an ultrasonic blade (740). Ultrasonic blade (730) is substantially similar to ultrasonic blade (42) described above. Clamp arm (720) is pivotally coupled with an outer tube (710), which may be provided as a component of shaft assembly (30). Clamp arm (720) is pivotable toward and away from ultrasonic blade (730). Various suitable ways in which clamp arm (720) may be actuated to selectively pivot toward and away from ultrasonic blade (730) will be apparent to those of ordinary skill in the art in view of the teachings herein. Clamp arm (720) includes a tissue pad (722), which may comprise polytetrafluoroethylene and/or any other suitable material(s); and/or may be configured in accordance with at least some of the teachings of U.S. Pub. No. 2006/0079874, the disclosure of which is incorporated by reference herein.

[0045] Outer tube (710) includes a distally projecting tongue (712), which further includes a blade support (714). Blade support (714) comprises a pad that engages ultrasonic blade (730) at a position corresponding to a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (730). This is illustrated in FIG. 17, which shows a wave (W) depicting the resonant ultrasonic vibrations communicated through ultrasonic blade (730), with a node (N) being at the same longitudinal position as blade support (714). The rest of tongue (712) does not contact ultrasonic blade (730); yet tongue (712) extends around a substantial portion of the underside exterior of ultrasonic blade (730). Tongue (712) thus serves as a partial shield, preventing tissue from contacting the shielded portion of ultrasonic blade (730). Blade support (714) is located just distal to the distal end of clamp arm (720) when clamp arm (720) is clamped against ultrasonic blade (730). Blade support (714) thus provides a demarcation between a tissue

clamping region (732) of ultrasonic blade (730) and a tissue scalpel region (734) of ultrasonic blade (730), which extends distally relative to blade support (714).

[0046] As best seen in FIG. 17, the distal tip of tissue scalpel region (734) is located at a position corresponding to an anti-node (AN) associated with resonant ultrasonic vibrations communicated through ultrasonic blade (730), such that tissue scalpel region (734) extends between a first anti-node (AN) and a first node (N). Tissue clamping region (732) extends between the first node (N) at blade support (714) and a second node (N), which is near the transition (742) from acoustic waveguide (740) to ultrasonic blade (730). Thus, it should be understood that a second anti-node (AN) is positioned at approximately the middle of tissue clamping region (732).

[0047] If an operator wishes to cut and seal tissue by clamping the tissue, the operator may simply position the tissue between clamp arm (720) and tissue clamping region of ultrasonic blade (730), actuate clamp arm (720) to clamp on the tissue, then activate ultrasonic blade (730) with ultrasonic vibrational energy. If the operator wishes to spot seal tissue or cut and seal tissue without clamping the tissue, the operator may simply engage the tissue with tissue scalpel region (734) and activate ultrasonic blade (730) with ultrasonic vibrational energy. Clamp arm (720) may remain in an open position as shown in FIG. 16 when the operator just uses tissue scalpel region (734). Alternatively, the operator may hold clamp arm (720) in a closed position, clamped down against tissue clamping region (732) of ultrasonic blade (730) during use of tissue scalpel region (734), even if no tissue is positioned between clamp arm (720) and tissue clamping region (732). Other suitable ways in which end effector (700) may be used will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0048] FIG. 18 shows another exemplary alternative end effector (800) that may be used in place of end effector (40) described above, such that end effector (800) may be readily incorporated into instrument (10). End effector (800) of this example comprises a clamp arm (820) and an ultrasonic blade (840). Ultrasonic blade (830) is substantially similar to ultrasonic blade (42) described above. Clamp arm (820) is pivotally coupled with an outer tube (810), which may be provided as a component of shaft assembly (30). Clamp arm (820) is pivotable toward and away from ultrasonic blade (830). In particular, outer tube (810) is configured to translate distally relative to ultrasonic blade (830) in order to pivot clamp arm (820) toward ultrasonic blade (830). Various suitable ways in which outer tube (810) may be actuated to selectively pivot clamp arm (820) toward and away from ultrasonic blade (830) will be apparent to those of ordinary skill in the art in view of the teachings herein. Clamp arm (820) includes a tissue pad (822), which may comprise polytetrafluoroethylene and/or any other suitable material(s); and/or may be configured in accordance with at least some of the teachings of U.S. Pub. No.

2006/0079874, the disclosure of which is incorporated by reference herein.

[0049] Outer tube (810) includes a distally projecting tongue (812), which further includes a blade support (814). Blade support (814) comprises a pad that engages ultrasonic blade (830) at a position corresponding to a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (830). The rest of tongue (812) does not contact ultrasonic blade (830); yet tongue (812) extends around a substantial portion of the underside exterior of ultrasonic blade (830). Tongue (812) thus serves as a partial shield, preventing tissue from contacting the shielded portion of ultrasonic blade (830). Blade support (814) is located just distal to the distal end of clamp arm (820) when clamp arm (20) is clamped against ultrasonic blade (820). Blade support (814) thus provides a demarcation between a tissue clamping region (832) of ultrasonic blade (830) and a tissue scalpel region (834) of ultrasonic blade (830), which extends distally relative to blade support (814). The distal tip of tissue scalpel region (834) is located at a position corresponding to an anti-node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (830), such that tissue scalpel region (834) extends between a first anti-node and a first node. Tissue clamping region (832) extends between the first node at blade support (814) and a second node, which is near the transition (842) from acoustic waveguide (840) to ultrasonic blade (830). Thus, it should be understood that a second anti-node is positioned at approximately the middle of tissue clamping region (832).

[0050] Tongue (812) of the present example further includes a distal shield portion (816) that is distal to blade support (814) and that is operable to selectively shield at least part of tissue scalpel region (834) from tissue. In some instances, at least part of distal shield portion (816) is configured in accordance with at least some of the teachings of U.S. Pub. No. 2012/0029546, the disclosure of which is incorporated by reference herein. Tongue (812) is slidable with outer tube (810), such that shield portion (816) is operable to selectively shield or un-shield tissue, based on the longitudinal position of tongue (812) and outer tube (810). In some versions, outer tube (810) closes clamp arm (820) when outer tube (810) is in a distal position; and shield portion (816) also shields scalpel region (834) from tissue when outer tube (810) is in a distal position. Thus, shielding and clamping may occur substantially simultaneously. In some other versions, clamp arm (820) and shield portion (816) are actuated independently. Various suitable ways in which actuation of clamp arm (820) and actuation of shield portion (816) may be decoupled and be thereby independent will be apparent to those of ordinary skill in the art in view of the teachings herein. It should also be understood that blade support (814) may remain in a fixed longitudinal position while outer tube (820) and tongue (812) translate. For instance, blade support (814) may be secured to a fixed frame. Regardless, it should be understood that end ef-

factor (800) may be operated in substantially the same manner as end effector (700), as described above.

[0051] FIGS. 19-26 show exemplary alternative forms that scalpel region (734, 834) of end effectors (700, 800) may take. In particular, FIG. 19 shows a distal end of an ultrasonic blade (1000) having a generally cylindraceous portion (1002) and a roughened tip (1004). Tip (1004) of this example is generally spherical and includes one or more of grit, recesses, or other protrusions to provide a rough exterior. FIG. 20 shows a distal end of an ultrasonic blade (1010) having a generally cylindraceous portion (1012) and a tip (1014) with a generally spherical section (1016) and a flat distal face (1018). FIGS. 21-22 show a distal end of an ultrasonic blade (1020) having a generally cylindraceous portion (1022) and a flattened, spatula-like section (1024). FIGS. 23-24 show a distal end of an ultrasonic blade (1030) having a generally cylindraceous portion (1032) and a curved, spatula-like section (1034). FIG. 25 shows a distal end of an ultrasonic blade (1040) having a generally cylindraceous portion (1042) and a tip (1044) with a laterally extending recess (1046) forming a hook (1048). FIG. 26 shows a distal end of an ultrasonic blade (1045) having a generally cylindraceous portion (1052) and a tip (1054) with a hammerhead configuration, including a pair of laterally presented serrated edges (1056). Of course, all of these configurations are merely illustrative. Still other suitable configurations will be apparent to those of ordinary skill in the art in view of the teachings herein.

30

V. Exemplary Alternative Ultrasonic End Effector with Tube Extension Pad

[0052] In ultrasonic instruments having a relatively long ultrasonic blade, there may be instances where the ultrasonic blade bends and deflects away from a longitudinal axis defined by the ultrasonic blade at rest. These deflections may occur when a clamp arm is pressing against the ultrasonic blade and/or when tissue is pressing against the ultrasonic blade. In some instances, these ultrasonic blade deflections may be undesirable. Having a relatively long ultrasonic blade might also increase the presence of nodal gaps, thereby increasing the prominence of acoustic cold spots as described above. It may be desirable to simultaneously address ultrasonic blade deflection and nodal gaps. An example of how this may be done will be described in greater detail below, while other examples will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0053] FIGS. 27-32 show another exemplary alternative end effector (1100) that may be used in place of end effector (40) described above, such that end effector (1100) may be readily incorporated into instrument (10). End effector (1100) of this example comprises a clamp arm (1130) and an ultrasonic blade (1120). Ultrasonic blade (1120) is substantially similar to ultrasonic blade (42) described above. Clamp arm (1130) is pivotally coupled with an outer tube (1110), which may be provided

as a component of shaft assembly (30). Clamp arm (1130) is pivotable toward and away from ultrasonic blade (1120). Various suitable ways in which clamp arm (1130) may be actuated to selectively pivot toward and away from ultrasonic blade (1120) will be apparent to those of ordinary skill in the art in view of the teachings herein. Clamp arm (1130) includes a metallic arm section (1132) and a tissue pad (1134), which may comprise polytetrafluoroethylene and/or any other suitable material(s); and/or may be configured in accordance with at least some of the teachings of U.S. Pub. No. 2006/0079874, the disclosure of which is incorporated by reference herein.

[0054] Outer tube (1110) includes a distally projecting tongue (1140), which further includes a polyimide pad (1142), which is positioned to engage ultrasonic blade (1120) at a location corresponding to a node associated with resonant ultrasonic vibrations communicated through ultrasonic blade (1120). Of course, polyimide is just one merely illustrative example of a material for pad (1142), and any other suitable material(s) may be used. As best seen in FIGS. 27 and 30, ultrasonic blade (1120) does not contact polyimide pad (1142) when ultrasonic blade (1120) is not under any kind of load. Thus, polyimide pad (1142) does not generate any additional heat in ultrasonic blade (1120) when ultrasonic blade is not under any kind of load.

[0055] As best seen in FIGS. 28 and 31, ultrasonic blade (1120) deflects into polyimide pad (1142) when clamp arm (1130) is pivoted into clamping engagement with ultrasonic blade (1120). When ultrasonic blade (1120) is activated while in contact with polyimide pad (1142), polyimide pad (1142) assists in generating additional heat in ultrasonic blade (1120) at the nodal region, thereby closing the nodal gap and addressing what might otherwise be an acoustic cold spot by providing a more even distribution of heat along ultrasonic blade (1120). Of course, while tissue is not shown in FIGS. 23 and 26, it should be understood that the same results may be obtained when tissue is clamped between clamp arm (1130) and ultrasonic blade (1120).

[0056] As best seen in FIGS. 29 and 32, ultrasonic blade (1120) deflects further away from polyimide pad (1142) when ultrasonic blade (1120) is used to perform a back-cutting operation (i.e., when the portion of ultrasonic blade (1120) opposite to clamp arm (1130) is pressed into tissue. Thus, polyimide pad (1142) does not provide any thermal impact during a back-cutting operation. This may be acceptable for users who only wish to use the distal-most portion of ultrasonic blade (1120) during back-cutting anyway, as the distal-most portion would already be sufficiently outside of a nodal gap since the distal tip is positioned at an anti-node.

VI. Miscellaneous

[0057] It should be understood that any of the versions of instruments described herein may include various other

features in addition to or in lieu of those described above. By way of example only, any of the instruments described herein may also include one or more of the various features disclosed in any of the various references that are incorporated by reference herein. It should also be understood that the teachings herein may be readily applied to any of the instruments described in any of the other references cited herein, such that the teachings herein may be readily combined with the teachings of any of the references cited herein in numerous ways. Other types of instruments into which the teachings herein may be incorporated will be apparent to those of ordinary skill in the art.

[0058] It should be appreciated that any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated material does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

[0059] Versions of the devices described above may have application in conventional medical treatments and procedures conducted by a medical professional, as well as application in robotic-assisted medical treatments and procedures. By way of example only, various teachings herein may be readily incorporated into a robotic surgical system such as the DAVINCI™ system by Intuitive Surgical, Inc., of Sunnyvale, California. Similarly, those of ordinary skill in the art will recognize that various teachings of U.S. Pat. No. 6,783,524, entitled "Robotic Surgical Tool with Ultrasound Cauterizing and Cutting Instrument," published August 31, 2004, the disclosure of which is incorporated by reference herein.

[0060] Versions described above may be designed to be disposed of after a single use, or they can be designed to be used multiple times. Versions may, in either or both cases, be reconditioned for reuse after at least one use. Reconditioning may include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, some versions of the device may be disassembled, and any number of the particular pieces or parts of the device may be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, some versions of the device may be reassembled for subsequent use either at a reconditioning facility, or by a user immediately prior to a procedure. Those skilled in the art will appreciate that reconditioning of a device may utilize a variety of tech-

niques for disassembly, cleaning/replacement, and re-assembly. Use of such techniques, and the resulting re-conditioned device, are all within the scope of the present application.

[0061] By way of example only, versions described herein may be sterilized before and/or after a procedure. In one sterilization technique, the device is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and device may then be placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation may kill bacteria on the device and in the container. The sterilized device may then be stored in the sterile container for later use. A device may also be sterilized using any other technique known in the art, including but not limited to beta or gamma radiation, ethylene oxide, or steam.

[0062] Having shown and described various embodiments of the present invention, further adaptations of the methods and systems described herein may be accomplished by appropriate modifications by one of ordinary skill in the art without departing from the scope of the present invention. Several of such potential modifications have been mentioned, and others will be apparent to those skilled in the art. For instance, the examples, embodiments, geometries, materials, dimensions, ratios, steps, and the like discussed above are illustrative and are not required. Accordingly, the scope of the present invention should be considered in terms of the following claims and is understood not to be limited to the details of structure and operation shown and described in the specification and drawings.

[0063] The following is a list of embodiments that may or may not be claimed hereinafter:

1. An apparatus for operating on tissue, the apparatus comprising:

(a) a shaft;
 (b) an acoustic waveguide configured to transmit ultrasonic vibration, wherein the acoustic waveguide extends along the shaft; and
 (c) an end effector, wherein the end effector comprises:

(i) an ultrasonic blade in acoustic communication with the acoustic waveguide, and
 (ii) a clamp arm pivotable toward the ultrasonic blade,
 wherein the end effector defines a first longitudinal region and a second longitudinal region,
 wherein the end effector is configured to clamp tissue between the clamp arm and the ultrasonic blade in the first longitudinal region,
 wherein the end effector is configured to sever tissue with the ultrasonic blade in the

second longitudinal region.

2. The apparatus of embodiment 1, wherein the clamp arm extends along the lengths of the first longitudinal region and the second longitudinal region.

3. The apparatus of embodiment 2, wherein the clamp arm is configured to cooperate with the ultrasonic blade to shear tissue along the second longitudinal region.

4. The apparatus of embodiment 3, wherein the clamp arm is configured to engage tissue along a horizontal plane along the first longitudinal region.

5. The apparatus of embodiment 4, wherein the clamp arm is configured to engage tissue along an oblique plane along the second longitudinal region.

6. The apparatus of embodiment 1, wherein the first longitudinal region is proximal to the second longitudinal region.

7. The apparatus of embodiment 1, wherein the shaft includes an outer tube, wherein the outer tube includes:

(i) a distally projecting tongue portion, and
 (ii) a blade support, wherein the blade support is positioned on the distally projecting tongue portion, wherein the blade support is positioned to contact the ultrasonic blade at a nodal region of the ultrasonic blade.

8. The apparatus of embodiment 7, wherein the tongue portion distally terminates within the first longitudinal region.

9. The apparatus of embodiment 7, wherein the blade support comprises a polyimide pad.

10. The apparatus of embodiment 7, wherein the blade support is positioned to be spaced apart from the ultrasonic blade in the absence of a load on the ultrasonic blade.

11. The apparatus of embodiment 7, wherein the blade support is positioned to separate the first longitudinal region from the second longitudinal region.

12. The apparatus of embodiment 1, wherein the clamp arm is coextensive with the first longitudinal region such that the clamp arm does not extend into the second longitudinal region.

13. The apparatus of embodiment 1, wherein the ultrasonic blade is configured to form an ultrasonic scalpel in the second longitudinal region.

14. The apparatus of embodiment 1, wherein the shaft comprises a tube, wherein the tube is longitudinally slidible relative to the acoustic waveguide. 10

15. The apparatus of embodiment 14, wherein the tube is operable to selectively pivot the clamp arm toward the ultrasonic blade. 5

16. The apparatus of embodiment 14, wherein the tube is operable to selectively shield the ultrasonic blade along the second longitudinal region. 15

17. The apparatus of embodiment 1, wherein the clamp arm comprises a clamp pad. 10

18. An apparatus for operating on tissue, the apparatus comprising: 15

- (a) a shaft;
- (b) an acoustic waveguide configured to transmit ultrasonic vibration, wherein the acoustic waveguide extends along the shaft; and
- (c) an end effector, wherein the end effector comprises: 20

- (i) an ultrasonic blade in acoustic communication with the acoustic waveguide, and
- (ii) a clamp arm pivotable toward the ultrasonic blade, wherein the clamp arm comprises a first clamp pad and a second clamp pad, wherein the first clamp pad is located at a position corresponding to a nodal region of the ultrasonic blade, wherein the first clamp pad has one or both of a higher melting temperature or a higher coefficient of friction than the second clamp pad. 25

19. The apparatus of embodiment 18, wherein the first clamp pad protrudes toward the ultrasonic blade relative to the second clamp pad. 30

20. An apparatus for operating on tissue, the apparatus comprising: 35

- (a) a shaft;
- (b) an acoustic waveguide configured to transmit ultrasonic vibration, wherein the acoustic waveguide extends along the shaft; and
- (c) an end effector, wherein the end effector comprises: 40

- (i) an ultrasonic blade in acoustic communication with the acoustic waveguide, and
- (ii) a clamp arm pivotable toward the ultrasonic blade, wherein the clamp arm includes a first region and a second region, wherein the first region is configured to clamp tissue against the ultrasonic blade 45

along a generally horizontal path, wherein the second region is configured to shear tissue with the ultrasonic blade along a generally oblique path, wherein the second region is longitudinally spaced from the second region. 50

Claims

1. An apparatus for operating on tissue, the apparatus comprising:

- (a) a shaft;
- (b) an acoustic waveguide configured to transmit ultrasonic vibration, wherein the acoustic waveguide extends along the shaft; and
- (c) an end effector, wherein the end effector comprises:

- (i) an ultrasonic blade in acoustic communication with the acoustic waveguide, and
- (ii) a clamp arm pivotable toward the ultrasonic blade, wherein the end effector defines a first longitudinal region and a second longitudinal region, wherein the end effector is configured to clamp tissue between the clamp arm and the ultrasonic blade in the first longitudinal region, wherein the end effector is configured to sever tissue with the ultrasonic blade in the second longitudinal region, wherein the shaft includes an outer tube, wherein the outer tube includes:

- (i) a distally projecting tongue portion, and
- (ii) a blade support, wherein the blade support is positioned on the distally projecting tongue portion, wherein the blade support is positioned to contact the ultrasonic blade at a nodal region of the ultrasonic blade. 55

2. The apparatus of claim 1, wherein the tongue portion distally terminates within the first longitudinal region. 60

3. The apparatus of claim 1, wherein the blade support comprises a polyimide pad. 65

4. The apparatus of claim 1, wherein the blade support is positioned to be spaced apart from the ultrasonic blade in the absence of a load on the ultrasonic blade. 70

5. The apparatus of claim 1, wherein the blade support

is positioned to separate the first longitudinal region from the second longitudinal region.

6. The apparatus of claim 1, wherein the shaft comprises a tube, wherein the tube is longitudinally slidable relative to the acoustic waveguide. 5
7. The apparatus of claim 6, wherein the tube is operable to selectively pivot the clamp arm toward the ultrasonic blade. 10
8. The apparatus of claim 6, wherein the tube is operable to selectively shield the ultrasonic blade along the second longitudinal region. 15
9. The apparatus of claim 1, wherein the clamp arm extends along the lengths of the first longitudinal region and the second longitudinal region.
10. The apparatus of claim 9, wherein the clamp arm is configured to cooperate with the ultrasonic blade to shear tissue along the second longitudinal region. 20
11. The apparatus of claim 10, wherein the clamp arm is configured to engage tissue along a horizontal plane along the first longitudinal region, optionally wherein the clamp arm is configured to engage tissue along an oblique plane along the second longitudinal region. 25
12. The apparatus of claim 1, wherein the first longitudinal region is proximal to the second longitudinal region. 30
13. The apparatus of claim 1, wherein the clamp arm is coextensive with the first longitudinal region such that the clamp arm does not extend into the second longitudinal region. 35
14. The apparatus of claim 1, wherein the ultrasonic blade is configured to form an ultrasonic scalpel in the second longitudinal region. 40
15. The apparatus of claim 1, wherein the clamp arm comprises a clamp pad. 45

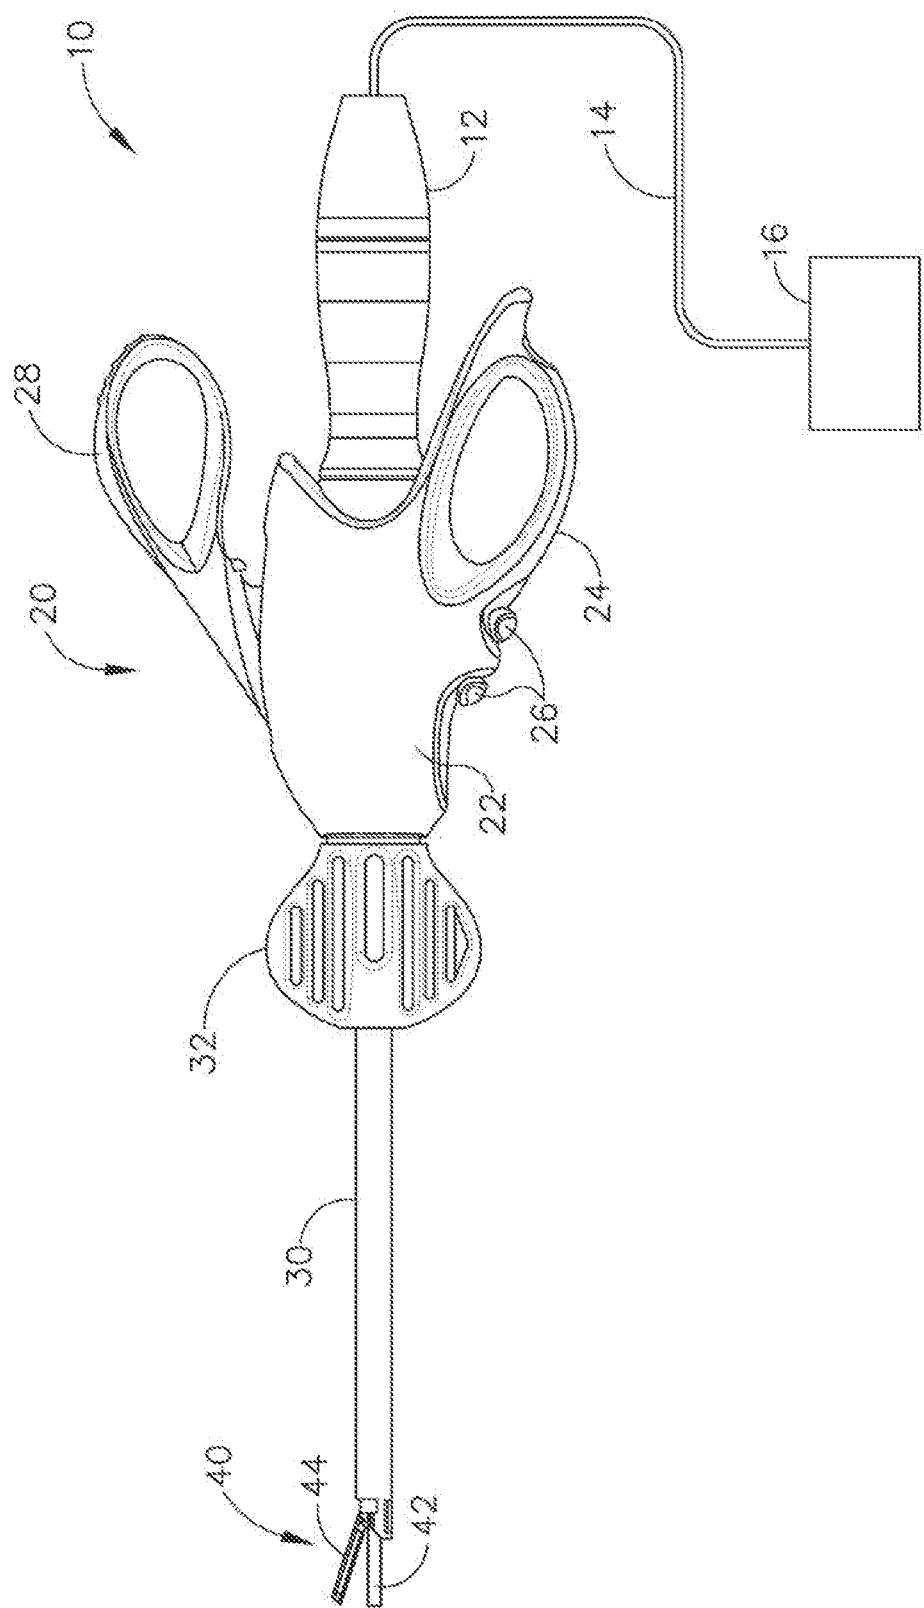


Fig. 1


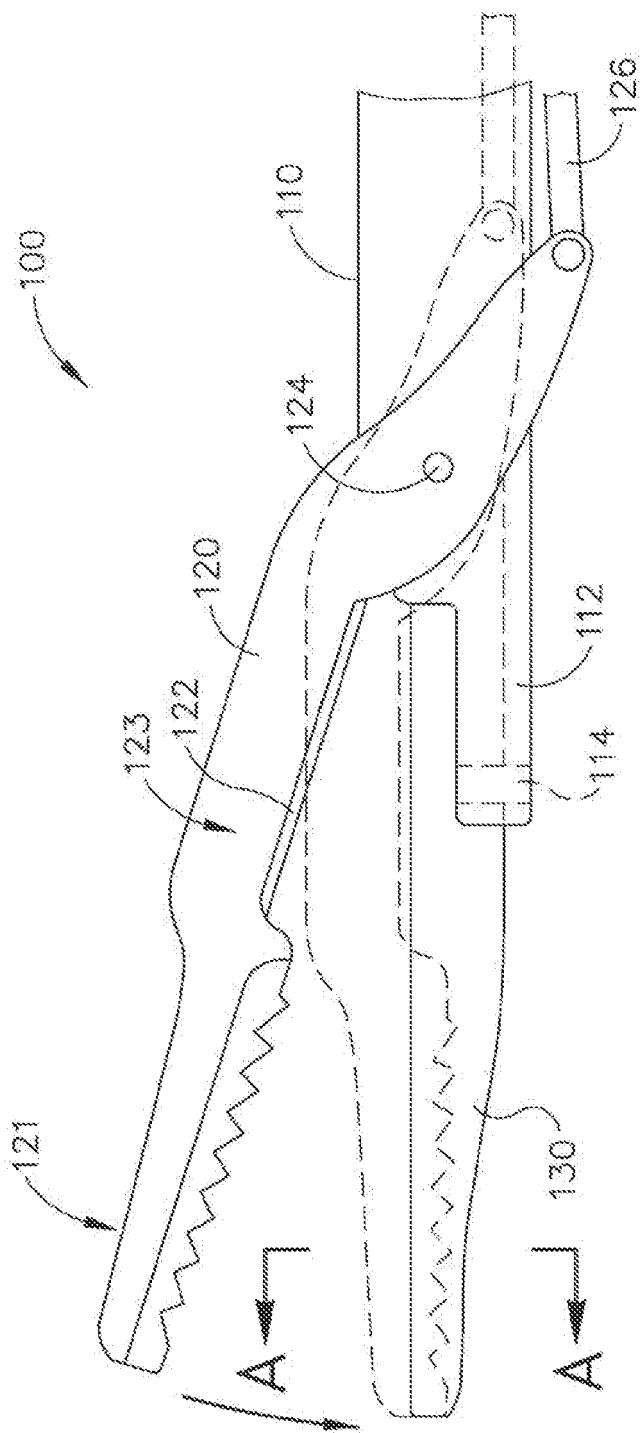


Fig. 2

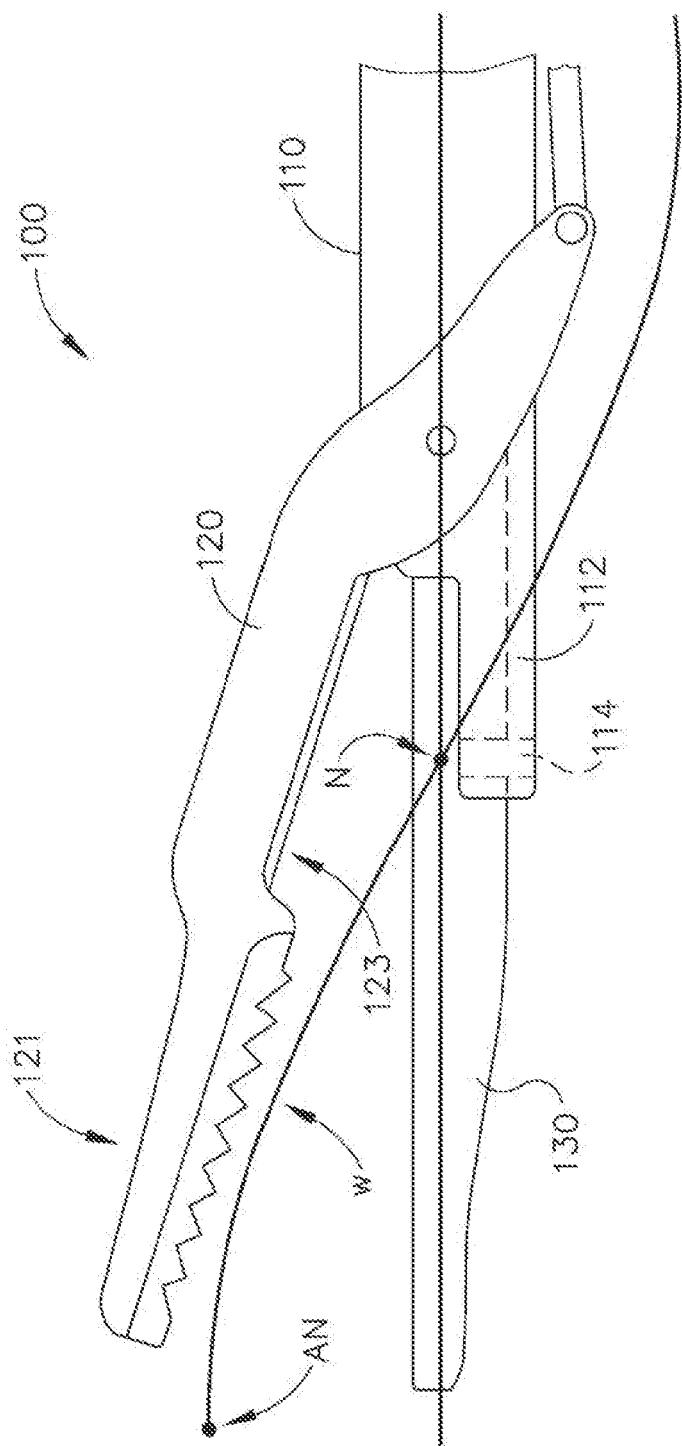

३०

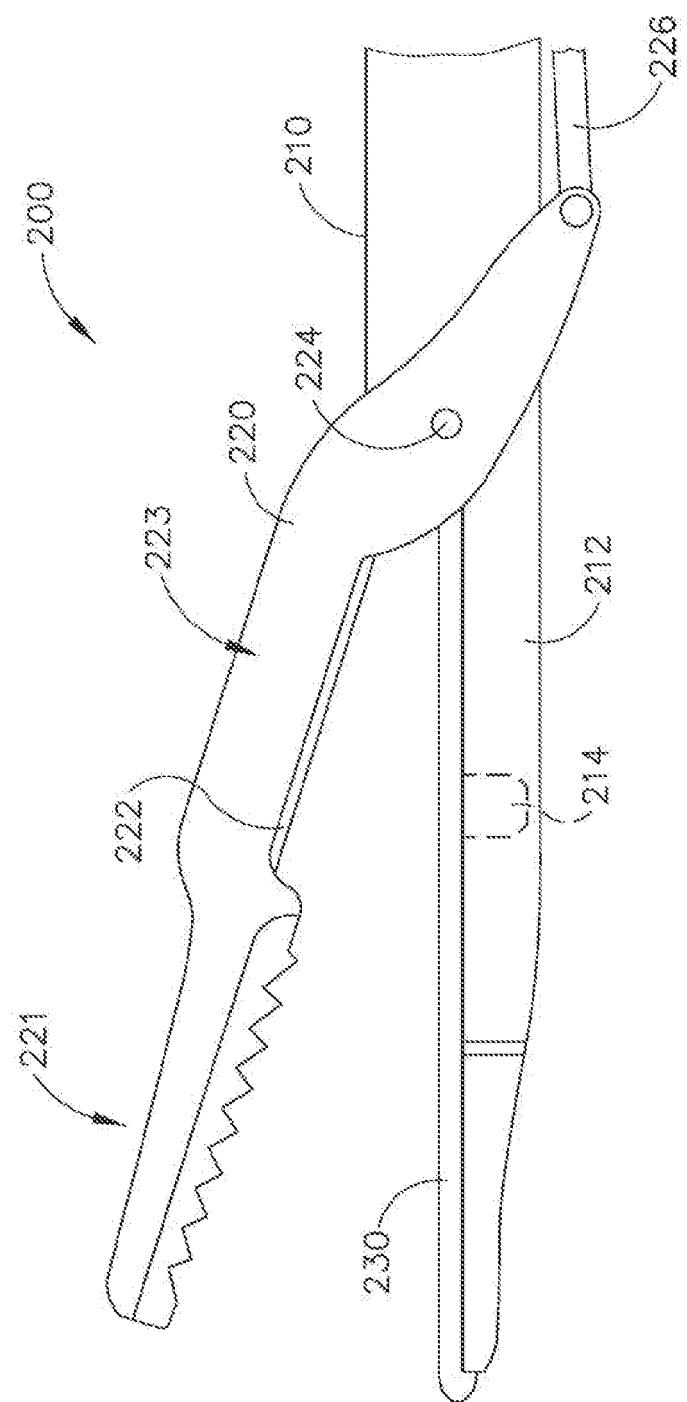


Fig. 4

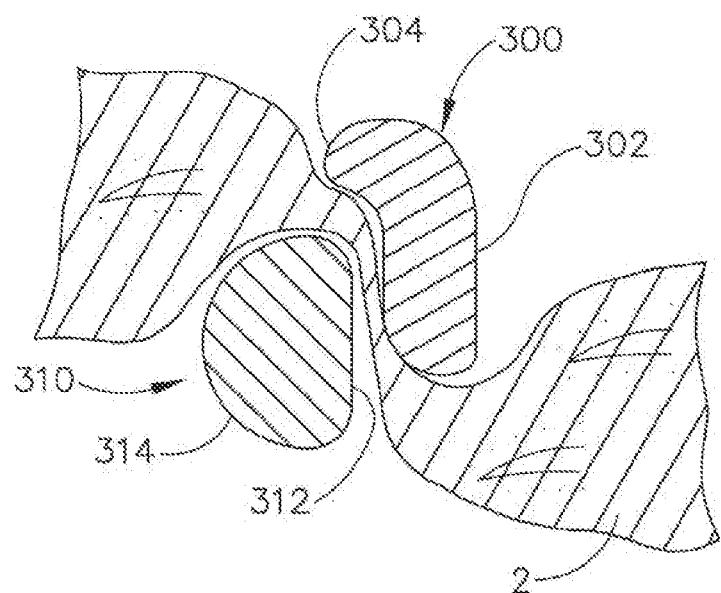


Fig.5

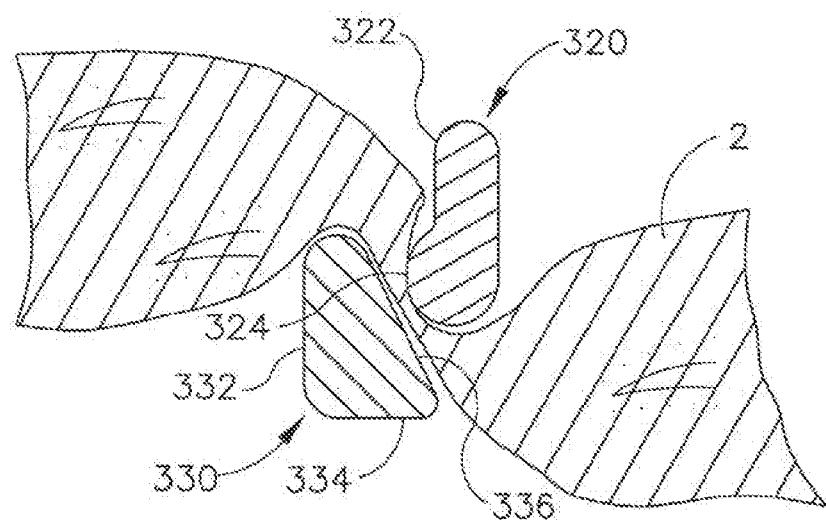


Fig.6

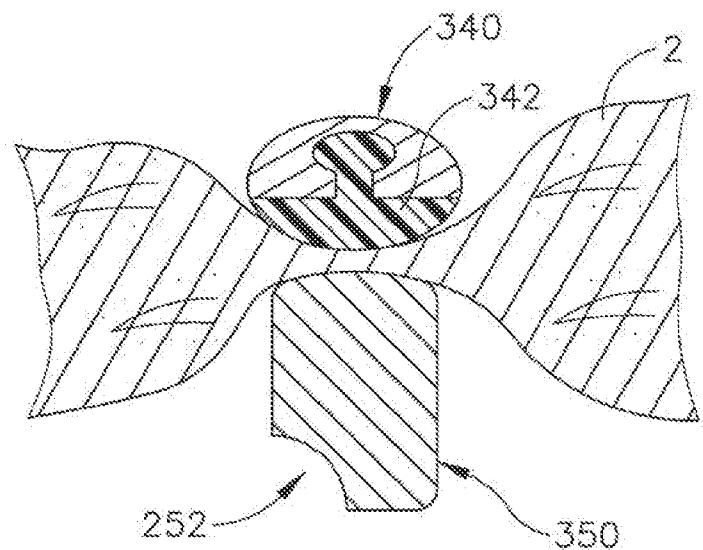


Fig.7

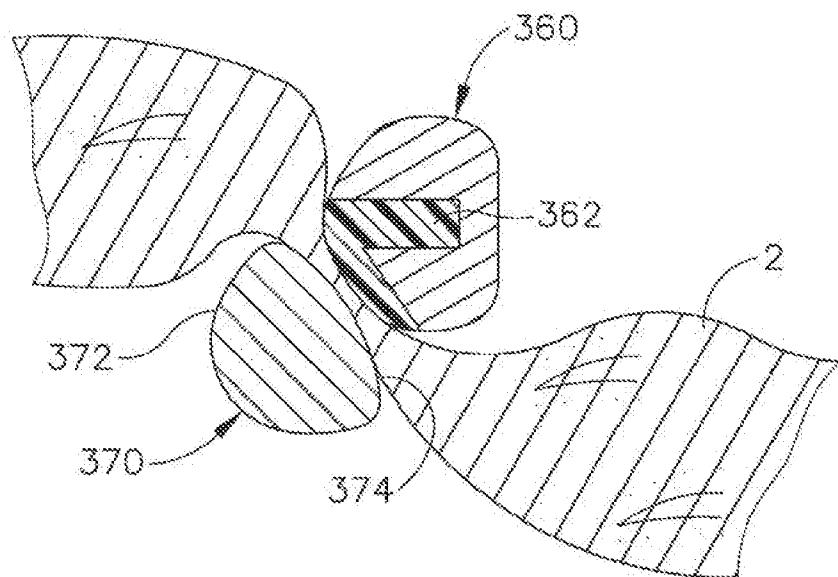


Fig.8

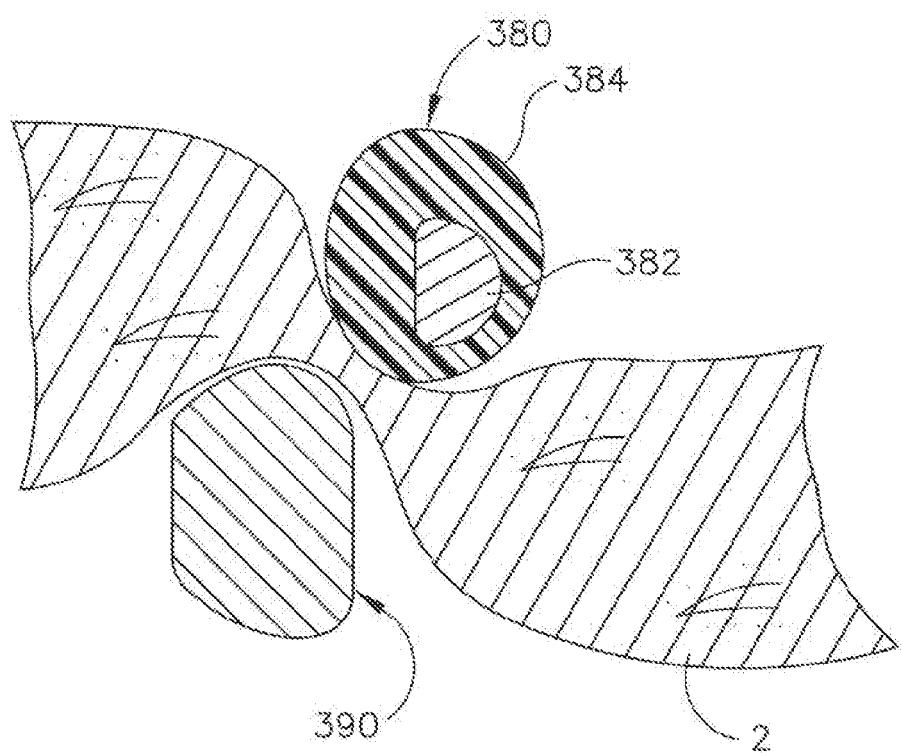
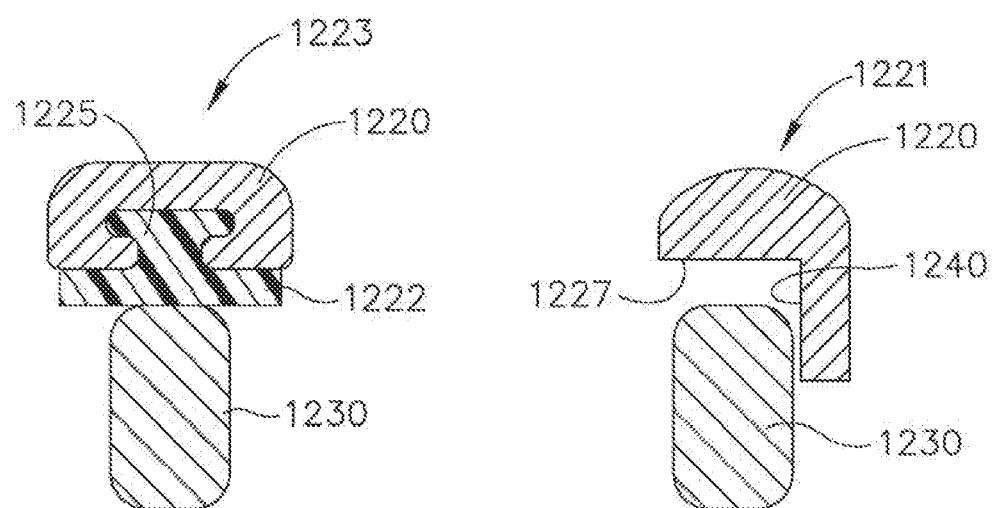
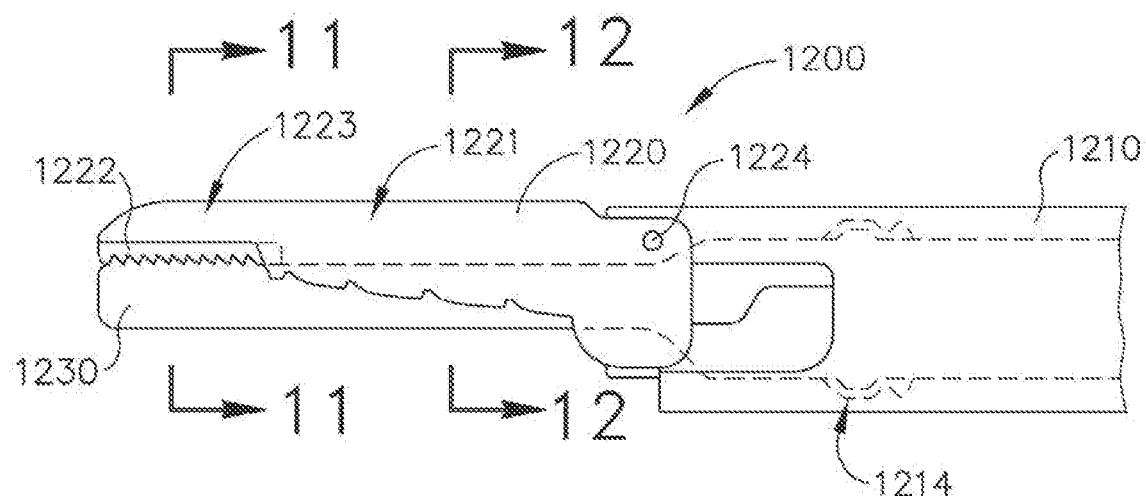


Fig.9



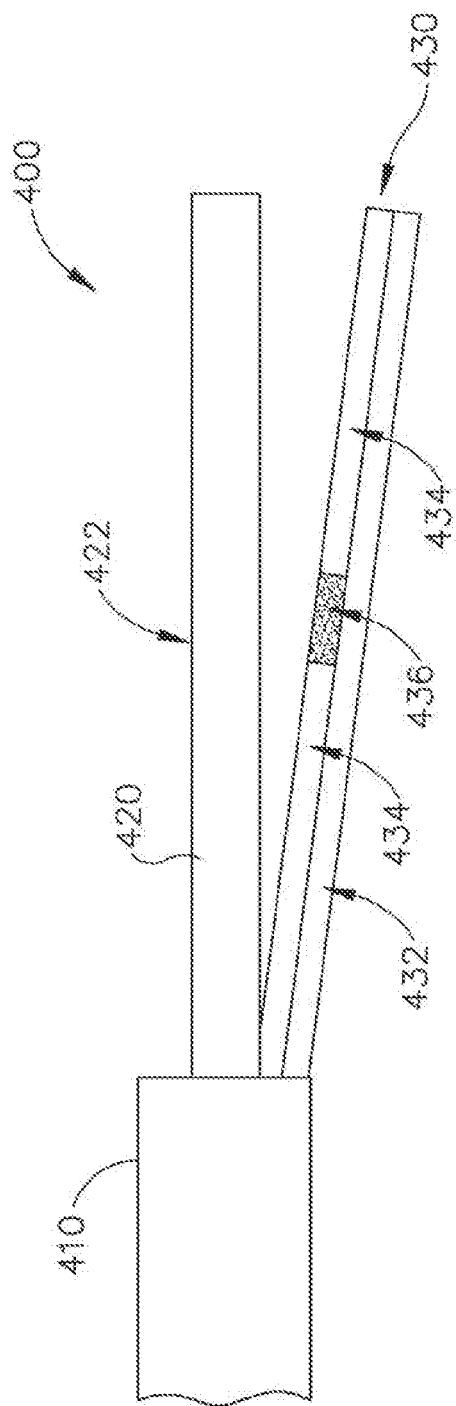


Fig. 13

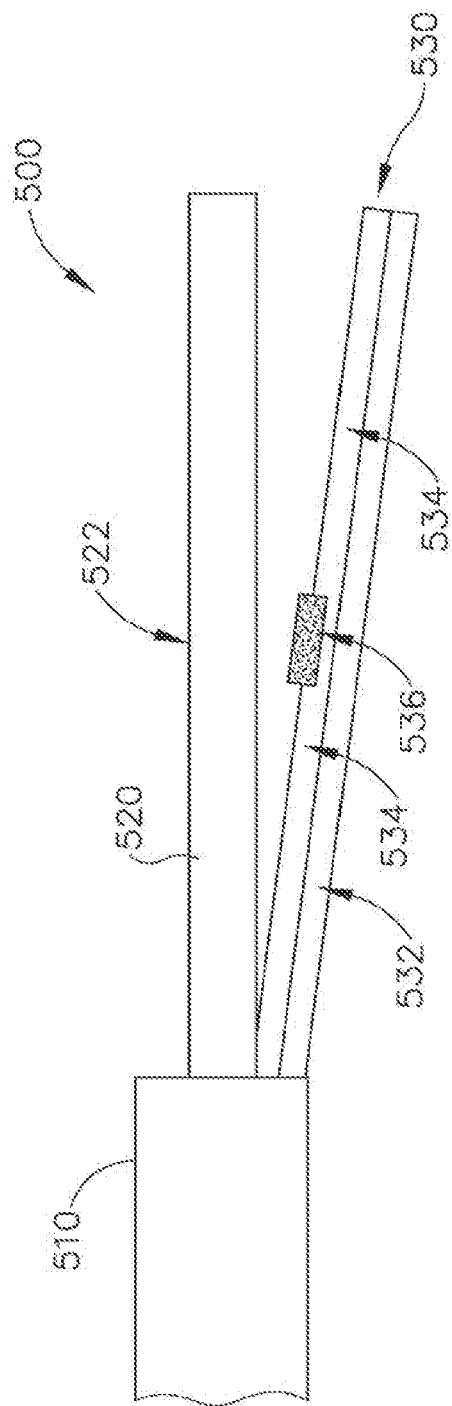


Fig. 14

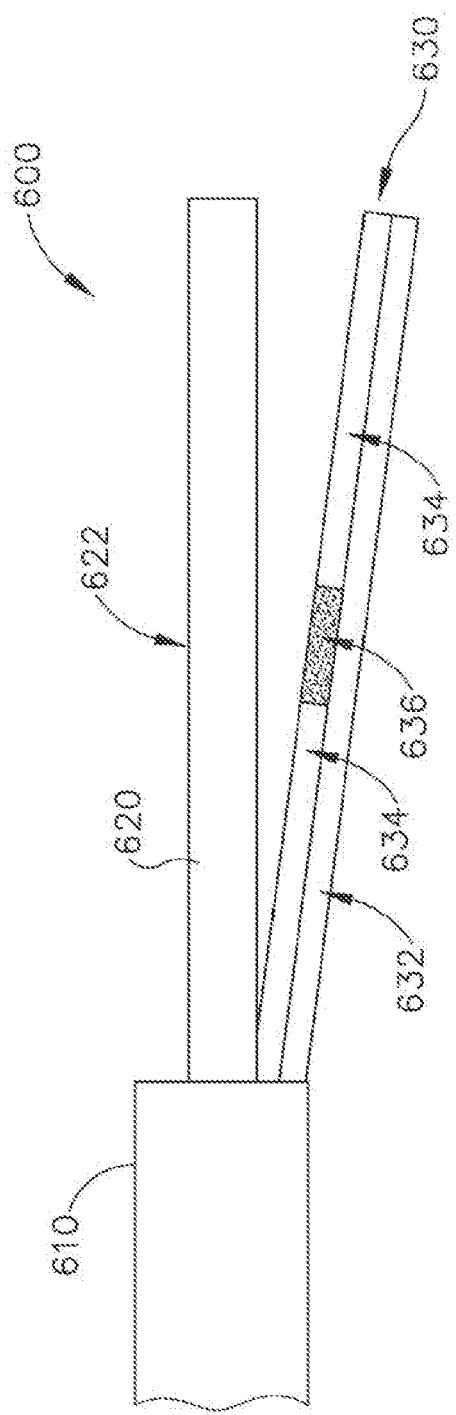


Fig. 15

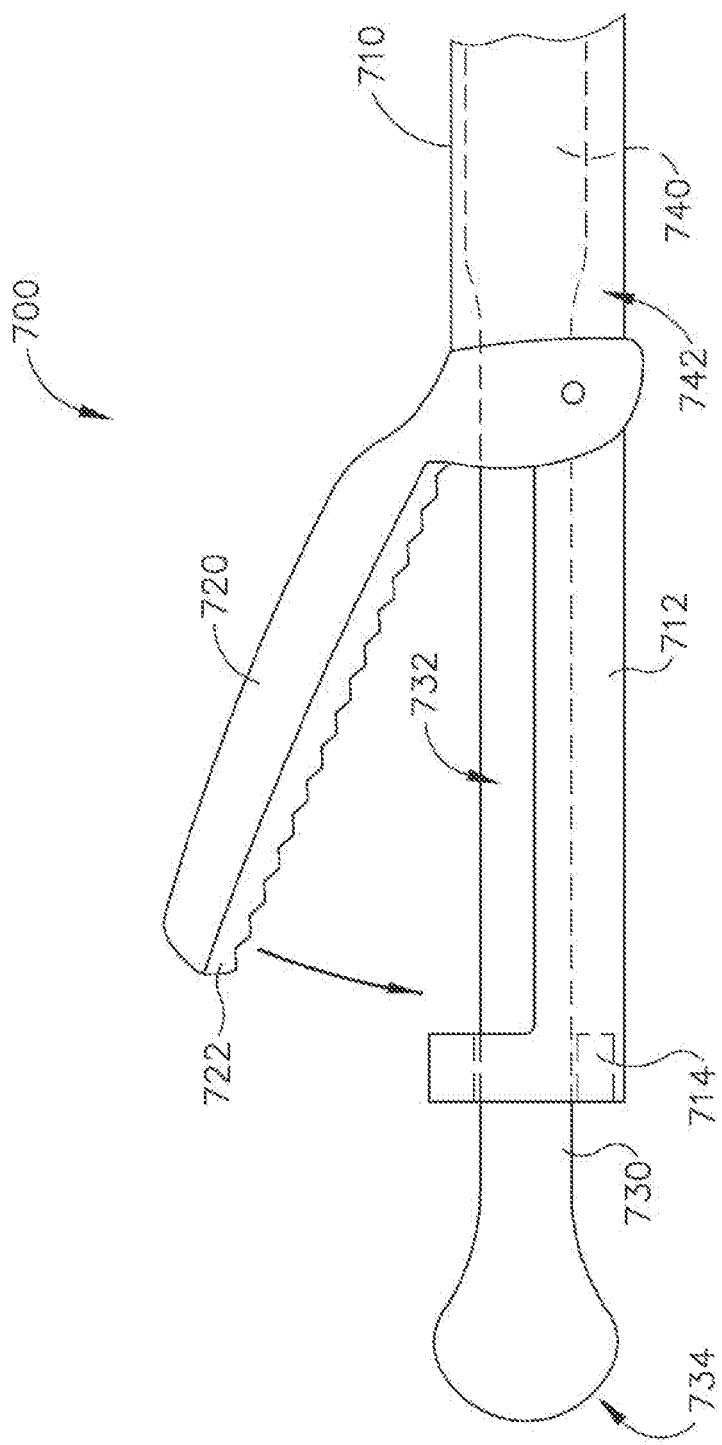


Fig. 16

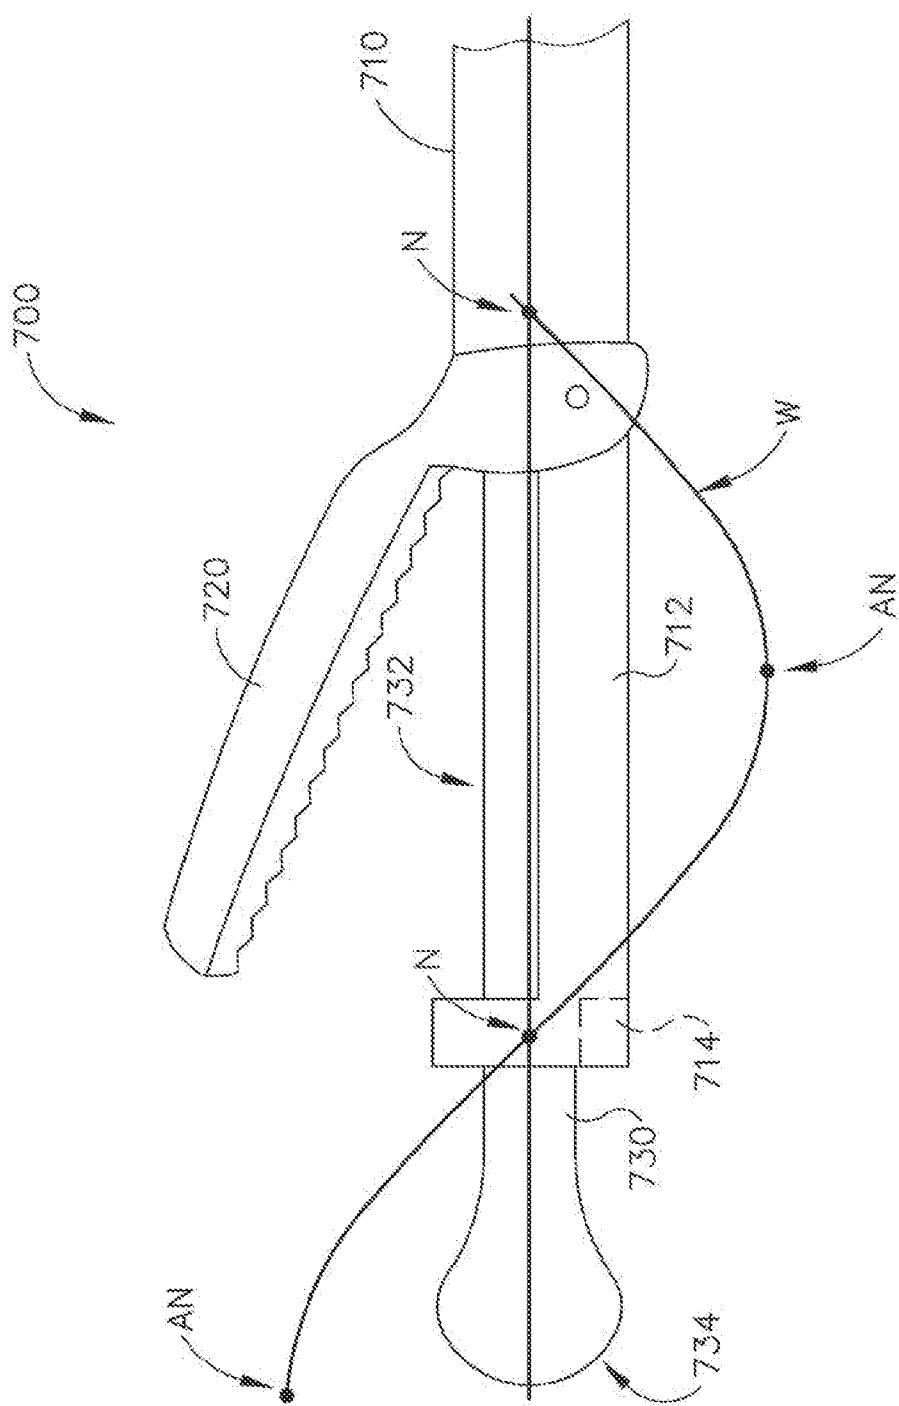


Fig. 17

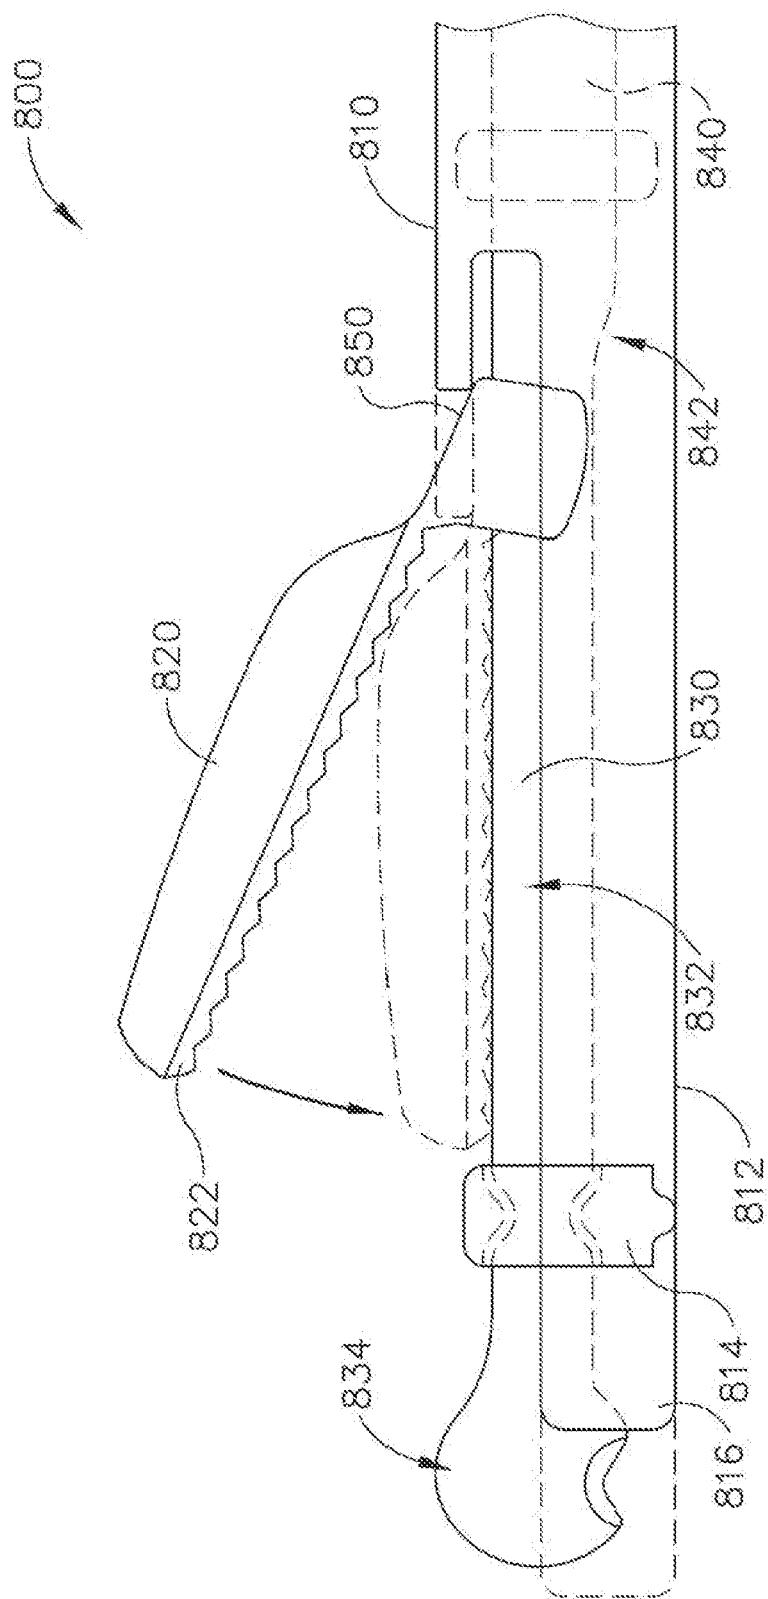


Fig. 18

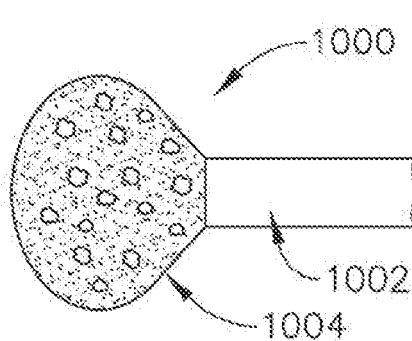


Fig.19

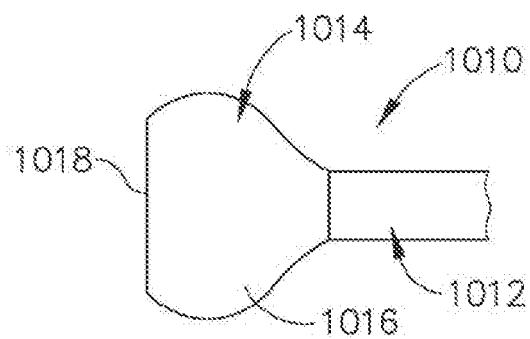


Fig.20

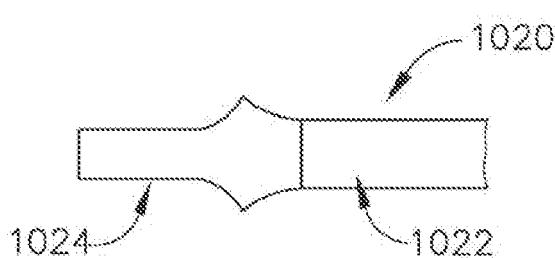


Fig.21

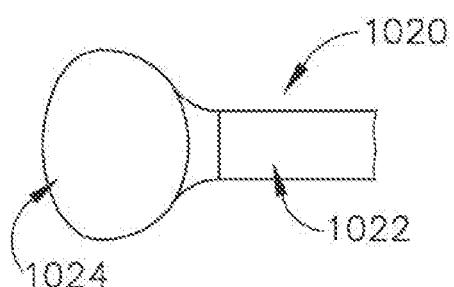


Fig.22

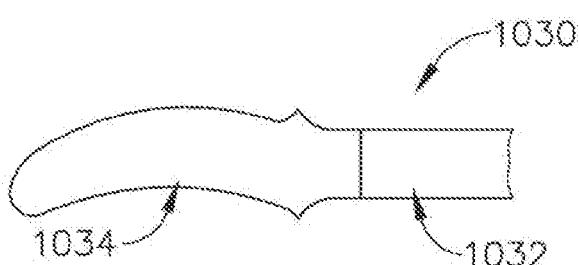


Fig.23

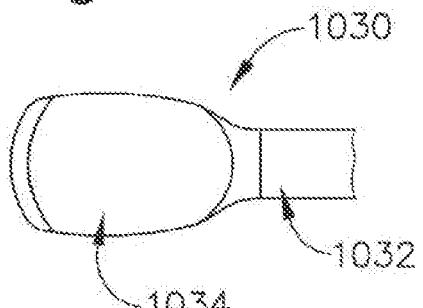


Fig.24

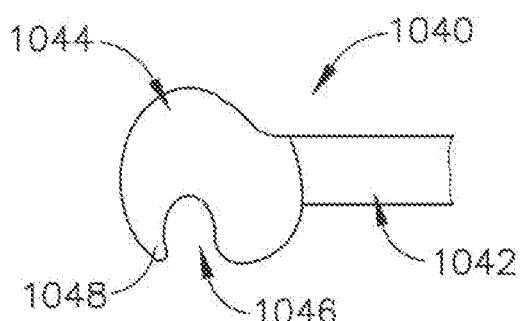


Fig.25

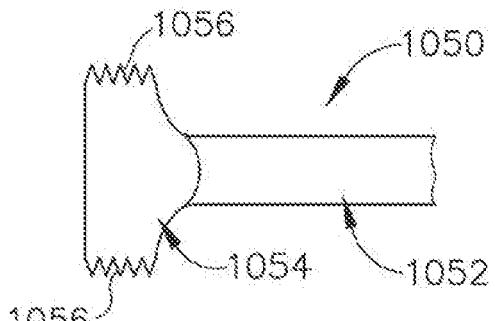


Fig.26

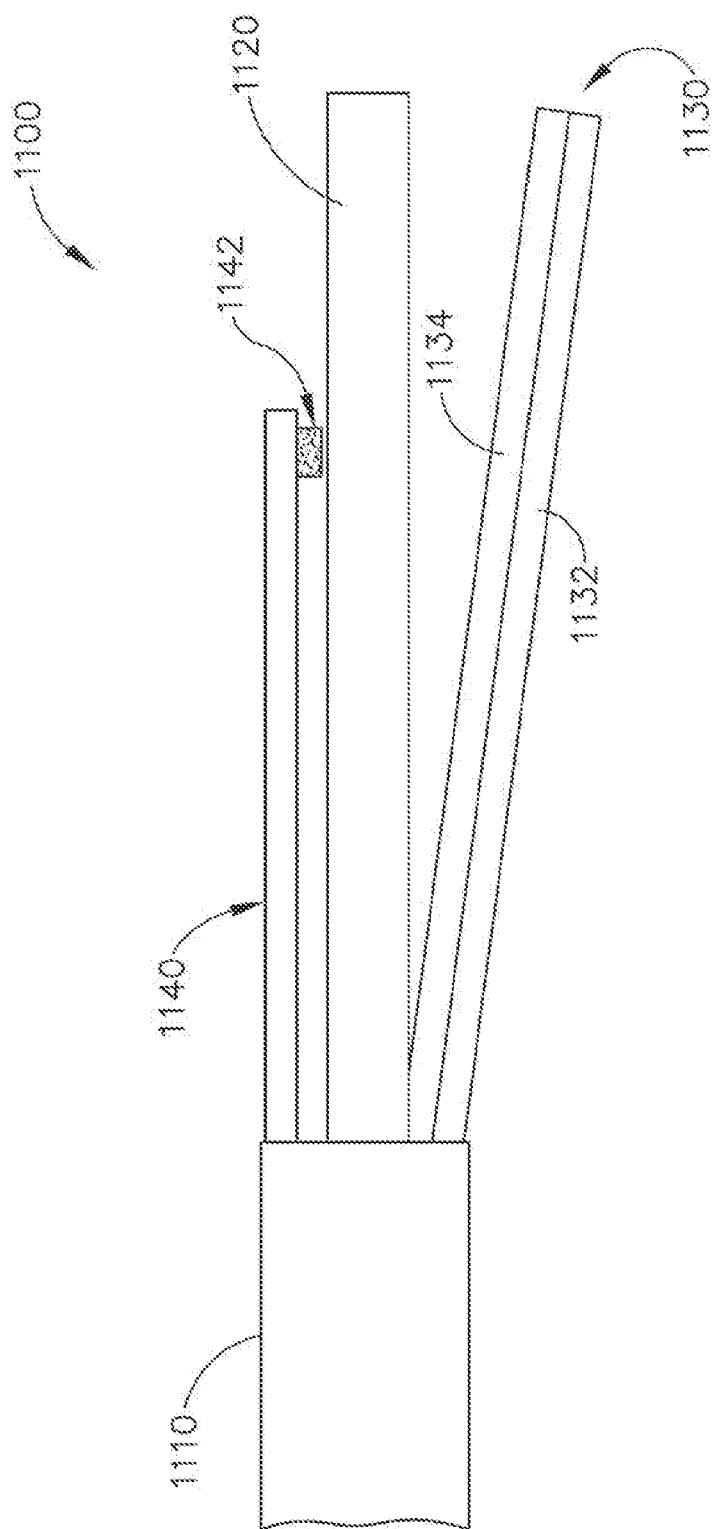


Fig. 27

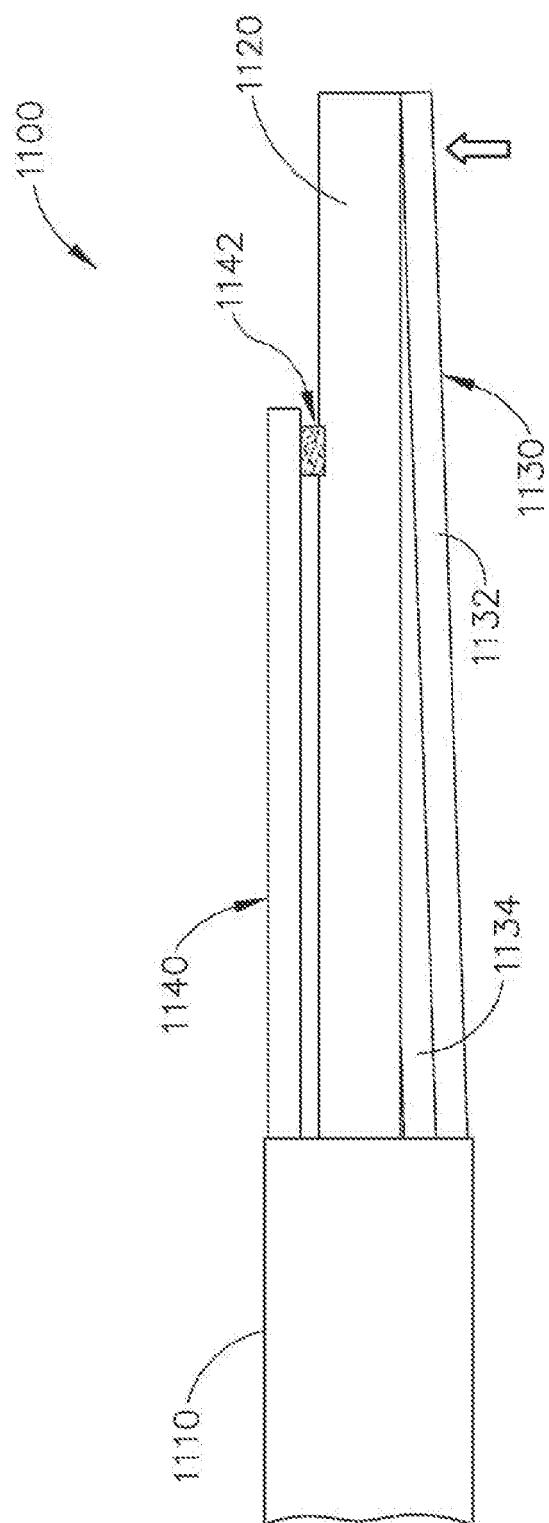


Fig.28

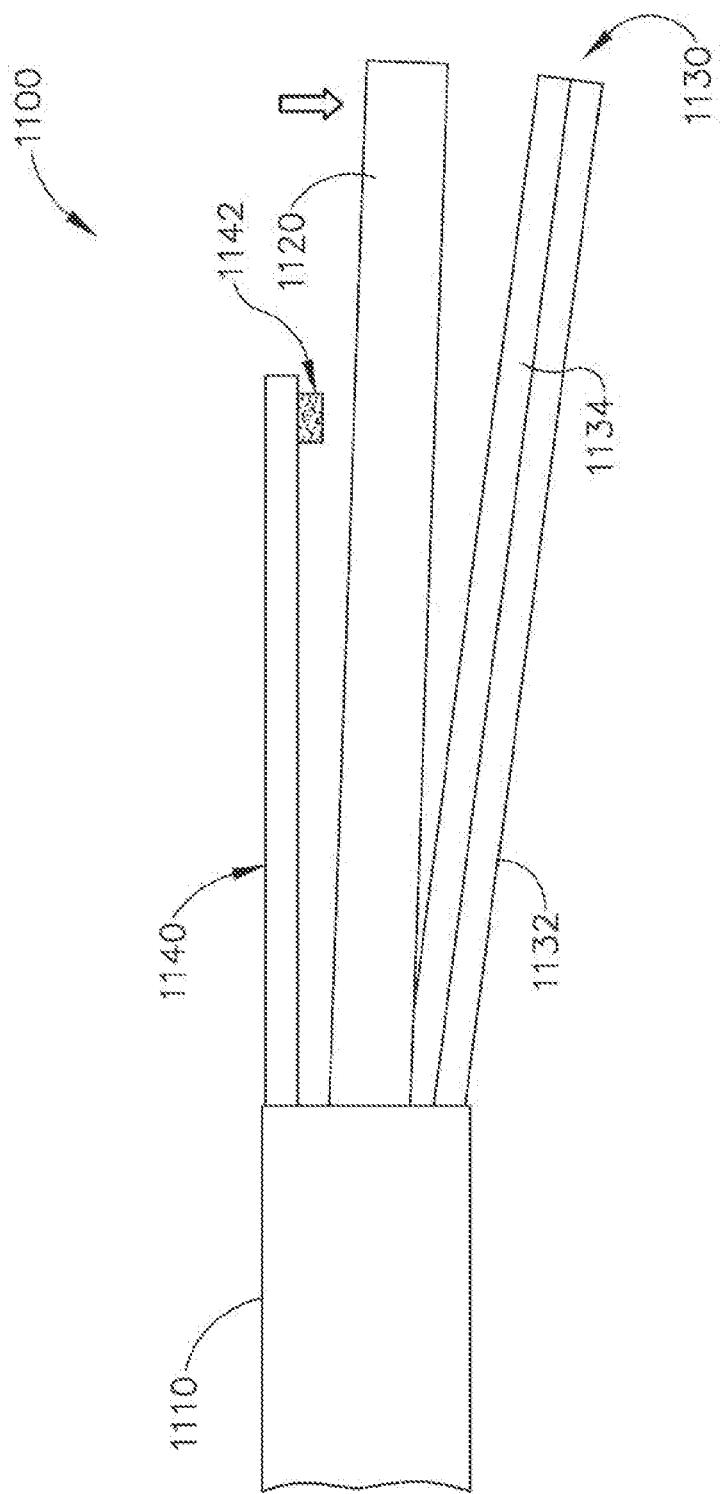


Fig.29

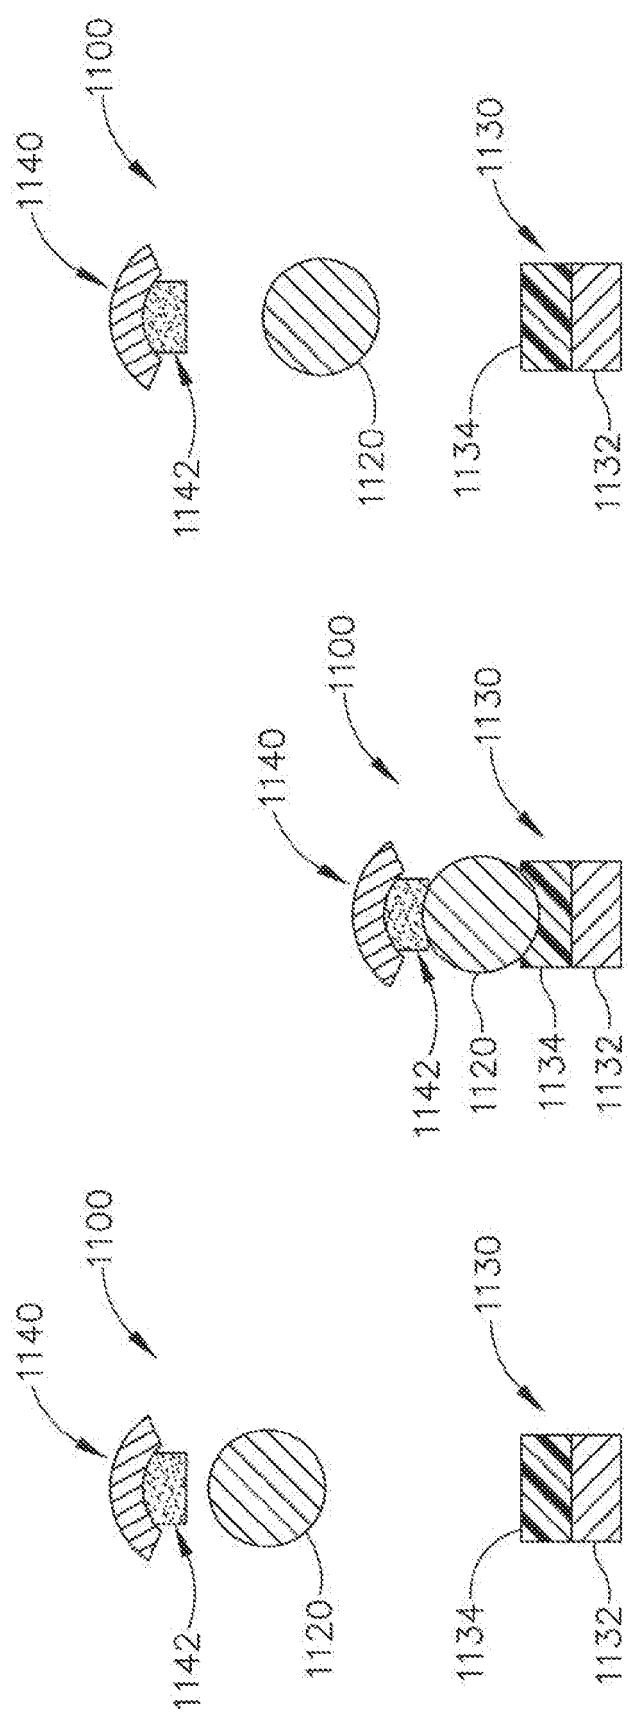


Fig. 30

Fig. 31

Fig. 32



EUROPEAN SEARCH REPORT

Application Number

EP 19 18 7882

5

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
10 Y	US 6 569 178 B1 (MIYAWAKI MAKOTO [JP] ET AL) 27 May 2003 (2003-05-27) * column 27, line 60 - column 29, line 56; figures 34-37,46 *	1-15	INV. A61B17/32
15 Y	----- US 2009/030311 A1 (STULEN FOSTER B [US] ET AL) 29 January 2009 (2009-01-29) * paragraphs [0091], [0131] - [0136], [0144], [0147]; figures 3b,14-16,22-25 *	1-15	
20 Y	----- US 5 322 055 A (DAVISON THOMAS W [US] ET AL) 21 June 1994 (1994-06-21) * column 13, line 3 - line 19; figures 8k-8o,9,10 *	13	
25 A	----- US 2009/143806 A1 (WITT DAVID A [US] ET AL) 4 June 2009 (2009-06-04) * paragraphs [0032], [0065]; figures 15,16 *	1-12,14, 15	
30 A	----- US 2007/198005 A1 (ICHIHASHI HIROSHI [JP] ET AL) 23 August 2007 (2007-08-23) * figures 7-15 *	1-15	TECHNICAL FIELDS SEARCHED (IPC)
35 A	----- US 2009/099582 A1 (ISAACS KAREN K [US] ET AL) 16 April 2009 (2009-04-16) * paragraphs [0116] - [0119]; figure 10C *	1-15	A61B
40			
45			
50 1	The present search report has been drawn up for all claims		
55	Place of search The Hague	Date of completion of the search 23 January 2020	Examiner Mayer-Martenson, E
CATEGORY OF CITED DOCUMENTS		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document			

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 19 18 7882

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

23-01-2020

10	Patent document cited in search report	Publication date	Patent family member(s)			Publication date
15	US 6569178 B1	27-05-2003	NONE			
20	US 2009030311 A1	29-01-2009	AU 2008282457 A1	05-02-2009	CA 2694652 A1	05-02-2009
25			CN 101765495 A	30-06-2010	EP 2185348 A2	19-05-2010
30			JP 5551071 B2	16-07-2014	JP 2010534525 A	11-11-2010
35	US 5322055 A	21-06-1994	US 2009030311 A1	29-01-2009	US 2013226207 A1	29-08-2013
40			US 2016338726 A1	24-11-2016	US 2019380733 A1	19-12-2019
45			WO 2009018083 A2	05-02-2009		
50	US 2009143806 A1	04-06-2009	CA 2153155 A1	04-08-1994	DE 69432741 D1	03-07-2003
55			DE 69432741 T2	25-03-2004	DE 69433704 D1	13-05-2004
			DE 69433704 T2	28-04-2005	DE 69434776 T2	28-06-2007
			EP 0681457 A1	15-11-1995	EP 1125555 A1	22-08-2001
			EP 1433425 A1	30-06-2004	JP H08505801 A	25-06-1996
			US 5322055 A	21-06-1994	US 9416631 A1	04-08-1994
			WO 9416631 A1	04-08-1994		

			US 2008331567 A1	11-06-2009	CA 2707223 A1	11-06-2009
			CN 101883530 A	10-11-2010	DK 2227155 T3	29-08-2016
			EP 2227155 A2	15-09-2010	JP 5976274 B2	23-08-2016
			JP 2011505198 A	24-02-2011	JP 2227155 T3	31-01-2017
			US 2009143806 A1	04-06-2009	US 2009143806 A1	04-06-2009
			US 2017143371 A1	25-05-2017	US 2017143877 A1	25-05-2017
			US 2017143877 A1	25-05-2017	US 2017196586 A1	13-07-2017
			US 2017196587 A1	13-07-2017	US 2017196587 A1	13-07-2017
			US 2017202573 A1	20-07-2017	US 2018263653 A1	20-09-2018
			US 2018289389 A1	11-10-2018	US 2019239919 A1	08-08-2019
			WO 2009073402 A2	11-06-2009		

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

page 1 of 2

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 19 18 7882

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
 The members are as contained in the European Patent Office EDP file on
 The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

23-01-2020

10	Patent document cited in search report	Publication date	Patent family member(s)		Publication date
15	US 2007198005 A1	23-08-2007	CN	101370440 A	18-02-2009
			EP	1987793 A1	05-11-2008
			JP	4879966 B2	22-02-2012
			JP	W02007097330 A1	16-07-2009
20			US	2007198005 A1	23-08-2007
			WO	2007097330 A1	30-08-2007
25	US 2009099582 A1	16-04-2009	AU	2008310869 A1	16-04-2009
			CA	2702075 A1	16-04-2009
			CN	101820825 A	01-09-2010
			EP	2242434 A1	27-10-2010
			JP	5587191 B2	10-09-2014
30			JP	2011500161 A	06-01-2011
			US	2009099582 A1	16-04-2009
35			WO	2009049016 A1	16-04-2009
40					
45					
50					
55	EPO FORM P0459				

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

page 2 of 2

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5322055 A [0001] [0009] [0017]
- US 5873873 A [0001] [0009] [0017]
- US 5980510 A [0001] [0009] [0017]
- US 6325811 B [0001] [0009] [0017]
- US 6783524 B [0001] [0009] [0017] [0059]
- US 20060079874 A [0001] [0009] [0017] [0022] [0033] [0044] [0048] [0053]
- US 20070191713 A [0001] [0009] [0017]
- US 20070282333 A [0001] [0009] [0017]
- US 20080200940 A [0001] [0009] [0017]
- US 20100069940 A [0001] [0009] [0017]
- US 20110015660 A [0001] [0009] [0017]
- US 20120029546 A [0001] [0025] [0050]
- US 53858812 [0001]
- US 65755312 [0001]
- US 20120112687 A [0002] [0009] [0017]
- US 20120116265 A [0002] [0009] [0017]
- US 61410603 [0002] [0009]
- US 538588 [0009] [0016] [0017]
- US 657553 [0009] [0016] [0017]
- US 20110087212 A [0012]
- US 20120078247 A [0016]

专利名称(译)	具有钳位功能的手术超声波剪刀		
公开(公告)号	EP3616631A1	公开(公告)日	2020-03-04
申请号	EP2019187882	申请日	2014-03-10
[标]申请(专利权)人(译)	ETHICON , LLC		
申请(专利权)人(译)	ETHICON LLC		
当前申请(专利权)人(译)	ETHICON LLC		
[标]发明人	WITT DAVID A STULEN FOSTER B PAPA CHRISTOPHER A BATTAGLIA VINCENT P JR		
发明人	MESSERLEY, JEFFREY D. WITT, DAVID A. STULEN, FOSTER B. PAPA, CHRISTOPHER A. BATTAGLIA, VINCENT P., JR.		
IPC分类号	A61B17/32		
CPC分类号	A61B17/320092 A61B2017/320093 A61B2017/320094 A61B2017/320095 A61B2017/320097		
优先权	13/834248 2013-03-15 US PCT/US2014/022462 2014-03-10 WO		
外部链接	Espacenet		

摘要(译)

用于在组织上操作的设备包括轴，声波导管和末端执行器。声波导管沿轴延伸，并构造成传输超声振动。末端执行器包括超声刀和夹持臂。超声刀与声波导管连通。夹臂可朝着超声刀枢转。末端执行器限定第一纵向区域和第二纵向区域。末端执行器构造成在第一纵向区域中将组织夹持在夹持臂和超声刀之间。末端执行器被配置为利用超声刀在第二纵向区域中切割组织。

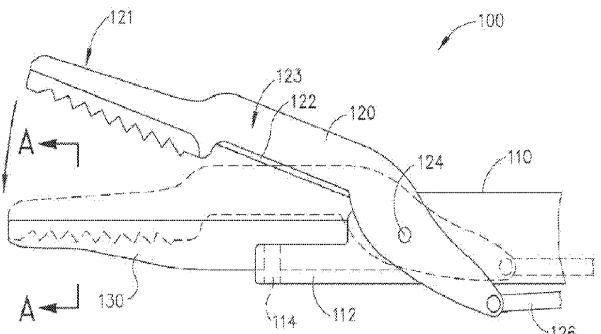


Fig.2