



(43) International Publication Date
9 October 2014 (09.10.2014)

(51) International Patent Classification:

A61B 17/22 (2006.01) A61B 18/26 (2006.01)
A61B 17/3207 (2006.01) A61M 25/09 (2006.01)
A61M 25/10 (2013.01)

(21) International Application Number:

PCT/US2014/019268

(22) International Filing Date:

28 February 2014 (28.02.2014)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

13/800,214 13 March 2013 (13.03.2013) US

(71) Applicant: THE SPECTRANETICS CORPORATION

[US/US]; 9965 Federal Drive, Colorado Springs, CO
80921-3617 (US).

(72) Inventor: GRACE, Kenneth, P.; 430 Hopi Trail, Wood-

land Park, CO 80863 (US).

(74) Agent: SWARTZ, Douglas, W.; Sheridan Ross P.C., 1560

Broadway, Suite 1200, Denver, CO 80202 (US).


(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: ASSISTED CUTTING BALLOON

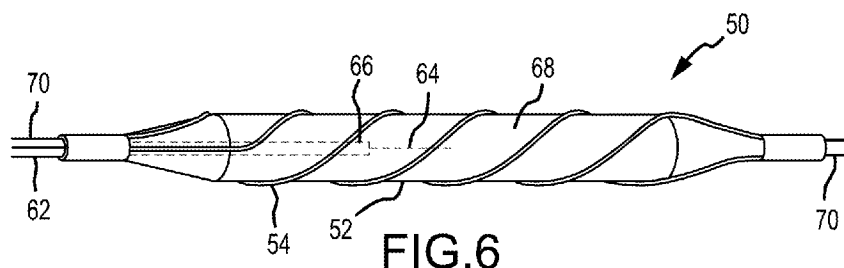

(57) Abstract: A dilation balloon is wrapped in one or more patterns with a wire or braided material having diamond abrasive or other abrasive material bonded thereto. The wire or braided material is vibrated in one or more ways to enhance the cutting action of the wire abrasive. The wire abrasive may be vibrated using high, low, or even ultrasonic waves transmitted to the wire abrasive via local or remote methods. Alternatively, the dilation balloon may be dilated with a contrast media that exhibits a high absorption to laser light. The contrast material is lased with a laser fiber or fibers inserted into the balloon interior, creating a substantial Shock-wave that vibrates the balloon and assists in the cracking or abrading of the surrounding plaque in contact with the dilation balloon. The cutting balloon may employ the abrasive coated wires described above or cutting blades.

ASSISTED CUTTING BALLOON

FIELD

[0001] This disclosure relates generally to cutting balloons utilized in balloon angioplasty and particularly to cutting balloons whose cutting action is assisted in one or
5 more ways to increase the cutting action while at the same time allowing for reduced pressure within the cutting balloon.

BACKGROUND

[0002] Coronary artery disease (CAD) affects millions of Americans, making it the most common form of heart disease. CAD most often results from a condition known as
10 atherosclerosis, wherein a waxy substance forms inside the arteries that supply blood to the heart. This substance, called plaque, is made of cholesterol, fatty compounds, calcium, and a blood-clotting material called fibrin. As the plaque builds up, the artery narrows, making it more difficult for blood to flow to the heart. As the blockage gets worse, blood flow to the heart slows, and a condition called angina pectoris, or simply angina, may
15 develop. Angina is like a squeezing, suffocating, or burning feeling in the chest. The pain usually happens when the heart has an extra demand for blood, such as during exercise or times of emotional stress. In time, the narrowed or blocked artery can lead to a heart attack. A number of medicines can be used to relieve the angina pain that comes with CAD, but these medicines cannot clear blocked arteries. A moderate to severely narrowed
20 coronary artery may need more aggressive treatment to reduce the risk of a heart attack.

[0003] Balloon angioplasty is a technique for mechanically widening narrowed or obstructed arteries, the latter typically being a result of atherosclerosis. An empty and collapsed balloon on a guide wire, known as a balloon catheter, is passed into the narrowed locations and then inflated to a fixed size using water pressures some 75 to 500
25 times normal blood pressure (6 to 20 atmospheres). The balloon is carefully inflated, first under low pressure, and then under higher pressure, until the narrowed area is widened. The balloon inflation crushes the fatty deposits it expands against, opening up the blood vessel for improved blood flow. The balloon is then deflated and withdrawn. Although the narrowing is improved in a majority of patients following
30 balloon dilation, over time, the artery can again become narrow in as many as 15% to 20% of cases, requiring further balloon dilation. A stent may or may not be inserted at the time of balloon dilation to ensure the vessel remains open.

[0004] Percutaneous coronary intervention (PCI) is a therapeutic procedure to treat the stenotic (narrowed) coronary arteries of the heart due to CAD. These stenotic segments are caused by the buildup of plaque that forms due to atherosclerosis. PCI is usually performed by an interventional cardiologist.

5 [0005] PCI includes the use of balloons, stents, and atherectomy devices. PCI is accomplished with a small balloon catheter inserted into an artery in the groin or arm, and advanced to the narrowing in the coronary artery. The balloon is then inflated to enlarge the narrowing in the artery. When successful, PCI allows more blood and oxygen to be delivered to the heart muscle and can relieve the chest pain of angina, improve the
10 prognosis of individuals with unstable angina, and minimize or stop a heart attack without having the patient undergo open heart coronary artery bypass graft (CABG) surgery.

[0006] Balloon angioplasty is also called percutaneous transluminal coronary angioplasty (PTCA). Both PCI and PTCA are non-surgical procedures. Balloon angioplasty can also be used to open narrowed vessels in many other parts of the
15 body. Peripheral angioplasty (PA) refers to the use of a balloon to open a blood vessel outside the coronary arteries. It is commonly done to treat atherosclerotic narrowing of the abdomen, leg, and renal arteries. PA can also be done to treat narrowing in veins. Often, PA is used in conjunction with peripheral stenting and atherectomy. For example, doctors can perform carotid angioplasty to open narrowed carotid arteries, which
20 are the arteries that supply blood to the brain. A stroke most often occurs when the carotid arteries become blocked and the brain does not get enough oxygen. Balloon angioplasty can also be performed in the aorta (the main artery that comes from the heart), the iliac artery (in the hip), the femoral artery (in the thigh), the popliteal artery (behind the knee), and the tibial and peroneal arteries (in the lower leg). The use of fluoroscopy assists the
25 doctor in the location of blockages in the coronary arteries as the contrast dye moves through the arteries. A small sample of heart tissue (biopsy) may be obtained during the procedure to be examined later under the microscope for abnormalities.

[0007] A cutting balloon (CB) is an angioplasty device used in PCI and PTCA and is a proven tool for the mechanical challenges of complex lesions that are often resistant to
30 conventional balloon angioplasty. A CB has a special balloon with small blades that are activated when the balloon is inflated. The CB typically has three or four atherotomes (microsurgical blades) bonded longitudinally to its surface, suitable for creating discrete longitudinal incisions in the atherosclerotic target coronary segment during balloon

inflation. Cutting balloon angioplasty (CBA) features three or four atherotomes, which are 3-5 times sharper than conventional surgical blades. The atherotomes, which are fixed longitudinally on the outer surface of a non-complaint balloon, expand radially and deliver longitudinal incisions in the plaque or target lesion, relieving its hoop stress. With the CBA, the increase in the vessel lumen diameter is obtained in a more controlled fashion and with a lower balloon inflation pressure than PCI and PTCA procedures utilizing conventional balloons. This controlled dilation could reduce the extent of vessel wall injury and the incidence of restenosis.

[0008] The advantage of CBA is its ability to reduce vessel stretch and vessel injury by scoring the target coronary segment longitudinally rather than causing an uncontrolled disruption of the atherosclerotic plaque or target lesion. The atherotomes deliver a controlled fault line during dilation to ensure that the crack propagation ensues in an orderly fashion. The CB also dilates the target vessel with less force to decrease the risk of a neoproliferative response and restenosis. The unique design of the CB is engineered to protect the vessel from the edges of the atherotomes when it is deflated. This minimizes the risk of trauma to the vessel as the balloon is passed to and from the target coronary segment. With CBA, balloon inflation pressures can still range between 14-16 atmospheres, though lower inflation pressures are recommended.

[0009] Angioplasty balloons that employ a woven mesh, cutting strings, or wires are also known in the art. These balloons have been shown to be more flexible and safer than balloons employing cutting blades and edges. The scoring elements can, for example, be in the form of a single wire or a plurality of wires wrapped around a dilation balloon in a helical configuration. Other angioplasty cutting balloon catheter assemblies have a catheter equipped with an inflatable balloon with an interior cavity and an expandable covering around the balloon. The expandable covering may be in the form of a mesh coating having a cross-hatched pattern. The mesh coating may be made of plastic or metal fibers, where at least some of the fibers have cutting edges. In operation, the cutting edges abrade the stenosis, plaque, or lesions along the vessel walls when the catheter assembly is reciprocally moved longitudinally or rotationally after inflation of the balloon.

SUMMARY

[0010] These and other needs are addressed by the various aspects, embodiments, and configurations of the present disclosure. The disclosure is generally directed to the use of

vibrations to enhance the performance of cutting balloons, particularly in angioplasty, in treating lesions, occlusions and plaque.

[0011] A method, according to this disclosure, can perform balloon angioplasty by the steps of:

5 (a) inserting an assisted cutting balloon into a target coronary segment partially occluded with plaque, the assisted cutting balloon having one or more cutting devices positioned on an exterior of the dilation balloon; and

(b) inflating the dilation balloon and vibrating the one or more cutting devices while the cutting balloon is inserted into the target coronary segment.

10 [0012] The expanding and vibrating dilation balloon can crush softer portions of the plaque, and/or the vibrating wire abrasive can cut the harder or calcified portions of the plaque.

[0013] An assisted cutting balloon for performing balloon angioplasty, according to this disclosure, can include:

15 (a) a dilation balloon;

(b) one or more cutting devices operably positioned on an exterior of the dilation balloon;

(c) a laser light source terminating at a distal end in the interior of the dilation balloon; and

20 (d) a contrast medium for inflating the dilation balloon.

[0014] As the dilation balloon is inflated with the contrast medium and/or after inflation, the laser light source can transmit pulsed laser light into the contrast medium creating shockwaves that propagate through the contrast medium, thereby causing the cutting device(s) to vibrate and assist in the cracking or abrading of the surrounding
25 plaque in contact with the balloon.

[0015] The contrast material commonly exhibits a high degree of optical absorption to the laser light. When a laser fiber or fibers inserted into the balloon interior emit optical energy into the contrast material, the material is believed to experience a rapid rate of energy absorption, creating the shockwave.

30 [0016] An assisted cutting balloon for performing balloon angioplasty, according to this disclosure, can include:

(a) a dilation balloon;

(b) one or more cutting devices operably positioned on an exterior of the dilation balloon; and

(c) a flexible wire waveguide connected at a distal end to the cutting device(s) and at a proximal end to an ultrasonic apparatus.

5 [0017] The ultrasonic apparatus can transmit ultrasonic waves through the flexible wire waveguide to the cutting device(s) causing the cutting device(s) to vibrate as and/or after the dilation balloon is inflated, thereby assisting in the cracking or abrading of the surrounding plaque in contact with the balloon.

10 [0018] The cutting device(s) can be a wire abrasive bound to an exterior of the dilation balloon.

[0019] In one application, wire or braid material is constructed with a diamond abrasive or other types of abrasive cutting material and is wrapped around a dilation balloon in a helical or other type of configuration. The wire or braided material is vibrated using high, low, or even ultrasonic waves transmitted to the wire or braided material via
15 local or remote methods, substantially enhancing the ability to cut or abrade the plaque.

[0020] The guide wire can be inserted into a vasculature system and moved past the target coronary segment, and the assisted cutting balloon translated over the guide wire to the target coronary segment.

[0021] In one procedure, the dilation balloon can be inflated with a contrast
20 medium. Specifically, a laser fiber and the assisted cutting balloon are translated along over the guide wire to the target coronary segment, with the distal end of the laser fiber terminating in the middle of the dilation balloon. A laser generator connected to a proximal end of the laser fiber emits laser light from the distal end of the laser fiber at a very short pulse duration, thereby creating shockwaves that propagate through the contrast
25 medium as the dilation balloon is inflating, causing the cutting device(s) to vibrate. The vibrations cause the cutting device(s) to cut or abrade harder or calcified portions of the plaque as the dilation balloon is inflating. The laser generator typically generates 308 nm laser light at pulse durations ranging from 120-140 nsec. While other types of laser generators can be employed, a common laser generator is an excimer laser.

30 [0022] To assist positioning within the body, the assisted cutting balloon, guide wire, and laser fiber can be enclosed in a multi-lumen catheter.

[0023] In another procedure, an ultrasonic apparatus having a flexible wire waveguide connected at a proximal end to the ultrasonic apparatus and connected at a

distal end to the cutting device(s) transmits ultrasonic waves through the flexible wire waveguide to the cutting device(s), causing the cutting device(s) to vibrate. The vibrating cutting device(s) cut the harder or calcified portions of the plaque as and/or after the dilation balloon is inflated.

5 [0024] In any of the above procedures, the balloon is commonly inflated to pressures ranging between about 1-30 atmospheres, 5-25 atmospheres, and 10-20 atmospheres.

[0025] The present disclosure can provide benefits relative to conventional cutting balloons. The use of vibration, at low, medium, or high frequencies, can enhance dramatically the performance of cutting balloons. Cutting device(s), particularly the wire
10 or braid materials constructed with diamond abrasives or other type of abrasive cutting materials, can cut, abrade, or otherwise modify plaque, particularly calcified or hard plaque, while leaving surrounding soft tissue and compliant balloon material substantially unaltered and undamaged. This can be a very effective method to assist in cracking or modifying plaque in arteries. The disclosure can avoid the need to inflate balloons to very
15 high pressures (*e.g.*, from about 15 to about 30 atms), thereby permitting the use of lower pressures (*e.g.*, typically no more than about 10 atms and even more typically no more than about 7.5 atms).

[0026] As used herein, “at least one,” “one or more,” and “and/or” are open-ended expressions that are both conjunctive and disjunctive in operation. For example, each of
20 the expressions “at least one of A, B and C,” “at least one of A, B, or C,” “one or more of A, B, and C,” “one or more of A, B, or C,” and “A, B, and/or C” means A alone, B alone, C alone, A and B together, A and C together, B and C together, or A, B and C together. When each one of A, B, and C in the above expressions refers to an element, such as X, Y, and Z, or class of elements, such as X1-Xm, Y1-Yn, and Z1-Zo, the phrase
25 is intended to refer to a single element selected from X, Y, and Z, a combination of elements selected from the same class (*e.g.*, X1 and X2) as well as a combination of elements selected from two or more classes (*e.g.*, Y1 and Z3).

[0027] It is to be noted that the term “a” or “an” entity refers to one or more of that entity. As such, the terms “a” (or “an”), “one or more,” and “at least one” can be used
30 interchangeably herein. It is also to be noted that the terms “comprising,” “including,” and “having” can be used interchangeably.

[0028] “Contrast medium” or “contrast media” is generally any substance used to change the imaging characteristics of a patient, thereby providing additional information

such as anatomical, morphological, and/or physiological. Contrast media can, for example, provide information regarding vasculature, vascular integrity, and/or qualitative assessment of vasculature function or operation. Positive contrast agents increase the attenuation of tissue, blood, urine, or outline spaces such as the gastrointestinal lumen or subarachnoid space. Two primary types of positive contrast agents are barium sulfate agents and various halogenated (*e.g.*, iodated) compounds. Negative contrast agents normally decrease attenuation by occupying a space, such as the bladder, gastrointestinal tract, or blood vessels. Negative contrast agents are typically gases, such as carbon dioxide and nitrous oxide. Another type of contrast media, namely MRI contrast agents, uses typically superparamagnetism. Finally, ultrasound contrast media, namely sonographic contrast agents, are typically composed of gas bubbles (air or perfluor gases) stabilized by a shell of phospholipids, surfactants, albumin, or polymers.

[0029] The term “means” as used herein shall be given its broadest possible interpretation in accordance with 35 U.S.C., Section 112, Paragraph 6. Accordingly, a claim incorporating the term “means” shall cover all structures, materials, or acts set forth herein, and all of the equivalents thereof. Further, the structures, materials or acts and the equivalents thereof, shall include all those described in the summary of the invention, brief description of the drawings, detailed description, abstract, and claims themselves.

[0030] “Ultrasound” refers to sound or other vibrations having an ultrasonic frequency, which is commonly a frequency above about 20 thousand cycles per second (20,000 Hz).

[0031] It should be understood that every maximum numerical limitation given throughout this disclosure is deemed to include each and every lower numerical limitation as an alternative, as if such lower numerical limitations were expressly written herein. Every minimum numerical limitation given throughout this disclosure is deemed to include each and every higher numerical limitation as an alternative, as if such higher numerical limitations were expressly written herein. Every numerical range given throughout this disclosure is deemed to include each and every narrower numerical range that falls within such broader numerical range, as if such narrower numerical ranges were all expressly written herein.

[0032] The preceding is a simplified summary of the disclosure to provide an understanding of some aspects of the disclosure. This summary is neither an extensive nor exhaustive overview of the disclosure and its various aspects, embodiments, and

configurations. It is intended neither to identify key or critical elements of the disclosure nor to delineate the scope of the disclosure but to present selected concepts of the disclosure in a simplified form as an introduction to the more detailed description presented below. As will be appreciated, other aspects, embodiments, and configurations of the disclosure are possible, utilizing alone or in combination, one or more of the features set forth above or described in detail below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0033] **FIG. 1** shows a schematic illustration of an embodiment of an assisted cutting balloon.

[0034] **FIG. 2** shows a schematic diagram of an embodiment of an ultrasonic generator apparatus.

[0035] **FIG. 3** shows a partial cross section view of a partially occluded artery with an assisted cutting balloon in place prior to inflation.

[0036] **FIG. 4** shows a partial cross section view of a partially occluded artery with an assisted cutting balloon in place and inflated.

[0037] **FIG. 5** shows a partial cross section view of a partially occluded artery with an assisted cutting balloon after deflation and ready for removal.

[0038] **FIG. 6** shows a schematic illustration of another embodiment of an assisted cutting balloon.

[0039] **FIG. 7** shows a schematic diagram of an embodiment of a laser generator apparatus.

[0040] The accompanying drawings are incorporated into and form a part of the specification to illustrate several examples of the present disclosure. These drawings, together with the description, explain the principles of the disclosure. The drawings simply illustrate preferred and alternative examples of how the disclosure can be made and used and are not to be construed as limiting the disclosure to only the illustrated and described examples. Further features and advantages will become apparent from the following, more detailed, description of the various aspects, embodiments, and configurations of the disclosure, as illustrated by the drawings referenced below.

DETAILED DESCRIPTION

[0041] **Figure 1** shows a schematic illustration of an embodiment of an assisted cutting balloon. Referring now to **FIG. 1**, Assisted Cutting Balloon **10** includes a Dilation Balloon **12**, which may be any conventional angioplasty balloon such as commonly used

by interventional cardiologists or radiologists, and a Wire Abrasive **14** mounted, attached, affixed, or otherwise bound, in a helical configuration, to the exterior of Dilation Balloon **12**. Wire Abrasive **14** may be one wire strand or many wire strands wrapped or braided together. The wire may be composed of any suitable material, with one or more metal and/or plastic fibers being typical. Diamond material or any other suitable abrasives may be used as an abrasive bonded to the wire. Diamond wire impregnated with diamond dust is relatively inexpensive and is readily available in various diameters and lengths. Multiple configurations of Dilation Balloon **12** may be used with different types of cutting wire or string wrap patterns or braids, such as diamond, cross-hatch, woven or unwoven mesh, reverse helical, longitudinal, radial, etc., around the exterior of the Dilation Balloon **12** and with different types of abrasive coated wire or cutting blades or atherotomes in a variety of geometrical shapes bonded or applied to Dilation Balloon **12**. Other cutting balloon configurations known to those of skill in the art may be employed as the Dilation Balloon **12**. Guide Wire **30** is inserted into the vasculature system of the subject and past Target Coronary Segment **32** (see **FIG. 3**). Assisted Cutting Balloon **10** is translated over Guide Wire **30** to Target Coronary Segment **32**.

[0042] **Figure 2** shows a schematic diagram of an embodiment of an ultrasonic generator apparatus. Referring now to **FIG. 2**, Ultrasonic Apparatus **16** includes a Piezoelectric Converter And Acoustic Horn **18** that operates with a resonant frequency. Piezoelectric Converter And Acoustic Horn **18** is driven by Ultrasonic Generator **20** at an adjustable resonant frequency or set of plural frequencies. The frequencies can be temporally fixed or varied during Assisted Cutting Balloon **12** operation. This ensures that resonance of Piezoelectric Converter And Acoustic Horn **18** is achieved despite minor alterations in the resonant frequency of the system. In addition, Ultrasonic Generator **20** has adjustable input power dial settings.

[0043] Flexible Wire Waveguide **22** is connected to Piezoelectric Converter And Acoustic Horn **18** at a Proximal End **24** and fixed tightly into the radiating face of Piezoelectric Converter And Acoustic Horn **18** ensuring a rigid connection between the two. Distal End **26** of Flexible Wire Waveguide **22** is rigidly connected to a Proximal End **28** of Wire Abrasive **14** (see **FIG. 1**). Other local or remote methods may be used to transmit high, low, or ultrasonic waves to Flexible Wire Waveguide **22** such as.

[0044] **Figure 3** shows a partial cross section view of a partially occluded artery with an assisted cutting balloon in place prior to inflation. Referring now to **FIG. 3**, Assisted

Cutting Balloon **10** has been translated over Guide Wire **30** to Target Coronary Segment **32**. The interior of Artery **34** is partially occluded with deposits of Plaque **36**.

[0045] **Figure 4** shows a partial cross section view of a partially occluded artery with an assisted cutting balloon in place and inflated. Referring now to **FIG. 4**, as Dilation Balloon **12** is inflated, Ultrasonic Apparatus **16** is powered on. Flexible Wire Waveguide **22** causes Wire Abrasive **14** to vibrate. Thus, as Wire Abrasive **14** of Dilation Balloon **12** comes into contact with Plaque **36**, Dilation Balloon **12** crushes the softer portions of Plaque **36** and the cutting action of Wire Abrasive **14**, which is enhanced due to the vibration imparted via Flexible Wire Waveguide **22**, cuts the harder or calcified portions of Plaque **36**. The enhanced cutting action reduces the inflation pressure necessary to 5 to 10 atmospheres which reduces the chance for damage to Artery **34**.

[0046] **Figure 5** shows a partial cross section view of a partially occluded artery with an assisted cutting balloon after deflation and ready for removal. Referring now to **FIG. 5**, Striations **38** can be seen in crushed Plaque **36** due to the cutting action of Wire Abrasive **14**. Assisted Cutting Balloon **10** is now ready for removal over Guide Wire **30**.

[0047] **Figure 6** shows a schematic illustration of another embodiment of an assisted cutting balloon. Referring now to **FIG. 6**, Assisted Cutting Balloon **50** includes a Dilation Balloon **52**, which may be any conventional angioplasty balloon such as commonly used by interventional cardiologists or radiologists, and a Wire Abrasive **54** mounted over or attached to Dilation Balloon **52**. Wire Abrasive **54** may be one wire strand or many wire strands braided together. Diamond material or any other suitable abrasives may be used as an abrasive bonded to the wire. Diamond wire impregnated with diamond dust is relatively inexpensive and is readily available in various diameters and lengths. Multiple configurations of Dilation Balloon **52** may be used with different types of wire wrap patterns or braids, such as diamond or cross-hatch, helical, etc., and with different types of abrasive coated wire or cutting blades in a variety of geometrical shapes bonded or applied to Dilation Balloon **12**. Guide Wire **70** is inserted into the subject and Assisted Cutting Balloon **50** is translated over Guide Wire **70** to a target coronary segment, such as Target Coronary Segment **32** shown in **FIG. 3**.

[0048] **Figure 7** shows a schematic diagram of an embodiment of a laser generator apparatus. Referring now to **FIG. 7**, a laser light source such as Laser Apparatus **56** includes a Laser Generator **58** controlled by a Computer **60**. Flexible Cladding **62** shields Laser Fiber **64**, which may be a single fiber or multiple fibers. Flexible Cladding **62** runs

parallel with Guide Wire **70** and both may be enclosed in a multi-lumen catheter along with Assisted Cutting Balloon **10**. Distal End **66** (see **FIG. 6**) of Flexible Cladding **62** terminates in the middle of Dilation Balloon **52**. Laser Fiber **64** extends a short distance from Distal End **66**. When Assisted Cutting Balloon **50** has been translated over Guide Wire **70** to a target coronary segment, it will appear like that shown in **FIG. 3**, where the interior of Artery **34** of Target Coronary Segment **32** is partially occluded with deposits of Plaque **36**.

[0049] Substituting now Assisted Cutting Balloon **50** for Assisted Cutting Balloon **10** shown in **FIG. 4**, Dilation Balloon **52** is inflated with Contrast Medium **68**. Contrast Medium **68** may be one of many different compounds as found in the ACR Manual of Contrast Media, Version 8, 2012. As Dilation Balloon **52** is inflated, Laser Apparatus **56** is activated, which, in one embodiment, may be an excimer laser that emits 308 nm laser light at very short pulse durations (120-140 nsec.) from Laser Fiber **64**. Contrast Medium **68** exhibits a very high absorption to this laser light. Due to the high absorption and short pulse width of the laser light, shockwaves are created that propagate through the volume of Contrast Medium **68** within Dilation Balloon **52**. The shockwaves assist in the cracking, crushing, or modification of Plaque **36** by Dilation Balloon **52**. The shockwave also causes Wire Abrasive **54** to vibrate. Thus, as Wire Abrasive **54** of Dilation Balloon **52** comes into contact with Plaque **36**, Dilation Balloon **52**, assisted by the shockwaves as well as by inflation, crushes the softer portions of Plaque **36**, and the cutting action of Wire Abrasive **54**, which is enhanced due to the vibration imparted via the shockwaves traveling through the volume of Contrast Medium **68**, cuts the harder or calcified portions of Plaque **36**. Dilation Balloon **52** is then deflated and ready for removal as shown in **FIG. 5**. Striations **38** will also be seen in crushed Plaque **36** due to the cutting action of Wire Abrasive **54**.

[0050] A number of variations and modifications of the disclosure can be used. It would be possible to provide for some features of the disclosure without providing others.

[0051] For example in one alternative embodiment, cutting blades may be used instead of abrasive wire.

[0052] In another example, other Assisted Cutting Balloon **12** vibrating mechanisms may be employed. Examples include mechanically induced vibration (e.g., by a micro-vibration motor), electrically induced vibration, electromechanically induced vibration

(e.g., by a micro-electromechanical system), magnetically induced vibration, electromagnetically induced vibration, and vibration induced by other sound or acoustical frequencies.

[0053] In another example, the vibration source may be positioned either remotely, as discussed and shown above, or locally, such as in the proximity of the balloon itself, or a combination thereof. Micro-components can be positioned in or near the balloon in the catheter itself whereby attenuation of vibrations remotely generated is reduced. For example, a micro-vibration motor, micro-electromechanical system, or micro-piezoelectric transducer can be positioned in the catheter in proximity to the balloon.

[0054] The present disclosure, in various aspects, embodiments, and configurations, includes components, methods, processes, systems and/or apparatus substantially as depicted and described herein, including various aspects, embodiments, configurations, subcombinations, and subsets thereof. Those of skill in the art will understand how to make and use the various aspects, embodiments, and configurations, after understanding the present disclosure. The present disclosure, in various aspects, embodiments, and configurations, includes providing devices and processes in the absence of items not depicted and/or described herein or in various aspects, embodiments, and configurations hereof, including in the absence of such items as may have been used in previous devices or processes, e.g., for improving performance, achieving ease and/or reducing cost of implementation.

[0055] The foregoing discussion of the disclosure has been presented for purposes of illustration and description. The foregoing is not intended to limit the disclosure to the form or forms disclosed herein. For example, in the foregoing Detailed Description, various features of the disclosure are grouped together in one or more, aspects, embodiments, and configurations for the purpose of streamlining the disclosure. The features of the aspects, embodiments, and configurations of the disclosure may be combined in alternate aspects, embodiments, and configurations other than those discussed above. This method of disclosure is not to be interpreted as reflecting an intention that the claimed disclosure requires more features than are expressly recited in each claim. Rather, as the following claims reflect, inventive aspects lie in less than all features of a single foregoing disclosed aspects, embodiments, and configurations. Thus, the following claims are hereby incorporated into this Detailed Description, with each claim standing on its own as a separate preferred embodiment of the disclosure.

[0056] Moreover, though the description of the disclosure has included descriptions of one or more aspects, embodiments, or configurations and certain variations and modifications, other variations, combinations, and modifications are within the scope of the disclosure, *e.g.*, as may be within the skill and knowledge of those in the art, after
5 understanding the present disclosure. It is intended to obtain rights which include alternative aspects, embodiments, and configurations to the extent permitted, including alternate, interchangeable and/or equivalent structures, functions, ranges or steps to those claimed, whether or not such alternate, interchangeable and/or equivalent structures, functions, ranges or steps are disclosed herein, and without intending to publicly dedicate
10 any patentable subject matter.

CLAIMS

What is claimed is:

1. A method for performing balloon angioplasty, the method comprising the steps of:

5 (a) inserting an assisted cutting balloon into a target coronary segment partially occluded with plaque, the assisted cutting balloon having a dilation balloon with one or more cutting devices operably positioned on an exterior of the dilation balloon;

(b) vibrating the one or more cutting devices; and

(c) inflating the dilation balloon;

10 whereby the expanding dilation balloon crushes the softer portions of the plaque and the vibrating one or more cutting devices cuts the harder or calcified portions of the plaque.

2. The method according to claim 1, wherein the one or more cutting devices comprise one or more wire abrasives bound to the exterior of the dilation balloon and
15 wherein step (a) further comprises the steps of:

inserting a guide wire into a vasculature system and past the target coronary segment; and

translating the assisted cutting balloon over the guide wire to the target coronary segment.

20 3. The method according to claim 2, wherein step (c) further comprises the step of:

inflating the dilation balloon with a contrast medium.

4. The method according to claim 3, further comprising the steps of:
translating a laser fiber along with the assisted cutting balloon over the guide wire to the
25 target coronary segment, the distal end of the laser fiber terminating in the middle of the dilation balloon;

powering on a laser generator connected to a proximal end of the laser fiber;
emitting laser light from the distal end of the laser fiber at very short pulse durations
creating shockwaves that propagate through the contrast medium as the dilation balloon is
30 inflating, causing the wire abrasive to vibrate; and

cutting by the wire abrasive as it vibrates the harder or calcified portions of the plaque as the dilation balloon is inflating.

5. The method according to claim 4, wherein the translating step further comprises the step of:

enclosing the assisted cutting balloon, the guide wire, and the laser fiber into a multi-lumen catheter.

5 6. The method according to claim 4, wherein the emitting step further comprises the step of:

generating, by the laser generator, 308 nm laser light at pulse durations ranging from 120-140 nsec that are emitted from the distal end of the laser fiber, wherein the laser generator is an excimer laser.

10 7. The method according to claim 4, further comprising the step of:

assisting the crushing of the softer portions of the plaque by the shockwaves propagating within the dilation balloon.

8. The method according to claim 1, wherein step (b) further comprises the steps of:

15 powering on an ultrasonic apparatus having a flexible wire waveguide connected at a proximal end to the ultrasonic apparatus, and connected at a distal end to the one or more cutting devices;

transmitting ultrasonic waves from the ultrasonic apparatus through the flexible wire waveguide to the one or more cutting devices, causing the one or more cutting
20 devices to vibrate; and

cutting by the one or more cutting devices as it vibrates the harder or calcified portions of the plaque as the dilation balloon is inflated.

9. The method according to claim 1 wherein step (c) further comprises the step of:

25 inflating the dilation balloon to a pressure ranging between 5 to 10 atmospheres.

10. An assisted cutting balloon for performing balloon angioplasty comprising: a dilation balloon;

one or more cutting devices operably positioned on an exterior of the dilation balloon; and

30 a flexible wire waveguide connected at a distal end to the one or more cutting devices and connected at a proximal end to an ultrasonic apparatus;

whereby the ultrasonic apparatus transmits ultrasonic waves through the flexible wire waveguide to the one or more cutting devices causing the one or more cutting devices to vibrate as and/or after the dilation balloon is inflated.

11. The assisted cutting balloon for performing balloon angioplasty according to claim 10, wherein the one or more cutting devices comprise a wire abrasive bound to an exterior of the dilation balloon and further comprising:

a guide wire for translating the assisted cutting balloon to a target coronary segment partially occluded with plaque, wherein the guide wire is inserted into a vasculature system and past the target coronary segment.

12. The assisted cutting balloon for performing balloon angioplasty according to claim 10, wherein the one or more cutting device during vibration cuts the harder or calcified portions of the plaque as the dilation balloon is inflated.

13. The assisted cutting balloon for performing balloon angioplasty according to claim 10, wherein the dilation balloon is inflated to a pressure ranging between 5 to 10 atmospheres.

14. The assisted cutting balloon for performing balloon angioplasty according to claim 11, wherein the wire abrasive is diamond dust, and the wire wrap pattern of the wire abrasive bound to the dilation balloon is one or more of diamond, cross-hatch, mesh, longitudinal, radial, and helical.

15. An assisted cutting balloon for performing balloon angioplasty comprising: a dilation balloon;

one or more cutting devices operably positioned on an exterior of the dilation balloon;

a laser light source terminating at a distal end in the interior of the dilation balloon; and

a contrast medium for inflating the dilation balloon;

whereby, as and/or after the dilation balloon is inflated with the contrast medium, the laser light source transmits pulsed laser light into the contrast medium creating shockwaves that propagate through the contrast medium causing the one or more cutting devices to vibrate.

16. The assisted cutting balloon for performing balloon angioplasty according to claim 15, wherein the one or more cutting devices comprise a wire abrasive bound to the exterior of the dilation balloon and further comprising:

a guide wire for translating the assisted cutting balloon and the laser light source to a target coronary segment partially occluded with plaque, wherein the guide wire is inserted into a vasculature system and past the target coronary segment.

17. The assisted cutting balloon for performing balloon angioplasty according to claim 15, wherein the laser light source further comprises:

a laser fiber translated along with the assisted cutting balloon to the target coronary segment;

a laser generator connected to a proximal end of the laser fiber and the distal end of the laser fiber terminates in the middle of the dilation balloon; and

10 a laser light emitted from the distal end of the laser fiber at very short pulse durations creating shockwaves that propagate through the contrast medium as the dilation balloon is inflating, causing the one or more cutting devices to vibrate, wherein, as the dilation balloon is inflated, the one or more cutting devices vibrate and cut harder or calcified portions of the plaque.

15 18. The assisted cutting balloon for performing balloon angioplasty according to claim 17, further comprising:

a multi-lumen catheter for enclosing the assisted cutting balloon, the guide wire, and the laser fiber.

19. The assisted cutting balloon for performing balloon angioplasty according to claim 15, wherein the laser light source is an excimer laser that generates 308 nm laser light at pulse durations ranging from 120-140 nsec.

20 20. The assisted cutting balloon for performing balloon angioplasty according to claim 16, wherein the wire abrasive is diamond dust, and the wire wrap pattern of the wire abrasive bound to the dilation balloon is one or more of diamond, cross-hatch, mesh, longitudinal, radial, and helical.

25

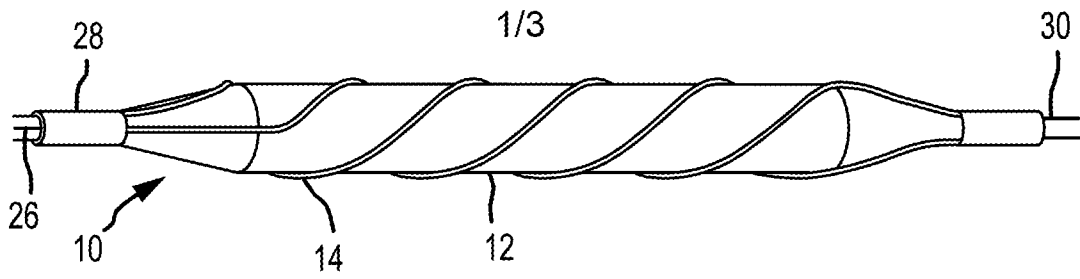


FIG. 1

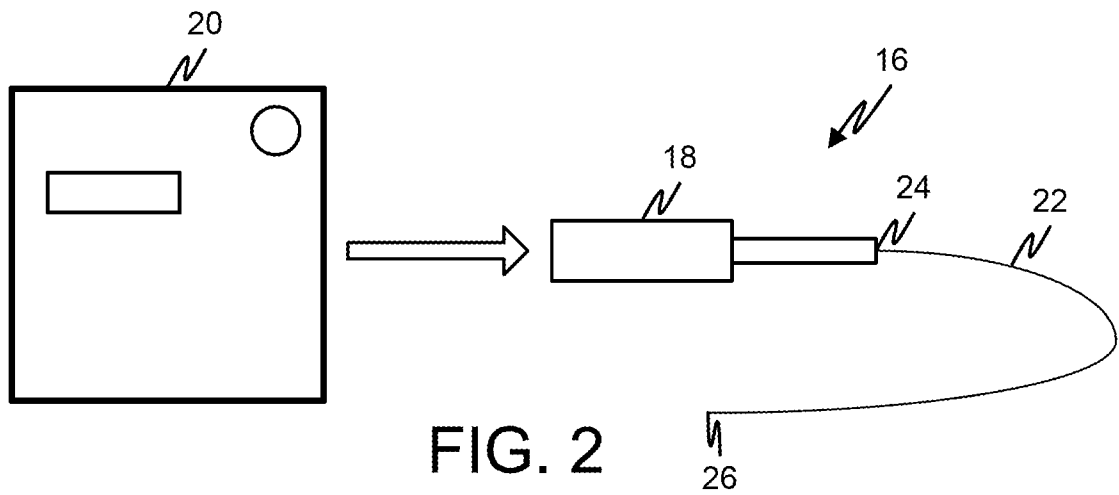


FIG. 2




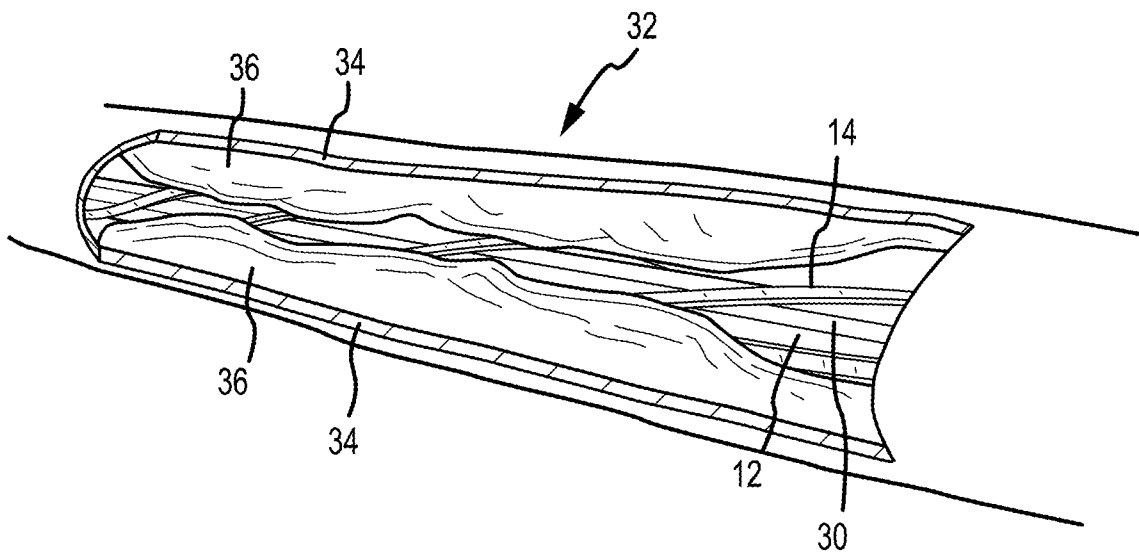


FIG. 3

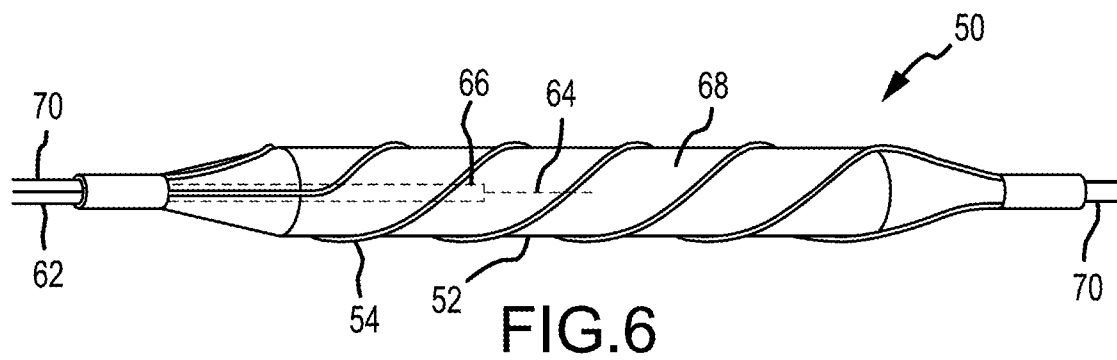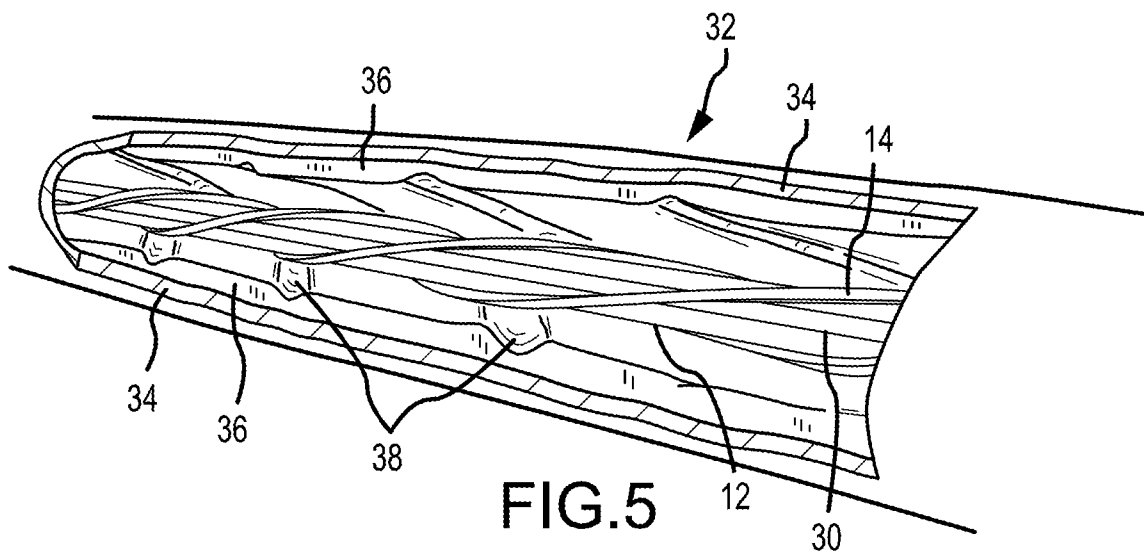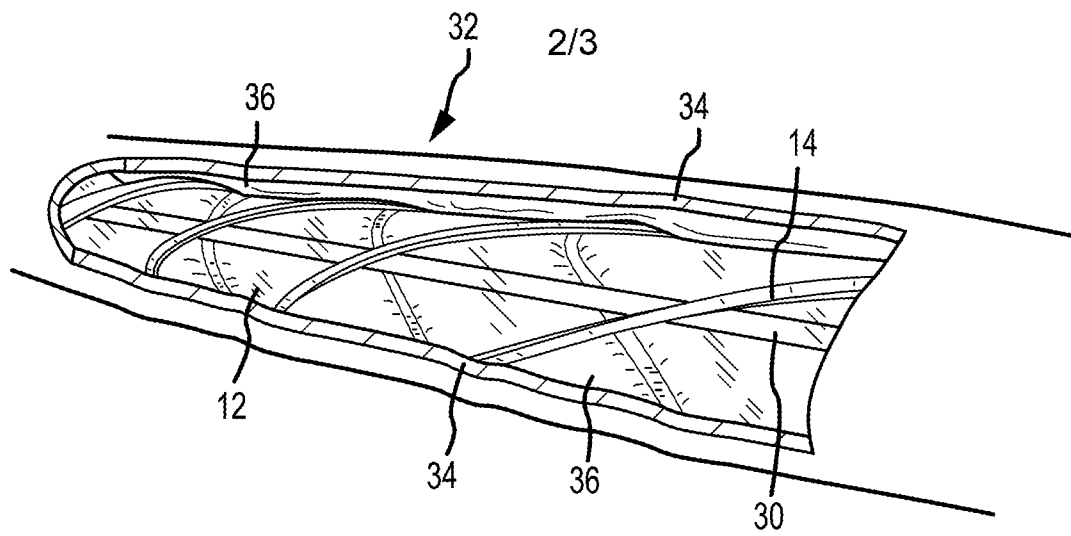

3/3

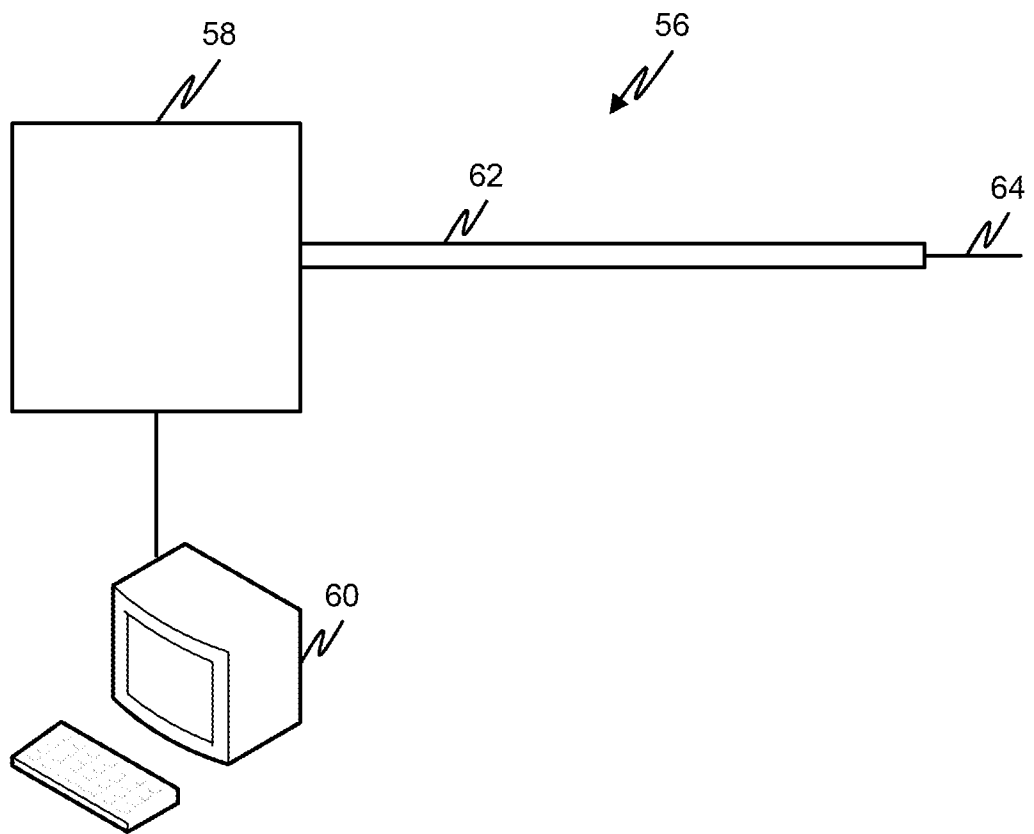


FIG. 7

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2014/019268**A. CLASSIFICATION OF SUBJECT MATTER****A61B 17/22(2006.01)i, A61B 17/3207(2006.01)i, A61M 25/10(2006.01)i, A61B 18/26(2006.01)i, A61M 25/09(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 17/22; A61M 29/00; A61B 17/221; A61M 37/00; A61B 6/00; C07D 301/12; A61B 17/3207; A61M 25/10; A61B 18/26; A61M 25/09

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: angioplasty, cutting device, dilation balloon, ultrasonic apparatus, laser light source, contrast medium, abrasive

C. DOCUMENTS CONSIDERED TO BE RELEVANT

| Category* | Citation of document, with indication, where appropriate, of the relevant passages | Relevant to claim No. |
|-----------|--|-----------------------|
| X | EP 0189329 A2 (FISCHELL, ROBERT E. et al.) 30 July 1986 See abstract; claims 1, 5-6 and 24; figure 5. | 10,12-13 |
| A | | 11,14-20 |
| A | US 2010-0222786 A1 (KASSAB, GHASSAN S.) 2 September 2010 See abstract; claims 32 and 34. | 10-20 |
| A | US 2009-0112239 A1 (TO, JOHN THAO) 30 April 2009 See abstract; claims 1 and 15; figure 7. | 10-20 |
| A | US 2011-0152683 A1 (GERRANS, LAWRENCE J. et al.) 23 June 2011 See abstract; claim 32. | 10-20 |
| A | US 2006-0189930 A1 (LARY, BANNING G. et al.) 24 August 2006 See abstract; claims 20-22; figure 5. | 10-20 |
| A | US 2007-0198047 A1 (SCHON, DONALD A. et al.) 23 August 2007 See abstract; claim 1; figure 1. | 10-20 |



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

12 June 2014 (12.06.2014)

Date of mailing of the international search report

13 June 2014 (13.06.2014)

Name and mailing address of the ISA/KR

International Application Division
Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City, 302-701,
Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

KIM, Eun Hee

Telephone No. +82-42-481-5543



INTERNATIONAL SEARCH REPORTInternational application No.
PCT/US2014/019268**Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 1-9
because they relate to subject matter not required to be searched by this Authority, namely:
Claims 1-9 pertain to methods for treatment of the human body by surgery, and thus relate to a subject matter which this International Searching Authority is not required, under Article 17(2)(a)(i) of the PCT and Rule 39.1(iv) of the Regulations under the PCT, to search.
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of any additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2014/019268

| Patent document cited in search report | Publication date | Patent family member(s) | Publication date |
|---|---------------------|--|--|
| EP 0189329 A2 | 30/07/1986 | EP 0189329 A2 EP 0189329 A3 | 30/07/1986 03/06/1987 |
| US 2010-0022786 A1 | 28/01/2010 | CN 101522653 A EP 2085393 A1 EP 2085393 A4 JP 2008-088106 A WO 2008-041654 A1 | 02/09/2009 05/08/2009 19/01/2011 17/04/2008 10/04/2008 |
| US 2009-0112239 A1 | 30/04/2009 | None | |
| US 2011-0152683 A1 | 23/06/2011 | EP 2495008 A1 US 2010-0121270 A1 US 2014-024903 A1 US 8226601 B2 US 8597239 B2 WO 2012-118919 A1 | 05/09/2012 13/05/2010 23/01/2014 24/07/2012 03/12/2013 07/09/2012 |
| US 2006-0189930 A1 | 24/08/2006 | CA 2452369 A1 EP 1409063 A1 EP 1409063 A4 JP 2004-533893 A US 2002-0010418 A1 US 2006-0189929 A1 US 7077836 B2 US 7985200 B2 WO 03-004087 A1 | 16/01/2003 21/04/2004 07/11/2007 11/11/2004 24/01/2002 24/08/2006 18/07/2006 26/07/2011 16/01/2003 |
| US 2007-0198047 A1 | 23/08/2007 | AT 551001 T CA 2633721 A1 EP 1962696 A2 EP 1962696 A4 EP 1962696 B1 JP 2009-520575 A US 2010-0241148 A1 WO 2007-075986 A2 WO 2007-075986 A3 | 15/04/2012 05/07/2007 03/09/2008 09/12/2009 28/03/2012 28/05/2009 23/09/2010 05/07/2007 07/05/2009 |

| | | | |
|----------------|---|---------|------------|
| 专利名称(译) | 辅助切割气球 | | |
| 公开(公告)号 | EP2967609A1 | 公开(公告)日 | 2016-01-20 |
| 申请号 | EP2014778867 | 申请日 | 2014-02-28 |
| [标]申请(专利权)人(译) | 斯佩克特尼克斯公司 | | |
| 申请(专利权)人(译) | THE SPECTRANETICS CORPORATION | | |
| 当前申请(专利权)人(译) | THE SPECTRANETICS CORPORATION | | |
| [标]发明人 | GRACE KENNETH P | | |
| 发明人 | GRACE, KENNETH, P. | | |
| IPC分类号 | A61B17/22 A61B17/3207 A61M25/10 A61B18/26 A61M25/09 | | |
| CPC分类号 | A61M25/104 A61B17/22 A61B17/22012 A61B17/2202 A61B17/320725 A61B18/26 A61B2017/22001 A61B2017/22014 A61B2017/22061 A61B2017/22062 A61B2017/22081 A61B2018/263 A61B2018/266 A61M2025/1088 A61M2025/109 | | |
| 优先权 | 13/800214 2013-03-13 US | | |
| 其他公开文献 | EP2967609A4 | | |
| 外部链接 | Espacenet | | |

摘要(译)

扩张球囊用一种或多种图案包裹在一起或多种图案中，所述线材或编织材料具有与其结合的金钢石磨料或其他研磨材料。金属丝或编织材料以一种或多种方式振动，以增强金属丝磨料的切割作用。可以使用通过局部或远程方法传递到线磨料的高，低或甚至超声波来振动线磨料。或者，扩张球囊可以用显示出对激光的高吸收的造影剂扩张。对比材料用激光纤维或插入球囊内部的纤维激光，产生大量的冲击波，振动球囊并有助于与扩张球囊接触的周围斑块的破裂或磨损。切割球囊可采用上述磨料涂覆的线或切割刀片。