


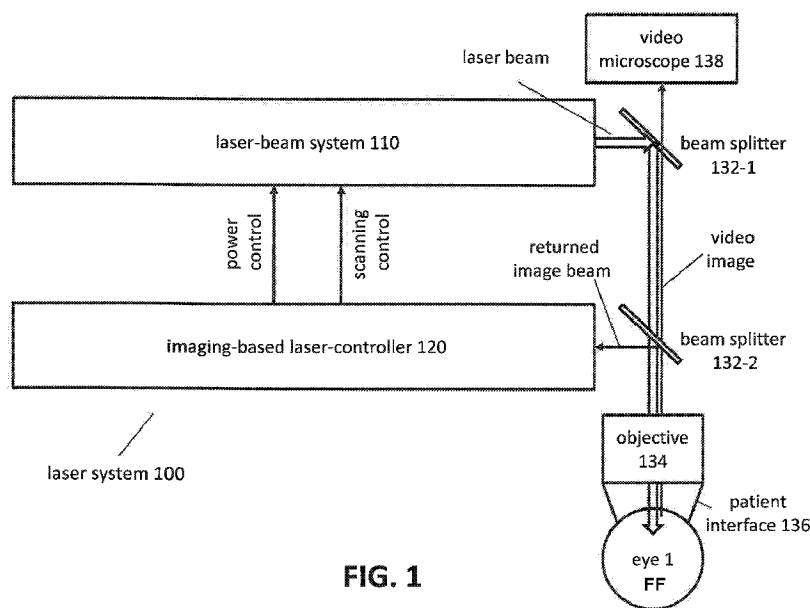

- (51) **International Patent Classification:**
A61F 9/008 (2006.01) *A61B 18/20* (2006.01)
- (21) **International Application Number:**
PCT/US2011/051360
- (22) **International Filing Date:**
13 September 2011 (13.09.2011)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
13/110,352 18 May 2011 (18.05.2011) US
- (71) **Applicant (for all designated States except US):** **ALCON LENSX, INC.** [US/US]; 33 Journey, Suite 175, Aliso Viejo, California 92656 (US).
- (72) **Inventors; and**
- (75) **Inventors/Applicants (for US only):** **CHAUDHARY, Gautam** [IN/US]; 22476 Caminito Esteban, Laguna Hills, California 92653 (US). **GOLDSTEIN, Peter** [US/US]; 10532 Boca Canyon Drive, Santa Ana, California 92705 (US). **HEGEDUS, Imre** [HU/HU]; Zoborhegy tér 7/a, H-1141 Budapest (HU). **SUÁREZ, Carlos German** [US/US]; 2544 Newman Avenue, Tustin, California 92782 (US).
- (74) **Agents:** **GERGELY T. ZIMANYI** et al.; Alcon Research, Ltd., IP Legal, 6201 South Freeway, Mail Code TB4-8, Fort Worth, Texas 76134-2099 (US).
- (81) **Designated States (unless otherwise indicated, for every kind of national protection available):** AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) **Designated States (unless otherwise indicated, for every kind of regional protection available):** ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) **Title:** IMAGING-CONTROLLED LASER SURGICAL SYSTEM**FIG. 1**

(57) **Abstract:** An imaging-based laser system can include a laser-beam system, configured to generate and scan a beam of laser pulses with an adjustable laser-power parameter to points of a scan-pattern in an eye, and an imaging-based laser-controller, configured to image a layer in the eye, to control the scanning of the beam of laser pulses to the points of the scan-pattern, and to control a laser-power parameter of the laser pulses according to the distance of the points of the scan-pattern from the imaged layer.

IMAGING-CONTROLLED LASER SURGICAL SYSTEM

CROSS REFERENCE TO RELATED APPLICATION

[0001] This application claims priority under 35 U.S.C. §119 to U.S. Patent Application Serial No. 13/110,352, filed May 18, 2011, the entire contents of which are
5 incorporated herein by reference.

TECHNICAL FIELD

[0002] This patent document describes a system and method for controlling a laser in an ophthalmic procedure. In more detail, this patent document describes an imaging-controlled laser system for controlling the power of a pulsed ophthalmic laser during
10 capsulotomy and cataract procedures, among others.

BACKGROUND

[0003] Laser systems have become essential for ophthalmic surgery. They have been employed in corneal procedures for some time now with high precision and therefore considerable success. In very recent times applications for other ophthalmic procedures
15 have been contemplated, including cataract procedures.

[0004] Lasers can be used for forming high precision cuts. These cuts are created by focusing or directing a rapid sequence of laser pulses to a scan-pattern or point-pattern. The points of the scan-pattern often form a line or layer and the laser pulses are directed to these points by a scanning system that includes deflection devices, mirrors and lenses
20 whose alignment can be changed very quickly. In typical laser systems the pulses can have a duration or pulse length in the nanosecond, picosecond, or even femtosecond range. The pulse repetition rate can be in the kHz to hundreds of kHz range.

[0005] The power or energy of the laser pulses can be chosen to exceed a so-called photodisruption threshold. Laser pulses with a power above this threshold can disrupt the
25 ophthalmic tissue at the target points, inducing the formation of bubbles. Lines or layers of these bubbles can weaken the mechanical connection between the tissue-portions on the opposite sides of the bubbles. Often the weakening is substantial, effectively cutting the

tissue. Therefore, a subsequent manual procedure can completely separate the tissue portions with ease.

[0006] One ophthalmic procedure which could benefit from using such a high precision laser cutting system is cataract surgery. A typical cataract surgery involves a capsulotomy step and a lysis or lens fragmentation step. During lysis, energy is applied to a lens nucleus to liquefy it. During lens fragmentation, or phaco-fragmentation, the nucleus of the lens can be cut into several pieces by scanning the laser along cutting surfaces to enable the subsequent piece-by-piece removal of the nucleus. The capsulotomy involves forming a circular cut on the anterior portion of the capsular bag of the lens to allow the surgeon to access and remove the cut-up pieces of the nucleus.

[0007] To optimize surgical laser systems for these complex ophthalmic procedures is a great challenge. However, the optimization promises great returns in terms of the precision and efficacy of the surgical procedures.

SUMMARY

[0008] One of the challenges of laser cataract surgery is that the procedures of capsulotomy and lens fragmentation can interfere with each other. In advanced laser systems the precision of the surgery can be enhanced by imaging the ophthalmic target tissue prior to the surgery and guide the laser pulses based on the image. If the lens fragmentation is performed first, then, as a surgical by-product, the capsule is expanded considerably and unevenly by the substantial amount of bubbles formed inside the capsule. Therefore, after the lens fragmentation, the capsule and lens has to be imaged for a second time to guide the subsequent circular cut of the capsulotomy. However, imaging the severely photodisrupted and distorted lens can be challenging. Also, the repeated imaging procedure consumes precious surgical time, increasing the discomfort of the patient, potentially undermining the precision of the entire procedure.

[0009] On the other hand, if the capsulotomy is performed first, it creates a substantial amount of bubbles in the anterior region of the lens and in the anterior aqueous chamber of the eye. The amount of bubbles is especially high if the lens is in a tilted position before the procedure, as explained below. These bubbles can increase the scattering of the laser pulses of the subsequent lens fragmentation considerably as the subsequent pulses are directed to the inside of the lens and thus propagate through the bubble-rich anterior region. The increased scattering can again potentially undermine the precision of the cataract procedure.

[0010] Thus, both sequences of the lens fragmentation and capsulotomy have drawbacks, as the first step can reduce the precision and control of the subsequent step. Therefore, laser systems that reduce, resolve, or eliminate one or more of these drawbacks can offer advantages.

[0011] Embodiments of the present invention can provide advantageous functionalities in view of these challenges. In particular, an embodiment of an imaging-based laser system can include a laser-beam system, configured to generate and scan a beam of laser pulses with an adjustable laser-power parameter to points of a scan-pattern in an eye, and an imaging-based laser-controller, configured to image a layer in the eye, to control the scanning of the beam of laser pulses to the points of the scan-pattern, and to control a

laser-power parameter of the laser pulses according to the distance of the points of the scan-pattern from the imaged layer.

[0012] An implementation of an imaging-based laser system can include a laser that generates and directs a beam of laser pulses into an eye, an imaging system that images a capsule layer of the eye, and a laser control system that controls the laser to direct the beam to spots within a tracking band of the imaged capsule layer with a laser-power parameter above a photo-disruption threshold, and to spots outside the tracking band of the imaged capsule layer with a laser-power parameter below a photo-disruption threshold, wherein the image-based laser system is configured to perform a capsulotomy before a lysis or lens- or phaco-fragmentation during a cataract procedure.

[0013] An implementation of an image-guided ophthalmic laser system can include a laser engine, configured to generate laser pulses, a beam modifier, configured to modify a laser-power parameter of the laser pulses, a laser scanner, configured to direct the laser pulses to scanning-points in an eye, an imaging system, configured to image a region in the eye, and a pattern generator, coupled to the imaging system, the beam modifier and the laser scanner, configured to generate coordinates of the scanning-points for the laser scanner, and to associate a laser-power parameter with the scanning-points depending on a distance of the scanning-points from a target-pattern.

[0014] In some implementations, a method of performing an imaging-controlled ophthalmic procedure can include imaging a layer in an eye, generating coordinates of points of a scan-pattern, determining a distance of the points of the scan-pattern from the imaged layer, and associating laser-power parameters with the points based on the determined distance.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015] **FIG. 1** illustrates an embodiment of a surgical laser system with an imaging-controlled laser system

[0016] **FIGS. 2A-D** illustrate embodiments of the laser-beam system.

5 [0017] **FIGS. 3A-E** illustrate embodiments of the imaging-based laser controller.

[0018] **FIGS. 4A-B** illustrate the scan-patterns for non-tilted and tilted lenses.

[0019] **FIGS. 5A-B** illustrate traditional scan-patterns for non-tilted and tilted lenses as a function of a scanning variable.

10 [0020] **FIGS. 6A-H** illustrate a scan-pattern along a circular scan with a distance-dependent laser-power parameter.

[0021] **FIG. 7** illustrates a determination of the z-depth of the imaged layer by using a model curve.

[0022] **FIG. 8A-B** illustrate methods of cataract surgery with the lens fragmentation and capsulotomy in different sequences.

15 [0023] **FIG. 9** illustrates a method of cataract surgery with an imaging-controlled laser system in detail.

[0024] **FIG. 10** illustrates a multi-extrema tracking-band laser scan-pattern after lens-fragmentation expanded the lens capsule in a non-uniform manner.

[0025] **FIGS. 11A-D** illustrate scan-patterns for tilted chop cuts.

20 [0026] **FIGS. 12A-B** illustrate scan-patterns for tilted volume cuts.

DETAILED DESCRIPTION

[0027] Implementations and embodiments described in this patent document offer improvements for the above described challenges.

[0028] FIG. 1 illustrates an imaging-based laser system 100, including a laser-beam system 110 to generate and scan a beam of laser pulses with an adjustable laser-power parameter to points of a scan-pattern in an eye 1, and an imaging-based laser-controller 120 to image a layer in the eye, to control the scanning of the beam of laser pulses to the points of the scan-pattern, and to control a laser-power parameter of the laser pulses according to the distance of the points of the scan-pattern from the imaged layer. The laser-controller 120 can perform these functions by sending a power control signal and a scanning control signal to the laser-beam system 110, for example.

[0029] The laser beam of the laser-beam system 110 can be guided into the main optical pathway at a beam-splitter 132-1 that can redirect the beam to an objective 134. The beam can propagate through the objective 134 and through a patient interface 136 to enter into the surgical eye 1.

[0030] The surgery can be assisted by imaging the eye 1 with various techniques. A visible imaging light can be used to create a video image that is processed by a video microscope 138. In addition, the imaging-based laser-controller 120 can shine an imaging beam on the eye and form an image based on the returned image beam. This imaging beam can be coupled into and out of the main optical path by a beam-splitter 132-2.

[0031] FIGS. 2A-D illustrate various embodiments of the laser-beam system 110.

[0032] FIG. 2A illustrates that embodiments of the laser-beam system 110 can include a laser engine 112 to generate the beam of laser pulses, a beam attenuator 114 to modify the laser-power parameter of the laser pulses, and a beam scanner 116 to direct the beam of laser pulses to the points of the scan-pattern in the eye. The laser engine 112 can generate laser pulses with a duration of nanoseconds, picoseconds or even femtoseconds, i.e. in the $10^{-9} - 10^{-15}$ sec range. These pulses can be generated at a repetition rate in a wide range of frequencies: from 0.1 kHz to 1,000 kHz, or in a range of 1 kHz to 500 kHz, or in some implementations in the 10 kHz to 100 kHz range. The power control signal of

the laser-controller 120 can be coupled into the beam attenuator 114 and the scanning control signal of the laser-controller 120 can be coupled into the beam scanner 116.

[0033] The beam attenuator 114 can include a Pockels cell, a polarizer-assembly, a mechanical shutter, an electro-mechanical shutter, or an energy wheel. Each of these implementations can modify a laser-power parameter of the laser pulses. The laser-power parameter can be a pulse energy, a pulse power, a pulse length or a pulse repetition rate of the laser pulses, among others. The beam attenuator 114 can modify one or more of these laser-power parameters. In a simple implementation, the beam attenuator 114 can shutter or block selected laser pulses. In another, a polarizer assembly can reduce the power of selected laser pulses by adjusting the relative angle of subsequent polarizing filters.

[0034] In the embodiment of **FIG. 2A**, the beam attenuator 114 can be located between the laser engine 112 and the beam scanner 116 in the path of the laser beam.

[0035] **FIG. 2B** illustrates and embodiment in which the beam attenuator 114 is at least partially integrated into the laser engine 112. In some cases, the beam attenuator 114 can be part of the laser engine 112. For example, a Pockels cell within the laser engine 112 can be the beam attenuator 114.

[0036] **FIG. 2C** illustrates and embodiment in which the beam attenuator 114 is located after the beam scanner 116 in the path of the laser beam.

[0037] Finally, **FIG. 2D** illustrates an embodiment in which the beam attenuator 114 and the beam scanner 116 are at least partially integrated.

[0038] **FIGS. 3A-E** illustrate various embodiments of the imaging-based laser-controller 120.

[0039] **FIG. 3A** illustrates that the laser-controller 120 can include an imaging system 122 to image the imaged layer in the eye and a pattern generator 124 to generate coordinates of the points of the scan-pattern, to associate laser-power parameters with the points depending on the distance of the points from the imaged layer, and to signal the generated coordinates of the points and the corresponding laser-power parameters to the laser-beam system 110. In some implementations, the imaging system 122 can image any

ophthalmic target in the anterior or posterior segment of the eye, targets from the cornea to the retina.

[0040] The pattern generator 124 can signal the generated coordinates of the points of the scan-pattern to the beam scanner 116 with a scanning control signal. Further, the
5 pattern generator 124 can signal the laser-power parameters corresponding to the points of the scan-pattern to the beam attenuator 114 with a power control signal. The laser-power parameter can be a pulse energy, a pulse power, a pulse length or a pulse repetition rate of the laser pulses.

[0041] The imaging system 122 can include an ophthalmic coherence tomography
10 (OCT) system, a Scheimpflug imaging system, a scanning imaging system, a single shot imaging system, an ultrasound imaging system, and a video imaging system. Here, the scanning imaging systems can create the image by scanning an imaging beam, whereas single shot imaging systems can acquire imaging information about an imaged area or volume in a single shot. The OCT system can be a time-domain OCT, a frequency-
15 domain OCT, or a spectrometer-based OCT system, among others.

[0042] FIG. 3B illustrates that in some implementations the laser-controller 120 can include an image-analyzer 126. The image analyzer 126 can receive the image of the imaged layer from the imaging system 122, perform an analysis of the imaged layer as described below and forward the result of the analysis to the pattern generator 124.

20 [0043] FIG. 3C illustrates that in some implementations the image analyzer 126 can be at least partially integrated with the imaging system 122. FIG. 3D illustrates that in some implementations the image analyzer 126 can be at least partially integrated with the pattern generator 124.

[0044] FIG. 3E illustrates that in some embodiments, the laser system 100 can
25 include an operator-interface 128 that can be coupled to one or more of the imaging system 122, the pattern generator 124 and the image analyzer 126.

[0045] FIGS. 4A-B set the stage to illustrate the operation of the laser system 100. The imaging system 122 can image the imaged layer in an image region that can be based on a loop, an arc, a line, or a two-dimensional pattern transverse to a z-axis of the imaging
30 system, and extends to a depth range D_{image} along the z-axis of the imaging system. The

imaging system 122 can support a determination of a z-depth coordinate of the imaged layer corresponding to a scanning coordinate along an image-scan.

[0046] FIG. 4A illustrates that the imaging system 122 can perform an imaging relevant for a capsulotomy step of a cataract procedure. The schematic cross section illustrates the anterior segment of the eye 1. The outermost layer is a cornea 210. A crystalline lens 220 is located behind the cornea 210, separated from it by an aqueous anterior chamber 230. The crystalline lens 220 is encapsulated in a thin capsule or capsular bag 222. The lens 220 is held in place by ciliary muscles 240. These muscles 240 also adjust the shape of the crystalline lens 220 as needed for bringing objects into focus.

[0047] As it has been described above, in order to facilitate the removal of a fragmented nucleus of the lens 220, the cataract surgery typically involves creating a circular capsulotomy cut 250 on the capsular bag 222. As a first step, the imaging system 122 can create an image 252 of the anterior segment of the eye by scanning along a scanning circle 254 and imaging the eye in a depth-range Dimage, defining an image-cylinder 260-i.

[0048] FIG. 5A illustrates that the image 252 typically includes an image 256 of the imaged anterior capsule layer of the lens 220 “unfolded” along a scanning variable, such as an angle along the circumference of the scanning circle 254. If a z-axis of the lens 220 is aligned with a z-axis of the laser system 100, the image 256 of the imaged layer is a flat line, indicating an essentially constant z-depth.

[0049] In other implementations, the image 252 can include the image of other ophthalmic targets, including corneal layers, portions of the sclera and even retinal layers. The zero depth level can be defined in a large number of ways, using a lens of the objective 134, a reference mirror of the imaging system 122, a level of the patient interface 136, or a level of an ophthalmic structure, such as the cornea 210.

[0050] By analyzing the image 252, a surgeon can recognize the image 256 of the imaged layer. Based on the z-depth of the imaged layer, the surgeon can decide where to direct the cutting laser beam to form the capsulotomy cut 250. The cutting laser beam is typically scanned along the same scanning circle 254 to form a cut-cylinder 260-c with a depth-range Dcut, typically smaller than Dimage. This way the placement of the cut-

cylinder 260-c benefits maximally from the information contained in the image 252, and in particular in the image 256 of the imaged layer. The capsulotomy cut 250 is formed where the cut-cylinder 260-c intersects the lens capsule 222. In practice, the cut cylinder 260-c is often formed as a stack of bubble-circles, where the individual circles are created
5 by directing the laser pulses along a circular scan-pattern at a fixed z-depth to cause photodisruption, followed by the formation of a similar circle at a slightly lesser z-depth.

[0051] In some typical cases, the image depth-range D_{image} can be 5 - 10 millimeters, whereas the cut depth-range D_{cut} can be in the range of 50 – 200 microns, in some cases 75 -150 microns, sometimes approximately 100 microns.

10 [0052] It is noted that the bubbles of the cut-cylinder 260-c can scatter and deflect laser pulses applied in subsequent surgical steps. For example, in a cataract surgery the capsulotomy can be followed by the lens fragmentation or lysis. The bubbles of the cut-cylinder 260-c can negatively impact the precision and efficiency of this subsequent lens-fragmentation by scattering the lens-fragmenting laser pulses.

15 [0053] Fortunately, when a z-axis of the lens 220 is parallel to a z-axis of the laser system 100, the depth range D_{cut} of the cut cylinder 260-c can be as little as 100 microns, creating only a limited number of bubbles. Thus, in the case of a well-aligned lens 220, the bubbles of the cut-cylinder 260-c introduce only a limited amount of scatter for the subsequent lens fragmentation laser pulses.

20 [0054] FIG. 4B illustrates, however, that in the typical surgical case the crystalline lens 220 can be tilted. This situation can occur for a variety of reasons. For example, the weight of the objective 134 can push the lens 220 sideways upon docking to the eye 1. Or, applying suction at the patient interface 136 to immobilize the eye 1 can lead to a tilting of the lens 220 as well.

25 [0055] FIG. 5B illustrates the image 252 of such a tilted lens 220 unfolded along the angular scanning variable of the scanning circle 254. In contrast to the non-tilted case of FIG. 5A, the image 256 of the tilted imaged layer can exhibit substantial sinusoidal oscillations. The amplitude of these oscillations can be as much as 300 – 500 microns. To make sure that the capsular bag 222 is cut everywhere along this sinusoid, the cut-cylinder
30 260-c can be formed with a much enlarged depth-range D_{cut} , exceeding the amplitude of the sinusoid. In the above example, D_{cut} can be 400 – 600 microns to be sure that the

capsular bag 222 was cut along the entire sinusoid. Clearly, this approach may create 4 – 6 times more photodisrupted bubbles during capsulotomy than the procedure for a non-tilted lens. Capsulotomy bubbles in such an increased number can scatter the laser pulses of the subsequent lens fragmentation to a substantial degree, threatening its precision and efficacy.

[0056] FIGS. 6A-H illustrate that some implementations of the laser system 100 can substantially reduce the number of photodisrupted bubbles by generating bubbles only in a narrow proximity of the imaged layer.

[0057] As described above, this outcome can be achieved, for example, by the imaging-based laser-controller 120 imaging the capsular bag 222, controlling the scanning of the beam of laser pulses to the points of the scan-pattern, and controlling a laser-power parameter of the laser pulses according to the distance of the points of the scan-pattern from the imaged layer.

[0058] FIGS. 6A-B illustrate that as the laser pulses are directed to points of the scan-pattern, the laser controller 120 can modify or adjust a laser-power parameter of the pulses. In particular, when a laser pulse is directed to a point of the scan pattern that is within a D_{cut} distance from the image 256 of the imaged layer along the z axis, the laser-controller 120 can adjust its laser-power parameter to a high value, e.g. above a photodisruption threshold. Whereas, when a laser pulse is directed to a point of the scan pattern that is farther than D_{cut} from the image 256 of the imaged layer, the laser-controller 120 can adjust its laser-power parameter value to a low value, such as below a photodisruption threshold.

[0059] The just-described method creates bubbles only in a D_{cut} proximity of the imaged layer and therefore substantially reduces the number of bubbles to a value close to the number of bubbles for a well-aligned lens. For this reason, the scattering of the subsequent lens-fragmenting laser pulses by these capsulotomy bubbles is substantially reduced. Using the earlier value of D_{cut} being 400 – 600 microns for a tilted lens and 100 microns for a non-tilted lens, the present method may reduce the scattering of the lens-fragmenting bubbles by a factor of 4 – 6: a considerable gain in precision and control.

[0060] FIG. 6A illustrates the implementation when the scanning of the capsulotomy laser pulses of the scan-pattern is performed along the z-axis for fixed points of the

circular scan. **FIG. 6B** illustrates the implementation when the scanning is performed along the circular scan with a fixed z-depth. This implementation can be used to create the above mentioned stacked circles. In either implementation, the points with high laser-power are placed within a tracking band 257 with a z-extent of D_{cut} .

5 **[0061] FIGS. 6C-E** illustrate the implementation when the laser pulses are scanned at fixed z-depths along the circular scan. A tracking band 257 can be defined as the set of points of the scan-pattern that are within the preselected distance D_{cut} from the image 256 of the imaged layer.

10 **[0062] FIGS. 6D-E** illustrate the laser power parameter of the pulses along the circular scan at two selected z-depths of 3600 microns and 3650 microns in an unfolded representation. The laser-controller 120 can control the laser power of the pulses that are directed to points inside the tracking band 257 to be above a photo-disruption threshold, and the laser power of the pulses that are directed to points outside the tracking band 257 to be below the photo-disruption threshold. In this embodiment, photodisrupted bubbles
15 are only generated at points within the tracking band 257, achieving the above functionality of the laser system 100.

20 **[0063] FIG. 6F** expresses the same operation in a folded representation. Here the value of the laser power parameter is shown as a function of the angular scanning variable (typically the angle), projected on the scanning circle 254 itself. Again, for those points of the scan-pattern that lie within the tracking band 257, the laser power is high - indicated by a thick line - whereas for those points that lie outside the tracking band 257, the laser power is low.

25 **[0064] FIGS. 6G-H** illustrate a related implementation, where the laser-power controller 120 controls the laser power parameter as a function of the distance of the points from the imaged layer, wherein the laser-power is a decreasing function of the distance. **FIG. 6G** illustrates the implementation where this function is essentially a two-valued step-function. **FIG. 6H** illustrates the implementation where this function is a continuous function, its value decaying with the increasing distance from the imaged layer. In some implementations, it may be easier to control the laser power in the continuous manner of
30 **FIG. 6H.**

[0065] The above-outlined implementations depend on the knowledge of the distance between the points of the scan-pattern and the imaged layer. Three stages are involved in determining this distance. First, the identity of the imaged layer is identified in the image 252 to determine the image 256 of the imaged layer. Then, the z-depth coordinate of the imaged layer is determined. Finally, the distance of the imaged layer and the points of the scan-pattern can be determined, for example, by taking the difference of the z-depth coordinates of the points of the scan-pattern and the imaged layer at the corresponding angular scanning coordinates, such as at the same angle.

[0066] Concerning the first step, the raw image 252 does not isolate or identify the imaged layer explicitly. Thus, establishing the identity of the imaged layer may necessitate an analysis of the image 252. As discussed earlier, this analysis of the image can be performed by the imaging system 122, the pattern generator 124, or the image analyzer 126, possibly assisted by an input from a system operator through the operator interface 128.

[0067] FIG. 7 illustrates that the imaging system 122 can support the identification of the imaged layer and the determination of its z-depth coordinates in different ways. In some implementations the laser system 100 can include the operator interface 128 and the imaging system 122 can support the identification of the imaged layer using an input from an operator through the operator interface 128.

[0068] For example, on a graphical user interface, or GUI, the operator interface 128 can prompt the operator to fit a model curve 258 to the spots in the image 252 representing the imaged layer. Since in the case of a tilted ellipsoid-shaped lens the image 256 of the imaged layer is typically a sinusoidal curve, the operator interface 128 can display a generic sinusoidal curve 258 on the GUI and prompt the operator to fit this model curve 258 to the layer-spots in the image 252. Once the operator fitted the model curve 258 to the layer-spots in the image 252, the model curve 258 can serve as the image 256 of the imaged layer.

[0069] The operator can achieve this task through various approaches: by shifting the model curve 258 by an Xshift in the X direction (i.e. adjusting the angle along the circular scan) and by shifting the model curve 258 by a Yshift in the Y direction (i.e. adjusting the z-depth coordinate). In other implementations the operator can be prompted to adjust the

scale of the model curve 258 to the scale of the sinusoidally located layer-spots in the image 252, i.e. to rescale the z-depth of the model curve 258 to fit the z-depth of the layer-spots. Many other fitting techniques can be implemented to achieve analogous functionalities.

5 **[0070]** The operator interface 128 can receive the input from the operator in many different ways, including through a keyboard, a touch-screen, a computer-communication channel, an external memory, a flash-drive, an internet connection, a speech-recognition apparatus or a wireless connection.

10 **[0071]** In other implementations, the determination of the identity and the z-depth of the imaged layer can be performed by the laser system 100 without the input of a surgeon or operator. In particular, the imaging system 122 can be configured to determine the identity and then the z-depth coordinate of the imaged layer by a processor or micro-computer performing a feature-recognition analysis of the image 252. For example, the imaging system 122 can determine the identity and coordinates of the imaged layer by
15 locating local maxima of the gradient of the spot intensity. In other implementations, an edge-recognition algorithm can be used. In these implementations, the imaging system 122 can identify the manifold of the maximum-gradient points as the image 256 of the imaged layer without resorting to fitting a model curve 258. In some implementations, of course, the imaging system 122 can make use of a model curve 258 to identify the image
20 256 of the imaged layer.

[0072] In the above implementations, once the identity of the imaged layer has been determined in the image 252, the z-depth coordinates of the imaged layer can be determined in a straightforward manner, for example, by counting the pixels in the image 252, or using a reference or a look-up table.

25 **[0073]** For the image analysis, the imaging system 122 can utilize a result of a pre-surgery measurement, statistical data, video image data, ophthalmic coherence tomography image data, or a model-based computation during the determination of the z-depth.

[0074] Once the z-depth of the imaged layer has been determined, the imaging system
30 122 can forward the z-depth and the corresponding scanning coordinates of the imaged layer to the pattern generator 124 to carry out the last stage, the determination of the

distance between the imaged layer and the points of the scan-pattern, generated by the pattern generator 124. This stage can be carried out, for example, by subtracting the z-depth coordinates of the points of the scan-pattern from the z-depth coordinates of the imaged layer that correspond to the same scanning variable, such as the same scanning angle.

[0075] Finally, having determined the distance of the points of the scan-pattern from the imaged layer, the pattern generator 124 can associate a laser-power parameter above a photodisruption threshold with those points that are closer to the imaged layer than a predetermined distance, and associate a laser-power parameter below a photodisruption threshold with those points that are farther from the imaged layer than the predetermined distance, as described in relation to **FIGS. 6A-H**.

[0076] In some implementations, the imaging system 122 only captures the image 252 but does not identify the imaged layer or determine its z-depth coordinates. In these embodiments, the imaging system 122 can simply forward the unprocessed image 252 to the pattern generator 124 without analyzing it. The pattern generator 124 can receive the image 252, identify the imaged layer and determine the z-depth coordinate of the imaged layer corresponding to a scanning coordinate along an image scan.

[0077] As above, in some implementations, the pattern generator 124 can determine the z-depth of the imaged layer by performing a feature-recognition analysis of the received image 252. In other implementations, the pattern generator 124 can receive an operator input through the operator interface 128 during the process of determining the z-depth of the imaged layer, as described before.

[0078] In these implementations, once the z-depth coordinates of the imaged layer have been determined, the pattern generator 124 can define a tracking band 257 as a manifold of the points of the scan-pattern that are within a predefined distance from the coordinates of the imaged layer. Then the pattern generator 124 can associate a laser-power parameter above a photodisruption threshold with points of the scan-pattern inside the tracking band 257, and a laser-power parameter below a photodisruption threshold with points of the scan-pattern outside the tracking band 257.

[0079] Yet other implementations of the laser controller 120 may include an image analyzer 126 that can determine the z-depth coordinate of the imaged layer corresponding

to a scanning coordinate along an image-scan. As was illustrated in **FIGS. 3B-D**, the image analyzer 126 can be self-standing or at least partially integrated with the imaging system 122 or the pattern generator 124.

5 **[0080]** The image analyzer 126 can identify the imaged layer and determine the z-depth coordinate of the imaged layer by performing a feature-recognition analysis of the image 252. In other implementations, the image analyzer 126 can determine the z-depth coordinate by making use of an operator input through an operator-interface 128.

10 **[0081]** The operation of the laser system 100 can be demonstrated on the example of the capsulotomy procedure, where the imaged layer is the lens capsule 222 between the lens 220 and the aqueous anterior chamber 230. In this case, the scan-pattern corresponds to the cut-cylinder 260-c intersecting the lens capsule 222 at the capsulotomy cut 250. The pattern generator 124 can associate a photodisruptive laser-power parameter with points inside a tracking band 257 related to the intersection 250 of the cut-cylinder 260-c and the lens capsule 222, and a non-photodisruptive laser-power parameter with points
15 outside the tracking band 257.

20 **[0082]** **FIG. 8A** illustrates a first cataract procedure 300 performed without the benefits of the laser system 100. The cataract procedure 300 can be practiced when the capsulotomy generates an excessive number of bubbles as in **FIGS. 4B - 5B**. To prevent excessive scattering by these capsulotomy bubbles, the lens fragmentation is performed prior to the capsulotomy. In detail, the cataract procedure 300 can include a first imaging 310 of the capsule 222, performed by an OCT procedure, followed by a lens fragmentation 320. During the lens fragmentation 320 the capsule 222 expands because of the large number of bubbles generated in the crystalline lens 220. The fragments of the lens 220 are removed through an opening, cut into the capsule 222 by a capsulotomy 340. However,
25 since the capsule 222 has expanded during the lens fragmentation 320, the results of the first imaging 310 are not reliable anymore. Therefore, the capsulotomy 340 has to be preceded by a second imaging 330. The second imaging 330 can take up precious surgical time and increase the discomfort of the patient. Both of these factors can endanger the efficacy of the cataract procedure 300.

30 **[0083]** **FIG. 8B** illustrates a cataract procedure 350 with an embodiment of the laser system 100. Since the laser system 100 is capable of creating only a limited number of

bubbles during the capsulotomy, the capsulotomy can be performed before the lens fragmentation. This change of sequence can reduce the surgical time to a considerable degree and thus increase the precision of the cataract procedure substantially.

[0084] In some detail, the cataract procedure 350 can include an imaging 360 of the capsule 222, e.g. by an OCT imaging system, followed by a capsulotomy 370, and completed by a lens fragmentation 380. Since the capsulotomy 370 does not deform the lens 220, there is no need for a second imaging, in contrast to the procedure 300.

[0085] FIG. 9 illustrates an imaging-controlled cataract method 400 in more detail. The method 400 can include an imaging 410 of an imaged ophthalmic layer in an imaged region of an eye, followed by an identifying 420 of the coordinates of the imaged layer from the image. These tasks can be performed, for example, by the imaging system 122 of the imaging-based laser-controller 120. The identifying 420 can include performing a feature-recognition analysis. In other cases, it can include receiving an operator-input through an operator interface 128. These tasks can be performed by the imaging system 122, the pattern generator 124 or the image analyzer 126.

[0086] Next, the method 400 can include a generating 430 of coordinates of points of a scan-pattern, and a determining 440 of a distance of the points of the scan-pattern from the imaged layer. These steps can be performed for example, by the pattern generator 124.

[0087] The method 400 can further include an associating 450 of laser-power parameters with the generated points based on their determined distance. The tasks 420 to 450 can include receiving possible inputs 422 – 452 from an operator of the laser system 100 through the operator interface 128.

[0088] The method can also include a signaling 460 of the generated coordinates of the points of the scan-pattern to the beam scanner 116 and a signaling 470 of the corresponding laser-power parameters to the beam attenuator 114.

[0089] FIG. 10 illustrates the case of surgical relevance when the lens capsule 222 has an uneven shape. This situation can arise in different circumstances. For example, the docking of the patient interface 136 can cause considerable deformation of the anterior segment of the eye 1. Or an ophthalmic trauma or a prior lens fragmentation procedure can result in an uneven lens shape. In any of these circumstances, the laser system 100

can be capable of analyzing an image 256 of the imaged layer that exhibits more than two local extrema. Visibly, a simple sinusoidal model curve 258 is insufficient to identify the imaged layer and to determine its z-depth coordinate in this case. Therefore, embodiments of the imaging system 122, the pattern generator 124 or the image analyzer 126 can be
5 capable of recognizing the imaged layer and determine its z-depth coordinate even in this more challenging case, for example, by using sophisticated feature-recognition software. Having determined and characterized the image 256 of the imaged layer can allow the pattern generator 124 to define the tracking band 257 to associate laser-power parameters with the spots of the scan-pattern accordingly.

10 [0090] FIGS. 11A-D illustrate that the imaging system 122 of the laser system 100 can image a region in the eye, the pattern generator 124 can generate coordinates of points of a scan-pattern for the beam scanner 116, and associate a laser-power parameter with the points of the scan-pattern depending on a distance of the points from a target-pattern.

[0091] An example for such a target pattern can be a chop pattern 500, including the
15 chop-planes 500-X and 500-Y. Such chop patterns 500 can be used for lens fragmentation. FIG. 11A illustrates the case when the z-axis of the lens 220 is aligned with the z-axis of the laser system 100. In this case the chop-planes 500-X and 500-Y are also parallel to the z-axis of the laser system 100.

[0092] FIG. 11B illustrates that if the lens 220 is tilted relative to the z-axis of the
20 laser system 100, as illustrated e.g. in FIG. 4B, then the chop planes 500-Xt and 500-Yt can be tilted as well. Since the scan-pattern often includes a first manifold of points at a first fixed z-depth, followed by a second manifold at a slightly lesser z-depth, the scan-pattern of tilted chop-planes with laser systems that cannot adjust the power of the laser pulses would create cuts into the capsular bag 222, leading to massive surgical
25 complications.

[0093] In contrast, embodiments of the laser system 100 can associate laser-parameters depending on the distance of the points of the scan-pattern from the chop planes 500-Xt and 500-Yt.

[0094] FIGS. 11C-D illustrate the points of the scan-pattern with low and high laser
30 power, generated by the pattern generator 124 to form the tilted 500-Xt and 500-Yt chop planes. Visibly, creating cuts by adjusting the power of the laser pulses depending on their

proximity to the target-pattern can avoid cutting into the capsular bag – a major surgical advantage.

[0095] FIG. 11D illustrates clearly that, as it was the case of the tracking band 257, a photodisruptive laser-power parameter can be associated with scan-points that are closer to the target-pattern 500-Xt and 500-Yt than a predetermined distance Dcut, and a non-
5 photodisruptive laser-power parameter with the scan-points that are farther from the target-pattern than the predetermined distance Dcut.

[0096] In other implementations, the cutting surface can be a circular surface-segment, a spiral surface-segment, a corneal access cut and a limbal relaxing cut.

10 [0097] FIGS. 12A-B illustrate that in some cases the target pattern 260-2 can be a target volume with an axis tilted relative to an optical axis of the laser system 100. Here, the scan pattern includes cylindrical patterns 260-1, and the laser-power parameter of the points of this scan-pattern is adjusted to form a tilted volume cut 260-2. Such a utility can be useful for correcting a refractive property of the lens 220, for example.

15 [0098] In some implementations, the pattern generator 124 can be configured to associate the laser-power parameters with the points of the scan-pattern depending additionally on a distance of the points from an ophthalmic layer, imaged by the imaging system 122.

[0099] While this specification contains many specifics, these should not be
20 construed as limitations on the scope of the invention or of what can be claimed, but rather as descriptions of features specific to particular embodiments. Certain features that are described in this specification in the context of separate embodiments can also be implemented in combination in a single embodiment. Conversely, various features that are described in the context of a single embodiment can also be implemented in multiple
25 embodiments separately or in any suitable subcombination. Moreover, although features can be described above as acting in certain combinations and even initially claimed as such, one or more features from a claimed combination can in some cases be excised from the combination, and the claimed combination can be directed to a subcombination or variation of a subcombination.

CLAIMS

1. An imaging-based laser system, comprising:

a laser-beam system, configured to generate and scan a beam of laser pulses with an adjustable laser-power parameter to points of a scan-pattern in an eye; and

5 an imaging-based laser-controller, configured

to image a layer in the eye,

to control the scanning of the beam of laser pulses to the points of the scan-pattern, and

10 to control a laser-power parameter of the laser pulses according to the distance of the points of the scan-pattern from the imaged layer.

2. The laser system of claim 1, the laser-beam system comprising:

a laser engine, configured to generate the beam of laser pulses;

15 a beam attenuator, configured to modify the laser-power parameter of the laser pulses; and

a beam scanner, configured to direct the beam of laser pulses to the points of the scan-pattern in the eye.

3. The laser system of claim 2, the beam attenuator comprising at least one of:

20 a Pockels cell, a polarizer-assembly, a mechanical shutter, an electro-mechanical shutter, and an energy wheel.

4. The laser system of claim 2, wherein:

25 the beam attenuator is disposed between the laser engine and the beam scanner in a path of the beam.

5. The laser system of claim 2, wherein:

the beam attenuator is disposed after the beam scanner in a path of the beam.

6. The laser system of claim 2, wherein:
the beam attenuator is part of the laser engine.

5 7. The laser system of claim 2, wherein:
the beam attenuator and the beam scanner are at least partially integrated.

8. The laser system of claim 1, the laser-controller comprising:
an imaging system, configured to image the imaged layer in the eye; and
10 a pattern generator, configured
to generate coordinates of the points of the scan-pattern,
to associate the laser-power parameter with the points depending on the
distance of the points from the imaged layer, and
to signal the coordinates of the points and the corresponding laser-power
15 parameters to the laser-beam system.

9. The laser system of claim 8, wherein:
the pattern generator is configured
to signal the coordinates to a beam scanner, and
20 to signal the laser-power parameter to a beam attenuator.

10. The laser system of claim 8, wherein:
the laser-power parameter is one of a pulse energy, a pulse power, a pulse
length and a pulse repetition rate.

25

11. The laser system of claim 8, the imaging system comprising:

at least one of an ophthalmic coherence tomography system, a Scheimpflug imaging system, a scanning imaging system, a single shot imaging system, an ultrasound imaging system, and a video imaging system.

5

12. The laser system of claim 8, wherein:

the imaging system is configured to image the imaged layer in an image region, wherein the image region

is based on one of a loop, an arc, a line, and a two-dimensional pattern transverse to an axis of the imaging system, and

10

extends to an image depth along the axis of the imaging system.

13. The laser system of claim 8, wherein:

the imaging system is configured to support a determination of a z-depth coordinate of the imaged layer corresponding to a scanning coordinate along an image-scan.

15

14. The laser system of claim 13, wherein:

the laser system comprises an operator interface; and

the imaging system is configured to support the determination of the z depth coordinate of the imaged layer using an input from an operator through the operator interface.

20

15. The laser system of claim 14, wherein:

the operator interface is configured to assist the operator to fit a model curve to the image of the imaged layer.

25

16. The laser system of claim 14, wherein:

the operator interface is capable of receiving the operator-input from at least one of a keyboard, a touch-screen, a computer-communication channel, an external memory, a flash-drive, an internet connection, a speech-recognition apparatus and a wireless connection.

5

17. The laser system of claim 13, wherein:

the imaging system is configured to determine the z-depth coordinate of the imaged layer by performing a feature-recognition analysis of the image of the imaged layer.

10

18. The laser system of claim 17, wherein:

the imaging system is configured to utilize at least one of a result of a pre-surgery measurement, statistical data, video image data, ophthalmic coherence tomography image data, and a model-based computation during the determination of the z-depth.

15

19. The laser system of claim 13, wherein:

the imaging system is configured to forward the z-depth and scanning coordinates of the imaged layer to the pattern generator; and

20

the pattern generator is configured

to determine the distance of the points of the scan-pattern from the imaged layer based on the forwarded coordinates of the imaged layer and the generated coordinates of the points,

25

to associate a first laser-power parameter above a photodisruption threshold with a first set of points closer to the imaged layer than a predetermined distance, and

to associate a second laser-power parameter below a photodisruption threshold with a second set of points farther from the imaged layer than the predetermined distance.

5 **20.** The laser system of claim 13, wherein:

the imaging system is configured to forward the z-depth and scanning coordinates of the imaged layer to the pattern generator; and

the pattern generator is configured

10 to determine the distance of the points of the scan-pattern from the imaged layer based on the forwarded coordinates of the imaged layer and the generated coordinates of the points, and

to associate with the coordinates of the points a laser-power parameter that is a decreasing function of the distance of the points from the imaged layer.

15 **21.** The laser system of claim 8, wherein:

the imaging system is configured to forward the image of the imaged layer to the pattern generator; and

the pattern generator is configured

to receive the image from the imaging system, and

20 to determine a z-depth coordinate of the imaged layer corresponding to a scanning coordinate along an image scan.

22. The laser system of claim 21, wherein:

25 the pattern generator is configured to determine the z-depth of the imaged layer in part by performing a feature-recognition analysis of the received image of the imaged layer.

23. The laser system of claim 21, wherein:

the pattern generator is configured to receive an operator input through an operator interface during the process of determining the z-depth of the imaged layer.

5

24. The laser system of claim 23, wherein:

the operator interface is capable of receiving the operator-input from at least one of a keyboard, a touch-screen, a computer-communication channel, an external memory, a flash-drive, an internet connection, a speech-recognition apparatus and a wireless connection.

10

25. The laser system of claim 21, wherein:

the pattern generator is configured

to define a tracking band as a manifold of points within a predefined distance from the coordinates of the imaged layer;

15

to associate a laser-power parameter above a photodisruption threshold with points of the scan-pattern inside the tracking band, and

to associate a laser-power parameter below a photodisruption threshold with points of the scan-pattern outside the tracking band.

20

26. The laser system of claim 8, the laser controller comprising:

an image analyzer, configured to determine a z-depth coordinate of the imaged layer corresponding to a scanning coordinate along an image-scan.

25

27. The laser system of claim 26, wherein:

the image analyzer is configured to determine the z-depth coordinate of the imaged layer by performing a feature-recognition analysis of the image of the imaged layer.

28. The laser system of claim 26, wherein:

the image analyzer is configured to determine the z-depth coordinate of the imaged layer by receiving an operator input through an operator-interface.

5 **29.** The laser system of claim 26, wherein:

the image analyzer is at least partially integrated with one of the imaging system and the pattern generator.

30. The laser system of claim 1, wherein:

10 the imaged layer is a lens capsule between a lens of an eye and an aqueous anterior chamber of the eye;

the scan-pattern corresponds to a cylindrical capsulotomy cut intersecting the lens capsule; and

the patter generator is configured

15 to associate a photodisruptive laser-power parameter with points inside a tracking band related to the intersection of the cylindrical capsulotomy cut and the lens capsule, and

to associate a non-photodisruptive laser-power parameter with points outside the tracking band.

20

31. The laser system of claim 30, wherein:

the laser system is configured to perform a capsulotomy before a lens fragmentation during a cataract procedure.

25 **32.** The laser system of claim 30, wherein:

the laser system is configured to be able to analyze an image of the capsule boundary layer with more than two local extrema by at least one of the pattern generator and an image analyzer.

33. An imaging-based laser system, comprising:

a laser that generates and directs a beam of laser pulses into an eye;

an imaging system that images a capsule layer of the eye; and

5 a laser control system that controls the laser to direct the beam

to spots within a tracking band of the imaged capsule layer with a laser-power parameter above a photo-disruption threshold, and

to spots outside the tracking band of the imaged capsule layer with a laser-power parameter below a photo-disruption threshold, wherein

10 the imaging-based laser system is configured to perform a capsulotomy before a lens fragmentation during a cataract procedure.

34. The laser system of claim 33, wherein:

15 the laser system is configured to create a tracking band with a depth range of less than 100 microns for an image of the capsule layer with a depth variation of 500 microns or more.

35. An image-guided ophthalmic laser system, comprising:

a laser engine, configured to generate laser pulses;

20 a beam modifier, configured to modify a laser-power parameter of the laser pulses;

a laser scanner, configured to direct the laser pulses to scanning-points in an eye;

an imaging system, configured to image a region in the eye; and

25 a pattern generator, coupled to the imaging system, the beam modifier and the laser scanner, configured

to generate coordinates of the scanning-points for the laser scanner, and

to associate a laser-power parameter with the scanning-points depending on a distance of the scanning-points from a target-pattern.

36. The laser system of claim 35, wherein:

5 the laser system is configured to direct the laser pulses to a target pattern that is tilted relative to an optical axis of the laser system.

37. The laser system of claim 36, wherein:

10 the target pattern is a tilted cutting surface of a lens fragmentation procedure, and

 the pattern generator is configured to associate

 a photodisruptive laser-power parameter with scanning-points closer to the target-pattern than a predetermined distance, and

15 a non-photodisruptive laser-power parameter with scanning-points farther from the target-pattern than the predetermined distance.

38. The laser system of claim 37, wherein:

 the cutting surface is one of a chopping plane, a circular surface-segment, a spiral surface-segment, a corneal access cut and a limbal relaxing cut.

20

39. The laser system of claim 36, wherein:

 the target pattern is a target volume with an axis tilted relative to an optical axis of the laser system.

25 **40.** The laser system of claim 35, wherein:

 the pattern generator is configured to associate the laser-power parameters with the scanning-points depending additionally on a distance of the scanning-points from an ophthalmic layer, imaged by the imaging system.

41. A method of performing an imaging-controlled ophthalmic procedure, comprising:

imaging a layer in an eye;

5 generating coordinates of points of a scan-pattern;

determining a distance of the points of the scan-pattern from the imaged layer;
and

associating laser-power parameters with the points based on the determined distance.

10

42. The method of claim 41, the method comprising:

identifying coordinates of the imaged layer from the image by performing a feature-recognition analysis.

15 43. The method of claim 41, the method comprising:

identifying coordinates of the imaged layer from the image in part by receiving an operator-input through an operator interface.

44. The method of claim 41, comprising:

20 signaling the generated coordinates of the points of the scan-pattern to a beam scanner; and

signaling the corresponding laser-power parameters to a beam attenuator.

Replacement Sheet

1 / 26

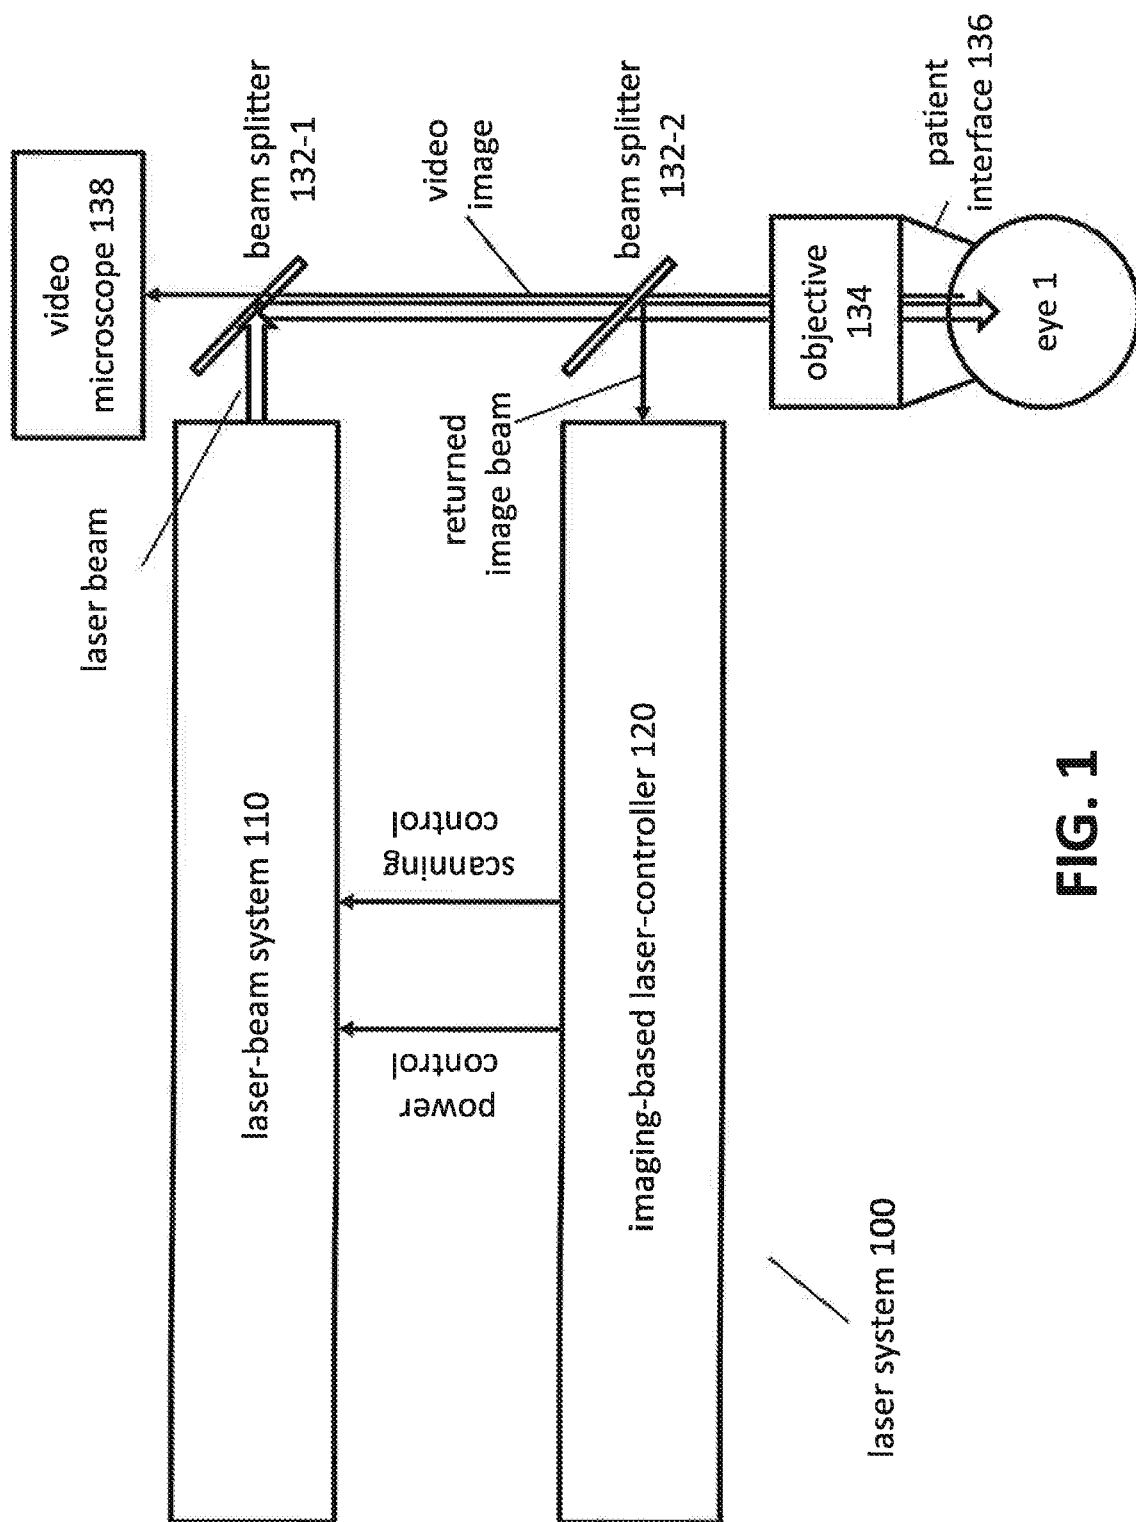


FIG. 1

Replacement Sheet

2 / 26

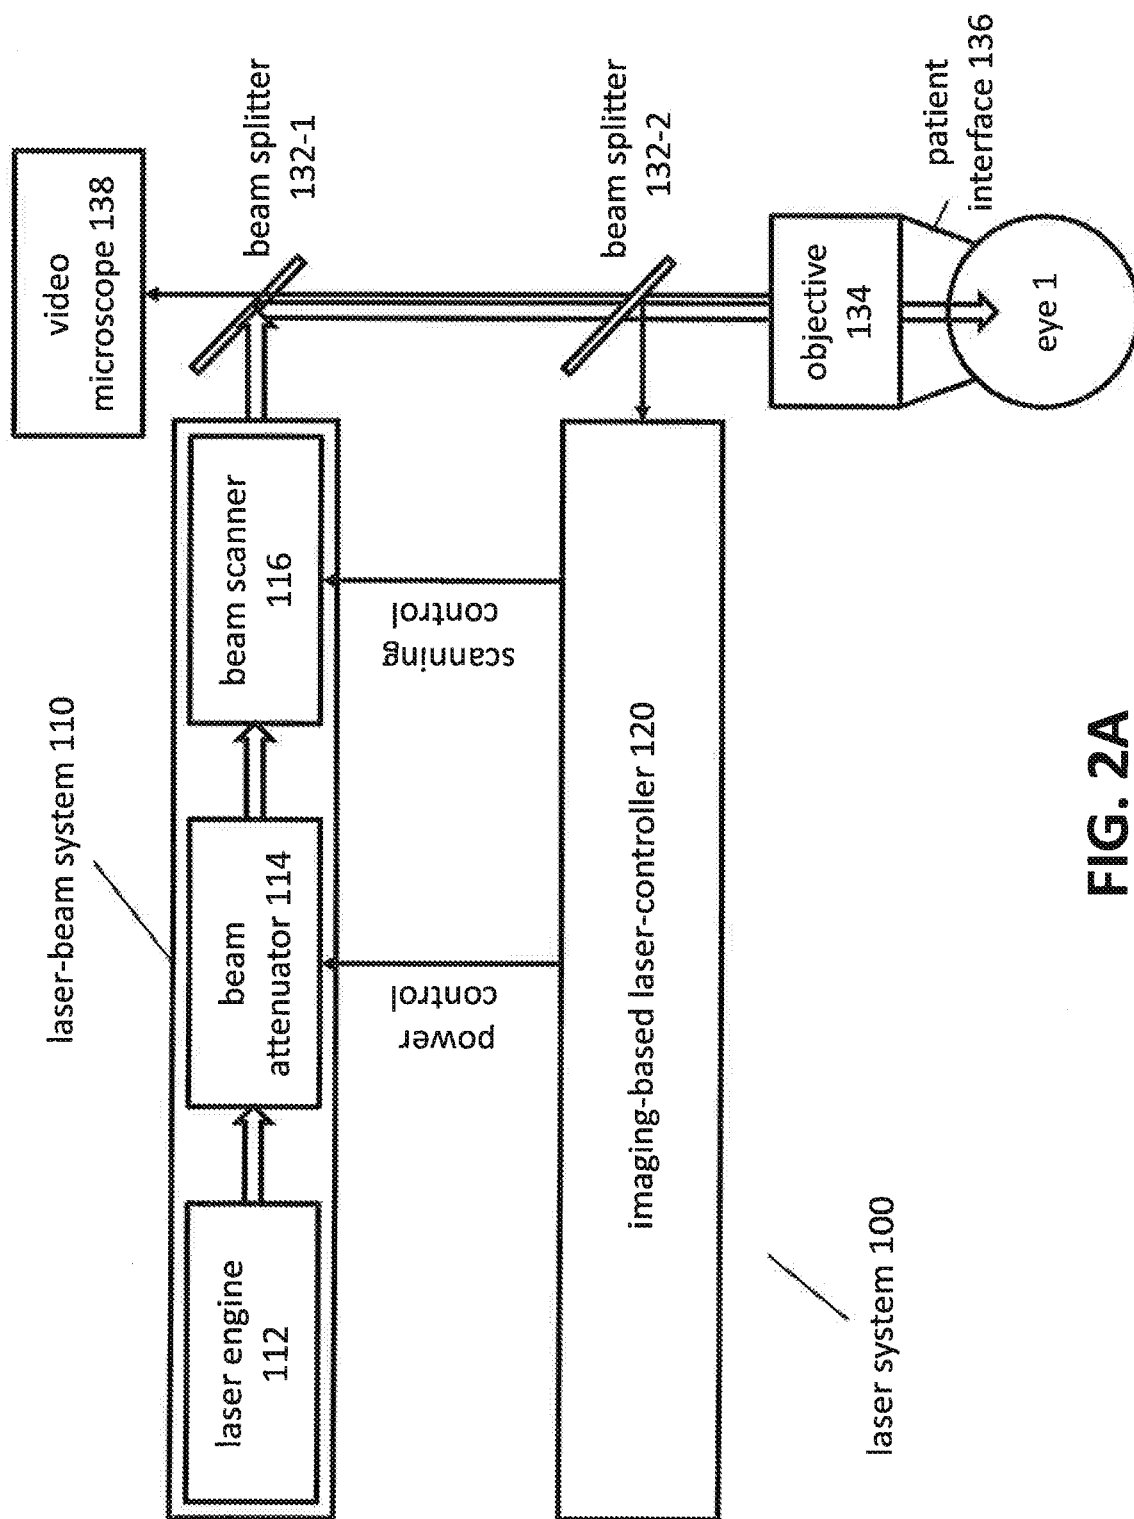


FIG. 2A

Replacement Sheet

3 / 26

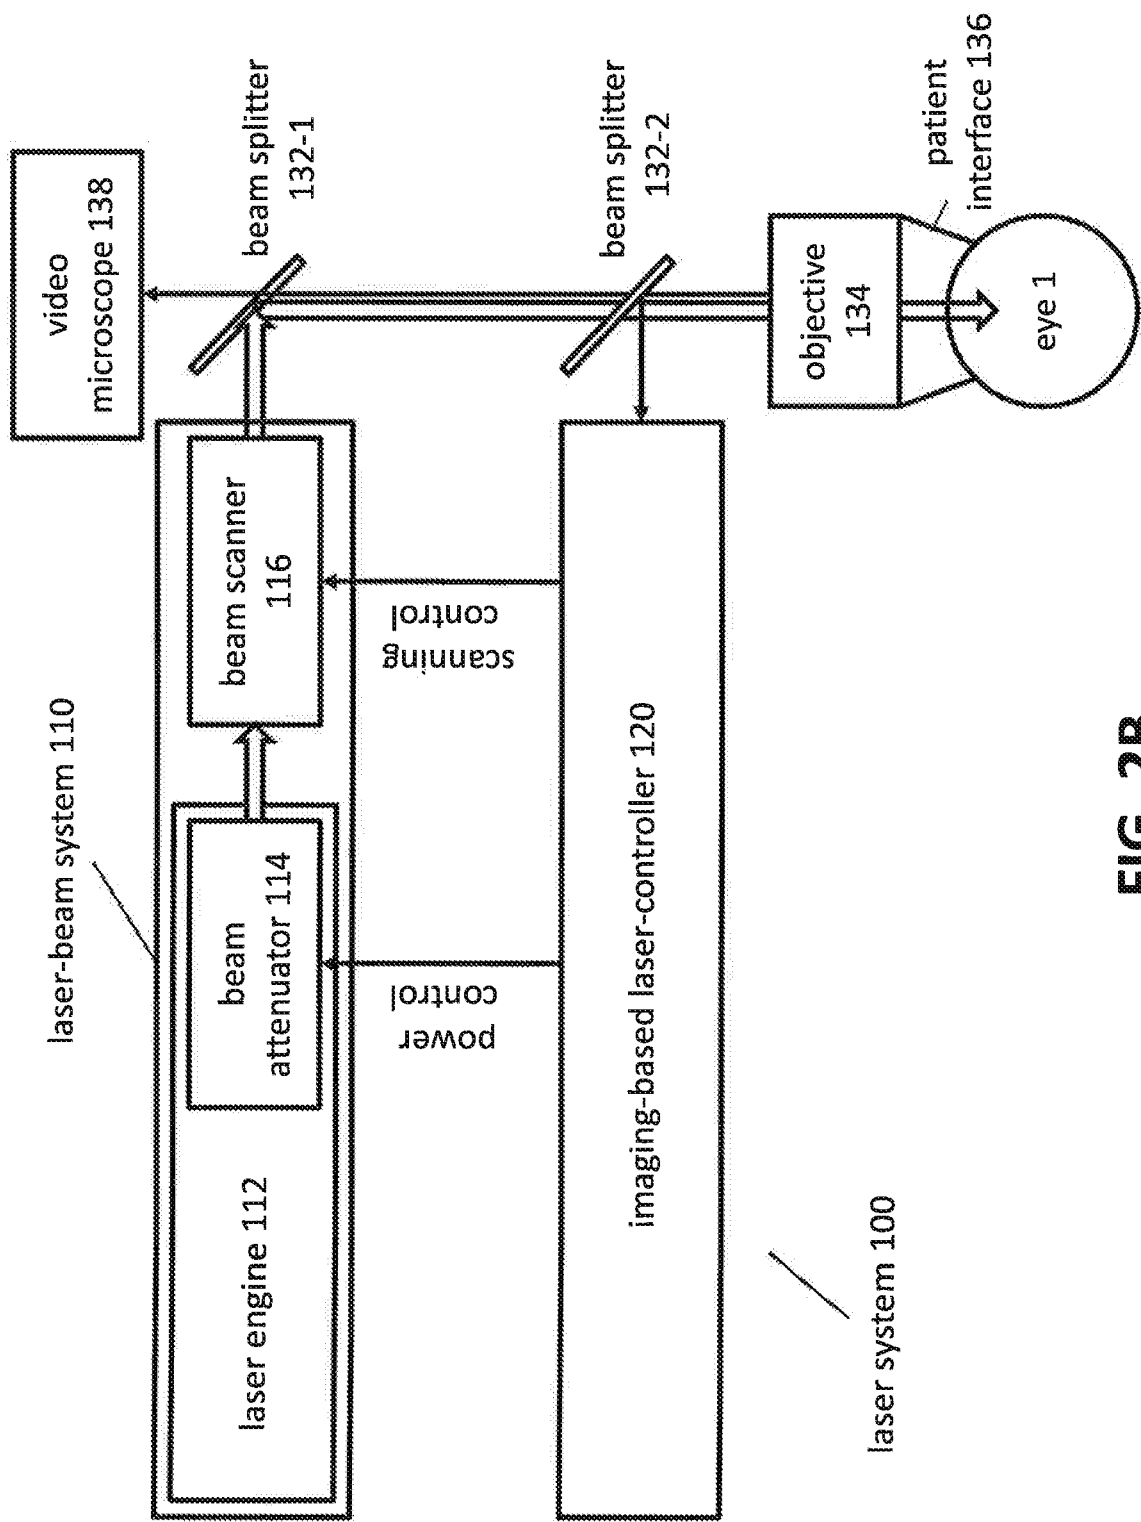


FIG. 2B

Replacement Sheet

4 / 26

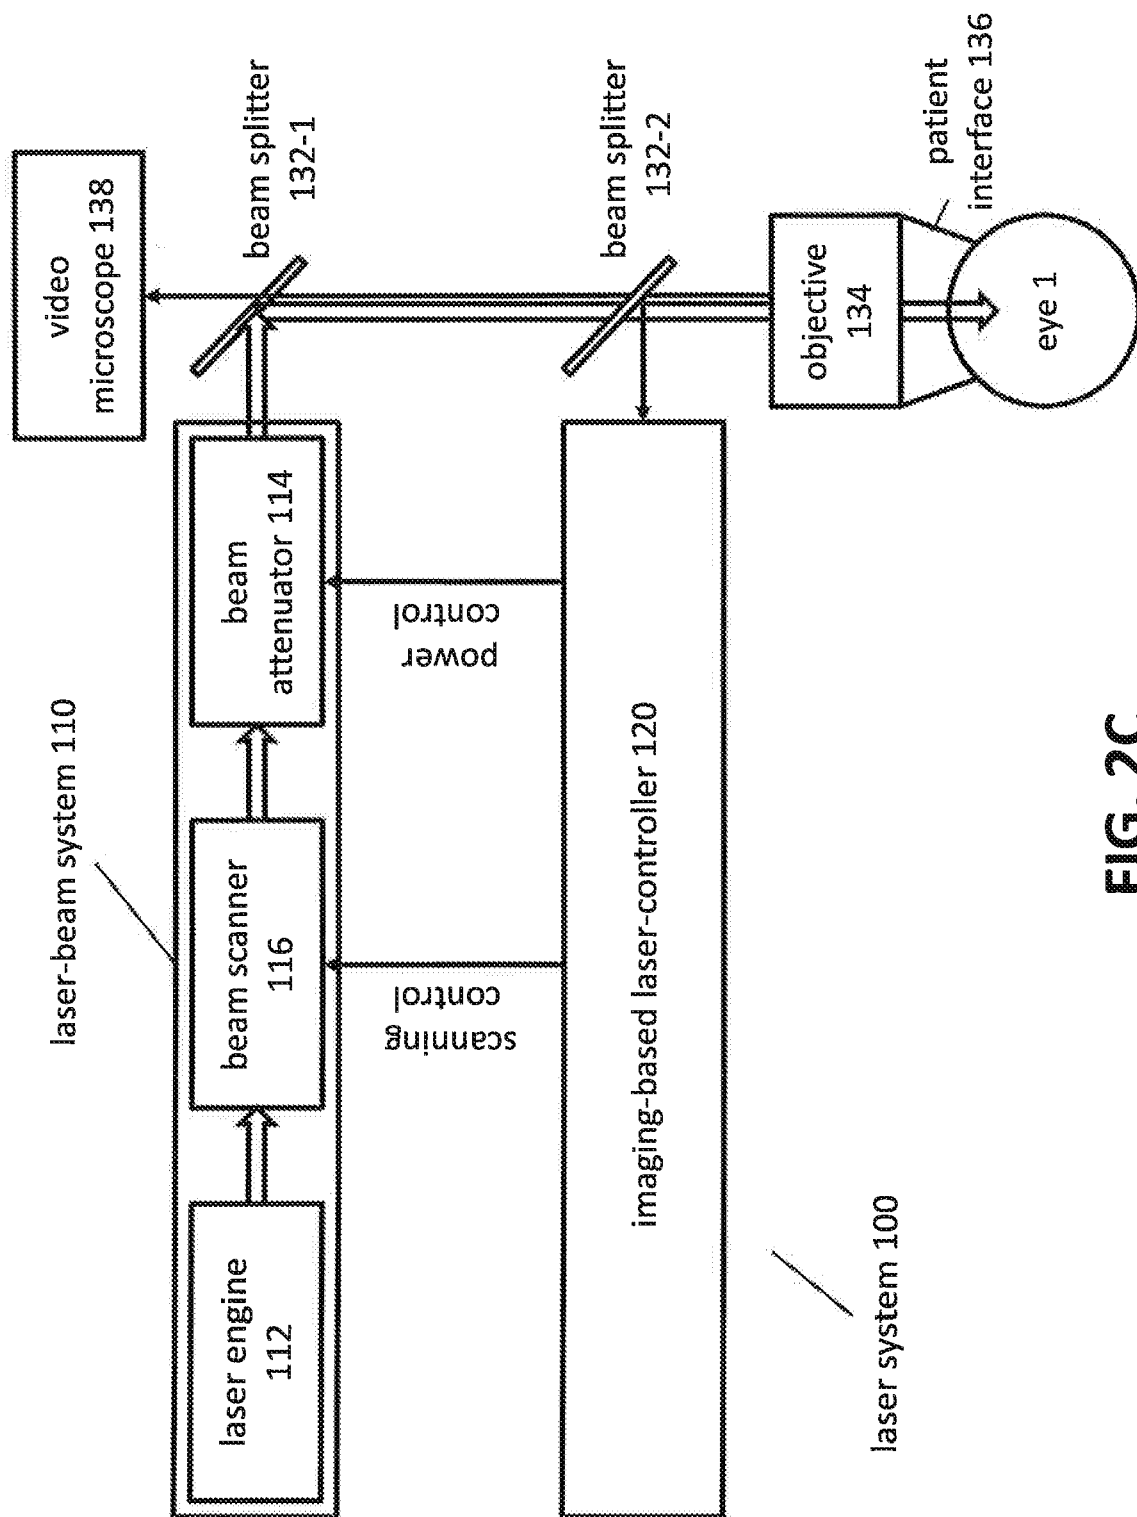


FIG. 2C

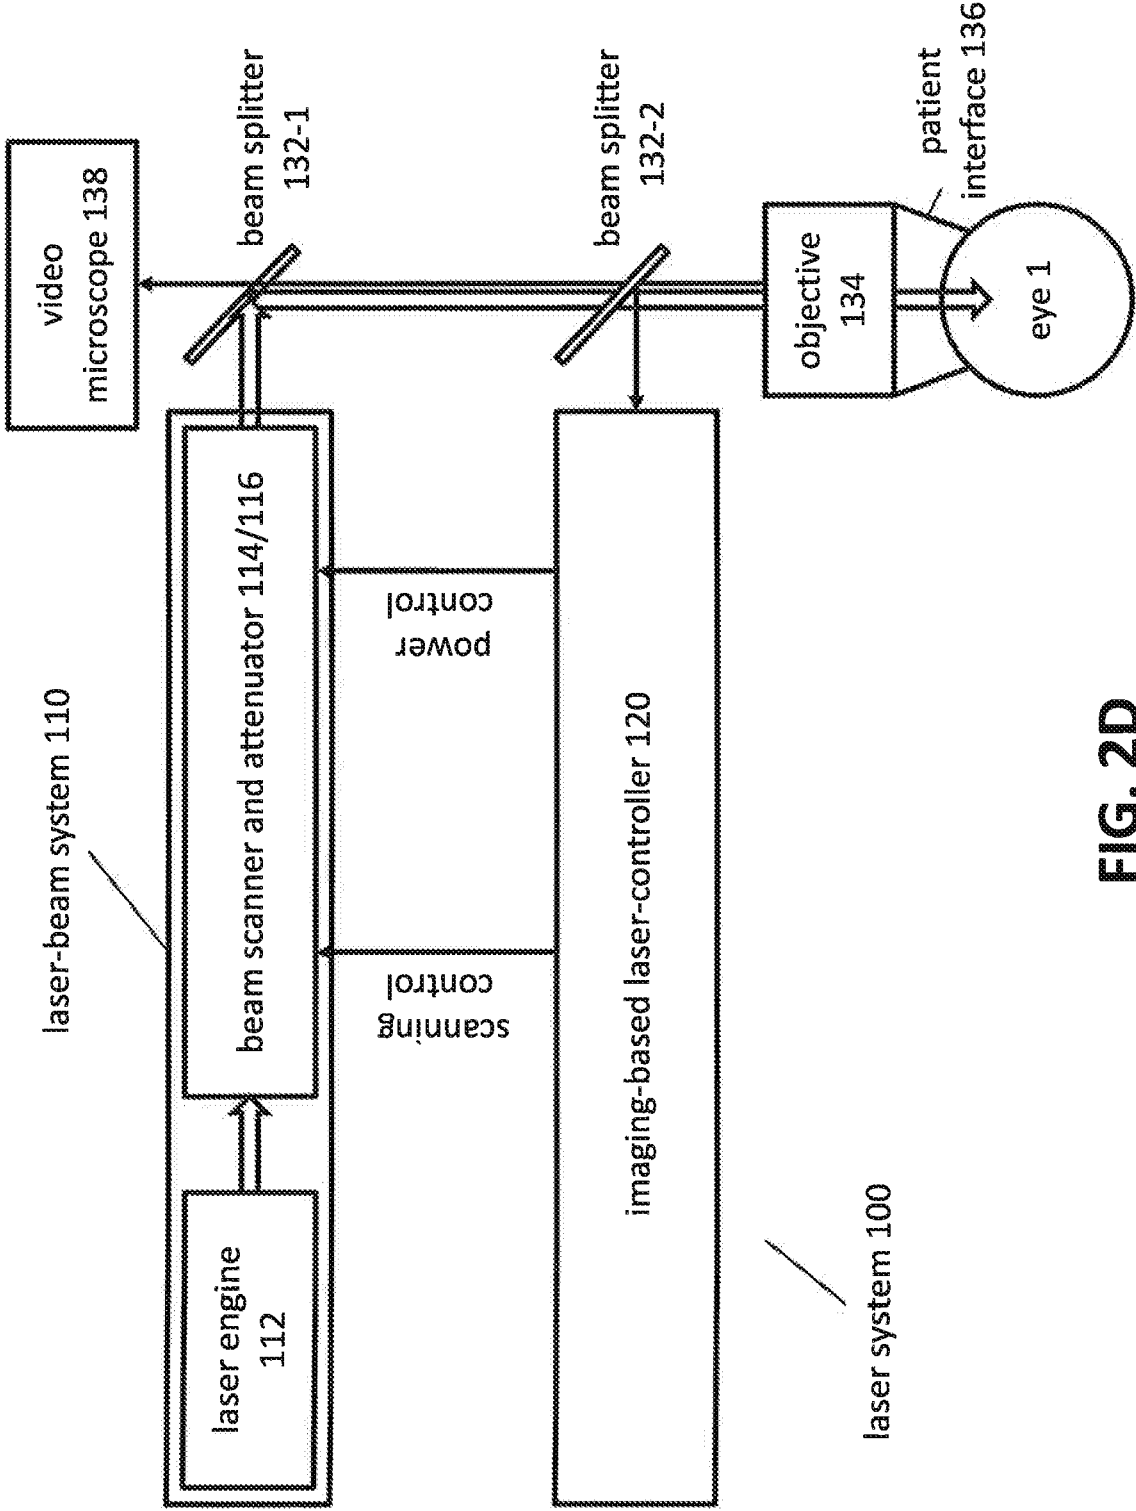


FIG. 2D

Replacement Sheet

6 / 26

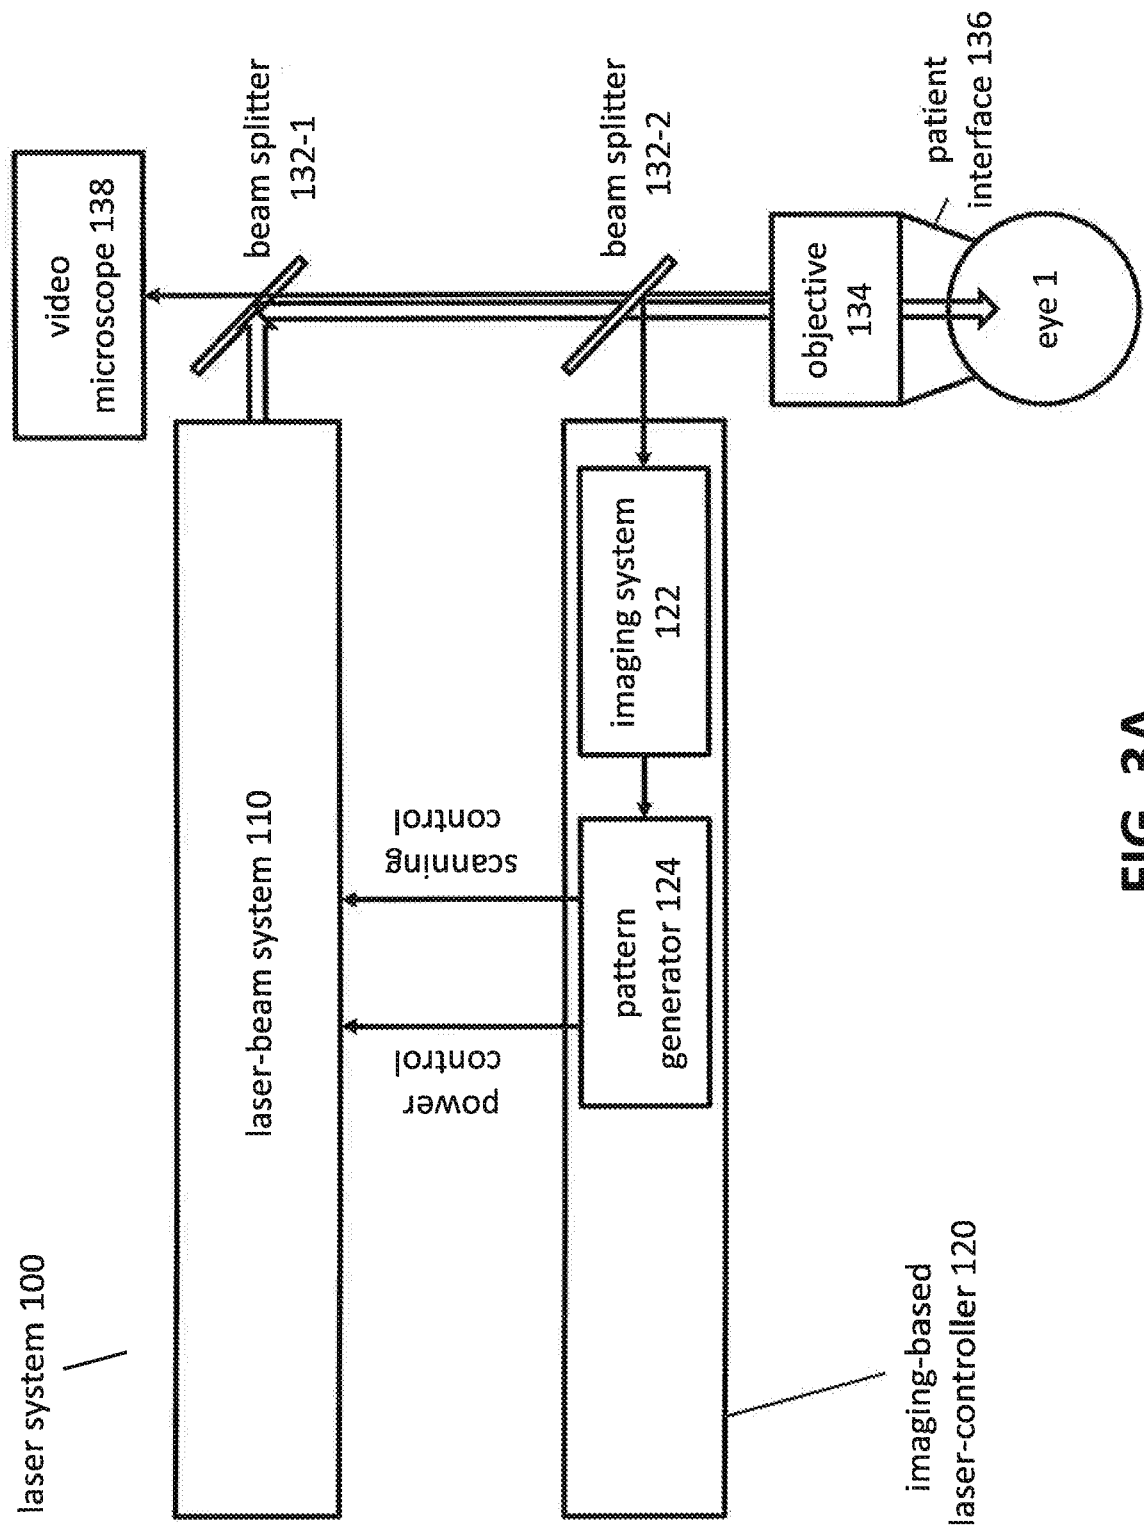


FIG. 3A

Replacement Sheet

7 / 26

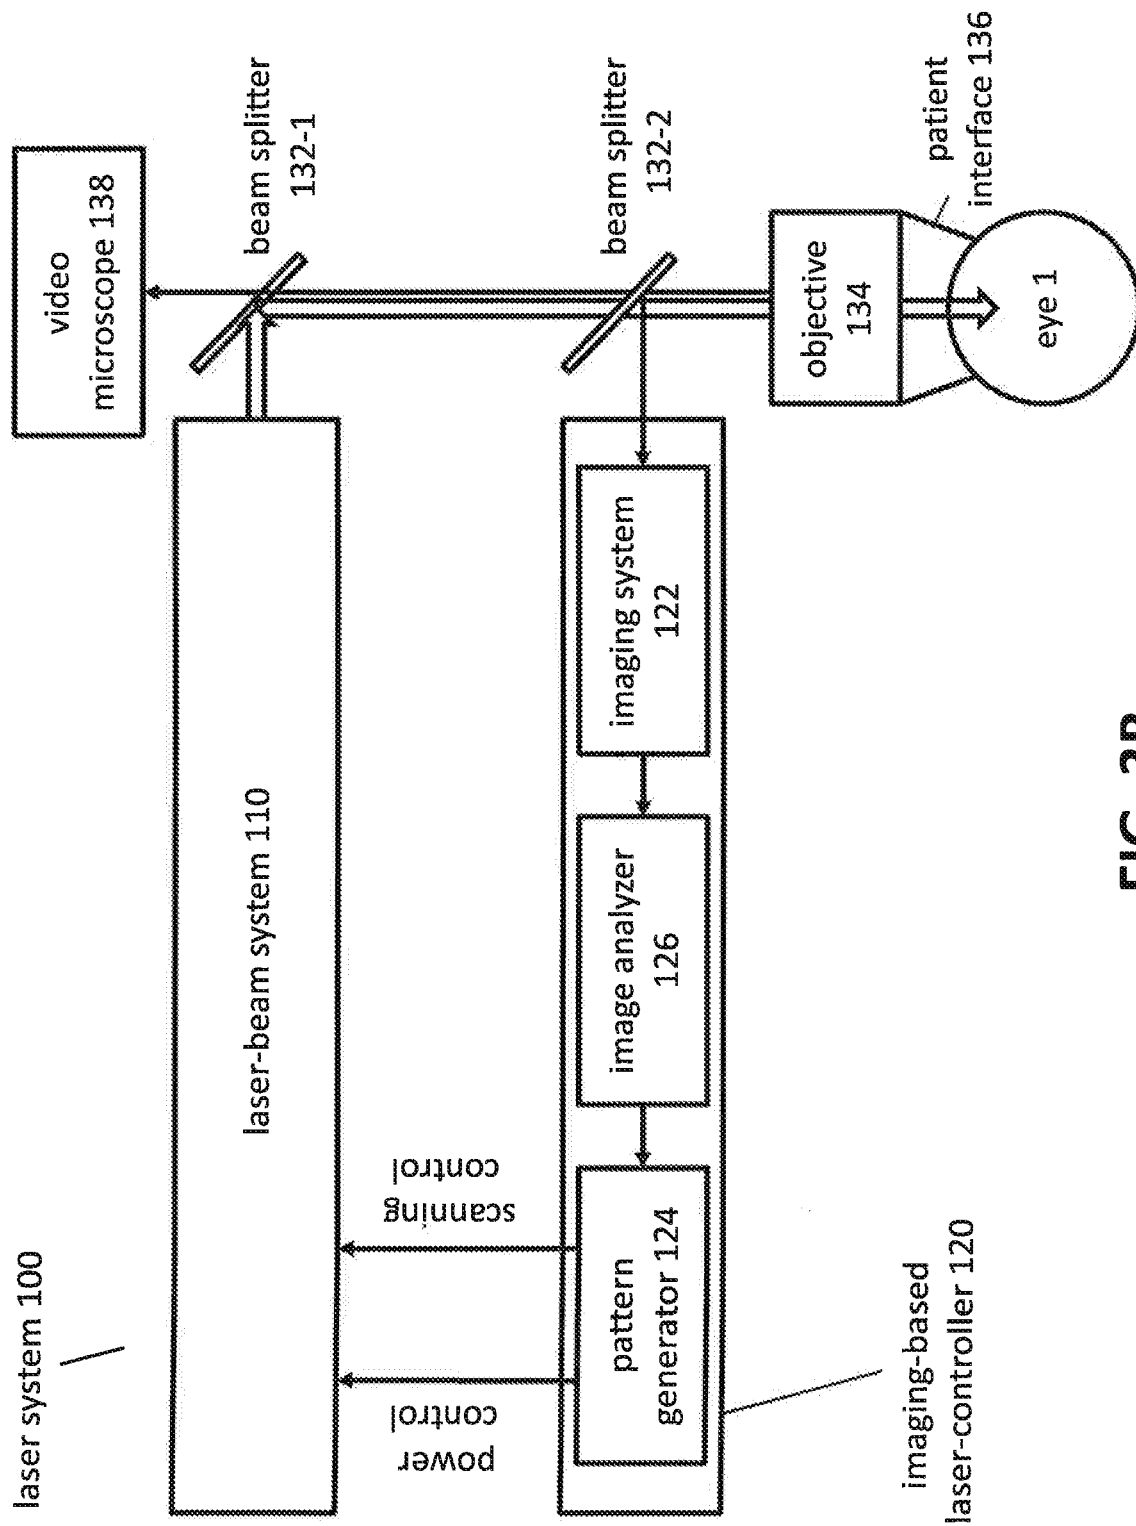


FIG. 3B

Replacement Sheet

8 / 26

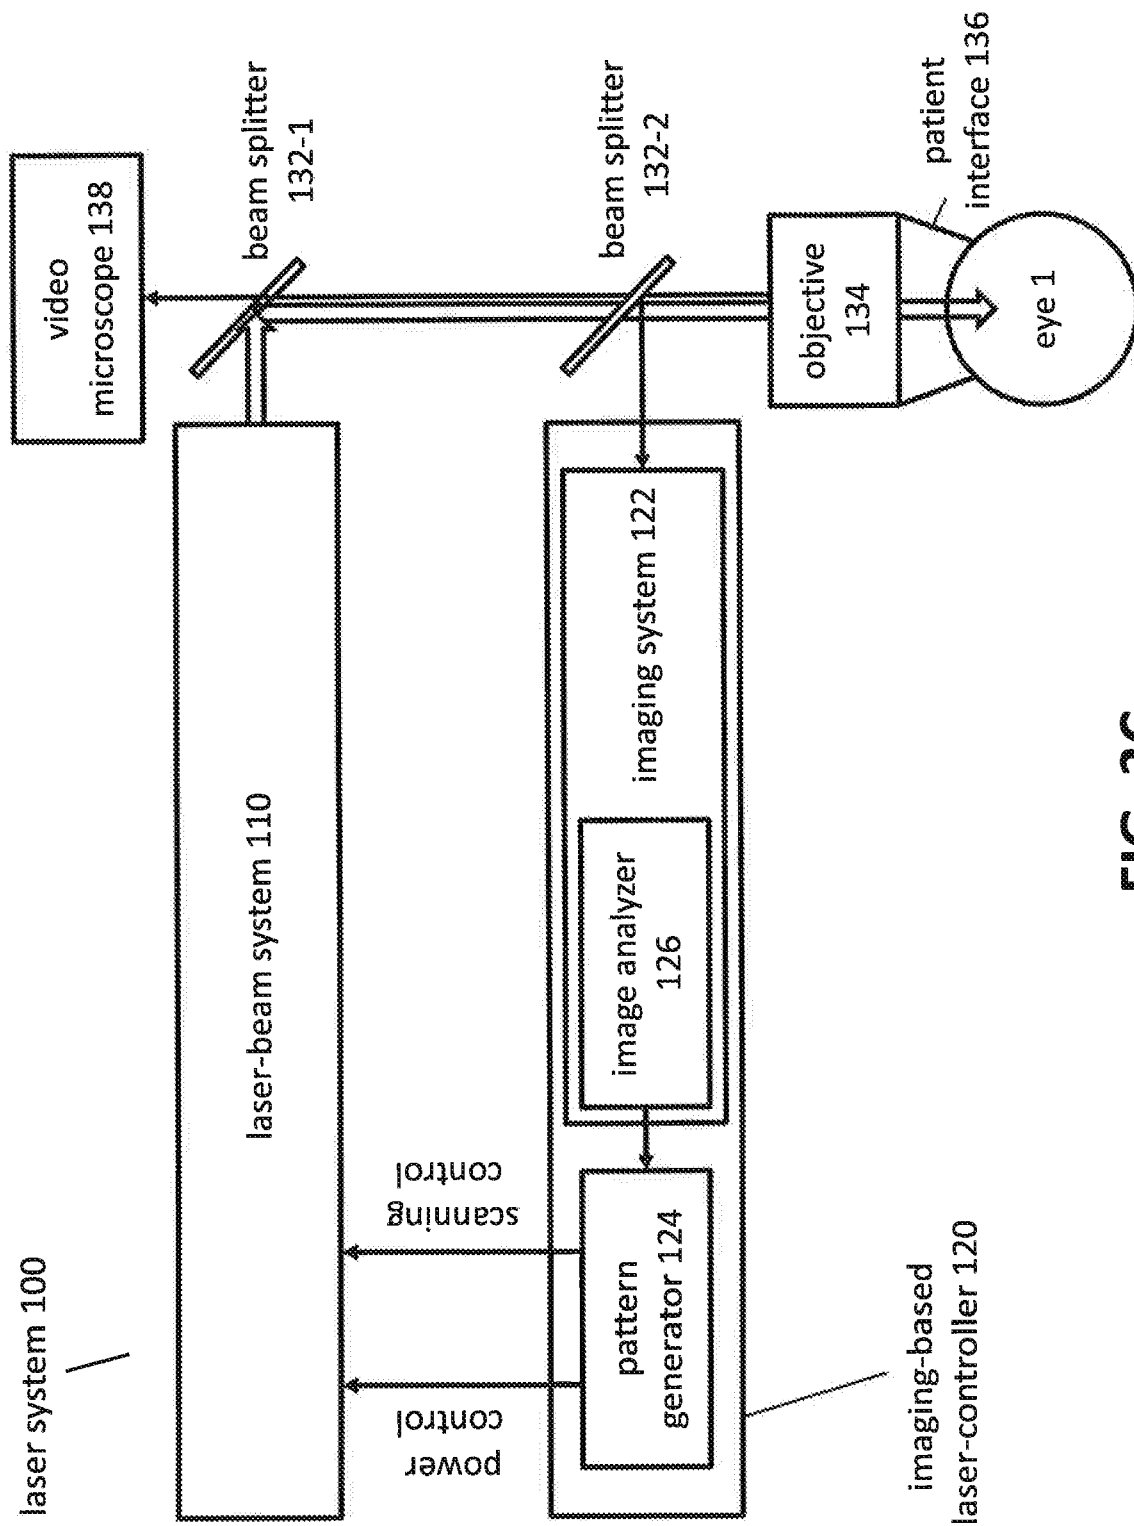


FIG. 3C

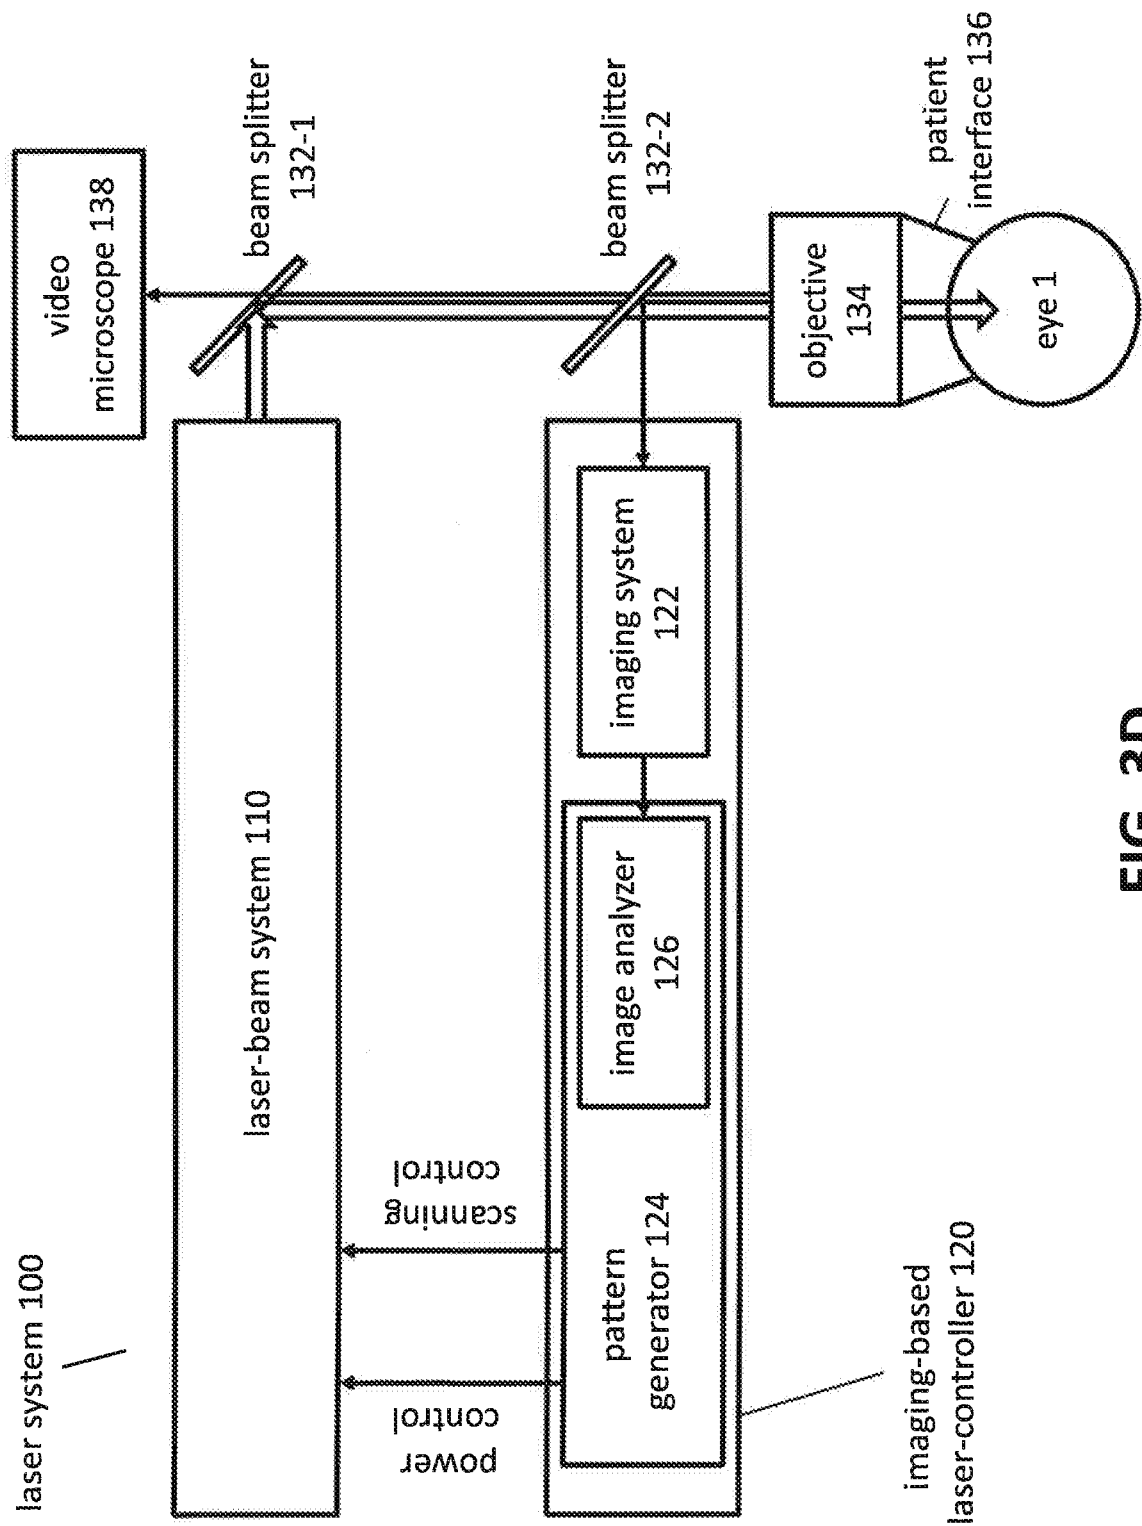


FIG. 3D

Replacement Sheet

10 / 26

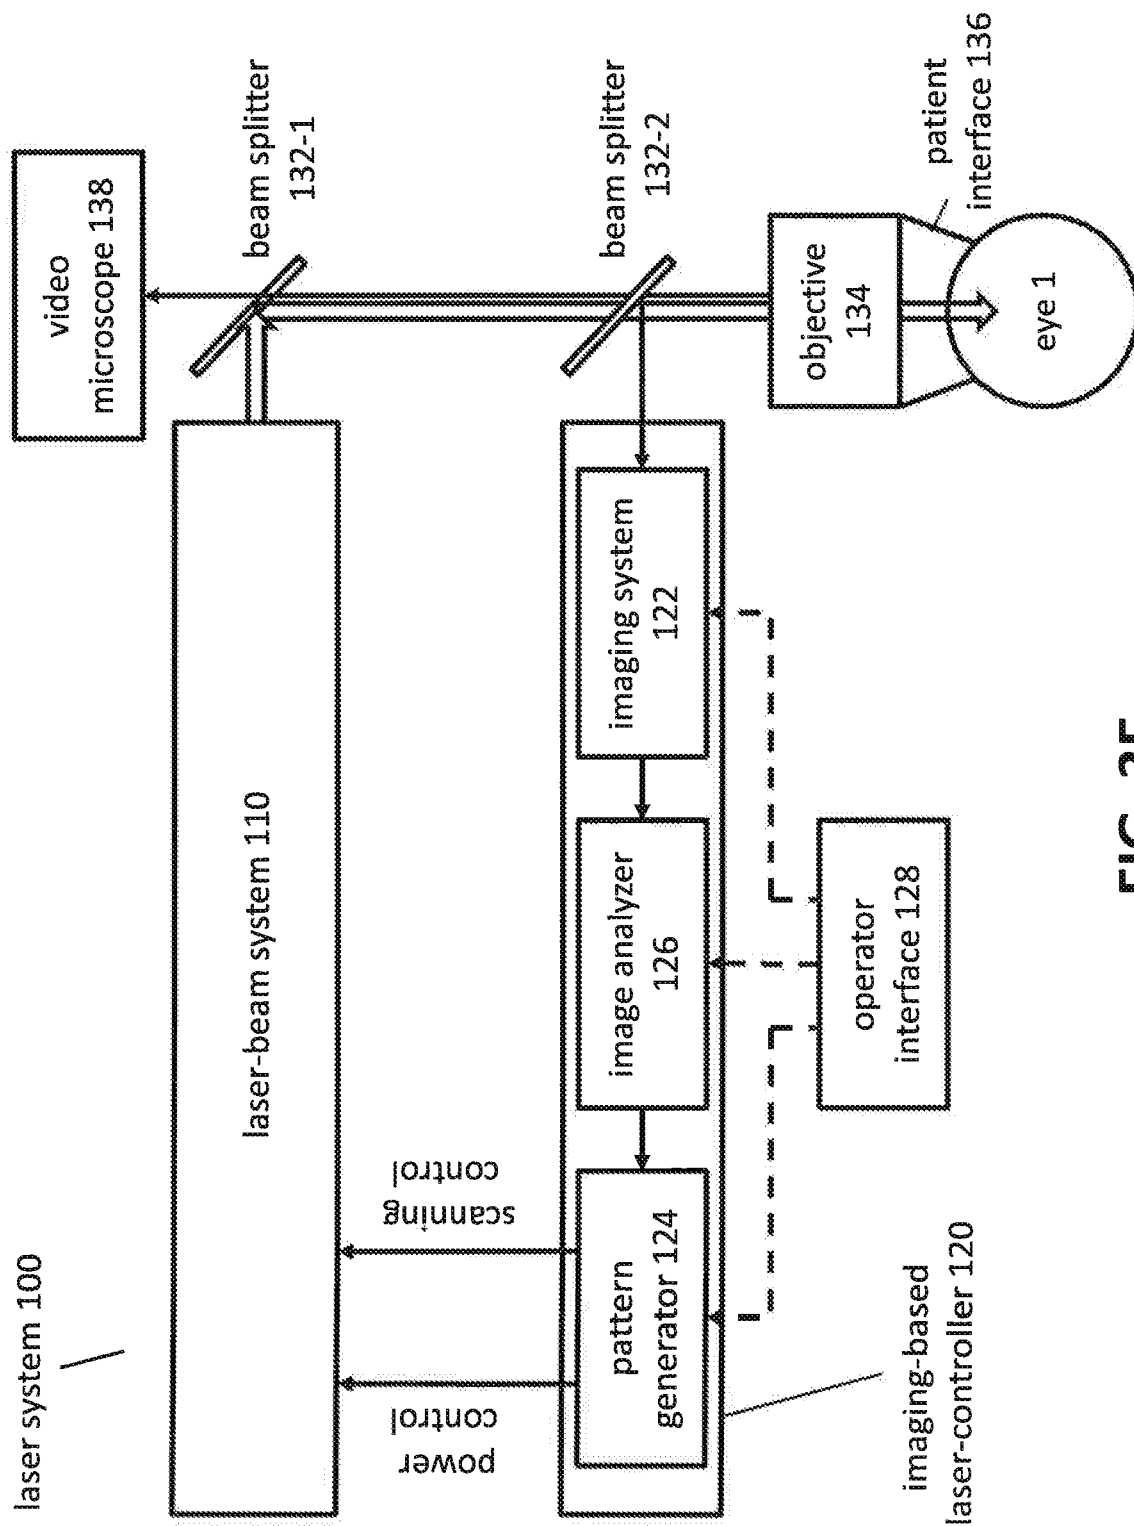


FIG. 3E

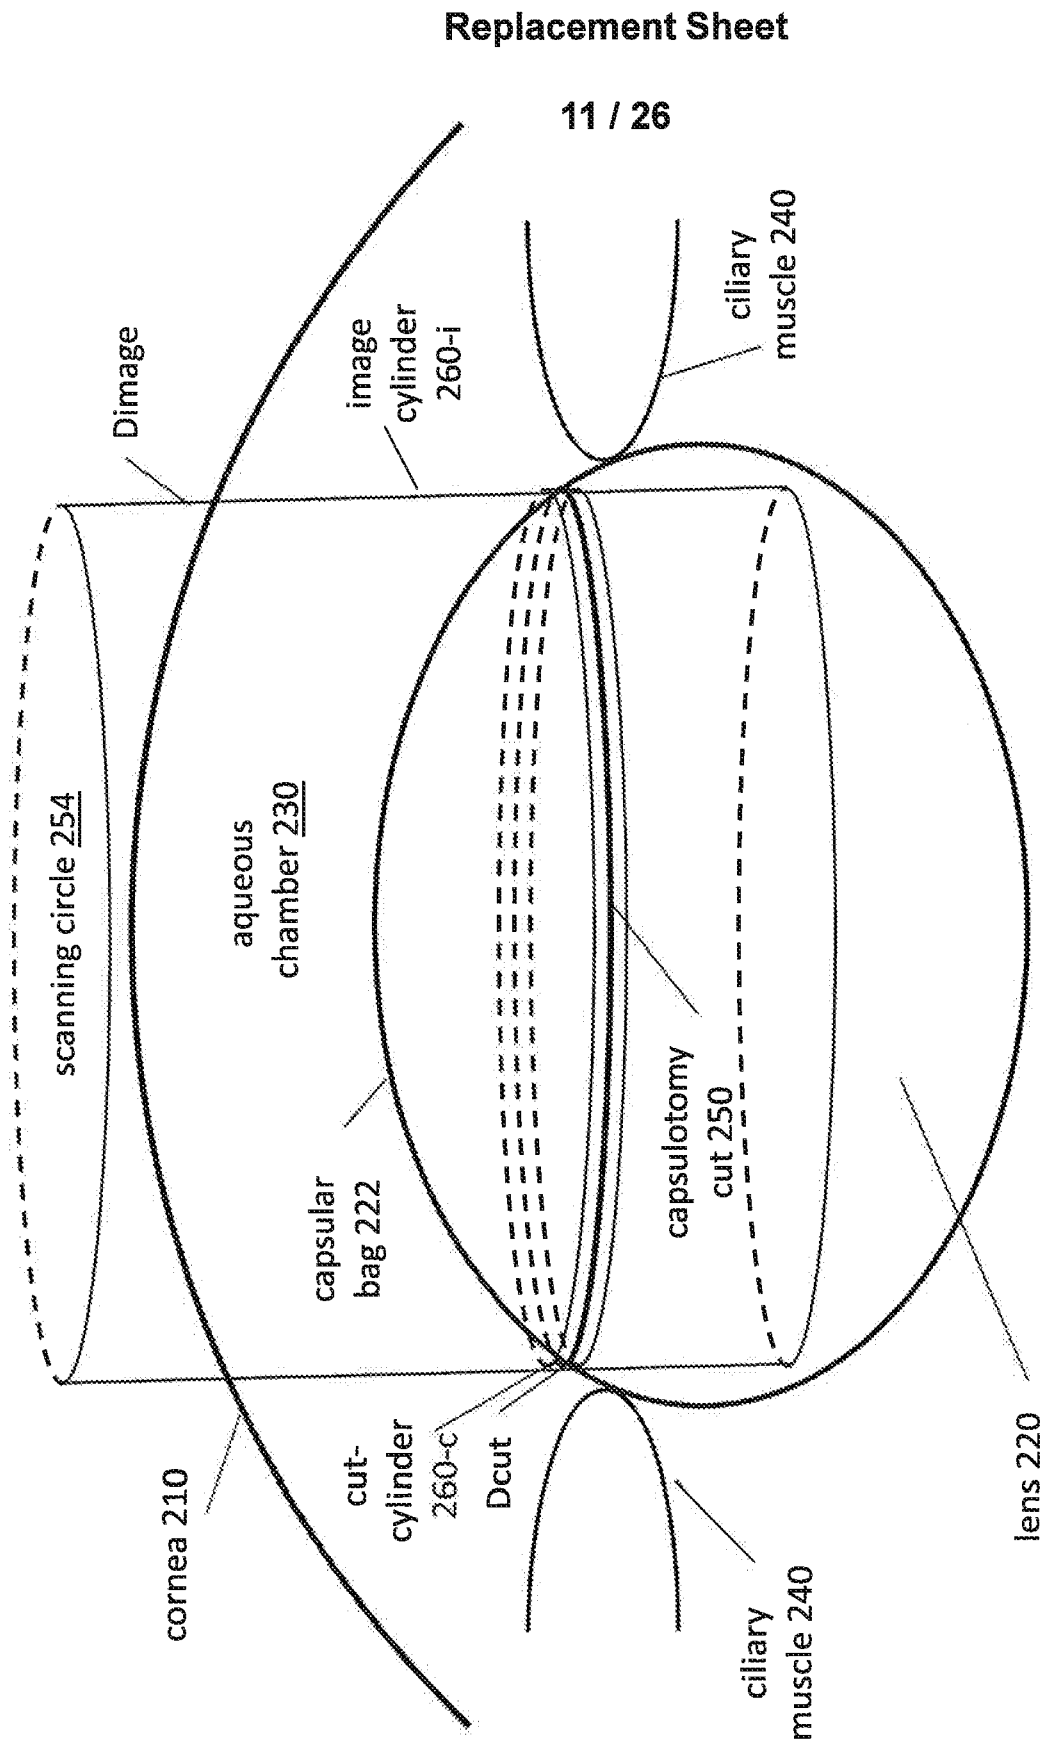


FIG. 4A


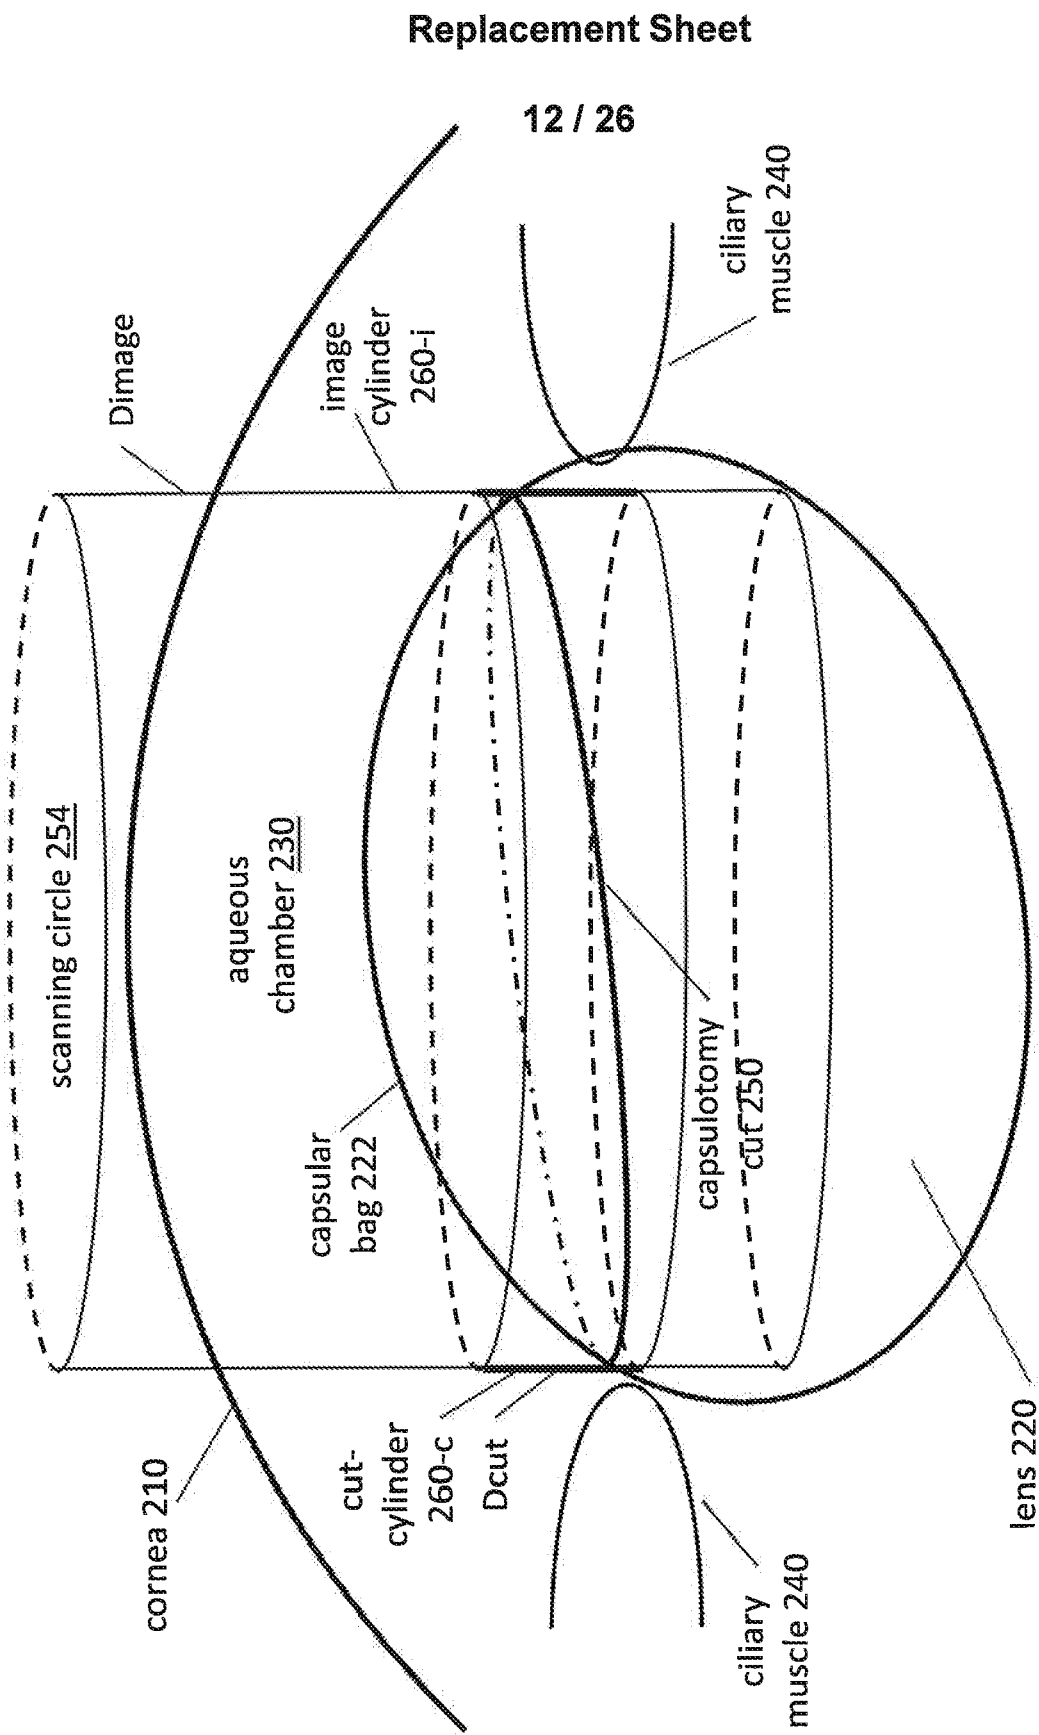


FIG. 4B

Replacement Sheet

13 / 26

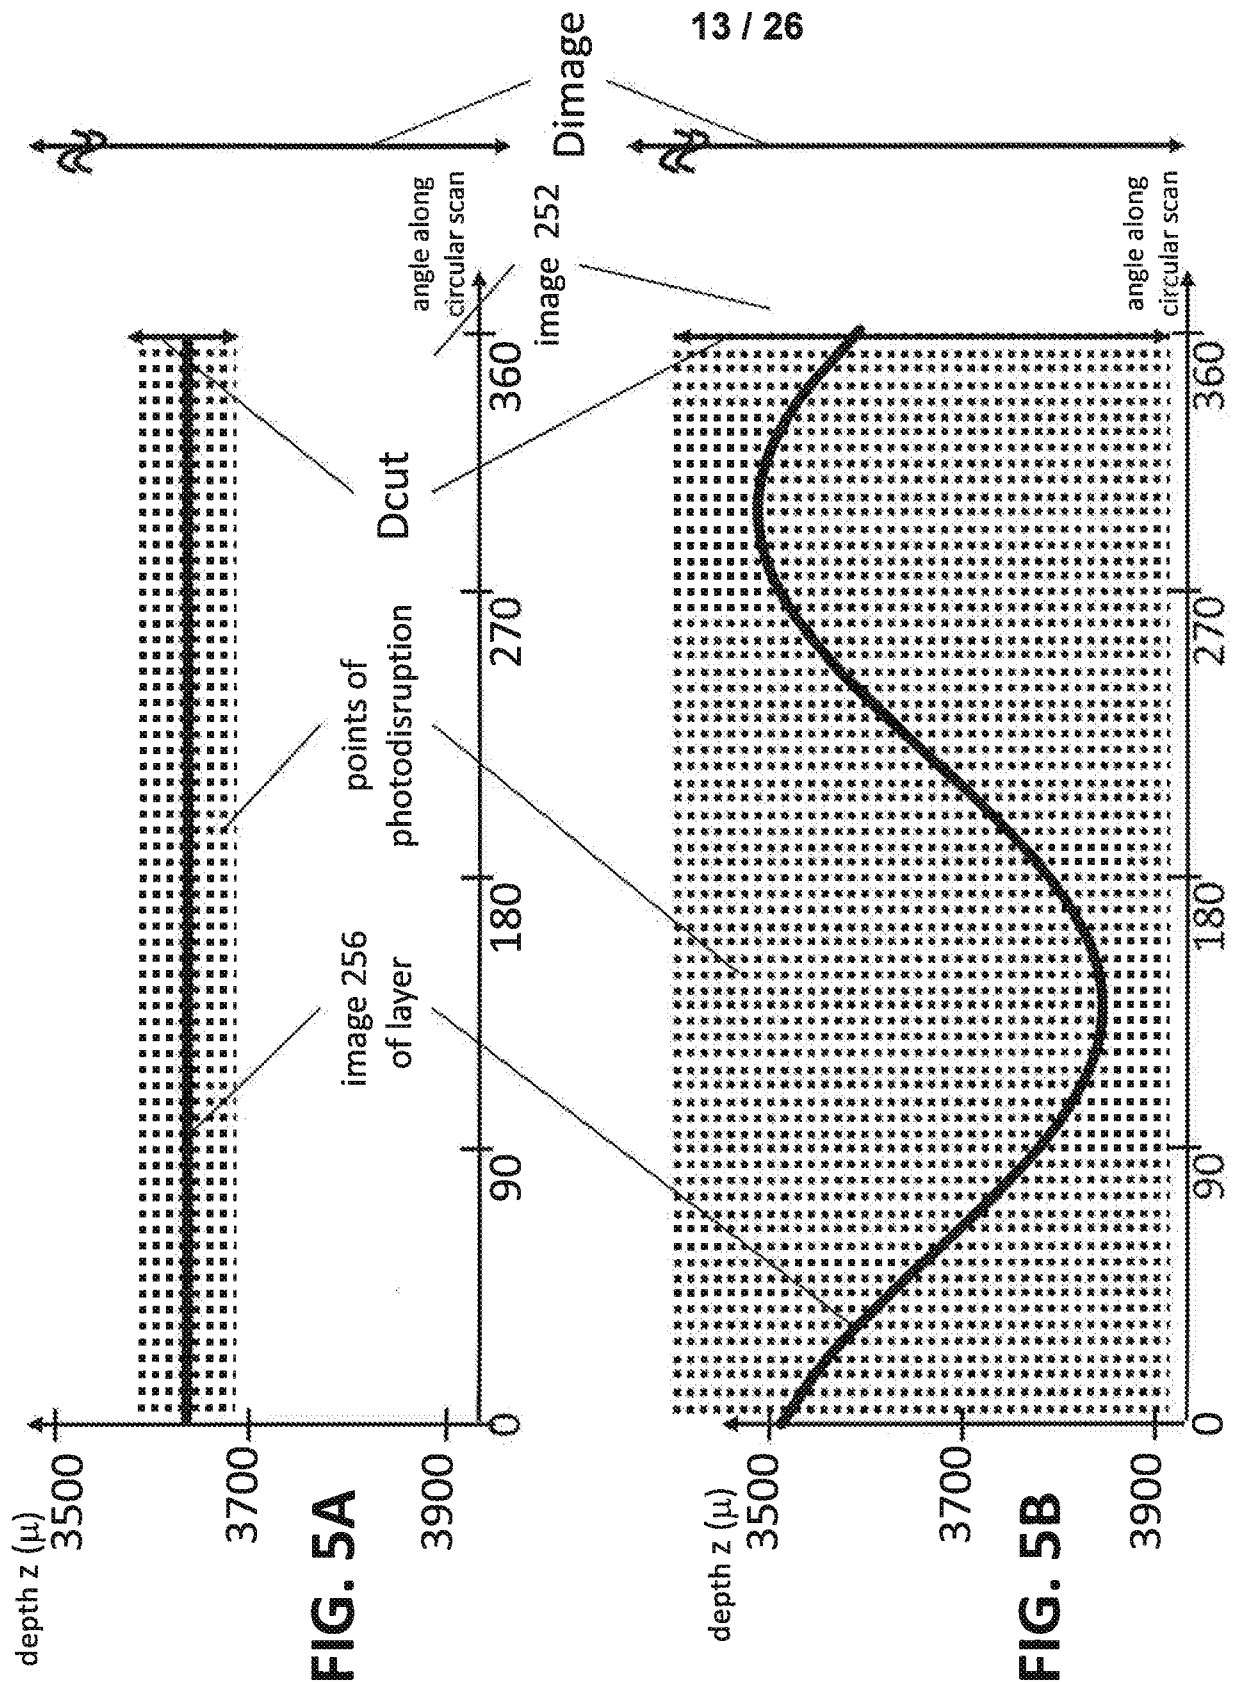

Replacement Sheet

14 / 26

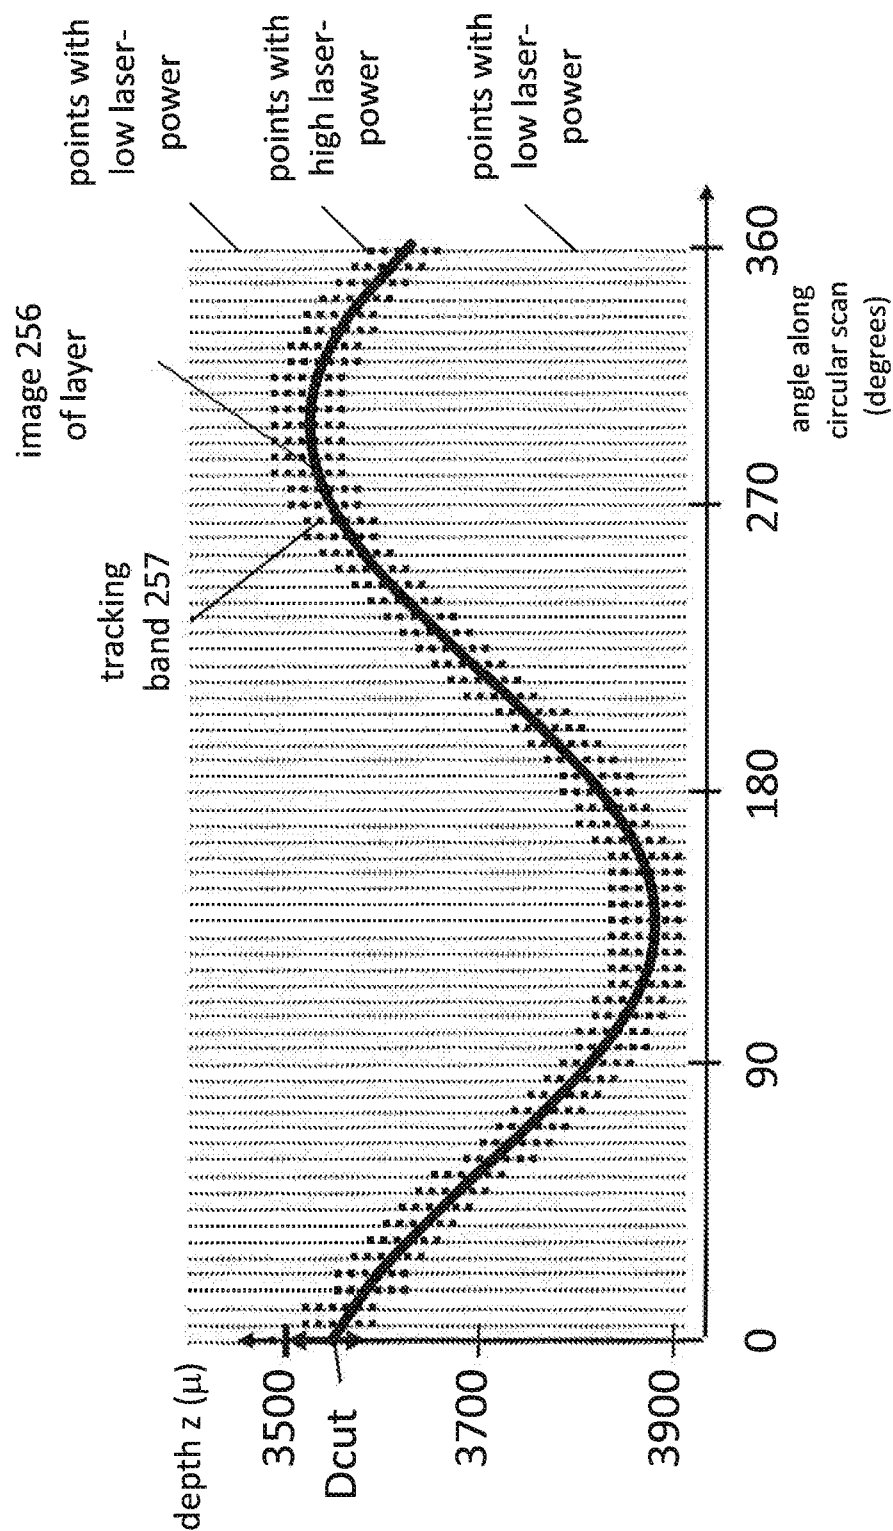


FIG. 6A

Replacement Sheet

15 / 26

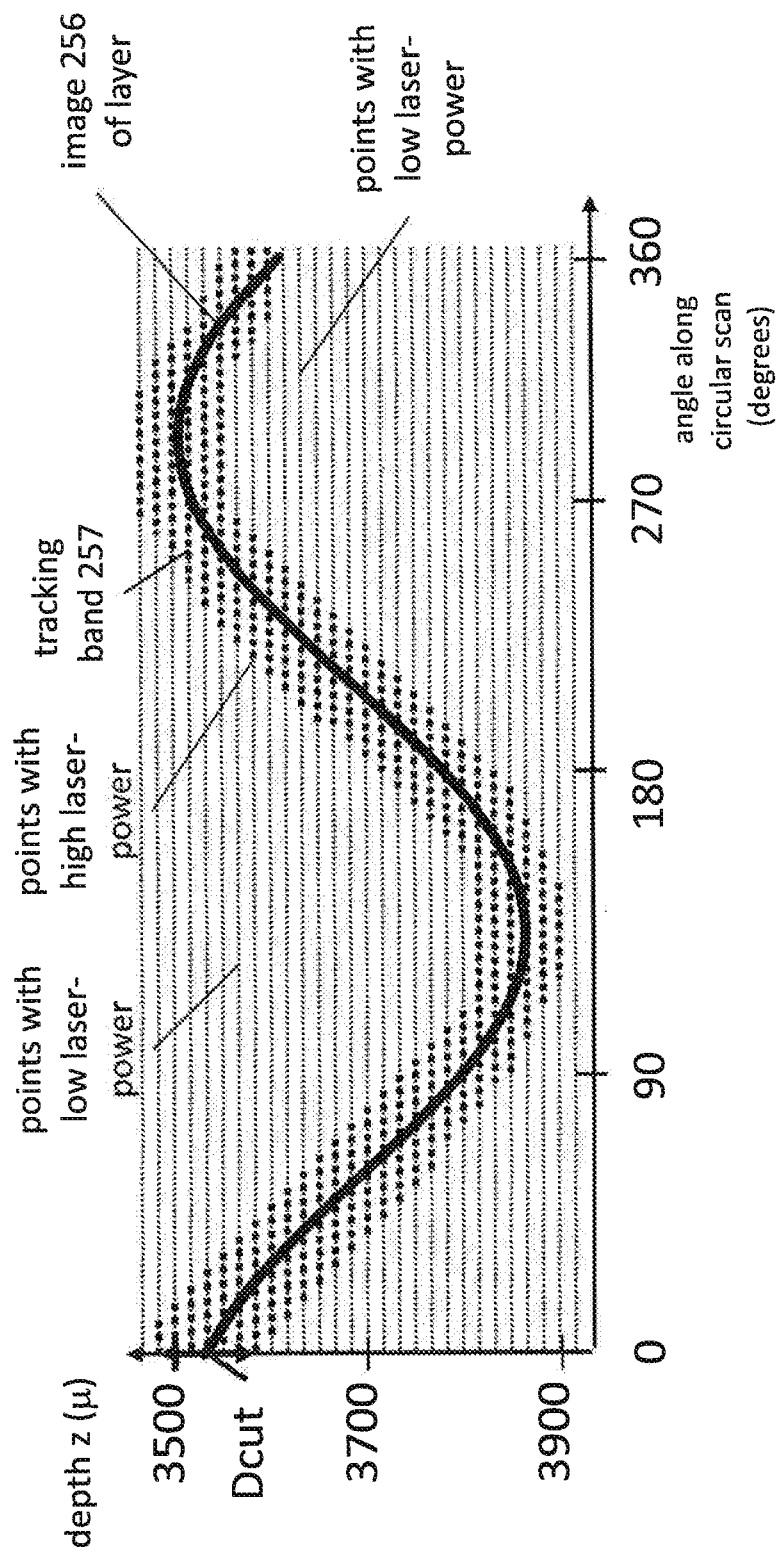


FIG. 6B

Replacement Sheet

16 / 26

FIG. 6C

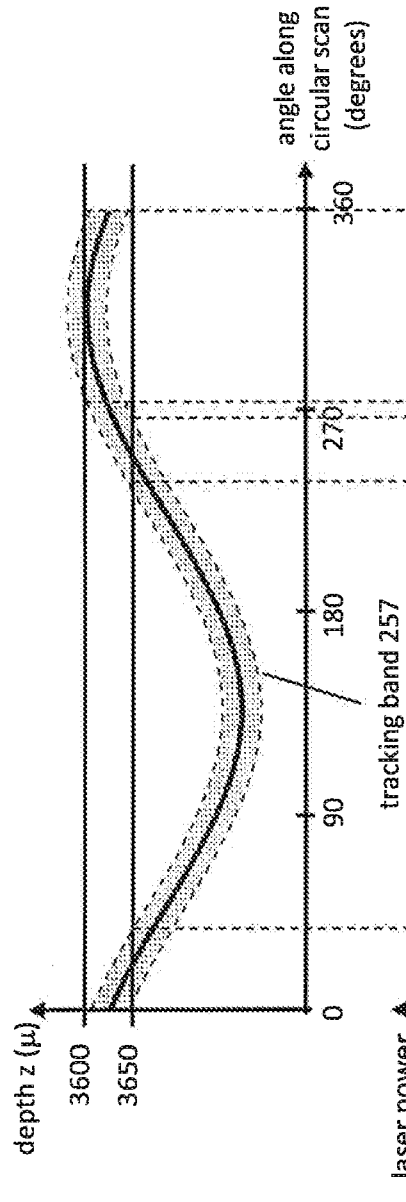


FIG. 6D


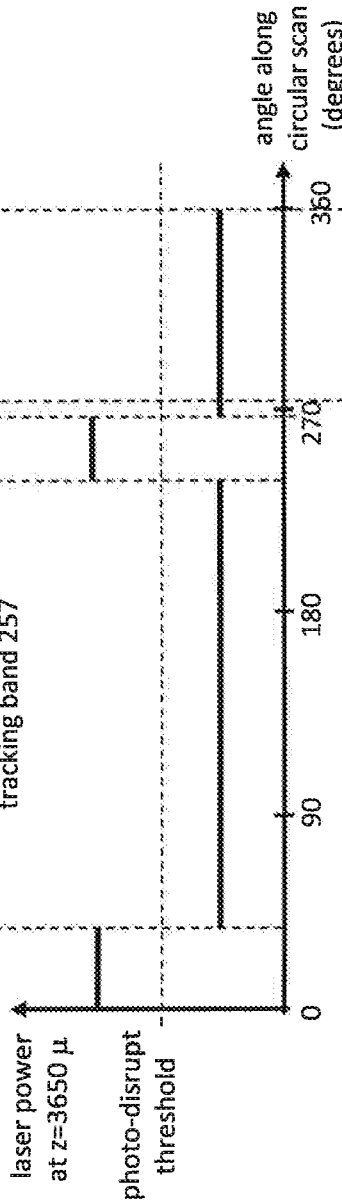


FIG. 6E

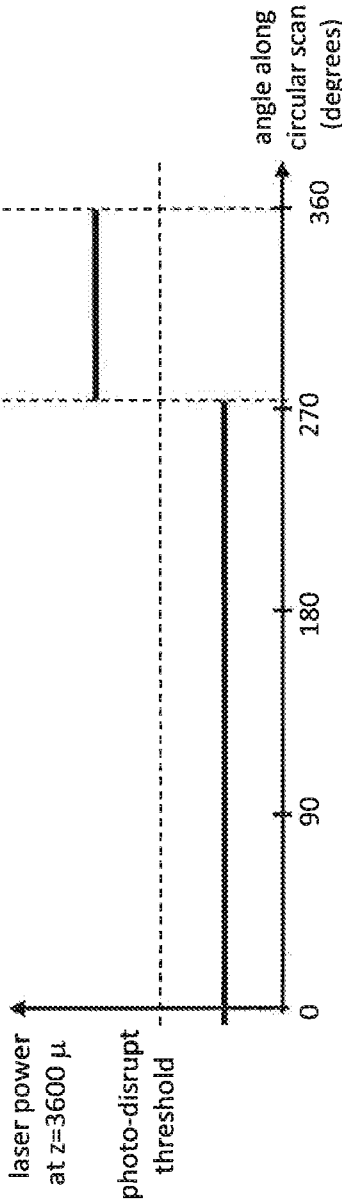

Replacement Sheet

17 / 26

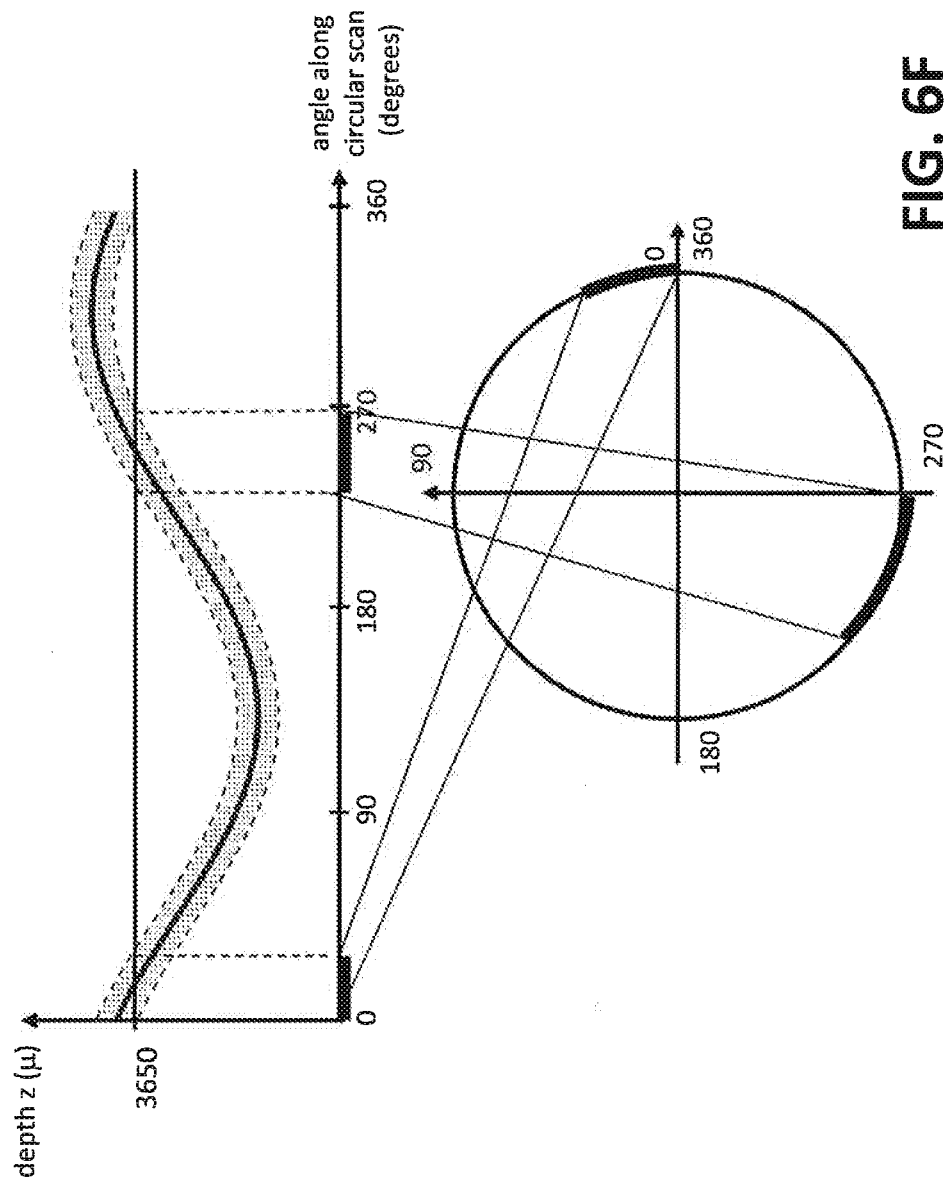


FIG. 6F

Replacement Sheet

18 / 26

FIG. 6G


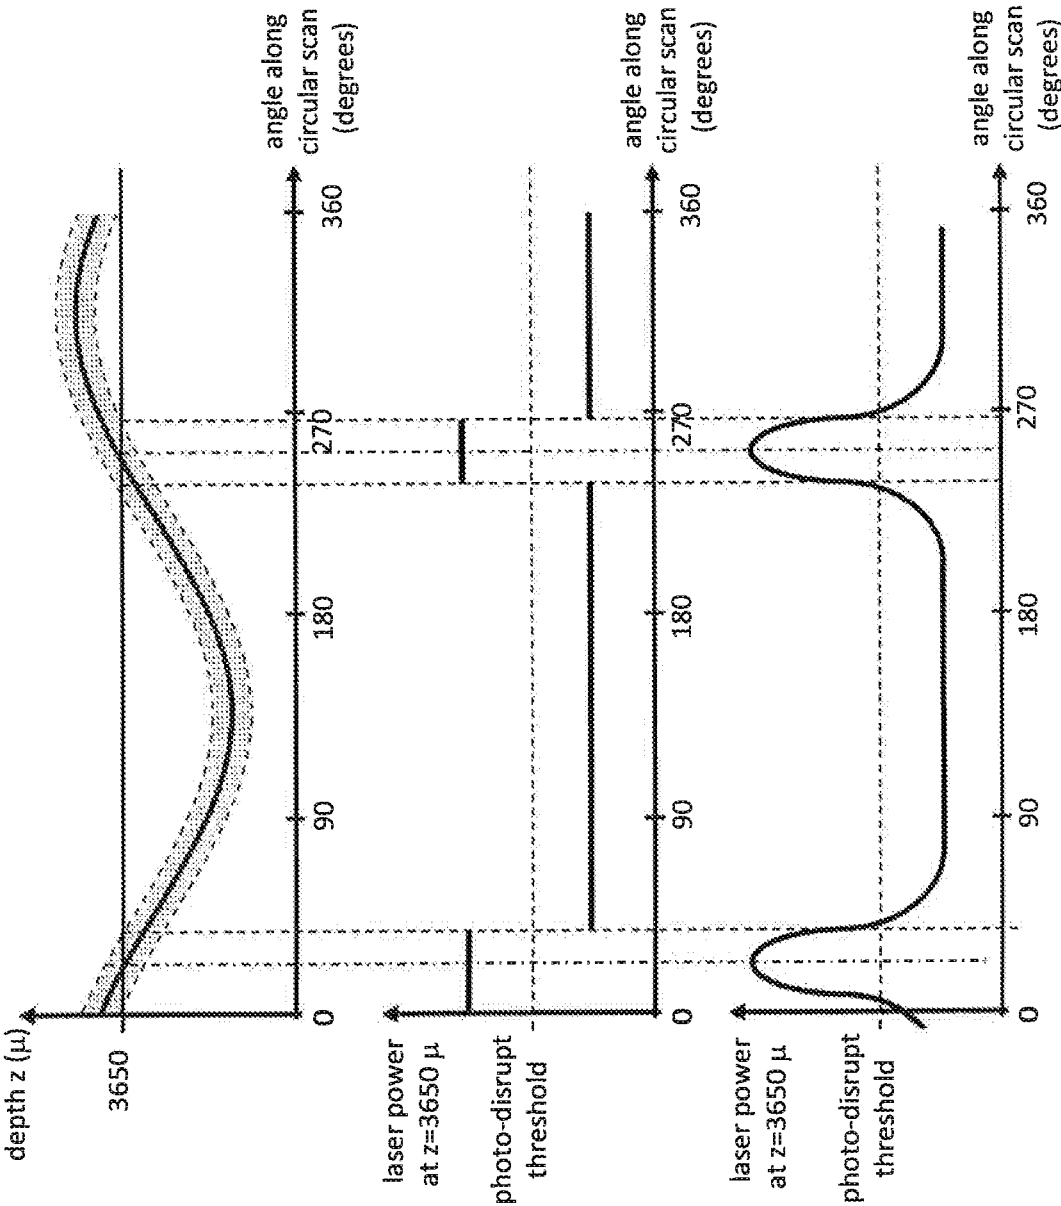


FIG. 6H

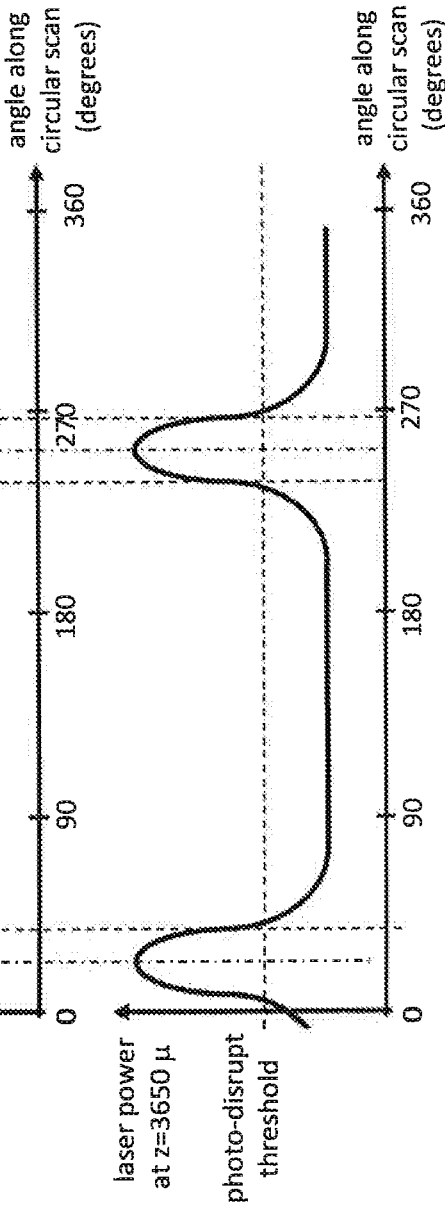

Replacement Sheet

19 / 26

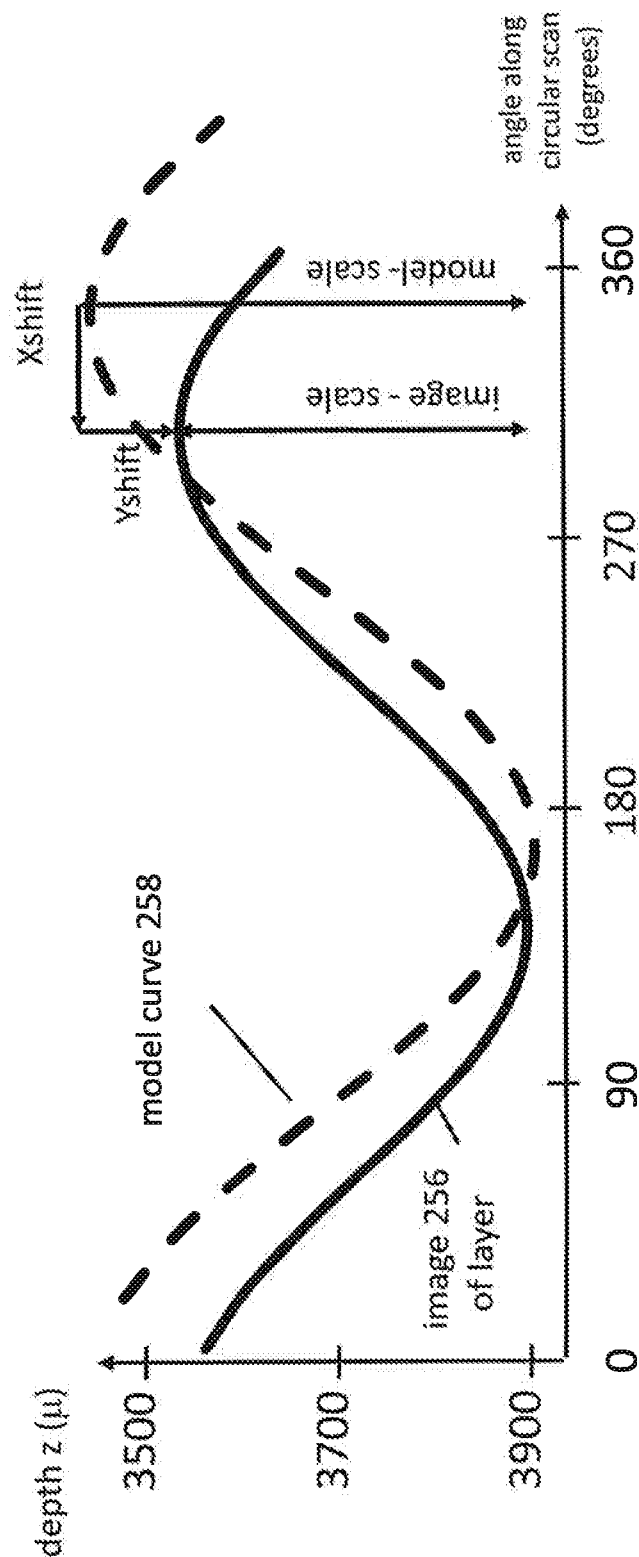


FIG. 7

Replacement Sheet

20 / 26

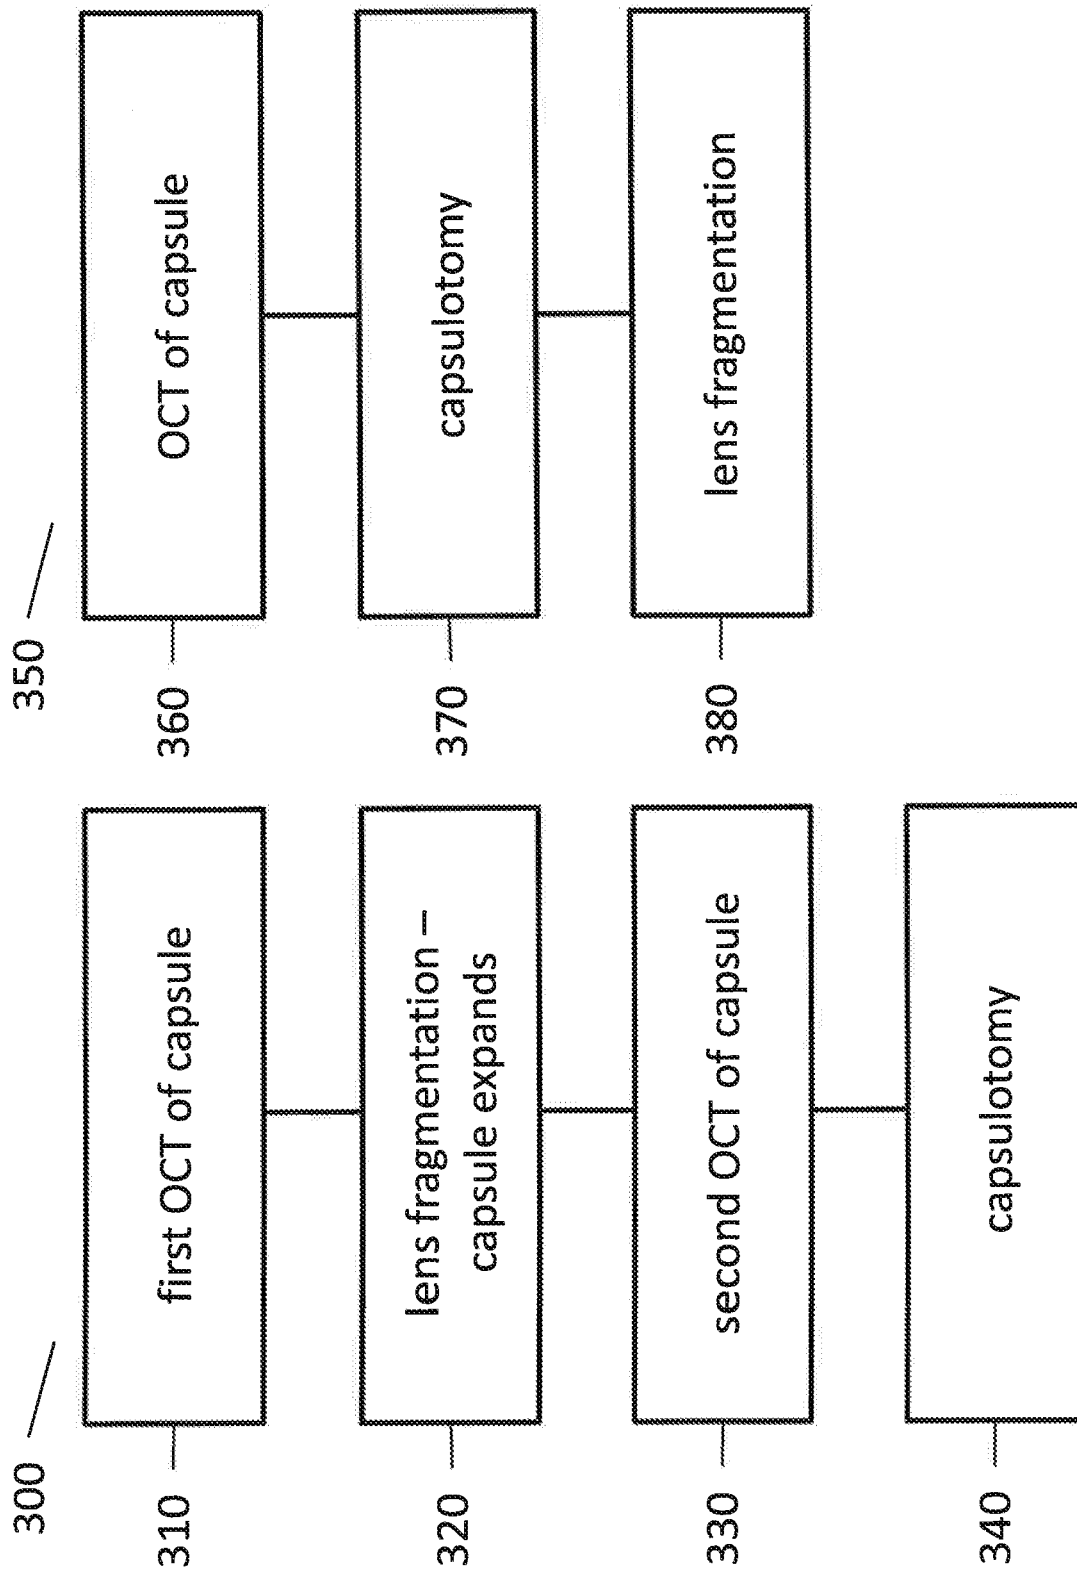


FIG. 8B

FIG. 8A

Replacement Sheet

21 / 26

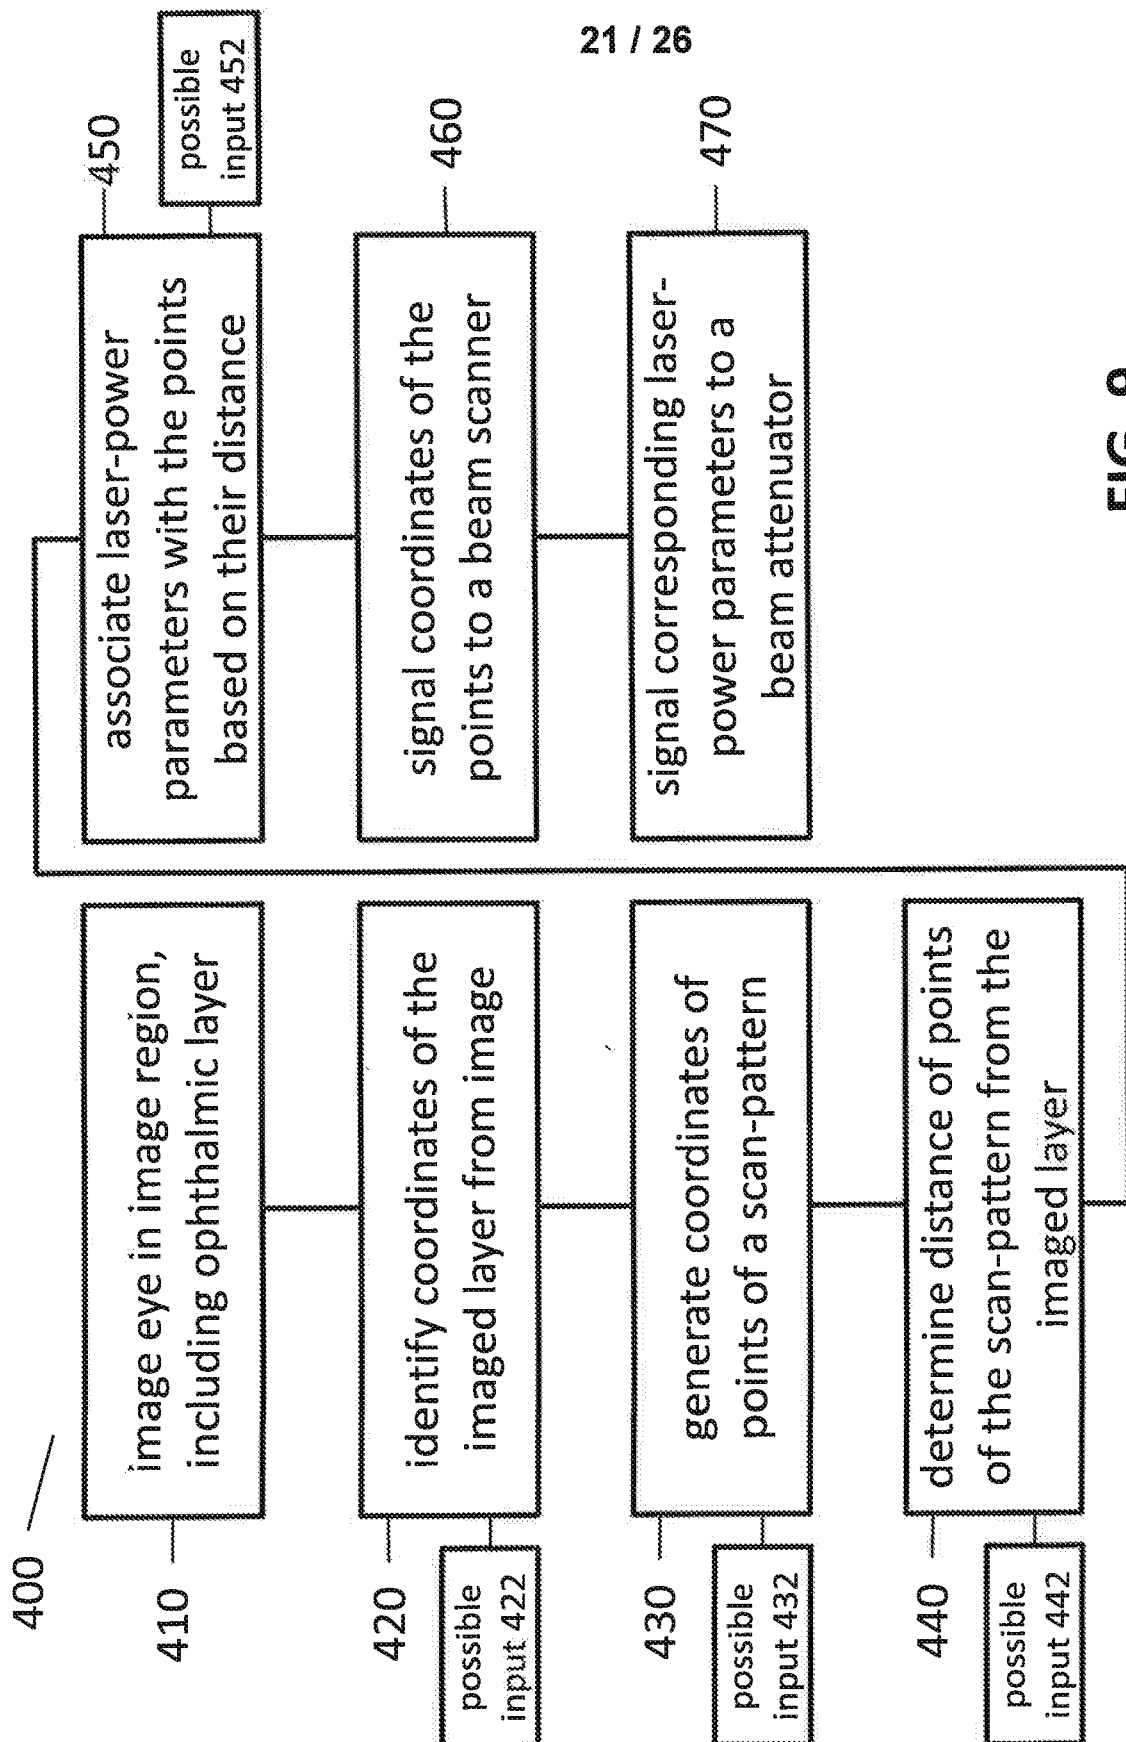


FIG. 9

Replacement Sheet

22 / 26

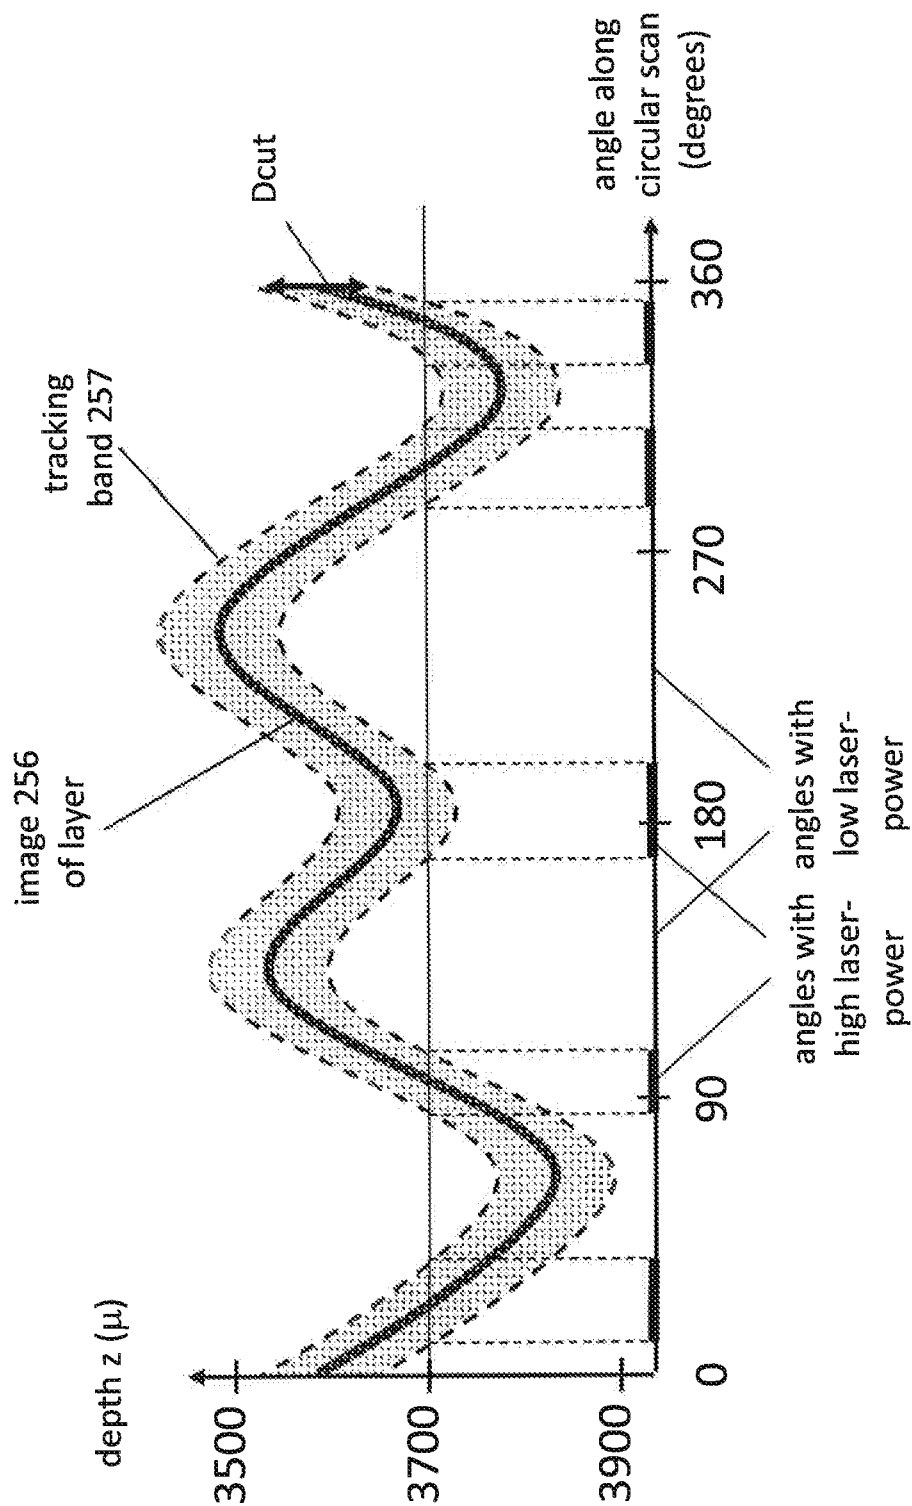


FIG. 10

Replacement Sheet

23 / 26

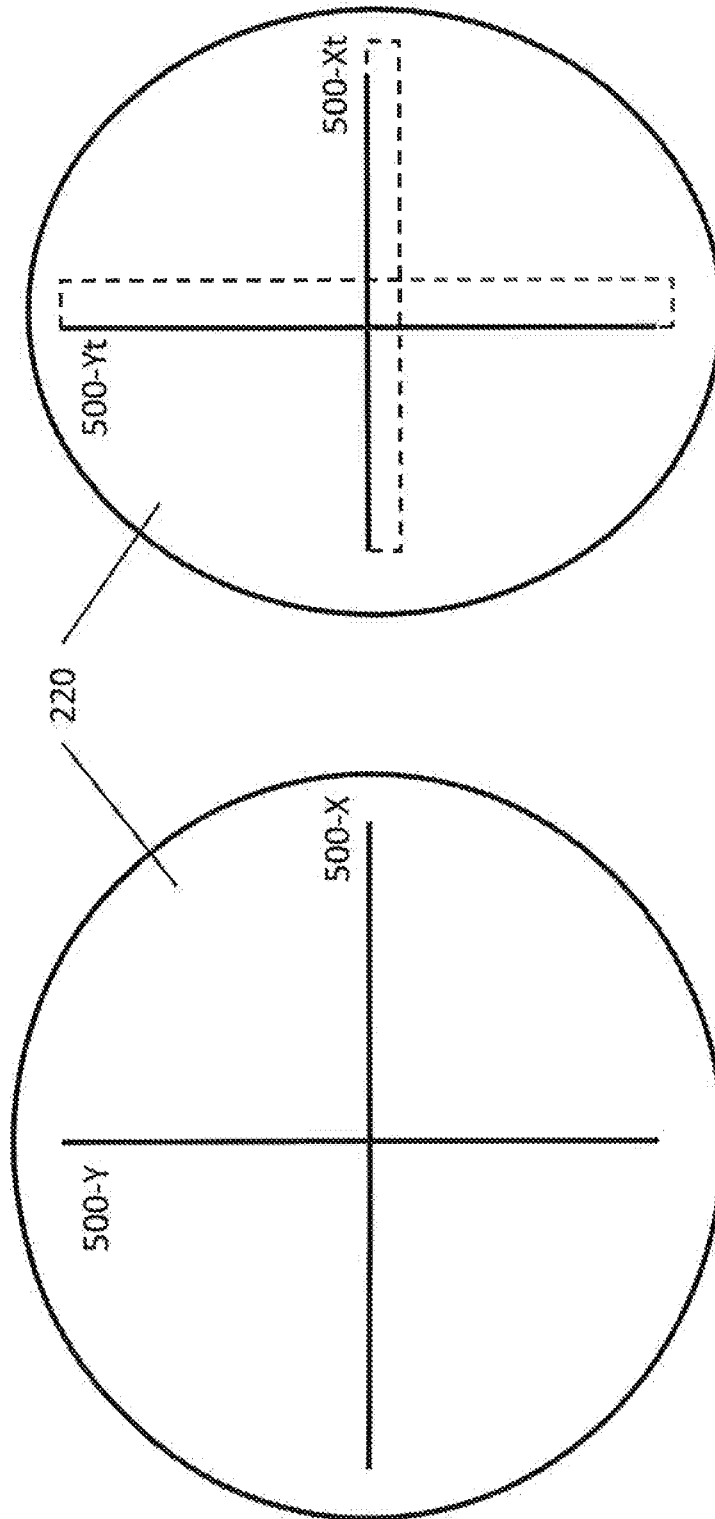


FIG. 11B

FIG. 11A

Replacement Sheet

24 / 26

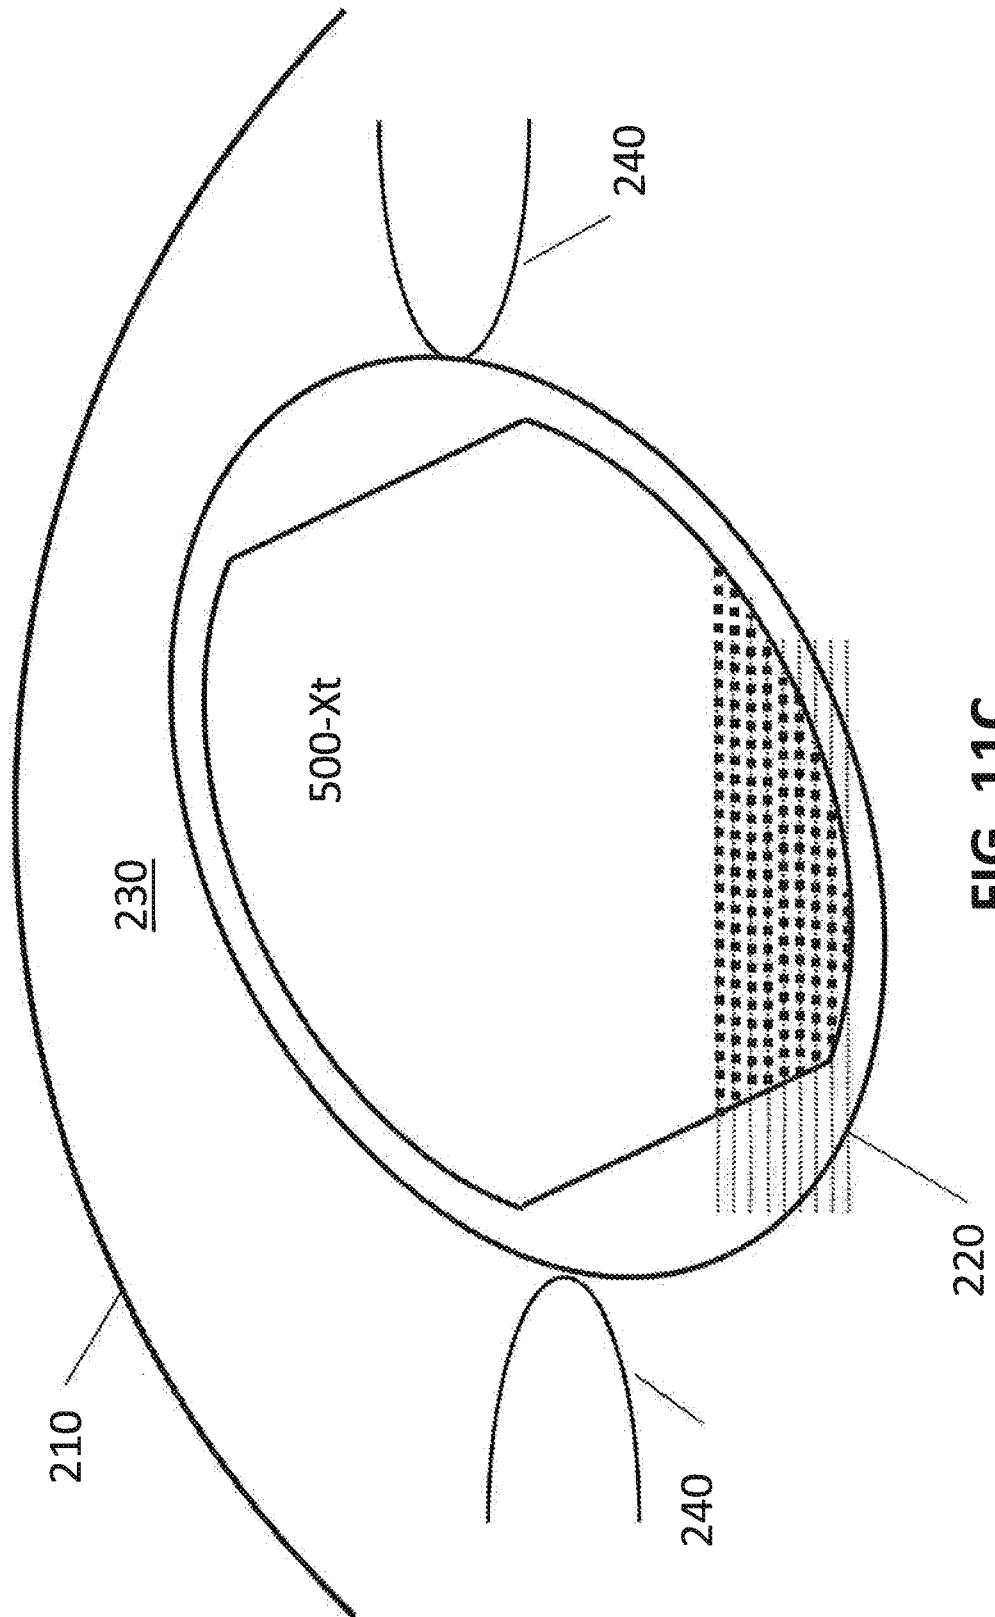


FIG. 11C

Replacement Sheet

25 / 26

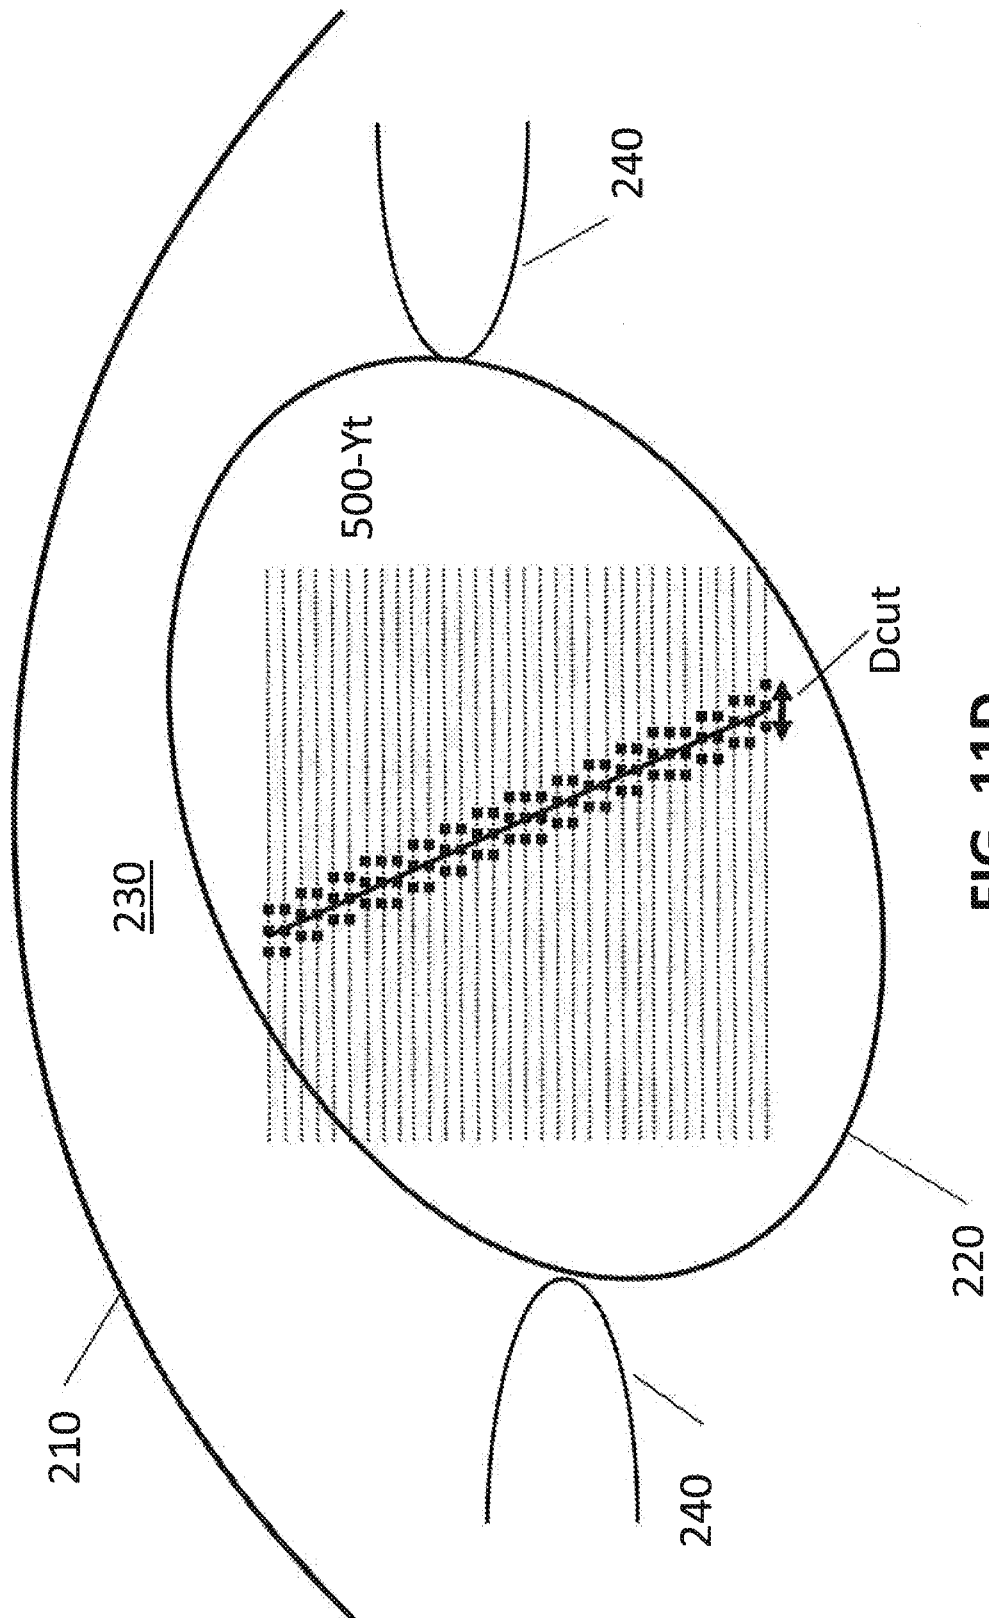


FIG. 11D

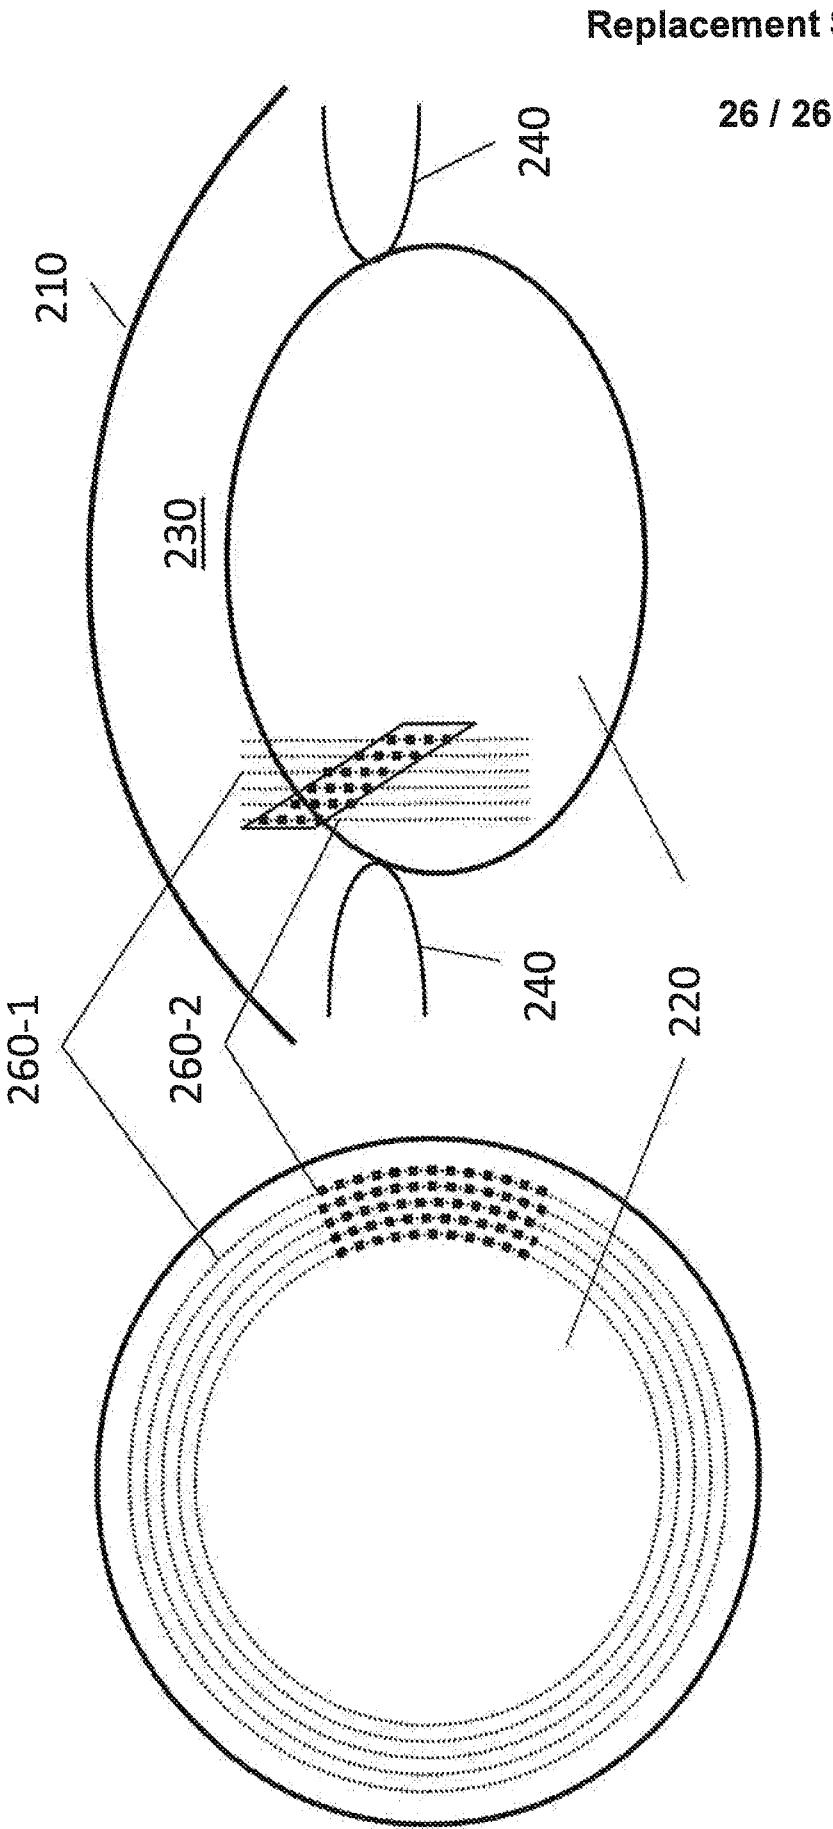


FIG. 12B

FIG. 12A

INTERNATIONAL SEARCH REPORT

International application No

PCT/US2011/051360

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61F9/008 A61B18/20
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61F A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2010/324543 A1 (KURTZ RONALD M [US] ET AL) 23 December 2010 (2010-12-23) figures 12-16, 18, 25, 26 paragraphs [0179], [0188] - [0190], [0210] - [0212] -----	1,2, 7-13, 17-22, 26,27, 30,32
X	US 2011/022036 A1 (FREY RUDOLPH W [US] ET AL) 27 January 2011 (2011-01-27) paragraphs [0045] - [0048], [0052], [0062], [0081], [0092], [0095], [0098], [0103] - [0105] claim 1 figures 8A-8D13, 14, 15 ----- -/-	1-13, 17-22, 25-27, 30,32



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

3 January 2012

Date of mailing of the international search report

29/06/2012

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Jansen, Birte

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2011/051360

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-13, 17-22, 25-27, 30, 32

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International application No

PCT/US2011/051360

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 2006/074469 A2 (OPTIMEDICA CORP [US]; BLUMENKRANZ MARK S [US]; PALANKER DANIEL V [US];) 13 July 2006 (2006-07-13) the whole document -----	1-13, 17-22, 25-27, 30,32

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-13, 17-22, 25-27, 30, 32

Imaging-based laser system with adjustable pulse power.

2. claims: 35-40

Imaging-based laser system, wherein the target pattern is tilted relative to an optical axis of the laser system;

3. claims: 14-16, 23, 24, 28, 29, 41-44

Method for performing an imaging-controlled ophthalmic procedure by identifying coordinates of the imaged layer in part by receiving an operator-input through an operator interface.

4. claims: 31, 33, 34

Imaging-based laser system that is configured to perform a capsulotomy before a lens fragmentation during a cataract procedure.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2011/051360

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2010324543 A1	23-12-2010	US 2010324543 A1	23-12-2010
		WO 2011163508 A2	29-12-2011

US 2011022036 A1	27-01-2011	AU 2010275380 A1	16-02-2012
		CA 2769097 A1	27-01-2011
		EP 2456385 A1	30-05-2012
		US 2011022036 A1	27-01-2011
		WO 2011011788 A1	27-01-2011

WO 2006074469 A2	13-07-2006	AU 2006203794 A1	13-07-2006
		EP 1835861 A2	26-09-2007
		JP 2008526384 A	24-07-2008
		US 2006195076 A1	31-08-2006
		US 2010191226 A1	29-07-2010
		US 2011178511 A1	21-07-2011
		US 2011178512 A1	21-07-2011
		WO 2006074469 A2	13-07-2006

专利名称(译)	成像控制的激光手术系统		
公开(公告)号	EP2688531A1	公开(公告)日	2014-01-29
申请号	EP2011764383	申请日	2011-09-13
申请(专利权)人(译)	ALCON LENSX INC.		
当前申请(专利权)人(译)	ALCON LENSX INC.		
[标]发明人	CHAUDHARY GAUTAM GOLDSTEIN PETER HEGEDUS IMRE SUAREZ CARLOS GERMAN CALLIGORI DAVID KARAVITIS MICHAEL		
发明人	CHAUDHARY, GAUTAM GOLDSTEIN, PETER HEGEDUS, IMRE SUÁREZ, CARLOS GERMAN CALLIGORI, DAVID KARAVITIS, MICHAEL		
IPC分类号	A61F9/008 A61B18/20 A61B18/00		
CPC分类号	A61F9/00825 A61B2018/00636 A61F2009/00844 A61F2009/00851 A61F2009/0087 A61F2009/00889		
优先权	13/110352 2011-05-18 US		
其他公开文献	EP2688531B1		
外部链接	Espacenet		

摘要(译)

基于成像的激光系统可以包括激光束系统，其被配置为生成并扫描具有可调激光功率参数的激光脉冲束到眼睛中的扫描图案的点，以及基于成像的激光控制器。 ，被配置为对眼睛中的层成像，以控制激光脉冲束扫描到扫描图案的点，并根据点的距离控制激光脉冲的激光功率参数。来自成像图层的扫描图案。