



US010034684B2

(12) **United States Patent**
Weisenburgh, II et al.

(10) **Patent No.:** **US 10,034,684 B2**
(45) **Date of Patent:** **Jul. 31, 2018**

(54) **APPARATUS AND METHOD FOR
DISSECTING AND COAGULATING TISSUE**

(71) Applicant: **Ethicon Endo-Surgery, LLC**,
Guaynabo, PR (US)

(72) Inventors: **William B. Weisenburgh, II**,
Maineville, OH (US); **Gregory W.
Johnson**, Milford, OH (US); **Cory G.
Kimball**, Hamilton, OH (US)

(73) Assignee: **Ethicon LLC**, Guaynabo, PR (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 268 days.

(21) Appl. No.: **14/739,792**

(22) Filed: **Jun. 15, 2015**

(65) **Prior Publication Data**

US 2016/0361084 A1 Dec. 15, 2016

(51) **Int. Cl.**
A61B 17/32 (2006.01)
A61N 7/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 17/320068** (2013.01); **A61B
17/320092** (2013.01); **A61N 7/00** (2013.01);
A61B 17/24 (2013.01); **A61B 2017/00477**
(2013.01); **A61B 2017/00991** (2013.01); **A61B
2017/320076** (2013.01); **A61B 2017/320084**
(2013.01); **A61B 2018/00589** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC **A61B 17/320068**; **A61B 17/320092**; **A61B
17/22004**; **A61B 17/3207**; **A61B
17/320783**; **A61B 2017/00296**; **A61B
2017/00778**; **A61B 17/24**; **A61B**

2017/00477; **A61B 2017/00991**; **A61B
2017/320076**; **A61B 2017/320084**; **A61B
2018/00607**; **A61B 2018/00994**; **A61B
2217/007**; **A61N 7/00**

USPC **606/169**; **604/22**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

969,528 A 9/1910 Disbrow
1,570,025 A 1/1926 Young
(Continued)

FOREIGN PATENT DOCUMENTS

AU 2003241752 A1 9/2003
CA 2535467 A1 4/1993
(Continued)

OTHER PUBLICATIONS

International Search Report for PCT/US2016/035958, dated Aug. 9,
2016 (4 pages).


(Continued)

Primary Examiner — Katherine M Shi

(57) **ABSTRACT**

A surgical instrument for cutting and coagulating tissue is provided that includes an elongate sheath and an ultrasonic blade. In one embodiment, an ultrasonic blade is positioned within a sheath such that movement of the sheath relative to the blade results in the dissection and/or coagulation of tissue therebetween. In another embodiment, an ultrasonic blade is positioned within a sheath such that movement of the blade relative to the sheath results in the dissection and/or coagulation of tissue therebetween. The size and shape of distal ends of the blade and sheath determine the size and shape of the tissue being cut and/or removed from a body.

8 Claims, 14 Drawing Sheets

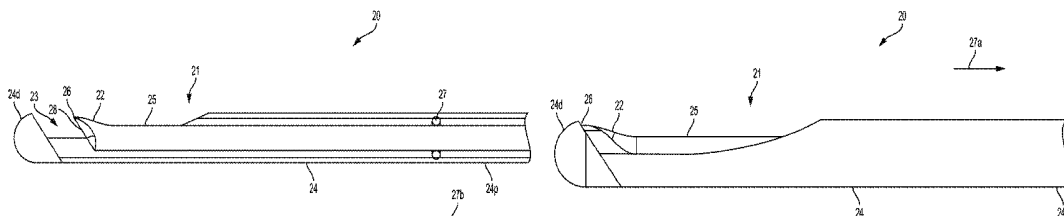

(51)	Int. Cl.		4,617,927 A	10/1986	Manes
	A61B 18/00	(2006.01)	4,633,119 A	12/1986	Thompson
	A61B 17/00	(2006.01)	4,634,420 A	1/1987	Spinosa et al.
	A61B 17/24	(2006.01)	4,640,279 A	2/1987	Beard
(52)	U.S. Cl.		4,641,053 A	2/1987	Takeda
			4,646,738 A	3/1987	Trott
			4,646,756 A	3/1987	Watmough et al.
	CPC	A61B 2018/00607 (2013.01); A61B	4,649,919 A	3/1987	Thimsen et al.
		2018/00994 (2013.01); A61B 2217/007	4,662,068 A	5/1987	Polonsky
		(2013.01)	4,674,502 A	6/1987	Imonti
			4,708,127 A	11/1987	Abdelghani
			4,712,722 A	12/1987	Hood et al.
			4,808,154 A	2/1989	Freeman
			4,819,635 A	4/1989	Shapiro
(56)	References Cited		4,827,911 A	5/1989	Broadwin et al.
	U.S. PATENT DOCUMENTS		4,832,683 A	5/1989	Idemoto et al.
			4,836,186 A	6/1989	Scholz
			4,838,853 A	6/1989	Parisi
			4,844,064 A	7/1989	Thimsen et al.
			4,850,354 A	7/1989	McGurk-Burleson et al.
			4,852,578 A	8/1989	Companion et al.
			4,860,745 A	8/1989	Farin et al.
			4,862,890 A	9/1989	Stasz et al.
			4,865,159 A	9/1989	Jamison
			4,867,157 A	9/1989	McGurk-Burleson et al.
			4,878,493 A	11/1989	Pasternak et al.
			4,881,550 A	11/1989	Kothe
			4,896,009 A	1/1990	Pawlowski
			4,903,696 A	2/1990	Stasz et al.
			4,915,643 A	4/1990	Samejima et al.
			4,922,902 A	5/1990	Wuchinich et al.
			4,965,532 A	10/1990	Sakurai
			4,979,952 A	12/1990	Kubota et al.
			4,981,756 A	1/1991	Rhandhawa
			5,013,956 A	5/1991	Kurozumi et al.
			5,015,227 A	5/1991	Broadwin et al.
			5,026,370 A	6/1991	Lottick
			5,026,387 A	6/1991	Thomas
			5,035,695 A	7/1991	Weber, Jr. et al.
			5,042,707 A	8/1991	Taheri
			5,084,052 A	1/1992	Jacobs
			5,105,117 A	4/1992	Yamaguchi
			5,109,819 A	5/1992	Custer et al.
			5,112,300 A	5/1992	Ureche
			5,123,903 A	6/1992	Quaid et al.
			5,126,618 A	6/1992	Takahashi et al.
			D327,872 S	7/1992	McMills et al.
			5,152,762 A	10/1992	McElhenney
			5,162,044 A	11/1992	Gahn et al.
			5,163,421 A	11/1992	Bernstein et al.
			5,163,537 A	11/1992	Radev
			5,167,725 A	12/1992	Clark et al.
			5,172,344 A	12/1992	Ehrlich
			5,174,276 A	12/1992	Crockard
			D332,660 S	1/1993	Rawson et al.
			5,176,677 A	1/1993	Wuchinich
			5,176,695 A	1/1993	Dulebohn
			5,184,605 A	2/1993	Grezeszykowski
			5,188,102 A	2/1993	Idemoto et al.
			D334,173 S	3/1993	Liu et al.
			5,209,719 A	5/1993	Baruch et al.
			5,213,569 A	5/1993	Davis
			5,214,339 A	5/1993	Naito
			5,218,529 A	6/1993	Meyer et al.
			5,221,282 A	6/1993	Wuchinich
			5,222,937 A	6/1993	Kagawa
			5,226,909 A	7/1993	Evans et al.
			5,226,910 A	7/1993	Kajiyama et al.
			5,241,236 A	8/1993	Sasaki et al.
			5,241,968 A	9/1993	Slater
			5,242,460 A	9/1993	Klein et al.
			5,254,129 A	10/1993	Alexander
			5,257,988 A	11/1993	L'Esperance, Jr.
			5,261,922 A	11/1993	Hood
			5,263,957 A	11/1993	Davison
			5,264,925 A	11/1993	Shipp et al.
			5,275,166 A	1/1994	Vaitekunas et al.
			5,275,607 A	1/1994	Lo et al.
			5,275,609 A	1/1994	Pingleton et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,282,800	A	2/1994	Foshee et al.	5,630,420	A	5/1997	Vaitekunas
5,282,817	A	2/1994	Hoogeboom et al.	5,632,717	A	5/1997	Yoon
5,285,795	A	2/1994	Ryan et al.	5,640,741	A	6/1997	Yano
5,300,068	A	4/1994	Rosar et al.	D381,077	S	7/1997	Hunt
5,304,115	A	4/1994	Pflueger et al.	5,649,937	A	7/1997	Bito
D347,474	S	5/1994	Olson	5,651,780	A	7/1997	Jackson et al.
5,307,976	A	5/1994	Olson et al.	5,653,713	A	8/1997	Michelson
5,312,023	A	5/1994	Green et al.	5,662,662	A	9/1997	Bishop et al.
5,312,425	A	5/1994	Evans et al.	5,669,922	A	9/1997	Hood
5,322,055	A	6/1994	Davison et al.	5,674,235	A	10/1997	Parisi
5,324,299	A	6/1994	Davison et al.	5,678,568	A	10/1997	Uchikubo et al.
5,326,013	A	7/1994	Green et al.	5,690,269	A	11/1997	Bolanos et al.
5,326,342	A	7/1994	Pflueger et al.	5,694,936	A	12/1997	Fujimoto et al.
5,344,420	A	9/1994	Hilal et al.	5,695,510	A	12/1997	Hood
5,345,937	A	9/1994	Middleman et al.	5,700,261	A	12/1997	Brinkerhoff
5,346,502	A	9/1994	Estabrook et al.	5,704,534	A	1/1998	Huitema et al.
5,353,474	A	10/1994	Good et al.	5,709,680	A	1/1998	Yates et al.
5,357,164	A	10/1994	Imabayashi et al.	5,711,472	A	1/1998	Bryan
5,357,423	A	10/1994	Weaver et al.	5,713,896	A	2/1998	Nardella
5,359,994	A	11/1994	Krauter et al.	5,715,817	A	2/1998	Stevens-Wright et al.
5,366,466	A	11/1994	Christian et al.	5,717,306	A	2/1998	Shipp
5,368,557	A	11/1994	Nita et al.	5,728,130	A	3/1998	Ishikawa et al.
5,370,645	A	12/1994	Kliceck et al.	5,730,752	A	3/1998	Alden et al.
5,371,429	A	12/1994	Manna	5,733,074	A	3/1998	Stöck et al.
5,374,813	A	12/1994	Shipp	5,741,226	A	4/1998	Strukel et al.
D354,564	S	1/1995	Medema	5,766,164	A	6/1998	Mueller et al.
5,381,067	A	1/1995	Greenstein et al.	5,772,659	A	6/1998	Becker et al.
5,387,215	A	2/1995	Fisher	5,776,155	A	7/1998	Beaupre et al.
5,389,098	A	2/1995	Tsuruta et al.	5,792,135	A	8/1998	Madhani et al.
5,394,187	A	2/1995	Shipp	5,792,138	A	8/1998	Shipp
5,396,266	A	3/1995	Brimhall	5,792,165	A	8/1998	Klieman et al.
5,403,312	A	4/1995	Yates et al.	5,797,959	A	8/1998	Castro et al.
5,403,334	A	4/1995	Evans et al.	5,805,140	A	9/1998	Rosenberg et al.
5,408,268	A	4/1995	Shipp	5,807,393	A	9/1998	Williamson, IV et al.
D358,887	S	5/1995	Feinberg	5,808,396	A	9/1998	Boukhny
5,411,481	A	5/1995	Allen et al.	5,810,859	A	9/1998	DiMatteo et al.
5,419,761	A	5/1995	Narayanan et al.	5,817,084	A	10/1998	Jensen
5,421,829	A	6/1995	Olichney et al.	5,817,119	A	10/1998	Klieman et al.
5,423,844	A	6/1995	Miller	5,823,197	A	10/1998	Edwards
5,438,997	A	8/1995	Sieben et al.	5,827,323	A	10/1998	Klieman et al.
5,445,639	A	8/1995	Kuslich et al.	5,828,160	A	10/1998	Sugishita
5,449,370	A	9/1995	Vaitekunas	5,833,696	A	11/1998	Whitfield et al.
5,451,220	A	9/1995	Ciervo	5,836,897	A	11/1998	Sakurai et al.
5,456,684	A	10/1995	Schmidt et al.	5,836,957	A	11/1998	Schulz et al.
5,471,988	A	12/1995	Fujio et al.	5,843,109	A	12/1998	Mehta et al.
5,472,443	A	12/1995	Cordis et al.	5,851,212	A	12/1998	Zirps et al.
5,478,003	A	12/1995	Green et al.	5,858,018	A	1/1999	Shipp et al.
5,483,501	A	1/1996	Park et al.	5,865,361	A	2/1999	Milliman et al.
5,486,162	A	1/1996	Brumbach	5,873,873	A	2/1999	Smith et al.
5,490,860	A	2/1996	Middle et al.	5,873,882	A	2/1999	Straub et al.
5,500,216	A	3/1996	Julian et al.	5,878,193	A	3/1999	Wang et al.
5,501,654	A	3/1996	Failla et al.	5,879,364	A	3/1999	Bromfield et al.
5,505,693	A	4/1996	Mackool	5,883,615	A	3/1999	Fago et al.
5,507,738	A	4/1996	Ciervo	5,893,835	A	4/1999	Witt et al.
5,527,331	A	6/1996	Kresch et al.	5,897,523	A	4/1999	Wright et al.
5,540,693	A	7/1996	Fisher	5,897,569	A	4/1999	Kellogg et al.
5,553,675	A	9/1996	Pitzen et al.	5,903,607	A	5/1999	Tailliet
5,558,671	A	9/1996	Yates	5,904,681	A	5/1999	West, Jr.
5,562,609	A	10/1996	Brumbach	5,906,627	A	5/1999	Spaulding
5,562,610	A	10/1996	Brumbach	5,906,628	A	5/1999	Miyawaki et al.
5,562,659	A	10/1996	Morris	5,911,699	A	6/1999	Anis et al.
5,573,424	A	11/1996	Poppe	5,916,229	A	6/1999	Evans
5,577,654	A	11/1996	Bishop	5,929,846	A	7/1999	Rosenberg et al.
5,591,187	A	1/1997	Dekel	5,935,143	A	8/1999	Hood
5,593,414	A	1/1997	Shipp et al.	5,935,144	A	8/1999	Estabrook
5,601,601	A	2/1997	Tal et al.	5,938,633	A	8/1999	Beaupre
5,603,773	A	2/1997	Campbell	5,944,718	A	8/1999	Austin et al.
5,607,436	A	3/1997	Pratt et al.	5,944,737	A	8/1999	Tsonton et al.
5,609,573	A	3/1997	Sandock	5,947,984	A	9/1999	Whipple
5,618,304	A	4/1997	Hart et al.	5,954,736	A	9/1999	Bishop et al.
5,618,492	A	4/1997	Auten et al.	5,954,746	A	9/1999	Holthaus et al.
5,620,447	A	4/1997	Smith et al.	5,957,882	A	9/1999	Nita et al.
5,626,587	A	5/1997	Bishop et al.	5,957,943	A	9/1999	Vaitekunas
5,626,595	A	5/1997	Sklar et al.	5,968,007	A	10/1999	Simon et al.
5,628,760	A	5/1997	Knoepfler	5,968,060	A	10/1999	Kellogg
				5,974,342	A	10/1999	Petrofsky
				D416,089	S	11/1999	Barton et al.
				5,980,510	A	11/1999	Tsonton et al.
				5,980,546	A	11/1999	Hood

(56)

References Cited

U.S. PATENT DOCUMENTS

5,989,274 A	11/1999	Davison et al.	6,273,852 B1	8/2001	Lehe et al.
5,989,275 A	11/1999	Estabrook et al.	6,274,963 B1	8/2001	Estabrook et al.
5,993,465 A	11/1999	Shipp et al.	6,277,115 B1	8/2001	Saadat
5,993,972 A	11/1999	Reich et al.	6,278,218 B1	8/2001	Madan et al.
5,994,855 A	11/1999	Lundell et al.	6,280,407 B1	8/2001	Manna et al.
6,024,741 A	2/2000	Williamson, IV et al.	6,283,981 B1	9/2001	Beaupre
6,024,750 A	2/2000	Mastri et al.	6,287,344 B1	9/2001	Wampler et al.
6,027,515 A	2/2000	Cimino	6,290,575 B1	9/2001	Shipp
6,031,526 A	2/2000	Shipp	6,299,591 B1	10/2001	Banko
6,033,375 A	3/2000	Brumbach	6,306,131 B1	10/2001	Hareyama
6,033,399 A	3/2000	Gines	6,306,157 B1	10/2001	Shchervinsky
6,036,667 A	3/2000	Manna et al.	6,309,400 B2	10/2001	Beaupre
6,036,707 A	3/2000	Spaulding	6,311,783 B1	11/2001	Harpell
6,048,224 A	4/2000	Kay	6,319,221 B1	11/2001	Savage et al.
6,050,943 A	4/2000	Slayton et al.	6,325,795 B1	12/2001	Lindemann et al.
6,051,010 A	4/2000	DiMatteo et al.	6,325,799 B1	12/2001	Goble
6,056,735 A	5/2000	Okada et al.	6,325,811 B1	12/2001	Messerly
6,063,098 A	5/2000	Houser et al.	6,328,751 B1	12/2001	Beaupre
6,066,132 A	5/2000	Chen et al.	6,332,891 B1	12/2001	Himes
6,066,151 A	5/2000	Miyawaki et al.	6,338,657 B1	1/2002	Harper et al.
6,068,627 A	5/2000	Orszulak et al.	6,340,352 B1	1/2002	Okada et al.
6,068,647 A	5/2000	Witt et al.	6,350,269 B1	2/2002	Shipp et al.
6,077,285 A	6/2000	Boukhny	6,352,532 B1	3/2002	Kramer et al.
6,083,191 A	7/2000	Rose	6,358,264 B2	3/2002	Banko
6,086,584 A	7/2000	Miller	6,364,888 B1	4/2002	Niemeyer et al.
6,090,120 A	7/2000	Wright et al.	6,379,320 B1	4/2002	Lafon et al.
6,096,033 A	8/2000	Tu et al.	D457,958 S	5/2002	Dycus et al.
6,099,542 A	8/2000	Cohn et al.	6,383,194 B1	5/2002	Pothula
6,109,500 A	8/2000	Alli et al.	6,384,690 B1	5/2002	Wilhelmsson et al.
6,110,127 A	8/2000	Suzuki	6,387,109 B1	5/2002	Davison et al.
6,113,594 A	9/2000	Savage	6,388,657 B1	5/2002	Natoli
6,117,152 A	9/2000	Huitema	6,391,042 B1	5/2002	Cimino
6,126,629 A	10/2000	Perkins	6,398,779 B1	6/2002	Buyse et al.
6,129,735 A	10/2000	Okada et al.	6,402,743 B1	6/2002	Orszulak et al.
6,129,740 A	10/2000	Michelson	6,402,748 B1	6/2002	Schoenman et al.
6,132,368 A	10/2000	Cooper	6,405,733 B1	6/2002	Fogarty et al.
6,132,427 A	10/2000	Jones et al.	6,416,486 B1	7/2002	Wampler
6,132,448 A	10/2000	Perez et al.	6,423,073 B2	7/2002	Bowman
6,139,320 A	10/2000	Hahn	6,423,082 B1	7/2002	Houser et al.
6,139,561 A	10/2000	Shibata et al.	6,425,906 B1	7/2002	Young et al.
6,142,615 A	11/2000	Qiu et al.	6,428,538 B1	8/2002	Blewett et al.
6,142,994 A	11/2000	Swanson et al.	6,428,539 B1	8/2002	Baxter et al.
6,147,560 A	11/2000	Erhage et al.	6,432,118 B1	8/2002	Messerly
6,152,902 A	11/2000	Christian et al.	6,436,114 B1	8/2002	Novak et al.
6,154,198 A	11/2000	Rosenberg	6,436,115 B1	8/2002	Beaupre
6,159,160 A	12/2000	Hsei et al.	6,440,062 B1	8/2002	Ouchi
6,159,175 A	12/2000	Strukel et al.	6,443,968 B1	9/2002	Holthaus et al.
6,162,194 A	12/2000	Shipp	6,443,969 B1	9/2002	Novak et al.
6,165,150 A	12/2000	Banko	6,449,006 B1	9/2002	Shipp
6,174,310 B1	1/2001	Kirwan, Jr.	6,454,781 B1	9/2002	Witt et al.
6,179,853 B1	1/2001	Sachse et al.	6,454,782 B1	9/2002	Schwemberger
6,183,426 B1	2/2001	Akisada et al.	6,458,142 B1	10/2002	Faller et al.
6,193,709 B1	2/2001	Miyawaki et al.	6,475,215 B1	11/2002	Tanrisever
6,204,592 B1	3/2001	Hur	6,480,796 B2	11/2002	Wiener
6,205,855 B1	3/2001	Pfeiffer	6,485,490 B2	11/2002	Wampler et al.
6,206,844 B1	3/2001	Reichel et al.	6,491,701 B2	12/2002	Tierney et al.
6,210,337 B1	4/2001	Dunham et al.	6,491,708 B2	12/2002	Madan et al.
6,210,402 B1	4/2001	Olsen et al.	6,497,715 B2	12/2002	Satou
6,210,403 B1	4/2001	Klicek	6,500,176 B1	12/2002	Truckai et al.
6,214,023 B1	4/2001	Whipple et al.	6,500,188 B2	12/2002	Harper et al.
6,228,080 B1	5/2001	Gines	6,500,312 B2	12/2002	Wedekamp
6,231,565 B1	5/2001	Tovey et al.	6,506,208 B2	1/2003	Hunt et al.
6,233,476 B1	5/2001	Strommer et al.	6,511,478 B1	1/2003	Burnside et al.
6,238,366 B1	5/2001	Savage et al.	6,511,493 B1	1/2003	Moutafis et al.
6,245,065 B1	6/2001	Panescu et al.	6,514,267 B2	2/2003	Jewett
6,251,110 B1	6/2001	Wampler	6,524,251 B2	2/2003	Rabiner et al.
6,252,110 B1	6/2001	Uemura et al.	6,524,316 B1	2/2003	Nicholson et al.
D444,365 S	7/2001	Bass et al.	6,527,736 B1	3/2003	Attinger et al.
D445,092 S	7/2001	Lee	6,533,784 B2	3/2003	Truckai et al.
D445,764 S	7/2001	Lee	6,537,272 B2	3/2003	Christopherson et al.
6,254,623 B1	7/2001	Haibel, Jr. et al.	6,537,291 B2	3/2003	Friedman et al.
6,257,241 B1	7/2001	Wampler	6,543,452 B1	4/2003	Lavigne
6,258,034 B1	7/2001	Hanafy	6,543,456 B1	4/2003	Freeman
6,267,761 B1	7/2001	Ryan	6,544,260 B1	4/2003	Markel et al.
6,270,831 B2	8/2001	Kumar et al.	6,558,376 B2	5/2003	Bishop
			6,561,983 B2	5/2003	Cronin et al.
			6,562,035 B1	5/2003	Levin
			6,565,558 B1	5/2003	Lindenmeier et al.
			6,572,563 B2	6/2003	Ouchi

(56)

References Cited

U.S. PATENT DOCUMENTS

6,572,632 B2	6/2003	Zisterer et al.	6,809,508 B2	10/2004	Donofrio
6,575,969 B1	6/2003	Rittman, III et al.	6,810,281 B2	10/2004	Brock et al.
6,582,427 B1	6/2003	Goble et al.	6,827,712 B2	12/2004	Tovey et al.
6,582,451 B1	6/2003	Marucci et al.	6,828,712 B2	12/2004	Battaglin et al.
D477,408 S	7/2003	Bromley	6,835,082 B2	12/2004	Gonnering
6,588,277 B2	7/2003	Giordano et al.	6,849,073 B2	2/2005	Hoey et al.
6,589,200 B1	7/2003	Schwemberger et al.	6,860,878 B2	3/2005	Brock
6,589,239 B2	7/2003	Khandkar et al.	6,863,676 B2	3/2005	Lee et al.
6,599,288 B2	7/2003	Maguire et al.	6,869,439 B2	3/2005	White et al.
6,607,540 B1	8/2003	Shipp	6,875,220 B2	4/2005	Du et al.
6,610,059 B1	8/2003	West, Jr.	6,877,647 B2	4/2005	Green et al.
6,616,450 B2	9/2003	Mossle et al.	6,882,439 B2	4/2005	Ishijima
6,619,529 B2	9/2003	Green et al.	6,887,209 B2	5/2005	Kadziauskas et al.
6,623,500 B1	9/2003	Cook et al.	6,887,252 B1	5/2005	Okada et al.
6,623,501 B2	9/2003	Heller et al.	6,899,685 B2	5/2005	Kermode et al.
6,626,848 B2	9/2003	Neuenfeldt	6,905,497 B2	6/2005	Truckai et al.
6,626,926 B2	9/2003	Friedman et al.	6,908,472 B2	6/2005	Wiener et al.
6,629,974 B2	10/2003	Penny et al.	6,913,579 B2	7/2005	Truckai et al.
6,633,234 B2	10/2003	Wiener et al.	6,915,623 B2	7/2005	Dey et al.
6,644,532 B2	11/2003	Green et al.	6,923,804 B2	8/2005	Eggers et al.
6,651,669 B1	11/2003	Burnside	6,926,712 B2	8/2005	Phan
6,652,513 B2	11/2003	Panescu et al.	6,926,716 B2	8/2005	Baker et al.
6,652,539 B2	11/2003	Shipp et al.	6,929,602 B2	8/2005	Hirakui et al.
6,652,545 B2	11/2003	Shipp et al.	6,929,632 B2	8/2005	Nita et al.
6,656,132 B1	12/2003	Ouchi	6,929,644 B2	8/2005	Truckai et al.
6,656,177 B2	12/2003	Truckai et al.	6,933,656 B2	8/2005	Matsushita et al.
6,660,017 B2	12/2003	Beaupre	D509,589 S	9/2005	Wells
6,662,127 B2	12/2003	Wiener et al.	6,942,660 B2	9/2005	Pantera et al.
6,663,941 B2	12/2003	Brown et al.	6,942,677 B2	9/2005	Nita et al.
6,666,860 B1	12/2003	Takahashi	6,945,981 B2	9/2005	Donofrio et al.
6,666,875 B1	12/2003	Sakurai et al.	6,946,779 B2	9/2005	Birgel
6,669,690 B1	12/2003	Okada et al.	6,948,503 B2	9/2005	Refior et al.
6,669,710 B2	12/2003	Moutafis et al.	D511,145 S	11/2005	Donofrio et al.
6,676,660 B2	1/2004	Wampler et al.	6,974,450 B2	12/2005	Weber et al.
6,678,621 B2	1/2004	Wiener et al.	6,976,844 B2	12/2005	Hickok et al.
6,679,875 B2	1/2004	Honda et al.	6,976,969 B2	12/2005	Messerly
6,679,899 B2	1/2004	Wiener et al.	6,977,495 B2	12/2005	Donofrio
6,682,544 B2	1/2004	Mastri et al.	6,979,332 B2	12/2005	Adams
6,685,701 B2	2/2004	Orszulak et al.	6,981,628 B2	1/2006	Wales
6,685,703 B2	2/2004	Pearson et al.	6,984,220 B2	1/2006	Wuchinich
6,689,145 B2	2/2004	Lee et al.	6,988,295 B2	1/2006	Tillim
6,689,146 B1	2/2004	Himes	6,994,708 B2	2/2006	Manzo
6,702,821 B2	3/2004	Bonutti	7,001,335 B2	2/2006	Adachi et al.
6,716,215 B1	4/2004	David et al.	7,011,657 B2	3/2006	Truckai et al.
6,719,692 B2	4/2004	Kleffner et al.	7,014,638 B2	3/2006	Michelson
6,719,776 B2	4/2004	Baxter	7,033,357 B2	4/2006	Baxter et al.
6,723,091 B2	4/2004	Goble et al.	7,037,306 B2	5/2006	Podany
D490,059 S	5/2004	Conway et al.	7,041,083 B2	5/2006	Chu et al.
6,731,047 B2	5/2004	Kauf et al.	7,041,088 B2	5/2006	Nawrocki et al.
6,733,506 B1	5/2004	McDevitt et al.	7,041,102 B2	5/2006	Truckai et al.
6,736,813 B2	5/2004	Yamauchi et al.	7,044,949 B2	5/2006	Orszulak et al.
6,739,872 B1	5/2004	Turri	7,066,893 B2	6/2006	Hibner et al.
6,740,079 B1	5/2004	Eggers et al.	7,066,895 B2	6/2006	Podany
D491,666 S	6/2004	Kimmell et al.	7,070,597 B2	7/2006	Truckai et al.
6,743,245 B2	6/2004	Lobdell	7,074,218 B2	7/2006	Washington et al.
6,746,284 B1	6/2004	Spink, Jr.	7,074,219 B2	7/2006	Levine et al.
6,746,443 B1	6/2004	Morley et al.	7,077,039 B2	7/2006	Gass et al.
6,752,815 B2	6/2004	Beaupre	7,077,845 B2	7/2006	Hacker et al.
6,755,825 B2	6/2004	Shoenman et al.	7,077,853 B2	7/2006	Kramer et al.
6,761,698 B2	7/2004	Shibata et al.	7,083,618 B2	8/2006	Couture
6,762,535 B2	7/2004	Take et al.	7,083,619 B2	8/2006	Truckai et al.
6,770,072 B1	8/2004	Truckai et al.	7,087,054 B2	8/2006	Truckai et al.
6,773,409 B2	8/2004	Truckai et al.	7,090,672 B2	8/2006	Underwood et al.
6,773,443 B2	8/2004	Truwit et al.	7,101,371 B2	9/2006	Dycus et al.
6,773,444 B2	8/2004	Messerly	7,101,378 B2	9/2006	Salameh et al.
6,778,023 B2	8/2004	Christensen	7,104,834 B2	9/2006	Robinson et al.
6,783,524 B2	8/2004	Anderson et al.	7,108,695 B2	9/2006	Witt et al.
6,786,382 B1	9/2004	Hoffman	7,111,769 B2	9/2006	Wales et al.
6,786,383 B2	9/2004	Stegelmann	7,112,201 B2	9/2006	Truckai et al.
6,790,173 B2	9/2004	Saadat et al.	D531,311 S	10/2006	Guerra et al.
6,790,216 B1	9/2004	Ishikawa	7,117,034 B2	10/2006	Kronberg
6,796,981 B2	9/2004	Wham et al.	7,118,564 B2	10/2006	Ritchie et al.
D496,997 S	10/2004	Dycus et al.	7,124,932 B2	10/2006	Isacson et al.
6,802,843 B2	10/2004	Truckai et al.	7,125,409 B2	10/2006	Truckai et al.
6,808,525 B2	10/2004	Latterell et al.	7,128,720 B2	10/2006	Podany
			7,131,860 B2	11/2006	Sartor et al.
			7,135,018 B2	11/2006	Ryan et al.
			7,135,030 B2	11/2006	Schwemberger et al.
			7,137,980 B2	11/2006	Buyse et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,144,403	B2	12/2006	Booth	7,464,846	B2	12/2008	Shelton, IV et al.
7,153,315	B2	12/2006	Miller	7,472,815	B2	1/2009	Shelton, IV et al.
D536,093	S	1/2007	Nakajima et al.	7,473,263	B2	1/2009	Johnston et al.
7,156,189	B1	1/2007	Bar-Cohen et al.	7,479,148	B2	1/2009	Beaupre
7,156,853	B2	1/2007	Muratsu	7,479,160	B2	1/2009	Branch et al.
7,157,058	B2	1/2007	Marhasin et al.	7,481,775	B2	1/2009	Weikel, Jr. et al.
7,159,750	B2	1/2007	Racenet et al.	7,488,285	B2	2/2009	Honda et al.
7,160,296	B2	1/2007	Pearson et al.	7,494,468	B2	2/2009	Rabiner et al.
7,160,299	B2	1/2007	Baily	7,502,234	B2	3/2009	Goliszek et al.
7,163,548	B2	1/2007	Stulen et al.	7,503,893	B2	3/2009	Kucklick
7,169,144	B2	1/2007	Hoey et al.	7,503,895	B2	3/2009	Rabiner et al.
7,169,146	B2	1/2007	Truckai et al.	7,506,790	B2	3/2009	Shelton, IV
7,179,254	B2	2/2007	Pendekanti et al.	7,506,791	B2	3/2009	Omaits et al.
7,179,271	B2	2/2007	Friedman et al.	7,524,320	B2	4/2009	Tierney et al.
7,186,253	B2	3/2007	Truckai et al.	7,530,986	B2	5/2009	Beaupre et al.
7,189,233	B2	3/2007	Truckai et al.	7,534,243	B1	5/2009	Chin et al.
D541,418	S	4/2007	Schechter et al.	D594,983	S	6/2009	Price et al.
7,198,635	B2	4/2007	Danek et al.	7,540,871	B2	6/2009	Gonnering
7,204,820	B2	4/2007	Akahoshi	7,544,200	B2	6/2009	Houser
7,207,997	B2	4/2007	Shipp et al.	7,549,564	B2	6/2009	Boudreaux
7,210,881	B2	5/2007	Greenberg	7,559,450	B2	7/2009	Wales et al.
7,211,079	B2	5/2007	Treat	7,567,012	B2	7/2009	Namikawa
7,217,128	B2	5/2007	Atkin et al.	7,568,603	B2	8/2009	Shelton, IV et al.
7,217,269	B2	5/2007	El-Galley et al.	7,569,057	B2	8/2009	Liu et al.
7,220,951	B2	5/2007	Truckai et al.	7,572,266	B2	8/2009	Young et al.
7,223,229	B2	5/2007	Inman et al.	7,572,268	B2	8/2009	Babaev
7,229,455	B2	6/2007	Sakurai et al.	7,578,820	B2	8/2009	Moore et al.
7,235,071	B2	6/2007	Gonnering	7,582,084	B2	9/2009	Swanson et al.
7,244,262	B2	7/2007	Wiener et al.	7,582,095	B2	9/2009	Shipp et al.
7,258,688	B1	8/2007	Shah et al.	7,585,181	B2	9/2009	Olsen
7,269,873	B2	9/2007	Brewer et al.	7,588,176	B2	9/2009	Timm et al.
7,273,483	B2	9/2007	Wiener et al.	7,601,119	B2	10/2009	Shahinian
D552,241	S	10/2007	Bromley et al.	7,607,557	B2	10/2009	Shelton, IV et al.
7,282,048	B2	10/2007	Goble et al.	7,621,930	B2	11/2009	Houser
7,285,895	B2	10/2007	Beaupre	7,641,653	B2	1/2010	Dalla Betta et al.
7,300,431	B2	11/2007	Dubrovsky	7,645,278	B2	1/2010	Ichihashi et al.
7,300,435	B2	11/2007	Wham et al.	7,654,431	B2	2/2010	Hueil et al.
7,300,446	B2	11/2007	Beaupre	7,659,833	B2	2/2010	Warner et al.
7,303,531	B2	12/2007	Lee et al.	7,665,647	B2	2/2010	Shelton, IV et al.
7,303,557	B2	12/2007	Wham et al.	7,670,334	B2	3/2010	Hueil et al.
7,306,597	B2	12/2007	Manzo	7,670,338	B2	3/2010	Albrecht et al.
7,309,849	B2	12/2007	Truckai et al.	7,674,263	B2	3/2010	Ryan
7,311,706	B2	12/2007	Schoenman et al.	7,678,069	B1	3/2010	Baker et al.
7,311,709	B2	12/2007	Truckai et al.	7,678,125	B2	3/2010	Shipp
7,317,955	B2	1/2008	McGreevy	7,682,366	B2	3/2010	Sakurai et al.
7,318,831	B2	1/2008	Alvarez et al.	7,686,770	B2	3/2010	Cohen
7,326,236	B2	2/2008	Andreas et al.	7,686,826	B2	3/2010	Lee et al.
7,331,410	B2	2/2008	Yong et al.	7,688,028	B2	3/2010	Phillips et al.
7,335,165	B2	2/2008	Truwit et al.	7,691,098	B2	4/2010	Wallace et al.
7,335,997	B2	2/2008	Wiener	7,699,846	B2	4/2010	Ryan
7,337,010	B2	2/2008	Howard et al.	7,713,202	B2	5/2010	Boukhny et al.
7,353,068	B2	4/2008	Tanaka et al.	7,714,481	B2	5/2010	Sakai
7,354,440	B2	4/2008	Truckai et al.	7,717,312	B2	5/2010	Beetel
7,361,172	B2	4/2008	Cimino	7,717,915	B2	5/2010	Miyazawa
7,364,577	B2	4/2008	Wham et al.	7,721,935	B2	5/2010	Racenet et al.
RE40,388	E	6/2008	Gines	D618,797	S	6/2010	Price et al.
7,380,695	B2	6/2008	Doll et al.	7,726,537	B2	6/2010	Olson et al.
7,380,696	B2	6/2008	Shelton, IV et al.	7,727,177	B2	6/2010	Bayat
7,381,209	B2	6/2008	Truckai et al.	7,738,969	B2	6/2010	Bleich
7,390,317	B2	6/2008	Taylor et al.	7,740,594	B2	6/2010	Hibner
7,404,508	B2	7/2008	Smith et al.	7,751,115	B2	7/2010	Song
7,408,288	B2	8/2008	Hara	D621,503	S	8/2010	Otten et al.
7,416,101	B2	8/2008	Shelton, IV et al.	7,766,210	B2	8/2010	Shelton, IV et al.
7,416,437	B2	8/2008	Sartor et al.	7,766,693	B2	8/2010	Sartor et al.
D576,725	S	9/2008	Shumer et al.	7,770,774	B2	8/2010	Mastri et al.
7,419,490	B2	9/2008	Falkenstein et al.	7,770,775	B2	8/2010	Shelton, IV et al.
7,422,139	B2	9/2008	Shelton, IV et al.	7,771,425	B2	8/2010	Dycus et al.
7,422,463	B2	9/2008	Kuo	7,771,444	B2	8/2010	Patel et al.
D578,643	S	10/2008	Shumer et al.	7,775,972	B2	8/2010	Brock et al.
D578,644	S	10/2008	Shumer et al.	7,776,036	B2	8/2010	Schechter et al.
D578,645	S	10/2008	Shumer et al.	7,778,733	B2	8/2010	Nowlin et al.
7,431,704	B2	10/2008	Babaev	7,780,054	B2	8/2010	Wales
7,441,684	B2	10/2008	Shelton, IV et al.	7,780,593	B2	8/2010	Ueno et al.
7,455,208	B2	11/2008	Wales et al.	7,780,651	B2	8/2010	Madhani et al.
7,462,181	B2	12/2008	Kraft et al.	7,780,659	B2	8/2010	Okada et al.
				7,784,662	B2	8/2010	Wales et al.
				7,796,969	B2	9/2010	Kelly et al.
				7,798,386	B2	9/2010	Schall et al.
				7,799,020	B2	9/2010	Shores et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,799,045 B2	9/2010	Masuda	8,246,575 B2	8/2012	Viola
7,803,152 B2	9/2010	Honda et al.	8,246,615 B2	8/2012	Behnke
7,806,891 B2	10/2010	Nowlin et al.	8,252,012 B2	8/2012	Stulen
7,810,693 B2	10/2010	Broehl et al.	8,253,303 B2	8/2012	Giordano et al.
7,811,283 B2	10/2010	Moses et al.	8,257,377 B2	9/2012	Wiener et al.
7,819,819 B2	10/2010	Quick et al.	8,257,387 B2	9/2012	Cunningham
7,821,143 B2	10/2010	Wiener	8,273,087 B2	9/2012	Kimura et al.
D627,066 S	11/2010	Romero	D669,992 S	10/2012	Schafer et al.
7,824,401 B2	11/2010	Manzo et al.	D669,993 S	10/2012	Merchant et al.
7,832,611 B2	11/2010	Boyden et al.	8,286,846 B2	10/2012	Smith et al.
7,834,484 B2	11/2010	Sartor	8,287,485 B2	10/2012	Kimura et al.
7,837,699 B2	11/2010	Yamada et al.	8,287,528 B2	10/2012	Wham et al.
7,845,537 B2	12/2010	Shelton, IV et al.	8,287,532 B2	10/2012	Carroll et al.
7,846,155 B2	12/2010	Houser et al.	8,292,888 B2	10/2012	Whitman
7,846,161 B2	12/2010	Dumbauld et al.	8,298,223 B2	10/2012	Wham et al.
7,854,735 B2	12/2010	Houser et al.	8,298,225 B2	10/2012	Gilbert
D631,155 S	1/2011	Peine et al.	8,303,576 B2	11/2012	Brock
7,861,906 B2	1/2011	Doll et al.	8,303,580 B2	11/2012	Wham et al.
7,862,560 B2	1/2011	Marion	8,303,583 B2	11/2012	Hosier et al.
7,876,030 B2	1/2011	Taki et al.	8,319,400 B2	11/2012	Houser et al.
D631,965 S	2/2011	Price et al.	8,323,302 B2	12/2012	Robertson et al.
7,878,991 B2	2/2011	Babaev	8,328,833 B2	12/2012	Cuny
7,879,033 B2	2/2011	Sartor et al.	8,333,778 B2	12/2012	Smith et al.
7,892,606 B2	2/2011	Thies et al.	8,333,779 B2	12/2012	Smith et al.
7,901,400 B2	3/2011	Wham et al.	8,334,468 B2	12/2012	Palmer et al.
7,901,423 B2	3/2011	Stulen et al.	8,334,635 B2	12/2012	Voegele et al.
7,905,881 B2	3/2011	Masuda et al.	8,337,407 B2	12/2012	Quistgaard et al.
7,909,824 B2	3/2011	Masuda et al.	8,338,726 B2	12/2012	Palmer et al.
7,922,061 B2	4/2011	Shelton, IV et al.	8,344,596 B2	1/2013	Nield et al.
7,922,651 B2	4/2011	Yamada et al.	8,348,967 B2	1/2013	Stulen
D637,288 S	5/2011	Houghton	8,357,103 B2	1/2013	Mark et al.
D638,540 S	5/2011	Ijiri et al.	8,366,727 B2	2/2013	Witt et al.
7,936,203 B2	5/2011	Zimlich	8,372,099 B2	2/2013	Deville et al.
7,951,095 B2	5/2011	Makin et al.	8,372,101 B2	2/2013	Smith et al.
7,951,165 B2	5/2011	Golden et al.	8,372,102 B2	2/2013	Stulen et al.
7,959,050 B2	6/2011	Smith et al.	8,374,670 B2	2/2013	Selkee
7,959,626 B2	6/2011	Hong et al.	8,377,059 B2	2/2013	Deville et al.
7,972,329 B2	7/2011	Refior et al.	8,377,085 B2	2/2013	Smith et al.
7,976,544 B2	7/2011	McClurken et al.	8,382,748 B2	2/2013	Geisel
7,981,050 B2	7/2011	Ritchart et al.	8,382,775 B1	2/2013	Bender et al.
7,998,157 B2	8/2011	Culp et al.	8,382,782 B2	2/2013	Robertson et al.
8,038,693 B2	10/2011	Allen	8,403,948 B2	3/2013	Deville et al.
8,057,498 B2	11/2011	Robertson	8,403,949 B2	3/2013	Palmer et al.
8,058,771 B2	11/2011	Giordano et al.	8,403,950 B2	3/2013	Palmer et al.
8,061,014 B2	11/2011	Smith et al.	8,418,073 B2	4/2013	Mohr et al.
8,070,711 B2	12/2011	Bassinger et al.	8,418,349 B2	4/2013	Smith et al.
8,070,762 B2	12/2011	Escudero et al.	8,419,757 B2	4/2013	Smith et al.
8,075,558 B2	12/2011	Truckai et al.	8,419,758 B2	4/2013	Smith et al.
8,089,197 B2	1/2012	Rinner et al.	8,419,759 B2	4/2013	Dietz
8,097,012 B2	1/2012	Kagarise	8,425,545 B2	4/2013	Smith et al.
8,105,323 B2	1/2012	Buyse et al.	8,430,898 B2	4/2013	Wiener et al.
8,142,461 B2	3/2012	Houser et al.	8,435,257 B2	5/2013	Smith et al.
8,152,801 B2	4/2012	Goldberg et al.	8,439,912 B2	5/2013	Cunningham et al.
8,152,825 B2	4/2012	Madan et al.	8,439,939 B2	5/2013	Deville et al.
8,157,145 B2	4/2012	Shelton, IV et al.	8,444,637 B2	5/2013	Podmore et al.
8,161,977 B2	4/2012	Shelton, IV et al.	8,444,662 B2	5/2013	Palmer et al.
8,162,966 B2	4/2012	Connor et al.	8,444,664 B2	5/2013	Balaney et al.
8,172,846 B2	5/2012	Brunnett et al.	8,460,288 B2	6/2013	Tamai et al.
8,172,870 B2	5/2012	Shipp	8,461,744 B2	6/2013	Wiener et al.
8,177,800 B2	5/2012	Spitz et al.	8,469,981 B2	6/2013	Robertson et al.
8,182,502 B2	5/2012	Stulen et al.	8,479,969 B2	7/2013	Shelton, IV
8,186,877 B2	5/2012	Klimovitch et al.	8,480,703 B2	7/2013	Nicholas et al.
D661,801 S	6/2012	Price et al.	8,485,413 B2	7/2013	Scheib et al.
D661,802 S	6/2012	Price et al.	8,486,057 B2	7/2013	Behnke, II
D661,803 S	6/2012	Price et al.	8,486,096 B2	7/2013	Robertson et al.
D661,804 S	6/2012	Price et al.	8,491,578 B2	7/2013	Manwaring et al.
8,197,472 B2	6/2012	Lau et al.	D687,549 S	8/2013	Johnson et al.
8,197,502 B2	6/2012	Smith et al.	8,506,555 B2	8/2013	Ruiz Morales
8,207,651 B2	6/2012	Gilbert	8,509,318 B2	8/2013	Tailliet
8,210,411 B2	7/2012	Yates et al.	8,512,359 B2	8/2013	Whitman et al.
8,226,675 B2	7/2012	Houser et al.	8,512,365 B2	8/2013	Wiener et al.
8,235,917 B2	8/2012	Joseph et al.	8,523,889 B2	9/2013	Stulen et al.
8,236,019 B2	8/2012	Houser	8,531,064 B2	9/2013	Robertson et al.
8,236,020 B2	8/2012	Smith et al.	8,535,340 B2	9/2013	Allen
8,241,271 B2	8/2012	Millman et al.	8,535,341 B2	9/2013	Allen
			8,546,996 B2	10/2013	Messierly et al.
			8,546,999 B2	10/2013	Houser et al.
			8,551,086 B2	10/2013	Kimura et al.
			8,568,400 B2	10/2013	Gilbert

(56)

References Cited

U.S. PATENT DOCUMENTS

8,573,461 B2	11/2013	Shelton, IV et al.	9,283,045 B2	3/2016	Rhee et al.
8,573,465 B2	11/2013	Shelton, IV	9,307,986 B2	4/2016	Hall et al.
8,579,928 B2	11/2013	Robertson et al.	9,326,788 B2	5/2016	Batross et al.
8,591,459 B2	11/2013	Clymer et al.	9,339,289 B2	5/2016	Robertson
8,591,506 B2	11/2013	Wham et al.	9,351,754 B2	5/2016	Vakharia et al.
8,591,536 B2	11/2013	Robertson	9,393,037 B2	7/2016	Olson et al.
D695,407 S	12/2013	Price et al.	9,408,622 B2	8/2016	Stulen et al.
D696,631 S	12/2013	Price et al.	9,414,853 B2	8/2016	Stulen et al.
8,602,031 B2	12/2013	Reis et al.	9,421,060 B2	8/2016	Monson et al.
8,602,288 B2	12/2013	Shelton, IV et al.	9,427,249 B2	8/2016	Robertson et al.
8,608,745 B2	12/2013	Guzman et al.	9,439,668 B2	9/2016	Timm et al.
8,616,431 B2	12/2013	Timm et al.	9,439,669 B2	9/2016	Wiener et al.
8,650,728 B2	2/2014	Wan et al.	9,439,671 B2	9/2016	Akagane et al.
8,652,155 B2	2/2014	Houser et al.	9,445,832 B2	9/2016	Wiener et al.
8,659,208 B1	2/2014	Rose et al.	2001/0025173 A1	9/2001	Ritchie et al.
8,663,220 B2	3/2014	Wiener et al.	2001/0025183 A1	9/2001	Shahidi et al.
8,690,582 B2	4/2014	Rohrbach et al.	2001/0025184 A1	9/2001	Messerly
8,696,366 B2	4/2014	Chen et al.	2001/0031950 A1	10/2001	Ryan
8,704,425 B2	4/2014	Giordano et al.	2001/0039419 A1	11/2001	Francischelli et al.
8,709,031 B2	4/2014	Stulen	2002/0002377 A1	1/2002	Cimino
8,747,351 B2	6/2014	Schultz	2002/0019649 A1	2/2002	Sikora et al.
8,749,116 B2	6/2014	Messerly et al.	2002/0022836 A1	2/2002	Goble et al.
8,752,749 B2	6/2014	Moore et al.	2002/0029055 A1	3/2002	Bonutti
8,753,338 B2	6/2014	Widenhouse et al.	2002/0049551 A1	4/2002	Friedman et al.
8,754,570 B2	6/2014	Voegele et al.	2002/0052617 A1	5/2002	Anis et al.
8,758,352 B2	6/2014	Cooper et al.	2002/0077550 A1	6/2002	Rabiner et al.
8,764,735 B2	7/2014	Coe et al.	2002/0156466 A1	10/2002	Sakurai et al.
8,771,270 B2	7/2014	Burbank	2002/0156493 A1	10/2002	Houser et al.
8,773,001 B2	7/2014	Wiener et al.	2003/0014087 A1	1/2003	Fang et al.
8,779,648 B2	7/2014	Giordano et al.	2003/0036705 A1	2/2003	Hare et al.
8,784,418 B2	7/2014	Romero	2003/0050572 A1	3/2003	Brautigam et al.
8,808,319 B2	8/2014	Houser et al.	2003/0055443 A1	3/2003	Spotnitz
8,827,992 B2	9/2014	Koss et al.	2003/0114851 A1	6/2003	Truckai et al.
8,845,537 B2	9/2014	Tanaka et al.	2003/0144680 A1	7/2003	Kellogg et al.
8,882,791 B2	11/2014	Stulen	2003/0199794 A1	10/2003	Sakurai et al.
8,888,776 B2	11/2014	Dietz et al.	2003/0204199 A1	10/2003	Novak et al.
8,888,809 B2	11/2014	Davison et al.	2003/0212332 A1	11/2003	Fenton et al.
8,899,462 B2	12/2014	Kostrzewski et al.	2003/0212363 A1	11/2003	Shipp
8,900,259 B2	12/2014	Houser et al.	2003/0212392 A1	11/2003	Fenton et al.
8,911,460 B2	12/2014	Neurohr et al.	2003/0212422 A1	11/2003	Fenton et al.
8,951,248 B2	2/2015	Messerly et al.	2003/0229344 A1	12/2003	Dycus et al.
8,951,272 B2	2/2015	Robertson et al.	2004/0030254 A1	2/2004	Babaev
8,956,349 B2	2/2015	Aldridge et al.	2004/0030330 A1	2/2004	Brassell et al.
8,961,547 B2	2/2015	Dietz et al.	2004/0047485 A1	3/2004	Sherrit et al.
8,968,283 B2	3/2015	Kharin	2004/0054364 A1	3/2004	Aranyi et al.
8,968,355 B2	3/2015	Malkowski et al.	2004/0064151 A1	4/2004	Mollenauer
8,974,477 B2	3/2015	Yamada	2004/0092921 A1	5/2004	Kadziauskas et al.
8,979,890 B2	3/2015	Boudreaux	2004/0092992 A1	5/2004	Adams et al.
8,986,287 B2	3/2015	Park et al.	2004/0097911 A1	5/2004	Murakami et al.
8,986,302 B2	3/2015	Aldridge et al.	2004/0097912 A1	5/2004	Gonnering
8,989,903 B2	3/2015	Weir et al.	2004/0097919 A1	5/2004	Wellman et al.
9,017,326 B2	4/2015	DiNardo et al.	2004/0097996 A1	5/2004	Rabiner et al.
9,039,695 B2	5/2015	Giordano et al.	2004/0116952 A1	6/2004	Sakurai et al.
9,043,018 B2	5/2015	Mohr	2004/0132383 A1	7/2004	Langford et al.
9,044,261 B2	6/2015	Houser	2004/0147934 A1	7/2004	Kiester
9,050,093 B2	6/2015	Aldridge et al.	2004/0167508 A1	8/2004	Wham et al.
9,050,124 B2	6/2015	Houser	2004/0176686 A1	9/2004	Hare et al.
9,060,775 B2	6/2015	Wiener et al.	2004/0176751 A1	9/2004	Weitzner et al.
9,060,776 B2	6/2015	Yates et al.	2004/0199193 A1	10/2004	Hayashi et al.
9,066,747 B2	6/2015	Robertson	2004/0204728 A1	10/2004	Haefner
9,072,539 B2	7/2015	Messerly et al.	2004/0215132 A1	10/2004	Yoon
9,089,360 B2	7/2015	Messerly et al.	2004/0243147 A1	12/2004	Lipow
9,095,367 B2	8/2015	Olson et al.	2004/0260300 A1	12/2004	Gorensek et al.
9,107,689 B2	8/2015	Robertson et al.	2005/0020967 A1	1/2005	Ono
9,113,940 B2	8/2015	Twomey	2005/0021018 A1	1/2005	Anderson et al.
9,168,054 B2	10/2015	Turner et al.	2005/0021065 A1	1/2005	Yamada et al.
9,198,714 B2	12/2015	Worrell et al.	2005/0033337 A1	2/2005	Muir et al.
9,220,527 B2	12/2015	Houser et al.	2005/0049546 A1	3/2005	Messerly et al.
9,226,766 B2	1/2016	Aldridge et al.	2005/0070800 A1	3/2005	Takahashi
9,226,767 B2	1/2016	Stulen et al.	2005/0096683 A1	5/2005	Ellins et al.
9,232,979 B2	1/2016	Parihar et al.	2005/0099824 A1	5/2005	Dowling et al.
9,237,921 B2	1/2016	Messerly et al.	2005/0103819 A1	5/2005	Racenet et al.
9,241,728 B2	1/2016	Price et al.	2005/0143769 A1	6/2005	White et al.
9,241,731 B2	1/2016	Boudreaux et al.	2005/0149108 A1	7/2005	Cox
9,259,234 B2	2/2016	Robertson et al.	2005/0165345 A1	7/2005	Laufer et al.
			2005/0177184 A1	8/2005	Easley
			2005/0182339 A1	8/2005	Lee et al.
			2005/0188743 A1	9/2005	Land
			2005/0192610 A1	9/2005	Houser et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2005/0209620 A1	9/2005	Du et al.	2008/0147092 A1	6/2008	Rogge et al.
2005/0222598 A1	10/2005	Ho et al.	2008/0171938 A1	7/2008	Masuda et al.
2005/0234484 A1	10/2005	Houser et al.	2008/0172051 A1	7/2008	Masuda et al.
2005/0249667 A1	11/2005	Tuszynski et al.	2008/0177268 A1	7/2008	Daum et al.
2005/0256405 A1	11/2005	Makin et al.	2008/0188878 A1	8/2008	Young
2005/0261581 A1	11/2005	Hughes et al.	2008/0200940 A1	8/2008	Eichmann et al.
2005/0261588 A1	11/2005	Makin et al.	2008/0208108 A1	8/2008	Kimura
2005/0273090 A1	12/2005	Nieman et al.	2008/0208231 A1	8/2008	Ota et al.
2005/0288659 A1	12/2005	Kimura et al.	2008/0214967 A1	9/2008	Aranyi et al.
2006/0030797 A1	2/2006	Zhou et al.	2008/0234709 A1	9/2008	Houser
2006/0058825 A1	3/2006	Ogura et al.	2008/0243106 A1	10/2008	Coe et al.
2006/0063130 A1	3/2006	Hayman et al.	2008/0243162 A1	10/2008	Shibata et al.
2006/0066181 A1	3/2006	Bromfield et al.	2008/0245371 A1	10/2008	Gruber
2006/0074442 A1	4/2006	Noriega et al.	2008/0249553 A1	10/2008	Gruber et al.
2006/0079874 A1	4/2006	Faller et al.	2008/0255423 A1	10/2008	Kondo et al.
2006/0079879 A1	4/2006	Faller et al.	2008/0262490 A1	10/2008	Williams
2006/0084963 A1	4/2006	Messerly	2008/0281200 A1	11/2008	Voic et al.
2006/0095046 A1	5/2006	Trieu et al.	2008/0281315 A1	11/2008	Gines
2006/0190034 A1	8/2006	Nishizawa et al.	2008/0281322 A1	11/2008	Sherman et al.
2006/0206100 A1	9/2006	Eskridge et al.	2008/0287948 A1	11/2008	Newton et al.
2006/0206115 A1	9/2006	Schomer et al.	2009/0023985 A1	1/2009	Ewers
2006/0211943 A1	9/2006	Beaupre	2009/0024141 A1	1/2009	Stahler et al.
2006/0217729 A1	9/2006	Eskridge et al.	2009/0048537 A1	2/2009	Lydon et al.
2006/0224160 A1	10/2006	Trieu et al.	2009/0054886 A1	2/2009	Yachi et al.
2006/0235306 A1	10/2006	Cotter et al.	2009/0054894 A1	2/2009	Yachi
2006/0247558 A1	11/2006	Yamada	2009/0076506 A1	3/2009	Baker
2006/0253050 A1	11/2006	Yoshimine et al.	2009/0082716 A1	3/2009	Akahoshi
2006/0264809 A1	11/2006	Hansmann et al.	2009/0088738 A1	4/2009	Guerra et al.
2006/0271030 A1	11/2006	Francis et al.	2009/0088785 A1	4/2009	Masuda
2007/0016235 A1	1/2007	Tanaka et al.	2009/0105750 A1	4/2009	Price et al.
2007/0016236 A1	1/2007	Beaupre	2009/0112229 A1	4/2009	Omori et al.
2007/0055228 A1	3/2007	Berg et al.	2009/0118751 A1	5/2009	Wiener et al.
2007/0056596 A1	3/2007	Fanney et al.	2009/0118802 A1	5/2009	Mioduski et al.
2007/0060915 A1	3/2007	Kucklick	2009/0138006 A1	5/2009	Bales et al.
2007/0060935 A1	3/2007	Schwardt et al.	2009/0143799 A1	6/2009	Smith et al.
2007/0063618 A1	3/2007	Bromfield	2009/0143800 A1	6/2009	Deville et al.
2007/0074584 A1	4/2007	Talarico et al.	2009/0143806 A1	6/2009	Witt et al.
2007/0078458 A1	4/2007	Dumbauld et al.	2009/0149801 A1	6/2009	Crandall et al.
2007/0106317 A1	5/2007	Shelton, IV et al.	2009/0163807 A1	6/2009	Sliwa
2007/0129716 A1	6/2007	Daw et al.	2009/0207923 A1	8/2009	Dress
2007/0130771 A1	6/2007	Ehlert et al.	2009/0216157 A1	8/2009	Yamada
2007/0131034 A1	6/2007	Ehlert et al.	2009/0223033 A1	9/2009	Houser
2007/0149881 A1	6/2007	Rabin	2009/0254077 A1	10/2009	Craig
2007/0156163 A1	7/2007	Davison et al.	2009/0254080 A1	10/2009	Honda
2007/0162050 A1	7/2007	Sartor	2009/0264909 A1	10/2009	Beaupre
2007/0166663 A1	7/2007	Telles et al.	2009/0270771 A1	10/2009	Takahashi
2007/0173803 A1	7/2007	Wham et al.	2009/0270812 A1	10/2009	Litscher et al.
2007/0173813 A1	7/2007	Odom	2009/0270853 A1	10/2009	Yachi et al.
2007/0173872 A1	7/2007	Neuenfeldt	2009/0270891 A1	10/2009	Beupre
2007/0175949 A1	8/2007	Shelton, IV et al.	2009/0270899 A1	10/2009	Carusillo et al.
2007/0185380 A1	8/2007	Kucklick	2009/0275940 A1	11/2009	Malackowski et al.
2007/0191712 A1	8/2007	Messerly et al.	2009/0299141 A1	12/2009	Downey et al.
2007/0219481 A1	9/2007	Babaev	2009/0318945 A1	12/2009	Yoshimine et al.
2007/0239028 A1	10/2007	Houser et al.	2009/0327715 A1	12/2009	Smith et al.
2007/0239101 A1	10/2007	Kellogg	2010/0004508 A1	1/2010	Naito et al.
2007/0249941 A1	10/2007	Salehi et al.	2010/0016785 A1	1/2010	Takuma
2007/0260234 A1	11/2007	McCullagh et al.	2010/0016852 A1	1/2010	Manzo et al.
2007/0265560 A1	11/2007	Soltani et al.	2010/0022825 A1	1/2010	Yoshie
2007/0275348 A1	11/2007	Lemon	2010/0030233 A1	2/2010	Whitman et al.
2007/0282335 A1	12/2007	Young et al.	2010/0030248 A1	2/2010	Palmer et al.
2007/0287933 A1	12/2007	Phan et al.	2010/0036370 A1	2/2010	Mirel et al.
2007/0288055 A1	12/2007	Lee	2010/0042077 A1	2/2010	Okada
2008/0009848 A1	1/2008	Paraschiv et al.	2010/0049180 A1	2/2010	Wells et al.
2008/0013809 A1	1/2008	Zhu et al.	2010/0057118 A1	3/2010	Dietz et al.
2008/0051812 A1	2/2008	Schmitz et al.	2010/0063525 A1	3/2010	Beaupre et al.
2008/0058585 A1	3/2008	Novak et al.	2010/0063528 A1	3/2010	Beaupre
2008/0058775 A1	3/2008	Darian et al.	2010/0069940 A1	3/2010	Miller et al.
2008/0058845 A1	3/2008	Shimizu et al.	2010/0106173 A1	4/2010	Yoshimine
2008/0077145 A1	3/2008	Boyden et al.	2010/0158307 A1	6/2010	Kubota et al.
2008/0082039 A1	4/2008	Babaev	2010/0168741 A1	7/2010	Sanai et al.
2008/0082098 A1	4/2008	Tanaka et al.	2010/0187283 A1	7/2010	Crainich et al.
2008/0097501 A1	4/2008	Blier	2010/0222714 A1	9/2010	Muir et al.
2008/0114364 A1	5/2008	Goldin et al.	2010/0228264 A1	9/2010	Robinson et al.
2008/0125768 A1	5/2008	Tahara et al.	2010/0234906 A1	9/2010	Koh
2008/0140158 A1	6/2008	Hamel et al.	2010/0262134 A1	10/2010	Jensen et al.
			2010/0274160 A1	10/2010	Yachi et al.
			2010/0280407 A1	11/2010	Polster
			2010/0292691 A1	11/2010	Brogna
			2010/0298743 A1	11/2010	Nield et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2010/0298851 A1	11/2010	Nield	2013/0123822 A1	5/2013	Wellman et al.
2010/0331742 A1	12/2010	Masuda	2013/0131660 A1	5/2013	Monson et al.
2011/0004233 A1	1/2011	Muir et al.	2013/0165929 A1	6/2013	Muir et al.
2011/0009850 A1	1/2011	Main et al.	2013/0217967 A1	8/2013	Mohr et al.
2011/0077648 A1	3/2011	Lee et al.	2013/0253498 A1	9/2013	Germain et al.
2011/0087218 A1	4/2011	Boudreaux et al.	2013/0274734 A1	10/2013	Maass et al.
2011/0112526 A1	5/2011	Fritz et al.	2013/0282038 A1	10/2013	Dannaher et al.
2011/0125151 A1	5/2011	Strauss et al.	2013/0296908 A1	11/2013	Schulte et al.
2011/0125174 A1	5/2011	Babaev	2013/0338661 A1	12/2013	Behnke, II
2011/0144806 A1	6/2011	Sandhu et al.	2013/0345689 A1	12/2013	Ruddenklau et al.
2011/0196404 A1 *	8/2011	Dietz A61B 17/22004 606/169	2014/0005640 A1	1/2014	Shelton, IV et al.
2011/0224689 A1	9/2011	Larkin et al.	2014/0005653 A1	1/2014	Shelton, IV et al.
2011/0238065 A1	9/2011	Hunt et al.	2014/0005656 A1	1/2014	Mucilli et al.
2011/0257650 A1	10/2011	Deville et al.	2014/0005661 A1	1/2014	Shelton, IV et al.
2011/0270126 A1	11/2011	Gunday et al.	2014/0005662 A1	1/2014	Shelton, IV et al.
2011/0290853 A1	12/2011	Shelton, IV et al.	2014/0005676 A1	1/2014	Shelton, IV et al.
2011/0290856 A1	12/2011	Shelton, IV et al.	2014/0005680 A1	1/2014	Shelton, IV et al.
2011/0295242 A1	12/2011	Spivey et al.	2014/0005681 A1	1/2014	Gee et al.
2012/0004655 A1	1/2012	Kim et al.	2014/0005702 A1	1/2014	Timm et al.
2012/0022525 A1	1/2012	Dietz et al.	2014/0005705 A1	1/2014	Weir et al.
2012/0022530 A1	1/2012	Woodruff et al.	2014/0005708 A1	1/2014	Shelton, IV et al.
2012/0022583 A1	1/2012	Sugalski et al.	2014/0005718 A1	1/2014	Shelton, IV et al.
2012/0059289 A1	3/2012	Nield et al.	2014/0012299 A1	1/2014	Stoddard et al.
2012/0065628 A1	3/2012	Naito	2014/0066962 A1	3/2014	Robertson et al.
2012/0071863 A1	3/2012	Lee et al.	2014/0087569 A1	3/2014	Lee
2012/0078139 A1	3/2012	Aldridge et al.	2014/0107538 A1	4/2014	Wiener et al.
2012/0078243 A1	3/2012	Worrell et al.	2014/0114327 A1	4/2014	Boudreaux et al.
2012/0078244 A1	3/2012	Worrell et al.	2014/0135804 A1	5/2014	Weisenburgh, II et al.
2012/0078247 A1	3/2012	Worrell et al.	2014/0155921 A1	6/2014	Price et al.
2012/0078278 A1	3/2012	Bales, Jr. et al.	2014/0180280 A1	6/2014	Sigmon, Jr.
2012/0080332 A1	4/2012	Shelton, IV et al.	2014/0243864 A1	8/2014	Voegele et al.
2012/0101495 A1	4/2012	Young et al.	2014/0276970 A1	9/2014	Messerly et al.
2012/0101501 A1	4/2012	Nishimura et al.	2015/0045819 A1	2/2015	Houser et al.
2012/0109159 A1	5/2012	Jordan et al.	2015/0066067 A1	3/2015	Stulen
2012/0116379 A1	5/2012	Yates et al.	2015/0073460 A1	3/2015	Stulen
2012/0116391 A1	5/2012	Houser et al.	2015/0112335 A1	4/2015	Boudreaux et al.
2012/0116394 A1	5/2012	Timm et al.	2015/0119914 A1	4/2015	Neurohr et al.
2012/0116395 A1	5/2012	Madan et al.	2015/0119915 A1	4/2015	Neurohr et al.
2012/0130256 A1	5/2012	Buyse et al.	2015/0119916 A1	4/2015	Dietz et al.
2012/0130365 A1	5/2012	McLawhorn	2015/0123348 A1	5/2015	Robertson et al.
2012/0136354 A1	5/2012	Rupp	2015/0157355 A1	6/2015	Price et al.
2012/0138660 A1	6/2012	Shelton, IV	2015/0157356 A1	6/2015	Gee
2012/0143211 A1	6/2012	Kishi	2015/0164533 A1	6/2015	Felder et al.
2012/0150170 A1	6/2012	Buyse et al.	2015/0164534 A1	6/2015	Felder et al.
2012/0165816 A1	6/2012	Kersten et al.	2015/0164535 A1	6/2015	Felder et al.
2012/0172873 A1	7/2012	Artale et al.	2015/0164536 A1	6/2015	Czarnecki et al.
2012/0172904 A1	7/2012	Muir et al.	2015/0164537 A1	6/2015	Cagle et al.
2012/0177005 A1	7/2012	Liang et al.	2015/0164538 A1	6/2015	Aldridge et al.
2012/0184946 A1	7/2012	Price et al.	2015/0182251 A1	7/2015	Messerly et al.
2012/0199630 A1	8/2012	Shelton, IV	2015/0182276 A1	7/2015	Wiener et al.
2012/0199632 A1	8/2012	Spivey et al.	2015/0182277 A1	7/2015	Wiener et al.
2012/0203143 A1	8/2012	Sanai et al.	2015/0196318 A1	7/2015	Messerly et al.
2012/0203247 A1	8/2012	Shelton, IV et al.	2015/0250495 A1	9/2015	Robertson et al.
2012/0209289 A1	8/2012	Duque et al.	2015/0257780 A1	9/2015	Houser
2012/0209303 A1	8/2012	Frankhouser et al.	2015/0257781 A1	9/2015	Houser et al.
2012/0210223 A1	8/2012	Eppolito	2015/0265308 A1	9/2015	Houser et al.
2012/0215220 A1	8/2012	Manzo et al.	2015/0327883 A1	11/2015	Messerly et al.
2012/0245582 A1	9/2012	Kimball et al.	2015/0328484 A1	11/2015	Messerly et al.
2012/0253370 A1	10/2012	Ross et al.	2015/0340586 A1	11/2015	Wiener et al.
2012/0269676 A1	10/2012	Houser et al.	2015/0351789 A1	12/2015	Robertson et al.
2012/0330307 A1	12/2012	Ladtkow et al.	2016/0030076 A1	2/2016	Faller et al.
2013/0012957 A1	1/2013	Shelton, IV et al.	2016/0089209 A1	3/2016	Parihar et al.
2013/0030433 A1	1/2013	Heard	2016/0089533 A1	3/2016	Turner et al.
2013/0035680 A1	2/2013	Ben-Haim et al.	2016/0095617 A1	4/2016	Price et al.
2013/0053840 A1	2/2013	Krapohl et al.	2016/0106509 A1	4/2016	Worrell et al.
2013/0072856 A1	3/2013	Frankhouser et al.	2016/0120563 A1	5/2016	Messerly et al.
2013/0072857 A1	3/2013	Frankhouser et al.	2016/0144204 A1	5/2016	Akagane
2013/0079762 A1	3/2013	Twomey et al.	2016/0192999 A1	7/2016	Stulen et al.
2013/0103023 A1	4/2013	Monson et al.	2016/0206342 A1	7/2016	Robertson et al.
2013/0103024 A1	4/2013	Monson et al.	2016/0262786 A1	9/2016	Madan et al.
2013/0110145 A1	5/2013	Weitzman	2016/0296249 A1	10/2016	Robertson
2013/0123776 A1	5/2013	Monson et al.	2016/0296250 A1	10/2016	Olson et al.
2013/0123777 A1	5/2013	Monson et al.	2016/0296251 A1	10/2016	Olson et al.
2013/0123782 A1	5/2013	Trees et al.	2016/0296252 A1	10/2016	Olson et al.
			2016/0317217 A1	11/2016	Batross et al.
			2016/0367281 A1	12/2016	Gee et al.
			2017/0000552 A1	1/2017	Asher et al.
			2017/0143371 A1	5/2017	Witt et al.
			2017/0143877 A1	5/2017	Witt et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2017/0196586 A1 7/2017 Witt et al.
 2017/0196587 A1 7/2017 Witt et al.
 2017/0202573 A1 7/2017 Witt et al.

FOREIGN PATENT DOCUMENTS

CN 1233944 A 11/1999
 CN 1253485 A 5/2000
 CN 2460047 Y 11/2001
 CN 1634601 A 7/2005
 CN 1640365 A 7/2005
 CN 1694649 A 11/2005
 CN 1775323 A 5/2006
 CN 1922563 A 2/2007
 CN 1951333 A 4/2007
 CN 101035482 A 9/2007
 CN 101040799 B 9/2007
 CN 101467917 A 1/2009
 CN 101396300 A 4/2009
 CN 101674782 A 3/2010
 CN 101883531 A 11/2010
 CN 202027624 U 11/2011
 CN 101313865 B 1/2013
 CN 102160045 A 8/2017
 DE 3904558 A1 8/1990
 DE 9210327 U1 11/1992
 DE 4323585 A1 1/1995
 DE 19608716 C1 4/1997
 DE 20021619 U1 3/2001
 DE 10042606 A1 8/2001
 EP 0136855 B1 9/1984
 EP 0171967 A2 2/1986
 EP 1839599 A1 10/1987
 EP 0336742 A2 4/1989
 EP 0342448 A1 11/1989
 EP 0424685 B1 5/1991
 EP 0443256 A1 8/1991
 EP 0456470 A1 11/1991
 EP 0238667 B1 2/1993
 EP 0598976 A2 1/1994
 EP 0677275 A2 3/1995
 EP 0482195 B1 1/1996
 EP 0695535 A1 2/1996
 EP 0741996 A2 11/1996
 EP 0612570 B1 6/1997
 EP 1108394 A2 6/2001
 EP 1138264 A1 10/2001
 EP 0908148 B1 1/2002
 EP 1229515 A2 8/2002
 EP 1285634 A1 2/2003
 EP 0908155 B1 6/2003
 EP 0705570 B1 4/2004
 EP 0765637 B1 7/2004
 EP 0870473 B1 9/2005
 EP 0624346 B1 11/2005
 EP 1594209 A1 11/2005
 EP 1199044 B1 12/2005
 EP 1609428 A1 12/2005
 EP 1199043 B1 3/2006
 EP 1433425 B1 6/2006
 EP 1256323 B1 9/2006
 EP 1698289 A2 9/2006
 EP 1704824 A1 9/2006
 EP 1749479 A1 2/2007
 EP 1815950 A1 8/2007
 EP 1844720 A1 10/2007
 EP 1862133 A1 12/2007
 EP 1875875 A1 1/2008
 EP 1199045 B1 6/2008
 EP 1964530 A1 9/2008
 EP 1972264 A1 9/2008
 EP 1974771 A1 10/2008
 EP 1435852 B1 12/2008
 EP 1498082 B1 12/2008
 EP 1707131 B1 12/2008

EP 1997438 A2 12/2008
 EP 1477104 B1 1/2009
 EP 2014218 A2 1/2009
 EP 2042112 A2 4/2009
 EP 1832259 B1 6/2009
 EP 2074959 A1 7/2009
 EP 2106758 A1 10/2009
 EP 2111813 A1 10/2009
 EP 2200145 A1 6/2010
 EP 1214913 B1 7/2010
 EP 2238938 A1 10/2010
 EP 2298154 A2 3/2011
 EP 1510178 B1 6/2011
 EP 1946708 B1 6/2011
 EP 2305144 A1 6/2011
 EP 2335630 A1 6/2011
 EP 1502551 B1 7/2011
 EP 2361562 A1 8/2011
 EP 2365608 A2 9/2011
 EP 2420197 A2 2/2012
 EP 2422721 A2 2/2012
 EP 1927321 B1 4/2012
 EP 2510891 A1 10/2012
 EP 2316359 B1 3/2013
 EP 1586275 B1 5/2013
 EP 1616529 B1 9/2013
 EP 2583633 B1 10/2014
 EP 2113210 B1 3/2016
 EP 2227155 B1 7/2016
 EP 2859858 B1 12/2016
 ES 2115068 T3 6/1998
 GB 1482943 A 8/1977
 GB 2032221 A 4/1980
 GB 2317566 A 4/1998
 GB 2379878 B 11/2004
 GB 2447767 B 8/2011
 JP S 50-100891 A 8/1975
 JP S 59-68513 U 5/1984
 JP S 59-141938 A 8/1984
 JP S 62-21343 A 9/1987
 JP S 62-227343 A 10/1987
 JP 62-292153 A 12/1987
 JP S 62-292154 A 12/1987
 JP S 63-109386 A 5/1988
 JP S 63-315049 A 12/1988
 JP H 01-151452 A 6/1989
 JP H 01-198540 A 8/1989
 JP H 02-71510 U 5/1990
 JP H 02-286149 A 11/1990
 JP H 02-292193 A 12/1990
 JP H 03-37061 A 2/1991
 JP H 04-25707 U 2/1992
 JP H 04-64351 A 2/1992
 JP H 04-30508 U 3/1992
 JP H 04-150847 A 5/1992
 JP H 04-152942 A 5/1992
 JP 05-095955 A 4/1993
 JP H 05-115490 A 5/1993
 JP H 06-70938 A 3/1994
 JP H 06-104503 A 4/1994
 JP H 06-217988 A 8/1994
 JP H 06-507081 A 8/1994
 JP H 07-500514 A 1/1995
 JP H 07-508910 A 10/1995
 JP H 07-308323 A 11/1995
 JP H 08-24266 A 1/1996
 JP H 08-275951 A 10/1996
 JP H 08-299351 A 11/1996
 JP H 08-336544 A 12/1996
 JP H 08-336545 A 12/1996
 JP H 09-503146 A 3/1997
 JP H 09-135553 A 5/1997
 JP H 09-140722 A 6/1997
 JP H 10-5237 A 1/1998
 JP H 10-295700 A 11/1998
 JP H 11-501543 A 2/1999
 JP H 11-128238 A 5/1999
 JP H 11-192235 A 7/1999
 JP H 11-253451 A 9/1999

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP	H 11-318918	A	11/1999	JP	2015-515339	A	5/2015
JP	2000-041991	A	2/2000	JP	5714508	B2	5/2015
JP	2000-070279	A	3/2000	JP	5836543	B1	12/2015
JP	2000-210299	A	8/2000	KR	100789356	B1	12/2007
JP	2000-271145	A	10/2000	RU	2154437	C1	8/2000
JP	2000-287987	A	10/2000	RU	22035	U1	3/2002
JP	2001-029353	A	2/2001	RU	2201169	C2	3/2003
JP	2001-502216	A	2/2001	RU	2304934	C2	8/2007
JP	2001-309925	A	11/2001	RU	2405603	C1	12/2010
JP	2002-177295	A	6/2002	SU	850068	A1	7/1981
JP	2002-186901	A	7/2002	WO	WO 92/22259	A2	12/1992
JP	2002-204808	A	7/2002	WO	WO 93/08757	A1	5/1993
JP	2002-238919	A	8/2002	WO	WO 93/14708	A1	8/1993
JP	2002-263579	A	9/2002	WO	WO 93/16646	A1	9/1993
JP	2002-301086	A	10/2002	WO	WO 93/20877	A1	10/1993
JP	2002-306504	A	10/2002	WO	WO 94/00059	A1	1/1994
JP	2002-330977	A	11/2002	WO	WO 94/21183	A1	9/1994
JP	2002-542690	A	12/2002	WO	WO 94/24949	A1	11/1994
JP	2003-000612	A	1/2003	WO	WO 95/09572	A1	4/1995
JP	2003-010201	A	1/2003	WO	WO 95/34259	A1	12/1995
JP	2003-510158	A	3/2003	WO	WO 96/30885	A1	10/1996
JP	2003-116870	A	4/2003	WO	WO 96/39086	A1	12/1996
JP	2003-126104	A	5/2003	WO	WO 98/16156	A1	4/1998
JP	2003-126110	A	5/2003	WO	WO 98/26739	A1	6/1998
JP	2003-153919	A	5/2003	WO	WO 98/35621	A1	8/1998
JP	2003-310627	A	5/2003	WO	WO 98/37815	A1	9/1998
JP	2003-530921	A	10/2003	WO	WO 98/47436	A1	10/1998
JP	2003-339730	A	12/2003	WO	WO 99/20213	A1	4/1999
JP	2004-129871	A	4/2004	WO	WO 99/52489	A1	10/1999
JP	2004-147701	A	5/2004	WO	WO 00/64358	A2	11/2000
JP	2005-027026	A	1/2005	WO	WO 00/74585	A2	12/2000
JP	2005-040222	A	2/2005	WO	WO 01/24713	A1	4/2001
JP	2005-066316	A	3/2005	WO	WO 01/54590	A1	8/2001
JP	2005-074088	A	3/2005	WO	WO 01/67970	A1	9/2001
JP	2005-507679	A	3/2005	WO	WO 01/95810	A2	12/2001
JP	2005-534451	A	11/2005	WO	WO 02/24080	A2	3/2002
JP	2006-006410	A	1/2006	WO	WO 02/38057	A1	5/2002
JP	2006-512149	A	4/2006	WO	WO 02/062241	A1	8/2002
JP	2006-116194	A	5/2006	WO	WO 03/082133	A1	10/2003
JP	2006-158525	A	6/2006	WO	WO 2004/012615	A1	2/2004
JP	2006-217716	A	8/2006	WO	WO 2004/026104	A2	4/2004
JP	2006-218296	A	8/2006	WO	WO 2004/032754	A2	4/2004
JP	2006-288431	A	10/2006	WO	WO 2004/032762	A1	4/2004
JP	2007-050181	A	3/2007	WO	WO 2004/032763	A2	4/2004
JP	2007-524459	A	8/2007	WO	WO 2004/037095	A2	5/2004
JP	2007-229454	A	9/2007	WO	WO 2004/060141	A2	7/2004
JP	2007-527747	A	10/2007	WO	WO 2004/098426	A1	11/2004
JP	2007-296369	A	11/2007	WO	WO 2004/112618	A2	12/2004
JP	2008-036390	A	2/2008	WO	WO 2005/117735	A1	12/2005
JP	2008-508065	A	3/2008	WO	WO 2005/122917	A1	12/2005
JP	2008-119250	A	5/2008	WO	WO 2006/012797	A1	2/2006
JP	2008-515562	A	5/2008	WO	WO 2006/042210	A2	4/2006
JP	2008-521503	A	6/2008	WO	WO 2006/058223	A2	6/2006
JP	D1339835	S	8/2008	WO	WO 2006/063199	A2	6/2006
JP	2008-212679	A	9/2008	WO	WO 2006/083988	A1	8/2006
JP	2008-536562	A	9/2008	WO	WO 2006/101661	A2	9/2006
JP	2008-284374	A	11/2008	WO	WO 2006/119139	A2	11/2006
JP	2009-511206	A	3/2009	WO	WO 2006/119376	A2	11/2006
JP	2009-082711	A	4/2009	WO	WO 2006/129465	A1	12/2006
JP	2009-517181	A	4/2009	WO	WO 2007/008703	A2	1/2007
JP	4262923	B2	5/2009	WO	WO 2007/008710	A2	1/2007
JP	2009-523567	A	6/2009	WO	WO 2007/038538	A1	4/2007
JP	2009-148557	A	7/2009	WO	WO 2007/040818	A1	4/2007
JP	2009-236177	A	10/2009	WO	WO 2007/047380	A2	4/2007
JP	2009-254819	A	11/2009	WO	WO 2007/047531	A2	4/2007
JP	2010-000336	A	1/2010	WO	WO 2007/056590	A1	5/2007
JP	2010-009686	A	1/2010	WO	WO 2007/087272	A2	8/2007
JP	2010-514923	A	5/2010	WO	WO 2007/089724	A2	8/2007
JP	2010-121865	A	6/2010	WO	WO 2007/143665	A2	12/2007
JP	2010-534522	A	11/2010	WO	WO 2008/016886	A2	2/2008
JP	2010-540186	A	12/2010	WO	WO 2008/042021	A1	4/2008
JP	2011-505198	A	2/2011	WO	WO 2008/049084	A2	4/2008
JP	2012-075899	A	4/2012	WO	WO 2008/051764	A2	5/2008
JP	2012-235658	A	11/2012	WO	WO 2008/089174	A2	7/2008
JP	5208761	B2	6/2013	WO	WO 2008/118709	A1	10/2008
				WO	WO 2008/130793	A1	10/2008
				WO	WO 2009/010565	A1	1/2009
				WO	WO 2009/018067	A1	2/2009
				WO	WO 2009/018406	A2	2/2009

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO 2009/027065	A1	3/2009
WO	WO 2009/046234	A2	4/2009
WO	WO 2009/073402	A2	6/2009
WO	WO 2009/088550	A2	7/2009
WO	WO 2009/120992	A2	10/2009
WO	WO 2009/141616	A1	11/2009
WO	WO 2010/017149	A1	2/2010
WO	WO 2010/068783	A1	6/2010
WO	WO 2011/008672	A2	1/2011
WO	WO 2011/044338	A2	4/2011
WO	WO 2011/052939	A2	5/2011
WO	WO 2011/060031	A1	5/2011
WO	WO 2011/100321	A2	8/2011
WO	WO 2011/144911	A1	11/2011
WO	WO 2012/044597	A1	4/2012
WO	WO 2012/061722	A2	5/2012
WO	WO 2012/128362	A1	9/2012
WO	WO 2012/135705	A1	10/2012
WO	WO 2012/135721	A1	10/2012
WO	WO 2013/018934	A1	2/2013
WO	WO 2013/062978	A2	5/2013
WO	WO 2014/092108	A1	6/2014
WO	WO 2016/009921	A1	12/2016

OTHER PUBLICATIONS

Technology Overview, printed from www.harmonicscalpel.com, Internet site, website accessed on Jun. 13, 2007, (3 pages).

Sherrit et al., "Novel Horn Designs for Ultrasonic/Sonic Cleaning Welding, Soldering, Cutting and Drilling," Proc. SPIE Smart Structures Conference, vol. 4701, Paper No. 34, San Diego, CA, pp. 353-360, Mar. 2002.

AST Products, Inc., "Principles of Video Contact Angle Analysis," 20 pages, (2006).

Lim et al., "A Review of Mechanism Used in Laparoscopic Surgical Instruments," Mechanism and Machine Theory, vol. 38, pp. 1133-1147, (2003).

Gooch et al., "Recommended Infection-Control Practices for Dentistry, 1993," Published: May 28, 1993; [retrieved on Aug. 23, 2008]. Retrieved from the internet: URL: <http://wonder.cdc.gov/wonder/prevguid/p0000191/p0000191.asp> (15 pages).

Huston et al., "Magnetic and Magnetostrictive Properties of Cube Textured Nickel for Magnetostrictive Transducer Applications," IEEE Transactions on Magnetics, vol. 9(4), pp. 636-640 (Dec. 1973).

Incropera et al., "Fundamentals of Heat and Mass Transfer", Wiley, New York (1990). (Book—not attached).

F. A. Duck, "Optical Properties of Tissue Including Ultraviolet and Infrared Radiation," pp. 43-71 in *Physical Properties of Tissue* (1990).

Orr et al., "Overview of Bioheat Transfer," pp. 367-384 in *Optical-Thermal Response of Laser-Irradiated Tissue*, A. J. Welch and M. J. C. van Gernert, eds., Plenum, New York (1995).

Campbell et al., "Thermal Imaging in Surgery," p. 19-3, in *Medical Infrared Imaging*, N. A. Diakides and J. D. Bronzino, Eds. (2008).

Sullivan, "Cost-Constrained Selection of Strand Diameter and Number in a Litz-Wire Transformer Winding," IEEE Transactions on Power Electronics, vol. 16, No. 2, Mar. 2001, pp. 281-288.

Sullivan, "Optimal Choice for Number of Strands in a Litz-Wire Transformer Winding," IEEE Transactions on Power Electronics, vol. 14, No. 2, Mar. 1999, pp. 283-291.

Graff, K.F., "Elastic Wave Propagation in a Curved Sonic Trans-mission Line," IEEE Transactions on Sonics and Ultrasonics, SU-17(1), 1-6 (1970).

Makarov, S. N., Ochmann, M., Desinger, K., "The longitudinal vibration response of a curved fiber used for laser ultrasound surgical therapy," Journal of the Acoustical Society of America 102, 1191-1199 (1997).

Morley, L. S. D., "Elastic Waves in a Naturally Curved Rod," Quarterly Journal of Mechanics and Applied Mathematics, 14: 155-172 (1961).

Walsh, S. J., White, R. G., "Vibrational Power Transmission in Curved Beams," Journal of Sound and Vibration, 233(3), 455-488 (2000).

<http://www.apicalinstr.com/generators.htm>.

<http://www.dotmed.com/listing/electrosurgical-unit/ethicon/ultracision-g110-1466724>.

<http://www.ethicon.com/gb-en/healthcare-professionals/products/energy-devices/capital/ge...>

<http://www.4-traders.com/JOHNSON-JOHNSON-4832/news/Johnson-Johnson-Ethicon-E...>

<http://www.medicalexpo.com/medical-manufacturer/electrosurgical-generator-6951.html>.

http://www.megadyne.com/es_generator.php.

<http://www.valleylab.com/product/es/generators/index.html>.

Covidien 501(k) Summary Soncision, dated Feb. 24, 2011 (7 pages).

Gerhard, Glen C., "Surgical Electrotechnology: Quo Vadis?," IEEE Transactions on Biomedical Engineering, vol. BME-31, No. 12, pp. 787-792, Dec. 1984.

Fowler, K.R., "A Programmable, Arbitrary Waveform Electrosurgical Device," IEEE Engineering in Medicine and Biology Society 10th Annual International Conference, pp. 1324, 1325 (1988).

LaCourse, J.R.; Vogt, M.C.; Miller, W.T., III; Selikowitz, S.M., "Spectral Analysis Interpretation of Electrosurgical Generator Nerve and Muscle Stimulation," IEEE Transactions on Biomedical Engineering, vol. 35, No. 7, pp. 505-509, Jul. 1988.

* cited by examiner

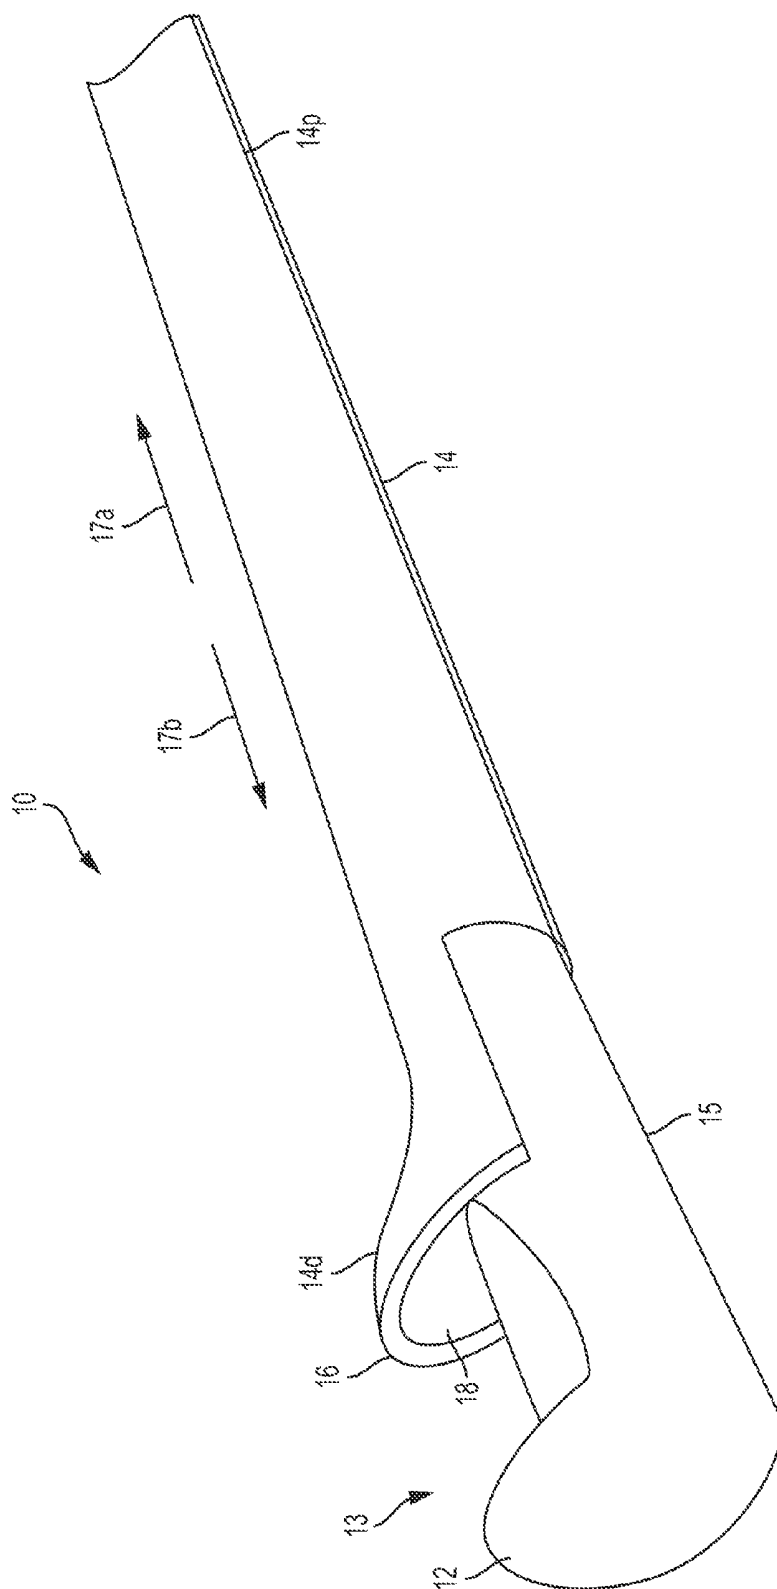


FIG. 1

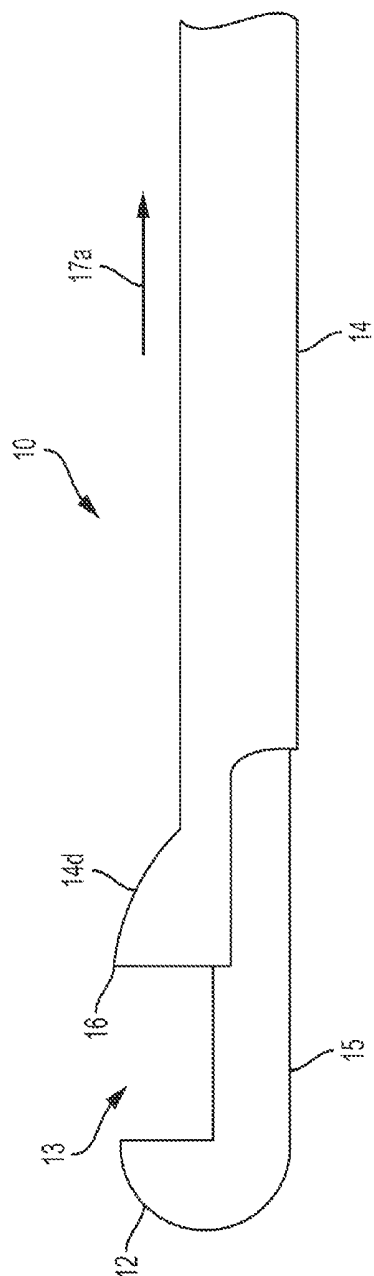


FIG. 2

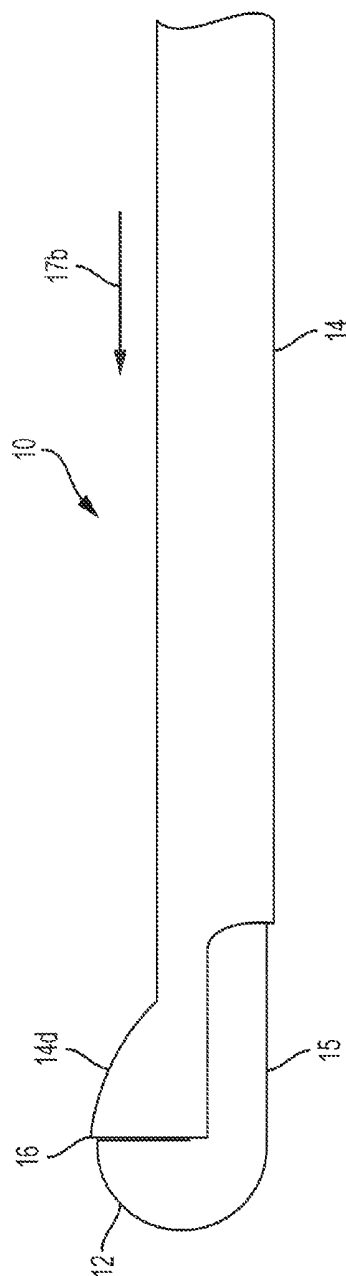


FIG. 3

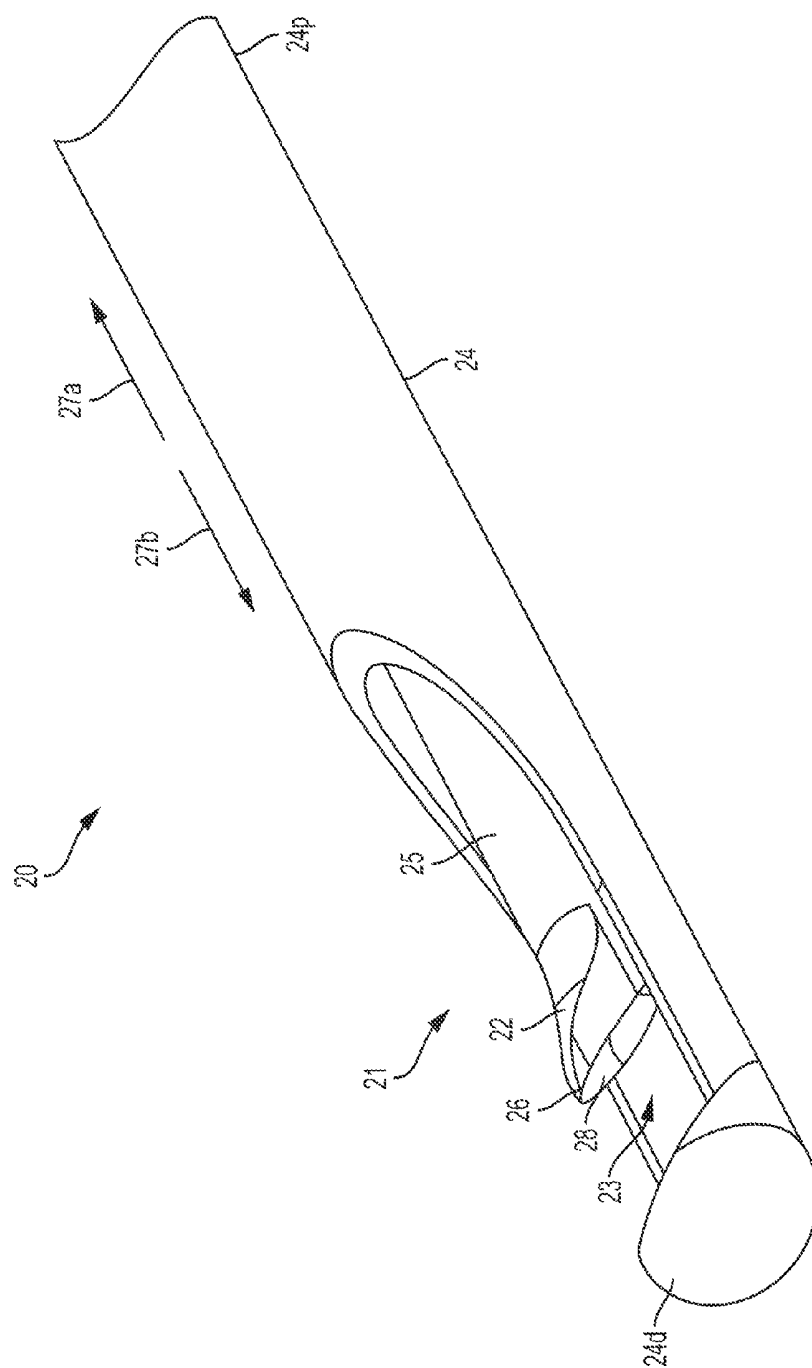


FIG. 4

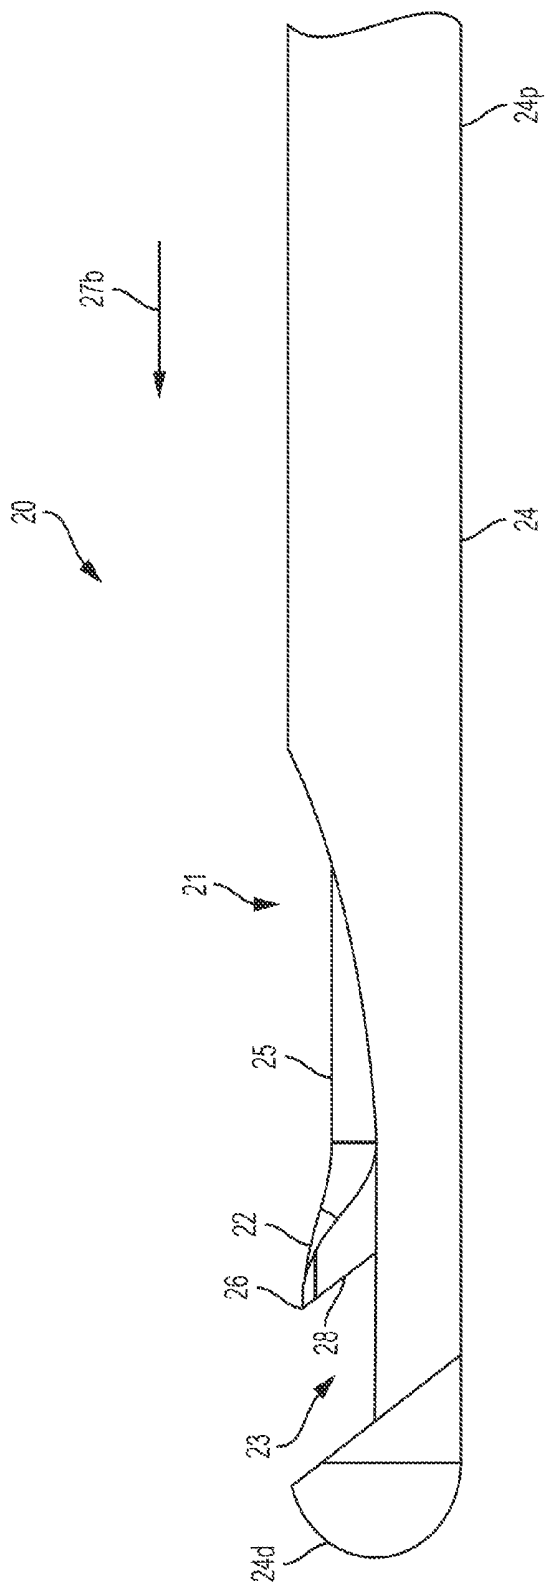


FIG. 5

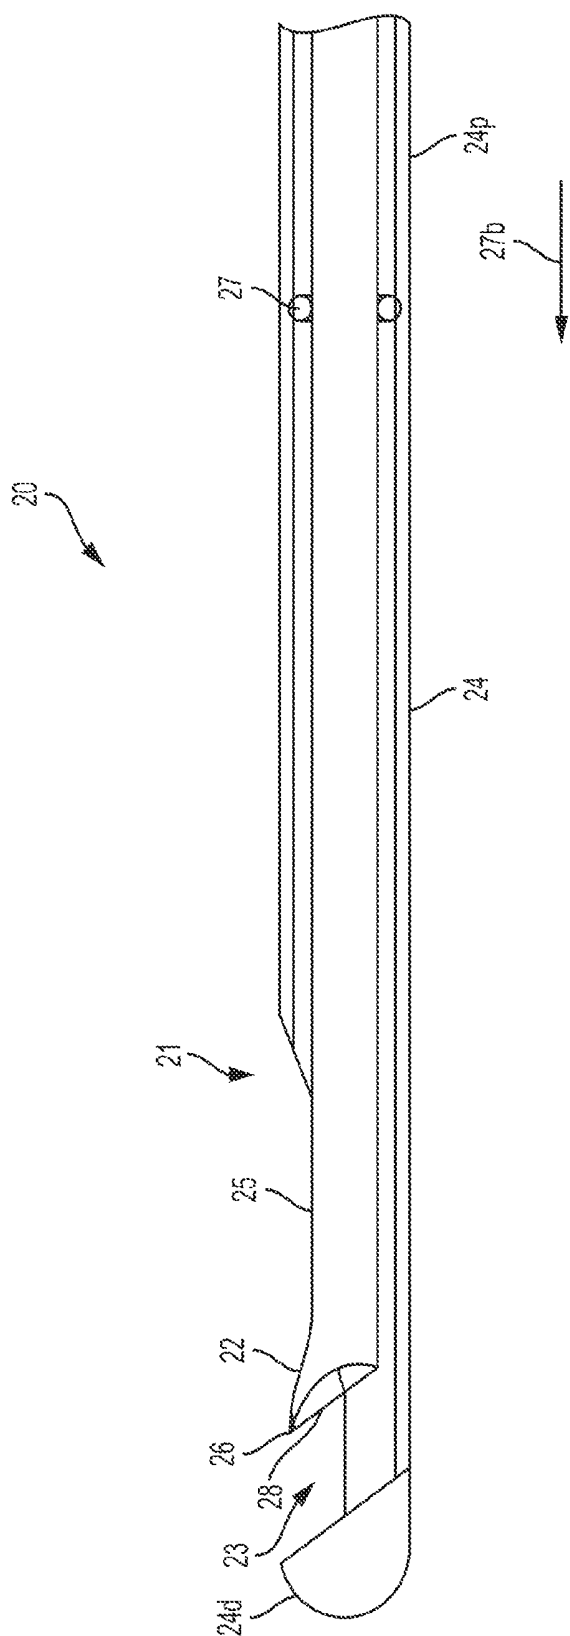


FIG. 6

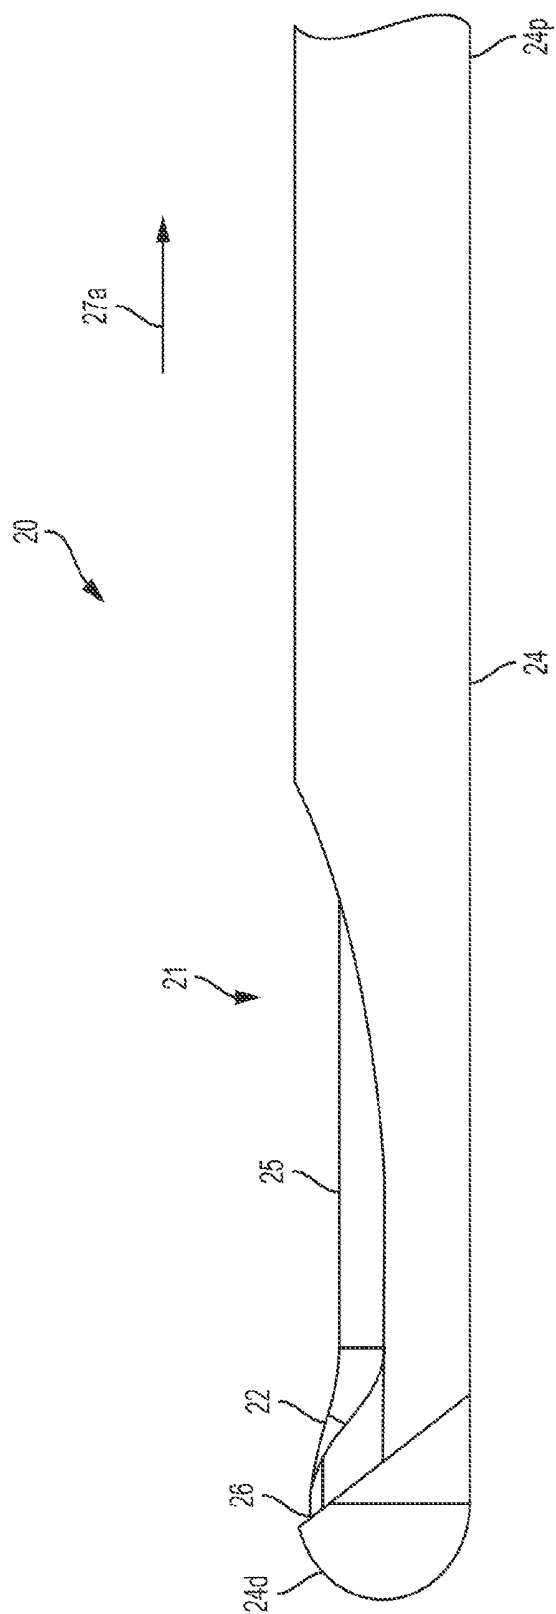


FIG. 7

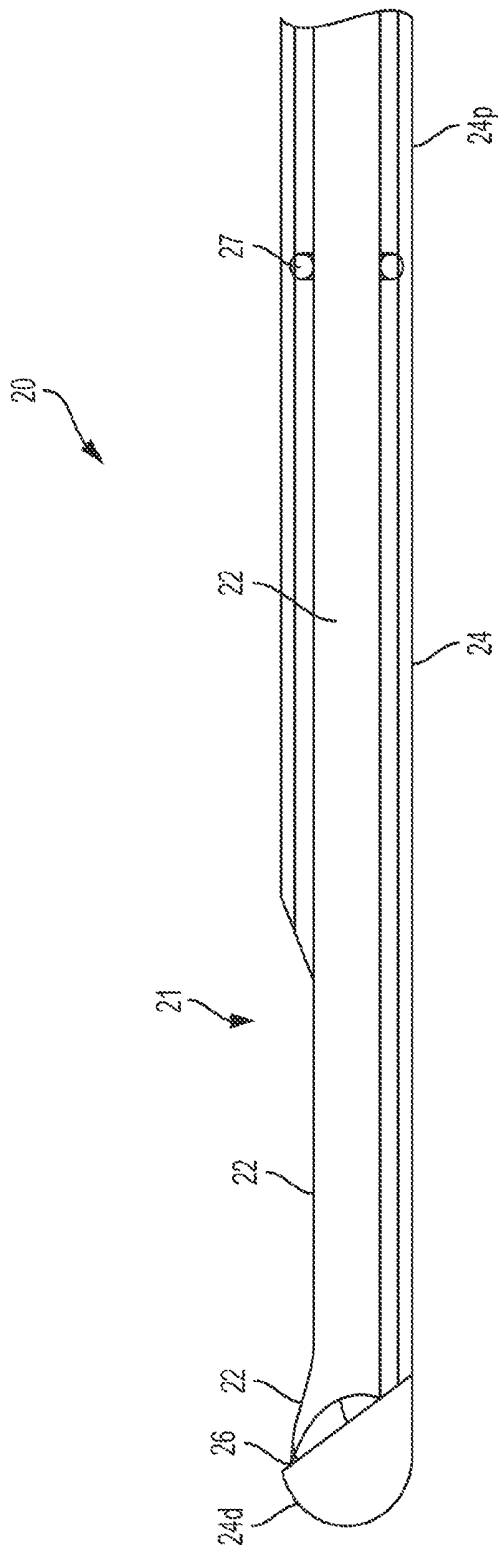


FIG. 8

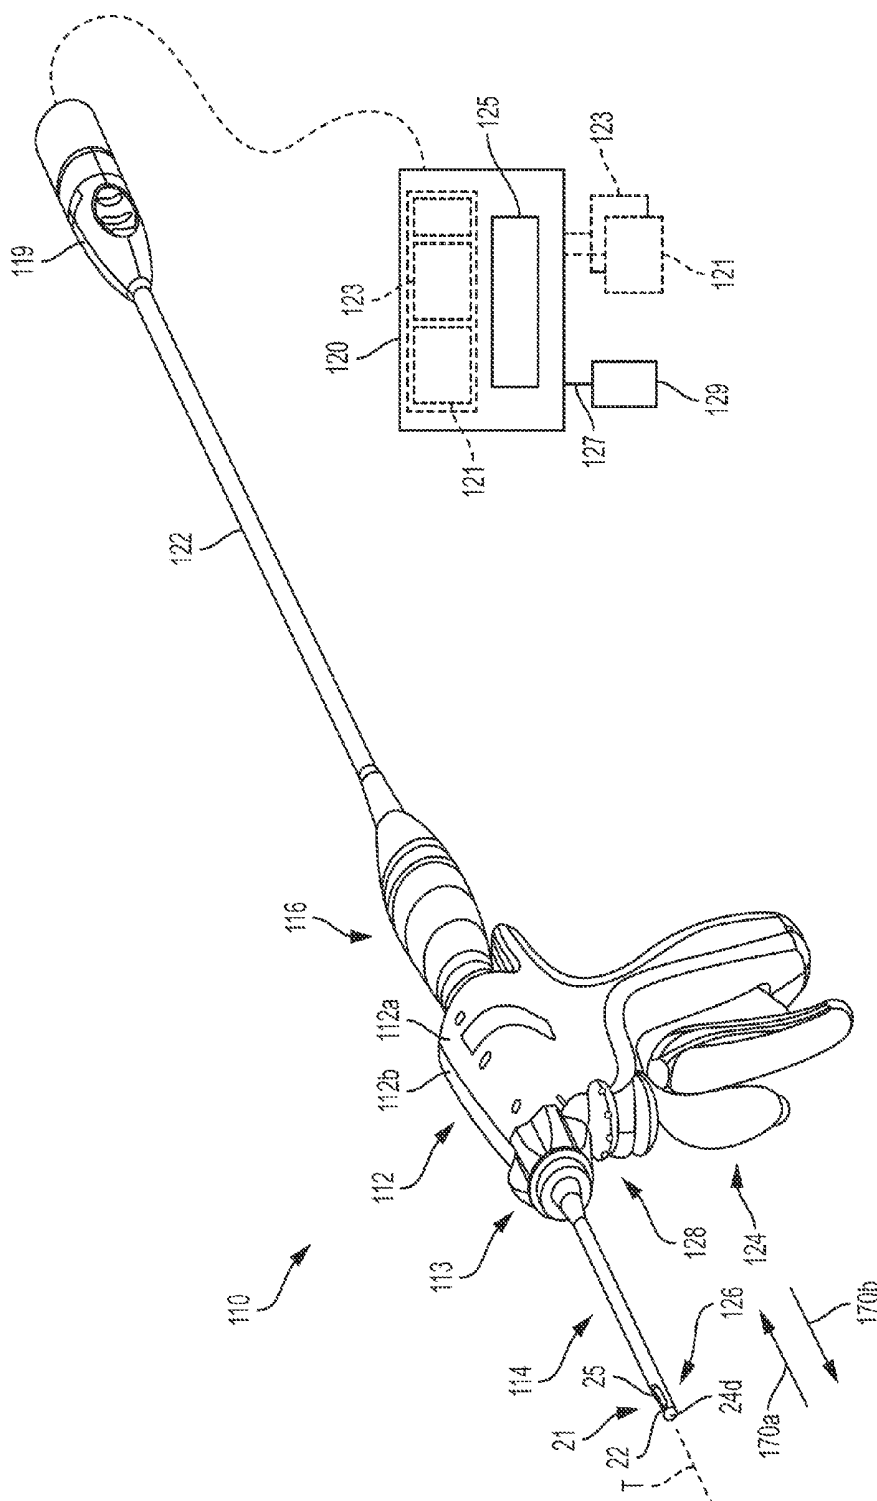


FIG. 9

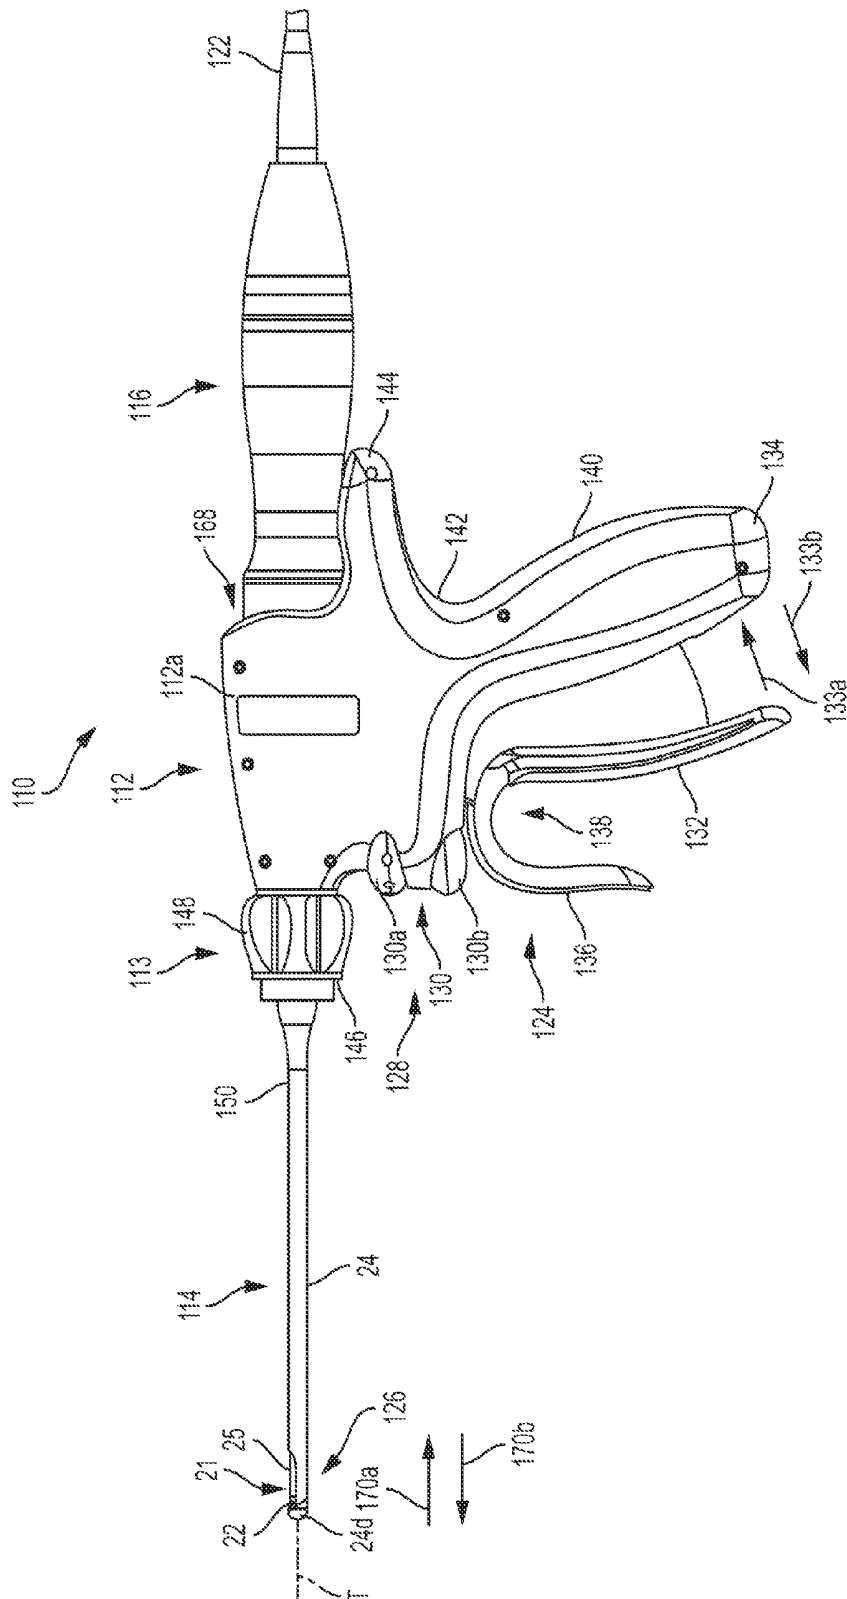


FIG. 10

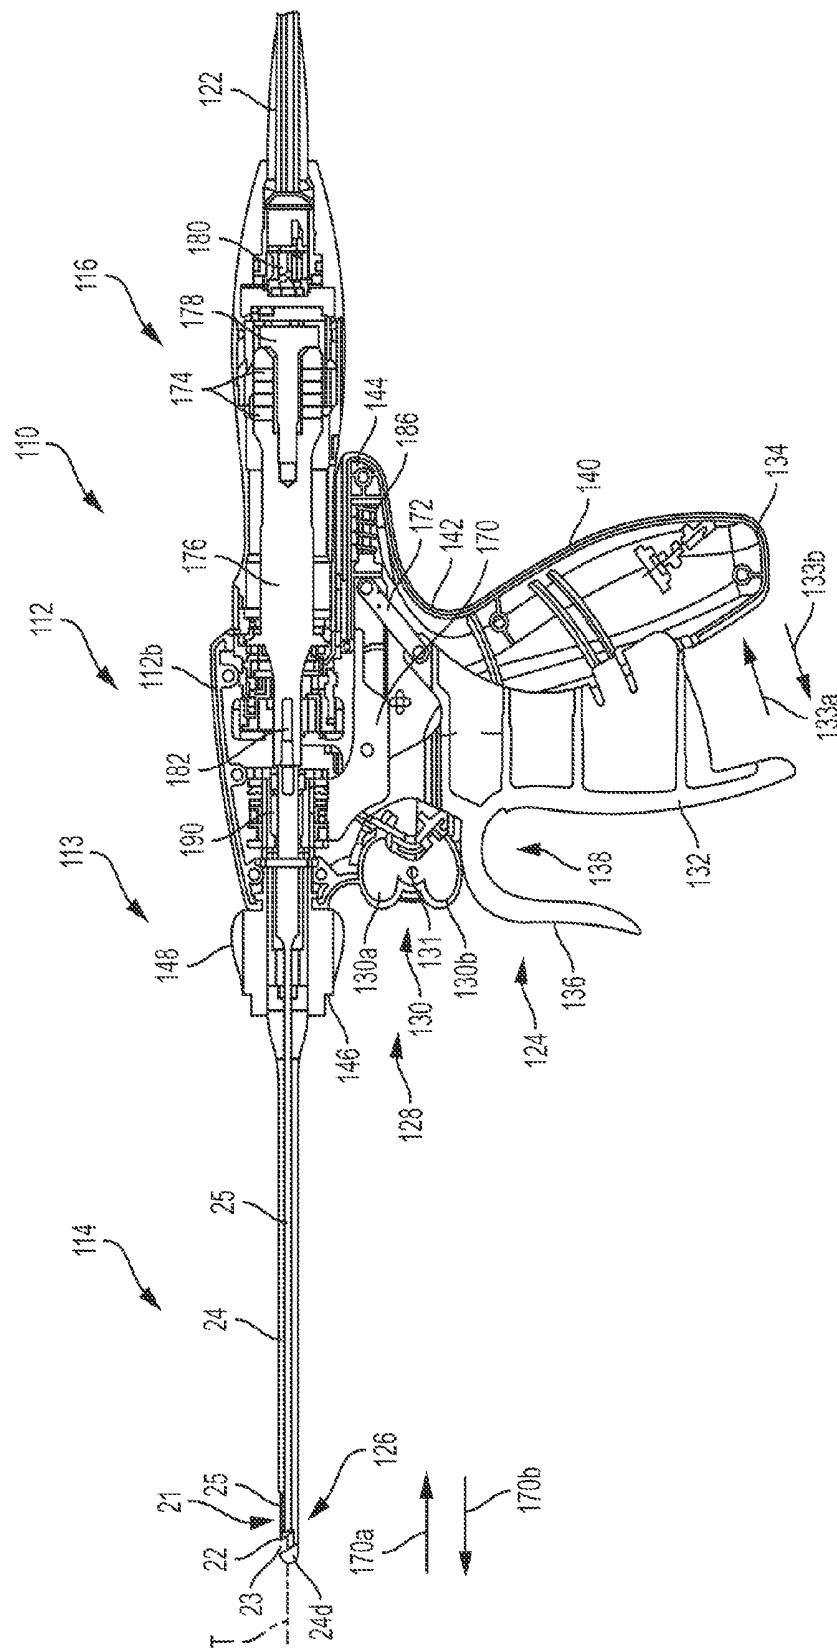


FIG. 11

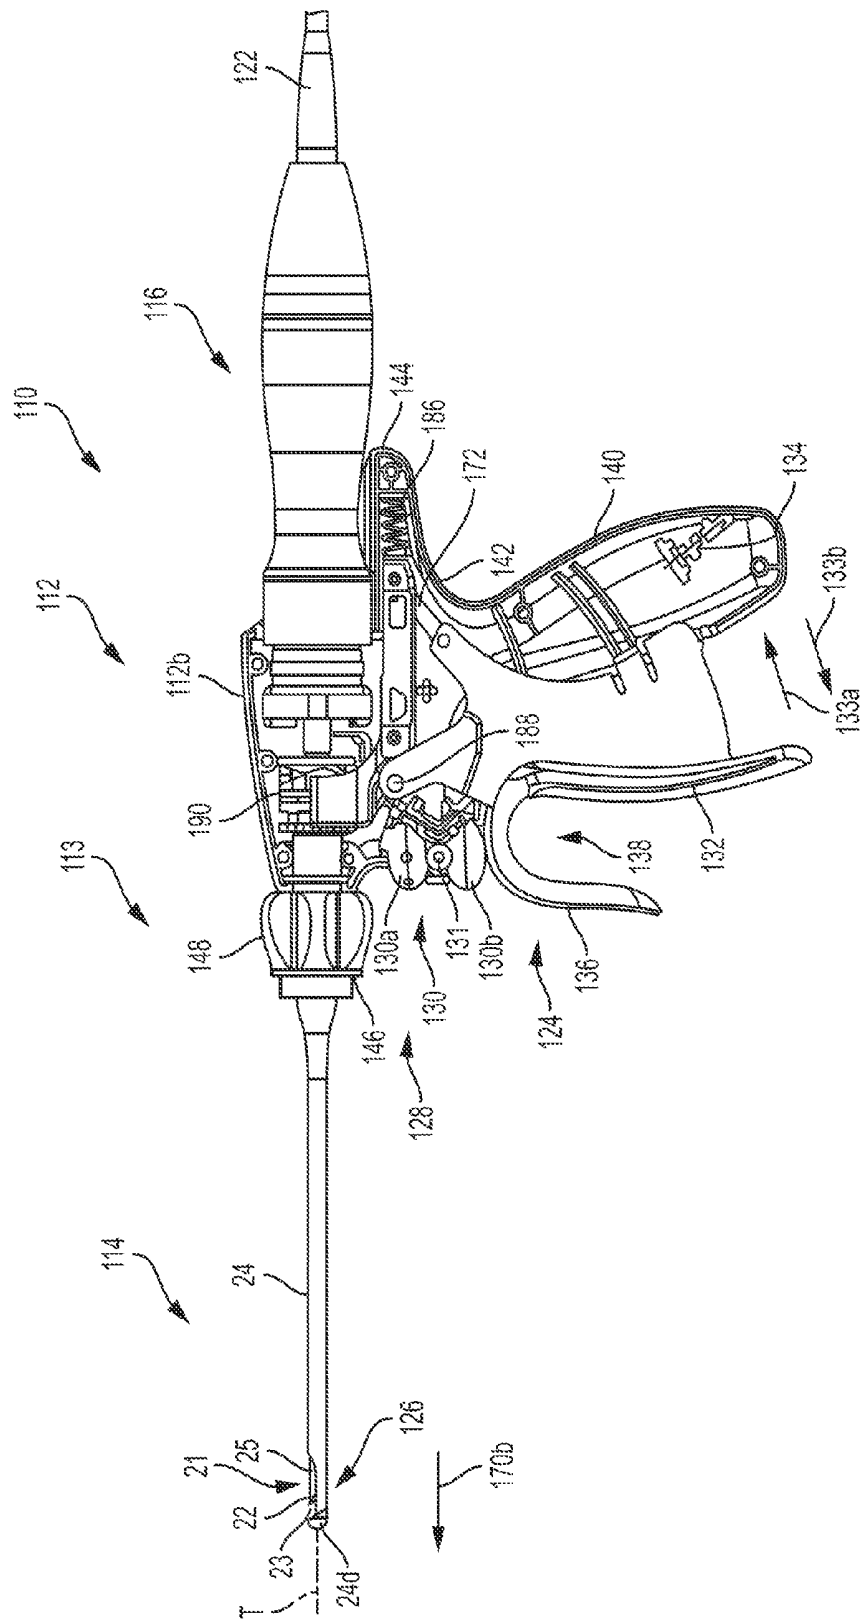


FIG. 12

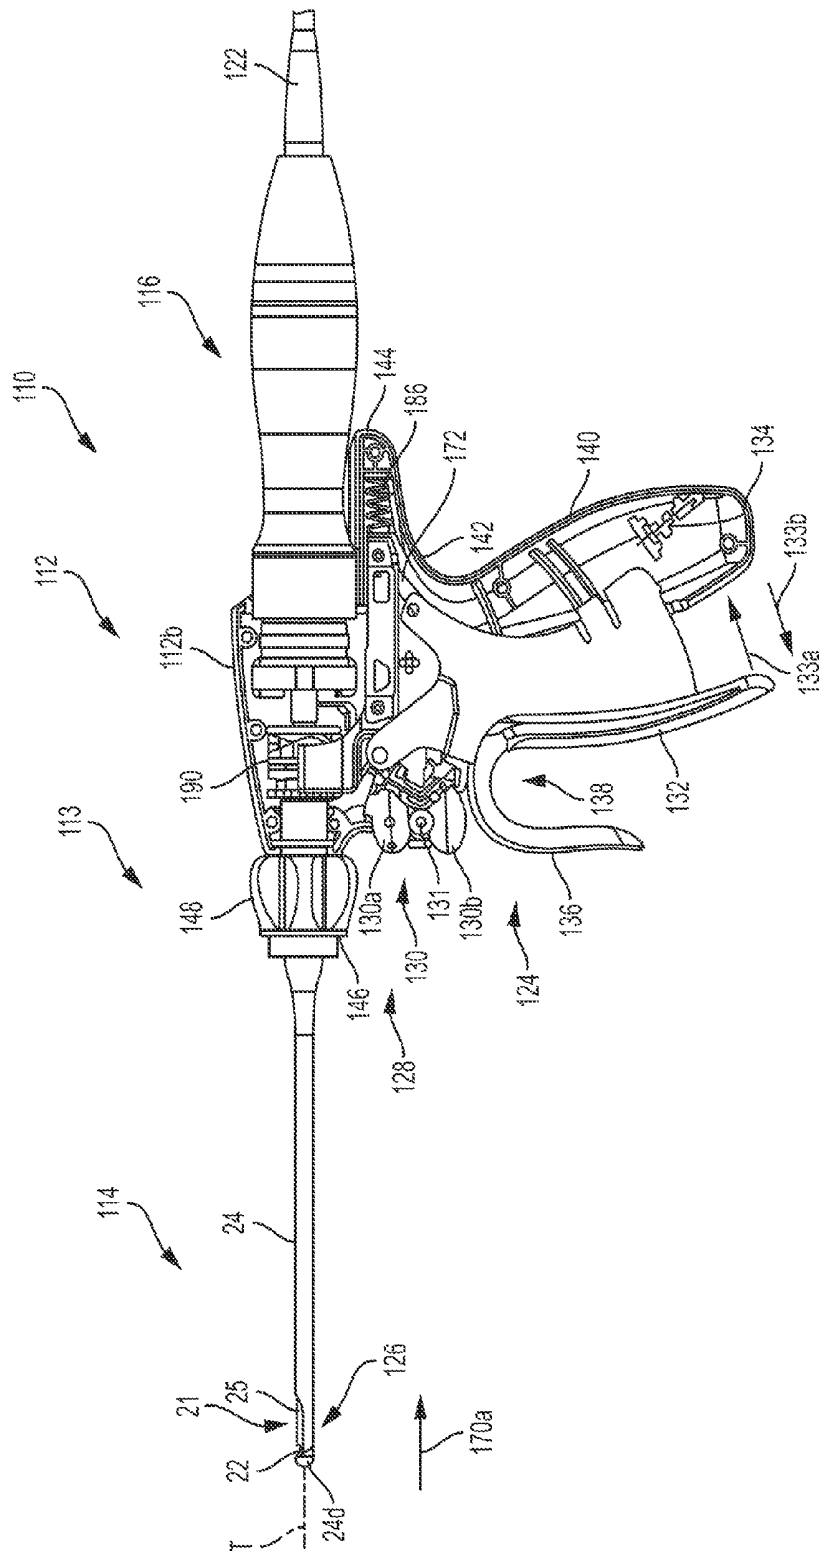


FIG. 13



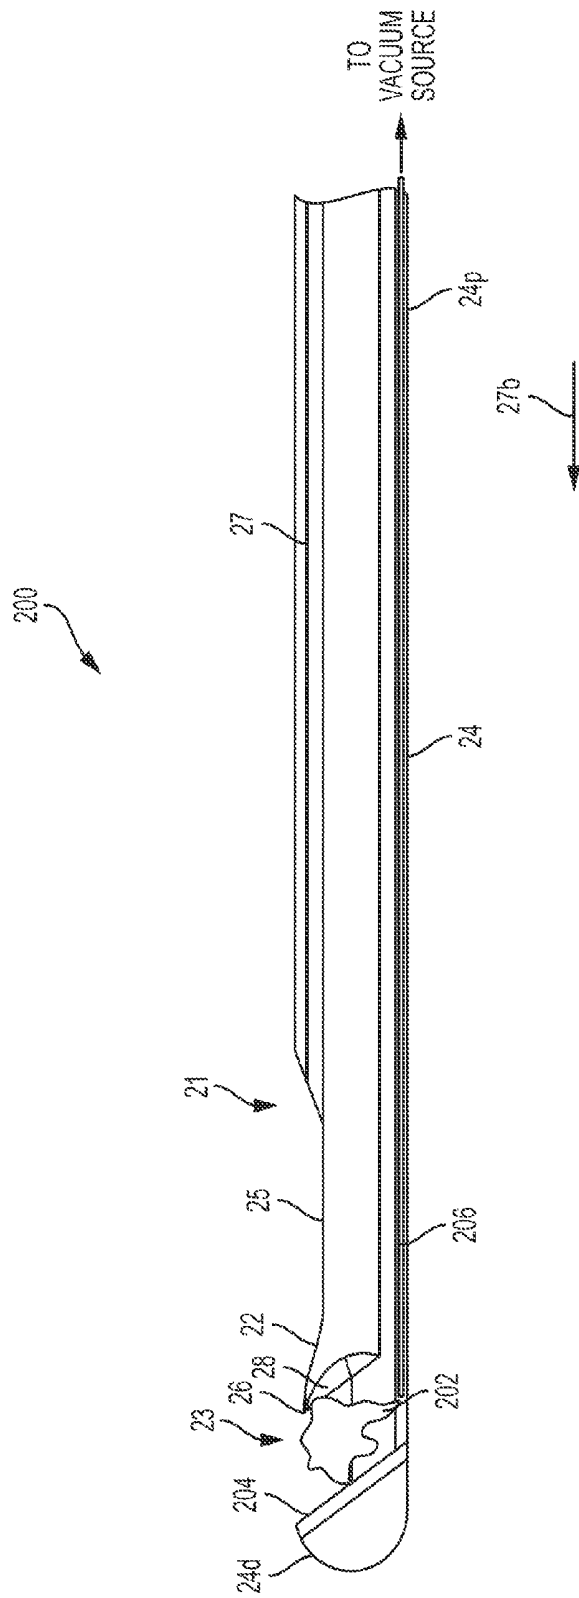


FIG. 14

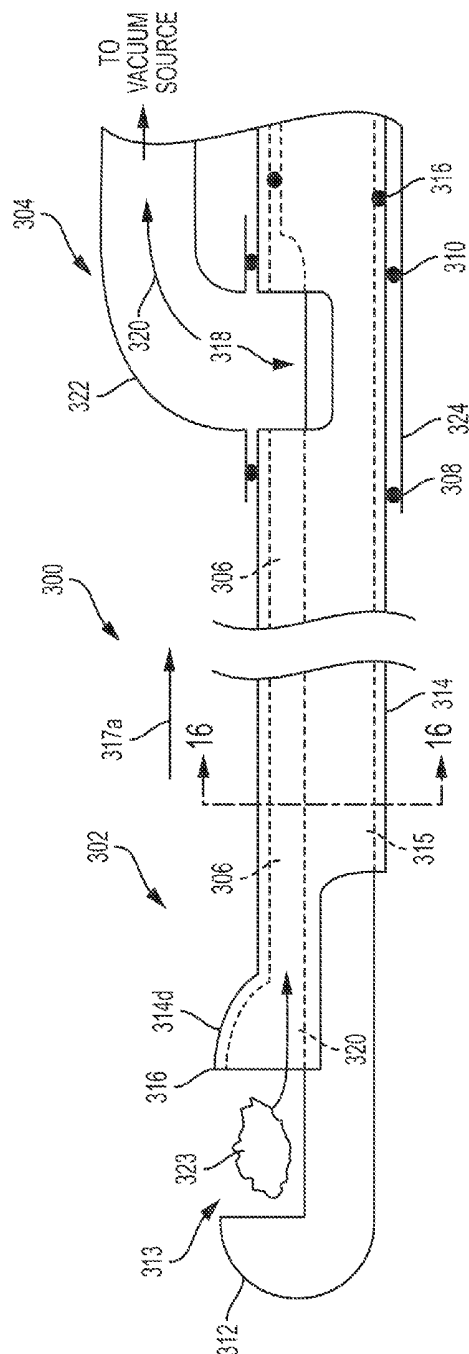

ॐ नमो भगवते वासुदेवाय

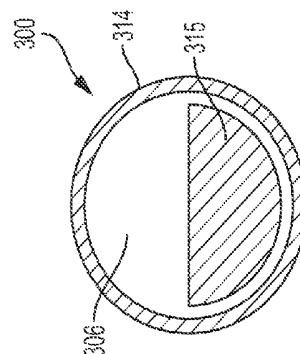

உ

APPARATUS AND METHOD FOR DISSECTING AND COAGULATING TISSUE

INTRODUCTION

The present embodiments of the invention relate to surgical instruments and, in various circumstances, to surgical cutting instruments for dissecting and coagulating tissue.

The present disclosure is related generally to surgical instruments including ultrasonic instruments. Ultrasonic surgical instruments, such as ultrasonic scalpels, are used in many applications in surgical procedures by virtue of their unique performance characteristics. Ultrasonic surgical instruments can be configured for open surgical use, laparoscopic, or endoscopic surgical procedures including robotic-assisted procedures.

Various surgical instruments utilize energy to cut and seal tissue that is being removed from a body. Some of these instruments include various jaws or other shearing elements to grasp tissue therein. Energy can be applied to the tissue such that the tissue can be cut and coagulated.

It may be desirable to minimize the bleeding at the site of the tissue removal and to have the ability to control the size of the tissue being removed and the space left behind in the body by the removed tissue.

SUMMARY

In one embodiment, an apparatus for dissection and coagulation of tissue is provided. The apparatus comprises an ultrasonic blade configured to dissect and seal tissue and having a proximal end and distal end, the distal end of the ultrasonic blade comprising a surface proximal of the distal end to engage tissue; and an elongate sheath configured to extend over the ultrasonic blade and being movable relative to the ultrasonic blade between a first position in which the elongate sheath is positioned over a proximal portion of the ultrasonic blade and a second position in which the elongate sheath moves distally towards the surface of the distal end of the ultrasonic blade such that tissue can be dissected therebetween.

In another embodiment, a distal end of the elongate sheath is sized and shaped to correspond to the size and shape of the surface of the distal end of the ultrasonic blade.

In another embodiment, the shape of the distal end of the ultrasonic blade and the distal end of the elongate sheath define a cavity at the location of the dissected tissue.

In another embodiment, the proximal end of the ultrasonic blade communicates with an excitation mechanism to deliver mechanical energy to at least one ultrasonic frequency to the distal end of the ultrasonic blade.

In another embodiment, a proximal end of the elongate sheath is configured to couple to an actuator to move the sheath between the first and second positions.

In another embodiment, the apparatus comprises a suction mechanism in the form of an elongate hollow tube positioned within the sheath and extending to the distal end thereof such that a distal end of the suction mechanism is configured to remove tissue dissected by the ultrasonic blade and the sheath.

In another embodiment, the suction mechanism is configured to irrigate an area located substantially around the tissue being dissected and removed.

In another embodiment, the distal end of the suction mechanism is positioned between the distal end of the sheath and the distal end of the ultrasonic blade.

In one embodiment, an apparatus for dissection and coagulation of tissue is provided. The apparatus comprises an elongate sheath having a proximal end and distal end, the distal end of the elongate sheath comprises a substantially flat surface proximal of the distal end to form an anvil; and an ultrasonic blade configured to dissect and seal tissue and being positioned within the elongate sheath, the ultrasonic blade being movable relative to the elongate sheath between a first position in which the ultrasonic blade is positioned a distance from the distal end of the elongate sheath and a second position in which the sheath moves proximally towards the distal end of the ultrasonic blade such that tissue can be dissected therebetween.

In another embodiment, a distal end of the ultrasonic blade is sized and shaped to correspond to the size and shape of the surface of the distal end of the elongate sheath forming the anvil.

In another embodiment, the shape of the distal end of the ultrasonic blade and the distal end of the elongate sheath create a cavity at the location of the dissected tissue.

In another embodiment, a proximal end of the ultrasonic blade communicates with a excitation mechanism to deliver energy to the distal end of the ultrasonic blade.

In another embodiment, a proximal end of the ultrasonic blade is configured to couple to an actuator to move the blade between the first and second positions.

In another embodiment, a suction mechanism in the form of an elongate hollow tube positioned within the sheath and extending to the distal end thereof such that a distal end of the suction mechanism is configured to remove tissue dissected by the ultrasonic blade and the sheath.

In another embodiment, the suction mechanism is configured to irrigate an area located substantially around the tissue being dissected and removed.

In another embodiment, the distal end of the suction mechanism is positioned between the distal end of the sheath and the distal end of the ultrasonic blade.

In one embodiment, an apparatus for dissection and coagulation of tissue is provided. The apparatus comprises an ultrasonic blade; an elongate sheath defining an aperture, wherein the ultrasonic blade is positioned within the aperture, the elongate sheath being movable distally relative to the ultrasonic blade between a first position defining a gap between a distal end of the sheath and the ultrasonic blade to receive target tissue in the gap, and a second position in which the elongate sheath is movable proximally towards the ultrasonic blade to grasp the target tissue therebetween; and a handle assembly mechanically coupled to the sheath to apply axial motion to the sheath.

In another embodiment, the ultrasonic blade comprises a curved surface for engaging the target tissue.

In another embodiment, a distal end of the ultrasonic blade extends distally beyond a distal end of the sheath.

In another embodiment, a distal end of the sheath extends distally beyond a distal end of the ultrasonic blade.

BRIEF DESCRIPTION OF THE DRAWINGS

The features and advantages of the various embodiments of the invention, and the manner of attaining them, will become more apparent and the embodiment of the invention itself will be better understood by reference to the following description of embodiments of the embodiment of the invention taken in conjunction with the accompanying drawings, wherein:

3

FIG. 1 is a perspective view of one embodiment of a surgical instrument having an ultrasonic blade positioned within a movable sheath, according to one embodiment;

FIG. 2 is a side view of the surgical instrument of FIG. 1 showing the movable sheath in a first position, according to one embodiment;

FIG. 3 is a side view of the surgical instrument of FIG. 1 showing the movable sheath in a second position, according to one embodiment;

FIG. 4 is a perspective view of another embodiment of a surgical instrument having a sheath that is movable relative to an ultrasonic blade, according to one embodiment;

FIG. 5 is a side view of the surgical instrument of FIG. 4 showing the movable sheath in a first position, according to one embodiment;

FIG. 6 is a cross-sectional side view of the surgical instrument of FIG. 5, according to one embodiment;

FIG. 7 is a side view of the surgical instrument of FIG. 4 showing the movable sheath in a second position, according to one embodiment;

FIG. 8 is a cross-sectional side view of the surgical instrument of FIG. 7, according to one embodiment;

FIG. 9 is perspective view of the surgical instrument of FIG. 1 or 4 coupled to a handle and a plug, according to one embodiment;

FIG. 10 is a side view of the surgical instrument of FIG. 9, according to one embodiment;

FIG. 11 is cross-sectional side view of the surgical instrument of FIG. 10, according to one embodiment;

FIG. 12 is a cross-sectional side view of the surgical instrument of FIG. 4 coupled to a handle with a movable sheath located in a first position where the sheath is movable relative to an ultrasonic blade, according to one embodiment;

FIG. 13 is a cross-sectional side view of the surgical instrument of FIG. 13 with a movable sheath located in a second position where the sheath is movable relative to an ultrasonic blade, according to one embodiment;

FIG. 14 is a cross-sectional side view of a surgical instrument having an ultrasonic blade positioned within a movable sheath, a suction tube, and a pad positioned on a distal end of the movable sheath, according to one embodiment;

FIG. 15 is a side view of a surgical instrument comprising an opening defined between the blade/ultrasonic waveguide and the outer tube, where in one embodiment the opening is configured to couple to a suction source; and

FIG. 16 is a sectional view taken along section line 16-16 of the distal end of the instrument shown in FIG. 15, according to one embodiment.

DESCRIPTION

Numerous specific details are set forth to provide a thorough understanding of the overall structure, function, manufacture, and use of the embodiments as described in the specification and illustrated in the accompanying drawings. It will be understood by those skilled in the art, however, that the embodiments may be practiced without such specific details. In other instances, well-known operations, components, and elements have not been described in detail so as not to obscure the embodiments described in the specification. Those of ordinary skill in the art will understand that the embodiments described and illustrated herein are non-limiting examples, and thus it can be appreciated that the specific structural and functional details disclosed herein

4

may be representative and illustrative. Variations and changes thereto may be made without departing from the scope of the claims.

Reference throughout the specification to “various embodiments,” “some embodiments,” “one embodiment,” or “an embodiment”, or the like, means that a particular feature, structure, or characteristic described in connection with the embodiment is included in at least one embodiment. Thus, appearances of the phrases “in various embodiments,” “in some embodiments,” “in one embodiment,” or “in an embodiment”, or the like, in places throughout the specification are not necessarily all referring to the same embodiment. Furthermore, the particular features, structures, or characteristics may be combined in any suitable manner in one or more embodiments. Thus, the particular features, structures, or characteristics illustrated or described in connection with one embodiment may be combined, in whole or in part, with the features structures, or characteristics of one or more other embodiments without limitation. Furthermore, it will be appreciated that for conciseness and clarity, spatial terms such as “vertical,” “horizontal,” “up,” and “down”, for example, may be used herein with respect to the illustrated embodiments. However, these terms are used to assist the reader and are not intended to be limiting and absolute.

The device described herein is a surgical instrument with improved ultrasonic forceps. The ultrasonic blade stays stationary while the anvil moves axially toward the blade in order to appose tissue. In this specific embodiment the end effector contains an ultrasonic blade and an anvil which matches the distal end of the blade so as to effect tissue between the two components as they translate relative to one another in an axial motion. The ultrasonic blade will be activated once the target tissue is apposed in the end effector. The activation of the ultrasonic blade will cauterize and cut through the target tissue. The device includes an ultrasonic transducer and an energy source if cordless, a cord if energy source is not in the device. The embodiments, however, are not limited in this context.

In another embodiment, a suction is applied to the target tissue to remove it after cutting is completed.

In another embodiment, monopolar and/or RF energy may be applied at the distal end for tissue effect.

Advantages of the disclosed embodiments include reduction in the amount of bleeding in surgical procedures such as, for example, otolaryngology (ENT) procedures. Specifically removing polyps or turbinate reduction. In current surgical procedures concerning the ear, nose and throat, when removing polyps or other tissues in that region of the body there is an excessive amount of bleeding that occurs, among other surgical procedures.

FIGS. 1-3 depict a surgical cutting and coagulating instrument 10 for dissecting and coagulating tissue according to one embodiment. In the illustrated embodiment, the instrument 10 includes an ultrasonic blade 12 positioned within an elongate sheath 14. The sheath 14 includes a distal end 14d and a proximal end 14p that is configured to couple to a handle that is configured to be grasped, manipulated and actuated by a clinician. The sheath 14 is movable relative to the ultrasonic blade 12 between a first proximal position in which the sheath 14 is positioned over a proximal portion of the blade 12 and a second position in which the sheath 14 moves distally in direction 17b such that tissue positioned in gap 13 between the blade 12 and the distal end 14d of the sheath 14 is dissected therebetween. Once the tissue is dissected, the sheath 14 is retracted proximally in direction 17a.

The elongate sheath **14** of the device can have a variety of configurations, and it can be flexible or rigid depending on the intended use. In one embodiment, the sheath **14** is relatively rigid. In other embodiments, at least portions of the sheath **14** can be semi-flexible or flexible to allow insertion therethrough. Thus, the instrument **10** can be adapted to be inserted in body cavities in endoscopic, laparoscopic, or open surgical procedures. One skilled in the art will appreciate that the sheath **14** can be made from a variety of biocompatible materials that have properties sufficient to enable the sheath **14** to be inserted and moved within channels of a body. The sheath **14** can also have an elongate length to allow the distal end of the sheath **14** to be positioned within the body while the proximal end remains external to the body. The inner lumens of the sheath **14** can also be used to pass other instruments or fluids through the instrument **10** for use during a surgical procedure, as will be discussed in more detail below.

The proximal end **14p** of the sheath **14** is configured to be coupled to an actuator operated by a handle assembly as discussed in connections with FIGS. 9-13 hereinbelow. The actuator can include various features, such as an actuating element for moving the sheath **14** between the first and second positions. The actuator can also include features to enable the delivery of energy from an energy source through the ultrasonic blade **12**. By way of non-limiting example, the actuating element can be a button, a switch, a knob, or any other member configured to actuate delivery of energy from an energy source. In lieu of an actuating element disposed on the handle, one skilled in the art will appreciate that the actuating element can be located elsewhere, including on a foot pedal. The energy source can be an internal energy source, such as a battery disposed in the handle, or the handle can be adapted to be coupled to an external energy source. An ultrasonic waveguide **15** is disposed and isolated from the sheath **14**. The ultrasonic blade **12** is disposed at the distal end of the ultrasonic waveguide **15**. The proximal end of the ultrasonic waveguide **15** is acoustically coupled to the ultrasonic transducer. The blade **12** can be formed integrally with the waveguide **15** or may be attached thereto by welding, screw, or bolt mechanisms. The ultrasonic waveguide **15** is positioned within the proximal end **14p** of the sheath **14** is configured to communicate with the ultrasonic transducer to deliver ultrasonic energy to the blade **12** at the distal end of the waveguide **15** such that tissue positioned between the blade **12** and the sheath **14** can be cut, coagulated, cauterized, evaluated, and the like. The ultrasonic energy delivered to the blade **12** can have various forms. For example, the energy can be of at least one ultrasonic frequency and be monopolar and/or RF energy sufficient to cut and coagulate tissue. In whatever form, e.g., ultrasonic vibrations or RF, the energy delivered to the tissue positioned in the gap **13** can be therapeutic or sub-therapeutic.

The ultrasonic blade **12** and the ultrasonic waveguide **15** positioned within the sheath **14** can also have a variety of configurations. The waveguide **15** can have an elongate length to allow a distal end of the blade **12** to be positioned within the body at the location of a tissue to be dissected such that the distal end of the blade **12** extends beyond the distal end of the sheath **14** while the proximal end remains external to the body. The ultrasonic blade **12** can have a diameter such that it can be positioned within the lumen of the sheath **14**.

The size and shape of the distal end of the blade **12** determines the size and shape of the dissected tissue and the cavity created when the tissue is cut and removed. In one

embodiment, the distal end of the blade **12** has a curved distal end with a substantially flat surface proximal of the curved distal end. For example, the distal end of the blade **12** can be in the form of an anvil and a pad. The distal end **14d** of the sheath **14** is sized and shaped to correspond to the size and shape of the distal end of the blade **12** such that the movement of the sheath **14** distally towards the distal end of the blade **12** creates a scissor action therebetween to cut tissue. The distal end **14d** of the sheath **14** includes an outer rim **16** that corresponds to the shape of the distal end of the blade **12**. The outer rim **16** forms a cavity **18** in the distal end **14d** of the sheath **14** such that, when tissue is dissected, a cavity that is substantially the size and shape of the cavity **18** of the distal end **14d** of the sheath **14** is formed where tissue is cut and removed from the body.

In the configuration illustrated in FIG. 2, the sheath **14** has been refracted proximally in direction **17a** to define a gap **13** for receiving target tissue therein. Once the target tissue is located in the gap **13**, as shown in FIG. 3, the sheath is advanced distally in direction **17b** to grasp the target tissue between the distal end of the ultrasonic blade **12** and the outer rim **16** defined by the distal end **14d** of the sheath **14**.

In other embodiments, rather than the sheath **14** being movable relative to the blade **12** as described above, the ultrasonic blade **22** can be configured to move relative to the sheath **24** such that tissue positioned between the ultrasonic blade **22** and the distal end **24d** of the sheath **24** is dissected therebetween. A movable ultrasonic blade **22** would require a movable ultrasonic transducer assembly that maintains close mechanical acoustic coupling between the transducer and the blade **22** through an ultrasonic waveguide.

FIGS. 4-8 depict a surgical cutting and coagulating instrument **20** for dissecting and coagulating tissue. In the illustrated embodiment, the instrument **20** includes an ultrasonic blade **22** coupled or formed integrally with an ultrasonic waveguide **25** positioned within an elongate sheath **24**. The sheath **24** includes a distal end **24d** and a proximal end **24p** that is configured to couple to a handle that is configured to be grasped, manipulated and actuated by a clinician. The sheath **24** defines an aperture **21** in which ultrasonic blade **22** is exposed allowing the sheath **24** to translate proximally in direction **27a** and distally in direction **27b**. The elongate sheath **24** is configured to be movable relative to the ultrasonic blade **22** between a first position in which the ultrasonic blade **22** is positioned a distance from the distal end **24d** of the elongate sheath **24** to define a gap **23** and a second position in which the sheath **24** moves proximally in direction **27a** towards the ultrasonic blade **22** to grasp the target tissue located in the gap **23** such that the target tissue can be dissected, treated, or evaluated by the ultrasonic blade **22**. Once the target tissue is dissected, treated, or evaluated, the sheath **24** can be advanced distally in direction **27b** to prepare the gap **23** for receiving more target tissue.

The size and shape of the distal end **24d** of the sheath **24** determines the size and shape of the target tissue and the cavity created when the tissue is cut and removed. In one embodiment, the distal end **24d** of the sheath **24** has a curved distal end with a substantially flat surface proximal of the curved distal end. For example, the distal end **24d** of the sheath **24** can be in the form of an anvil and a pad. The distal end of the ultrasonic blade **22** is sized and shaped to correspond to the size and shape of the distal end **24d** of the sheath **24** such that the movement of the sheath **24** proximally in direction **27a** towards the ultrasonic blade **22** creates a scissor or guillotine action therebetween to cut the target tissue. The distal end of the ultrasonic blade **22** defines an outer rim **26** that corresponds to the shape of the distal

end **24d** of the sheath **24**, which defines a cavity. The outer rim **26** defines a surface **28** at the distal end of the ultrasonic blade **22** such that, when tissue is dissected, the cavity defined by the distal end **24d** of the sheath **24** is substantially the size and shape of the surface **28** of the distal end of the ultrasonic blade **22** is formed where the target tissue is cut and removed from the body of the patient.

FIG. 5 is a side view of the surgical instrument **20** of FIG. 4 showing the movable sheath **24** in a first position. The sheath **24** is in the process of moving distally in direction **27b** to define the gap **23** for receiving the target tissue therein.

FIG. 6 is a cross-sectional side view of the surgical instrument **20** of FIG. 5. As shown, the sheath **24** is acoustically isolated from the ultrasonic waveguide **25** by resilient members **27**, which are positioned at nodes along the length of the waveguide **25**. The resilient isolation members **27** are located at the nodes to minimize or eliminate any acoustic coupling or vibratory transfer of energy from the waveguide **25** to the outer sheath **24**. It will be appreciated that mechanical displacement at the nodes is minimized whereas mechanical displacement at the antinodes is maximized.

FIG. 7 is a side view of the surgical instrument **20** of FIG. 4 showing the movable sheath **24** in a second position. Once the target tissue is located in the gap **23**, the sheath **24** is retracted proximally in direction **27a** to grasp the target tissue between the surface **28** (FIGS. 4-6) of the ultrasonic blade **22** and the distal end **24d** of the sheath **24**.

As explained above, other instruments can be passed through the device for use during a surgical procedure. In one embodiment, a suction and/or irrigation device can be used in combination with the instructions shown in FIGS. 1-8 such that the tissue that is dissected using an ultrasonic blade can be removed without the need to remove cutting and coagulating instrument. For example, a suction device can be positioned within the lumen of the sheath such that suction can occur in the space between the sheath and the ultrasonic blade. In one exemplary embodiment, a suction mechanism can be in the form of an elongate hollow tube positioned within either sheath **14**, **24** and extending to the distal end thereof such that a distal end of the suction mechanism is configured to remove tissue dissected by the ultrasonic blade and the sheath. The suction mechanism can also include additional features to effect the area of tissue dissection and removal. For example, the suction mechanism can also include features such that the suction mechanism can irrigate an area located substantially around the tissue being dissected and removed by the blade and the sheath.

As explained above, the instruments **10**, **20** shown in connection with FIGS. 1-8 can be coupled to a handle assembly to move the sheath **14**, **24** relative to the ultrasonic blade **12**, **22**. As previously discussed, the instruments **10**, **20** shown in connection with FIGS. 1-8 can be adapted and configured to move the ultrasonic blade **12**, **22** relative to the sheath **14**, **24**. This configuration would require the ultrasonic transducer and the acoustic assembly to be movable rather than the sheath **14**, **24**.

The description now turns to FIG. 9, where a perspective view of the surgical instrument of FIGS. 4-8 coupled to a handle, plug, and generator is illustrated. In the illustrated embodiment, the ultrasonic surgical instrument **110** may be employed in various surgical procedures including endoscopic or traditional open surgical procedures. In one example embodiment, the ultrasonic surgical instrument **110** comprises a handle assembly **112**, an elongated shaft assembly

bly **114**, an ultrasonic transducer **116**, and an ultrasonic waveguide **25** comprising an ultrasonic blade **22** at a distal end thereof. The handle assembly **112** comprises a trigger assembly **124**, a distal rotation assembly **113**, and a switch assembly **128**. The elongated shaft assembly **114** comprises an end effector **126**. The end effector **126** is formed of the distal end **24d** of the sheath **24**, which comprises an aperture **21** configured to receive a reciprocating ultrasonic blade **22** therein to dissect tissue or mutually grasp, cut, and coagulate vessels and/or tissue in cooperation with the ultrasonic blade **22**. The sheath **24** is mechanically coupled to actuating elements in the handle assembly **112** to actuate the sheath **24**, for example, to translate the sheath **24** proximally towards the ultrasonic blade **22** to grasp tissue within the aperture **21** defined by the sheath **24** or to reciprocate the sheath **24** distally away from the ultrasonic blade **22** prepare the aperture **21** for grasping tissue. When the sheath **24** extended distally in direction **170b**, a gap **23** (FIGS. 11 and 12) is defined to receive target tissue therein for further therapeutic or sub-therapeutic treatment by the ultrasonic blade **22**. When the sheath **24** is refracted proximally in direction **170a**, the target tissue is grasped between the ultrasonic blade **22** and the distal end **24d** of the sheath **24**.

The handle assembly **112** is adapted to receive the ultrasonic transducer **116** at the proximal end. The ultrasonic transducer **116** can be mechanically engaged to the elongated shaft assembly **114** and portions of the end effector **126**. The ultrasonic transducer **116** can be electrically coupled to a generator **120** via a cable **122** and plug **119**. In certain instances, the generator can be integrated with the handle assembly **112**, for example. Although the majority of the drawings depict a multiple end effector **126** for use in connection with laparoscopic surgical procedures, the ultrasonic surgical instrument **110** may be employed in more traditional open surgical procedures and in other embodiments, may be configured for use in endoscopic procedures. For the purposes herein, the ultrasonic surgical instrument **110** is described in terms of an endoscopic instrument; however, it is contemplated that an open and/or laparoscopic version of the ultrasonic surgical instrument **110** also may include the same or similar operating components and features as described herein. In one example embodiment, the handle assembly **112** is formed from two (2) housing portions or shrouds comprising a first portion **112a** and a second portion **112b**. The first and second portions **112a** and **112b** (as well as the other components described below) may be assembled together in any fashion known in the art. For example, alignment pins, snap-like interfaces, tongue and groove interfaces, locking tabs, adhesive ports, may all be utilized either alone or in combination for assembly purposes.

In various embodiments, the generator **120** comprises several functional elements, such as modules and/or blocks. Different functional elements or modules may be configured for driving different kinds of surgical devices. For example, an ultrasonic generator module **121** may drive an ultrasonic device, such as the ultrasonic surgical instrument **110**. In some example embodiments, the generator **120** also comprises an electrosurgery/RF generator module **123** for driving an electrosurgical device (or an electrosurgical embodiment of the ultrasonic surgical instrument **110**). In the example embodiment illustrated in FIG. 9, the generator **120** includes a control system **125** integral with the generator **120**, and a foot switch **129** connected to the generator via a cable **127**. The generator **120** may also comprise a triggering mechanism for activating a surgical instrument, such as the instrument **110**. The triggering mechanism may include a

power switch (not shown) as well as a foot switch **129**. When activated by the foot switch **129**, the generator **120** may provide energy to drive the acoustic assembly of the surgical instrument **110** and to drive the end effector **118** at a predetermined excursion level. The generator **120** drives or excites the acoustic assembly at any suitable resonant frequency of the acoustic assembly and/or derives the therapeutic/sub-therapeutic electromagnetic/RF energy.

In one embodiment, the electrosurgical/RF generator module **123** may be implemented as an electrosurgery unit (ESU) capable of supplying power sufficient to perform bipolar electrosurgery using radio frequency (RF) energy. In one embodiment, the ESU can be a bipolar ERBE ICC 350 sold by ERBE USA, Inc. of Marietta, Ga. In bipolar electrosurgery applications, as previously discussed, a surgical instrument having an active electrode and a return electrode can be utilized, wherein the active electrode and the return electrode can be positioned against, or adjacent to, the tissue to be treated such that current can flow from the active electrode to the return electrode through the tissue. Accordingly, the electrosurgical/RF module **123** generator may be configured for therapeutic purposes by applying electrical energy to the tissue **T** sufficient for treating the tissue (e.g., cauterization).

In one embodiment, the electrosurgical/RF generator module **123** may be configured to deliver a subtherapeutic RF signal to implement a tissue impedance measurement module. In one embodiment, the electrosurgical/RF generator module **123** comprises a bipolar radio frequency generator as described in more detail below. In one embodiment, the electrosurgical/RF generator module **112** may be configured to monitor electrical impedance **Z**, of tissue **T** and to control the characteristics of time and power level based on the tissue **T** by way of a return electrode provided on a clamp member of the end effector **126**. Accordingly, the electrosurgical/RF generator module **123** may be configured for subtherapeutic purposes for measuring the impedance or other electrical characteristics of the tissue **T**. Techniques and circuit configurations for measuring the impedance or other electrical characteristics of tissue **T** are discussed in more detail in commonly assigned U.S. Patent Publication No. 2011/0015631, titled "Electrosurgical Generator for Ultrasonic Surgical Instrument," the disclosure of which is herein incorporated by reference in its entirety.

A suitable ultrasonic generator module **121** may be configured to functionally operate in a manner similar to the GEN300 sold by Ethicon Endo-Surgery, Inc. of Cincinnati, Ohio as is disclosed in one or more of the following U.S. patents, all of which are incorporated by reference herein in their entireties: U.S. Pat. No. 6,480,796 (METHOD FOR IMPROVING THE START UP OF AN ULTRASONIC SYSTEM UNDER ZERO LOAD CONDITIONS); U.S. Pat. No. 6,537,291 (METHOD FOR DETECTING BLADE BREAKAGE USING RATE AND/OR IMPEDANCE INFORMATION); U.S. Pat. No. 6,662,127 (METHOD FOR DETECTING PRESENCE OF A BLADE IN AN ULTRASONIC SYSTEM); U.S. Pat. No. 6,977,495 (DETECTION CIRCUITRY FOR SURGICAL HANDPIECE SYSTEM); U.S. Pat. No. 7,077,853 (METHOD FOR CALCULATING TRANSDUCER CAPACITANCE TO DETERMINE TRANSDUCER TEMPERATURE); U.S. Pat. No. 7,179,271 (METHOD FOR DRIVING AN ULTRASONIC SYSTEM TO IMPROVE ACQUISITION OF BLADE RESONANCE FREQUENCY AT STARTUP); and U.S. Pat. No. 7,273,483 (APPARATUS AND METHOD FOR ALERTING GENERATOR FUNCTION IN AN ULTRASONIC SURGICAL SYSTEM). Furthermore, U.S.

Patent Application Publication No. 2014/0005702 A1, entitled ULTRASONIC SURGICAL INSTRUMENTS WITH DISTALLY POSITIONED TRANSDUCERS, and filed on Jun. 29, 2012, is incorporated by reference herein in its entirety.

It will be appreciated that in various embodiments, the generator **120** may be configured to operate in several modes. In one mode, the generator **120** may be configured such that the ultrasonic generator module **121** and the electrosurgical/RF generator module **123** may be operated independently.

For example, the ultrasonic generator module **121** may be activated to apply ultrasonic energy to the end effector **126** and subsequently, either therapeutic sub-therapeutic RF energy may be applied to the ultrasonic blade **22** of the end effector **126** by the electrosurgical/RF generator module **123**. As previously discussed, the sub-therapeutic electrosurgical/RF energy may be applied to tissue clamped between claim elements of the end effector **126** to measure tissue impedance to control the activation, or modify the activation, of the ultrasonic generator module **121**. Tissue impedance feedback from the application of the sub-therapeutic energy also may be employed to activate a therapeutic level of the electrosurgical/RF generator module **123** to seal the tissue (e.g., vessel) clamped between claim elements of the end effector **126**.

In another embodiment, the ultrasonic generator module **121** and the electrosurgical/RF generator module **123** may be activated simultaneously. In one example, the ultrasonic generator module **121** is simultaneously activated with a sub-therapeutic RF energy level to measure tissue impedance simultaneously while an ultrasonic blade **22**, for example, of the end effector **126** cuts and coagulates tissue (or vessel) clamped in the aperture **21** defined between the ultrasonic blade **22** and the distal end **24d** of the sheath **24**. Such feedback may be employed, for example, to modify the drive output of the ultrasonic generator module **121**. In another example, the ultrasonic generator module **121** may be driven simultaneously with electrosurgical/RF generator module **123** such that the ultrasonic blade **22** of the end effector **126** is employed for cutting the damaged tissue while the electrosurgical/RF energy is applied to electrode portions of the end effector **126** for sealing the tissue (or vessel).

When the generator **120** is activated via the triggering mechanism, electrical energy is continuously applied by the generator **120** to a transducer stack or assembly of the acoustic assembly. In another embodiment, electrical energy is intermittently applied (e.g., pulsed) by the generator **120**. A phase-locked loop in the control system of the generator **120** may monitor feedback from the acoustic assembly. The phase lock loop adjusts the frequency of the electrical energy sent by the generator **120** to match the resonant frequency of the selected longitudinal mode of vibration of the acoustic assembly. In addition, a second feedback loop in the control system **125** maintains the electrical current supplied to the acoustic assembly at a pre-selected constant level in order to achieve substantially constant excursion at the end effector **118** of the acoustic assembly. In yet another embodiment, a third feedback loop in the control system **125** monitors impedance between electrodes located in the end effector **126**.

In ultrasonic operation mode, the electrical signal supplied to the acoustic assembly may cause the distal end of the end effector **118**, to vibrate longitudinally in the range of, for example, approximately 20 kHz to 250 kHz. According to various embodiments, the ultrasonic blade **166** may

vibrate in the range of about 54 kHz to 56 kHz, for example, at about 55.5 kHz. In other embodiments, the ultrasonic blade **22** may vibrate at other frequencies including, for example, about 31 kHz or about 80 kHz. The excursion of the vibrations at the ultrasonic blade **22** can be controlled by, for example, controlling the amplitude of the electrical signal applied to the transducer assembly of the acoustic assembly by the generator **120**. As noted above, the triggering mechanism of the generator **120** allows a user to activate the generator **120** so that electrical energy may be continuously or intermittently supplied to the acoustic assembly. The generator **120** also has a power line for insertion in an electro-surgical unit or conventional electrical outlet. It is contemplated that the generator **120** can also be powered by a direct current (DC) source, such as a battery. The generator **120** can comprise any suitable generator, such as Model No. GEN04, and/or Model No. GEN11 available from Ethicon Endo-Surgery, Inc.

In various instances, when the acoustic assembly is energized, a vibratory motion standing wave is generated through the acoustic assembly. The amplitude of the vibratory motion at any point along the acoustic assembly depends on the location along the acoustic assembly at which the vibratory motion is measured. A minimum or zero crossing in the vibratory motion standing wave is generally referred to as a node (i.e., where motion is usually minimal), and an absolute value maximum or peak in the standing wave is generally referred to as an anti-node.

FIG. **10** is a side view of the surgical instrument **110** of FIG. **9** showing the handle assembly **112**, the distal rotation assembly **113**, the elongated shaft assembly **114**, and the end effector **126** showing the aperture **21** formed in the sheath **24**, the ultrasonic waveguide **25**, the ultrasonic blade **22**, and the distal end **24d** of the sheath **24**. In the illustrated embodiment, the end effector **126** is located at a distal end of the elongated shaft assembly **114**. A proximal end **150** of the elongated shaft assembly **114** mechanically engages the handle assembly **112** and the distal rotation assembly **113**. The proximal end **150** of the elongated shaft assembly **114** is received within the handle assembly **112** and the distal rotation assembly **113**.

In the illustrated embodiment, the trigger assembly **124** comprises a trigger **132** that operates in conjunction with a fixed handle **134**. The fixed handle **134** and the trigger **132** are ergonomically formed and adapted to interface comfortably with the user. The fixed handle **134** is integrally associated with the handle assembly **112**. The trigger **132** is pivotally movable relative to the fixed handle **134** as explained in more detail below with respect to the operation of the ultrasonic surgical instrument **110**. The trigger **132** is pivotally movable in direction **133a** toward the fixed handle **134** when the user applies a squeezing force against the trigger **132**. A spring element **186** (FIGS. **11-13**) may cause the trigger **132** to pivotally move in direction **133b** when the user releases the squeezing force against the trigger **132**.

In one example embodiment, the trigger **132** comprises an elongated trigger hook **136**, which defines an aperture **138** between the elongated trigger hook **136** and the trigger **132**. The aperture **138** is suitably sized to receive one or multiple fingers of the user therethrough. The trigger **132** also may comprise a resilient portion molded over the trigger substrate. The overmolded resilient portion **133a** is formed to provide a more comfortable contact surface for control of the trigger **132** in outward direction **133b**. In one example embodiment, the overmolded resilient portion may be provided over a portion of the elongated trigger hook **136**. The proximal surface of the elongated trigger hook **136** remains

uncoated or coated with a non-resilient substrate to enable the user to easily slide their fingers in and out of the aperture **138**. In another embodiment, the geometry of the trigger **132** forms a loop which defines an aperture **138** suitably sized to receive one or multiple fingers of the user therethrough. A fully closed loop trigger also may comprise a resilient portion molded over the trigger substrate.

In one example embodiment, the fixed handle **134** comprises a proximal contact surface **140** and a grip anchor or saddle surface **142**. The saddle surface **142** rests on the web where the thumb and the index finger are joined on the hand. The proximal contact surface **140** has a pistol grip contour that receives the palm of the hand in a normal pistol grip with no rings or apertures. The profile curve of the proximal contact surface **140** may be contoured to accommodate or receive the palm of the hand. A stabilization tail **144** is located towards a more proximal portion of the handle assembly **112**. The stabilization tail **144** may be in contact with the uppermost web portion of the hand located between the thumb and the index finger to stabilize the handle assembly **112** and make the handle assembly **112** more controllable.

In one example embodiment, the switch assembly **128** may comprise a toggle switch **130**. The toggle switch **130** may be implemented as a single component with a central pivot **131** (FIGS. **11-13**) located within inside the handle assembly **112** to eliminate the possibility of simultaneous activation. In one example embodiment, the toggle switch **130** comprises a first projecting knob **130a** (top) and a second projecting knob **130b** (bottom) to set the power setting of the ultrasonic transducer **116** between a minimum power level (e.g., MIN) and a maximum power level (e.g., MAX). In another embodiment, the rocker switch may pivot between a standard setting and a special setting. The special setting may allow one or more special programs to be implemented by the device. The toggle switch **130** rotates about the central pivot as the first projecting knob **130a** and the second projecting knob **130b** are actuated. The one or more projecting knobs **130a**, **130b** are coupled to one or more arms that move through a small arc and cause electrical contacts to close or open an electric circuit to electrically energize or de-energize the ultrasonic transducer **116** in accordance with the activation of the first or second projecting knob **130bs**. The toggle switch **130** is coupled to the generator **120** (FIG. **9**) to control the activation of the ultrasonic transducer **116**. The toggle switch **130** comprises one or more electrical power setting switches to activate the ultrasonic transducer **116** to set one or more power settings for the ultrasonic transducer **116**. The forces required to activate the toggle switch **130** are directed substantially toward the saddle point **142**, thus avoiding any tendency of the instrument to rotate in the hand when the toggle switch **130** is activated.

In one example embodiment, the first and second projecting knobs **130a**, **130b** are located on the distal end of the handle assembly **112** such that they can be easily accessible by the user to activate the power with minimal, or substantially no, repositioning of the hand grip, making it suitable to maintain control and keep attention focused on the surgical site (e.g., a monitor in a laparoscopic procedure) while activating the toggle switch **130**. The projecting knobs **130a**, **130b** may be configured to wrap around the side of the handle assembly **112** to some extent to be more easily accessible by variable finger lengths and to allow greater freedom of access to activation in awkward positions or for shorter fingers.

In the illustrated embodiment, the first projecting knob **130a** comprises a plurality of tactile elements, e.g., textured projections or “bumps” in the illustrated embodiment, to allow the user to differentiate the first projecting knob **130a** from the second projecting knob **130b**. It will be appreciated by those skilled in the art that several ergonomic features may be incorporated into the handle assembly **112**. Such ergonomic features are described in U.S. Pat. App. Pub. No. 2009/0105750 entitled “Ergonomic Surgical Instruments” which is incorporated by reference herein in its entirety.

In one example embodiment, the toggle switch **130** may be operated by the hand of the user. The user may easily access the first and second projecting knob **130bs** at any point while also avoiding inadvertent or unintentional activation at any time. The toggle switch **130** may readily be operated with a finger to control the power to the ultrasonic assembly **16** and/or to the ultrasonic assembly **116**. For example, the index finger may be employed to activate the first contact portion to turn on the ultrasonic assembly **116** to a maximum (MAX) power level. The index finger may be employed to activate the second contact portion to turn on the ultrasonic assembly **116** to a minimum (MIN) power level. In another embodiment, the rocker switch may pivot the instrument **110** between a standard setting and a special setting. The special setting may allow one or more special programs to be implemented by the instrument **110**. The toggle switch **130** may be operated without the user having to look at the first or second projecting knob **130a**, **130b**. For example, the first projecting knob **130a** or the second projecting knob **130b** may comprise a texture or projections to tactilely differentiate between the first and second projecting knobs **130a**, **130b** without looking.

In one example embodiment, the distal rotation assembly **113** is rotatable without limitation in either direction about a longitudinal axis “T.” The distal rotation assembly **113** is mechanically engaged to the elongated shaft assembly **114**. The distal rotation assembly **113** is located on a distal end of the handle assembly **112**. The distal rotation assembly **113** comprises a cylindrical hub **146** and a rotation knob **148** formed over the hub **146**. The hub **146** mechanically engages the elongated shaft assembly **114**. The rotation knob **148** may comprise fluted polymeric features and may be engaged by a finger (e.g., an index finger) to rotate the elongated shaft assembly **114**. The hub **146** may comprise a material molded over the primary structure to form the rotation knob **148**. The rotation knob **148** may be overmolded over the hub **146**. The hub **146** comprises an end cap portion that is exposed at the distal end. The end cap portion of the hub **146** may contact the surface of a trocar during laparoscopic procedures. The hub **146** may be formed of a hard durable plastic such as polycarbonate to alleviate any friction that may occur between the end cap portion and the trocar. The rotation knob **148** may comprise “scallops” or flutes formed of raised ribs and concave portions located between the ribs to provide a more precise rotational grip. In one example embodiment, the rotation knob **148** may comprise a plurality of flutes (e.g., three or more flutes). In other embodiments, any suitable number of flutes may be employed. The rotation knob **148** may be formed of a softer polymeric material overmolded onto the hard plastic material. For example, the rotation knob **148** may be formed of pliable, resilient, flexible polymeric materials including Versaflex® TPE alloys made by GLS Corporation, for example. This softer overmolded material may provide a greater grip and more precise control of the movement of the rotation knob **148**. It will be appreciated that any materials that provide adequate resistance to sterilization, are biocompat-

ible, and provide adequate frictional resistance to surgical gloves may be employed to form the rotation knob **148**. The rotation knob **148** is coupled to the shaft assembly **114** and is able to rotate the shaft assembly clockwise or counter-clockwise up to an including 360 degrees.

Referring to FIGS. 9-10, the elongated shaft assembly **114** comprises a proximal end **150** adapted to mechanically engage the handle assembly **112** and the distal rotation assembly **113**, and a distal end **152** adapted to mechanically engage the end effector **126**. The elongated shaft assembly **114** comprises an outer tubular sheath **24** which is mechanically coupled to the trigger **132** to reciprocate the outer tubular sheath **24**. A proximal end of the ultrasonic blade **22** is acoustically coupled to an ultrasonic waveguide, which is acoustically coupled to the ultrasonic transducer **116**. The outer sheath **24** is mechanically coupled to the trigger **132** of the handle assembly **112** through a yoke **170** (FIG. 11) and linkage **172** (FIG. 11) to move the sheath **24** in either direction **170a** or **170b** in response to the actuation and/or release of the trigger **132** in direction **133b** or **133a**, respectively. The pivotably moveable trigger **132** may generate reciprocating motion of the outer sheath **24** along the longitudinal axis “T.” Such motion may be used, for example, to clamp, grip, or grasp tissue located within of the gap **23** defined between the distal end **24d** of the sheath **24** and the distal end of the ultrasonic blade **22**. A linkage **172** (FIG. 11) translates the pivotal rotation of the trigger **132** to axial movement of a yoke **170** (FIG. 11) coupled to an actuation mechanism, which controls the reciprocation of the outer sheath **24** relative to the ultrasonic blade **22** in the end effector **126**.

In one example embodiment, the ultrasonically actuatable blade **22** is acoustically coupled to the ultrasonic transducer **116**. The trigger **132** on the handle assembly **112** is ultimately connected to a drive assembly, which together, mechanically cooperate to effect movement of the outer sheath **24**. Squeezing the trigger **132** in direction **133a** moves the outer sheath **24** proximally in direction **170a** from an open position to a closed position to grasp tissue located in the gap **23** between the distal end of the ultrasonic blade **22** and the distal end **24d** of the sheath **24**. Releasing the trigger **132** in direction **133b** moves the outer sheath **24** distally in direction **170b** from a closed position to an open position, wherein the ultrasonic blade **22** and the distal portion **24d** are disposed in a spaced relation relative to one another.

The proximal portion of the handle assembly **112** comprises a proximal opening **168** to receive the distal end of the ultrasonic assembly **116**. The ultrasonic assembly **116** is inserted in the proximal opening **168** and is mechanically engaged to the elongated shaft assembly **114**.

FIG. 11 is cross-sectional side view of the surgical instrument **110** of FIG. 10. The trigger **132** pivotally moves about pivot **188** (FIG. 12) between the first and second portions **112a**, **112b** (FIG. 9) of the handle assembly **112**. The trigger **132** is mechanically coupled to a linkage **172**, which is coupled to a yoke **170** to convert pivotal motion of the trigger **132** to axial motion of the yoke **170**. The yoke **170** is operably coupled to a drive member **190**. The drive member **190** is connected to the outer sheath **24**. As the trigger **132** is squeezed, the trigger **132** moves in direction **133a** towards the fixed handle **134** portion and pivots about the pivot point **188** (FIGS. 12 and 13) and the linkage **172** drives the yoke **170** axially in a proximal direction **170a** to retract the sheath **24** and close the gap **23** between the blade **22** and the distal end **24d** of the sheath **24** to grasp target tissue therebetween. As the yoke **170** is driven proximally,

the yoke **170** compresses a return spring **186**. When the trigger **132** is released, the return spring **186** returns the trigger **132** to its initial position in direction **133b** and drives the yoke **170** axially in a distal direction **170b** to advance the sheath **24** distally and open the gap **23** between the blade **22** and the distal end **24d** of the sheath **24** to receive target tissue therebetween.

In the embodiment illustrated in FIG. **11**, a cross-sectional view of the ultrasonic transducer **116** is shown within a partial cutaway view of the handle assembly **112**. One example embodiment of the ultrasonic surgical instrument **110** comprises the ultrasonic signal generator **120** (FIG. **9**) coupled to the ultrasonic transducer **116**, comprising a hand piece housing **112b**, and an ultrasonically actuatable single or multiple element end effector **126**. As previously discussed, the end effector **126** comprises an ultrasonically actuatable blade **22**. The ultrasonic transducer **116**, which is known as a "Langevin stack," generally includes a transduction portion, a first resonator portion or end-bell **178**, and a second resonator portion or fore-bell **176**, and ancillary components. The total construction of these components is a resonator. The ultrasonic transducer **116** is preferably an integral number of one-half system wavelengths ($n\lambda/2$; where "n" is any positive integer; e.g., $n=1, 2, 3 \dots$) in length. An acoustic assembly includes the ultrasonic transducer **116**, a nose cone, a velocity transformer, and a surface.

In one example embodiment, the distal end of the end-bell **178** is connected to the proximal end of the transduction portion, and the proximal end of the fore-bell **176** is connected to the distal end of the transduction portion. The fore-bell **176** and the end-bell **178** have a length determined by a number of variables, including the thickness of the transduction portion, the density and modulus of elasticity of the material used to manufacture the end-bell **178** and the fore-bell **176**, and the resonant frequency of the ultrasonic transducer **116**. The fore-bell **176** may be tapered inwardly from its proximal end to its distal end to amplify the ultrasonic vibration amplitude as the velocity transformer, or alternately may have no amplification. A suitable vibrational frequency range may be about 20 Hz to 32 kHz and a well-suited vibrational frequency range may be about 30-10 kHz. A suitable operational vibrational frequency may be approximately 55.5 kHz, for example.

In one example embodiment, the piezoelectric elements **174** may be fabricated from any suitable material, such as, for example, lead zirconate-titanate, lead meta-niobate, lead titanate, barium titanate, or other piezoelectric ceramic material. An electrical coupling **180** includes positive and negative electrodes electrically coupled to the piezoelectric elements **174**. The piezoelectric elements include a bore extending through the center. The positive and negative electrodes are electrically coupled to wires coupled to the piezoelectric elements **174**. The wires are encased within the cable **122** and electrically connectable to the ultrasonic signal generator **120** (FIG. **9**).

The ultrasonic transducer **116** of the acoustic assembly converts the electrical signal from the ultrasonic signal generator **120** into mechanical energy that results in primarily a standing acoustic wave of longitudinal vibratory motion of the ultrasonic transducer **116** and the ultrasonic blade **22** portion of the end effector **126** at ultrasonic frequencies. In another embodiment, the vibratory motion of the ultrasonic transducer **116** may act in a different direction. For example, the vibratory motion may comprise a local longitudinal component of a more complicated motion of the tip of the elongated shaft assembly **114**. A suitable generator is available as model number GEN11, from Ethicon Endo-

Surgery, Inc., Cincinnati, Ohio. When the acoustic assembly **106** is energized, a vibratory motion standing wave is generated through the acoustic assembly. The ultrasonic surgical instrument **110** is designed to operate at a resonance such that an acoustic standing wave pattern of predetermined amplitude is produced. The amplitude of the vibratory motion at any point along the acoustic assembly **106** depends upon the location along the acoustic assembly at which the vibratory motion is measured. A minimum or zero crossing in the vibratory motion standing wave is generally referred to as a node (i.e., where motion is minimal), and a local absolute value maximum or peak in the standing wave is generally referred to as an anti-node (e.g., where local motion is maximal). The distance between an anti-node and its nearest node is one-quarter wavelength ($\lambda/4$).

The wires transmit an electrical signal from the ultrasonic signal generator **120** (FIG. **9**) to the positive and negative electrodes. The piezoelectric elements **174** are energized by the electrical signal supplied from the ultrasonic signal generator **120** in response to an actuator, such as a foot switch, for example, to produce an acoustic standing wave in the acoustic assembly. The electrical signal causes disturbances in the piezoelectric elements **174** in the form of repeated small displacements resulting in large alternating compression and tension forces within the material. The repeated small displacements cause the piezoelectric elements **174** to expand and contract in a continuous manner along the axis of the voltage gradient, producing longitudinal waves of ultrasonic energy. The ultrasonic energy is transmitted through the acoustic assembly to the ultrasonic blade **22** portion of the end effector **126** via a transmission component or an ultrasonic transmission waveguide **25** of the elongated shaft assembly **114**.

In one example embodiment, in order for the acoustic assembly to deliver energy to the ultrasonic blade **22** portion of the end effector **126**, all components of the acoustic assembly must be acoustically coupled to the blade **22**. The distal end of the ultrasonic transducer **116** may be acoustically coupled at the surface to the proximal end of the ultrasonic transmission waveguide **25** by a threaded connection such as a stud **182** to the fore-bell **176**.

In one example embodiment, the components of the acoustic assembly are preferably acoustically tuned such that the length of any assembly is an integral number of one-half wavelengths ($n\lambda/2$), where the wavelength λ is the wavelength of a pre-selected or operating longitudinal vibration drive frequency f_d of the acoustic assembly. It is also contemplated that the acoustic assembly may incorporate any suitable arrangement of acoustic elements.

In one example embodiment, the ultrasonic blade **22** may have a length substantially equal to an integral multiple of one-half system wavelengths ($n\lambda/2$). A distal end of the blade **22** may be disposed near an antinode in order to provide the maximum longitudinal excursion of the distal end. When the transducer assembly is energized, the distal end of the blade **22** may be configured to move in the range of, for example, approximately 10 to 500 microns peak-to-peak, and preferably in the range of about 30 to 64 microns at a predetermined vibrational frequency of 55 kHz, for example.

In one example embodiment, the ultrasonic blade **22** may be coupled to the ultrasonic transmission waveguide **25**. The blade **22** and the ultrasonic transmission waveguide **25** as illustrated are formed as a single unit construction from a material suitable for transmission of ultrasonic energy. Examples of such materials include Ti6Al4V (an alloy of Titanium including Aluminum and Vanadium), Aluminum,

Stainless Steel, or other suitable materials. Alternately, the blade **22** may be separable (and of differing composition) from the ultrasonic transmission waveguide **25**, and coupled by, for example, a stud, weld, glue, quick connect, or other suitable known methods. The length of the ultrasonic transmission waveguide **25** may be substantially equal to an integral number of one-half wavelengths ($n\lambda/2$), for example. The ultrasonic transmission waveguide **25** may be preferably fabricated from a solid core shaft constructed out of material suitable to propagate ultrasonic energy efficiently, such as the titanium alloy discussed above (i.e., Ti6Al4V) or any suitable aluminum alloy, or other alloys, for example.

The switch assembly **128** comprises a toggle switch **130** that is pivotally movable about pivot **131**. The toggle switch **130** may be implemented as a single component with a central pivot **131** located within inside the handle assembly **112** to eliminate the possibility of simultaneous activation. In one example embodiment, the toggle switch **130** comprises a first projecting knob **130a** (top) and a second projecting knob **130b** (bottom) to set the power setting of the ultrasonic transducer **116** between a minimum power level (e.g., MIN) and a maximum power level (e.g., MAX). In another embodiment, the rocker switch may pivot about pivot **131** between a standard setting and a special setting.

FIG. **12** is a cross-sectional side view of the surgical instrument **110** of FIG. **11** coupled to a handle assembly **112** with a movable sheath **24** in a first position. As shown in FIG. **12**, the trigger **132** is located in a first position such that the sheath **24** is in a distally extended position in direction **170b** to define a gap **23** between the distal end **24d** of the sheath **24** and the ultrasonic blade **22**. In this configuration, target tissue can be positioned in the gap **23** for further therapeutic or sub-therapeutic treatment. Once the target tissue is positioned in the gap **23**, the trigger **132** can be squeezed to clamp or grasp the target tissue between the distal end **24d** of the sheath **24** and the distal end of the ultrasonic blade **22**.

FIG. **13** is a cross-sectional side view of the surgical instrument **110** of FIG. **12** with a movable sheath **24** in a second position. As shown in FIG. **13**, the trigger **132** is located in a second position such that the sheath **24** is in a proximally extended position in direction **170a** to eliminate the gap **23** between the distal end **24d** of the sheath **24** and the ultrasonic blade **22**. In this configuration, target tissue positioned in the gap **23** is grasped for further therapeutic or sub-therapeutic treatment. Once the target tissue is positioned in the gap **23**, the trigger **132** is squeezed to clamp or grasp the target tissue between the distal end **24d** of the sheath **24** and the distal end of the ultrasonic blade **22**.

FIG. **14** is a cross-sectional side view of a surgical instrument **200** having an ultrasonic blade **22** positioned within a movable sheath **24**, a suction tube **206**, and a pad **204** positioned on a distal end of the movable sheath **24**, according to one embodiment. The suction tube **206** is fluidically coupled to a vacuum source and serves to suction target tissue **202** debris after the ultrasonic blade **22** cuts the target tissue **202**. A pad **204** is positioned on a distal end **24d** of the sheath **24** facing the surface **28** of the ultrasonic blade **22**. The target tissue **202** is grasped between the pad **204** and the surface **28** of the ultrasonic blade **22**. The pad **204** can be a non-stick polymeric pad made of Teflon, for example, and provides a surface upon which pressure can be applied while the ultrasonic blade **22** is activated to achieve better performance when cutting and coagulating the target tissue **202**.

FIG. **15** is a side view of a surgical instrument **300** comprising an opening **306** defined between the blade **312**/ultrasonic waveguide **315** and the outer tube **314**, where in one embodiment the opening **306** is configured to couple to a suction and/or irrigation source at the handle end **304**. FIG. **16** is a sectional view taken along section line **16-16** of the distal end of the instrument shown in FIG. **15**, according to one embodiment. FIG. **16** illustrates a section portion of the ultrasonic waveguide **315** (or blade **312**) located within the outer sheath **314** defining an opening **306** for the tissue **323** to travel through. FIGS. **15** and **16** show the blade **312**/waveguide **315** with a linear longitudinal cavity **306** from a gap **313** for tissue **323** engagement distally to the proximally located suction/irrigation in order to remove the transected tissue **323**. The illustrated embodiment comprises a "half moon" profile located above the blade **312**/waveguide **315** at 12 o'clock and fluidically coupled to a suction and/or irrigation source at the handle end **304**.

The illustration in FIG. **15** shows a distal end **302** and a proximal "handle" end of the **304** instrument **300**. In the illustrated embodiment, the distal end **302** of the instrument **300** includes an ultrasonic blade **312** positioned within an elongate sheath **314**. The sheath **314** includes a distal end **314d** and a proximal end (not shown) that is configured to couple to a handle that is configured to be grasped, manipulated and actuated by a clinician. The sheath **314** is movable relative to the ultrasonic blade **312** between a first proximal position in which the sheath **314** is positioned over a proximal portion of the blade **312** and a second position in which the sheath **314** moves distally in direction **317b** such that tissue **323** positioned in the gap **313** between the blade **312** and the distal end **314d** of the sheath **314** is dissected therebetween. Once the tissue **313** is dissected, the sheath **314** is retracted proximally in direction **317a**.

The opening **306** is defined between the blade **312**/ultrasonic waveguide **315** and is configured to receive the tissue **323** after dissection. The blade **312** and the ultrasonic waveguide **315** are configured such that the opening **306** (e.g., "trough" or "channel") defined between the blade **312**/waveguide **315** and the sheath **314** is configured for the tissue **323** to travel from the distal end **302** to the proximal end **304** of the instrument **300**. The proximal end **304** comprises a first seal disposed at the handle to encompass the outer sheath **314** with an outer tube **324**, and a second seal between the waveguide **315** and the outer sheath **314** such that the tissue **323** will travel through the opening **306** in the waveguide **315** and out of an opening **318** defined in the outer sheath **314**.

The first seal comprises first and second mechanical gaskets **308**, **310** and the second seal comprises a third mechanical gasket **316**. The mechanical gaskets **308**, **310**, **316** may be resilient O-ring types of seals, also known as a packing, or a toric joint, and may be any mechanical gasket in the shape of a torus or loop of elastomer with a round cross-section, designed to be seated in a groove and compressed during assembly between two or more parts, creating a seal at the interface. A tube **322** is located between the first seal and is in fluid communication with the opening **318** defined in the outer sheath **314**. Accordingly, the opening **306** is in fluid communication with the tube **322** such when a suction **320** is applied by a vacuum source, the dissected tissue **323** is sucked through the opening **306** and out of the tube **322** to the vacuum source.

The vacuum source is in fluid is provided in most modern hospitals and is available from wall outlets located throughout the building. Other sources of vacuum may include electric pumps, gas-powered venturi suction units, and

mechanical devices, such as hand pumps and wound drainage systems, for example. The major source of vacuum in hospitals is a pump in the basement of the building. By emptying a receiver or reservoir tank, the pump creates a vacuum that can be delivered through connecting pipes to wall outlets in patient care areas and hospital departments. When the vacuum pressure falls to a predetermined level, a switch engages the pump to restore vacuum pressure; when the vacuum builds back up, the switch disengages and no further vacuum is created. Generally the pump is set to begin operation when the vacuum level of the system drops to 19 inHg (483 mmHg) and ceases operation when the level reaches 25 inHg (635 mmHg). In most hospitals, a duplex pump system is used for safety; each pump is capable of maintaining minimum vacuum levels. A duplex system allows for periodic shut-down of each pump for service and repairs and also provides a backup source for negative pressure, should one of the pumps fail to operate properly.

Although the various embodiments of the devices have been described herein in connection with certain disclosed embodiments, many modifications and variations to those embodiments may be implemented. Also, where materials are disclosed for certain components, other materials may be used. Furthermore, according to various embodiments, a single component may be replaced by multiple components, and multiple components may be replaced by a single component, to perform a given function or functions. The foregoing description and following claims are intended to cover all such modification and variations.

The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

Preferably, the invention described herein will be processed before surgery. First, a new or used instrument is obtained and if necessary cleaned. The instrument can then be sterilized. In one sterilization technique, the instrument is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and instrument are then placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation kills bacteria on the instrument and in the container. The sterilized instrument can then be stored in the sterile container. The sealed container keeps the instrument sterile until it is opened in the medical facility.

While this invention has been described as having exemplary designs, the present invention may be further modified within the spirit and scope of the disclosure. This application is therefore intended to cover any variations, uses, or adaptations of the invention using its general principles. Further, this application is intended to cover such departures from the present disclosure as come within known or customary practice in the art to which this invention pertains.

Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

What is claimed is:

1. An apparatus for dissection and coagulation of tissue, comprising:

a proximal portion;

an elongate sheath having a proximal end and distal end, the distal end of the elongate sheath comprising a substantially flat surface proximal of the distal end to form an anvil; and

an ultrasonic blade configured to dissect and sea tissue based on vibrational motion and being positioned within the elongate sheath, wherein the elongate sheath is configured for gross axial motion relative to the proximal portion and the ultrasonic blade without gross axial motion of the ultrasonic blade, and wherein the gross axial motion comprises movement between;

a first position in which the ultrasonic blade is positioned a first distance from the distal end of the elongate sheath, and

a second position in which the ultrasonic blade is positioned a second distance from the distal end of the elongate sheath when the elongate sheath moves proximally towards the distal end of the ultrasonic blade such that tissue can be dissected therebetween, wherein the second distance is less than the first distance.

2. The apparatus of claim 1, wherein the distal end of the ultrasonic blade is sized and shaped to correspond to the size and shape of the substantially flat surface of the distal end of the elongate sheath forming the anvil.

3. The apparatus of claim 2, wherein the shape of the distal end of the ultrasonic blade and the distal end of the elongate sheath create a cavity at the location of the dissected tissue.

4. The apparatus of claim 1, wherein a proximal end of the ultrasonic blade communicates with an excitation mechanism to deliver energy to the distal end of the ultrasonic blade.

5. The apparatus of claim 1, wherein a proximal end of the ultrasonic blade is configured to couple to an actuator to move the ultrasonic blade between the first and second positions.

6. The apparatus of claim 1, further comprising a suction mechanism in the form of an elongate hollow tube positioned within the elongate sheath and extending to the distal end thereof such that a distal end of the suction mechanism is configured to remove tissue dissected by the ultrasonic blade and the elongate sheath.

7. The apparatus of claim 6, wherein the suction mechanism is configured to irrigate an area located substantially around the tissue being dissected and removed.

21

8. The apparatus of claim **6**, wherein the distal end of the suction mechanism is positioned between the distal end of the elongate sheath and the distal end of the ultrasonic blade.

* * * * *

22

专利名称(译)	用于解剖和凝结组织的装置和方法		
公开(公告)号	US10034684	公开(公告)日	2018-07-31
申请号	US14/739792	申请日	2015-06-15
[标]申请(专利权)人(译)	爱惜康内镜外科，LLC		
申请(专利权)人(译)	爱惜康内镜外科，LLC		
当前申请(专利权)人(译)	ETHICON LLC		
[标]发明人	WEISENBURGH II WILLIAM B JOHNSON GREGORY W KIMBALL CORY G		
发明人	WEISENBURGH, II, WILLIAM B. JOHNSON, GREGORY W. KIMBALL, CORY G.		
IPC分类号	A61B17/32 A61N7/00 A61B18/00 A61B17/00 A61B17/24		
CPC分类号	A61B17/320068 A61B17/320092 A61N7/00 A61B17/24 A61B2017/00477 A61B2017/320078 A61B2017/320084 A61B2018/00589 A61B2018/00607 A61B2018/00994 A61B2217/007 A61B2017/00991 A61B18/1206 A61B18/1482 A61B2017/320069 A61B2017/32007 A61B2017/320089 A61B2017/320093 A61B2017/320094 A61B2017/320095 A61B2017/320071		
其他公开文献	US20160361084A1		
外部链接	Espacenet		

摘要(译)

提供了一种用于切割和凝固组织的手术器械，其包括细长护套和超声刀。在一个实施例中，超声刀定位在护套内，使得护套相对于刀片的运动导致其间的组织的解剖和/或凝固。在另一个实施例中，超声刀定位在护套内，使得刀片相对于护套的运动导致其间的组织解剖和/或凝固。刀片和鞘的远端的尺寸和形状决定了被切割和/或从身体移除的组织的尺寸和形状。

