



US009962182B2

(12) **United States Patent**
Dietz et al.

(10) **Patent No.:** **US 9,962,182 B2**
(45) **Date of Patent:** **May 8, 2018**

(54) **ULTRASONIC SURGICAL INSTRUMENTS
WITH MOVING CUTTING IMPLEMENT**

(71) Applicant: **Ethicon Endo-Surgery, Inc.**,
Cincinnati, OH (US)

(72) Inventors: **Timothy G. Dietz**, Wayne, PA (US);
Gregory W. Johnson, Milford, OH
(US); **Sean P. Conlon**, Loveland, OH
(US); **Daniel J. Mumaw**, Liberty
Township, OH (US); **Jerome R.**
Morgan, Cincinnati, OH (US); **William**
D. Dannaher, Cincinnati, OH (US);
Omar J. Vakharia, Cincinnati, OH
(US); **Richard W. Timm**, Cincinnati,
OH (US); **Matthew C. Miller**,
Cincinnati, OH (US); **Galen C.**
Robertson, Apex, NC (US)

(73) Assignee: **Ethicon LLC**, Guaynabo, PR (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 264 days.

(21) Appl. No.: **14/590,574**

(22) Filed: **Jan. 6, 2015**

(65) **Prior Publication Data**

US 2015/0119916 A1 Apr. 30, 2015

Related U.S. Application Data

(62) Division of application No. 12/703,893, filed on Feb.
11, 2010, now Pat. No. 8,961,547.

(51) **Int. Cl.**

A61B 17/32 (2006.01)
A61B 17/22 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 17/320068** (2013.01); **A61B**
17/22004 (2013.01); **A61B 17/3207** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC **A61B 17/320783**; **A61B 17/22004**; **A61B**
17/320068; **A61B 17/3207**;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

969,528 A 9/1910 Disbrow
1,570,025 A 1/1926 Young

(Continued)

FOREIGN PATENT DOCUMENTS

AU 2003241752 A1 9/2003
CA 2535467 A1 4/1993

(Continued)

OTHER PUBLICATIONS

Technology Overview, printed from www.harmonicscalpel.com,
Internet site, website accessed on Jun. 13, 2007, (3 pages).



(Continued)

Primary Examiner — Victor Nguyen

(57) **ABSTRACT**

In various embodiments, a surgical instrument for operation
in an aqueous environment is provided. In at least one
embodiment, the surgical instrument may include a hollow
sheath and a blade disposed at least partially within the
sheath. Coupled to the blade may be at least one ultrasonic
transducer, which, in turn, may be coupled to a drive system.
The drive system may be configured to deliver gross axial
motions to the blade such that the blade translates with
respect to the hollow sheath when the drive system is
activated. Accordingly, tissue may be cut by the blade with
gross axial movement of the blade and/or ultrasonic vibra-
tional motion provided by the ultrasonic transducer(s). In
alternative embodiments, the blade may be rotated axially
instead of translated with respect to the hollow sheath.

8 Claims, 24 Drawing Sheets

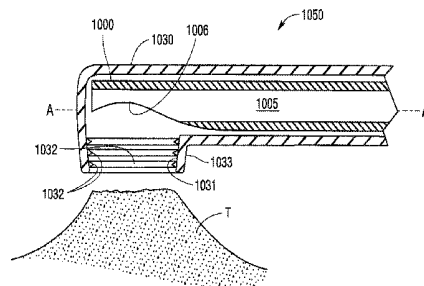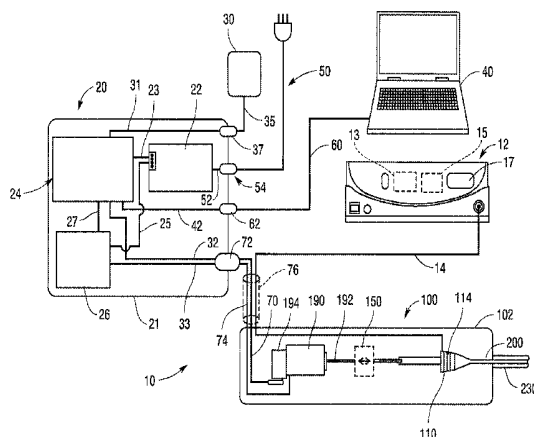

- (51) **Int. Cl.**
A61B 17/3207 (2006.01)
A61B 17/00 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61B 17/320783* (2013.01); *A61B 17/320092* (2013.01); *A61B 2017/00296* (2013.01); *A61B 2017/00778* (2013.01)
- (58) **Field of Classification Search**
 CPC A61B 2017/22011; A61B 17/32; A61B 17/22; A61B 17/32002
 See application file for complete search history.
- (56) **References Cited**
 U.S. PATENT DOCUMENTS
- | | | | | | |
|---------------|---------|-------------------------------------|-------------|---------|------------------------|
| 1,813,902 A | 7/1931 | Bovie | 4,494,759 A | 1/1985 | Kieffer |
| 2,188,497 A | 1/1940 | Calva | 4,504,264 A | 3/1985 | Kelman |
| 2,425,245 A | 8/1947 | Johnson | 4,512,344 A | 4/1985 | Barber |
| 2,442,966 A | 6/1948 | Wallace | 4,526,571 A | 7/1985 | Wuchinich |
| 2,597,564 A | 5/1952 | Bugg | 4,541,638 A | 9/1985 | Ogawa et al. |
| 2,704,333 A | 3/1955 | Calosi et al. | 4,545,374 A | 10/1985 | Jacobson |
| 2,736,960 A | 3/1956 | Armstrong | 4,574,615 A | 3/1986 | Bower et al. |
| 2,748,967 A | 6/1956 | Roach | 4,617,927 A | 10/1986 | Manes |
| 2,845,072 A | 7/1958 | Shafer | 4,633,119 A | 12/1986 | Thompson |
| 2,849,788 A | 9/1958 | Creek | 4,634,420 A | 1/1987 | Spinosa et al. |
| 2,874,470 A | 2/1959 | Richards | 4,640,279 A | 2/1987 | Beard |
| 2,990,616 A | 7/1961 | Balamuth et al. | 4,641,053 A | 2/1987 | Takeda |
| RE25,033 E | 8/1961 | Balamuth et al. | 4,646,738 A | 3/1987 | Trott |
| 3,015,961 A | 1/1962 | Roney | 4,646,756 A | 3/1987 | Watmough et al. |
| 3,033,407 A | 5/1962 | Alfons | 4,649,919 A | 3/1987 | Thimsen et al. |
| 3,053,124 A | 9/1962 | Balamuth et al. | 4,662,068 A | 5/1987 | Polonsky |
| 3,082,805 A | 3/1963 | Royce | 4,674,502 A | 6/1987 | Imonti |
| 3,322,403 A * | 5/1967 | Murphy B01F 13/002
366/247 | 4,708,127 A | 11/1987 | Abdelghani |
| 3,432,691 A | 3/1969 | Shoh | 4,712,722 A | 12/1987 | Hood et al. |
| 3,433,226 A | 3/1969 | Boyd | 4,808,154 A | 2/1989 | Freeman |
| 3,489,930 A | 1/1970 | Shoh | 4,819,635 A | 4/1989 | Shapiro |
| 3,513,848 A | 5/1970 | Winston et al. | 4,827,911 A | 5/1989 | Broadwin et al. |
| 3,514,856 A | 6/1970 | Camp et al. | 4,832,683 A | 5/1989 | Idemoto et al. |
| 3,526,219 A | 9/1970 | Balamuth | 4,836,186 A | 6/1989 | Scholz |
| 3,554,198 A | 1/1971 | Tatoian et al. | 4,838,853 A | 6/1989 | Parisi |
| 3,606,682 A | 9/1971 | Camp et al. | 4,844,064 A | 7/1989 | Thimsen et al. |
| 3,614,484 A | 10/1971 | Shoh | 4,850,354 A | 7/1989 | McGurk-Burleson et al. |
| 3,616,375 A | 10/1971 | Inoue | 4,852,578 A | 8/1989 | Companion et al. |
| 3,629,726 A | 12/1971 | Popescu | 4,862,890 A | 9/1989 | Stasz et al. |
| 3,636,943 A | 1/1972 | Balamuth | 4,865,159 A | 9/1989 | Jamison |
| 3,668,486 A | 6/1972 | Silver | 4,867,157 A | 9/1989 | McGurk-Burleson et al. |
| 3,702,948 A | 11/1972 | Balamuth | 4,878,493 A | 11/1989 | Pasternak et al. |
| 3,776,238 A | 12/1973 | Peyman et al. | 4,881,550 A | 11/1989 | Kothe |
| 3,805,787 A * | 4/1974 | Banko A61F 9/00745
601/2 | 4,896,009 A | 1/1990 | Pawlowski |
| 3,809,977 A | 5/1974 | Balamuth et al. | 4,903,696 A | 2/1990 | Stasz et al. |
| 3,830,098 A | 8/1974 | Antonevich | 4,915,643 A | 4/1990 | Samejima et al. |
| 3,854,737 A | 12/1974 | Gilliam, Sr. | 4,922,902 A | 5/1990 | Wuchinich et al. |
| 3,862,630 A | 1/1975 | Balamuth | 4,965,532 A | 10/1990 | Sakurai |
| 3,875,945 A | 4/1975 | Friedman | 4,979,952 A | 12/1990 | Kubota et al. |
| 3,885,438 A | 5/1975 | Harris, Sr. et al. | 4,981,756 A | 1/1991 | Rhandhawa |
| 3,900,823 A | 8/1975 | Sokal et al. | 5,013,956 A | 5/1991 | Kurozumi et al. |
| 3,918,442 A | 11/1975 | Nikolaev et al. | 5,015,227 A | 5/1991 | Broadwin et al. |
| 3,924,335 A | 12/1975 | Balamuth et al. | 5,026,370 A | 6/1991 | Lottick |
| 3,946,738 A | 3/1976 | Newton et al. | 5,026,387 A | 6/1991 | Thomas |
| 3,955,859 A | 5/1976 | Stella et al. | 5,035,695 A | 7/1991 | Weber, Jr. et al. |
| 3,956,826 A | 5/1976 | Perdreux, Jr. | 5,042,707 A | 8/1991 | Taheri |
| 4,012,647 A | 3/1977 | Balamuth et al. | 5,084,052 A | 1/1992 | Jacobs |
| 4,074,719 A | 2/1978 | Semm | 5,105,117 A | 4/1992 | Yamaguchi |
| 4,156,187 A | 5/1979 | Murry et al. | 5,109,819 A | 5/1992 | Custer et al. |
| 4,167,944 A | 9/1979 | Banko | 5,112,300 A | 5/1992 | Ureche |
| 4,188,927 A | 2/1980 | Harris | 5,123,903 A | 6/1992 | Quaid et al. |
| 4,200,106 A | 4/1980 | Douvas et al. | 5,126,618 A | 6/1992 | Takahashi et al. |
| 4,203,444 A | 5/1980 | Bonnell et al. | D327,872 S | 7/1992 | McMills et al. |
| 4,300,083 A | 11/1981 | Heiges | 5,152,762 A | 10/1992 | McElhenney |
| 4,302,728 A | 11/1981 | Nakamura | 5,162,044 A | 11/1992 | Gahn et al. |
| 4,306,570 A | 12/1981 | Matthews | 5,163,421 A | 11/1992 | Bernstein et al. |
| 4,445,063 A | 4/1984 | Smith | 5,163,537 A | 11/1992 | Radev |
| 4,491,132 A | 1/1985 | Aikins | 5,167,725 A | 12/1992 | Clark et al. |
| | | | 5,172,344 A | 12/1992 | Ehrlich |
| | | | 5,174,276 A | 12/1992 | Crockard |
| | | | D332,660 S | 1/1993 | Rawson et al. |
| | | | 5,176,677 A | 1/1993 | Wuchinich |
| | | | 5,176,695 A | 1/1993 | Dulebohn |
| | | | 5,184,605 A | 2/1993 | Grezeszykowski |
| | | | 5,188,102 A | 2/1993 | Idemoto et al. |
| | | | D334,173 S | 3/1993 | Liu et al. |
| | | | 5,209,719 A | 5/1993 | Baruch et al. |
| | | | 5,213,569 A | 5/1993 | Davis |
| | | | 5,214,339 A | 5/1993 | Naito |
| | | | 5,218,529 A | 6/1993 | Meyer et al. |
| | | | 5,221,282 A | 6/1993 | Wuchinich |
| | | | 5,222,937 A | 6/1993 | Kagawa |
| | | | 5,226,909 A | 7/1993 | Evans et al. |
| | | | 5,226,910 A | 7/1993 | Kajiyama et al. |
| | | | 5,241,236 A | 8/1993 | Sasaki et al. |
| | | | 5,241,968 A | 9/1993 | Slater |
| | | | 5,242,460 A | 9/1993 | Klein et al. |
| | | | 5,254,129 A | 10/1993 | Alexander |
| | | | 5,257,988 A | 11/1993 | L'Esperance, Jr. |

(56)

References Cited

U.S. PATENT DOCUMENTS

5,261,922 A	11/1993	Hood	5,618,304 A	4/1997	Hart et al.
5,263,957 A	11/1993	Davison	5,618,492 A	4/1997	Auten et al.
5,264,925 A	11/1993	Shipp et al.	5,620,447 A	4/1997	Smith et al.
5,275,166 A	1/1994	Vaitekunas et al.	5,626,587 A	5/1997	Bishop et al.
5,275,607 A	1/1994	Lo et al.	5,626,595 A	5/1997	Sklar et al.
5,275,609 A	1/1994	Pingleton et al.	5,628,760 A	5/1997	Knoepfler
5,282,800 A	2/1994	Foshee et al.	5,630,420 A	5/1997	Vaitekunas
5,282,817 A	2/1994	Hoogetboom et al.	5,632,717 A	5/1997	Yoon
5,285,795 A	2/1994	Ryan et al.	5,640,741 A	6/1997	Yano
5,300,068 A	4/1994	Rosar et al.	D381,077 S	7/1997	Hunt
5,304,115 A	4/1994	Pflueger et al.	5,649,937 A	7/1997	Bitto
D347,474 S	5/1994	Olson	5,651,780 A	7/1997	Jackson et al.
5,307,976 A	5/1994	Olson et al.	5,653,713 A	8/1997	Michelson
5,312,023 A	5/1994	Green et al.	5,662,662 A	9/1997	Bishop et al.
5,312,425 A	5/1994	Evans et al.	5,669,922 A	9/1997	Hood
5,322,055 A	6/1994	Davison et al.	5,674,235 A	10/1997	Parisi
5,324,299 A	6/1994	Davison et al.	5,678,568 A	10/1997	Uchikubo et al.
5,326,013 A	7/1994	Green et al.	5,690,269 A	11/1997	Bolano et al.
5,326,342 A	7/1994	Pflueger et al.	5,694,936 A	12/1997	Fujimoto et al.
5,344,420 A	9/1994	Hilal et al.	5,695,510 A	12/1997	Hood
5,345,937 A	9/1994	Middleman et al.	5,700,261 A	12/1997	Brinkerhoff
5,346,502 A	9/1994	Estabrook et al.	5,704,534 A	1/1998	Huitema et al.
5,353,474 A	10/1994	Good et al.	5,709,680 A	1/1998	Yates et al.
5,357,164 A	10/1994	Imabayashi et al.	5,711,472 A	1/1998	Bryan
5,357,423 A	10/1994	Weaver et al.	5,713,896 A	2/1998	Nardella
5,359,994 A	11/1994	Krauter et al.	5,715,817 A	2/1998	Stevens-Wright et al.
5,366,466 A	11/1994	Christian et al.	5,717,306 A	2/1998	Shipp
5,368,557 A	11/1994	Nita et al.	5,728,130 A	3/1998	Ishikawa et al.
5,370,645 A	12/1994	Klicek et al.	5,730,752 A	3/1998	Alden et al.
5,371,429 A	12/1994	Manna	5,733,074 A	3/1998	Stöck et al.
5,374,813 A	12/1994	Shipp	5,741,226 A	4/1998	Strukel et al.
D354,564 S	1/1995	Medema	5,766,164 A	6/1998	Mueller et al.
5,381,067 A	1/1995	Greenstein et al.	5,772,659 A	6/1998	Becker et al.
5,387,215 A	2/1995	Fisher	5,792,135 A	8/1998	Madhani et al.
5,389,098 A	2/1995	Tsuruta et al.	5,792,138 A	8/1998	Shipp
5,394,187 A	2/1995	Shipp	5,792,165 A	8/1998	Klieman et al.
5,396,266 A	3/1995	Brimhall	5,797,959 A	8/1998	Castro et al.
5,403,312 A	4/1995	Yates et al.	5,805,140 A	9/1998	Rosenberg et al.
5,403,334 A	4/1995	Evans et al.	5,808,396 A	9/1998	Boukhny
5,408,268 A	4/1995	Shipp	5,810,859 A	9/1998	DiMatteo et al.
D358,887 S	5/1995	Feinberg	5,817,084 A	10/1998	Jensen
5,411,481 A	5/1995	Allen et al.	5,817,119 A	10/1998	Klieman et al.
5,419,761 A	5/1995	Narayanan et al.	5,823,197 A	10/1998	Edwards
5,421,829 A	6/1995	Olichney et al.	5,827,323 A	10/1998	Klieman et al.
5,423,844 A	6/1995	Miller	5,828,160 A	10/1998	Sugishita
5,438,997 A	8/1995	Sieben et al.	5,833,696 A	11/1998	Whitfield et al.
5,445,639 A	8/1995	Kuslich et al.	5,836,897 A	11/1998	Sakurai et al.
5,449,370 A	9/1995	Vaitekunas	5,836,957 A	11/1998	Schulz et al.
5,451,220 A	9/1995	Ciervo	5,843,109 A	12/1998	Mehta et al.
5,456,684 A	10/1995	Schmidt et al.	5,851,212 A	12/1998	Zirps et al.
5,471,988 A	12/1995	Fujio et al.	5,858,018 A	1/1999	Shipp et al.
5,472,443 A	12/1995	Cordis et al.	5,865,361 A	2/1999	Milliman et al.
5,478,003 A	12/1995	Green et al.	5,873,873 A	2/1999	Smith et al.
5,483,501 A	1/1996	Park et al.	5,873,882 A	2/1999	Straub et al.
5,486,162 A	1/1996	Brumbach	5,878,193 A	3/1999	Wang et al.
5,490,860 A	2/1996	Middle et al.	5,879,364 A	3/1999	Bromfield et al.
5,500,216 A	3/1996	Julian et al.	5,883,615 A	3/1999	Fago et al.
5,501,654 A	3/1996	Failla et al.	5,893,835 A	4/1999	Witt et al.
5,505,693 A	4/1996	Mackool	5,897,523 A	4/1999	Wright et al.
5,507,738 A	4/1996	Ciervo	5,897,569 A	4/1999	Kellogg et al.
5,527,331 A	6/1996	Kresch et al.	5,903,607 A	5/1999	Tailliet
5,540,693 A	7/1996	Fisher	5,904,681 A	5/1999	West, Jr.
5,553,675 A	9/1996	Pitzen et al.	5,906,627 A	5/1999	Spaulding
5,558,671 A	9/1996	Yates	5,906,628 A	5/1999	Miyawaki et al.
5,562,609 A	10/1996	Brumbach	5,911,699 A	6/1999	Anis et al.
5,562,610 A	10/1996	Brumbach	5,916,229 A	6/1999	Evans
5,562,659 A	10/1996	Morris	5,929,846 A	7/1999	Rosenberg et al.
5,573,424 A	11/1996	Poppe	5,935,143 A	8/1999	Hood
5,577,654 A	11/1996	Bishop	5,935,144 A	8/1999	Estabrook
5,591,187 A	1/1997	Dekel	5,938,633 A	8/1999	Beaupre
5,593,414 A	1/1997	Shipp et al.	5,944,718 A	8/1999	Austin et al.
5,601,601 A	2/1997	Tal et al.	5,944,737 A	8/1999	Tsonton et al.
5,603,773 A	2/1997	Campbell	5,947,984 A	9/1999	Whipple
5,607,436 A	3/1997	Pratt et al.	5,954,736 A	9/1999	Bishop et al.
5,609,573 A	3/1997	Sandock	5,954,746 A	9/1999	Holthaus et al.
			5,957,882 A	9/1999	Nita et al.
			5,957,943 A	9/1999	Vaitekunas
			5,968,007 A	10/1999	Simon et al.
			5,968,060 A	10/1999	Kellogg

(56)

References Cited

U.S. PATENT DOCUMENTS

5,974,342 A	10/1999	Petrofsky	6,257,241 B1	7/2001	Wampler
D416,089 S	11/1999	Barton et al.	6,258,034 B1	7/2001	Hanafy
5,980,510 A	11/1999	Tsonton et al.	6,267,761 B1	7/2001	Ryan
5,980,546 A	11/1999	Hood	6,270,831 B2	8/2001	Kumar et al.
5,989,274 A	11/1999	Davison et al.	6,273,852 B1	8/2001	Lehe et al.
5,989,275 A	11/1999	Estabrook et al.	6,274,963 B1	8/2001	Estabrook et al.
5,993,465 A	11/1999	Shipp et al.	6,277,115 B1	8/2001	Saadat
5,993,972 A	11/1999	Reich et al.	6,278,218 B1	8/2001	Madan et al.
5,994,855 A	11/1999	Lundell et al.	6,280,407 B1	8/2001	Manna et al.
6,024,741 A	2/2000	Williamson, IV et al.	6,283,981 B1	9/2001	Beaupre
6,024,750 A	2/2000	Mastri et al.	6,287,344 B1	9/2001	Wampler et al.
6,027,515 A	2/2000	Cimino	6,290,575 B1	9/2001	Shipp
6,031,526 A	2/2000	Shipp	6,299,591 B1	10/2001	Banko
6,033,375 A	3/2000	Brumbach	6,306,131 B1	10/2001	Hareyama
6,033,399 A	3/2000	Gines	6,306,157 B1	10/2001	Shchervinsky
6,036,667 A	3/2000	Manna et al.	6,309,400 B2	10/2001	Beaupre
6,036,707 A	3/2000	Spaulding	6,311,783 B1	11/2001	Harpell
6,048,224 A	4/2000	Kay	6,319,221 B1	11/2001	Savage et al.
6,050,943 A	4/2000	Slayton et al.	6,325,795 B1	12/2001	Lindemann et al.
6,051,010 A	4/2000	DiMatteo et al.	6,325,799 B1	12/2001	Goble
6,056,735 A	5/2000	Okada et al.	6,325,811 B1	12/2001	Messerly
6,063,098 A	5/2000	Houser et al.	6,328,751 B1	12/2001	Beaupre
6,066,132 A	5/2000	Chen et al.	6,332,891 B1	12/2001	Himes
6,066,151 A	5/2000	Miyawaki et al.	6,338,657 B1	1/2002	Harper et al.
6,068,627 A	5/2000	Orszulak et al.	6,340,352 B1	1/2002	Okada et al.
6,068,647 A	5/2000	Witt et al.	6,350,269 B1	2/2002	Shipp et al.
6,077,285 A	6/2000	Boukhny	6,352,532 B1	3/2002	Kramer et al.
6,083,191 A	7/2000	Rose	6,358,264 B2	3/2002	Banko
6,086,584 A	7/2000	Miller	6,364,888 B1	4/2002	Niemeyer et al.
6,090,120 A	7/2000	Wright et al.	6,379,320 B1	4/2002	Lafon et al.
6,096,033 A	8/2000	Tu et al.	D457,958 S	5/2002	Dycus et al.
6,099,542 A	8/2000	Cohn et al.	6,383,194 B1	5/2002	Pothula
6,109,500 A	8/2000	Alli et al.	6,384,690 B1	5/2002	Wilhelmsson et al.
6,110,127 A	8/2000	Suzuki	6,387,109 B1	5/2002	Davison et al.
6,113,594 A	9/2000	Savage	6,388,657 B1	5/2002	Natoli
6,117,152 A	9/2000	Huitema	6,391,042 B1	5/2002	Cimino
6,126,629 A	10/2000	Perkins	6,398,779 B1	6/2002	Buyse et al.
6,129,735 A	10/2000	Okada et al.	6,402,743 B1	6/2002	Orszulak et al.
6,129,740 A	10/2000	Michelson	6,402,748 B1	6/2002	Schoenman et al.
6,132,368 A	10/2000	Cooper	6,405,733 B1	6/2002	Fogarty et al.
6,132,427 A	10/2000	Jones et al.	6,416,486 B1	7/2002	Wampler
6,132,448 A	10/2000	Perez et al.	6,423,073 B2	7/2002	Bowman
6,139,320 A	10/2000	Hahn	6,423,082 B1	7/2002	Houser et al.
6,139,561 A	10/2000	Shibata et al.	6,425,906 B1	7/2002	Young et al.
6,142,615 A	11/2000	Qiu et al.	6,428,538 B1	8/2002	Blewett et al.
6,142,994 A	11/2000	Swanson et al.	6,428,539 B1	8/2002	Baxter et al.
6,147,560 A	11/2000	Erhage et al.	6,432,118 B1	8/2002	Messerly
6,152,902 A	11/2000	Christian et al.	6,436,114 B1	8/2002	Novak et al.
6,154,198 A	11/2000	Rosenberg	6,436,115 B1	8/2002	Beaupre
6,159,160 A	12/2000	Hsei et al.	6,440,062 B1	8/2002	Ouchi
6,159,175 A	12/2000	Strukel et al.	6,443,968 B1	9/2002	Holthaus et al.
6,162,194 A	12/2000	Shipp	6,443,969 B1	9/2002	Novak et al.
6,165,150 A	12/2000	Banko	6,449,006 B1	9/2002	Shipp
6,174,310 B1	1/2001	Kirwan, Jr.	6,454,781 B1	9/2002	Witt et al.
6,179,853 B1	1/2001	Sachse et al.	6,454,782 B1	9/2002	Schwemberger
6,183,426 B1	2/2001	Akisada et al.	6,458,142 B1	10/2002	Faller et al.
6,193,709 B1	2/2001	Miyawaki et al.	6,475,215 B1	11/2002	Tanrisever
6,204,592 B1	3/2001	Hur	6,480,796 B2	11/2002	Wiener
6,205,855 B1	3/2001	Pfeiffer	6,485,490 B2	11/2002	Wampler et al.
6,206,844 B1	3/2001	Reichel et al.	6,491,701 B2	12/2002	Tierney et al.
6,210,337 B1	4/2001	Dunham et al.	6,491,708 B2	12/2002	Madan et al.
6,210,402 B1	4/2001	Olsen et al.	6,497,715 B2	12/2002	Satou
6,210,403 B1	4/2001	Klicek	6,500,176 B1	12/2002	Truckai et al.
6,214,023 B1	4/2001	Whipple et al.	6,500,188 B2	12/2002	Harper et al.
6,228,080 B1	5/2001	Gines	6,500,312 B2	12/2002	Wedekamp
6,231,565 B1	5/2001	Tovey et al.	6,506,208 B2	1/2003	Hunt et al.
6,233,476 B1	5/2001	Strommer et al.	6,511,478 B1	1/2003	Burnside et al.
6,238,366 B1	5/2001	Savage et al.	6,511,493 B1	1/2003	Moutafis et al.
6,245,065 B1	6/2001	Panescu et al.	6,514,267 B2	2/2003	Jewett
6,251,110 B1	6/2001	Wampler	6,524,251 B2	2/2003	Rabiner et al.
6,252,110 B1	6/2001	Uemura et al.	6,524,316 B1	2/2003	Nicholson et al.
D444,365 S	7/2001	Bass et al.	6,527,736 B1	3/2003	Attinger et al.
D445,092 S	7/2001	Lee	6,533,784 B2	3/2003	Truckai et al.
D445,764 S	7/2001	Lee	6,537,272 B2	3/2003	Christopherson et al.
6,254,623 B1	7/2001	Haibel, Jr. et al.	6,537,291 B2	3/2003	Friedman et al.
			6,543,452 B1	4/2003	Lavigne
			6,543,456 B1	4/2003	Freeman
			6,544,260 B1	4/2003	Markel et al.
			6,558,376 B2	5/2003	Bishop

(56)

References Cited

U.S. PATENT DOCUMENTS

6,561,983 B2	5/2003	Cronin et al.	6,796,981 B2	9/2004	Wham et al.
6,562,035 B1	5/2003	Levin	D496,997 S	10/2004	Dycus et al.
6,565,558 B1	5/2003	Lindenmeier et al.	6,802,843 B2	10/2004	Truckai et al.
6,572,563 B2	6/2003	Ouchi	6,808,525 B2	10/2004	Latterell et al.
6,572,632 B2	6/2003	Zisterer et al.	6,809,508 B2	10/2004	Donofrio
6,575,969 B1	6/2003	Rittman, III et al.	6,810,281 B2	10/2004	Brock et al.
6,582,427 B1	6/2003	Goble et al.	6,827,712 B2	12/2004	Tovey et al.
6,582,451 B1	6/2003	Marucci et al.	6,828,712 B2	12/2004	Battaglin et al.
6,599,288 B2	6/2003	Maguire et al.	6,835,082 B2	12/2004	Gonnering
D477,408 S	7/2003	Bromley	6,849,073 B2	2/2005	Hoey et al.
6,588,277 B2	7/2003	Giordano et al.	6,860,878 B2	3/2005	Brock
6,589,200 B1	7/2003	Schwemberger et al.	6,863,676 B2	3/2005	Lee et al.
6,589,239 B2	7/2003	Khandkar et al.	6,869,439 B2	3/2005	White et al.
6,607,540 B1	8/2003	Shipp	6,875,220 B2	4/2005	Du et al.
6,610,059 B1	8/2003	West, Jr.	6,877,647 B2	4/2005	Green et al.
6,616,450 B2	9/2003	Mossle et al.	6,882,439 B2	4/2005	Ishijima
6,619,529 B2	9/2003	Green et al.	6,887,209 B2	5/2005	Kadziauskas et al.
6,623,500 B1	9/2003	Cook et al.	6,887,252 B1	5/2005	Okada et al.
6,623,501 B2	9/2003	Heller et al.	6,899,685 B2	5/2005	Kermode et al.
6,626,848 B2	9/2003	Neuenfeldt	6,905,497 B2	6/2005	Truckai et al.
6,626,926 B2	9/2003	Friedman et al.	6,908,472 B2	6/2005	Wiener et al.
6,629,974 B2	10/2003	Penny et al.	6,913,579 B2	7/2005	Truckai et al.
6,633,234 B2	10/2003	Wiener et al.	6,915,623 B2	7/2005	Dey et al.
6,644,532 B2	11/2003	Green et al.	6,923,804 B2	8/2005	Eggers et al.
6,651,669 B1	11/2003	Burnside	6,926,712 B2	8/2005	Phan
6,652,513 B2	11/2003	Panescu et al.	6,926,716 B2	8/2005	Baker et al.
6,652,539 B2	11/2003	Shipp et al.	6,929,602 B2	8/2005	Hirakui et al.
6,652,545 B2	11/2003	Shipp et al.	6,929,632 B2	8/2005	Nita et al.
6,656,132 B1	12/2003	Ouchi	6,929,644 B2	8/2005	Truckai et al.
6,656,177 B2	12/2003	Truckai et al.	6,933,656 B2	8/2005	Matsushita et al.
6,660,017 B2	12/2003	Beaupre	D509,589 S	9/2005	Wells
6,662,127 B2	12/2003	Wiener et al.	6,942,660 B2	9/2005	Pantera et al.
6,663,941 B2	12/2003	Brown et al.	6,942,677 B2	9/2005	Nita et al.
6,666,860 B1	12/2003	Takahashi	6,945,981 B2	9/2005	Donofrio et al.
6,666,875 B1	12/2003	Sakurai et al.	6,946,779 B2	9/2005	Birgel
6,669,690 B1	12/2003	Okada et al.	6,948,503 B2	9/2005	Refior et al.
6,669,710 B2	12/2003	Moutafis et al.	D511,145 S	11/2005	Donofrio et al.
6,676,660 B2	1/2004	Wampler et al.	6,974,450 B2	12/2005	Weber et al.
6,678,621 B2	1/2004	Wiener et al.	6,976,844 B2	12/2005	Hickok et al.
6,679,875 B2	1/2004	Honda et al.	6,976,969 B2	12/2005	Messerly
6,679,899 B2	1/2004	Wiener et al.	6,977,495 B2	12/2005	Donofrio
6,682,544 B2	1/2004	Mastri et al.	6,979,332 B2	12/2005	Adams
6,685,701 B2	2/2004	Orszulak et al.	6,981,628 B2	1/2006	Wales
6,685,703 B2	2/2004	Pearson et al.	6,984,220 B2	1/2006	Wuchinich
6,689,145 B2	2/2004	Lee et al.	6,988,295 B2	1/2006	Tillim
6,689,146 B1	2/2004	Himes	6,994,708 B2	2/2006	Manzo
6,702,821 B2	3/2004	Bonutti	7,001,335 B2	2/2006	Adachi et al.
6,716,215 B1	4/2004	David et al.	7,011,657 B2	3/2006	Truckai et al.
6,719,692 B2	4/2004	Kleffner et al.	7,014,638 B2	3/2006	Michelson
6,719,776 B2	4/2004	Baxter	7,033,357 B2	4/2006	Baxter et al.
6,723,091 B2	4/2004	Goble et al.	7,037,306 B2	5/2006	Podany
D490,059 S	5/2004	Conway et al.	7,041,083 B2	5/2006	Chu et al.
6,731,047 B2	5/2004	Kauf et al.	7,041,088 B2	5/2006	Nawrocki et al.
6,733,506 B1	5/2004	McDevitt et al.	7,041,102 B2	5/2006	Truckai et al.
6,736,813 B2	5/2004	Yamauchi et al.	7,044,949 B2	5/2006	Orszulak et al.
6,739,872 B1	5/2004	Turri	7,066,893 B2	6/2006	Hibner et al.
6,740,079 B1	5/2004	Eggers et al.	7,066,895 B2	6/2006	Podany
D491,666 S	6/2004	Kimmell et al.	7,070,597 B2	7/2006	Truckai et al.
6,743,245 B2	6/2004	Lobdell	7,074,218 B2	7/2006	Washington et al.
6,746,284 B1	6/2004	Spink, Jr.	7,074,219 B2	7/2006	Levine et al.
6,746,443 B1	6/2004	Morley et al.	7,077,039 B2	7/2006	Gass et al.
6,752,815 B2	6/2004	Beaupre	7,077,845 B2	7/2006	Hacker et al.
6,755,825 B2	6/2004	Shoenman et al.	7,077,853 B2	7/2006	Kramer et al.
6,761,698 B2	7/2004	Shibata et al.	7,083,618 B2	8/2006	Couture
6,762,535 B2	7/2004	Take et al.	7,083,619 B2	8/2006	Truckai et al.
6,770,072 B1	8/2004	Truckai et al.	7,087,054 B2	8/2006	Truckai et al.
6,773,409 B2	8/2004	Truckai et al.	7,090,672 B2	8/2006	Underwood et al.
6,773,443 B2	8/2004	Truwit et al.	7,101,371 B2	9/2006	Dycus et al.
6,773,444 B2	8/2004	Messerly	7,101,378 B2	9/2006	Salameh et al.
6,778,023 B2	8/2004	Christensen	7,104,834 B2	9/2006	Robinson et al.
6,783,524 B2	8/2004	Anderson et al.	7,108,695 B2	9/2006	Witt et al.
6,786,382 B1	9/2004	Hoffman	7,111,769 B2	9/2006	Wales et al.
6,786,383 B2	9/2004	Stegelmann	7,112,201 B2	9/2006	Truckai et al.
6,790,173 B2	9/2004	Saadat et al.	D531,311 S	10/2006	Guerra et al.
6,790,216 B1	9/2004	Ishikawa	7,117,034 B2	10/2006	Kronberg
			7,118,564 B2	10/2006	Ritchie et al.
			7,124,932 B2	10/2006	Isaacson et al.
			7,125,409 B2	10/2006	Truckai et al.
			7,128,720 B2	10/2006	Podany

(56)

References Cited

U.S. PATENT DOCUMENTS

7,131,860	B2	11/2006	Sartor et al.	7,441,684	B2	10/2008	Shelton, IV et al.
7,135,018	B2	11/2006	Ryan et al.	7,455,208	B2	11/2008	Wales et al.
7,135,030	B2	11/2006	Schwemmerberger et al.	7,462,181	B2	12/2008	Kraft et al.
7,137,980	B2	11/2006	Buyse et al.	7,464,846	B2	12/2008	Shelton, IV et al.
7,144,403	B2	12/2006	Booth	7,472,815	B2	1/2009	Shelton, IV et al.
7,153,315	B2	12/2006	Miller	7,473,263	B2	1/2009	Johnston et al.
D536,093	S	1/2007	Nakajima et al.	7,479,148	B2	1/2009	Beaupre
7,156,189	B1	1/2007	Bar-Cohen et al.	7,479,160	B2	1/2009	Branch et al.
7,156,853	B2	1/2007	Muratsu	7,481,775	B2	1/2009	Weikel, Jr. et al.
7,157,058	B2	1/2007	Marhasin et al.	7,488,285	B2	2/2009	Honda et al.
7,159,750	B2	1/2007	Racenet et al.	7,494,468	B2	2/2009	Rabiner et al.
7,160,296	B2	1/2007	Pearson et al.	7,502,234	B2	3/2009	Goliszek et al.
7,160,299	B2	1/2007	Baily	7,503,893	B2	3/2009	Kucklick
7,163,548	B2	1/2007	Stulen et al.	7,503,895	B2	3/2009	Rabiner et al.
7,169,144	B2	1/2007	Hoey et al.	7,506,790	B2	3/2009	Shelton, IV
7,169,146	B2	1/2007	Truckai et al.	7,506,791	B2	3/2009	Omaits et al.
7,179,254	B2	2/2007	Pendekanti et al.	7,524,320	B2	4/2009	Tierney et al.
7,179,271	B2	2/2007	Friedman et al.	7,530,986	B2	5/2009	Beaupre et al.
7,186,253	B2	3/2007	Truckai et al.	7,534,243	B1	5/2009	Chin et al.
7,189,233	B2	3/2007	Truckai et al.	D594,983	S	6/2009	Price et al.
D541,418	S	4/2007	Schechter et al.	7,540,871	B2	6/2009	Gonnering
7,198,635	B2	4/2007	Danek et al.	7,544,200	B2	6/2009	Houser
7,204,820	B2	4/2007	Akahoshi	7,549,564	B2	6/2009	Boudreaux
7,207,997	B2	4/2007	Shipp et al.	7,559,450	B2	7/2009	Wales et al.
7,210,881	B2	5/2007	Greenberg	7,567,012	B2	7/2009	Namikawa
7,211,079	B2	5/2007	Treat	7,568,603	B2	8/2009	Shelton, IV et al.
7,217,128	B2	5/2007	Atkin et al.	7,569,057	B2	8/2009	Liu et al.
7,217,269	B2	5/2007	El-Galley et al.	7,572,266	B2	8/2009	Young et al.
7,220,951	B2	5/2007	Truckai et al.	7,572,268	B2	8/2009	Babaev
7,223,229	B2	5/2007	Inman et al.	7,578,820	B2	8/2009	Moore et al.
7,229,455	B2	6/2007	Sakurai et al.	7,582,084	B2	9/2009	Swanson et al.
7,235,071	B2	6/2007	Gonnering	7,582,095	B2	9/2009	Shipp et al.
7,244,262	B2	7/2007	Wiener et al.	7,585,181	B2	9/2009	Olsen
7,258,688	B1	8/2007	Shah et al.	7,588,176	B2	9/2009	Timm et al.
7,269,873	B2	9/2007	Brewer et al.	7,601,119	B2	10/2009	Shahinian
7,273,483	B2	9/2007	Wiener et al.	7,607,557	B2	10/2009	Shelton, IV et al.
D552,241	S	10/2007	Bromley et al.	7,621,930	B2	11/2009	Houser
7,282,048	B2	10/2007	Goble et al.	7,641,653	B2	1/2010	Dalla Betta et al.
7,285,895	B2	10/2007	Beaupré	7,645,278	B2	1/2010	Ichihashi et al.
7,300,431	B2	11/2007	Dubrovsky	7,654,431	B2	2/2010	Hueil et al.
7,300,435	B2	11/2007	Wham et al.	7,659,833	B2	2/2010	Warner et al.
7,300,446	B2	11/2007	Beaupre	7,665,647	B2	2/2010	Shelton, IV et al.
7,303,531	B2	12/2007	Lee et al.	7,670,334	B2	3/2010	Hueil et al.
7,303,557	B2	12/2007	Wham et al.	7,670,338	B2	3/2010	Albrecht et al.
7,306,597	B2	12/2007	Manzo	7,674,263	B2	3/2010	Ryan
7,309,849	B2	12/2007	Truckai et al.	7,678,069	B1	3/2010	Baker et al.
7,311,706	B2	12/2007	Schoenman et al.	7,678,125	B2	3/2010	Shipp
7,311,709	B2	12/2007	Truckai et al.	7,682,366	B2	3/2010	Sakurai et al.
7,317,955	B2	1/2008	McGreevy	7,686,770	B2	3/2010	Cohen
7,318,831	B2	1/2008	Alvarez et al.	7,686,826	B2	3/2010	Lee et al.
7,326,236	B2	2/2008	Andreas et al.	7,688,028	B2	3/2010	Phillips et al.
7,331,410	B2	2/2008	Yong et al.	7,691,098	B2	4/2010	Wallace et al.
7,335,165	B2	2/2008	Truwit et al.	7,699,846	B2	4/2010	Ryan
7,335,997	B2	2/2008	Wiener	7,713,202	B2	5/2010	Boukhny et al.
7,337,010	B2	2/2008	Howard et al.	7,714,481	B2	5/2010	Sakai
7,353,068	B2	4/2008	Tanaka et al.	7,717,312	B2	5/2010	Beetel
7,354,440	B2	4/2008	Truckai et al.	7,717,915	B2	5/2010	Miyazawa
7,364,577	B2	4/2008	Wham et al.	7,721,935	B2	5/2010	Racenet et al.
RE40,388	E	6/2008	Gines	D618,797	S	6/2010	Price et al.
7,380,695	B2	6/2008	Doll et al.	7,726,537	B2	6/2010	Olson et al.
7,380,696	B2	6/2008	Shelton, IV et al.	7,727,177	B2	6/2010	Bayat
7,381,209	B2	6/2008	Truckai et al.	7,738,969	B2	6/2010	Bleich
7,390,317	B2	6/2008	Taylor et al.	7,740,594	B2	6/2010	Hibner
7,404,508	B2	7/2008	Smith et al.	7,751,115	B2	7/2010	Song
7,408,288	B2	8/2008	Hara	D621,503	S	8/2010	Often et al.
7,416,101	B2	8/2008	Shelton, IV et al.	7,766,210	B2	8/2010	Shelton, IV et al.
7,416,437	B2	8/2008	Sartor et al.	7,766,693	B2	8/2010	Sartor et al.
D576,725	S	9/2008	Shumer et al.	7,770,774	B2	8/2010	Mastri et al.
7,419,490	B2	9/2008	Falkenstein et al.	7,770,775	B2	8/2010	Shelton, IV et al.
7,422,139	B2	9/2008	Shelton, IV et al.	7,771,425	B2	8/2010	Dycus et al.
7,422,463	B2	9/2008	Kuo	7,771,444	B2	8/2010	Patel et al.
D578,643	S	10/2008	Shumer et al.	7,775,972	B2	8/2010	Brock et al.
D578,644	S	10/2008	Shumer et al.	7,776,036	B2	8/2010	Schechter et al.
D578,645	S	10/2008	Shumer et al.	7,778,733	B2	8/2010	Nowlin et al.
7,431,704	B2	10/2008	Babaev	7,780,054	B2	8/2010	Wales
				7,780,593	B2	8/2010	Ueno et al.
				7,780,651	B2	8/2010	Madhani et al.
				7,780,659	B2	8/2010	Okada et al.
				7,784,662	B2	8/2010	Wales et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,796,969 B2	9/2010	Kelly et al.	8,236,019 B2	8/2012	Houser
7,798,386 B2	9/2010	Schall et al.	8,236,020 B2	8/2012	Smith et al.
7,799,020 B2	9/2010	Shores et al.	8,241,271 B2	8/2012	Millman et al.
7,799,045 B2	9/2010	Masuda	8,246,575 B2	8/2012	Viola
7,803,152 B2	9/2010	Honda et al.	8,246,615 B2	8/2012	Behnke
7,806,891 B2	10/2010	Nowlin et al.	8,252,012 B2	8/2012	Stulen
7,810,693 B2	10/2010	Broehl et al.	8,253,303 B2	8/2012	Giordano et al.
7,811,283 B2	10/2010	Moses et al.	8,257,377 B2	9/2012	Wiener et al.
7,819,819 B2	10/2010	Quick et al.	8,257,387 B2	9/2012	Cunningham
7,821,143 B2	10/2010	Wiener	8,273,087 B2	9/2012	Kimura et al.
D627,066 S	11/2010	Romero	D669,992 S	10/2012	Schafer et al.
7,824,401 B2	11/2010	Manzo et al.	D669,993 S	10/2012	Merchant et al.
7,832,611 B2	11/2010	Boyden et al.	8,286,846 B2	10/2012	Smith et al.
7,834,484 B2	11/2010	Sartor	8,287,485 B2	10/2012	Kimura et al.
7,837,699 B2	11/2010	Yamada et al.	8,287,528 B2	10/2012	Wham et al.
7,845,537 B2	12/2010	Shelton, IV et al.	8,287,532 B2	10/2012	Carroll et al.
7,846,155 B2	12/2010	Houser et al.	8,292,888 B2	10/2012	Whitman
7,846,161 B2	12/2010	Dumbauld et al.	8,298,223 B2	10/2012	Wham et al.
7,854,735 B2	12/2010	Houser et al.	8,298,225 B2	10/2012	Gilbert
D631,155 S	1/2011	Peine et al.	8,303,576 B2	11/2012	Brock
7,861,906 B2	1/2011	Doll et al.	8,303,580 B2	11/2012	Wham et al.
7,862,560 B2	1/2011	Marion	8,303,583 B2	11/2012	Hosier et al.
7,876,030 B2	1/2011	Taki et al.	8,319,400 B2	11/2012	Houser et al.
D631,965 S	2/2011	Price et al.	8,323,302 B2	12/2012	Robertson et al.
7,878,991 B2	2/2011	Babaev	8,333,778 B2	12/2012	Smith et al.
7,879,033 B2	2/2011	Sartor et al.	8,333,779 B2	12/2012	Smith et al.
7,892,606 B2	2/2011	Thies et al.	8,334,468 B2	12/2012	Palmer et al.
7,901,400 B2	3/2011	Wham et al.	8,334,635 B2	12/2012	Voegelé et al.
7,901,423 B2	3/2011	Stulen et al.	8,337,407 B2	12/2012	Quistgaard et al.
7,905,881 B2	3/2011	Masuda et al.	8,338,726 B2	12/2012	Palmer et al.
7,909,824 B2	3/2011	Masuda et al.	8,344,596 B2	1/2013	Nield et al.
7,922,061 B2	4/2011	Shelton, IV et al.	8,348,967 B2	1/2013	Stulen
7,922,651 B2	4/2011	Yamada et al.	8,357,103 B2	1/2013	Mark et al.
D637,288 S	5/2011	Houghton	8,366,727 B2	2/2013	Witt et al.
D638,540 S	5/2011	Ijiri et al.	8,372,099 B2	2/2013	Deville et al.
7,936,203 B2	5/2011	Zimlich	8,372,101 B2	2/2013	Smith et al.
7,951,095 B2	5/2011	Makin et al.	8,372,102 B2	2/2013	Stulen et al.
7,951,165 B2	5/2011	Golden et al.	8,374,670 B2	2/2013	Selkee
7,959,050 B2	6/2011	Smith et al.	8,377,059 B2	2/2013	Deville et al.
7,959,626 B2	6/2011	Hong et al.	8,377,085 B2	2/2013	Smith et al.
7,972,329 B2	7/2011	Refior et al.	8,382,748 B2	2/2013	Geisel
7,976,544 B2	7/2011	McClurken et al.	8,382,775 B1	2/2013	Bender et al.
7,981,050 B2	7/2011	Ritchart et al.	8,382,782 B2	2/2013	Robertson et al.
7,998,157 B2	8/2011	Culp et al.	8,403,948 B2	3/2013	Deville et al.
8,038,693 B2	10/2011	Allen	8,403,949 B2	3/2013	Palmer et al.
8,057,498 B2	11/2011	Robertson	8,403,950 B2	3/2013	Palmer et al.
8,058,771 B2	11/2011	Giordano et al.	8,418,073 B2	4/2013	Mohr et al.
8,061,014 B2	11/2011	Smith et al.	8,418,349 B2	4/2013	Smith et al.
8,070,711 B2	12/2011	Bassinger et al.	8,419,757 B2	4/2013	Smith et al.
8,070,762 B2	12/2011	Escudero et al.	8,419,758 B2	4/2013	Smith et al.
8,075,558 B2	12/2011	Truckai et al.	8,419,759 B2	4/2013	Dietz
8,089,197 B2	1/2012	Rinner et al.	8,425,545 B2	4/2013	Smith et al.
8,097,012 B2	1/2012	Kagarise	8,430,898 B2	4/2013	Wiener et al.
8,105,323 B2	1/2012	Buyse et al.	8,435,257 B2	5/2013	Smith et al.
8,142,461 B2	3/2012	Houser et al.	8,439,912 B2	5/2013	Cunningham et al.
8,152,801 B2	4/2012	Goldberg et al.	8,439,939 B2	5/2013	Deville et al.
8,152,825 B2	4/2012	Madan et al.	8,444,637 B2	5/2013	Podmore et al.
8,157,145 B2	4/2012	Shelton, IV et al.	8,444,662 B2	5/2013	Palmer et al.
8,161,977 B2	4/2012	Shelton, IV et al.	8,444,664 B2	5/2013	Balanév et al.
8,162,966 B2	4/2012	Connor et al.	8,460,288 B2	6/2013	Tamai et al.
8,172,846 B2	5/2012	Brunnett et al.	8,461,744 B2	6/2013	Wiener et al.
8,172,870 B2	5/2012	Shipp	8,469,981 B2	6/2013	Robertson et al.
8,177,800 B2	5/2012	Spitz et al.	8,479,969 B2	7/2013	Shelton, IV
8,182,502 B2	5/2012	Stulen et al.	8,480,703 B2	7/2013	Nicholas et al.
8,186,877 B2	5/2012	Klimovitch et al.	8,485,413 B2	7/2013	Scheib et al.
D661,801 S	6/2012	Price et al.	8,486,057 B2	7/2013	Behnke, II
D661,802 S	6/2012	Price et al.	8,486,096 B2	7/2013	Robertson et al.
D661,803 S	6/2012	Price et al.	8,491,578 B2	7/2013	Manwaring et al.
D661,804 S	6/2012	Price et al.	D687,549 S	8/2013	Johnson et al.
8,197,472 B2	6/2012	Lau et al.	8,506,555 B2	8/2013	Ruiz Morales
8,197,502 B2	6/2012	Smith et al.	8,509,318 B2	8/2013	Tailliet
8,207,651 B2	6/2012	Gilbert	8,512,359 B2	8/2013	Whitman et al.
8,210,411 B2	7/2012	Yates et al.	8,512,365 B2	8/2013	Wiener et al.
8,226,675 B2	7/2012	Houser et al.	8,523,889 B2	9/2013	Stulen et al.
8,235,917 B2	8/2012	Joseph et al.	8,531,064 B2	9/2013	Robertson et al.
			8,535,340 B2	9/2013	Allen
			8,535,341 B2	9/2013	Allen
			8,546,996 B2	10/2013	Messerly et al.
			8,546,999 B2	10/2013	Houser et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,551,086 B2	10/2013	Kimura et al.	9,283,045 B2	3/2016	Rhee et al.
8,568,400 B2	10/2013	Gilbert	9,326,788 B2	5/2016	Batross et al.
8,573,461 B2	11/2013	Shelton, IV et al.	9,339,289 B2	5/2016	Robertson
8,573,465 B2	11/2013	Shelton, IV	9,351,754 B2	5/2016	Vakharia et al.
8,579,928 B2	11/2013	Robertson et al.	9,393,037 B2	7/2016	Olson et al.
8,591,459 B2	11/2013	Clymer et al.	9,408,622 B2	8/2016	Stulen et al.
8,591,506 B2	11/2013	Wham et al.	9,414,853 B2	8/2016	Stulen et al.
8,591,536 B2	11/2013	Robertson	9,421,060 B2	8/2016	Monson et al.
D695,407 S	12/2013	Price et al.	9,427,249 B2	8/2016	Robertson et al.
D696,631 S	12/2013	Price et al.	9,439,668 B2	9/2016	Timm et al.
8,602,031 B2	12/2013	Reis et al.	9,439,669 B2	9/2016	Wiener et al.
8,602,288 B2	12/2013	Shelton, IV et al.	9,445,832 B2	9/2016	Wiener et al.
8,608,745 B2	12/2013	Guzman et al.	2001/0025173 A1	9/2001	Ritchie et al.
8,616,431 B2	12/2013	Timm et al.	2001/0025183 A1	9/2001	Shahidi et al.
8,623,027 B2	1/2014	Price et al.	2001/0025184 A1	9/2001	Messerly
8,650,728 B2	2/2014	Wan et al.	2001/0031950 A1	10/2001	Ryan
8,652,155 B2	2/2014	Houser et al.	2001/0039419 A1	11/2001	Francischelli et al.
8,659,208 B1	2/2014	Rose et al.	2002/0002377 A1	1/2002	Cimino
8,663,220 B2	3/2014	Wiener et al.	2002/0019649 A1	2/2002	Sikora et al.
8,690,582 B2	4/2014	Rohrbach et al.	2002/0022836 A1	2/2002	Goble et al.
8,696,366 B2	4/2014	Chen et al.	2002/0029055 A1	3/2002	Bonutti
8,704,425 B2	4/2014	Giordano et al.	2002/0049551 A1	4/2002	Friedman et al.
8,709,031 B2	4/2014	Stulen	2002/0052617 A1	5/2002	Anis et al.
8,747,351 B2	6/2014	Schultz	2002/0077550 A1	6/2002	Rabiner et al.
8,749,116 B2	6/2014	Messerly et al.	2002/0156466 A1	10/2002	Sakurai et al.
8,752,749 B2	6/2014	Moore et al.	2002/0156493 A1	10/2002	Houser et al.
8,753,338 B2	6/2014	Widenhouse et al.	2003/0014087 A1	1/2003	Fang et al.
8,754,570 B2	6/2014	Voegele et al.	2003/0036705 A1	2/2003	Hare et al.
8,758,352 B2	6/2014	Cooper et al.	2003/0050572 A1	3/2003	Brautigam et al.
8,764,735 B2	7/2014	Coe et al.	2003/0055443 A1	3/2003	Spotnitz
8,771,270 B2	7/2014	Burbank	2003/0114851 A1	6/2003	Truckai et al.
8,773,001 B2	7/2014	Wiener et al.	2003/0144680 A1	7/2003	Kellogg et al.
8,779,648 B2	7/2014	Giordano et al.	2003/0199794 A1	10/2003	Sakurai et al.
8,784,418 B2	7/2014	Romero	2003/0204199 A1	10/2003	Novak et al.
8,808,319 B2	8/2014	Houser et al.	2003/0212332 A1	11/2003	Fenton et al.
8,827,992 B2	9/2014	Koss et al.	2003/0212363 A1	11/2003	Shipp
8,845,537 B2	9/2014	Tanaka et al.	2003/0212392 A1	11/2003	Fenton et al.
8,882,791 B2	11/2014	Stulen	2003/0212422 A1	11/2003	Fenton et al.
8,888,776 B2	11/2014	Dietz et al.	2003/0229344 A1	12/2003	Dycus et al.
8,888,809 B2	11/2014	Davison et al.	2004/0030254 A1	2/2004	Babaev
8,899,462 B2	12/2014	Kostrzewski et al.	2004/0030330 A1	2/2004	Brassell et al.
8,900,259 B2	12/2014	Houser et al.	2004/0047485 A1	3/2004	Sherrit et al.
8,911,460 B2	12/2014	Neurohr et al.	2004/0054364 A1	3/2004	Aranyi et al.
8,951,248 B2	2/2015	Messerly et al.	2004/0064151 A1	4/2004	Mollenauer
8,956,349 B2	2/2015	Aldridge et al.	2004/0092921 A1	5/2004	Kadziasukas et al.
8,968,283 B2	3/2015	Kharin	2004/0092992 A1	5/2004	Adams et al.
8,968,355 B2	3/2015	Malkowski et al.	2004/0097911 A1	5/2004	Murakami et al.
8,974,477 B2	3/2015	Yamada	2004/0097912 A1	5/2004	Gonnering
8,979,890 B2	3/2015	Boudreaux	2004/0097919 A1	5/2004	Wellman et al.
8,986,287 B2	3/2015	Park et al.	2004/0097996 A1	5/2004	Rabiner et al.
8,986,302 B2	3/2015	Aldridge et al.	2004/0116952 A1	6/2004	Sakurai et al.
8,989,903 B2	3/2015	Weir et al.	2004/0132383 A1	7/2004	Langford et al.
9,017,326 B2	4/2015	DiNardo et al.	2004/0147934 A1	7/2004	Kiester
9,039,695 B2	5/2015	Giordano et al.	2004/0167508 A1	8/2004	Wham et al.
9,043,018 B2	5/2015	Mohr	2004/0176686 A1	9/2004	Hare et al.
9,044,261 B2	6/2015	Houser	2004/0176751 A1	9/2004	Weitzner et al.
9,050,093 B2	6/2015	Aldridge et al.	2004/0199193 A1	10/2004	Hayashi et al.
9,050,124 B2	6/2015	Houser	2004/0204728 A1	10/2004	Haefner
9,060,775 B2	6/2015	Wiener et al.	2004/0215132 A1	10/2004	Yoon
9,060,776 B2	6/2015	Yates et al.	2004/0243147 A1	12/2004	Lipow
9,066,747 B2	6/2015	Robertson	2004/0260300 A1	12/2004	Gorensek et al.
9,072,539 B2	7/2015	Messerly et al.	2005/0020967 A1	1/2005	Ono
9,089,360 B2	7/2015	Messerly et al.	2005/0021018 A1	1/2005	Anderson et al.
9,095,367 B2	8/2015	Olson et al.	2005/0021065 A1	1/2005	Yamada et al.
9,107,689 B2	8/2015	Robertson et al.	2005/0033337 A1	2/2005	Muir et al.
9,113,940 B2	8/2015	Twomey	2005/0049546 A1	3/2005	Messerly et al.
9,168,054 B2	10/2015	Turner et al.	2005/0070800 A1	3/2005	Takahashi
9,198,714 B2	12/2015	Worrell et al.	2005/0096683 A1	5/2005	Ellins et al.
9,220,527 B2	12/2015	Houser et al.	2005/0099824 A1	5/2005	Dowling et al.
9,226,766 B2	1/2016	Aldridge et al.	2005/0103819 A1	5/2005	Racenet et al.
9,226,767 B2	1/2016	Stulen et al.	2005/0143769 A1	6/2005	White et al.
9,232,979 B2	1/2016	Parihar et al.	2005/0149108 A1	7/2005	Cox
9,237,921 B2	1/2016	Messerly et al.	2005/0165345 A1	7/2005	Laufer et al.
9,241,728 B2	1/2016	Price et al.	2005/0177184 A1	8/2005	Easley
9,241,731 B2	1/2016	Boudreaux et al.	2005/0182339 A1	8/2005	Lee et al.
			2005/0188743 A1	9/2005	Land
			2005/0192610 A1	9/2005	Houser et al.
			2005/0209620 A1	9/2005	Du et al.
			2005/0222598 A1	10/2005	Ho et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2005/0234484 A1	10/2005	Houser et al.	2008/0140158 A1	6/2008	Hamel et al.
2005/0249667 A1	11/2005	Tuszynski et al.	2008/0147092 A1	6/2008	Rogge et al.
2005/0256405 A1	11/2005	Makin et al.	2008/0171938 A1	7/2008	Masuda et al.
2005/0261581 A1	11/2005	Hughes et al.	2008/0172051 A1	7/2008	Masuda et al.
2005/0261588 A1	11/2005	Makin et al.	2008/0177268 A1	7/2008	Daum et al.
2005/0273090 A1	12/2005	Nieman et al.	2008/0188878 A1	8/2008	Young
2005/0288659 A1	12/2005	Kimura et al.	2008/0200940 A1	8/2008	Eichmann et al.
2006/0030797 A1	2/2006	Zhou et al.	2008/0208108 A1	8/2008	Kimura
2006/0058825 A1	3/2006	Ogura et al.	2008/0208231 A1	8/2008	Ota et al.
2006/0063130 A1	3/2006	Hayman et al.	2008/0214967 A1	9/2008	Aranyi et al.
2006/0066181 A1	3/2006	Bromfield et al.	2008/0234709 A1	9/2008	Houser
2006/0074442 A1	4/2006	Noriega et al.	2008/0243106 A1	10/2008	Coe et al.
2006/0079874 A1	4/2006	Faller et al.	2008/0243162 A1	10/2008	Shibata et al.
2006/0079879 A1	4/2006	Faller et al.	2008/0245371 A1	10/2008	Gruber
2006/0084963 A1	4/2006	Messerly	2008/0249553 A1	10/2008	Gruber et al.
2006/0095046 A1	5/2006	Trieu et al.	2008/0255423 A1	10/2008	Kondo et al.
2006/0190034 A1	8/2006	Nishizawa et al.	2008/0262490 A1	10/2008	Williams
2006/0206100 A1	9/2006	Eskridge et al.	2008/0281200 A1	11/2008	Voic et al.
2006/0206115 A1	9/2006	Schomer et al.	2008/0281315 A1	11/2008	Gines
2006/0211943 A1	9/2006	Beaupre	2008/0281322 A1	11/2008	Sherman et al.
2006/0217729 A1	9/2006	Eskridge et al.	2008/0287948 A1	11/2008	Newton et al.
2006/0224160 A1	10/2006	Trieu et al.	2009/0023985 A1	1/2009	Ewers
2006/0235306 A1	10/2006	Cotter et al.	2009/0024141 A1	1/2009	Stahler et al.
2006/0247558 A1	11/2006	Yamada	2009/0048537 A1	2/2009	Lydon et al.
2006/0253050 A1	11/2006	Yoshimine et al.	2009/0054886 A1	2/2009	Yachi et al.
2006/0264809 A1	11/2006	Hansmann et al.	2009/0054894 A1	2/2009	Yachi
2006/0271030 A1	11/2006	Francis et al.	2009/0076506 A1	3/2009	Baker
2007/0016235 A1	1/2007	Tanaka et al.	2009/0082716 A1	3/2009	Akahoshi
2007/0016236 A1	1/2007	Beaupre	2009/0088738 A1	4/2009	Guerra et al.
2007/0055228 A1	3/2007	Berg et al.	2009/0088785 A1	4/2009	Masuda
2007/0056596 A1	3/2007	Fanney et al.	2009/0112229 A1	4/2009	Omori et al.
2007/0060915 A1	3/2007	Kucklick	2009/0118751 A1	5/2009	Wiener et al.
2007/0060935 A1	3/2007	Schwardt et al.	2009/0118802 A1	5/2009	Mioduski et al.
2007/0063618 A1	3/2007	Bromfield	2009/0138006 A1	5/2009	Bales et al.
2007/0074584 A1	4/2007	Talarico et al.	2009/0143799 A1	6/2009	Smith et al.
2007/0078458 A1	4/2007	Dumbauld et al.	2009/0143800 A1	6/2009	Deville et al.
2007/0106317 A1	5/2007	Shelton, IV et al.	2009/0143806 A1	6/2009	Witt et al.
2007/0129716 A1	6/2007	Daw et al.	2009/0149801 A1	6/2009	Crandall et al.
2007/0130771 A1	6/2007	Ehlert et al.	2009/0163807 A1	6/2009	Sliwa
2007/0131034 A1	6/2007	Ehlert et al.	2009/0207923 A1	8/2009	Dress
2007/0149881 A1	6/2007	Rabin	2009/0216157 A1	8/2009	Yamada
2007/0156163 A1	7/2007	Davison et al.	2009/0223033 A1	9/2009	Houser
2007/0162050 A1	7/2007	Sartor	2009/0254077 A1	10/2009	Craig
2007/0166663 A1	7/2007	Telles et al.	2009/0254080 A1	10/2009	Honda
2007/0167736 A1 *	7/2007	Dietz A61B 10/0275 600/411	2009/0264909 A1	10/2009	Beaupre
2007/0173803 A1	7/2007	Wham et al.	2009/0270771 A1	10/2009	Takahashi
2007/0173813 A1	7/2007	Odom	2009/0270812 A1	10/2009	Litscher et al.
2007/0173872 A1	7/2007	Neuenfeldt	2009/0270853 A1	10/2009	Yachi et al.
2007/0175949 A1	8/2007	Shelton, IV et al.	2009/0270891 A1	10/2009	Beupre
2007/0185380 A1	8/2007	Kucklick	2009/0270899 A1	10/2009	Carusillo et al.
2007/0191712 A1	8/2007	Messerly et al.	2009/0275940 A1	11/2009	Malackowski et al.
2007/0219481 A1	9/2007	Babaev	2009/0299141 A1	12/2009	Downey et al.
2007/0239028 A1 *	10/2007	Houser A61B 17/320092 600/471	2009/0318945 A1	12/2009	Yoshimine et al.
2007/0239101 A1	10/2007	Kellogg	2009/0327715 A1	12/2009	Smith et al.
2007/0249941 A1	10/2007	Salehi et al.	2010/0004508 A1	1/2010	Naito et al.
2007/0260234 A1	11/2007	McCullagh et al.	2010/0016785 A1	1/2010	Takuma
2007/0265560 A1	11/2007	Soltani et al.	2010/0016852 A1	1/2010	Manzo et al.
2007/0275348 A1	11/2007	Lemon	2010/0022825 A1	1/2010	Yoshie
2007/0282335 A1	12/2007	Young et al.	2010/0030233 A1	2/2010	Whitman et al.
2007/0287933 A1	12/2007	Phan et al.	2010/0030248 A1	2/2010	Palmer et al.
2007/0288055 A1	12/2007	Lee	2010/0036370 A1	2/2010	Mirel et al.
2008/0009848 A1	1/2008	Paraschiv et al.	2010/0042077 A1	2/2010	Okada
2008/0013809 A1	1/2008	Zhu et al.	2010/0049180 A1	2/2010	Wells et al.
2008/0051812 A1	2/2008	Schmitz et al.	2010/0057118 A1	3/2010	Dietz et al.
2008/0058585 A1	3/2008	Novak et al.	2010/0063525 A1	3/2010	Beaupre et al.
2008/0058775 A1	3/2008	Darian et al.	2010/0063528 A1	3/2010	Beaupre
2008/0058845 A1	3/2008	Shimizu et al.	2010/0069940 A1	3/2010	Miller et al.
2008/0077145 A1	3/2008	Boyden et al.	2010/0106173 A1	4/2010	Yoshimine
2008/0082039 A1	4/2008	Babaev	2010/0158307 A1	6/2010	Kubota et al.
2008/0082098 A1	4/2008	Tanaka et al.	2010/0168741 A1	7/2010	Sanai et al.
2008/0097501 A1	4/2008	Blier	2010/0187283 A1	7/2010	Crainich et al.
2008/0114364 A1	5/2008	Goldin et al.	2010/0222714 A1	9/2010	Muir et al.
2008/0125768 A1	5/2008	Tahara et al.	2010/0228264 A1	9/2010	Robinson et al.
			2010/0234906 A1	9/2010	Koh
			2010/0262134 A1	10/2010	Jensen et al.
			2010/0274160 A1	10/2010	Yachi et al.
			2010/0280407 A1	11/2010	Polster
			2010/0292691 A1	11/2010	Brogna
			2010/0298743 A1	11/2010	Nield et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2010/0298851	A1	11/2010	Nield	2013/0123782	A1	5/2013	Trees et al.
2010/0331742	A1	12/2010	Masuda	2013/0123822	A1	5/2013	Wellman et al.
2011/0004233	A1	1/2011	Muir et al.	2013/0131660	A1	5/2013	Monson et al.
2011/0009850	A1	1/2011	Main et al.	2013/0165929	A1	6/2013	Muir et al.
2011/0077648	A1	3/2011	Lee et al.	2013/0217967	A1	8/2013	Mohr et al.
2011/0087218	A1	4/2011	Boudreaux et al.	2013/0253498	A1	9/2013	Germain et al.
2011/0112526	A1	5/2011	Fritz et al.	2013/0274734	A1	10/2013	Maass et al.
2011/0125151	A1	5/2011	Strauss et al.	2013/0282038	A1	10/2013	Dannaher et al.
2011/0125174	A1	5/2011	Babaev	2013/0296908	A1	11/2013	Schulte et al.
2011/0144806	A1	6/2011	Sandhu et al.	2013/0338661	A1	12/2013	Behnke, II
2011/0196398	A1	8/2011	Robertson et al.	2013/0345689	A1	12/2013	Ruddenklau et al.
2011/0196399	A1	8/2011	Robertson et al.	2014/0005640	A1	1/2014	Shelton, IV et al.
2011/0196404	A1	8/2011	Dietz et al.	2014/0005653	A1	1/2014	Shelton, IV et al.
2011/0224689	A1	9/2011	Larkin et al.	2014/0005656	A1	1/2014	Mucilli et al.
2011/0238065	A1	9/2011	Hunt et al.	2014/0005661	A1	1/2014	Shelton, IV et al.
2011/0257650	A1	10/2011	Deville et al.	2014/0005662	A1	1/2014	Shelton, IV et al.
2011/0270126	A1	11/2011	Gunday et al.	2014/0005676	A1	1/2014	Shelton, IV et al.
2011/0290853	A1	12/2011	Shelton, IV et al.	2014/0005680	A1	1/2014	Shelton, IV et al.
2011/0290856	A1	12/2011	Shelton, IV et al.	2014/0005681	A1	1/2014	Gee et al.
2011/0295242	A1	12/2011	Spivey et al.	2014/0005702	A1	1/2014	Timm et al.
2012/0004655	A1	1/2012	Kim et al.	2014/0005705	A1	1/2014	Weir et al.
2012/0022525	A1	1/2012	Dietz et al.	2014/0005708	A1	1/2014	Shelton, IV et al.
2012/0022530	A1	1/2012	Woodruff et al.	2014/0005718	A1	1/2014	Shelton, IV et al.
2012/0022583	A1	1/2012	Sugalski et al.	2014/0012299	A1	1/2014	Stoddard et al.
2012/0059289	A1	3/2012	Nield et al.	2014/0066962	A1	3/2014	Robertson et al.
2012/0065628	A1	3/2012	Naito	2014/0087569	A1	3/2014	Lee
2012/0071863	A1	3/2012	Lee et al.	2014/0107538	A1	4/2014	Wiener et al.
2012/0078139	A1	3/2012	Aldridge et al.	2014/0114327	A1	4/2014	Boudreaux et al.
2012/0078243	A1	3/2012	Worrell et al.	2014/0135804	A1	5/2014	Weisenburgh, II et al.
2012/0078244	A1	3/2012	Worrell et al.	2014/0155921	A1	6/2014	Price et al.
2012/0078247	A1	3/2012	Worrell et al.	2014/0180280	A1	6/2014	Sigmon, Jr.
2012/0078278	A1	3/2012	Bales, Jr. et al.	2014/0243864	A1	8/2014	Voegele et al.
2012/0080332	A1	4/2012	Shelton, IV et al.	2014/0276970	A1	9/2014	Messerly et al.
2012/0101495	A1	4/2012	Young et al.	2015/0045819	A1	2/2015	Houser et al.
2012/0101501	A1	4/2012	Nishimura et al.	2015/0066067	A1	3/2015	Stulen
2012/0109159	A1	5/2012	Jordan et al.	2015/0073460	A1	3/2015	Stulen
2012/0116379	A1	5/2012	Yates et al.	2015/0112335	A1	4/2015	Boudreaux et al.
2012/0116391	A1	5/2012	Houser et al.	2015/0119914	A1	4/2015	Neurohr et al.
2012/0116394	A1	5/2012	Timm et al.	2015/0119915	A1	4/2015	Neurohr et al.
2012/0116395	A1	5/2012	Madan et al.	2015/0123348	A1	5/2015	Robertson et al.
2012/0130256	A1	5/2012	Buyse et al.	2015/0157355	A1	6/2015	Price et al.
2012/0130365	A1	5/2012	McLawhorn	2015/0157356	A1	6/2015	Gee
2012/0136354	A1	5/2012	Rupp	2015/0164533	A1	6/2015	Felder et al.
2012/0138660	A1	6/2012	Shelton, IV	2015/0164534	A1	6/2015	Felder et al.
2012/0143211	A1	6/2012	Kishi	2015/0164535	A1	6/2015	Felder et al.
2012/0150170	A1	6/2012	Buyse et al.	2015/0164536	A1	6/2015	Czarnecki et al.
2012/0165816	A1	6/2012	Kersten et al.	2015/0164537	A1	6/2015	Cagle et al.
2012/0172873	A1	7/2012	Artale et al.	2015/0164538	A1	6/2015	Aldridge et al.
2012/0172904	A1	7/2012	Muir et al.	2015/0182251	A1	7/2015	Messerly et al.
2012/0177005	A1	7/2012	Liang et al.	2015/0182276	A1	7/2015	Wiener et al.
2012/0184946	A1	7/2012	Price et al.	2015/0182277	A1	7/2015	Wiener et al.
2012/0199630	A1	8/2012	Shelton, IV	2015/0196318	A1	7/2015	Messerly et al.
2012/0199632	A1	8/2012	Spivey et al.	2015/0250495	A1	9/2015	Robertson et al.
2012/0203143	A1	8/2012	Sanai et al.	2015/0257780	A1	9/2015	Houser
2012/0203247	A1	8/2012	Shelton, IV et al.	2015/0257781	A1	9/2015	Houser et al.
2012/0209289	A1	8/2012	Duque et al.	2015/0265308	A1	9/2015	Houser et al.
2012/0209303	A1	8/2012	Frankhouser et al.	2015/0327883	A1	11/2015	Messerly et al.
2012/0210223	A1	8/2012	Eppolito	2015/0328484	A1	11/2015	Messerly et al.
2012/0215220	A1	8/2012	Manzo et al.	2015/0340586	A1	11/2015	Wiener et al.
2012/0245582	A1	9/2012	Kimball et al.	2015/0351789	A1	12/2015	Robertson et al.
2012/0253370	A1	10/2012	Ross et al.	2016/0030076	A1	2/2016	Faller et al.
2012/0269676	A1	10/2012	Houser et al.	2016/0089209	A1	3/2016	Parihar et al.
2012/0330307	A1	12/2012	Ladtow et al.	2016/0089533	A1	3/2016	Turner et al.
2013/0012957	A1	1/2013	Shelton, IV et al.	2016/0095617	A1	4/2016	Price et al.
2013/0030433	A1	1/2013	Heard	2016/0106509	A1	4/2016	Worrell et al.
2013/0035680	A1	2/2013	Ben-Haim et al.	2016/0120563	A1	5/2016	Messerly et al.
2013/0053840	A1	2/2013	Krapohl et al.	2016/0144204	A1	5/2016	Akagane
2013/0072856	A1	3/2013	Frankhouser et al.	2016/0192999	A1	7/2016	Stulen et al.
2013/0072857	A1	3/2013	Frankhouser et al.	2016/0206342	A1	7/2016	Robertson et al.
2013/0079762	A1	3/2013	Twomey et al.	2016/0262786	A1	9/2016	Madan et al.
2013/0103023	A1	4/2013	Monson et al.	2016/0296249	A1	10/2016	Robertson
2013/0103024	A1	4/2013	Monson et al.	2016/0296250	A1	10/2016	Olson et al.
2013/0110145	A1	5/2013	Weitzman	2016/0296251	A1	10/2016	Olson et al.
2013/0123776	A1	5/2013	Monson et al.				
2013/0123777	A1	5/2013	Monson et al.				

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0296252 A1 10/2016 Olson et al.
 2016/0317217 A1 11/2016 Batross et al.
 2016/0367281 A1 12/2016 Gee et al.

FOREIGN PATENT DOCUMENTS

CN 1233944 A 11/1999
 CN 1253485 A 5/2000
 CN 1634601 A 7/2005
 CN 1640365 A 7/2005
 CN 1694649 A 11/2005
 CN 1922563 A 2/2007
 CN 1951333 A 4/2007
 CN 101040799 A 9/2007
 CN 101467917 A 1/2009
 CN 202027624 U 11/2011
 DE 3904558 A1 8/1990
 DE 9210327 U1 11/1992
 DE 4323585 A1 1/1995
 DE 19608716 C1 4/1997
 DE 20021619 U1 3/2001
 DE 10042606 A1 8/2001
 EP 0136855 B1 9/1984
 EP 0171967 A2 2/1986
 EP 1839599 A1 10/1987
 EP 0336742 A2 4/1989
 EP 0342448 A1 11/1989
 EP 0424685 B1 5/1991
 EP 0443256 A1 8/1991
 EP 0456470 A1 11/1991
 EP 0238667 B1 2/1993
 EP 0598976 A2 1/1994
 EP 0677275 A2 3/1995
 EP 0482195 B1 1/1996
 EP 0695535 A1 2/1996
 EP 0741996 A2 11/1996
 EP 0612570 B1 6/1997
 EP 1108394 A2 6/2001
 EP 1138264 A1 10/2001
 EP 0908148 B1 1/2002
 EP 1229515 A2 8/2002
 EP 1285634 A1 2/2003
 EP 0908155 B1 6/2003
 EP 0705570 B1 4/2004
 EP 0765637 B1 7/2004
 EP 0870473 B1 9/2005
 EP 0624346 B1 11/2005
 EP 1594209 A1 11/2005
 EP 1199044 B1 12/2005
 EP 1609428 A1 12/2005
 EP 1199043 B1 3/2006
 EP 1433425 B1 6/2006
 EP 1256323 B1 9/2006
 EP 1698289 A2 9/2006
 EP 1704824 A1 9/2006
 EP 1749479 A1 2/2007
 EP 1815950 A1 8/2007
 EP 1844720 A1 10/2007
 EP 1862133 A1 12/2007
 EP 1875875 A1 1/2008
 EP 1199045 B1 6/2008
 EP 1964530 A1 9/2008
 EP 1972264 A1 9/2008
 EP 1974771 A1 10/2008
 EP 1435852 B1 12/2008
 EP 1498082 B1 12/2008
 EP 1707131 B1 12/2008
 EP 1997438 A2 12/2008
 EP 1477104 B1 1/2009
 EP 2014218 A2 1/2009
 EP 2042112 A2 4/2009
 EP 1832259 B1 6/2009
 EP 2074959 A1 7/2009
 EP 2106758 A1 10/2009
 EP 2111813 A1 10/2009

EP 2200145 A1 6/2010
 EP 1214913 B1 7/2010
 EP 2238938 A1 10/2010
 EP 2298154 A2 3/2011
 EP 1510178 B1 6/2011
 EP 1946708 B1 6/2011
 EP 2305144 A1 6/2011
 EP 2335630 A1 6/2011
 EP 1502551 B1 7/2011
 EP 2361562 A1 8/2011
 EP 2365608 A2 9/2011
 EP 2420197 A2 2/2012
 EP 2422721 A2 2/2012
 EP 1927321 B1 4/2012
 EP 2510891 A1 10/2012
 EP 2316359 B1 3/2013
 EP 1586275 B1 5/2013
 EP 1616529 B1 9/2013
 EP 2583633 B1 10/2014
 EP 2113210 B1 3/2016
 EP 2227155 B1 7/2016
 EP 2859858 B1 12/2016
 GB 1482943 A 8/1977
 GB 2032221 A 4/1980
 GB 2317566 A 4/1998
 GB 2379878 B 11/2004
 GB 2447767 B 8/2011
 JP S 50-100891 A 8/1975
 JP S 59-68513 U 5/1984
 JP S 59141938 A 8/1984
 JP 62-221343 A 9/1987
 JP S 62-227343 A 10/1987
 JP 62-292153 A 12/1987
 JP S 62-292154 A 12/1987
 JP 63-109386 A 5/1988
 JP 63-315049 A 12/1988
 JP H 01-151452 A 6/1989
 JP H 01-198540 A 8/1989
 JP 02-71510 U 5/1990
 JP 2-286149 A 11/1990
 JP H 02-292193 A 12/1990
 JP H 03-37061 A 2/1991
 JP 04-25707 U 2/1992
 JP H 04-64351 A 2/1992
 JP 4-30508 U 3/1992
 JP H 04-150847 A 5/1992
 JP H 04-152942 A 5/1992
 JP 05-095955 A 4/1993
 JP H 05-115490 A 5/1993
 JP H 06-70938 A 3/1994
 JP 6-104503 A 4/1994
 JP 6-507081 A 8/1994
 JP H 06-217988 A 8/1994
 JP H 7-508910 A 10/1995
 JP 7-308323 A 11/1995
 JP 8-24266 A 1/1996
 JP 8-275951 A 10/1996
 JP H 08-299351 A 11/1996
 JP H 08-336545 A 12/1996
 JP H09-503146 A 3/1997
 JP H 09-135553 A 5/1997
 JP H 09-140722 A 6/1997
 JP H 10-5237 A 1/1998
 JP 10-295700 A 11/1998
 JP H 11-501543 A 2/1999
 JP H 11-128238 A 5/1999
 JP H 11-192235 A 7/1999
 JP 11-253451 A 9/1999
 JP H 11-318918 A 11/1999
 JP 2000-041991 A 2/2000
 JP 2000-070279 A 3/2000
 JP 2000-210299 A 8/2000
 JP 2000-271145 A 10/2000
 JP 2000-287987 A 10/2000
 JP 2001-029353 A 2/2001
 JP 2001-502216 A 2/2001
 JP 2001-309925 A 11/2001
 JP 2002-186901 A 7/2002
 JP 2002-204808 A 7/2002

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP 2002-238919 A 8/2002
 JP 2002-263579 A 9/2002
 JP 2002-301086 A 10/2002
 JP 2002-306504 A 10/2002
 JP 2002-330977 A 11/2002
 JP 2002-542690 A 12/2002
 JP 2003-000612 A 1/2003
 JP 2003-010201 A 1/2003
 JP 2003-510158 A 3/2003
 JP 2003-116870 A 4/2003
 JP 2003-126104 A 5/2003
 JP 2003-126110 A 5/2003
 JP 2003-310627 A 5/2003
 JP 2003-530921 A 10/2003
 JP 2003-339730 A 12/2003
 JP 2004-129871 A 4/2004
 JP 2004-147701 A 5/2004
 JP 2005027026 A 1/2005
 JP 2005-040222 A 2/2005
 JP 2005-066316 A 3/2005
 JP 2005-074088 A 3/2005
 JP 2005-534451 A 11/2005
 JP 2006-006410 A 1/2006
 JP 2006-512149 A 4/2006
 JP 2006-116194 A 5/2006
 JP 2006-158525 A 6/2006
 JP 2006-218296 A 8/2006
 JP 2006217716 A 8/2006
 JP 2006-288431 A 10/2006
 JP 2007-050181 A 3/2007
 JP 2007-229454 A 9/2007
 JP 2007-527747 A 10/2007
 JP 2008-036390 A 2/2008
 JP 2008-508065 A 3/2008
 JP 2008-119250 A 5/2008
 JP 2008-521503 A 6/2008
 JP D1339835 S 8/2008
 JP 2008-212679 A 9/2008
 JP 2008-536562 A 9/2008
 JP 2008-284374 A 11/2008
 JP 2009-511206 A 3/2009
 JP 2009-517181 A 4/2009
 JP 4262923 B2 5/2009
 JP 2009-523567 A 6/2009
 JP 2009-148557 A 7/2009
 JP 2009-236177 A 10/2009
 JP 2009-254819 A 11/2009
 JP 2010-000336 A 1/2010
 JP 2010-009686 A 1/2010
 JP 2010-514923 A 5/2010
 JP 2010-121865 A 6/2010
 JP 2010-534522 A 11/2010
 JP 2010-540186 A 12/2010
 JP 2011-505198 A 2/2011
 JP 2012-235658 A 11/2012
 JP 5208761 B2 6/2013
 JP 5714508 B2 5/2015
 JP 5836543 B1 12/2015
 RU 2154437 C1 8/2000
 RU 22035 U1 3/2002
 WO WO 92/22259 A2 12/1992
 WO WO 93/08757 A1 5/1993
 WO WO 93/14708 A1 8/1993
 WO WO 93/16646 A1 9/1993
 WO WO 93/20877 A1 10/1993
 WO WO 94/21183 A1 9/1994
 WO WO 94/24949 A1 11/1994
 WO WO 95/09572 A1 4/1995
 WO WO 95/34259 A1 12/1995
 WO WO 96/30885 A1 10/1996
 WO WO 96/39086 A1 12/1996
 WO WO 98/16156 A1 4/1998
 WO WO 98/26739 A1 6/1998
 WO WO 98/35621 A1 8/1998
 WO WO 98/37815 A1 9/1998

WO WO 98/47436 A1 10/1998
 WO WO 99/20213 A1 4/1999
 WO WO 99/52489 A1 10/1999
 WO WO 00/64358 A2 11/2000
 WO WO 00/74585 A2 12/2000
 WO WO 01/24713 A1 4/2001
 WO WO 01/54590 A1 8/2001
 WO WO 01/67970 A1 9/2001
 WO WO 01/95810 A2 12/2001
 WO WO 02/24080 A2 3/2002
 WO WO 02/38057 A1 5/2002
 WO WO 02/062241 A1 8/2002
 WO WO 03/082133 A1 10/2003
 WO WO 2004/012615 A1 2/2004
 WO WO 2004/026104 A2 4/2004
 WO WO 2004/032754 A2 4/2004
 WO WO 2004/032762 A1 4/2004
 WO WO 2004/032763 A2 4/2004
 WO WO 2004/037095 A2 5/2004
 WO WO 2004/060141 A2 7/2004
 WO WO 2004/098426 A1 11/2004
 WO WO 2004/112618 A2 12/2004
 WO WO 2005/117735 A1 12/2005
 WO WO 2005/122917 A1 12/2005
 WO WO 2006/012797 A1 2/2006
 WO WO 2006/042210 A2 4/2006
 WO WO 2006/058223 A2 6/2006
 WO WO 2006/063199 A2 6/2006
 WO WO 2006/083988 A1 8/2006
 WO WO 2006/101661 A2 9/2006
 WO WO 2006/119139 A2 11/2006
 WO WO 2006/119376 A2 11/2006
 WO WO 2006/129465 A1 12/2006
 WO WO 2007/008703 A2 1/2007
 WO WO 2007/008710 A2 1/2007
 WO WO 2007/038538 A1 4/2007
 WO WO 2007/040818 A1 4/2007
 WO WO 2007/047380 A2 4/2007
 WO WO 2007/047531 A2 4/2007
 WO WO 2007/056590 A1 5/2007
 WO WO 2007/087272 A2 8/2007
 WO WO 2007/089724 A2 8/2007
 WO WO 2007/143665 A2 12/2007
 WO WO 2008/016886 A2 2/2008
 WO WO 2008/042021 A1 4/2008
 WO WO 2008/049084 A2 4/2008
 WO WO 2008/051764 A2 5/2008
 WO WO 2008/089174 A2 7/2008
 WO WO 2008/118709 A1 10/2008
 WO WO 2008/130793 A1 10/2008
 WO WO 2009/010565 A1 1/2009
 WO WO 2009/018067 A1 2/2009
 WO WO 2009/018406 A2 2/2009
 WO WO 2009/027065 A1 3/2009
 WO WO 2009/046234 A2 4/2009
 WO WO 2009/073402 A2 6/2009
 WO WO 2009/120992 A2 10/2009
 WO WO 2009/141616 A1 11/2009
 WO WO 2010/017149 A1 2/2010
 WO WO 2010/068783 A1 6/2010
 WO WO 2011/008672 A2 1/2011
 WO WO 2011/052939 A2 5/2011
 WO WO 2011/100321 A2 8/2011
 WO WO 2011/144911 A1 11/2011
 WO WO 2012/061722 A2 5/2012
 WO WO 2012/128362 A1 9/2012
 WO WO 2012/135705 A1 10/2012
 WO WO 2012/135721 A1 10/2012
 WO WO 2013/018934 A1 2/2013
 WO WO 2013/062978 A2 5/2013
 WO WO 2014/092108 A1 6/2014
 WO WO 2016/009921 A1 12/2016

OTHER PUBLICATIONS

Sherrit et al., "Novel Horn Designs for Ultrasonic/Sonic Cleaning Welding, Soldering, Cutting and Drilling," Proc. SPIE Smart Struc-

(56)

References Cited

OTHER PUBLICATIONS

tures Conference, vol. 4701, Paper No. 34, San Diego, CA, pp. 353-360, Mar. 2002.

AST Products, Inc., "Principles of Video Contact Angle Analysis," 20 pages, (2006).

Lim et al., "A Review of Mechanism Used in Laparoscopic Surgical Instruments," *Mechanism and Machine Theory*, vol. 38, pp. 1133-1147, (2003).

Gooch et al., "Recommended Infection-Control Practices for Dentistry, 1993," Published: May 28, 1993; [retrieved on Aug. 23, 2008]. Retrieved from the internet: URL: <http://wonder.cdc.gov/wonder/prevguid/p0000191/p0000191.asp> (15 pages).

Huston et al., "Magnetic and Magnetostrictive Properties of Cube Textured Nickel for Magnetostrictive Transducer Applications," *IEEE Transactions on Magnetics*, vol. 9(4), pp. 636-640 (Dec. 1973).

Incropera et al., "Fundamentals of Heat and Mass Transfer", Wiley, New York (1990). (Book—not attached).

F. A. Duck, "Optical Properties of Tissue Including Ultraviolet and Infrared Radiation," pp. 43-71 in *Physical Properties of Tissue* (1990).

Orr et al., "Overview of Bioheat Transfer," pp. 367-384 in *Optical-Thermal Response of Laser-Irradiated Tissue*, A. J. Welch and M. J. C. van Gernert, eds., Plenum, New York (1995).

Campbell et al., "Thermal Imaging in Surgery," p. 19-3, in *Medical Infrared Imaging*, N. A. Diakides and J. D. Bronzino, Eds. (2008).

Sullivan, "Cost-Constrained Selection of Strand Diameter and Number in a Litz-Wire Transformer Winding," *IEEE Transactions on Power Electronics*, vol. 16, No. 2, Mar. 2001, pp. 281-288.

Sullivan, "Optimal Choice for Number of Strands in a Litz-Wire Transformer Winding," *IEEE Transactions on Power Electronics*, vol. 14, No. 2, Mar. 1999, pp. 283-291.

Graff, K.F., "Elastic Wave Propagation in a Curved Sonic Transmission Line," *IEEE Transactions on Sonics and Ultrasonics*, SU-17(1), 1-6 (1970).

Makarov, S. N., Ochmann, M., Desinger, K., "The longitudinal vibration response of a curved fiber used for laser ultrasound surgical therapy," *Journal of the Acoustical Society of America* 102, 1191-1199 (1997).

Morley, L. S. D., "Elastic Waves in a Naturally Curved Rod," *Quarterly Journal of Mechanics and Applied Mathematics*, 14: 155-172 (1961).

Walsh, S. J., White, R. G., "Vibrational Power Transmission in Curved Beams," *Journal of Sound and Vibration*, 233(3), 455-488 (2000).

<http://www.apicalinstr.com/generators.htm>.

<http://www.dotmed.com/listing/electrosurgical-unit/ethicon/ultracision-g110-/1466724>.

<http://www.ethicon.com/gb-en/healthcare-professionals/products/energy-devices/capital/ge...>

<http://www.4-traders.com/JOHNSON-JOHNSON-4832/news/Johnson-Johnson-Ethicon-E...>

<http://www.medicalexpo.com/medical-manufacturer/electrosurgical-generator-6951.html>.

http://www.megadyne.com/es_generator.php.

<http://www.valleylab.com/product/es/generators/index.html>.

Covidien 501(k) Summary Sublicense, dated Feb. 24, 2011 (7 pages).

Gerhard, Glen C., "Surgical Electrotechnology: Quo Vadis?," *IEEE Transactions on Biomedical Engineering*, vol. BME-31, No. 12, pp. 787-792, Dec. 1984.

Fowler, K.R., "A Programmable, Arbitrary Waveform Electrosurgical Device," *IEEE Engineering in Medicine and Biology Society 10th Annual International Conference*, pp. 1324, 1325 (1988).

LaCourse, J.R.; Vogt, M.C.; Miller, W.T., III; Selikowitz, S.M., "Spectral Analysis Interpretation of Electrosurgical Generator Nerve and Muscle Stimulation," *IEEE Transactions on Biomedical Engineering*, vol. 35, No. 7, pp. 505-509, Jul. 1988.

U.S. Appl. No. 13/751,680, filed Jan. 28, 2013.

International Search Report for PCT/US2011/024180, dated Apr. 12, 2011 included in the PCT Publication for WO 2011/100313 A1 (73 pages).

International Preliminary Report on Patentability for PCT/US2011/024180, dated Aug. 14, 2012 (7 pages).

* cited by examiner

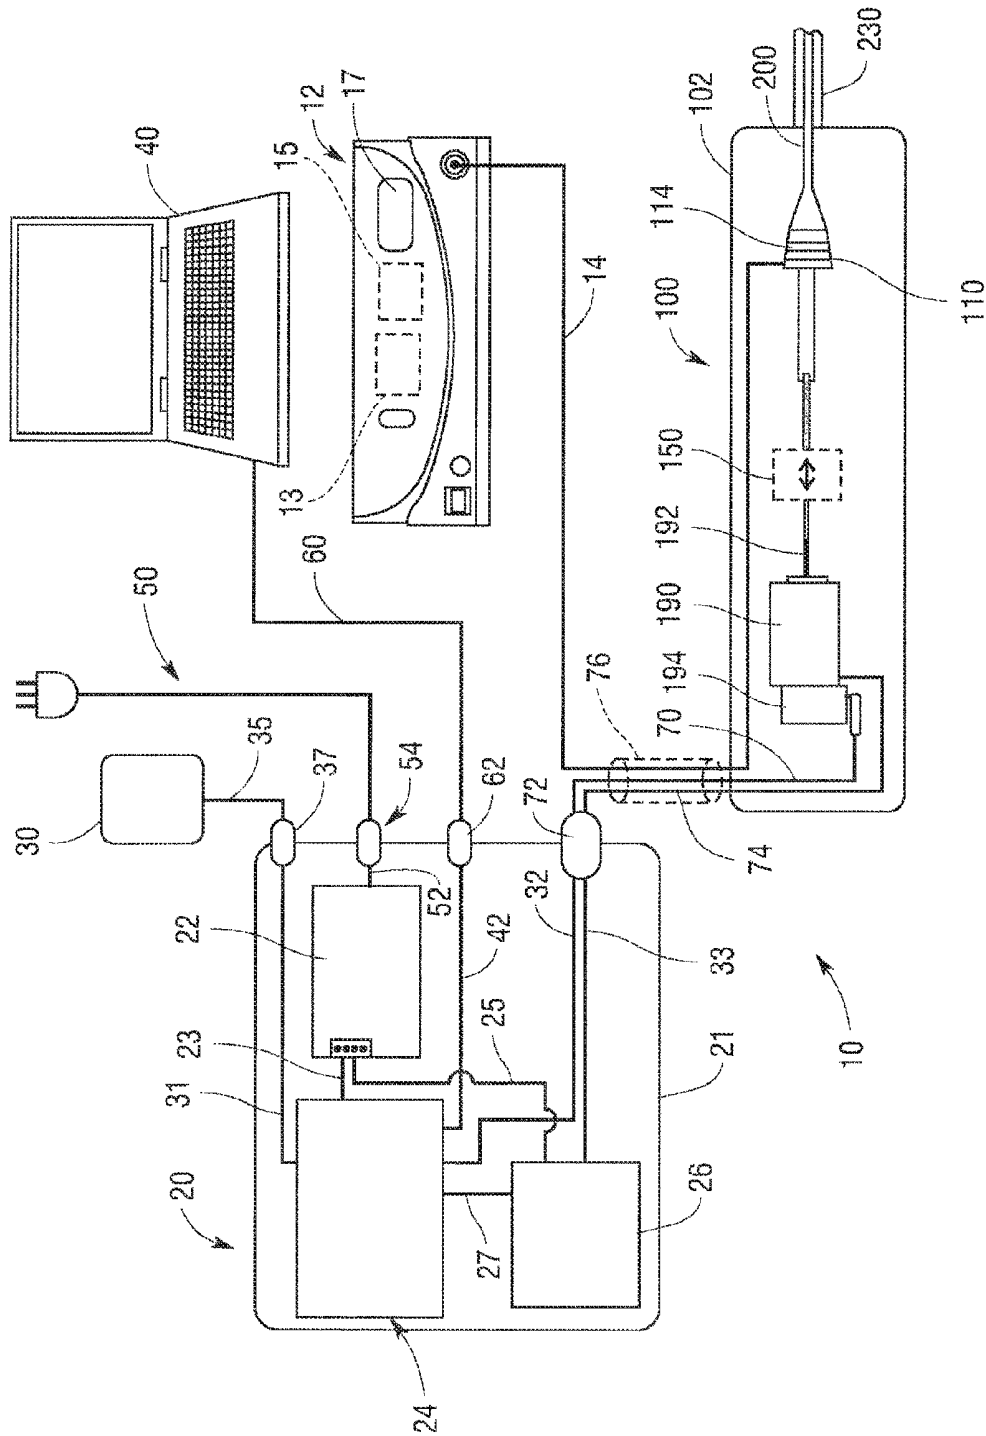


Fig. 1

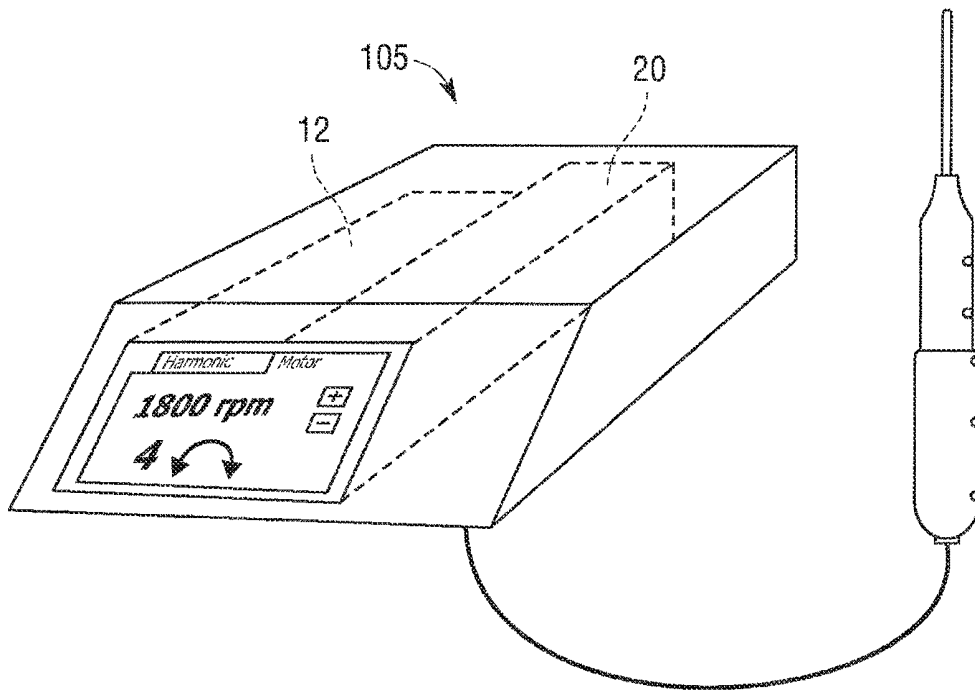


Fig. 1A

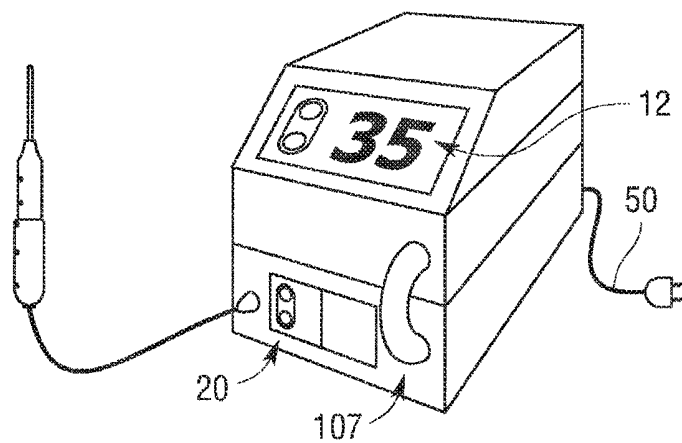


Fig. 1B

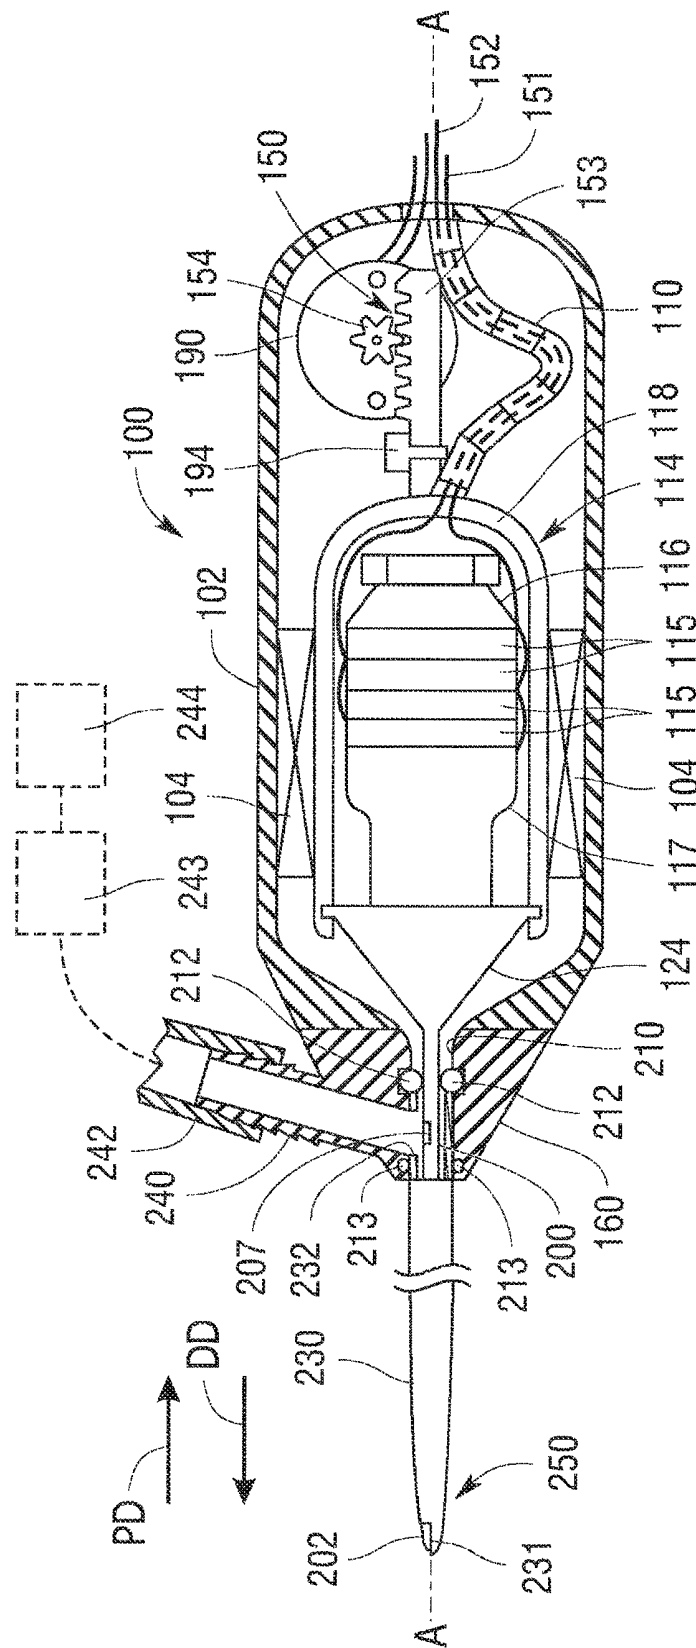


Fig. 2

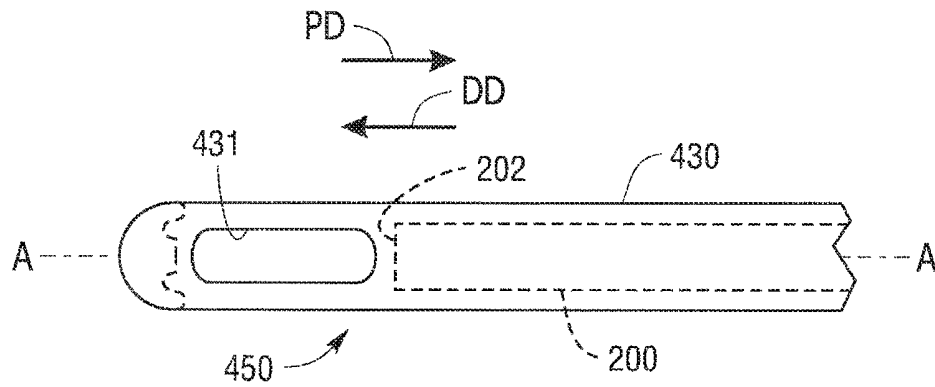


Fig. 3

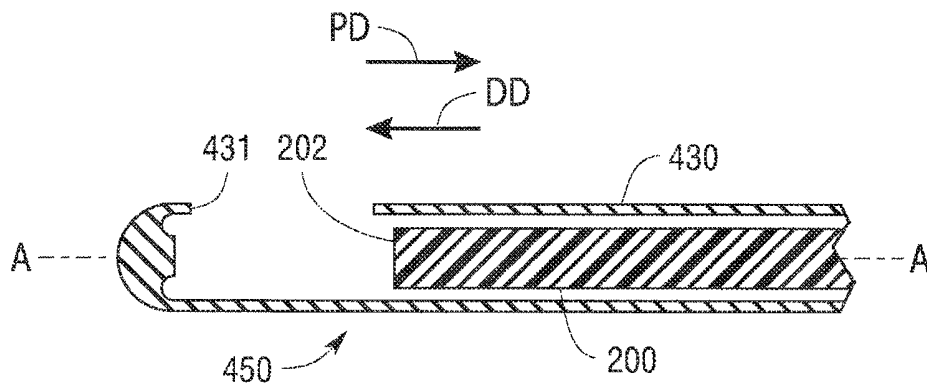


Fig. 4

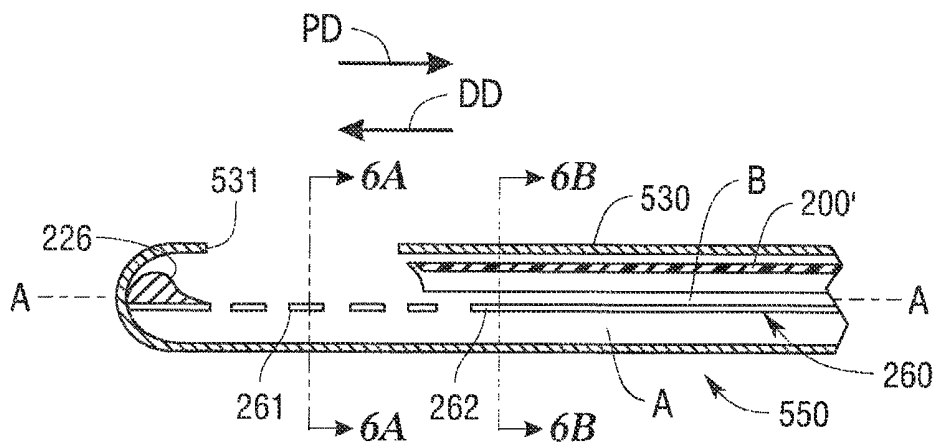


Fig. 5

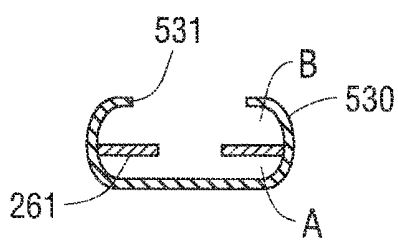


Fig. 6A

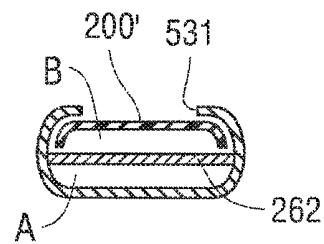
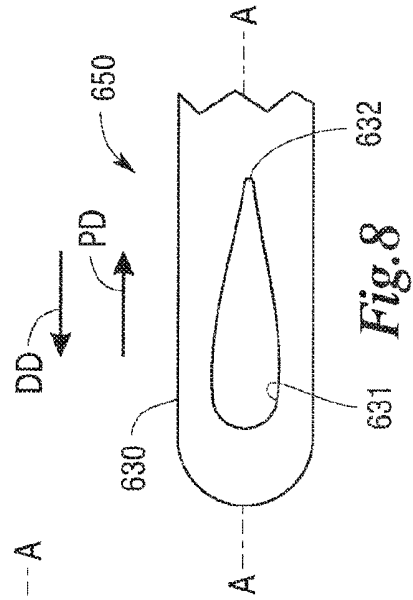
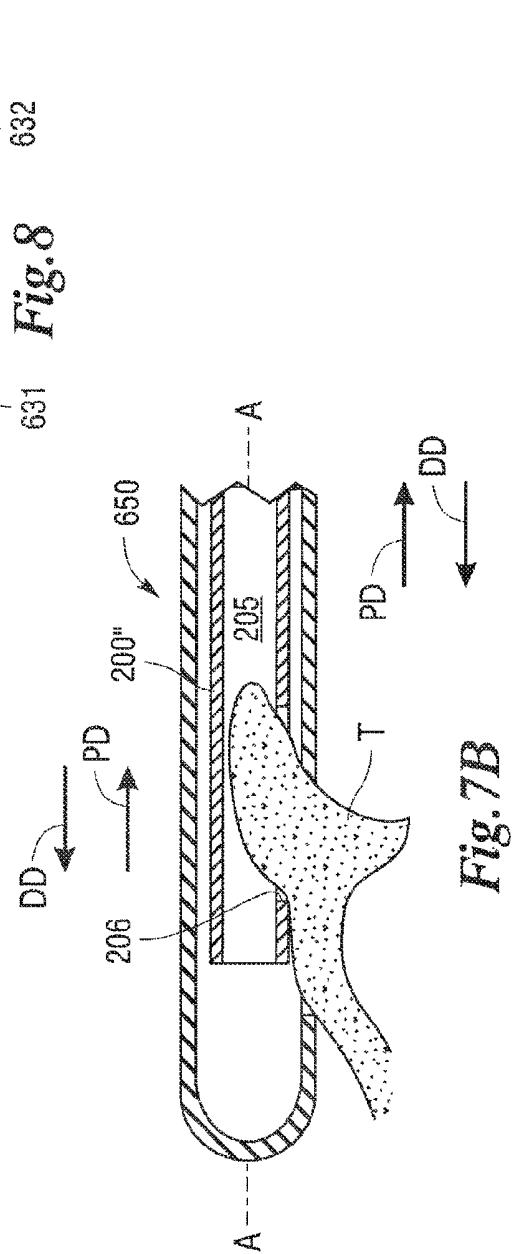
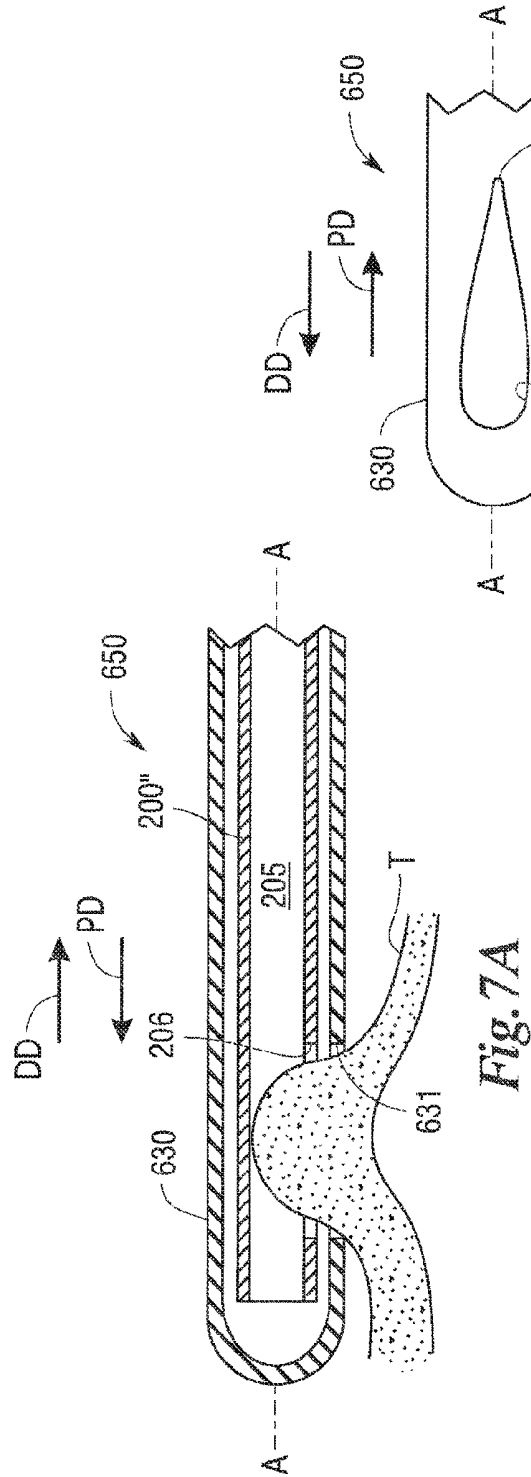
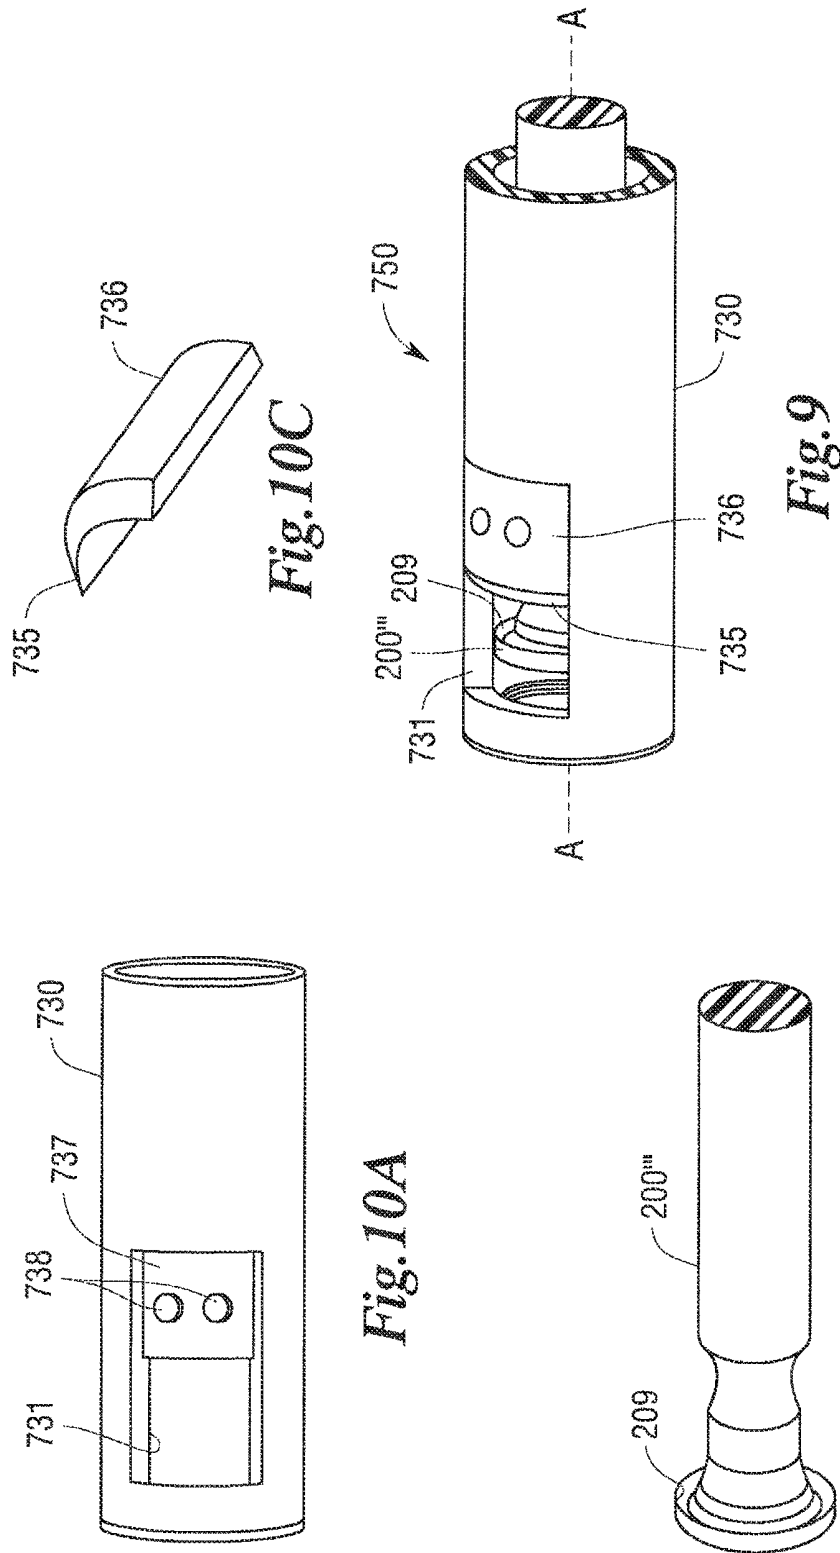


Fig. 6B





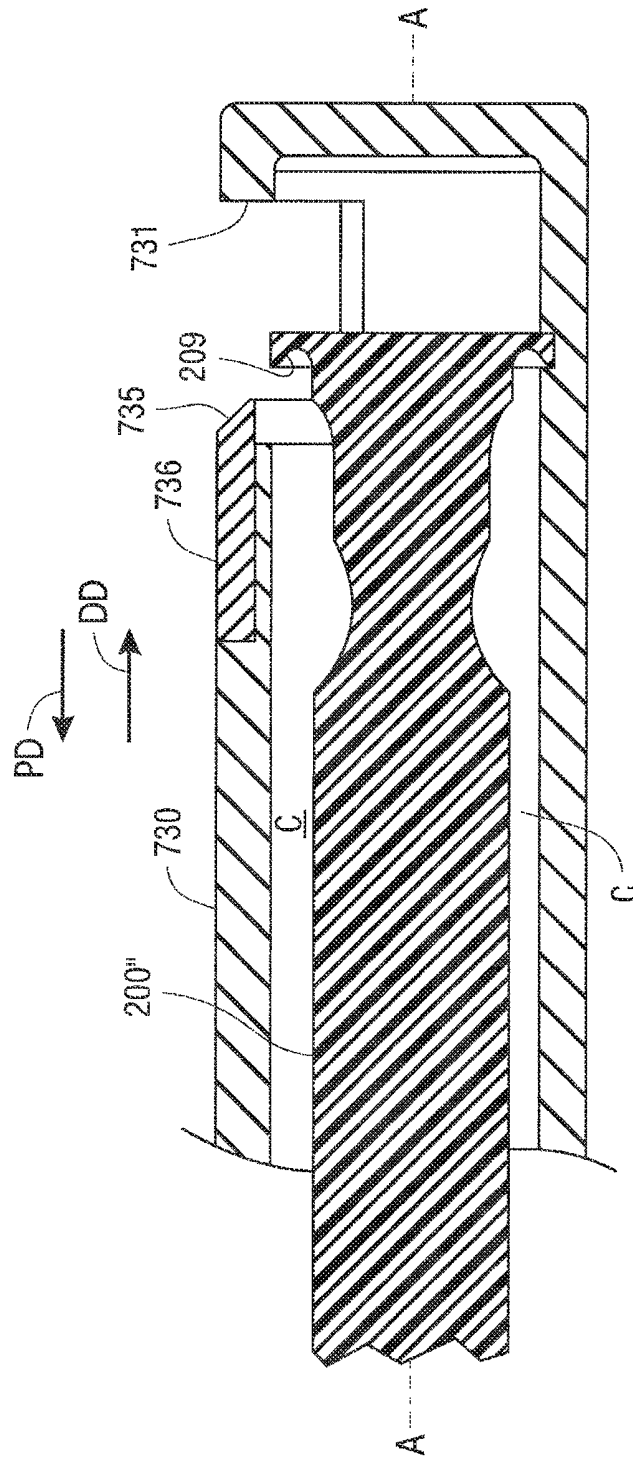


Fig. 11

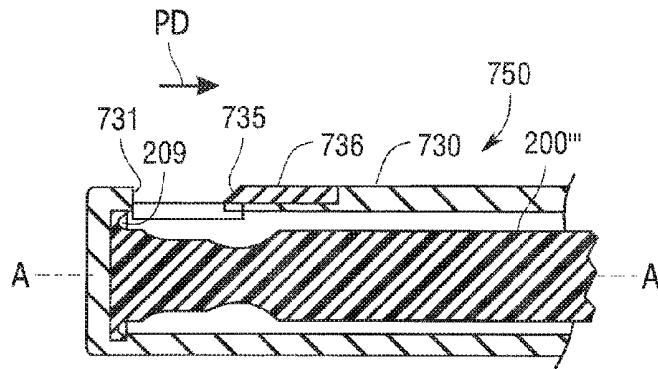


Fig. 12A

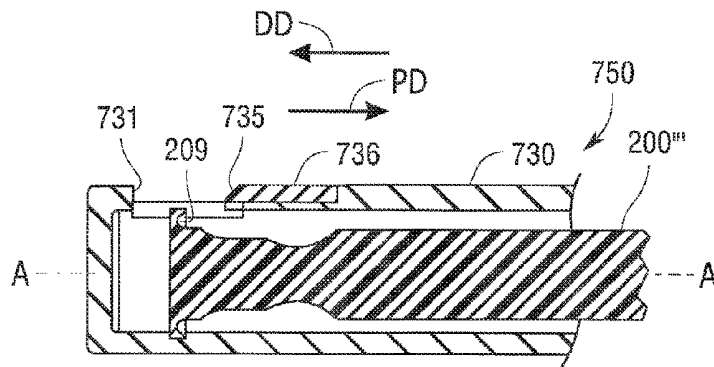


Fig. 12B

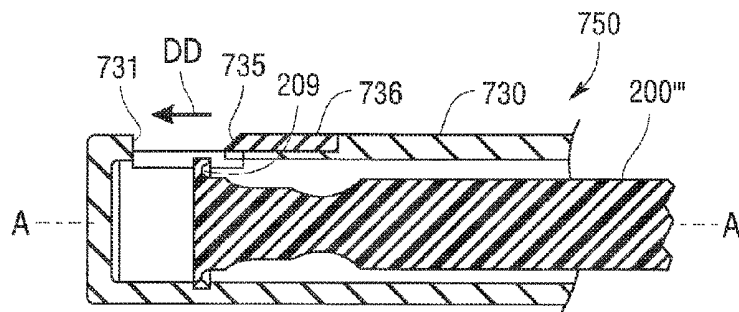
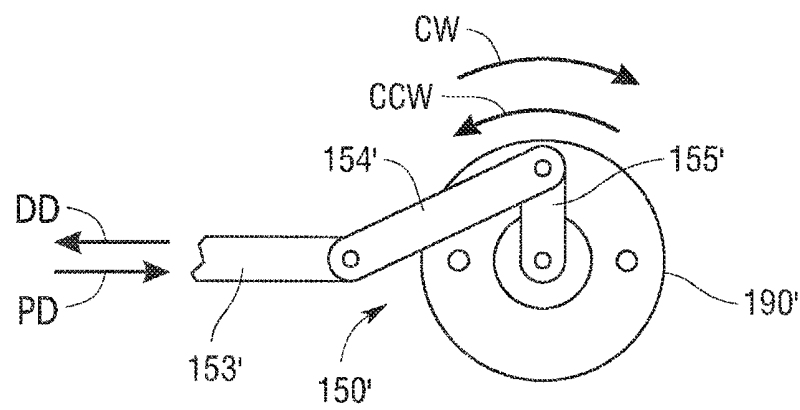


Fig. 12C

*Fig. 13*

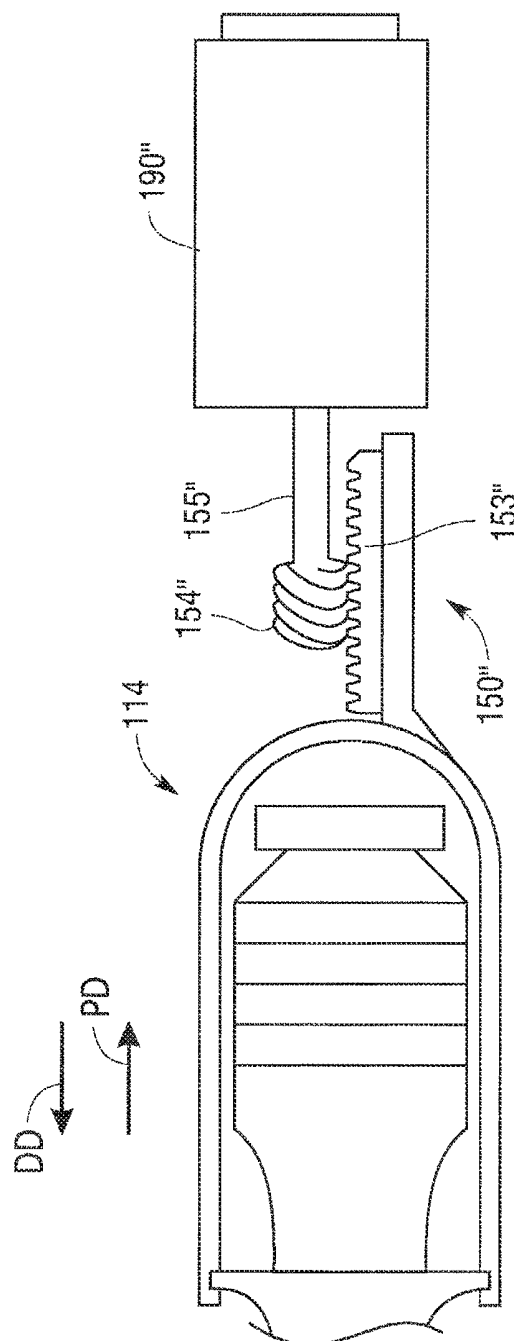
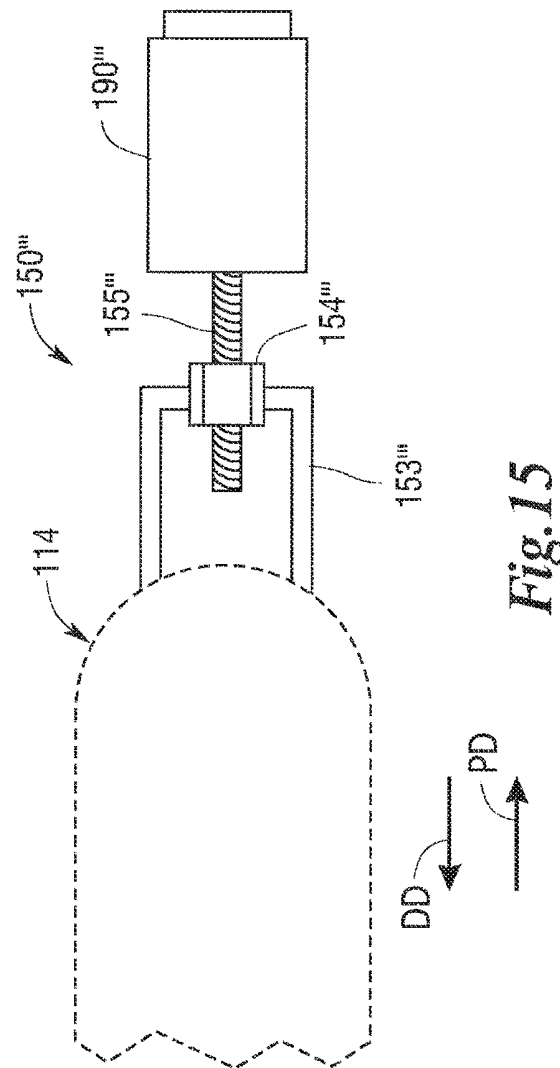
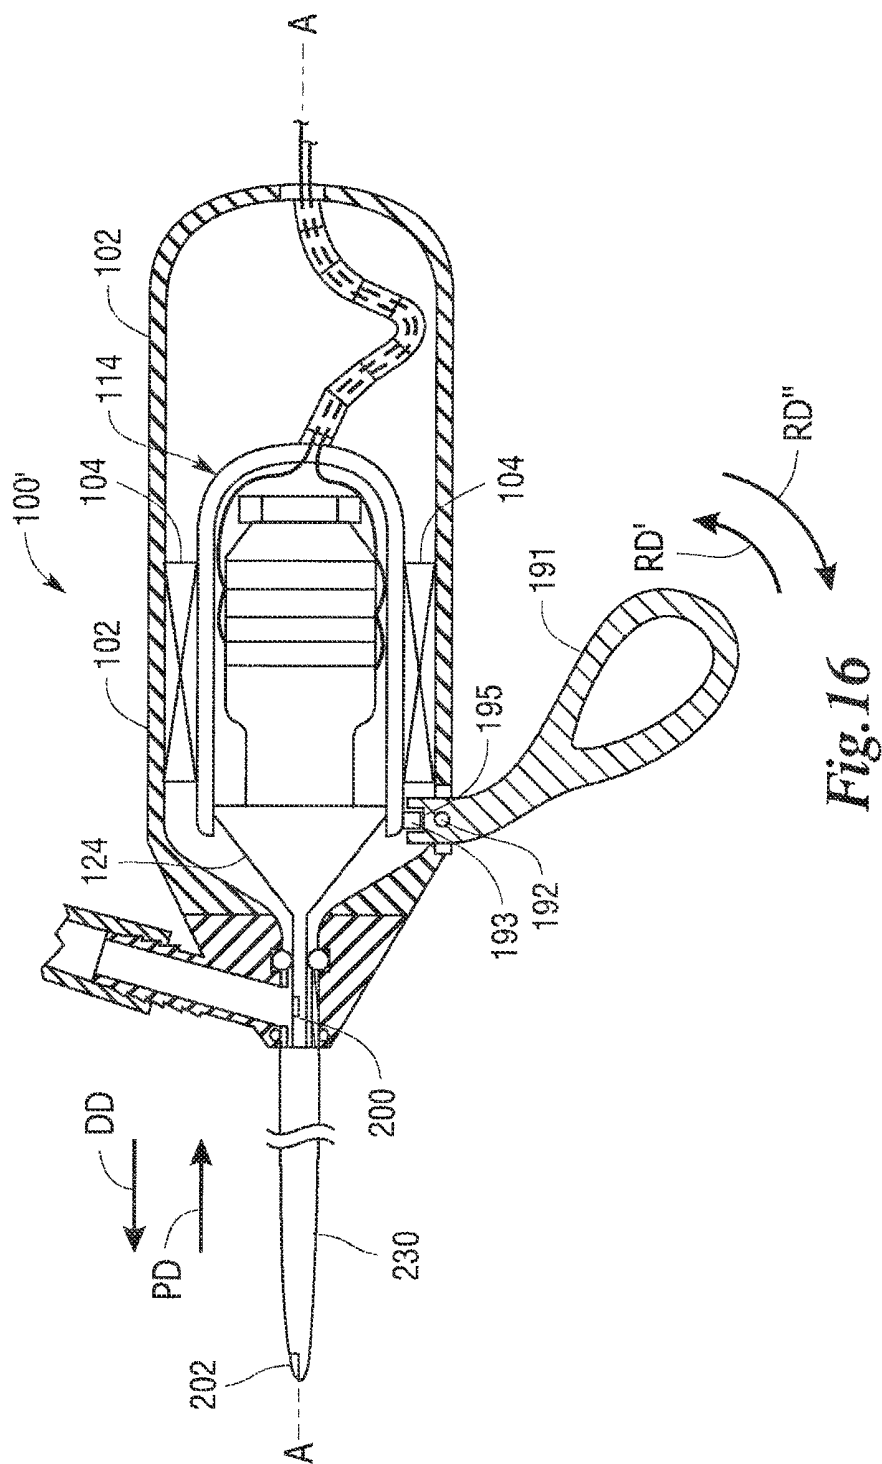
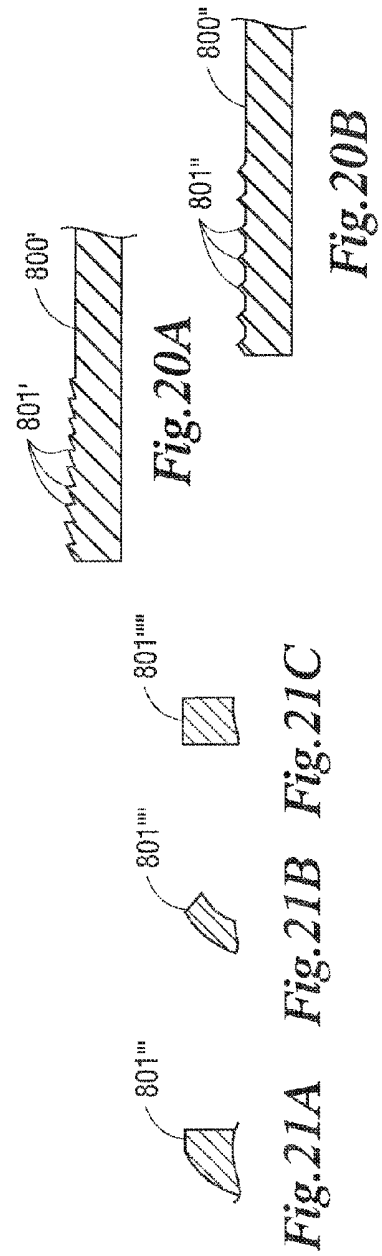
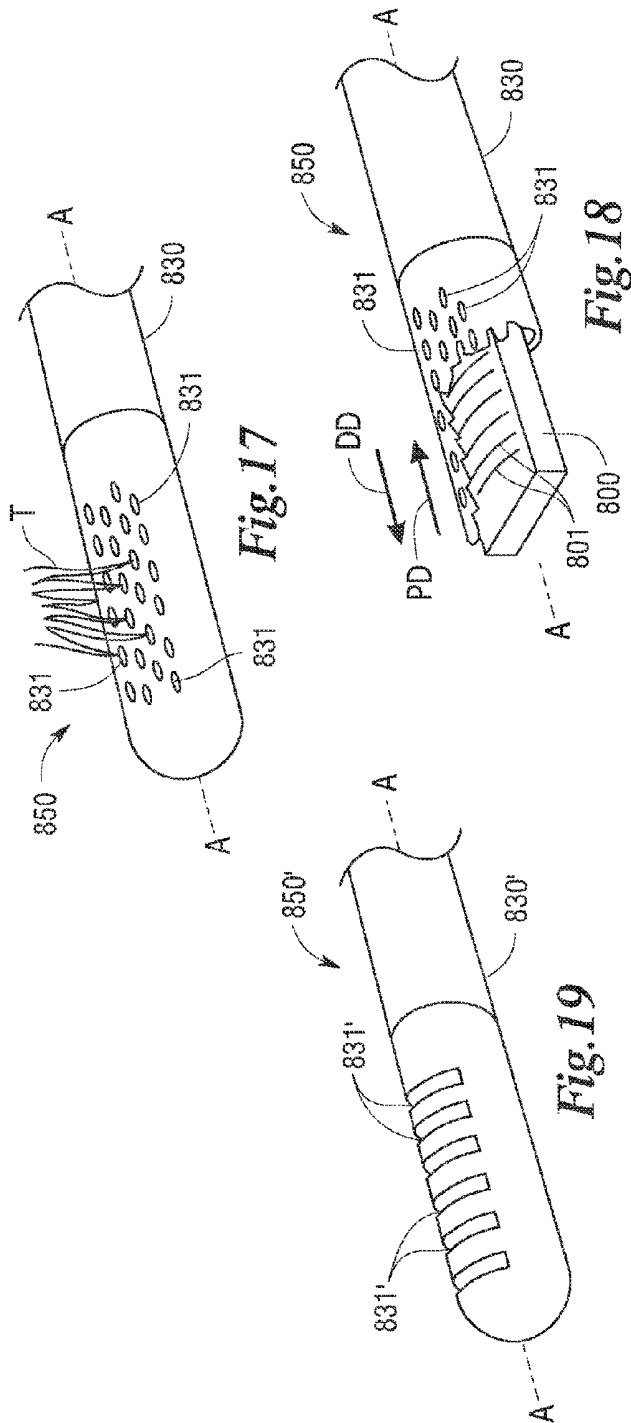


Fig. 14







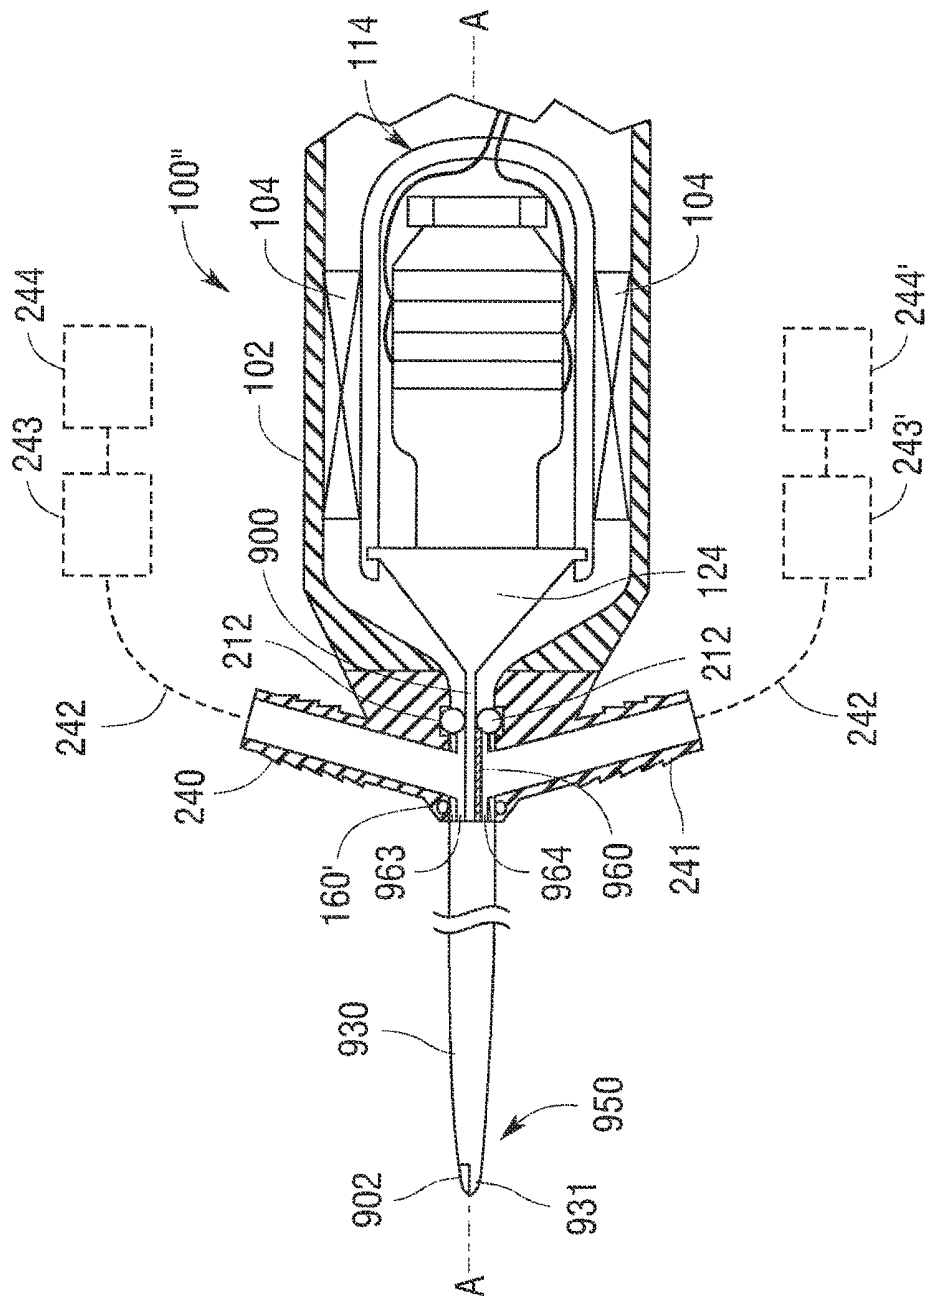
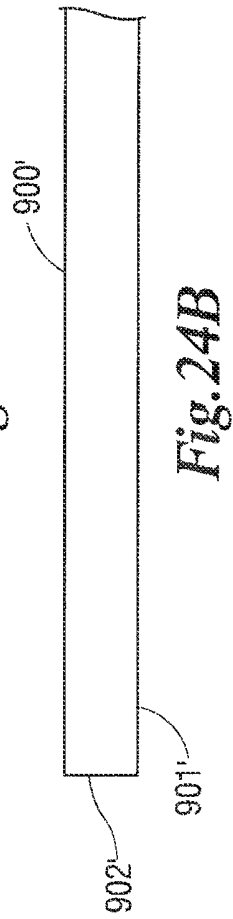
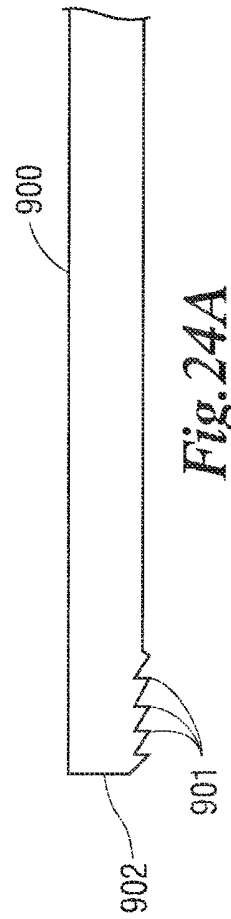
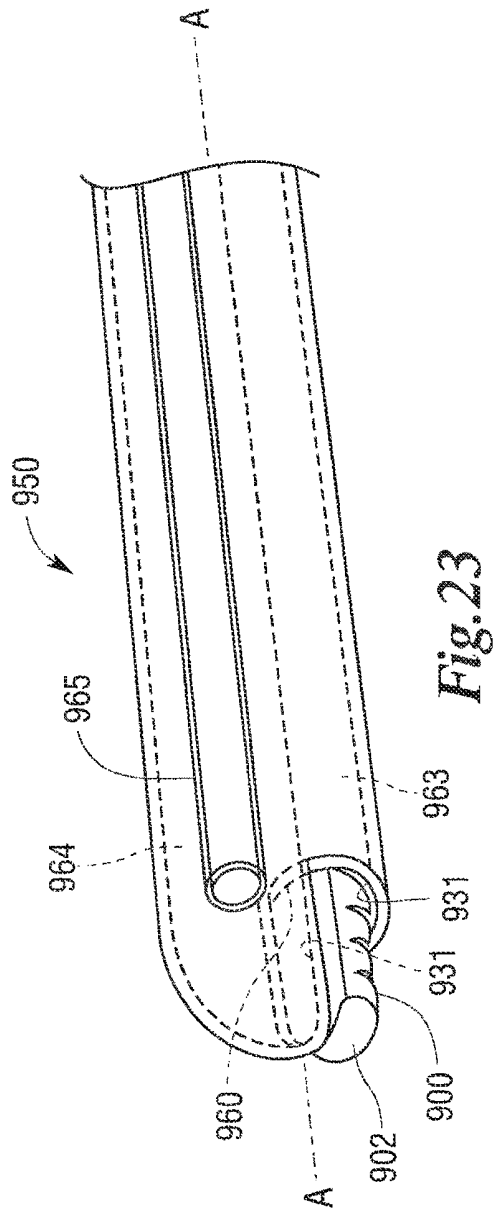


Fig. 22



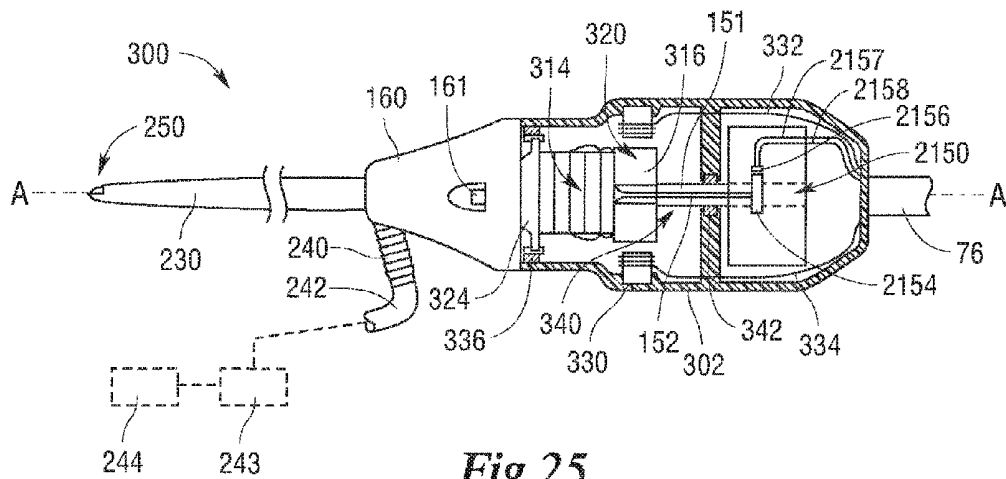


Fig. 25

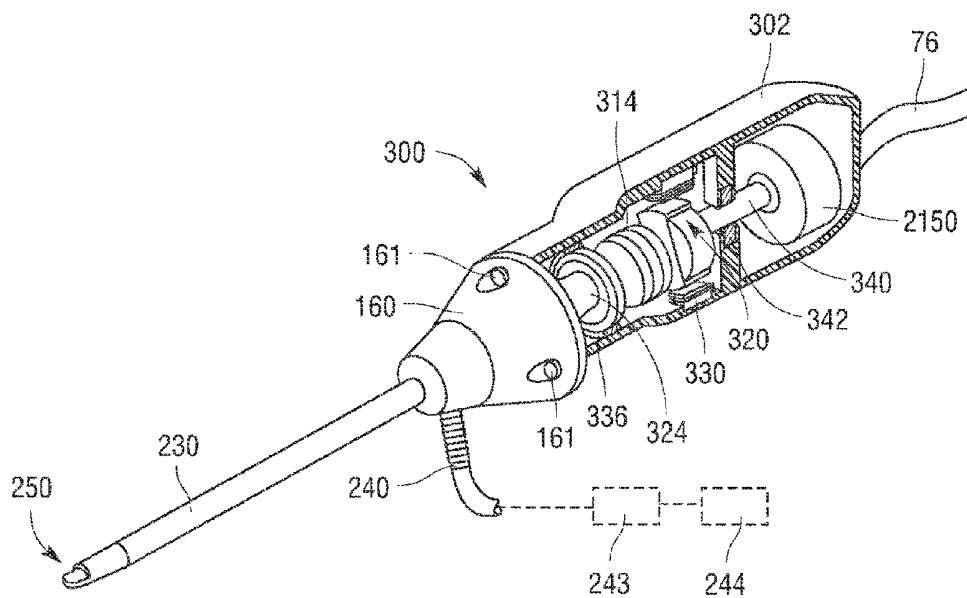


Fig. 26

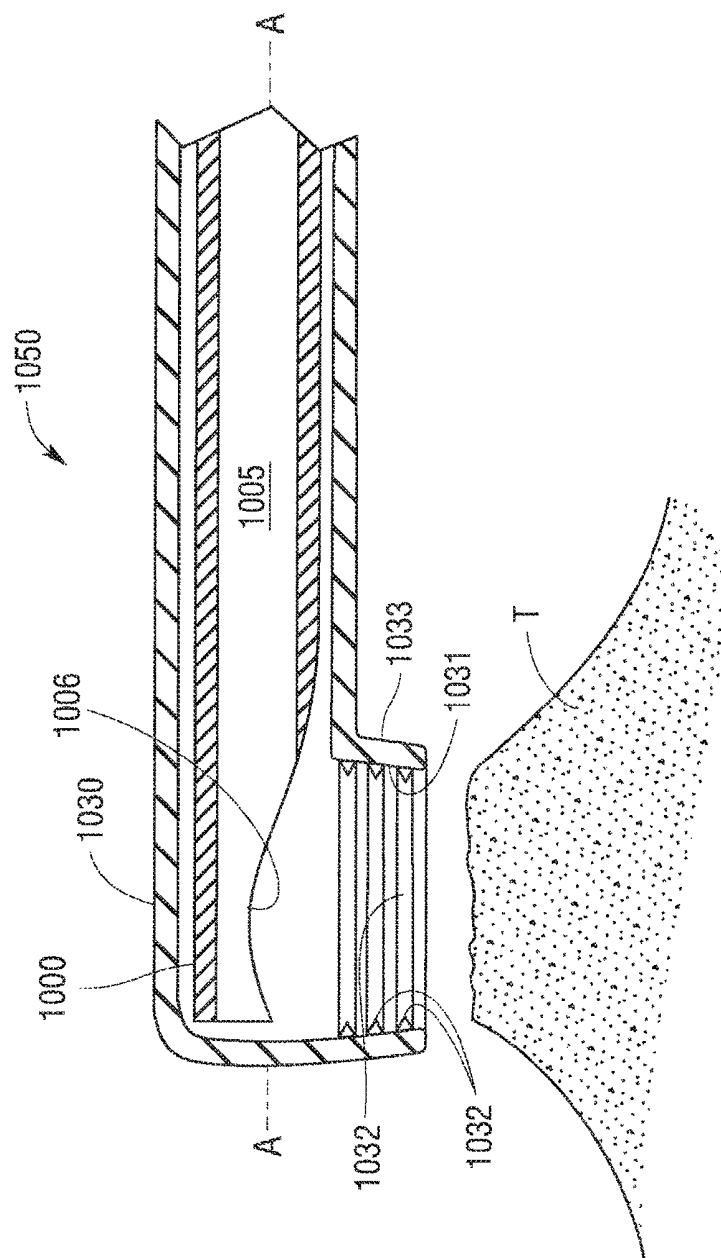


Fig. 27




Fig. 28




Fig. 29

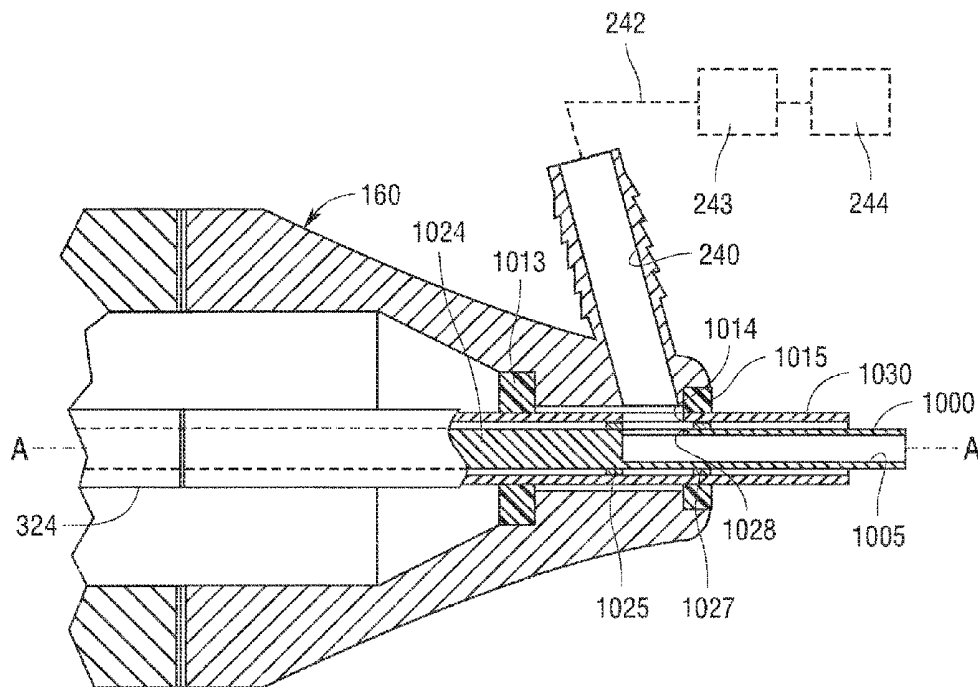


Fig.30

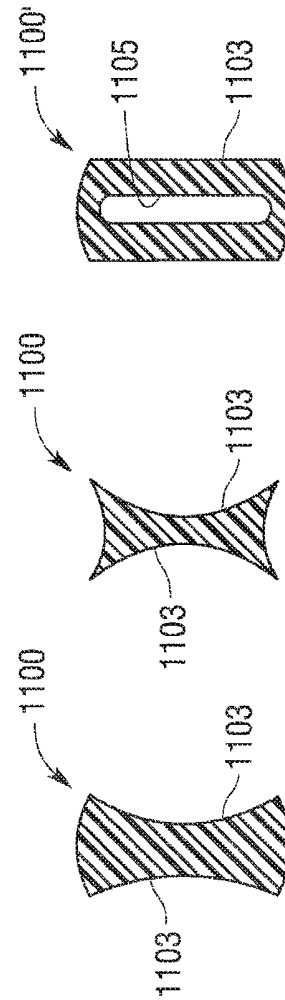
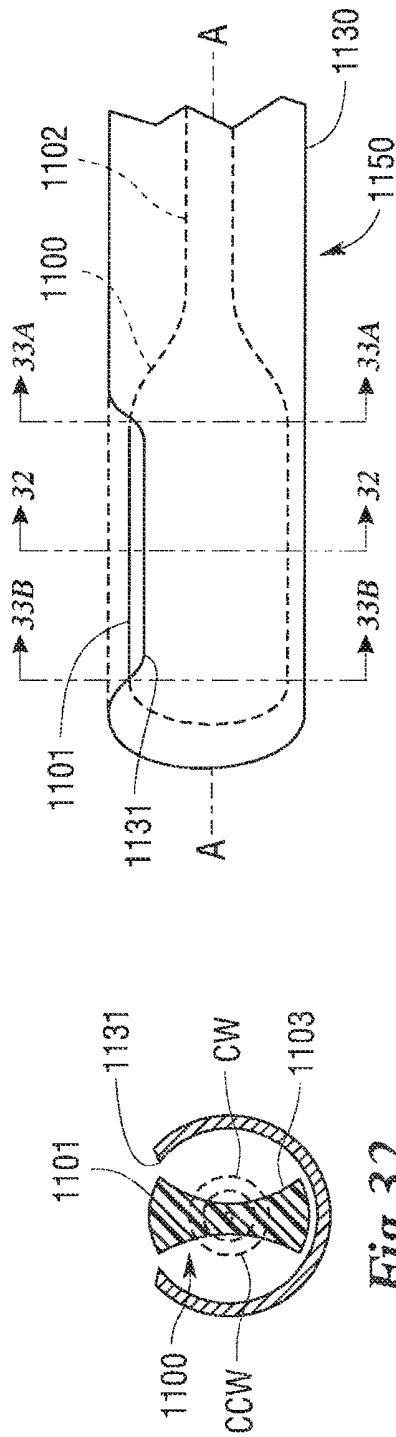
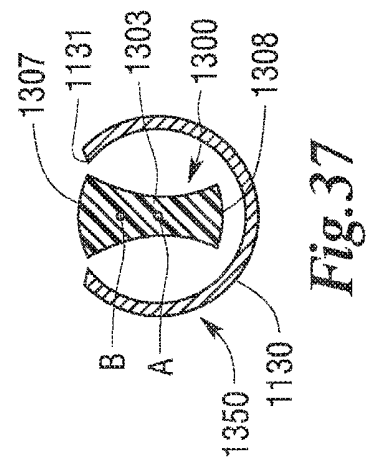
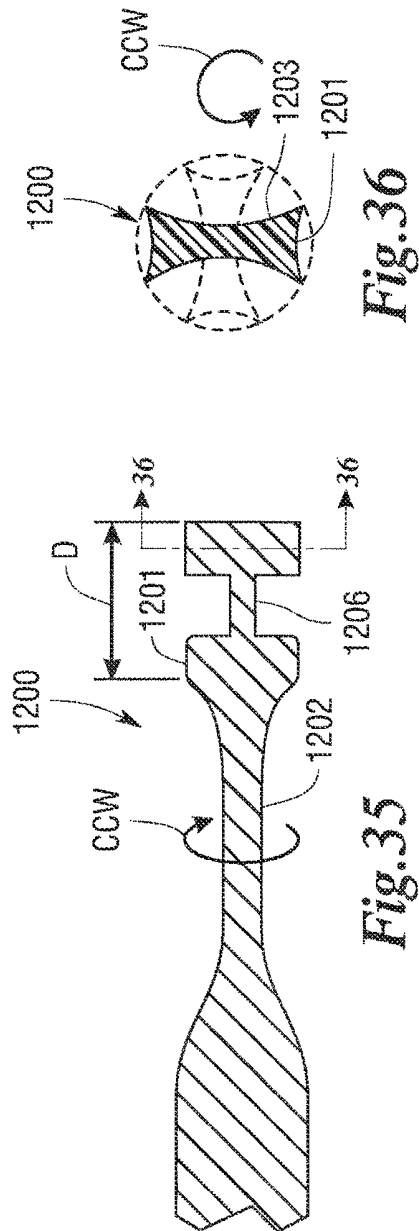


Fig. 34

Fig. 33B

Fig. 33A



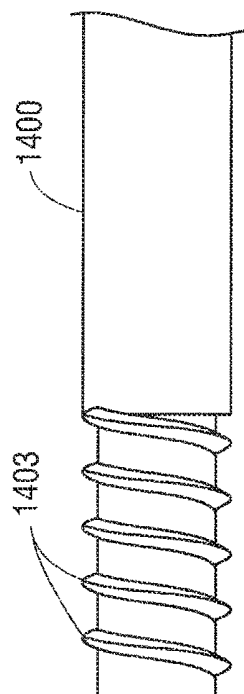


Fig. 39

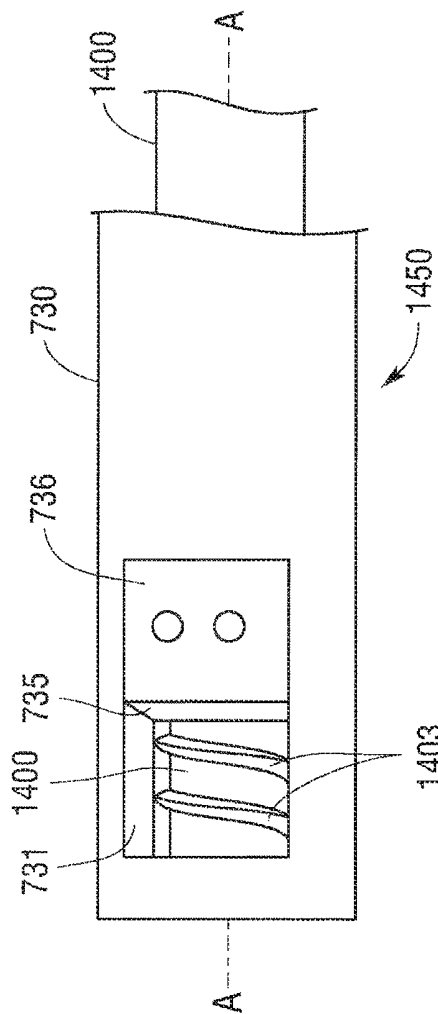


Fig. 38

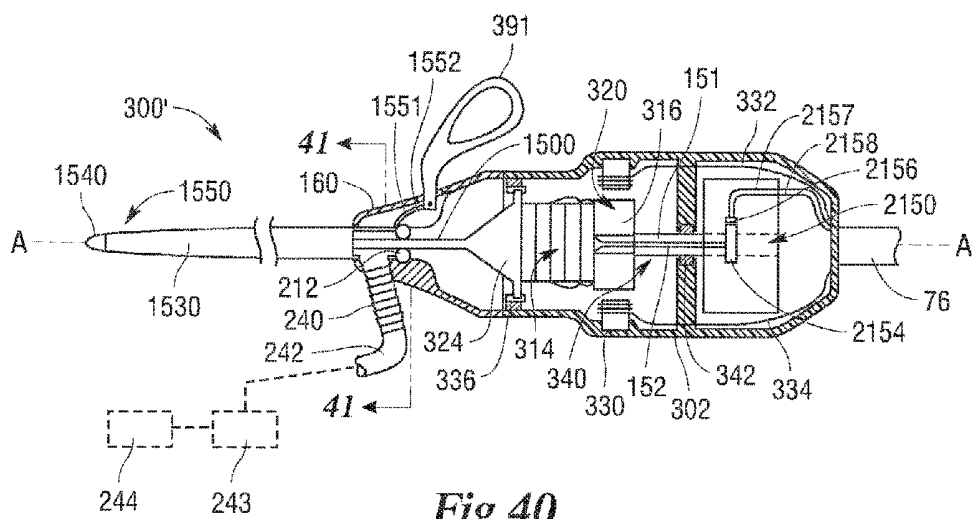


Fig. 40




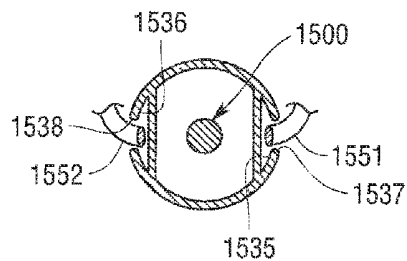


Fig. 41

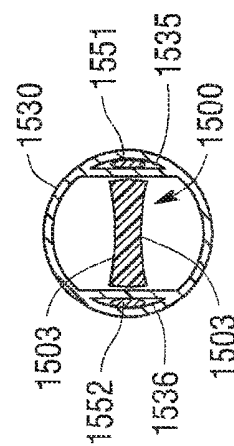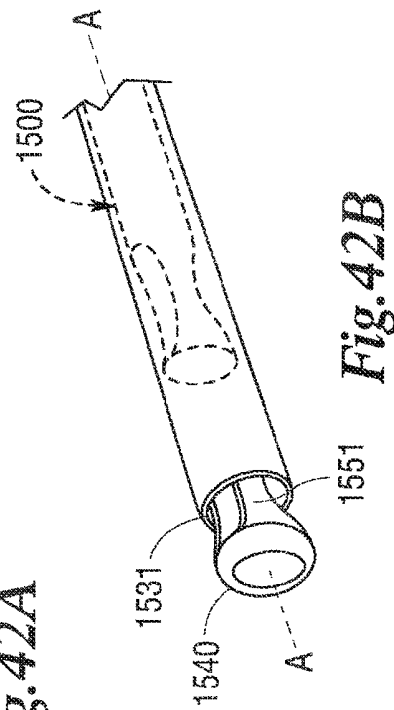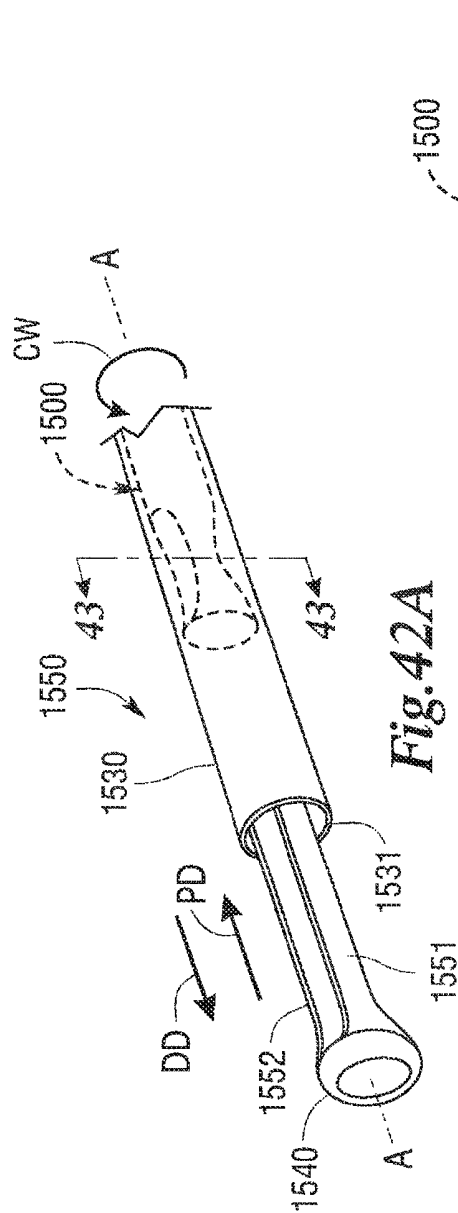

ULTRASONIC SURGICAL INSTRUMENTS WITH MOVING CUTTING IMPLEMENT

CROSS REFERENCE TO RELATED APPLICATIONS

This application is a divisional application claiming priority under 35 U.S.C. § 121 to U.S. patent application Ser. No. 12/703,893, entitled ULTRASONIC SURGICAL INSTRUMENTS WITH MOVING CUTTING IMPLEMENT, filed Feb. 11, 2010, now U.S. Pat. No. 9,259,234, the entire disclosure of which is hereby incorporated by reference herein.

BACKGROUND

The present disclosure generally relates to ultrasonic surgical systems and, more particularly, to ultrasonic systems that allow surgeons to perform cutting and coagulation of tissue.

Over the years, a variety of different types of non-ultrasonically powered cutters and shaving devices for performing surgical procedures have been developed. Some of these devices employ a rotary cutting instrument and other devices employ a reciprocating cutting member. For example, shavers are widely used in arthroscopic surgery. Arthroscopic surgery involves performing surgery in the joint space. To perform the surgery, the joints are commonly filled with pressurized saline for distention and visualization.

The aforementioned devices generally consist of a power supply, a handpiece, and a single-use end effector. The end effector commonly has an inner and outer tube. The inner tube rotates relative to the outer tube and will cut tissue with its sharpened edges. The inner tube can rotate continuously or oscillate. In addition, such device may employ a suction channel that travels through the interior of the inner tube. For example, U.S. Pat. No. 4,850,354 to McGurk-Burleson, et al., discloses a non-ultrasonically powered surgical cutting instrument that comprises a rotary cutter for cutting material with a shearing action. It employs an inner cutting member which is rotatable within an outer tube.

U.S. Pat. No. 3,776,238 to Peyman et al. discloses an ophthalmic instrument in which tissue is cut by a chopping action set-up by the sharp end of an inner tube moving against the inner surface of the end of an outer tube. U.S. Pat. No. 5,226,910 to Kajiyama et al. discloses another surgical cutting instrument that has an inner member which moves relative to an outer member to cut tissue entering through an aperture in the outer member.

U.S. Pat. No. 4,922,902 to Wuchinich et al. discloses a method and apparatus for endoscopic removal of tissue utilizing an ultrasonic aspirator. The device uses an ultrasonic probe which disintegrates compliant tissue and aspirates it through a narrow orifice. U.S. Pat. No. 4,634,420 to Spinoso et al. discloses an apparatus and method for removing tissue from an animal and includes an elongated instrument having a needle or probe, which is vibrated at an ultrasonic frequency in the lateral direction. The ultrasonic movement of the needle breaks-up the tissue into fragments. Pieces of tissue can be removed from the area of treatment by aspiration through a conduit in the needle. U.S. Pat. No. 3,805,787 to Banko discloses yet another ultrasonic instrument that has a probe that is shielded to narrow the beam of ultrasonic energy radiated from the tip of the probe. In one embodiment the shield extends past the free-end of the probe to prevent the probe from coming into contact with the

tissue. U.S. Pat. No. 5,213,569 to Davis discloses a phaco-emulsification needle which focuses the ultrasonic energy. The focusing surfaces can be beveled, curved or faceted. U.S. Pat. No. 6,984,220 to Wuchinich and U.S. Patent Publication No. U.S. 2005/0177184 to Easley disclose ultrasonic tissue dissection systems that provide combined longitudinal and torsional motion through the use of longitudinal-torsional resonators. U.S. Patent Publication No. U.S. 2006/0030797 A1 to Zhou et al. discloses an orthopedic surgical device that has a driving motor for driving an ultrasound transducer and horn. An adapter is provided between the driving motor and transducer for supplying ultrasonic energy signals to the transducer.

While the use of ultrasonically powered surgical instruments provide several advantages over traditional mechanically powered saws, drills, and other instruments, temperature rise in bone and adjacent tissue due to frictional heating at the bone/tissue interface can still be a significant problem. Current arthroscopic surgical tools include punches, reciprocating shavers and radio frequency (RF) devices. Mechanical devices such as punches and shavers create minimal tissue damage, but can sometimes leave behind ragged cut lines, which are undesirable. RF devices can create smoother cut lines and also ablate large volumes of soft tissue; however, they tend to create more tissue damage than mechanical means. Thus, devices which could provide increased cutting precision while forming smooth cutting surfaces without creating excessive tissue damage would be desirable.

The foregoing discussion is intended only to illustrate the present field and should not be taken as a disavowal of claim scope.

SUMMARY

In various embodiments, a surgical instrument is provided. In at least one embodiment, the surgical instrument can comprise a hollow sheath, a blade disposed at least partially within the hollow sheath, at least one ultrasonic transducer operably coupled to the blade, and a drive system. In these embodiments, the drive system can communicate with the transducer to deliver axial motions to the blade such that the blade translates with respect to the hollow sheath when the drive system is activated.

In at least one embodiment, a surgical instrument is provided that can comprise a hollow sheath, a blade disposed at least partially within the hollow sheath, at least one ultrasonic transducer coupled to the blade, and a drive system. In these embodiments, the drive system can communicate with the transducer to deliver rotational motions to the blade such that the blade rotates with respect to the hollow sheath when the drive system is activated. Further, in these embodiments, the hollow sheath can include at least one opening therein and at least one tooth positioned in the opening. Moreover, in these embodiments, the tooth can be configured to grip tissue positioned within the opening.

In at least one embodiment, a surgical instrument is provided that can comprise a hollow sheath including at least one opening therein, a blade disposed at least partially within the hollow sheath, an ultrasonic transducer coupled to the blade, a tissue gripping member movably supported by the hollow shaft, and a drive system coupled to the tissue gripping member. In these embodiments, the drive system can be configured to deliver axial motions to the tissue

gripping member such that the tissue gripping member translates with respect to the hollow sheath when the drive system is activated.

BRIEF DESCRIPTION OF THE FIGURES

The novel features of the embodiments described herein are set forth with particularity in the appended claims. The embodiments, however, both as to organization and methods of operation may be better understood by reference to the following description, taken in conjunction with the accompanying drawings as follows.

FIG. 1 is a schematic view of a non-limiting embodiment of a surgical control system embodiment.

FIG. 1A is a perspective view of a non-limiting embodiment of a control system enclosure.

FIG. 1B is a perspective view of another non-limiting embodiment of a control system enclosure arrangement.

FIG. 2 is a partial cross-sectional view of a non-limiting embodiment of a handheld surgical instrument employing a linear drive system.

FIG. 3 is a top view of a distal portion of a non-limiting embodiment of a surgical instrument.

FIG. 4 is a side cross-sectional view of the distal portion of the surgical instrument of FIG. 3.

FIG. 5 is a side cross-section view of a distal portion of a non-limiting embodiment of a surgical instrument.

FIG. 6A is a front cross-sectional view of the distal portion of the surgical instrument of FIG. 5, taken along line 6A-6A.

FIG. 6B is another front cross-sectional view of the distal portion of the surgical instrument of FIG. 5, taken along line 6B-6B.

FIG. 7A is a side cross-section view of a distal portion of a non-limiting embodiment of a surgical instrument; a blade of the instrument is shown in a first axial position.

FIG. 7B is another side cross-sectional view of the distal portion of the surgical instrument of FIG. 7A; the blade is shown translated axially to a second axial position.

FIG. 8 is a top view of the distal portion of the surgical instrument of FIG. 7A.

FIG. 9 is a perspective view of a distal portion of a non-limiting embodiment of a surgical instrument.

FIG. 10A is a perspective view of a distal portion of a hollow sheath of the surgical instrument of FIG. 9.

FIG. 10B is a perspective view of a distal portion of a blade of the surgical instrument of FIG. 9.

FIG. 10C is a perspective view of a shearing plate of the surgical instrument of FIG. 9.

FIG. 11 is a side cross-sectional view of the distal portion of the surgical instrument of FIG. 9.

FIGS. 12A-12C are a series of side cross-sectional views of the distal portion of the surgical instrument of FIG. 9 showing the blade in different axial positions as the blade translates with respect to the hollow sheath.

FIG. 13 is a side view of a non-limiting embodiment of a linear drive system for use in a surgical instrument, such as the surgical instrument of FIG. 2.

FIG. 14 is a side view of a non-limiting embodiment of another linear drive system for use in a surgical instrument, such as the surgical instrument of FIG. 2.

FIG. 15 is a side view of a non-limiting embodiment of another linear drive system for use in a surgical instrument, such as the surgical instrument of FIG. 2.

FIG. 16 is a partial cross-sectional view of a non-limiting embodiment of a surgical instrument employing another linear drive system.

FIG. 17 is a perspective view of a distal portion of a non-limiting embodiment of a surgical instrument including a plurality of openings in a hollow sheath; tissue is shown being drawn into the openings.

FIG. 18 is a partial cutaway view of the distal portion of the surgical instrument of FIG. 17, showing a toothed blade.

FIG. 19 is a perspective view of a distal portion of another non-limiting embodiment of a surgical instrument including a plurality of openings in a hollow sheath.

FIGS. 20A-20B are side cross-sectional views of distal portions of toothed blades for use in a surgical instrument, such as the surgical instruments of FIGS. 17-19.

FIGS. 21A-21C are side cross-sectional views of individual teeth that may be used with a toothed blade.

FIG. 22 is a partial cross-sectional view of a non-limiting embodiment of a surgical instrument employing two suction lumens.

FIG. 23 is a perspective view of a distal portion of the surgical instrument of FIG. 22.

FIGS. 24A and 24B are side views of distal portions of blades for a surgical instrument, such as the surgical instrument of FIG. 22.

FIG. 25 is a partial cross-sectional view of a non-limiting embodiment of a surgical instrument employing a rotational drive system.

FIG. 26 is a perspective view of the surgical instrument of FIG. 25.

FIG. 27 is a side cross-sectional view of a distal portion of a non-limiting embodiment of a surgical instrument including teeth defined in an opening of a hollow sheath for gripping tissue.

FIGS. 28-29 are partial views of teeth that may be used in a surgical instrument, such as the surgical instrument of FIG. 27.

FIG. 30 is a side cross-section view of a nose piece and associated components of a surgical instrument, such as the surgical instrument of FIG. 27.

FIG. 31 is a side view of a distal portion of a non-limiting embodiment of a surgical instrument including a rotatable blade.

FIG. 32 is a cross-section view of the surgical instrument of FIG. 31, taken along line 32-32.

FIG. 33A is a cross-section view of the blade of the surgical instrument of FIG. 31, taken along line 33A-33A.

FIG. 33B is a cross-sectional view of the blade of the surgical instrument of FIG. 31, taken along line 33B-33B.

FIG. 34 is a cross-section view of another non-limiting embodiment of a blade for a surgical instrument, such as the surgical instrument of FIG. 31.

FIG. 35 is a side cross-sectional view of another non-limiting embodiment of a blade for a surgical instrument, such as the surgical instrument of FIG. 31.

FIG. 36 is a cross-sectional view of the blade of FIG. 35, taken along line 36-36.

FIG. 37 is a front cross-sectional view of a distal portion of a non-limiting embodiment of a surgical instrument including a mass balanced blade.

FIG. 38 is a top view of a distal portion of a non-limiting embodiment of a surgical instrument including a blade with a screw surface.

FIG. 39 is a top view of the distal portion of the blade of the surgical instrument of FIG. 38.

FIG. 40 is a partial cross-sectional view of a non-limiting embodiment of a surgical instrument including a movable tissue gripping member.

FIG. 41 is a cross-sectional view of a hollow sheath, cables, and a blade of the surgical instrument of FIG. 40, taken along line 41-41.

FIG. 42A is a perspective view of a distal portion of the surgical instrument of FIG. 40; the tissue gripping member is shown in an extended position.

FIG. 42B is a perspective view of the distal portion of the surgical instrument of FIG. 40; the tissue gripping member is shown in a retracted position.

FIG. 43 is a cross-section view of the hollow sheath, cables, and blade of the surgical instrument of FIG. 40, taken along line 43-43 in FIG. 42A.

DETAILED DESCRIPTION

The owner of the present application also owns the following U.S. Patent Applications that were filed on Feb. 11, 2010, and which are herein incorporated by reference in their respective entireties:

U.S. patent application Ser. No. 12/703,860, now U.S. Pat. No. 8,531,064, entitled ULTRASONICALLY POWERED SURGICAL INSTRUMENTS WITH ROTATING CUTTING IMPLEMENT;

U.S. patent application Ser. No. 12/703,864, now U.S. Pat. No. 8,323,302, entitled METHODS OF USING ULTRASONICALLY POWERED SURGICAL INSTRUMENTS WITH ROTATABLE CUTTING IMPLEMENTS;

U.S. patent application Ser. No. 12/703,866, now U.S. Pat. No. 8,951,272, entitled SEAL ARRANGEMENTS FOR ULTRASONICALLY POWERED SURGICAL INSTRUMENTS;

U.S. patent application Ser. No. 12/703,870, now U.S. Pat. No. 9,259,234, entitled ULTRASONIC SURGICAL INSTRUMENTS WITH ROTATABLE BLADE AND HOLLOW SHEATH ARRANGEMENTS;

U.S. patent application Ser. No. 12/703,875, now U.S. Pat. No. 8,469,981, entitled ROTATABLE CUTTING IMPLEMENT ARRANGEMENTS FOR ULTRASONIC SURGICAL INSTRUMENTS;

U.S. patent application Ser. No. 12/703,877, now U.S. Pat. No. 8,382,782, entitled ULTRASONIC SURGICAL INSTRUMENTS WITH PARTIALLY ROTATING BLADE AND FIXED PAD ARRANGEMENT;

U.S. patent application Ser. No. 12/703,879, now U.S. Pat. No. 8,486,096, entitled DUAL PURPOSE SURGICAL INSTRUMENT FOR CUTTING AND COAGULATING TISSUE;

U.S. patent application Ser. No. 12/703,885, now U.S. Pat. No. 8,579,928, entitled OUTER SHEATH AND BLADE ARRANGEMENTS FOR ULTRASONIC SURGICAL INSTRUMENTS; and

U.S. patent application Ser. No. 12/703,899, now U.S. Pat. No. 8,419,759, entitled ULTRASONIC SURGICAL INSTRUMENT WITH COMB-LIKE TISSUE TRIMMING DEVICE.

Certain embodiments will now be described to provide an overall understanding of the principles of the structure, function, manufacture, and use of the devices and methods disclosed herein. One or more examples of these embodiments are illustrated in the accompanying drawings. Those of ordinary skill in the art will understand that the devices and methods specifically described herein and illustrated in the accompanying drawings are non-limiting embodiments and that the scope of these embodiments is defined solely by the claims. The features illustrated or described in connection with one embodiment may be combined with the features of other embodiments. Further, where an ordering

of steps in a process is indicated, such ordering may be rearranged or the steps may be carried out contemporaneously as desired unless illogical or the listed order is explicitly required. Such modifications and variations are intended to be included within the scope of the appended claims.

In the following description, like reference characters designate like or corresponding parts throughout the several views. Also in the following description, it is to be understood that terms such as “forward,” “rearward,” “front,” “back,” “right,” “left,” “over,” “under,” “top,” “bottom,” “upwardly,” “downwardly,” “proximally,” “distally,” and the like are words of convenience and are not to be construed as limiting terms. The description below is for the purpose of describing various embodiments and is not intended to limit the appended claims.

Various embodiments are directed to improved ultrasonic surgical systems and instruments configured for effecting tissue dissecting, cutting, and/or coagulation during surgical procedures as well as the cutting implements employed thereby. In one embodiment, an ultrasonic surgical instrument apparatus is configured for use in open surgical procedures, but has applications in other types of surgery, such as laparoscopic, endoscopic, and robotic-assisted procedures. Versatile use is facilitated by selective use of ultrasonic energy, the selective gross axial and/or rotational motion of the cutting/coagulation implement, and/or suction applied near and/or through the cutting/coagulation implement.

It will be appreciated that the terms “proximal” and “distal” are used herein with reference to a clinician gripping a handpiece assembly. Thus, an end effector is distal with respect to the more proximal handpiece assembly. It will be further appreciated that, for convenience and clarity, spatial terms such as “top” and “bottom” also are used herein with respect to the clinician gripping the handpiece assembly. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

FIG. 1 illustrates in schematic form one non-limiting embodiment of a surgical system 10. The surgical system 10 may include an ultrasonic generator 12 and an ultrasonic surgical instrument assembly 100 that may include ultrasonic producing components. As will be discussed in further detail below, the ultrasonic generator 12 may be connected by a cable 14 to an ultrasonic transducer assembly 114 in a housing portion 102 of the surgical instrument assembly 100. The transducer assembly 114 may include one or more ultrasonic transducers capable of producing ultrasonic vibrations. Further, attached to the ultrasonic transducer assembly 114 may be a horn 124 for amplifying and/or focusing ultrasonic motions created by the transducer assembly 114. Coupled to the horn 124 may be a blade 200 disposed at least partially within a hollow sheath 230 extending from the housing portion 102. In one embodiment, the system 10 further includes a motor control system 20 that includes a power supply 22 that is coupled to a control module 24 by cable 23 to supply, for example, 24VDC thereto. The motor control module 24 may comprise a control module manufactured by National Instruments under Model No. NI cRIO-9073. However, other motor control modules may be employed. Any of a number of power supplies may be successfully employed for power supply 22. The power supply 22 may be further coupled to a motor drive 26 by cable 25 to also supply 24VDC thereto. The motor drive 26 may comprise a motor drive manufactured by National Instruments. However, other motor drives may be success-

fully employed. Control module **24** may also be coupled to the motor drive **26** by cable **27** for supplying power thereto. A conventional foot pedal **30** or other control switch arrangement may be attached to the control module **24** by a cable **31**. As will be discussed in further detail below, the ultrasonic surgical instrument **100** may include a drive system that may include a motor **190** that has an encoder **194** associated therewith. The drive system may communicate with the transducer assembly **114**, via a rotational-to-linear motion converter **150** (described below), to deliver gross axial motions to the blade **200** such that the blade translates with respect to the hollow sheath when the drive system is activated. The motor **190** may comprise a motor manufactured by National Instruments under Model No. CTP12ELF10MAA00. However, other motors may be employed. The encoder **194** may comprise a linear encoder manufactured by US Digital under Model No. E2-500-197-I-D-D-B. However, other motors and encoders may be used. The encoder **194** may be coupled to the motor control module **24** by an encoder cable **32** and the motor **190** may be coupled to the motor drive **26** by cable **33**. The surgical system **10** may also include a computer **40** that may communicate by Ethernet cable **42** with the motor control module **24**.

As can also be seen in FIG. 1, in various embodiments, the motor control system **20** may be housed in an enclosure **21**. To facilitate easy portability of the system, various components may be attached to the motor control system **20** by removable cable connectors. For example, foot pedal switch **30** may be attached to a detachable cable connector **37** by cable **35** to facilitate quick attachment of the foot pedal to the control system **20**. A/C power may be supplied to the power supply **22** by a conventional plug/cable **50** that is attached to a detachable cable connector **54** that is attached to cable **52**. The computer **40** may have a cable **60** that is attached to detachable cable connector **62** that is coupled to cable **42**. The encoder **194** may have an encoder cable **70** that is attached to a detachable connector **72**. Likewise, the motor **190** may have a cable **74** that is attached to the detachable connector **72**. The detachable connector **72** may be attached to the control module **24** by cable **32** and the connector **72** may be attached to the motor drive **26** by cable **33**. Thus, cable connector **72** serves to couple the encoder **194** to the control module **24** and the motor **190** to the motor drive **26**. The cables **70** and **74** may be housed in a common sheath **76**.

In an alternative embodiment, the ultrasonic generator **12** and the control system **20** may be housed in the same enclosure **105**. See FIG. 1A. In yet another embodiment, the ultrasonic generator **12** may electrically communicate with the motor control system **20** by a jumper cable **107**. Such arrangement may share a data link as well as a common means for supplying power (cord **50**). See FIG. 1B.

In various embodiments, the ultrasonic generator **12** may include an ultrasonic generator module **13** and a signal generator module **15**. See FIG. 1. The ultrasonic generator module **13** and/or the signal generator module **15** each may be integrated with the ultrasonic generator **12** or may be provided as separate circuit modules electrically coupled to the ultrasonic generator **12** (shown in phantom to illustrate this option). In one embodiment, the signal generator module **15** may be formed integrally with the ultrasonic generator module **13**. The ultrasonic generator **12** may comprise an input device **17** located on a front panel of the generator **12** console. The input device **17** may comprise any suitable device that generates signals suitable for programming the operation of the generator **12** in a known manner. Still with

reference to FIG. 1, the cable **14** may comprise multiple electrical conductors, such as copper wires, for the application of electrical energy to positive (+) and negative (−) electrodes of an ultrasonic transducer assembly **114** as will be discussed in further detail below.

Various forms of ultrasonic generators, ultrasonic generator modules and signal generator modules are known. For example, such devices are disclosed in commonly owned U.S. patent application Ser. No. 12/503,770, now U.S. Pat. No. 8,461,744, entitled ROTATING TRANSDUCER MOUNT FOR ULTRASONIC SURGICAL INSTRUMENTS, filed Jul. 15, 2009, which is herein incorporated by reference in its entirety. Other such devices are disclosed in one or more of the following U.S. Patents, all of which are incorporated by reference herein: U.S. Pat. No. 6,480,796 (METHOD FOR IMPROVING THE START UP OF AN ULTRASONIC SYSTEM UNDER ZERO LOAD CONDITIONS); U.S. Pat. No. 6,537,291 (METHOD FOR DETECTING A LOOSE BLADE IN A HANDLE CONNECTED TO AN ULTRASONIC SURGICAL SYSTEM); U.S. Pat. No. 6,626,926 (METHOD FOR DRIVING AN ULTRASONIC SYSTEM TO IMPROVE ACQUISITION OF BLADE RESONANCE FREQUENCY AT STARTUP); U.S. Pat. No. 6,633,234 (METHOD FOR DETECTING BLADE BREAKAGE USING RATE AND/OR IMPEDANCE INFORMATION); U.S. Pat. No. 6,662,127 (METHOD FOR DETECTING PRESENCE OF A BLADE IN AN ULTRASONIC SYSTEM); U.S. Pat. No. 6,678,621 (OUTPUT DISPLACEMENT CONTROL USING PHASE MARGIN IN AN ULTRASONIC SURGICAL HANDLE); U.S. Pat. No. 6,679,899 (METHOD FOR DETECTING TRANSVERSE VIBRATIONS IN AN ULTRASONIC HANDLE); U.S. Pat. No. 6,908,472 (APPARATUS AND METHOD FOR ALTERING GENERATOR FUNCTIONS IN AN ULTRASONIC SURGICAL SYSTEM); U.S. Pat. No. 6,977,495 (DETECTION CIRCUITRY FOR SURGICAL HANDPIECE SYSTEM); U.S. Pat. No. 7,077,853 (METHOD FOR CALCULATING TRANSDUCER CAPACITANCE TO DETERMINE TRANSDUCER TEMPERATURE); U.S. Pat. No. 7,179,271 (METHOD FOR DRIVING AN ULTRASONIC SYSTEM TO IMPROVE ACQUISITION OF BLADE RESONANCE FREQUENCY AT STARTUP); and U.S. Pat. No. 7,273,483 (APPARATUS AND METHOD FOR ALERTING GENERATOR FUNCTION IN AN ULTRASONIC SURGICAL SYSTEM).

As can be seen in FIG. 2, an ultrasonic surgical instrument **100** may comprise a housing **102** that houses the motor **190**, the encoder **194**, the ultrasonic transducer assembly **114**, and the horn **124**. The transducer assembly **114** may be movably supported within the housing **102** by conventional linear bearings **104**, such as rollers. Extending from the horn **124** may be the blade **200**, which passes through the hollow sheath **230** to a window or opening **231** defined therein. As shown in FIG. 2, a distal end **202** of the blade **200** may be seen through the opening **231** at a distal portion **250** of the surgical instrument **100**. The housing **102** may be provided in two or more parts that are attached together by fasteners such as screws, snap features, etc. and/or by one or more adhesives and may be fabricated from, for example, polycarbonate, stainless steel, or other material. The motor **190** may be mounted to the housing **102** and may mechanically communicate with the ultrasonic transducer by way of a rotational-to-linear motion converter **150**, which may comprise a rack member **153** and a pinion **154**. Additional gears may be added between the pinion **154** and the rack member **153** to achieve desired gear reductions, if desired. Further, the rack member **153** may hold the encoder **194** and be

attached to the transducer assembly 114. Accordingly, activation of the motor 190 may turn pinion 154, and thus drive rack 153, encoder 194, transducer assembly 114, horn 124, and blade 200 in a proximal direction "PD" or a distal direction "DD" parallel to or coaxial with the hollow sheath's longitudinal axis A-A. The motor 190 may comprise, for example, a stepper motor manufactured by National Instruments under Model No. CTP12ELF10MAA00. However, other motors, such as brushless DC or other types, may be employed to effectuate, for example, "gross" axial motion of the blade 200 relative to the hollow sheath 230 on the order of 1 to 15 mm. The encoder 194 may convert the position and/or speed of the rack member 154 into electrical pulses that provide position, speed, and/or other control information to the control module 24. Further, the encoder 194 may include an in-line force sensor (not shown), such as a piezoelectric sensor, that may measure a load experienced by the blade's distal end 202 and communicated to the rack member 153, such as the load provided by tissue when the surgical instrument is used in a surgical operation.

Referring still to FIG. 2, the ultrasonic transducer assembly 114 may include a housing 118 that supports piezoelectric ultrasonic transducers 115 for converting electrical energy to mechanical energy that results in longitudinal vibrational motion of the ends of the transducers 115. The ultrasonic transducers 115 may comprise a stack of ceramic piezoelectric elements with a motion null point located at some point along the stack. The ultrasonic transducers 115 may be mounted between a proximal end piece 116 and a distal end piece 117. In addition, the horn 124 may be mounted to the distal end piece 117 at the null point on one side and to the blade 200 on the other side. As a result, the blade 200 will vibrate in the longitudinal direction at an ultrasonic frequency rate with the ultrasonic transducer assembly 114. The ends of the ultrasonic transducer assembly 114 achieve maximum motion with a portion of the stack constituting a motionless node, when the ultrasonic transducer assembly 114 is driven at maximum current at the transducer's resonant frequency. However, the current providing the maximum motion will vary with each instrument and is a value stored in the non-volatile memory of the instrument so the system can use it.

The parts of the surgical instrument 100 may be designed such that the combination will oscillate at the same resonant frequency. In particular, the elements may be tuned such that the resulting length of each such element is one-half wavelength or a multiple thereof. Longitudinal back and forth motion is amplified as the diameter closer to the blade 200 of the acoustical mounting horn 124 decreases. Thus, the horn 124 as well as the blade 200 may be shaped and dimensioned so as to amplify blade motion and provide ultrasonic vibration in resonance with the rest of the acoustic system, which produces the maximum back and forth motion of the end of the acoustical mounting horn 124 close to the blade 200. A motion from 20 to 25 microns at the ultrasonic transducers 115 may be amplified by the horn 124 into blade movement of about 40 to 100 microns.

Referring briefly back to FIG. 1, when power is applied to the ultrasonic instrument 110 by operation of the foot pedal 30 or other switch arrangement, the control system 20 may, for example, cause the blade 200 to vibrate longitudinally at approximately 55.5 kHz, and the amount of longitudinal movement will vary proportionately with the amount of driving power (current) applied, as adjustably selected by the user. When relatively high cutting power is applied, the blade 200 may be designed to move longitudinally in the

range of about 40 to 100 microns at the ultrasonic vibrational rate. Such ultrasonic vibration of the blade 200 will generate heat as the blade contacts tissue, i.e., the acceleration of the blade 200 through the tissue converts the mechanical energy of the moving blade 200 to thermal energy in a very narrow and localized area. This localized heat creates a narrow zone of coagulation, which will reduce or eliminate bleeding in small vessels, such as those less than one millimeter in diameter. The cutting efficiency of the blade 200, as well as the degree of hemostasis, will vary with the level of driving power applied, the cutting rate or force applied by the surgeon to the blade, the nature of the tissue type, and the vascularity of the tissue.

Referring again to FIG. 2, when power is applied to motor 190, motor 190, via pinion 154, applies a "gross axial motion" to the rack member 153 to cause the ultrasonic transducer assembly 114 and blade 200 to translate with respect to the hollow sheath 230. As used herein, the term "gross axial motion," and the like, is to be distinguished from "ultrasonic motion," and the like, that may be achieved by way of the ultrasonic transducer assembly. The term "gross axial motion" instead encompasses translational motion that is not solely generated by operation of the ultrasonic transducer assembly 114.

To provide the ultrasonic instrument 110 with power from the ultrasonic generator 12 (see FIG. 1), a multiple-segment jointed protector 110 may be employed. As can be seen in FIG. 2, conductors 151, 152 are coupled to the ultrasonic transducer assembly 114 and extend out of the instrument through the housing 102. Further, the protector 110 may be attached to the instrument housing 102 at one end and to the transducer assembly housing 118 at the other end. The conductors 151, 152 may pass through one or more holes in the transducer assembly housing. Accordingly, ultrasonic signals from the ultrasonic generator 12 are transferred to the ultrasonic transducers 115 through the conductors 151, 152. The protector 110 may prevent the conductors 151, 152 from being damaged or pinched by the mechanical components of the instrument 100 when the motor 190 is activated.

Referring still to FIG. 2, various embodiments also include a distal nosepiece 160 that may be removably attached to the distal end of the housing 102 by fasteners and/or adhesives (not shown). The nosepiece 160 may be fabricated from, for example, stainless steel, aluminum, or plastic. In various embodiments, the distal end 202 of the blade 200 extends through a hollow portion 210 of the nosepiece 160. The hollow sheath 230 may likewise extend through the hollow portion 210. The hollow portion 210 may include an annular groove in which a proximal seal 212 may be held against the end of the hollow sheath 230 and against the blade 200. The seal 212 may comprise, for example, a silicone O-ring, a brazing, or a press-fit seal, and serve to establish a substantially fluid-tight and/or airtight seal between the nosepiece 160, blade 200, and hollow sheath 230.

Also in various embodiments, the hollow sheath 230 may be coaxially aligned with the blade 200 and be attached to the hollow portion 210 of the nosepiece 160 by, for example, welding, press-fitting, threading, adhering with glue or other adhesive(s), etc. As can be seen in FIG. 2, a suction port 240 may be attached to the nosepiece 160 to communicate with a proximal hole 232 in the hollow sheath 230. A flexible tube 242 may be attached to the suction port 240 and communicate with a collection receptacle 243 that is coupled to a source of vacuum, generally depicted as 244. Thus, the hollow sheath 230 forms a suction path extending around the blade 200 that begins at the distal portion 250 of the outer

sheath 230, such as at the opening 231, and goes out through the hole 232 to the suction port 240. Those of ordinary skill in the art will appreciate that alternate suction paths are also possible. Further, a distal seal 213, similar to proximal seal 212, may be held in the nosepiece 160 and may help further seal the hollow sheath 230 therein such that the suction path from the opening 231, through the sheath 230, out hole 232, and through the port 240 is maintained with minimal or no ingress of air from outside the aforementioned path.

Various embodiments of the surgical system 10 (see FIG. 1) provide the ability to selectively apply ultrasonic axial motion to the blade 200 and gross axial motion to the blade 200 as well. If desired, the clinician may simply activate the ultrasonic transducer assembly 114 without activating the motor 190. In such cases, the instrument 100 may be used in ultrasonic mode simply as an ultrasonic instrument. Frequency ranges for longitudinal ultrasonic motion may be on the order of, for example, 30-80 kHz. Similarly, the clinician may desire to activate the motor 190 without activating the ultrasonic transducer assembly 114. Thus, gross axial motion will be applied to the blade 200 in the translational mode, without the application of longitudinal ultrasonic motion thereto. Gross axial speeds may be, for example, on the order of 0.25 in/s to 5 in/s. In other applications, the clinician may desire to use the instrument 100 in the ultrasonic and translational modes wherein the blade 200 will experience longitudinal ultrasonic motion from the transducer assembly 114 and gross axial motion from the motor 190. Further, the blade 200 may translate back and forth within the hollow sheath 230 by reversing the output of the motor. By way of example, the motor 190 may first cause the blade 200 to move in the distal direction DD. The encoder 194 may then sense or calculate when the blade 200 has reached the distal end of the hollow sheath 230 and then provide feedback causing the motor 190 to reverse, thereby moving the blade 200 in the proximal direction PD until the encoder 194 again senses or calculates that the blade 200 has moved sufficiently in the proximal direction PD, and then the encoder 194 may again provide feedback causing the motor to reverse again. Various such gross translational oscillatory or reciprocating motions may thereby be achieved. Moreover, those of ordinary skill in the art will readily appreciate that various embodiments of the surgical system 10 may be affectively employed in connection with arthroscopic as well as other surgical applications.

The surgical instrument 100 may have various distal portions 250. FIGS. 3 and 4 illustrate an example of a distal portion 450 of another non-limiting embodiment of a surgical instrument wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. In these embodiments, the surgical instrument includes a hollow sheath 430, a blade 200 disposed at least partially within the hollow sheath 430, an ultrasonic transducer (not shown, see transducers 115 in FIG. 2) operably coupled to the blade, and a drive system (also not shown, see motor 190 in FIG. 2) communicating with the transducer to deliver axial motions to the blade 200 such that the blade 200 translates, for example in the proximal and distal directions, PD and DD, respectively, with respect to the hollow sheath 430 when the drive system is activated. In such embodiments, the blade 200 may have a tube-like shape and may cut tissue when the same is drawn into and/or through the opening 431 of the hollow sheath 430 by suction therethrough. Accordingly, tissue that is drawn into the sheath 430 may be cut by activating the ultrasonic transducers to create ultrasonic motion of the blade 200 and/or by activating the motor to cause the blade

200 to translate with gross axial motion with respect to the hollow sheath 430. The distal end 202 of the blade 200 may be shaped to enhance cutting by having a sharp edge or a scalloped shape. The latter shape may assist in the cutting of tough tissues.

FIGS. 5-6B illustrate another example of a distal portion 550 of another non-limiting embodiment of a surgical instrument wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. FIG. 5 is a cross-sectional view taken along a longitudinal axis of the hollow sheath 530 and FIGS. 6A and 6B are cross-sectional views taken along their respective lines in FIG. 5. In these embodiments, a septum 260 may divide the interior of the hollow sheath 530 into a suction portion "A" and a blade portion "B." The suction portion A may communicate with a suction port (not shown, see port 240, described above). Further, the septum 260 may be divided into a perforated portion 261 and a solid portion 262, both of which may be integrally formed with the hollow sheath 530. Alternatively, all of the septum 260 may be perforated. In any event, suction may be applied to the instrument such that, during a surgical operation, tissue is pulled toward suction portion A, by way of the perforated portion 261. Such configurations may help properly position tissue through opening 531 such that the blade 200' may be moved into and cut the tissue held therethrough. Further, referring to FIG. 5, a pad 226 may be fixed to the sheath 530 and/or to the septum 260 to provide a cutting surface against which the blade 200' may cut tissue, when the blade 200' is moved into contact therewith. Also, as can be seen in FIG. 6B, the blade 200' may include a U-shape to reduce mass.

Referring still to FIGS. 5-6B, in at least one embodiment, tissue may be cut as follows. First, suction may be applied to the suction portion A of the hollow sheath 530 such that tissue is drawn into the opening 531. Second, the ultrasonic transducers may cause the blade 200' to vibrate ultrasonically. Third, the blade 200' may be advanced in the distal direction DD such that the blade 200' cuts the tissue by both gross axially movement and ultrasonic vibrational movement. Third, the blade 200' may be retracted while suction is maintained, thereby capturing and/or drawing the severed tissue into the suction portion A of the hollow sheath 530.

FIGS. 7A-8 illustrate another example of a distal portion 650 of another non-limiting embodiment of a surgical instrument wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. FIGS. 7A and 7B are longitudinal cross-sectional views of the instrument's distal portion 650, with the blade 200" in a first position in FIG. 7A and in a second position in FIG. 7B. FIG. 8 is a top view of the distal portion 650 showing a teardrop-shaped opening 631 in hollow sheath 630. In these embodiments, the blade 200" may further include a lumen 205 through which suction may also be applied. Accordingly, the blade 200" may include a distal aperture 206 and a proximal aperture 207 (see FIG. 2). As best seen in FIG. 2, the proximal aperture 207 may be positioned within the nosepiece 160 (see FIG. 2). In any event, referring back to FIGS. 7A-7B, suction may be applied through the lumen 205 such that tissue "T" may be drawn into the blade 200" via distal aperture 206 when the blade 200" is in the first axial position, see FIG. 7A. After the tissue is drawn into the blade 200" (see FIG. 7A), the tissue T may be pinched between the distal aperture 206 and a narrow portion 632 of the opening 631 by translating the blade 200" in the proximal direction to the second axial position, see FIG. 7B. Thereafter, the tissue may be cut by activating the ultrasonic transducer(s), as described above.

13

The opening's narrow portion **632**, combined with the pinching of the tissue therein, may help more easily sever tissue with the ultrasonic vibrational motion of the blade **200**".

FIGS. 9-12C illustrate another example of a distal portion **750** of another non-limiting embodiment of a surgical instrument wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. In these embodiments, the hollow sheath **730** may further include a beveled shearing surface **735** against which the blade **200**" may cut tissue at opening **731**. The beveled shearing surface **735** may be similar to a single tooth in that it provides a sharpened edge against which tissue may be cut. FIG. 9 is a perspective view of the distal portion **750** of the surgical instrument. FIG. 10A is a perspective view of the distal portion of the hollow sheath, FIG. 10B is a perspective view of the distal portion of the blade **200**", and FIG. 10C is a perspective view of a shearing plate **736**. The shearing surface **735** may be integrally formed with or attached to the sheath **730**. In at least one embodiment, the shearing surface **735** may be formed from a portion of a shearing plate **736**. In such embodiments, the shearing plate may be held in place on the hollow sheath **200**" via press pins, epoxy, snap features, etc. As seen in FIG. 10A, the hollow sheath **730** may include a recess **737** and protrusions **738** extending therefrom for receiving the plate **736**. Further, as best seen in the cross-sectional view provided in FIG. 11, the blade **200**" may further include a sharpened surface **209** that is complimentary to the beveled shearing surface **735**. Also, proximal to the sharpened surface **209**, sufficient clearance "C" may exist between the blade **200**" and the inner surface of the hollow sheath **730** such that suction may communicate from the suction port (not shown, see port **240** in FIG. 2) to the opening **731**. Further, the clearance C may be large enough to allow tissue to be drawn through the hollow sheath **730** between the blade **200**" and the sheath **730**.

Further, as noted above, the blade **200**" may move axially past the opening **731**. For example, FIGS. 12A-12C illustrate a series of side cross-sectional views of the distal portion **750** of the surgical instrument with the blade **200**" in different axial positions as the blade **200**" translates with respect to the hollow sheath **730**. FIG. 12A shows the blade **200**" in a distal-most axial position, FIG. 12B shows the blade **200**" in an interim position, and FIG. 12C shows the blade **200**" in a proximal position. In at least one embodiment, the instrument may function as follows. First, as the blade moves axially past the opening **731**, the blade **200**" may receive ultrasonic motions from one or more ultrasonic transducers (see transducers **115** in FIG. 2), as described above. Further, before or as the blade is moving, suction may be applied to the hollow sheath **730**. As the two shearing surfaces **735**, **209** approach one another, they may cut tissue fibrils hanging in the opening **731**. The severed tissue fragments may then be moved through the clearance space C between the blade **200**" and the hollow sheath **730** and ultimately evacuated out of the instrument via the suction port, described above.

Referring briefly back to FIG. 2, while the drive system described above utilizes a rack-and-pinion arrangement as the instrument's rotational-to-linear motion converter **150**, other converters may be employed. For example, referring now to FIG. 13, a converter **150'** may include a slider-crank mechanism configured to transform the rotary drive from the electric motor **190'** into linear motion. In such embodiments, the converter **150'** may include a slide member **153'** coupled to a first crank member **154'** which, in turn, is coupled to a

14

second crank member **155'** that is attached to the motor's axle. As the motor causes the second crank member **155'** to rotate in a clockwise "CW" or counter-clockwise "CCW" direction, the first crank member **154'** causes the slide member **153'** to slide in the proximal or distal direction, PD or DD, respectively. The slide member **153'**, which may be coupled to the ultrasonic transducer assembly (see assembly **114** in FIG. 2), may thereby effectuate the gross axial movement of the transducer assembly and thus the blade, as described above. Note that in this and other examples of rotational-to-linear converters described below, various components of the surgical instrument, such as the housing, are omitted for clarity. Additionally, the blade may grossly reciprocate with respect to the hollow sheath because the slide member **153'** may move proximally and then distally as the motor **190'** rotates the second crank member **155'**.

By way of another example, a rotational-to-linear motion converter **150"** may include a worm gear. Referring to FIG. 14, a motor **190"** is shown with its axle **155"** projecting toward transducer assembly **114**. Coupled to the axle **155"** may be a worm gear **154"** that is threadingly engaged with a threaded member **153"**. The threaded member **153"** is subsequently coupled to the transducer assembly **114**. Accordingly, activation of the motor **190"** may cause the worm gear **154"** to rotate about its axis, thereby driving the threaded assembly **153"**, and, thus, ultimately, the transducer assembly **114** and the blade (not shown), in a proximal or distal direction, PD or DD, respectively.

Another exemplary rotational-to-linear motion converter **150"** may include a lead screw. Referring to FIG. 15, a motor **190"** is shown with a lead screw **155"** serving as its axle. The lead screw **155"** may be threadingly engaged with a nut **154"** that is attached to support members **153"**. Accordingly, activation of the motor **190"** may cause the lead screw **155"** to rotate **154"** about its axis, thereby driving the nut **154"**, support members **153"**, transducer assembly **114** (shown in phantom), and, ultimately, the blade, in a proximal or distal direction, PD or DD, respectively.

Further, while the above drive systems have utilized a motor, manual drive systems may be used. For example, referring to FIG. 16, another example of a non-limiting embodiment of a surgical instrument **100'** is shown wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. In these embodiments, a trigger **191** may be pivotally coupled to the housing **102** by a pivot pin **192**. The handle may further include a groove **195** in which a projection **193** of the transducer assembly **114** is received. Accordingly, moving the trigger **191** in a first rotational direction RD' may cause the transducer assembly **114** and the blade **200** to move in a distal direction DD. Moving the trigger in a second rotational direction RD" may also cause the transducer assembly **114** and the blade **200** to move in a proximal direction PD. In use, a user may grasp the housing **102** and activate the trigger **191** with his or her thumb or finger(s).

In various embodiments, other opening configurations at a distal portion of the instrument, such as distal portion **250**, see FIG. 2, may be employed. Focusing now on one non-limiting embodiment, FIGS. 17-18 illustrate another example of a distal portion **850** of another non-limiting embodiment of a surgical instrument wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. FIG. 17 is a perspective view of the distal portion **850** including a plurality of openings **831** in the hollow sheath **830**. Tissue "T" is shown being drawn or drawn into the openings **831**

by way of a suction port (not shown, see port **240** in FIG. 2) communicating with the hollow sheath **830**. FIG. 18 is a partial cutaway view of the distal portion **850** of the surgical instrument. In these embodiments, the multiple openings **831** may be advantageous over one single opening for pulling the fibrous tissue T therethrough and into contact with blade **800** while stabilizing the tissue T for the blade **800** to cut. The openings **831** may be formed as perforations, or a grid of holes, in the hollow sheath **830**. Alternatively, referring to FIG. 19, the openings **831'** may be formed as slits in the sheath **830'** of the distal portion **850'**.

Additionally, in at least one embodiment, the blade **800** may only receive ultrasonic axial movement thereto, as discussed above. Accordingly, a drive system, also as discussed above (including, for instance a motor and/or trigger), may be unnecessary. However, in an alternative embodiment, the blade **800** may receive gross axial motions thereto and be operably coupled to a drive system for moving the blade in proximal or distal directions, PD or DD, respectively, see FIG. 18.

Further, a rasped or toothed blade may further enhance the cutting ability of the instrument. For example, referring to FIG. 18, the blade **800** may include teeth **801** projecting toward and positioned with respect to the openings **831** such that the teeth may contact tissue drawn into the openings **831**. The teeth may further have varying profiles. Referring now to FIGS. 20A-21C, a variety of blade teeth profiles, **801'**, **801''**, **801'''**, **801''''**, **801'''''**, are illustrated. The aforementioned teeth profiles may provide advantageous cutting ability to the blade, such as blades **800**, **800'**, and/or **800''**.

While some embodiments described above include one suction port, in various embodiments, other suction configurations may be employed. Focusing now on one non-limiting embodiment, FIGS. 22-23 illustrate another example of a surgical instrument **100''** wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. FIG. 22 is a partial cross-sectional view of part of the surgical instrument **100''** employing two suction lumens and two suction ports and FIG. 23 is a perspective view of the distal portion **950** of the surgical instrument **100''**. Referring to FIG. 22, the surgical instrument may include a housing **102** containing the transducer assembly **114** coupled to the horn **124**, among other things. As discussed above, the horn may subsequently be attached to the blade **900**. Additionally, the nose piece **160'** may include a first suction port **240** and a second suction port **241** which may be coupled to independent collection receptacles **243**, **243'** and/or vacuum sources **244**, **244'** by flexible tubing **242**, **242'**. The hollow sheath **930** may further include a septum **960** dividing the interior of the hollow sheath into a first lumen **963** and a second lumen **964**. The septum **960** may extend to the proximal end of the hollow sheath and abut against proximal seal **212**. The first suction port **240** may communicate with the first lumen **963** and the second port **241** may communicate with the second lumen **964**. Referring to FIG. 23, the first and second lumens **963** and **964**, respectively, can be seen extending to the hollow sheath's opening **931**. Accordingly, applying suction to ports **240** and **241** (see FIG. 22) may create two suction paths, via the first and second lumens **963** and **964**, that communicate with the opening **931** for applying suction thereto. The suction dynamics at the opening **931** may be further modified by applying different amounts of suction to the first port **240** and the second port **241**.

A blade **900** may be disposed at least partially within the first suction lumen **963**. Further, the distal end **902** of the blade **900** may extend through the opening **931**. Further, a

suction tube **965** may be added to the second lumen **964** to enhance the suction force applied at or near the opening **931**. In any event, tissue may be drawn toward the first lumen **963** and/or the second lumen **964** when suction is applied to one or both of suction ports **240**, **241**. The dual suction lumens **963**, **964** may provide enhanced contact and suction of tissue in a liquid environment, such as that experienced during arthroscopic surgery. The two lumens **963**, **964** may provide a reliable device capable of pulling in fibrous tissue and evacuating debris therethrough.

Referring to FIG. 24A, which illustrates a side view of a distal portion of the blade **900**, the blade **900** may be rasped or include teeth **901** near its distal end **902**. The teeth **901** may help improve tissue ablation by adding an optimized surface for friction to occur in a liquid environment. Additionally, while the blade **900** may be coupled to an ultrasonic transducer, such as one or more contained in the ultrasonic transducer assembly **114** (see FIG. 22), so that the blade **900** may experience ultrasonic vibrational motion, the blade **900** may also be coupled to a drive system configured to apply gross axial motion thereto, as described above, thereby enhancing the cutting ability of the blade **900**. Further, in at least one embodiment and referring to FIG. 23, the blade's distal end **902** may be retracted into the hollow sheath **930** by the drive system such that the blade does not unintentionally cut tissue until desired, at which point the blade may be extended back through the opening **931**.

Alternatively, other blade configurations may be employed. For example, referring to FIG. 24B, a blade **900'** may contain a flat surface **901'** near its distal end **902'**. In such embodiments, the surface itself may generate enough friction, when ultrasonic vibrational motion is applied thereto, to cut tissue.

While some of the embodiments described above have disclosed gross axial motion of a blade to provide various advantages, similar advantages may be obtained with a surgical instrument that instead utilizes gross rotational motion of a blade. Focusing now on one non-limiting embodiment, FIGS. 25-26 illustrate another surgical instrument **300** wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. In these embodiments, the surgical instrument **300** includes a housing **302** that houses a transducer assembly **314** that is attached to an ultrasonic horn **324**. The ultrasonic horn **324** may be coupled to the proximal end of the blade **200**, as discussed above. The ultrasonic horn **324** may be rotatably supported within the housing **302** by a distal bearing **336**. A nosepiece **160** may be attached to the housing **302** by fasteners **161** in the manner described above.

In this embodiment, a drive system may be provided that communicates with the transducer assembly **314** to deliver rotational motions thereto such that the blade rotates with respect to the hollow sheath **230** when the drive system is activated. For example, the ultrasonic transducer assembly **314** may have magnets **316** embedded or otherwise attached thereto to form an integral motor rotor, generally designated as **320**. A motor stator ring **330** is mounted within the housing **302** as shown. Conductors **332**, **334** are attached to the motor stator ring **330** and pass through the common sheath **76** to be attached to the motor cable **33** in the control system **20** as described above. A hollow shaft **340** extends through the motor rotor **320** to form a passage for conductors **151**, **152**. Conductors **151**, **152** are coupled to the ultrasonic transducer assembly **314** and an inner contact **2154**. The inner contact **2154** is attached to a portion of the hollow shaft **340** that rotatably extends into a slip ring assembly

2150 that is also supported within the housing 302. The hollow shaft 340 is rotatably supported within the housing 302 by a proximal bearing 342. The slip ring assembly 2150 is fixed (i.e., non-rotatable) within the housing 302 and includes a fixed outer contact 2156 that is coupled to conductors 2157, 2158 that form a generator cable 14. When power is supplied to the motor stator 330, the rotor 320 and the integral ultrasonic transducer 314 are caused to rotate about axis A-A. Ultrasonic signals from the ultrasonic generator 12 are transferred to the inner contact 2154 by virtue of rotating contact or electrical communication between the inner contact 2154 and the outer contact 2156. Those signals are transmitted to the ultrasonic transducer assembly 314 by conductors 151, 152. A suction may be applied between the blade 200 and hollow sheath 230 through port 240. A collection receptacle 243 and source of suction 240 may be attached to the port 240 by tube 242. The distal end of the blade is exposed through a window in the distal end of the hollow sheath 230 at the distal portion 250 of the instrument to expose the blade to tissue as will be further discussed below.

Additional details regarding surgical instrument 300 and other embodiments of surgical instruments with rotating blades may be found in U.S. patent application Ser. No. 12/703,860, now U.S. Pat. No. 8,531,064, entitled ULTRASONIC SURGICAL INSTRUMENTS WITH ROTATING CUTTING IMPLEMENT, filed on Feb. 11, 2010, which is incorporated herein by reference in its entirety.

In at least one embodiment, the distal portion of a surgical instrument may be configured to grip tissue that is being cut. Focusing now on one non-limiting embodiment, FIG. 27 illustrates an example of the distal portion 1050 of the surgical instrument wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. The hollow sheath 1030 may include an opening 1031 therein that is positioned such that tissue may be drawn therethrough and into contact with the blade 1000. The opening 1031 may further include one or more teeth 1032 that are configured to grip tissue positioned within the opening 1031. Additionally, the opening 1031 may project away from the blade 1000, or otherwise be shaped to increase the surface area of the opening to increase suction force at the opening 1031 when suction is applied to the instrument, as described above. Thus, tissue "T", which is shown being drawn toward the opening 1031, may be better held by the instrument when the blade 1000 is ultrasonically activated and/or grossly translated or rotated. Holding or gripping the tissue T when the blade is cutting may be advantageous to prevent the tissue T from bypassing a cutting edge 1006 of the blade 1000.

The teeth 1032 may be annular ribs as shown in FIG. 27. Alternatively, referring to FIGS. 28-29, which show various teeth options, the teeth 1032 may be hooks 1032', fish-scale like tabs 1032", or a roughened surface (not shown). FIG. 29 shows the tissue T being gripped by the tabs 1032".

Further, as noted above, the blade may grossly rotate or translate with respect to the hollow shaft, by way a drive system as described above. Also, in at least one embodiment, the blade may be hollow and define a lumen 1005 therein through which suction may be applied to draw tissue toward and into contact with the blade 1000. In at least one embodiment, the suction port 240 (see FIGS. 25-26) may communicate exclusively with the lumen 1005. In other words, the suction path may be limited to the lumen 1005 and not include the space between the hollow sheath 1030 and the blade 1000. In more detail, referring to FIG. 30, which illustrates an embodiment of nosepiece 160 and

various related components, the hollow sheath 1030 is supported within a hollow nosepiece 160 that has a suction port 240 therein. A flexible tube 242 may be attached to the suction port 240 and communicate with a collection receptacle 243 that is coupled to a source of suction, generally depicted as 244. The hollow sheath 1030 may be supported within the nosepiece 160 by a proximal seal 1013 and a distal seal 1015 which are located on each side of the suction port 240 and which serve to establish fluid tight seals therebetween. The hollow sheath 1030 is provided with at least one proximal opening 1014 in registration with the suction port 240 between the proximal seal 1013 and the distal seal 1015. In addition, the blade 1000 is rotatably supported within the hollow sheath 1030 by at least a proximal blade seal 1025 and a distal blade seal 1027. At least one blade discharge port 1028 may be provided through the lumen 1005 of the blade 1000 between the proximal blade seal 1025 and the distal blade seal 1027 to discharge into the at least one proximal sheath opening 1014.

In various embodiments, in a rotary surgical instrument, such as surgical instrument 300 described above, it may be desirable to reduce the blade mass to optimize rotational cutting speed. Thus, in at least one non-limiting embodiment, focusing now on FIGS. 31-32, a blade 1100 may be paddle shaped. FIG. 31 is a side view of a distal portion 1150 of a surgical instrument including the rotatable blade 1100 and FIG. 32 is a cross-section view of the distal portion 1150, taken along line 32-32. A hollow sheath 1130 may include opening 1131, as discussed above. The blade 1100 may be disposed at least partially within the hollow sheath 1130 and include a wide portion 1101 and a narrow portion 1102. The narrow portion 1102 may extend proximally and be coupled to the horn 324 (see FIG. 25). The wide portion 1102 of the blade 1100 may extend toward and/or into the opening 1131.

In at least one embodiment, referring to FIG. 32, the blade 1100 may include a concave surface or surfaces 1103 to further reduce rotational inertia as the blade 1100 rotates in a clockwise "CW" or counterclockwise "CCW" direction. Additionally, the concave surfaces 1103 may vary along the cross section of the blade 1100 to enhance the blade's cutting ability. Referring now to FIGS. 33A and 33B, the cross-section of blade 1100 at lines 33A-33A and 33B-33B, respectively, can be seen. The distal portion of the concave surfaces 1103 (see FIG. 33A) may be thicker and taller than the proximal portion of the same (see FIG. 33B). Alternatively, referring to FIG. 34, the mass of a blade 1100' may be reduced by forming a hole 1105 along the longitudinal axis of the blade 1100'. In at least one embodiment, the hole 1105 may be milled into the blade 1100'.

In at least one embodiment, referring to FIGS. 35-36, the mass of a blade 1200 usable with hollow sheath 1130 described above, may be reduced by using a blade including a gap 1206 positioned such that it may align within the opening 1131 of the sheath 1130, see FIG. 31. Again, referring to FIG. 35, the blade 1200 may include a narrow portion 1202 and a wide portion 1201. The wide portion 1201 may further define the gap 1206 therein that may be positioned such that the gap 1206 is next to or coincident with the opening 1131, when the blade 1200 is used with sheath 1130, see FIG. 31. The length "D" of the wide portion 1201 may be such that the length D is at least as long as is the opening 1131, see FIG. 31. Again, as described above and referring to FIG. 36, the wide portion 1201 of the blade 1200 may include a concave surface 1203 to reduce blade mass. Alternatively, a blade may further reduce blade mass by incorporating a blade that is mass balanced such that it

may have an elliptical center that is offset from the axis of rotation. For example, referring to FIG. 37, an axial or front cross-sectional view of a distal portion 1350 of a surgical instrument including a blade 1300 is shown positioned within the hollow sheath 1130, as described above. The blade 1300 may be configured to rotate about axis "A." However, the concave surface 1303 may not be symmetric about that axis. For example, a first side 1307 of the blade 1300 may be wider than a second side 1308. In such embodiments, the elliptical center "B" may be offset from the rotational axis A. Accordingly, the blade may be made from a non-homogenous material such that distribution of mass about the rotational axis A is balanced and the blade may rotate at high speeds without damaging itself or the hollow sheath 1130.

Alternative rotational blade configurations are possible. For example, referring to FIGS. 38-39, a non-limiting embodiment is provided in which a blade 1400 may include a screw surface 1403 positioned next to an opening 731 in a hollow sheath 730. The sheath 730 may be similar to the sheath 730 seen in FIG. 9 and discussed above. For example, the sheath 730 may also include a shearing plate 736 with a beveled shearing surface 735 positioned in the opening 731, as discussed above. Also as noted above, the beveled shearing surface 735 may be similar to a single tooth in that it provides a sharpened edge against which tissue may be cut. In any event, the screw surface 1403 may function like an auger and as the blade 1400 is rotated, the screw surface 1403 may pull tissue toward the shearing plate 736 to enhance the cutting of tissue.

In various embodiments, tissue may be gripped by a movable tissue gripping member to enhance the cutting thereof. Focusing now on one non-limiting embodiment, FIGS. 40-43 illustrate another surgical instrument 300' wherein like numbers previously used to describe the various embodiments disclosed above are used to designate like components. FIG. 40 is a partial cross-sectional view of the surgical instrument 300'. The surgical instrument 300' may be similar to surgical 300 describe above and seen in FIG. 25, for example, except at least that it further includes a drive system including a trigger 391 pivotally coupled to the nosepiece 160 that is subsequently connected to and configured to cause a tissue gripping member 1550 to move with respect to a hollow sheath 1530 (see FIGS. 42A-42B). Additionally, as discussed above, the blade 1500 is configured to rotate at least partially within the hollow sheath 1530.

As noted above, the drive system may be configured to deliver axial motions to the tissue gripping member 1540 such that the tissue gripping member translates with respect to the hollow sheath 1530 when the drive system is activated. In more detail, focusing now on FIGS. 42A-42B, FIG. 42A is a perspective view of a distal portion 1550 of the surgical instrument 300' with the tissue gripping member 1540 shown in an extended position and FIG. 42B is a perspective view of the distal portion 1550 with the tissue gripping member 1540 shown in a retracted position. The hollow sheath 1530 may include a distal opening 1531 that opens towards the distal direction DD. Further, extending from the opening 1531 may be the tissue gripping member 1540. At least one and optionally two load-bearing cables 1551, 1552 may be coupled to the tissue gripping member 1540 and extend in the proximal direction PD therefrom. As used herein, a cable can include a solid core cable, a twisted wire cable, a chain, a band, a rope, etc., and any other load-bearing member. Inside the hollow sheath 1530, referring to FIG. 43, which shows a cross-section view of the

hollow sheath 1530, cables 1551, 1552, and blade 1500, taken along line 43-43 in FIG. 42A, may be channels 1535, 1536 that are sized and configured to receive the cables 1535, 1536 therein. Although not shown, the channels may open at a distal opening (not shown) at or near the sheath's opening 1531. Referring still to FIG. 43, the blade 1500 may include concave surfaces 1503 as discussed above for facilitating the cutting of tissue; alternatively the blade may include a screw surface also as described above. Focusing back on FIGS. 40 and 41, FIG. 41 shows a cross-sectional view of the hollow sheath 1550, cables 1551, 1552, and blade 1500, taken along line 41-41, which is at or near the proximal end of the sheath 1550. As can be seen in FIG. 41, within the nosepiece 160, the cables 1551, 1552 may pass out of the channels 1535, 1536 of the hollow sheath 1530 by way of holes 1537, 1538 defined therein. The cables may be coupled to a trigger 391 which is pivotally mounted to the nosepiece. Accordingly, movement of the trigger 391 by a user may cause the cables 1551, 1552 and, subsequently, the tissue gripping member 1540 to axially move or translate with respect to the hollow sheath 1530.

The surgical instrument 300' may be used as follows. First, a user may manipulate the trigger 391 to extend the tissue gripping member 1540, as seen in FIG. 42. Next, the user may place tissue between the hollow sheath 1530 and the gripping member 1540. Optionally, suction may be applied to port 240 to assist in the positioning of the tissue. Then, the user may move the trigger 391 such that the gripping member 1540 retracts to a position like the one seen in FIG. 42B, thereby pulling tissue into the hollow sheath 1530 and into contact with the blade 1500. At the same time or after retracting the gripping member 1540, the user may activate the ultrasonic transducer assembly 314 such that ultrasonic vibrational motion is applied to the blade 1500. Optionally, power may also be supplied to the motor stator 330 such that the rotor 320, the integral ultrasonic transducer 314, and the blade 1500 are caused to rotate about axis A-A. The gripped tissue may therefore be cut by one or both of the ultrasonic vibrational motion and the gross rotational motion of the blade 1500. After cutting the tissue, the remnants may be suctioned out of the instrument 300' via port 240, as described above. The above exemplary steps may be repeated to cut additional tissue.

The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

Preferably, the various embodiments described herein will be processed before surgery. First, a new or used instrument is obtained and if necessary cleaned. The instrument can then be sterilized. In one sterilization technique, the instrument is placed in a closed and sealed container, such as a plastic or TYVEK® bag. The container and instrument are

then placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation kills bacteria on the instrument and in the container. The sterilized instrument can then be stored in the sterile container. The sealed container keeps the instrument sterile until it is opened in the medical facility. Sterilization can also be done by any number of ways known to those skilled in the art including beta or gamma radiation, ethylene oxide, and/or steam.

In various embodiments, an ultrasonic surgical instrument can be supplied to a surgeon with a waveguide and/or end effector already operably coupled with a transducer of the surgical instrument. In at least one such embodiment, the surgeon, or other clinician, can remove the ultrasonic surgical instrument from a sterilized package, plug the ultrasonic instrument into a generator, as outlined above, and use the ultrasonic instrument during a surgical procedure. Such a system can obviate the need for a surgeon, or other clinician, to assemble a waveguide and/or end effector to the ultrasonic surgical instrument. After the ultrasonic surgical instrument has been used, the surgeon, or other clinician, can place the ultrasonic instrument into a sealable package, wherein the package can be transported to a sterilization facility. At the sterilization facility, the ultrasonic instrument can be disinfected, wherein any expended parts can be discarded and replaced while any reusable parts can be sterilized and used once again. Thereafter, the ultrasonic instrument can be reassembled, tested, placed into a sterile package, and/or sterilized after being placed into a package. Once sterilized, the reprocessed ultrasonic surgical instrument can be used once again.

Although various embodiments have been described herein, many modifications and variations to those embodiments may be implemented. For example, different types of end effectors may be employed. Also, where materials are disclosed for certain components, other materials may be used. The foregoing description and following claims are intended to cover all such modification and variations.

Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated material does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

What is claimed is:

1. A surgical instrument, comprising:

a hollow sheath including at least one opening therein and at least one tooth positioned in the at least one opening, wherein the at least one tooth is configured to grip tissue positioned within the at least one opening;

a blade disposed at least partially within the hollow sheath, wherein the blade comprises a tip, and wherein the tip is configured to cut tissue;

at least one ultrasonic transducer coupled to the blade;

a drive system communicating with the at least one ultrasonic transducer to deliver rotational motions to the blade such that the blade rotates with respect to the hollow sheath when the drive system is activated; and wherein the hollow sheath comprises a hollow projection that projects away from the blade and the at least one tooth is defined in the hollow projection.

2. The surgical instrument of claim 1, wherein the blade comprises a concave surface positioned next to the at least one opening.

3. The surgical instrument of claim 2, wherein the blade includes an elliptical center that is offset from a rotational axis of the blade.

4. The surgical instrument of claim 1, wherein the at least one tooth comprises a beveled shearing surface.

5. The surgical instrument of claim 1, wherein the blade comprises a screw surface positioned next to the at least one opening.

6. The surgical instrument of claim 1, wherein the blade further includes a lumen defined therein.

7. The surgical instrument of claim 1, wherein the blade is paddle shaped.

8. A surgical instrument, comprising:

a hollow sheath including at least one opening therein and at least one tooth positioned in the at least one opening, wherein the at least one tooth is configured to grip tissue positioned within the at least one opening;

a blade disposed at least partially within the hollow sheath, wherein the blade comprises an end portion, and wherein the end portion is configured to cut tissue;

at least one ultrasonic transducer coupled to the blade;

a drive system communicating with the at least one ultrasonic transducer to deliver rotational motions to the blade such that the blade rotates with respect to the hollow sheath when the drive system is activated; and wherein the hollow sheath comprises a hollow projection that projects away from the blade and the at least one tooth is defined in the hollow projection.

* * * * *

专利名称(译)	带移动切割工具的超声波手术器械		
公开(公告)号	US9962182	公开(公告)日	2018-05-08
申请号	US14/590574	申请日	2015-01-06
[标]申请(专利权)人(译)	伊西康内外科公司		
申请(专利权)人(译)	爱惜康内镜手术，INC.		
当前申请(专利权)人(译)	ETHICON LLC		
[标]发明人	DIETZ TIMOTHY G JOHNSON GREGORY W CONLON SEAN P MUMAW DANIEL J MORGAN JEROME R DANNAHER WILLIAM D VAKHARIA OMAR J TIMM RICHARD W MILLER MATTHEW C ROBERTSON GALEN C		
发明人	DIETZ, TIMOTHY G. JOHNSON, GREGORY W. CONLON, SEAN P. MUMAW, DANIEL J. MORGAN, JEROME R. DANNAHER, WILLIAM D. VAKHARIA, OMAR J. TIMM, RICHARD W. MILLER, MATTHEW C. ROBERTSON, GALEN C.		
IPC分类号	A61B17/32 A61B17/3207 A61B17/22 A61B17/00		
CPC分类号	A61B17/320068 A61B17/22004 A61B17/3207 A61B17/320783 A61B2017/00778 A61B17/320092 A61B2017/00296 A61B2017/320069 A61B2017/320071 A61B2017/320089 A61B2017/320095		
审查员(译)	NGUYEN , VICTOR		
其他公开文献	US20150119916A1		
外部链接	Espacenet USPTO		

摘要(译)

在各种实施例中，提供了用于在含水环境中操作的手术器械。在至少一个实施例中，手术器械可以包括至少部分地设置在护套内的中空护套和刀片。与刀片耦合的可以是至少一个超声波换能器，其又可以耦合到驱动系统。驱动系统可以被配置为向叶片递送总的轴向运动，使得当驱动系统被激活时叶片相对于中空护套平移。因此，组织可以通过叶片的总体轴向移动和/或由超声换能器提供的超声振动运动而被叶片切割。在替代实施例中，叶片可以轴向旋转而不是相对于中空护套平移。

