



US006626890B2

(12) **United States Patent**
Nguyen et al.

(10) **Patent No.:** **US 6,626,890 B2**
(45) **Date of Patent:** **Sep. 30, 2003**

(54) **FAT REMOVAL DEVICE AND METHOD**

(56)

References Cited

(75) Inventors: **Hien Nguyen**, Fountain Valley, CA (US); **Jeffrey P. Wall**, Hunnington Beach, CA (US); **Suresh K. Wadhvani**, Mission Viejo, CA (US); **Payam Adlparvar**, Lake Forest, CA (US); **Bruce Stambaugh**, Anaheim, CA (US); **Tony R. Brown**, 6605 E. Canyon Hills Rd., Anaheim Hills, CA (US) 92807

U.S. PATENT DOCUMENTS

4,735,605	A	*	4/1988	Swartz	604/22
4,867,157	A	*	9/1989	McGurk-Burleson et al.	606/170
4,932,935	A	*	6/1990	Swartz	604/22
5,569,178	A	*	10/1996	Henley	604/22
5,823,990	A	*	10/1998	Henley	604/22
5,906,609	A		5/1999	Assa et al.	

* cited by examiner

(73) Assignee: **Tony R. Brown**, Anaheim, CA (US)

Primary Examiner—Alfred Basichas

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(74) *Attorney, Agent, or Firm*—Burns, Doane, Swecker & Mathhis, LLP

(57)

ABSTRACT

A fat removal device includes a screen which includes passages through which fat can be extruded, to be cut or melted away from the surface of an internal organ. The device includes a blade to cut the fat or radiofrequency monopolar or bipolar electrodes to melt the fat, aspiration to remove the fat away from the screen and blade, irrigation to irrigate the screen and blade, and an electrocautery member to cauterize the capillary bed of the fat. Methods of using removing the fat layer from the surface of an internal body organ are also described.

(21) Appl. No.: **09/874,360**

(22) Filed: **Jun. 6, 2001**

(65) **Prior Publication Data**


US 2002/0188280 A1 Dec. 12, 2002

(51) **Int. Cl.**⁷ **A61M 1/00**; A61B 17/32

(52) **U.S. Cl.** **604/542**; 604/540; 604/902; 606/170

(58) **Field of Search** 604/542, 540, 604/902, 264, 22; 606/167, 170, 180

53 Claims, 31 Drawing Sheets

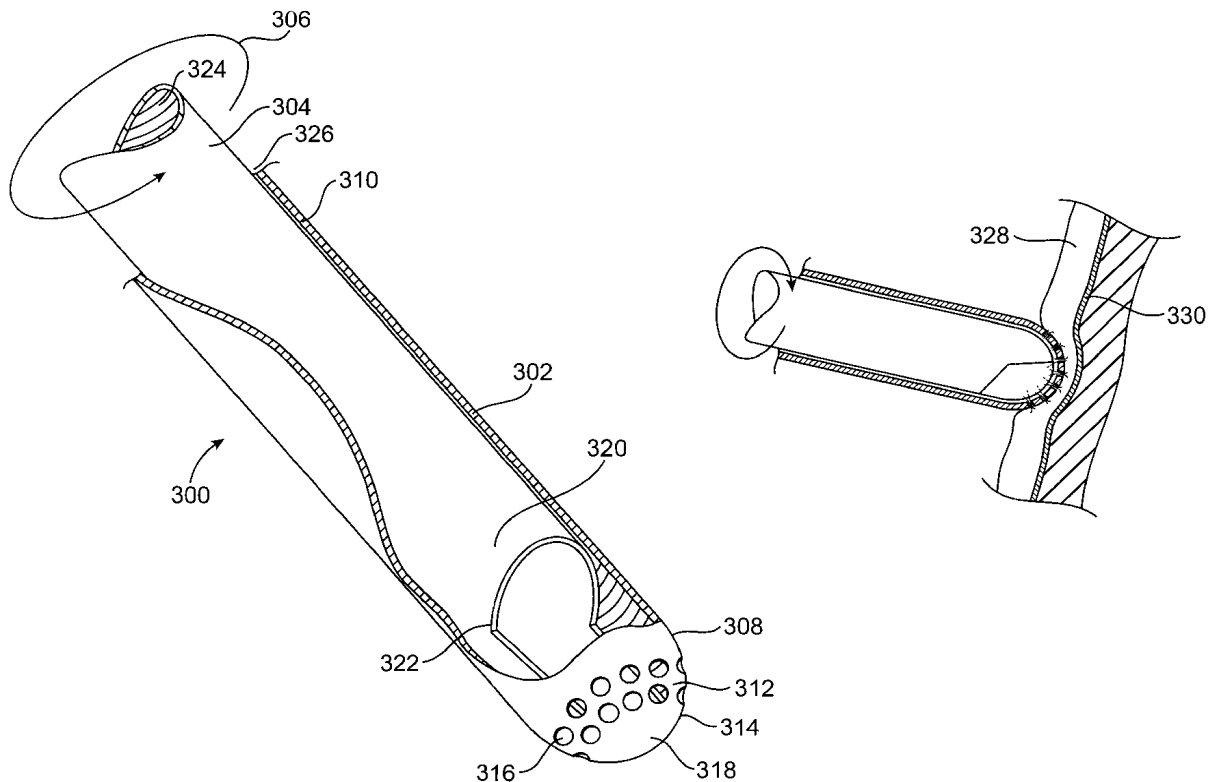

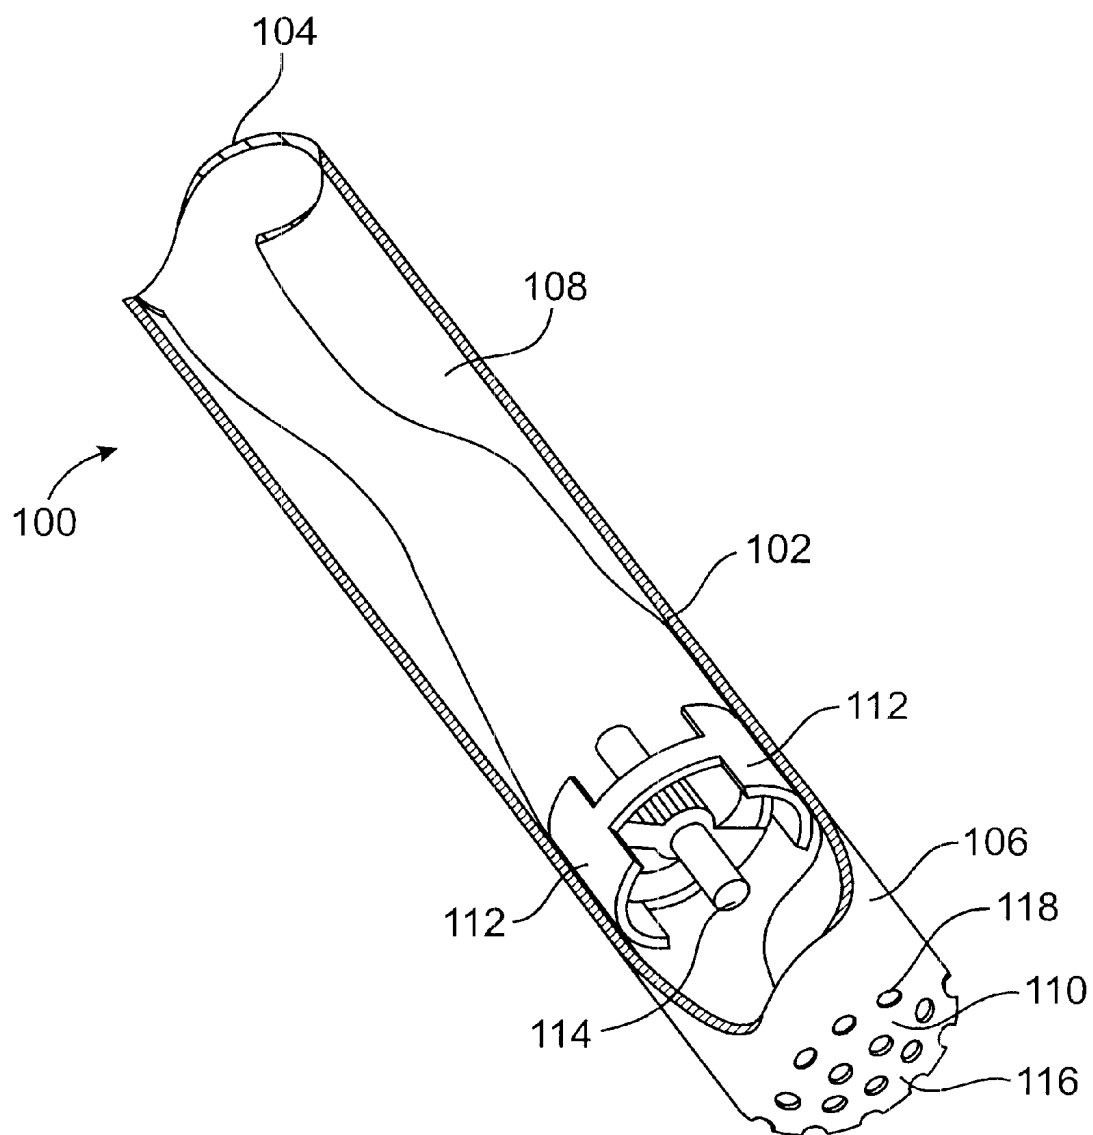


FIG. 1

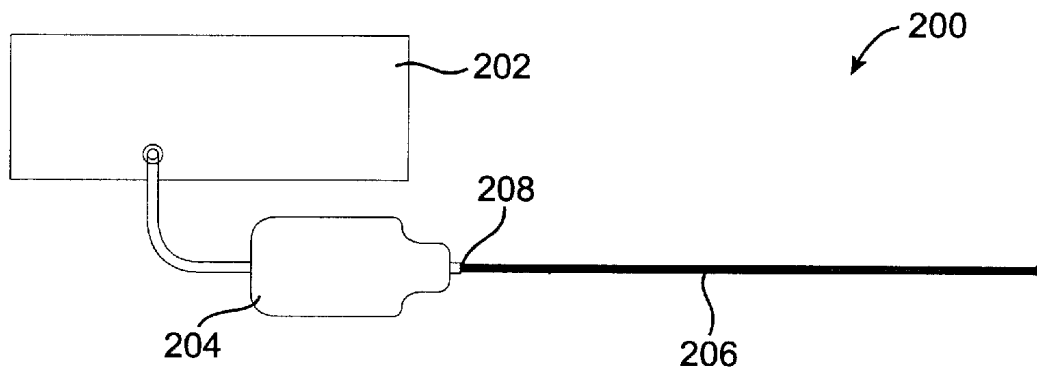


FIG. 2

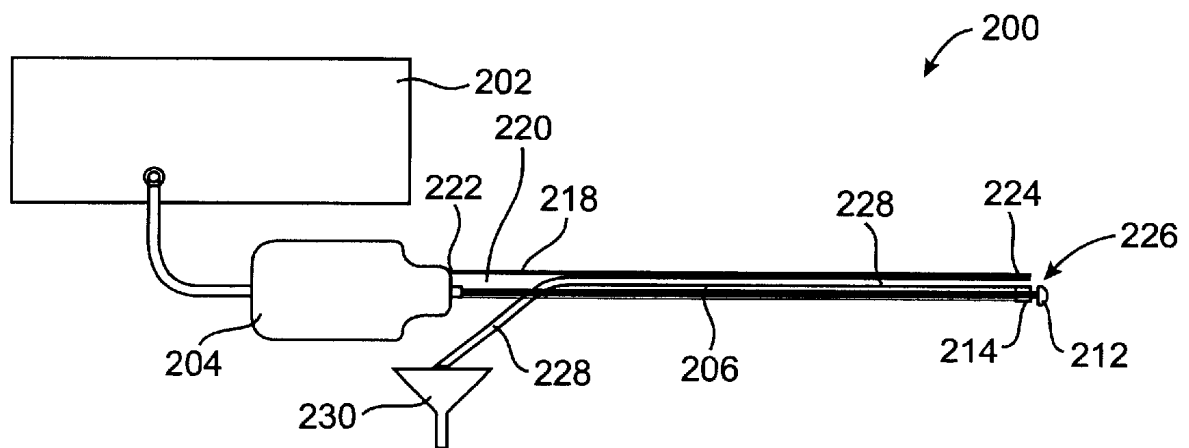


FIG. 3

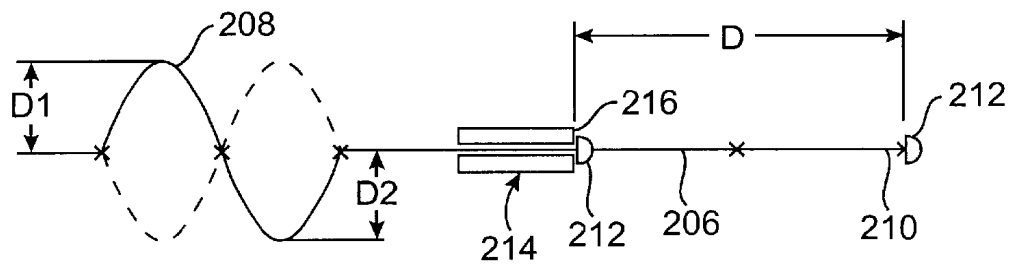


FIG. 4

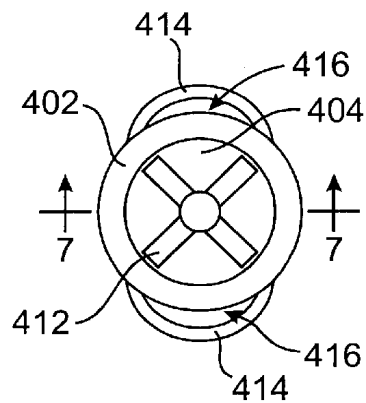


FIG. 8

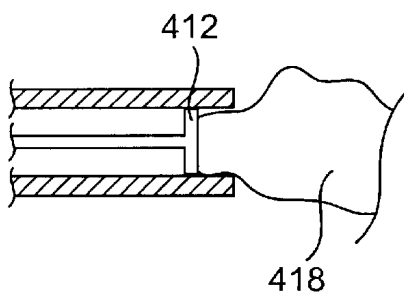


FIG. 9

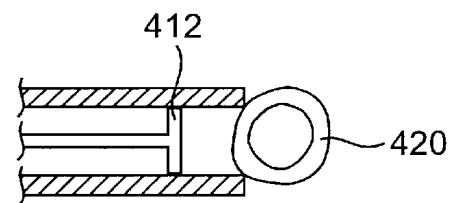
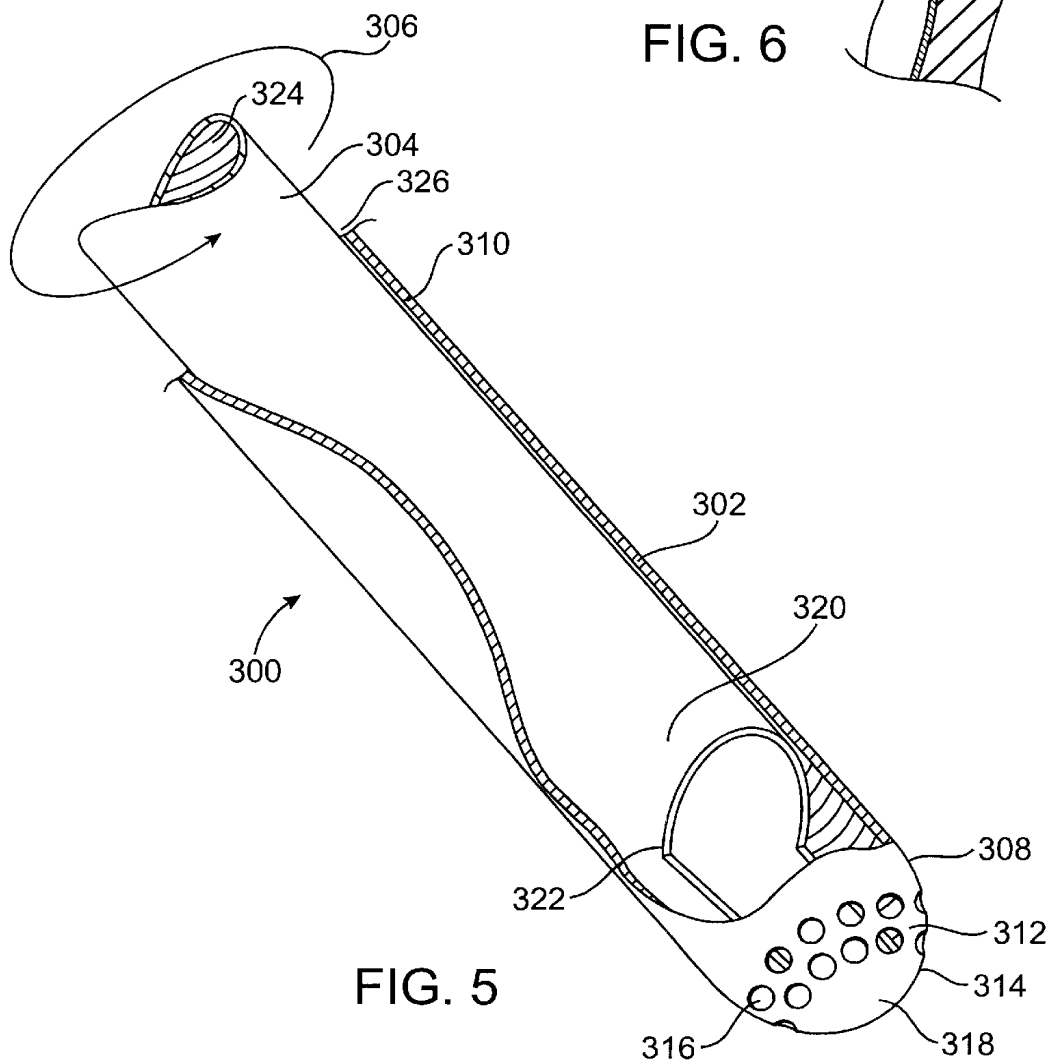
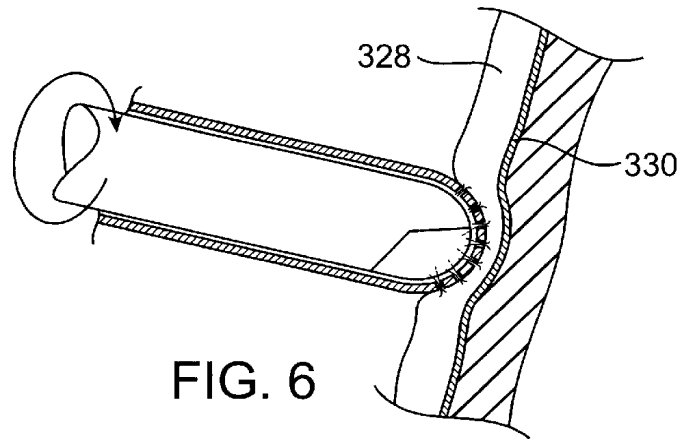
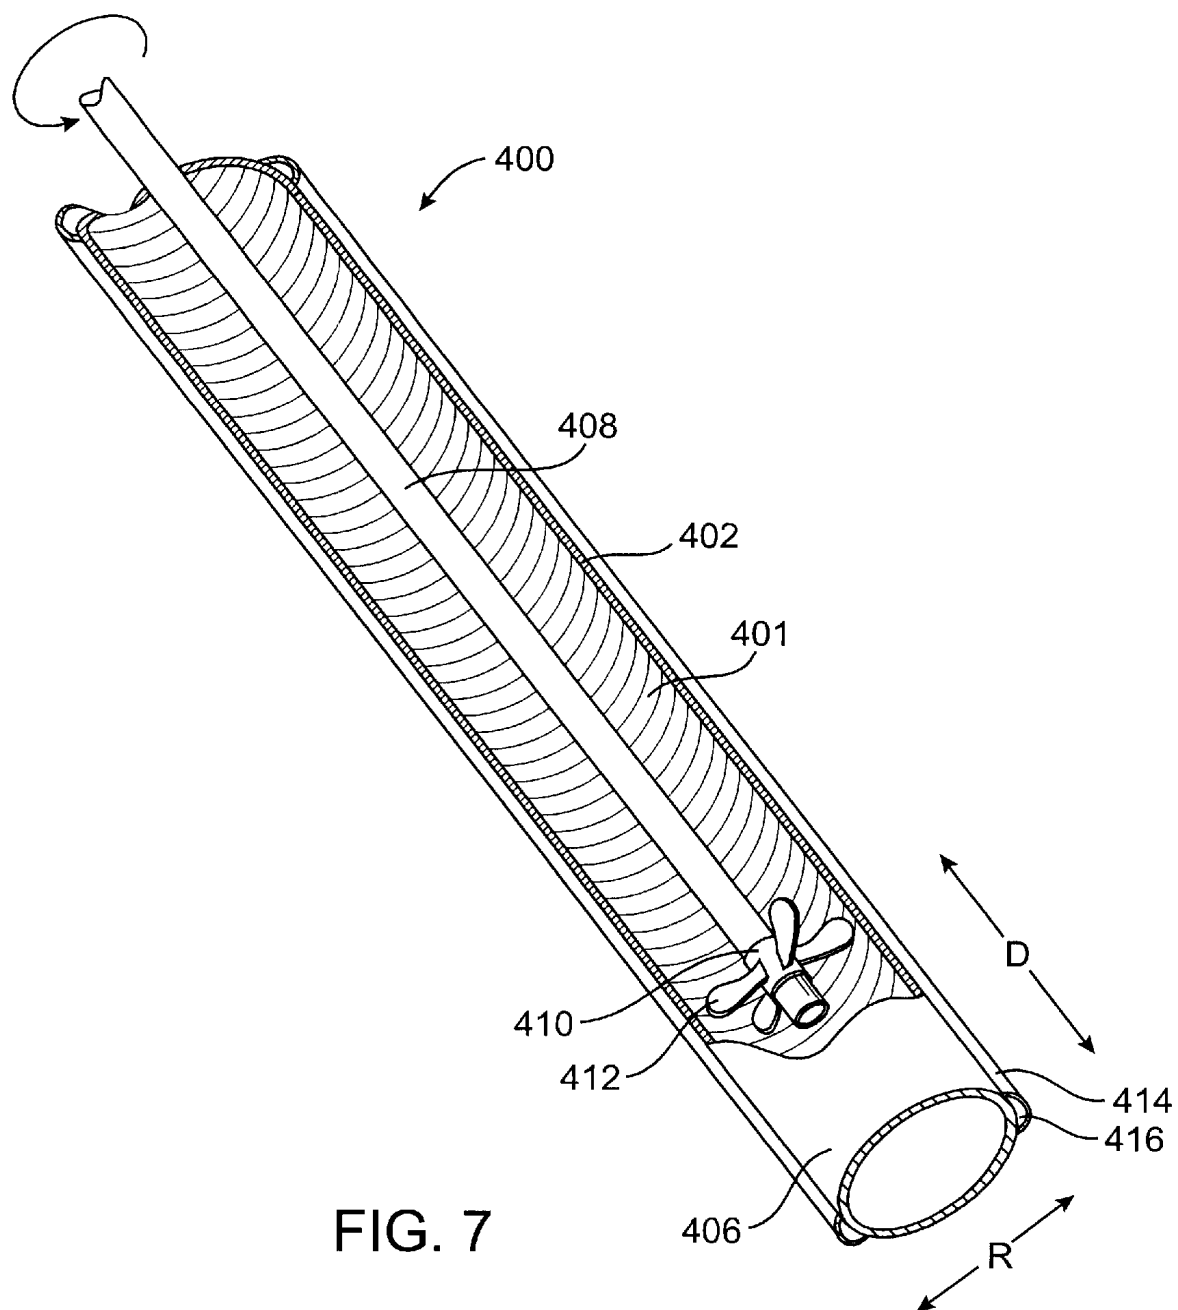


FIG. 10





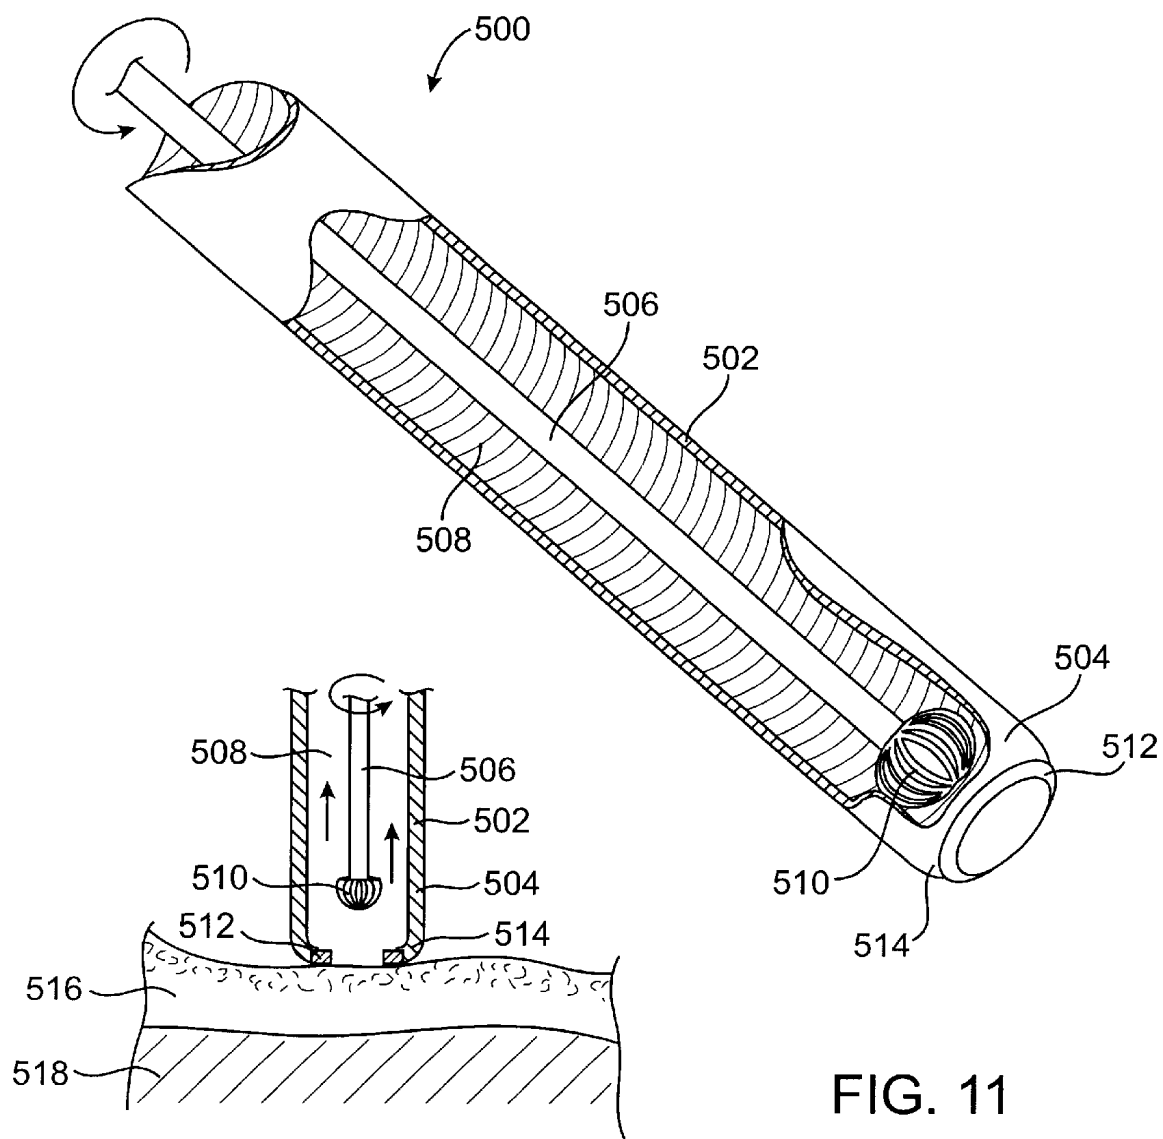
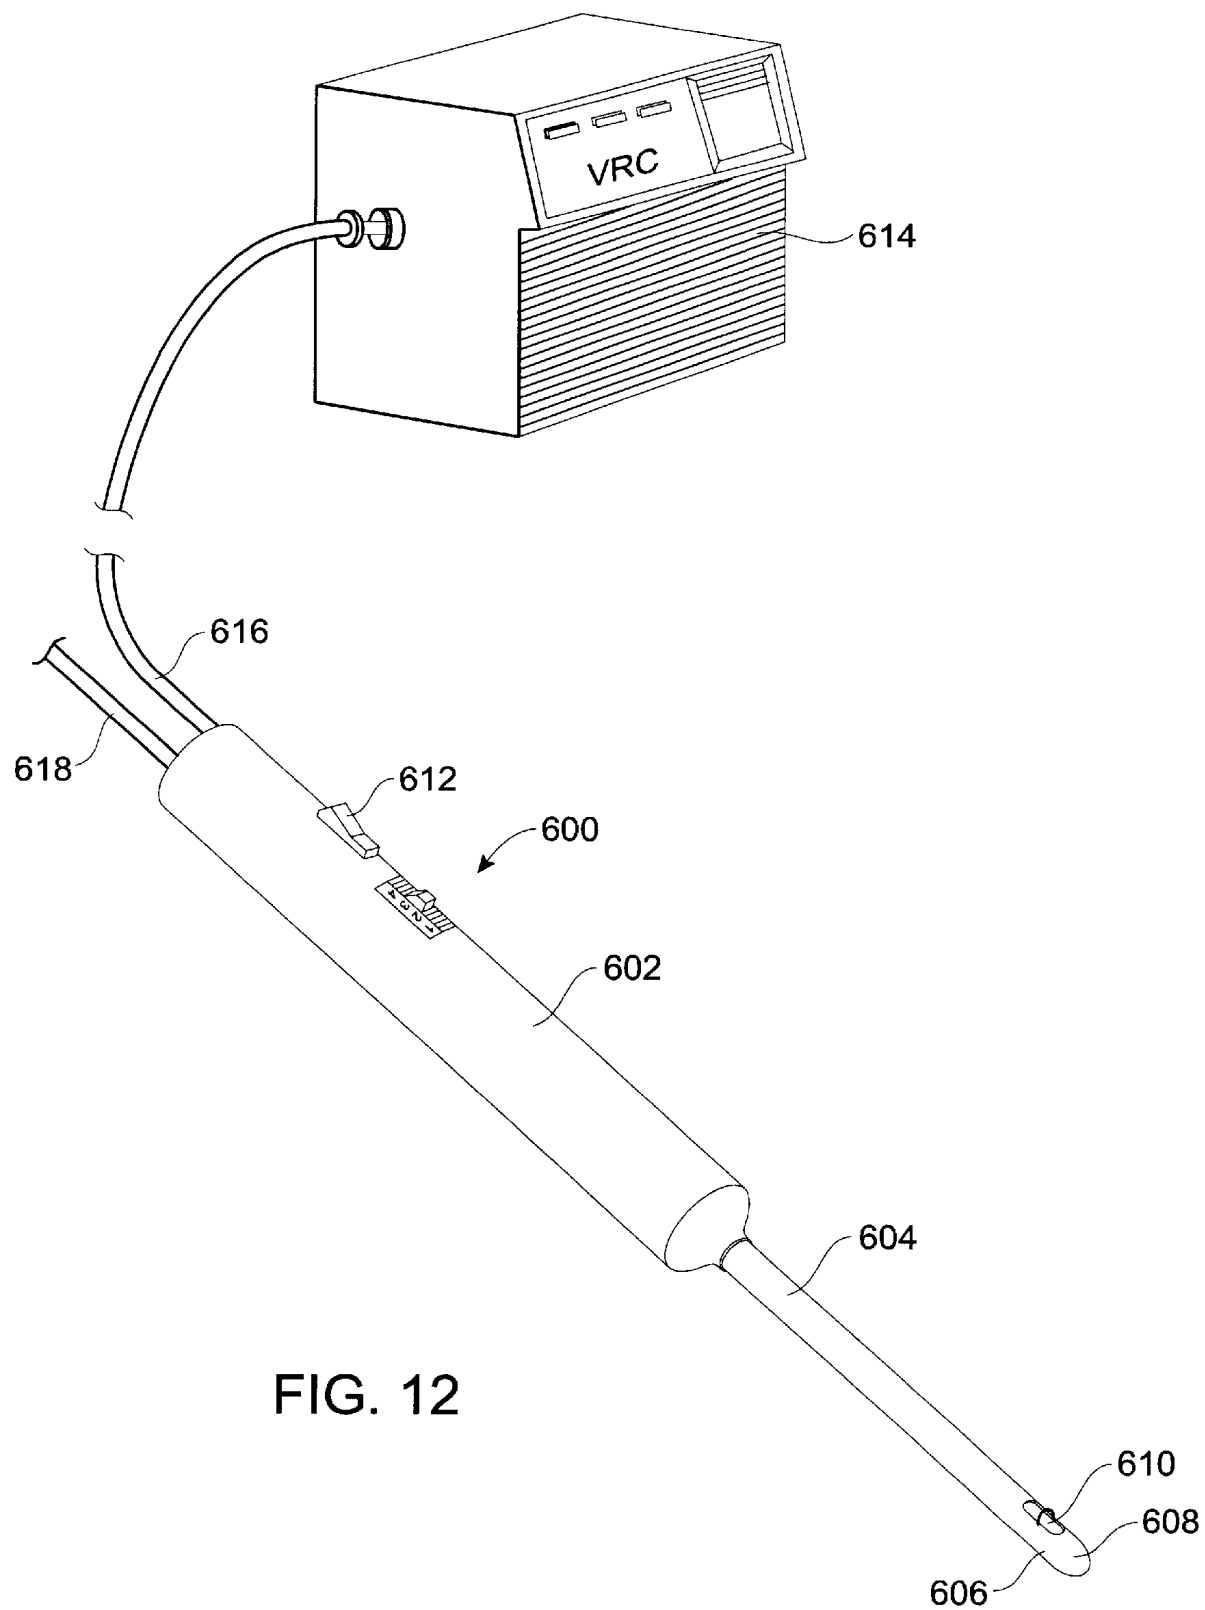


FIG. 11



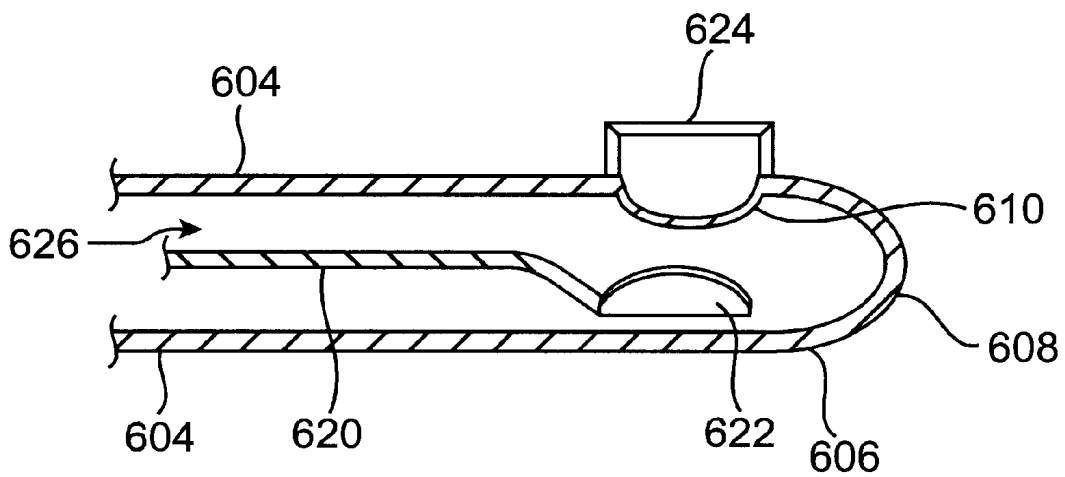


FIG. 13

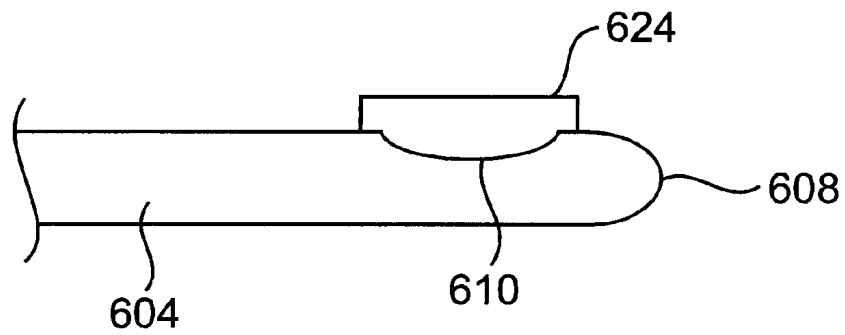


FIG. 14

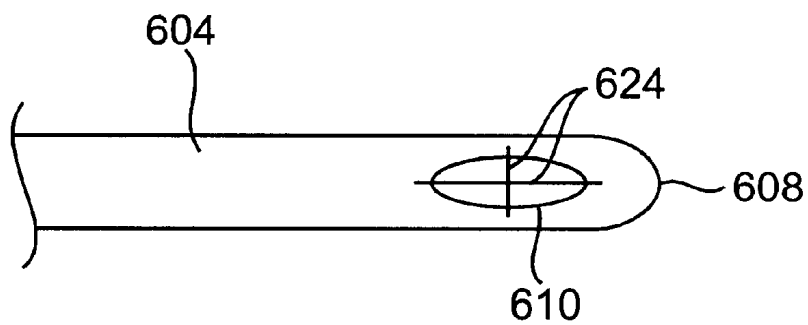
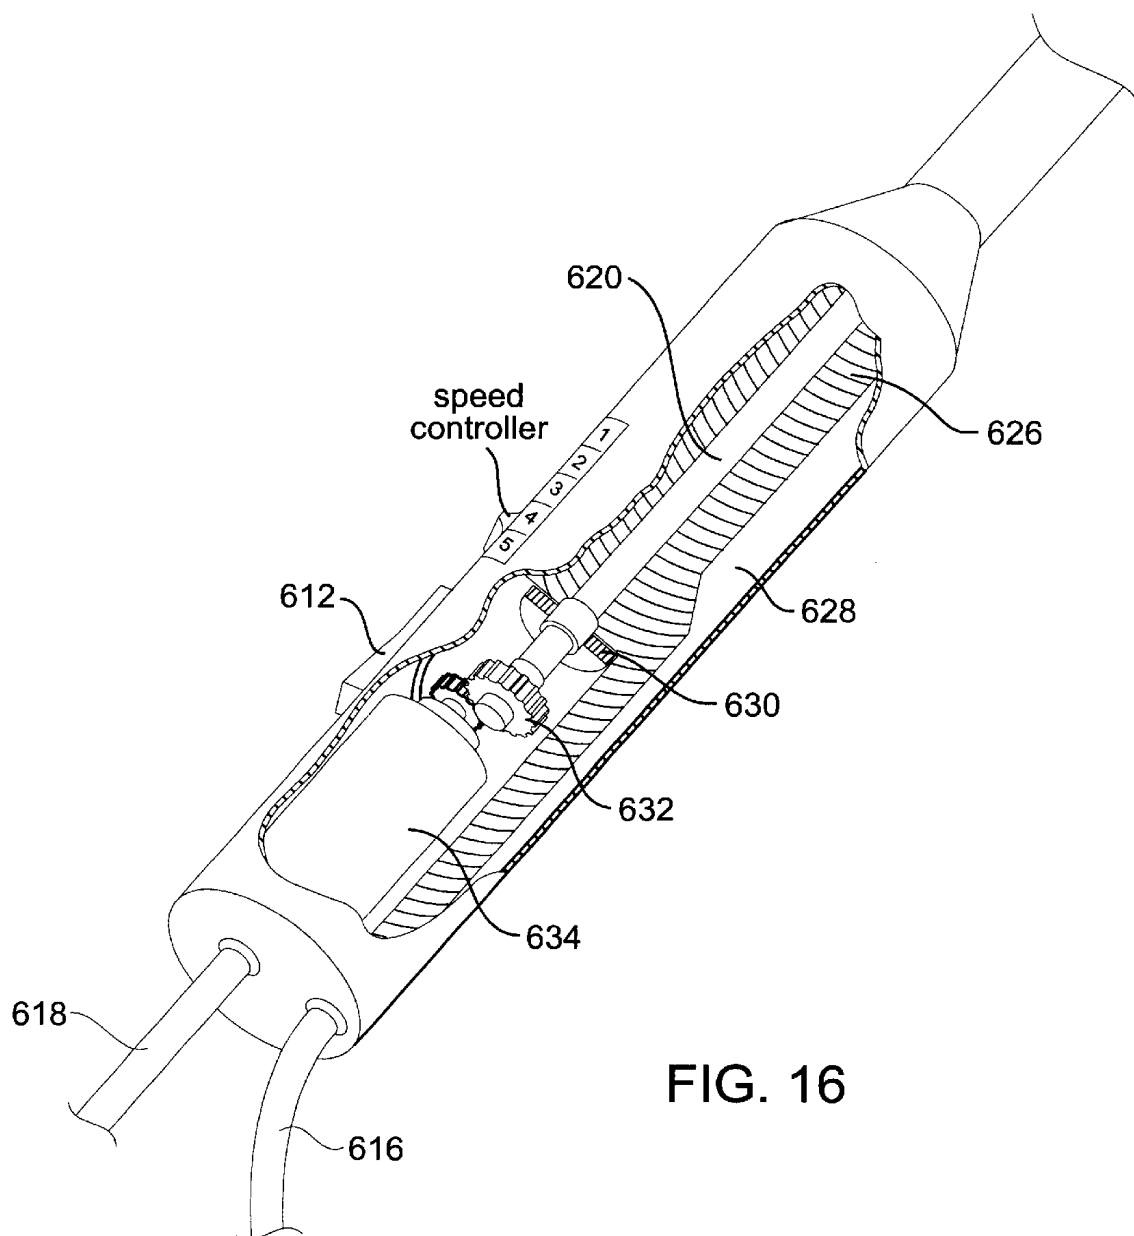


FIG. 15



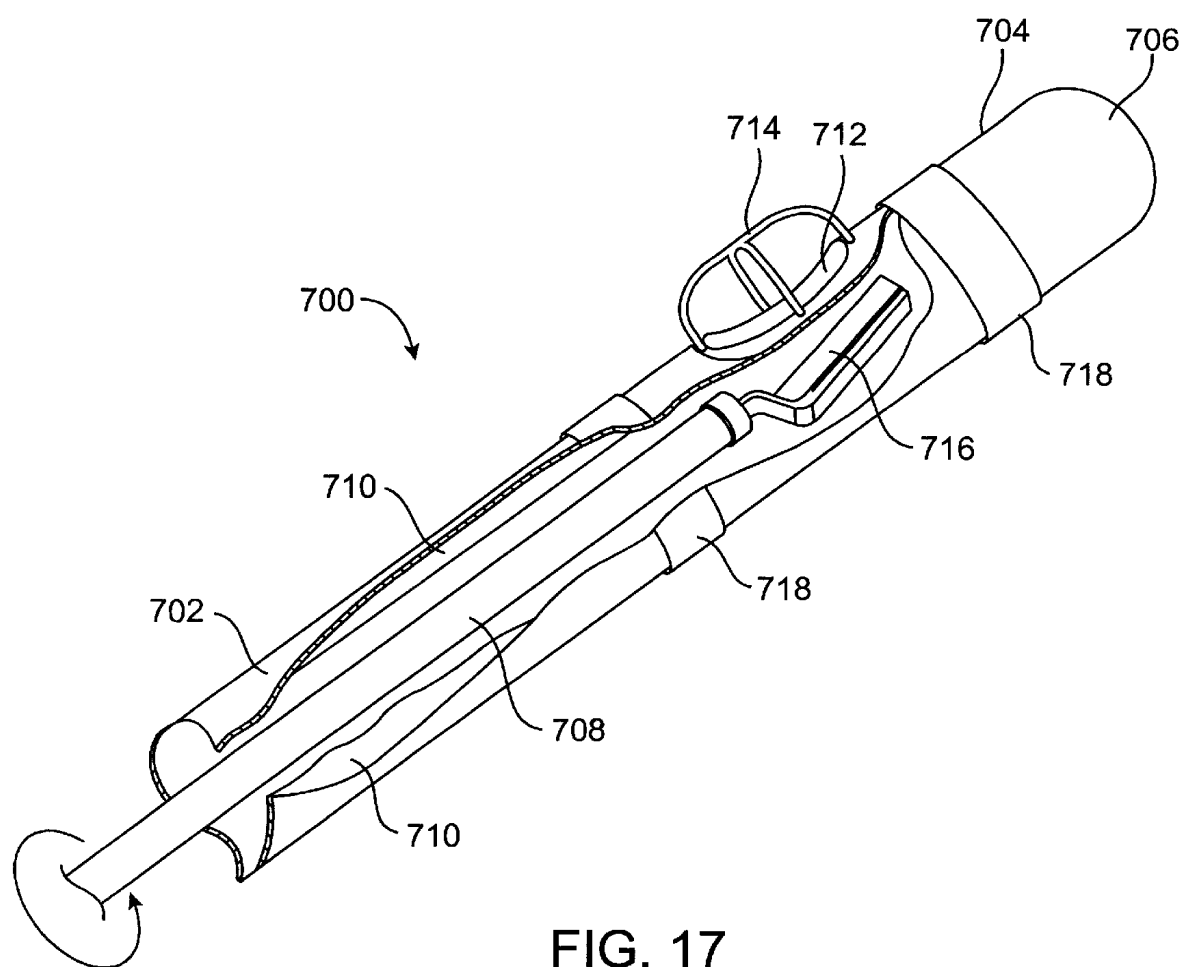


FIG. 17

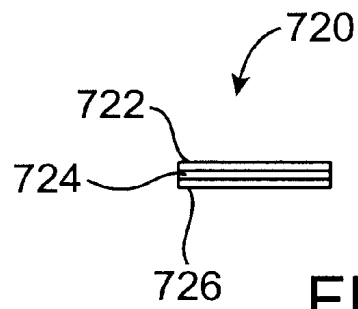


FIG. 18

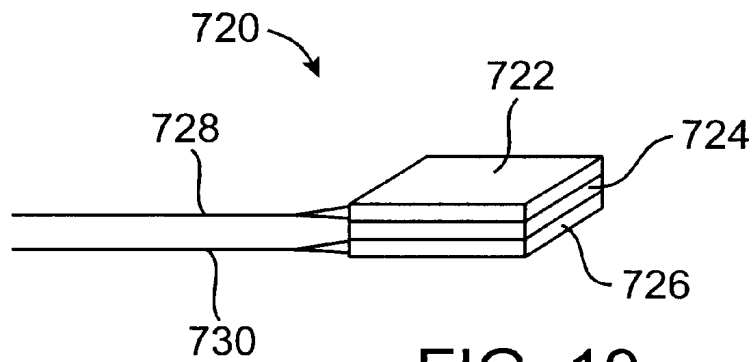


FIG. 19

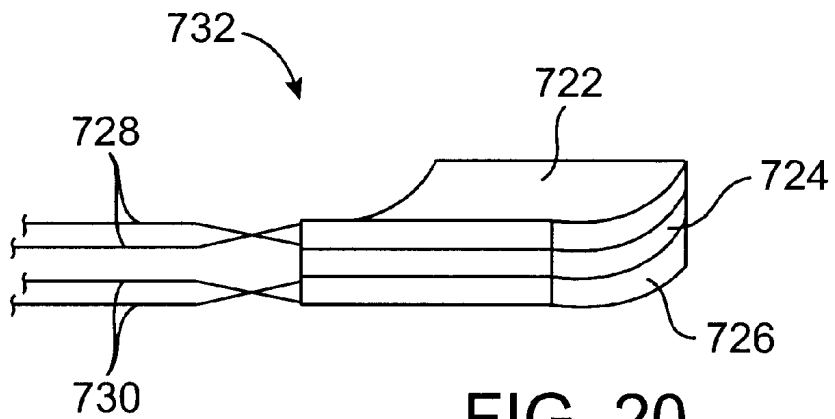
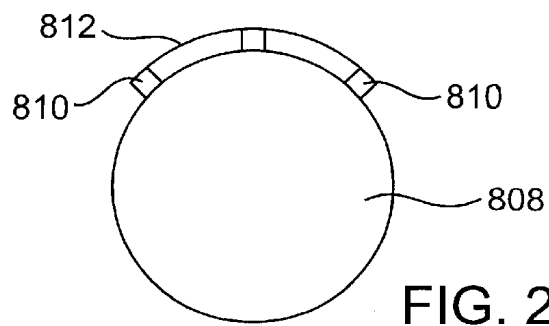
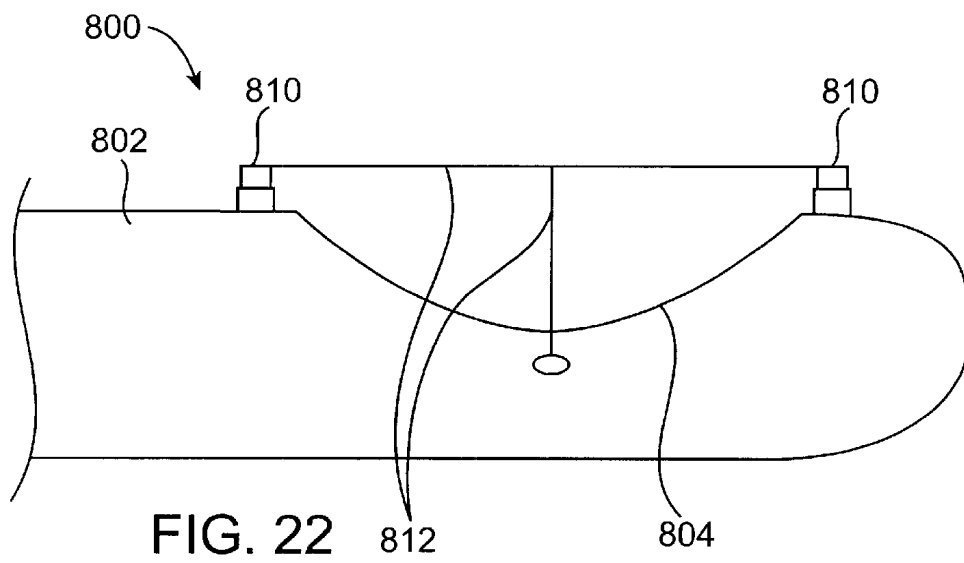
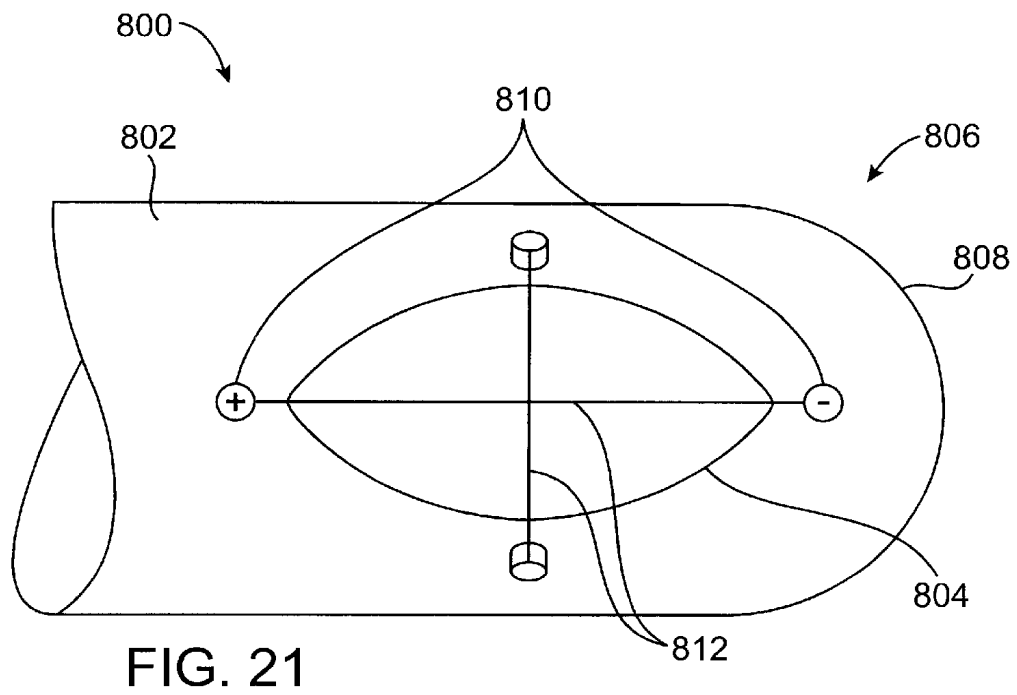


FIG. 20



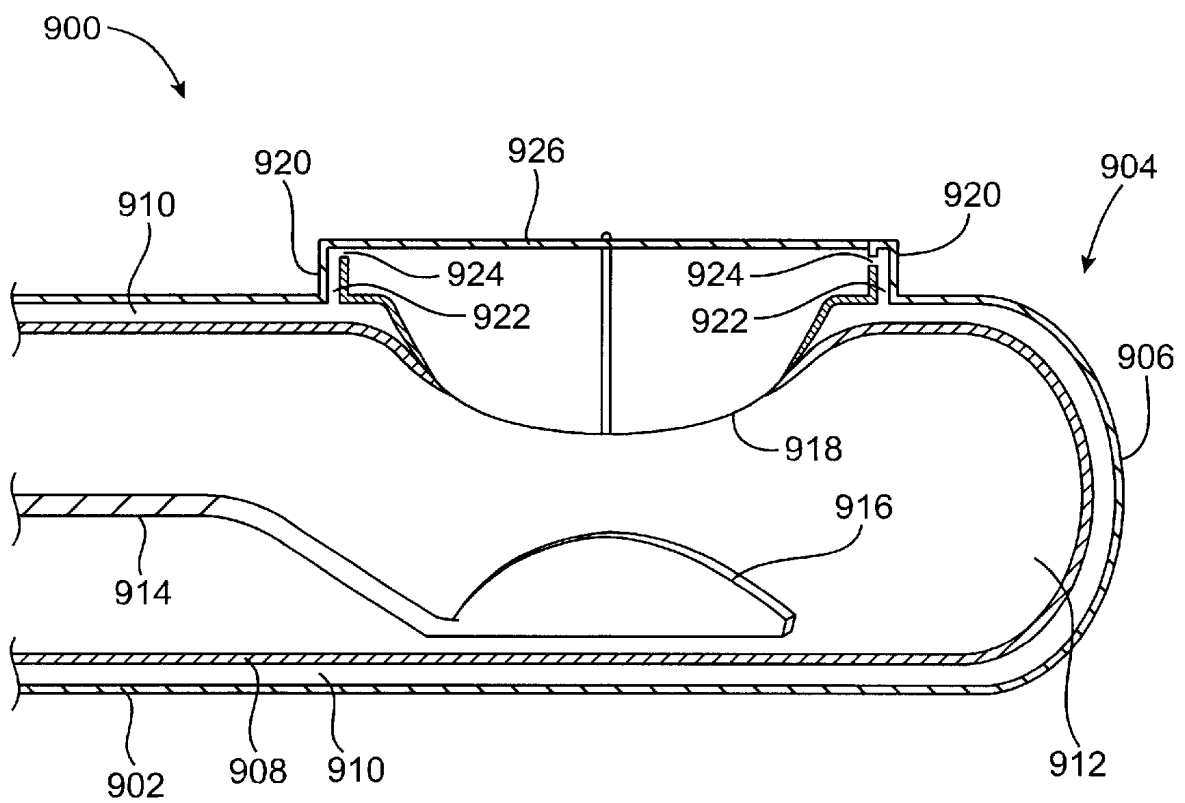


FIG. 24

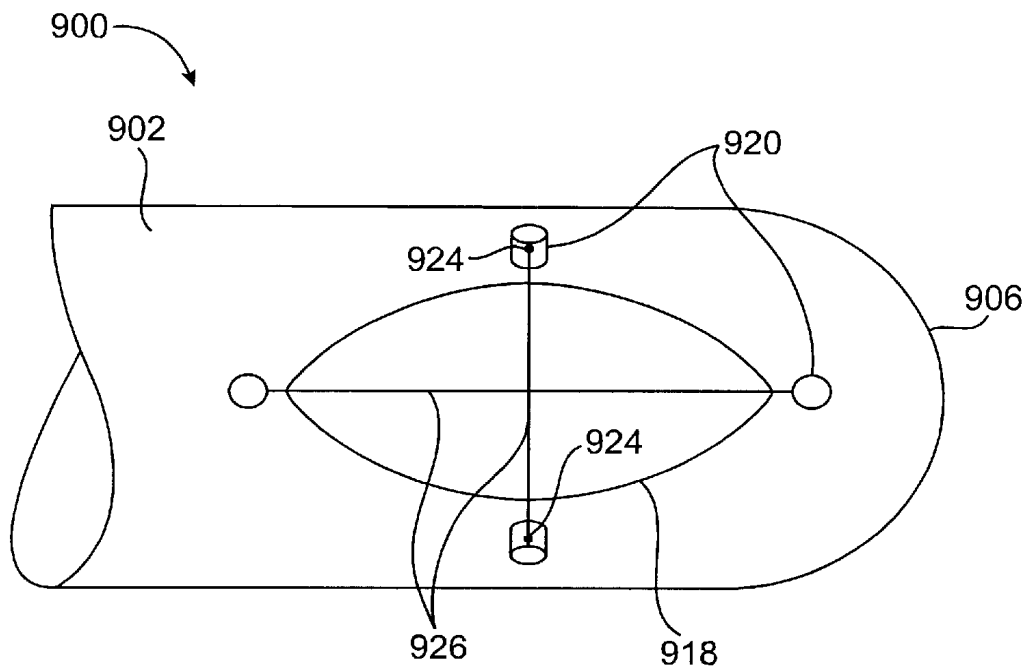
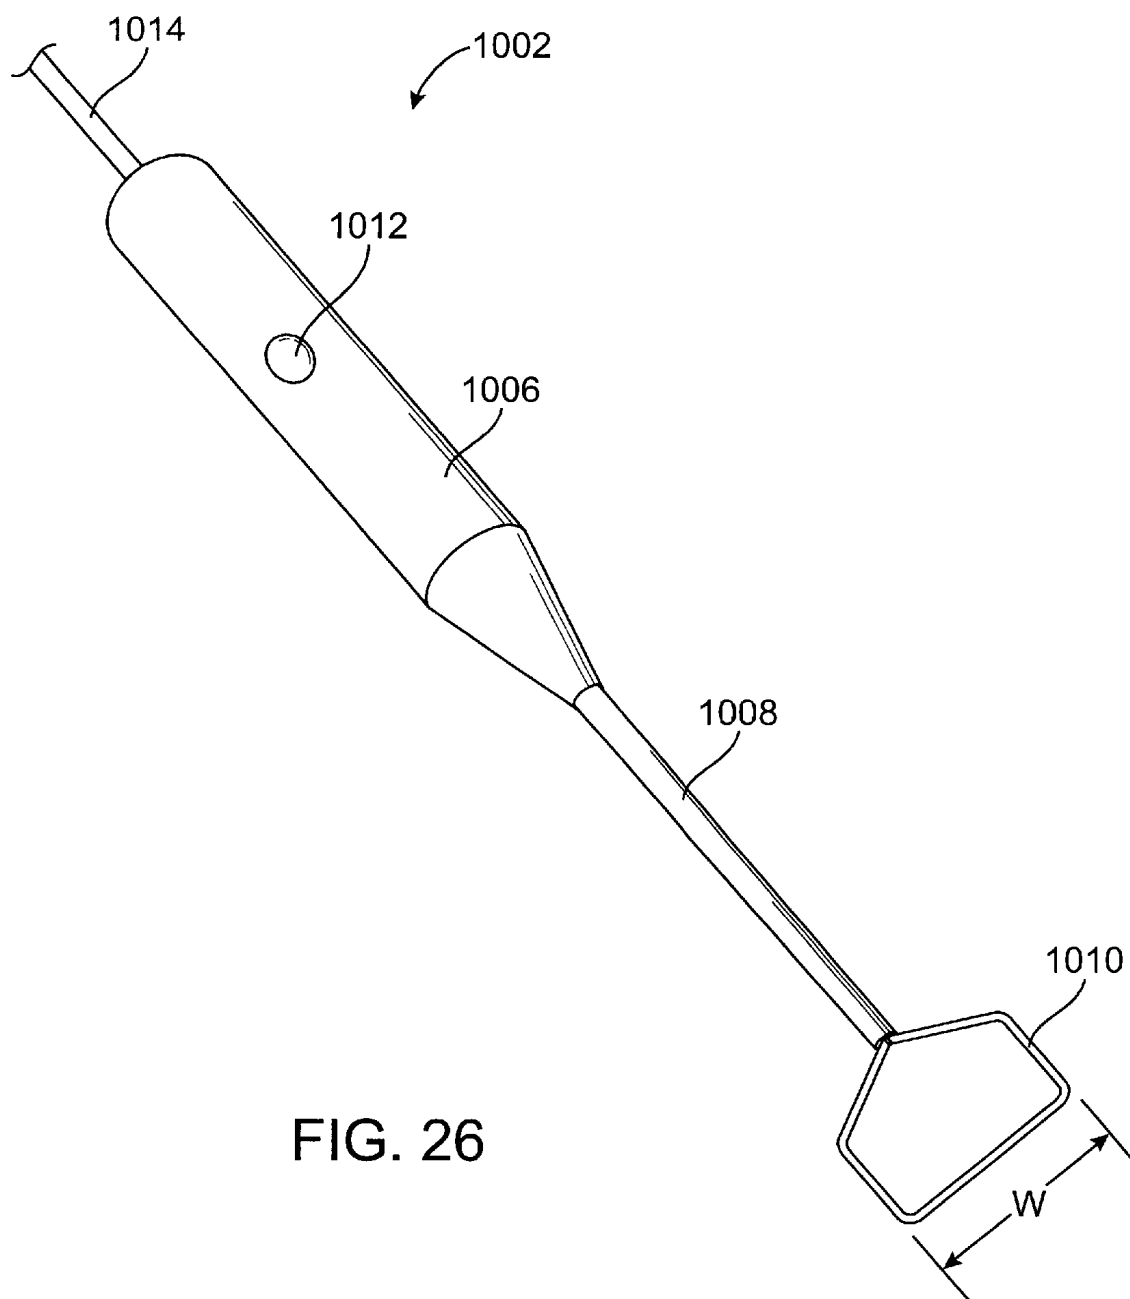


FIG. 25



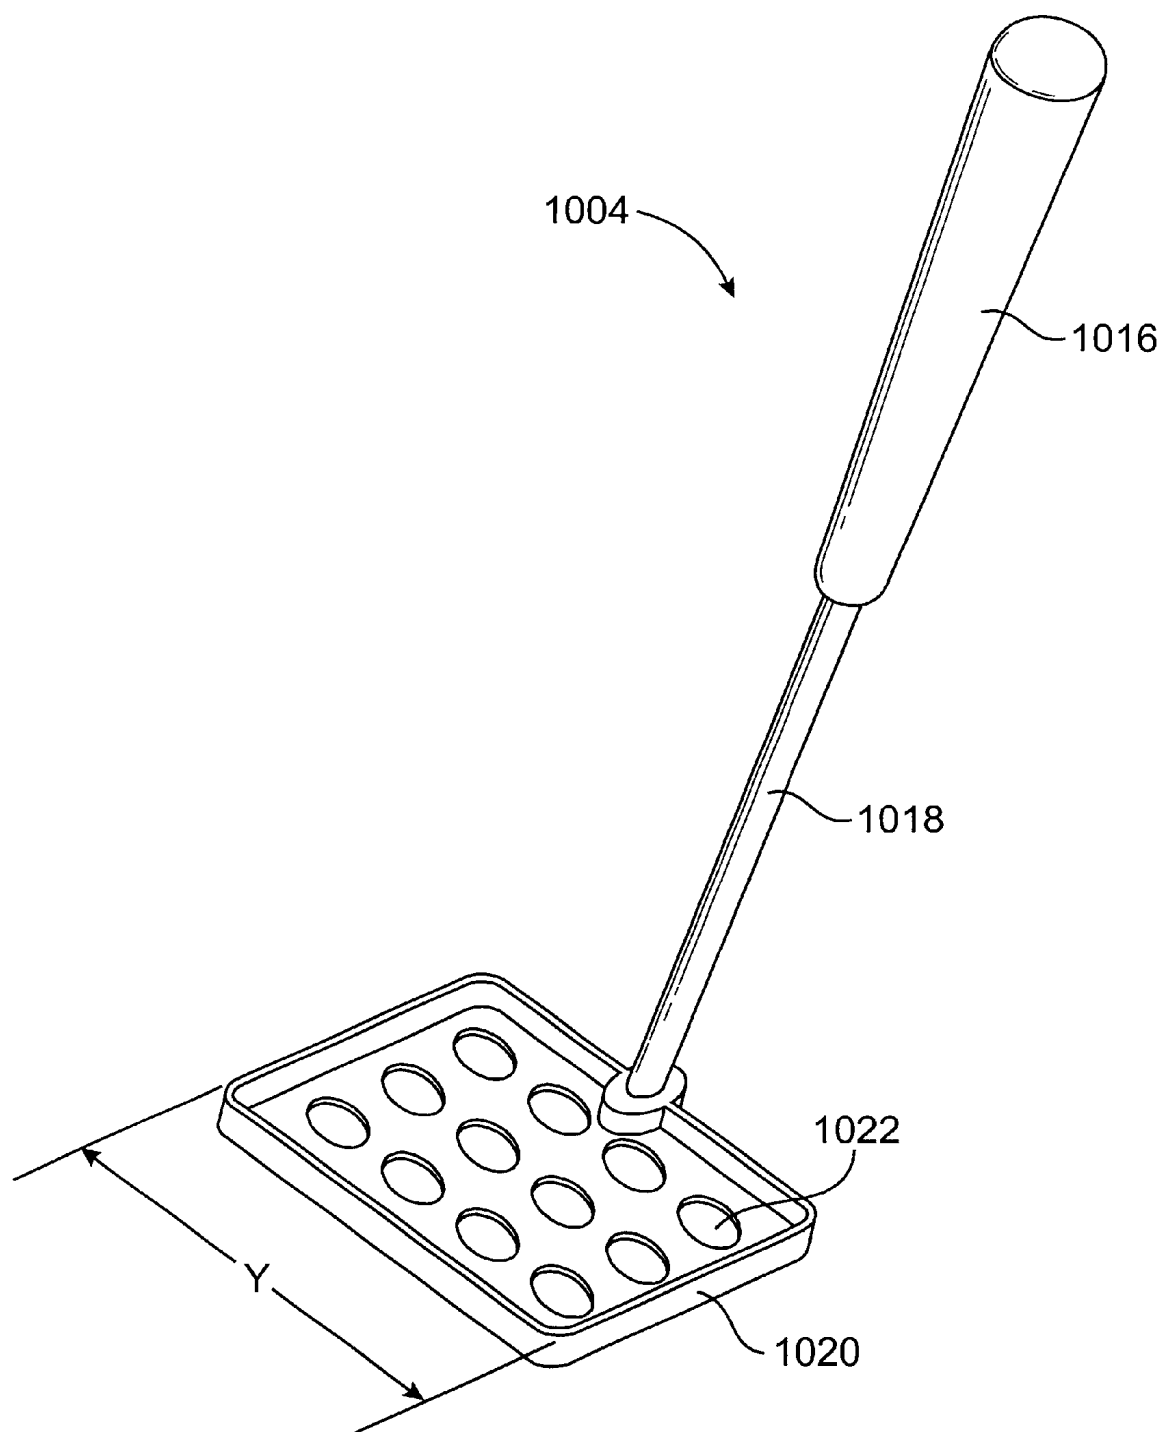


FIG. 27

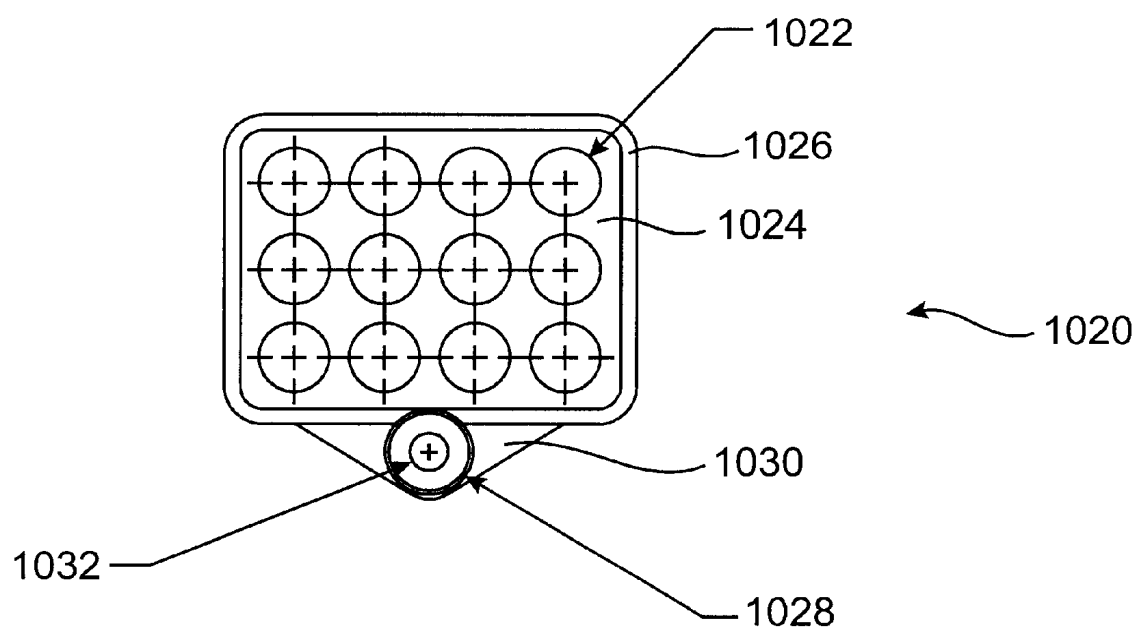


FIG. 28

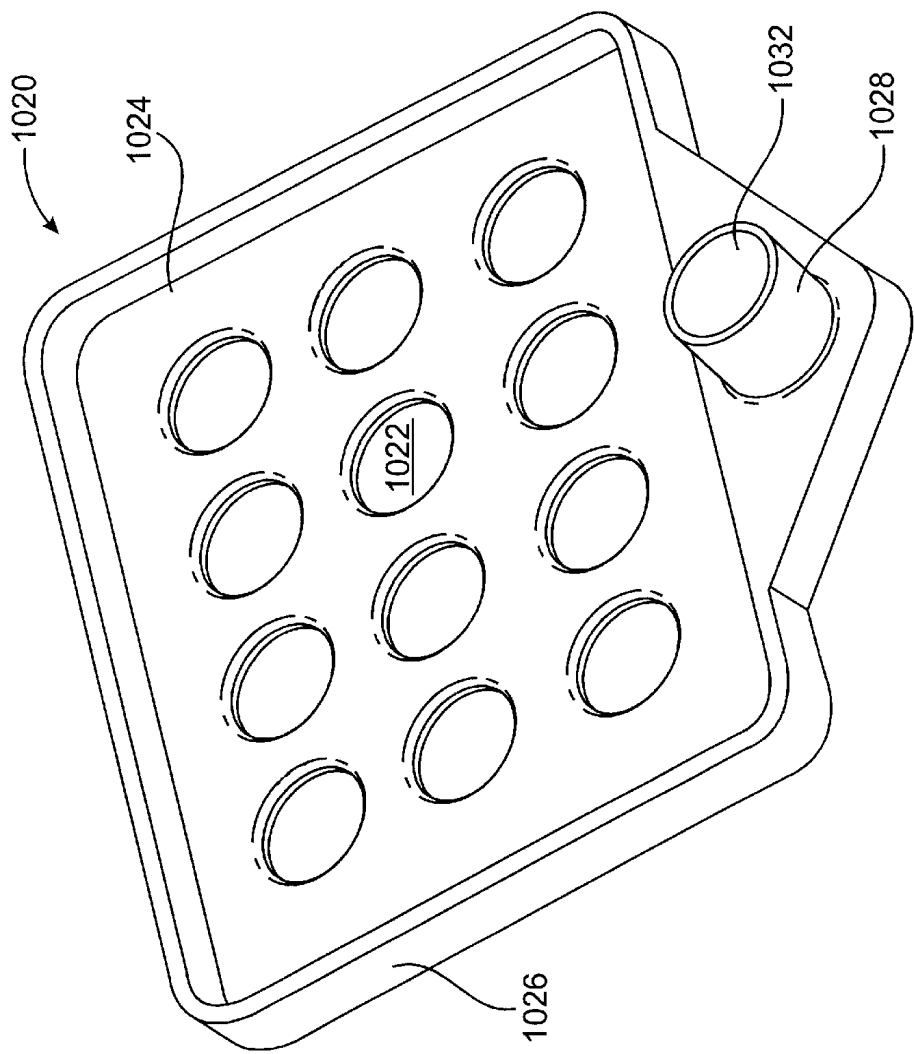
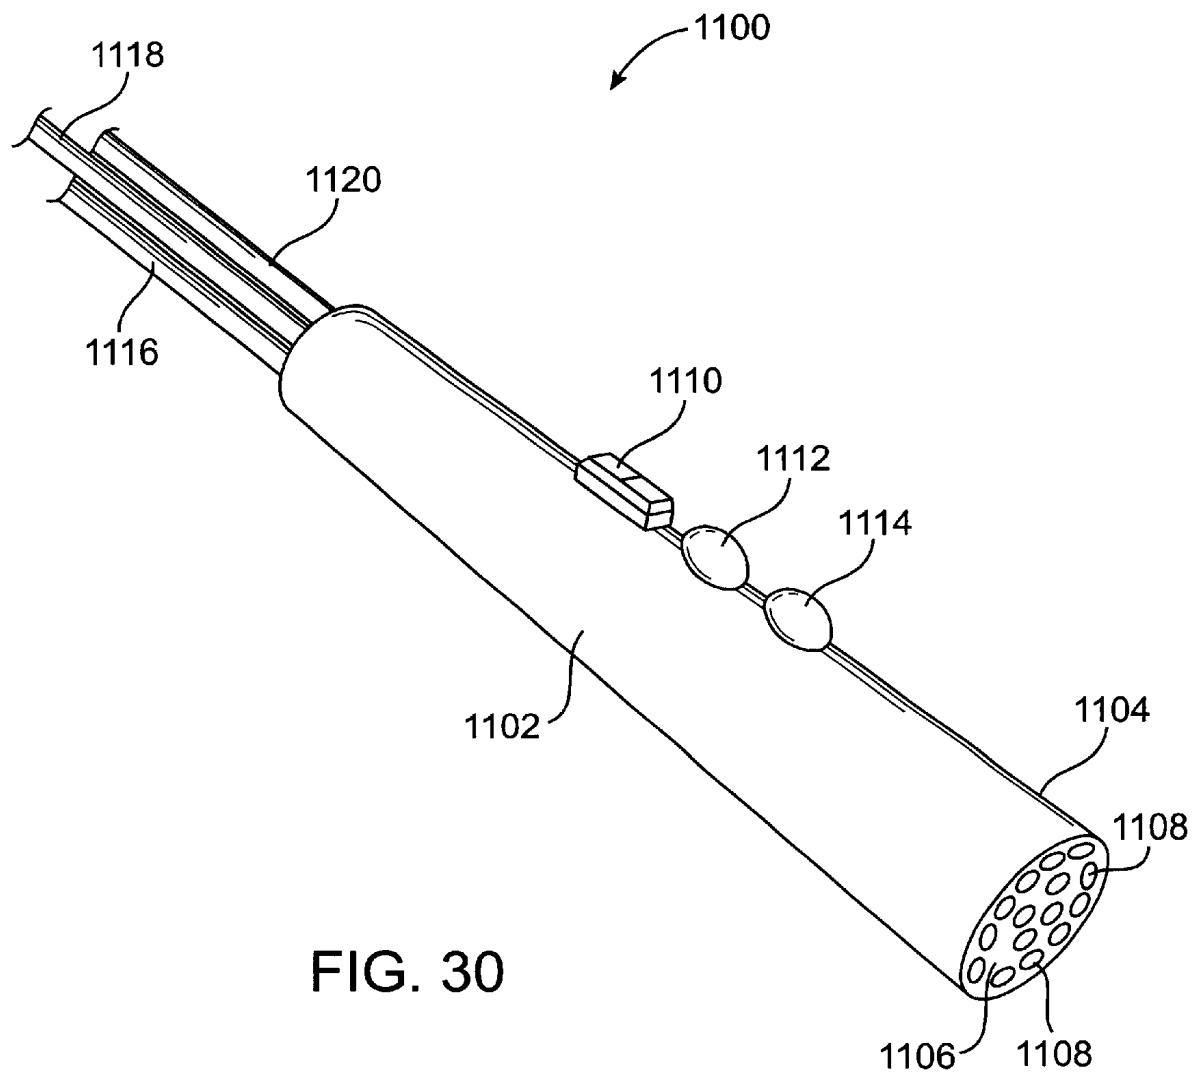


FIG. 29



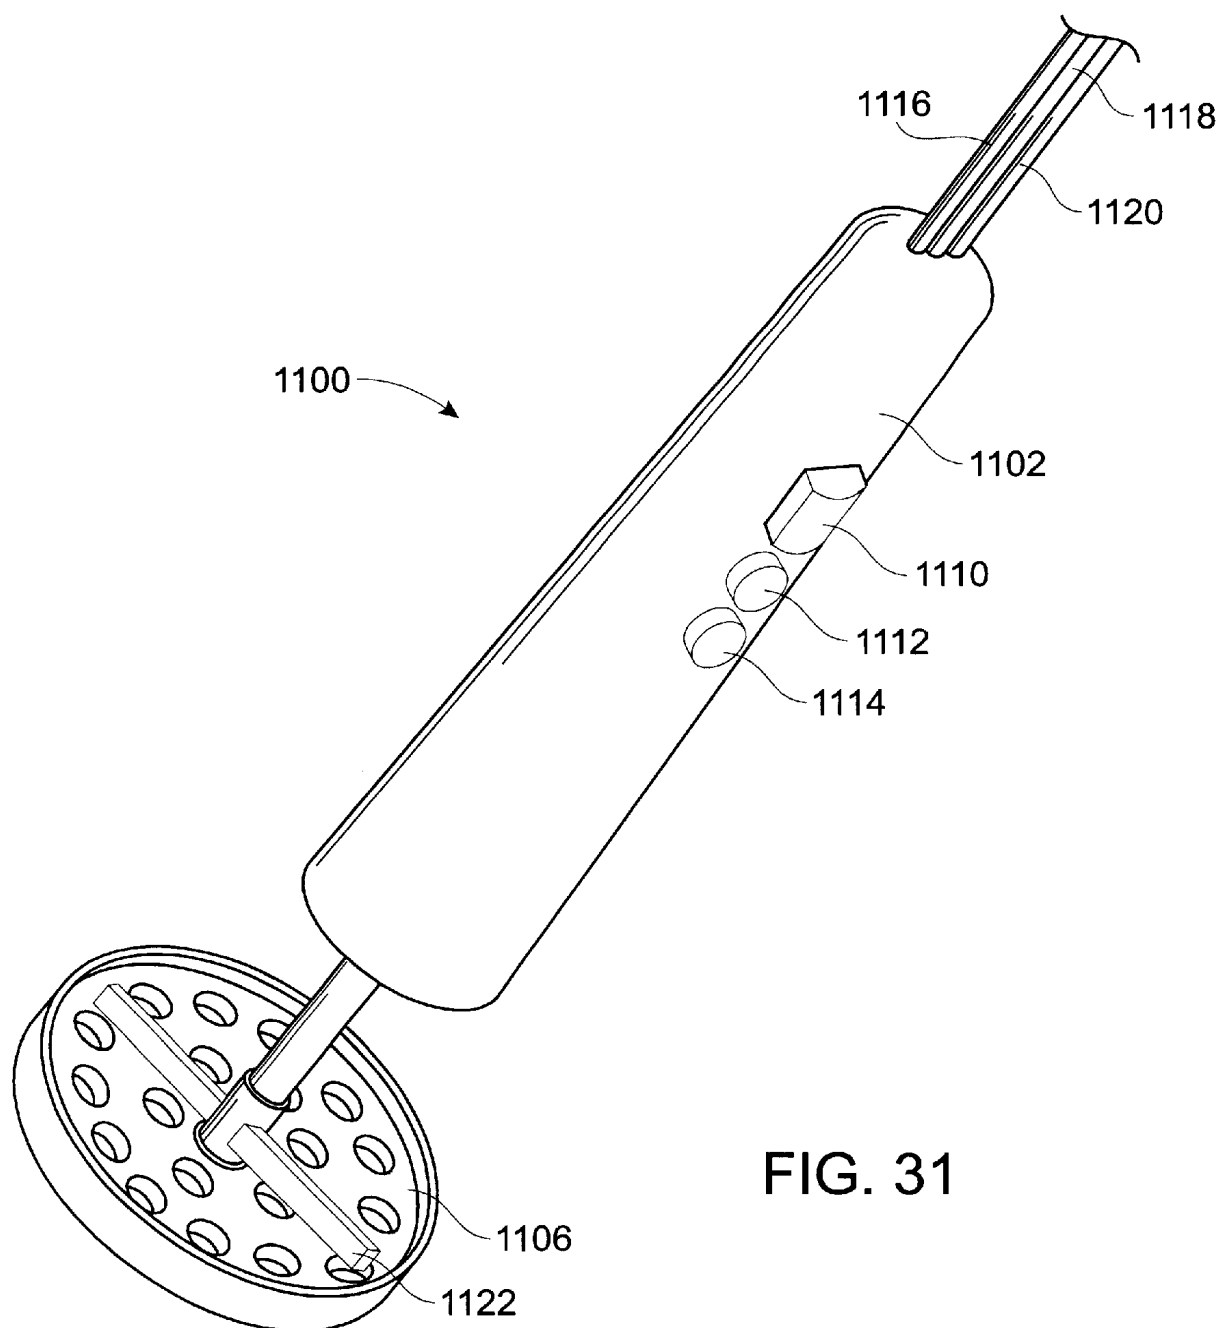


FIG. 31

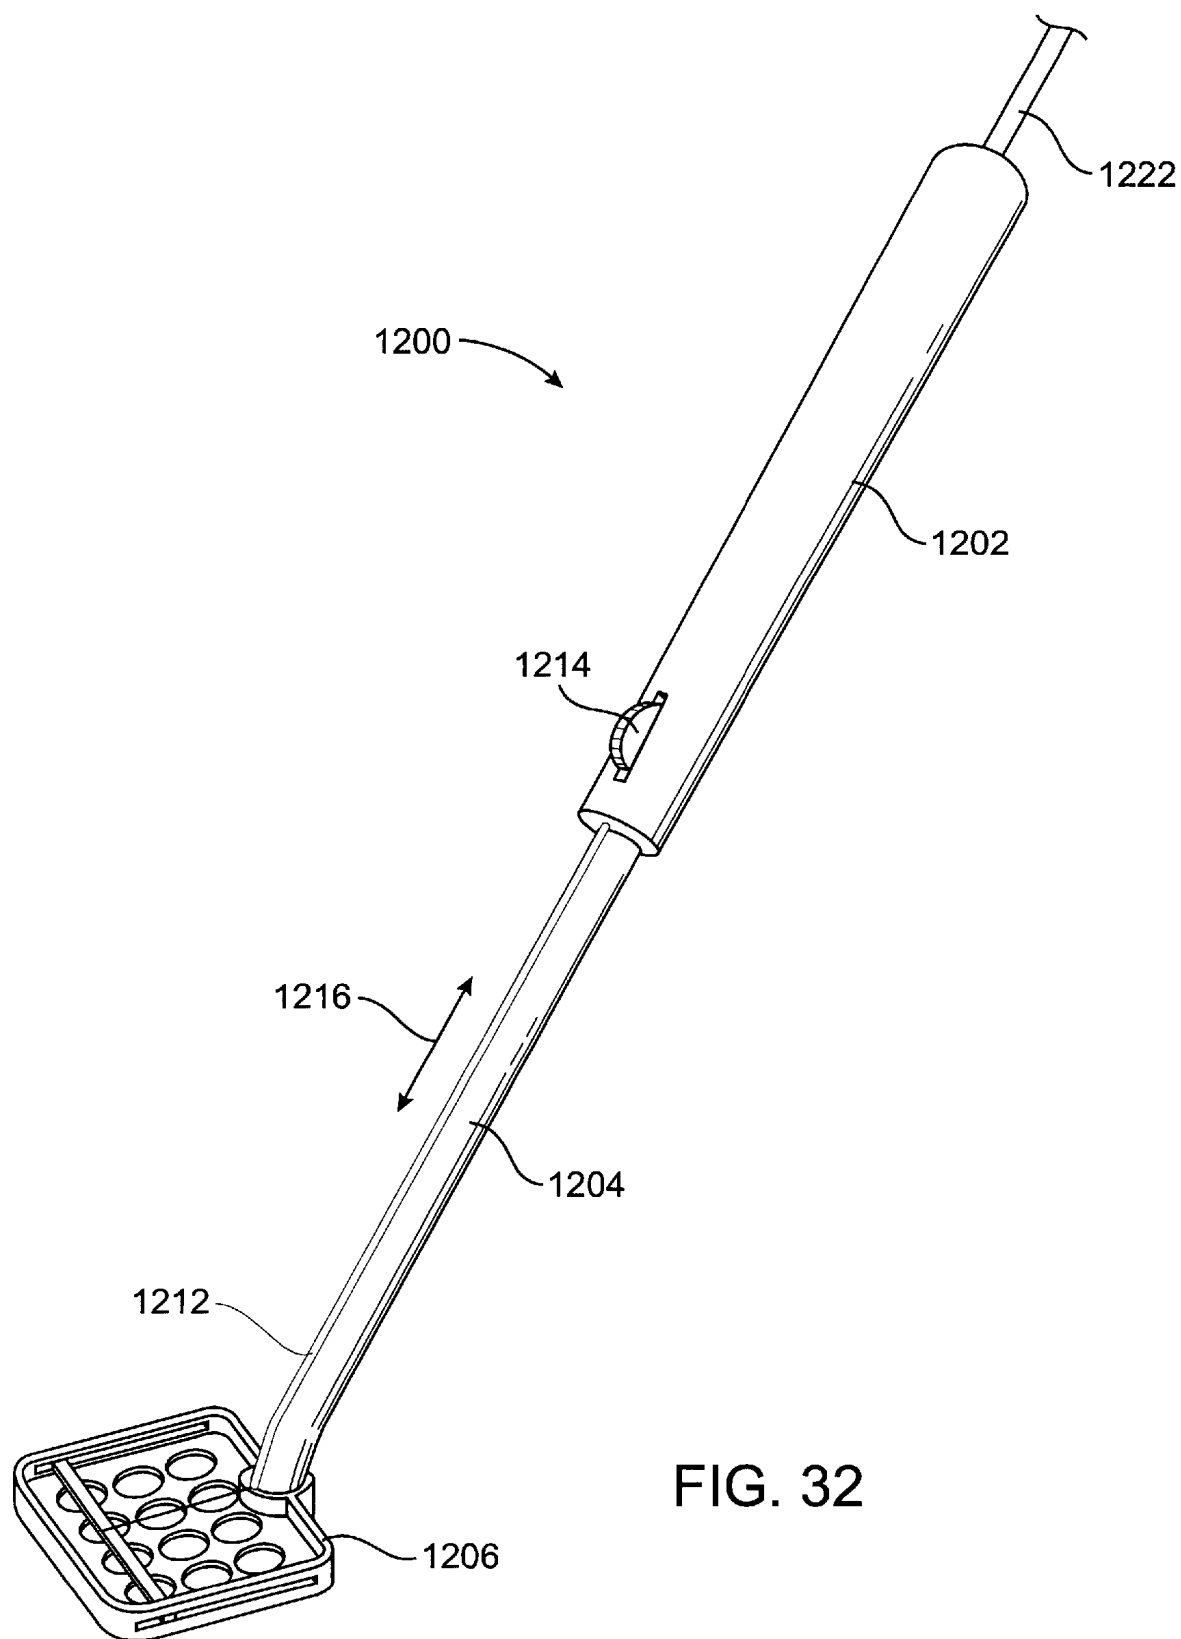


FIG. 32

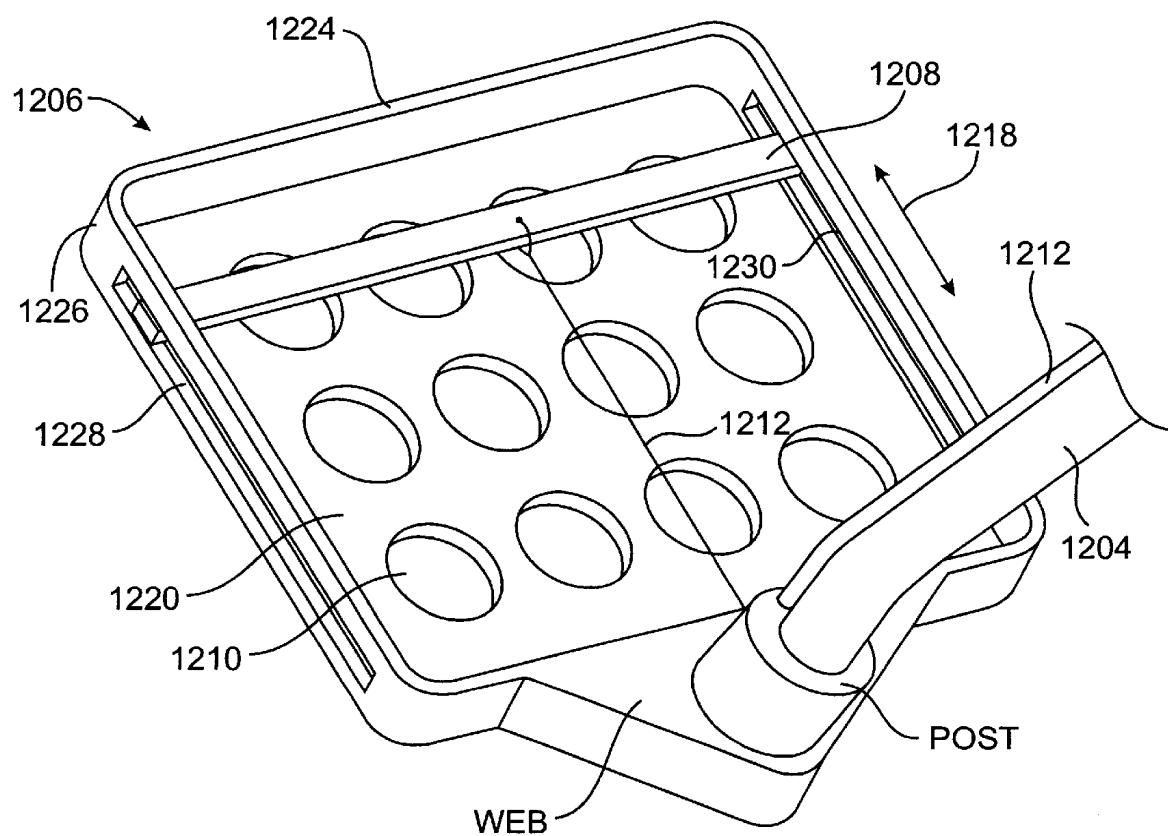
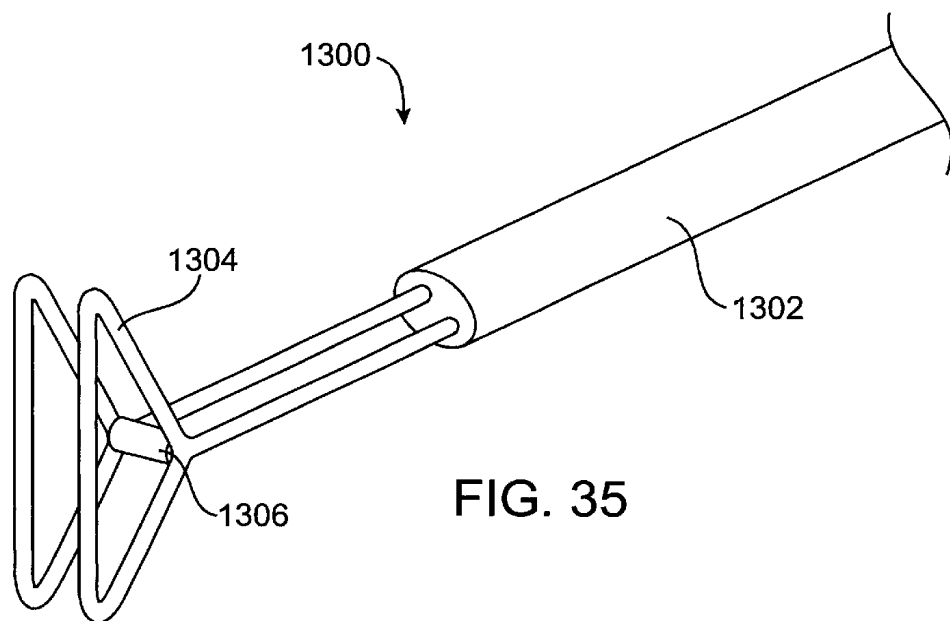
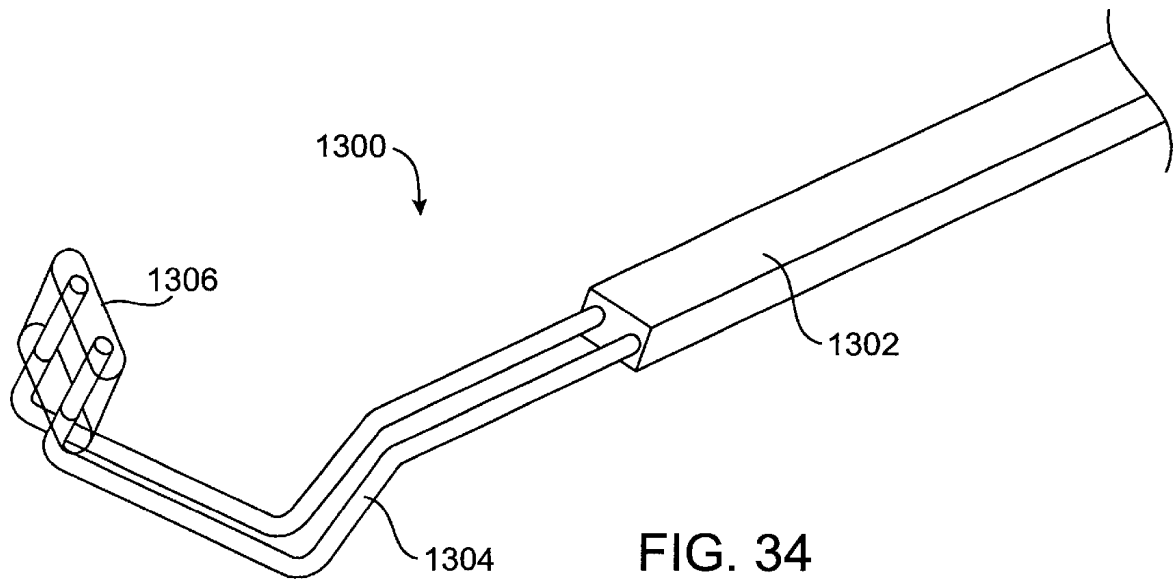
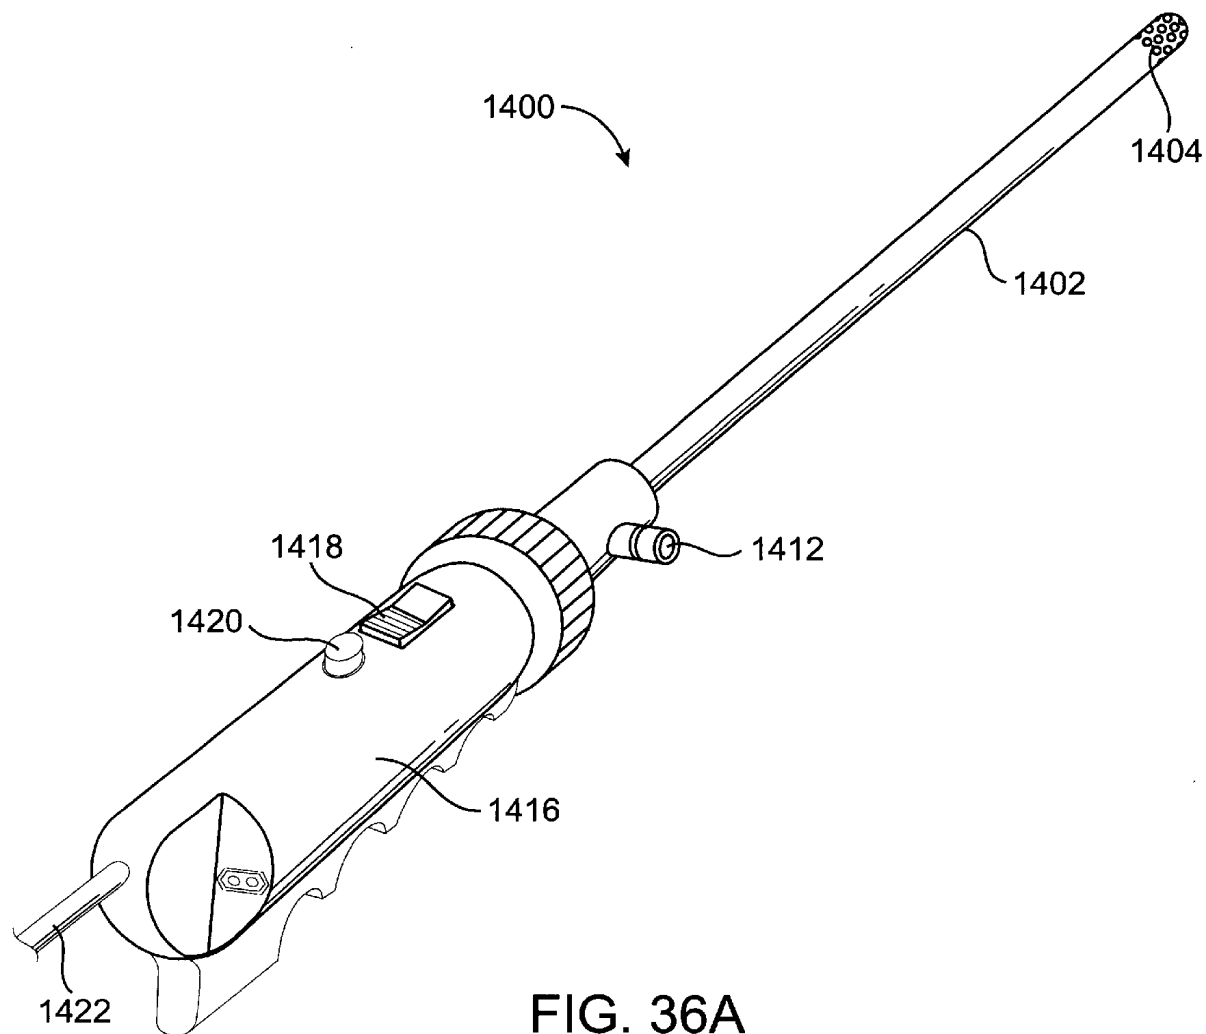


FIG. 33





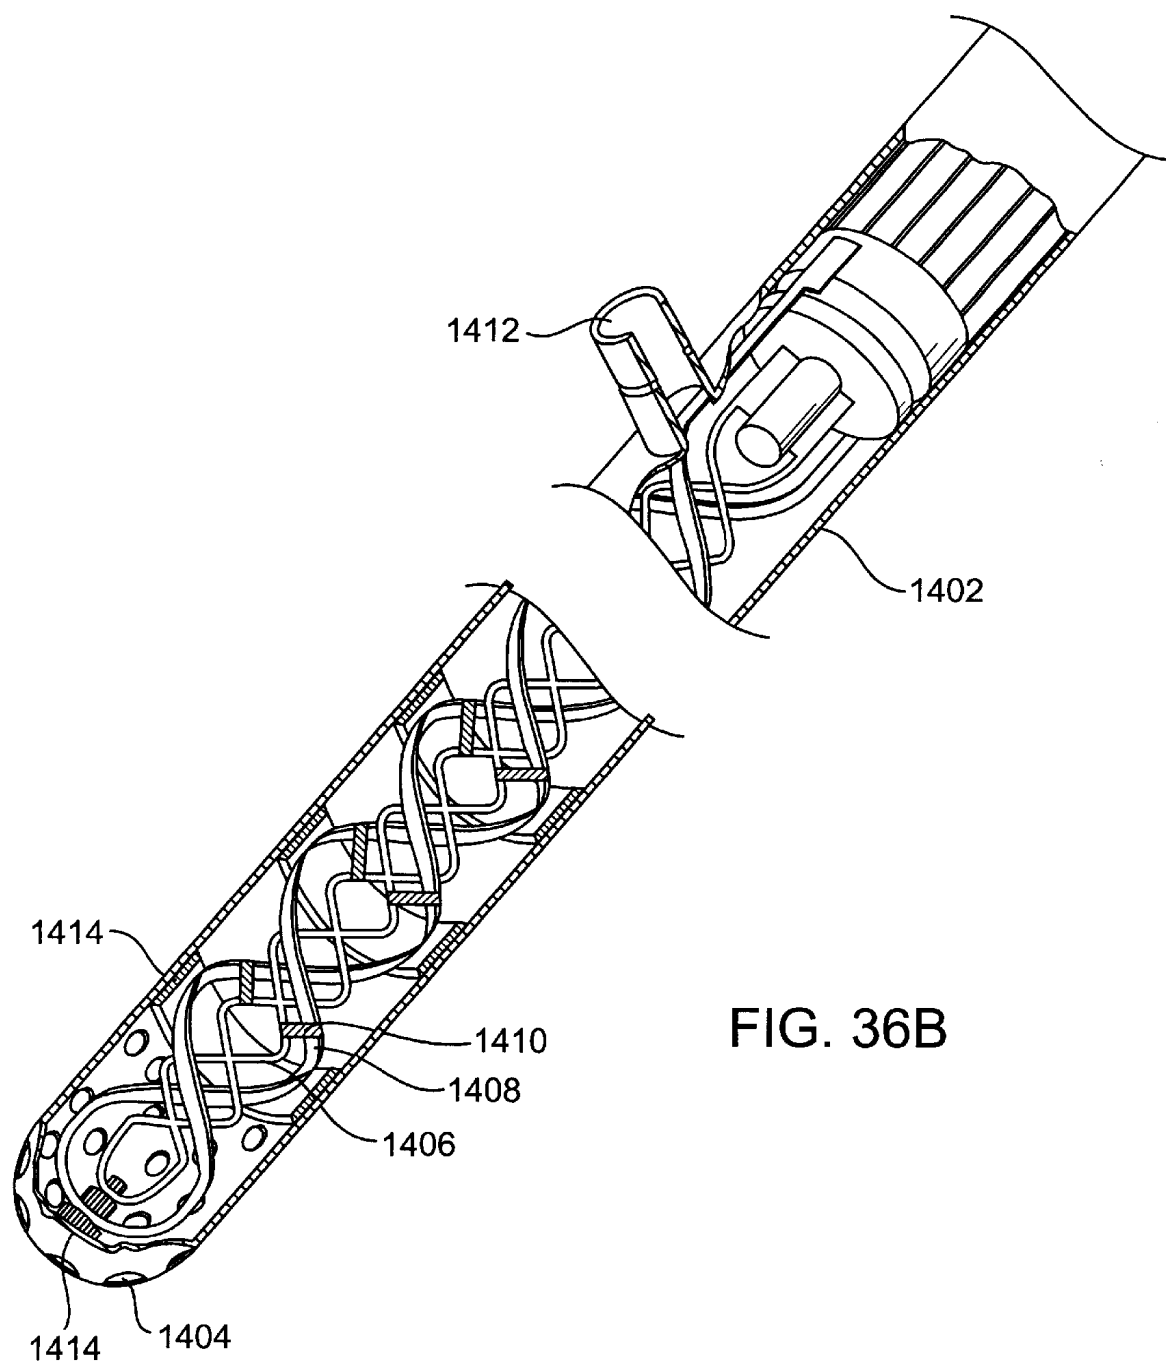


FIG. 36B

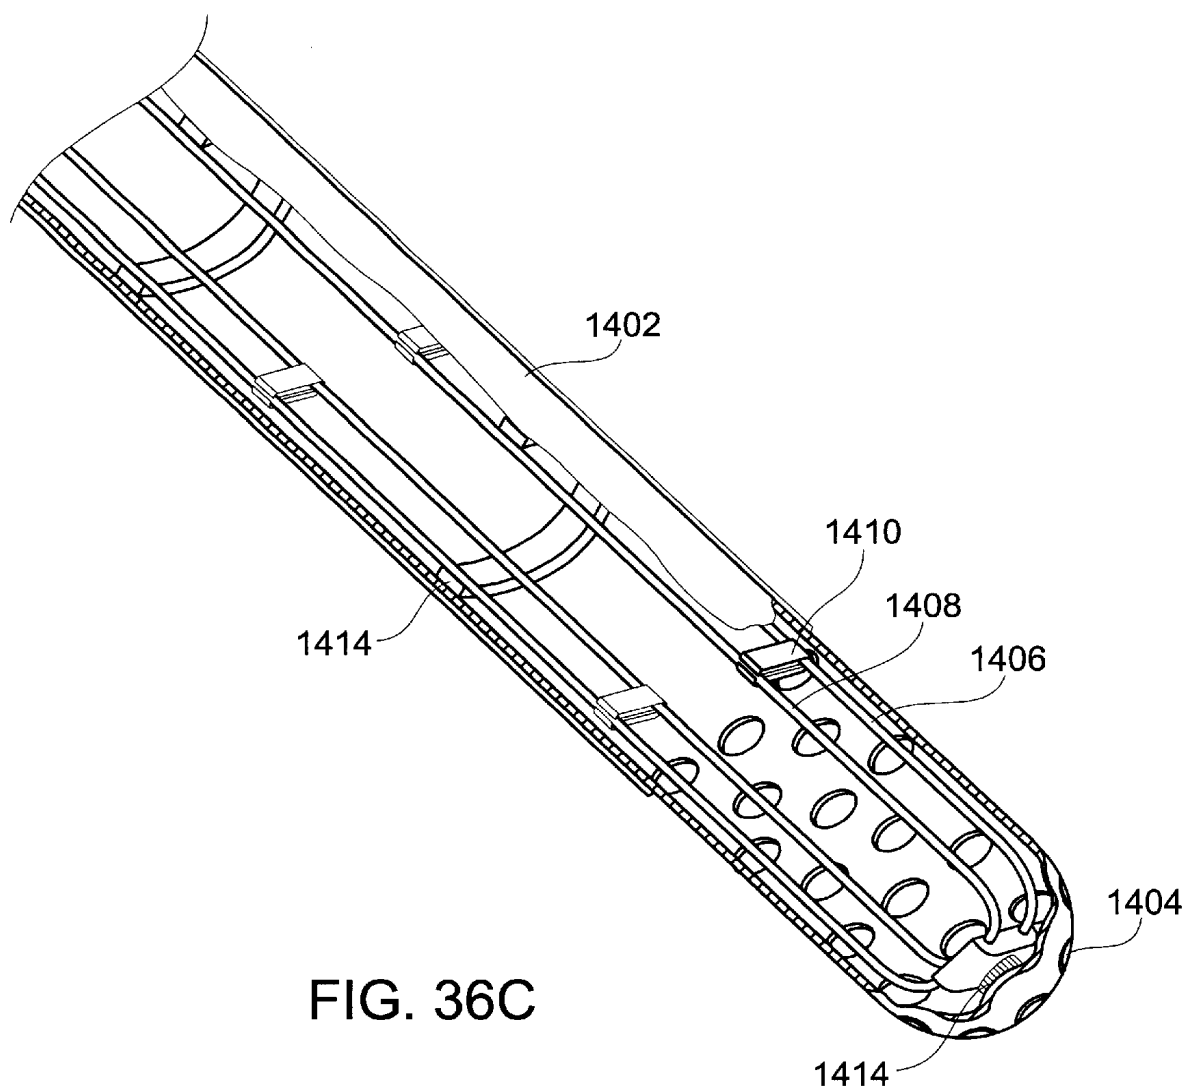
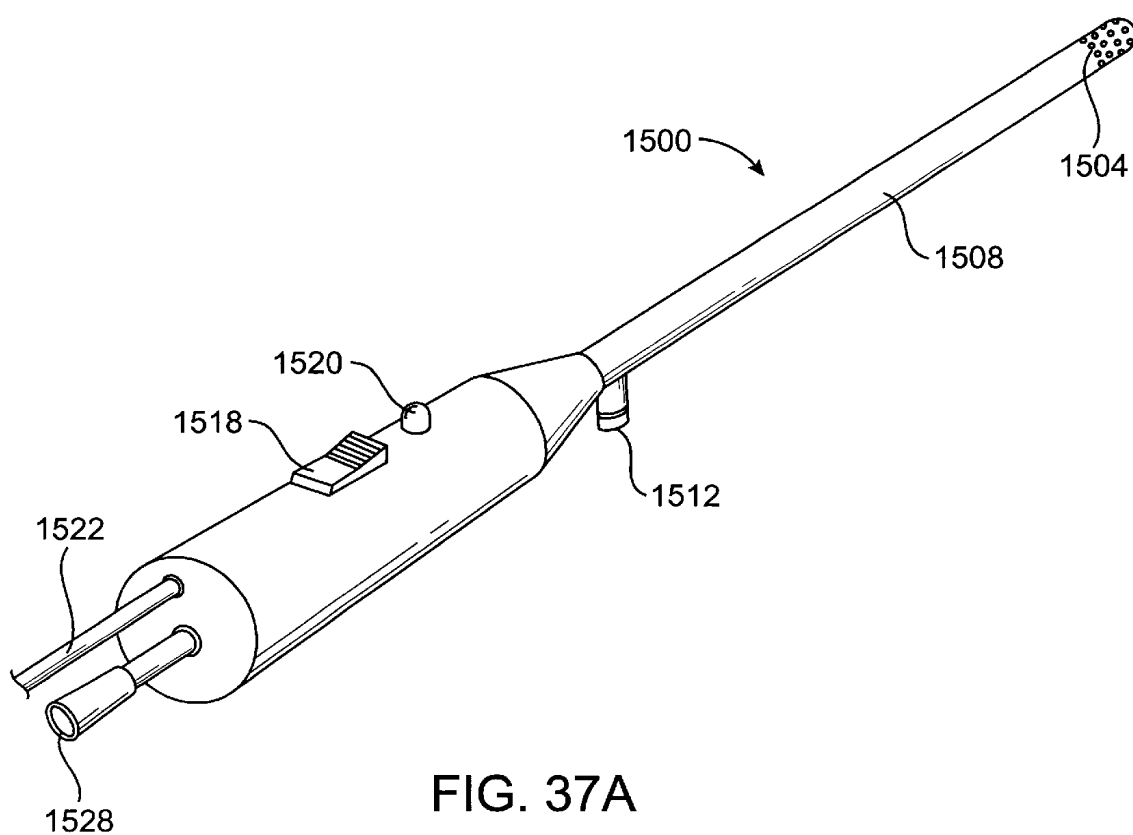


FIG. 36C



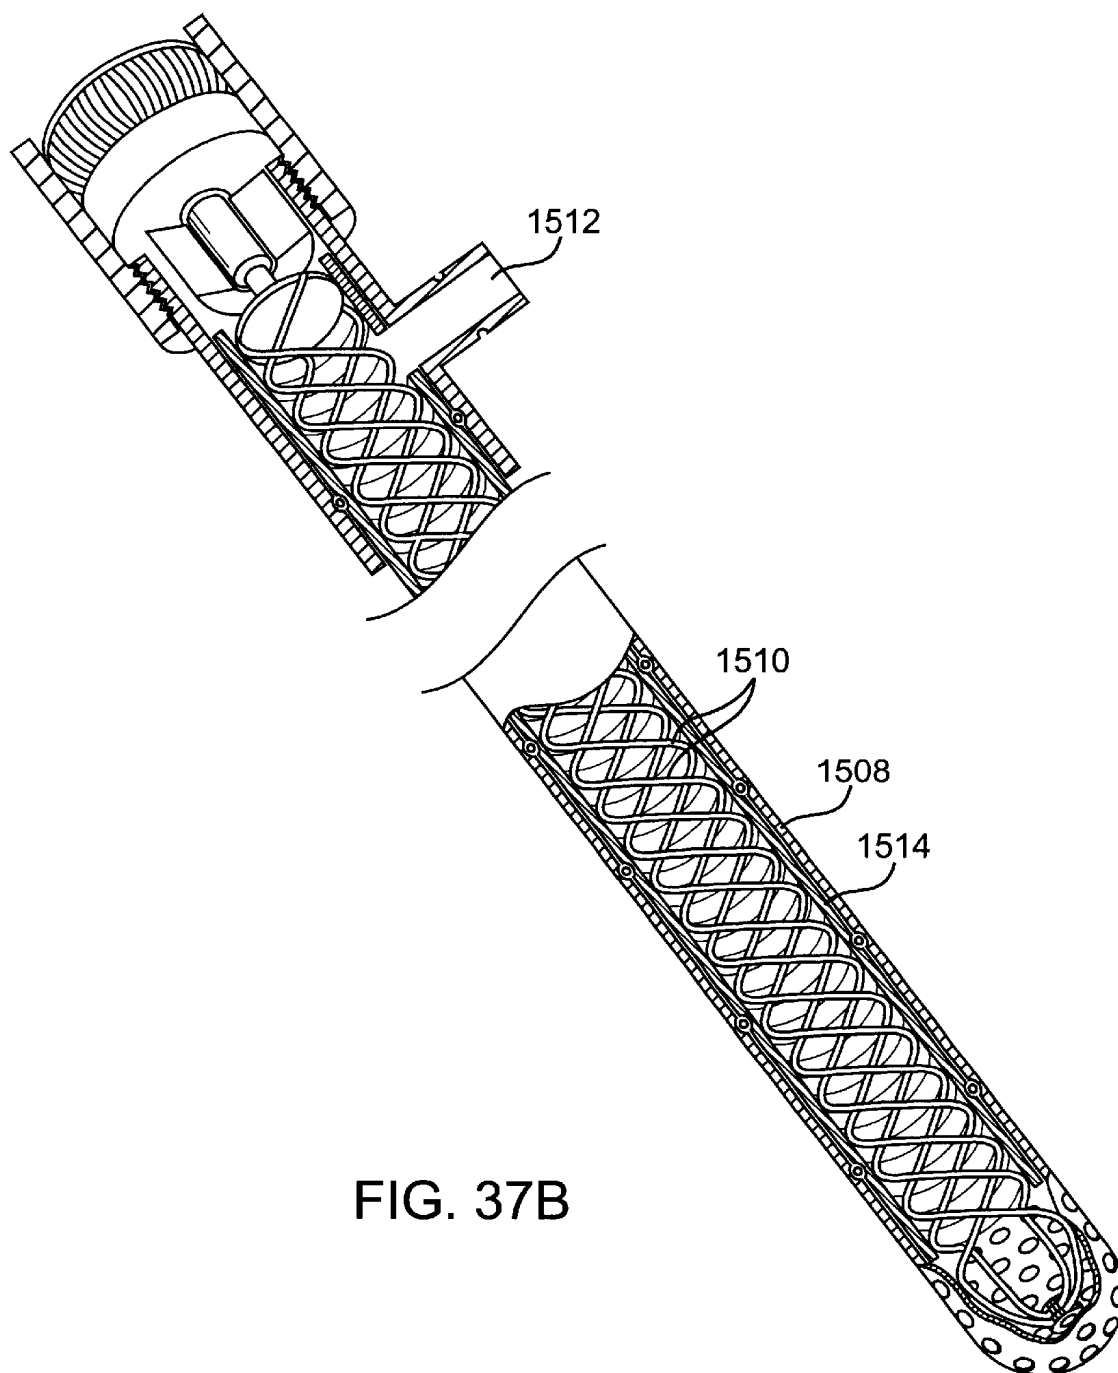
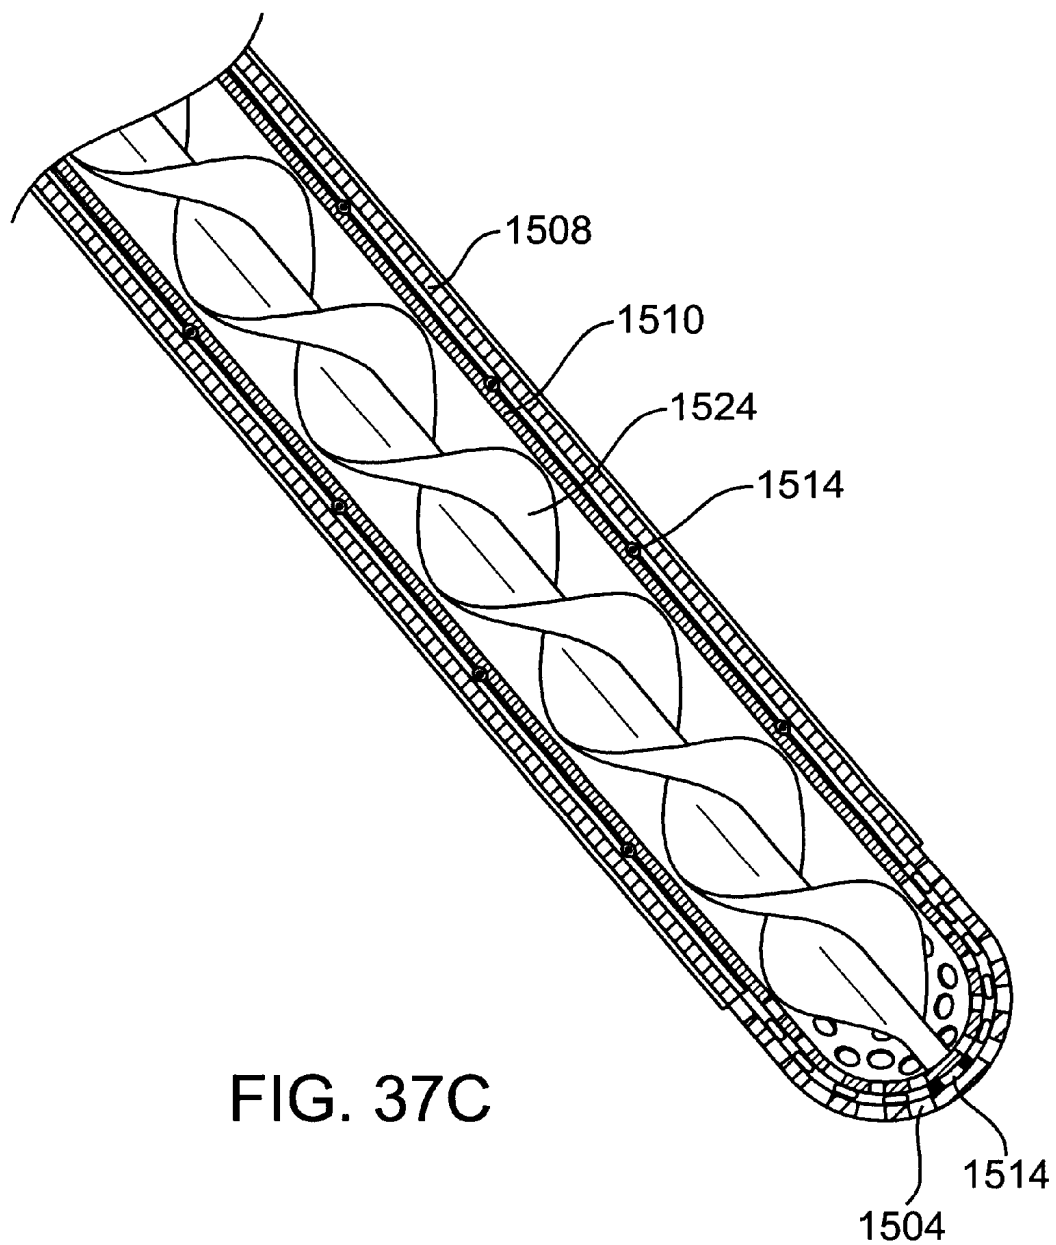


FIG. 37B



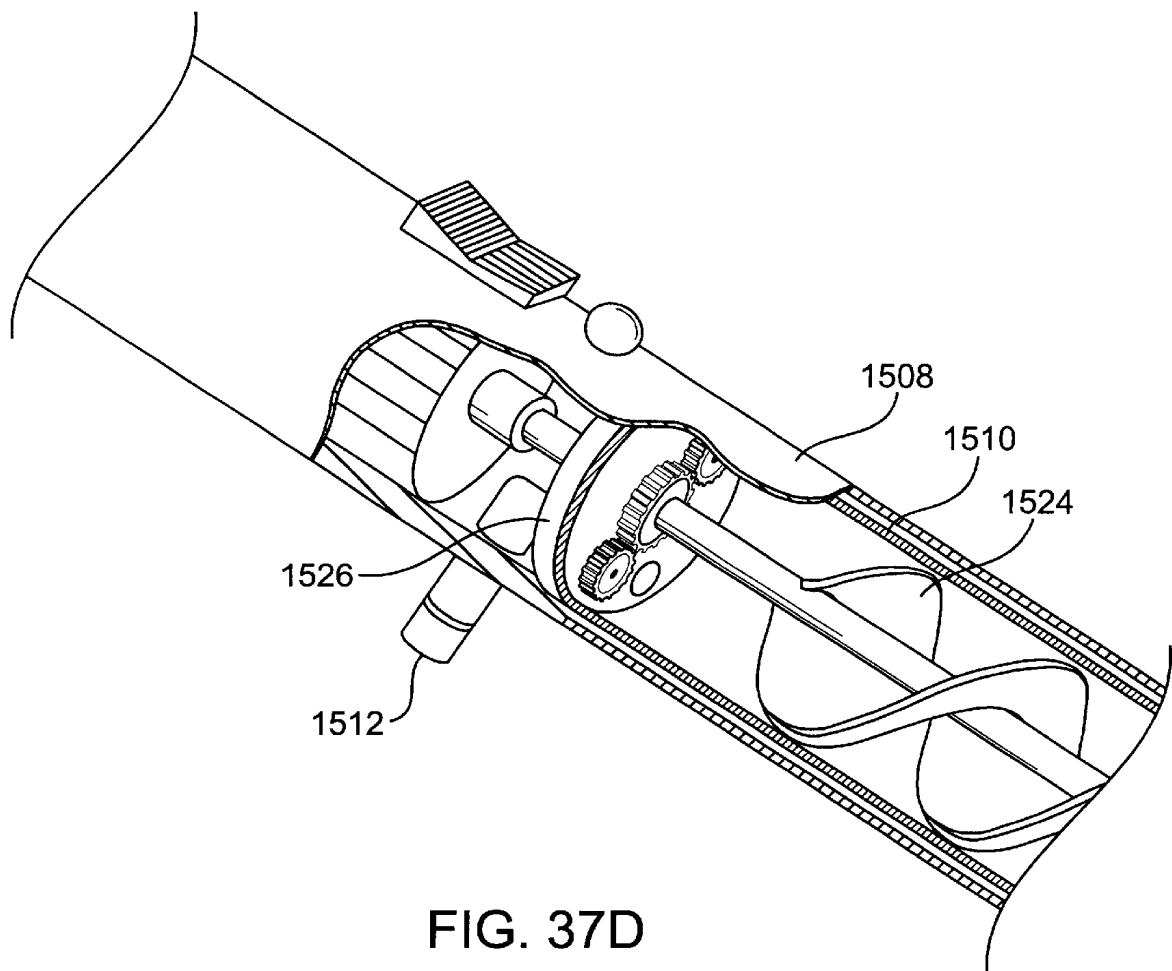


FIG. 37D


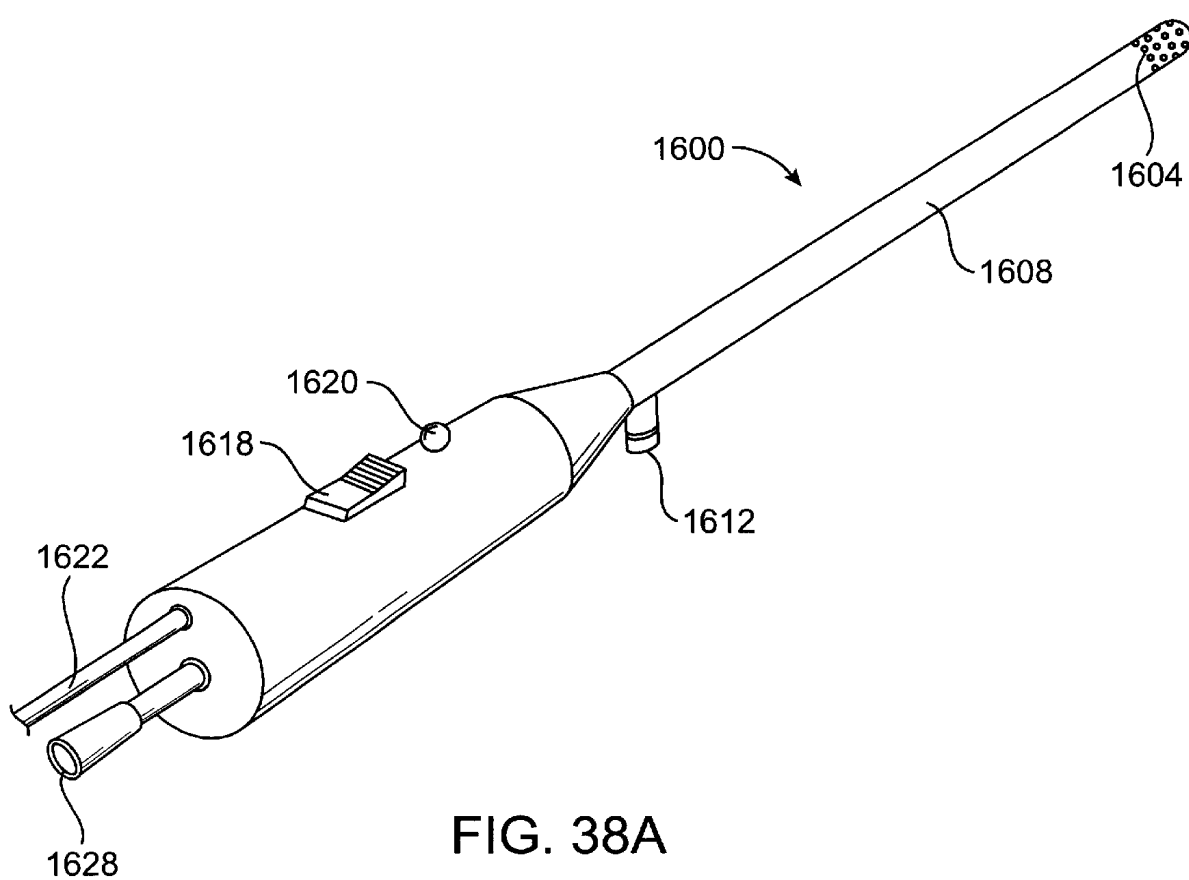


FIG. 38A

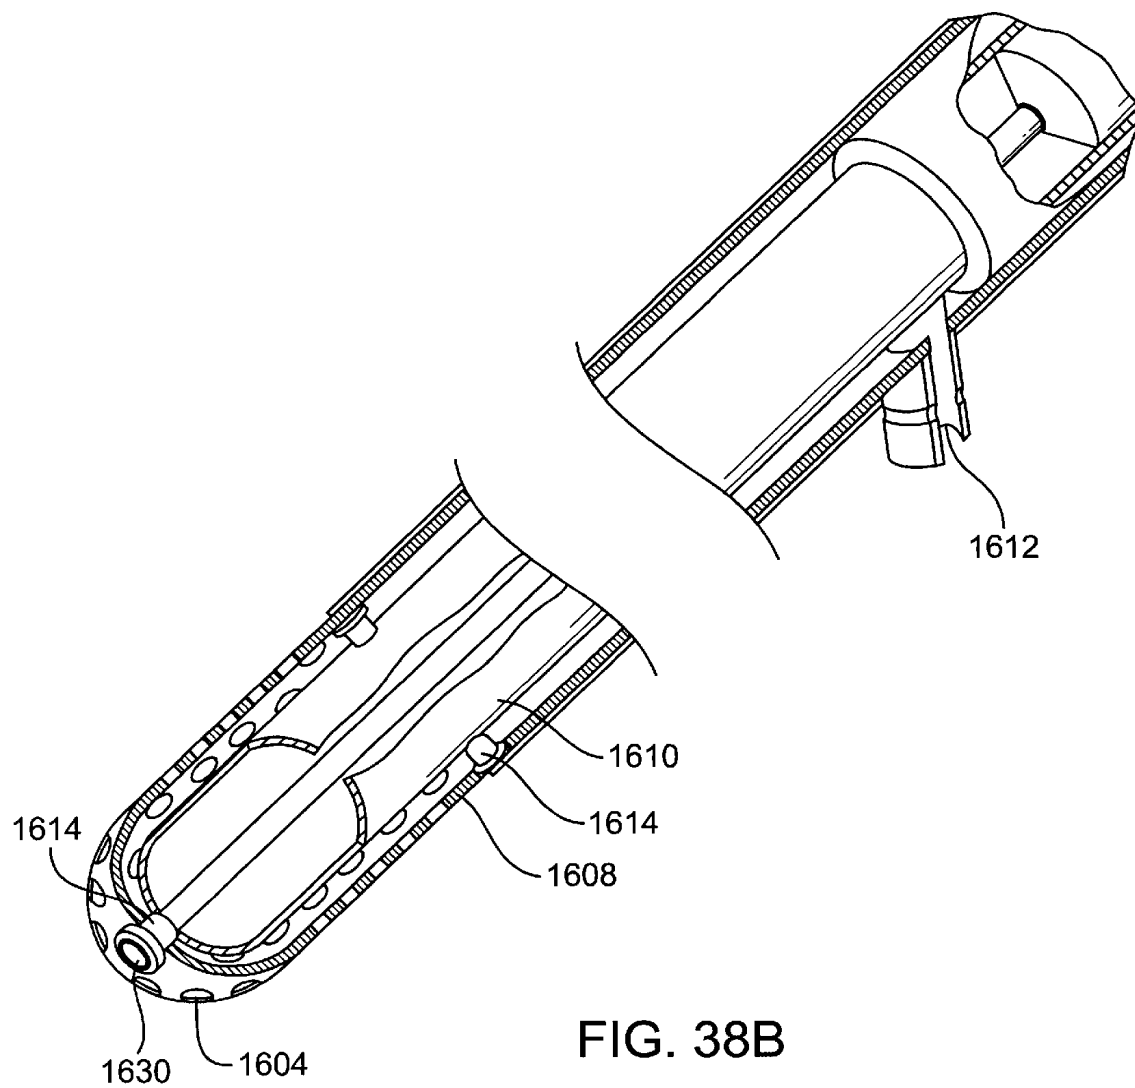

FAT REMOVAL DEVICE AND METHOD

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention relates to apparatus and methods for removing fat from the external surface of an internal organ, and more specifically to apparatus and methods for selectively removing all or part of the fatty layer on the epicardial surface of a mammalian patient.

2. Brief Description of the Related Art

Recent advances in cardiology, radiology, and cardiothoracic surgery have allowed patients suffering from various diseases of the internal organs to benefit from less invasive techniques to surgically treat their conditions. With the advent of newer techniques, however, come newer difficulties in the application of these techniques to all the qualified patients.

Recent advanced techniques and devices allow for the correction of numerous defects of the internal organs, e.g., the heart, by access to the surface of the organs. For example, performing coronary artery bypass surgery on a beating heart has been used to treat coronary artery disease, attaching leads to the exterior surface of the heart to collect diagnostic data and to pace the heart, or performing atrial fibrillation procedures. In all of these procedures, however, often a thick layer of fatty tissue must be removed from around the heart to expose the myocardial tissue to be treated. To further complicate the procedure, the fatty layer may be enveloped in a tougher layer of connective tissue, the epicardium, which must first be incised to expose the fat underneath. Furthermore, the vasculature which provide blood to the heart itself, the coronary arteries and veins, may be located on the exterior of the cardiac tissue and under and in the fat. The coronary arteries and cardiac veins traverse the myocardial surface, supplying oxygenated blood and conducting deoxygenated blood away from the cardiac tissues, respectively. Typically, the epicardium is cut with a scalpel to expose the fat underneath, which in turn is incised with a scalpel to expose the surface of the heart to perform a procedure, e.g., bypass surgery, pacing lead attachment, atrial fibrillation procedures, etc. The use of a scalpel to remove the fat clearly presents a level of danger to the patient's coronary arteries which is only marginally tolerable; the consequences of mishap are severe.

The fat layer is generally a semi liquid form at body temperature. At elevated temperatures the fatty tissue will become more liquified. The cell membranes of the fat tissue can be ruptured when they are mechanically stressed, which will allow the fat contents of the cell to flow freely.

Prior devices exist which aspirate fat or other substances from the body of a patient, but which are not suitable for removing the fat layer from the external surface of an internal body organ. Laparoscopes exist, but are not useful because they cannot break up fatty tissue while ensuring that larger blood vessels which are located under the fat are not also severed. Numerous atherectomy devices have been proposed, however they are far too small to be effectively employed to remove the sometimes large volumes of fat which covers the organ, and also do not provide any protection for the underlying blood vessels.

SUMMARY OF THE INVENTION

In accordance with a first exemplary embodiment of the present invention, a fat removing device comprises a can-

nula having a longitudinal axis, a proximal end, a distal end, a lumen extending proximally along said longitudinal axis, and an opening in said cannula at said distal end which fluidly communicates said lumen with the exterior of said cannula, and a protective mesh attached to said distal end and distal of said opening, said mesh including openings sized to permit human fat cells to extrude through said openings when said mesh is pressed against a mass of human fatty tissue, said openings also sized to prevent a human blood vessel which underlies said human fatty tissue from passing through said openings when said mesh is pressed against said mass of human fatty tissue.

In accordance with a second exemplary embodiment of the present invention, a fat removing device comprises a cannula having a longitudinal axis, a proximal end, a distal end, a lumen extending proximally along said longitudinal axis, and an opening in said cannula at said distal end which fluidly communicates said lumen with the exterior of said cannula, and an energy transmitting wire located in said cannula and including a tip distal of said cannula distal end, said wire and tip being longitudinally movable at a frequency and magnitude which at least partially disrupts the cell walls of said human fat cells.

In accordance with a third exemplary embodiment of the present invention, a fat removing device comprises a cannula having a longitudinal axis, a proximal end, a distal end, an outer diameter R, a lumen extending proximally along said longitudinal axis, and an opening in said cannula at said distal end which fluidly communicates said lumen with the exterior of said cannula, and a cutting element in said lumen adjacent said cannula distal end, said cutting element spaced from said cannula distal end a distance D, wherein R and D are together selected to permit human fat cells to extrude into said cannula opening when said cannula distal end is pressed against a mass of human fatty tissue, R and D are together selected also being sized to prevent a human blood vessel which underlies said human fatty tissue from passing into said cannula opening when said cannula distal end is pressed against said mass of human fatty tissue.

In accordance with a fourth exemplary embodiment of the present invention, a fat removing device comprises a cannula having a longitudinal axis, a proximal end, a distal end, a tip at said distal end, a lumen extending proximally along said longitudinal axis, and an opening in said cannula at said distal end which fluidly communicates said lumen with the exterior of said cannula, said cannula tip being angled inward, and a cutting element in said lumen adjacent said cannula distal end, wherein said cannula tip angle is selected to permit human fat cells to extrude into said cannula opening when said cannula distal end is pressed against a mass of human fatty tissue, said cannula tip angle also being selected to prevent a human blood vessel which underlies said human fatty tissue from passing into said cannula opening when said cannula distal end is pressed against said mass of human fatty tissue.

In accordance with a fifth exemplary embodiment of the present invention, a fat removing device comprises a cannula having a longitudinal axis, a proximal end, a distal end, a closed tip at said distal end, a lumen extending proximally along said longitudinal axis, and an opening in said cannula proximal of said distal end which fluidly communicates said lumen with the exterior of said cannula, a rotatable shaft in said cannula, a blade attached to said rotatable shaft adjacent said opening, wherein when said cannula opening is pressed against a mass of human fatty tissue, and when said rotatable shaft is caused to rotate, said blade rotates and cuts fatty tissue which has extruded through said opening, said can-

3

nula opening being sized to prevent a human blood vessel which underlies said human fatty tissue from passing into said cannula opening when pressed against said mass of human fatty tissue.

In accordance with a sixth exemplary embodiment of the present invention, a fat removal tool for removing fat from the outer surface of an internal body organ comprises a screen having at least one passageway sized to allow fat cells to extrude through the screen while preventing a blood vessel selected from the group consisting of a patient's coronary arteries, a patient's cardiac veins, and both, from passing through said screen, and a separate cutting member positionable adjacent to said screen to cut fat which has been extruded through said screen passageway.

In accordance with a seventh exemplary embodiment of the present invention, a fat removal tool for removing fat from the outer surface of an internal body organ comprises a handle having a proximal end, a distal end, and a hollow interior, a screen at said handle distal end, said screen including at least one passage therethrough, a rotatable blade in said handle and immediately proximal of said screen, and a rotatable shaft attached to said blade and extending proximally from said rotatable blade.

In accordance with an eighth exemplary embodiment of the present invention, a fat removal tool for removing fat from the outer surface of an internal body organ comprises a screen having at least one passageway sized to allow fat cells to extrude through the screen while preventing a blood vessel selected from the group consisting of a patient's coronary arteries, a patient's cardiac veins, and both, from passing through said screen, and a cutting member adjacent to said screen and movable over said screen to cut fat which has been extruded through said screen passageway.

In accordance with a ninth exemplary embodiment of the present invention, a method of removing a fat layer from the surface of an internal body organ comprises the steps of exposing a portion of said fat layer, pressing said fat layer with a surface having at least one hole, extruding fat through said at least one hole, and cutting said fat that has extruded through said hole on a side of said surface opposite said fat layer.

In accordance with a tenth exemplary embodiment of the present invention, a method of removing a fat layer from the surface of an internal body organ comprises the steps of exposing a portion of said fat layer, pressing said fat layer with a surface which vibrates at a frequency and magnitude sufficient to rupture cell walls contained in said fat layer, and aspirating fatty tissue.

In accordance with an eleventh exemplary embodiment of the present invention, a fat removal tool comprises two bipolar wires each having a cross-sectional diameter and a centerline, each bipolar wire having a cross-sectional diameter from about 0.150 inches to about 0.045 inches, the two bipolar wires spaced from each other at a centerline-to-centerline distance from about 0.040 inches to about 0.200 inches.

In accordance with a twelfth exemplary embodiment of the present invention, a fat removal tool comprises a first outer sheath electrode having a lumen and a distal end, the outer sheath electrode including holes at the distal end to allow fat to enter the lumen, and a second helical wireform inner rotatable electrode positioned in the lumen to rotate relative to the holes to move to the proximal end of the tool any fat that is melted upon application of radio frequency energy between the first and second electrodes. such that a vacuum source can remove the fat from the tool.

4

Still other objects, features, and attendant advantages of the present invention will become apparent to those skilled in the art from a reading of the following detailed description of embodiments constructed in accordance therewith, taken in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

The invention of the present application will now be described in more detail with reference to preferred embodiments of the apparatus and method, given only by way of example, and with reference to the accompanying drawings, in which:

FIG. 1 illustrates a cross-sectional view of a first exemplary embodiment in accordance with the present invention;

FIG. 2 schematically illustrates a view of a second exemplary embodiment in accordance with the present invention;

FIG. 3 further illustrates the device of FIG. 2;

FIG. 4 illustrates portions of the device of FIG. 2;

FIG. 5 illustrates a cross-sectional view of a third exemplary embodiment in accordance with the present invention, in use;

FIG. 6 illustrates an elevational distal end view of the device of FIG. 5;

FIG. 7 illustrates a cross-sectional view of a fourth exemplary embodiment in accordance with the present invention, taken along line 7—7 in FIG. 8;

FIG. 8 illustrates an elevational distal end view of the device of FIG. 7;

FIGS. 9 and 10 illustrate the device of FIG. 7, in use;

FIG. 11 illustrates a cross-sectional view of a fifth exemplary embodiment in accordance with the present invention, in use;

FIG. 12 schematically illustrates a view of a sixth exemplary embodiment in accordance with the present invention;

FIG. 13 illustrates a cross-sectional view of distal portions of the device of FIG. 12;

FIG. 14 illustrates an elevational side view of the device of FIG. 12;

FIG. 15 illustrates a top plan view of the device of FIG. 12;

FIG. 16 illustrates a cross-sectional view of proximal portions of the device of FIG. 12;

FIG. 17 illustrates a cross-sectional view of distal portions of a seventh exemplary embodiment in accordance with the present invention;

FIG. 18 illustrates an elevational side view of an alternate embodiment of portions of the device of FIG. 17;

FIG. 19 illustrates a perspective view of the device of FIG. 18;

FIG. 20 illustrates a perspective view of another alternate embodiment of portions of the device of FIG. 17;

FIG. 21 illustrates a top plan view of a eighth exemplary embodiment in accordance with the present invention;

FIG. 22 illustrates an elevational side view of distal portions of the device of FIG. 21;

FIG. 23 illustrates an elevational end view of distal portions of the device of FIG. 21;

FIG. 24 illustrates a cross-sectional view of distal portions of a ninth exemplary embodiment in accordance with the present invention;

FIG. 25 illustrates a top plan view of the portions of the device in FIG. 24;

5

FIG. 26 illustrates a perspective view of portions of a tenth exemplary embodiment in accordance with the present invention;

FIG. 27 illustrates a perspective view of other portions of the device of FIG. 26;

FIG. 28 schematically illustrates a top plan view of portions of the device in FIG. 27;

FIG. 29 illustrates a perspective view of the portions of FIG. 28;

FIG. 30 illustrates a perspective view of an eleventh exemplary embodiment in accordance with the present invention;

FIG. 31 illustrates a perspective view of the device of FIG. 30, with portions broken away;

FIG. 32 illustrates a perspective view of a twelfth exemplary embodiment in accordance with the present invention;

FIG. 33 illustrates an enlarged perspective view of portions of the embodiment illustrated in FIG. 32;

FIG. 34 illustrates a bipolar RF device for removal of fat for open chest procedures according to yet further aspects of the present invention;

FIG. 35 illustrates another bipolar RF device for removal of fat for open chest procedures;

FIGS. 36A, B and C illustrate bipolar wire electrodes that rotate within a sheath for transthoracic procedures;

FIGS. 37A, B, C and D illustrate a device with one of the bipolar electrodes being the outer sheath and the other being an electrode that rotates relative to the other electrode also with the potential of an auger type device to move the melted fat from the distal to the proximal end of the device; and

FIGS. 38A and B illustrate a device similar to the device in FIG. 37 with a central lumen to accept an endoscope for viewing the area of treatment or a therapeutic device like a lead attachment device.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

Referring to the drawing figures, like reference numerals designate identical or corresponding elements throughout the several figures.

FIG. 1 illustrates a cross-sectional view of a first exemplary embodiment 100 of a fat removal device in accordance with the present invention. Device 100 includes a cannula 102 including a proximal end 104, a distal end 106, and an aspiration or suction lumen 108 extending between the proximal and distal ends. A source of vacuum (not illustrated) is fluidly connected to lumen 108 to aspirate all the fat and fluid which enters into the lumen. Device 100 further includes a protective mesh 110 extending from or a part of the distal end 106 of the cannula 102, which includes openings 118 of a size preselected to allow fatty tissues and fat cells to extrude through the mesh, while preventing blood vessels of certain sizes from entering into the cannula, as will be described in greater detail below.

Cannula 102 further includes a source of vibrational energy 112, e.g., an ultrasonic transducer, which supplies vibrational energy to the fatty tissue against which the cannula is pressed. This vibrational energy is conducted at a frequency which is selected to substantially disrupt or otherwise rupture the outer membranes of the cells which make up the fatty tissue. The frequency of operation of the source 112 will vary upon the exact nature of the fatty tissue which is desired to break up, and will be readily determinable by one of ordinary skill in the art. Cannula 102 further includes

6

a heat radiating element or heater 114, e.g., a resistive heating element, for heating the fatty tissue against which the cannula is pressed. Heat generated by heater 114 aids in breaking up the fatty tissues by the vibrational energy supplied by the source 112, by heating and thereby reducing the viscosity of the contents of the cells ruptured by the vibrational energy supplied by source 112. Together, source 112 and heater 114 are positioned at the distal tip just above holes 118 or mesh 110 generate a cell rupture zone 1116 in which the cells of the fatty tissue against which cannula 102 is pressed are ruptured, heated, and aspirated into lumen 108 of the cannula. Furthermore, the heat transfer from heater 114 functions to cauterize the capillary bed which is part of the fatty tissue, thereby minimizing bleeding of the tissue and the chances for infection to set in, and aids in postoperative healing of these tissues. Source 112 and heater 114 are connected to appropriate power sources at the proximal end 104 of the cannula 102 (not illustrated), as will be readily appreciated by one of ordinary skill in the art.

As discussed briefly above, mesh 110 or holes 118 is constructed to allow only the capillary blood vessels of the fatty tissue to enter into the interior of cannula 102, so that the larger blood vessels, the exposure of which is the object of the process of removing the fatty tissue layer, will not be harmed by the device 100. These blood vessels are effected less by the heat from heater 114, as a slight increase in temperature would have little effect on the vessel walls of these larger blood vessels, and they furthermore have a greater heat capacity and ability to conduct heat away from the operative site by blood flowing through them.

The function of the device 100 illustrated in FIG. 1 will now be briefly described. Cannula 102 is pressed up against the outer fatty tissue layer of an organ the outer surface of which it is desired to access directly. Cannula 102 can be inserted through an appropriately sized endoscope (e.g., thoracoscope), or can be inserted directly via an opening created in the patient's body via full or partial thorachotomy. If an overlying layer of tissue covers the layer of fatter tissue, e.g. the epicardium, it is cut to expose the underlying fatty tissue. Distal end 106 is pressed against the fatty tissue. Suction is applied to lumen 108, vibrational energy is emitted from source 112, and heat is delivered from heater 114, preferably simultaneously, but optionally in any serial combination. Fatty tissue cells are ruptured by the application of vibrational energy, with the aid of an increase in the temperature of the cells from heater 114, and the contents of the ruptured cells are aspirated through mesh 110 or holes 118, into lumen 108, and proximally through cannula 102. Mesh 110 or holes 118 prevent blood vessels larger than the capillary bed that vascularizes the fatty tissue layer from being drawn into the lumen 108. The cannula is moved to a new site on the fatty tissue layer when a sufficient amount of the fat has been removed to perform another procedure on the surface of the organ.

FIGS. 2-4 schematically illustrate views of a second exemplary embodiment of a fat removal device 200 in accordance with the present invention. Device 200 includes an RF or ultrasonic generator 202 connected to a transducer 204. Transducer 204 causes oscillatory lateral motion of a proximal end 208 of a wire 206. This lateral motion is transformed into longitudinal motion of the distal end 210 of wire 206 by a restraint bushing 214 positioned between the proximal and distal ends of the wire. In the exemplary embodiment illustrated in FIGS. 2-4, bushing 214 is positioned at the distal end of the device 200; however, bushing 214 may be positioned anywhere along the length of wire 206 and still be within the spirit and scope of the invention.

Distal end **210** of wire **206** includes a tip **212**, which is preferably enlarged, and more preferably is in the form of a hemisphere, which moves longitudinally to impact against fatty tissue against which the device is pressed. As illustrated in FIG. 4, as generator **202** laterally moves the proximal end **208** of wire **206**, the wire sweeps over an area between two sine curves between two maxima D_1 and D_2 . The longitudinal distance D that the distal tip **212** of wire **206** travels between the most proximal and most distal positions satisfies the equation:

$$D=2(D_1+D_2).$$

Wire **206** may be formed of any biocompatible material which is able to transmit the ultrasonic energy from generator **202**. Preferably, wire **206** is formed of a nickel-titanium alloy, commonly referred to as Nitinol®, or may be formed of a surgical stainless steel, although other materials can be used, such as platinum, etc. Wire **206** preferably has an outer diameter of about 0.05 inches, although the wire can be formed larger or smaller, to increase or decrease its strength, and to tune the wire to eliminate any higher order, steady state or transient harmonics which may arise by application of the oscillatory motion to the wire, as will be readily apparent to one of ordinary skill in the art.

Device **200** also includes a cannula **218** having a lumen **220** through which wire is inserted. Lumen **220** extends from a proximal end **222** to a distal end **224** of the cannula. Cannula **218** includes an aspiration port **226** at the distal end **224** thereof, which is in fluid communication with an aspiration conduit **228** extending through the wall of the cannula to a source of vacuum and a collection jar **230**. Aspiration port **226** is preferably located at the distalmost end of cannula **218**; however, the aspiration port can be optionally located on the sidewall of the cannula, or both end and side aspiration ports may be provided to provide additional area through which to aspirate tissue, and to provide a vacuum break if any of the aspiration ports become clogged or otherwise blocked. Bushing **214** is positioned inside lumen **220** to restrain wire **206** and transform the lateral motion of wire **206** into longitudinal motion. Cannula **218** may also optionally include a source of irrigation fluid (not illustrated) in fluid communication with lumen **200**, and an irrigation port (not illustrated) adjacent the distal end **224** of the cannula, for supplying irrigation fluid to the distal tip. Irrigation fluid may be optionally supplied to assist in heating, cooling, or selectively heating and cooling the tissue and tip **212**.

The function of device **200** and a preferred method of use thereof will now be described with reference to FIGS. 2-4. Two incisions are made under the chest of a patient. The first incision is used to introduce an endoscopic, e.g., laparoscopic, device to view the surface of the organ from which it is desired to remove a layer of fatty tissue, e.g., the heart. The endoscope, which has an external diameter preferably not greater than about 2 mm to about 3 mm and has a focal length between about 1 cm and about 1.5 cm provides detailed images of the surface of the heart regardless the up and down movement of the beating heart. The endoscope is a common device, the details of which will be readily apparent to one of ordinary skill in the art.

A second incision is made to introduce ultrasonic drilling device **200**. Ultrasonic generator **202** is coupled to transducer **204** to generate and transmit ultrasonic energy between about 18 KHz and about 20 KHz. A drilling tip **212** is attached to the distal end of wire **206** to increase the area of application of the ultrasonic energy to the fatty tissue.

Wire **206** is now inserted into cannula **218**, which has its proximal end **222** connected to transducer **204**. When trans-

ducer **204** applies its oscillatory energy through wire **206**, the wire will vibrate inside the cannula **218**. As the distal end **224** of the wire is constrained inside bushing **214**, the sine wave motion is transformed into longitudinal or back and forth motion. Because of the particular geometry of device **200**, longitudinal displacement of tip **212** occurs at a frequency twice that of the frequency at which generator **202** is operated. This effectively make tip **212** a high-speed drill bit which impacts against fatty tissue against which the tip **212** is pressed, disrupting the cell walls of the tissue in a manner similar to the disruption caused by device **100**, described above. Furthermore, the length D of the displacement of the tip **212** can be very closely controlled by changing the frequency at which generator **202** operates, which will change the wavelength of the sine curves illustrated in FIG. 4, and therefore distances D_1 and D_2 .

As fatty tissue is disrupted by the operation of tip **212**, the tissue is aspirated through aspiration conduit **228** to jar **230**. If desired, irrigation fluid may also be provided to heat the fatty tissue to make the contents of the ruptured cells less viscous. Also, irrigation fluid may be provided to cool the tip **212** in the event that it becomes overheated, and to wash the surgical site.

FIGS. 5 and 6 schematically illustrate views of a third exemplary embodiment of a fat removal device **300** in accordance with the present invention. Device **300** includes an outer cannula **302** having a longitudinally extending lumen **310** therein, and an inner cannula **304** mounted to rotate in the outer cannula's lumen, as indicated by arrow **306**. Outer cannula **302** includes a distal end **308** which has a barrier **312** including at least one, and preferably a mesh or array of holes **316** which partially covers the open distal end of the outer cannula **302**. As will be described in greater detail below, barrier **312** is provided to allow fatty tissue cells to extrude through the mesh or holes **316** in the barrier, while excluding blood vessels having a certain size, which underlie the fatty tissue layer, from passing through the barrier and into the lumen **310**. Barrier **312** may take any of a number of configurations.

For example, barrier **312** can be a mesh or array of holes **316**, a screen, a porous or slotted plate, hemisphere, dome, frustocone, or other geometry which functions to allow fatty tissue cells to extrude through the barrier when the barrier is pressed against fatty tissue, while excluding blood vessels having a certain size from passage through the barrier. In the exemplary embodiment illustrated in FIGS. 5 and 6, barrier **312** includes a dome or hemispherical member **314** which is joined to or integral with the distal end **308** of outer cannula **302**. Member **314** includes an array of holes or passages **316** which are sized to allow fatty tissue to pass therethrough, but a small enough that certain sizes of blood vessels will not pass through the dome member.

For example, and not by way of limitation, passages **316** have diameters between about 0.125 inches and about 0.300 inches, preferably about 0.156 inches. The spacing between the holes, from the centerline of one hole to the centerline of an adjacent hole, has been found by the inventors herein to be advantageously from about 0.176 to 0.230 inches, and is more preferably at a distance of 0.196 inches. The depth of passages **316**, which corresponds in this embodiment to the thickness of member **314**, is between about 0.015 inches and about 0.050 inches, preferably about 0.030 inches. Barrier **314** can be made of any number of suitable materials which are biocompatible, of moderate to high strength, and are readily manufactured to the required specifications. For example, barrier **314** can be formed of plastics, including thermoplastic and thermoset materials, metals, including stainless steel and Nitinol, or ceramics.

As illustrated in FIG. 6, barrier 314 includes a central portion 318 which does not include any passages 316 therethrough. Central portion 318 is provided as a bearing surface for the device 300 when it is pressed against and into fatty tissue, so that any larger blood vessels which may underlie the fatty tissue layer will not be in direct contact with passages 316, thus further ensuring that such larger blood vessels will not enter the passages.

Inner cannula 304 includes an elongates shaft which extends to a distal end 320. Distal end 320 has a shape which is complimentary to and extends into barrier 312. In the embodiment illustrated in FIGS. 5 and 6, the distal end 320 of the inner cannula is dome or hemispherical shaped. Distal end 320 also includes a blade, shearing member, scraper, or the like, designated 322 in FIG. 5. In the embodiment illustrated in FIG. 5, blade 322 is formed in the distal end 320 by the removal of a portion of the surface of the distal end of the inner cannula 304, leaving a portion of the surface the edges of which act as the blade 322. For example, $\frac{1}{3}$ (120 degrees) of the distal end of the inner cannula can be removed to form blade 322. Thus, upon rotation of the inner cannula within the outer cannula, blade 322 rotates adjacent to the inner surface of barrier 316, and cuts, shears, and/or scrapes any material from the inner surface of the barrier which extends into the space swept out by the blade.

Inner cannula further includes a longitudinally extending lumen 324 which fluidly communicates the open portions of the distal end 322 with the proximal end of the inner cannula (not illustrated). Lumen 324 is preferably connected to a source of vacuum so that lumen 324 acts as an aspiration lumen. If desired, lumen 310 can be connected to a source of irrigation fluid, which fluid would then flow in the annular gap 326 between the inner and outer cannulae toward the distal end of the device 300.

Device 300 alternatively can incorporate a heating devices to heat the fatty tissue layer's cells to aid in extruding them through barrier 312, and to cauterize the capillary bed which vascularizes the fatty tissue. For example, barrier 312 can include or itself be a heater which is selectively operable to slightly raise the temperature of the fatty tissue layer. Alternatively, irrigation fluid supplied through lumen 310 can be heated to provide a similar effect. To cauterized the fatty tissue capillary bed, preferably blade 322 is formed as an electrocautery tool, and is in electrical communication with an appropriate source of electrical power (not illustrated).

The function of device 300 will now be described with reference to FIGS. 5 and 6. The outer surface of the fatty tissue layer is made accessible to device 300, as described above. Barrier 312 is pressed up against fatty tissue layer 328, while, if provided, the tissue is heated by a heater in proximity to the fat. Inner cannula 304 is rotated, causing blade 322 to sweep past the inner openings of passages 316. As fat is extruded through passages 316 by application of pressure by barrier 312, it is cut or wiped away from the inner surface of the barrier, and simultaneously the capillary bed of the fatty tissue is cauterized by blade 322. Irrigation fluid can be continuously or selectively supplied through lumen 310, while aspiration through lumen 324 carries the irrigation fluid and fat away from the distal end of device 300. Myocardial tissue or a larger blood vessel 330 is effectively protected from the action of blade 322 because the size of passages 316 and the presence of central portion prevents the tissue or vessel from entering into the passages.

FIGS. 7-10 schematically illustrate views of a fourth exemplary embodiment of a fat removal device 400 in accordance with the present invention. As illustrated in

cross-section in FIG. 7, as taken along line 7-7 in FIG. 8, device 400 includes a cannula 402 having a lumen 404 longitudinally extending from a distal end 406 toward a proximal end (not illustrated). A rotatable shaft 408 extends through lumen 404 toward distal end 406, terminating at a rotary cutting element 410 having at least one, and preferably a plurality of, cutting blades 412. Blades 412 are alternatively also formed as electrocautery tools, as described above in the preceding embodiments, for cauterizing the capillary bed in the fatty tissue cut by device 400. In an alternative embodiment (not illustrated), blades 412 are shaped as an auger, paddle, propeller, or fan blade, such that the leading edge of each blade as it rotates is ahead of the trailing edge of each blade, which will cause any tissue and fluid impinged upon by each of the blades to be pushed proximally. The distalmost extent of blades 412 is located a distance D from the distalmost end of cannula 402. Cannula 402 has an outer diameter at its distal end of R.

As illustrated in the end view of FIG. 8, device 400 is further provided with at least one, and preferably a plurality of, external fluid flow conduits 414, each defining a fluid flow lumen 416. Lumina 416 can be formed alone by each of the conduits 414, or, as illustrated in FIG. 8, can be formed between the outer surface of cannula 402 and the inner surface of each of conduits, in order to reduce the cross-sectional profile of device 400 without compromising the cross-sectional area of each of the lumina. Conduits 414 are preferably irrigation conduits, and are preferably in fluid communication with a source of irrigation fluid at their proximal ends (not illustrated). As discussed above, the irrigation fluid is preferably heated and either continuously or selectively delivered through conduits 414.

As with the preceding embodiments, device 400 is constructed to allow fatty tissue to enter into cannula 402, but prevents larger blood vessels and organ tissue from being impinged upon and cut by blades 412. In the embodiment illustrated in FIGS. 7-10, this is accomplished by selecting the distances D and R and their ratio (D/R) to preclude entry of these structures from being cut by blades 412. By way of example and not by limitation, in one embodiment of device 400, D is about 0.079 inches (2.0 mm), R is about 0.079 inches (2.0 mm), and D/R is about 1.0. Thus, as illustrated in FIGS. 9 and 10, compliant materials such as fatty tissue 418 can extrude into lumen 404 to be cut and cauterized by blades 412 (FIG. 9), while less compliant materials such as organ tissue and larger blood vessels 420 cannot extend into the lumen to be cut by the blades.

The function of device 400 will now be described with reference to FIGS. 7-10. In a manner similar to devices 100, 200, and 300, device 400 is pressed against fatty tissue 418 to extrude the tissue into lumen 404. Rotating blades 412 cut, and preferably simultaneously cauterize, the tissue and its capillary bed, while irrigation fluid is supplied through conduits 414 to the surgical site. Cut tissue and fluid is aspirated through lumen 404, aided by the action of blades 412 pushing the tissue and fluid proximally. Larger blood vessels 420 and organ tissues are precluded from entering into lumen 404 far enough to be cut by blades 412.

FIG. 11 schematically illustrates a view of a fifth exemplary embodiment of a fat removal device 500 in accordance with the present invention. Device 500 is similar to device 400 in some respects. Device 500 includes a cannula 502 extending from a distal end 502 toward a proximal end 504 (not illustrated). A rotatable shaft 506 is located in a longitudinally extending lumen 508. Shaft 506 carries a cutting head 510 which is recessed in lumen 508 from the distal end 502, and is optionally also constructed as an electrocautery

11

tool. Distal end **502** preferably is provided with heaters **512** at the distalmost end of cannula **502**, for heating fatty tissue **516** against which the cannula is pressed. Heaters **512** can be any suitable heater, including RF and DC heaters. Lumen **508** is preferably in fluid communication with a source of suction (not illustrated) so that lumen **508** will act as an aspiration lumen. The tip **514** is preferably directed radially inwardly, to preclude larger blood vessels and organ tissue **518** from entering into lumen **508**, similar to the function of the dimensions D and R of the distalmost end of device **400**. Irrigation conduits (not illustrated) may optionally be provided on the exterior of cannula **502**, similar to conduits **414**.

The function of device **500** will now be described with reference to FIG. **11**. In a manner similar to devices **100**, **200**, **300**, and **400**, device **500** is pressed against fatty tissue **516** to extrude the tissue into lumen **508**. Rotating blade **510** cuts, and preferably simultaneously cauterizes, the tissue and its capillary bed, while irrigation fluid is optionally supplied to the surgical site. Cut tissue and fluid is aspirated through lumen **508**. Larger blood vessels and organ tissues **518** are precluded from entering into lumen **508** far enough to be cut by blade **510**.

FIGS. **12–16** schematically illustrate views of a sixth exemplary embodiment of a fat removal device **600** in accordance with the present invention. Device **600** includes a handle **602** shaped to be easily grasped by a practitioner's hand, and a cannula **604** extending distally from the handle toward a distal end **606**. Distal end **606** is closed off, as at **608**, and includes a vacuum port or opening **610** which is sized and constructed allow fatty tissue to enter into the opening, which preventing larger blood vessels and organ tissue from entering.

A vacuum source **614** is in fluid communication with opening **610** through aspiration conduit **616** and handle **602**, as will be described in greater detail below. Handle **602** further includes a switch or lever **612** for selectively operating device **600**, and is connected to a source of power (not illustrated) via conduit **618**.

FIG. **13** illustrates a cross-sectional view of the distal tip **606** of the fat removal device **600**. Tip **606** is preferably constructed out of a hollow tube, such as a hypotube made of stainless steel, Nitinol, or a rigid polymer, has a blunt distal end **608** to prevent damaging tissue with the end of the probe, and includes a fluid lumen **626**. On the side of the tube is a vacuum port **610** to allow fat to be sucked into the cannula. A centrally located rotatable knife blade shaft **620** is provided within the cannular. Attached to the distal end of the shaft **620** is a semicircular knife blade **622** that rotates along the inner surface of the tube to cut the fat that has been sucked into the cannula.

Optionally, an artery/vein guard **624** is attached to the outer surface of the cannula that keeps medium sized arteries out of the port. In the embodiment illustrated in FIGS. **12–16**, guard **624** is a piece of thin protective material that projects from the outer surface of the cannula a short distance and then traverses the port opening. FIG. **15** illustrates an alternate configuration for guard **624**, where the guard has a cross-hair configuration to prevent damage to the blood vessels, e.g., coronary arteries or veins, when device **600** is used at different angles to the organ, e.g., heart. Other types of guards could also be used within the spirit and scope of the invention, such as posts located around the port opening, and/or a wide mesh around the port opening, as described above with reference to devices **100** and **300**. By way of example and not by limitation, the largest spacings between the portions of guard **624** which traverse port **610** are preferably between about 0.039 inches (1.0 mm) and about 0.078 inches (2.0 mm).

12

Knife blade **622** is preferably formed in an arc, so that the fatty tissue which enters into port **610** is sheared and carried into lumen **626**. Optionally, the knife blade is connected to a source of electric energy (not illustrated) such that the blade can cauterize while it cuts the fat. The knife blade may also be constructed as a unipolar cauterizer, in which case a grounding pad (not illustrated) would be connected to the patient in a location remote from the blade. The knife blade can also be constructed as a bipolar cauterizer, in which case the knife blade would be one pole, and distal tip **606** would be another pole. If a bipolar configuration is utilized, the distal tip **606** is preferably insulated from the rest of the cannula, by being formed separately with an insulating segment between the distal tip and the remainder of the cannula, and the inner surface of the cannula would have to be insulated from the rotating knife blade **622**, for example by coating with an appropriate dielectric material, e.g., PTFE.

Turning now to FIG. **16**, handle **602** of the fat remover device is schematically illustrated. Handle **602** is provided with a means for turning the remover on and off **612**, such as an on/off lever. Means **612** is operatively connected to the sources of power and vacuum to turn them on and off. A connection **628** is made between the vacuum tubing **616** and lumen **626**. A seal **630**, e.g., an O-ring, is placed around the knife blade shaft **620** to ensure that the vacuum is not lost proximal of the port opening **610** in the distal tip **606**. At the proximal end of the knife blade shaft **620**, a gear **632** is provided which attaches the shaft **620** to a motor assembly **634**. Motor **634** could be an electric motor, a pneumatic motor, as are commonly found in dental drills, or any other standard type of motor. The power source (not illustrated) to which motor **634** is connected is a source of power appropriate for powering motor **634**, e.g., a source of DC power, AC power, high pressure air, or high vacuum. The knife **622** can be operated at any desired speed (revolutions per minute), either a fixed or selectively variable as will be readily apparent to one of ordinary skill in the art.

There are numerous modifications that can be made to device **600** without departing from the inventive concept herein. For instance, rotating knife blade **622** could be attached via a rotating tube (not illustrated) instead of shaft **620** (or shaft **620** could be made to include a longitudinally extending lumen), and the aspiration lumen would always be in the center of the cannula and the rotating tube. Furthermore, the amount of vacuum supplied can vary to optimize sucking of the fat. Port **610** and guard **624** can optionally be provided at the distalmost end of device **600**.

The function of device **600** will now be described with reference to FIGS. **12–16**. Device **600** is preferably used by a health care practitioner by incising the epicardium connective tissue layer and inserting tip **608** of the device into an area of fat to be removed. On/off lever **612** is depressed, vacuum applied, and knife **622** would begin rotating. Optionally, if provided, power is supplied to blade **622** so that it acts as a cauterizer. The practitioner would then carefully remove the fat from under the epicardium and over the myocardium while leaving the coronary vessels intact, but pressing the distal tip **606** of device **600** against the fatty tissue, which will extrude through guard **624**, and be cut by the blade. The use of the vessel protectors should allow the practitioner to be able to remove fat from close to the coronary blood vessels without damaging them, because the coronary vessels would not enter into port **610** because of guard **624**.

Once the fat is removed from an area of the heart, the practitioner can then inspect the area and determine if there

13

is any bleeding from the small vessels that were connecting the fat tissue. These could then be cauterized using a standard electrocautery tool, if device 600 either is not provided with an electrocautery function, or if the electrocautery was incomplete. If the knife blade also served as an electrocauterizer, then there should be very limited bleeding and oozing from the fat removal.

FIGS. 17–20 schematically illustrate views of portions of a seventh exemplary embodiment of a fat removal device 700 in accordance with the present invention. Device 700 is a modification of device 600; accordingly, only those features of device 700 which differ from corresponding features of device 600 will be described. Device 700 includes a longitudinally extending cannula 702 which terminates at a distal end 704 in a closed blunt tip 706. A longitudinally extended rotatable shaft 708 extends through a lumen 710 of cannula 702. An aspiration port 712 fluidly communicates lumen 710 with the exterior of cannula 702. An artery/vein guard 714 extends out from around port 712 in a manner similar to artery/vein guard 624, described above.

Blade 716 is attached or otherwise formed at the distal end of shaft 708 immediately adjacent to port 712. Blade 716 is similar, but not identical to, blade 622. Blade 716 is shaped with a profile which is similar to an auger or the like, to push the material which extrudes through port 712 in a proximal direction when the blade rotates. Different from an auger, however, blade 716 still has a curved profile when viewed from the distal end thereof, and tapers proximally down toward shaft 708. Additionally, device 700 is provided with a bipolar electrocautery element, which in the embodiment illustrated in FIGS. 17–20 includes blade 716. Blade 716 forms one pole of the bipolar electrocautery element, while device 700 is further provided with ring electrodes 718 which extend around cannula 702 on the proximal and distal sides of port 712. Thus, blade 716 is one pole, while ring electrodes 718 are the other pole, of the bipolar electrocautery element. Suitable electrical leads for ring electrodes 718 are provided to provide a voltage at the ring electrodes (not illustrated), which leads can be located inside lumen 710 and through the wall of cannula 702, can be located on the exterior surface of the cannula, or can be embedded in the cannula wall itself. The details of bipolar electrocautery are well known by one of ordinary skill in the art, and are therefore not described herein.

FIGS. 18–20 illustrate an alternative embodiment of blade 718, which itself is a bipolar electrocautery device. Blade 720, an end view of which is illustrated in FIG. 18, includes at least three layers: a top conductive layer 722, which forms one pole of the bipolar electrocauterizer; a middle insulating layer 724; and a bottom layer 726, which forms a second pole of the bipolar electrocauterizer. FIG. 19 illustrates a perspective view of blade 720, and further illustrates electrical conductors 728 and 730 leading to top layer 722 and bottom layer 726, respectively. Conductors 728, 730 may be carried by shaft 708, or may be formed integral therewith. Suitable electrical insulation is provided around conductors 728, 730, as will be readily apparent to one of ordinary skill in the art. FIG. 20 illustrates yet another embodiment of the blade for device 700, in which blade 732 is curved in a manner similar to blade 622, described above.

The function of device 700 is the same as for device 600, except that the bipolar electrocautery element of device 700, and specifically blade 716, cauterizes the capillary bed of the fatty tissue which is cut by the blade.

FIGS. 21–23 schematically illustrate views of portions of an eighth exemplary embodiment of a fat removal device 800 in accordance with the present invention. Device 800 is

14

similar to devices 600 and 700, except that the fat is heated using RF monopolar or bipolar electrodes that protrude from the outer surface of the distal end of the device to heat, melt, and/or soften the fat to make it easier for the fat to be sucked into the vacuum port opening.

Turning now to FIGS. 21–23, device 800 includes a cannula 802 having a distal end 806 terminating in a blunt tip 808. An artery/vein guard 812 is positioned over a vacuum port opening 804 in the distal end 806 to prevent blood vessel, e.g., a coronary artery/vein, from being sucked into the fat removing device 800. Artery/vein guards 812 do not conduct electric energy and are attached to electrode posts 810 protruding from the outer surface of the cannula adjacent to port opening 804. Electrodes 810 are used to deliver RF energy to the fat tissue to heat the tissue to help make the tissue easier to be sucked into the tube. Electrodes 810 can be operated to heat the fatty tissue over a range of temperatures. Preferably, electrodes 810 heat the adjacent fat to a temperature between about 37 degrees centigrade and about 45 degrees centigrade, which the non-fatty tissues should tolerate well. Higher temperatures are also usable without damaging the underlying organ tissue, if for shorter periods of time. For example, if the vacuum is very high, temperatures over 100 degrees centigrade could be used without damaging the myocardium or coronary vessels in that the heat transfer would be primarily taken up in the fat and would be taken away quickly by aspiration. According to another embodiment, a thermocouple could be provided at the intersection of artery/vein guard members 812 to give temperature feedback to an RF controller. One suitable controller is a Stellartech RF generator, available from Stellartech Research Corporation, Mountain View, Calif.

The function of device 800 is the same as for device 700, except that RF electrodes 810 of device 800, heats the fatty tissue which is cut by the blade (not illustrated).

FIGS. 24 and 25 schematically illustrate views of portions of a ninth exemplary embodiment of a fat removal device 900 in accordance with the present invention. Device 900 is similar to the devices 600, 700, and 800, with the addition of structures for spraying pressurized liquid from at least one spray nozzle to assist in cutting the fatty tissue.

Turning now to the drawing figures, FIG. 24 illustrates a cross-sectional view of distal portions of device 900, while FIG. 25 illustrates a top plan view of the distal end of the device. Device 900 includes an inner cannula 908 and an outer cannula 902, which form a fluid lumen 910 between them and which is in fluid communication with a source of pressurized fluid (not illustrated) at the proximal end of device 900. Inner cannula 908 has an inner fluid lumen 912, which is preferably in fluid communication with a source of suction. Distal end 904 of device 900 includes a blunt tip 906, similar to the blunt tips of devices 600, 700, and 800.

A rotatable shaft 914 extends through lumen 912 and carries rotatable blade 916 at distal portions thereof immediately adjacent aspiration port 918. Blade 916 can alternatively be constructed similar to blades 622, 716, 720, or 732, described above. Artery/vein guards 926 are also provided to prevent a blood vessel from entering into port 918. To assist in cutting fat which is adjacent to port 918, device 900 includes high pressure spray nozzles 924 carried on posts 920 which extend away from outer cannula 902 around port 918. Nozzles 924 are in fluid communication with lumen 910, which carries high pressure fluid, via connecting conduits 922 in posts 920. Nozzles 924 are directed inwardly, that is, toward the center of opening 918. Preferably, artery/vein guard 926 is carried by posts 920.

As described above, the high pressure liquid can be optionally heated for delivery to nozzles 924. Heating the

15

liquid can help melt, soften, and/or dissolve the fat such that the fat is sucked into vacuum port **918** opening easier. The liquid can also lubricate the fat such that aspiration lumen **912** does not get clogged with fat.

Optionally, RF electrodes (not illustrated) could be further incorporated into device **900**, to help heat, melt, and/or soften the fat. The RF electrodes are preferably placed on top of spray nozzles **920**. A thermocouple (not illustrated) could also be included, preferably at the intersection of artery/vein guard **926**.

There are numerous further modifications to device **900** that can be made without departing from the inventive concept herein. For example, the liquid could be pumped to spray nozzle(s) **922** instead of using a pressurized reservoir. Different liquid solutions could be used, such as ones including therapeutic agents, lipophilic agents to aid in dissolving the fat, or the like. The vacuum pressure can be increased to assist the removal of the fat. The knife blade can be made in different configurations, as described above. The knife blade can be connected to a rotating tube, as described above, instead of rotating shaft **914** and the vacuum lumen can be inside the rotating tube.

The function of device **900** is the substantially the same as for device **800**, except that pressurized fluid is sprayed out of nozzles **922** while blade **916** cuts tissue. Furthermore, the pressurized liquid can be heated, which in turn will heat the fat and help drive the fat into the vacuum port opening to be cut by the rotating knife blade. As described above, RF energy may also be used to help heat, melt, and/or soften the fat.

FIGS. 26–29 schematically illustrate views of portions of a tenth exemplary embodiment of a fat removal device **1000** in accordance with the present invention. Device **1000** includes an electrocautery wand **1002** (see FIG. 26) and a fat extrusion tool **1004** (see FIG. 27). Wand **1002** includes a handle portion **1006**, from which an extension **1008** extends. An electrocautery loop **1010** extends from the distal end of extension **1008**. Electrocautery loops per se are well known to one of ordinary skill in the art. Handle **1006** includes a control switch **1012** which functions to control the application of energy to loop **1010**, thereby controlling the cauterizing function of the loop. A power cable **1014** extends from a proximal end of handle **1006**.

Fat extrusion tool **1004** is constructed to be used in conjunction with wand **1002**. Tool **1004** includes a handle **1016**, an extension **1018**, and a screen **1020** attached to the extension. Screen **1020** includes at least one, and preferably a plurality of holes or passages **1022** through which fat can be extruded, to be wiped away and cauterized by loop **1010** of wand **1002**. As illustrated in the embodiment of FIGS. 27–29, passages **1022** are more preferably arranged in a regular array, although the passages can be arranged in irregular patterns, or even randomly, and still be within the spirit and scope of the present invention. Screen **1020** is specially sized constructed to be usable with wand **1002**, as described in greater detail with reference to FIG. 28.

Turning now to FIG. 28, which is a schematic illustration of screen **1020**, and FIG. 29, which is a perspective illustration of the screen, the screen has a generally rectangular configuration. Screen **1020** can also be formed in other geometric configurations, such as circles, ovals, squares, triangles, and the like. Screen **1020** includes a plate **1024** through which passages **1022** are formed. An upstanding lip **1026** extends from plate **1024**, and defines the working area of screen **1020**. The width Y of plate **1024** between opposite sides of lip **1026** is selected to be approximately the same as, and preferably slightly greater than, width W of electrocau-

16

tery loop **1010** (see FIG. 26). By selecting dimensions Y and W in this manner, lip **1026** also functions as a restrain on the range of motion of loop **1010**, indicating to the practitioner that the loop is adjacent the edge of screen **1020**. Thus, lip **1026** aids in preventing cauterization of tissue other than that which has been made to extrude through passages **1022** of screen **1020**.

Screen **1020** further includes a flange **1030** attached to one side of plate **1024**, which includes an upstanding post **1028**. Post **1028** includes a central blind bore **1032**. Post **1028** is provided as a means to attach handle **1016** and extension **1018** to screen **1020**, for which extension **1018** is provided with a member (not illustrated) which mates with blind bore **1032** to join the extension to the screen. Flange **1030** distributes forces transmitted through handle **1016** and extension **1018** to screen **1020**, as described below.

In a preferred embodiment of device **1000**, passages **1022** have diameters between about 0.125 inches and about 0.300 inches, preferably about 0.156 inches. The spacing between the passages is between about 0.010 inches and about 0.500 inches, preferably about 0.040 inches. The depth of passages **1022**, which corresponds in this embodiment to the thickness of plate **1024**, is between about 0.015 inches and about 0.050 inches, preferably about 0.030 inches. Screen **1020** can be made of any number of suitable materials which are biocompatible, of moderate to high strength, and are readily manufactured to the required specifications. For example, screen **1020** can be formed of plastics, including thermoplastic and thermoset materials, metals, including stainless steel and Nitinol, or ceramics.

The function of device **1000** will now be described with reference to FIGS. 26–29. An organ which has a fatty tissue layer is exposed by, e.g., thoracotomy. A practitioner grasps wand **1002** and tool **1004** in each hand, and presses tool **1004** against the surface of the fat. Fat is thereby caused to extrude through the passages **1022**. The practitioner then presses control switch **1012**, and wipes electrocautery loop **1010** across that portion of plate **1024** inside lip **1026** to simultaneously scrape the fat away and cauterize the capillary bed in the fatty tissue. If desired, loop **1010** may be used without application of energy to the loop, and control switch **1012** may be selectively operated to cauterize only some of the time. When a sufficient amount of fat has been wiped away from a particular site, the screen is moved to another location on the organ, e.g., heart, to remove fat from that location.

FIGS. 30 and 31 schematically illustrate views of an eleventh exemplary embodiment of a fat removal device **1100** in accordance with the present invention. Device **1100** includes a handle **1102** configured to be easily grasped by the hand of a practitioner. Distal end **1104** of handle **1102** includes a screen **1106** having at least one, and preferably a plurality of passages or holes **1108** therethrough. Passages **1108** fluidly communicate the exterior of handle **1102** with the interior thereof. Handle **1102** further includes control switches **1110**, **1112**, and **1114**, for selectively controlling the flow of fluid through irrigation conduit **1116**, aspiration conduit **1118**, and power through cable **1120**. A motor (not illustrated) is provided in handle **1102**.

FIG. 31 illustrates handle **1102** with the distal portions of the handle broken away to expose blade **1122** which is rotatably carried in handle **1102**. Blade **1122** is similar to blades **322**, **410**, and **510**, described in greater detail above. Blade **1122** may optionally be constructed as an electrocautery device, also described in greater detail above, for which an additional control switch (not illustrated) on handle **1102** would be provided.

The function of device **1100** will now be described with reference to FIGS. **30** and **31**. An organ which has a fatty tissue layer is exposed by, e.g., thoracotomy. A practitioner grasps wand handle **1102** in a hand, and presses screen **1106** against the surface of the fat to be removed. By activating the switch fat is thereby caused to extrude through the passages **1022**. The practitioner then selectively presses control switches **1110**, **1112**, and **1114** to selectively irrigate the inner surface of screen **1106**, aspirate any fat which has been extruded through the screen, and rotate blade **1122** to cut fat which has been extruded through the screen. Optionally, power is supplied to an electrocautery element (not illustrated) in device **1100**, which preferably is blade **1122**, to cauterize the capillary bed of the fatty tissue. When a sufficient amount of fat has been removed, the practitioner moves handle **1102** to another site, and presses screen **1122** against the fat.

FIGS. **32** and **33** schematically illustrate views of a twelfth exemplary embodiment of a fat removal device **1200** in accordance with the present invention. Device **1200** includes a handle **1202** configured to be easily grasped by the hand of a practitioner. An extension **1204** extends distally from handle **1202** and connects to a plate **1206**. Plate **1206** is preferably constructed very similar to plate **1024** described above with reference to FIGS. **27–29**, with several differences described in greater detail below.

An electrocautery wire **1208** is provided in device **1200** to cut fat tissue that extrudes through the holes **1210** in plate **1206**, in a fashion similar to the embodiments described above. Wire **1208** is connected to an actuator **1212** which extends proximally up through or along the exterior of extension **1204** and into handle **1202**. A slidable control member **1214** is attached to actuator **1212**, and extends from an interior of handle **1202** (not illustrated) so that a practitioner can slide actuator **1212** proximally and distally along the handle, as indicated by arrow **1216**. Proximal and distal movement of actuator **1212** causes wire **1208** to move back and forth, as indicated by arrow **1218**, in and along a top surface **1220** of plate **1206**. Actuator **1212** preferably is formed of an electrically conductive material, or includes an electrical conductor (not illustrated) therein. A power lead **1222** is connected to a proximal portion of actuator **1212** so that electric power transmitted from the power lead is transmitted to wire **1208**.

FIG. **33** illustrates an enlarged perspective view of portions of device **1200**. Plate **1206** includes a recessed top surface **1220** in which holes **1210** are formed. The size and placement of holes **1210** are substantially similar to the size and placement of passages **1022** in screen **1020**, described above with reference to FIGS. **27–29**. Plate **1206** includes a raised edge **1224** which preferably extends around the entire periphery of the plate. A sidewall **1226** extends between edge **1224** and surface **1220**. A pair of slots **1228**, **1230** are formed into sidewall **1226**, which receive the ends of wire **1208**. Wire **1208** thus can slide in slots **1228**, **1230** back and forth, as indicated by arrow **1218**, in and along top surface **1220** of plate **1206**. As illustrated in FIG. **33**, actuator **1212** extends through extension **1204**, through edge **1224**, through sidewall **1226**, and connects to wire **1208**. In accordance with yet another embodiment of the present invention (not illustrated), actuator **1212** can extend along an outer surface of extension **1204**. Optionally, actuator **1212** can be to wire **1208** by a pulley (not illustrated).

The function of device **1200** will now be described with reference to FIGS. **32** and **33**. An organ which has a fatty tissue layer is exposed by, e.g., thoracotomy. A practitioner grasps handle **1202**, and presses plate **1206** against the

surface of the fat. Fat is thereby caused to extrude through holes **1210**. The practitioner then slides control member **1214** and slides wire **1208** across surface **1220** to simultaneously scrape the fat away and cauterize the capillary bed in the fatty tissue. If desired, wire **1208** may be used without application of energy to the loop. When a sufficient amount of fat has been wiped away from a particular site, device **1200** is moved to another location on the organ, e.g., heart, to remove fat from that location.

FIGS. **34** and **35** schematically illustrate views of a thirteenth exemplary embodiment of a bipolar radio frequency fat removal device **1300** in accordance with the present invention. Device **1300** includes a handle **1302**, two identical bi-polar electrodes **1304**, and a spacer bar **1306**. The bi-polar electrodes **1304** can be made any shape, including straight electrodes to fit the contour of the surface they are to be applied to. It has been found that an efficacious electrode has a wire diameter of about 0.015–0.045 inches, with a preferable wire diameter of 0.031 inches, and that the electrodes be spaced apart from about 0.040 to about 0.200 inches, with a preferable spacing of 0.080 inches, from the centerline of one wire to the centerline of the other wire. A high impedance (e.g., 500 to 2500 ohms) RF generator is used to apply power between the two electrodes **1304** through the fat in the immediate area, thereby melting the fat. If needed, an artery/vein guard, such as that shown in FIGS. **27–29**, can be used for their protection. If further desired, an aspiration device can be used to collect the melted fat, as will be readily appreciated by one of skill in the art.

FIGS. **36A**, **B** and **C** illustrate a fourteenth exemplary embodiment of a bipolar radio frequency fat removal device **1400** which includes a shaft **1402** with distal holes **1404** that is placed through a thoracotomy by the proximal handle **1416** with an on/off switch **1418**, power on/off light indicator **1420**, a vacuum port **1412**, and RF power connection **1422**. FIG. **36B** again illustrates the sheath **1402** with distal tip holes **1404** for fat to enter and bipolar electrodes **1406** and **1408** being rotating wireforms evenly spaced apart by spacers **1410**. The wireform bipolar electrodes of preferable diameters between about 0.015 to 0.045 inches, with a more preferable diameter of 0.031, one spaced inside the other at a centerline to centerline distance from 0.040 to 0.2000 inches, with a preferable distance of 0.080 inches, are formed in a spiral or helical configuration and rotated in such a fashion to move the melted fat to the proximal end of the device for removal through a vacuum port **1412**. FIG. **36C** illustrates the same device as in FIG. **36B**, except the electrodes **1406** and **1408** are positioned beside each other at the same spacing as in FIG. **36B**. The proximal, handle end of the device is constructed to mate with a rotating mechanism with rotating seals such that the wire form electrodes are rotated as a unit and held in position relative to the outer sheath by spacers **1414**. Notably, the wireforms only need to extend slightly beyond the holes **1404** and from there back to the proximal end of the device can be of any form or configuration as long as the spacing between the electrodes is maintained. It should also be noted that in the preferred embodiment the holes **1404** in FIGS. **36A**, **B** and **C** would extend only 180 degrees of the 360 degrees around the axis of the sheath **1408**.

The function of the device in FIGS. **36A**, **B** and **C** will now be described. Using the handle **1416** the sheath **1402** is pushed through the thoracotomy until the distal tip **1404** is pressed against the fat. The suction, RF power and inner electrodes rotating motor are turned on and the distal tip **1404** positioned over the area of fat to be removed and

advanced as the fat is melted away and removed from the area by the vacuum.

FIGS. 37A, B, C, and D illustrate a fifteenth embodiment of a bipolar radio frequency fat removal device **1500** similar to the fourteenth embodiment except as shown by FIGS. 37B and C. The outer sheath **1508**, which includes distal holes **1504**, is used as one of the electrode and there is a single rotating inner electrode **1510** of wireform or solid form with spacers **1514** maintaining the required spacing between the electrodes, and there is an inner auger **1524** in FIG. 37C which is rotated to move the fat from the distal to the proximal end of the device. FIG. 37D illustrated a gear box that rotates the inner electrode **1510** relative to the outer electrode **1508**, and rotates the auger **1524** relative to the inner electrode **1510** to optimize melting and movement of the fat to the exit vacuum port **1512**. Item **1528** in FIG. 37A will be explained in the discussion of FIG. 38. It should also be noted that in the preferred embodiment the holes **1504** in FIGS. 37A, B and C would extend only 180 degrees of the 360 degrees around the axis of the sheath **1508**.

The functions of the device in FIGS. 37A, B, C and D are generally the same as in FIGS. 36A, B and C except there is a gear box to rotate only one inner electrode and in addition there is a rotating auger to move the fat from the distal tip to the proximal end of the sheath and out the vacuum port.

The sixteenth embodiment depicted by FIGS. 38A and B is similar to embodiments fourteenth and fifteen illustrated by FIGS. 36 and 37, except there is a central lumen **1630** starting at the distal tip and running axially to the proximal outlet **1628** allowing for use of an endoscope to view the area being treated and/or to provide a conduit for a therapeutic device such as pacing lead attachment or other desired therapeutic procedures. In this version, the fat enters holes **1604** and is melted by bipolar electrodes **1608** and **1610**, evenly spaced by spacer **1614**, and the melted fat travels between the two bipolar electrodes to the proximal end and out the vacuum port **1612**. Further optionally, the device may include holes in the inner electrode **1610** for transmission of the melted fat from the distal tip to the vacuum port via a proximal hole in electrode **1610** communicating with vacuum port **1612**. Rotation of the inner electrode relative to the outer electrode may alternatively be performed in accordance with the present invention. In a preferred embodiment, the holes **1604** in FIGS. 38A, B, and C would extend only 180 degrees of the 360 degrees around the axis of the sheath **1608**.

The function of the device in FIGS. 38A and B is similar to the two previously described devices, with the exceptions that there is a lumen along the axis of the device to accept an angioscope to view the area being treated or a therapeutic device to treat the area, attach diagnostic or pacing leads, etc. This device can, but does not have to, have a moving inner electrode.

While the invention has been described in detail with reference to preferred embodiments thereof, it will be apparent to one skilled in the art that various changes can be made, and equivalents employed, without departing from the scope of the invention.

What is claimed is:

1. A fat removing device comprising:

a cannula having a longitudinal axis, a proximal end, a distal end, a lumen extending proximally along said longitudinal axis, and an opening in said cannula at said distal end which fluidly communicates said lumen with the exterior of said cannula;

a protective mesh attached to said distal end and distal of said opening, said mesh including openings sized to

permit human fat cells to extrude through said openings when said mesh is pressed against a mass of human fatty tissue, said openings also sized to prevent a human blood vessel which underlies said human fatty tissue from passing through said openings when said mesh is pressed against said mass of human fatty tissue.

2. A fat removing device in accordance with claim 1, further comprising an ultrasonic energy transducer positioned adjacent said distal end which operates at a frequency and magnitude which at least partially disrupts the cell walls of said human fat cells.

3. A fat removing device in accordance with claim 1, further comprising a heater positioned adjacent said distal end which heats said human fat cells when said heater is energized to deliver heat.

4. A fat removing device in accordance with claim 3, wherein said heater is positioned a distance from said mesh and capable of delivering heat energy to said human fat cells to cauterize a capillary bed in said mass of human fatty tissue when energized to deliver heat.

5. A fat removing device in accordance with claim 1, wherein said cannula is rigid.

6. A fat removing device in accordance with claim 1, wherein said protective mesh is dome-shaped.

7. A fat removing device in accordance with claim 6, wherein said dome-shaped protective mesh comprises a plurality of passages therethrough, and a distalmost bearing portion which does not include any passages.

8. A fat removing device in accordance with claim 1, further comprising:

a cutting element in the cannula, wherein said protective mesh has a shape, and said cutting element has substantially the same shape and is spaced from said protective screen.

9. A fat removing device in accordance with claim 1, wherein said cannula is an outer cannula, and further comprising an inner cannula positioned in said outer cannula, said inner cannula being rotatable in said outer cannula, said inner cannula including a cutting element positioned adjacent and proximal to said protective mesh, whereby when said inner cannula is rotated, and said device is pressed against human fatty tissue to extrude fatty tissue through said openings, said cutting element cuts off said extruded fatty tissue proximal of said protective mesh.

10. A fat removing device in accordance with claim 9, wherein said inner cannula comprises a blade formed by the removal of a portion of said inner cannula.

11. A fat removing device in accordance with claim 9, further comprising an annular lumen extending between said inner cannula and said outer cannula.

12. A fat removing device in accordance with claim 9, wherein said inner cannula comprises a distal end and a lumen extending proximally from said distal end.

13. The fat removal device of claim 1, wherein the openings in the mesh are between 0.125 and 0.300 inches across.

14. A fat removing device comprising:

a cannula having a longitudinal axis, a proximal end, a distal end, a closed tip at said distal end, a lumen extending proximally along said longitudinal axis, and an opening in said cannula proximal of said distal end which fluidly communicates said lumen with the exterior of said cannula;

a rotatable shaft in said cannula;

a blade attached to said rotatable shaft adjacent said opening;

wherein when said cannula opening is pressed against a mass of human fatty tissue, and when said rotatable

21

shaft is caused to rotate, said blade rotates and cuts fatty tissue which has extruded through said opening, said cannula opening being sized to prevent a human blood vessel which underlies said human fatty tissue from passing into said cannula opening when pressed against said mass of human fatty tissue.

15. A fat removing device in accordance with claim 14, wherein said blade is mounted to said rotatable shaft offset from an axis of rotation of said rotatable shaft.

16. A fat removing device in accordance with claim 14, wherein said blade is cup-shaped.

17. A fat removing device in accordance with claim 14, further comprising a vein guard mounted on an exterior surface of said cannular immediately adjacent to said opening.

18. A fat removing device in accordance with claim 17, wherein said vein guard comprises a thin member which extends from a point distal of said opening to a point proximal of said opening and extends across said opening.

19. A fat removing device in accordance with claim 18, wherein said thin member is a first thin member, and said vein guard comprises a second thin member which extends across said first thin member.

20. A fat removing device in accordance with claim 14, wherein said blade is formed of a material which allows said at least one blade to be energized as an electrocautery tool.

21. A fat removing device in accordance with claim 14, wherein said rotatable shaft has an axis of rotation, said blade includes a distal tip and a proximal end, said blade angling relative to said axis of rotation from said distal tip to said proximal end, said blade being curved in a direction substantially perpendicular to said axis of rotation so that said blade acts as an auger when rotated about said axis of rotation.

22. A fat removing device in accordance with claim 14, further comprising at least one ring electrode on the exterior of said cannula, wherein said at least one ring electrode and said blade together form two poles of a bipolar electrocautery circuit.

23. A fat removing device in accordance with claim 14, wherein said blade is formed of at least three layers, including a top layer formed of an electrically conductive material, a bottom layer formed of an electrically conductive material, and a middle layer formed of an electrically insulative material, wherein when said top layer and said bottom layer are connected to opposite poles of an electrocauterizing device, said blade is a bipolar electrocauterizer.

24. A fat removing device in accordance with claim 14, further comprising at least one RF electrode protruding from the exterior of said cannula adjacent to said opening.

25. A fat removing device in accordance with claim 24, wherein said at least one RF electrode comprises two RF electrodes protruding from said cannula on opposite sides of said opening.

26. A fat removing device in accordance with claim 24, wherein said at least one RF electrode comprises four RF electrodes.

27. A fat removing device in accordance with claim 14, further comprising at least one fluid nozzle adjacent said opening and directed toward said opening, and a high pressure fluid lumen in fluid communication with said at least one nozzle, wherein when said cannula is pressed against fatty tissue and fatty tissue is thereby caused to extrude into said opening, and high pressure fluid is caused to flow through said high pressure fluid lumen and out said at least one nozzle, said high pressure fluid cuts said fatty tissue.

22

28. A fat removing device in accordance with claim 27, wherein said at least one fluid nozzle comprises two fluid nozzles.

29. The fat removal device of claim 14, wherein the cannula opening is between 0.125 and 0.300 inches across.

30. A fat removal tool for removing fat from the outer surface of an internal body organ, comprising:

a screen having at least one passageway sized to allow fat cells to extrude through the screen while preventing a blood vessel selected from the group consisting of a patient's coronary arteries, a patient's cardiac veins, and both, from passing through said screen;

a separate cutting member positionable adjacent to said screen to cut fat which has been extruded through said screen passageway.

31. A fat removal tool in accordance with claim 30, wherein said at least one passageway comprises a plurality of passageways arranged in a regular array.

32. A fat removal tool in accordance with claim 30, wherein said screen includes a substantially rectangular plate in which said at least one passageway is formed, said plate including a peripheral upstanding lip.

33. A fat removal tool in accordance with claim 30, further comprising a handle attached to said screen.

34. The fat removal tool of claim 30, wherein the passageways in the screen are between 0.125 and 0.300 inches across.

35. A fat removal tool for removing fat from the outer surface of an internal body organ, comprising:

a handle having a proximal end, a distal end, and a hollow interior;

a screen at said handle distal end, said screen including at least one passage therethrough, the at least one passage being dimensioned to allow fat cells to extrude through while preventing a blood vessel from passing there-through;

a rotatable blade in said handle and immediately proximal of said screen; and

a rotatable shaft attached to said blade and extending proximally from said rotatable blade.

36. A fat removal tool in accordance with claim 35, wherein said screen is circular and flat.

37. A fat removal tool in accordance with claim 35, further comprising a source of suction in fluid communication with said hollow interior, a source of irrigation fluid in fluid communication with said hollow interior, and a source of electric power in electrical communication with said rotatable blade.

38. A fat removal tool in accordance with claim 37, said handle further comprising a suction control switch which controls fluid flow to said source of suction, an irrigation control switch which controls fluid flow to said hollow interior, and a power control switch which controls current flow to said rotatable blade.

39. The fat removal tool of claim 35, wherein the at least one passageway in the screen is between 0.125 and 0.300 inches across.

40. A fat removal tool for removing fat from the outer surface of an internal body organ, comprising:

a screen having at least one passageway sized to allow fat cells to extrude through the screen while preventing a blood vessel selected from the group consisting of a patient's coronary arteries, a patient's cardiac veins, and both, from passing through said screen;

a cutting member adjacent to said screen and movable over said screen to cut fat which has been extruded through said screen passageway.

23

41. A fat removal tool in accordance with claim 40, further comprising a handle, and an extension connected between said handle and said screen.

42. A fat removal tool in accordance with claim 41, further comprising an actuator connected to said cutting member and extending proximally from said cutting member to said handle, said actuator being movable along said handle, wherein movement of said actuator along said handle moves said cutting member over said screen to cut fat which has been extruded through said screen passageway.

43. A fat removal tool in accordance with claim 42, wherein said actuator includes electrically conductive portions in electrical communication with said cutting member, and said cutting member is formed of a material which allows said cutting member to be energized as an electrocautery tool.

44. A fat removal tool in accordance with claim 40, wherein said screen comprises a substantially rectangular plate in which said at least one passageway is formed, a peripheral upstanding lip, and a sidewall extending between said lip and said plate.

45. A fat removal tool in accordance with claim 44, further comprising two slots formed in said sidewall, said cutting member having two ends slidably located in said slots, wherein when said actuator is moved along said handle, said actuator slides said cutting member in said slots and over said screen to cut fat which has been extruded through said screen passageway.

46. The fat removal tool of claim 40, wherein the at least one passageway in the screen is between 0.125 and 0.300 inches across.

47. A method of removing a fat layer from the surface of an internal body organ, comprising the steps:

24

exposing a portion of said fat layer;

pressing said fat layer with a surface having at least one hole, the hole being dimensioned to allow fat cells to extrude through while preventing a blood vessel from passing therethrough;

extruding fat through said at least one hole; and

cutting said fat that has extruded through said hole on a side of said surface opposite said fat layer.

48. A method in accordance with claim 47, wherein said step of extruding fat further comprises the step of preventing blood vessels from passing through said at least one hole.

49. A method in accordance with claim 47, wherein said step of cutting said fat further comprises cutting said fat with an electrocautery cutting element.

50. A method in accordance with claim 47, further comprising heating fatty tissue in said fat layer at a time selected from the group consisting of prior to said cutting step, during said cutting step, and both prior and during said cutting step.

51. A method in accordance with claim 47, wherein said step of pressing said fat layer further comprises pressing with a surface having at least one hole located on a distalmost end of a cannula.

52. A method in accordance with claim 47, wherein said step of pressing said fat layer further comprises pressing with a surface having at least one hole located proximal of a distalmost end of a cannula.

53. The method of claim 47, wherein the hole is dimensioned with a diameter of between 0.125 and 0.300 inches across.

* * * * *

专利名称(译)	脂肪去除装置和方法		
公开(公告)号	US6626890	公开(公告)日	2003-09-30
申请号	US09/874360	申请日	2001-06-06
[标]申请(专利权)人(译)	阮HIEN WALL JEFFREY P —瓦德瓦尼SURESHk ADLPARVAR PAYAM 斯坦博BRUCE BROWN TONY - [R		
申请(专利权)人(译)	阮HIEN WALL JEFFREY P. —瓦德瓦尼SURESH K. ADLPARVAR PAYAM 斯坦博BRUCE BROWN TONY R.		
当前申请(专利权)人(译)	BROWN , TONY R.		
[标]发明人	NGUYEN HIEN WALL JEFFREY P WADHWANI SURESH K ADLPARVAR PAYAM STAMBAUGH BRUCE BROWN TONY R		
发明人	NGUYEN, HIEN WALL, JEFFREY P. WADHWANI, SURESH K. ADLPARVAR, PAYAM STAMBAUGH, BRUCE BROWN, TONY R.		
IPC分类号	A61B17/32 A61B18/14 A61M1/00 A61B17/22 A61B17/00		
CPC分类号	A61B17/320016 A61B17/32002 A61B18/1402 A61B17/320068 A61B18/14 A61B2017/00243 A61B2017/00685 A61B2017/320775 A61B2018/00196 A61B2018/00208 A61B2018/00464 A61B2018/00595 A61B2018/1435 A61B2018/1861 A61B2019/481 A61B2218/002 A61B2218/007 A61M1/0084 A61M2202/08 Y10S604/902 A61B2017/320069 A61B2017/32007 A61B2090/08021		
审查员(译)	BASICHAS , ALFRED		
其他公开文献	US20020188280A1		
外部链接	Espacenet USPTO		

摘要(译)

一种脂肪去除装置包括筛网，所述筛网包括通道，脂肪可以通过所述通道被挤出，被切割或熔化远离内脏器官的表面。该装置包括用于切割脂肪或射频单极或双极电极的刀片以熔化脂肪，抽吸以从屏幕和刀片移除脂肪，用于冲洗筛网和刀片的灌溉，以及用于烧灼毛细血管床的电烙器构件。脂肪。还描述了使用从体内器官表面去除脂肪层的方法。

