




US 20140094687A1





(19) **United States**(12) **Patent Application Publication**
Razzaque et al.(10) **Pub. No.: US 2014/0094687 A1**(43) **Pub. Date: Apr. 3, 2014**(54) **IMAGE ANNOTATION IN IMAGE-GUIDED
MEDICAL PROCEDURES****Publication Classification**(51) **Int. Cl.***A61B 5/00* (2006.01)*A61B 6/03* (2006.01)*A61B 8/12* (2006.01)*A61B 19/00* (2006.01)*A61B 18/14* (2006.01)(52) **U.S. Cl.**CPC *A61B 5/748* (2013.01); *A61B 19/5244*(2013.01); *A61B 18/1477* (2013.01); *A61B**8/12* (2013.01); *A61B 6/032* (2013.01)USPC **600/424**(71) Applicant: **InnerOptic Technology, Inc.,**
Hillsborough, NC (US)(72) Inventors: **Sharif Razzaque**, Chapel Hill, NC (US);
Andrei State, Chapel Hill, NC (US)(73) Assignee: **InnerOptic Technology, Inc.,**
Hillsborough, NC (US)(21) Appl. No.: **14/047,628**(22) Filed: **Oct. 7, 2013****Related U.S. Application Data**(63) Continuation of application No. 13/014,596, filed on
Jan. 26, 2011, now Pat. No. 8,554,307.(60) Provisional application No. 61/322,991, filed on Apr.
12, 2010, provisional application No. 61/387,132,
filed on Sep. 28, 2010.


(57)

ABSTRACT

Presented herein are methods, systems, devices, and computer-readable media for image annotation in image-guided medical procedures. Some embodiments herein allow physicians or other operators to use one or more medical devices in order to define annotations in 3D space. These annotations may later be displayed to the physician or operator in 3D space in the position in which they were first drawn or otherwise generated. In some embodiments, the operator may use various available medical devices, such as needles, scalpels, or even a finger in order to define the annotation. Embodiments herein may allow an operator to more conveniently and efficiently annotate visualizable medical data.

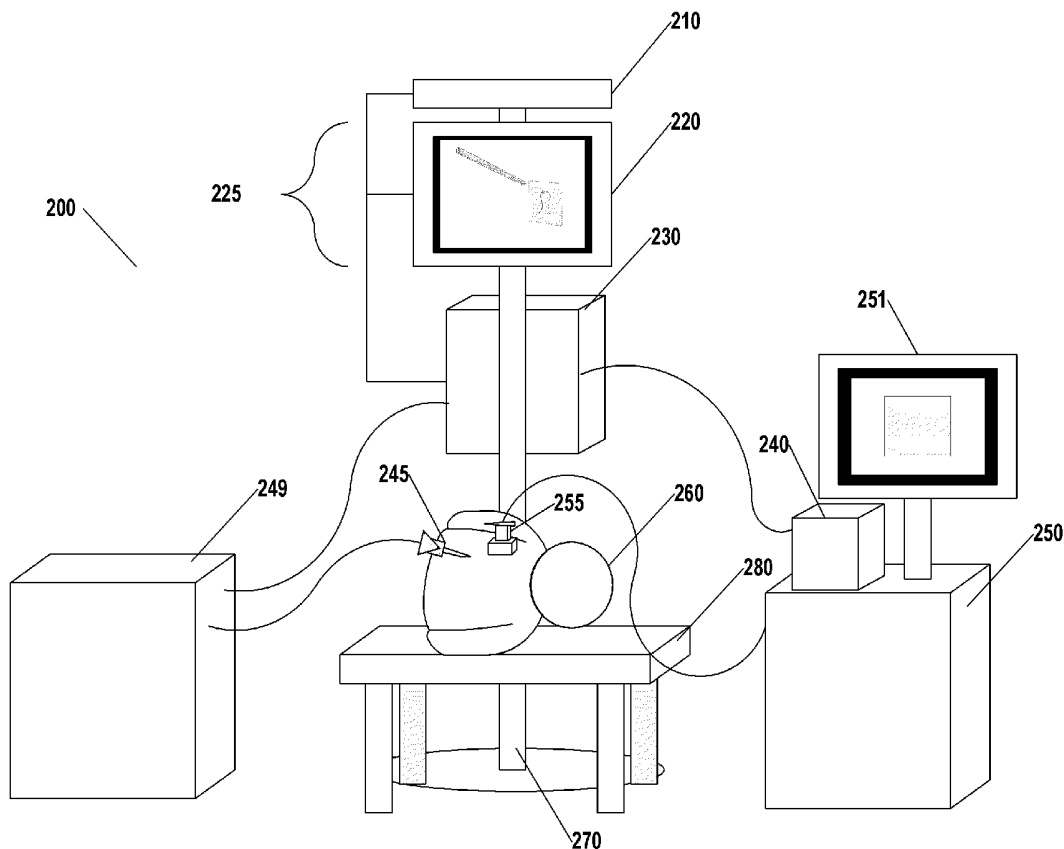

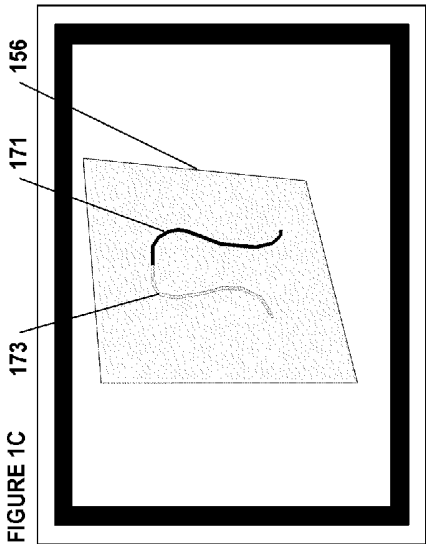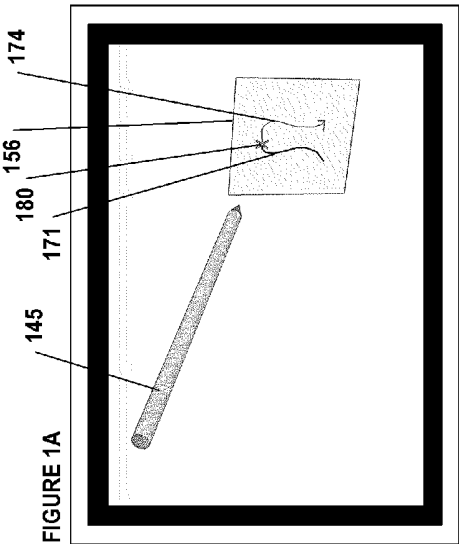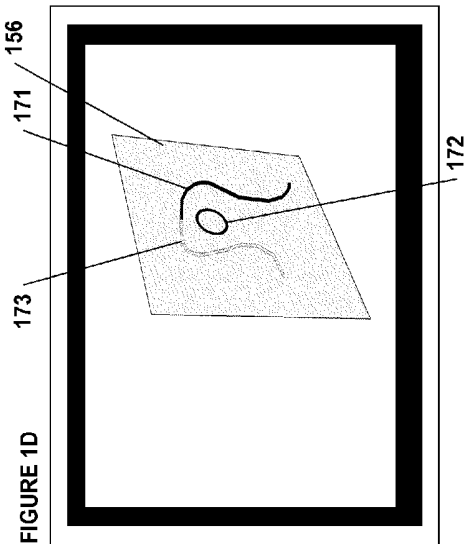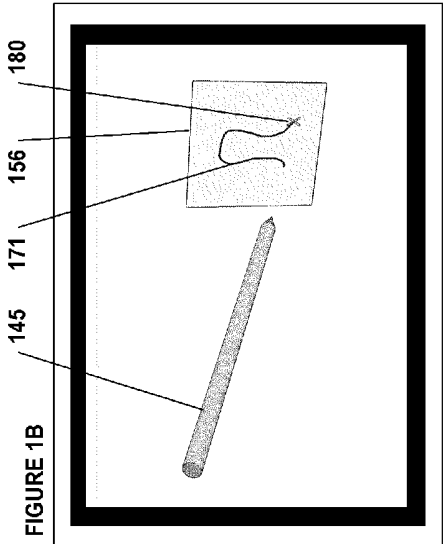

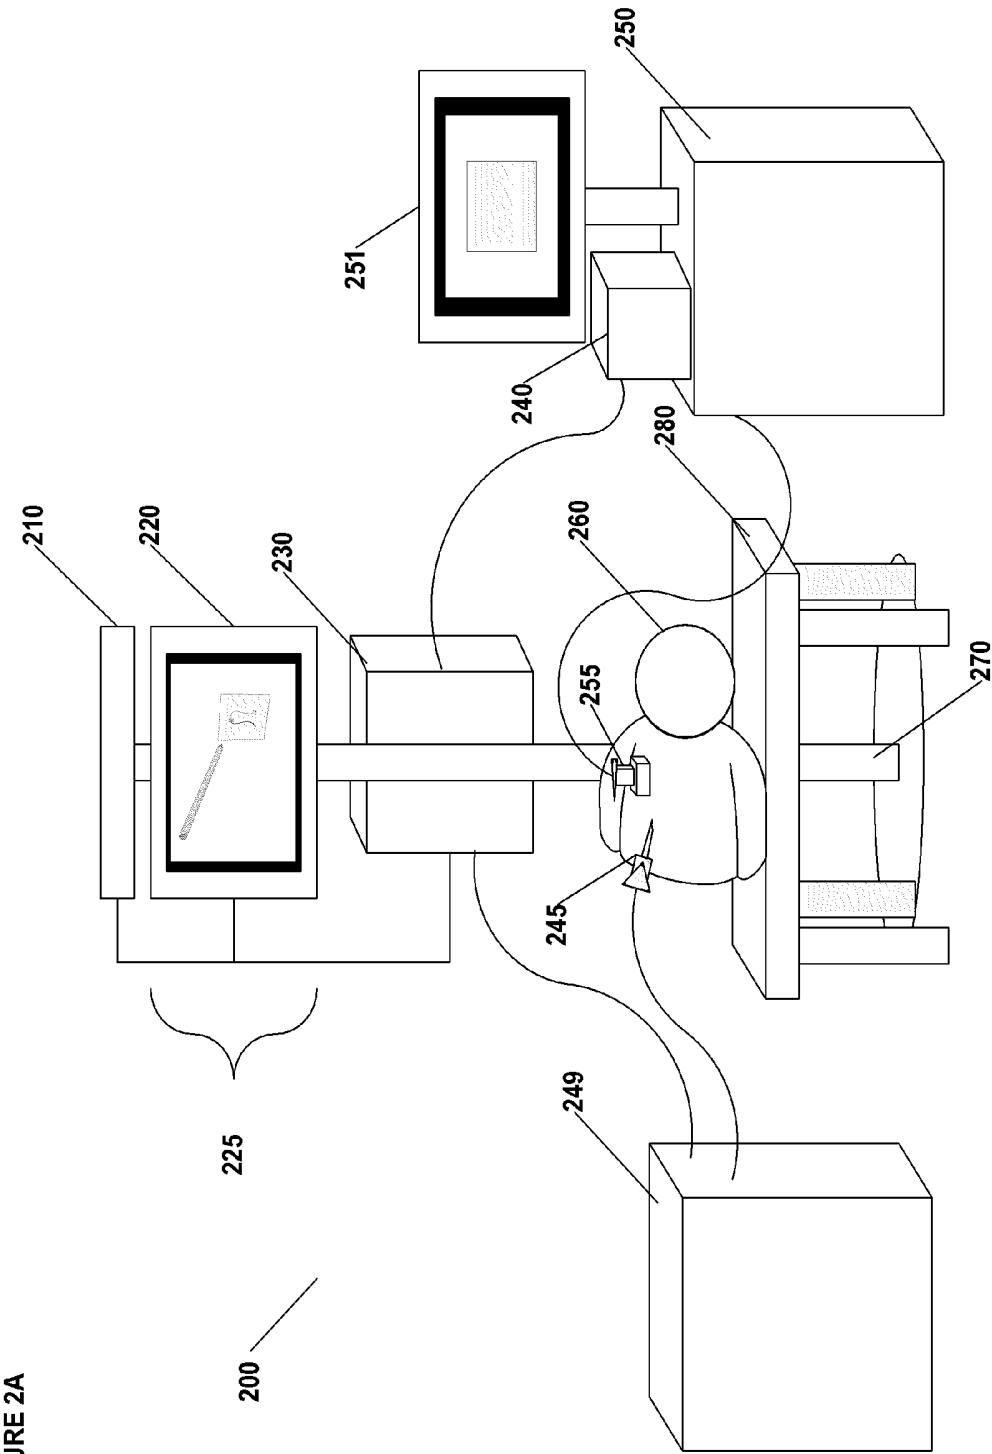

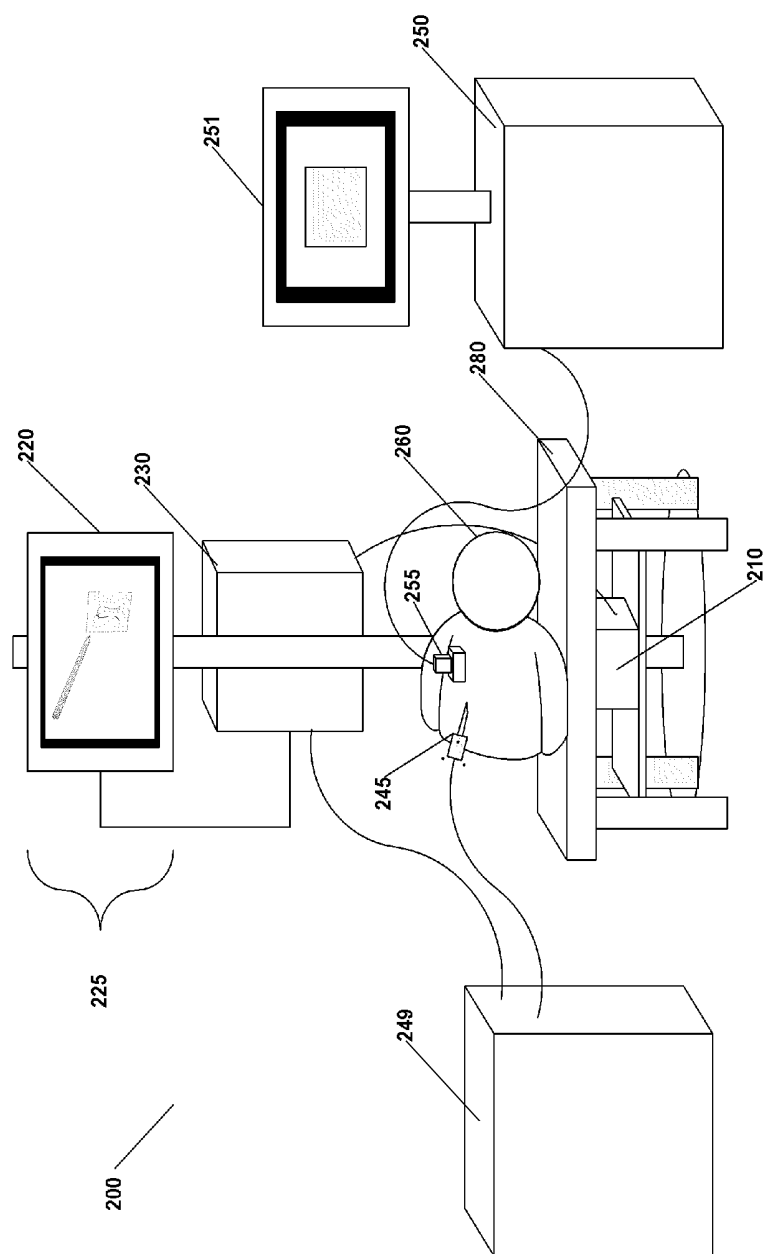
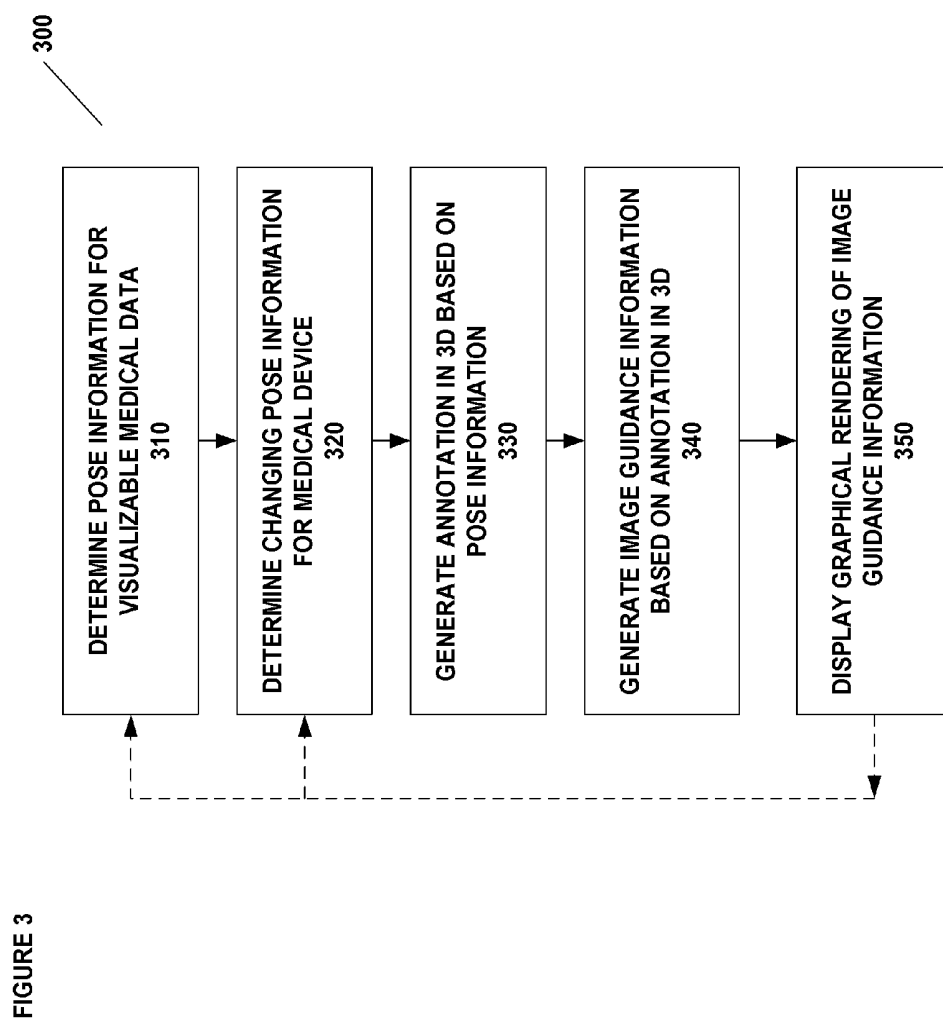
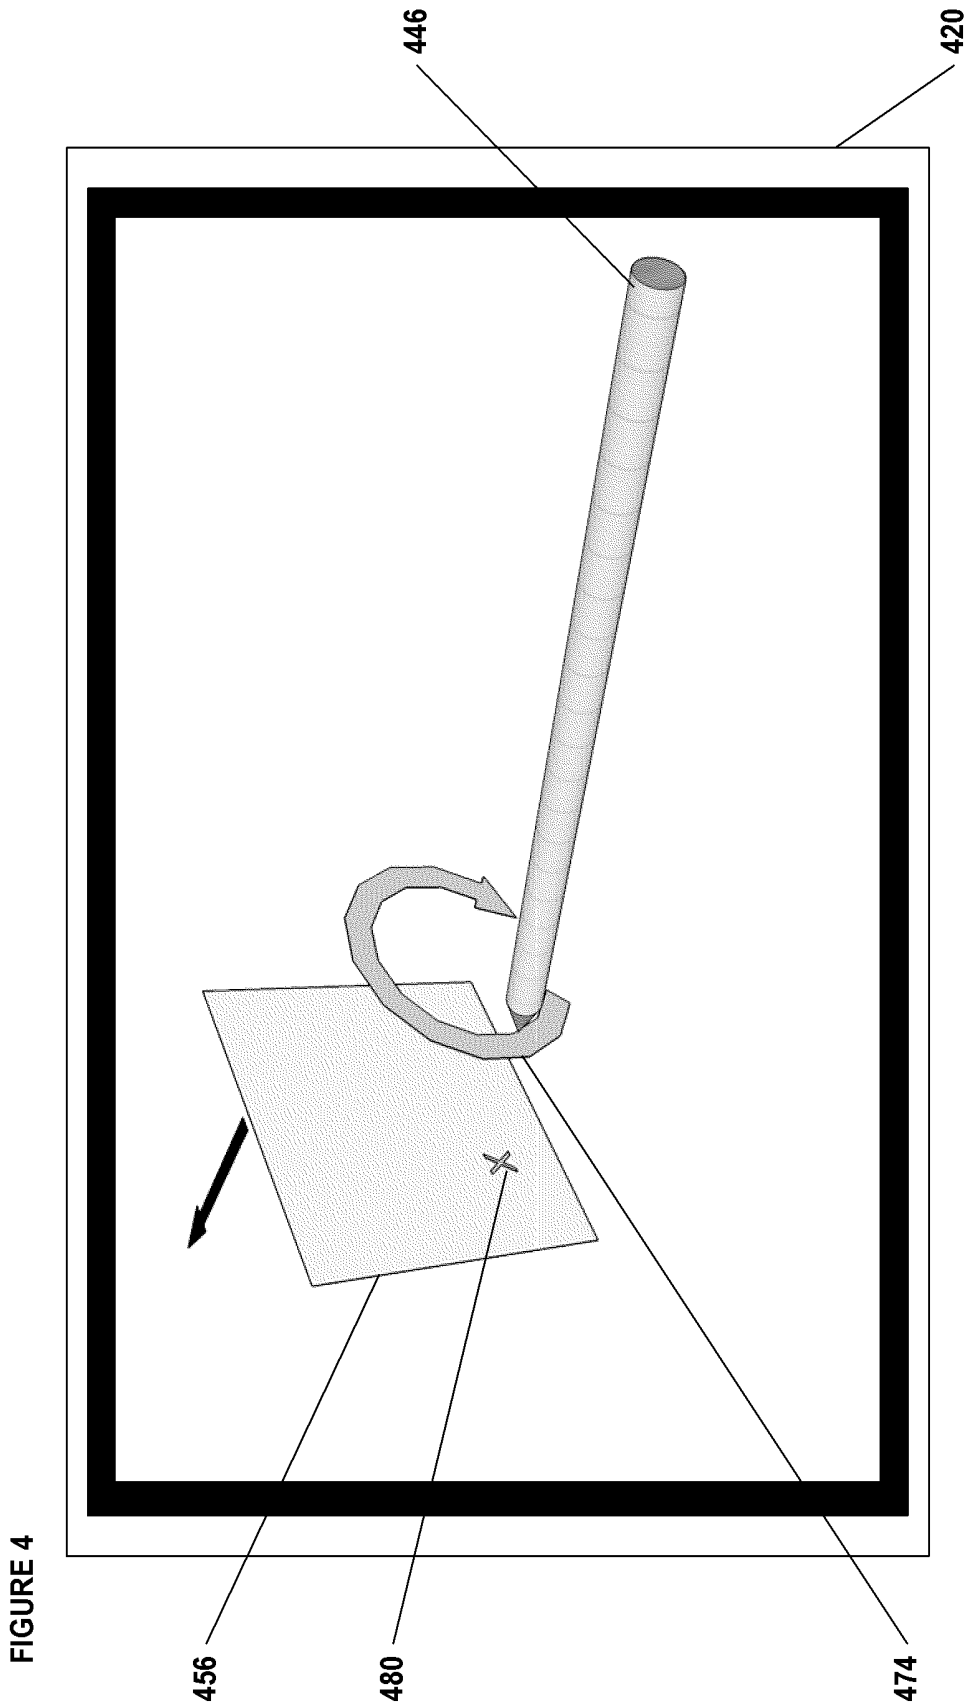
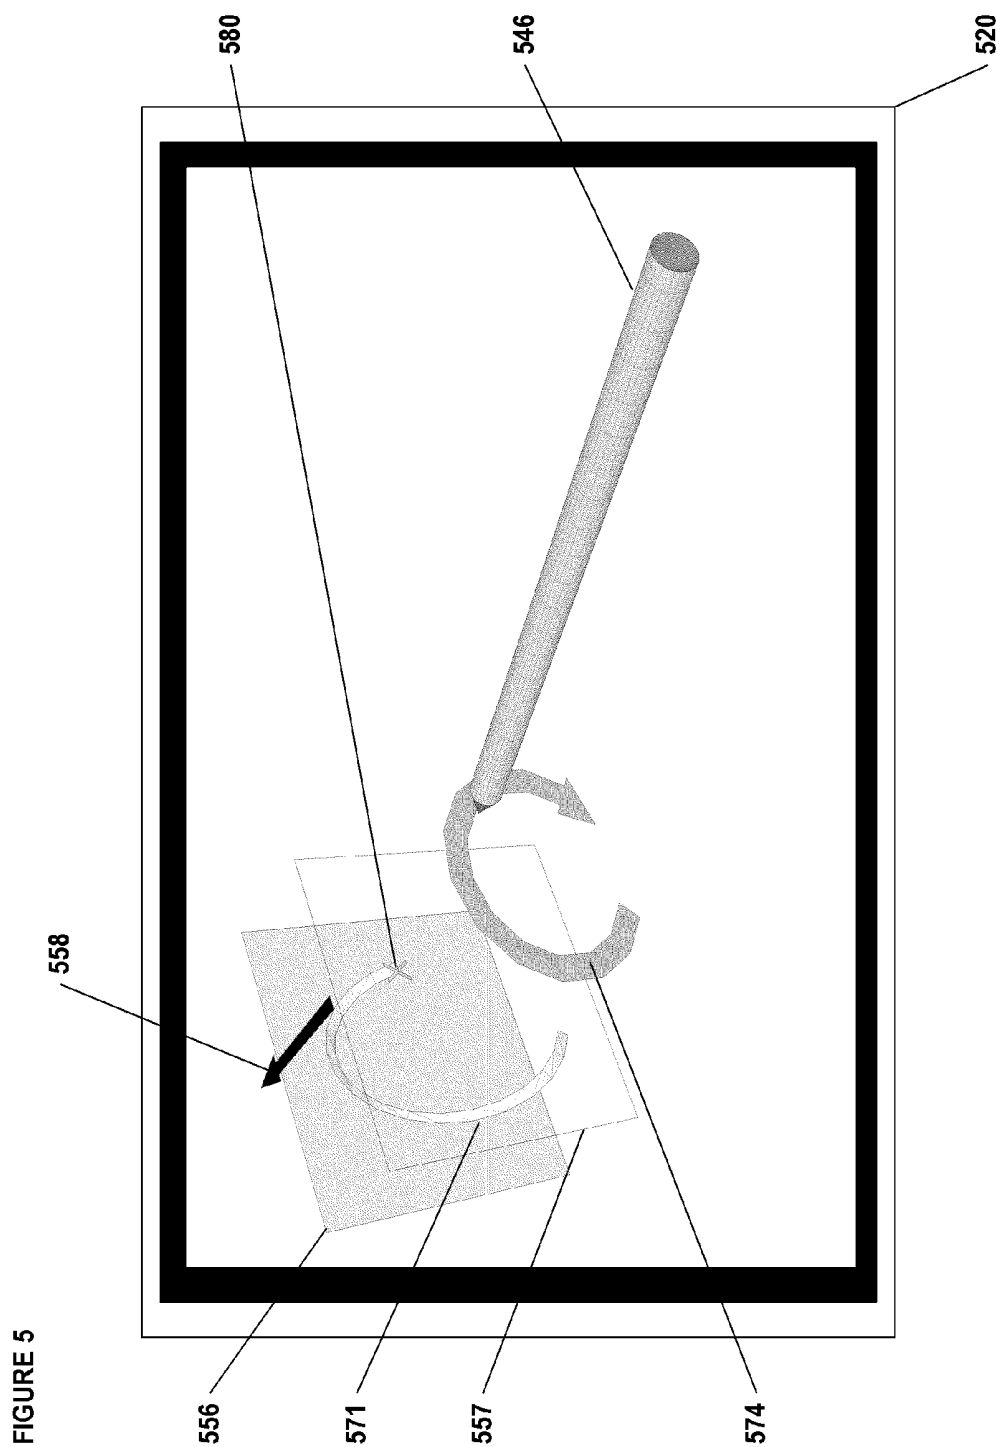
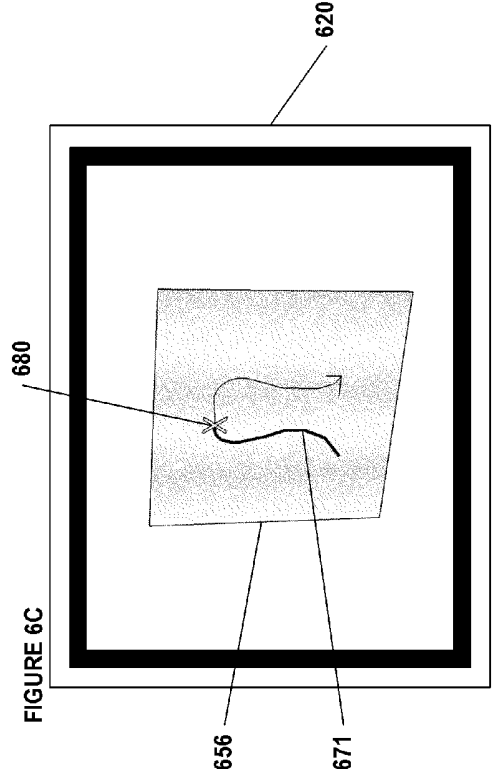
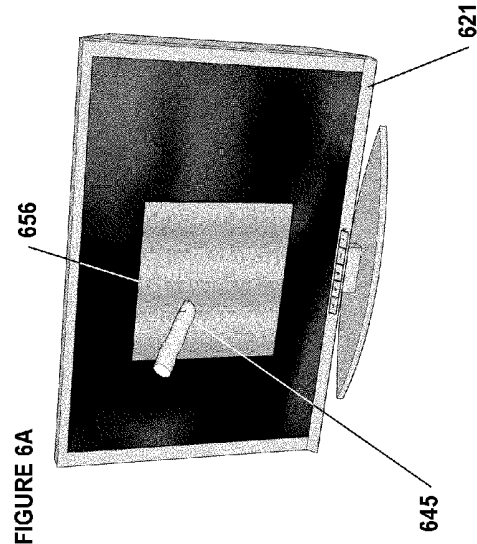
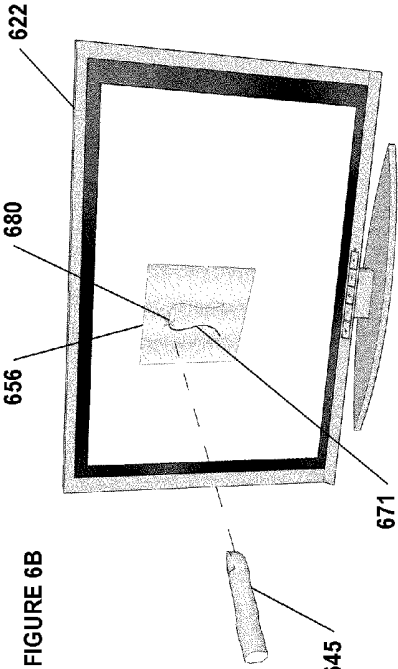


FIGURE 2B









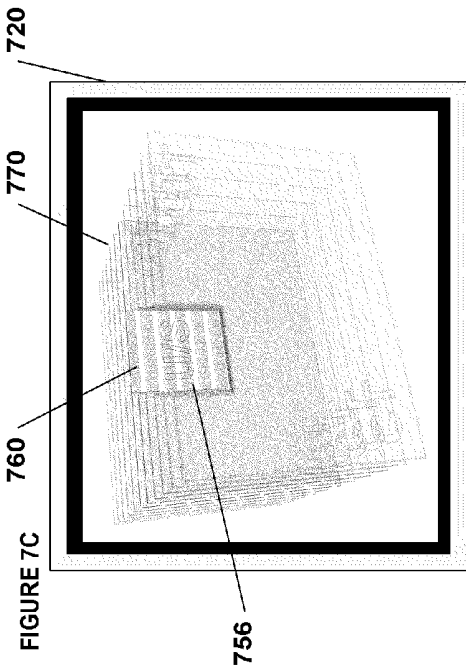
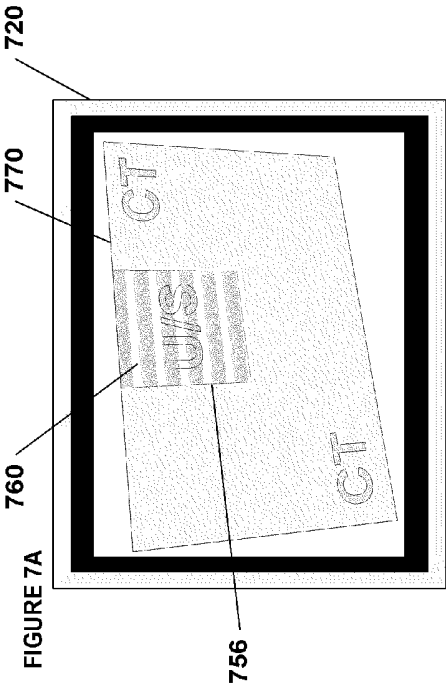
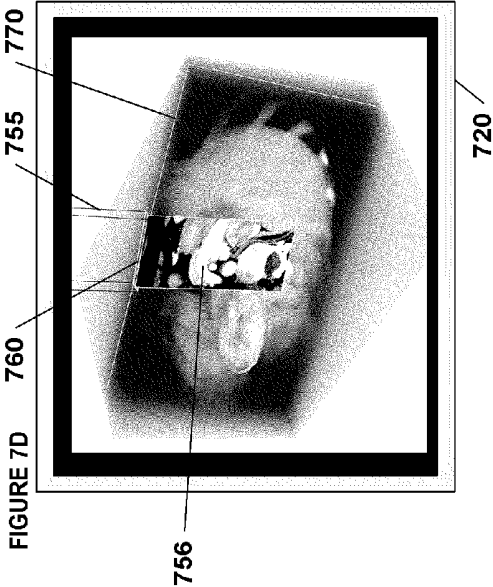
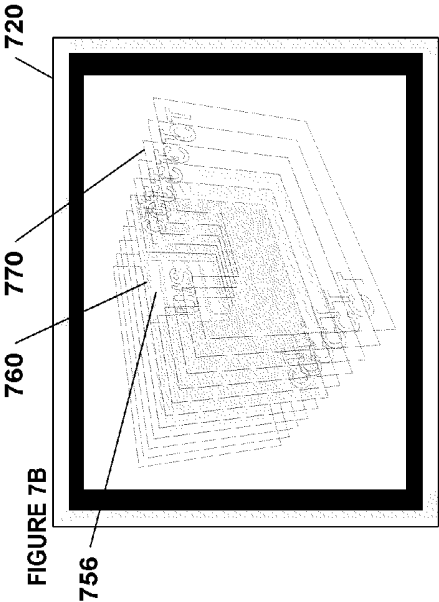


IMAGE ANNOTATION IN IMAGE-GUIDED MEDICAL PROCEDURES

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. application Ser. No. 13/014,596, which claims benefit to U.S. Provisional Patent Application No. 61/322,991 filed Apr. 12, 2010, and U.S. Provisional Patent Application No. 61/387,132, filed Sep. 28, 2010. Each of the provisional applications, 61/322,991 and 61/387,132 is incorporated by reference herein in its entirety for all purposes.

FIELD

[0002] The embodiments herein disclosed relate to computer-assisted medical procedures and more specifically to image annotation in image-guided medical procedures.

BACKGROUND

[0003] The past few decades have seen incredible developments of technology and systems for computer-assisted, image-based, and image-guided surgery and other medical procedures. These advances in image-guided surgery are tied in part to technical and scientific improvements in imaging and three-dimensional (3D) computer graphics. For example, some of the early work of in this field in the late 1980's provided new 3D graphics rendering techniques, medical image shape detection, and head-mounted displays. These are some of the building blocks of later image-guided surgery systems developed in the mid-1990's and thereafter. Image-guided surgery makes use of imaging to aid a surgeon in performing more effective and more accurate surgeries.

[0004] Current image-guided surgery systems, however, do not provide adequate mechanisms to annotate images. The process of annotation is difficult and extremely time-consuming. Further, it would be difficult, disruptive, and time consuming for a surgeon or other operator to annotate an image during a medical procedure.

[0005] One or more of these problems and others are addressed by the systems, methods, devices, computer-readable media, techniques, and embodiments described herein. That is, some of the embodiments described herein may address one or more issues, while other embodiments may address different issues.

SUMMARY

[0006] Presented herein are methods, systems, devices, and computer-readable media for image annotation in image-guided medical procedures. In some embodiments, pose information is determined for visualizable medical data and changing pose information is determined for a medical device over time. An annotation in 3D space may be generated based on the pose information over time for the medical device and the pose information for the visualizable medical data; and image guidance information may be generated based at least in part on the annotation in 3D space. A graphical rendering of the image guidance information may be displayed on one or more displays.

[0007] In some embodiments, a system may determine device type information for a first medical device; real-time emplacement information for the first medical device; and real-time emplacement information for a second medical device. The system may also determine the real-time relative

emplacements of the first and second medical devices with the computer system and real-time prediction information for the first medical device. The image guidance system may then generate image guidance information based on the real-time relative emplacements of the first and second medical devices, the real-time prediction information for the first medical device, and data related to the second medical device. A graphical rendering of the image guidance information may be displayed on one or more displays. It is possible that determining changing pose information for the medical device over time include determining the changing pose information for the medical device over time relative to a 2D screen displaying the visualizable medical data; and/or generating the annotation in 3D space based on the pose information over time for the medical device and the pose information for the visualizable medical data may include determining the annotation in 3D space based at least in part on the 2D pose information.

[0008] Numerous other embodiments are described throughout herein. Although various embodiments are described herein, it is to be understood that not necessarily all objects, advantages, features or concepts need to be achieved in accordance with any particular embodiment. Thus, for example, those skilled in the art will recognize that the invention may be embodied or carried out in a manner that achieves or optimizes one advantage or group of advantages as taught or suggested herein without necessarily achieving other objects or advantages as may be taught or suggested herein.

[0009] All of these embodiments are intended to be within the scope of the invention herein disclosed. These and other embodiments will become readily apparent to those skilled in the art from the following detailed description having reference to the attached figures, the invention not being limited to any particular disclosed embodiment(s).

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] FIGS. 1A-1D illustrate four example interfaces for image annotation in image-guided medical procedures.

[0011] FIGS. 2A and 2B illustrate example systems for image annotation in image-guided medical procedures.

[0012] FIG. 3 is a flow diagram that illustrates an example method for image annotation in image-guided medical procedures.

[0013] FIG. 4 illustrates a fifth example interface for image annotation in image-guided medical procedures.

[0014] FIG. 5 illustrates a sixth example interface for image annotation in image-guided medical procedures.

[0015] FIGS. 6A-6C illustrate three additional example interfaces for image annotation in image-guided medical procedures.

[0016] FIGS. 7A-7D illustrates a tenth example interface for image annotation in image-guided medical procedures.

DETAILED DESCRIPTION

Overview

[0017] In some embodiments herein, an operator, surgeon or other medical practitioner may annotate images during an image-guided medical procedure. In some embodiments, the operator may use medical devices that are typically present during the medical procedure to annotation the medical images. As depicted in FIGS. 2A and 2B, and as described more below, an operator, such as a surgeon or other medical

practitioner, may use a first medical device **245** (e.g., an ablation needle) and a second medical device **255** (e.g., an ultrasound transducer) during a medical procedure and one or both of these medical devices **245** and **255** may be used for image annotation.

[0018] FIGS. 1A-1D illustrate examples of image annotation in image-guided medical procedures. FIGS. 1A-1D show a representation on a computer screen **120** of an annotation being made with a medical device (represented on the display **120** as medical device **145**). The medical device may be used to annotate an image **156**. FIG. 1A illustrates the manipulation of a needle **145** pointing at an image **156** (e.g., an ultrasound image **156**). The operator can make an annotation by moving the needle **145** through space in order to draw curve **171** on image **156**. Arrow **174** may indicate the direction that the operator plans to or will draw in the future. In some embodiments, arrow **174** is not displayed. Indicator **180** may represent the place on image **156** currently pointed to by needle **145**. Indicator **180** may be any appropriate indicator such as an "X," an arrow, a differently-colored area, etc. In FIG. 1B the operator has further moved needle **145** in order to complete the annotation **171** on image **156**. As is depicted in FIG. 1B, the indicator **180** of the intersection between the axis of the needle **145** and the image **156** has now reached the lower-right quadrant of the image **156**.

[0019] The image **156** may be associated with a medical device, such as an ultrasound transducer (not pictured in FIGS. 1A-1D). The image **156** may be an ultrasound image **156**, or the image **156** may be a slice or image from other 3D visualizable medical data such as is described in Image Management in Image-Guided Medical Procedures, to Sharif Razzaque et al., filed concurrently herewith, which is incorporated by reference for all purposes.

[0020] The annotation **171**, although it has been drawn on an image **156**, may actually be located in 3D space-defined by the placement of the image **156** and the annotation **171**. FIG. 1C depicts image **156**, associated with the ultrasound transducer turned or rotated about its vertical axis (axis not depicted in FIG. 1C). Therefore, part of the annotation **171** is depicted in front of the image **156**, and part of the annotation **173** is behind the image **156**, thus illustrating the existence in 3D space of the annotation **171/173**. The location and display of annotations in 3D space will allow an operator to make an annotation for a feature (e.g., a tumor, cyst, or vein), and allow her to locate that feature again later.

[0021] FIG. 1D illustrates that an operator may make a second annotation **172** on the image **156**. Part of the first annotation **171** is in front of the image **156** and part **173** is behind. By manipulating the pose of the image **156** (by manipulating the ultrasound transducer), the operator can choose new locations within 3D space for annotations. As noted above, the annotations may be for a blood vessel, tumor, or any other object or location of interest for the operator. There need not even be a particular object in the medical image that the operator is annotating. The operator may, for example, sign her name or write a note. For example, an operator may circle or make marks near multiple tumors, trace a line such as annotation **171** along a vein or artery, etc. In some embodiments, if the operator moves image **156** during annotation, the operator may make non-planar annotation (see, e.g., FIGS. 4 and 5). As such, the operator may be able to make a sphere or other non-planar annotation in order to

annotate the volumetric aspects of a feature of interest. For example, the operator may draw the outline of a sphere around a tumor or cyst.

[0022] Using embodiments described herein, a radiologist or other practitioner is not limited to marking tumors or other anatomical references on individual slices of CT scans. Instead, the radiologist may move in an intuitive manner through the CT scan. Further, various embodiments may decrease the time it takes to annotate an image, and/or to display those annotations, during a medical procedure, thereby reducing cost.

[0023] By allowing multiple annotations and by enabling the operator to place annotations in 3D space, various embodiments herein allow the operator to mark multiple objects of interest and view the location of those marks of interest at a later time. The annotations may be displayed using any display technique, such as those described in Image Management in Image-Guided Medical Procedures, to Sharif Razzaque et al., filed concurrently herewith and incorporated by reference above for all purposes.

[0024] Images may be annotated using embodiments herein during all a portion of a medical procedure. In one embodiment, the image annotation will only occur during an image annotation "session" (e.g. a period of time during which image annotation is performed, and before and after which, image annotation is not performed). An image annotation "session" may be initiated and/or terminated by the operator performing a key stroke, issuing a command (such as a verbal command), performing a gesture with a medical device or hand, pressing a button on the medical device, pressing a foot pedal, pressing a button on the medical device (e.g., a button on a Wacom pen), etc.

[0025] As used herein, the term "medical device" is a broad term that encompasses but is not limited to a device, item, or part used in the medical procedure. For example, a medical device could include an ablation needle, an ultrasound transducer, a cauterizer, a scalpel, a glove covering an operator's hand, the operator's hand or finger, etc. The medical device used for pose information could even be the operator's head, eyes, or gaze direction. Pose information for the medical device may be obtained using any system, device, method, or technique, such as those disclosed herein.

Example Systems

[0026] FIG. 2A illustrates a first exemplary system for image management in image guided surgery. FIG. 2B illustrates a second exemplary system for image management in image guided surgery. In many respects, the embodiments illustrated by FIGS. 2A and 2B are similar and use similar numbering. Where the two are different, those differences are noted. The differences between the two figures may include that, in FIG. 2A, two position sensing units **210** and **240** are shown, whereas in FIG. 2B, only a single position sensing unit **210** is shown.

[0027] In one embodiment, position sensing units **210** and **240** may be tracking systems **210** and **240** and may track surgical instruments **245** and **255** and provide data to the image guidance unit **230**. The image guidance unit **230** may process or combine the data and show image guidance data on display **220**. This image guidance data may be used by a physician to guide a procedure and improve care. There are numerous other possible embodiments of system **200**. For example, many of the depicted modules may be joined together to form a single module and may even be imple-

mented in a single computer or machine. Further, position sensing units 210 and 240 may be combined and track all relevant surgical instruments 245 and 255, as discussed in more detail below and exemplified in FIG. 2B. Additional imaging units 250 may be included and combined imaging data from the multiple imaging units 250 may be processed by image guidance unit 230 and shown on display unit 220. Additionally, two or more surgical systems 249 may also be included.

[0028] Information about and from multiple surgical systems 249 and/or attached surgical instruments 245 may be processed by image guidance unit 230 and shown on display 220. These and other possible embodiments are discussed in more detail below. Imaging unit 250 may be coupled to image guidance unit 230. In one embodiment, imaging unit 250 may be coupled to a second display unit 251. The second display unit 251 may display imaging data from imaging unit 250. The imaging data displayed on display unit 220 and displayed on second display unit 251 may be, but are not necessarily, the same. In an embodiment, the imaging unit 250 is an ultrasound machine 250, the movable imaging device 255 is an ultrasound transducer 255 or ultrasound 255, and the second display unit 251 is a display associated with the ultrasound machine 250 that displays the ultrasound images from the ultrasound machine 250. In one embodiment, a movable imaging unit 255 may not be connected directly to an imaging unit 250, but may instead be connected to image guidance unit 230. The movable imaging unit 255 may be useful for allowing a user to indicate what portions of a first set of imaging data should be displayed. For example, the movable imaging unit 255 may be an ultrasound transducer 255 or a tracked operative needle or other device 255, for example, and may be used by a user to indicate what portions of imaging data, such as a pre-operative CT scan, to show on a display unit 220 as image 225. Further, in some embodiments, there could be a third set of pre-operative imaging data that could be displayed with the first set of imaging data.

[0029] In some embodiments, system 200 comprises a first position sensing unit 210, a display unit 220, and second position sensing unit 240 (if it is included) all coupled to image guidance unit 230. In one embodiment, first position sensing unit 210, display unit 220, and image guidance unit 230 are all physically connected to stand 270. Image guidance unit 230 may be used to produce images 225 that are displayed on display unit 220. The images 225 produced on display unit 220 by the image guidance unit 230 may be determined based on ultrasound or other visual images from first surgical instrument 245 and second surgical instrument 255. For example, if first surgical instrument 245 is an ablation needle 245 and second surgical instrument 255 is an ultrasound probe 255, then images 225 produced on display 220 may include the video or images from the ultrasound probe 255 combined with graphics, such as projected needle drive or projected ablation volume, determined based on the pose of ablation needle 245. If first surgical instrument 245 is an ultrasound probe 245 and second surgical instrument 255 is a laparoscopic camera 255, then images 225 produced on display 220 may include the video from the laparoscopic camera 255 combined with ultrasound data superimposed on the laparoscopic image. More surgical instrument may be added to the system. For example, the system may include an ultrasound probe, ablation needle, laparoscopic camera, cauterizer, scalpel and/or any other surgical instrument or medical device. The system may also process and/or display pre-

viously collected data, such as preoperative CT scans, X-Rays, MRIs, laser scanned 3D surfaces etc.

[0030] The term “pose” as used herein is a broad term encompassing its plain and ordinary meaning and may refer to, without limitation, emplacement, position, orientation, the combination of position and orientation, or any other appropriate location information. In some embodiments, the imaging data obtained from one or both of surgical instruments 245 and 255 may include other modalities such as a CT scan, MRI, open-magnet MRI, optical coherence tomography, positron emission tomography (“PET”) scans, fluoroscopy, ultrasound, or other preoperative, or intraoperative 2D or 3D anatomical imaging data. In some embodiments, surgical instruments 245 and 255 may also be scalpels, implantable hardware, or any other device used in surgery. Any appropriate surgical system 249 or imaging unit 250 may be coupled to the corresponding medical instruments 245 and 255.

[0031] As noted above, images 225 produced may also be generated based on live, intraoperative, or real-time data obtained using second surgical instrument 255, which is coupled to second imaging unit 250. The term “real-time” as used herein is a broad term and has its ordinary and customary meaning, including without limitation instantaneously or nearly instantaneously. The use of the term realtime may also mean that actions are performed or data is obtained with the intention to be used immediately, upon the next cycle of a system or control loop, or any other appropriate meaning. Additionally, as used herein, real-time data may be data that is obtained at a frequency that would allow a surgeon to meaningfully interact with the data during surgery. For example, in some embodiments, real-time data may be a medical image of a patient that is updated one time per second or multiple times per second.

[0032] Second surgical instrument 255 may be coupled to second position sensing unit 240. Second position sensing unit 240 may be part of imaging unit 250 or it may be separate. Second position sensing unit 240 may be used to determine the pose of second surgical instrument 255. In some embodiments, first and/or second position sensing units 210 and/or 240 may be magnetic trackers and magnetic may be coils coupled to surgical instruments 245 and/or 255. In some embodiments, first and/or second position sensing units 210 and/or 240 may be optical trackers and visually-detectable fiducials may be coupled to surgical instruments 245 and/or 255.

[0033] Images 225 may be produced based on intraoperative or real-time data obtained using first surgical instrument 245, which is coupled to first surgical system 249. In FIGS. 2A and 2B, first surgical system 249 is shown as coupled to image guidance unit 230. The coupling between the first surgical system 249 and image guidance unit 230 may not be present in all embodiments. In some embodiments, the coupling between first surgical system 249 and image guidance unit 230 may be included where information about first surgical instrument 245 available to first surgical system 249 is useful for the processing performed by image guidance unit 230. For example, in some embodiments, first surgical instrument 245 is an ablation needle 245 and first surgical system 249 is an ablation system 249. In some embodiments, it may be useful to send a signal about the relative strength of planned ablation from ablation system 249 to image guidance unit 230 in order that image guidance unit 230 can show a predicted ablation volume. In other embodiments, first surgical system 249 may not be coupled to image guidance unit

230. Example embodiments including images and graphics that may be displayed are included below.

[0034] In an embodiment, first position sensing unit **210** tracks the pose of first surgical device **245**. First position sensing unit **210** may be an optical tracker **210** and first surgical device **245** may have optical fiducials attached thereto. The pose of optical fiducials may be detected by first position sensing unit **210**, and, therefrom, the pose of first surgical device **245** may be determined.

[0035] In various embodiments, as depicted in FIG. 2B, a single position sensing unit **210** may track both first medical device **245** and second medical device **255**. In FIG. 2B, in some embodiments, position sensing unit **210** is a magnetic tracker and is mounted below a surgical table **280**. Such an arrangement may be useful when the tracking volume of the position sensing unit **210** is dependent on the location of the position sensing unit, as with many magnetic trackers. Magnetic tracking coils may be mounted in or on the medical devices **245** and **255**.

[0036] In some embodiments, either or both of the first position sensing unit **210** and the second position sensing unit **240** may be an Ascension Flock of Birds, Nest of Birds, driveBAY, medSAFE, trakSTAR, miniBIRD, MotionSTAR, pciBIRD, or Calypso 4D Localization System and tracking units attached to the first and/or second surgical or medical devices **245** and **255** may be magnetic tracking coils. The term “tracking unit,” as used herein, is a broad term encompassing its plain and ordinary meaning and includes without limitation all types of magnetic coils or other magnetic field sensing devices for use with magnetic trackers, fiducials or other optically detectable markers for use with optical trackers, such as those discussed above and below. Tracking units could also include optical position sensing devices such as the HiBall tracking system and the first and second position sensing units **210** and **240** may be part of a HiBall tracking systems. Tracking units may also include a GPS device or signal emitting device that would allow for tracking of the position and, optionally, orientation of the tracking unit. In some embodiments, a signal emitting device might include a radio-frequency identifier (RFID). In such embodiments, the first and/or second position sensing unit **210** and **240** may take in the GPS coordinates of the tracking units or may, for example, triangulate the radio frequency signal being emitted by the RFID associated with tracking units. The tracking systems may also include one or more 3D mice.

[0037] In some embodiments, either or both of the first position sensing unit **210** and the second position sensing unit **240** may be an Aurora® Electromagnetic Measurement System using sensor coils for tracking units attached to the first and/or second surgical devices **245** and **255**. In some embodiments, either or both of the first position sensing unit **210** and the second position sensing unit **240** may also be an optical 3D tracking system using fiducials. Such optical 3D tracking systems may include the NDI Polaris Spectra, Vicra, Certus, PhaseSpace IMPULSE, Vicon MX, InterSense IS-900, NaturalPoint OptiTrack, Polhemus FastTrak, IsoTrak, or Claron MicronTracker2. In some embodiments, either or both of position sensing units **210** and **240** may each be an inertial 3D tracking system comprising a compass, accelerometer, tilt sensor and/or gyro, such as the InterSense InertiaCube or the Wii controller. In some embodiments, either or both of position sensing units **210** and **240** may be attached to or affixed on the corresponding surgical device **245** and **255**. In some embodiments, the position sensing units, **210** and **240**, may

include sensing devices such as the HiBall tracking system, a GPS device, or signal emitting device that would allow for tracking of the position and, optionally, orientation of the tracking unit. In some embodiments, a position sensing unit **210** or **240** may be affixed to either or both of the surgical devices **245** and **255**. The surgical devices **245** or **255** may be tracked by the position sensing units **210** or **240**. A world reference, such as the display **220** may also be tracked by the position sensing unit **210** or **240** in order to determine the poses of the surgical devices **245** and **255** with respect to the world. Devices **245** and **255** may also include or have coupled thereto one or more accelerometers, which may be used to estimate movement, position, and location of the devices.

[0038] In an embodiment, the display unit **220** displays 3D images to a user, such as a physician. Stereoscopic 3D displays separate the imagery shown to each of the user's eyes. This can be accomplished by a stereoscopic display, a lenticular auto-stereoscopic display, or any other appropriate type of display. The display **220** may be an alternating row or alternating column display. Example alternating row displays include the Miracube G240S, as well as Zalman Trimon Monitors. Alternating column displays include devices manufactured by Sharp, as well as many “auto-stereoscopic” displays (e.g., Philips). Display **220** may also be a cathode ray tube. Cathode Ray Tube (CRT) based devices, may use temporal sequencing, showing imagery for the left and right eye in temporal sequential alternation; this method may also be used by newer, projection-based devices, as well as by 120-Hz-switchable liquid crystal display (LCD) devices.

[0039] In one embodiment, a user may wear a head mounted display in order to receive 3D images from the image guidance unit **230**. In such embodiments, a separate display, such as the pictured display unit **220**, may be omitted. The 3D graphics may be produced using underlying data models, stored in the image guidance unit **230** and projected onto one or more 2D planes in order to create left and right eye images for a head mount, lenticular, or other 3D display. The underlying 3D model may be updated based on the relative poses of the various devices **245** and **255**, as determined by the position sensing unit(s), and/or based on new data associated with the devices **245** and **255**. For example, if the second device is an ultrasound probe **255**, then the underlying data model may be updated to reflect the most recent ultrasound image. If the first device **245** is an ablation needle, then the underlying model may be updated to reflect any changes related to the needle, such as power or duration information. Any appropriate 3D graphics processing may be used for rendering including processing based on OpenGL, Direct3D, Java 3D, etc. Whole, partial, or modified 3D graphics packages may also be used, such packages including 3DS Max, SolidWorks, Maya, Form Z, Cybermotion 3D, VTK, Slicer, or any others. In some embodiments, various parts of the needed rendering may occur on traditional or specialized graphics hardware. The rendering may also occur on the general CPU, on programmable hardware, on a separate processor, be distributed over multiple processors, over multiple dedicated graphics cards, or using any other appropriate combination of hardware or technique.

[0040] One or more modules, units, devices, or elements of various embodiments may be packaged and/or distributed as part of a kit. For example, in one embodiment, an ablation needle, tracking elements, 3D viewing glasses, and/or a portion of an ultrasound wand may form a kit. Other embodiments may have different elements or combinations of ele-

ments grouped and/or packaged together. Kits may be sold or distributed separately from or with the other portions of the system.

[0041] There are numerous other examples of image guidance systems which may use, incorporate, support, or provide for the techniques, methods, processes, and systems described herein, such as the 3D computer-graphics-based assigned to InnerOptic Technologies, Inc. that provides for displaying guidance data from multiple sources, U.S. application Ser. No. 11/833,134, filed Aug. 2, 2007, the contents of which are incorporated by reference herein in their entirety for all purposes. The image guidance may also be performed at least in part using the techniques described in U.S. patent application Ser. No. 11/828,826, filed 7/26/2007, U.S. Pat. No. 7,728,868, U.S. patent application Ser. No. 12/299,899, U.S. patent application Ser. No. 12/483,099, U.S. patent application Ser. No. 12/893,123, U.S. patent application Ser. No. 12/842,261, and/or U.S. patent application Ser. No. 12/703,118, each of which is incorporated by reference herein in its entirety for all purposes.

Methods for Image Annotation in Image-Guided Medical Procedures

[0042] FIG. 3 depicts a method 300 for image annotation in image-guided medical procedures. As just one example embodiment, pose information for an ultrasound transducer and its associated ultrasound image may be determined in block 310. In block 320, changing pose information for an ablation needle may be determined in block 320. The pose information may change as an operator moves the ablation needle and/or the ultrasound transducer. An annotation may be generated in block 330 based on, for example, the intersection of an axis of the ablation needle and the ultrasound image plane. Image guidance information may be generated in block 340 based on the annotation in 3D space (and include, e.g., the annotation, the ultrasound image, a depiction of the ablation needle, and/or other imaging or guidance information). In block 350, the image guidance information may be displayed.

[0043] In block 310, pose information for visualizable medical data is determined. “Visualizable medical data” is a broad term that encompasses its ordinary and customary meaning and includes, without limitation, any two-dimensional (2D) or 3D medical data that can be visualized. The visualizable medical data may also be volumetric and can include, without limitation, one or more of a CT scan, an MRI, other 3D preoperative imaging data, other volume data, segmented internal organs, segmented blood vessels, annotations, tumors, etc. The visualizable medical data may also include 2D medical data such as ultrasounds, X-rays, or segments or slices of 3D medical data.

[0044] In some embodiments, the visualizable medical data may be associated with a medical device, such as an ultrasound probe, etc., and the medical device may be tracked in the medical scene. In such embodiments, the pose information for the visualizable medical data may be determined in block 310 from the pose of the associated medical device (that is tracked in the medical scene). For example, if the visualizable medical data is associated with an ultrasound probe and the ultrasound probe is tracked, then the pose of the visualizable medical data can be determined from the pose of the ultrasound probe. This can be the case even if the visualizable medical data is not generated by the medical device. For example, if the medical device is an ultrasound transducer and

the visualizable medical data is a slice or image from a CT scan that is being navigated using the ultrasound transducer (see, for example, Image Management in Image-Guided Medical Procedures, to Sharif Razzaque et al., filed concurrently herewith, which is incorporated by reference above for all purposes) then the pose for that slice or image from the CT scan can still be determined based on the pose of the medical device.

[0045] When navigating/visualizing CT or other volumetric data with a medical device such as an ultrasound transducer, pose information for the medical device may be updated over time. Pose information for the underlying volumetric visualizable medical data set may also be determined (e.g., relative to the medical scene). The pose information for the underlying volumetric visualizable medical data (e.g., a CT scan or other volumetric data) may be determined separately from the pose information of the medical device used to visualize the medical data. Further, in some embodiments, the pose information for the visualizable medical data may initially be determined in order to register or approximately register the 3D visualizable medical data with the medical scene being visualized for the operator. Various techniques for registering the visualizable medical data with the medical scene may be used, including matching features in 3D space with features in the visualizable medical data known to be in the medical scene, such as tumors, bones, blood vessels, etc. Manual registration may also be possible where an operator or other technician manipulates the pose of the visualizable medical data relative to the scene.

[0046] In block 320, changing pose information is determined for a medical device. The medical device for which pose information is determined in block 320 may be different from a medical device used for visualization of data in block 310.

[0047] Returning again to block 320, pose information for the medical device may be determined using any system, device, method, or technique such as the tracking systems described herein. For example, if the medical device is an ablation needle, such as ablation needle 245 in FIGS. 2A and 2B, then determining the pose information for the ablation needle 245 may include receiving tracking information from one or more position sensors sensing the position of ablation needle 245.

[0048] As depicted in FIGS. 6A-6C, pose information for the medical device may be determined in other ways as well. For example, as shown in FIG. 6A, a display 621 may have a touchscreen that allows an operator to use her finger 645 as the medical device 645 to indicate the location of an annotation. The visualizable medical data 656 may be shown on display 621. As the operator moves her finger 645, an annotation may appear on display 621 (not pictured in FIG. 6A) or on a separate display of the image 656, as depicted in FIG. 6C. In FIG. 6C, we see an annotation 671 that has been drawn by an operator up to point 680. This annotation 671 is positioned on image 656 and both are displayed on display 620. An operator may have dual displays 621 and 620 and be able to see both simultaneously.

[0049] The medical device 645 used to point to an object on a screen may also be a stylus, needle, or any other appropriate medical device 645. Further, in some embodiments, the device used for input may not be a screen 621, but may instead be a drawing tablet, or other input device (in which case image 656 may or may not be displayed on the device).

[0050] In some embodiments, a medical device, such as finger 645 in FIG. 6B, may be used to point at an image 656 displayed on a display 622. An operator may be able to point medical device 645 at the image 656 in order to define an annotation 671 up to a point 680. Pointing with medical device 645 at display 622 may define an intersection between medical device 645 and image 656. That intersection may define the point 680 that is used to define or generate the annotation 671. The medical device 645 used to point at the screen may also be a remote (such as a Nintendo Wii controller), a surgical instrument, such as an ablation needle or scalpel, eye gaze or head direction, or any other appropriate medical device.

[0051] Returning again to FIG. 3 and block 320, as pose information changes over time (e.g., because the medical device is being moved), such as described above with respect to FIGS. 1A-1D, the changing pose information for the medical device over time is determined. In one embodiment, changing pose information is collected before proceeding to block 330. In another embodiment, the changing pose information for the medical device is collected iteratively and blocks 330-350 are performed as part of those iterations. Further, in some embodiments, pose information for the visualizable medical data, changing pose information for the medical device, and the other blocks are performed iteratively. In yet other embodiments, pose information in block 310 for the visualizable medical data and changing pose information for the medical device in block 320 are updated within the system as the updated pose information is received and this latest pose information is used in subsequent blocks 330-350.

[0052] In block 330, annotations are generated in 3D space based on the pose information received in blocks 310 and 320. That is, the pose for the visualizable medical data (block 310) and the pose for the medical device (block 320) may be used to determine the annotations in 3D space (block 330). Referring again to FIGS. 1A-1D, needle 145 and/or image 156 may have their poses change over time. The needle 145 and the image 156 may together define a point or mark 180 that changes over time as the poses of device 145 and image 156 change. That is, if point 180 is defined by an axis extending out of the tip of needle 145 and its intersection with the plane of the image 156, then as the needle 145 moves and/or the image 156 moves, the point 180 will change. As point 180 changes over time, it defines a curve, spline, segmented line, or other annotation that the operator is making. The annotations defined by these one or more movements is shown in FIG. 1B as annotation 171.

[0053] FIG. 4 depicts a medical device 446 and an image 456 that together define an intersection point 480. The curve 474 shows a motion that an operator is going to make (curve 474 may or may not be displayed on display 420). As depicted in FIG. 5, after the operator has moved the medical device 546 through part of the desired curve of movement 574, an annotation 571 is created by the movement of intersection point 580. In this case, both device 546 and image 556 have been moved so annotation 571 is not planar. Instead, annotation 571 is a three-dimensional surface. The movement of image 556 is also illustrated by the outline 557 of the image's original placement at the start of the annotation (outline 557 may or may not be displayed on display 520)-and by arrow 558. As discussed briefly above, the annotation determined may be a spline, a series of lines, a series of triangles, a point cloud, a series of voxels, or any other appropriate representation in 3D

space. The generated annotation may also be termed or thought of as "virtual ink." In some embodiments, the annotation may be termed "virtual ink" when it corresponds to the drawing of ink on the image plane as the drawing instrument and image plane move.

[0054] After an annotation has been created in 3D space in block 330 then in block 340 image guidance information is generated based on the annotation. Generating image guidance information based on the annotation in block 330 may include generating a 3D model or series of 3D models that represent the medical scene to be displayed to the operator. For example, as depicted in FIG. 1D, after a first annotation 171/173 is defined and a second annotation 172 is defined, generating image guidance data may include registering in the same 3D space, or determining transformations among, the various annotations 171-173 and the image 156. If the image 156 is, for example, a planar representation of 3D visualizable medical data, such as a CT scan, then determining the guidance information in block 340 may include incorporating a planar slice of the CT data corresponding to the image 156. Further, determining image guidance information may include numerous other techniques, methods, and systems, such as those described in Image Management in Image-Guided Medical Procedures, to Sharif Razzaque et al., filed concurrently herewith, which is incorporated by reference above for all purposes.

[0055] After image guidance information has been generated based on the annotation in block 340, a graphical rendering of the image guidance information is displayed in block 350. In some embodiments, the display of graphical information can be monoscopic or stereoscopic. Further, multiple rendering techniques may be used. Edges or areas near the edge of a region of interest defined by the annotation, a medical device, or the image, may be displayed in a blurred or fading manner. Objects near objects of interest such as the image, the annotation, or the medical device may be displayed in sharper focus, may be displayed brighter, etc. In one embodiment, if an additional set of 3D visualizable medical data is displayed, a tunnel or cut-through that set of medical data may be made so that an image can be shown. Consider for example, FIG. 6B. If another set of 3D data is being displayed on display 622 (not depicted in FIG. 6B), then the additional data may have a cut-through so that image 656 can be seen and the areas surrounding image 656 on display 622 may show the additional visualizable medical data. Turning to FIG. 1B, it is possible that medical device 145 and/or image 156 may define a region of interest and items in that region of interest may be displayed distinctly from the rest of the data displayed on screen 120. For example, if additional medical data is being displayed, then data from that additional medical display may be displayed within a region of interest around image 156 and/or medical device 145.

[0056] Turning to FIG. 7A, in some embodiments, a medical device may define a region of interest 760 in which an ultrasound image 756 may be shown in focus. Outside the region of interest 760, the CT scan 770 may be displayed. As depicted in FIG. 7A, a single slice of CT data 770 may be displayed outside the region of interest 760, or, as depicted in FIG. 7B, multiple slices of CT data 770 may be displayed outside the region of interest. Further, as depicted in FIG. 7C, the slices of CT data may be rendered differently depending on the distance from the region of interest. For example, planes of CT scan data 770 may be rendered more transparently (less brightly, etc) the further each is from the plane

containing the region of interest. The slices of CT data may be the slices from the underlying CT data, or the slices may be generated to be, e.g., parallel or nearly parallel, with a plane associated with the region of interest **760**. FIG. **7C** also depicts that a tunnel may be cut through the rendered slices of the CT scan **770** in order to display the region of interest **760** without or with little overlap. This tunnel may be altered as the region of interest or CT scan data are moved to always allow the operator to view the region of interest. FIG. **7D** depicts a semi-realistic rendering of a CT scan **770** around a region of interest **760**. Inside the region of interest **760**, an ultrasound image **756** is displayed. Also displayed on display **720** in FIG. **7D**, is an outline of the medical device **755**.

[0057] As noted extensively herein, the data shown in the region of interest may be any appropriate visualizable medical data, not limited to ultrasound or CT data. Further, the data displayed outside of the region of interest may be any visualizable medical data, and may even be from the same data set as the data shown in the region of interest. For example, MRI data may be shown in fading planes outside of the region of interest and in focus (and visualizable through a tunnel) inside the region of interest. Further, annotation may be displayed along with the rendering of the visualizable medical data inside and/or outside of the region of interest. In this manner, an operator may see the annotations in the context of the visualizable medical data.

[0058] In rendering the annotation, each point of the line segment, spline segment, point cloud, etc. may be made transparent and/or blurry based on its distance from the region of interest, and its rendering may be controlled using various graphic techniques, such as bit maps and pixel shaders, such as those discussed in Image Management in Image-Guided Medical Procedures, to Sharif Razzaque et al., filed concurrently herewith, which is incorporated by reference above for all purposes.

[0059] The blocks of process **300** may be performed in a different order, may be augmented by other blocks or may have sub-blocks within the blocks shown. Further, the process **300** may be performed on a single computer or processor, on multiple computers or processors, on a single or multiple virtual machines, and/or in a distributed fashion on multiple processors, devices, machines, or virtual machines.

Example Procedure

[0060] Consider an example ablation procedure. Lesions, which are often less than 3 cm in width, are typical targets of ablation. A physician may be able to see the lesions in a CT scan more clearly than she can in an ultrasound image. The physician may mark the lesions with annotations by navigating around the CT scan data using the techniques herein and various techniques in Image Management in Image-Guided Medical Procedures, to Sharif Razzaque et al., filed concurrently herewith, which is incorporated by reference above for all purposes.

[0061] That is, the physician may manipulate a medical device, such as an ultrasound transducer, in order to navigate and view CT data preoperatively (or intraoperatively). The physician may be able to see the small lesions in the CT data. The physician can then annotate those lesions, perhaps by circling, creating a sphere around them, and/or drawing an arrow pointing to them, using annotation the techniques herein.

[0062] Intraoperatively, the physician may be able to leverage the preoperative lesion annotation. The physician may

use intraoperative ultrasound in order to spot the current location of the various lesions, guided at least in part by the annotation made in 3D space relative to the CT scan. By doing this, the physician has utilized both the relative ease of discovery of lesions on the CT scan as well as the intraoperative accuracy of locating the lesions in the ultrasound. This can increase accuracy and reduce operative times and the problems and costs associated therewith.

[0063] Although an example of an ablation is given, these techniques may be used with numerous other procedures, such as laparoscopic, endoscopic, arthroscopic, robotic and percutaneous procedures, resections, tissue transplantation, training, diagnostic, as well as drug delivery procedures, etc.

Other Embodiments

[0064] The processes, computer readable medium, and systems described herein may be performed on various types of hardware, such as computer systems or computing devices. In some embodiments, position sensing units **210** and **240**, display unit **220**, image guidance unit **230**, and/or any other module or unit of embodiments herein may each be separate computing devices, applications, or processes or may run as part of the same computing devices, applications, or processes-or one of more may be combined to run as part of one application or process-and/or each or one or more may be part of or run on a computing device. Computing devices or computer systems may include a bus or other communication mechanism for communicating information, and a processor coupled with the bus for processing information. A computer system or device may have a main memory, such as a random access memory or other dynamic storage device, coupled to the bus. The main memory may be used to store instructions and temporary variables. The computer system or device may also include a read-only memory or other static storage device coupled to the bus for storing static information and instructions. The computer systems or devices may also be coupled to a display, such as a CRT, LCD monitor, LED array, e-paper, projector, or stereoscopic display. Input devices may also be coupled to the computer system or device. These input devices may include a mouse, a trackball, touchscreen, tablet, foot pedal, or cursor direction keys. Computer systems or devices described herein may include the image guidance unit **230**, first and second position sensing units **210** and **240**, and imaging unit **250**.

[0065] Each computer system or computing device may be implemented using one or more physical computers, processors, embedded devices, field programmable gate arrays (FPGAs), or computer systems or portions thereof. The instructions executed by the computer system or computing device may also be read in from a computer-readable medium. The computer-readable medium may be non-transitory, such as a CD, DVD, optical or magnetic disk, laserdisc, flash memory, or any other medium that is readable by the computer system or device. In some embodiments, hardwired circuitry may be used in place of or in combination with software instructions executed by the processor. Communication among modules, systems, devices, and elements may be over a direct or switched connections, and wired or wireless networks or connections, via directly connected wires, or any other appropriate communication mechanism. Transmission of information may be performed on the hardware layer using any appropriate system, device, or protocol, including those related to or utilizing Firewire, PCI, PCI express, CardBus, USB, CAN, SCSI, IDA, RS232, RS422, RS485, 802.11, etc.

The communication among modules, systems, devices, and elements may include handshaking, notifications, coordination, encapsulation, encryption, headers, such as routing or error detecting headers, or any other appropriate communication protocol or attribute. Communication may also messages related to HTTP, HTTPS, FTP, TCP, IP, ebMS OASIS/ebXML, DICOM, DICOS, secure sockets, VPN, encrypted or unencrypted pipes, MIME, SMTP, MIME Multipart/Related Content-type, SQL, etc.

[0066] Any appropriate 3D graphics processing may be used for displaying or rendering, including processing based on OpenGL, Direct3D, Java 3D, etc. Whole, partial, or modified 3D graphics packages may also be used, such packages including 3DS Max, SolidWorks, Maya, Form Z, Cybermotion 3D, VTK, Slicer, Blender or any others. In some embodiments, various parts of the needed rendering may occur on traditional or specialized graphics hardware. The rendering may also occur on the general CPU, on programmable hardware, on a separate processor, be distributed over multiple processors, over multiple dedicated graphics cards, or using any other appropriate combination of hardware or technique.

[0067] The features and attributes of the specific embodiments disclosed above may be combined in different ways to form additional embodiments, all of which fall within the scope of the present disclosure.

[0068] Conditional language used herein, such as, among others, “can,” “could,” “might,” “may,” “e.g.,” and the like, unless specifically stated otherwise, or otherwise understood within the context as used, is generally intended to convey that certain embodiments include, while other embodiments do not include, certain features, elements and/or states. Thus, such conditional language is not generally intended to imply that features, elements and/or states are in any way required for one or more embodiments or that one or more embodiments necessarily include logic for deciding, with or without author input or prompting, whether these features, elements and/or states are included or are to be performed in any particular embodiment.

[0069] Any process descriptions, elements, or blocks in the processes, methods, and flow diagrams described herein and/or depicted in the attached figures should be understood as potentially representing modules, segments, or portions of code which include one or more executable instructions for implementing specific logical functions or steps in the process. Alternate implementations are included within the scope of the embodiments described herein in which elements or functions may be deleted, executed out of order from that shown or discussed, including substantially concurrently or in reverse order, depending on the functionality involved, as would be understood by those skilled in the art.

[0070] All of the methods and processes described above may be embodied in, and fully automated via, software code modules executed by one or more general purpose computers or processors, such as those computer systems described above. The code modules may be stored in any type of computer-readable medium or other computer storage device. Some or all of the methods may alternatively be embodied in specialized computer hardware.

[0071] It should be emphasized that many variations and modifications may be made to the above-described embodiments, the elements of which are to be understood as being among other acceptable examples. All such modifications and variations are intended to be included herein within the scope of this disclosure and protected by the following claims.

1. (canceled)
2. A method for image annotation in image guided medical procedures, comprising:
 - determining, with one or more computing devices, position and orientation of a first medical device;
 - determining position and orientation of an imaging area based at least on the position and orientation of the first medical device;
 - causing one or more displays to display a perspective view of the imaging area within a virtual 3D space based at least on the position and orientation of the first medical device relative to a position of a user;
 - tracking, with the one or more computing devices, a position of a second medical device; and
 - causing the one or more displays to display an annotation in the virtual 3D space based at least on an intersection of at least a portion of the second medical device with the perspective view of the imaging area.
3. The method of claim 2, wherein the at least a portion of the second medical device comprises an axis or trajectory of the second medical device.
4. The method of claim 2, wherein the second medical device comprises at least one of a needle, a stylus, an ultrasound transducer, a cauterizer, a scalpel, a glove, a finger, and a gaze of a user.
5. The method of claim 2, wherein causing the one or more displays to display the annotation comprises causing the one or more displays to display the annotation based at least on the intersection of the at least a portion of the second medical device with the perspective view of the imaging area over time.
6. The method of claim 2, wherein the position of the user comprises a predetermined location.
7. A system for image annotation in image-guided medical procedures, comprising:
 - one or more computing devices in communication with one or more displays, a first medical device, and a second medical device, wherein the one or more computing devices are configured to:
 - determine position and orientation of the first medical device;
 - determine position and orientation of an imaging area based at least on the position and orientation of the first medical device;
 - cause the one or more displays to display a perspective view of the imaging area within a virtual 3D space based at least on the position and orientation of the first medical device relative to a position of a user;
 - track a position of the second medical device; and
 - cause the one or more displays to display an annotation in the virtual 3D space based at least on an intersection of at least a portion of the second medical device with the perspective view of the imaging area.
8. The system of claim 7, wherein the one or more computing devices are further configured to receive at least one image of a portion of a patient based at least on the position and orientation of the first medical device, and wherein the perspective view of the imaging area comprises a perspective view of the at least one image.
9. The system of claim 7, wherein the at least a portion of the second medical device comprises an axis or trajectory of the second medical device.

10. The system of claim 7, wherein the intersection comprises contact between the at least a portion of the second medical device and the one or more displays.

11. The system of claim 7, wherein the second medical device comprises at least one of a needle, a stylus, an ultrasound transducer, a cauterizer, and a scalpel.

12. The system of claim 7, wherein the second medical device comprises at least one of a glove, a finger, and a gaze of a user.

13. The system of claim 7, wherein the one or more computing devices are further configured to cause the one or more displays to display virtual ink at the intersection of the at least a portion of the second medical device and the perspective view of the imaging area.

14. The system of claim 7, wherein to cause the one or more displays to display the annotation, the one or more computing devices are configured to cause the one or more displays to display the annotation based at least on the intersection of the at least a portion of the second medical device with the perspective view of the imaging area over time.

15. The system of claim 7, wherein to track the position of the second medical device the one or more computing devices are configured to receive input from a touch screen and determine position based on the input from the touch screen.

16. The system of claim 7, wherein to track position of the second medical device the one or more computing devices are configured to receive input from a remote pointer and determine position based on the input from the remote pointer.

17. The system of claim 7, wherein the position of the user comprises a predetermined location.

18. A non-transient computer-readable medium comprising computer-executable instructions, said computer-executable instructions, when executing on one or more computing devices, cause the one or more computing devices to:

determine position and orientation of a first medical device;

determine position and orientation of an imaging area based at least on the position and orientation of the first medical device;

cause one or more displays to display a perspective view of the imaging area within a virtual 3D space based at least on the position and orientation of the first medical device relative to a position of a user;

track a position of a second medical device; and

cause the one or more displays to display an annotation in the virtual 3D space based at least on an intersection of at least a portion of the second medical device with the perspective view of the imaging area.

19. The non-transient computer-readable medium of claim 18, wherein the at least a portion of the second medical device comprises an axis or trajectory of the second medical device.

20. The non-transient computer-readable medium of claim 18, wherein causing the one or more displays to display the annotation comprises causing the one or more displays to display the annotation based at least on the intersection of the at least a portion of the second medical device with the perspective view of the imaging area over time.

21. The non-transient computer-readable medium of claim 18, wherein the position of the user comprises a predetermined location.

* * * * *

专利名称(译)	图像引导医疗程序中的图像注释		
公开(公告)号	US20140094687A1	公开(公告)日	2014-04-03
申请号	US14/047628	申请日	2013-10-07
[标]申请(专利权)人(译)	INNEROPTIC TECH		
申请(专利权)人(译)	INNEROPTIC TECHNOLOGY , INC.		
当前申请(专利权)人(译)	INNEROPTIC TECHNOLOGY , INC.		
[标]发明人	RAZZAQUE SHARIF STATE ANDREI		
发明人	RAZZAQUE, SHARIF STATE, ANDREI		
IPC分类号	A61B5/00 A61B6/03 A61B8/12 A61B19/00 A61B18/14		
CPC分类号	A61B5/748 A61B19/5244 A61B6/032 A61B8/12 A61B18/1477 A61B34/20 A61B6/4494 A61B6/466 A61B6/468 A61B6/5217 A61B6/5247 A61B8/466 A61B8/468 A61B8/483 A61B8/5223 A61B34/25 A61B90/37 A61B2017/00207 A61B2034/2048 A61B2034/2051 A61B2034/2055 A61B2090/378		
优先权	61/387132 2010-09-28 US 61/322991 2010-04-12 US		
其他公开文献	US9107698		
外部链接	Espacenet USPTO		

摘要(译)

这里给出的是用于图像引导的医疗过程中的图像标注的方法，系统，设备和计算机可读介质。本文的一些实施例允许医生或其他操作者使用一个或多个医疗设备以便在3D空间中定义注释。这些注释可以稍后在3D空间中在医生或操作者的首次绘制或以其他方式生成的位置显示。在一些实施例中，操作者可以使用各种可用的医疗设备，例如针，手术刀，或甚至手指，以便定义注释。本文的实施例可以允许操作者更方便和有效地注释可视化医学数据。

