



US010376305B2

(12) **United States Patent**
Yates et al.

(10) **Patent No.:** **US 10,376,305 B2**
(45) **Date of Patent:** **Aug. 13, 2019**

(54) **METHODS AND SYSTEMS FOR ADVANCED
HARMONIC ENERGY**

(71) Applicant: **Ethicon Endo-Surgery, LLC**,
Guaynabo, PR (US)

(72) Inventors: **David C. Yates**, West Chester, OH
(US); **Amy M. Krumm**, Cincinnati,
OH (US); **Mark A. Davison**, Mason,
OH (US)

(73) Assignee: **Ethicon LLC**, Guaynabo, PR (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 315 days.

(21) Appl. No.: **15/229,562**

(22) Filed: **Aug. 5, 2016**

(65) **Prior Publication Data**

US 2018/0036065 A1 Feb. 8, 2018

(51) **Int. Cl.**
A61B 18/12 (2006.01)
A61B 18/14 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 18/1445** (2013.01); **A61B 18/1206**
(2013.01); **A61B 18/1482** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC A61B 18/1445; A61B 18/1442; A61B
18/1206; A61B 2018/0063;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

969,528 A 9/1910 Disbrow
1,570,025 A 1/1926 Young
(Continued)

FOREIGN PATENT DOCUMENTS

AU 2003241752 A1 9/2003
CA 2535467 A1 4/1993
(Continued)

OTHER PUBLICATIONS

Henriques F.C., "Studies in thermal injury V. The predictability and
the significance of thermally induced rate processes leading to
irreversible epidermal injury." Archives of Pathology, 434, pp.
489-502 (1947).


(Continued)

Primary Examiner — Thomas A Giuliani

(57) **ABSTRACT**

Aspects of the present disclosure are presented for a medical
instrument configured to adjust the power level for sealing
procedures to account for changes in tissue impedance levels
over time. In some aspects, a medical instrument may be
configured to apply power according to a power algorithm to
seal tissue by applying a gradually lower amount of power
over time as the tissue impedance level begins to rise out of
the "bathtub region," which is the time period during energy
application where the tissue impedance is low enough for
electrosurgical energy to be effective for sealing tissue. In
some aspects, the power is then cut once the tissue imped-
ance level exceeds the "bathtub region." By gradually reduc-
ing the power, a balance is achieved between still applying
an effective level of power for sealing and prolonging the
time in which the tissue impedance remains in the "bathtub
region."

20 Claims, 16 Drawing Sheets

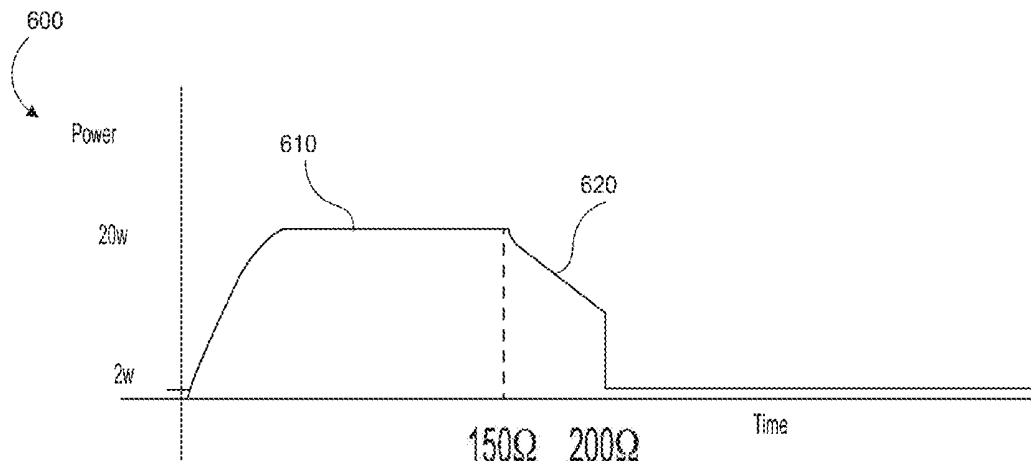

- (51) **Int. Cl.**
A61B 18/00 (2006.01)
A61B 17/32 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61B 17/320092* (2013.01); *A61B 2018/0063* (2013.01); *A61B 2018/00208* (2013.01); *A61B 2018/00642* (2013.01); *A61B 2018/00678* (2013.01); *A61B 2018/00702* (2013.01); *A61B 2018/00875* (2013.01); *A61B 2018/00994* (2013.01)
- (58) **Field of Classification Search**
 CPC *A61B 2018/00875*; *A61B 2018/00642*; *A61B 2018/00702*; *A61B 18/085*; *A61B 18/1482*; *A61B 2018/1273*; *A61B 2018/128*; *A61B 2018/00678*; *A61B 2018/00666*; *A61B 2018/00994*; *A61B 2018/063*
 USPC 606/33, 34, 37, 38, 41, 42, 45, 48, 52; 607/98, 99, 101, 105, 115, 116
 See application file for complete search history.
- (56) **References Cited**
 U.S. PATENT DOCUMENTS
- | | | | | | |
|-------------|---------|--------------------|-------------|---------|------------------------|
| 1,813,902 A | 7/1931 | Bovie | 3,900,823 A | 8/1975 | Sokal et al. |
| 2,188,497 A | 1/1940 | Calva | 3,918,442 A | 11/1975 | Nikolaev et al. |
| 2,366,274 A | 1/1945 | Luth et al. | 3,924,335 A | 12/1975 | Balamuth et al. |
| 2,425,245 A | 8/1947 | Johnson | 3,946,738 A | 3/1976 | Newton et al. |
| 2,442,966 A | 6/1948 | Wallace | 3,955,859 A | 5/1976 | Stella et al. |
| 2,458,152 A | 1/1949 | Eakins | 3,956,826 A | 5/1976 | Perdreux, Jr. |
| 2,510,693 A | 6/1950 | Green | 4,005,714 A | 2/1977 | Hiltebrandt |
| 2,597,564 A | 5/1952 | Bugg | 4,012,647 A | 3/1977 | Balamuth et al. |
| 2,704,333 A | 3/1955 | Calosi et al. | 4,034,762 A | 7/1977 | Cosens et al. |
| 2,736,960 A | 3/1956 | Armstrong | 4,058,126 A | 11/1977 | Leveen |
| 2,748,967 A | 6/1956 | Roach | 4,074,719 A | 2/1978 | Semm |
| 2,845,072 A | 7/1958 | Shafer | 4,156,187 A | 5/1979 | Murry et al. |
| 2,849,788 A | 9/1958 | Creek | 4,167,944 A | 9/1979 | Banko |
| 2,867,039 A | 1/1959 | Zach | 4,188,927 A | 2/1980 | Harris |
| 2,874,470 A | 2/1959 | Richards | 4,200,106 A | 4/1980 | Douvas et al. |
| 2,990,616 A | 7/1961 | Balamuth et al. | 4,203,430 A | 5/1980 | Takahashi |
| RE25,033 E | 8/1961 | Balamuth et al. | 4,203,444 A | 5/1980 | Bonnell et al. |
| 3,015,961 A | 1/1962 | Roney | 4,220,154 A | 9/1980 | Semm |
| 3,033,407 A | 5/1962 | Alfons | 4,237,441 A | 12/1980 | van Konynenburg et al. |
| 3,053,124 A | 9/1962 | Balamuth et al. | 4,281,785 A | 8/1981 | Brooks |
| 3,082,805 A | 3/1963 | Royce | 4,300,083 A | 11/1981 | Heiges |
| 3,166,971 A | 1/1965 | Stoecker | 4,302,728 A | 11/1981 | Nakamura |
| 3,322,403 A | 5/1967 | Murphy | 4,304,987 A | 12/1981 | Van Konynenburg |
| 3,432,691 A | 3/1969 | Shoh | 4,306,570 A | 12/1981 | Matthews |
| 3,433,226 A | 3/1969 | Boyd | 4,314,559 A | 2/1982 | Allen |
| 3,489,930 A | 1/1970 | Shoh | 4,445,063 A | 4/1984 | Smith |
| 3,513,848 A | 5/1970 | Winston et al. | 4,463,759 A | 8/1984 | Garito et al. |
| 3,514,856 A | 6/1970 | Camp et al. | 4,491,132 A | 1/1985 | Aikins |
| 3,525,912 A | 8/1970 | Wallin | 4,492,231 A | 1/1985 | Auth |
| 3,526,219 A | 9/1970 | Balamuth | 4,494,759 A | 1/1985 | Kieffer |
| 3,554,198 A | 1/1971 | Tatoian et al. | 4,504,264 A | 3/1985 | Kelman |
| 3,580,841 A | 5/1971 | Cadotte et al. | 4,512,344 A | 4/1985 | Barber |
| 3,606,682 A | 9/1971 | Camp et al. | 4,526,571 A | 7/1985 | Wuchinich |
| 3,614,484 A | 10/1971 | Shoh | 4,535,773 A | 8/1985 | Yoon |
| 3,616,375 A | 10/1971 | Inoue | 4,541,638 A | 9/1985 | Ogawa et al. |
| 3,629,726 A | 12/1971 | Popescu | 4,545,374 A | 10/1985 | Jacobson |
| 3,636,943 A | 1/1972 | Balamuth | 4,545,926 A | 10/1985 | Fouts, Jr. et al. |
| 3,668,486 A | 6/1972 | Silver | 4,549,147 A | 10/1985 | Kondo |
| 3,702,948 A | 11/1972 | Balamuth | 4,550,870 A | 11/1985 | Krumme et al. |
| 3,703,651 A | 11/1972 | Blowers | 4,553,544 A | 11/1985 | Nomoto et al. |
| 3,776,238 A | 12/1973 | Peyman et al. | 4,562,838 A | 1/1986 | Walker |
| 3,777,760 A | 12/1973 | Essner | 4,574,615 A | 3/1986 | Bower et al. |
| 3,805,787 A | 4/1974 | Banko | 4,582,236 A | 4/1986 | Hirose |
| 3,809,977 A | 5/1974 | Balamuth et al. | 4,617,927 A | 10/1986 | Manes |
| 3,830,098 A | 8/1974 | Antonevich | 4,633,119 A | 12/1986 | Thompson |
| 3,854,737 A | 12/1974 | Gilliam, Sr. | 4,634,420 A | 1/1987 | Spinosa et al. |
| 3,862,630 A | 1/1975 | Balamuth | 4,640,279 A | 2/1987 | Beard |
| 3,875,945 A | 4/1975 | Friedman | 4,641,053 A | 2/1987 | Takeda |
| 3,885,438 A | 5/1975 | Harris, Sr. et al. | 4,646,738 A | 3/1987 | Trott |
| | | | 4,646,756 A | 3/1987 | Watmough et al. |
| | | | 4,649,919 A | 3/1987 | Thimsen et al. |
| | | | 4,662,068 A | 5/1987 | Polonsky |
| | | | 4,674,502 A | 6/1987 | Imonti |
| | | | 4,694,835 A | 9/1987 | Strand |
| | | | 4,708,127 A | 11/1987 | Abdelghani |
| | | | 4,712,722 A | 12/1987 | Hood et al. |
| | | | 4,735,603 A | 4/1988 | Goodson et al. |
| | | | 4,761,871 A | 8/1988 | O'Connor et al. |
| | | | 4,808,154 A | 2/1989 | Freeman |
| | | | 4,819,635 A | 4/1989 | Shapiro |
| | | | 4,827,911 A | 5/1989 | Broadwin et al. |
| | | | 4,830,462 A | 5/1989 | Karny et al. |
| | | | 4,832,683 A | 5/1989 | Idemoto et al. |
| | | | 4,836,186 A | 6/1989 | Scholz |
| | | | 4,838,853 A | 6/1989 | Parisi |
| | | | 4,844,064 A | 7/1989 | Thimsen et al. |
| | | | 4,849,133 A | 7/1989 | Yoshida et al. |
| | | | 4,850,354 A | 7/1989 | McGurk-Burleson et al. |
| | | | 4,852,578 A | 8/1989 | Companion et al. |
| | | | 4,860,745 A | 8/1989 | Farin et al. |
| | | | 4,862,890 A | 9/1989 | Stasz et al. |
| | | | 4,865,159 A | 9/1989 | Jamison |
| | | | 4,867,157 A | 9/1989 | McGurk-Burleson et al. |
| | | | 4,878,493 A | 11/1989 | Pasternak et al. |
| | | | 4,880,015 A | 11/1989 | Nierman |
| | | | 4,881,550 A | 11/1989 | Kothe |
| | | | 4,896,009 A | 1/1990 | Pawlowski |
| | | | 4,903,696 A | 2/1990 | Stasz et al. |
| | | | 4,910,389 A | 3/1990 | Sherman et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

4,915,643 A	4/1990	Samejima et al.	5,275,609 A	1/1994	Pingleton et al.
4,920,978 A	5/1990	Colvin	5,282,800 A	2/1994	Foshee et al.
4,922,902 A	5/1990	Wuchinich et al.	5,282,817 A	2/1994	Hoogeboom et al.
4,936,842 A	6/1990	D'Amelio et al.	5,285,795 A	2/1994	Ryan et al.
4,954,960 A	9/1990	Lo et al.	5,285,945 A	2/1994	Brinkerhoff et al.
4,965,532 A	10/1990	Sakurai	5,290,286 A	3/1994	Parins
4,979,952 A	12/1990	Kubota et al.	5,300,068 A	4/1994	Rosar et al.
4,981,756 A	1/1991	Rhandhawa	5,304,115 A	4/1994	Pflueger et al.
5,001,649 A	3/1991	Lo et al.	D347,474 S	5/1994	Olson
5,013,956 A	5/1991	Kurozumi et al.	5,307,976 A	5/1994	Olson et al.
5,015,227 A	5/1991	Broadwin et al.	5,309,927 A	5/1994	Welch
5,020,514 A	6/1991	Heckele	5,312,023 A	5/1994	Green et al.
5,026,370 A	6/1991	Lottick	5,312,425 A	5/1994	Evans et al.
5,026,387 A	6/1991	Thomas	5,318,563 A	6/1994	Malis et al.
5,035,695 A	7/1991	Weber, Jr. et al.	5,318,564 A	6/1994	Eggers
5,042,707 A	8/1991	Taheri	5,318,589 A	6/1994	Lichtman
5,061,269 A	10/1991	Muller	5,322,055 A	6/1994	Davison et al.
5,075,839 A	12/1991	Fisher et al.	5,324,299 A	6/1994	Davison et al.
5,084,052 A	1/1992	Jacobs	5,326,013 A	7/1994	Green et al.
5,099,840 A	3/1992	Goble et al.	5,326,342 A	7/1994	Pflueger et al.
5,104,025 A	4/1992	Main et al.	5,330,471 A	7/1994	Eggers
5,105,117 A	4/1992	Yamaguchi	5,330,502 A	7/1994	Hassler et al.
5,106,538 A	4/1992	Barma et al.	5,339,723 A	8/1994	Huitema
5,108,383 A	4/1992	White	5,342,356 A	8/1994	Ellman et al.
5,109,819 A	5/1992	Custer et al.	5,342,359 A	8/1994	Rydell
5,112,300 A	5/1992	Ureche	5,344,420 A	9/1994	Hilal et al.
5,113,139 A	5/1992	Furukawa	5,345,937 A	9/1994	Middleman et al.
5,123,903 A	6/1992	Quaid et al.	5,346,502 A	9/1994	Estabrook et al.
5,126,618 A	6/1992	Takahashi et al.	5,353,474 A	10/1994	Good et al.
D327,872 S	7/1992	McMills et al.	5,357,164 A	10/1994	Imabayashi et al.
5,152,762 A	10/1992	McElhenney	5,357,423 A	10/1994	Weaver et al.
5,156,633 A	10/1992	Smith	5,359,994 A	11/1994	Krauter et al.
5,160,334 A	11/1992	Billings et al.	5,361,583 A	11/1994	Huitema
5,162,044 A	11/1992	Gahn et al.	5,366,466 A	11/1994	Christian et al.
5,163,421 A	11/1992	Bernstein et al.	5,368,557 A	11/1994	Nita et al.
5,163,537 A	11/1992	Radev	5,370,645 A	12/1994	Klicek et al.
5,163,945 A	11/1992	Ortiz et al.	5,371,429 A	12/1994	Manna
5,167,619 A	12/1992	Wuchinich	5,374,813 A	12/1994	Shipp
5,167,725 A	12/1992	Clark et al.	D354,564 S	1/1995	Medema
5,172,344 A	12/1992	Ehrlich	5,381,067 A	1/1995	Greenstein et al.
5,174,276 A	12/1992	Crockard	5,383,874 A	1/1995	Jackson et al.
D332,660 S	1/1993	Rawson et al.	5,387,207 A	2/1995	Dyer et al.
5,176,677 A	1/1993	Wuchinich	5,387,215 A	2/1995	Fisher
5,176,695 A	1/1993	Dulebohn	5,389,098 A	2/1995	Tsuruta et al.
5,184,605 A	2/1993	Grzeszykowski	5,394,187 A	2/1995	Shipp
5,188,102 A	2/1993	Idemoto et al.	5,395,312 A	3/1995	Desai
D334,173 S	3/1993	Liu et al.	5,395,363 A	3/1995	Billings et al.
5,190,517 A	3/1993	Zieve et al.	5,395,364 A	3/1995	Anderhub et al.
5,190,541 A	3/1993	Abele et al.	5,396,266 A	3/1995	Brimhall
5,196,007 A	3/1993	Ellman et al.	5,396,900 A	3/1995	Slater et al.
5,205,459 A	4/1993	Brinkerhoff et al.	5,400,267 A	3/1995	Denen et al.
5,209,719 A	5/1993	Baruch et al.	5,403,312 A	4/1995	Yates et al.
5,213,569 A	5/1993	Davis	5,403,334 A	4/1995	Evans et al.
5,214,339 A	5/1993	Naito	5,408,268 A	4/1995	Shipp
5,217,460 A	6/1993	Knoepfler	D358,887 S	5/1995	Feinberg
5,218,529 A	6/1993	Meyer et al.	5,411,481 A	5/1995	Allen et al.
5,221,282 A	6/1993	Wuchinich	5,417,709 A	5/1995	Slater
5,222,937 A	6/1993	Kagawa	5,419,761 A	5/1995	Narayanan et al.
5,226,909 A	7/1993	Evans et al.	5,421,829 A	6/1995	Olichney et al.
5,226,910 A	7/1993	Kajiyama et al.	5,423,844 A	6/1995	Miller
5,231,989 A	8/1993	Middleman et al.	5,428,504 A	6/1995	Bhatla
5,234,428 A	8/1993	Kaufman	5,429,131 A	7/1995	Scheinman et al.
5,241,236 A	8/1993	Sasaki et al.	5,438,997 A	8/1995	Sieben et al.
5,241,968 A	9/1993	Slater	5,441,499 A	8/1995	Fritzsche
5,242,339 A	9/1993	Thornton	5,443,463 A	8/1995	Stern et al.
5,242,460 A	9/1993	Klein et al.	5,445,638 A	8/1995	Rydell et al.
5,246,003 A	9/1993	DeLonzor	5,445,639 A	8/1995	Kuslich et al.
5,254,129 A	10/1993	Alexander	5,449,370 A	9/1995	Vaitekunas
5,257,988 A	11/1993	L'Esperance, Jr.	5,451,053 A	9/1995	Garrido
5,258,006 A	11/1993	Rydell et al.	5,451,220 A	9/1995	Ciervo
5,261,922 A	11/1993	Hood	5,451,227 A	9/1995	Michaelson
5,263,957 A	11/1993	Davison	5,456,684 A	10/1995	Schmidt et al.
5,264,925 A	11/1993	Shipp et al.	5,458,598 A	10/1995	Feinberg et al.
5,275,166 A	1/1994	Vaitekunas et al.	5,465,895 A	11/1995	Knodel et al.
5,275,607 A	1/1994	Lo et al.	5,471,988 A	12/1995	Fujio et al.
			5,472,443 A	12/1995	Cordis et al.
			5,476,479 A	12/1995	Green et al.
			5,478,003 A	12/1995	Green et al.
			5,480,409 A	1/1996	Riza

(56)

References Cited

U.S. PATENT DOCUMENTS

5,483,501 A	1/1996	Park et al.	5,690,269 A	11/1997	Bolanos et al.
5,484,436 A	1/1996	Eggers et al.	5,693,051 A	12/1997	Schulze et al.
5,486,162 A	1/1996	Brumbach	5,694,936 A	12/1997	Fujimoto et al.
5,486,189 A	1/1996	Mudry et al.	5,695,510 A	12/1997	Hood
5,490,860 A	2/1996	Middle et al.	5,700,261 A	12/1997	Brinkerhoff
5,496,317 A	3/1996	Goble et al.	5,704,534 A	1/1998	Huitema et al.
5,500,216 A	3/1996	Julian et al.	5,707,369 A	1/1998	Vaitekunas et al.
5,501,654 A	3/1996	Failla et al.	5,709,680 A	1/1998	Yates et al.
5,504,650 A	4/1996	Katsui et al.	5,711,472 A	1/1998	Bryan
5,505,693 A	4/1996	MacKool	5,713,896 A	2/1998	Nardella
5,507,297 A	4/1996	Slater et al.	5,715,817 A	2/1998	Stevens-Wright et al.
5,507,738 A	4/1996	Ciervo	5,716,366 A	2/1998	Yates
5,509,922 A	4/1996	Aranyi et al.	5,717,306 A	2/1998	Shipp
5,511,556 A	4/1996	DeSantis	5,720,742 A	2/1998	Zacharias
5,520,704 A	5/1996	Castro et al.	5,720,744 A	2/1998	Eggleson et al.
5,522,839 A	6/1996	Pilling	5,723,970 A	3/1998	Bell
5,527,331 A	6/1996	Kresch et al.	5,728,130 A	3/1998	Ishikawa et al.
5,531,744 A	7/1996	Nardella et al.	5,730,752 A	3/1998	Alden et al.
5,540,681 A	7/1996	Strul et al.	5,733,074 A	3/1998	Stock et al.
5,540,693 A	7/1996	Fisher	5,735,848 A	4/1998	Yates et al.
5,542,916 A	8/1996	Hirsch et al.	5,741,226 A	4/1998	Strukel et al.
5,548,286 A	8/1996	Craven	5,743,906 A	4/1998	Parins et al.
5,549,637 A	8/1996	Crainich	5,752,973 A	5/1998	Kieturakis
5,553,675 A	9/1996	Pitzen et al.	5,755,717 A	5/1998	Yates et al.
5,558,671 A *	9/1996	Yates A61B 17/07207	5,762,255 A	6/1998	Chrisman et al.
		606/34	5,766,164 A	6/1998	Mueller et al.
5,562,609 A	10/1996	Brumbach	5,772,659 A	6/1998	Becker et al.
5,562,610 A	10/1996	Brumbach	5,776,155 A	7/1998	Beaupre et al.
5,562,659 A	10/1996	Morris	5,779,701 A	7/1998	McBrayer et al.
5,563,179 A	10/1996	Stone et al.	5,782,834 A	7/1998	Lucey et al.
5,569,164 A	10/1996	Lurz	5,792,135 A	8/1998	Madhani et al.
5,571,121 A	11/1996	Heifetz	5,792,138 A	8/1998	Shipp
5,573,424 A	11/1996	Poppe	5,792,165 A	8/1998	Klieman et al.
5,573,534 A	11/1996	Stone	5,796,188 A	8/1998	Bays
5,577,654 A	11/1996	Bishop	5,797,941 A	8/1998	Schulze et al.
5,584,830 A	12/1996	Ladd et al.	5,797,958 A	8/1998	Yoon
5,591,187 A	1/1997	Dekel	5,797,959 A	8/1998	Castro et al.
5,593,414 A	1/1997	Shipp et al.	5,800,432 A	9/1998	Swanson
5,599,350 A	2/1997	Schulze et al.	5,800,449 A	9/1998	Wales
5,600,526 A	2/1997	Russell et al.	5,805,140 A	9/1998	Rosenberg et al.
5,601,601 A	2/1997	Tal et al.	5,807,393 A	9/1998	Williamson, IV et al.
5,603,773 A	2/1997	Campbell	5,808,396 A	9/1998	Boukhny
5,607,436 A	3/1997	Pratt et al.	5,810,811 A	9/1998	Yates et al.
5,607,450 A	3/1997	Zvenyatsky et al.	5,810,859 A	9/1998	DiMatteo et al.
5,609,573 A	3/1997	Sandock	5,817,033 A	10/1998	DeSantis et al.
5,611,813 A	3/1997	Lichtman	5,817,084 A	10/1998	Jensen
5,618,304 A	4/1997	Hart et al.	5,817,093 A	10/1998	Williamson, IV et al.
5,618,307 A	4/1997	Donlon et al.	5,817,119 A	10/1998	Klieman et al.
5,618,492 A	4/1997	Auten et al.	5,823,197 A	10/1998	Edwards
5,620,447 A	4/1997	Smith et al.	5,827,271 A *	10/1998	Buyse A61B 18/1206
5,624,452 A	4/1997	Yates			606/40
5,626,587 A	5/1997	Bishop et al.	5,827,323 A	10/1998	Klieman et al.
5,626,595 A	5/1997	Sklar et al.	5,828,160 A	10/1998	Sugishita
5,628,760 A	5/1997	Knoepfler	5,833,696 A	11/1998	Whitfield et al.
5,630,420 A	5/1997	Vaitekunas	5,836,897 A	11/1998	Sakurai et al.
5,632,432 A	5/1997	Schulze et al.	5,836,909 A	11/1998	Cosmesu
5,632,717 A	5/1997	Yoon	5,836,943 A	11/1998	Miller, III
5,640,741 A	6/1997	Yano	5,836,957 A	11/1998	Schulz et al.
D381,077 S	7/1997	Hunt	5,836,990 A	11/1998	Li
5,647,871 A	7/1997	Levine et al.	5,843,109 A	12/1998	Mehta et al.
5,649,937 A	7/1997	Bito et al.	5,851,212 A	12/1998	Zirps et al.
5,651,780 A	7/1997	Jackson et al.	5,853,412 A	12/1998	Mayenberger
5,653,713 A	8/1997	Michelson	5,858,018 A	1/1999	Shipp et al.
5,655,100 A	8/1997	Ebrahim et al.	5,865,361 A	2/1999	Milliman et al.
5,658,281 A	8/1997	Heard	5,873,873 A	2/1999	Smith et al.
5,662,662 A	9/1997	Bishop et al.	5,873,882 A	2/1999	Straub et al.
5,662,667 A	9/1997	Knodel	5,876,401 A	3/1999	Schulze et al.
5,665,085 A	9/1997	Nardella	5,878,193 A	3/1999	Wang et al.
5,665,100 A	9/1997	Yoon	5,879,364 A	3/1999	Bromfield et al.
5,669,922 A	9/1997	Hood	5,880,668 A	3/1999	Hall
5,674,219 A	10/1997	Monson et al.	5,883,615 A	3/1999	Fago et al.
5,674,220 A	10/1997	Fox et al.	5,891,142 A	4/1999	Eggers et al.
5,674,235 A	10/1997	Parisi	5,893,835 A	4/1999	Witt et al.
5,678,568 A	10/1997	Uchikubo et al.	5,897,523 A	4/1999	Wright et al.
5,688,270 A	11/1997	Yates et al.	5,897,569 A	4/1999	Kellogg et al.
			5,903,607 A	5/1999	Tailliet
			5,904,681 A	5/1999	West, Jr.
			5,906,625 A	5/1999	Bito et al.
			5,906,627 A	5/1999	Spaulding

(56)

References Cited

U.S. PATENT DOCUMENTS

5,906,628 A	5/1999	Miyawaki et al.	6,132,429 A	10/2000	Baker
5,910,129 A	6/1999	Koblish et al.	6,132,448 A	10/2000	Perez et al.
5,911,699 A	6/1999	Anis et al.	6,139,320 A	10/2000	Hahn
5,913,823 A	6/1999	Hedberg et al.	6,139,561 A	10/2000	Shibata et al.
5,916,229 A	6/1999	Evans	6,142,615 A	11/2000	Qiu et al.
5,921,956 A	7/1999	Grinberg et al.	6,142,994 A	11/2000	Swanson et al.
5,929,846 A	7/1999	Rosenberg et al.	6,144,402 A	11/2000	Norsworthy et al.
5,935,143 A	8/1999	Hood	6,147,560 A	11/2000	Erhage et al.
5,935,144 A	8/1999	Estabrook	6,152,902 A	11/2000	Christian et al.
5,938,633 A	8/1999	Beaupre	6,152,923 A	11/2000	Ryan
5,944,718 A	8/1999	Austin et al.	6,154,198 A	11/2000	Rosenberg
5,944,737 A	8/1999	Tsonton et al.	6,159,160 A	12/2000	Hsei et al.
5,947,984 A	9/1999	Whipple	6,159,175 A	12/2000	Strukel et al.
5,954,717 A	9/1999	Behl et al.	6,162,194 A	12/2000	Shipp
5,954,736 A	9/1999	Bishop et al.	6,162,208 A	12/2000	Hipps
5,954,746 A	9/1999	Holthaus et al.	6,165,150 A	12/2000	Banko
5,957,882 A	9/1999	Nita et al.	6,174,309 B1	1/2001	Wrublewski et al.
5,957,943 A	9/1999	Vaitekunas	6,174,310 B1	1/2001	Kirwan, Jr.
5,968,007 A	10/1999	Simon et al.	6,176,857 B1	1/2001	Ashley
5,968,060 A	10/1999	Kellogg	6,179,853 B1	1/2001	Sachse et al.
5,974,342 A	10/1999	Petrofsky	6,183,426 B1	2/2001	Akisada et al.
D416,089 S	11/1999	Barton et al.	6,187,003 B1	2/2001	Buyse et al.
5,980,510 A	11/1999	Tsonton et al.	6,190,386 B1	2/2001	Rydell
5,980,546 A	11/1999	Hood	6,193,709 B1	2/2001	Miyawaki et al.
5,984,938 A	11/1999	Yoon	6,204,592 B1	3/2001	Hur
5,989,274 A	11/1999	Davison et al.	6,205,855 B1	3/2001	Pfeiffer
5,989,275 A	11/1999	Estabrook et al.	6,206,844 B1	3/2001	Reichel et al.
5,993,465 A	11/1999	Shipp et al.	6,206,876 B1	3/2001	Levine et al.
5,993,972 A	11/1999	Reich et al.	6,210,337 B1	4/2001	Dunham et al.
5,994,855 A	11/1999	Lundell et al.	6,210,402 B1	4/2001	Olsen et al.
6,003,517 A	12/1999	Sheffield et al.	6,210,403 B1	4/2001	Klicek
6,013,052 A	1/2000	Durman et al.	6,214,023 B1	4/2001	Whipple et al.
6,024,741 A	2/2000	Williamson, IV et al.	6,228,080 B1	5/2001	Gines
6,024,744 A	2/2000	Kese et al.	6,231,565 B1	5/2001	Tovey et al.
6,024,750 A	2/2000	Mastri et al.	6,233,476 B1	5/2001	Strommer et al.
6,027,515 A	2/2000	Cimino	6,238,366 B1	5/2001	Savage et al.
6,031,526 A	2/2000	Shipp	6,245,065 B1	6/2001	Panescu et al.
6,033,375 A	3/2000	Brumbach	6,251,110 B1	6/2001	Wampler
6,033,399 A	3/2000	Gines	6,252,110 B1	6/2001	Uemura et al.
6,036,667 A	3/2000	Manna et al.	D444,365 S	7/2001	Bass et al.
6,036,707 A	3/2000	Spaulding	D445,092 S	7/2001	Lee
6,039,734 A	3/2000	Goble	D445,764 S	7/2001	Lee
6,048,224 A	4/2000	Kay	6,254,623 B1	7/2001	Haibel, Jr. et al.
6,050,943 A	4/2000	Slayton et al.	6,257,241 B1	7/2001	Wampler
6,050,996 A	4/2000	Schmaltz et al.	6,258,034 B1	7/2001	Hanafy
6,051,010 A	4/2000	DiMatteo et al.	6,259,230 B1	7/2001	Chou
6,056,735 A	5/2000	Okada et al.	6,267,761 B1	7/2001	Ryan
6,063,098 A	5/2000	Houser et al.	6,270,831 B2	8/2001	Kumar et al.
6,066,132 A	5/2000	Chen et al.	6,273,852 B1	8/2001	Lehe et al.
6,066,151 A	5/2000	Miyawaki et al.	6,274,963 B1	8/2001	Estabrook et al.
6,068,627 A	5/2000	Orszulak et al.	6,277,115 B1	8/2001	Saadat
6,068,629 A	5/2000	Haissaguerre et al.	6,277,117 B1	8/2001	Tetzlaff et al.
6,068,647 A	5/2000	Witt et al.	6,278,218 B1	8/2001	Madan et al.
6,074,389 A	6/2000	Levine et al.	6,280,407 B1	8/2001	Manna et al.
6,077,285 A	6/2000	Boukhny	6,283,981 B1	9/2001	Beaupre
6,080,149 A	6/2000	Huang et al.	6,287,344 B1	9/2001	Wampler et al.
6,083,191 A	7/2000	Rose	6,290,575 B1	9/2001	Shipp
6,086,584 A	7/2000	Miller	6,292,700 B1	9/2001	Morrison et al.
6,090,120 A	7/2000	Wright et al.	6,299,591 B1	10/2001	Banko
6,091,995 A	7/2000	Ingle et al.	6,306,131 B1	10/2001	Hareyama et al.
6,096,033 A	8/2000	Tu et al.	6,306,157 B1	10/2001	Shchervinsky
6,099,483 A	8/2000	Palmer et al.	6,309,400 B2	10/2001	Beaupre
6,099,542 A	8/2000	Cohn et al.	6,311,783 B1	11/2001	Harpell
6,099,550 A	8/2000	Yoon	6,319,221 B1	11/2001	Savage et al.
6,109,500 A	8/2000	Alli et al.	6,325,795 B1	12/2001	Lindemann et al.
6,110,127 A	8/2000	Suzuki	6,325,799 B1	12/2001	Goble
6,113,594 A	9/2000	Savage	6,325,811 B1	12/2001	Messeryly
6,117,152 A	9/2000	Huitema	6,328,751 B1	12/2001	Beaupre
H001904 H	10/2000	Yates et al.	6,332,891 B1	12/2001	Himes
6,126,629 A	10/2000	Perkins	6,338,657 B1	1/2002	Harper et al.
6,126,658 A	10/2000	Baker	6,340,352 B1	1/2002	Okada et al.
6,129,735 A	10/2000	Okada et al.	6,340,878 B1	1/2002	Oglesbee
6,129,740 A	10/2000	Michelson	6,350,269 B1	2/2002	Shipp et al.
6,132,368 A	10/2000	Cooper	6,352,532 B1	3/2002	Kramer et al.
6,132,427 A	10/2000	Jones et al.	6,356,224 B1	3/2002	Wohlfarth
			6,358,246 B1	3/2002	Behl et al.
			6,358,264 B2	3/2002	Banko
			6,364,888 B1	4/2002	Niemeyer et al.
			6,379,320 B1	4/2002	Lafon et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

D457,958 S	5/2002	Dycus et al.	6,575,969 B1	6/2003	Rittman, III et al.
6,383,194 B1	5/2002	Pothula	6,582,427 B1	6/2003	Goble et al.
6,384,690 B1	5/2002	Wilhelmsson et al.	6,582,451 B1	6/2003	Marucci et al.
6,387,109 B1	5/2002	Davison et al.	6,584,360 B2	6/2003	Francischelli et al.
6,388,657 B1	5/2002	Natoli	D477,408 S	7/2003	Bromley
6,390,973 B1	5/2002	Ouchi	6,585,735 B1	7/2003	Frazier et al.
6,391,026 B1	5/2002	Hung et al.	6,588,277 B2	7/2003	Giordano et al.
6,391,042 B1	5/2002	Cimino	6,589,200 B1	7/2003	Schwemberger et al.
6,398,779 B1	6/2002	Buyse et al.	6,589,239 B2	7/2003	Khandkar et al.
6,402,743 B1	6/2002	Orszulak et al.	6,590,733 B1	7/2003	Wilson et al.
6,402,748 B1	6/2002	Schoenman et al.	6,599,288 B2	7/2003	Maguire et al.
6,405,733 B1	6/2002	Fogarty et al.	6,602,252 B2	8/2003	Mollenauer
6,409,722 B1	6/2002	Hoey et al.	6,607,540 B1	8/2003	Shipp
H002037 H	7/2002	Yates et al.	6,610,059 B1	8/2003	West, Jr.
6,416,486 B1	7/2002	Wampler	6,610,060 B2	8/2003	Mulier et al.
6,419,675 B1	7/2002	Gallo, Sr.	6,611,793 B1	8/2003	Burnside et al.
6,423,073 B2	7/2002	Bowman	6,616,450 B2	9/2003	Mossle et al.
6,423,082 B1	7/2002	Houser et al.	6,619,529 B2	9/2003	Green et al.
6,425,906 B1	7/2002	Young et al.	6,620,161 B2	9/2003	Schulze et al.
6,428,538 B1	8/2002	Blewett et al.	6,622,731 B2	9/2003	Daniel et al.
6,428,539 B1	8/2002	Baxter et al.	6,623,482 B2	9/2003	Pendekanti et al.
6,430,446 B1	8/2002	Knowlton	6,623,500 B1	9/2003	Cook et al.
6,432,118 B1	8/2002	Messerly	6,623,501 B2	9/2003	Heller et al.
6,436,114 B1	8/2002	Novak et al.	6,626,848 B2	9/2003	Neuenfeldt
6,436,115 B1	8/2002	Beaupre	6,626,926 B2	9/2003	Friedman et al.
6,440,062 B1	8/2002	Ouchi	6,629,974 B2	10/2003	Penny et al.
6,443,968 B1	9/2002	Holthaus et al.	6,633,234 B2	10/2003	Wiener et al.
6,443,969 B1	9/2002	Novak et al.	6,635,057 B2	10/2003	Harano et al.
6,449,006 B1	9/2002	Shipp	6,644,532 B2	11/2003	Green et al.
6,454,781 B1	9/2002	Witt et al.	6,651,669 B1	11/2003	Burnside
6,454,782 B1	9/2002	Schwemberger	6,652,513 B2	11/2003	Panescu et al.
6,458,128 B1	10/2002	Schulze	6,652,539 B2	11/2003	Shipp et al.
6,458,142 B1	10/2002	Faller et al.	6,652,545 B2	11/2003	Shipp et al.
6,464,689 B1	10/2002	Qin et al.	6,656,132 B1	12/2003	Ouchi
6,464,702 B2	10/2002	Schulze et al.	6,656,177 B2	12/2003	Truckai et al.
6,468,270 B1	10/2002	Hovda et al.	6,656,198 B2	12/2003	Tsonton et al.
6,475,215 B1	11/2002	Tanrisever	6,660,017 B2	12/2003	Beaupre
6,480,796 B2	11/2002	Wiener	6,662,127 B2	12/2003	Wiener et al.
6,485,490 B2	11/2002	Wampler et al.	6,663,941 B2	12/2003	Brown et al.
6,491,690 B1	12/2002	Goble et al.	6,666,860 B1	12/2003	Takahashi
6,491,701 B2	12/2002	Tierney et al.	6,666,875 B1	12/2003	Sakurai et al.
6,491,708 B2	12/2002	Madan et al.	6,669,690 B1	12/2003	Okada et al.
6,497,715 B2	12/2002	Satou	6,669,710 B2	12/2003	Moutafis et al.
6,500,112 B1	12/2002	Khouri	6,673,248 B2	1/2004	Chowdhury
6,500,176 B1	12/2002	Truckai et al.	6,676,660 B2	1/2004	Wampler et al.
6,500,188 B2	12/2002	Harper et al.	6,678,621 B2	1/2004	Wiener et al.
6,500,312 B2	12/2002	Wedekamp	6,679,875 B2	1/2004	Honda et al.
6,503,248 B1	1/2003	Levine	6,679,882 B1	1/2004	Kornerup
6,506,208 B2	1/2003	Hunt et al.	6,679,899 B2	1/2004	Wiener et al.
6,511,478 B1	1/2003	Burnside et al.	6,682,501 B1	1/2004	Nelson et al.
6,511,480 B1	1/2003	Tetzlaff et al.	6,682,544 B2	1/2004	Mastri et al.
6,511,493 B1	1/2003	Moutafis et al.	6,685,700 B2	2/2004	Behl et al.
6,514,252 B2	2/2003	Nezhat et al.	6,685,701 B2	2/2004	Orszulak et al.
6,514,267 B2	2/2003	Jewett	6,685,703 B2	2/2004	Pearson et al.
6,517,565 B1	2/2003	Whitman et al.	6,689,145 B2	2/2004	Lee et al.
6,524,251 B2	2/2003	Rabiner et al.	6,689,146 B1	2/2004	Himes
6,524,316 B1	2/2003	Nicholson et al.	6,690,960 B2	2/2004	Chen et al.
6,527,736 B1	3/2003	Attinger et al.	6,695,840 B2	2/2004	Schulze
6,531,846 B1	3/2003	Smith	6,702,821 B2	3/2004	Bonutti
6,533,784 B2	3/2003	Truckai et al.	6,716,215 B1	4/2004	David et al.
6,537,272 B2	3/2003	Christopherson et al.	6,719,692 B2	4/2004	Kleffner et al.
6,537,291 B2	3/2003	Friedman et al.	6,719,765 B2	4/2004	Bonutti
6,543,452 B1	4/2003	Lavigne	6,719,776 B2	4/2004	Baxter et al.
6,543,456 B1	4/2003	Freeman	6,722,552 B2	4/2004	Fenton, Jr.
6,544,260 B1	4/2003	Markel et al.	6,723,091 B2	4/2004	Goble et al.
6,551,309 B1	4/2003	LePivert	D490,059 S	5/2004	Conway et al.
6,554,829 B2	4/2003	Schulze et al.	6,731,047 B2	5/2004	Kauf et al.
6,558,376 B2	5/2003	Bishop	6,733,498 B2	5/2004	Paton et al.
6,561,983 B2	5/2003	Cronin et al.	6,733,506 B1	5/2004	McDevitt et al.
6,562,035 B1	5/2003	Levin	6,736,813 B2	5/2004	Yamauchi et al.
6,562,037 B2	5/2003	Paton et al.	6,739,872 B1	5/2004	Turri
6,565,558 B1	5/2003	Lindenmeier et al.	6,740,079 B1	5/2004	Eggers et al.
6,572,563 B2	6/2003	Ouchi	D491,666 S	6/2004	Kimmell et al.
6,572,632 B2	6/2003	Zisterer et al.	6,743,245 B2	6/2004	Lobdell
6,572,639 B1	6/2003	Ingle et al.	6,746,284 B1	6/2004	Spink, Jr.
			6,746,443 B1	6/2004	Morley et al.
			6,752,815 B2	6/2004	Beaupre
			6,755,825 B2	6/2004	Shoenman et al.
			6,761,698 B2	7/2004	Shibata et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,762,535	B2	7/2004	Take et al.	6,981,628	B2	1/2006	Wales
6,766,202	B2	7/2004	Underwood et al.	6,984,220	B2	1/2006	Wuchinich
6,770,072	B1	8/2004	Truckai et al.	6,988,295	B2	1/2006	Tillim
6,773,409	B2	8/2004	Truckai et al.	6,994,708	B2	2/2006	Manzo
6,773,435	B2	8/2004	Schulze et al.	6,994,709	B2	2/2006	Lida
6,773,443	B2	8/2004	Truwit et al.	7,000,818	B2	2/2006	Shelton, IV et al.
6,773,444	B2	8/2004	Messerly	7,001,335	B2	2/2006	Adachi et al.
6,775,575	B2	8/2004	Bommannan et al.	7,001,379	B2	2/2006	Behl et al.
6,778,023	B2	8/2004	Christensen	7,001,382	B2	2/2006	Gallo, Sr.
6,783,524	B2	8/2004	Anderson et al.	7,011,657	B2	3/2006	Truckai et al.
6,786,382	B1	9/2004	Hoffman	7,014,638	B2	3/2006	Michelson
6,786,383	B2	9/2004	Stegelmann	7,025,732	B2	4/2006	Thompson et al.
6,789,939	B2	9/2004	Schrodinger et al.	7,033,357	B2	4/2006	Baxter et al.
6,790,173	B2	9/2004	Saadat et al.	7,037,306	B2	5/2006	Podany et al.
6,790,216	B1	9/2004	Ishikawa	7,041,083	B2	5/2006	Chu et al.
6,794,027	B1	9/2004	Araki et al.	7,041,088	B2	5/2006	Nawrocki et al.
6,796,981	B2	9/2004	Wham et al.	7,041,102	B2	5/2006	Truckai et al.
D496,997	S	10/2004	Dycus et al.	7,044,949	B2	5/2006	Orszulak et al.
6,800,085	B2	10/2004	Selmon et al.	7,052,496	B2	5/2006	Yamauchi
6,802,843	B2	10/2004	Truckai et al.	7,055,731	B2	6/2006	Shelton, IV et al.
6,808,525	B2	10/2004	Latterell et al.	7,063,699	B2	6/2006	Hess et al.
6,809,508	B2	10/2004	Donofrio	7,066,893	B2	6/2006	Hibner et al.
6,810,281	B2	10/2004	Brock et al.	7,066,895	B2	6/2006	Podany
6,811,842	B1	11/2004	Ehrnsperger et al.	7,066,936	B2	6/2006	Ryan
6,814,731	B2	11/2004	Swanson	7,070,597	B2	7/2006	Truckai et al.
6,819,027	B2	11/2004	Saraf	7,074,218	B2	7/2006	Washington et al.
6,821,273	B2	11/2004	Mollenauer	7,074,219	B2	7/2006	Levine et al.
6,827,712	B2	12/2004	Tovey et al.	7,077,039	B2	7/2006	Gass et al.
6,828,712	B2	12/2004	Battaglin et al.	7,077,845	B2	7/2006	Hacker et al.
6,835,082	B2	12/2004	Gonnering	7,077,853	B2	7/2006	Kramer et al.
6,835,199	B2	12/2004	McGuckin, Jr. et al.	7,083,618	B2	8/2006	Couture et al.
6,840,938	B1	1/2005	Morley et al.	7,083,619	B2	8/2006	Truckai et al.
6,843,789	B2	1/2005	Goble	7,087,054	B2	8/2006	Truckai et al.
6,849,073	B2	2/2005	Hoey et al.	7,090,672	B2	8/2006	Underwood et al.
6,860,878	B2	3/2005	Brock	7,094,235	B2	8/2006	Francischelli
6,860,880	B2	3/2005	Treat et al.	7,101,371	B2	9/2006	Dycus et al.
6,863,676	B2	3/2005	Lee et al.	7,101,372	B2	9/2006	Dycus et al.
6,866,671	B2	3/2005	Tierney et al.	7,101,373	B2	9/2006	Dycus et al.
6,869,439	B2	3/2005	White et al.	7,101,378	B2	9/2006	Salameh et al.
6,875,220	B2	4/2005	Du et al.	7,104,834	B2	9/2006	Robinson et al.
6,877,647	B2	4/2005	Green et al.	7,108,695	B2	9/2006	Witt et al.
6,882,439	B2	4/2005	Ishijima	7,111,769	B2	9/2006	Wales et al.
6,887,209	B2	5/2005	Kadziauskas et al.	7,112,201	B2	9/2006	Truckai et al.
6,887,252	B1	5/2005	Okada et al.	D531,311	S	10/2006	Guerra et al.
6,893,435	B2	5/2005	Goble	7,117,034	B2	10/2006	Kronberg
6,898,536	B2	5/2005	Wiener et al.	7,118,564	B2	10/2006	Ritchie et al.
6,899,685	B2	5/2005	Kernode et al.	7,118,570	B2	10/2006	Tetzlaff et al.
6,905,497	B2	6/2005	Truckai et al.	7,124,932	B2	10/2006	Isaacson et al.
6,908,463	B2	6/2005	Treat et al.	7,125,409	B2	10/2006	Truckai et al.
6,908,472	B2	6/2005	Wiener et al.	7,128,720	B2	10/2006	Podany
6,913,579	B2	7/2005	Truckai et al.	7,131,860	B2	11/2006	Sartor et al.
6,915,623	B2	7/2005	Dey et al.	7,131,970	B2	11/2006	Moses et al.
6,923,804	B2	8/2005	Eggers et al.	7,135,018	B2	11/2006	Ryan et al.
6,923,806	B2	8/2005	Hooven et al.	7,135,030	B2	11/2006	Schwemberger et al.
6,926,712	B2	8/2005	Phan	7,137,980	B2	11/2006	Buyse et al.
6,926,716	B2	8/2005	Baker et al.	7,143,925	B2	12/2006	Shelton, IV et al.
6,926,717	B1	8/2005	Garito et al.	7,144,403	B2	12/2006	Booth
6,929,602	B2	8/2005	Hirakui et al.	7,147,138	B2	12/2006	Shelton, IV
6,929,622	B2	8/2005	Chian	7,153,315	B2	12/2006	Miller
6,929,632	B2	8/2005	Nita et al.	D536,093	S	1/2007	Nakajima et al.
6,929,644	B2	8/2005	Truckai et al.	7,156,189	B1	1/2007	Bar-Cohen et al.
6,933,656	B2	8/2005	Matsushita et al.	7,156,846	B2	1/2007	Dycus et al.
D509,589	S	9/2005	Wells	7,156,853	B2	1/2007	Muratsu
6,942,660	B2	9/2005	Pantera et al.	7,157,058	B2	1/2007	Marhasin et al.
6,942,677	B2	9/2005	Nita et al.	7,159,750	B2	1/2007	Racenet et al.
6,945,981	B2	9/2005	Donofrio et al.	7,160,296	B2	1/2007	Pearson et al.
6,946,779	B2	9/2005	Birgel	7,160,298	B2	1/2007	Lawes et al.
6,948,503	B2	9/2005	Refior et al.	7,160,299	B2	1/2007	Baily
6,953,461	B2	10/2005	McClurken et al.	7,163,548	B2	1/2007	Stulen et al.
D511,145	S	11/2005	Donofrio et al.	7,169,144	B2	1/2007	Hoey et al.
6,974,450	B2	12/2005	Weber et al.	7,169,146	B2	1/2007	Truckai et al.
6,976,844	B2	12/2005	Hickok et al.	7,169,156	B2	1/2007	Hart
6,976,969	B2	12/2005	Messerly	7,179,254	B2	2/2007	Pendekanti et al.
6,977,495	B2	12/2005	Donofrio	7,179,271	B2	2/2007	Friedman et al.
6,979,332	B2	12/2005	Adams	7,186,253	B2	3/2007	Truckai et al.
				7,189,233	B2	3/2007	Truckai et al.
				7,195,631	B2	3/2007	Dumbauld
				D541,418	S	4/2007	Schechter et al.
				7,198,635	B2	4/2007	Danek et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,204,820 B2	4/2007	Akahoshi	7,422,582 B2	9/2008	Malackowski et al.
7,207,471 B2	4/2007	Heinrich et al.	D578,643 S	10/2008	Shumer et al.
7,207,997 B2	4/2007	Shipp et al.	D578,644 S	10/2008	Shumer et al.
7,210,881 B2	5/2007	Greenberg	D578,645 S	10/2008	Shumer et al.
7,211,079 B2	5/2007	Treat	7,431,704 B2	10/2008	Babaev
7,217,128 B2	5/2007	Atkin et al.	7,431,720 B2	10/2008	Pendekanti et al.
7,217,269 B2	5/2007	Ei-Galley et al.	7,435,582 B2	10/2008	Zimmermann et al.
7,220,951 B2	5/2007	Truckai et al.	7,441,684 B2	10/2008	Shelton, IV et al.
7,223,229 B2	5/2007	Inman et al.	7,442,193 B2	10/2008	Shields et al.
7,225,964 B2	6/2007	Mastri et al.	7,445,621 B2	11/2008	Dumbauld et al.
7,226,448 B2	6/2007	Bertolero et al.	7,455,208 B2	11/2008	Wales et al.
7,229,455 B2	6/2007	Sakurai et al.	7,462,181 B2	12/2008	Kraft et al.
7,232,440 B2	6/2007	Dumbauld et al.	7,464,846 B2	12/2008	Shelton, IV et al.
7,235,071 B2	6/2007	Gonnering	7,472,815 B2	1/2009	Shelton, IV et al.
7,235,073 B2	6/2007	Levine et al.	7,473,145 B2	1/2009	Ehr et al.
7,241,294 B2	7/2007	Reschke	7,473,253 B2	1/2009	Dycus et al.
7,244,262 B2	7/2007	Wiener et al.	7,473,263 B2	1/2009	Johnston et al.
7,251,531 B2	7/2007	Mosher et al.	7,479,148 B2	1/2009	Beaupre
7,252,641 B2	8/2007	Thompson et al.	7,479,160 B2	1/2009	Branch et al.
7,252,667 B2	8/2007	Moses et al.	7,481,775 B2	1/2009	Weikel, Jr. et al.
7,258,688 B1	8/2007	Shah et al.	7,488,285 B2	2/2009	Honda et al.
7,267,677 B2	9/2007	Johnson et al.	7,488,319 B2	2/2009	Yates
7,267,685 B2	9/2007	Butaric et al.	7,491,201 B2	2/2009	Shields et al.
7,269,873 B2	9/2007	Brewer et al.	7,494,468 B2	2/2009	Rabiner et al.
7,273,483 B2	9/2007	Wiener et al.	7,494,501 B2	2/2009	Ahlberg et al.
D552,241 S	10/2007	Bromley et al.	7,498,080 B2	3/2009	Tung et al.
7,282,048 B2	10/2007	Goble et al.	7,502,234 B2	3/2009	Goliszek et al.
7,285,895 B2	10/2007	Beaupre	7,503,893 B2	3/2009	Kucklick
7,287,682 B1	10/2007	Ezzat et al.	7,503,895 B2	3/2009	Rabiner et al.
7,297,149 B2	11/2007	Vitali et al.	7,506,790 B2	3/2009	Shelton, IV
7,300,431 B2	11/2007	Dubrovsky	7,506,791 B2	3/2009	Omaits et al.
7,300,435 B2	11/2007	Wham et al.	7,510,107 B2	3/2009	Timm et al.
7,300,446 B2	11/2007	Beaupre	7,513,025 B2	4/2009	Fischer
7,300,450 B2	11/2007	Vleugels et al.	7,517,349 B2	4/2009	Truckai et al.
7,303,531 B2	12/2007	Lee et al.	7,524,320 B2	4/2009	Tierney et al.
7,303,557 B2	12/2007	Wham et al.	7,530,986 B2	5/2009	Beaupre et al.
7,306,597 B2	12/2007	Manzo	7,534,243 B1	5/2009	Chin et al.
7,307,313 B2	12/2007	Ohyanagi et al.	7,535,233 B2	5/2009	Kojovic et al.
7,309,849 B2	12/2007	Truckai et al.	D594,983 S	6/2009	Price et al.
7,311,706 B2	12/2007	Schoenman et al.	7,540,871 B2	6/2009	Gonnering
7,311,709 B2	12/2007	Truckai et al.	7,540,872 B2	6/2009	Schechter et al.
7,317,955 B2	1/2008	McGreevy	7,543,730 B1	6/2009	Marczyk
7,318,831 B2	1/2008	Alvarez et al.	7,544,200 B2	6/2009	Houser
7,326,236 B2	2/2008	Andreas et al.	7,549,564 B2	6/2009	Boudreaux
7,329,257 B2	2/2008	Kanehira et al.	7,550,216 B2	6/2009	Ofer et al.
7,331,410 B2	2/2008	Yong et al.	7,553,309 B2	6/2009	Buyse et al.
7,335,165 B2	2/2008	Truwit et al.	7,554,343 B2	6/2009	Bromfield
7,335,997 B2	2/2008	Wiener	7,559,450 B2	7/2009	Wales et al.
7,337,010 B2	2/2008	Howard et al.	7,559,452 B2	7/2009	Wales et al.
7,353,068 B2	4/2008	Tanaka et al.	7,566,318 B2	7/2009	Haefner
7,354,440 B2	4/2008	Truckal et al.	7,567,012 B2	7/2009	Namikawa
7,357,287 B2	4/2008	Shelton, IV et al.	7,568,603 B2	8/2009	Shelton, IV et al.
7,357,802 B2	4/2008	Palanker et al.	7,569,057 B2	8/2009	Liu et al.
7,361,172 B2	4/2008	Cimino	7,572,266 B2	8/2009	Young et al.
7,364,577 B2	4/2008	Wham et al.	7,572,268 B2	8/2009	Babaev
7,367,976 B2	5/2008	Lawes et al.	7,578,820 B2	8/2009	Moore et al.
7,371,227 B2	5/2008	Zeiner	7,582,084 B2	9/2009	Swanson et al.
RE40,388 E	6/2008	Gines	7,582,086 B2	9/2009	Privitera et al.
7,380,695 B2	6/2008	Doll et al.	7,582,087 B2	9/2009	Tetzlaff et al.
7,380,696 B2	6/2008	Shelton, IV et al.	7,582,095 B2	9/2009	Shipp et al.
7,381,209 B2	6/2008	Truckai et al.	7,585,181 B2	9/2009	Olsen
7,384,420 B2	6/2008	Dycus et al.	7,586,289 B2	9/2009	Andruk et al.
7,390,317 B2	6/2008	Taylor et al.	7,587,536 B2	9/2009	McLeod
7,396,356 B2	7/2008	Mollenauer	7,588,176 B2	9/2009	Timm et al.
7,403,224 B2	7/2008	Fuller et al.	7,594,925 B2	9/2009	Danek et al.
7,404,508 B2	7/2008	Smith et al.	7,597,693 B2	10/2009	Garrison
7,407,077 B2	8/2008	Ortiz et al.	7,601,119 B2	10/2009	Shahinian
7,408,288 B2	8/2008	Hara	7,601,136 B2	10/2009	Akahoshi
7,412,008 B2	8/2008	Lliev	7,604,150 B2	10/2009	Boudreaux
7,416,101 B2	8/2008	Shelton, IV et al.	7,607,557 B2	10/2009	Shelton, IV et al.
7,416,437 B2	8/2008	Sartor et al.	7,621,930 B2	11/2009	Houser
D576,725 S	9/2008	Shumer et al.	7,628,791 B2	12/2009	Garrison et al.
7,419,490 B2	9/2008	Falkenstein et al.	7,628,792 B2	12/2009	Guerra
7,422,139 B2	9/2008	Shelton, IV et al.	7,632,267 B2	12/2009	Dahla
7,422,463 B2	9/2008	Kuo	7,632,269 B2	12/2009	Truckai et al.
			7,641,653 B2	1/2010	Dalla Betta et al.
			7,641,671 B2	1/2010	Crainich
			7,644,848 B2	1/2010	Swayze et al.
			7,645,240 B2	1/2010	Thompson et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,645,277	B2	1/2010	McClurken et al.	7,811,283	B2	10/2010	Moses et al.
7,645,278	B2	1/2010	Ichihashi et al.	7,815,641	B2	10/2010	Dodde et al.
7,648,499	B2	1/2010	Orszulak et al.	7,819,298	B2	10/2010	Hall et al.
7,654,431	B2	2/2010	Hueil et al.	7,819,299	B2	10/2010	Shelton, IV et al.
7,655,003	B2	2/2010	Lorang et al.	7,819,819	B2	10/2010	Quick et al.
7,658,311	B2	2/2010	Boudreaux	7,819,872	B2	10/2010	Johnson et al.
7,659,833	B2	2/2010	Warner et al.	7,821,143	B2	10/2010	Wiener
7,662,151	B2	2/2010	Crompton, Jr. et al.	D627,066	S	11/2010	Romero
7,665,647	B2	2/2010	Shelton, IV et al.	7,824,401	B2	11/2010	Manzo et al.
7,666,206	B2	2/2010	Taniguchi et al.	7,832,408	B2	11/2010	Shelton, IV et al.
7,667,592	B2	2/2010	Ohyama et al.	7,832,611	B2	11/2010	Boyden et al.
7,670,334	B2	3/2010	Hueil et al.	7,832,612	B2	11/2010	Baxter, III et al.
7,670,338	B2	3/2010	Albrecht et al.	7,834,484	B2	11/2010	Sartor
7,674,263	B2	3/2010	Ryan	7,837,699	B2	11/2010	Yamada et al.
7,678,069	B1	3/2010	Baker et al.	7,845,537	B2	12/2010	Shelton, IV et al.
7,678,105	B2	3/2010	McGreevy et al.	7,846,155	B2	12/2010	Houser et al.
7,678,125	B2	3/2010	Shipp	7,846,159	B2	12/2010	Morrison et al.
7,682,366	B2	3/2010	Sakurai et al.	7,846,160	B2	12/2010	Payne et al.
7,686,770	B2	3/2010	Cohen	7,846,161	B2	12/2010	Dumbauld et al.
7,686,826	B2	3/2010	Lee et al.	7,854,735	B2	12/2010	Houser et al.
7,688,028	B2	3/2010	Phillips et al.	D631,155	S	1/2011	Peine et al.
7,691,095	B2	4/2010	Bednarek et al.	7,861,906	B2	1/2011	Doll et al.
7,691,098	B2	4/2010	Wallace et al.	7,862,560	B2	1/2011	Marion
7,699,846	B2	4/2010	Ryan	7,871,392	B2	1/2011	Sartor
7,703,459	B2	4/2010	Saadat et al.	7,876,030	B2	1/2011	Taki et al.
7,703,653	B2	4/2010	Shah et al.	D631,965	S	2/2011	Price et al.
7,708,735	B2	5/2010	Chapman et al.	7,877,852	B2	2/2011	Unger et al.
7,708,751	B2	5/2010	Hughes et al.	7,878,991	B2	2/2011	Babaev
7,708,768	B2	5/2010	Danek et al.	7,879,033	B2	2/2011	Sartor et al.
7,713,202	B2	5/2010	Boukhny et al.	7,879,035	B2	2/2011	Garrison et al.
7,714,481	B2	5/2010	Sakai	7,879,070	B2	2/2011	Ortiz et al.
7,717,312	B2	5/2010	Beetel	7,892,606	B2	2/2011	Thies et al.
7,717,915	B2	5/2010	Miyazawa	7,896,875	B2	3/2011	Heim et al.
7,721,935	B2	5/2010	Racenet et al.	7,897,792	B2	3/2011	Iikura et al.
7,722,527	B2	5/2010	Bouchier et al.	7,901,400	B2	3/2011	Wham et al.
7,722,607	B2	5/2010	Dumbauld et al.	7,901,423	B2	3/2011	Stulen et al.
D618,797	S	6/2010	Price et al.	7,905,881	B2	3/2011	Masuda et al.
7,726,537	B2	6/2010	Olson et al.	7,909,220	B2	3/2011	Viola
7,727,177	B2	6/2010	Bayat	7,909,820	B2	3/2011	Lipson et al.
7,738,969	B2	6/2010	Bleich	7,909,824	B2	3/2011	Masuda et al.
7,740,594	B2	6/2010	Hibner	7,918,848	B2	4/2011	Lau et al.
7,751,115	B2	7/2010	Song	7,919,184	B2	4/2011	Mohapatra et al.
7,753,904	B2	7/2010	Shelton, IV et al.	7,922,061	B2	4/2011	Shelton, IV et al.
7,753,908	B2	7/2010	Swanson	7,922,651	B2	4/2011	Yamada et al.
7,762,445	B2	7/2010	Heinrich et al.	7,931,649	B2	4/2011	Couture et al.
D621,503	S	8/2010	Otten et al.	D637,288	S	5/2011	Houghton
7,766,210	B2	8/2010	Shelton, IV et al.	D638,540	S	5/2011	Ijiri et al.
7,766,693	B2	8/2010	Sartor et al.	7,935,114	B2	5/2011	Takashino et al.
7,766,910	B2	8/2010	Hixson et al.	7,936,203	B2	5/2011	Zimlich
7,768,510	B2	8/2010	Tsai et al.	7,951,095	B2	5/2011	Makin et al.
7,770,774	B2	8/2010	Mastri et al.	7,951,165	B2	5/2011	Golden et al.
7,770,775	B2	8/2010	Shelton, IV et al.	7,955,331	B2	6/2011	Truckai et al.
7,771,425	B2	8/2010	Dycus et al.	7,956,620	B2	6/2011	Gilbert
7,771,444	B2	8/2010	Patel et al.	7,959,050	B2	6/2011	Smith et al.
7,775,972	B2	8/2010	Brock et al.	7,959,626	B2	6/2011	Hong et al.
7,776,036	B2	8/2010	Schechter et al.	7,963,963	B2	6/2011	Francischelli et al.
7,776,037	B2	8/2010	Odom	7,967,602	B2	6/2011	Lindquist
7,778,733	B2	8/2010	Nowlin et al.	7,972,328	B2	7/2011	Wham et al.
7,780,054	B2	8/2010	Wales	7,972,329	B2	7/2011	Refior et al.
7,780,593	B2	8/2010	Ueno et al.	7,976,544	B2	7/2011	McClurken et al.
7,780,651	B2	8/2010	Madhani et al.	7,980,443	B2	7/2011	Scheib et al.
7,780,659	B2	8/2010	Okada et al.	7,981,050	B2	7/2011	Ritchart et al.
7,780,663	B2	8/2010	Yates et al.	7,981,113	B2	7/2011	Truckai et al.
7,784,662	B2	8/2010	Wales et al.	7,997,278	B2	8/2011	Uitley et al.
7,784,663	B2	8/2010	Shelton, IV	7,998,157	B2	8/2011	Culp et al.
7,789,883	B2	9/2010	Takashino et al.	8,020,743	B2	9/2011	Shelton, IV
7,793,814	B2	9/2010	Racenet et al.	8,028,885	B2	10/2011	Smith et al.
7,796,969	B2	9/2010	Kelly et al.	8,033,173	B2	10/2011	Ehlert et al.
7,798,386	B2	9/2010	Schall et al.	8,038,693	B2	10/2011	Allen
7,799,020	B2	9/2010	Shores et al.	8,048,070	B2	11/2011	O'Brien et al.
7,799,045	B2	9/2010	Masuda	8,052,672	B2	11/2011	Laufer et al.
7,803,152	B2	9/2010	Honda et al.	8,056,720	B2	11/2011	Hawkes
7,803,156	B2	9/2010	Eder et al.	8,056,787	B2	11/2011	Boudreaux et al.
7,806,891	B2	10/2010	Nowlin et al.	8,057,468	B2	11/2011	Konesky
7,810,693	B2	10/2010	Broehl et al.	8,057,498	B2	11/2011	Robertson
				8,058,771	B2	11/2011	Giordano et al.
				8,061,014	B2	11/2011	Smith et al.
				8,066,167	B2	11/2011	Measamer et al.
				8,070,036	B1	12/2011	Knodel

(56)

References Cited

U.S. PATENT DOCUMENTS

8,070,711	B2	12/2011	Bassinger et al.	8,287,485	B2	10/2012	Kimura et al.
8,070,762	B2	12/2011	Escudero et al.	8,287,528	B2	10/2012	Wham et al.
8,075,555	B2	12/2011	Truckai et al.	8,287,532	B2	10/2012	Carroll et al.
8,075,558	B2	12/2011	Truckai et al.	8,292,886	B2	10/2012	Kerr et al.
8,089,197	B2	1/2012	Rinner et al.	8,292,888	B2	10/2012	Whitman
8,092,475	B2	1/2012	Cotter et al.	8,292,905	B2	10/2012	Taylor et al.
8,096,459	B2	1/2012	Ortiz et al.	8,298,223	B2	10/2012	Wham et al.
8,097,012	B2	1/2012	Kagarise	8,298,225	B2	10/2012	Gilbert
8,100,894	B2	1/2012	Mucko et al.	8,298,232	B2	10/2012	Unger
8,105,323	B2	1/2012	Buyse et al.	8,298,233	B2	10/2012	Mueller
8,114,104	B2	2/2012	Young et al.	8,303,576	B2	11/2012	Brock
8,118,276	B2	2/2012	Sanders et al.	8,303,579	B2	11/2012	Shibata
8,128,624	B2	3/2012	Couture et al.	8,303,580	B2	11/2012	Wham et al.
8,133,218	B2	3/2012	Daw et al.	8,303,583	B2	11/2012	Hosier et al.
8,136,712	B2	3/2012	Zingman	8,303,613	B2	11/2012	Crandall et al.
8,141,762	B2	3/2012	Bedi et al.	8,306,629	B2	11/2012	Mioduski et al.
8,142,421	B2	3/2012	Cooper et al.	8,308,040	B2	11/2012	Huang et al.
8,142,461	B2	3/2012	Houser et al.	8,319,400	B2	11/2012	Houser et al.
8,147,485	B2	4/2012	Wham et al.	8,323,302	B2	12/2012	Robertson et al.
8,147,508	B2	4/2012	Madan et al.	8,323,310	B2	12/2012	Kingsley
8,152,801	B2	4/2012	Goldberg et al.	8,328,761	B2	12/2012	Widenhouse et al.
8,152,825	B2	4/2012	Madan et al.	8,328,802	B2	12/2012	Deville et al.
8,157,145	B2	4/2012	Shelton, IV et al.	8,328,833	B2	12/2012	Cuny
8,161,977	B2	4/2012	Shelton, IV et al.	8,328,834	B2	12/2012	Isaacs et al.
8,162,966	B2	4/2012	Connor et al.	8,333,778	B2	12/2012	Smith et al.
8,172,846	B2	5/2012	Brunnett et al.	8,333,779	B2	12/2012	Smith et al.
8,172,870	B2	5/2012	Shipp	8,334,468	B2	12/2012	Palmer et al.
8,177,800	B2	5/2012	Spitz et al.	8,334,635	B2	12/2012	Voegelé et al.
8,182,502	B2	5/2012	Stulen et al.	8,337,407	B2	12/2012	Quistgaard et al.
8,186,560	B2	5/2012	Hess et al.	8,338,726	B2	12/2012	Palmer et al.
8,186,877	B2	5/2012	Klimovitch et al.	8,344,596	B2	1/2013	Nield et al.
8,187,267	B2	5/2012	Pappone et al.	8,348,880	B2	1/2013	Messerly et al.
D661,801	S	6/2012	Price et al.	8,348,947	B2	1/2013	Takashino et al.
D661,802	S	6/2012	Price et al.	8,348,967	B2	1/2013	Stulen
D661,803	S	6/2012	Price et al.	8,357,103	B2	1/2013	Mark et al.
D661,804	S	6/2012	Price et al.	8,357,149	B2	1/2013	Govari et al.
8,197,472	B2	6/2012	Lau et al.	8,357,158	B2	1/2013	McKenna et al.
8,197,479	B2	6/2012	Olson et al.	8,361,066	B2	1/2013	Long et al.
8,197,502	B2	6/2012	Smith et al.	8,361,072	B2	1/2013	Dumbauld et al.
8,207,651	B2	6/2012	Gilbert	8,361,569	B2	1/2013	Saito et al.
8,210,411	B2	7/2012	Yates et al.	8,366,727	B2	2/2013	Witt et al.
8,221,415	B2	7/2012	Francischelli	8,372,064	B2	2/2013	Douglass et al.
8,226,580	B2	7/2012	Govari et al.	8,372,099	B2	2/2013	Deville et al.
8,226,675	B2	7/2012	Houser et al.	8,372,101	B2	2/2013	Smith et al.
8,231,607	B2	7/2012	Takuma	8,372,102	B2	2/2013	Stulen et al.
8,235,917	B2	8/2012	Joseph et al.	8,374,670	B2	2/2013	Selkee
8,236,018	B2	8/2012	Yoshimine et al.	8,377,044	B2	2/2013	Coe et al.
8,236,019	B2	8/2012	Houser	8,377,059	B2	2/2013	Deville et al.
8,236,020	B2	8/2012	Smith et al.	8,377,085	B2	2/2013	Smith et al.
8,241,235	B2	8/2012	Kahler et al.	8,382,748	B2	2/2013	Geisel
8,241,271	B2	8/2012	Millman et al.	8,382,775	B1	2/2013	Bender et al.
8,241,282	B2	8/2012	Unger et al.	8,382,782	B2	2/2013	Robertson et al.
8,241,283	B2	8/2012	Guerra et al.	8,382,792	B2	2/2013	Chojin
8,241,284	B2	8/2012	Dycus et al.	8,397,971	B2	3/2013	Yates et al.
8,241,312	B2	8/2012	Messerly	8,403,945	B2	3/2013	Whitfield et al.
8,246,575	B2	8/2012	Viola	8,403,948	B2	3/2013	Deville et al.
8,246,615	B2	8/2012	Behnke	8,403,949	B2	3/2013	Palmer et al.
8,246,616	B2	8/2012	Amoah et al.	8,403,950	B2	3/2013	Palmer et al.
8,246,618	B2	8/2012	Bucciaglia et al.	8,409,234	B2	4/2013	Stahler et al.
8,251,994	B2	8/2012	McKenna et al.	8,414,577	B2	4/2013	Boudreaux et al.
8,252,012	B2	8/2012	Stulen	8,418,073	B2	4/2013	Mohr et al.
8,253,303	B2	8/2012	Giordano et al.	8,418,349	B2	4/2013	Smith et al.
8,257,377	B2	9/2012	Wiener et al.	8,419,757	B2	4/2013	Smith et al.
8,257,387	B2	9/2012	Cunningham	8,419,758	B2	4/2013	Smith et al.
8,262,563	B2	9/2012	Bakos et al.	8,419,759	B2	4/2013	Dietz
8,267,300	B2	9/2012	Boudreaux	8,423,182	B2	4/2013	Robinson et al.
8,267,935	B2	9/2012	Couture et al.	8,425,410	B2	4/2013	Murray et al.
8,273,087	B2	9/2012	Kimura et al.	8,425,545	B2	4/2013	Smith et al.
D669,992	S	10/2012	Schafer et al.	8,430,811	B2	4/2013	Hess et al.
D669,993	S	10/2012	Merchant et al.	8,430,876	B2	4/2013	Kappus et al.
8,277,446	B2	10/2012	Heard	8,430,897	B2	4/2013	Novak et al.
8,277,447	B2	10/2012	Garrison et al.	8,430,898	B2	4/2013	Wiener et al.
8,277,471	B2	10/2012	Wiener et al.	8,435,257	B2	5/2013	Smith et al.
8,282,669	B2	10/2012	Gerber et al.	8,439,912	B2	5/2013	Cunningham et al.
8,286,846	B2	10/2012	Smith et al.	8,439,939	B2	5/2013	Deville et al.
				8,444,637	B2	5/2013	Podmore et al.
				8,444,662	B2	5/2013	Palmer et al.
				8,444,664	B2	5/2013	Balanév et al.
				8,453,906	B2	6/2013	Huang et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,454,639 B2	6/2013	Du et al.	8,628,529 B2	1/2014	Aldridge et al.
8,459,525 B2	6/2013	Yates et al.	8,632,461 B2	1/2014	Glossop
8,460,284 B2	6/2013	Aronow et al.	8,638,428 B2	1/2014	Brown
8,460,288 B2	6/2013	Tamai et al.	8,640,788 B2	2/2014	Dachs, II et al.
8,460,292 B2	6/2013	Truckai et al.	8,647,350 B2	2/2014	Mohan et al.
8,461,744 B2	6/2013	Wiener et al.	8,650,728 B2	2/2014	Wan et al.
8,469,981 B2	6/2013	Robertson et al.	8,652,120 B2	2/2014	Giordano et al.
8,479,969 B2	7/2013	Shelton, IV	8,652,132 B2	2/2014	Tsuchiya et al.
8,480,703 B2	7/2013	Nicholas et al.	8,652,155 B2	2/2014	Houser et al.
8,484,833 B2	7/2013	Cunningham et al.	8,657,489 B2	2/2014	Ladurner et al.
8,485,413 B2	7/2013	Scheib et al.	8,659,208 B1	2/2014	Rose et al.
8,485,970 B2	7/2013	Widenhouse et al.	8,663,220 B2	3/2014	Wiener et al.
8,486,057 B2	7/2013	Behnke, II	8,663,222 B2	3/2014	Anderson et al.
8,486,096 B2	7/2013	Robertson et al.	8,663,223 B2	3/2014	Masuda et al.
8,491,578 B2	7/2013	Manwaring et al.	8,663,262 B2	3/2014	Smith et al.
8,491,625 B2	7/2013	Homer	8,668,691 B2	3/2014	Heard
8,496,682 B2	7/2013	Guerra et al.	8,668,710 B2	3/2014	Slipszenko et al.
D687,549 S	8/2013	Johnson et al.	8,684,253 B2	4/2014	Giordano et al.
8,506,555 B2	8/2013	Ruiz Morales	8,685,016 B2	4/2014	Wham et al.
8,509,318 B2	8/2013	Tailliet	8,685,020 B2	4/2014	Weizman et al.
8,512,336 B2	8/2013	Couture	8,690,582 B2	4/2014	Rohrbach et al.
8,512,359 B2	8/2013	Whitman et al.	8,696,366 B2	4/2014	Chen et al.
8,512,364 B2	8/2013	Kowalski et al.	8,696,665 B2	4/2014	Hunt et al.
8,512,365 B2	8/2013	Wiener et al.	8,696,666 B2	4/2014	Sanai et al.
8,518,067 B2	8/2013	Masuda et al.	8,702,609 B2	4/2014	Hadjicostis
8,521,331 B2	8/2013	Itkowitz	8,702,704 B2	4/2014	Shelton, IV et al.
8,523,882 B2	9/2013	Huitema et al.	8,704,425 B2	4/2014	Giordano et al.
8,523,889 B2	9/2013	Stulen et al.	8,708,213 B2	4/2014	Shelton, IV et al.
8,528,563 B2	9/2013	Gruber	8,709,031 B2	4/2014	Stulen
8,529,437 B2	9/2013	Taylor et al.	8,709,035 B2	4/2014	Johnson et al.
8,529,565 B2	9/2013	Masuda et al.	8,715,270 B2	5/2014	Weitzner et al.
8,531,064 B2	9/2013	Robertson et al.	8,715,277 B2	5/2014	Weizman
8,535,311 B2	9/2013	Schall	8,721,640 B2	5/2014	Taylor et al.
8,535,340 B2	9/2013	Allen	8,721,657 B2	5/2014	Kondoh et al.
8,535,341 B2	9/2013	Allen	8,734,443 B2	5/2014	Hixson et al.
8,540,128 B2	9/2013	Shelton, IV et al.	8,747,238 B2	6/2014	Shelton, IV et al.
8,546,996 B2	10/2013	Messerly et al.	8,747,351 B2	6/2014	Schultz
8,546,999 B2	10/2013	Houser et al.	8,747,404 B2	6/2014	Boudreaux et al.
8,551,077 B2	10/2013	Main et al.	8,749,116 B2	6/2014	Messerly et al.
8,551,086 B2	10/2013	Kimura et al.	8,752,264 B2	6/2014	Ackley et al.
8,562,592 B2	10/2013	Conlon et al.	8,752,749 B2	6/2014	Moore et al.
8,562,598 B2	10/2013	Falkenstein et al.	8,753,338 B2	6/2014	Widenhouse et al.
8,562,600 B2	10/2013	Kirkpatrick et al.	8,754,570 B2	6/2014	Voegelé et al.
8,562,604 B2	10/2013	Nishimura	8,758,342 B2	6/2014	Bales et al.
8,568,390 B2	10/2013	Mueller	8,758,352 B2	6/2014	Cooper et al.
8,568,400 B2	10/2013	Gilbert	8,764,735 B2	7/2014	Coe et al.
8,568,412 B2	10/2013	Brandt et al.	8,764,747 B2	7/2014	Cummings et al.
8,569,997 B2	10/2013	Lee	8,767,970 B2	7/2014	Eppolito
8,573,461 B2	11/2013	Shelton, IV et al.	8,770,459 B2	7/2014	Racenet et al.
8,573,465 B2	11/2013	Shelton, IV	8,771,269 B2	7/2014	Sherman et al.
8,574,231 B2	11/2013	Boudreaux et al.	8,771,270 B2	7/2014	Burbank
8,574,253 B2	11/2013	Gruber et al.	8,771,293 B2	7/2014	Surti et al.
8,579,176 B2	11/2013	Smith et al.	8,773,001 B2	7/2014	Wiener et al.
8,579,897 B2	11/2013	Vakharia et al.	8,777,944 B2	7/2014	Frankhouser et al.
8,579,928 B2	11/2013	Robertson et al.	8,779,648 B2	7/2014	Giordano et al.
8,585,727 B2	11/2013	Polo	8,783,541 B2	7/2014	Shelton, IV et al.
8,588,371 B2	11/2013	Ogawa et al.	8,784,415 B2	7/2014	Malackowski et al.
8,591,459 B2	11/2013	Clymer et al.	8,784,418 B2	7/2014	Romero
8,591,506 B2	11/2013	Wham et al.	8,790,342 B2	7/2014	Stulen et al.
8,591,536 B2	11/2013	Robertson	8,795,274 B2	8/2014	Hanna
D695,407 S	12/2013	Price et al.	8,795,276 B2	8/2014	Dietz et al.
D696,631 S	12/2013	Price et al.	8,795,327 B2	8/2014	Dietz et al.
8,597,193 B2	12/2013	Grunwald et al.	8,800,838 B2	8/2014	Shelton, IV
8,602,031 B2	12/2013	Reis et al.	8,801,710 B2	8/2014	Ullrich et al.
8,602,288 B2	12/2013	Shelton, IV et al.	8,808,204 B2	8/2014	Irisawa et al.
8,603,089 B2	12/2013	Viola	8,808,319 B2	8/2014	Houser et al.
8,608,044 B2	12/2013	Hueil et al.	8,814,856 B2	8/2014	Elmouelhi et al.
8,608,745 B2	12/2013	Guzman et al.	8,814,870 B2	8/2014	Paraschiv et al.
8,613,383 B2	12/2013	Beckman et al.	8,820,605 B2	9/2014	Shelton, IV
8,616,431 B2	12/2013	Timm et al.	8,821,388 B2	9/2014	Naito et al.
8,622,274 B2	1/2014	Yates et al.	8,827,992 B2	9/2014	Koss et al.
8,623,011 B2	1/2014	Spivey	8,834,466 B2	9/2014	Cummings et al.
8,623,016 B2	1/2014	Fischer	8,834,518 B2	9/2014	Faller et al.
8,623,027 B2	1/2014	Price et al.	8,844,789 B2	9/2014	Shelton, IV et al.
8,623,044 B2	1/2014	Timm et al.	8,845,537 B2	9/2014	Tanaka et al.
			8,845,630 B2	9/2014	Mehta et al.
			8,848,808 B2	9/2014	Dress
			8,851,354 B2	10/2014	Swensgard et al.
			8,852,184 B2	10/2014	Kucklick

(56)

References Cited

U.S. PATENT DOCUMENTS

8,858,547 B2	10/2014	Brogna	9,050,093 B2	6/2015	Aldridge et al.
8,862,955 B2	10/2014	Cesari	9,050,098 B2	6/2015	Deville et al.
8,864,749 B2	10/2014	Okada	9,050,123 B2	6/2015	Krause et al.
8,864,757 B2	10/2014	Klimovitch et al.	9,050,124 B2	6/2015	Houser
8,864,761 B2	10/2014	Johnson et al.	9,055,961 B2	6/2015	Manzo et al.
8,870,865 B2	10/2014	Frankhouser et al.	9,059,547 B2	6/2015	McLawhorn
8,876,726 B2	11/2014	Amit et al.	9,060,770 B2	6/2015	Shelton, IV et al.
8,876,858 B2	11/2014	Braun	9,060,775 B2	6/2015	Wiener et al.
8,882,766 B2	11/2014	Couture et al.	9,060,776 B2	6/2015	Yates et al.
8,882,791 B2	11/2014	Stulen	9,066,723 B2	6/2015	Beller et al.
8,888,776 B2	11/2014	Dietz et al.	9,066,747 B2	6/2015	Robertson
8,888,783 B2	11/2014	Young	9,072,523 B2	7/2015	Houser et al.
8,888,809 B2	11/2014	Davison et al.	9,072,535 B2	7/2015	Shelton, IV et al.
8,899,462 B2	12/2014	Kostrzewski et al.	9,072,536 B2	7/2015	Shelton, IV et al.
8,900,259 B2	12/2014	Houser et al.	9,072,539 B2	7/2015	Messerly et al.
8,906,016 B2	12/2014	Boudreaux et al.	9,084,624 B2	7/2015	Larkin et al.
8,906,017 B2	12/2014	Rioux et al.	9,089,327 B2	7/2015	Worrell et al.
8,911,438 B2	12/2014	Swoyer et al.	9,089,360 B2	7/2015	Messerly et al.
8,911,460 B2	12/2014	Neurohr et al.	9,095,362 B2	8/2015	Dachs, II et al.
8,920,412 B2	12/2014	Fritz et al.	9,101,385 B2	8/2015	Shelton, IV et al.
8,920,421 B2	12/2014	Rupp	9,107,689 B2	8/2015	Robertson et al.
8,926,607 B2	1/2015	Norvell et al.	9,107,690 B2	8/2015	Bales, Jr. et al.
8,926,608 B2	1/2015	Bacher et al.	9,113,900 B2	8/2015	Buyse et al.
8,926,620 B2	1/2015	Chasmawala et al.	9,113,907 B2	8/2015	Allen, IV et al.
8,931,682 B2	1/2015	Timm et al.	9,113,940 B2	8/2015	Twomey
8,932,282 B2	1/2015	Gilbert	9,119,657 B2	9/2015	Shelton, IV et al.
8,932,299 B2	1/2015	Bono et al.	9,119,957 B2	9/2015	Gantz et al.
8,936,614 B2	1/2015	Allen, IV	9,125,662 B2	9/2015	Shelton, IV
8,939,974 B2	1/2015	Boudreaux et al.	9,125,667 B2	9/2015	Stone et al.
8,951,248 B2	2/2015	Messerly et al.	9,144,453 B2	9/2015	Rencher et al.
8,951,272 B2	2/2015	Robertson et al.	9,147,965 B2	9/2015	Lee
8,956,349 B2	2/2015	Aldridge et al.	9,149,324 B2	10/2015	Huang et al.
8,960,520 B2	2/2015	McCuen	9,149,325 B2	10/2015	Worrell et al.
8,961,515 B2	2/2015	Twomey et al.	9,161,803 B2	10/2015	Yates et al.
8,961,547 B2	2/2015	Dietz et al.	9,165,114 B2	10/2015	Jain et al.
8,967,443 B2	3/2015	McCuen	9,168,054 B2	10/2015	Turner et al.
8,968,283 B2	3/2015	Kharin	9,168,085 B2	10/2015	Juzkiw et al.
8,968,294 B2	3/2015	Maass et al.	9,168,089 B2	10/2015	Buyse et al.
8,968,355 B2	3/2015	Malkowski et al.	9,179,912 B2	11/2015	Yates et al.
8,974,447 B2	3/2015	Kimball et al.	9,186,204 B2	11/2015	Nishimura et al.
8,974,477 B2	3/2015	Yamada	9,186,796 B2	11/2015	Ogawa
8,974,479 B2	3/2015	Ross et al.	9,192,380 B2	11/2015	(Tarinelli) Racenet et al.
8,979,843 B2	3/2015	Timm et al.	9,192,421 B2	11/2015	Garrison
8,979,844 B2	3/2015	White et al.	9,192,428 B2	11/2015	Houser et al.
8,979,890 B2	3/2015	Boudreaux	9,192,431 B2	11/2015	Woodruff et al.
8,986,287 B2	3/2015	Park et al.	9,198,714 B2	12/2015	Worrell et al.
8,986,297 B2	3/2015	Daniel et al.	9,198,776 B2	12/2015	Young
8,986,302 B2	3/2015	Aldridge et al.	9,204,879 B2	12/2015	Shelton, IV
8,989,903 B2	3/2015	Weir et al.	9,204,891 B2	12/2015	Weitzman
8,991,678 B2	3/2015	Wellman et al.	9,204,918 B2	12/2015	Germain et al.
8,992,422 B2	3/2015	Spivey et al.	9,204,923 B2	12/2015	Manzo et al.
9,005,199 B2	4/2015	Beckman et al.	9,216,050 B2	12/2015	Condie et al.
9,011,437 B2	4/2015	Woodruff et al.	9,216,051 B2	12/2015	Fischer et al.
9,011,471 B2	4/2015	Timm et al.	9,216,062 B2	12/2015	Duque et al.
9,017,326 B2	4/2015	DiNardo et al.	9,220,483 B2	12/2015	Frankhouser et al.
9,017,355 B2	4/2015	Smith et al.	9,220,527 B2	12/2015	Houser et al.
9,023,071 B2	5/2015	Miller et al.	9,220,559 B2	12/2015	Worrell et al.
9,028,397 B2	5/2015	Naito	9,226,750 B2	1/2016	Weir et al.
9,028,476 B2	5/2015	Bonn	9,226,751 B2	1/2016	Shelton, IV et al.
9,028,478 B2	5/2015	Mueller	9,226,766 B2	1/2016	Aldridge et al.
9,028,494 B2	5/2015	Shelton, IV et al.	9,226,767 B2	1/2016	Stulen et al.
9,028,519 B2	5/2015	Yates et al.	9,232,979 B2	1/2016	Parihar et al.
9,031,667 B2	5/2015	Williams	9,237,891 B2	1/2016	Shelton, IV
9,033,973 B2	5/2015	Krapohl et al.	9,237,921 B2	1/2016	Messerly et al.
9,035,741 B2	5/2015	Hamel et al.	9,241,060 B1	1/2016	Fujisaki
9,039,690 B2	5/2015	Kersten et al.	9,241,692 B2	1/2016	Gunday et al.
9,039,695 B2	5/2015	Giordano et al.	9,241,728 B2	1/2016	Price et al.
9,039,731 B2	5/2015	Joseph	9,241,730 B2	1/2016	Babaev
9,043,018 B2	5/2015	Mohr	9,241,731 B2	1/2016	Boudreaux et al.
9,044,227 B2	6/2015	Shelton, IV et al.	9,241,768 B2	1/2016	Sandhu et al.
9,044,238 B2	6/2015	Orszulak	9,247,953 B2	2/2016	Palmer et al.
9,044,243 B2	6/2015	Johnson et al.	9,254,165 B2	2/2016	Aronow et al.
9,044,245 B2	6/2015	Condie et al.	9,259,234 B2	2/2016	Robertson et al.
9,044,256 B2	6/2015	Cadeddu et al.	9,259,265 B2	2/2016	Harris et al.
9,044,261 B2	6/2015	Houser	9,265,567 B2	2/2016	Orban, III et al.
			9,265,926 B2	2/2016	Strobl et al.
			9,277,962 B2	3/2016	Koss et al.
			9,282,974 B2	3/2016	Shelton, IV
			9,283,027 B2	3/2016	Monson et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

9,283,045 B2	3/2016	Rhee et al.	9,574,644 B2	2/2017	Parihar
9,289,256 B2	3/2016	Shelton, IV et al.	9,597,143 B2	3/2017	Madan et al.
9,295,514 B2	3/2016	Shelton, IV et al.	9,610,091 B2	4/2017	Johnson et al.
9,301,759 B2	4/2016	Spivey et al.	9,610,114 B2	4/2017	Baxter, III et al.
9,305,497 B2	4/2016	Seo et al.	9,615,877 B2	4/2017	Tyrrell et al.
9,307,388 B2	4/2016	Liang et al.	9,623,237 B2	4/2017	Turner et al.
9,307,986 B2	4/2016	Hall et al.	9,636,135 B2	5/2017	Stulen
9,308,009 B2	4/2016	Madan et al.	9,636,165 B2	5/2017	Larson et al.
9,308,014 B2	4/2016	Fischer	9,638,770 B2	5/2017	Dietz et al.
9,314,261 B2	4/2016	Bales, Jr. et al.	9,642,644 B2	5/2017	Houser et al.
9,314,292 B2	4/2016	Trees et al.	9,642,669 B2	5/2017	Takashino et al.
9,314,301 B2	4/2016	Ben-Haim et al.	9,643,052 B2	5/2017	Tchao et al.
9,326,754 B2	5/2016	Polster	9,649,111 B2	5/2017	Shelton, IV et al.
9,326,787 B2	5/2016	Sanai et al.	9,649,126 B2	5/2017	Robertson et al.
9,326,788 B2	5/2016	Batross et al.	9,655,670 B2	5/2017	Larson et al.
9,333,025 B2	5/2016	Monson et al.	9,662,131 B2	5/2017	Omori et al.
9,333,034 B2	5/2016	Hancock	9,668,806 B2	6/2017	Unger et al.
9,339,289 B2	5/2016	Robertson	9,675,374 B2	6/2017	Stulen et al.
9,339,323 B2	5/2016	Eder et al.	9,675,375 B2	6/2017	Houser et al.
9,339,326 B2	5/2016	McCullagh et al.	9,687,290 B2	6/2017	Keller
9,345,534 B2	5/2016	Artale et al.	9,700,309 B2	7/2017	Jaworek et al.
9,345,900 B2	5/2016	Wu et al.	9,700,339 B2	7/2017	Nield
9,351,642 B2	5/2016	Nadkarni et al.	9,700,343 B2	7/2017	Messerly et al.
9,351,726 B2	5/2016	Leimbach et al.	9,705,456 B2	7/2017	Gilbert
9,351,754 B2	5/2016	Vakharia et al.	9,707,004 B2	7/2017	Houser et al.
9,352,173 B2	5/2016	Yamada et al.	9,707,027 B2	7/2017	Ruddenklau et al.
9,358,065 B2	6/2016	Ladtow et al.	9,707,030 B2	7/2017	Davison et al.
9,364,230 B2	6/2016	Shelton, IV et al.	9,713,507 B2	7/2017	Stulen et al.
9,370,400 B2	6/2016	Parihar	9,717,548 B2	8/2017	Couture
9,370,611 B2	6/2016	Ross et al.	9,717,552 B2	8/2017	Cosman et al.
9,375,230 B2	6/2016	Ross et al.	9,724,118 B2	8/2017	Schulte et al.
9,375,232 B2	6/2016	Hunt et al.	9,724,152 B2	8/2017	Horlle et al.
9,375,256 B2	6/2016	Cunningham et al.	9,737,326 B2	8/2017	Worrell et al.
9,375,267 B2	6/2016	Kerr et al.	9,737,355 B2	8/2017	Yates et al.
9,385,831 B2	7/2016	Marr et al.	9,737,358 B2	8/2017	Beckman et al.
9,386,983 B2	7/2016	Swensgard et al.	9,743,929 B2	8/2017	Leimbach et al.
9,393,037 B2	7/2016	Olson et al.	9,743,946 B2	8/2017	Faller et al.
9,398,911 B2	7/2016	Auld	9,743,947 B2	8/2017	Price et al.
9,402,680 B2	8/2016	Ginnebaugh et al.	9,757,142 B2	9/2017	Shimizu
9,402,682 B2	8/2016	Worrell et al.	9,757,186 B2	9/2017	Boudreaux et al.
9,408,606 B2	8/2016	Shelton, IV	9,764,164 B2	9/2017	Wiener et al.
9,408,622 B2	8/2016	Stulen et al.	9,770,285 B2	9/2017	Zoran et al.
9,408,660 B2	8/2016	Strobl et al.	9,782,214 B2	10/2017	Houser et al.
9,414,853 B2	8/2016	Stulen et al.	9,788,851 B2	10/2017	Dannaher et al.
9,414,880 B2	8/2016	Monson et al.	9,795,405 B2	10/2017	Price et al.
9,421,060 B2	8/2016	Monson et al.	9,795,436 B2	10/2017	Yates et al.
9,427,249 B2	8/2016	Robertson et al.	9,795,808 B2	10/2017	Messerly et al.
9,439,668 B2	9/2016	Timm et al.	9,801,648 B2	10/2017	Houser et al.
9,439,669 B2	9/2016	Wiener et al.	9,802,033 B2	10/2017	Hibner et al.
9,439,671 B2	9/2016	Akagane	9,808,308 B2	11/2017	Faller et al.
9,445,832 B2	9/2016	Wiener et al.	9,814,514 B2	11/2017	Shelton, IV et al.
9,451,967 B2	9/2016	Jordan et al.	9,820,768 B2	11/2017	Gee et al.
9,456,863 B2	10/2016	Moua	9,820,771 B2	11/2017	Norton et al.
9,456,864 B2	10/2016	Witt et al.	9,820,806 B2	11/2017	Lee et al.
9,468,498 B2	10/2016	Sigmon, Jr.	9,839,443 B2	12/2017	Brockman et al.
9,486,236 B2	11/2016	Price et al.	9,848,901 B2	12/2017	Robertson et al.
9,492,146 B2	11/2016	Kostrzewski et al.	9,848,902 B2	12/2017	Price et al.
9,492,224 B2	11/2016	Boudreaux et al.	9,848,937 B2	12/2017	Trees et al.
9,498,245 B2	11/2016	Voegele et al.	9,861,428 B2	1/2018	Trees et al.
9,498,275 B2	11/2016	Wham et al.	9,867,651 B2	1/2018	Wham
9,504,483 B2	11/2016	Houser et al.	9,867,670 B2	1/2018	Brannan et al.
9,504,520 B2	11/2016	Worrell et al.	9,872,725 B2	1/2018	Worrell et al.
9,504,524 B2	11/2016	Behnke, II	9,872,726 B2	1/2018	Morisaki
9,504,855 B2	11/2016	Messerly et al.	9,877,720 B2	1/2018	Worrell et al.
9,510,850 B2	12/2016	Robertson et al.	9,877,776 B2	1/2018	Boudreaux
9,510,906 B2	12/2016	Boudreaux et al.	9,883,884 B2	2/2018	Neurohr et al.
9,522,029 B2	12/2016	Yates et al.	9,888,958 B2	2/2018	Evans et al.
9,522,032 B2	12/2016	Behnke	9,907,563 B2	3/2018	Germain et al.
9,526,564 B2	12/2016	Rusin	9,913,656 B2	3/2018	Stulen
9,526,565 B2	12/2016	Strobl	9,913,680 B2	3/2018	Voegele et al.
9,545,253 B2	1/2017	Worrell et al.	9,918,730 B2	3/2018	Trees et al.
9,554,846 B2	1/2017	Boudreaux	9,925,003 B2	3/2018	Parihar et al.
9,554,854 B2	1/2017	Yates et al.	9,949,785 B2	4/2018	Price et al.
9,560,995 B2	2/2017	Addison et al.	9,949,788 B2	4/2018	Boudreaux
9,561,038 B2	2/2017	Shelton, IV et al.	9,962,182 B2	5/2018	Dietz et al.
			9,987,033 B2	6/2018	Neurohr et al.
			10,004,526 B2	6/2018	Dycus et al.
			10,010,339 B2	7/2018	Witt et al.
			10,010,341 B2	7/2018	Houser et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

10,022,142 B2	7/2018	Aranyi et al.	2004/0142667 A1	7/2004	Lochhead et al.
10,022,567 B2	7/2018	Messerly et al.	2004/0147934 A1	7/2004	Kiester
10,022,568 B2	7/2018	Messerly et al.	2004/0147945 A1	7/2004	Fritzsche
10,028,761 B2	7/2018	Leimbach et al.	2004/0158237 A1	8/2004	Abboud et al.
10,028,786 B2	7/2018	Mucilli et al.	2004/0167508 A1	8/2004	Wham et al.
10,034,684 B2	7/2018	Weisenburgh, II et al.	2004/0176686 A1	9/2004	Hare et al.
10,034,704 B2	7/2018	Asher et al.	2004/0176751 A1	9/2004	Weitzner et al.
10,045,794 B2	8/2018	Witt et al.	2004/0193148 A1 *	9/2004	Wham A61B 18/1206
10,045,810 B2	8/2018	Schall et al.			606/40
10,045,819 B2	8/2018	Jensen et al.	2004/0193150 A1	9/2004	Sharkey et al.
10,070,916 B2	9/2018	Artale	2004/0193153 A1	9/2004	Sartor et al.
10,085,762 B2	10/2018	Timm et al.	2004/0199193 A1	10/2004	Hayashi et al.
10,085,792 B2	10/2018	Johnson et al.	2004/0215132 A1	10/2004	Yoon
10,092,310 B2	10/2018	Boudreaux et al.	2004/0243147 A1	12/2004	Lipow
10,092,344 B2	10/2018	Mohr et al.	2004/0249374 A1	12/2004	Tetzlaff et al.
10,092,348 B2	10/2018	Boudreaux	2004/0260273 A1	12/2004	Wan
10,111,699 B2	10/2018	Boudreaux	2004/0260300 A1	12/2004	Gorensek et al.
10,111,703 B2	10/2018	Cosman, Jr. et al.	2004/0267311 A1	12/2004	Viola et al.
10,117,667 B2	11/2018	Robertson et al.	2005/0015125 A1	1/2005	Mioduski et al.
10,117,702 B2	11/2018	Danziger et al.	2005/0020967 A1	1/2005	Ono
10,130,410 B2	11/2018	Strobl et al.	2005/0021018 A1	1/2005	Anderson et al.
10,130,412 B2	11/2018	Wham	2005/0021065 A1	1/2005	Yamada et al.
2001/0025173 A1	9/2001	Ritchie et al.	2005/0021078 A1	1/2005	Vleugels et al.
2001/0025183 A1	9/2001	Shahidi	2005/0033278 A1	2/2005	McClurken et al.
2001/0025184 A1	9/2001	Messerly	2005/0033337 A1	2/2005	Muir et al.
2001/0031950 A1	10/2001	Ryan	2005/0070800 A1	3/2005	Takahashi
2001/0039419 A1	11/2001	Francischelli et al.	2005/0088285 A1	4/2005	Jei
2002/0002377 A1	1/2002	Cimino	2005/0090817 A1	4/2005	Phan
2002/0002380 A1	1/2002	Bishop	2005/0096683 A1	5/2005	Ellins et al.
2002/0019649 A1	2/2002	Sikora et al.	2005/0099824 A1	5/2005	Dowling et al.
2002/0022836 A1	2/2002	Goble et al.	2005/0131390 A1	6/2005	Heinrich et al.
2002/0029036 A1	3/2002	Goble et al.	2005/0143769 A1	6/2005	White et al.
2002/0029055 A1	3/2002	Bonutti	2005/0149108 A1	7/2005	Cox
2002/0049551 A1	4/2002	Friedman et al.	2005/0165429 A1	7/2005	Douglas et al.
2002/0052617 A1	5/2002	Anis et al.	2005/0171522 A1	8/2005	Christopherson
2002/0077550 A1	6/2002	Rabiner et al.	2005/0177184 A1	8/2005	Easley
2002/0107517 A1	8/2002	Witt et al.	2005/0182339 A1	8/2005	Lee et al.
2002/0156466 A1	10/2002	Sakurai et al.	2005/0188743 A1	9/2005	Land
2002/0156493 A1	10/2002	Houser et al.	2005/0192610 A1	9/2005	Houser et al.
2003/0014053 A1	1/2003	Nguyen et al.	2005/0192611 A1	9/2005	Houser
2003/0014087 A1	1/2003	Fang et al.	2005/0222598 A1	10/2005	Ho et al.
2003/0036705 A1	2/2003	Hare et al.	2005/0234484 A1	10/2005	Houser et al.
2003/0050572 A1	3/2003	Brautigam et al.	2005/0249667 A1	11/2005	Tuszynski et al.
2003/0055443 A1	3/2003	Spotnitz	2005/0256405 A1	11/2005	Makin et al.
2003/0109875 A1	6/2003	Tetzlaff et al.	2005/0261588 A1	11/2005	Makin et al.
2003/0114851 A1	6/2003	Truckai et al.	2005/0262175 A1	11/2005	Iino et al.
2003/0130693 A1	7/2003	Levin et al.	2005/0267464 A1	12/2005	Truckai et al.
2003/0139741 A1	7/2003	Goble et al.	2005/0271807 A1	12/2005	Iijima et al.
2003/0144680 A1	7/2003	Kellogg et al.	2005/0273090 A1	12/2005	Nieman et al.
2003/0158548 A1	8/2003	Phan et al.	2005/0288659 A1	12/2005	Kimura et al.
2003/0171747 A1	9/2003	Kanehira et al.	2006/0025757 A1	2/2006	Heim
2003/0199794 A1	10/2003	Sakurai et al.	2006/0030797 A1	2/2006	Zhou et al.
2003/0204199 A1	10/2003	Novak et al.	2006/0058825 A1	3/2006	Ogura et al.
2003/0212332 A1	11/2003	Fenton et al.	2006/0063130 A1	3/2006	Hayman et al.
2003/0212363 A1	11/2003	Shipp	2006/0064086 A1	3/2006	Odom
2003/0212392 A1	11/2003	Fenton et al.	2006/0066181 A1	3/2006	Bromfield et al.
2003/0212422 A1	11/2003	Fenton et al.	2006/0074442 A1	4/2006	Noriega et al.
2003/0225332 A1	12/2003	Okada et al.	2006/0079874 A1	4/2006	Faller et al.
2003/0229344 A1	12/2003	Dycus et al.	2006/0079879 A1	4/2006	Faller et al.
2004/0030254 A1	2/2004	Babaev	2006/0095046 A1	5/2006	Trieu et al.
2004/0030330 A1	2/2004	Brassell et al.	2006/0109061 A1	5/2006	Dobson et al.
2004/0047485 A1	3/2004	Sherrit et al.	2006/0159731 A1	7/2006	Shoshan
2004/0054364 A1	3/2004	Aranyi et al.	2006/0190034 A1	8/2006	Nishizawa et al.
2004/0064151 A1	4/2004	Mollenauer	2006/0206100 A1	9/2006	Eskridge et al.
2004/0087943 A1	5/2004	Dycus et al.	2006/0206115 A1	9/2006	Schomer et al.
2004/0092921 A1	5/2004	Kadziauskas et al.	2006/0211943 A1	9/2006	Beaupre
2004/0092992 A1	5/2004	Adams et al.	2006/0217729 A1	9/2006	Eskridge et al.
2004/0097911 A1	5/2004	Murakami et al.	2006/0224160 A1	10/2006	Trieu et al.
2004/0097912 A1	5/2004	Gonnering	2006/0247558 A1	11/2006	Yamada
2004/0097919 A1	5/2004	Wellman et al.	2006/0253050 A1	11/2006	Yoshimine et al.
2004/0097996 A1	5/2004	Rabiner et al.	2006/0264809 A1	11/2006	Hansmann et al.
2004/0116952 A1	6/2004	Sakurai et al.	2006/0264995 A1	11/2006	Fanton et al.
2004/0122423 A1	6/2004	Dycus et al.	2006/0270916 A1	11/2006	Skwarek et al.
2004/0132383 A1	7/2004	Langford et al.	2006/0271030 A1	11/2006	Francis et al.
2004/0138621 A1	7/2004	Jahns et al.	2006/0293656 A1	12/2006	Shadduck et al.
			2007/0016235 A1	1/2007	Tanaka et al.
			2007/0016236 A1	1/2007	Beaupre
			2007/0021738 A1	1/2007	Hasser et al.
			2007/0027468 A1	2/2007	Wales et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2007/0055228 A1	3/2007	Berg et al.	2009/0048537 A1	2/2009	Lydon et al.
2007/0056596 A1	3/2007	Fanney et al.	2009/0048589 A1	2/2009	Takashino et al.
2007/0060935 A1	3/2007	Schwardt et al.	2009/0054886 A1	2/2009	Yachi et al.
2007/0063618 A1	3/2007	Bromfield	2009/0054889 A1	2/2009	Newton et al.
2007/0067123 A1	3/2007	Jungerman	2009/0054894 A1	2/2009	Yachi
2007/0073185 A1	3/2007	Nakao	2009/0076506 A1	3/2009	Baker
2007/0073341 A1	3/2007	Smith et al.	2009/0082716 A1	3/2009	Akahoshi
2007/0074584 A1	4/2007	Talarico et al.	2009/0082766 A1	3/2009	Unger et al.
2007/0106317 A1	5/2007	Shelton et al.	2009/0088785 A1	4/2009	Masuda
2007/0118115 A1	5/2007	Artale et al.	2009/0090763 A1	4/2009	Zemlok et al.
2007/0130771 A1	6/2007	Ehlert et al.	2009/0118751 A1	5/2009	Wiener et al.
2007/0135803 A1	6/2007	Belson	2009/0143799 A1	6/2009	Smith et al.
2007/0149881 A1	6/2007	Rabin	2009/0143800 A1	6/2009	Deville et al.
2007/0156163 A1	7/2007	Davison et al.	2009/0163807 A1	6/2009	Sliwa
2007/0166663 A1	7/2007	Telles et al.	2009/0182322 A1	7/2009	D'Amelio et al.
2007/0173803 A1	7/2007	Wham et al.	2009/0182331 A1	7/2009	D'Amelio et al.
2007/0173813 A1	7/2007	Odom	2009/0182332 A1	7/2009	Long et al.
2007/0173872 A1	7/2007	Neuenfeldt	2009/0216157 A1	8/2009	Yamada
2007/0185474 A1	8/2007	Nahen	2009/0223033 A1	9/2009	Houser
2007/0191712 A1	8/2007	Messerly et al.	2009/0240244 A1	9/2009	Malis et al.
2007/0191713 A1	8/2007	Eichmann et al.	2009/0248021 A1	10/2009	McKenna
2007/0203483 A1	8/2007	Kim et al.	2009/0254077 A1	10/2009	Craig
2007/0208336 A1	9/2007	Kim et al.	2009/0254080 A1	10/2009	Honda
2007/0208340 A1	9/2007	Ganz et al.	2009/0264909 A1	10/2009	Beaupre
2007/0219481 A1	9/2007	Babaev	2009/0270771 A1	10/2009	Takahashi
2007/0232926 A1	10/2007	Stulen et al.	2009/0270812 A1	10/2009	Litscher et al.
2007/0232928 A1	10/2007	Wiener et al.	2009/0270853 A1	10/2009	Yachi et al.
2007/0236213 A1	10/2007	Paden et al.	2009/0270891 A1	10/2009	Beaupre
2007/0239101 A1	10/2007	Kellogg	2009/0270899 A1	10/2009	Carusillo et al.
2007/0249941 A1	10/2007	Salehi et al.	2009/0287205 A1	11/2009	Ingle
2007/0260242 A1	11/2007	Dycus et al.	2009/0299141 A1	12/2009	Downey et al.
2007/0265560 A1	11/2007	Soltani et al.	2009/0327715 A1	12/2009	Smith et al.
2007/0265613 A1	11/2007	Edelstein et al.	2010/0004508 A1	1/2010	Naito et al.
2007/0265616 A1	11/2007	Couture et al.	2010/0022825 A1	1/2010	Yoshie
2007/0265620 A1	11/2007	Kraas et al.	2010/0030233 A1	2/2010	Whitman et al.
2007/0275348 A1	11/2007	Lemon	2010/0036370 A1	2/2010	Mirel et al.
2007/0287933 A1	12/2007	Phan et al.	2010/0042093 A9	2/2010	Wham et al.
2007/0288055 A1	12/2007	Lee	2010/0049180 A1	2/2010	Wells et al.
2008/0005213 A1	1/2008	Holtzman	2010/0057118 A1	3/2010	Dietz et al.
2008/0013809 A1	1/2008	Zhu et al.	2010/0063525 A1	3/2010	Beaupre et al.
2008/0015575 A1	1/2008	Odom et al.	2010/0063528 A1	3/2010	Beaupre
2008/0039746 A1	2/2008	Hissong et al.	2010/0081863 A1	4/2010	Hess et al.
2008/0051812 A1	2/2008	Schmitz et al.	2010/0081864 A1	4/2010	Hess et al.
2008/0058775 A1	3/2008	Darian et al.	2010/0081883 A1	4/2010	Murray et al.
2008/0058845 A1	3/2008	Shimizu et al.	2010/0094323 A1	4/2010	Isaacs et al.
2008/0071269 A1	3/2008	Hilario et al.	2010/0106173 A1	4/2010	Yoshimine
2008/0077145 A1	3/2008	Boyden et al.	2010/0158307 A1	6/2010	Kubota et al.
2008/0082039 A1	4/2008	Babaev	2010/0168741 A1	7/2010	Sanai et al.
2008/0082098 A1	4/2008	Tanaka et al.	2010/0179536 A1 *	7/2010	Podhajsky A61B 18/1206 606/34
2008/0097501 A1	4/2008	Blier	2010/0187283 A1	7/2010	Crainich et al.
2008/0114355 A1	5/2008	Wayne et al.	2010/0204721 A1	8/2010	Young et al.
2008/0114364 A1	5/2008	Goldin et al.	2010/0222714 A1	9/2010	Muir et al.
2008/0122496 A1	5/2008	Wagner	2010/0222752 A1	9/2010	Collins, Jr. et al.
2008/0125768 A1	5/2008	Tahara et al.	2010/0228250 A1	9/2010	Brogna
2008/0147058 A1	6/2008	Horrell et al.	2010/0234906 A1	9/2010	Koh
2008/0147062 A1	6/2008	Truckai et al.	2010/0274160 A1	10/2010	Yachi et al.
2008/0147092 A1	6/2008	Rogge et al.	2010/0274278 A1	10/2010	Fleenor et al.
2008/0171938 A1	7/2008	Masuda et al.	2010/0298743 A1	11/2010	Nield et al.
2008/0177268 A1	7/2008	Daum et al.	2010/0331742 A1	12/2010	Masuda
2008/0188755 A1	8/2008	Hart	2011/0004233 A1	1/2011	Muir et al.
2008/0200940 A1	8/2008	Eichmann et al.	2011/0028964 A1	2/2011	Edwards
2008/0208108 A1	8/2008	Kimura	2011/0087220 A1	4/2011	Felder et al.
2008/0208231 A1	8/2008	Ota et al.	2011/0125149 A1	5/2011	Ei-Galley et al.
2008/0214967 A1	9/2008	Aranyi et al.	2011/0125151 A1	5/2011	Strauss et al.
2008/0234709 A1	9/2008	Houser	2011/0160725 A1 *	6/2011	Kabaya A61B 18/1206 606/42
2008/0243162 A1	10/2008	Shibata et al.	2011/0238010 A1	9/2011	Kirschenman et al.
2008/0255413 A1	10/2008	Zemlok et al.	2011/0276049 A1	11/2011	Gerhardt
2008/0281200 A1	11/2008	Voic et al.	2011/0278343 A1	11/2011	Knodel et al.
2008/0281315 A1	11/2008	Gines	2011/0279268 A1	11/2011	Konishi et al.
2008/0287944 A1	11/2008	Pearson et al.	2011/0284014 A1	11/2011	Cadeddu et al.
2008/0287948 A1	11/2008	Newton et al.	2011/0290856 A1	12/2011	Shelton, IV et al.
2008/0296346 A1	12/2008	Shelton, IV et al.	2011/0295295 A1	12/2011	Shelton, IV et al.
2008/0300588 A1	12/2008	Groth et al.	2011/0306967 A1	12/2011	Payne et al.
2009/0012516 A1	1/2009	Curtis et al.	2011/0313415 A1	12/2011	Fernandez et al.
2009/0023985 A1	1/2009	Ewers	2012/0004655 A1	1/2012	Kim et al.
			2012/0016413 A1	1/2012	Timm et al.
			2012/0022519 A1	1/2012	Huang et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0022526 A1	1/2012	Aldridge et al.	2015/0313667 A1	11/2015	Allen, IV
2012/0022583 A1	1/2012	Sugalski et al.	2015/0320480 A1	11/2015	Cosman, Jr. et al.
2012/0059289 A1	3/2012	Nield et al.	2015/0320481 A1	11/2015	Cosman, Jr. et al.
2012/0071863 A1	3/2012	Lee et al.	2015/0340586 A1	11/2015	Wiener et al.
2012/0078139 A1	3/2012	Aldridge et al.	2016/0030076 A1	2/2016	Faller et al.
2012/0078244 A1	3/2012	Worrell et al.	2016/0045248 A1	2/2016	Unger et al.
2012/0080344 A1	4/2012	Shelton, IV	2016/0051316 A1	2/2016	Boudreaux
2012/0101495 A1	4/2012	Young et al.	2016/0051317 A1	2/2016	Boudreaux
2012/0109186 A1	5/2012	Parrott et al.	2016/0058492 A1	3/2016	Yates et al.
2012/0116265 A1	5/2012	Houser et al.	2016/0074108 A1	3/2016	Woodruff et al.
2012/0116266 A1	5/2012	Houser et al.	2016/0128762 A1	5/2016	Harris et al.
2012/0116381 A1	5/2012	Houser et al.	2016/0144204 A1	5/2016	Akagane
2012/0143211 A1	6/2012	Kishi	2016/0157927 A1	6/2016	Corbett et al.
2012/0150049 A1	6/2012	Zielinski et al.	2016/0175024 A1	6/2016	Yates et al.
2012/0150169 A1	6/2012	Zielinski et al.	2016/0175029 A1	6/2016	Witt et al.
2012/0172904 A1	7/2012	Muir et al.	2016/0175032 A1	6/2016	Yang
2012/0253328 A1	10/2012	Cunningham et al.	2016/0199123 A1	7/2016	Thomas et al.
2012/0265241 A1	10/2012	Hart et al.	2016/0199125 A1	7/2016	Jones
2012/0296371 A1	11/2012	Kappus et al.	2016/0206342 A1	7/2016	Robertson et al.
2013/0023925 A1	1/2013	Mueller	2016/0228171 A1	8/2016	Boudreaux
2013/0035685 A1	2/2013	Fischer et al.	2016/0262786 A1	9/2016	Madan et al.
2013/0085510 A1	4/2013	Stefanchik et al.	2016/0270840 A1	9/2016	Yates et al.
2013/0123776 A1	5/2013	Monson et al.	2016/0270841 A1	9/2016	Strobl et al.
2013/0158659 A1	6/2013	Bergs et al.	2016/0270842 A1	9/2016	Strobl et al.
2013/0158660 A1	6/2013	Bergs et al.	2016/0270843 A1	9/2016	Boudreaux et al.
2013/0165929 A1	6/2013	Muir et al.	2016/0278848 A1	9/2016	Boudreaux et al.
2013/0214025 A1	8/2013	Zemlok et al.	2016/0287311 A1	10/2016	Friedrichs
2013/0253256 A1	9/2013	Griffith et al.	2016/0296249 A1	10/2016	Robertson
2013/0296843 A1	11/2013	Boudreaux et al.	2016/0296250 A1	10/2016	Olson et al.
2013/0338647 A1	12/2013	Bacher et al.	2016/0296251 A1	10/2016	Olson et al.
2014/0001231 A1	1/2014	Shelton, IV et al.	2016/0296252 A1	10/2016	Olson et al.
2014/0001234 A1	1/2014	Shelton, IV et al.	2016/0296268 A1	10/2016	Gee et al.
2014/0005640 A1	1/2014	Shelton, IV et al.	2016/0296270 A1	10/2016	Strobl et al.
2014/0005678 A1	1/2014	Shelton, IV et al.	2016/0317217 A1	11/2016	Batross et al.
2014/0005702 A1	1/2014	Timm et al.	2016/0338726 A1	11/2016	Stulen et al.
2014/0005705 A1	1/2014	Weir et al.	2016/0346001 A1	12/2016	Vakharia et al.
2014/0005718 A1	1/2014	Shelton, IV et al.	2016/0367273 A1	12/2016	Robertson et al.
2014/0012299 A1	1/2014	Stoddard et al.	2016/0367281 A1	12/2016	Gee et al.
2014/0014544 A1	1/2014	Bugnard et al.	2016/0374708 A1	12/2016	Wiener et al.
2014/0114327 A1	4/2014	Boudreaux et al.	2016/0374709 A1	12/2016	Timm et al.
2014/0114334 A1 *	4/2014	Olson A61B 17/32006 606/169	2016/0374712 A1	12/2016	Stulen et al.
2014/0121569 A1	5/2014	Schafer et al.	2016/0374752 A1	12/2016	Hancock et al.
2014/0135804 A1	5/2014	Weisenburgh, II et al.	2017/0000512 A1	1/2017	Conlon et al.
2014/0194874 A1	7/2014	Dietz et al.	2017/0000513 A1	1/2017	Conlon et al.
2014/0194875 A1	7/2014	Reschke et al.	2017/0000516 A1	1/2017	Stulen et al.
2014/0246475 A1	9/2014	Hall et al.	2017/0000541 A1	1/2017	Yates et al.
2014/0263541 A1	9/2014	Leimbach et al.	2017/0000542 A1	1/2017	Yates et al.
2014/0276659 A1	9/2014	Juergens et al.	2017/0000553 A1	1/2017	Wiener et al.
2014/0276754 A1	9/2014	Gilbert et al.	2017/0000554 A1	1/2017	Yates et al.
2014/0276797 A1	9/2014	Batchelor et al.	2017/0056056 A1	3/2017	Wiener et al.
2014/0276970 A1	9/2014	Messerly et al.	2017/0056058 A1	3/2017	Voegele et al.
2014/0330271 A1	11/2014	Dietz et al.	2017/0086876 A1	3/2017	Wiener et al.
2015/0032100 A1 *	1/2015	Coulson A61B 18/1233 606/35	2017/0086908 A1	3/2017	Wiener et al.
2015/0032150 A1	1/2015	Ishida et al.	2017/0086909 A1	3/2017	Yates et al.
2015/0080876 A1	3/2015	Worrell et al.	2017/0086910 A1	3/2017	Wiener et al.
2015/0080887 A1	3/2015	Sobajima et al.	2017/0086911 A1	3/2017	Wiener et al.
2015/0080912 A1	3/2015	Sapre	2017/0086912 A1	3/2017	Wiener et al.
2015/0088178 A1	3/2015	Stulen et al.	2017/0086913 A1	3/2017	Yates et al.
2015/0112335 A1	4/2015	Boudreaux et al.	2017/0086914 A1	3/2017	Wiener et al.
2015/0157356 A1	6/2015	Gee	2017/0090507 A1	3/2017	Wiener et al.
2015/0164533 A1	6/2015	Felder et al.	2017/0095267 A1	4/2017	Messerly et al.
2015/0164534 A1	6/2015	Felder et al.	2017/0105757 A1	4/2017	Weir et al.
2015/0164535 A1	6/2015	Felder et al.	2017/0105782 A1	4/2017	Scheib et al.
2015/0164536 A1	6/2015	Czarnecki et al.	2017/0105786 A1	4/2017	Scheib et al.
2015/0164537 A1	6/2015	Cagle et al.	2017/0105791 A1	4/2017	Yates et al.
2015/0164538 A1	6/2015	Aldridge et al.	2017/0143371 A1	5/2017	Witt et al.
2015/0182276 A1	7/2015	Wiener et al.	2017/0143877 A1	5/2017	Witt et al.
2015/0182277 A1	7/2015	Wiener et al.	2017/0189095 A1	7/2017	Danziger et al.
2015/0230853 A1	8/2015	Johnson et al.	2017/0189096 A1	7/2017	Danziger et al.
2015/0230861 A1	8/2015	Woloszko et al.	2017/0189101 A1	7/2017	Yates et al.
2015/0257780 A1	9/2015	Houser	2017/0196586 A1	7/2017	Witt et al.
2015/0272659 A1	10/2015	Boudreaux et al.	2017/0196587 A1	7/2017	Witt et al.
2015/0272660 A1	10/2015	Boudreaux et al.	2017/0202570 A1	7/2017	Shelton, IV et al.
			2017/0202571 A1	7/2017	Shelton, IV et al.
			2017/0202572 A1	7/2017	Shelton, IV et al.
			2017/0202591 A1	7/2017	Shelton, IV et al.
			2017/0202592 A1	7/2017	Shelton, IV et al.
			2017/0202593 A1	7/2017	Shelton, IV et al.
			2017/0202594 A1	7/2017	Shelton, IV et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2017/0202595 A1 7/2017 Shelton, IV
 2017/0202596 A1 7/2017 Shelton, IV et al.
 2017/0202597 A1 7/2017 Shelton, IV et al.
 2017/0202598 A1 7/2017 Shelton, IV et al.
 2017/0202599 A1 7/2017 Shelton, IV et al.
 2017/0202605 A1 7/2017 Shelton, IV et al.
 2017/0202607 A1 7/2017 Shelton, IV et al.
 2017/0202608 A1 7/2017 Shelton, IV et al.
 2017/0202609 A1 7/2017 Shelton, IV et al.
 2017/0207467 A1 7/2017 Shelton, IV et al.
 2017/0209167 A1 7/2017 Nield
 2017/0238991 A1 8/2017 Worrell et al.
 2017/0245875 A1 8/2017 Timm et al.
 2017/0312014 A1 11/2017 Strobl et al.
 2017/0312015 A1 11/2017 Worrell et al.
 2017/0312016 A1 11/2017 Strobl et al.
 2017/0319228 A1 11/2017 Worrell et al.
 2017/0319265 A1 11/2017 Yates et al.
 2017/0348064 A1 12/2017 Stewart et al.
 2018/0014872 A1 1/2018 Dickerson
 2018/0028257 A1 2/2018 Yates et al.
 2018/0036061 A1 2/2018 Yates et al.
 2018/0042658 A1 2/2018 Shelton, IV et al.
 2018/0064961 A1 3/2018 Wiener et al.
 2018/0098785 A1 4/2018 Price et al.
 2018/0098808 A1 4/2018 Yates et al.
 2018/0116706 A9 5/2018 Wiener et al.
 2018/0146976 A1 5/2018 Clauda et al.
 2018/0177545 A1 6/2018 Boudreaux et al.
 2018/0235691 A1 8/2018 Voegelé et al.
 2018/0280083 A1 10/2018 Parihar et al.

FOREIGN PATENT DOCUMENTS

CN 1233944 A 11/1999
 CN 1253485 A 5/2000
 CN 2460047 Y 11/2001
 CN 1634601 A 7/2005
 CN 1640365 A 7/2005
 CN 1694649 A 11/2005
 CN 1775323 A 5/2006
 CN 1922563 A 2/2007
 CN 2868227 Y 2/2007
 CN 1951333 A 4/2007
 CN 101035482 A 9/2007
 CN 101040799 A 9/2007
 CN 101396300 A 4/2009
 CN 101467917 A 7/2009
 CN 101474081 A 7/2009
 CN 101674782 A 3/2010
 CN 101883531 A 11/2010
 CN 102160045 A 8/2011
 CN 202027624 U 11/2011
 CN 102834069 A 12/2012
 CN 101313865 B 1/2013
 DE 3904558 A1 8/1990
 DE 9210327 U1 11/1992
 DE 4300307 A1 7/1994
 DE 4323585 A1 1/1995
 DE 19608716 C1 4/1997
 DE 29623113 U1 10/1997
 DE 20004812 U1 9/2000
 DE 20021619 U1 3/2001
 DE 10042606 A1 8/2001
 DE 10201569 A1 7/2003
 EP 0171967 A2 2/1986
 EP 0336742 A2 10/1989
 EP 0136855 B1 11/1989
 EP 0342448 A1 11/1989
 EP 0443256 A1 8/1991
 EP 0456470 A1 11/1991
 EP 0238667 B1 2/1993
 EP 0340803 B1 8/1993
 EP 0598976 A2 6/1994
 EP 0630612 A1 12/1994

EP 0424685 B1 5/1995
 EP 0677275 A2 10/1995
 EP 0482195 B1 1/1996
 EP 0695535 A1 2/1996
 EP 0705571 A1 4/1996
 EP 0741996 B1 11/1996
 EP 0612570 B1 6/1997
 EP 0557806 B1 5/1998
 EP 0640317 B1 9/1999
 EP 1108394 A2 6/2001
 EP 1138264 A1 10/2001
 EP 0908148 B1 1/2002
 EP 1229515 A2 8/2002
 EP 0722696 B1 12/2002
 EP 1285634 A1 2/2003
 EP 0908155 B1 6/2003
 EP 0705570 B1 4/2004
 EP 0765637 B1 7/2004
 EP 0870473 B1 9/2005
 EP 0624346 B1 11/2005
 EP 1594209 A1 11/2005
 EP 1199044 B1 12/2005
 EP 1609428 A1 12/2005
 EP 1199043 B1 3/2006
 EP 1293172 B1 4/2006
 EP 0875209 B1 5/2006
 EP 1433425 B1 6/2006
 EP 1256323 B1 8/2006
 EP 1698289 A2 9/2006
 EP 1704824 A1 9/2006
 EP 1749479 A1 2/2007
 EP 1767157 A1 3/2007
 EP 1254637 B1 8/2007
 EP 1815950 A1 8/2007
 EP 1839599 A1 10/2007
 EP 1844720 A1 10/2007
 EP 1862133 A1 12/2007
 EP 1875875 A1 1/2008
 EP 1878399 A1 1/2008
 EP 1915953 A1 4/2008
 EP 1532933 B1 5/2008
 EP 1199045 B1 6/2008
 EP 1707143 B1 6/2008
 EP 1943957 A2 7/2008
 EP 1964530 A1 9/2008
 EP 1972264 A1 9/2008
 EP 1974771 A1 10/2008
 EP 1435852 B1 12/2008
 EP 1498082 B1 12/2008
 EP 1707131 B1 12/2008
 EP 1477104 B1 1/2009
 EP 2014218 A2 1/2009
 EP 1849424 B1 4/2009
 EP 2042112 A2 4/2009
 EP 2042117 A1 4/2009
 EP 2060238 A1 5/2009
 EP 1832259 B1 6/2009
 EP 2074959 A1 7/2009
 EP 1810625 B1 8/2009
 EP 2090256 A2 8/2009
 EP 2092905 A1 8/2009
 EP 2105104 A2 9/2009
 EP 1747761 B1 10/2009
 EP 2106758 A1 10/2009
 EP 2111813 A1 10/2009
 EP 2131760 A1 12/2009
 EP 1769766 B1 2/2010
 EP 2151204 A1 2/2010
 EP 2153791 A1 2/2010
 EP 2200145 A1 6/2010
 EP 1214913 B1 7/2010
 EP 2238938 A1 10/2010
 EP 2243439 A1 10/2010
 EP 2298154 A2 3/2011
 EP 2305144 A1 4/2011
 EP 1510178 B1 6/2011
 EP 1946708 B1 6/2011
 EP 2335630 A1 6/2011
 EP 1502551 B1 7/2011

(56) References Cited							
FOREIGN PATENT DOCUMENTS							
EP	1728475	B1	8/2011	JP	H11318918	A	11/1999
EP	2353518	A1	8/2011	JP	2000041991	A	2/2000
EP	2361562	A1	8/2011	JP	2000070279	A	3/2000
EP	2365608	A2	9/2011	JP	2000210299	A	8/2000
EP	2420197	A2	2/2012	JP	2000271145	A	10/2000
EP	2422721	A2	2/2012	JP	2000287987	A	10/2000
EP	1927321	B1	4/2012	JP	2001029353	A	2/2001
EP	2436327	A1	4/2012	JP	2001502216	A	2/2001
EP	2529681	A1	12/2012	JP	2001309925	A	11/2001
EP	1767164	B1	1/2013	JP	2002059380	A	2/2002
EP	2316359	B1	3/2013	JP	2002177295	A	6/2002
EP	2090238	B1	4/2013	JP	2002186901	A	7/2002
EP	2578172	A2	4/2013	JP	2002204808	A	7/2002
EP	1586275	B1	5/2013	JP	2002238919	A	8/2002
EP	1616529	B1	9/2013	JP	2002263579	A	9/2002
EP	1997438	B1	11/2013	JP	2002301086	A	10/2002
EP	2668922	A1	12/2013	JP	2002306504	A	10/2002
EP	2508143	B1	2/2014	JP	2002330977	A	11/2002
EP	2583633	B1	10/2014	JP	2002542690	A	12/2002
EP	2076195	B1	12/2015	JP	2003000612	A	1/2003
EP	2113210	B1	3/2016	JP	2003010201	A	1/2003
EP	2510891	B1	6/2016	JP	2003510158	A	3/2003
EP	2227155	B1	7/2016	JP	2003116870	A	4/2003
EP	2859858	B1	12/2016	JP	2003126104	A	5/2003
ES	2115068	T3	6/1998	JP	2003126110	A	5/2003
GB	1482943	A	8/1977	JP	2003153919	A	5/2003
GB	2032221	A	4/1980	JP	2003530921	A	10/2003
GB	2317566	A	4/1998	JP	2003310627	A	11/2003
GB	2379878	B	11/2004	JP	2003339730	A	12/2003
GB	2472216	A	2/2011	JP	2004129871	A	4/2004
GB	2447767	B	8/2011	JP	2004147701	A	5/2004
JP	S50100891	A	8/1975	JP	2005003496	A	1/2005
JP	S5968513	U	5/1984	JP	2005027026	A	1/2005
JP	S59141938	A	8/1984	JP	2005040222	A	2/2005
JP	S62221343	A	9/1987	JP	2005066316	A	3/2005
JP	S62227343	A	10/1987	JP	2005074088	A	3/2005
JP	S62292153	A	12/1987	JP	2005507679	A	3/2005
JP	S62292154	A	12/1987	JP	2005534451	A	11/2005
JP	S63109386	A	5/1988	JP	2005337119	A	12/2005
JP	S63315049	A	12/1988	JP	2006006410	A	1/2006
JP	H01151452	A	6/1989	JP	2006068396	A	3/2006
JP	H01198540	A	8/1989	JP	2006075376	A	3/2006
JP	H0271510	U	5/1990	JP	2006081664	A	3/2006
JP	H02286149	A	11/1990	JP	2006114072	A	4/2006
JP	H02292193	A	12/1990	JP	2006512149	A	4/2006
JP	H0337061	A	2/1991	JP	2006116194	A	5/2006
JP	H0425707	U	2/1992	JP	2006158525	A	6/2006
JP	H0464351	A	2/1992	JP	2006217716	A	8/2006
JP	H0430508	U	3/1992	JP	2006218296	A	8/2006
JP	H04150847	A	5/1992	JP	2006288431	A	10/2006
JP	H04152942	A	5/1992	JP	2007050181	A	3/2007
JP	H0595955	A	4/1993	JP	2007-524459	A	8/2007
JP	H05115490	A	5/1993	JP	2007229454	A	9/2007
JP	H0670938	A	3/1994	JP	2007527747	A	10/2007
JP	H06104503	A	4/1994	JP	2007296369	A	11/2007
JP	H06217988	A	8/1994	JP	200801876	A	1/2008
JP	H06507081	A	8/1994	JP	2008018226	A	1/2008
JP	H 07500514	A	1/1995	JP	200833644	A	2/2008
JP	H07308323	A	11/1995	JP	2008036390	A	2/2008
JP	H07508910	A	11/1995	JP	2008508065	A	3/2008
JP	H0824266	A	1/1996	JP	2008119250	A	5/2008
JP	H08299050	A	9/1996	JP	2008515562	A	5/2008
JP	H08275951	A	10/1996	JP	2008521503	A	6/2008
JP	H08299351	A	11/1996	JP	2008188160	A	8/2008
JP	H08336544	A	12/1996	JP	D1339835	S	8/2008
JP	H08336545	A	12/1996	JP	2008212679	A	9/2008
JP	H09503146	A	3/1997	JP	2008536562	A	9/2008
JP	H09135553	A	5/1997	JP	2008284374	A	11/2008
JP	H09140722	A	6/1997	JP	2009511206	A	3/2009
JP	H105237	A	1/1998	JP	2009082711	A	4/2009
JP	H10295700	A	11/1998	JP	2009517181	A	4/2009
JP	H11501543	A	2/1999	JP	4262923	B2	5/2009
JP	H11128238	A	5/1999	JP	2009523567	A	6/2009
JP	H11192235	A	7/1999	JP	2009148557	A	7/2009
JP	H11253451	A	9/1999	JP	2009236177	A	10/2009
				JP	2009254819	A	11/2009
				JP	2010000336	A	1/2010
				JP	2010009686	A	1/2010
				JP	2010514923	A	5/2010

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP	2010121865	A	6/2010	WO	WO-2004032762	A1	4/2004
JP	2010534522	A	11/2010	WO	WO-2004032763	A2	4/2004
JP	2010540186	A	12/2010	WO	WO-2004037095	A2	5/2004
JP	2011505198	A	2/2011	WO	WO-2004060141	A2	7/2004
JP	2012/075899	A	4/2012	WO	WO-2004078051	A2	9/2004
JP	2012071186	A	4/2012	WO	WO-2004098426	A1	11/2004
JP	2012235658	A	11/2012	WO	WO-2004112618	A2	12/2004
JP	5208761	B2	6/2013	WO	WO-2005052959	A2	6/2005
JP	5714508	B2	5/2015	WO	WO-2005117735	A1	12/2005
JP	2015515339	A	5/2015	WO	WO-2005122917	A1	12/2005
JP	5836543	B1	12/2015	WO	WO-2006012797	A1	2/2006
KR	100789356	B1	12/2007	WO	WO-2006021269	A1	3/2006
RU	2154437	C1	8/2000	WO	WO-2006036706	A1	4/2006
RU	22035	U1	3/2002	WO	WO-2006042210	A2	4/2006
RU	2201169	C2	3/2003	WO	WO-2006055166	A2	5/2006
RU	2304934	C2	8/2007	WO	WO-2006058223	A2	6/2006
RU	2405603	C1	12/2010	WO	WO-2006063199	A2	6/2006
SU	850068	A1	7/1981	WO	WO-2006083988	A1	8/2006
WO	WO-8103272	A1	11/1981	WO	WO-2006101661	A2	9/2006
WO	WO-9222259	A2	12/1992	WO	WO-2006119139	A2	11/2006
WO	WO-9307817	A1	4/1993	WO	WO-2006119376	A2	11/2006
WO	WO-9308757	A1	5/1993	WO	WO-2006129465	A1	12/2006
WO	WO-9314708	A1	8/1993	WO	WO-2007008703	A2	1/2007
WO	WO-9316646	A1	9/1993	WO	WO-2007008710	A2	1/2007
WO	WO-9320877	A1	10/1993	WO	WO-2007038538	A1	4/2007
WO	WO-9322973	A1	11/1993	WO	WO-2007040818	A1	4/2007
WO	WO-9400059	A1	1/1994	WO	WO-2007047380	A2	4/2007
WO	WO-9421183	A1	9/1994	WO	WO-2007047531	A2	4/2007
WO	WO-9424949	A1	11/1994	WO	WO-2007056590	A1	5/2007
WO	WO-9509572	A1	4/1995	WO	WO-2007087272	A2	8/2007
WO	WO-9510978	A1	4/1995	WO	WO-2007089724	A2	8/2007
WO	WO-9534259	A1	12/1995	WO	WO-2007143665	A2	12/2007
WO	WO-9630885	A1	10/1996	WO	WO-2008016886	A2	2/2008
WO	WO-9635382	A1	11/1996	WO	WO-2008020964	A2	2/2008
WO	WO-9639086	A1	12/1996	WO	WO-2008042021	A1	4/2008
WO	WO-9710764	A1	3/1997	WO	WO-2008045348	A2	4/2008
WO	WO-9800069	A1	1/1998	WO	WO-2008049084	A2	4/2008
WO	WO-9816156	A1	4/1998	WO	WO-2008051764	A2	5/2008
WO	WO-9826739	A1	6/1998	WO	WO-2008089174	A2	7/2008
WO	WO-9835621	A1	8/1998	WO	WO-2008099529	A1	8/2008
WO	WO-9837815	A1	9/1998	WO	WO-2008101356	A1	8/2008
WO	WO-9840020	A1	9/1998	WO	WO-2008118709	A1	10/2008
WO	WO-9847436	A1	10/1998	WO	WO-2008130793	A1	10/2008
WO	WO-9857588	A1	12/1998	WO	WO-2009010565	A1	1/2009
WO	WO-9920213	A1	4/1999	WO	WO-2009018067	A1	2/2009
WO	WO-9923960	A1	5/1999	WO	WO-2009018406	A2	2/2009
WO	WO-9940857	A1	8/1999	WO	WO-2009022614	A1	2/2009
WO	WO-9940861	A1	8/1999	WO	WO-2009027065	A1	3/2009
WO	WO-9952489	A1	10/1999	WO	WO-2009036818	A1	3/2009
WO	WO-0024330	A1	5/2000	WO	WO-2009039179	A1	3/2009
WO	WO-0024331	A1	5/2000	WO	WO-2009046234	A2	4/2009
WO	WO-0025691	A1	5/2000	WO	WO-2009059741	A1	5/2009
WO	WO-0064358	A2	11/2000	WO	WO-2009073402	A2	6/2009
WO	WO-0074585	A2	12/2000	WO	WO-2009082477	A2	7/2009
WO	WO-0124713	A1	4/2001	WO	WO-2009088550	A2	7/2009
WO	WO-0128444	A1	4/2001	WO	WO-2009120992	A2	10/2009
WO	WO-0154590	A1	8/2001	WO	WO-2009141616	A1	11/2009
WO	WO-0167970	A1	9/2001	WO	WO-2009149234	A1	12/2009
WO	WO-0172251	A1	10/2001	WO	WO-2010017149	A1	2/2010
WO	WO-0195810	A2	12/2001	WO	WO-2010017266	A1	2/2010
WO	WO-0224080	A2	3/2002	WO	WO-2010068783	A1	6/2010
WO	WO-0238057	A1	5/2002	WO	WO-2010104755	A1	9/2010
WO	WO-02062241	A1	8/2002	WO	WO-2011008672	A2	1/2011
WO	WO-02080797	A1	10/2002	WO	WO-2011/044338	A2	4/2011
WO	WO-03001986	A2	1/2003	WO	WO-2011044343	A2	4/2011
WO	WO-03013374	A1	2/2003	WO	WO-2011052939	A2	5/2011
WO	WO-03020339	A2	3/2003	WO	WO-2011060031	A1	5/2011
WO	WO-03028541	A2	4/2003	WO	WO-2011084768	A1	7/2011
WO	WO-03030708	A2	4/2003	WO	WO-2011089717	A1	7/2011
WO	WO-03068046	A2	8/2003	WO	WO-2011100321	A2	8/2011
WO	WO-03082133	A1	10/2003	WO	WO-2011144911	A1	11/2011
WO	WO-2004011037	A2	2/2004	WO	WO-2012044597	A1	4/2012
WO	WO-2004012615	A1	2/2004	WO	WO-2012044606	A2	4/2012
WO	WO-2004026104	A2	4/2004	WO	WO-2012061638	A1	5/2012
WO	WO-2004032754	A2	4/2004	WO	WO-2012061722	A2	5/2012
				WO	WO-2012128362	A1	9/2012
				WO	WO-2012135705	A1	10/2012
				WO	WO-2012135721	A1	10/2012
				WO	WO-2012/150567	A1	11/2012

(56) References Cited

FOREIGN PATENT DOCUMENTS

WO	WO-2012166510	A1	12/2012
WO	WO-2013018934	A1	2/2013
WO	WO-2013034629	A1	3/2013
WO	WO-2013062978	A2	5/2013
WO	WO-2013102602	A2	7/2013
WO	WO-2013154157	A1	10/2013
WO	WO-2014092108	A1	6/2014
WO	WO-2015197395	A8	12/2015
WO	WO-2016009921	A1	1/2016

OTHER PUBLICATIONS

Chen et al., "Heat-Induced Changes in the Mechanics of a Collagenous Tissue: Isothermal Free Shrinkage," Transactions of the ASME, vol. 119, pp. 372-378 (Nov. 1997).

Chen et al., "Phenomenological Evolution Equations for Heat-Induced Shrinkage of a Collagenous Tissue," IEEE Transactions on Biomedical Engineering, vol. 45, No. 10, pp. 1234-1240 (Oct. 1998).

Harris et al., "Altered Mechanical Behavior of Epicardium Due to Isothermal Heating Under Biaxial Isotonic Loads," Journal of Biomechanical Engineering, vol. 125, pp. 381-388 (Jun. 2003).

Moran et al., "Thermally Induced Shrinkage of Joint Capsule," Clinical Orthopaedics and Related Research, No. 281, pp. 248-255 (Dec. 2000).

Wall et al., "Thermal modification of collagen," J Shoulder Elbow Surg, No. 8, pp. 339-344 (Jul./Aug. 1999).

Wells et al., "Altered Mechanical Behavior of Epicardium Under Isothermal Biaxial Loading," Transactions of the ASME, Journal of Biomedical Engineering, vol. 126, pp. 492-497 (Aug. 2004).

Gibson, "Magnetic Refrigerator Successfully Tested," U.S. Department of Energy Research News, accessed online on Aug. 6, 2010 at <http://www.eurekalert.org/features/doi/2001-11/dl-mrs062802.php> (Nov. 1, 2001).

Humphrey, J.D., "Continuum Thermomechanics and the Clinical Treatment of Disease and Injury," Appl. Mech. Rev., vol. 56, No. 2 pp. 231-260 (Mar. 2003).

Kurt Gieck & Reiner Gieck, *Engineering Formulas* § 7.7 (7th ed. 1997).

National Semiconductors Temperature Sensor Handbook—<http://www.national.com/appinfo/tempsensors/files/temphb.pdf>; accessed online: Apr. 1, 2011.

Chen et al., "Heat-induced changes in the mechanics of a collagenous tissue: pseudoelastic behavior at 37° C," Journal of Biomechanics, 31, pp. 211-216 (1998).

Hayashi et al., "The Effect of Thermal Heating on the Length and Histologic Properties of the Glenohumeral Joint Capsule," American Journal of Sports Medicine, vol. 25, Issue 1, 11 pages (Jan. 1997), URL: <http://www.mdconsult.com/das/article/body/156183648-2/jorg=journal&source=MI&sp=1> . . . , accessed Aug. 25, 2009.

Lee et al., "A multi-sample denaturation temperature tester for collagenous biomaterials," Med. Eng. Phys., vol. 17, No. 2, pp. 115-121 (Mar. 1995).

Weir, C.E., "Rate of shrinkage of tendon collagen—heat, entropy and free energy of activation of the shrinkage of untreated tendon. Effect of acid salt, pickle, and tannage on the activation of tendon collagen." Journal of the American Leather Chemists Association, 44, pp. 108-140 (1949).

Wright, et al., "Time-Temperature Equivalence of Heat-Induced Changes in Cells and Proteins," Feb., 1998. ASME Journal of Biomechanical Engineering, vol. 120, pp. 22-26.

Arnoczky et al., "Thermal Modification of Connective Tissues: Basic Science Considerations and Clinical Implications," J. Am Acad Orthop Surg, vol. 8, No. 5, pp. 305-313 (Sep./Oct. 2000).

Chen et al., "Heat-Induced Changes in the Mechanics of a Collagenous Tissue: Isothermal, Isotonic Shrinkage," Transactions of the ASME, vol. 120, pp. 382-388 (Jun. 1998).

Harris et al., "Kinetics of Thermal Damage to a Collagenous Membrane Under Biaxial Isotonic Loading," IEEE Transactions on Biomedical Engineering, vol. 51, No. 2, pp. 371-379 (Feb. 2004).

Covidien Brochure, [Value Analysis Brief], LigaSure Advance™ Pistol Grip, dated Rev. Apr. 2010 (7 pages).

Covidien Brochure, LigaSure Impact™ Instrument LF4318, dated Feb. 2013 (3 pages).

Covidien Brochure, LigaSure Atlas™ Hand Switching Instruments, dated Dec. 2008 (2 pages).

Covidien Brochure, The LigaSure™ 5 mm Blunt Tip Sealer/Divider Family, dated Apr. 2013 (2 pages).

Sullivan, "Optimal Choice for No. Of Strands in a Litz-Wire Transformer Winding," IEEE Transactions on Power Electronics, vol. 14, No. 2, Mar. 1999, pp. 283-291.

<https://www.kjmagnetics.com/fieldcalculator.asp>, retrieved Jul. 11, 2016, backdated to Nov. 11, 2011 via <https://web.archive.org/web/20111116164447/http://www.kjmagnetics.com/fieldcalculator.asp>.

Douglas, S.C. "Introduction to Adaptive Filter". Digital Signal Processing Handbook. Ed. Vijay K. Madisetti and Douglas B. Williams. Boca Raton: CRC Press LLC, 1999.

Leonard I. Malis, M.D., "The Value of Irrigation During Bipolar Coagulation," 1989.

Covidien Brochure, The LigaSure Precise™ Instrument, dated Mar. 2011 (2 pages).

Jang, J. et al. "Neuro-fuzzy and Soft Computing." Prentice Hall, 1997, pp. 13-89, 199-293, 335-393, 453-496, 535-549.

AST Products, Inc., "Principles of Video Contact Angle Analysis," 20 pages, (2006).

Lim et al., "A Review of Mechanism Used in Laparoscopic Surgical Instruments," Mechanism and Machine Theory, vol. 38, pp. 1133-1147, (2003).

F. A. Duck, "Optical Properties of Tissue Including Ultraviolet and Infrared Radiation," pp. 43-71 in Physical Properties of Tissue (1990).

Erbe Electrosurgery VIO® 200 S, (2012), p. 7, 12 pages, accessed Mar. 31, 2014 at http://www.erbe-med.com/erbe/media/Marketingmaterialien/85140170_ERBE_EN_VIO_200_S_D027541.

Graff, K.F., "Elastic Wave Propagation in a Curved Sonic Transmission Line," IEEE Transactions on Sonics and Ultrasonics, SU-17(1), 1-6 (1970).

Makarov, S. N., Ochmann, M., Desinger, K., "The longitudinal vibration response of a curved fiber used for laser ultrasound surgical therapy," Journal of the Acoustical Society of America 102, 1191-1199 (1997).

Morley, L. S. D., "Elastic Waves in a Naturally Curved Rod," Quarterly Journal of Mechanics and Applied Mathematics, 14: 155-172 (1961).

Walsh, S. J., White, R. G., "Vibrational Power Transmission in Curved Beams," Journal of Sound and Vibration, 233(3), 455-488 (2000).

Covidien 501(k) Summary Sonication, dated Feb. 24, 2011 (7 pages).

Gerhard, Glen C., "Surgical Electrotechnology: Quo Vadis?," IEEE Transactions on Biomedical Engineering, vol. BME-31, No. 12, pp. 787-792, Dec. 1984.

Technology Overview, printed from www.harmonicscalpel.com, Internet site, website accessed on Jun. 13, 2007, (3 pages).

Sheritt et al., "Novel Horn Designs for Ultrasonic/Sonic Cleaning Welding, Soldering, Cutting and Drilling," Proc. SPIE Smart Structures Conference, vol. 4701, Paper No. 34, San Diego, CA, pp. 353-360, Mar. 2002.

Gooch et al., "Recommended Infection-Control Practices for Dentistry, 1993," Published: May 28, 1993; [retrieved on Aug. 23, 2008]. Retrieved from the internet: URL: <http://wonder.cdc.gov/wonder/prevguid/p0000191/p0000191.asp> (15 pages).

Huston et al., "Magnetic and Magnetostrictive Properties of Cube Textured Nickel for Magnetostrictive Transducer Applications," IEEE Transactions on Magnetics, vol. 9(4), pp. 636-640 (Dec. 1973).

Sullivan, "Cost-Constrained Selection of Strand Diameter and Number in a Litz-Wire Transformer Winding," IEEE Transactions on Power Electronics, vol. 16, No. 2, Mar. 2001, pp. 281-288.

(56)

References Cited

OTHER PUBLICATIONS

Fowler, K.R., "A Programmable, Arbitrary Waveform Electrosurgical Device," IEEE Engineering in Medicine and Biology Society 10th Annual International Conference, pp. 1324, 1325 (1988).
LaCourse, J.R.; Vogt, M.C.; Miller, W.T., III; Selikowitz, S.M., "Spectral Analysis Interpretation of Electrosurgical Generator Nerve and Muscle Stimulation," IEEE Transactions on Biomedical Engineering, vol. 35, No. 7, pp. 505-509, Jul. 1988.
Orr et al., "Overview of Bioheat Transfer," pp. 367-384 in Optical-Thermal Response of Laser-Irradiated Tissue, A. J. Welch and M. J. C. van Gernert, eds., Plenum, New York (1995).
Campbell et al., "Thermal Imaging in Surgery," p. 19-3, in Medical Infrared Imaging, N. A. Diakides and J. D. Bronzino, Eds. (2008).
Hörmann et al., "Reversible and irreversible denaturation of collagen fibers." Biochemistry, 10, pp. 932-937 (1971).
Dean, D.A., "Electrical Impedance Spectroscopy Study of Biological Tissues," J. Electrostat, 66(3-4), Mar. 2008, pp. 165-177. Accessed Apr. 10, 2018: <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC2597841/>.

* cited by examiner

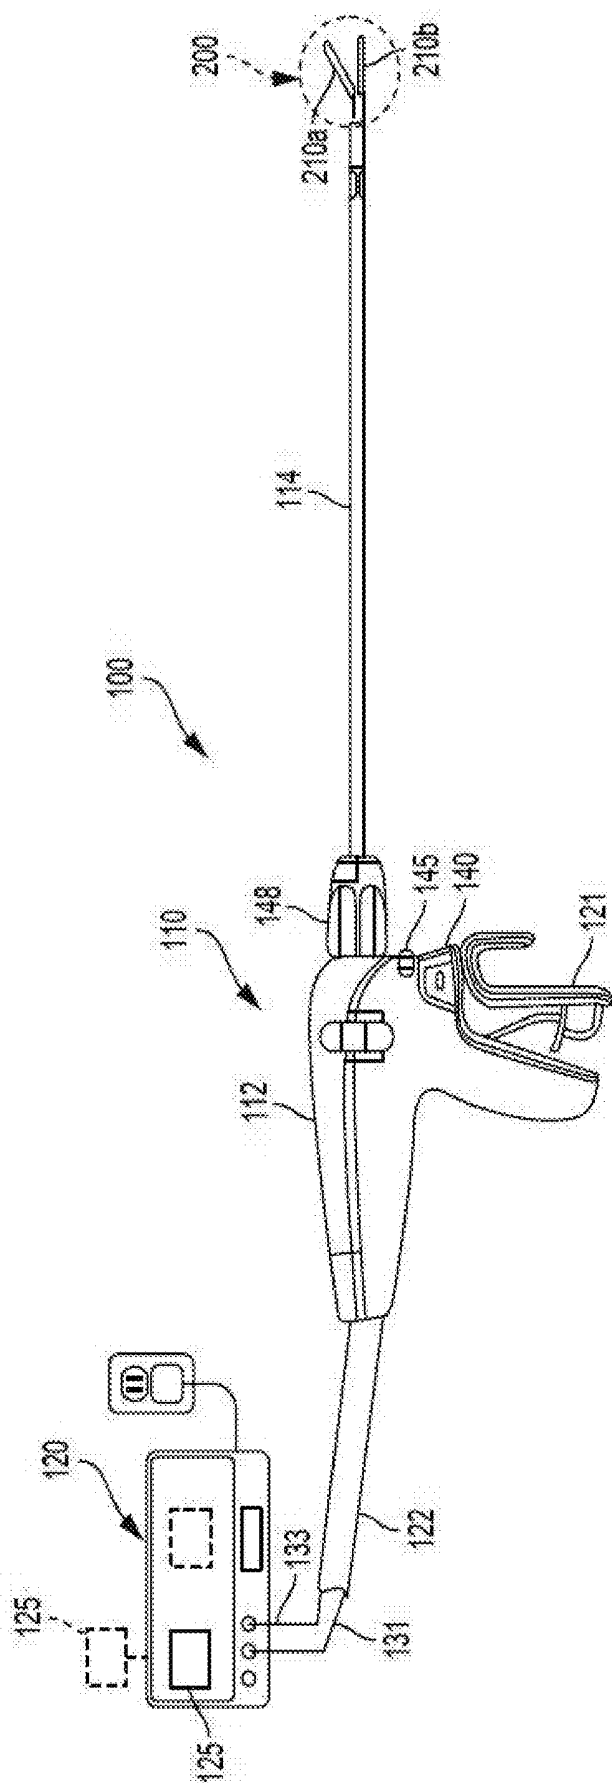


FIG. 1 A

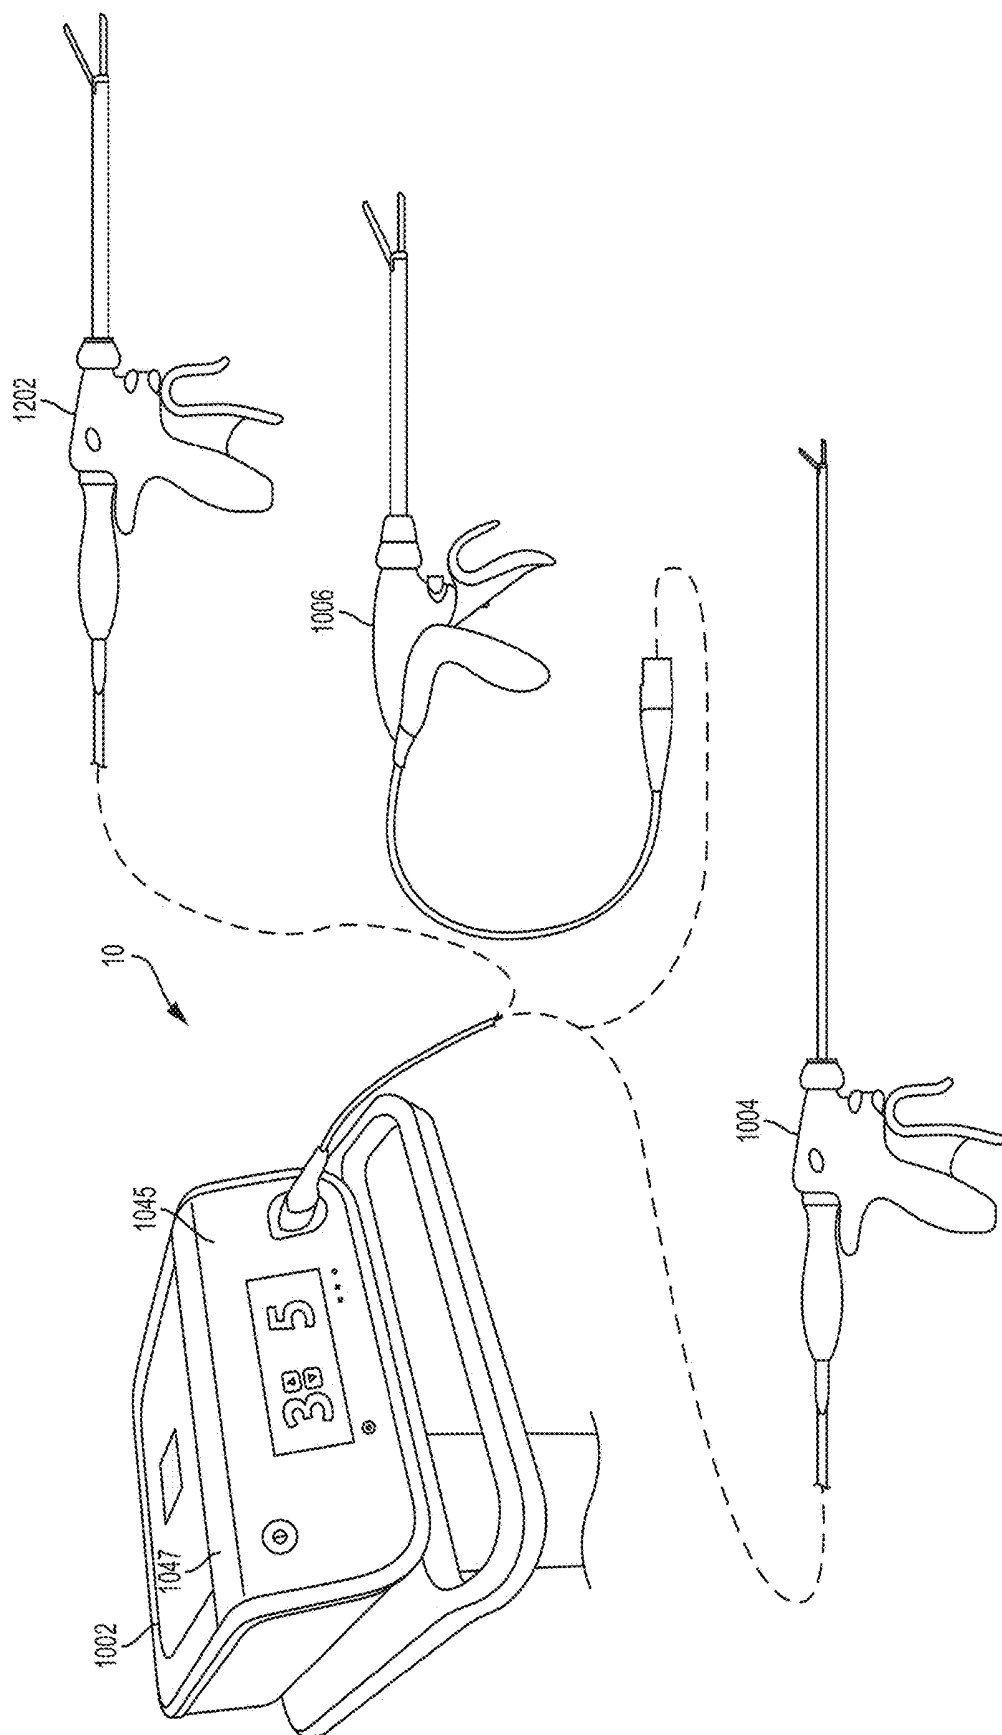


FIG. 1B


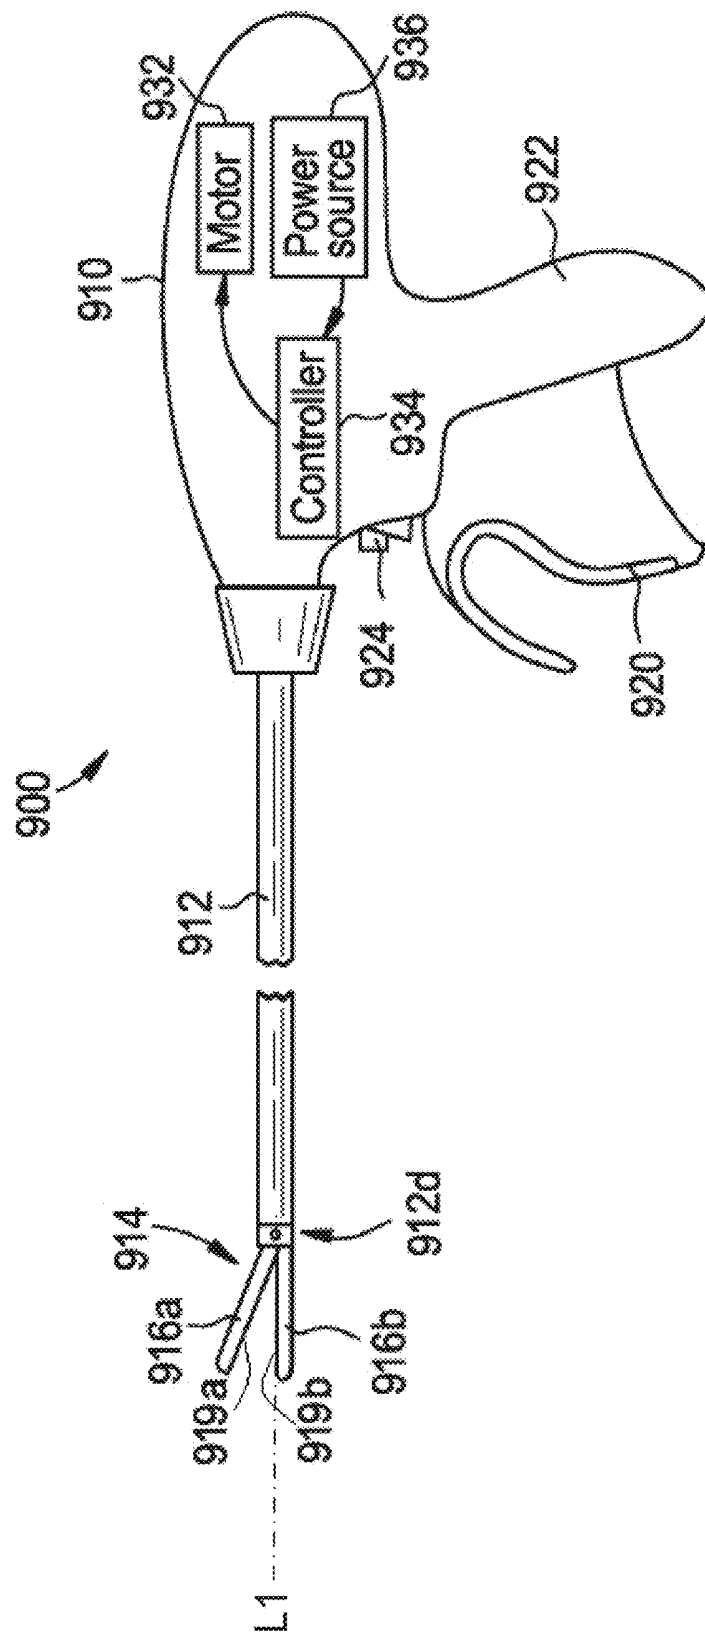


FIG. 1C

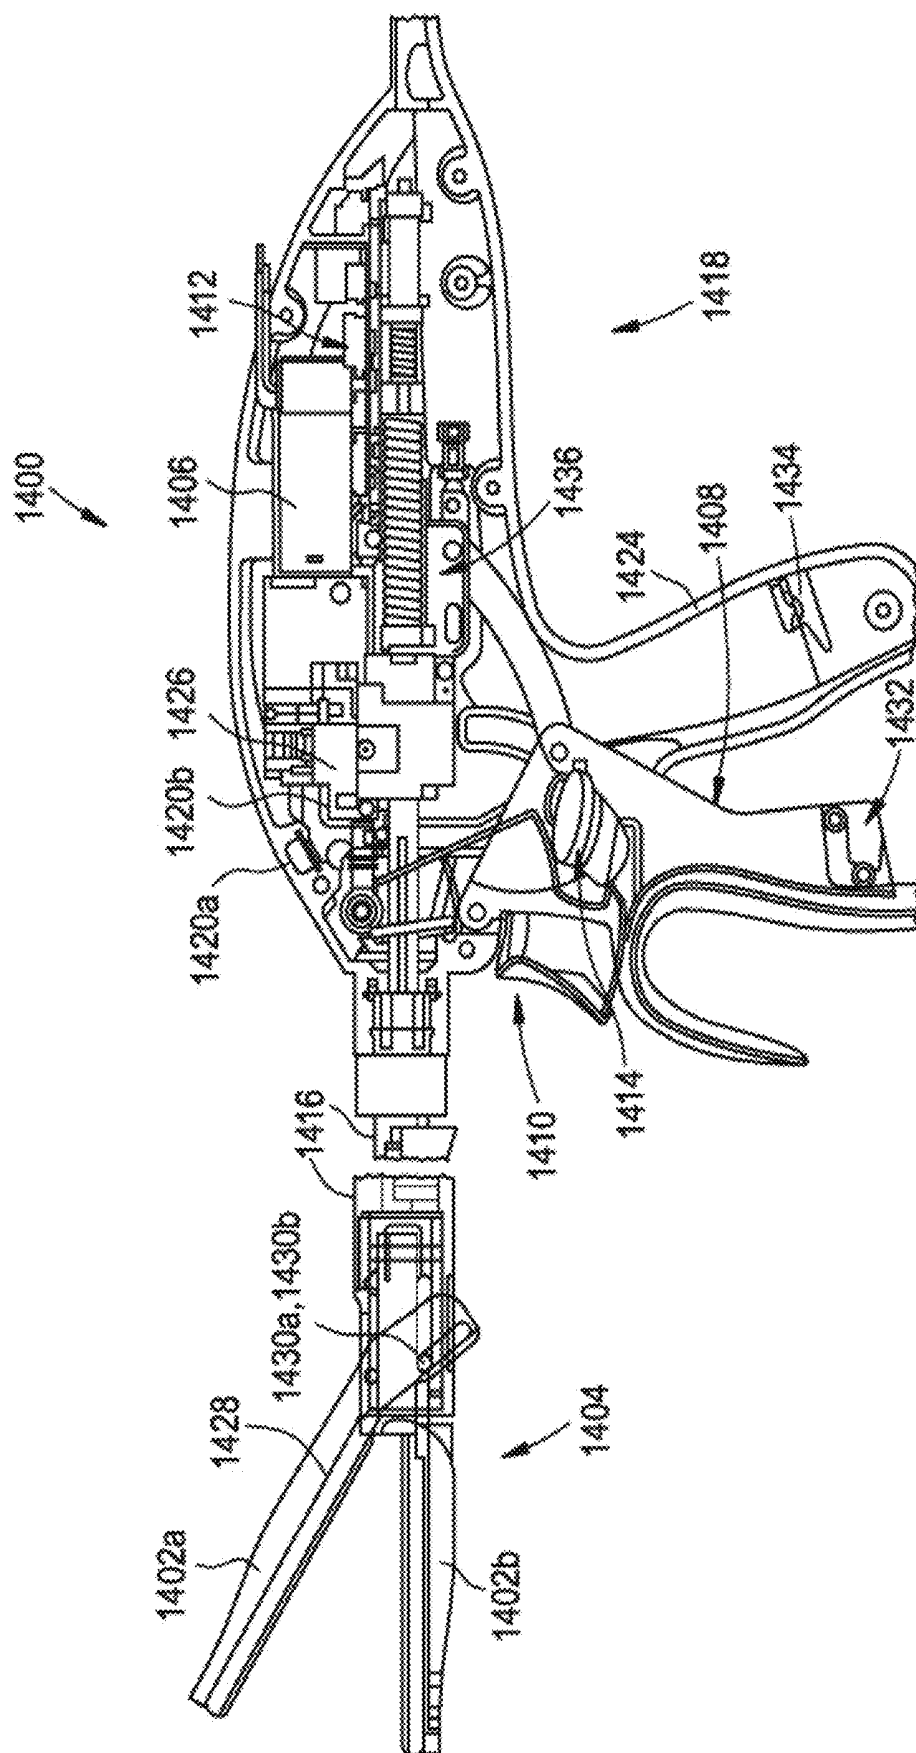

100

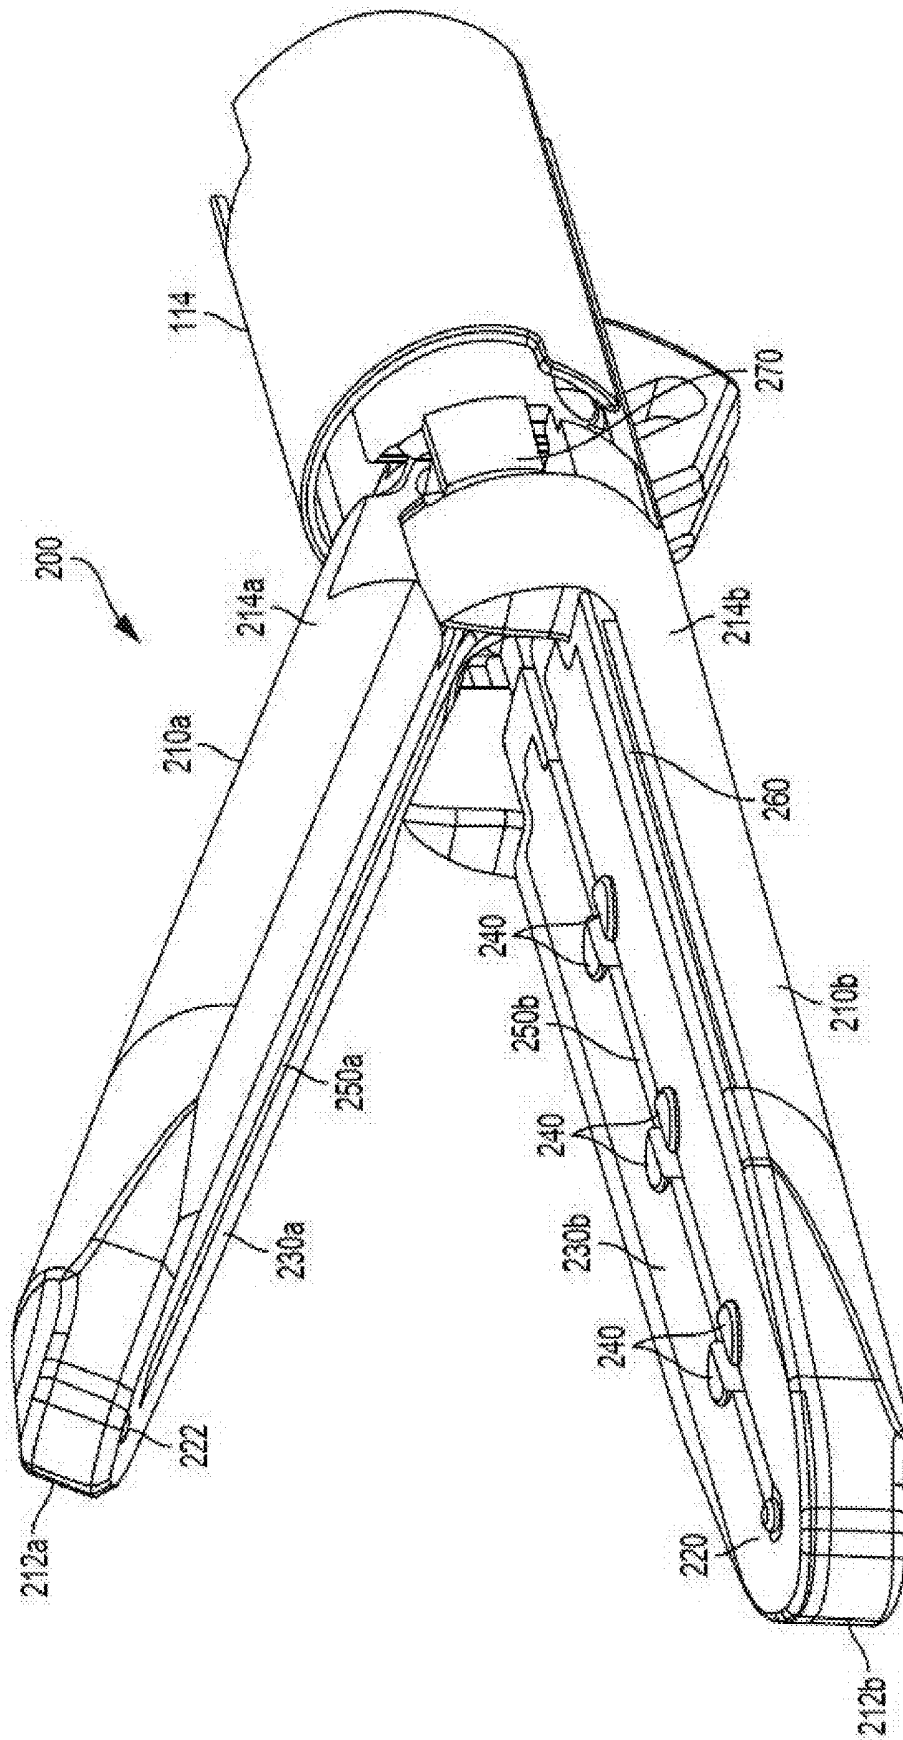


FIG. 2

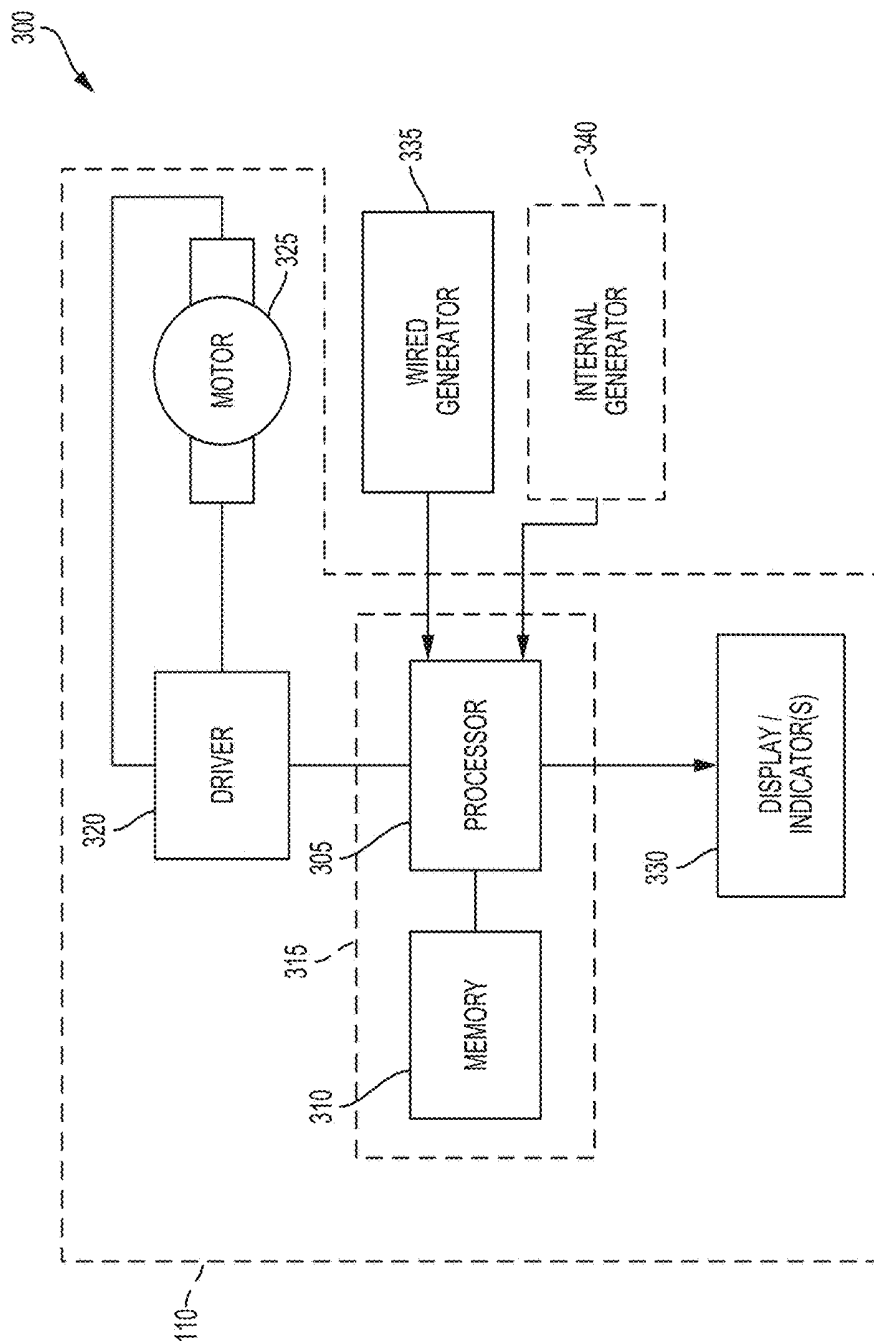


FIG. 3

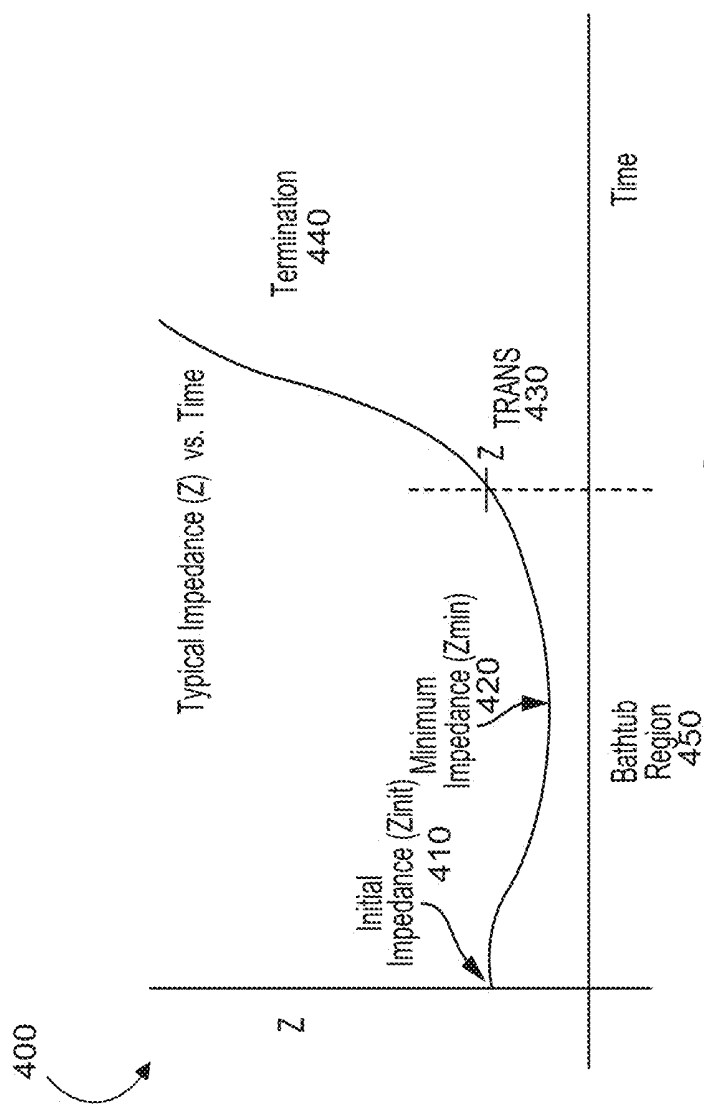


FIG. 4A

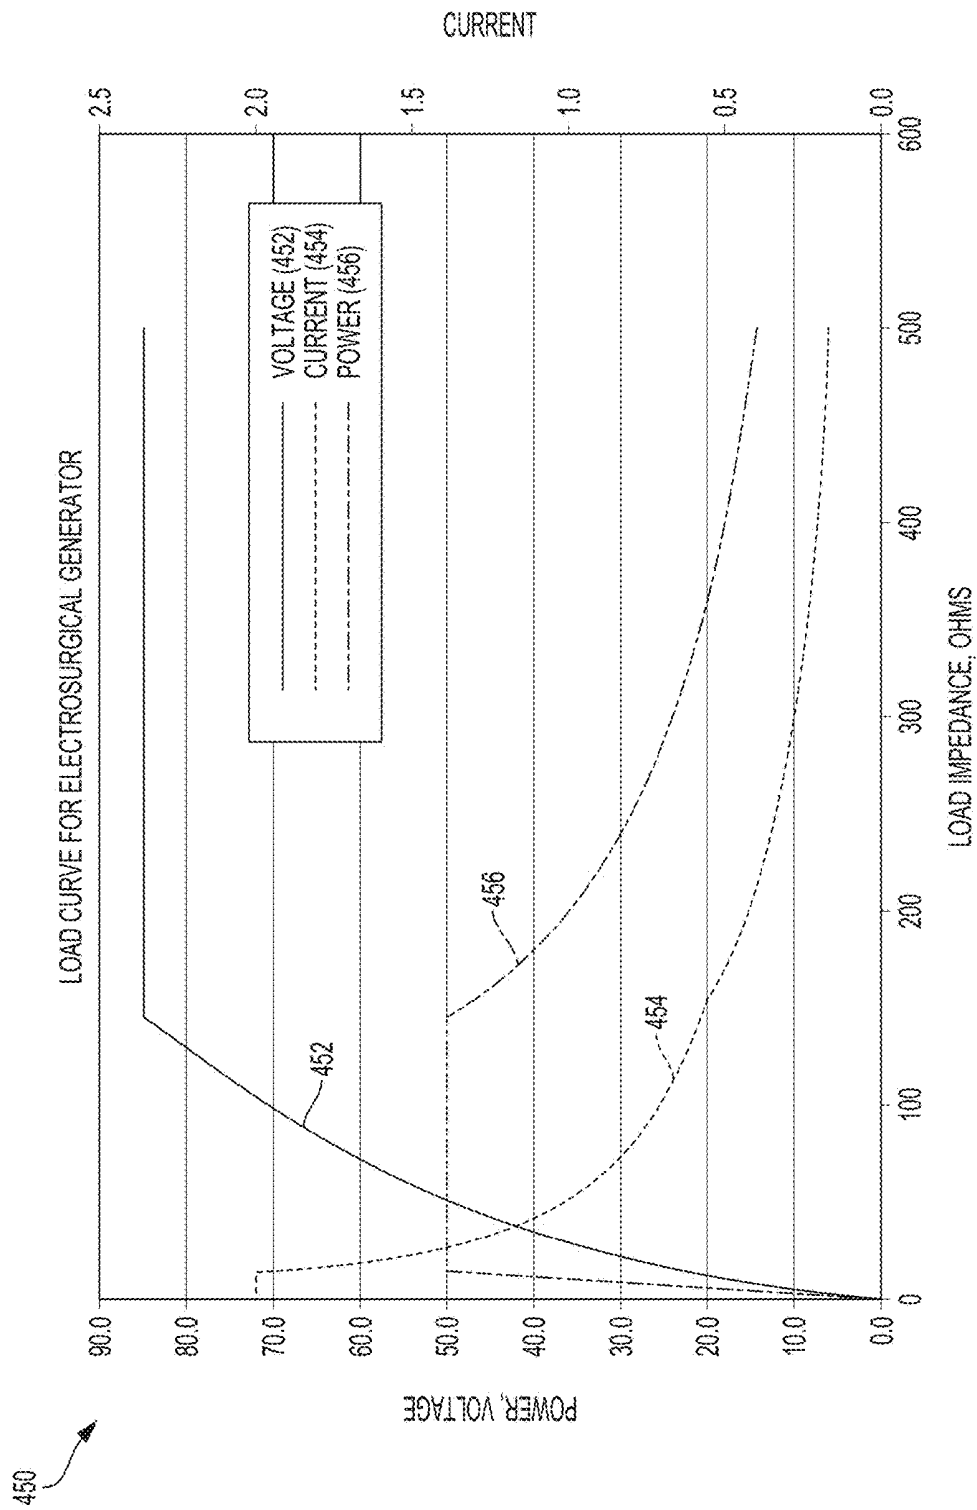


FIG. 4B

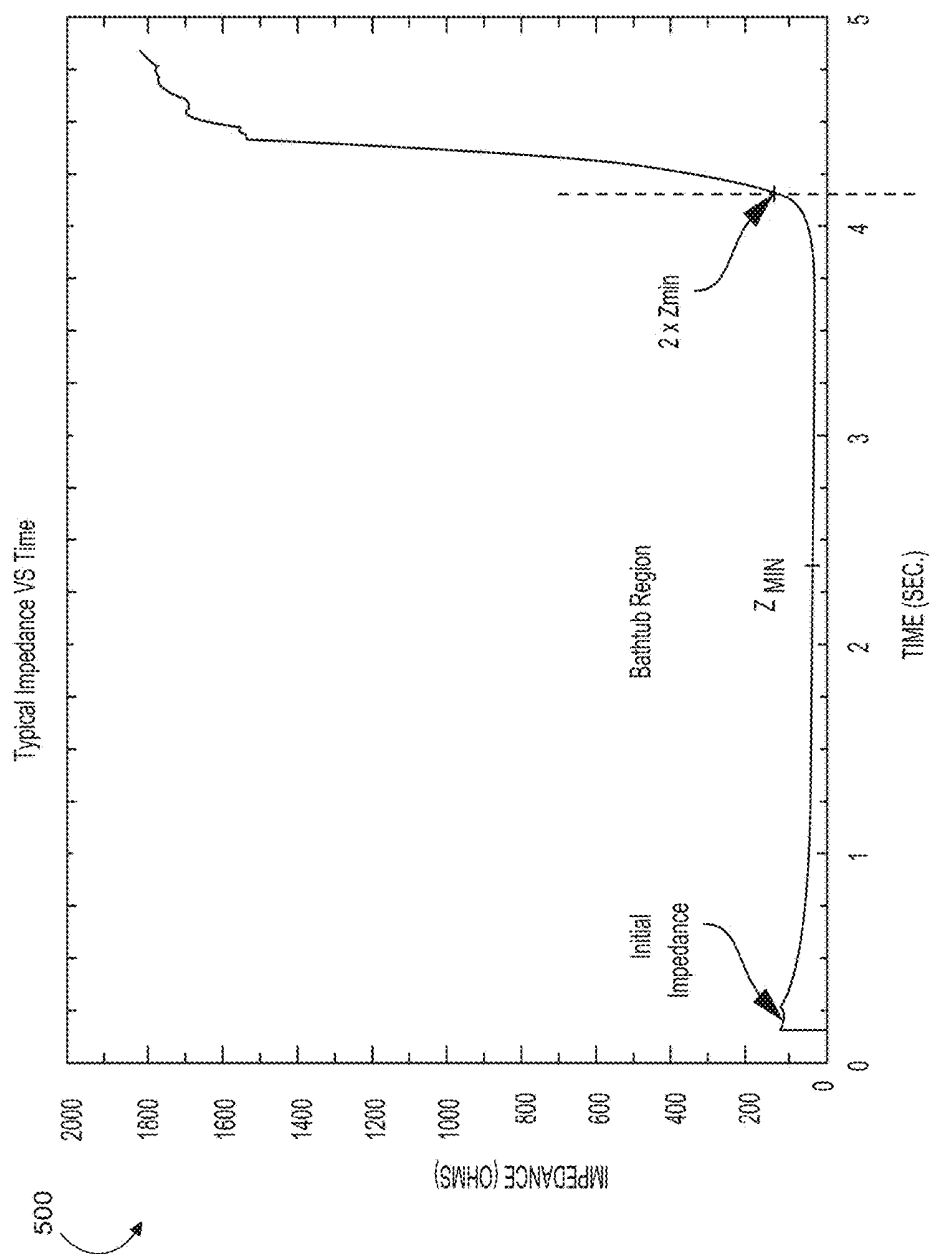


FIG. 5

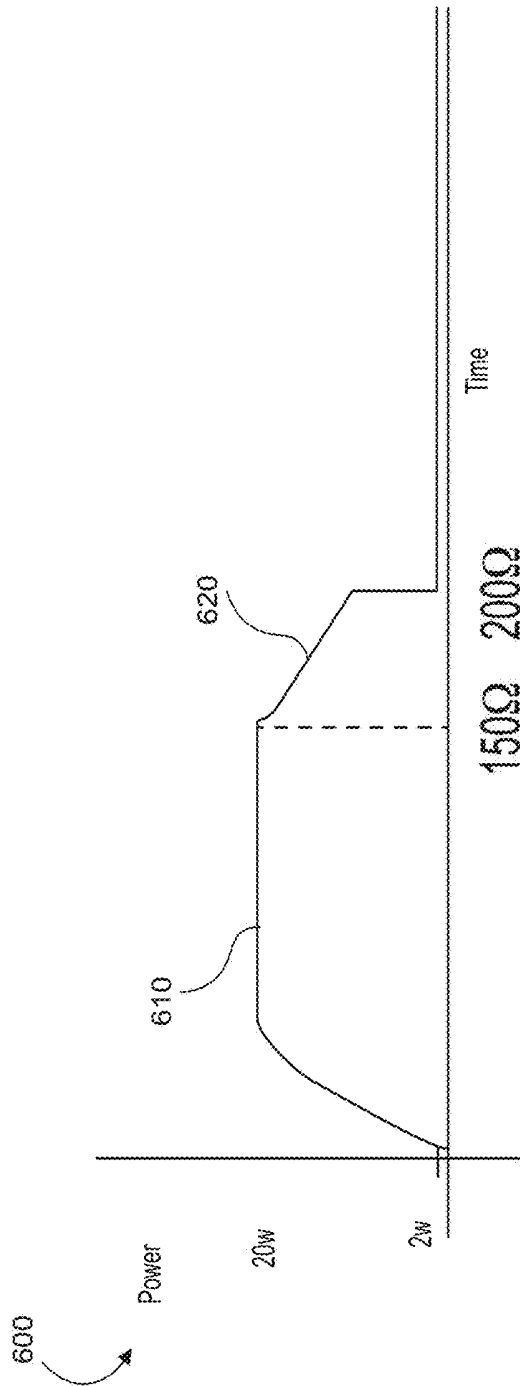


FIG. 6A

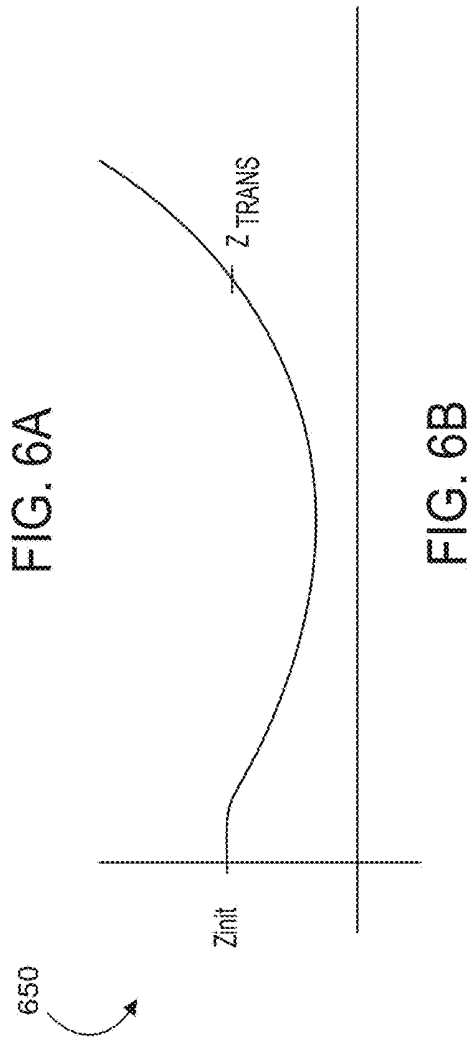


FIG. 6B

700

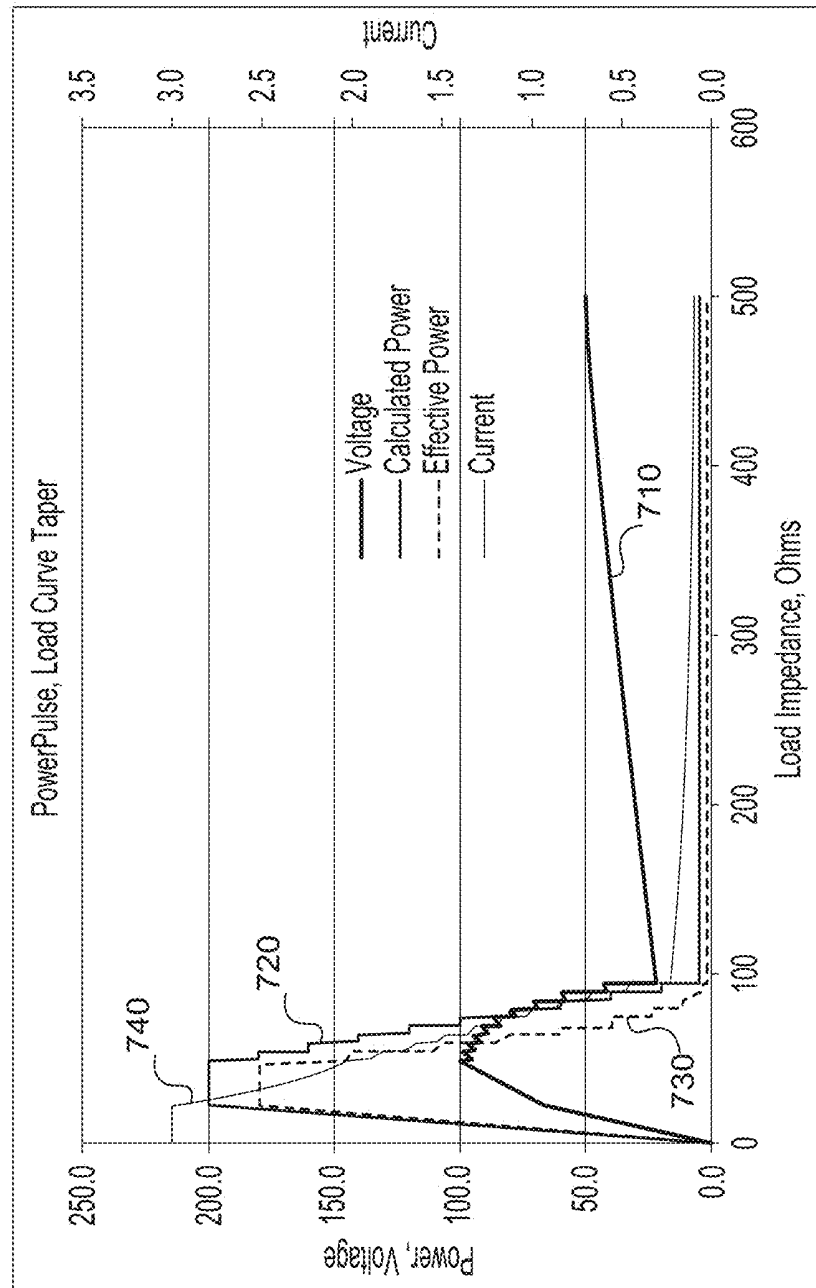


FIG. 7

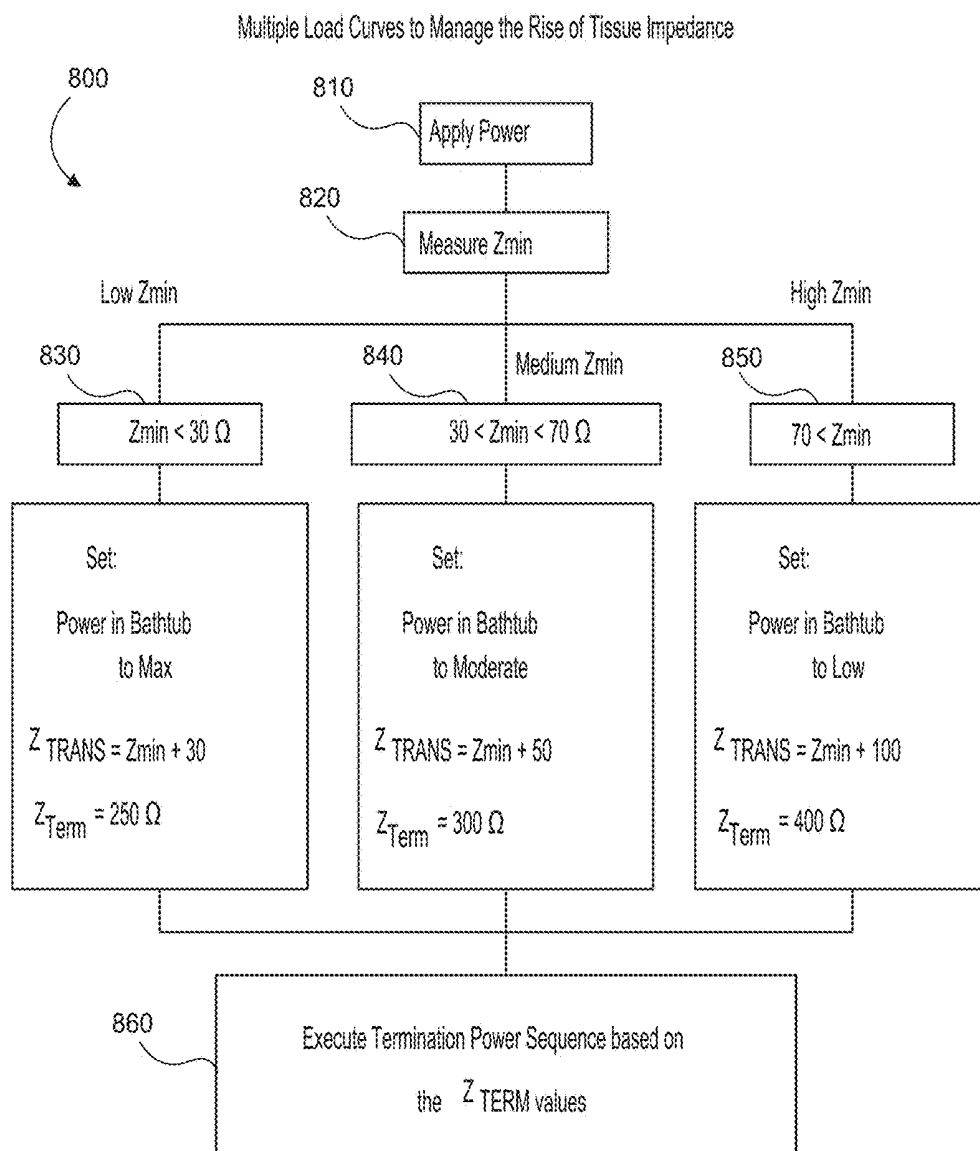


FIG. 8

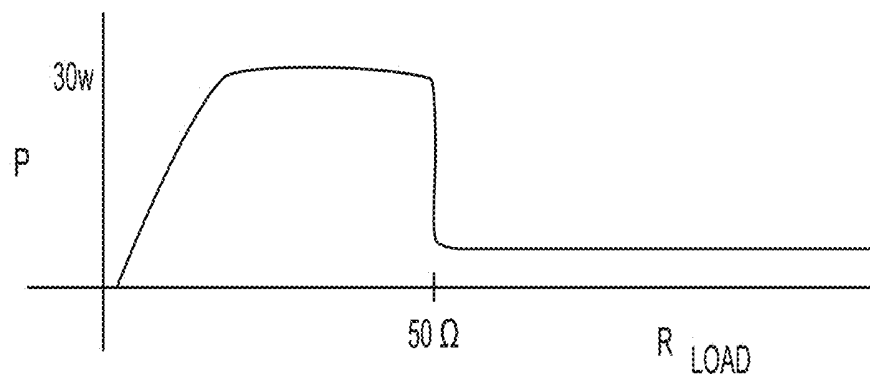


FIG. 9

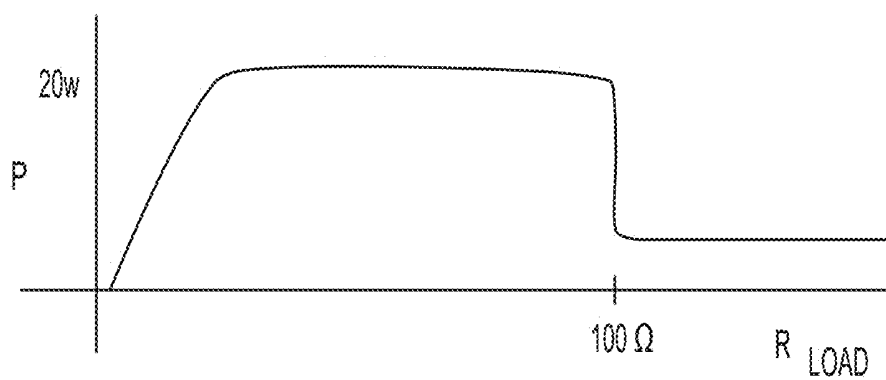


FIG. 10

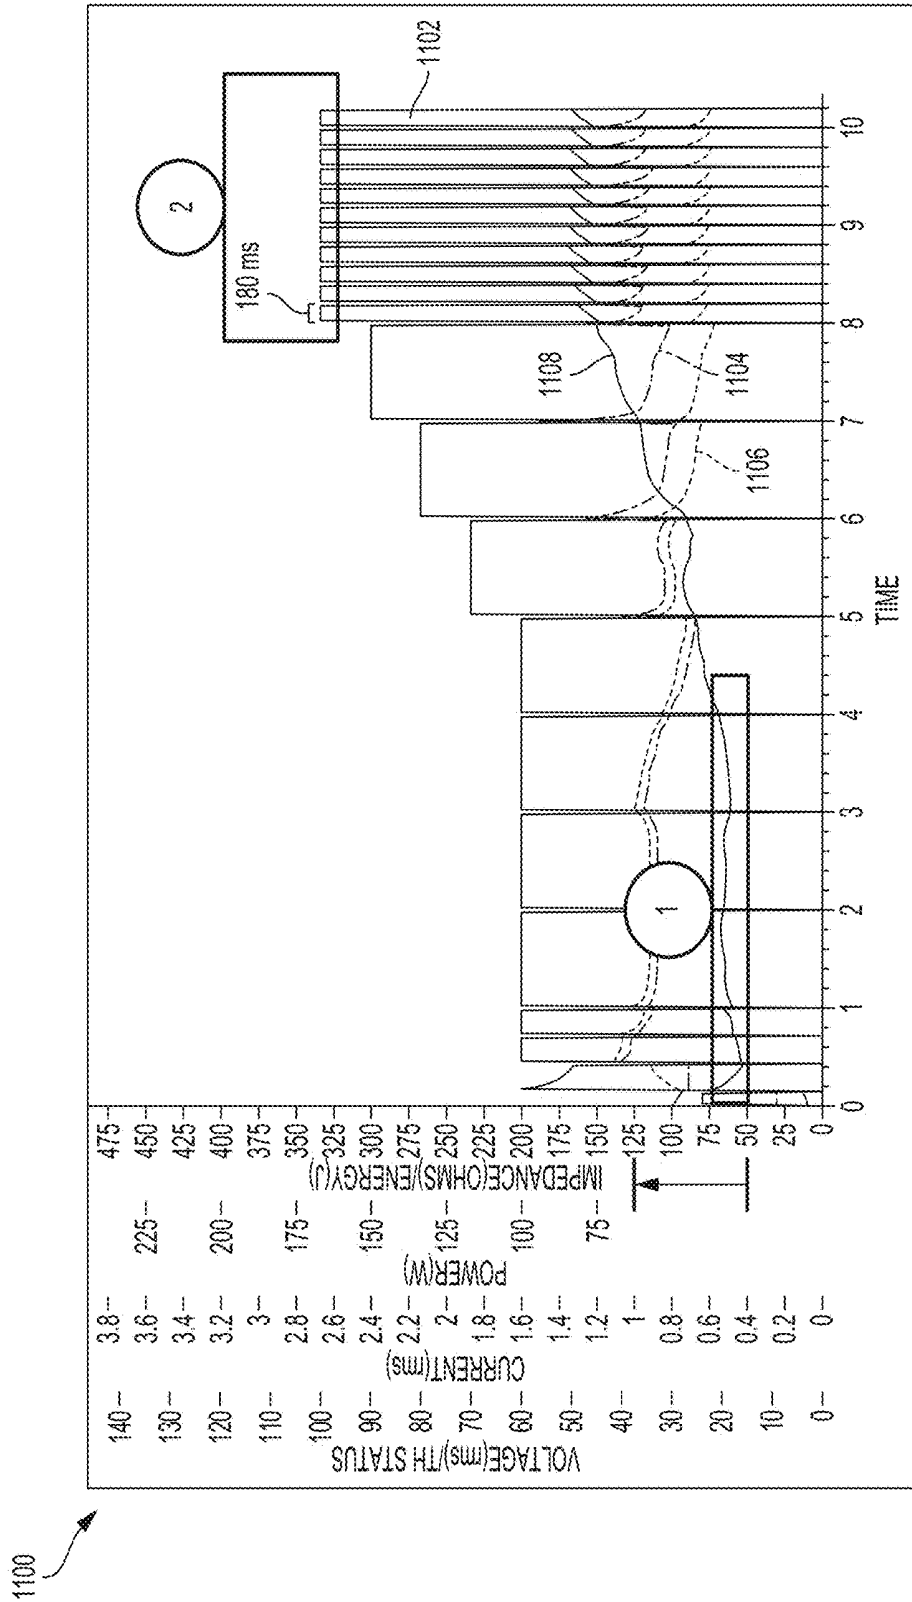


FIG. 11

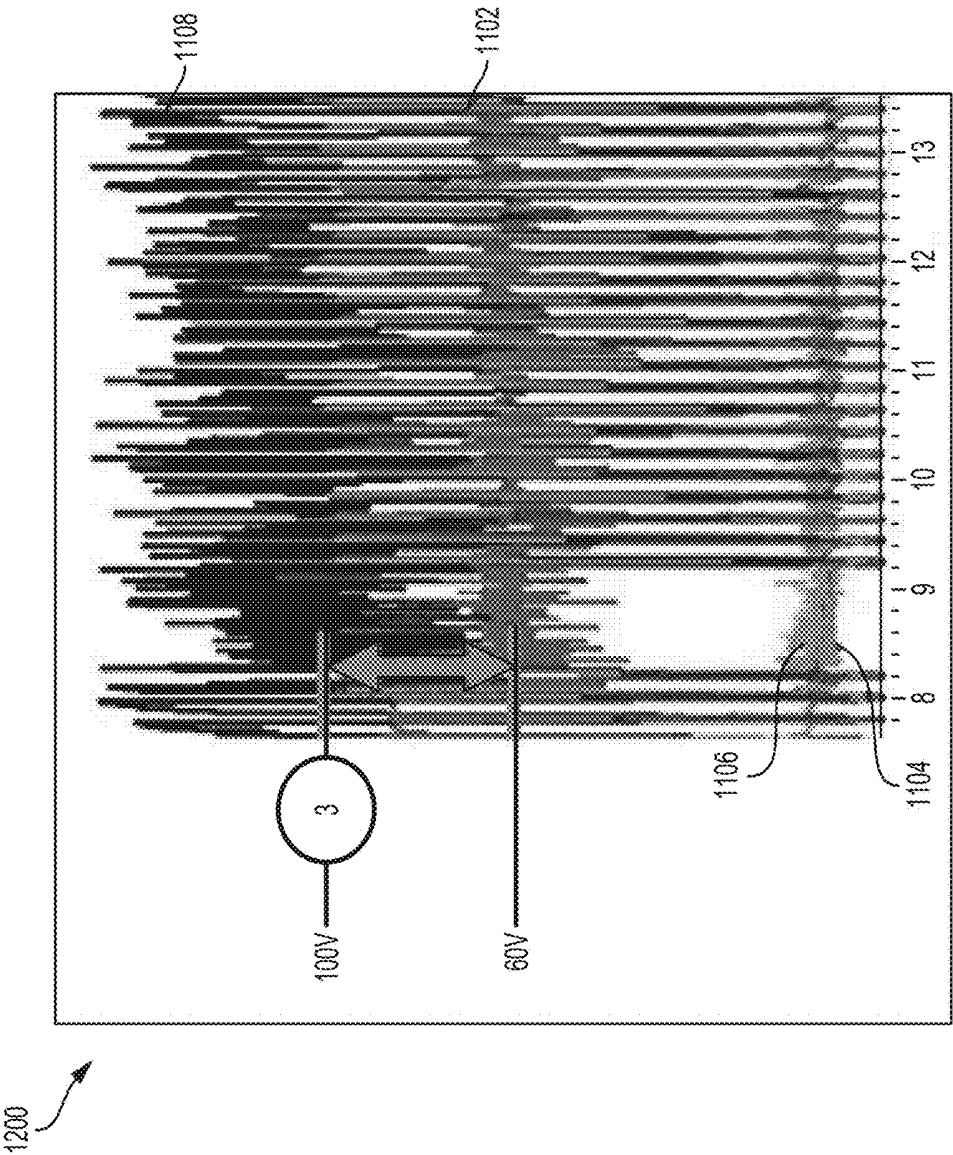


FIG. 12

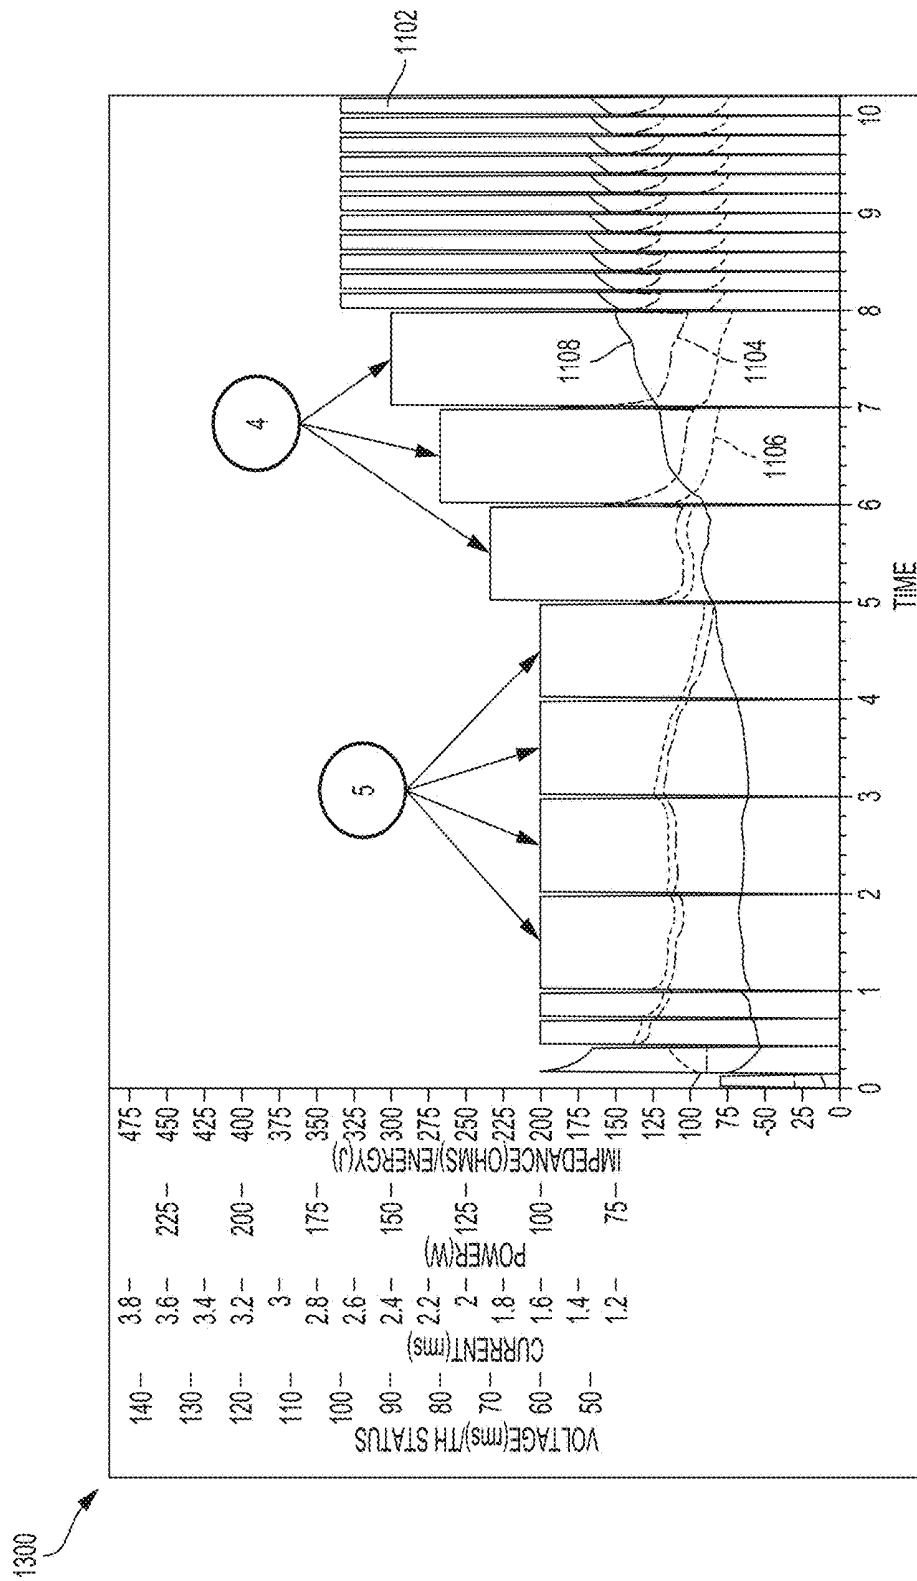


FIG. 13

METHODS AND SYSTEMS FOR ADVANCED HARMONIC ENERGY

TECHNICAL FIELD

The present disclosure is related generally to medical devices with various mechanisms for grasping and sealing tissue. In particular, the present disclosure is related to electrosurgical instruments configured to regulate the application of energy applied to a surgical site to prolong the sealing time duration when performing sealing procedures.

BACKGROUND

Electrosurgical instruments are a type of surgical instrument used in many surgical operations. Electrosurgical instruments apply electrical energy to tissue in order to treat tissue. An electrosurgical instrument may comprise an instrument having a distally-mounted end effector comprising one or more electrodes. The end effector can be positioned against tissue such that electrical current is introduced into the tissue. Electrosurgical instruments can be configured for bipolar or monopolar operation. During bipolar operation, current is introduced into and returned from the tissue by active and return electrodes, respectively, of the end effector. During monopolar operation, current is introduced into the tissue by an active (or source) electrode of the end effector and returned through a return electrode (e.g., a grounding pad) separately located on a patient's body. Heat generated by the current flow through the tissue may form hemostatic seals within the tissue and/or between tissues and thus may be particularly useful for sealing blood vessels, for example. The end effector of an electrosurgical instrument sometimes also comprises a cutting member that is moveable relative to the tissue and the electrodes to transect the tissue.

Energy applied by an electrosurgical instrument can be transmitted to the instrument by a generator. The generator may form an electrosurgical signal that is applied to an electrode or electrodes of the electrosurgical instrument. The generator may be external or integral to the electrosurgical instrument. The electrosurgical signal may be in the form of radio frequency ("RF") energy. For example, RF energy may be provided at a frequency range of between 100 kHz and 1 MHz. During operation, an electrosurgical instrument can transmit RF energy through tissue, which causes ionic agitation, or friction, in effect resistive heating, thereby increasing the temperature of the tissue. Because a sharp boundary may be created between the affected tissue and the surrounding tissue, surgeons can operate with a high level of precision and control, without sacrificing un-targeted adjacent tissue. The low operating temperatures of RF energy may be useful for removing, shrinking, or sculpting soft tissue while simultaneously sealing blood vessels. RF energy may work particularly well on connective tissue, which is primarily comprised of collagen and shrinks when contacted by heat. In some cases, the instrument may also be configured to apply ultrasonic energy to create homeostasis. The generator may be configured to transmit energy which is converted into ultrasonic vibrations at the end effector. The energy transmitted to the tissue may similarly cause resistive heating through the ultrasonic vibrations.

During the application of the energy to tissue, the impedance of the tissue indicates the condition of the tissue. After a certain amount of energy applied, the impedance of the tissue dramatically increases and reduces the effectiveness of the further energy applied in the sealing procedure.

Furthermore, as the tissue impedance approaches this threshold level where further energy applied is no longer effective, certain chemical processes in the tissue occur that would be desirable to be controlled better. The period of time under which the tissue responds to the sealing energy is sometimes referred to as the "bathtub region," based on the shape of the level of impedance over time at which the tissue effectively responds to the sealing energy. There is a need therefore to better control the rise of impedance levels in the tissue and to prolong the period under which the tissue still responds (e.g., prolong the "bathtub region") to applied energy during sealing procedures. While several devices have been made and used, it is believed that no one prior to the inventors has made or used the device described in the appended claims.

SUMMARY

In some aspects, a surgical system is provided.

In one aspect, the surgical system may include: an end effector comprising at least one energy delivery component configured to transmit electrosurgical energy at a number of different power levels (i.e., rates of energy delivery or levels of energy delivery) to tissue at a surgical site; and a control circuit communicatively coupled to the energy delivery component and programmed to: for a first application period, cause the energy delivery component to transmit the electrosurgical energy at a first power level or rate of energy delivery, the first application period comprising a point in time where impedance of the tissue reaches a minimum value; for a second application period after the first application period, cause the energy delivery component to transmit the electrosurgical energy at a decreasing power level or rate of energy level from the first power level until a second power level is reached, the second power level lower than the first power level and the second application period comprising a point in time where the impedance of the tissue rises above the minimum impedance value; for a third application period after the second application period, cause the energy delivery component to transmit the electrosurgical energy at a third power level, the third power level lower than the second power level and the third application period comprising a point in time where the impedance of the tissue rises above a transition impedance threshold level.

In another aspect of the surgical system, the first application period and the second application period combined comprise a time period where the electrosurgical energy causes sealing of the tissue at the surgical site.

In another aspect of the surgical system, the third application period further comprises a time period where the impedance of the tissue rises to a level such that the electrosurgical energy no longer causes sealing of the tissue at the surgical site.

In another aspect, the surgical system further comprises at least one sensor configured to measure an initial level of impedance in the tissue and a minimum level of impedance in the tissue.

In another aspect of the surgical system, the control circuit is further programmed to determine a beginning of the third application period based on the measured initial level of impedance in the tissue.

In another aspect of the surgical system, the control circuit is further programmed to determine a beginning of the third application period based on the measured minimum level of impedance in the tissue.

In another aspect of the surgical system, the first application period and the second application period combined comprise a continuous time period where the tissue impedance remains below an initial level of impedance in the tissue.

In another aspect of the surgical system, the energy delivery component is configured to transmit RF and ultrasonic energy.

In other aspects, a method for transmitting electrosurgical energy to tissue at a surgical site by a surgical system is provided. The method may include: causing, by an energy delivery component of a surgical system, electrosurgical energy to be applied to the tissue; measuring, by at least one sensor of the surgical system, a benchmark level of impedance of the tissue; determining, among a plurality of power load curve algorithms, a power load curve algorithm to be applied to the energy delivery component, based on the measured benchmark level of impedance of the tissue; based on the determined power load curve algorithm: for a first application period, causing the energy delivery component to transmit the electrosurgical energy at a first power level, the first application period comprising a point in time where impedance of the tissue reaches a minimum value; for a second application period after the first application period, cause the energy delivery component to transmit the electrosurgical energy at a decreasing power level from the first power level until a second power level is reached, the second power level lower than the first power level and the second application period comprising a point in time where the impedance of the tissue rises above the minimum impedance value; for a third application period after the second application period, cause the energy delivery component to transmit the electrosurgical energy at a third power level, the third power level lower than the second power level and the third application period comprising a point in time where the impedance of the tissue rises above a transition impedance threshold level.

In other aspects of the method, determining the power load curve algorithm comprises determining whether the benchmark level of impedance is less than a first threshold impedance value, whether the benchmark level of impedance is greater than the first threshold impedance value and less than a second threshold impedance value, and whether the benchmark level of impedance is greater than the second threshold impedance value.

In other aspects of the method, the first application period and the second application period combined comprise a time period where the electrosurgical energy is delivered at a higher rate and causes sealing of the tissue at the surgical site.

In other aspects of the method, the third application period further comprises a time period where the impedance of the tissue rises to a level such that the electrosurgical energy is delivered at a lower rate and no longer causes sealing of the tissue at the surgical site.

In other aspects of the method, the benchmark level of impedance is the minimum impedance value or an initial level of impedance of the tissue.

In other aspects of the method, a beginning of the third application period is based on the measured benchmark level of impedance.

In other aspects of the method, the first application period and the second application period combined comprise a continuous time period where the tissue impedance remains below an initial level of impedance in the tissue.

In other aspects of the method, the energy delivery component is configured to transmit RF and ultrasonic energy.

In other aspects, a surgical instrument is provided. The surgical instrument may include: a handle assembly; a shaft coupled to a distal end of the handle assembly; an end effector coupled to a distal end of the shaft and comprising at least one energy delivery component configured to transmit electrosurgical energy to tissue at a surgical site; and a control circuit communicatively coupled to the energy delivery component and programmed to: for a first application period, cause the energy delivery component to transmit the electrosurgical energy at a first energy level, the first application period comprising a point in time where impedance of the tissue reaches a minimum value; for a second application period after the first application period, cause the energy delivery component to transmit the electrosurgical energy at a decreasing energy level from the first energy level until a second energy level is reached, the second energy level lower than the first energy level and the second application period comprising a point in time where the impedance of the tissue rises above the minimum impedance value; for a third application period after the second application period, cause the energy delivery component to transmit the electrosurgical energy at a third energy level, the third energy level lower than the second energy level and the third application period comprising a point in time where the impedance of the tissue rises above a transition impedance threshold level.

In another aspect of the surgical instrument, the first application period and the second application period combined comprise a time period where the electrosurgical energy causes sealing of the tissue at the surgical site.

In another aspect of the surgical instrument, the third application period further comprises a time period where the impedance of the tissue rises to a level such that the electrosurgical energy no longer causes sealing of the tissue at the surgical site.

In another aspect, the surgical instrument further comprises at least one sensor configured to measure an initial level of impedance in the tissue and a minimum level of impedance in the tissue.

In other aspects, a non-transitory computer readable medium is presented. The computer readable medium may include instructions that, when executed by a processor, cause the processor to perform operations comprising any of the operations described in any one of the previous aspects.

The foregoing summary is illustrative only and is not intended to be in any way limiting. In addition to the illustrative aspects and features described above, further aspects and features will become apparent by reference to the drawings and the following detailed description.

BRIEF DESCRIPTION OF THE DRAWINGS

The novel features of the aspects described herein are set forth with particularity in the appended claims. The aspects, however, both as to organization and methods of operation may be better understood by reference to the following description, taken in conjunction with the accompanying drawings as follows.

FIG. 1A shows one example of a surgical instrument system, according to some aspects.

FIG. 1B shows another example of a surgical instrument system, in this case showing multiple versions of a surgical instrument configured to deliver RF energy, ultrasonic energy, or a combination of both, according to some aspects.

FIG. 1C is a side, partially transparent schematic view of one aspect of a powered surgical device.

FIG. 1D is a side, partially transparent schematic view of another aspect of a powered surgical device.

FIG. 2 shows a perspective view of an end effector with jaws open, according to some aspects.

FIG. 3 is a block diagram describing further details of power supply elements of a surgical system, the surgical instrument coupled to a generator, according to some aspects.

FIG. 4A provides a visual depiction of the level of impedance over time present in tissue undergoing a sealing procedure during surgery.

FIG. 4B provides further details of various electrical readings of the surgical instrument system undergoing the sealing procedure during surgery.

FIG. 5 provides another example of the level of tissue impedance over time, this time using more empirical data.

FIG. 6A illustrates an example power profile of an amount of electrosurgical energy applied by a surgical instrument to tissue at a surgical site over time, in order to extend or prolong the bathtub region, according to some aspects.

FIG. 6B shows an example adjusted impedance profile over time as a result of the adjusted power applied to the surgical instrument, such as the example power profile in FIG. 6A, according to some aspects.

FIG. 7 shows an example power profile of the tapered load curve concept introduced in FIG. 6A, with additional power characteristics superimposed.

FIG. 8 provides an example of how multiple load curves may be programmed into the surgical instrument to apply different power adjustments based on impedance measurements during the sealing procedures.

FIG. 9 shows a visual depiction of an example load curve under the low minimum impedance threshold (see FIG. 8), according to some aspects.

FIG. 10 shows a visual depiction of an example load curve under the medium minimum impedance threshold (see FIG. 8), according to some aspects.

FIG. 11 is a graphical representation of impedance threshold and minimum pulse duration showing an example of additional adjustments that can be made to varying the power to account for other tissue properties.

FIG. 12 is a graphical illustration of voltage cutback caused by an impedance threshold greater than 325 Ohms, according to one aspect of the present invention.

FIG. 13 is a graphical illustration of a power pulse region of the graphical illustration shown in FIG. 11, according to one aspect of the present disclosure.

DETAILED DESCRIPTION

In the following detailed description, reference is made to the accompanying drawings, which form a part hereof. In the drawings, similar symbols and reference characters typically identify similar components throughout the several views, unless context dictates otherwise. The illustrative aspects described in the detailed description, drawings, and claims are not meant to be limiting. Other aspects may be utilized, and other changes may be made, without departing from the scope of the subject matter presented here.

The following description of certain examples of the technology should not be used to limit its scope. Other examples, features, aspects, aspects, and advantages of the technology will become apparent to those skilled in the art from the following description, which is, by way of illustration, one of the best modes contemplated for carrying out

the technology. As will be realized, the technology described herein is capable of other different and obvious aspects, all without departing from the technology. Accordingly, the drawings and descriptions should be regarded as illustrative in nature and not restrictive.

It is further understood that any one or more of the teachings, expressions, aspects, examples, etc. described herein may be combined with any one or more of the other teachings, expressions, aspects, examples, etc. that are described herein. The following described teachings, expressions, aspects, examples, etc. should, therefore, not be viewed in isolation relative to each other. Various suitable ways in which the teachings herein may be combined will be readily apparent to those of ordinary skill in the art in view of the teachings herein. Such modifications and variations are intended to be included within the scope of the claims.

Also, in the following description, it is to be understood that terms such as front, back, inside, outside, upper, lower, and the like are words of convenience and are not to be construed as limiting terms. Terminology used herein is not meant to be limiting insofar as devices described herein, or portions thereof, may be attached or utilized in other orientations. The various aspects will be described in more detail with reference to the drawings. Throughout this disclosure, the term “proximal” is used to describe the side of a component, e.g., a shaft, a handle assembly, etc., closer to a user operating the surgical instrument, e.g., a surgeon, and the term “distal” is used to describe the side of the component farther from the user operating the surgical instrument.

Aspects of the present disclosure are presented for a medical instrument configured to adjust the power level for sealing procedures to account for changes in tissue impedance levels over time. Typically during sealing procedures, a period of time exists where the tissue impedance level is low enough to allow for the tissue to respond to energy applied to it. The impedance level typically dips slightly over time initially, and then rises. After a certain point, due to various heating and chemical factors, the level of impedance rises dramatically, and energy applied to the tissue is no longer effective. Further example details of the limits of any power sources over a range of loads are described in some of the accompanying figures, below. The period of time where the level of impedance is low enough for applied energy to be effective is sometimes referred to as the “bathtub” region, due to the initial dip in the level of impedance and subsequent slow rise. It is desirable to manipulate the level of power applied to the tissue in order to extend or prolong the length of this bathtub region, so that the period of time for sealing and manipulating the tissue may be extended.

In some aspects, a medical instrument may be configured to apply power according to a power algorithm to seal tissue by applying a gradually lower amount of power over to time as the tissue impedance level begins to rise out of the “bathtub region.” In some aspects, the power is then cut once the tissue impedance level exceeds the “bathtub region.” By gradually reducing the power, a balance is achieved between still applying an effective level of power for sealing and prolonging the time in which the tissue impedance remains in the “bathtub region,” due to the reduced power.

The medical instrument of the present disclosures may include additional features. An end effector of the electrosurgical device may include multiple members arranged in various configurations to collectively perform the aforementioned functions. As used herein, an end effector may be referred to as a jaw assembly or clamp jaw assembly comprising an upper jaw member and a lower jaw member

where at least one of the upper jaw member and the lower jaw member may be movable relative to the other. Each of the jaw members may be adapted to connect to an electrosurgical energy source. Each jaw member may incorporate an electrode. The electrode may be a positive or negative electrode. In a bipolar electrosurgical device, the electrodes may be adapted for connection to the opposite terminals of the electrosurgical energy source, such as a bipolar radio frequency (RF) generator, so as to generate a current flow therebetween. An electrosurgical energy may be selectively communicated through tissue held between the jaw members to effect a tissue seal and/or treatment. Tissue may be coagulated from the current flowing between the opposite polarity electrodes on each jaw member.

At least one jaw member may include a knife channel defined therein configured to reciprocate a knife there along for severing tissue held between the jaw members. The knife channel may be an extended slot in the jaw member. The knife may be provided within a recess associated with the at least one jaw member. The electrosurgical device may have both coagulation and cutting functions. This may eliminate or reduce instrument interchange during a surgery. Cutting may be achieved using mechanical force alone or a combination of mechanical force and the electrosurgical energy. The electrosurgical energy may be selectively used for coagulation and/or cutting. The knife may be made from an electrically conductive material adapted to connect to the electrosurgical source, and selectively activatable to separate tissue disposed between the jaw members. The knife may be spring biased such that once tissue is severed, the knife may automatically return to an unengaged position within the knife channel or a retracted position in the recess.

In some aspects, the jaw members may be movable relative to each other. During operation of the electrosurgical device, at least one of the jaw members may move from a first, open position where the jaw members can be disposed around a mass of tissue, to a second, closed position where the jaw members grasp the tissue. The jaw members therefore may move through a graspers-like range of motion, similar to that of conventional pliers. In the second position, current flows between the jaw members to achieve hemostasis of the tissue captured therebetween. The jaw members may be configured to have a relatively thick proximal portion to resist bending. At least one of the jaw members may have a three-dimensional configuration with a D-shaped cross-sectional. The three-dimensional configuration with the D-shaped cross-sectional may resist bending. A lock mechanism may be included to lock the jaw members in the closed position. The lock mechanism may set the clamp pressure between the jaw members. At least one electrically conductive gap setting member may be provided between the jaw members to establish a desired gap between electrodes in bipolar electrosurgical devices.

The electrosurgical device may incorporate components to grasp a tissue via the end effector, deliver energy to the tissue via one or more electrodes, and cut the tissue via a dissecting device such as a tissue knife. The structural capabilities of any aspect of an electrosurgical device may be designed for use in one or more of a variety of surgical procedures. In some surgical procedures, the treated tissue may be readily accessible to an end effector affixed to a relatively straight and unbendable shaft. In some alternative surgical procedures, the tissue may not be readily accessible to the end effector on such a shaft. In such procedures, the electrosurgical device may incorporate a shaft designed to bend so that the end effector may contact the tissue requiring treatment. In such a device, the shaft may include one or

more articulated joints that may permit the shaft to bend under control by the user. A sliding knife may include a feature to provide actuating force to the sliding knife. A knife actuator may be operably coupled to the shaft for selectively reciprocating the knife through the knife channel.

A front portion assembly may be designed for a specific surgical procedure, while a reusable handle assembly, configured to releasably attach to a front portion assembly, may be designed to provide control of surgical functions common to each front portion assembly, such as tissue grasping, cauterizing, and cutting. Consequently, the number and types of devices required for surgeries can be reduced. The reusable handle assembly may be designed to automate common functions of the electrosurgical device. Device intelligence may be provided by a controller located in the reusable handle assembly that is configured to receive information from a front portion assembly. Such information may include data regarding the type and use of the front portion assembly. Alternatively, information may include data indicative of the position and/or activation of control components (such as buttons or slides that can be manipulated) that may indicate what system functions should be activated and in what manner.

In some non-limiting examples, the controller may supply the RF current when the energy activation control is placed in an activating position by the user. In some alternative non-limiting examples, the controller may supply the RF current for a predetermined period of time once the energy activation control is placed in an activating position. In yet another non-limiting example, the controller may receive data related to the position of the jaws and prevent the RF current from being supplied to the one or more tissue cauterization power contacts if the jaws are not in a closed position.

In some aspects, any of the mentioned examples also may be configured to articulate along at least one axis through various means, including, for example, a series of joints, one or more hinges or flexure bearings, and one or more cam or pulley systems. Other features may include cameras or lights coupled to one or more of the members of the end effector, and various energy options for the surgical device.

The electrosurgical device can be configured to source energy in various forms including, without limitation, electrical energy, monopolar and/or bipolar RF energy, microwave energy, reversible and/or irreversible electroporation energy, and/or ultrasonic energy, heat energy, or any combination thereof, to the tissue of a patient either independently or simultaneously. The energy can be transmitted to the electrosurgical device by a power source in electrical communication with the electrosurgical device. The power source may be a generator. The power source may be connected to the electrosurgical device via a suitable transmission medium such as a cable. The power source may be separate from the electrosurgical device or may be formed integrally with the electrosurgical device to form a unitary electrosurgical system. In one non-limiting example, the power source may include one or more batteries located within a portion of the electrosurgical device. It may be understood that the power source may source energy for use on the tissue of the patient as well as for any other electrical use by other devices, including, without limitation, lights, sensors, communication systems, indicators, and displays, which operate in relation to and/or with the electrosurgical device to form an electrosurgical system. In some aspects, the power source may source energy for use in measuring tissue effects with an RF impedance measuring portion. The remaining sources of energy, such as ultrasonic energy, may

then be controlled based on the measured tissue effects. Similarly, multiple types of energy from one or more sources may be combined to interact in distinct ways. For example, an instrument with both RF and ultrasonic capabilities may allow for different energy types to perform different functions during a single procedure. For example, RF energy may be used to seal, while other energy types, such as ultrasonic energy, may be used to cut the tissue. In general, the present disclosures may be applied to these devices with combination elements (e.g., instruments having both RF and ultrasonic energy functionalities), and aspects are not so limited. Similar concepts include the systems and methods described in U.S. Pat. No. 9,017,326, "IMPEDANCE MONITORING APPARATUS, SYSTEM, AND METHOD FOR ULTRASONIC SURGICAL INSTRUMENTS," which is incorporated herein by reference.

The electrosurgical device may be configured to source electrical energy in the form of RF energy. The electrosurgical device can transmit the RF energy through tissue compressed between two or more jaws. Such RF energy may cause ionic agitation in the tissue, in effect producing resistive heating, and thereby increasing the temperature of the tissue. Increased temperature of the tissue may lead to tissue cauterization. In some surgical procedures, RF energy may be useful for removing, shrinking, or sculpting soft tissue while simultaneously sealing blood vessels. RF energy may work particularly well on connective tissue, which is primarily composed of collagen and shrinks when contacted by heat. Because a sharp boundary may be created between the affected tissue and the surrounding tissue, surgeons can operate with a high level of precision and control, without sacrificing untargeted adjacent tissue.

The RF energy may be in a frequency range described in EN 60601-2-2:2009+A11:2011, Definition 201.3.218—HIGH FREQUENCY. For example, the frequency in monopolar RF applications may be typically restricted to less than 5 MHz. However, in bipolar RF applications, the frequency can be almost anything. Frequencies above 200 kHz can be typically used for monopolar applications in order to avoid the unwanted stimulation of nerves and muscles that would result from the use of low frequency current. Lower frequencies may be used for bipolar applications if the risk analysis shows the possibility of neuromuscular stimulation has been mitigated to an acceptable level. Normally, frequencies above 5 MHz are not used in order to minimize the problems associated with high frequency leakage currents. Higher frequencies may, however, be used in the case of bipolar applications. It is generally recognized that 10 mA is the lower threshold of thermal effects on tissue.

As discussed above, the electrosurgical device may be used in conjunction with a generator. The generator may be an electrosurgical generator characterized by a fixed internal impedance and fixed operating frequency that deliver maximum power to an external load (e.g., tissue), such as having an electrical impedance in the range of about 50 ohms to 150 ohms. In this type of bipolar electrosurgical generator, the applied voltage may increase monotonically as the load impedance increases toward the maximum "open circuit" voltage as the load impedance increases to levels of tens of thousands of ohms or more. In addition, the electrosurgical device may be used with a bipolar electrosurgical generator having a fixed operating frequency and an output voltage that may be substantially constant over a range of load impedances of tens of ohms to tens of thousands of ohms including "open circuit" conditions. The electrosurgical device may be advantageously used with a bipolar electro-

surgical generator of either a variable voltage design or substantially constant voltage design in which the applied voltage may be interrupted when the delivered current decreases below a predetermined level. Such bipolar generators may be referred to as automatic generators in that they may sense the completion of the coagulation process and terminate the application of voltage, often accompanied by an audible indication in the form of a cessation of a "voltage application" tone or the annunciation of a unique "coagulation complete" tone. Further, the electrosurgical device may be used with an electrosurgical generator whose operating frequency may vary with the load impedance as a means to modulate the applied voltage with changes in load impedance.

Various aspects of electrosurgical devices use therapeutic and/or sub-therapeutic electrical energy to treat tissue. Some aspects may be utilized in robotic applications. Some aspects may be adapted for use in a hand operated manner. In one non-limiting example, an electrosurgical device may include a proximal handle, a distal working end or end effector, and an introducer or elongated shaft disposed in-between.

Additional details regarding electrosurgical end effectors, jaw closing mechanisms, and electrosurgical energy-delivery surfaces are described in the following U.S. patents and published patent applications: U.S. Pat. Nos. 7,087,054; 7,083,619; 7,070,597; 7,041,102; 7,011,657; 6,929,644; 6,926,716; 6,913,579; 6,905,497; 6,802,843; 6,770,072; 6,656,177; and 6,533,784; and U.S. Pat. App. Pub. Nos. 2010/0036370 and 2009/0076506, all of which are incorporated herein by reference in their entirety and made part of this specification.

FIG. 1A shows one example of a surgical instrument system **100**, according to aspects of the present disclosure. The surgical instrument system **100** comprises an electrosurgical instrument **110**. The electrosurgical instrument **110** may comprise a proximal handle **112**, a distal working end or end effector **200** and an introducer or elongated shaft **114** disposed in-between. Alternatively, the end effector may be attached directly to the handle as in scissor style devices such as the electrosurgical instrument described in U.S. Pat. No. 7,582,087.

The electrosurgical system **100** can be configured to supply energy, such as electrical energy, ultrasonic energy, heat energy, or any combination thereof, to the tissue of a patient either independently or simultaneously, for example. In one example, the electrosurgical system **100** may include a generator **120** in electrical communication with the electrosurgical instrument **110**. The generator **120** may be connected to the electrosurgical instrument **110** via a suitable transmission medium such as a cable **122**. In one example, the generator **120** may be coupled to a controller, such as a control unit **125**, for example. In various aspects, the control unit **125** may be formed integrally with the generator **120** or may be provided as a separate circuit module or device electrically coupled to the generator **120** (shown in phantom to illustrate this option). The control unit **125** may include automated or manually operated controls to control the amount of current delivered by the generator **120** to the electrosurgical instrument **110**. Although as presently disclosed, the generator **120** is shown separate from the electrosurgical instrument **110**, in some aspects, the generator **120** (and/or the control unit **125**) may be formed integrally with the electrosurgical instrument **110** to form a unitary electrosurgical system **100**, where a battery located within the electrosurgical instrument **110** may be the energy source

11

and a circuit coupled to the battery produces the suitable electrical energy, ultrasonic energy, or heat energy.

In one aspect, the generator **120** may comprise an input device located on a front panel of the generator **120** console. The input device may comprise any suitable device that generates signals suitable for programming the operation of the generator **120**, such as a keyboard, or input port, for example. In one example, one or more electrodes in the first jaw **210a** and one or more electrodes in the second jaw **210b** may be coupled to the generator **120**. The cable **122** may comprise multiple electrical conductors for the application of electrical energy to a first electrode (which may be designated as a + electrode) and to a second electrode (which may be designated as a - electrode) of the electrosurgical instrument **110**. It may be recognized that + and - designations are made solely for convenience and do not indicate an electrical polarity. An end of each of the conductors may be placed in electrical communication with a terminal of the generator **120**. The generator **120** may have multiple terminals, each configured to contact one or more of the conductors. The control unit **125** may be used to activate the generator **120**, which may serve as an electrical source. In various aspects, the generator **120** may comprise an RF source, an ultrasonic source, a direct current source, and/or any other suitable type of electrical energy source, for example, which may be activated independently or simultaneously.

In various aspects, the electrosurgical system **100** may comprise at least one supply conductor **131** and at least one return conductor **133**, wherein current can be supplied to the electrosurgical instrument **110** via the at least one supply conductor **131** and wherein the current can flow back to the generator **120** via the at least one return conductor **133**. In various aspects, the at least one supply conductor **131** and the at least one return conductor **133** may comprise insulated wires and/or any other suitable type of conductor. As described below, the at least one supply conductor **131** and the at least one return conductor **133** may be contained within and/or may comprise the cable **122** extending between, or at least partially between, the generator **120** and the end effector **200** of the electrosurgical instrument **110**. The generator **120** can be configured to apply a sufficient voltage differential between the supply conductor **131** and the return conductor **133** such that sufficient current can be supplied to the end effector **200** to perform the intended electrosurgical operation.

The shaft **114** may have a cylindrical or rectangular cross-section, for example, and can comprise a thin-wall tubular sleeve that extends from the proximal handle **112**. The shaft **114** may include a bore extending therethrough for carrying actuator mechanisms, for example, an axially moveable member for actuating the jaws **210a**, **210b** and for carrying electrical leads for delivery of electrical energy to electrosurgical components of the end effector **200**. The proximal handle **112** may include a jaw closure trigger **121** configured to adjust the position of the jaws **210a**, **210b** with respect to each other. In one non-limiting example, the jaw closure trigger **121** may be coupled to an axially moveable member disposed within the shaft **114** by a shuttle operably engaged to an extension of the jaw closure trigger **121**.

The end effector **200** may be adapted for capturing and transecting tissue and for contemporaneously welding the captured tissue with controlled application of energy (e.g., RF energy). The first jaw **210a** and the second jaw **210b** may be closed thereby capturing or engaging tissue. The first jaw **210a** and second jaw **210b** also may apply compression to the tissue. In some aspects, the shaft **114**, along with the first

12

jaw **210a** and second jaw **210b**, can be rotated, for example, a full 360°. For example, a rotation knob **148** may be rotatable about the longitudinal axis of the shaft **114** and may be coupled to the shaft **114** such that rotation of the knob **148** causes corresponding rotation of the shaft **114**. The first jaw **210a** and the second jaw **210b** can remain openable and/or closeable while rotated.

Also illustrated in FIG. **1** are a knife advancement control **140** and an energy activation control **145** located on the proximal handle **112**. In some non-limiting examples, the knife advancement control **140** and the energy activation control **145** may be depressible buttons positioned to permit a user to control knife advancement or energy activation by the use of one or more fingers.

FIG. **1B** illustrates a second example of a surgical system **10** comprising a generator **1002** and various surgical instruments **1004**, **1006**, **1202** usable therewith, according to some aspects. The generator **1002** may be configurable for use with a variety of surgical devices. According to various forms, the generator **1002** may be configurable for use with different surgical devices of different types including, for example, the ultrasonic device **1004**, electrosurgical or RF surgical devices, such as, the RF device **1006**, and multi-function devices **1202** that integrate electrosurgical RF and ultrasonic energies delivered simultaneously from the generator **1002**. Although in the form of FIG. **1B**, the generator **1002** is shown separate from the surgical devices **1004**, **1006**, **1202** in one form, the generator **1002** may be formed integrally with either of the surgical devices **1004**, **1006**, **1202** to form a unitary surgical system. The generator **1002** comprises an input device **1045** located on a front panel of the generator **1002** console. The input device **1045** may comprise any suitable device that generates signals suitable for programming the operation of the generator **1002**. The generator **1002** may also comprise an output device **1047** (FIG. **1**) located, for example, on a front panel of the generator **1002** console. The output device **1047** includes one or more devices for providing a sensory feedback to a user. Such devices may comprise, for example, visual feedback devices (e.g., an LCD display screen, LED indicators), audio feedback devices (e.g., a speaker, a buzzer) or tactile feedback devices (e.g., haptic actuators).

FIG. **1C** illustrates one aspect of a surgical device **900** configured to grasp and cut tissue. The surgical device **900** can include a proximal handle portion **910**, a shaft portion **912**, and an end effector **914** configured to grasp tissue. The proximal handle portion **910** can be any type of pistol-grip or other type of handle known in the art that is configured to carry various actuators **924**, such as actuator levers, triggers or sliders, configured to actuate the end effector **914**. As illustrated, the proximal handle portion **910** can include a closure grip **920** and a stationary grip **922**. Movement of the closure grip **920** toward and away from the stationary grip **922**, such as by manual movement by a hand of a user, can adjust a position of the end effector **914**. The shaft portion **912** can extend distally from the proximal handle portion **910** and can have a bore (not shown) extending there-through. The bore can carry mechanisms for actuating the end effector **914**, such as a jaw closure tube and/or a drive shaft. As discussed further below, one or more sensors (not shown) can be coupled to the surgical device **900** and can be configured to sense data that can be used in controlling an output of the device's motor **932**. The device's motor **932** can be coupled to a controller **934**, which in turn may be coupled to the power source **936**.

The end effector **914** can have a variety of sizes, shapes, and configurations. As shown in FIG. **1C**, the end effector

13

914 can include a first, upper jaw 16a and a second, lower jaw 916b each disposed at a distal end 912d of the shaft portion 912. One or both of the upper and lower jaws 916a, 916b can be configured to close or approximate about a longitudinal axis L1 of the end effector 914. Both of the jaws 916a, 916b can be moveable relative to the shaft portion 912 such that the end effector 914 can be moved between open and closed positions, or only one the upper and lower jaws 916a, 916b can be configured to move relative to the shaft portion 912 and to the other of the jaws 916a, 916b so as to move the end effector 914 between open and closed positions. When the end effector 914 is in the open position, the jaws 916a, 916b can be positioned at a distance apart from one another with space therebetween. As discussed further below, tissue can be positioned within the space between the jaws 916a, 916b. When the end effector 914 is in the closed position, a longitudinal axis of the upper jaw 916a can be substantially parallel to a longitudinal axis of the lower jaw 916b, and the jaws 916a, 916b can be moved toward one another such that the distance therebetween is less than when the end effector 914 is in the open position. In some aspects, facing engagement surfaces 919a, 919b of the jaws 916a, 916b can be in direct contact with one another when the end effector 914 is in the closed position such that the distance between is substantially zero. As illustrated, the upper jaw 16a is configured to pivot relative to the shaft portion 912 and relative to the lower jaw 916b while the lower jaw 916b remains stationary. As illustrated, the jaws 916a, 916b have a substantially elongate and straight shape, but a person skilled in the art will appreciate that one or both of the jaws 916a, 916b can be curved along the longitudinal axis L1 of the end effector 914. The longitudinal axis L1 of the end effector 914 can be parallel to and coaxial with a longitudinal axis of the shaft portion 912 at least when the end effector 914 is in the closed configuration, and if the end effector 914 is configured to articulate relative to the shaft portion 912, when the end effector 914 is not articulated relative to the shaft portion 912.

FIG. 1D illustrates another aspect of a surgical device 1400 configured to cut and seal tissue clamped between first and second jaws 1402a, 1402b of the device's end effector 1404. The device 1400 can be configured to separately cut and seal tissue and configured to simultaneously cut and seal tissue, with a user of the device 1400 being able to decide whether cutting and sealing occurs separately or simultaneously. The device 1400 can generally be configured similar to the device 900 of FIG. 1C. The device 1400 can include a motor 1406, a closure trigger 1408, a firing actuator 1410, a controller 1412, a cutting element (not shown), a power connector (not shown) configured to attach to an external power source (not shown), an energy actuator 1414, an elongate shaft 1416 extending from a handle portion 1418 of the device 1400, a sensor 1420a, 1420b, the end effector 1404 at a distal end of the shaft 1416, a stationary handle 1424, and a gear box 1426 that can be operatively connected to the motor 1406 and configured to transfer output from the motor 1406 to the cutting element. As illustrated, the controller 1412 includes a printed circuit board (PCB), the sensor 1420a includes a Hall effect sensor, and the other sensor 1420b includes a Hall effect sensor. One of the jaws 1420a includes an insulator 1428 configured to facilitate safe energy application to tissue clamped by the end effector 1404. Each of the jaws 1402a, 1402b can include a proximal slot 1430a, 1430b configured to facilitate opening and closing of the end effector 1404, as will be appreciated by a person skilled in the art. The device 1400 can be configured to lock the closure trigger 1408 in the closed position, such

14

as by the closure trigger 1408 including a latch 1432 configured to engage a corresponding latch 1434 on the stationary handle 1424 when the closure trigger 1408 is drawn close enough thereto so as to lock the closure trigger 1408 in position relative to the stationary handle 1424. The closure trigger latch 1432 can be configured to be manually released by a user so as to unlock and release the closure trigger 1408. A bias spring 1436 included in the handle portion 1418 can be coupled to the closure trigger 1408 and cause the closure trigger 1408 to open, e.g., move away from the stationary handle 1424, when the closure trigger 1408 is unlocked.

FIG. 2 shows a perspective view of the end effector 200 with the jaws 210a, 210b open, according to one aspect of the present disclosure. The end effector 200 may be attached to any of the various surgical instruments provided herein, including those configured to supply RF energy, ultrasonic energy, or various combinations of energy to the end effector 200. The end effector 200 may comprise the first or upper jaw 210a and the second or lower jaw 210b, which may be straight or curved. The upper jaw 210a may comprise a first distal end 212a and a first proximal end 214a. The lower jaw 210b may comprise a second distal end 212b and a second proximal end 214b. The first distal end 212a and the second distal end 212b may be collectively referred to as the distal end of the end effector when the jaws 210a, 210b are in a closed configuration. The first proximal end 214a and the second proximal end 214b may be collectively referred to as the proximal end of the end effector 200. The jaws 210a, 210b are pivotally coupled at the first and second proximal ends 214a, 214b. As shown in FIG. 2, The lower jaw 210b is fixed and the upper jaw 210a is pivotally movable relative to the lower jaw 210b from an open position to a closed position and vice versa. In the closed position, the first and second distal ends 212a, 212b are in proximity. In the open position, the first and second distal ends 214a, 214b are spaced apart. In other aspects, the upper jaw 210a may be fixed and the lower jaw 210b may be movable. In other aspects, both the upper and lower jaws 210a, 210b may be movable. The end effector 200 may comprise a pivot assembly 270 located at or in proximity to the proximal end of the end effector, which sets an initial gap between the jaws 210a, 210b at the proximal end of the end effector 200 in a closed position.

In some aspects, the first jaw 210a and the second jaw 210b may each comprise an elongated slot or channel 250a and 250b, respectively, disposed along their respective middle portions. The channels 250a and 250b may be sized and configured to accommodate the movement of an axially moveable member (not shown), which may comprise a tissue-cutting element, for example, comprising a sharp distal edge. The upper jaw 210a may comprise a first energy delivery surface 230a. The lower jaw 210b may comprise a second energy delivery surface 230b. The first and second energy delivery surfaces 230a, 230b face each other when the jaws 210a, 210b are in a closed configuration. The first energy delivery surface 230a may extend in a "U" shape around the channel 250a, connecting at the first distal end 212a. The second energy delivery surface 230b may extend in a "U" shape around the channel 250b, connecting at the second distal end 212b. The first and second energy delivery surfaces 230a, 230b may comprise electrically conductive material such as copper, gold plated copper, silver, platinum, stainless steel, aluminum, or any suitable electrically conductive biocompatible material, for example. The second energy delivery surface 230b may be connected to the supply conductor 131 shown in FIG. 1A, for example, thus

forming the first electrode **220** in the electrosurgical instrument **110**. The first energy delivery surface **230a** may be connected and the return conductor **133** shown in FIG. 1A, thus forming the second electrode **222** the electrosurgical instrument **110**. For example, the first energy delivery surface **230a** may be grounded. Opposite connection is also possible. The first and second electrodes **220**, **222** can be configured to pass energy through tissue positioned between the electrodes **220**, **222**. The energy may comprise, for example, radiofrequency (RF) energy, sub-therapeutic RF energy, therapeutic RF energy, ultrasonic energy, and/or other suitable forms of energy.

As shown in FIG. 2, the second energy delivery surface **230b** is formed by a conductive layer disposed, or at least partially disposed, along at least a portion of the body of the lower jaw **210b**. The electrically conductive layer comprising the second energy delivery surface **230b** may extend to the second distal end **212b**, and thus operation of the end effector **200** is possible without actually grasping the tissue. The lower jaw **210b** may further comprise an electrically insulative layer **260** arranged between the conductive layer and the body of the lower jaw **210b**. The electrically insulative layer **260** may comprise electrically insulative material such as ceramic or nylon. Furthermore, the first energy delivery surface **230a** is formed of an electrically conductive layer disposed, or at least partially disposed, along at least a portion of the body of the upper jaw **210a**. The upper jaw **210a** also may comprise an electrically insulative layer arranged between the conductive layer and the body of the upper jaw **210a**.

The upper and lower jaws **210a** and **210b** may each comprise one or more electrically insulative tissue engaging members arranged on the first or second energy delivery surface **230a**, **230b**, respectively. Each of the electrically insulative tissue engaging members may protrude from the energy delivery surface and define a height above the energy delivery surface, and thus is sometimes referred to as a "tooth." The electrically insulative tissue engaging members may comprise electrically insulative material such as ceramic or nylon. As shown in FIG. 2, the electrically insulative tissue engaging members **240** are arranged longitudinally, e.g., along the length of the lower jaw **210b**, from the send proximal end **214b** to the second distal end **212b** and on the second energy delivery surface **230b**. As shown in FIG. 2, the electrically insulative tissue engaging members **240** are in pairs, and each pair is arranged next to the channel **250b** and is separated by the channel **250b**. These paired electrically insulative tissue engaging members **240** as arranged here are sometimes referred to as "teeth."

In other aspects, other configurations of the electrically insulative tissue engaging members **240** are possible. For example, the electrically insulative tissue engaging members **240** may be located at a distance away from the channel. For example, the electrically insulative tissue engaging members **240** may be arranged in a grid on the energy delivery surface. In other aspects, the electrically insulative tissue engaging members **240** may not have the half cylindrical cross sections as shown in FIG. 2, and may have cylindrical cross sections or rectangular cross sections. In other aspects, electrically insulative tissue engaging members **240** may be arranged on the first energy delivery surface **230a**, or may be arranged on both of the first and second energy delivery surfaces **230a**, **230b**.

FIG. 3 is a block diagram of a surgical system **300** comprising a motor-driven surgical grasping instrument **900**, **1400** (FIGS. 10, 1D) according to some aspects of the

present disclosure, the surgical instrument coupled to a generator **335** (**340**), according to some aspects. The motor-driven surgical cutting and fastening instrument **2** described in the present disclosure may be coupled to a generator **335** (**340**) configured to supply power to the surgical instrument through external or internal means. FIG. 3 describes examples of the portions for how electrosurgical energy may be delivered to the end effector. In certain instances, the motor-driven surgical instrument **110** may include a microcontroller **315** coupled to an external wired generator **335** or internal generator **340**. Either the external generator **335** or the internal generator **340** may be coupled to A/C mains or may be battery operated or combinations thereof. The electrical and electronic circuit elements associated with the motor-driven surgical instrument **110** and/or the generator elements **335**, **340** may be supported by a control circuit board assembly, for example. The microcontroller **315** may generally comprise a memory **310** and a microprocessor **305** ("processor") operationally coupled to the memory **310**. The microcontroller **315** may be configured to regulate the electrosurgical energy applied at the end effector according to the concepts disclosed herein and described more below. The processor **305** may control a motor driver **320** circuit generally utilized to control the position and velocity of the motor **325**. The motor **325** may be configured to control transmission of energy to the electrodes at the end effector of the surgical instrument. In certain instances, the processor **305** can signal the motor driver **320** to stop and/or disable the motor **325**, as described in greater detail below. In certain instances, the processor **305** may control a separate motor override circuit which may comprise a motor override switch that can stop and/or disable the motor **325** during operation of the surgical instrument in response to an override signal from the processor **305**. The processor may be communicatively coupled to a display/indicator **330**. It should be understood that the term processor as used herein includes any suitable microprocessor, microcontroller, or other basic computing device that incorporates the functions of a computer's central processing unit (CPU) on an integrated circuit or at most a few integrated circuits. The processor is a multipurpose, programmable device that accepts digital data as input, processes it according to instructions stored in its memory, and provides results as output. It is an example of sequential digital logic, as it has internal memory. Processors operate on numbers and symbols represented in the binary numeral system.

In some cases, the processor **305** may be any single core or multicore processor such as those known under the trade name ARM Cortex by Texas Instruments. In some cases, any of the surgical instruments of the present disclosures may comprise a safety processor such as, for example, a safety microcontroller platform comprising two microcontroller-based families such as TMS570 and RM4x known under the trade name Hercules ARM Cortex R4, also by Texas Instruments. Nevertheless, other suitable substitutes for microcontrollers and safety processor may be employed, without limitation. In one instance, the safety processor may be configured specifically for IEC 61508 and ISO 26262 safety critical applications, among others, to provide advanced integrated safety features while delivering scalable performance, connectivity, and memory options.

In certain instances, the microcontroller **315** may be an LM 4F230H5QR, available from Texas Instruments, for example. In at least one example, the Texas Instruments LM4F230H5QR is an ARM Cortex-M4F Processor Core comprising on-chip memory **310** of 256 KB single-cycle flash memory, or other non-volatile memory, up to 40 MHz,

a prefetch buffer to improve performance above 40 MHz, a 32 KB single-cycle serial random access memory (SRAM), internal read-only memory (ROM) loaded with StellarisWare® software, 2 KB electrically erasable programmable read-only memory (EEPROM), one or more pulse width modulation (PWM) modules, one or more quadrature encoder inputs (QEI) analog, one or more 12-bit Analog-to-Digital Converters (ADC) with 12 analog input channels, among other features that are readily available for the product datasheet. Other microcontrollers may be readily substituted for use in the motor-driven surgical instrument 110. Accordingly, the present disclosure should not be limited in this context.

Referring again to FIG. 3, the surgical system 300 may include a wired generator 335, for example. In certain instances, the wired generator 335 may be configured to supply power through external means, such as through electrical wire coupled to an external generator. In some cases, the surgical system 300 also may include or alternatively include an internal generator 340. The internal generator 340 may be configured to supply power through internal means, such as through battery power or other stored capacitive source. Further descriptions of the internal generator 340 and the wired generator 335 are described below.

In certain instances, the motor-driven surgical instrument 110 may comprise one or more embedded applications implemented as firmware, software, hardware, or any combination thereof. In certain instances, the motor-driven surgical instrument 110 may comprise various executable modules such as software, programs, data, drivers, and/or application program interfaces (APIs), for example.

Referring to FIG. 4A, graph 400 and provides a visual depiction of the level of impedance over time present in tissue undergoing a sealing procedure during surgery. This example graph 400 provides a conceptual framework for the types of power adjustments employed according to the present disclosures. Here, time zero represents the first point at which a surgical instrument, such as instrument 110, applies electrosurgical energy to tissue at a surgical site. The Y axis represents the level of tissue impedance (Z) present when a substantially constant level of power is applied to the tissue via an end effector of the instrument 110. At time zero, the tissue exhibits an initial level of impedance (Z_{init}) 410. The initial level of impedance 410 may be based on native physiological properties about the tissue, such as density, amount of moisture, and what type of tissue it is. Over a short period of time, it is known that the level of impedance actually dips slightly as power is continuously applied to the tissue. This is a common phenomenon that occurs in all kinds of tissue. A minimum level of impedance (Z_{min}) 420 is eventually reached. From here, the overall level of impedance monotonically increases, and at first increases with a slow rise. Eventually, a transition point is reached such that level of impedance starts to dramatically rise above the initial level of impedance 410. This point is generally known as a transition impedance level (Z_{trans}) 430. After the transition impedance 430 is reached, the level of impedance rises dramatically over time, and beyond this point the tissue impedance is generally too high for electrosurgical energy to have a substantial impact on the tissue. Therefore, termination 440 of the electrosurgical energy generally occurs soon after the transition impedance 430 point is reached. Thus, the period of time between the initial impedance 410 and when the transition impedance 430 is reached is generally the only effective time when electrosurgical energy may be applied to the tissue with any positive effect. This region is sometimes

known as the bathtub region 450, due to the general shape of the curve over this time period. It is therefore desirable extend or prolong the bathtub region 450 in order to increase the amount of time where electrosurgical energy may be applied.

Referring to FIG. 4B, graph 450 shows an example of a typical load curve for a generator configured to provide power to an electrosurgical system of the present disclosure. The left vertical axis represents power (W) and voltage (V), the right vertical axis represents current (A), and the horizontal axis represents load impedance (Ohms). The voltage curve 452, current curve 454, and power curve 456 are shown as functions of load impedance. As shown, the amount of power and voltage applied to tissue typically reaches an impassable threshold, even over ever increasing load impedances. Looked at another way, the amount of energy applied to the tissue at a surgical site has a noticeable effect only up to certain levels of load impedances, and after a certain impedance threshold, such as 175 ohms, applying more or sustained power typically has little to no benefit. Graph 450 therefore provides further detail on why exceeding the transition impedance threshold, as shown in graph 400, generally represents the cutoff point to which power should continue to be applied.

Referring to FIG. 5, graph 500 provides another example of the level of tissue impedance over time, this time using more empirical data. As shown, the level of tissue impedance stays relatively low until the transition impedance level is reached, which occurs a little after four seconds in this example. In some cases, the transition impedance level is defined by the point at which the level of impedance rises above twice the value of the minimum impedance level, while in other cases it may be defined as the point at which the initial impedance level is reached again. Regardless of which definition is used, the transition impedance level generally occurs at around the same time, assuming a constant level of power is applied to the tissue. Furthermore, it is known that the transition impedance level is reliably a function of the initial impedance level of the tissue. In other words, depending on what the initial level of impedance is, the transition impedance level can be predicted reliably in the tissue.

Referring to FIG. 6A, graph 600 illustrates an example power profile of an amount of electrosurgical energy applied by a surgical instrument 110 to tissue at a surgical site over time, in order to extend or prolong the bathtub region, according to some aspects. The continuous, piecewise curve 610 shows that the level of power changes in multiple stages. Initially, the electrosurgical energy applied rises to a predetermined level of power, such as 20 W in this case. This represents the initial desired level of power used for the surgical procedure in question. While the tissue impedance is generally in the bathtub region, this initial level of power is acceptable. However, as the tissue impedance begins to change and rises toward the transition impedance level, according to some aspects, the level of power is tapered down at a steady rate, rather than the level of power be constantly maintained like in conventional methods. In this example, it is supposed that the transition impedance level is 200 ohms, and may have been determined based on a measurement of the initial impedance level. Thus, as the tissue impedance rises but before it reaches the transition impedance level, such as when the tissue impedance reaches 75% of the transition impedance level (i.e., 150 ohms), the power system of the surgical instrument 110 may cause the level of power to decrease at a steady rate, as shown in the downward sloped region 620. For example, the power level

may be dropped by 50% over the course of time where the tissue impedance level continues to climb until it reaches the transition impedance level. Finally, once the transition impedance level is reached, the power to the surgical instrument **110** may be cut dramatically, as further application of power beyond the transition impedance level may be ineffective or may even cause unwanted damage to the tissue. In some aspects, the tapering of the power may be achieved in a number of ways that are all within the purview of this disclosure. For example, the microprocessor **315** (see FIG. **3**) may regulate the power coming from generators **335** or **340** via pulse width modulation or by applying an increase in resistance via the driver **320**. In general, the present disclosures may employ any methods for lowering the power known to those with skill in the art, and aspects are not so limited.

Referring to FIG. **6B**, graph **650** shows an example adjusted impedance profile over time as a result of the adjusted power applied to the surgical instrument **110**, such as the example power profile **610**, according to some aspects. As shown, the rise in impedance out of the bathtub region may be made more gradual due to the tapering of the power made according to aspects of the present disclosure. In addition, the overall length of the bathtub region may be extended or prolonged. The gradual rise of the tissue impedance may also allow for better care and treatment of the tissue under surgery. Conventionally, continuous power applied to the tissue after the transition impedance level is reached may cause unwanted damage to the tissue, such as burning tissue, sizzling, and popping. Due to the adjustments disclosed herein, this unwanted damage may be reduced or even eliminated.

Referring to FIG. **7**, graph **700** shows an example power profile of the tapered load curve concept introduced in FIG. **6A**, with additional power characteristics superimposed. Here, the curve **710** as shown by the thick line represents a measure of voltage as a function of load impedance in the tissue. The curve **720** as shown by the medium line represents a measure of calculated power applied to the tissue as a function of load impedance. The calculated power may be the measure of power that is determined by the power system of the surgical instrument **110**, while the curve **730** as shown by the dashed line represents the actual or effective power applied to the tissue. As shown, both of these curves exhibit a power taper that is reduced in a stepwise manner. This may be caused by the power being duty cycled at different rates over time, i.e., via pulse width modulation. The curve **740** as shown by the thin line represents a measure of current. The scale for the current is shown on the right-hand side, while the scale for power and voltage is shown on the left.

As shown, the power is tapered off in this example when the load impedance is measured to be approximately 60 to 70 ohms, and the power is nearly completely cut off when the load impedance is measured to be about 100 ohms. The voltage drops dramatically during the tapered region of the power profile, but begins to slowly rise again due to the low but constant application of power applied while the load impedance continues to increase. Practically, the power may be cut off long before the load impedance reaches these higher levels.

Referring to FIG. **8**, in some aspects, the surgical instrument **110** may be configured to apply different power algorithms to manage the rise of tissue impedance, based on varying levels of initial tissue impedance at the surgical site. The flowchart **800** provides an example of how multiple load curves may be programmed into the surgical instrument

110 to apply different power adjustments based on impedance measurements during the sealing procedures. For example, an algorithm to adjust the power may begin at block **810** that includes applying power to the end effector and ultimately to the tissue in question at the surgical site. At block **820**, while the end effector is applying the electrosurgical energy to the tissue, the impedance may be measured, and the minimum impedance may be determined based on the point at which the impedance eventually begins to rise. The end effector may include one or more sensors configured to monitor the impedance, voltage, or current, and may apply a number of mathematical formulas to determine what the measured impedance is. Various examples for how the tissue impedance may be measured are described in U.S. patent application Ser. Nos. 14/230,349 and 14/660,620, which are incorporated herein by reference.

In this example, three different power profiles may be available to be applied to the tissue, based on the measured level of minimum impedance: low, medium, and high. In this example, at block **830**, the low minimum impedance threshold is defined as when the minimum impedance is less than 30 ohms. At block **840**, the medium minimum impedance threshold is defined as when the minimum impedance is between 30 and 70 ohms. At block **850**, the high minimum impedance threshold is defined as when the minimum impedance is greater than 70 ohms. Based on the measured minimum impedance falling into one of these three categories, the load curve may be adjusted according to three characteristics. For example, if following the low minimum impedance profile, the power level in the bathtub region may be set to a maximum available power level (e.g., 30 W), the transition impedance threshold may be defined as 30 ohms greater than the measured minimum impedance, and the impedance at which all power is terminated may be set to 250 ohms. Based on these three characteristics, the power load curve may be generated. Examples of these different load curves are visually depicted in FIGS. **9** and **10**, below. As another example, if following the medium minimum impedance profile, the power level in the bathtub may be set to a moderate available power level (e.g., 20 W), the transition impedance threshold may be defined as 50 ohms greater than the measured minimum impedance, and the impedance at which all power is terminated may be set to 300 ohms. As a third example, if following the high minimum impedance profile, the power level in the bathtub region may be set to a low available power level (e.g., 10 W), the transition impedance threshold may be defined as 100 ohms greater than the measured minimum impedance, and the impedance at which all power is terminated may be set to 400 ohms.

In some aspects, rather than the minimum impedance being measured, and initial impedance may be measured and the load curves may be varied based on measured initial impedance levels. It may be apparent to those with skill in the art how the examples provided herein may be modified to account for an initial impedance level being measured, rather than the minimum impedance level being measured. For example, the calculation of the transition impedance may be offset by a different factor to account for the difference in value between the minimum impedance and the initial impedance. In addition, the thresholds under which the different load curves may be followed (e.g., blocks **830**, **840**, and **850**) may be based on modified criteria according to the different ranges of initial impedance.

The power system in the medical instrument **110** may apply power to the tissue according to the load curve, depending on which load curve is chosen. In all cases, the

power system may be configured to taper the power and the bathtub region as the impedance begins to slowly rise toward the transition impedance level, consistent with the concepts described in FIGS. 6A and 7.

Once the medical instrument 110 has finished applying power according to one of the load curves, a termination procedure may be executed at block 860. In some aspects, the termination power sequence may be based on what termination impedance value was set in the previous blocks of flowchart 800. For example, a series of termination pulses may be transmitted to the end effector of the medical instrument 110.

Referring to FIG. 9, a visual depiction of an example load curve under the low minimum impedance threshold is shown (see FIG. 8), according to some aspects. In this example, it may have been determined that the minimum impedance is 20 ohms, and therefore that the transition impedance level is 50 ohms (i.e., 30 ohms greater than the minimum impedance). The power level in the bathtub region may be set to a maximum level, such as 30 W. After the transition impedance level is reached, the power level may be dropped to a minimum, and may be ultimately terminated once the impedance reaches 250 ohms (not shown). In some aspects, the power level is dramatically cut once the transition impedance level is reached, while in other cases the power level may be tapered to decrease more gradually prior to the transition impedance being reached.

Referring to FIG. 10, a visual depiction of an example load curve under the moderate impedance threshold is shown (see FIG. 8), according to some aspects. In this example, it may have been determined that the minimum impedance is 50 ohms, and therefore that the transition impedance level is 100 ohms (i.e., 50 ohms greater than the minimum impedance). The power level in the bathtub region may be set to a moderate level, such as 20 W. After the transition impedance level is reached, the power level may be dropped to a minimum, and may be ultimately terminated once the impedance reaches 300 ohms (not shown). In some aspects, the power level is dramatically cut once the transition impedance level is reached, while in other cases the power level may be tapered to decrease more gradually prior to the transition impedance being reached.

In general, the example power algorithms and concepts from which these examples are based on may be adapted to many different types of electrode configurations, and aspects are not so limited. Various examples include electrodes of various length and width, including wider, narrower, longer or shorter electrodes than the examples shown herein; electrodes using I-Beam technology; motorized electrosurgical systems (similar to those described herein); scissor-type electrodes; and hand-held forceps-like instruments, whether open, laparoscopic or robotic. The power algorithms described herein may be set and adapted to these different scenarios by adjusting the various parameters as shown and described herein.

FIG. 11 is a graphical illustration 1100 of impedance threshold and minimum pulse duration showing an example of additional adjustments that can be made to varying the power to account for other tissue properties, according to one aspect of the present disclosure. The vertical axis represents, from left to right, Voltage (rms), Current (rms), Power (W), and Impedance (Ohms)/Energy (J) and the horizontal axis represents Time. Accordingly, a voltage curve 1102, current curve 1104, power curve 1106, and impedance/energy curve 1108 are shown superimposed as a function of time. Referring to FIG. 11, the illustration 1100 shows an example of additional adjustments that can be

made to varying the power, in order to account for other tissue properties. The illustration 1100 shows example impedance thresholds and minimum pulse durations over time, along with corresponding levels of power, voltage and current. In some aspects, the initial power level applied to the tissue may be based on additional factors, and the power adjustments may be varied to prolong the bathtub region based on these initial varied power levels, according to some aspects. For example, fatty tissues tend to have higher impedances during sealing. These impedances are often greater than 50 ohms after the initial pulses of energy are delivered to the tissue. Without accounting for these tissue properties, if the tissue impedance is greater than 50 ohms, the tissue will not receive full power from the generator. In response, increasing this threshold from 50 to 125 ohms (see circle 1 in illustration 1100) may enable the generator to deliver full power into the base mesentery, thus reducing sealing cycle time. In this case, if human tissue is more resistive than 125 ohms, then long seal times could occur. The threshold may be therefore need to be increased beyond 125 ohms in other circumstances.

Regarding minimum pulse duration, it has been observed that with short 180 millisecond (ms) pulses, the impedance (black curve, e.g., curve within circle 1) tends to stall and not rise quickly (see the movement of this curve within the time span under circle 2). In order to allow the tissue impedance to increase, the duration of the pulse on time can be increased. Thus, in some aspects, the minimum pulse width may be increased from 180 ms to 480 ms for composite load curve (CLC) tables.

FIG. 12 is a graphical illustration 1200 of voltage cutback caused by an impedance threshold greater than 325 Ohms, according to one aspect of the present invention. As shown, the voltage curve 1102 based on the CLC table bounces between 60 and 100 Volts (see circle 3 in illustration 1100) as tissue impedance approaches a 300 Ohm termination impedance. This bouncing causes the impedance rise rate to slow down as can be seen in the bouncing impedance/energy curve 1108. The voltage cutback is caused by a 325 Ohm threshold programmed in the original algorithm. If the 325 Ohm threshold is exceeded, the generator is configured to reduce the applied voltage from 100 volts to 60 volts. Accordingly, one aspect of the algorithm described herein does not include an impedance threshold that is greater than 325 Ohms.

FIG. 13 is a graphical illustration 1300 of a power pulse region of the graphical illustration 1100 shown in FIG. 11, according to one aspect of the present disclosure. In one aspect, the algorithm is configured such that the duration of the power pulse is 1 second for each step of the voltage curve 1102. It was observed that during the later half of each 1 second pulse the rise rate (slope) of the impedance curve 1108 would decrease (see circle 4 in illustration 1300). Accordingly, in one aspect of the algorithm, the duration of the power pulse is decreased to 0.5 seconds for each step of the voltage curve 1102 to prevent the impedance trajectory from stalling during the power pulse. In accordance with the 0.5 seconds duration of the power pulse, the number of power pulses is reduced from 4 to 3 (see circle 5 in illustration 1300). The duration of each power pulse remains 1 second. This allows tissue which is done earlier to proceed through the algorithm and thus finish sooner.

In general, aspects of the present disclosure may allow for various types of adjustments to be made to the amount of electrosurgical energy applied to the tissue at the surgical site, based on measured levels of impedance in the surgical tissue. For example, the power algorithms made differ if the

type of energy applied to the surgical tissue includes RF energy versus ultrasonic energy. The various characteristics of the load curves may need to be adjusted, e.g., what the maximum power level can be set to, what should the transition impedance be set to, when should the energy be terminated, at what level impedance should the power begin to taper off, etc., due to how the tissue may respond based on the different types of energy being applied to it. However, in general, the general shapes of the power profiles should remain consistent, and it may simply be a matter of determining what values should be set for the critical characteristics of the load curves, based on a measured minimum impedance or initial impedance, and in some aspects also based on various other characteristics of the types of energy applied to the tissue.

In some cases, various aspects may be implemented as an article of manufacture. The article of manufacture may include a computer readable storage medium arranged to store logic, instructions and/or data for performing various operations of one or more aspects. In various aspects, for example, the article of manufacture may comprise a magnetic disk, optical disk, flash memory or firmware containing computer program instructions suitable for execution by a general purpose processor or application specific processor. The aspects, however, are not limited in this context.

The functions of the various functional elements, logical blocks, modules, and circuits elements described in connection with the aspects disclosed herein may be implemented in the general context of computer executable instructions, such as software, control modules, logic, and/or logic modules executed by the processing unit. Generally, software, control modules, logic, and/or logic modules comprise any software element arranged to perform particular operations. Software, control modules, logic, and/or logic modules can comprise routines, programs, objects, components, data structures, and the like that perform particular tasks or implement particular abstract data types. An implementation of the software, control modules, logic, and/or logic modules and techniques may be stored on and/or transmitted across some form of computer-readable media. In this regard, computer-readable media can be any available medium or media useable to store information and accessible by a computing device. Some aspects also may be practiced in distributed computing environments where operations are performed by one or more remote processing devices that are linked through a communications network. In a distributed computing environment, software, control modules, logic, and/or logic modules may be located in both local and remote computer storage media including memory storage devices.

Additionally, it is to be appreciated that the aspects described herein illustrate example implementations, and that the functional elements, logical blocks, modules, and circuits elements may be implemented in various other ways which are consistent with the described aspects. Furthermore, the operations performed by such functional elements, logical blocks, modules, and circuits elements may be combined and/or separated for a given implementation and may be performed by a greater number or fewer number of components or modules. As will be apparent to those of skill in the art upon reading the present disclosure, each of the individual aspects described and illustrated herein has discrete components and features which may be readily separated from or combined with the features of any of the other several aspects without departing from the scope of the

present disclosure. Any recited method can be carried out in the order of events recited or in any other order which is logically possible.

Unless specifically stated otherwise, it may be appreciated that terms such as “processing,” “computing,” “calculating,” “determining,” or the like, refer to the action and/or processes of a computer or computing system, or similar electronic computing device, such as a general purpose processor, a DSP, ASIC, FPGA, or other programmable logic device, discrete gate or transistor logic, discrete hardware components, or any combination thereof designed to perform the functions described herein that manipulates and/or transforms data represented as physical quantities (e.g., electronic) within registers and/or memories into other data similarly represented as physical quantities within the memories, registers, or other such information storage, transmission, or display devices.

It is worthy to note that some aspects may be described using the expression “coupled” and “connected” along with their derivatives. These terms are not intended as synonyms for each other. For example, some aspects may be described using the terms “connected” and/or “coupled” to indicate that two or more elements are in direct physical or electrical contact with each other. The term “coupled,” however, also may mean that two or more elements are not in direct contact with each other, but yet still co-operate or interact with each other. With respect to software elements, for example, the term “coupled” may refer to interfaces, message interfaces, and application program interface, exchanging messages, and so forth.

The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

Although various aspects have been described herein, many modifications, variations, substitutions, changes, and equivalents to those aspects may be implemented and will occur to those skilled in the art. Also, where materials are disclosed for certain components, other materials may be used. It is therefore to be understood that the foregoing description and the appended claims are intended to cover all such modifications and variations as falling within the scope of the disclosed aspects. The following claims are intended to cover all such modification and variations.

The invention claimed is:

1. A surgical system comprising:

- an end effector comprising at least one energy delivery component configured to transmit electrosurgical energy to tissue at a surgical site; and
- a control circuit communicatively coupled to the at least one energy delivery component and programmed to:
 - for a first application period, cause the at least one energy delivery component to transmit the electro-

25

surgical energy at a first power level, the first application period comprising a point in time where impedance of the tissue reaches a minimum impedance value;

for a second application period after the first application period, cause the at least one energy delivery component to transmit the electrosurgical energy, starting from a predetermined proportion of a transition impedance threshold level and decreasing the electrosurgical energy at a steady rate from the first power level until a second power level is reached, wherein the second power level is lower than the first power level and the second application period comprises a point in time where the impedance of the tissue rises above the minimum impedance value; and

for a third application period after the second application period, directly after reaching the second power level, cause the at least one energy delivery component to reduce the second power level to a third power level while maintaining a constant level of the impedance of the tissue to transmit the electrosurgical energy at the third power level upon the impedance of the tissue reaching the transition impedance threshold level, the third power level lower than the second power level and the third application period comprising a point in time where the impedance of the tissue rises above the transition impedance threshold level.

2. The surgical system of claim 1, wherein the first application period and the second application period combined comprise a time period where the electrosurgical energy is delivered at a higher rate and causes sealing of the tissue at the surgical site.

3. The surgical system of claim 1, wherein the third application period further comprises a time period where the impedance of the tissue rises to a level such that the electrosurgical energy is delivered at a lower rate and no longer causes sealing of the tissue at the surgical site.

4. The surgical system of claim 1, further comprising at least one sensor configured to measure an initial level of impedance in the tissue and the minimum impedance value in the tissue.

5. The surgical system of claim 4, wherein the control circuit is further programmed to determine a beginning of the third application period based on the measured initial level of impedance in the tissue.

6. The surgical system of claim 4, wherein the control circuit is further programmed to determine a beginning of the third application period based on the measured minimum impedance value in the tissue.

7. The surgical system of claim 1, wherein the first application period and the second application period combined comprise a continuous time period where the impedance of the tissue remains below an initial level of impedance in the tissue.

8. The surgical system of claim 1, wherein the at least one energy delivery component is configured to transmit RF and ultrasonic energy.

9. A method for transmitting electrosurgical energy to tissue at a surgical site by a surgical system, the method comprising:

causing, by an energy delivery component of a surgical system, electrosurgical energy to be applied to the tissue;

measuring, by at least one sensor of the surgical system, a benchmark level of impedance of the tissue; and

26

determining, among a plurality of power load curve algorithms, a power load curve algorithm to be applied to the energy delivery component, based on the measured benchmark level of impedance of the tissue;

based on the determined power load curve algorithm: for a first application period, causing the energy delivery component to transmit the electrosurgical energy at a first power level, the first application period comprising a point in time where impedance of the tissue reaches a minimum impedance value;

for a second application period after the first application period, causing the energy delivery component to transmit the electrosurgical energy, starting from a predetermined proportion of a transition impedance threshold level and decreasing the electrosurgical energy at a steady rate from the first power level until a second power level is reached, wherein the second power level is lower than the first power level and the second application period comprises a point in time where the impedance of the tissue rises above the minimum impedance value; and

for a third application period after the second application period, directly after reaching the second power level, causing the energy delivery component to reduce the second power level to a third power level while maintaining a constant level of the impedance of the tissue to transmit the electrosurgical energy at the third power level upon the impedance of the tissue reaching the transition impedance threshold level, the third power level lower than the second power level and the third application period comprising a point in time where the impedance of the tissue rises above the transition impedance threshold level.

10. The method of claim 9, wherein determining the power load curve algorithm comprises determining whether the benchmark level of impedance is less than a first threshold impedance value, whether the benchmark level of impedance is greater than the first threshold impedance value and less than a second threshold impedance value, and whether the benchmark level of impedance is greater than the second threshold impedance value.

11. The method of claim 9, wherein the first application period and the second application period combined comprise a time period where the electrosurgical energy is delivered at a higher rate and causes sealing of the tissue at the surgical site.

12. The method of claim 9, wherein the third application period further comprises a time period where the impedance of the tissue rises to a level such that the electrosurgical energy is delivered at a lower rate and no longer causes sealing of the tissue at the surgical site.

13. The method of claim 9, wherein the benchmark level of impedance is the minimum impedance value or an initial level of impedance of the tissue.

14. The method of claim 9, wherein a beginning of the third application period is based on the measured benchmark level of impedance.

15. The method of claim 9, wherein the first application period and the second application period combined comprise a continuous time period where the impedance of the tissue remains below an initial level of impedance in the tissue.

16. The method of claim 9, wherein the energy delivery component is configured to transmit RF and ultrasonic energy.

27

17. A surgical instrument comprising:
 a handle assembly;
 a shaft coupled to a distal end of the handle assembly;
 an end effector coupled to a distal end of the shaft and
 comprising at least one energy delivery component 5
 configured to transmit electrosurgical energy to tissue
 at a surgical site; and
 a control circuit communicatively coupled to the at least
 one energy delivery component and programmed to:
 for a first application period, cause the at least one 10
 energy delivery component to transmit the electro-
 surgical energy at a first power level, the first appli-
 cation period comprising a point in time where
 impedance of the tissue reaches a minimum imped- 15
 ance value;
 for a second application period after the first applica-
 tion period, cause the at least one energy delivery
 component to transmit the electrosurgical energy,
 starting from a predetermined proportion of a transi- 20
 tion impedance threshold level and decreasing the
 electrosurgical energy at a steady rate from the first
 power level until a second power level is reached,
 wherein the second power level is lower than the first 25
 power level and the second application period com-
 prises a point in time where the impedance of the
 tissue rises above the minimum impedance value;
 and

28

for a third application period after the second applica-
 tion period, directly after reaching the second power
 level, cause the at least one energy delivery compo-
 nent to reduce the second power level to a third
 power level while maintaining a constant level of the
 impedance of the tissue to transmit the electrosurgi-
 cal energy at the third power level upon the imped-
 ance of the tissue reaching the transition impedance
 threshold level, the third power level lower than the
 second power level and the third application period
 comprising a point in time where the impedance of
 the tissue rises above the transition impedance
 threshold level.

18. The surgical instrument of claim 17, wherein the first
 application period and the second application period com-
 bined comprise a time period where the electrosurgical
 energy is delivered at a higher rate and causes sealing of the
 tissue at the surgical site.

19. The surgical instrument of claim 17, wherein the third
 application period further comprises a time period where the
 impedance of the tissue rises to a level such that the
 electrosurgical energy is delivered at a lower rate and no
 longer causes sealing of the tissue at the surgical site.

20. The surgical instrument of claim 17, further compris-
 ing at least one sensor configured to measure an initial level
 of impedance in the tissue and the minimum impedance
 value in the tissue.

* * * * *

专利名称(译)	高级谐波能量的方法和系统		
公开(公告)号	US10376305	公开(公告)日	2019-08-13
申请号	US15/229562	申请日	2016-08-05
[标]申请(专利权)人(译)	爱惜康内镜外科，LLC		
申请(专利权)人(译)	爱惜康内镜外科，LLC		
当前申请(专利权)人(译)	ETHICON LLC		
[标]发明人	YATES DAVID C KRUMM AMY M DAVISON MARK A		
发明人	YATES, DAVID C. KRUMM, AMY M. DAVISON, MARK A.		
IPC分类号	A61B18/12 A61B18/14 A61B18/00 A61B17/32		
CPC分类号	A61B18/1445 A61B18/1206 A61B18/1482 A61B2018/00875 A61B2018/00994 A61B2018/00702 A61B2018/0063 A61B2018/00208 A61B2018/00642 A61B2018/00678 A61B17/320092 A61B2017/320094 A61B2017/320095		
其他公开文献	US20180036065A1		
外部链接	Espacenet		

摘要(译)

本公开的各方面被呈现用于医疗器械，该医疗器械被配置为调节用于密封过程的功率水平以考虑组织阻抗水平随时间的变化。在一些方面，医疗器械可被配置成根据功率算法施加功率以通过随着组织阻抗水平开始上升到“浴盆区域”之外的时间施加逐渐降低的功率量来密封组织，这是在能量施加期间的时间段，其中组织阻抗足够低以使电外科能量有效地密封组织。在一些方面，一旦组织阻抗水平超过“浴盆区域”，则切断电源。通过逐渐降低功率，在仍然施加有效功率水平用于密封和延长组织阻抗的时间之间实现平衡。留在“浴缸区”。

