



US 20020016544A1

(19) **United States**(12) **Patent Application Publication**
Hareyama et al.(10) **Pub. No.: US 2002/0016544 A1**(43) **Pub. Date: Feb. 7, 2002**(54) **THERAPEUTIC SYSTEM**(30) **Foreign Application Priority Data**(75) Inventors: **Norihiko Hareyama**, Tokyo (JP); **Toru Nagase**, Tokyo (JP); **Shinji Hatta**, Tokyo (JP)

Mar. 25, 1998 (JP)..... 10-077231


Publication Classification


Correspondence Address:

**FRISHAUF, HOLTZ, GOODMAN &
LANGER & CHICK, PC
767 THIRD AVENUE
25TH FLOOR
NEW YORK, NY 10017-2023 (US)**(51) **Int. Cl.⁷** **A61B 5/055**(52) **U.S. Cl.** **600/411; 600/407**(57) **ABSTRACT**(73) Assignee: **Olympus Optical Co. Ltd.**, Tokyo (JP)(21) Appl. No.: **09/894,723**(22) Filed: **Jun. 28, 2001****Related U.S. Application Data**

(62) Division of application No. 09/266,310, filed on Mar. 11, 1999.

A therapeutic system comprising a therapeutic applicator for treating living tissues and an observation unit for determining the position of the applicator. The therapeutic energy applied from the applicator to the living tissues is controlled in accordance with data representing the position of the applicator, determined by the observation unit. It is therefore easy to operate the system even if the applicator and the observation unit (e.g., an MRI apparatus) are used at the same time. The image of the living tissues remains clear during the use of the therapeutic applicator.

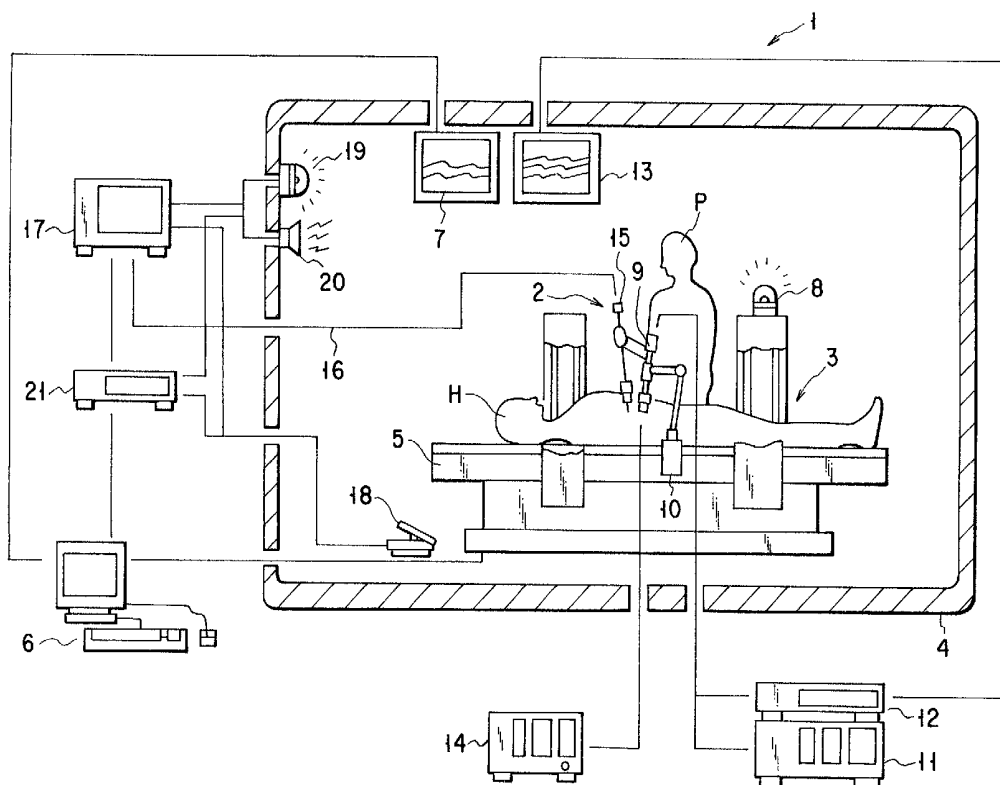

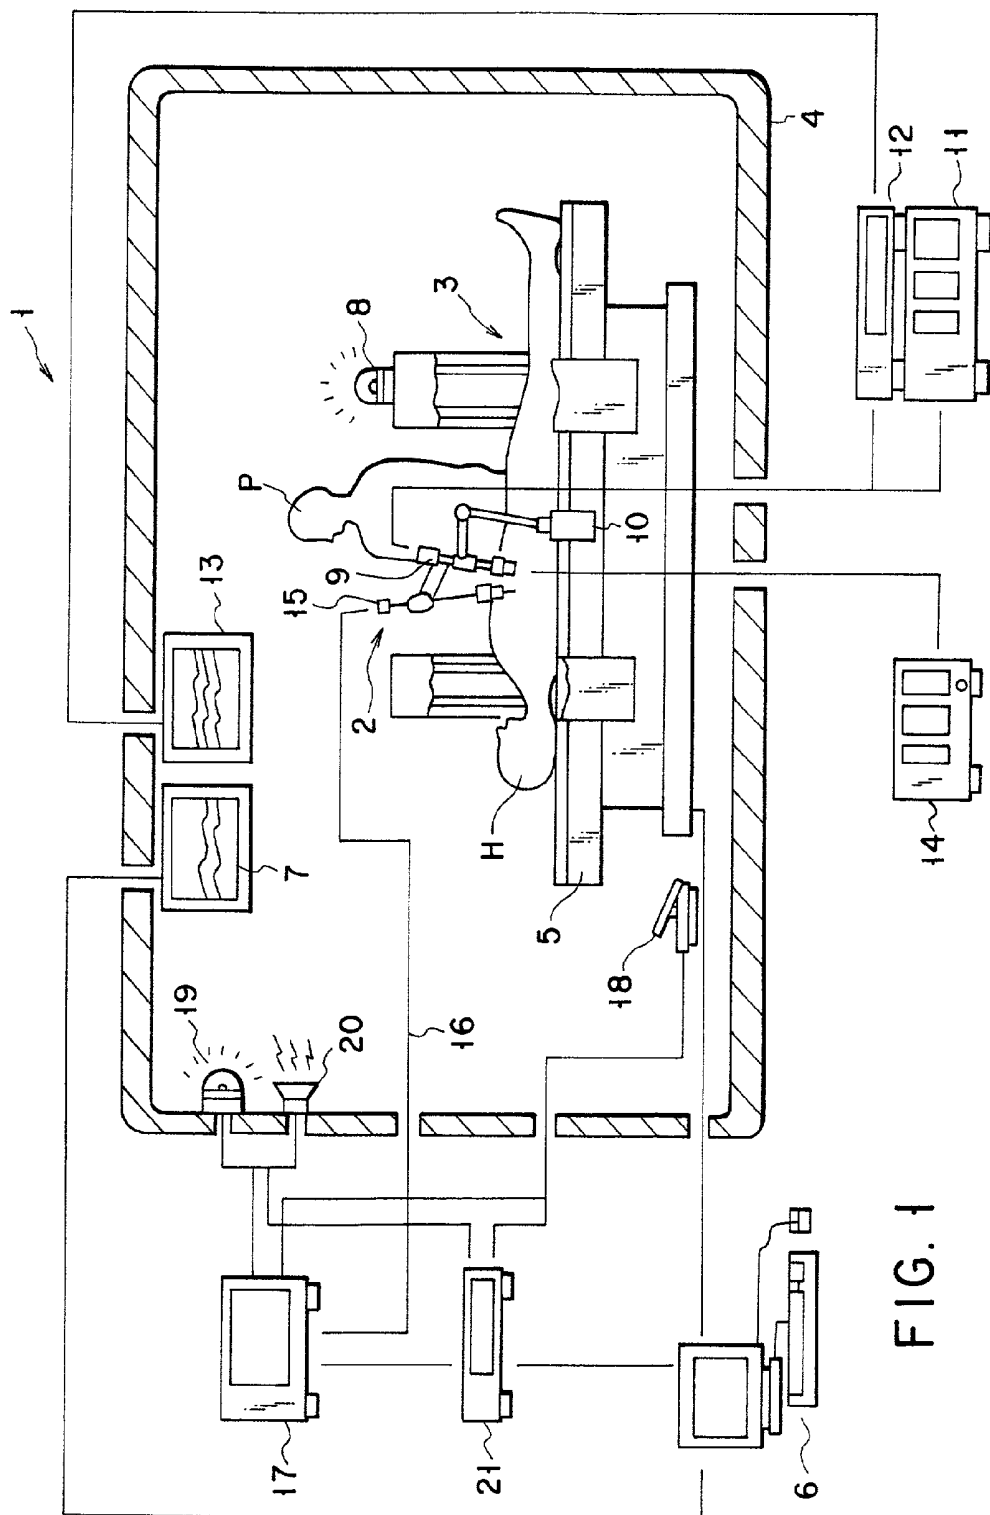

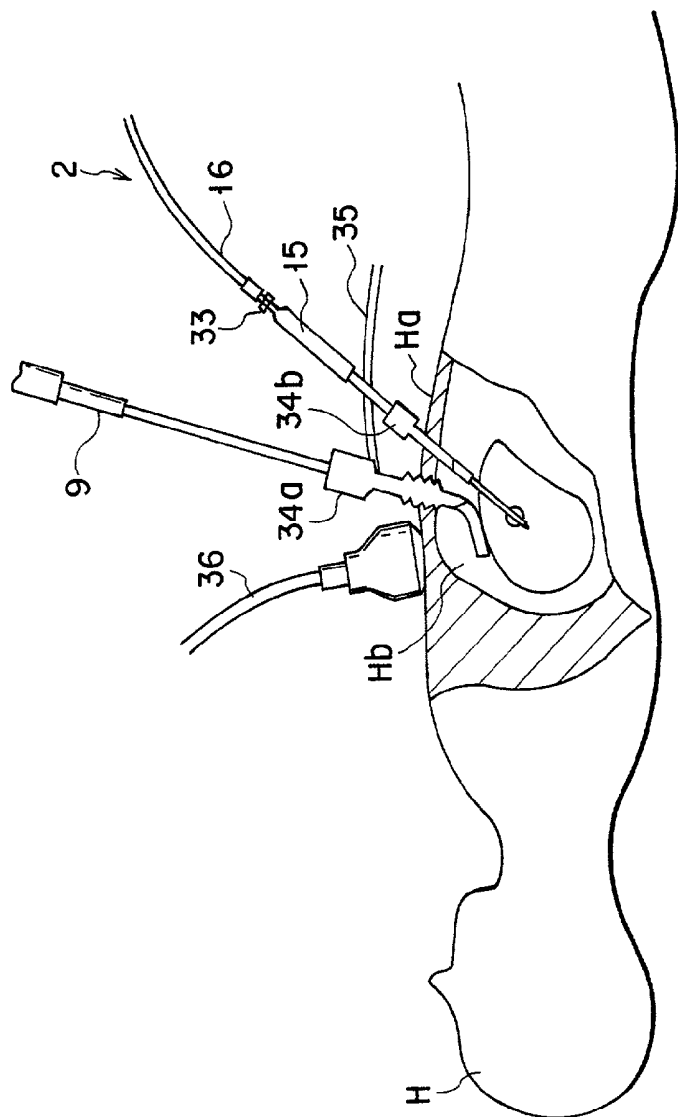


FIG. 2A

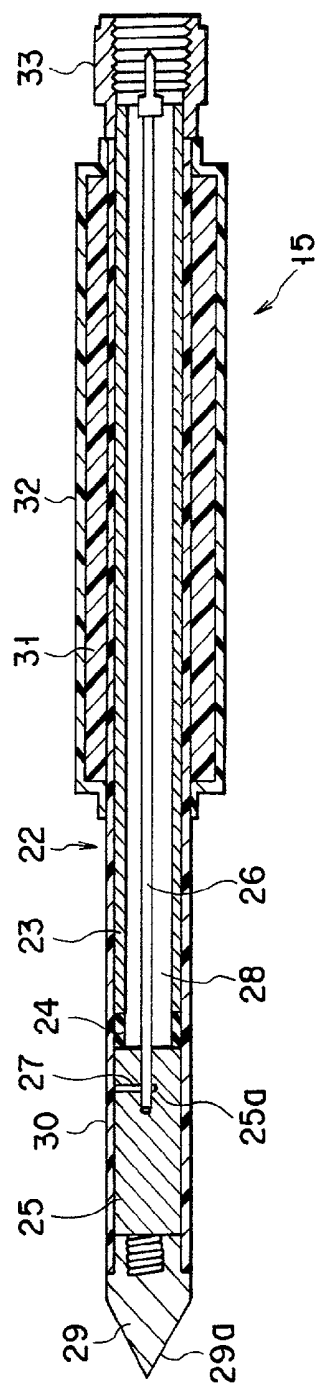


FIG. 2B

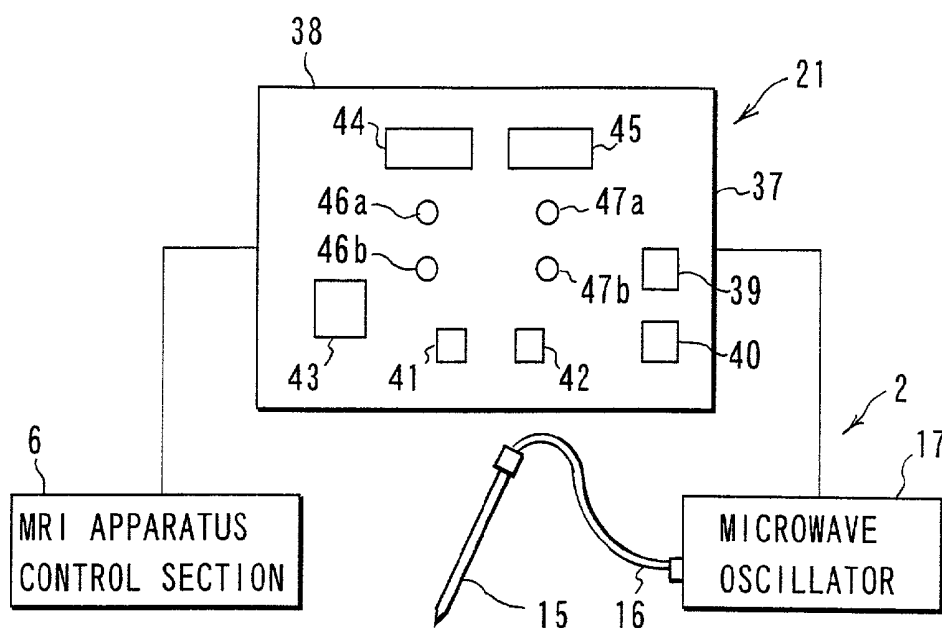


FIG. 3

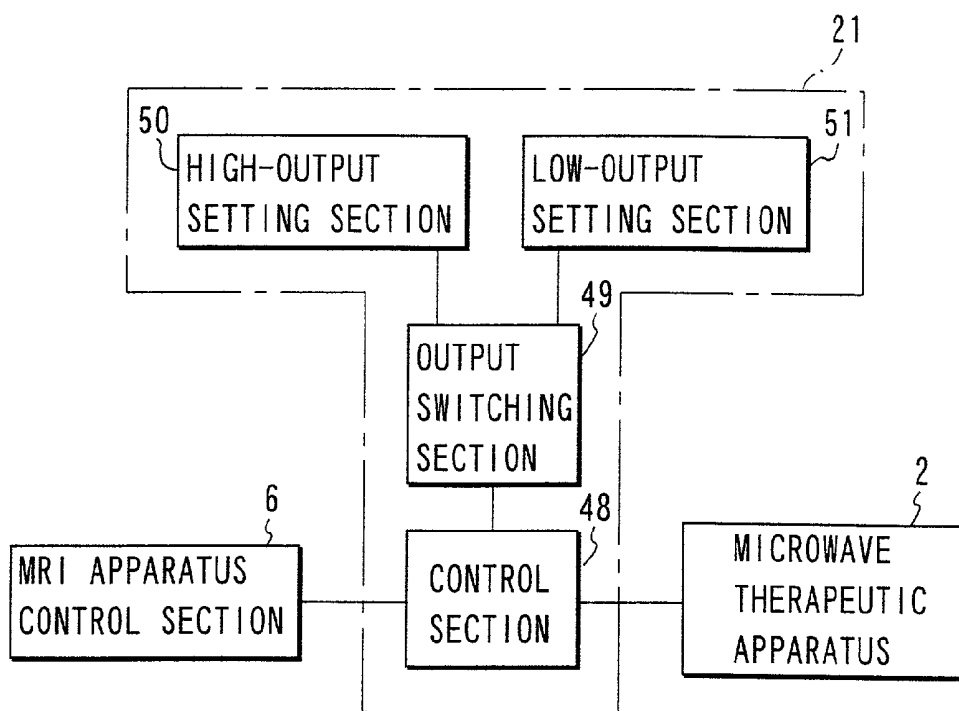


FIG. 4

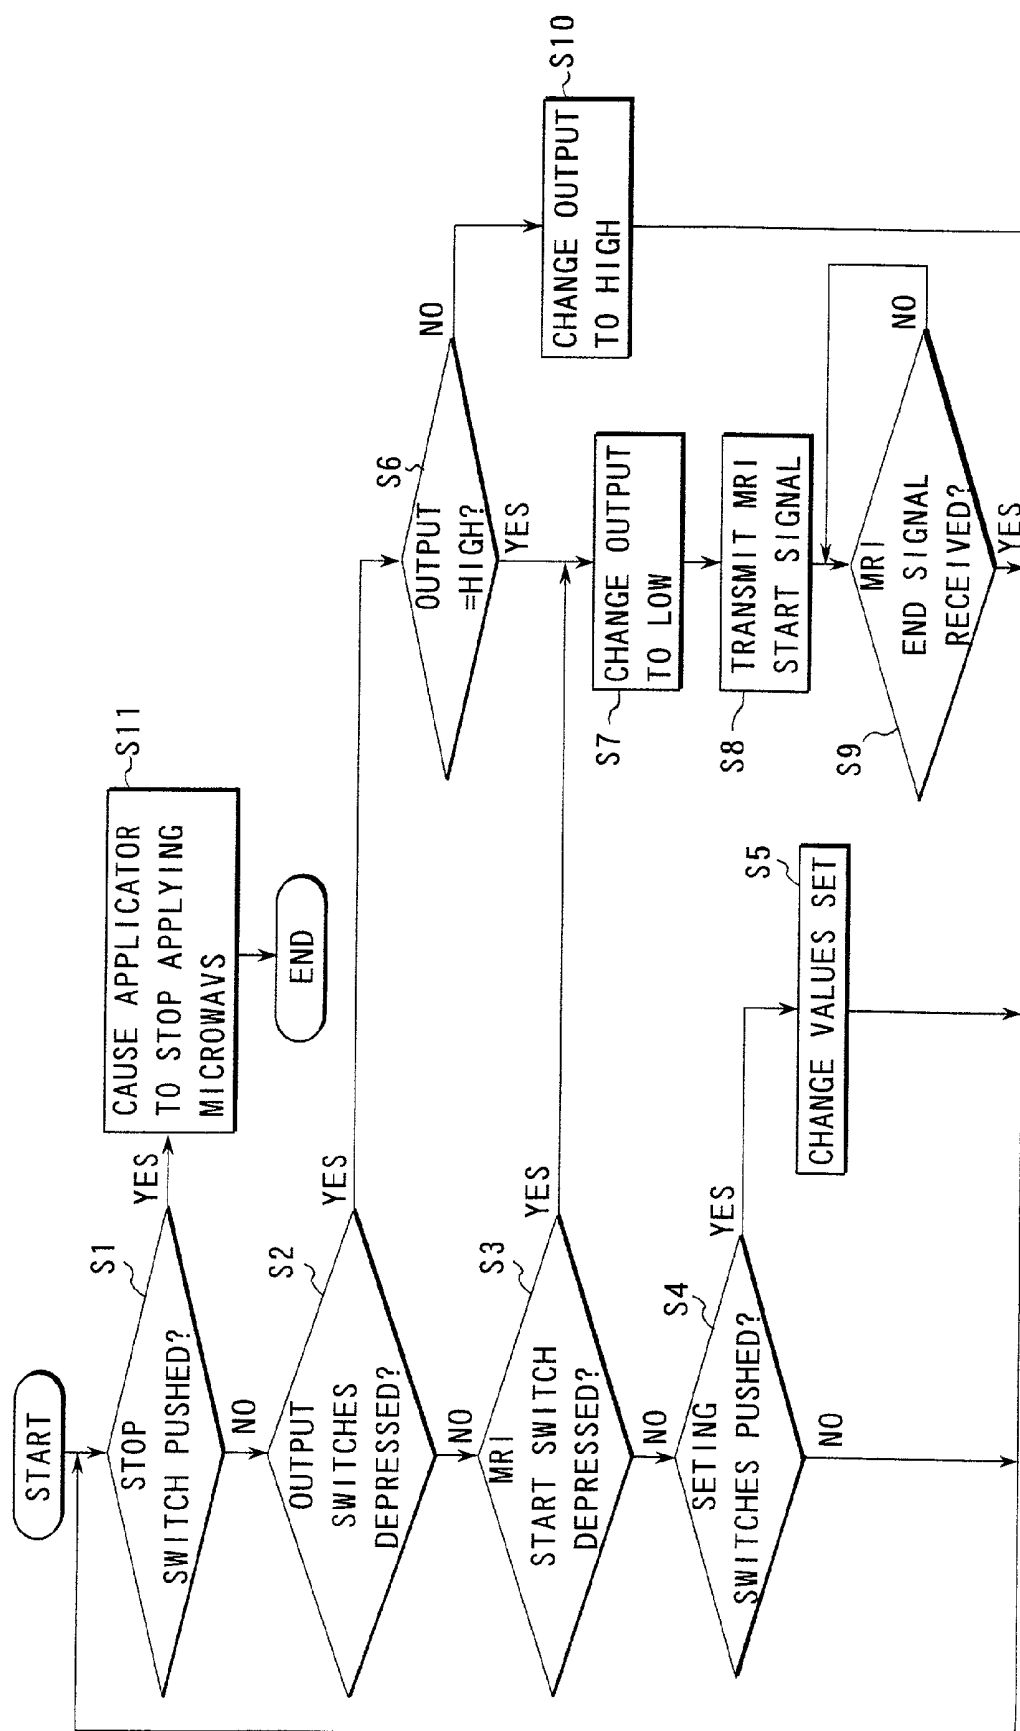


FIG. 5

FIG. 6

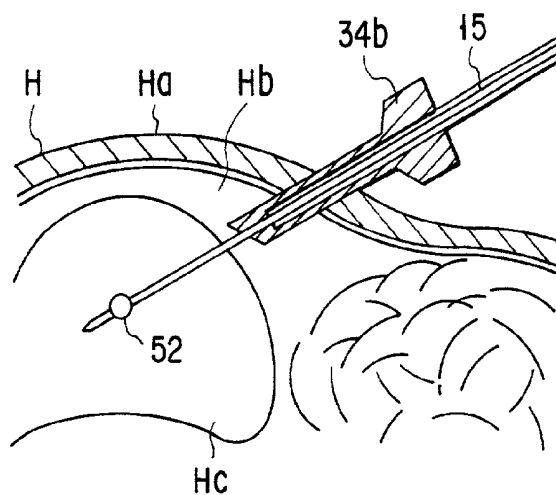


FIG. 7

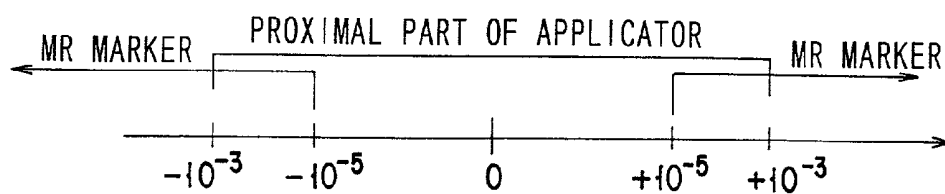
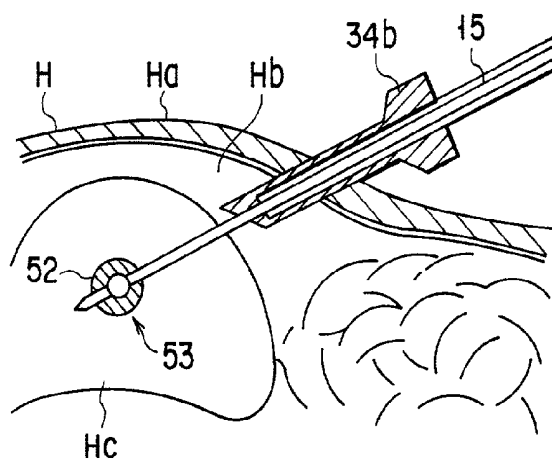


FIG. 8

FIG. 9

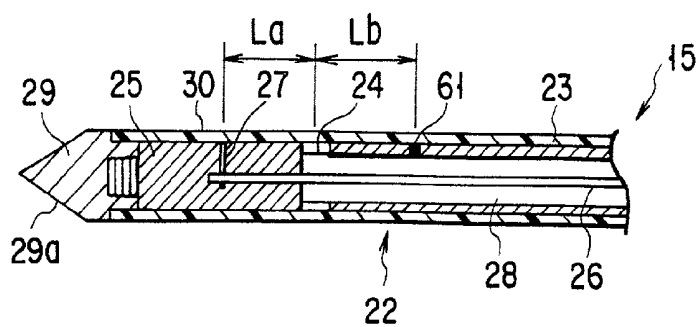


FIG. 10

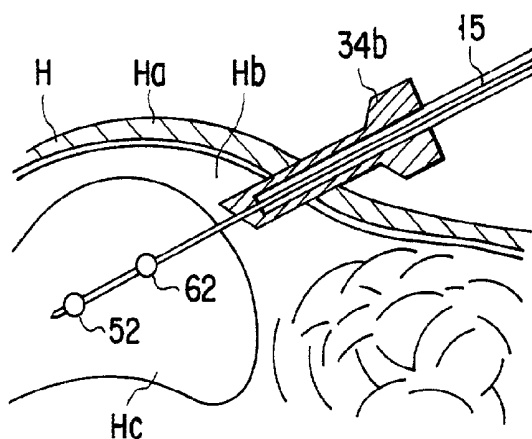


FIG. 11

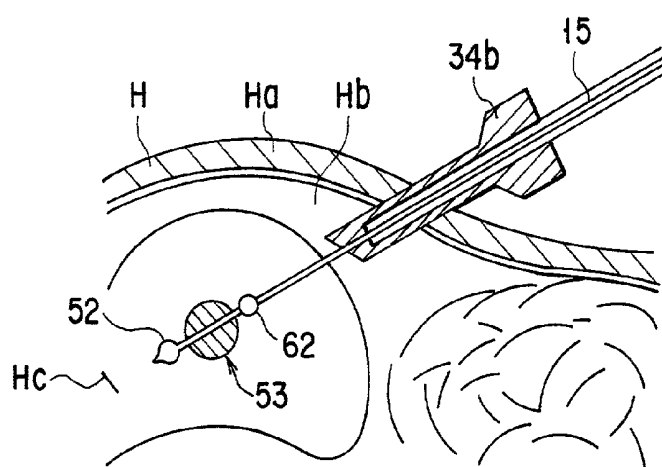


FIG. 12

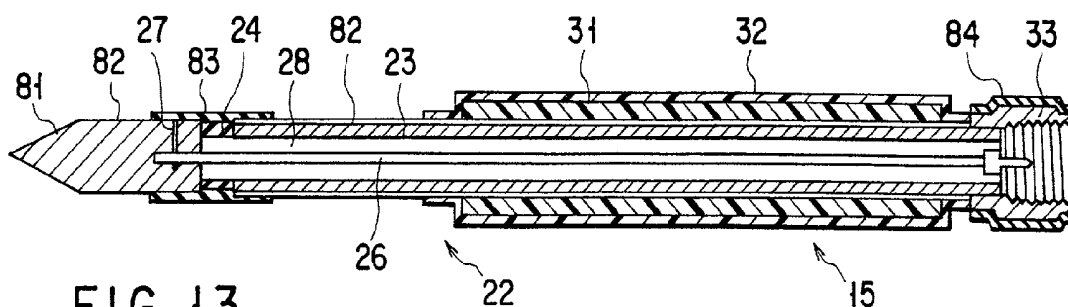
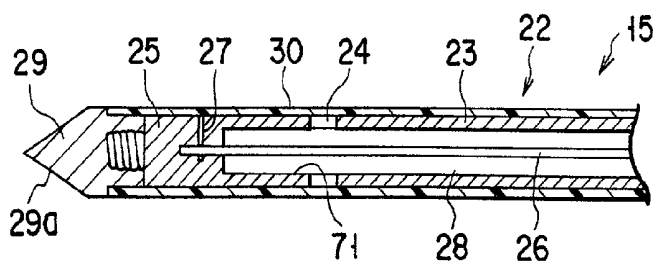


FIG. 13

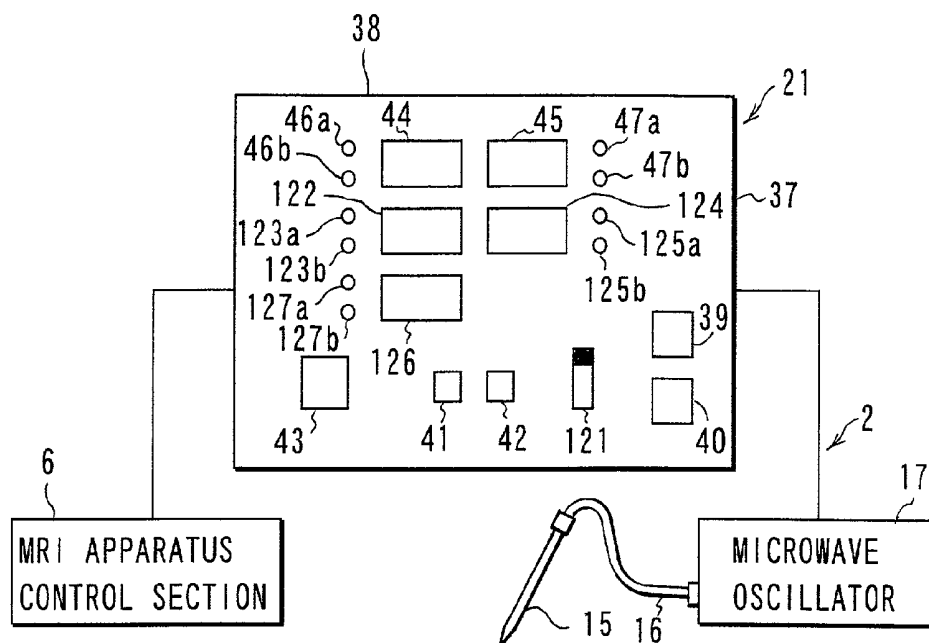


FIG. 18

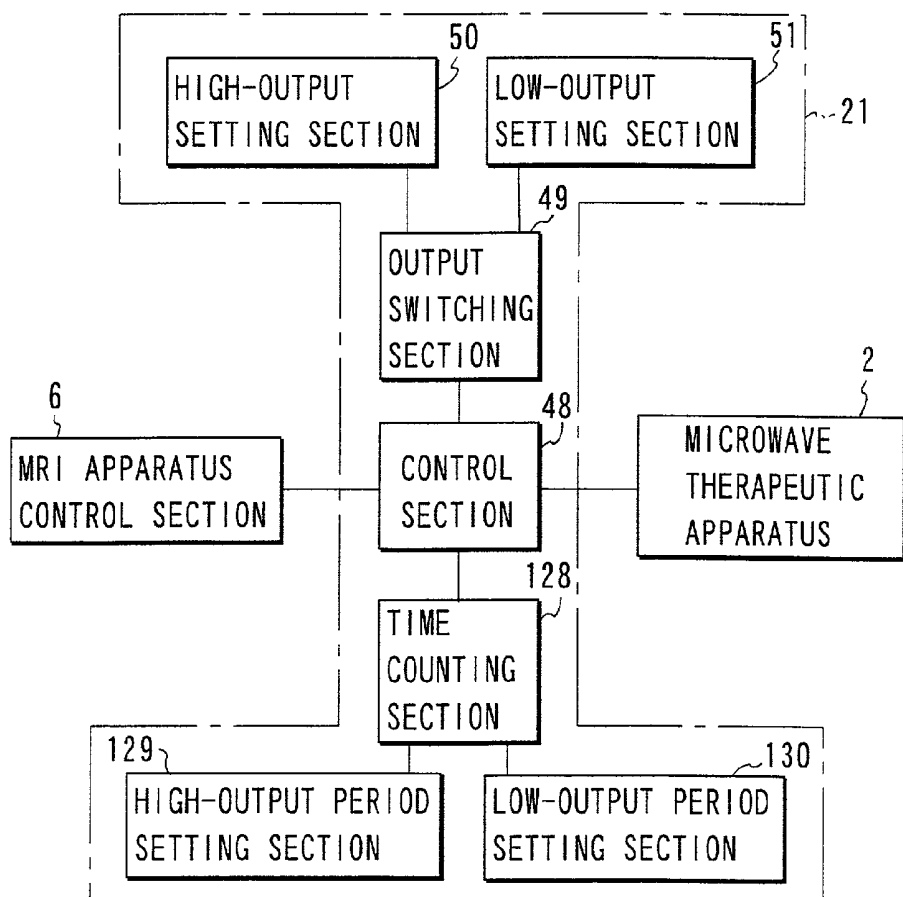


FIG. 19

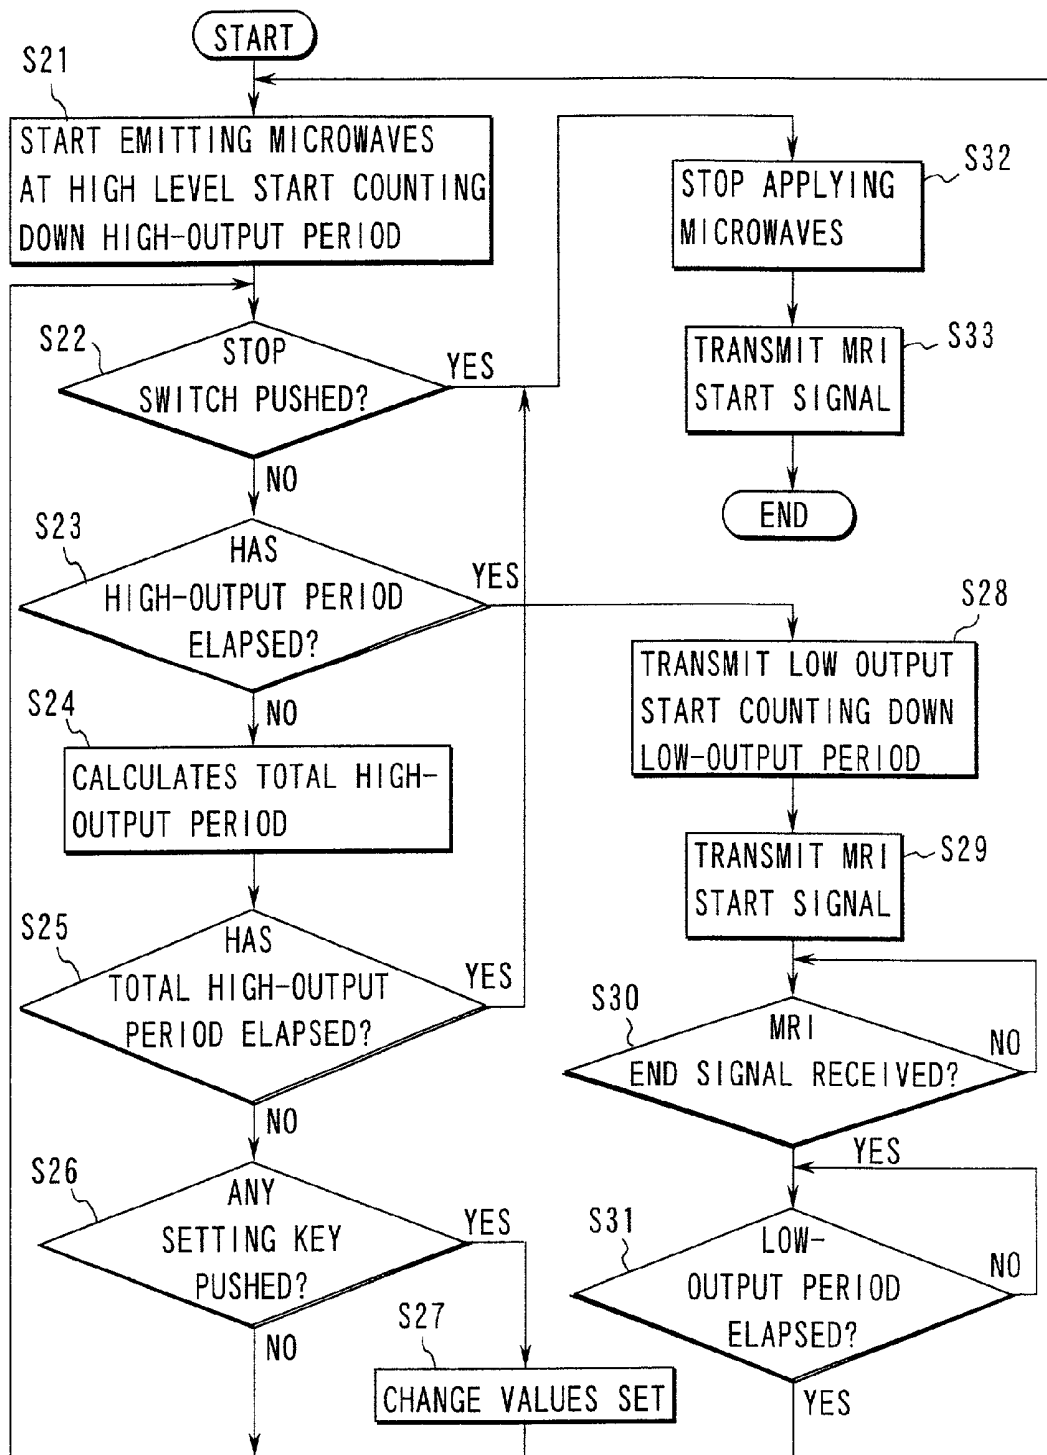


FIG. 20

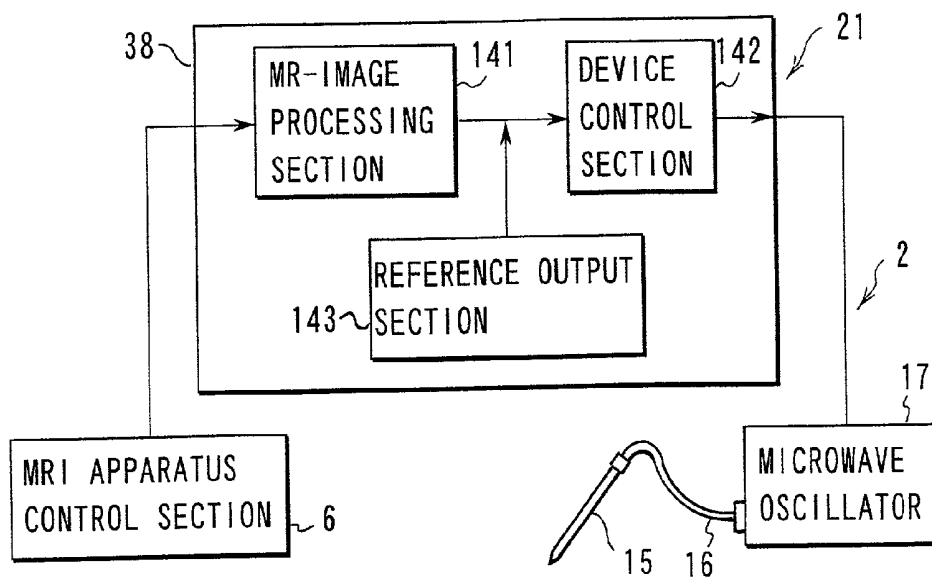


FIG. 21

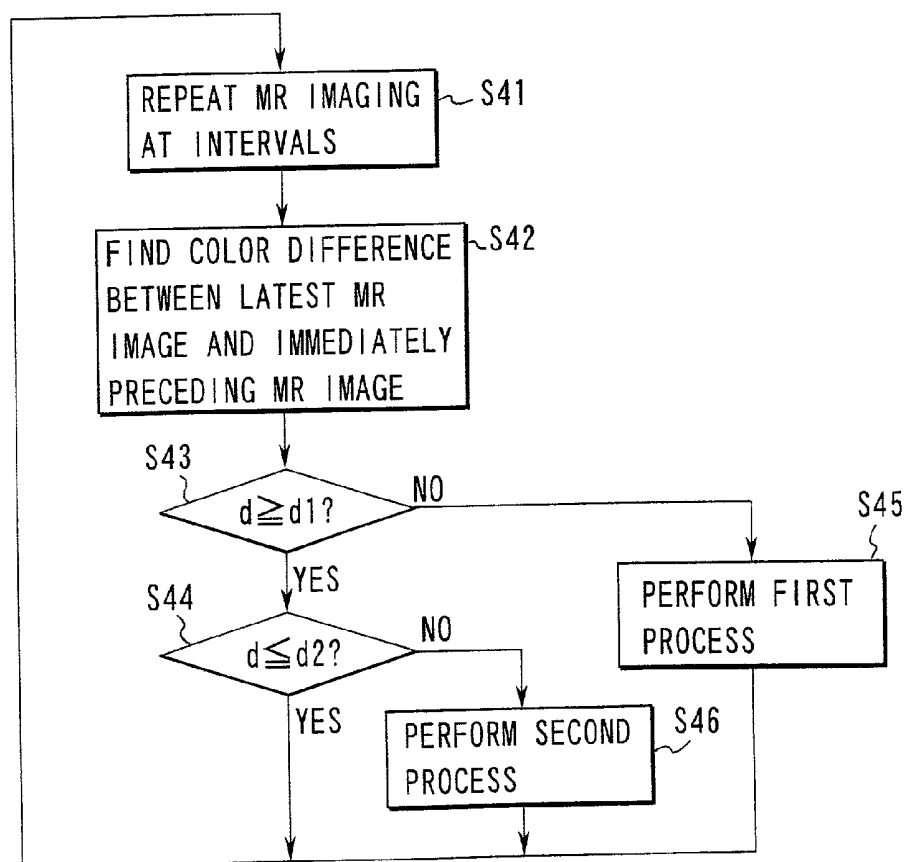


FIG. 22

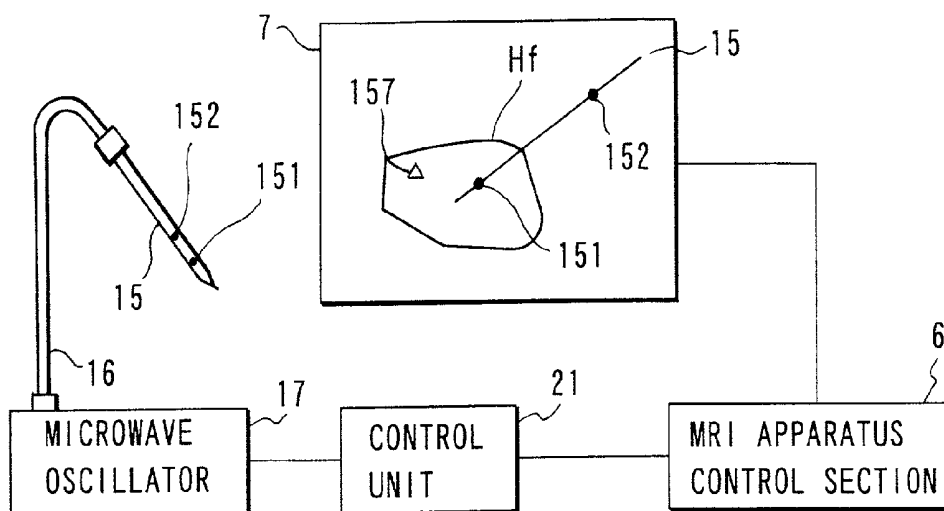


FIG. 23

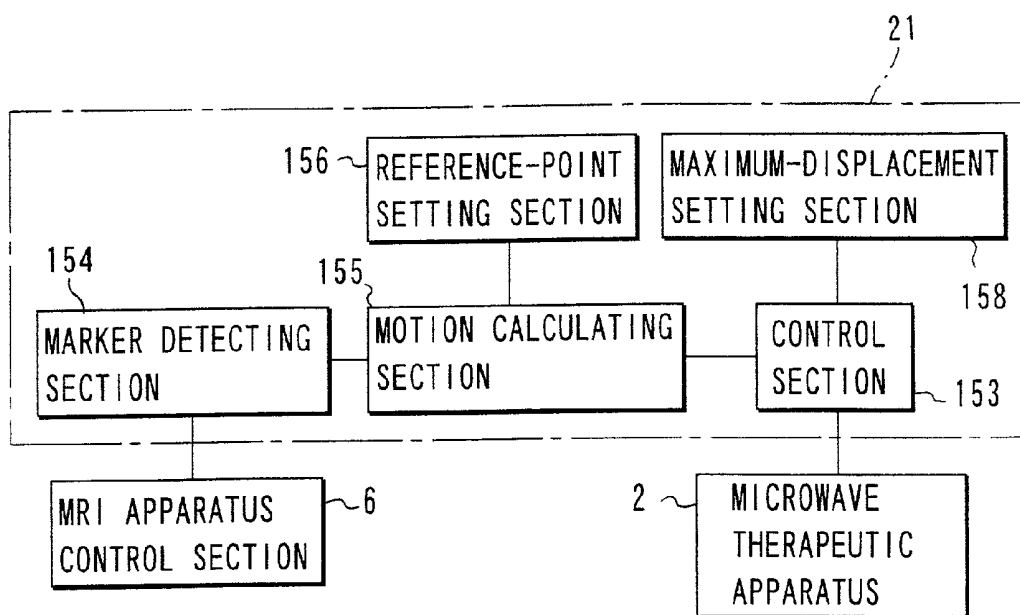


FIG. 24

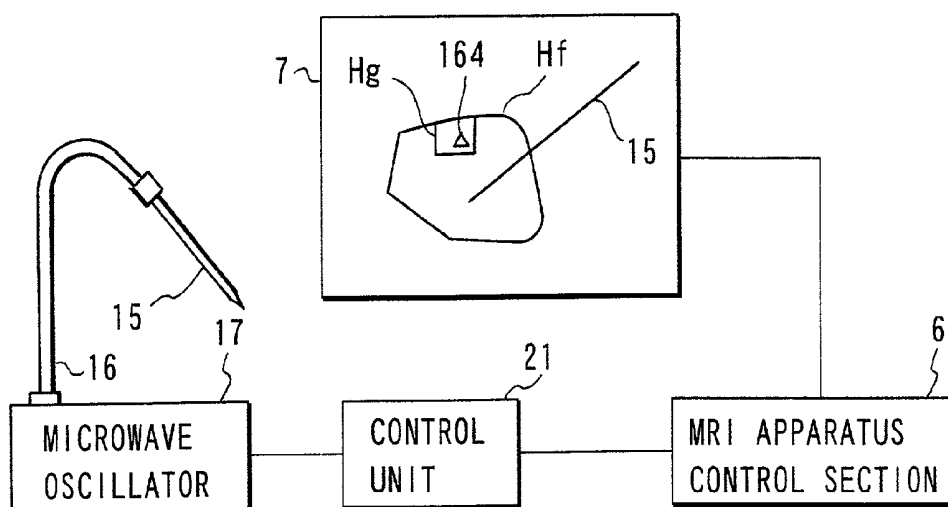


FIG. 25

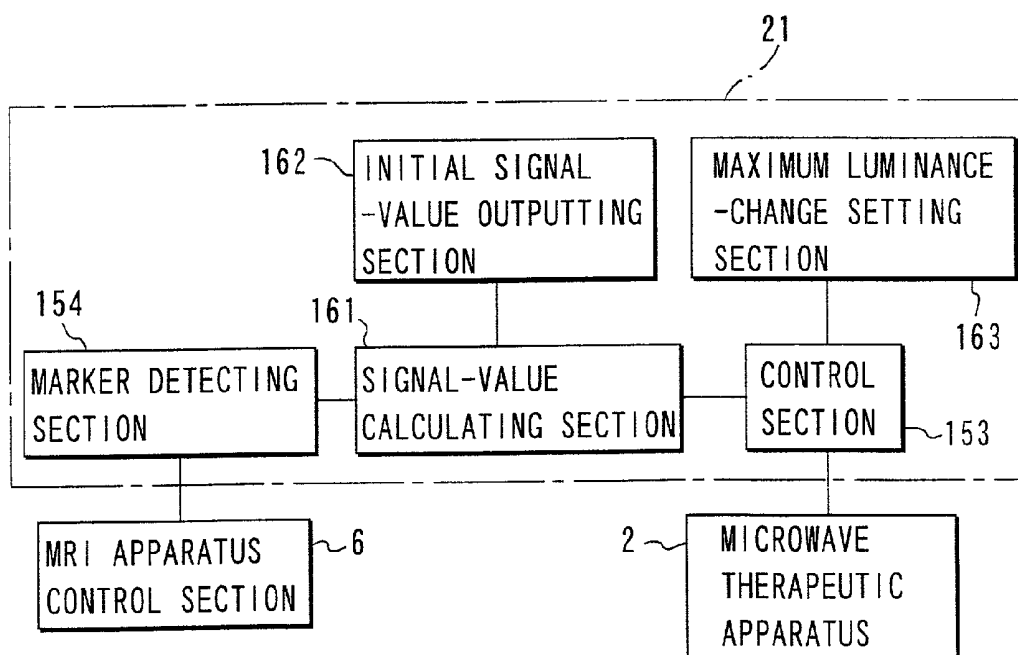


FIG. 26

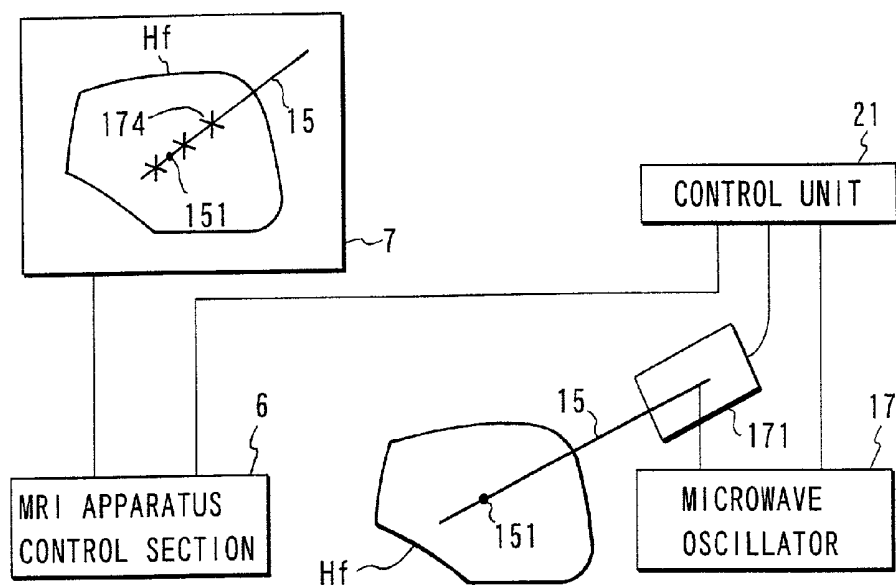


FIG. 27

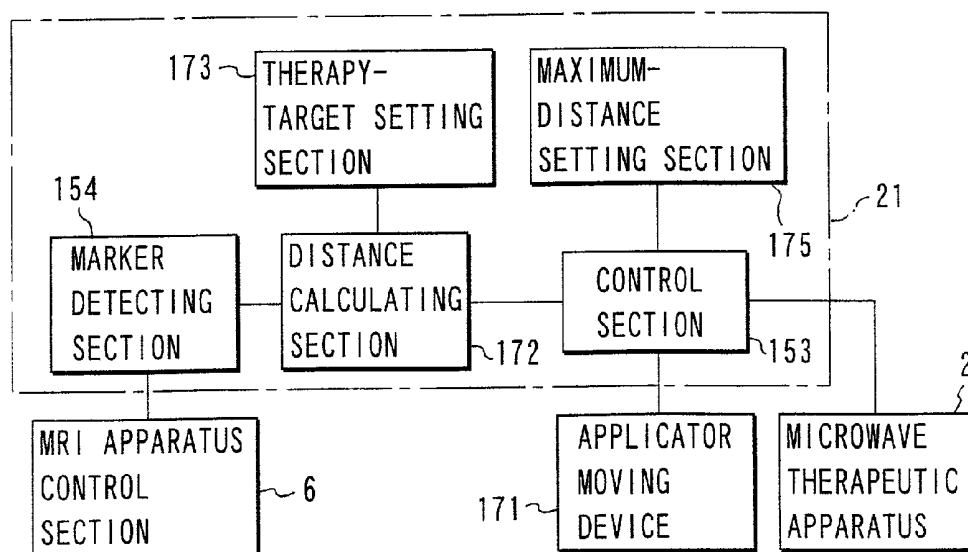
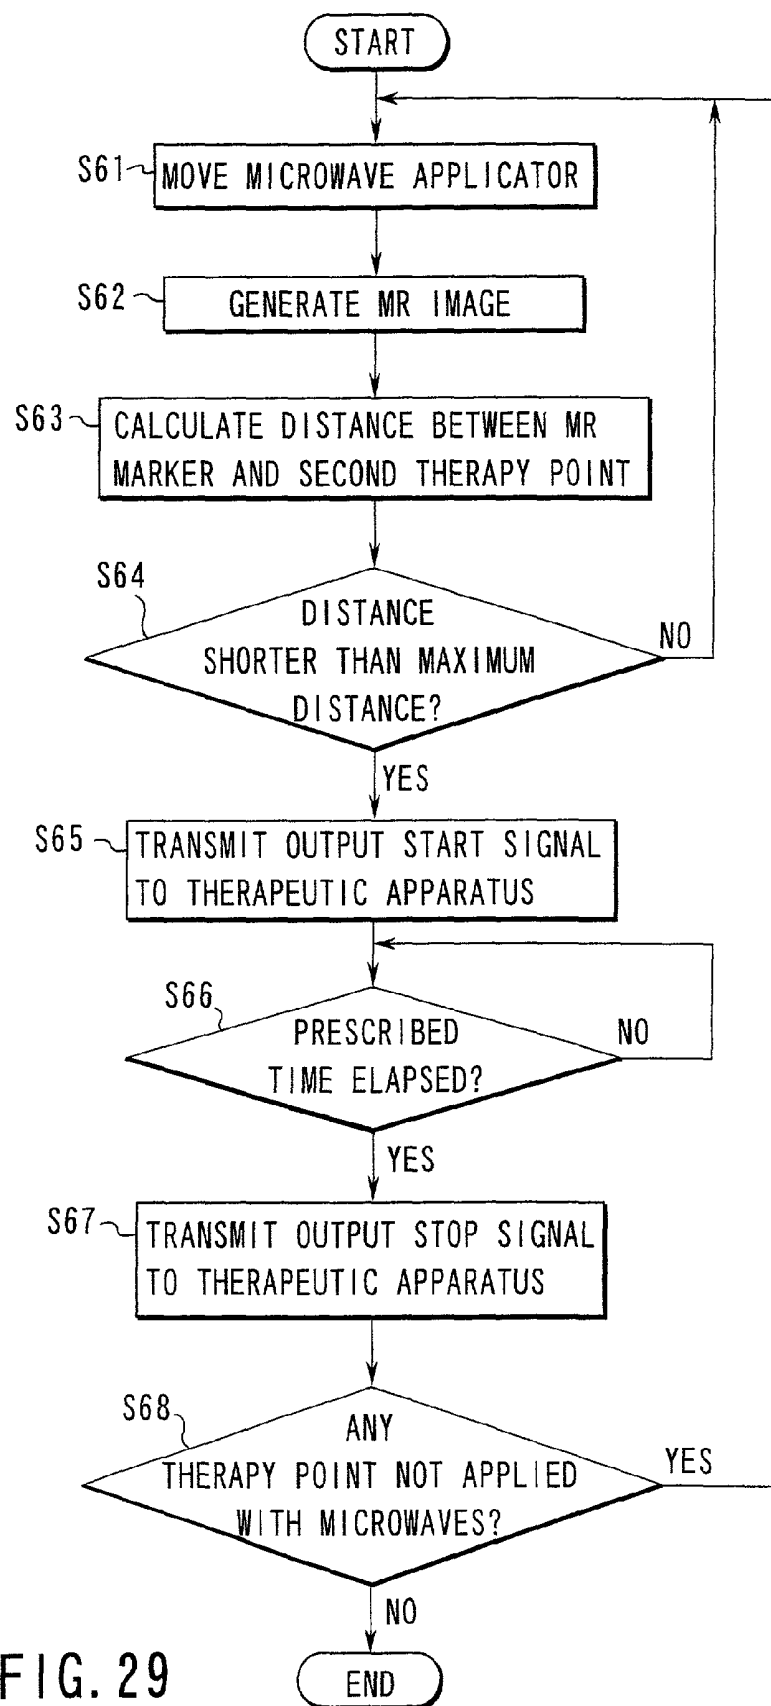


FIG. 28



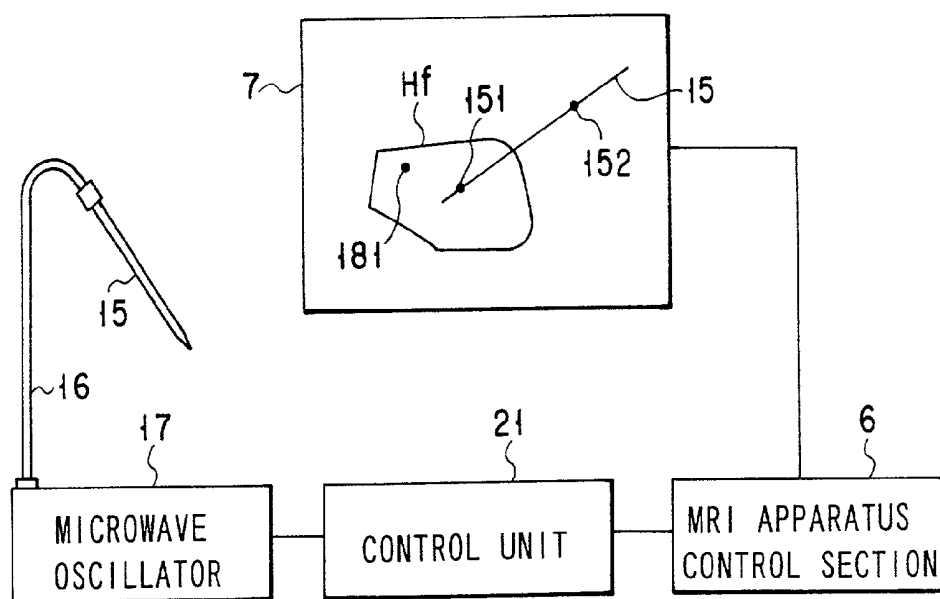


FIG. 30

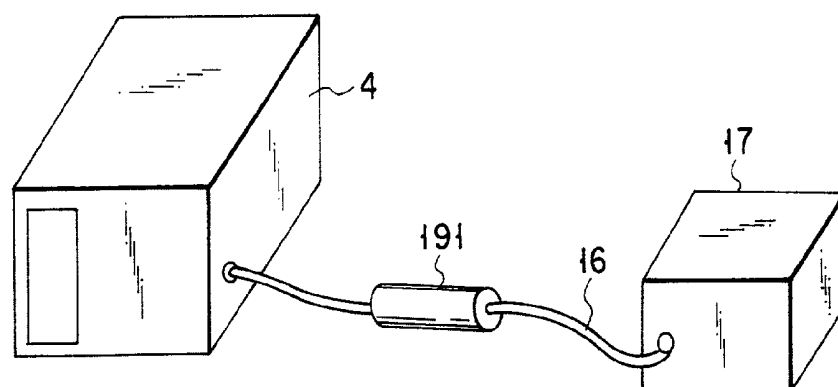


FIG. 31

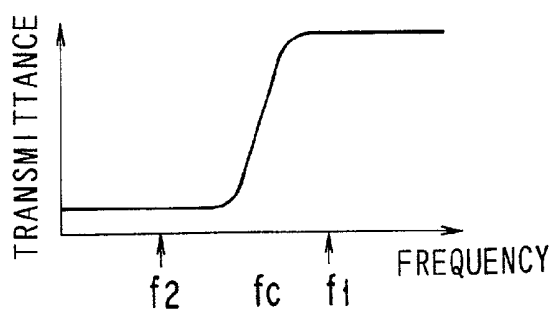


FIG. 32

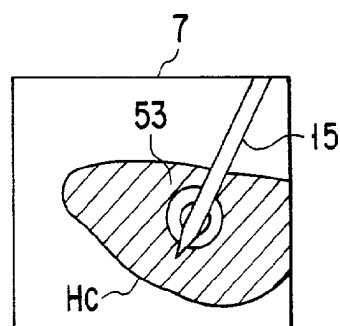


FIG. 33

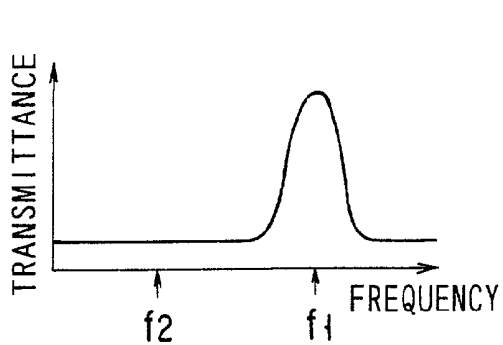


FIG. 34A

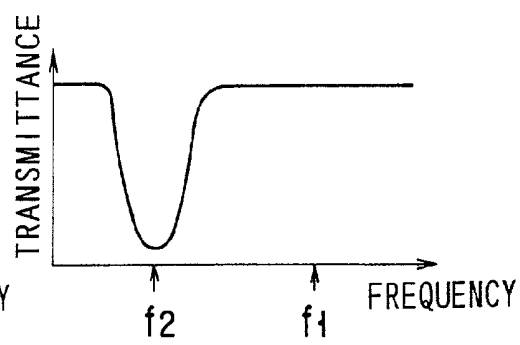


FIG. 34B

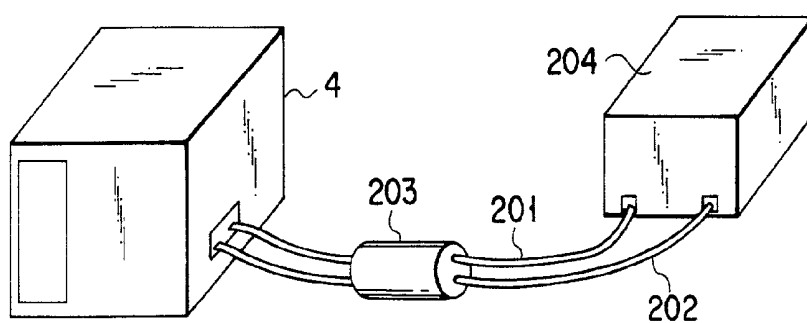


FIG. 35

FIG. 36

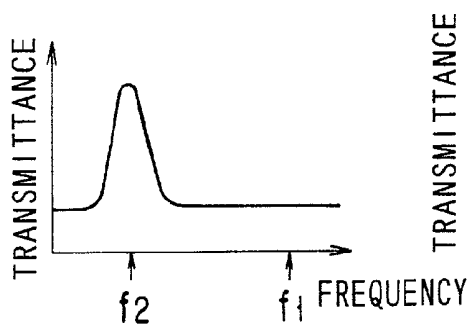
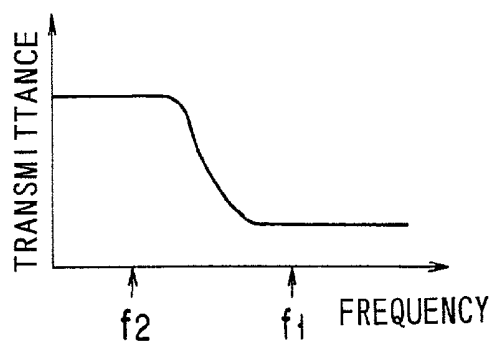


FIG. 37A

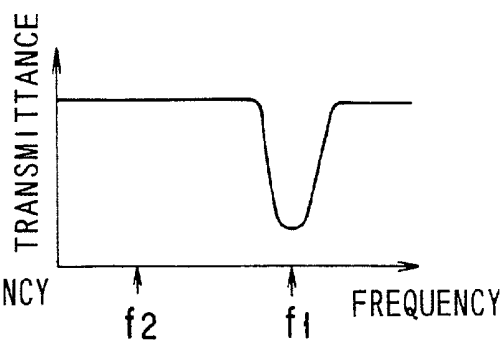
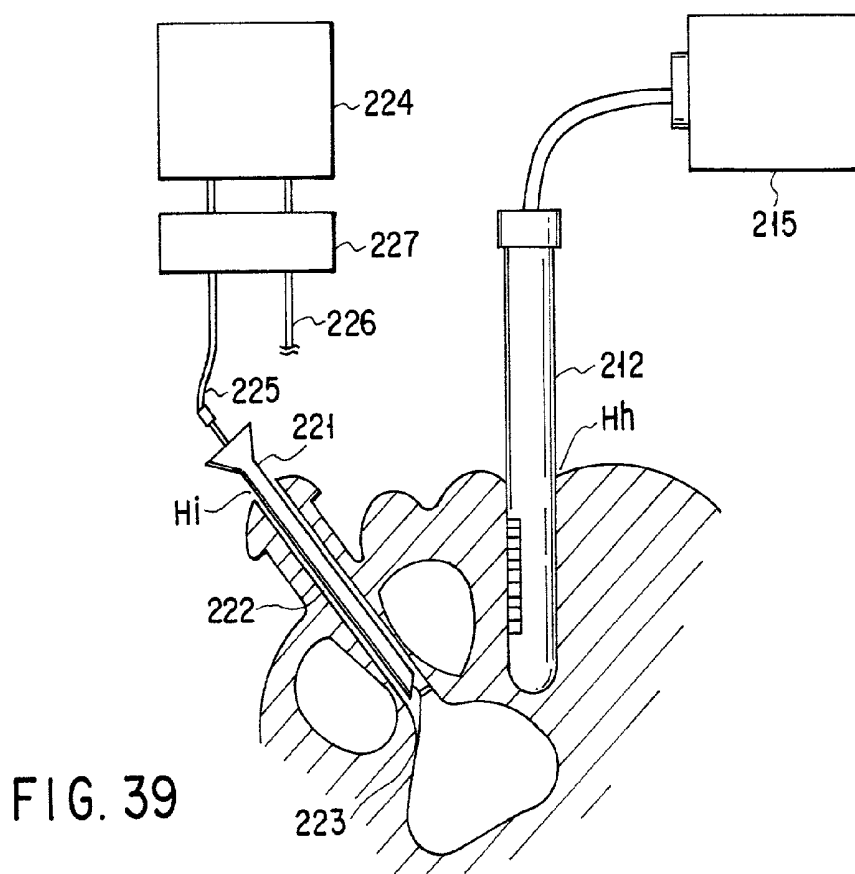
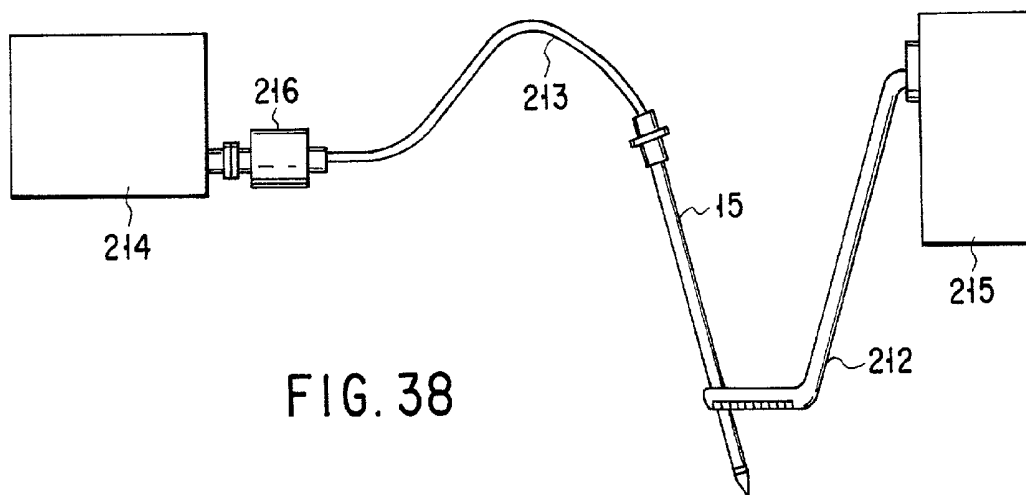


FIG. 37B



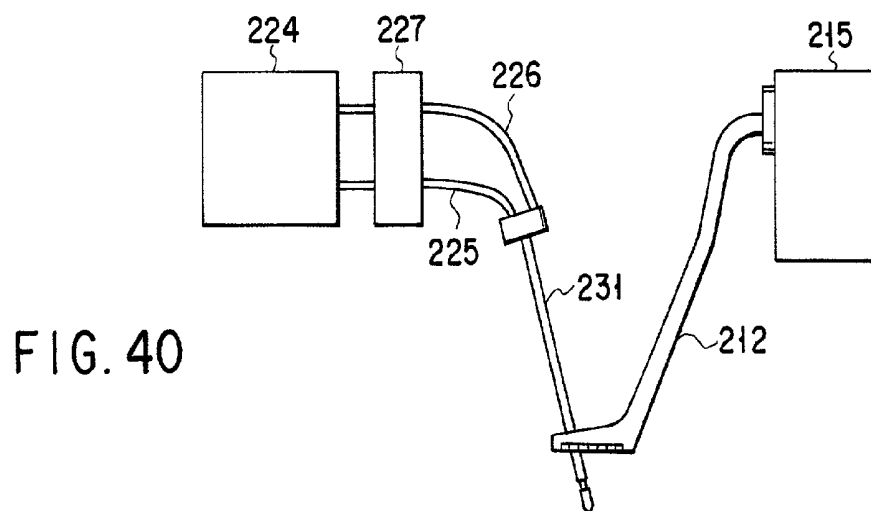


FIG. 40

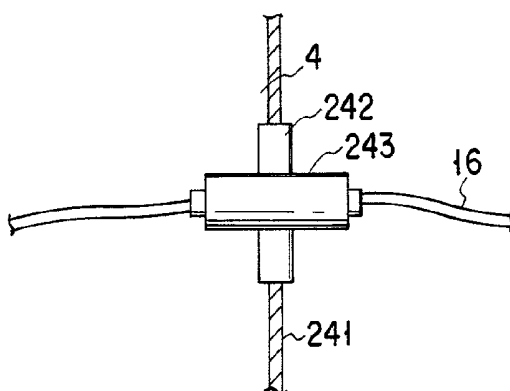


FIG. 41

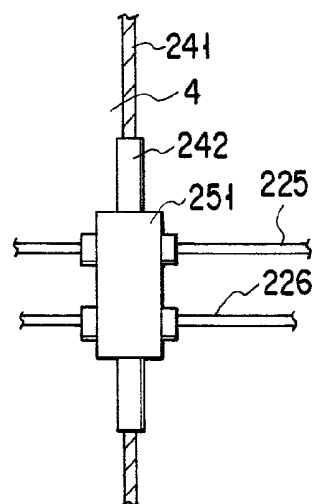


FIG. 42

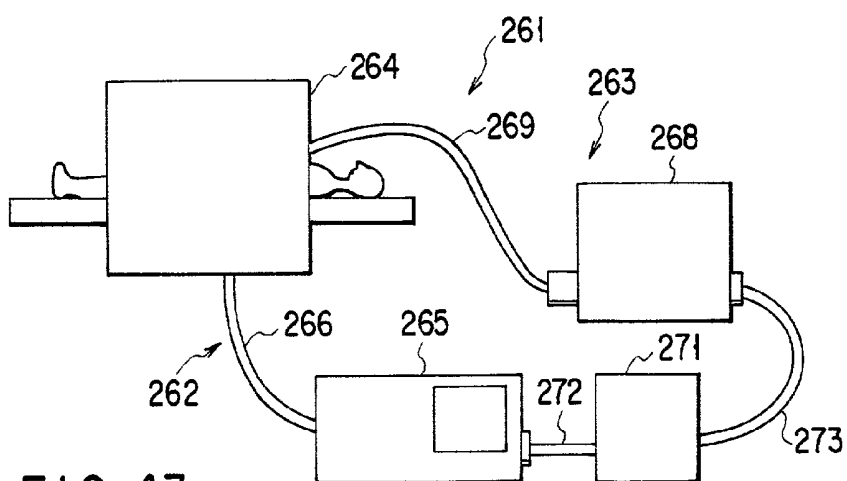


FIG. 43

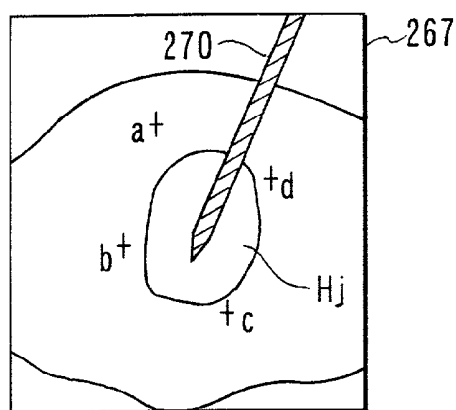


FIG. 44

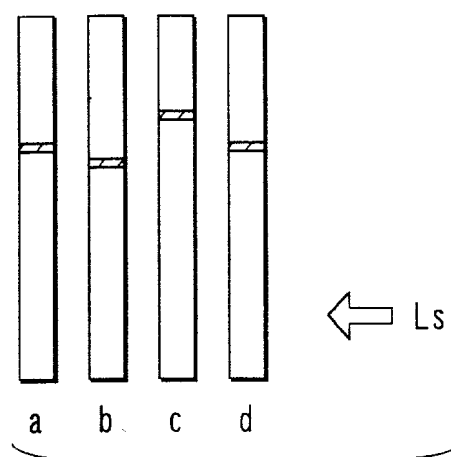


FIG. 45

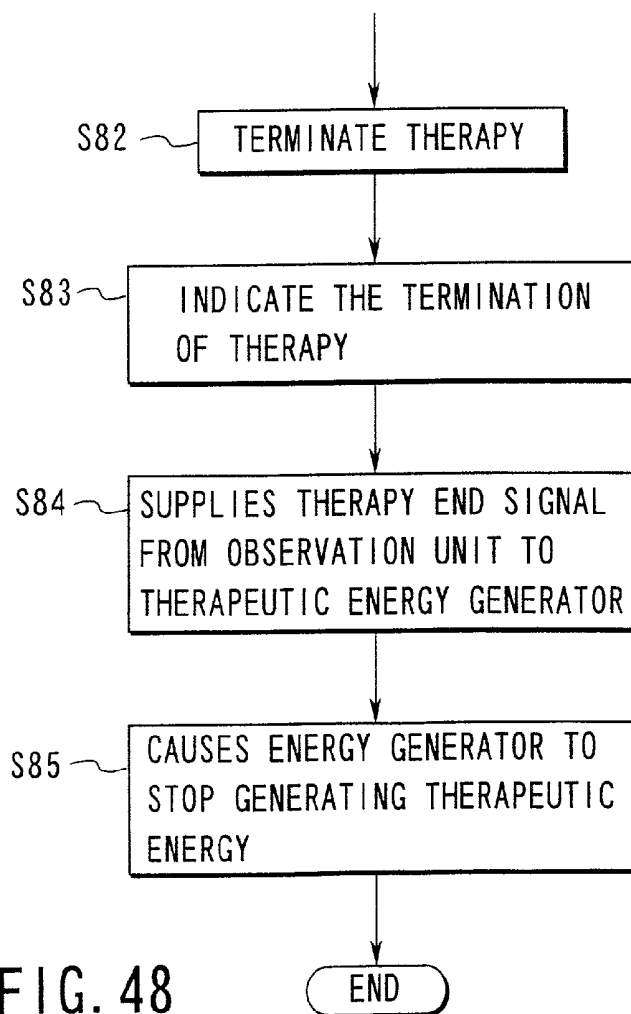


FIG. 48

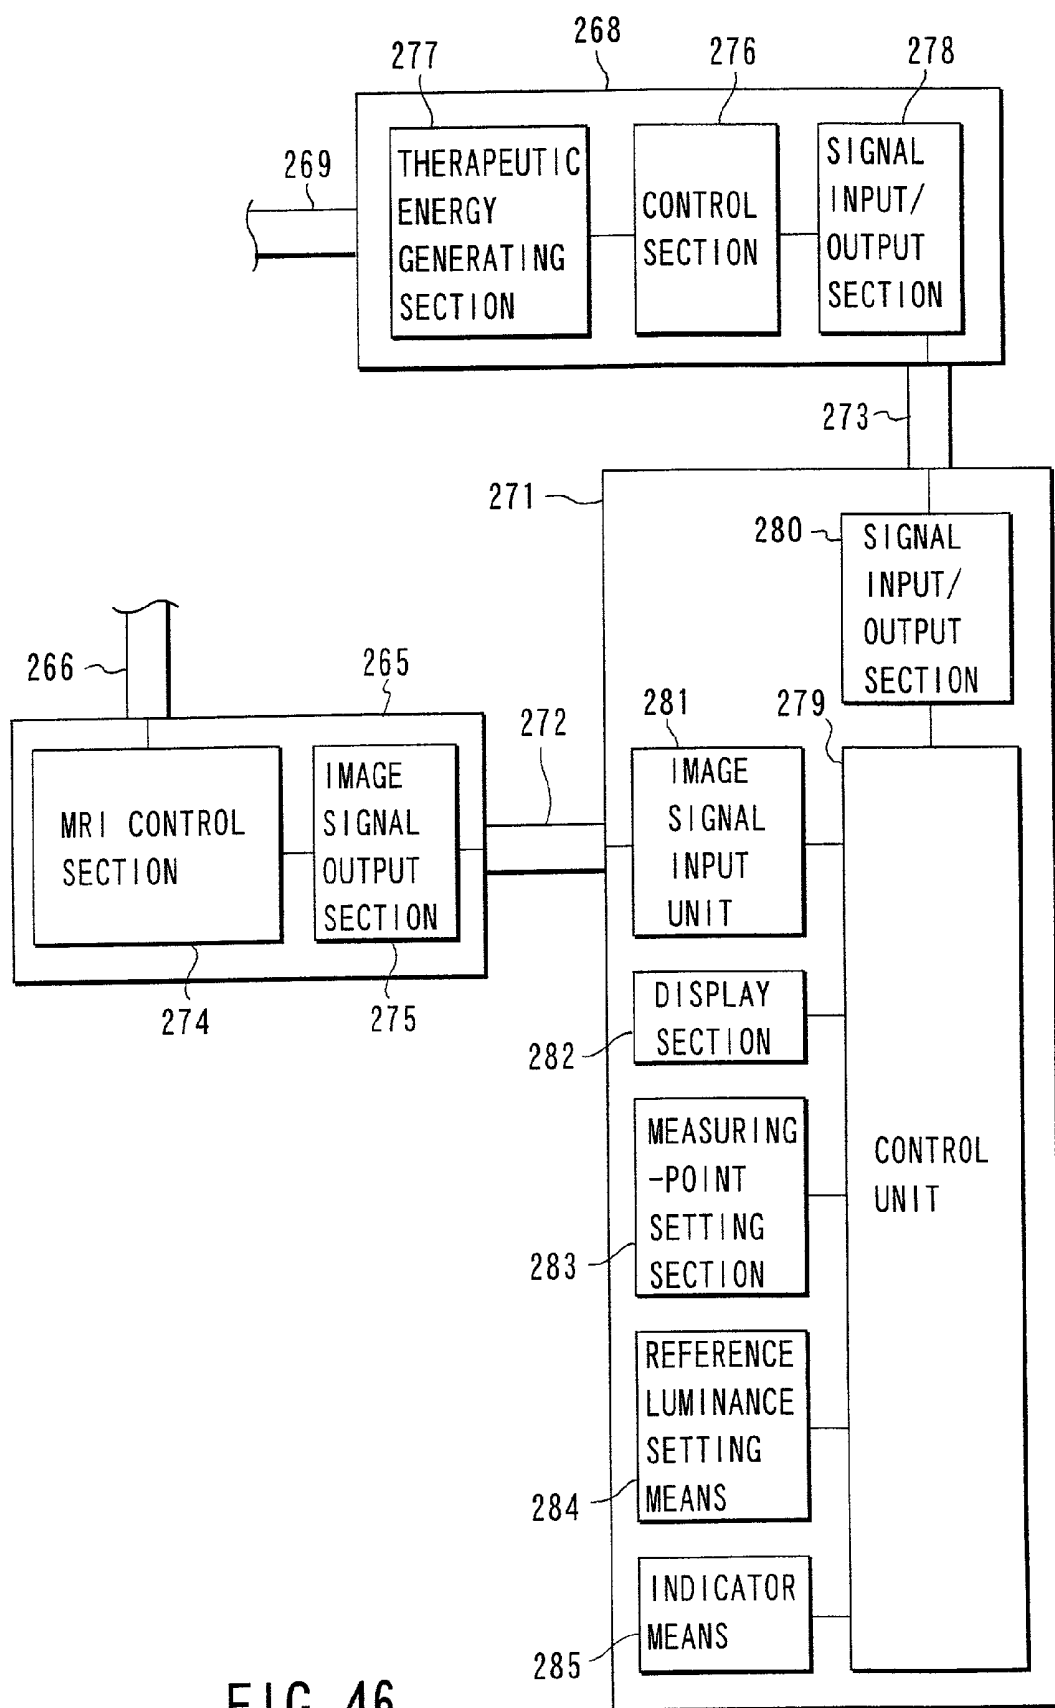


FIG. 46

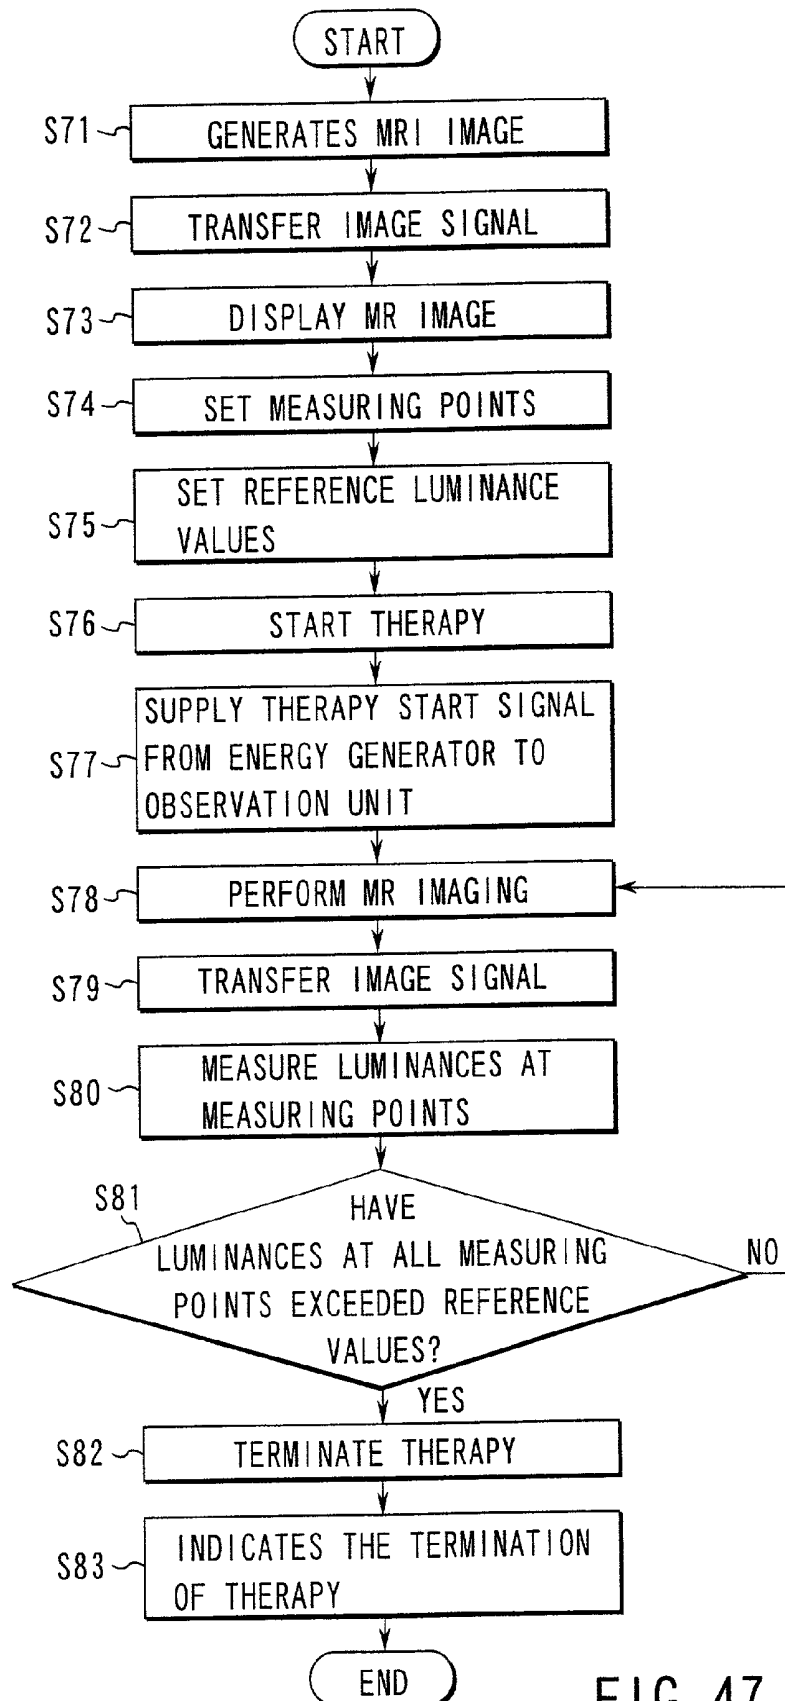


FIG. 47

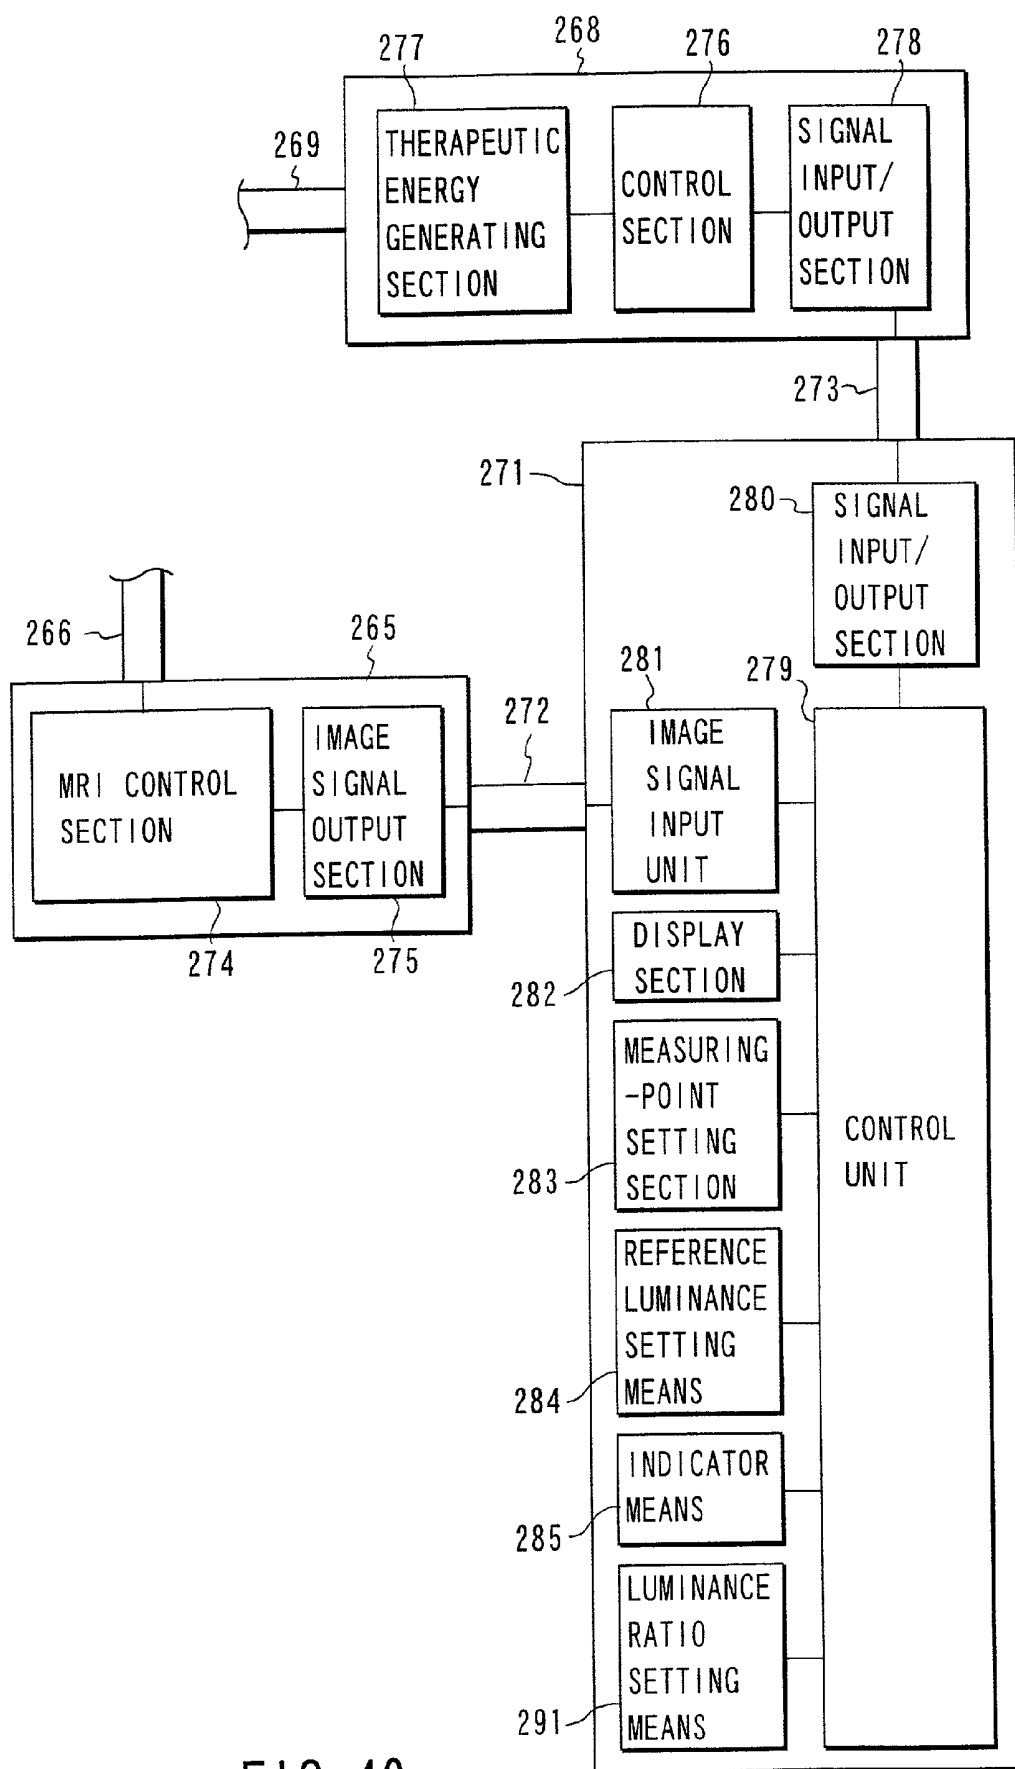


FIG. 49

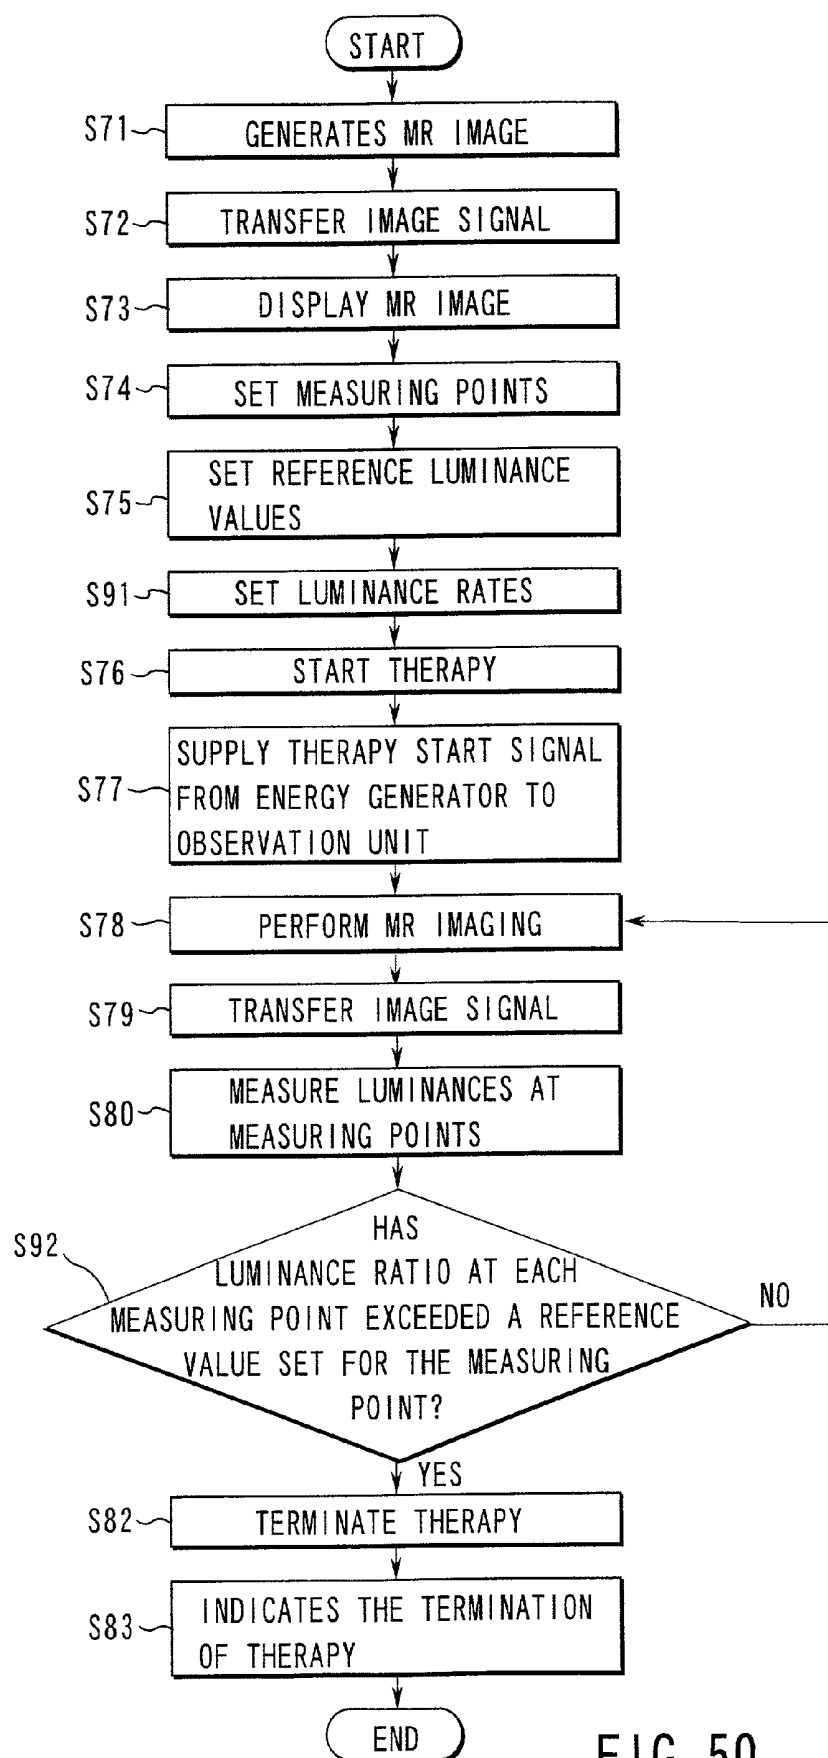


FIG. 50

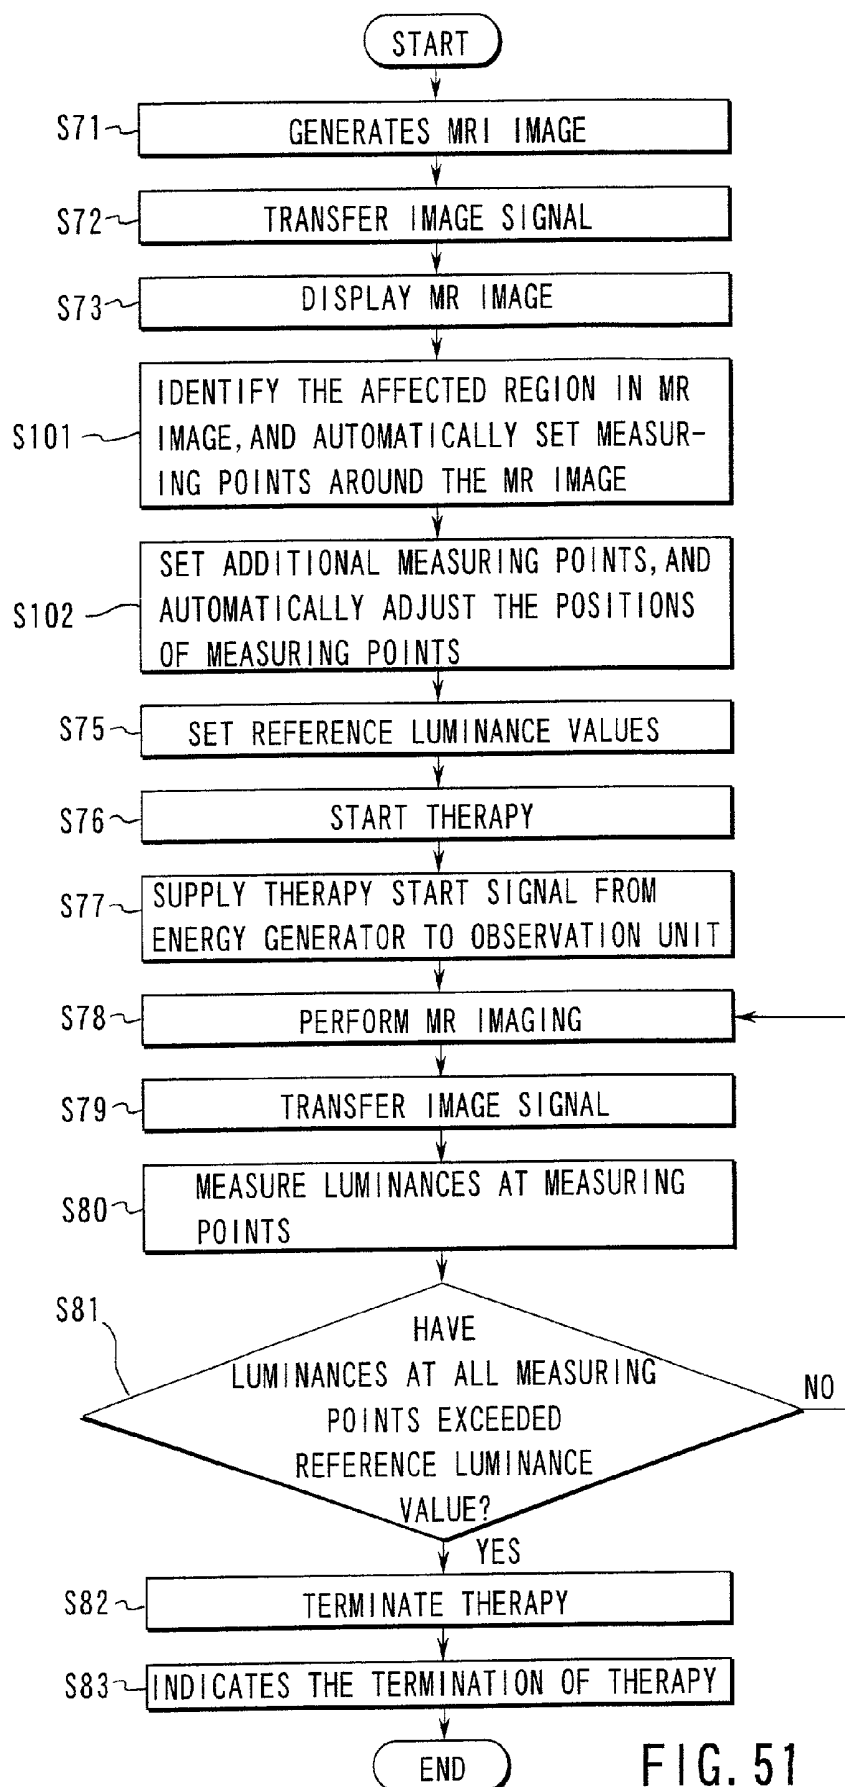


FIG. 51

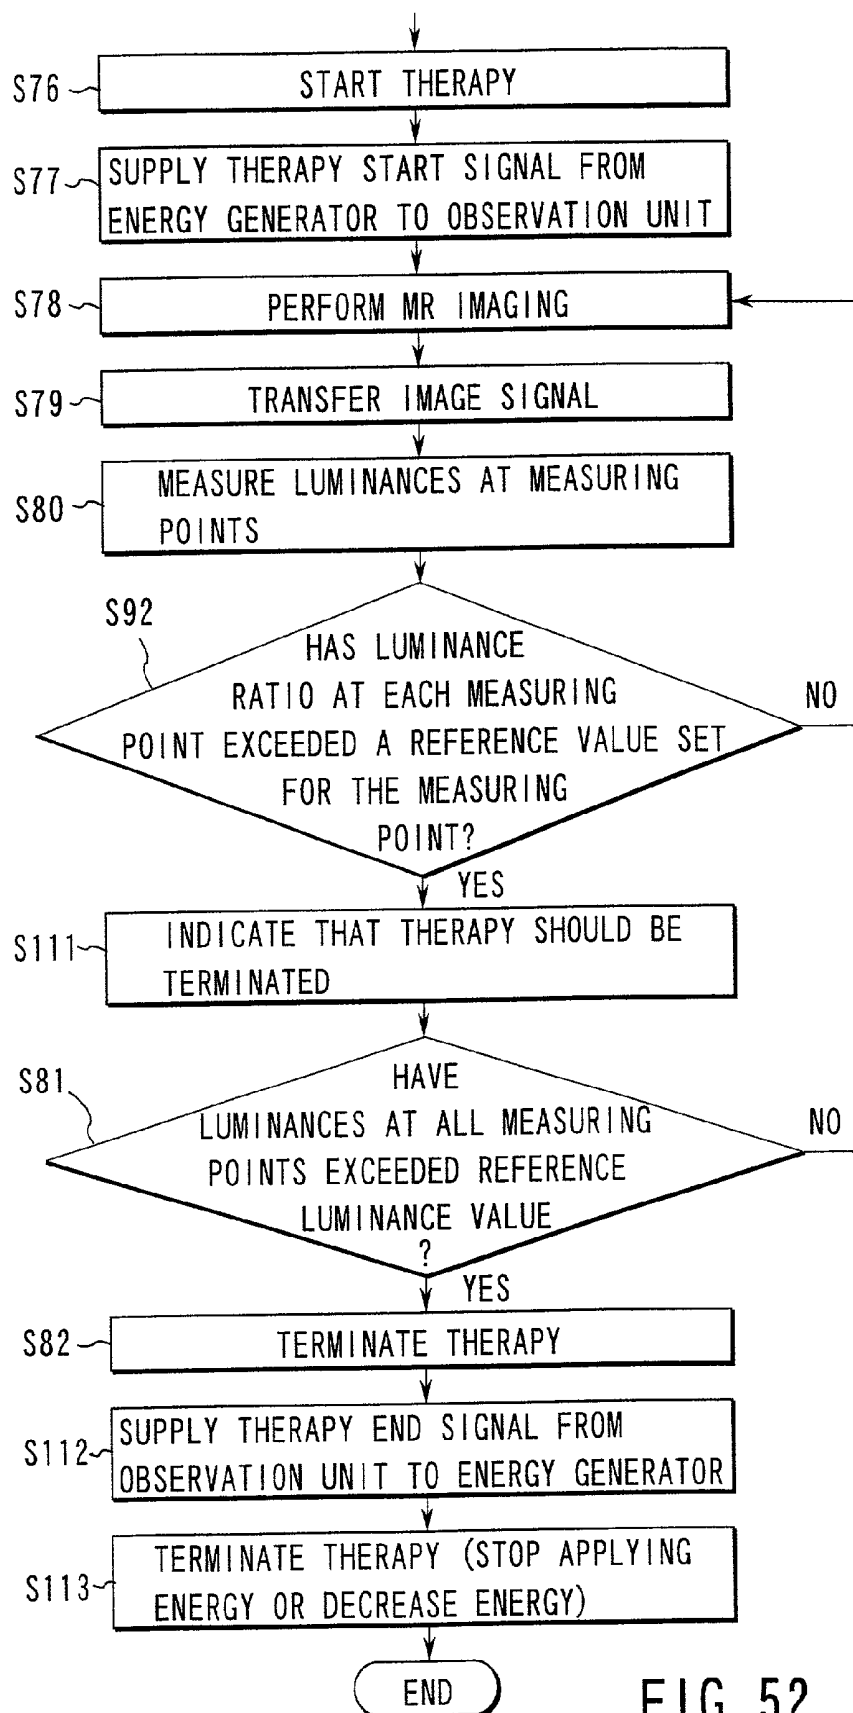


FIG. 52

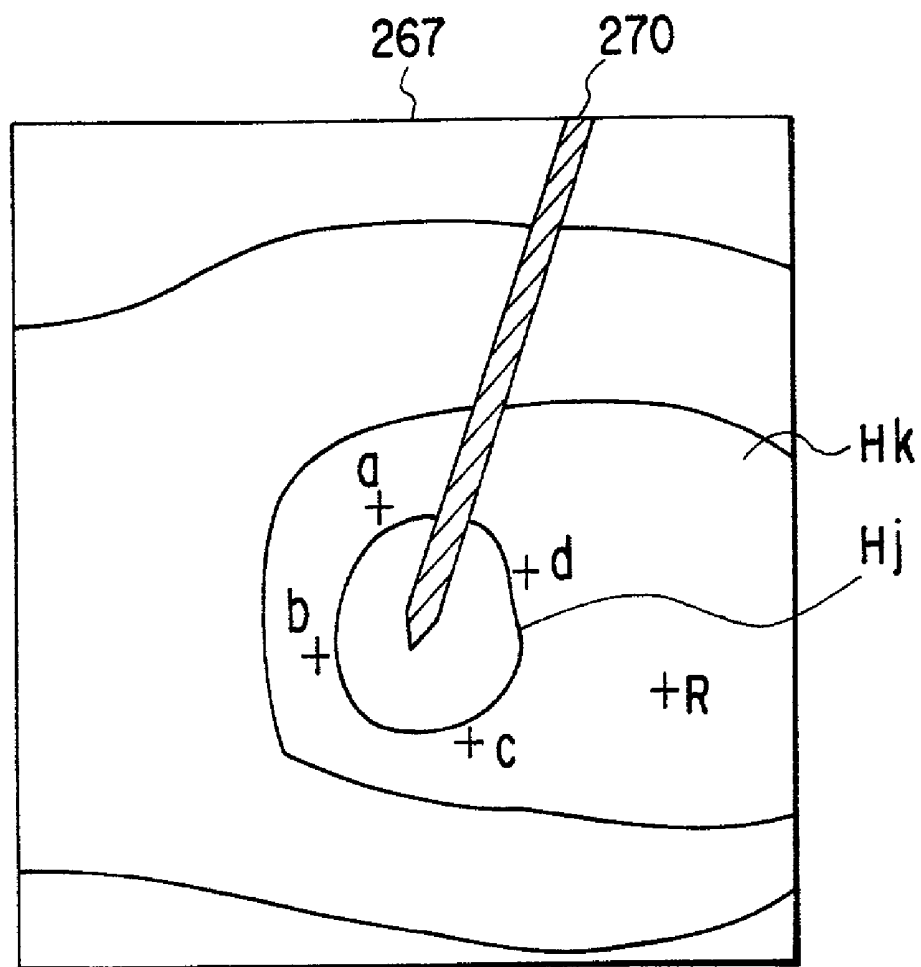
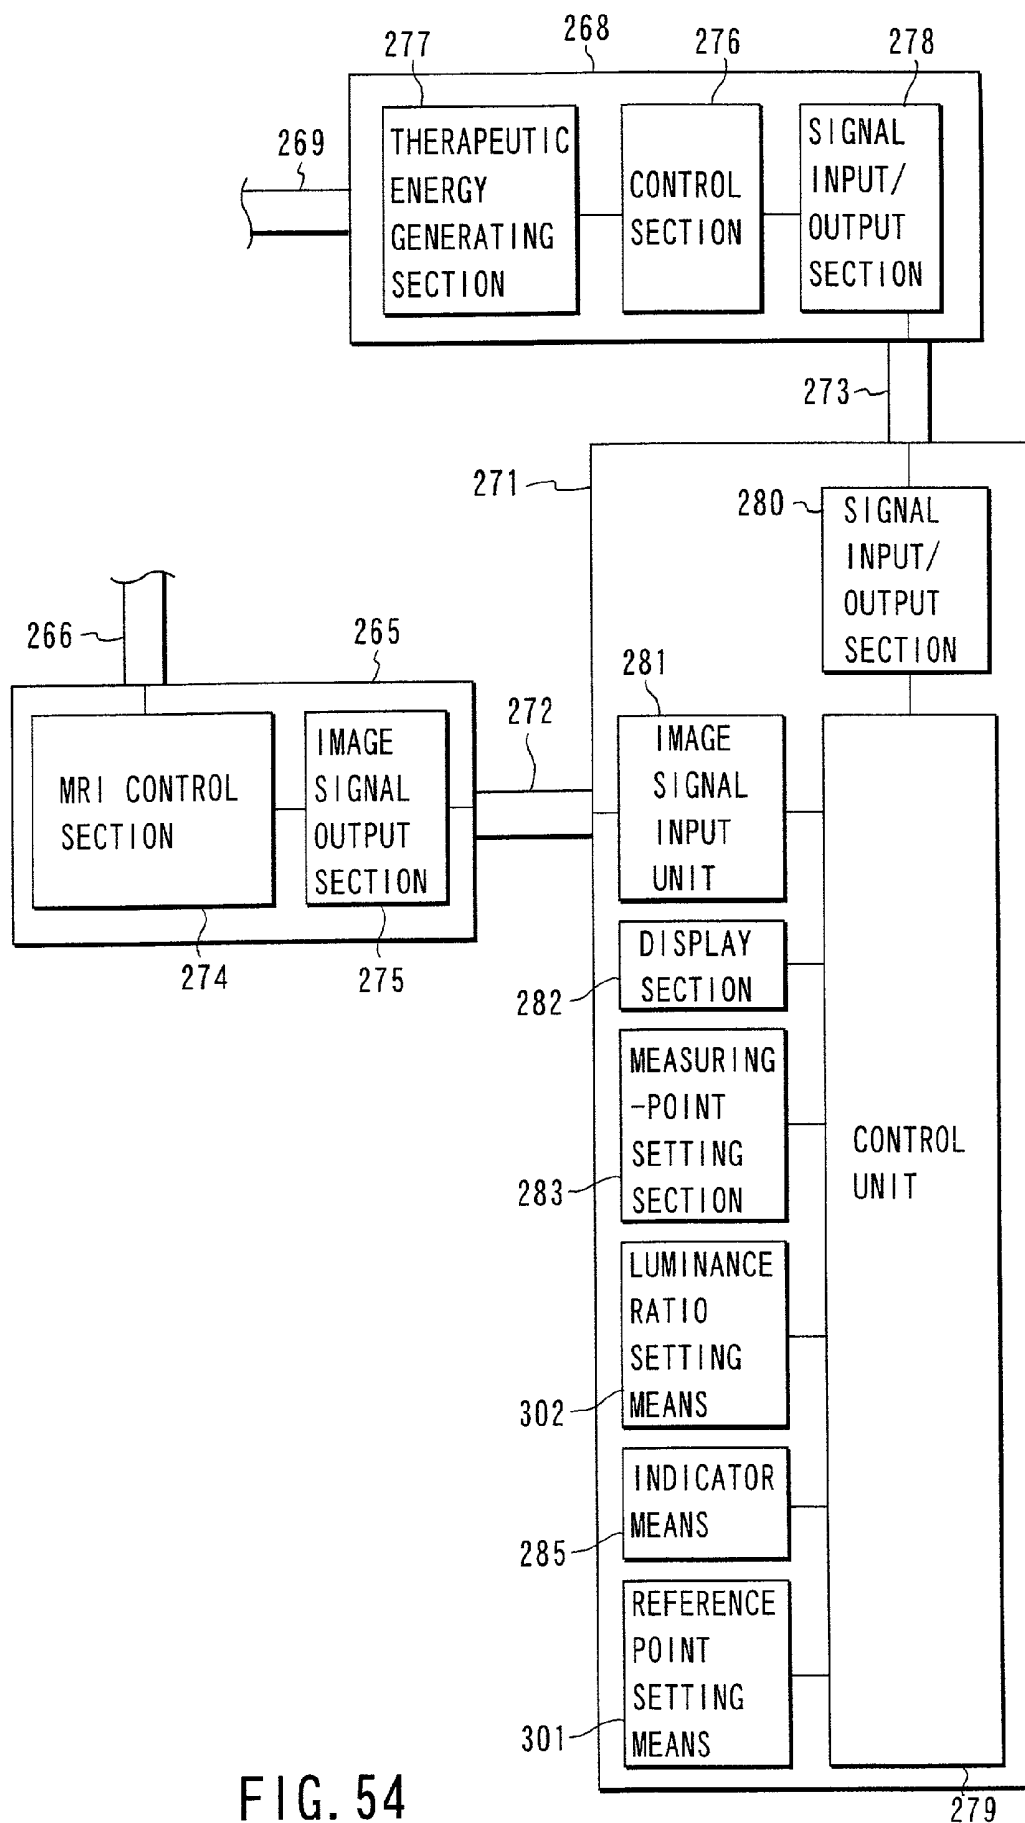


FIG. 53



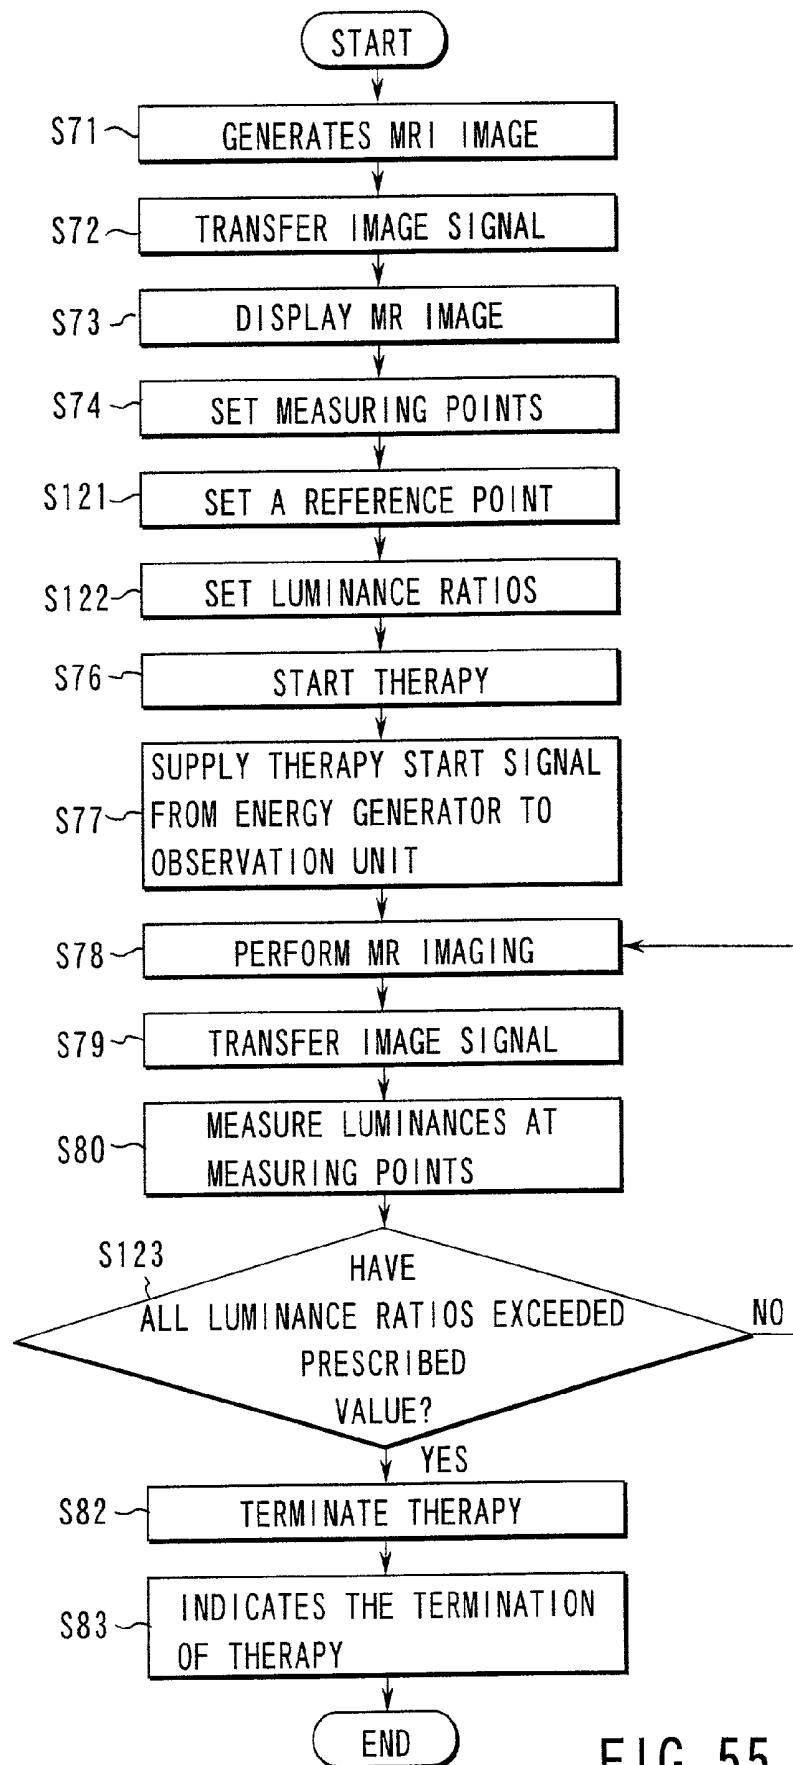


FIG. 55

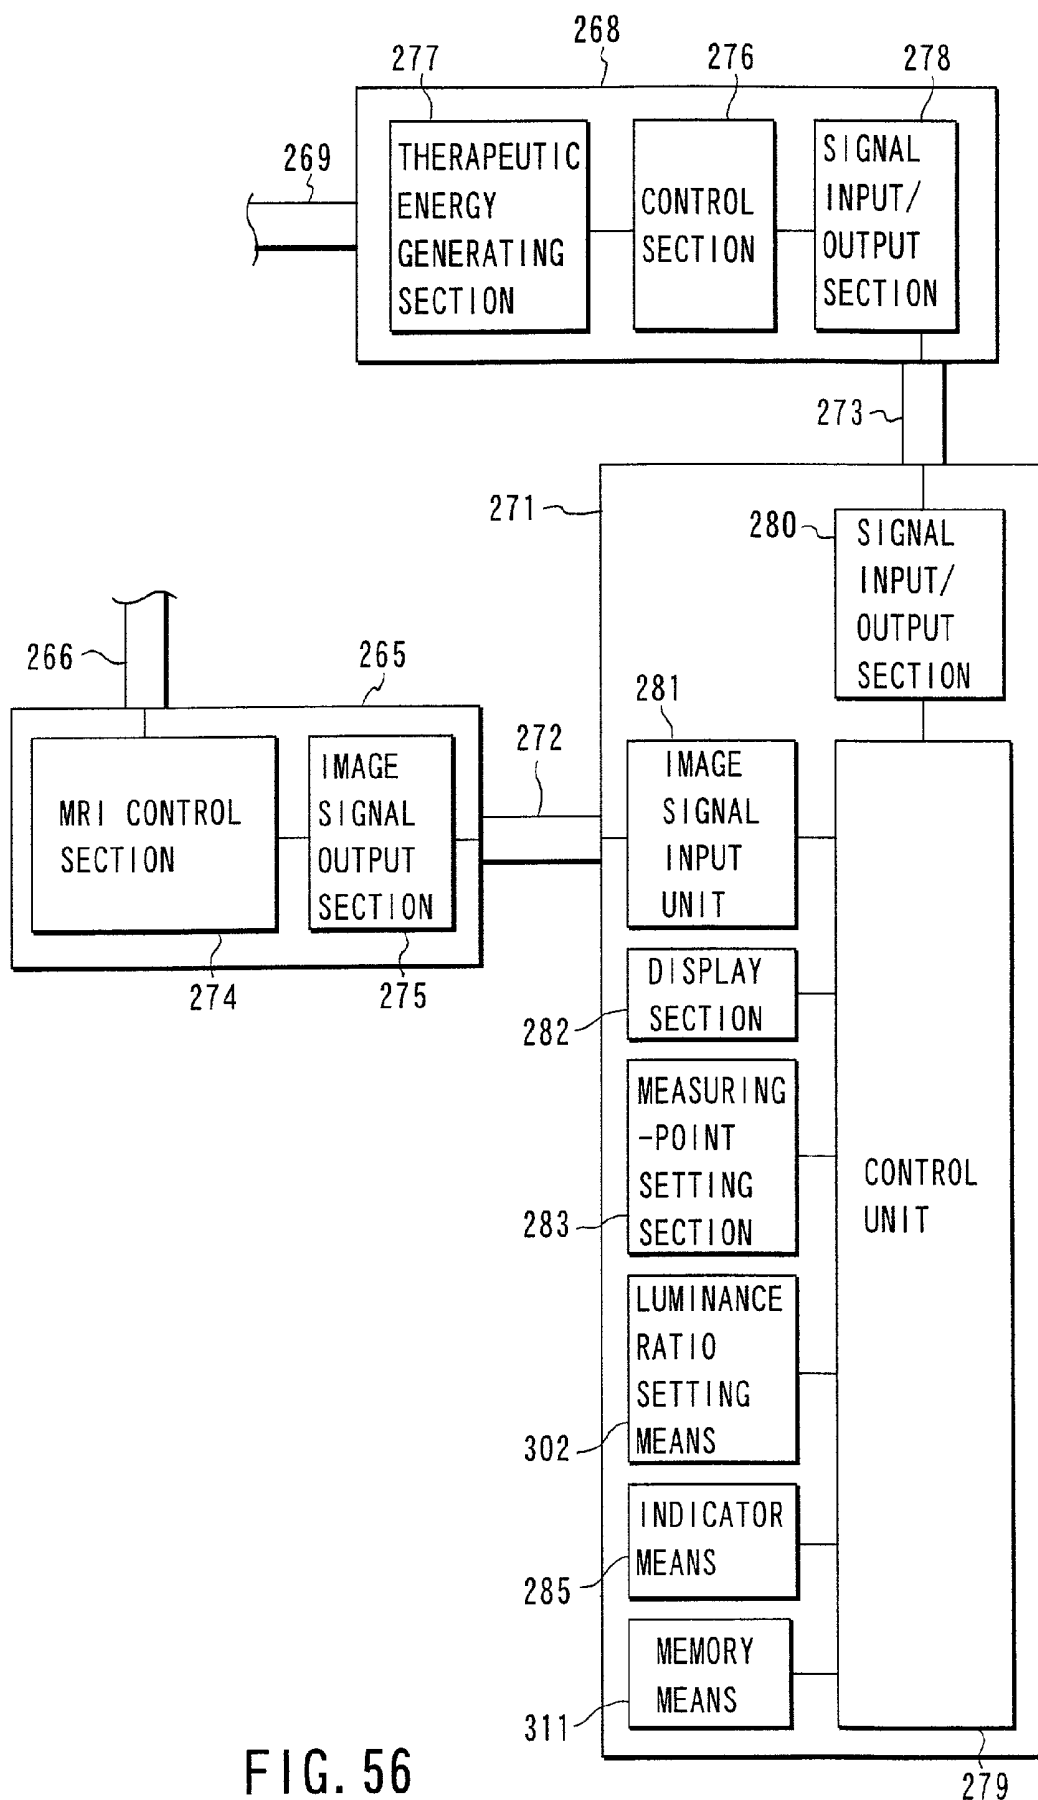


FIG. 56

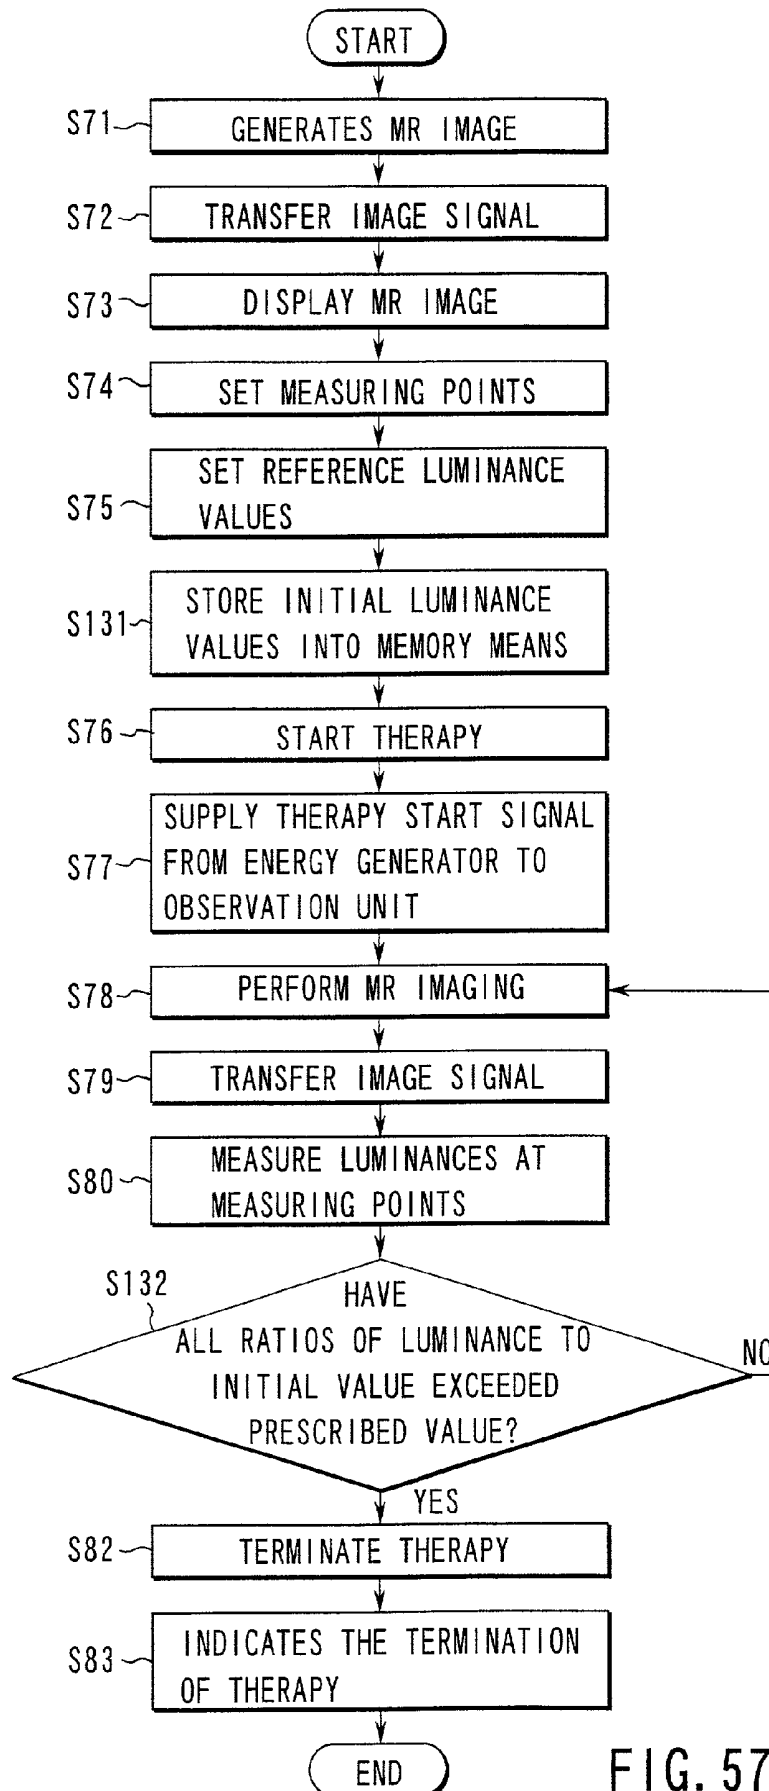


FIG. 57

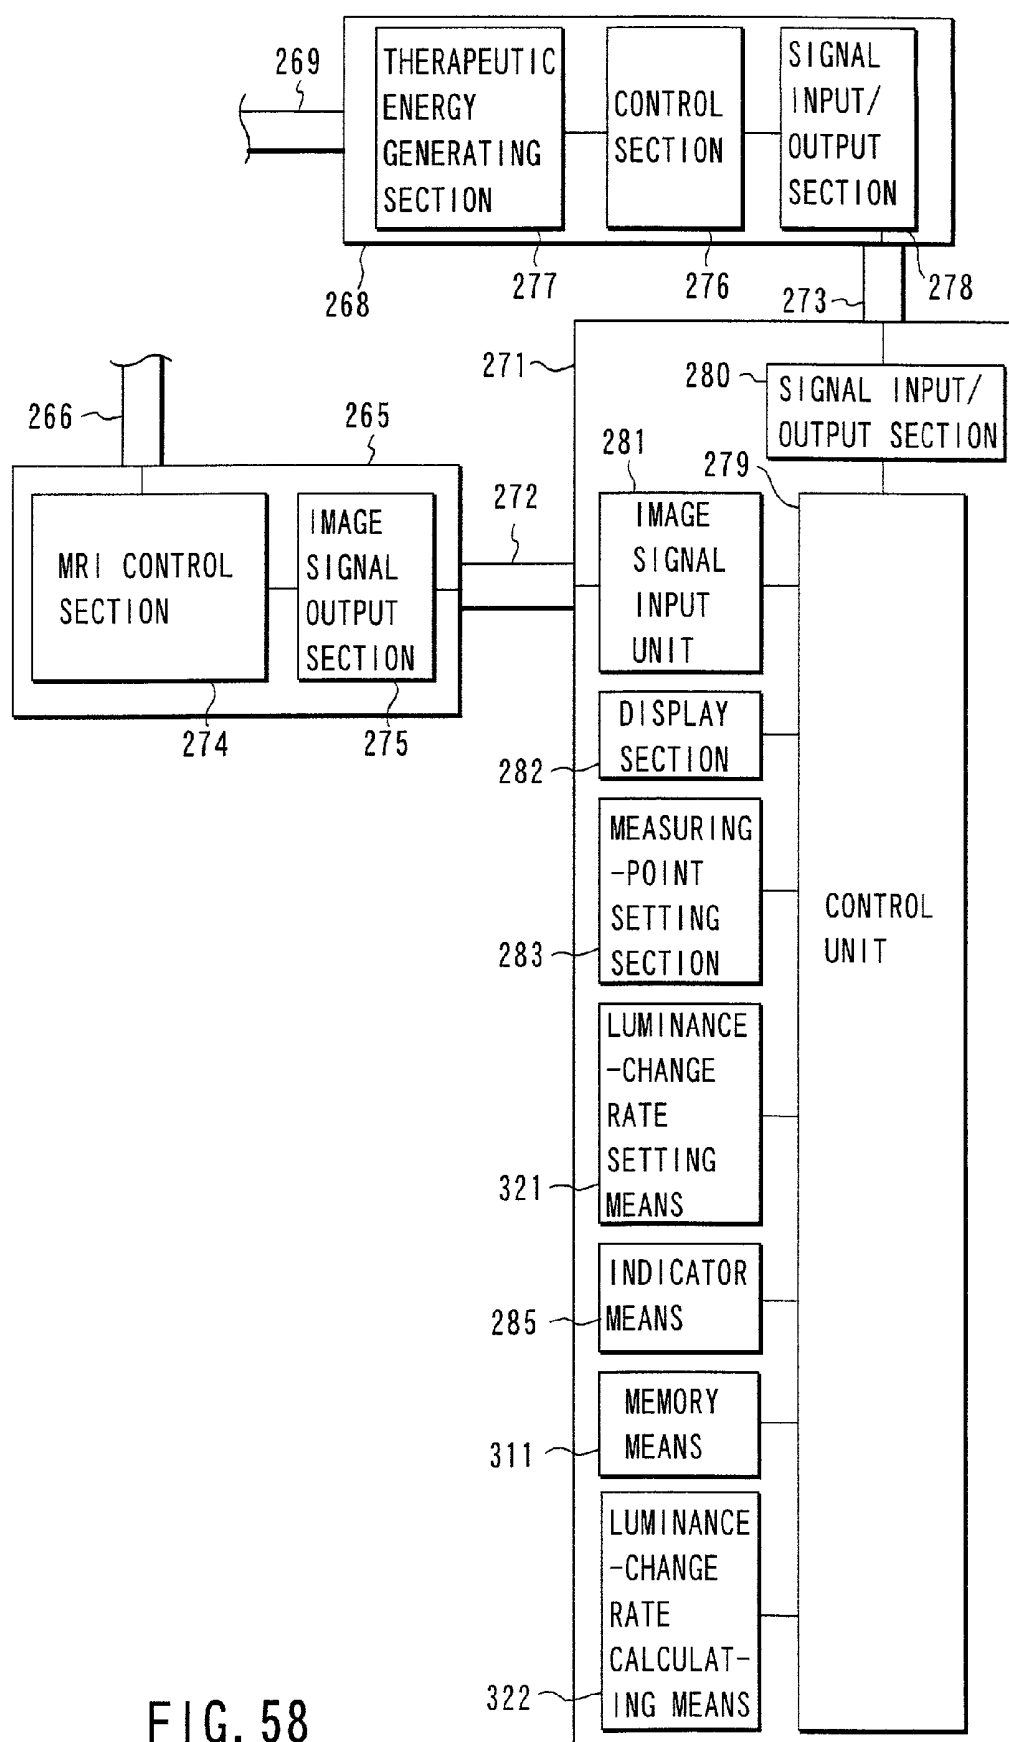


FIG. 58

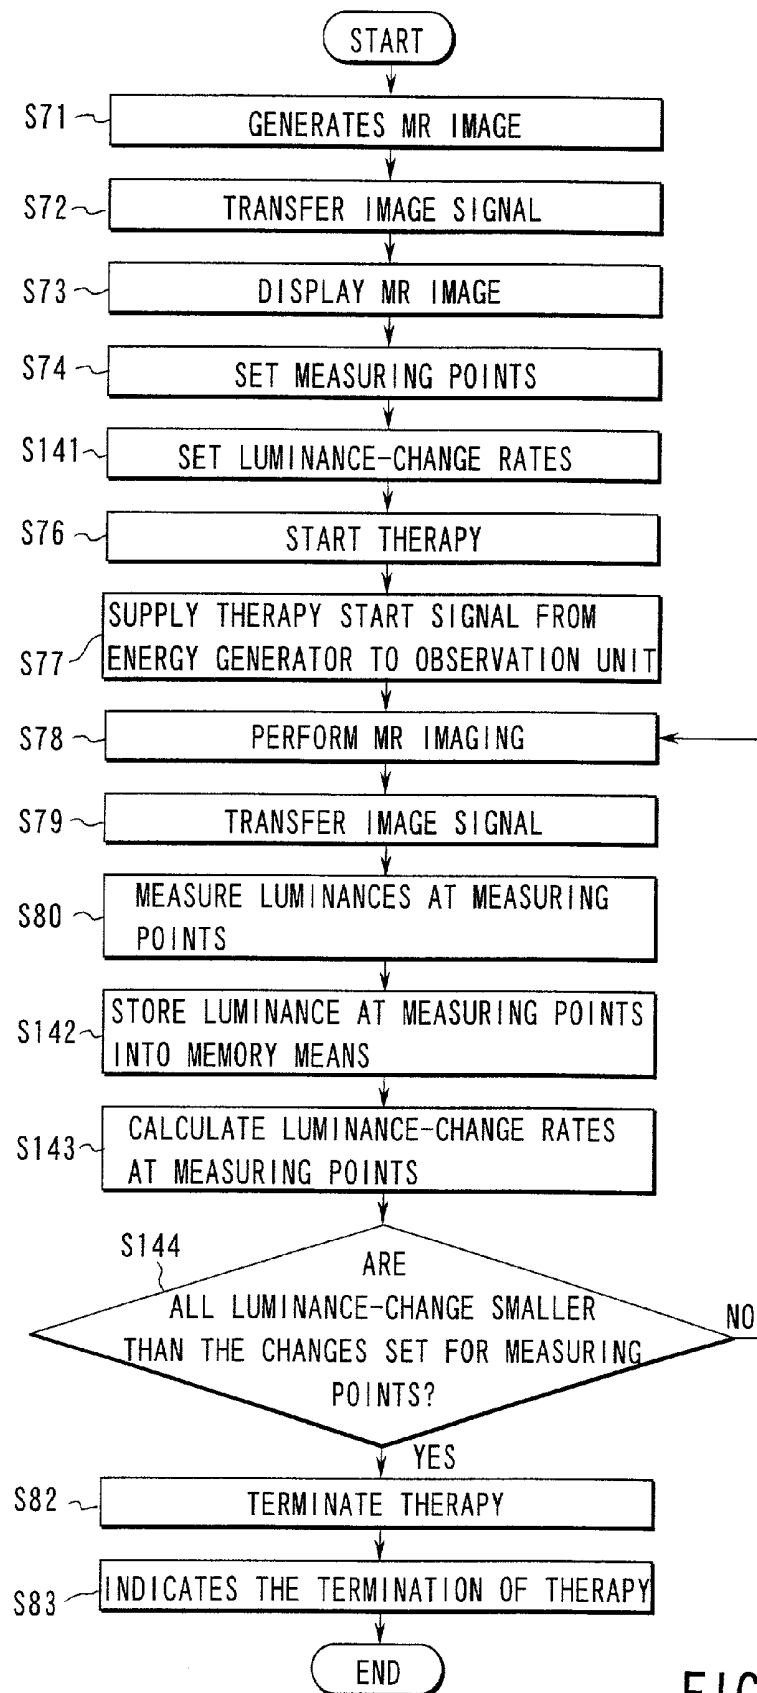


FIG. 59

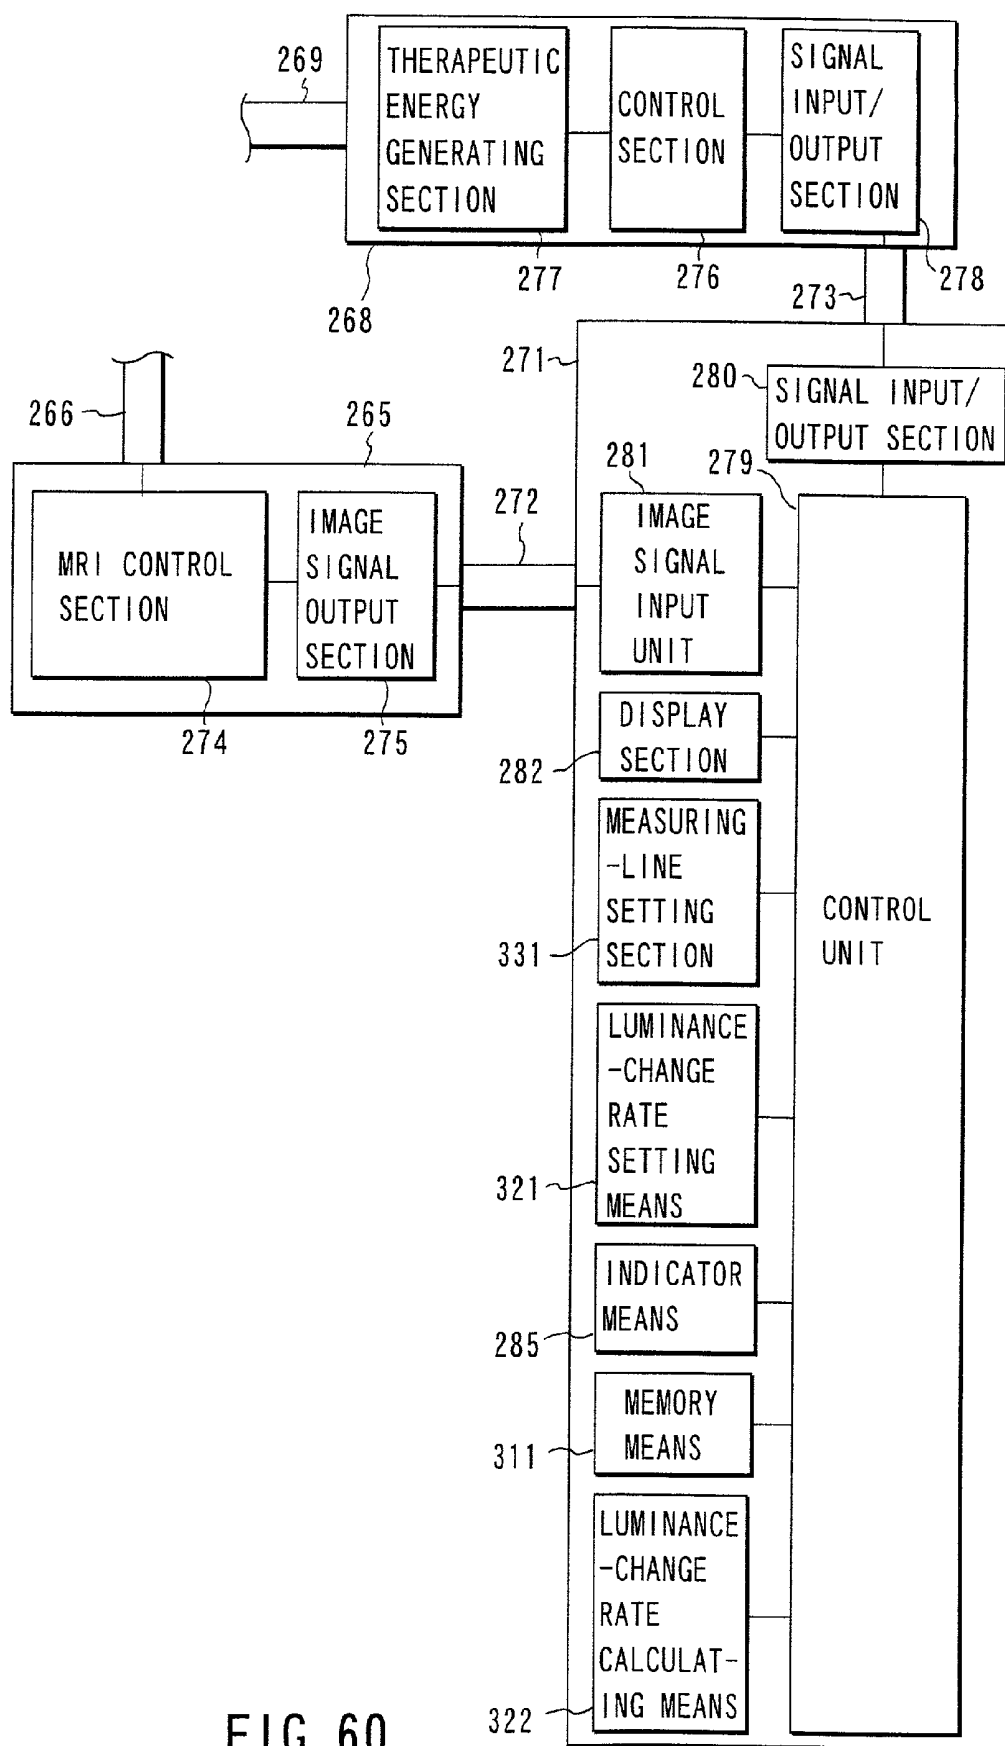


FIG. 60

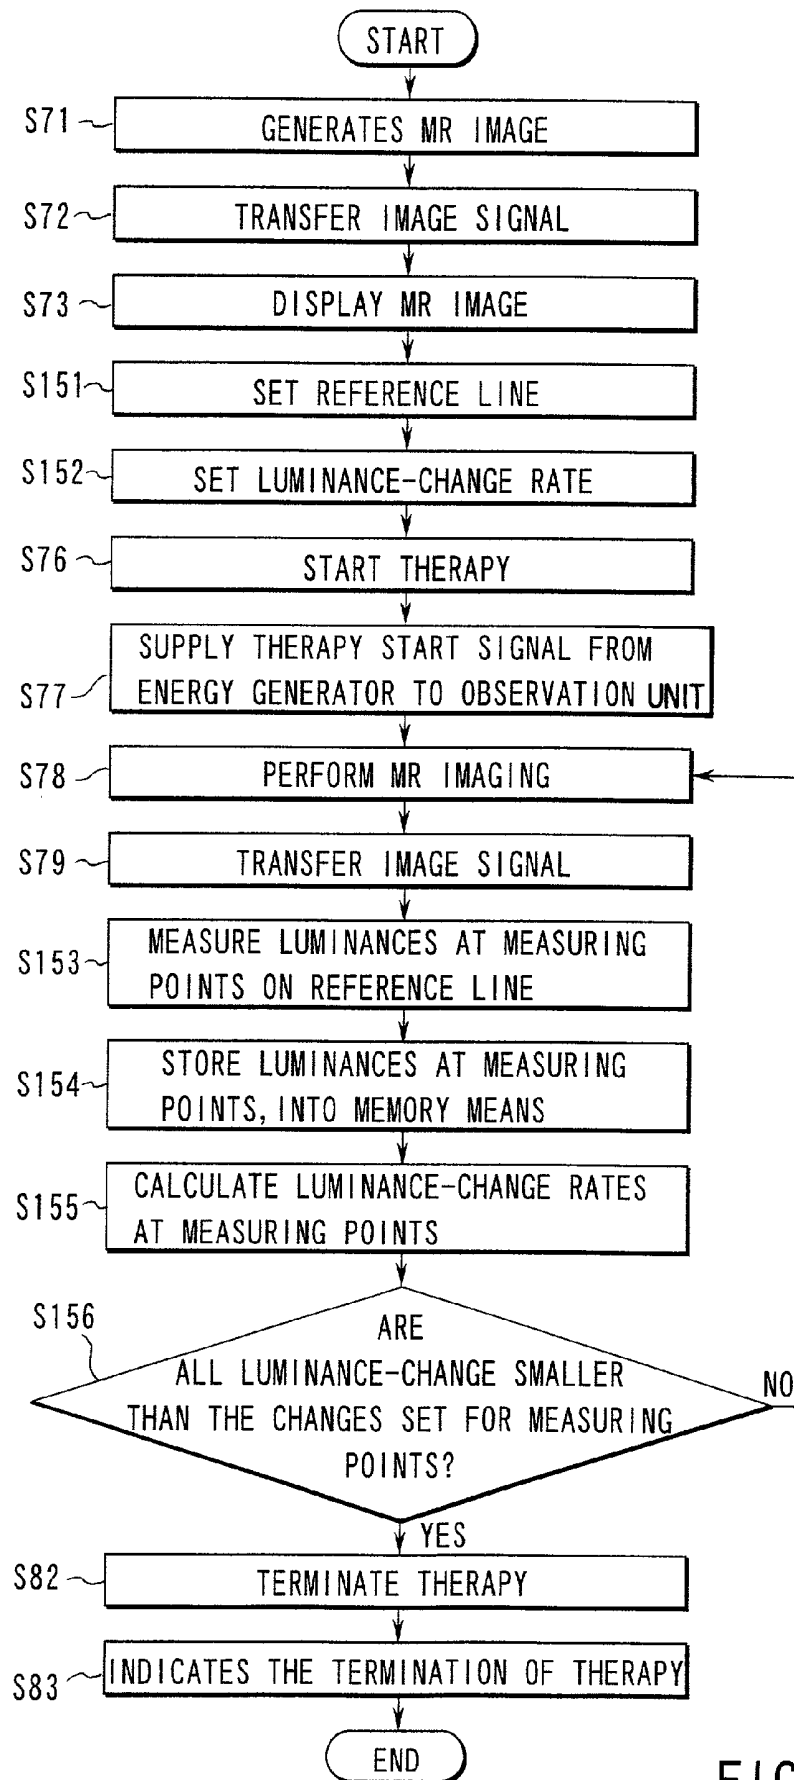
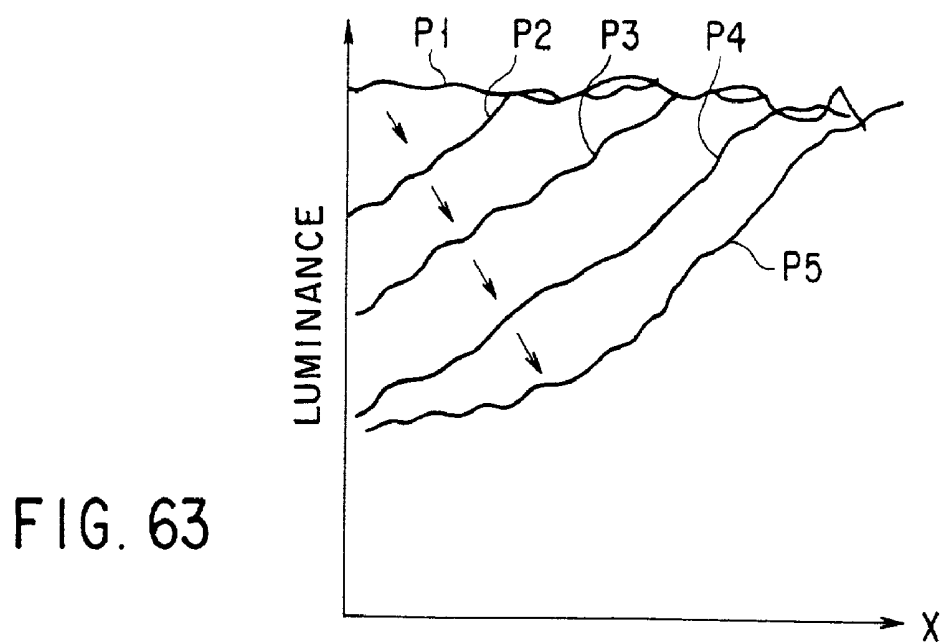
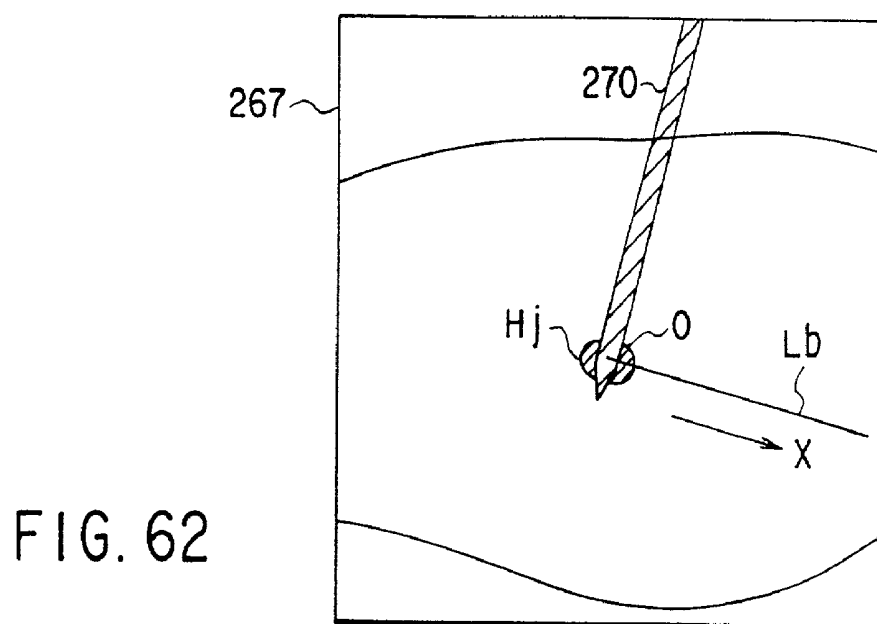


FIG. 61



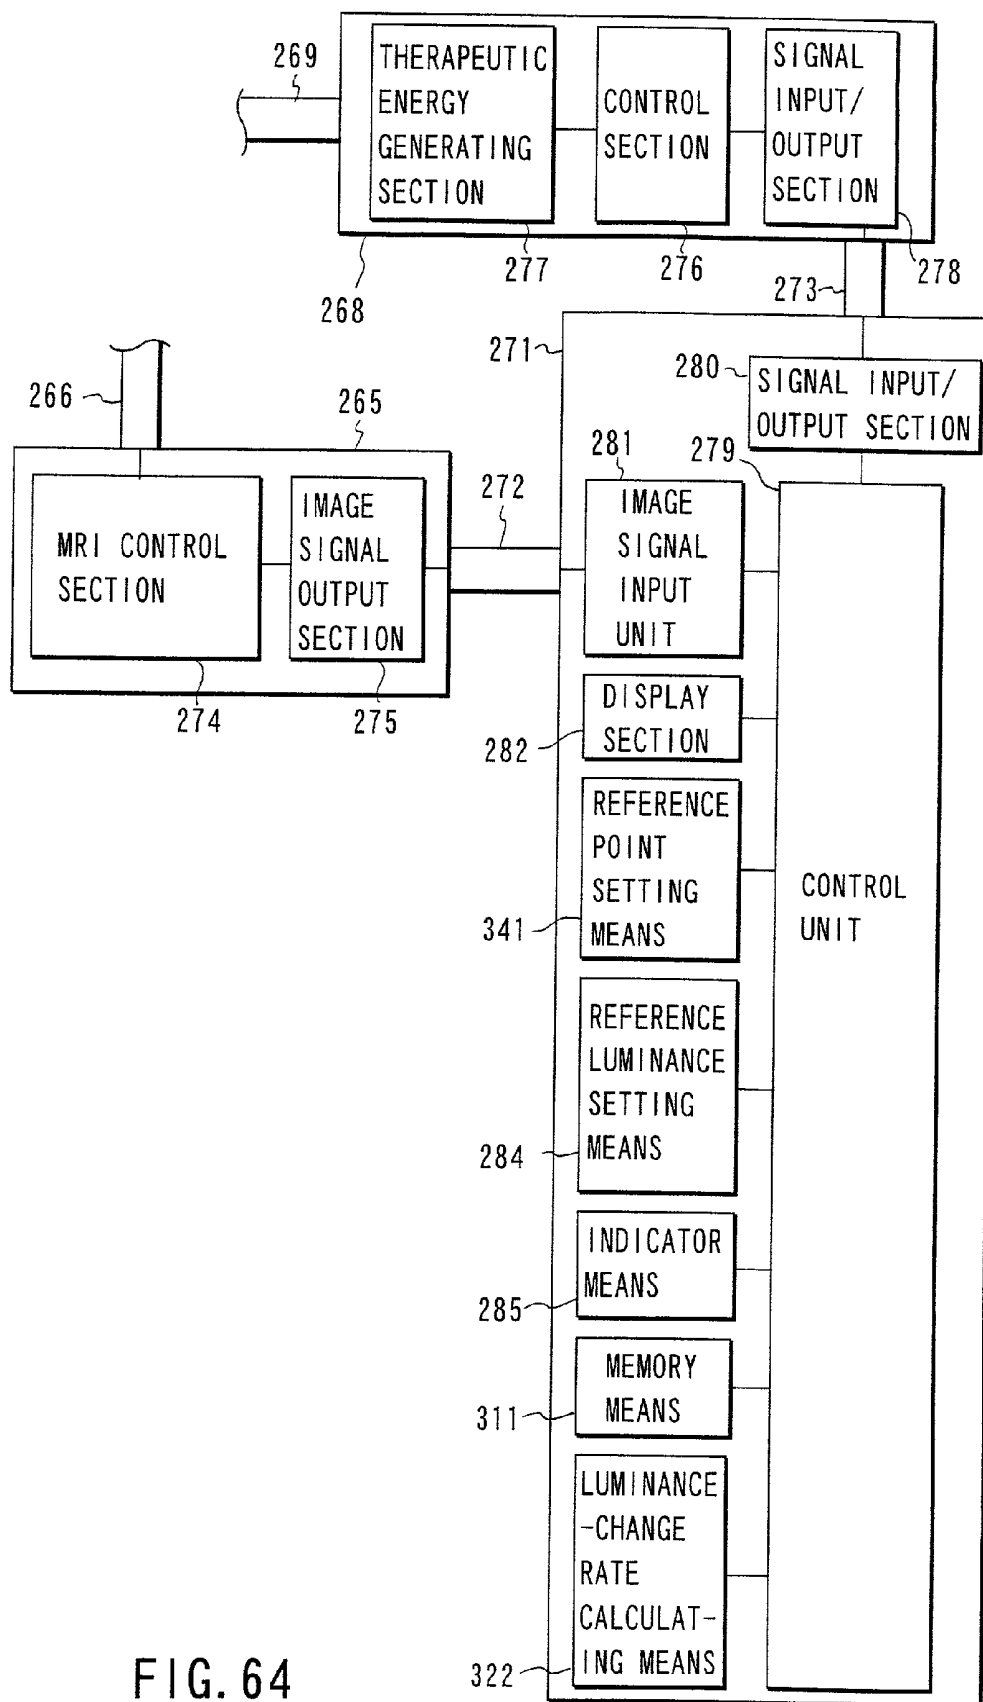


FIG. 64

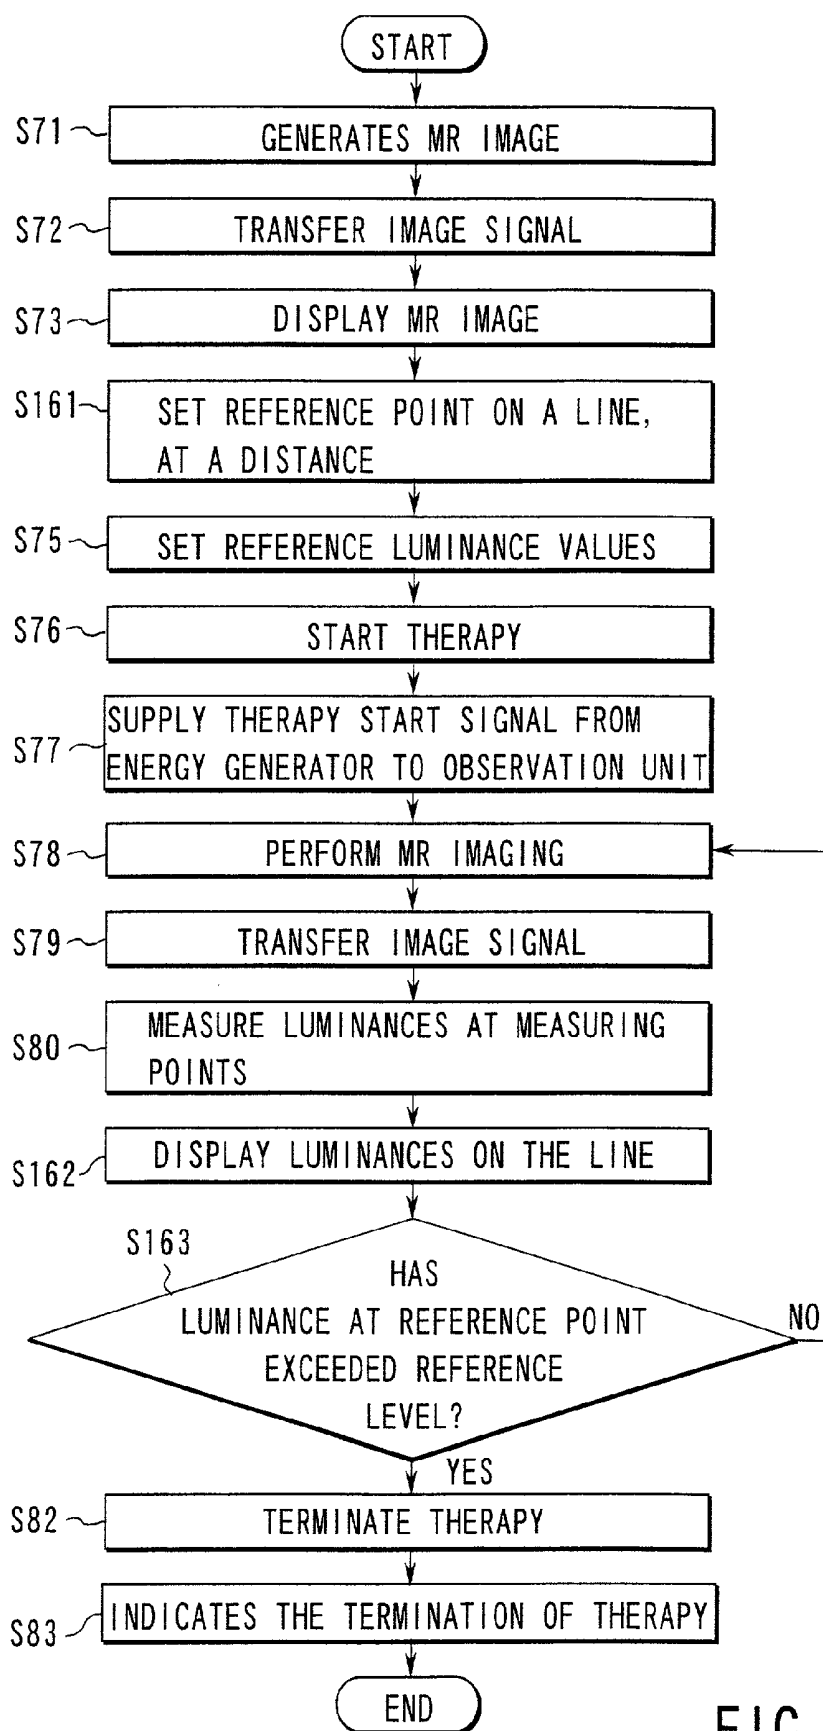


FIG. 65

FIG. 66

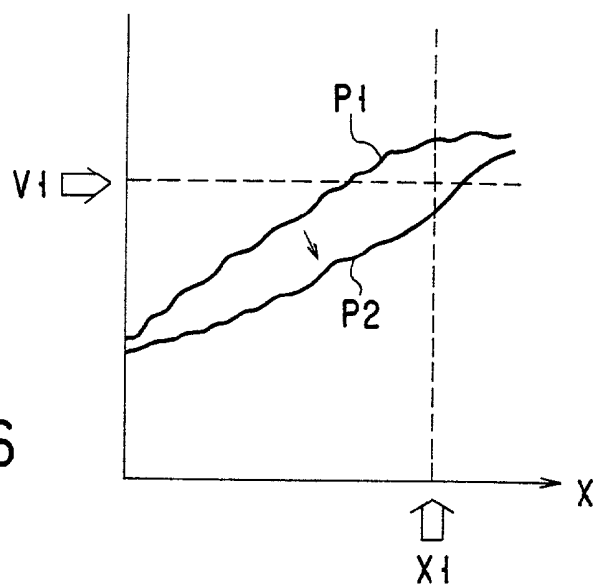
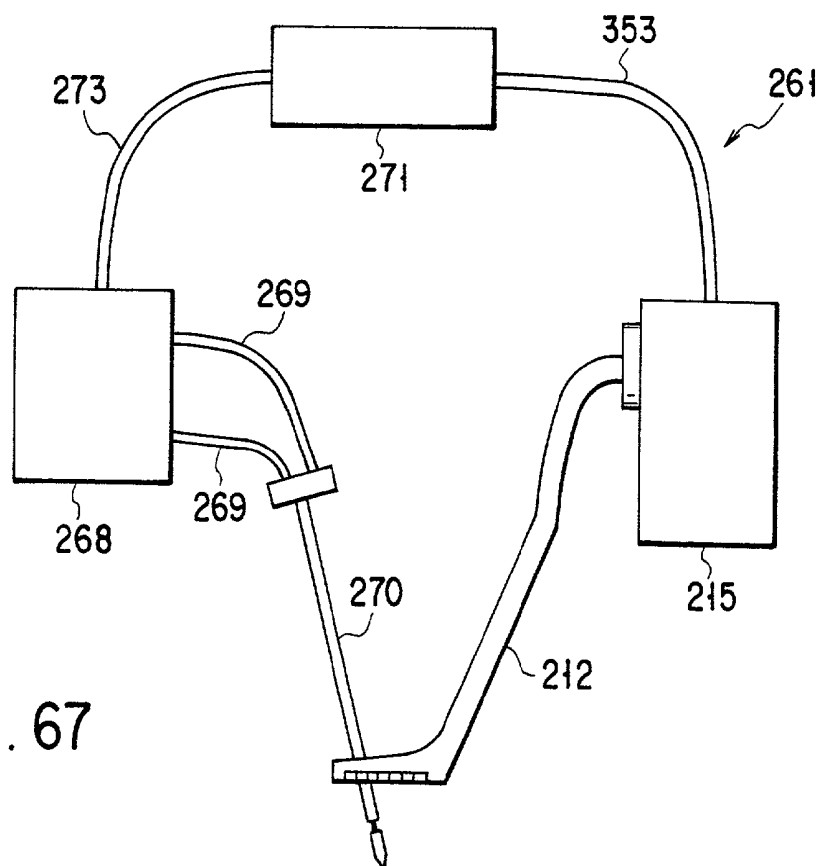


FIG. 67



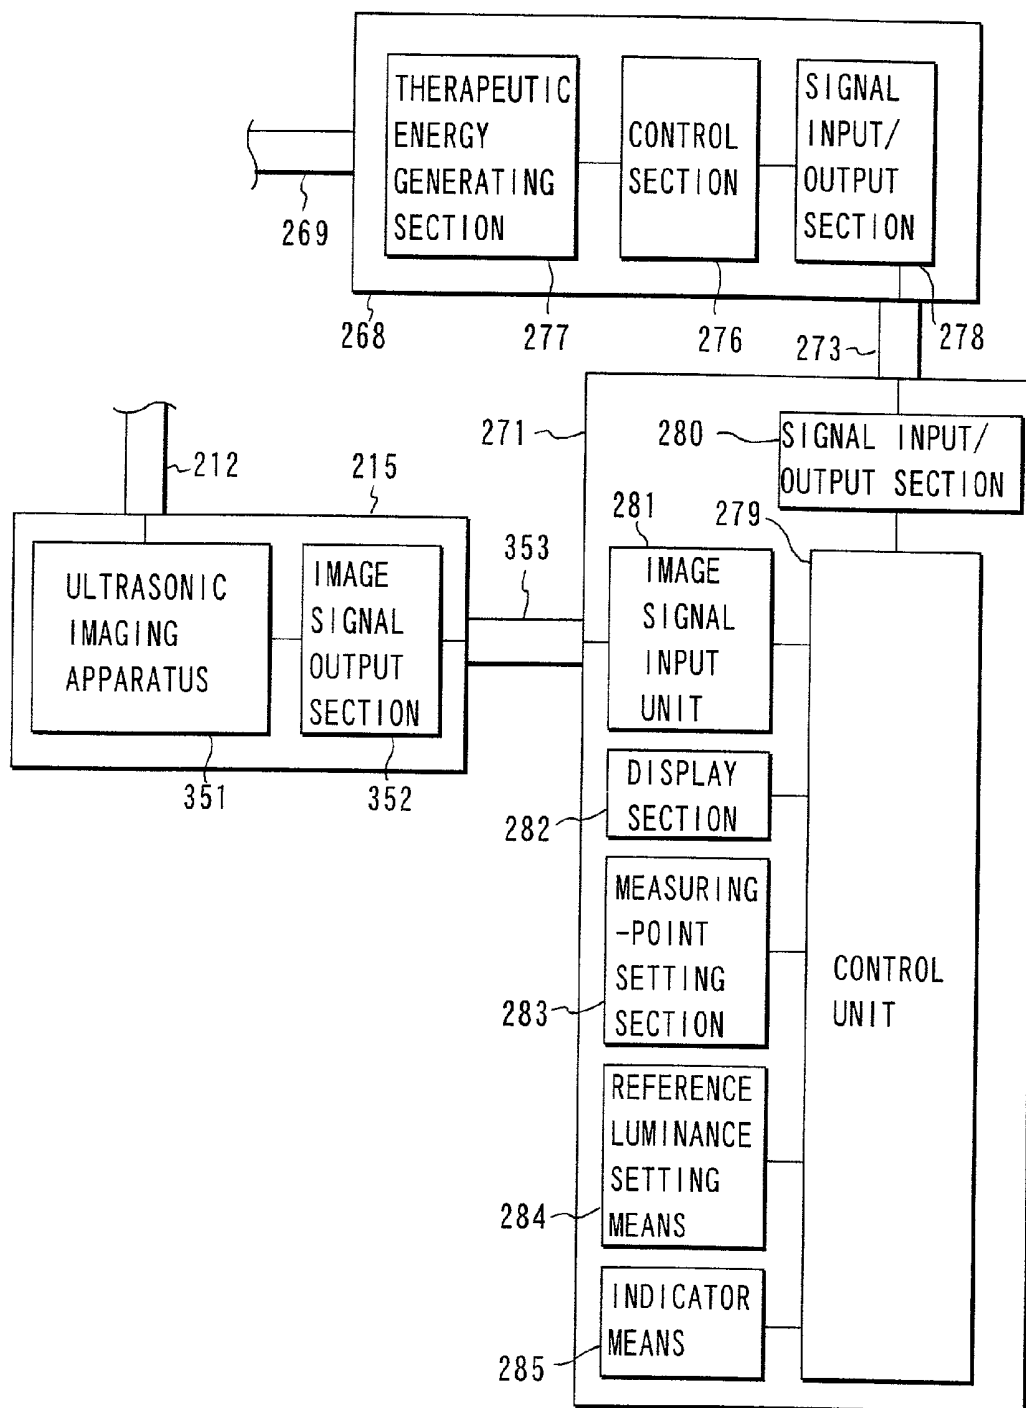


FIG. 68

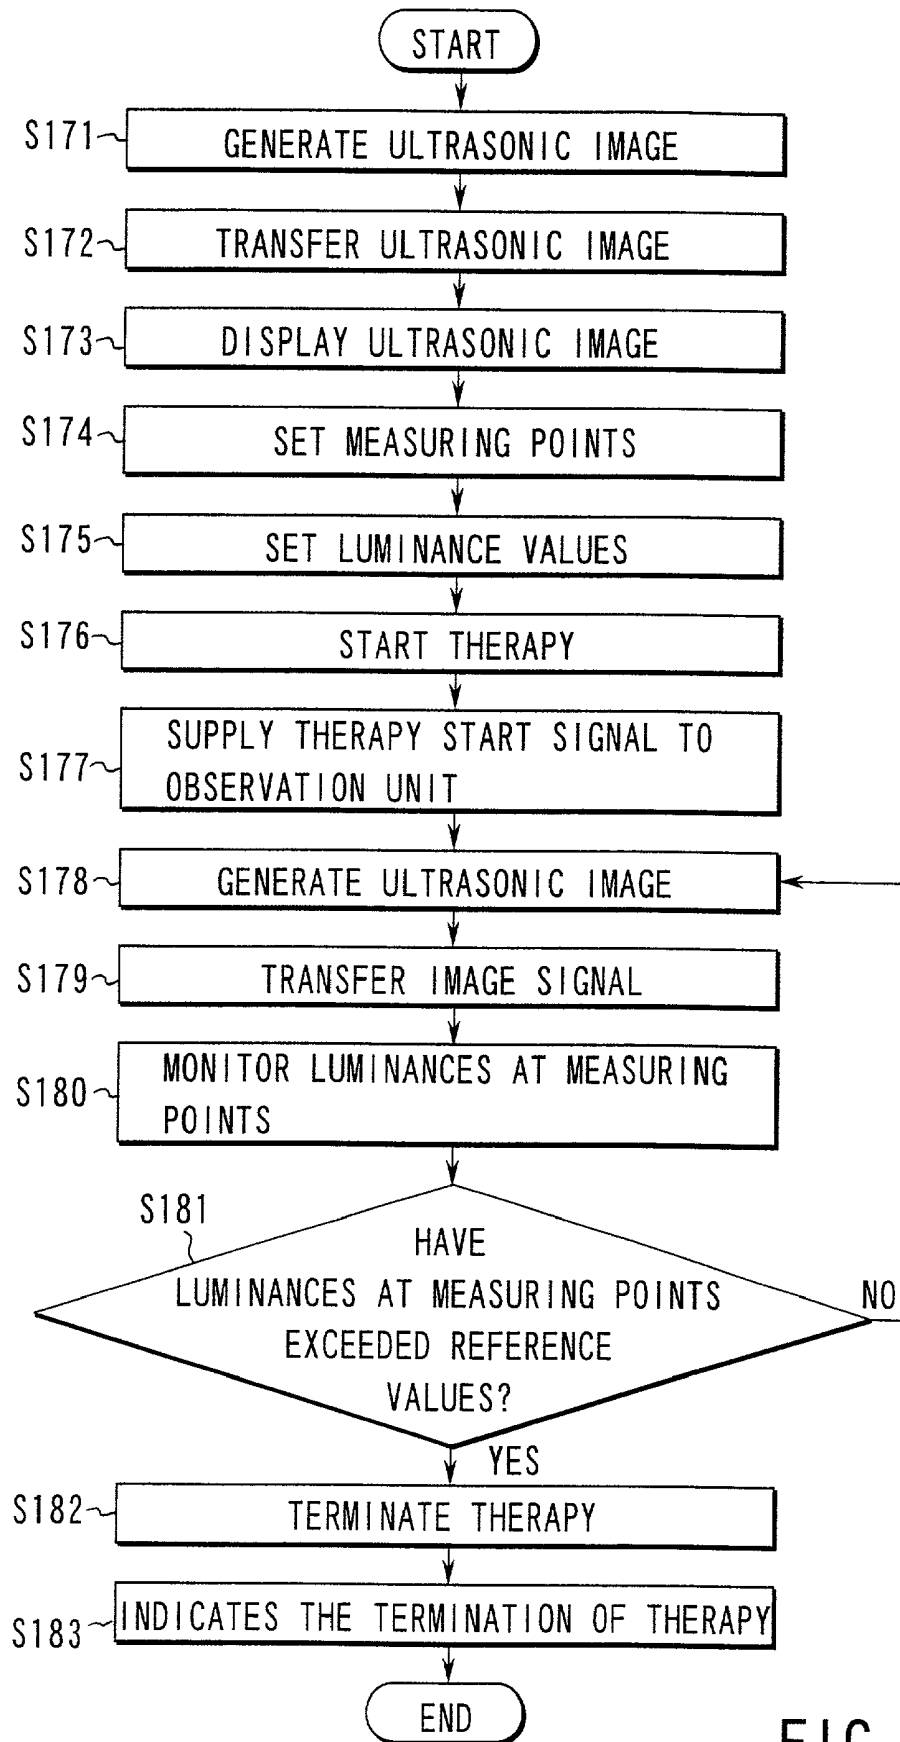


FIG. 69

THERAPEUTIC SYSTEM

BACKGROUND OF THE INVENTION

[0001] The present invention relates to a therapeutic system comprising a medical applicator to be inserted into a living body and an observation means such as an MRI (Magnetic Resonance Imaging) apparatus.

[0002] Generally, a therapeutic system comprises a medical applicator such as a high-frequency instrument and an observation means such as an MRI apparatus. Before the medical applicator is inserted into a patient, the affected tissue within the patient, to which the applicator should be guided, is detected by the observation means. The medical applicator is inserted into the patient and guided to the affected tissue. The applicator is operated, thereby effectively performing high-frequency treatment on the affected tissue.

[0003] In the conventional medical system, the applicator and the observation means are driven independently of each other. To drive the applicator and the observation means at the same time, they must be simultaneously controlled, while being observed. Simultaneous control of the medical applicator and the observation means is troublesome.

[0004] To make matters worse, the noise in the electromagnetic waves emitted from the applicator may distort the image generated by the observation means (e.g., MRI device). The image of the affected tissue may be also distorted to become unclear, while high-frequency waves are applied to the affected tissue.

BRIEF SUMMARY OF THE INVENTION

[0005] The present invention has been made in view of the foregoing. Its object is to provide a therapeutic system in which the medical applicator and the observation means (e.g., MRI apparatus) can be easily operated at the same time and in which the image generated by the observation means remains clear all the time the medical applicator is used.

[0006] To achieve the object, a therapeutic system according to the invention comprises: a therapeutic applicator adapted to be inserted into a body cavity, for applying therapeutic energy to treat living tissues present in the body cavity; observation means for indicating a position which the therapeutic applicator takes in the body cavity; and control means for controlling the therapeutic energy applied from the therapeutic applicator to the living tissues, on the basis of data representing the position which the therapeutic applicator takes in the body cavity.

[0007] During the therapy, the observation means indicates the position the therapeutic applicator takes in the body cavity. The control means controls the therapeutic energy applied from the applicator to the living tissues, in accordance with the data representing the position of the applicator.

[0008] Hence, it is easy to operate the system even if the applicator and the observation unit (e.g., an MRI apparatus) are used at the same time. The image of the living tissues remains clear during the use of the therapeutic applicator.

[0009] Additional objects and advantages of the invention will be set forth in the description which follows, and in part will be obvious from the description, or may be learned by

practice of the invention. The objects and advantages of the invention may be realized and obtained by means of the instrumentalities and combinations particularly pointed out hereinafter.

BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWING

[0010] The accompanying drawings, which are incorporated in and constitute a part of the specification, illustrate presently preferred embodiments of the invention, and together with the general description given above and the detailed description of the preferred embodiments given below, serve to explain the principles of the invention.

[0011] FIG. 1 is a schematic representation of a therapeutic system, which is the first embodiment of the present invention;

[0012] FIG. 2A is a partially sectional view of a patient, illustrating how the medical apparatus is used to perform treatment on the patient;

[0013] FIG. 2B is a longitudinal sectional view of the microwave applicator incorporated in the first embodiment of the invention;

[0014] FIG. 3 is a diagrammatic view showing the connection of the control unit to some other components of the first embodiment;

[0015] FIG. 4 is a block diagram of the control section incorporated in the first embodiment;

[0016] FIG. 5 is a flow chart explaining the operation of the first embodiment of the invention;

[0017] FIG. 6 is a longitudinal sectional view of the patient, showing the applicator of the first embodiment, which is inserted into the peritoneal cavity of the patient;

[0018] FIG. 7 is a longitudinal sectional view of the patient, showing an MR image of the region of the affected tissue, which is being coagulated by the microwave applicator of the first embodiment;

[0019] FIG. 8 is a diagram illustrating the range of magnetic susceptibility for the main body of the microwave applicator, and also the range of magnetic susceptibility for the MR marker formed in the main body;

[0020] FIG. 9 is a longitudinal sectional view of the distal portion of the microwave applicator provided in a therapeutic system, which is the second embodiment of the present invention;

[0021] FIG. 10 is a longitudinal sectional view of the patient, showing the applicator of the second embodiment, which is inserted into the peritoneal cavity of the patient;

[0022] FIG. 11 is a longitudinal sectional view of the patient, showing an MR image of the region of the affected tissue, which is being coagulated by the microwave applicator of the second embodiment;

[0023] FIG. 12 is a longitudinal sectional view of the distal portion of the microwave applicator provided in a therapeutic system, which is the third embodiment of the present invention;

[0024] **FIG. 13** is a longitudinal sectional view of the microwave applicator incorporated in a therapeutic system, which is the fourth embodiment of this invention;

[0025] **FIG. 14** is a perspective view showing the insertion section of an endoscope and a applicator incorporated in a therapeutic system according to the a fifth embodiment of the invention;

[0026] **FIG. 15** is a perspective view of the applicator incorporated in the fifth embodiment;

[0027] **FIG. 16** is a longitudinal sectional view of the applicator provided in a therapeutic system according to the sixth embodiment of the invention;

[0028] **FIG. 17** is a longitudinal sectional view of the applicator incorporated in a therapeutic system according to the seventh embodiment of the invention;

[0029] **FIG. 18** is a diagrammatic view showing the connection of the control unit to some other components of a therapeutic system according to the eighth embodiment of the present invention;

[0030] **FIG. 19** is a block diagram of the control section incorporated in the eighth embodiment;

[0031] **FIG. 20** is a flow chart explaining the operation of the eighth embodiment of the invention;

[0032] **FIG. 21** is a schematic representation of a therapeutic system, which is the ninth embodiment of the present invention;

[0033] **FIG. 22** is a flow chart explaining the operation of the ninth embodiment shown in **FIG. 21**;

[0034] **FIG. 23** is a block diagram schematically showing a therapeutic system, which is the tenth embodiment of the invention;

[0035] **FIG. 24** is a block diagram depicting the connection of the control unit to some other components of the tenth embodiment;

[0036] **FIG. 25** is a schematic representation of a therapeutic system according to the eleventh embodiment of the present invention;

[0037] **FIG. 26** is a block diagram illustrating the connection of the control unit to some other components of the eleventh embodiment;

[0038] **FIG. 27** is a schematic representation of a therapeutic system according to the twelfth embodiment of the this invention;

[0039] **FIG. 28** is a block diagram illustrating the connection of the control unit to some other components of the twelfth embodiment;

[0040] **FIG. 29** is a flow chart explaining the operation of the twelfth embodiment shown in **FIG. 27**;

[0041] **FIG. 30** is a block diagram schematically showing a therapeutic system according to the thirteenth embodiment of the invention;

[0042] **FIG. 31** is a perspective view of a therapeutic system, which is the fourteenth embodiment of the present invention;

[0043] **FIG. 32** is a graph representing the operating characteristic of the coaxial filter used in the fourteenth embodiment;

[0044] **FIG. 33** is a diagram showing an MR tomogram generated in the fourteenth embodiment;

[0045] **FIG. 34A** is a graph illustrating the operation characteristic of the coaxial filter used in a therapeutic system according to the fifteenth embodiment of the invention;

[0046] **FIG. 34B** is a graph representing the operation characteristic of the coaxial filter used in a therapeutic system according to the sixteenth embodiment of this invention;

[0047] **FIG. 35** is a perspective view of a therapeutic system, which is the seventeenth embodiment of the present invention;

[0048] **FIG. 36** is a graph representing the operation characteristic of the filter used in a therapeutic system according to the seventeenth embodiment of this invention;

[0049] **FIG. 37A** is a graph depicting the operation characteristic of the filter used in a therapeutic system according to the eighteenth embodiment of the invention;

[0050] **FIG. 37B** is a graph representing the operation characteristic of the filter used in a therapeutic system according to the nineteenth embodiment of the present invention;

[0051] **FIG. 38** is a schematic representation of a therapeutic system according to the twentieth embodiment of the present invention;

[0052] **FIG. 39** is a diagram schematically showing a therapeutic system according to the twenty-first embodiment of this invention;

[0053] **FIG. 40** is a diagram schematically showing a therapeutic system according to the twenty-second embodiment of the present invention;

[0054] **FIG. 41** is a diagram showing the coaxial filters incorporated in a therapeutic system according to the twenty-third embodiment of the present invention;

[0055] **FIG. 42** is a diagram showing the filter incorporated in a therapeutic system according to the twenty-fourth embodiment of the invention;

[0056] **FIG. 43** is a schematic representation of a therapeutic system according to the twenty-fifth embodiment of the present invention;

[0057] **FIG. 44** shows an MR image generated in the twenty-fifth embodiment shown in **FIG. 43**;

[0058] **FIG. 45** is a diagram showing the luminances detected at various points in the MR image shown in **FIG. 44**;

[0059] **FIG. 46** is a block diagram depicting the observation unit that is incorporated in the twenty-fifth embodiment;

[0060] **FIG. 47** is a flow chart explaining the operation of the twenty-fifth embodiment;

[0061] FIG. 48 is a flow chart explaining the operation of a therapeutic system according to the twenty-sixth embodiment of the invention;

[0062] FIG. 49 is a block diagram of the observation unit incorporated in a therapeutic system according to the twenty-seventh embodiment of the present invention;

[0063] FIG. 50 is a flow chart explaining the operation of the system shown in FIG. 49;

[0064] FIG. 51 is a flow chart explaining the operation of a therapeutic system according to the twenty-eighth embodiment of the invention;

[0065] FIG. 52 is a flow chart explaining the operation of a therapeutic system according to the twenty-ninth embodiment of this invention;

[0066] FIG. 53 is a diagram illustrating the image displayed by the display provided in the observation unit incorporated in a therapeutic system according to the thirtieth embodiment of the present invention;

[0067] FIG. 54 is a block diagram depicting the observation unit provided in the thirtieth embodiment;

[0068] FIG. 55 is a flow chart explaining the operation of the thirtieth embodiment;

[0069] FIG. 56 is a block diagram of the observation unit incorporated in a therapeutic system according to the thirty-first embodiment of the present invention;

[0070] FIG. 57 is a flow chart explaining the operation of the thirty-first embodiment;

[0071] FIG. 58 is a block diagram of the observation unit incorporated in a therapeutic system according to the thirty-second embodiment of the present invention;

[0072] FIG. 59 is a flow chart explaining the operation of the thirty-second embodiment;

[0073] FIG. 60 is a block diagram of the observation unit incorporated in a therapeutic system according to the thirty-third embodiment of the present invention;

[0074] FIG. 61 is a flow chart explaining the operation of the thirty-third embodiment;

[0075] FIG. 62 is a diagram showing a part of the image displayed by the display provided in the observation unit incorporated in the thirty-third embodiment;

[0076] FIG. 63 is a graph illustrating how luminance changes along the reference line set in an MR image generated in the thirty-third embodiment;

[0077] FIG. 64 is a block diagram showing the observation unit provided in a therapeutic system according to the thirty-fourth embodiment of the present invention;

[0078] FIG. 65 is a flow chart explaining the operation of the thirty-fourth embodiment;

[0079] FIG. 66 is a diagram showing an MR image displayed by the display section incorporated in the observation unit of the thirty-fourth embodiment;

[0080] FIG. 67 is a schematic representation of a therapeutic system according to the thirty-fifth embodiment of the present invention;

[0081] FIG. 68 is a block diagram depicting the observation unit provided in the thirty-fifth embodiment; and

[0082] FIG. 69 is a flow chart explaining the operation of the thirty-fifth embodiment.

DETAILED DESCRIPTION OF THE INVENTION

[0083] The first embodiment of the present invention will be described with reference to FIGS. 1 to 8. FIG. 1 shows the first embodiment, which is a therapeutic system 1. The therapeutic system 1 comprises a microwave therapeutic apparatus 2 and an MRI apparatus (observation means) 3. The microwave therapeutic apparatus 2 is designed to apply therapeutic energy to a subject to heal an affected tissue existing in the living body. The MRI apparatus 3 is designed to show MR (Magnetic Resonance) images to a doctor.

[0084] The MRI apparatus 3 has an MR gantry 5 installed in an MR inspection room 4. The MR gantry 5 is provided to support a patient H. The MR gantry 5 is connected to an MRI apparatus control section 6 located outside the MR inspection room 4.

[0085] A first monitor 7 is provided inside the MR inspection room 4 and connected to the MRI control section 6, for displaying MR images of the patient H lying on the MR gantry 5 during the MR inspection. A light 8 is mounted on a stand protruding upwardly from the gantry 5. A scope holder 10 is secured to one side of the gantry 5. The holder 10 holds an endoscope 8 (either a laparoscope 9 or an ultrasonic endoscope). The endoscope 8 is connected to a light-source device 11 and a video processor 12, both located outside the MR inspection room 4.

[0086] A second monitor 13 is provided in the MR inspection room 4. The second monitor 13 is connected to the video processor 12. To perform MR inspection on the patient H, the illumination light is applied from the light-source device 11 through the endoscope 9 into the peritoneal cavity of the patient H, which contains an affected tissue. The light reflected from everything in the peritoneal cavity is applied to the endoscope 9. The endoscope 9 forms an image of the peritoneal cavity. The video processor 12 converts the image into a video signal, which is supplied to the second monitor 13 provided in the MR inspection room 4. The second monitor 13 displays the image of the peritoneal cavity.

[0087] The therapeutic system has a pneumoperitoneal device 14. The pneumoperitoneal device 14 is driven when the endoscope 9 is used. The device 14 supplies gas into the peritoneal cavity of the patient H in order to accomplish pneumoperitoneum.

[0088] The microwave therapeutic apparatus 2 comprises a microwave applicator (medical applicator) 15. The microwave applicator 15 is connected by a microwave relay cable 16 with a microwave oscillator 17, which is located in the MR inspection room 4. A foot switch 18, an indicator lamp 19 and a speaker 20 are connected to the microwave oscillator 17, which is provided in the MR inspection room 4.

[0089] The therapeutic system further comprises a control unit (control means) 21 for controlling the microwave therapeutic apparatus 2. The control unit 21 is arranged outside the MR inspection room 4. The microwave oscillator 17 and

MRI apparatus control section 6, both located outside the room 4, are connected to the control unit 21. The foot switch 18, indicator lamp 19 and speaker 20, all located in the room 4, are also connected to the control unit 21.

[0090] The microwave applicator 15 has a rod-shaped main body 22 that is shown in FIG. 2B. The main body 22 comprises a conductor 23, an insulator 24, and a distal conductor 25. The outer conductor 23 and the insulator 24 are hollow cylinders, whereas the distal conductor 25 is a solid cylinder. The conductors 23 and 25 and the insulator 24 have substantially the same diameter. They are connected together in axial alignment, with the insulator 24 interposed between the conductors 23 and 25. The microwave applicator 15 has an MW (Microwave) antenna, the center part of which is arranged in the insulator 24.

[0091] An inner conductor 26, which is a thin rod, extends through the outer conductor 23 and the insulator 24 in axial alignment therewith. The distal part of the inner conductor 26 is inserted into the axial hole made in the distal conductor 25. The distal conductor 25 has a radial hole 25a that communicates with the axial hole. The radial hole 25a is filled with solder, which functions as an MR marker 27 to be used in magnetic resonance imaging (MRI). The solder holds the distal part of the inner conductor 26 firmly and steadily in the axial hole of the distal conductor 25, while electrically connecting the inner conductor 26 to the distal conductor 25. The annular space defined by the outer conductor 23, insulator 24 and inner conductor 26 is filled with a dielectric body 28.

[0092] A distal tip 29 is set in screw engagement with the distal conductor 25. The distal end of the tip 29 is shaped like a corn, forming a sharp piercing part 29a.

[0093] The main body 22 of the microwave applicator 15 has its outer circumferential surface covered with a transparent layer 30 made of fluororesin. A resin cylinder 31, which serves as a grip, is mounted on the proximal end portion of the main body 22. The outer circumferential surface of the resin cylinder 31 is covered with a resin coating 32.

[0094] A coaxial connector 33 is coupled to the proximal end of the main body 22. The microwave relay cable 16 can be connected to the coaxial connector 33 as is shown in FIG. 2A.

[0095] The outer conductor 23, distal conductor 25 and inner conductor 26 are made of material, such as Cu, which has magnetic susceptibility ranging from -10^{-3} to $+10^{-3}$, as is shown in FIG. 8. The solder, which forms the MR marker 27, has magnetic susceptibility of -10^{-5} or less, or $+10^{-5}$ or more. Thus, the main body 22 of the applicator 15 has an MR marker 27, which has magnetic susceptibility greater in absolute value than the magnetic susceptibility of the material of the main body 22.

[0096] Before therapy is performed on the patient H by means of the therapeutic system 1, trocars 34a and 34b are set in the abdominal wall Ha of the patient H as is illustrated in FIG. 2A. The endoscope 9 is inserted through the trocar 34a into the peritoneal cavity Hb of the patient H. The microwave applicator 15 is inserted through the trocar 34b into the peritoneal cavity Hb. An air-supplying tube 35 is connected to the trocar 34a. An ultrasonic probe 36 is placed

on the abdomen of the patient H to apply ultrasonic waves into the peritoneal cavity Hb.

[0097] As shown in FIG. 3, the control unit 21 has a unit case 37 and an operation panel 38. The operation panel 38 is provided on the unit case 37. Various switches are arranged on the operation panel 38. They are a start switch 39, a stop switch 40, a high output switch 41, a low output switch 42, an MRI start switch 43, a high output display 44, a low output display 45, high-output setting switches 46a and 46b, and low-output setting switches 47a and 47b.

[0098] As shown in FIG. 4, the control unit 21 comprises a control section 48, an output switching section 49, a high-output setting section 50, and a low-output setting section 51. The high-output setting section 50 and the low-output setting sections 51 are connected to the output switching section 49. The high-output setting switches 46a and 46b are connected to the high-output setting section 50. The low-output setting switches 47a and 47b are connected to the low-output setting sections 51.

[0099] The high output switch 41 and low output switch 42 are connected to the output switching section 49. The start switch 39, stop switch 40, MRI start switch 43, high output display 44 and low output display 45 are connected to the control section 48.

[0100] The operation of the therapeutic system 1 will be described. First, the patient H is laid on the MR gantry 5 provided in the MR inspection room 4, as is illustrated in FIG. 1. Then, as shown in FIG. 2A, trocars 34a and 34b are set in the abdominal wall Ha of the patient H. The insertion section of the endoscope 9 is inserted into the peritoneal cavity Hb of the patient H through the trocar 34a, and the microwave applicator 15 is inserted into the peritoneal cavity Hb through the trocar 34b. If necessary, the ultrasonic probe 36 is placed on the abdomen of the patient H.

[0101] Illumination light is applied from the light-source device 11 through the endoscope 9 to, for example, the affected tissue presents in the peritoneal cavity Hb of the patient H. The endoscope 9 forms an image of the peritoneal cavity Hb. The video processor 12 converts the image into a video signal. The video signal is supplied to the second monitor 13 provided in the MR inspection room 4. The second monitor 13 displays the endoscopic image of the peritoneal cavity Hb.

[0102] During MR inspection, the first monitor 7 provided in the MR inspection room 4 displays an MR image of the patient H lying on the MR gantry 5. The first monitor 7 displays the image of the microwave applicator 15, too, as shown in FIGS. 6 and 7. In FIGS. 6 and 7, Hc indicates the liver of the patient, 52 denotes the artifact resulting from the MR marker 27, and 53 designates the region coagulated when the microwave applicator 15 applies microwaves to the affected tissue.

[0103] In the present embodiment, the control unit 21 is operated, setting the output of the microwave applicator 15, before the microwave applicator 15 is used. The output of the microwave applicator 15 can be set at two values, i.e., high and low. The high output is set when the high-output setting switches 46a and 46b are pushed. The low output is set when the low-output setting switches 47a and 47b are pushed. The high output is selected when the high output switch 41 is pushed, and the low output is selected when the

low output switch 42 is pushed. Alternatively, the high output and the low output may be switched from one to the other, every time an output-changeover switch (not shown) is pushed.

[0104] After the output has been set for the microwave applicator 15, the start switch 39 of the control unit 21 is depressed. Then, the control unit 21 transmits an output start signal to the microwave therapeutic apparatus 2. At the same time, the control unit 21 transmits a control signal to the microwave therapeutic apparatus 2. The control signal corresponds to the output value set in the control unit 21. Upon receipt of the output start signal, the microwave therapeutic apparatus 2 starts operating, whereby the microwave applicator 15 applies microwaves to the affected tissue present in the peritoneal cavity Hb. Thus, microwave therapy is started.

[0105] During the microwave therapy, the control unit 21 transmits a control signal to the microwave therapeutic apparatus 2, controlling the output of the apparatus 2. At the same time, the control unit 21 transmits an MRI start signal to the MRI apparatus 3. In response to the MRI start signal, the MRI apparatus 3 starts generating an MR image of the patient H. The output signal from the MRI apparatus control section 6 is input to the control section 48 of the control unit 21, whereby the MRI apparatus 3 provides an MR image that indicates the position of the microwave applicator 15.

[0106] The data representing the position of the microwave applicator 15 is supplied to the control unit 21. In accordance with this data the control unit 21 controls the output of the microwave applicator 15, i.e., the therapeutic energy to be applied from the applicator 15 to the affected tissue existing in the peritoneal cavity Hb.

[0107] How the control unit 21 controls the microwave applicator 15 will be explained, with reference to the flow chart of FIG. 5.

[0108] First, it is determined in Step S1 whether the stop switch 40 has been pushed or not. If NO in Step S1, the operation goes to Step S2. In Step S2, it is determined whether the high output switch 41 and low output switch 42 of the output-switching section 49 have been depressed or not. If it is determined that neither the switch 41 nor the switch 42 has been depressed, the operation goes to Step S3.

[0109] In Step S3, it is determined whether the MRI start switch 43 has been depressed or not. If NO in Step S3, the operation goes to Step S4.

[0110] In Step S4, it is determined whether the setting switches (i.e., high-output setting switches 46a and 46b and low-output setting switches 47a and 47b) have been pushed or not. If YES in Step S4, the operation goes to Step S5. In Step S5, the various values set are changed. The operation then returns to Step S1. If NO in Step S4, the values set are not changed, and the operation returns to Step S1.

[0111] If YES in Step S2, that is, if the output switch 41 or the output switch 42, or both switches 41 and 42 have been pushed, the operation goes to Step S6. In Step S6, it is determined whether the microwave output of the microwave oscillator 17 is high or not. If YES in Step S6, the operation goes to Step S7.

[0112] In Step S7, the microwave output of the microwave oscillator 17 is changed to low. Then, in Step S8, the control unit 21 transmits an MRI start signal to the MRI apparatus

3. Thus, the microwave therapeutic apparatus 2 is controlled such that the output of the oscillator 17, if high, is changed to low when the MRI start switch 43 is pushed while the microwave applicator 15 is applying microwaves to the affected tissue. The control unit 21 then transmits an MRI start signal to the MRI apparatus 3.

[0113] After the control unit 21 transmits an MRI start signal to the MRI apparatus 3 in Step S8, the operation goes to Step S9. In Step S9 it is determined whether or not the control unit 21 has received an MRI end signal from the MRI apparatus 3. Step S9 is repeated until it is determined that the unit 21 has received an MRI end signal. If YES in Step S9, the operation returns to Step S1. Hence, after the completion of the MR imaging, the output of the microwave oscillator 17 remains not changed to high until the control unit 21 receives an MRI end signal from the MRI apparatus 3.

[0114] If NO in Step S6, that is, if the microwave output of the microwave oscillator 17 is not high, the operation goes to Step S10. In Step S10 the microwave output of the microwave oscillator 17 is changed to high. The operation then returns to Step S1.

[0115] When the stop switch 40 is pushed while the microwave therapeutic apparatus 2 is operating, it is determined in Step S1 that the stop switch 40 has been depressed. In this case, the operation goes to Step S11. In Step S11, the control unit 21 transmits an output stop signal to the microwave therapeutic apparatus 2. In response to the output stop signal, the apparatus 2 stops operating. As a result, the microwave applicator 15 ceases to apply microwaves to the affected tissue existing in the peritoneal cavity Hb. The microwave therapy is thereby terminated.

[0116] If NO in Step S1, that is, if it is determined that the stop switch 40 has not been pushed, either the high output switch 41 or the output-changeover switch (not shown) may be depressed after the MR imaging has completed. In this case, the microwave therapeutic apparatus 2 is controlled to change the output of the microwave oscillator 17 to high.

[0117] The low output switch 42 may be pushed while the output of the microwave oscillator 17 remains high, thus changing the output of the oscillator 17 to low. Alternatively, the stop switch 40 may be pushed while the output of the microwave oscillator 17 remains high, thereby causing the oscillator 17 to stop generating microwaves. In either case, the control unit 21 transmits an MRI start signal to the MRI apparatus 3.

[0118] The therapeutic system 1 described above, i.e., the first embodiment of the invention, is advantageous in the following respects.

[0119] When the microwave therapeutic apparatus 2 and the MRI apparatus 3 are used simultaneously, the output of the microwave applicator 15, i.e., the energy applied to the affected tissue, is automatically decreased. The noise in the electromagnetic waves applied from the applicator 15 imposes on the MRI image generated by the MRI apparatus 3 can therefore be minimized. The MRI image of the peritoneal cavity Hb, showing the affected tissue, is sufficiently clear even while the microwave therapeutic apparatus 2 is being used. Further, therefore may be also distorted to become unclear, while high-frequency waves are applied to the affected tissue. Since the MRI image is not blurred,

showing the affected tissue somewhat larger than it is, there is no possibility that microwaves are applied to anything existing around the affected tissue.

[0120] In the first embodiment, the microwave therapeutic apparatus 2 can continuously perform microwave therapy, while the MR imaging is being effected. It is therefore possible to prevent the temperature of the living tissue from falling during the MR imaging. This helps to accomplish effective therapy.

[0121] Further, it is easy to operate the microwave therapeutic apparatus 2 and the MRI apparatus 3 at the same time. This is because the control unit 21 automatically decreases the output of the microwave applicator 15 (i.e., the energy applied to the affected tissue) while the MRI apparatus 3 is performing MR imaging.

[0122] Still further, the main body 22 of the microwave applicator 15 is electrically insulated reliably and is biologically adapted, because the outer surface of the main body 22 is covered with a transparent layer 30 made of fluororesin. In addition, no living tissues will stick to the main body 22 of the applicator 15 when the microwave applicator 15 is used to cauterize the affected tissue.

[0123] In the first embodiment, the solder, forming the MR marker 27, electrically connects the distal part of the inner conductor 26 to the distal conductor 25. Hence, the artifact 52 resulting from the MR marker 27 located before the center of the MW antenna of the applicator 15 can be shown in the MR image as shown in FIG. 6. The artifact 52 thus shown serves to locate the center of the MW antenna, from which therapeutic energy is emitted. This helps to enhance the operability of the microwave applicator 15 and the safety and reliability of the microwave therapy. Moreover, the microwave applicator 15 is easy to assemble since the MR marker 27 is located in front of the center part of the MW (Microwave) antenna, which is arranged in the insulator 24.

[0124] The MRI apparatus 3, which serves as means for determining the position of the microwave applicator 15, may be replaced by an ultrasonic imaging apparatus or an X-ray CT (Computed Tomography) apparatus. Furthermore, the microwave therapeutic apparatus 2, which is used as the therapeutic apparatus, may be replaced by a laser apparatus, a RF therapeutic apparatus, an HF therapeutic apparatus, or an ultrasonic-wave apparatus. Moreover, a tissue-separating current may be supplied to the microwave applicator 15 for a short time when the stop switch 40 is pushed at the end of the microwave therapy. Still further, a graduation may be printed on the microwave applicator 15 so that the doctor may know how deep the applicator 15 has been inserted into the peritoneal cavity Hb, by reading the graduation shown in the RM image of the patient H.

[0125] The therapeutic system 1, which is the first embodiment of the invention, comprises a therapeutic applicator for applying therapy to a living tissue and an observation means for determining the position of the applicator. The energy applied from the applicator to the living tissue is controlled in accordance with the data representing the position of the applicator. Hence, it is easy to operate the therapeutic applicator and the observation means, such as an MRI apparatus, at the same time. Further, the observation means provides a clear MR image of the patient while the therapeutic applicator is being used.

[0126] FIGS. 9 to 11 show the second embodiment of the present invention. The second embodiment is identical to the first embodiment (FIGS. 1 to 8), except for the structure of the microwave applicator 15.

[0127] As shown in FIG. 9, the microwave applicator 15 has two MR markers 27 and 61. The first MR marker 27 of the same type as the one used in the first embodiment is arranged at a position which is distal to the center part of the MW antenna (i.e., the center part of the insulator 24) of the applicator 15. The second MR marker 61, which is made of solder, is arranged at a position, which is proximal to the center part of the MW antenna.

[0128] The distance La between the first MR marker 27 and the center part of the MW antenna, and the distance L2 between the second MR marker 61 and the center part of the MW antenna have relation of $La > Lb$, $La < Lb$, or $La = Lb$. The second MR marker 61 may be made of material other than solder, such as one having magnetic susceptibility of -10^{-3} or less, or $+10^{-3}$ or more.

[0129] The microwave applicator 15 has its center of energy-emission at the center part of the MW antenna, which lies between the first MR marker 27 and the second MR marker 61. Therefore, two artifacts 52 and 62 will appear in an MR image that has been generated by the MRI apparatus 3, as is illustrated in FIG. 10.

[0130] The second embodiment is advantageous in some respects. As shown in FIG. 11, neither the artifact 52 nor the artifact 62 conceals the image of an affected tissue that is treated with microwave (i.e., coagulated region 53). This is because the center of energy-emission (i.e., center part of the MW antenna) is located between the first MR marker 27 and second MR marker 61, both made of solder and resulting in the first artifact 52 and second artifact 62, respectively. As a result, how the living tissue is coagulated can be clearly observed. This enables the doctor to know how the living tissue changes, from the beginning of the microwave therapy he or she is performing by the use of the microwave applicator 15. The safety of the microwave therapy can therefore be enhanced.

[0131] FIG. 12 shows the microwave applicator 15 incorporated in a therapeutic system according to the third embodiment of the invention. The third embodiment differs from the first embodiment (FIGS. 1 to 8) in the structure of the microwave applicator 15. As FIG. 12 shows, the distal conductor 25 has an axial hole 71 made in its proximal end part. The hole 71 communicates with the interior of the outer conductor 23, which is a hollow cylinder. The distal end part of the dielectric body 28 is inserted in the axial hole 71.

[0132] The distal end part of the dielectric body 28, which is inserted in the axial hole 71 renders the distal conductor 25 more rigid than in the case where only the distal part of the inner conductor 26 supports the distal conductor 25 as in the first embodiment. Ultimately, the dielectric body 28 serves to strengthen the junction between the distal conductor 25 and the insulator 24, which are relatively fragile.

[0133] FIG. 13 shows the microwave applicator 15 incorporated in a therapeutic system, which is the fourth embodiment of the invention. The fourth embodiment differs from the first embodiment (FIGS. 1 to 8) in the structure of the microwave applicator 15. As FIG. 13 shows, the microwave applicator 15 has a distal conductor 81, instead of the distal

conductor **25** and the distal tip **29**. Further, a titanium coating **82**, instead of the transparent layer **30** made of fluororesin, covers the distal conductor **81** and the outer conductor **23**.

[0134] An insulating sheath **83** is mounted on the proximal part of the distal conductor **81**, the insulator **24**, and the distal part of the outer conductor **23**. An insulating cover **84** is mounted on the outer circumferential surface of the coaxial connector **33**.

[0135] The titanium coating **82** can be thinner than the fluororesin layer **30** to have the same strength. Hence, the main body **22** of the microwave applicator **15** can have a smaller outer diameter than its counterpart of the first embodiment. In addition, MR markers can be made of the titanium coating **83** covering the distal conductor **81** and the outer conductor **23**.

[0136] FIGS. 14 and 15 depict the flexible applicator **91** incorporated in a therapeutic system, which is the fifth embodiment of the present invention. The flexible applicator **91** is designed for accomplishing therapy on affected tissues in the esophageal veins, the bile duct, or the like.

[0137] As shown in FIG. 14, the flexible applicator **91** has an elongated insertion section **94**. The insertion section **94** comprises a flexible coaxial cable **95**, an MW antenna **96**, and an insulating sheath **97**. The insertion section **94** is guided into a body cavity through the instrument channel **93** of an MR-compatible endoscope (or an MR endoscope) **92**. The flexible coaxial cable **95** is provided in the insertion section **94** and comprises an inner conductor and an outer conductor surrounding the inner conductor. The MW antenna **96**, which applies therapeutic energy, is connected to the distal end of the coaxial cable **95**. The insulating sheath **97** covers the flexible coaxial cable **95** and the MW antenna **96**.

[0138] The MW antenna **96** comprises a distal conductor **98**, a proximal conductor **99**, and a dielectric body **100**. The distal conductor **98** is connected to the inner conductor of the coaxial cable **95**. The proximal conductor **99** is connected to the outer conductor of the coaxial cable **95**. The dielectric body **100** is interposed between the distal conductor **98** and the proximal conductor **99**.

[0139] An MR marker **101** is provided on the distal part of the flexible coaxial cable **95**, at a position proximal to the MW antenna **96**. A sheath **102** made of fluororesin is mounted on the entire insertion section **94** of the flexible applicator **91**.

[0140] To use the flexible applicator **91**, the insertion section of the MR-compatible endoscope **92** is inserted into a tubular cavity, e.g., the esophagus Hd, of the patient. The distal end of the insertion section is guided to the vicinity of the affected tissue, e.g., phlebeurysm He, existing in the esophagus Hd. Then, the insertion section **94** of the flexible applicator **91** is inserted into the esophagus Hd through the instrument channel **93** of the MR-compatible endoscope **92**. The doctor can set the MW antenna **96** at a desired position with respect to the surface of the esophagus Hd, referring to the position of the MR marker **101** on the flexible applicator **91**. Once set so, the MW antenna **96** can coagulate or cauterize the phlebeurysm He efficiently.

[0141] The fifth embodiment described above is advantageous in that the MW antenna **96**, i.e., the means for emitting

therapeutic energy, can be easily located. This is because the ring-shaped MR marker **101** is provided on the distal part of the insertion section **92** of the flexible applicator **91**, at a position proximal to the MW antenna **96**. The doctor can therefore correctly place the MW antenna **96** at a desired position with respect to the surface of the tubular cavity. Once set so, the MW antenna **96** can coagulate or cauterize the affected tissue present in the tubular cavity. Thus, the operability of the microwave applicator **15** and the safety and reliability of the microwave therapy can be enhanced. As a result, even if either coagulation or necrosis is induced in the thin wall of a tubular organ, necrosis or decudation of the tissue will occur, and no pits will be formed in the wall of the tubular organ.

[0142] FIG. 16 shows the flexible applicator **91** incorporated in a therapeutic system, which is the sixth embodiment of the present invention. The flexible applicator **91** differs from its counterpart of the fifth embodiment, as will be described below.

[0143] In the fifth embodiment, one the ring-shaped MR marker **101** is provided on the distal part of the insertion section **94** of the flexible applicator **91**, at a position proximal to the MW antenna **96**. In the sixth embodiment, a second MR marker **103** is arranged at the rear of the ring-shaped MR marker **101**. The dielectric body **100** is the middle part of the MW antenna **96** that applies microwave to coagulate or cauterize the affected tissue in the wall of the tubular organ. The distance La between the body **100** and the front MR marker **101** is equal to the distance Lb between the front MR marker **101** and the second MR marker **103**. While the flexible applicator **91** is being used, the position of the dielectric body **100** can be inferred from the distance Lb between the MR marker **101** and **103**.

[0144] In the sixth embodiment, the second MR marker **103** is located at the back of the MR marker **101** which is identical to its counter part of the fifth embodiment, and the distance La is equal to the distance Lb ($La=Lb$). Hence, it is easier for a doctor to locate the dielectric body **100** that is the center of energy-emission.

[0145] FIG. 17 shows the monopolar paracentetic applicator **111** incorporated in a therapeutic system that is the seventh embodiment of the invention.

[0146] The mono-polar paracentetic applicator **111** is used in combination with an electrode provided outside the patient. The applicator **111** has a needle electrode **112** made of titanium. A connector **113** is mounted on the distal part of the needle electrode **112**. A connector housing **114** is mounted on the connector **113**.

[0147] A needle **115** having a length La is attached to the distal end of the needle electrode **112**. Two ring-shaped MR markers **116** and **117** are provided on the distal part of the electrode **112**, at the back of the needle **115**. The MR markers **116** and **117** are spaced apart by a distance Lc. The distance Lc is equal to the distance Lb between the tip of the needle **115** and the front MR marker **116** ($Lb=Lc$). The needle electrode **112** is covered with a fluororesin coating **118**.

[0148] While the mono-polar paracentetic applicator **111** is being used, the position of the tip of the needle **115** attached to the distal end of the needle electrode **112** can be inferred from the distance Lc between the MR markers **116**

and 117. Further, the applicator 111 may have a smaller diameter, ultimately reducing the pain the patient may have while receiving the therapy. This is possible because the needle 115 having an appropriate length L_a is attached to the distal end of the needle electrode 112 made of titanium.

[0149] FIGS. 18 to 20 show a therapeutic system according to the eighth embodiment of the present invention. The eighth embodiment is identical to the first embodiment (FIGS. 1 to 8), except for the structure of the control unit 21.

[0150] As shown in FIG. 18, some additional switches and displays are provided on the operation panel 38 of the control unit 21. The additional switches are: an automatic/manual switch 121, high-output period setting switches 123a and 123b, low-output period setting switches 125a and 125b, and total high-output period setting switches 127a and 127b. The additional displays are a high-output period display 122, a low-output display 124, and a total high-output period display 126. The control unit 21 is set into automatic control mode or manual control mode by operating the switch 121. Once set in the manual mode, the control unit 21 can operate in the same way as in the first embodiment to perform various controls. Once set in the automatic control mode, the control unit 21 can perform various controls in accordance with the periods of time that have been set by operating the switches 123a, 123b, 125a, 125b, 127a and 127b.

[0151] As shown in FIG. 19, the control section 48 that is provided in the control unit 21 is connected to a time counting section 128. The time counting section 128 is connected to a high-output period setting section 129 and a low-output period setting section 130.

[0152] How the control unit 21 controls the microwave applicator 15 in the eighth embodiment will be explained.

[0153] First, the operation panel 38 of the control unit 21 is operated, setting conditions in which the applicator 15 of the microwave therapeutic apparatus 2 should be operated. More specifically, the high-output period setting switches 123a and 123b are operated, setting a high-output period for which the applicator 15 is to apply microwaves at high level. The high-output period display 122 displays the high-output period thus set. Similarly, the low-output period setting switches 125a and 125b are operated, setting a low-output period for which the applicator 15 is to apply microwaves at low level. The low-output display 124 displays the low-output period thus set. Further, the total high-output period setting switches 127a and 127b are operated, setting a total high-output period for which the applicator 15 is to apply microwaves at high level. The total high-output period display 126 displays the total high-output period.

[0154] Next, the automatic/manual switch 121 is operated, whereby the control unit 21 is set into either the automatic control mode or the manual control mode. If the control unit 2 is set into the manual control mode, the high-output period, low-output period and total high-output period set by operating the operation panel 38 will be invalidated. In this case, the control unit 21 will operate in the same way as in the first embodiment.

[0155] If the control unit 2 is set into the automatic control mode, the control unit 21 will perform various controls in accordance with the various periods set by operating the operation panel 38, as will be described with reference to the flow chart of FIG. 20.

[0156] First, the start switch 39 of the control unit 21 is depressed. The control unit 21 generates a signal representing the high-output period. This signal is supplied to the microwave therapeutic apparatus 2. The microwave applicator 15 of the therapeutic apparatus 2 starts emitting microwaves in Step S21. At the same time, the time counting section 128 starts counting down the high-output period. Then, in Step S22, it is then determined whether the stop switch 40 has been pushed or not.

[0157] If NO in Step S22, that is, if the stop switch 40 has not been pushed, the operation goes to Step S23. In Step S23, it is determined whether the high-output period has elapsed or not. If NO in Step S23, the operation goes to Step S24, in which a total high-output period is calculated. Then, in Step S25, it is determined whether the total high-output period has elapsed or not. If NO in Step S25, it is determined in Step S26 whether any setting switches have been pushed or not. If YES in Step S26, the operation goes to Step S27, in which the various values set are changed. The operation then returns to Step S22. If NO in Step S26, the operation returns directly to Step S22.

[0158] If YES in Step S23, that is, if it is determined that the high-output period has elapsed, the operation goes to Step S28. In Step S28, the low output is transmitted to the microwave therapeutic apparatus 2. The output of the apparatus 2 is thereby switched to the low value. The microwave applicator 15 of the apparatus 2 starts emitting microwaves. At the same time, the time counting section 128 starts counting down the low-output period.

[0159] Thereafter, in Step S29, the control unit 21 transmits an MRI start signal to the MRI apparatus 3. Then, in Step S30, it is determined whether or not the control unit 21 has received an MRI end signal from the MRI apparatus 3. If NO, Step S30 is repeated until the high-output period elapses. Upon lapse of the high-output period, the output of the microwave therapeutic apparatus 2 is switched to the low value, and the MRI apparatus 3 starts MRI imaging.

[0160] If YES in Step S30, that is, if it is determined that the control unit 21 has received an MRI end signal from the MRI apparatus 3, the operation goes to Step S31. In Step S31, it is determined whether the low-output period has elapsed or not. If NO, Step S31 is repeated. If YES, the operation returns to Step S21. In Step S21, the output of the microwave therapeutic apparatus 2 is switched to the high value again, only if the control unit 21 has received an MRI end signal.

[0161] The microwave applicator 15 emits high-output microwaves and low-output microwaves alternately and repeatedly. The applicator 15 stops emitting microwaves when the total high-output period set elapses. Then, the MRI apparatus 3 carries out MR imaging. Thereafter, the microwave therapy is terminated.

[0162] If YES in Step S22, that is, if it is determined that the stop switch 40 has been pushed in the course of the microwave therapy, the control unit 21 transmits an output stop signal to the microwave therapeutic apparatus 2. In response to the output stop signal, the oscillator 17 stops generating microwaves. As a result, the microwave applicator 15 ceases to apply microwaves in Step S32. Then, in Step S33, the control unit 21 transmits an MRI start signal to the MRI apparatus 3, which performs MR imaging.

[0163] In the eighth embodiment, the various output periods set by operating the operation panel 38 will be invalidated when the automatic/manual switch 121 provided on the panel 38 of the control unit 21 is operated, thereby setting the control unit 21 into the manual control mode. In this case, the control unit 21 will operate in the same way as in the first embodiment. Thus, the microwave output of the microwave oscillator 15, i.e., the therapeutic energy applied to the living tissue, is automatically decreased while both the microwave therapeutic apparatus 2 and the MRI apparatus 3 are operating at the same time, the latter performing MR imaging. The influence that the noise in the microwaves applied from the applicator 15 imposes on the MRI apparatus 3 can therefore be minimized. As a result, the image provided by the MRI apparatus 3 is sufficiently clear even while the microwave therapeutic apparatus 2 is being used.

[0164] Furthermore, once the control unit 21 has been set into the automatic control mode by operating the automatic/manual switch 121, the microwave applicator 15 automatically emit high-output microwaves and low-output microwaves alternately and repeatedly, and the MRI apparatus 3 automatically repeats the MR imaging. Hence, the eighth embodiment can achieve the same advantages as the first embodiment.

[0165] In the eighth embodiment, the MRI apparatus 3 may be replaced by an ultrasonic imaging apparatus or an X-ray CT apparatus. And the microwave therapeutic apparatus 2 may be replaced by a laser apparatus, an RF therapeutic apparatus, an HF therapeutic apparatus, or an ultrasonic-wave apparatus. Moreover, a tissue-separating current may be supplied to the microwave applicator 15 for a short time when the stop switch 40 is pushed at the end of the microwave therapy. If such a current is so supplied to the microwave applicator 15, bleeding will be prevented at the living tissue when the applicator 15 (i.e., electrode) is pulled out of the tissue after the completion of the microwave therapy.

[0166] FIGS. 21 and 22 show a therapeutic system according to the ninth embodiment of the invention. The ninth embodiment is identical to the first embodiment (FIGS. 1 to 8), except for the structure of the control unit 21.

[0167] As shown in FIG. 21, the control unit 21 comprises an MR-image processing section 141, a therapeutic device control section 142, and a reference output section 143.

[0168] In the ninth embodiment, the MRI apparatus 3 repeats MR imaging at intervals, while the microwave applicator 15 is applying microwaves to an affected tissue. How this is performed will be explained below, with reference to the flow chart of FIG. 22.

[0169] First, the MRI apparatus 3 repeats MR imaging at certain intervals in Step S41. In Step S42, the previous MR image and the latest MR image are compared, finding a color difference d between the MR images compared. An increase in the size of the treated region is determined from the color difference d .

[0170] Next, in Step S43, it is determined whether the color difference d obtained in Step S42 is equal to or greater than the minimum proper color difference $d1$. If YES, that is, if $d \geq d1$, the operation goes to Step S44. In Step S44, it is determined whether the color difference d is equal to or less

than the maximum proper color difference $d2$. If YES, that is, if $d \leq d2$, the operation returns to Step S41.

[0171] If the color difference d falls outside a prescribed range of proper values, the output of the microwave applicator 15 is changed as will be described below.

[0172] Namely, if NO in Step S43, that is, if $d < d1$, the therapy speed is too low. In this case, the operation goes to Step S45, in which one of the following processes A to D is carried out.

[0173] A. To increase the output of the applicator 15

[0174] B. To lengthen the period of outputting microwaves

[0175] C. To increase the temperature set for the living tissue

[0176] D. To alter the output waveform to increase the therapy speed

[0177] If NO in Step S44, that is, if $d > d2$, the therapy speed is too high. In this case, the operation goes to Step S46, in which one of the following processes A to D is carried out.

[0178] A. to decrease the output of the applicator 15

[0179] B. To shorten the period of outputting microwaves

[0180] C. To decrease the temperature set for the living tissue

[0181] D. To alter the output waveform to decrease the therapy speed

[0182] The ninth embodiment described above is advantageous in that the safety and reliability of the microwave therapy can be enhanced. This is because the microwave therapeutic apparatus 2 is controlled to effect the therapy at the best possible speed.

[0183] In the ninth embodiment, too, the MRI apparatus 3 may be replaced by an ultrasonic imaging apparatus or an X-ray CT apparatus. Further, the microwave therapeutic apparatus 2 may be replaced by a laser apparatus, an RF therapeutic apparatus, an HF therapeutic apparatus, or an ultrasonic-wave apparatus.

[0184] FIGS. 23 and 24 show a therapeutic system according to the tenth embodiment of the invention. The tenth embodiment is identical to the therapeutic system 1 (FIGS. 1 to 8) that is the first embodiment, except for the following respects.

[0185] As shown in FIG. 23, the microwave applicator 15 has two MR markers 151 and 152. As shown in FIG. 24, the control unit 21 incorporates a control section 153, a marker detecting section 154, and a motion calculating section 155. The control section 153 is connected to the microwave therapeutic apparatus 2. The marker detecting section 154 is connected to the MRI apparatus control section 6 provided in the MRI apparatus 3. The motion calculating section 155 is connected to and located between the control section 153 and the marker detecting section 154.

[0186] A reference-point setting section 156 is connected to the motion calculating section 155. The section 156 is designed to set a reference point 157 at a given position on

the MR screen of the first monitor 7. The first monitor 7 is provided to display an MR image generated by the MRI apparatus 3. More specifically, the first monitor 7 displays the image of the organ Hf being treated and the image of the microwave applicator 15, as is illustrated in FIG. 23. A maximum-displacement setting section 158 is connected to the control section 153.

[0187] The control section 153 provided in the control unit 21 monitors the positional relation of the two MR markers 151 and 512 and the reference point 157 in order to detect the displacement of the microwave applicator 15. Upon detecting an excessive displacement of the applicator 15 from the reference point 157, the control section 153 causes the microwave oscillator 17 to stop generating microwaves.

[0188] The operation of the therapeutic system 1 according to the tenth embodiment will be explained.

[0189] At first, the doctor operates the maximum-displacement setting section 158, thus setting the maximum displacement the applicator 15 may have with respect to the reference point 157 without causing troubles. Then, the doctor pierces the organ Hf with the microwave applicator 15. The MRI apparatus 3 generates MR images of the organ Hf and applicator 15, which are displayed on the MR screen of the first monitor 7. The doctor operates the reference-point setting section 156, thereby setting a reference point 157 on the MR screen of the first monitor 7. The data representing the positional relation the MR markers 151 and 152 on the applicator 15 and the reference point 157 have at this time is stored, as an initial position value, into the memory (not shown) incorporated in the control section 153.

[0190] Every time the MRI apparatus 3 generates an MR image of the organ Hf and applicator 15, the positional relation of the MR markers 151 and 152 and the reference point 157 is detected. If the displacement of the microwave applicator 15 exceeds the maximum value set by operating the maximum-displacement setting section 158, it is determined that the applicator 15 has been displaced excessively. In this case, the control section 153 causes the microwave oscillator 17 to stop generating microwaves.

[0191] Moreover, if neither the MR marker 151 nor the MR marker 512 is displayed on the MR screen of the first monitor 7, the section 153 causes the microwave oscillator 17 to stop generating microwaves.

[0192] In the tenth embodiment, the microwave oscillator 17 automatically stops generating microwaves when the microwave applicator 15 is displaced excessively. That is, since the output of the microwave therapeutic apparatus 2 is controlled in accordance with the positional relation of the images MR markers and reference point, all generated by the MRI apparatus 3, the safety and reliability of the microwave therapy can be enhanced.

[0193] Also in the tenth embodiment, the MRI apparatus 3 may be replaced by an ultrasonic imaging apparatus or an X-ray CT apparatus. Further, the microwave therapeutic apparatus 2 may be replaced by a laser apparatus, an RF therapeutic apparatus, an HF therapeutic apparatus, or an ultrasonic-wave apparatus.

[0194] FIGS. 25 and 26 show a therapeutic system according to the eleventh embodiment of the present inven-

tion. The eleventh embodiment is identical to the tenth embodiment (FIGS. 23 and 24), except for the structure of the control unit 21.

[0195] As depicted in FIG. 26, a signal-value change calculating section 161 is used in place of the motion calculating section 155. The section 161 is connected to and arranged between the control section 153 and the marker detecting section 154.

[0196] Further, an initial signal-value outputting section 162 is connected to the signal-value change calculating section 161. A maximum luminance-change setting section 163 is connected to the control section 153. As in the tenth embodiment, the first monitor 7 displays the image of the organ Hf being treated and the image of the microwave applicator 15, as is illustrated in FIG. 25. In FIG. 25, Hg denotes a protected region of the organ Hf.

[0197] A monitor marker 164 can be displayed on the MR screen of the first monitor 7, for example in the protected region Hg of the organ Hf that should be protected from any damage. The monitor marker 164 can be moved to any desired position on the MR screen, by operating an appropriate input device such as a keyboard or a mouse.

[0198] The operation of the eleventh embodiment will be described. First, the doctor pierces the organ Hf with the microwave applicator 15. Then, the MRI apparatus 3 generates MR images of the organ Hf and applicator 15, which are displayed on the MR screen of the first monitor 7. The doctor moves the applicator 15, setting the monitor marker 164 in the protected region Hg of the organ Hf displayed on the MR screen of the first monitor 7. Data representing the luminance of the image of the protected region Hg designated by the monitor marker 164 is stored, as initial value, into the memory (not shown) incorporated in the control section 153.

[0199] Further, the doctor operates the maximum luminance-change setting section 163, setting a maximum luminance change. Every time the MRI apparatus 3 generates an MR image of the organ Hf and applicator 15 after the microwave therapy has been started, the luminance of the image of the protected region Hg is compared with the initial value stored in the memory of the control section 153, thereby determining a change in luminance. If the luminance change exceeds the maximum luminance change set by operating the maximum luminance-change setting section 163, it is determined that degeneration has occurred in the protected region Hg of the organ Hf. In this case, the control section 153 causes the microwave oscillator 17 to stop generating microwaves.

[0200] As indicated above, the monitor marker 164 is set in any region of the MR image of the organ Hf that should be protected from damage. When the luminance change in the region of the MR image exceeds the preset maximum luminance change, it is determined that degeneration has occurred in this region. Then, the control section 153 causes the microwave oscillator 17 to stop generating microwaves. Hence, the eleventh embodiment helps to enhance the safety and reliability of the microwave therapy.

[0201] In the eleventh embodiment, too, the MRI apparatus 3 may be replaced by an ultrasonic imaging apparatus or an X-ray CT apparatus. Further, the microwave therapeutic

apparatus 2 may be replaced by a laser apparatus, an RF therapeutic apparatus, an HF therapeutic apparatus, or an ultrasonic-wave apparatus.

[0202] FIGS. 27 to 29 show a therapeutic system according to the twelfth embodiment of this invention. The twelfth embodiment is identical to the therapeutic system 1 (FIGS. 23 and 24), i.e., the tenth embodiment, except for the following respects.

[0203] As shown in FIG. 28, the twelfth embodiment has an applicator moving device 171, a distance calculating section 172, a therapy-point (target) setting section 173, and a maximum-distance setting section 175. The applicator moving device 171 is provided outside the control unit 21 and connected to the control section 153 of the control unit 21, for moving the microwave applicator 15 in the axial direction thereof. The distance calculating section 172, therapy-point setting section 173 and maximum-distance setting section 175 are provided in the control unit 21.

[0204] The distance calculating section 172 is connected to and located between the control section 153 and the marker detecting section 154. The therapy-point setting section 173 is connected to the distance calculating section 172, for setting a plurality of therapy points 174 on the MR screen of the first monitor 7 that displays an MR image generated by the MRI apparatus 3. The therapy points 174 indicate those parts of the organ Hf that must be treated with microwaves. The applicator moving device 171 moves the microwave applicator 15 under the control of the control section 153, until the MR marker 151 on the applicator 15 to a therapy point 174. The applicator 15 then applies microwaves to the parts of the organ Hf, i.e. the therapy points 174. The doctor operates the maximum-distance setting section 175, setting the longest distance the MR marker 151 can be moved from one therapy point 174 to another, without causing any trouble during the microwave therapy.

[0205] The operation of the twelfth embodiment will be explained. First, the doctor pierces the organ Hf with the microwave applicator 15. The MRI apparatus 3 generates MR images of the organ Hf and applicator 15, which are displayed on the MR screen of the first monitor 7. The doctor operates the therapy-point setting section 173, setting therapy points 174 on the MR screen of the first monitor 7.

[0206] Thereafter, the control section 153 controls the applicator moving device 171, which moves the applicator 15 until the monitor marker 151 reaches the first therapy point 174. The applicator 15 is operated, applying microwaves to that part of the organ Hf which is located at the first therapy point 174. When the part of the organ Hf is treated thoroughly, the applicator 15 stops applying microwaves under the control of the control section 153. The control section 153 controls the applicator moving device 171, which moves the microwave applicator 15 in the axial direction thereof, so that the MR marker 151 may move to the second therapy point 174.

[0207] How the microwave applicator 15 is moved, to move the MR marker 151 from the first therapy point 174 to the second therapy point 171, will be described with reference to the flow chart of FIG. 29.

[0208] At first, in Step S61, the applicator moving device 171 moves the microwave applicator 15 toward the second

therapy point 174. In Step S62, the MRI apparatus 3 performs MR imaging, whereby an MR image is displayed on the MR screen of the first monitor 7.

[0209] Thereafter, in Step S63, the distance calculating section 172 calculates the distance between the MR marker 151 and the second therapy point 174. In Step S64, it is determined whether the distance calculated in Step S63 is longer than the maximum distance set by operating the maximum-distance setting section 175. If NO, the operation returns to Step S61, and Steps 62 and 63 are repeated.

[0210] If YES in Step S64, that is, if the distance calculated in Step S63 is equal to or shorter than the maximum distance, it is determined that the MR marker 151 has moved to the second therapy point 174. In this case, the operation goes to Step S65. In Step S65, the control unit 21 transmits an output start signal to the microwave therapeutic apparatus 2. In response to the output start signal, the applicator 15 starts applying microwaves to that part of the organ Hf which is located at the second therapy point 174.

[0211] In Step S66, it is determined whether a prescribed period of time has elapsed or not from the start of application of microwaves. If NO, the operation returns to Step S66. If YES, the operation goes to Step S67, in which the control unit 21 transmits an output stop signal to the microwave therapeutic apparatus 2. In response to the output stop signal, the applicator 15 stops applying microwaves.

[0212] Then, in Step S68 it is determined whether there is any therapy point 174 to which microwaves have not been applied. If YES, the operation returns to Step S61. Steps S61 to S68 are repeated until it is determined in Step S 68 that microwaves have been applied to all therapy points 174 set by operating the therapy-point setting section 173. Then, the microwave applicator 15 is no longer moved in the organ Hf, because the microwave therapy has been performed at every therapy point 174 he or she had set by operating the therapy-point setting section 173.

[0213] As mentioned above, the twelfth embodiment has the applicator moving device 171 for moving the applicator 15 in the axial direction thereof, and the therapy-point (target) setting section 173 for setting therapy points 174 on the MR screen of the first monitor 7. The control section 153 controls the device 171 such that the MR marker 151 on the applicator 15 moves from one therapy point 174 to the next one. Hence, the microwave therapeutic apparatus 2 can automatically effect microwave therapy sequentially at all therapy points 174. Therefore, it is easy to operate the microwave therapeutic apparatus 2 and the MRI apparatus 3 at the same time in the therapeutic system according to the twelfth embodiment.

[0214] Also in the twelfth embodiment, the MRI apparatus 3 may be replaced by an ultrasonic imaging apparatus or an X-ray CT apparatus. Further, the microwave therapeutic apparatus 2 may be replaced by a laser apparatus, an RF therapeutic apparatus, an HF therapeutic apparatus, or an ultrasonic-wave apparatus.

[0215] FIG. 30 shows a therapeutic system according to the thirteenth embodiment of the invention. The thirteenth embodiment is identical to the therapeutic system 1 (FIGS. 23 and 24), i.e., the tenth embodiment, except for the following respects.

[0216] As illustrated in FIG. 30, a reference-point marker 181 is set on the MR screen of the first monitor 7 that displays an MR image generated by the MRI apparatus 3. The positional relation between the reference-point marker 181, on the one hand, and the MR markers 151 and 152 on the microwave applicator 15, on the other hand, is detected every time the MRI apparatus generates an MR image. If the distance between each MR marker and the reference-point marker 181 is longer than a preset value, it is determined that the microwave applicator 15 has been excessively moved in the organ Hf being treated with microwaves. In so, the control unit 21 causes the microwave oscillator 17 to stop generating microwaves.

[0217] Neither the MR marker 151 nor the MR marker 152 may be displayed on the MR screen of the first monitor 7. In this case, the control unit 21 causes the microwave oscillator 17 to stop generating microwaves.

[0218] In the thirteenth embodiment, the microwave oscillator 17 automatically stops generating microwaves when the applicator 15 is moved too much with respect to the reference-point marker 181. Hence, the safety and reliability of the microwave therapy can be enhanced, even if the patient H lying on the MR gantry 5 during the MR inspection.

[0219] FIGS. 31 to 33 show a therapeutic system, which is the fourteenth embodiment of the present invention. This embodiment is identical to the therapeutic system 1 (FIGS. 1 to 8), i.e., the first embodiment, except for the following respects.

[0220] The microwave oscillator 17, which is provided outside the MR inspection room 4 as shown in FIG. 31, incorporates a magnetron. The magnetron is used as a microwave generator, for generating high-frequency microwaves for therapeutic purpose. The magnetron is connected to the microwave applicator 15 provided in the MR inspection room 4, by a microwave relay cable 16 that is a coaxial cable. A coaxial filter 191 is provided on the microwave relay cable 16. Hence, the coaxial filter 191 is arranged between the output section of the magnetron and the input section of the MR inspection room 4.

[0221] The coaxial filter 191 operates as a high-pass filter (HPF) having a threshold frequency f_c . The threshold frequency f_c is lower than the frequency f_1 of the therapeutic microwaves and higher than the intermediate frequency f_2 of the MRI waves, as is seen from FIG. 32. That is, $f_1 > f_c > f_2$. Thus, the coaxial filter 191 transmits the therapeutic microwaves and attenuates the waves.

[0222] The MRI apparatus 3 is provided in the MR inspection room 4, though not shown in FIG. 31. The MRI apparatus 3 generates an MR tomogram of the illustrated in FIG. 33. The MR tomogram includes an image of the patient's liver Hc and a region 53 thereof, coagulated as the microwave applicator 15 (not shown) applies microwaves in the lever Hc.

[0223] As described above, the coaxial filter 191 is provided on the microwave relay cable 16 that connects the microwave applicator 15 and the magnetron which are provided in the MR inspection room 4 and the microwave oscillator 17, respectively. The filter 191 can therefore remove noise, if any, in the therapeutic microwaves before these microwaves are transmitted into the MR inspection

room 4, while not attenuating the therapeutic microwaves at all. The MRI tomogram is free from the influence of the noise in the therapeutic microwaves. This makes it possible to carry out microwave therapy and MR imaging at the same time. Hence, there will arise no problem if a magnetron, which is an inexpensive component but generates noise over a broad band, is used to generate therapeutic microwaves. In addition, the coaxial filter 191 can be a simple filter such as a waveguide or the like.

[0224] A therapeutic system according to the fifteenth embodiment of the present invention will be described with reference to FIG. 34A. The fifteenth embodiment differs from the fourteenth embodiment (FIGS. 31 to 33), only in the operating characteristic of the coaxial filter 191. The coaxial filter 191 operates as a band-pass filter (BPF), not as a high-pass filter as in the fourteenth embodiment. As can be understood from FIG. 34A, the coaxial filter 191 transmits therapeutic microwaves having frequency f_1 and attenuates the MRI microwaves. The cut-off frequency f_c of the filter 191 has an upper-limit value f_{cH} and a lower-limit value f_{cL} . These values f_{cH} and f_{cL} , the frequency f_1 of the therapeutic microwaves, and the intermediate frequency f_2 of the MRI waves have the relationship of: $f_1 > f_{cH} > f_{cL} > f_2$.

[0225] In the fifteen embodiment, the coaxial filter 191 is a band-pass filter. Therefore, the microwave therapy and the MR imaging can be effected at the same time by the use of a single filter, regardless of the intermediate frequency f_2 of the MRI waves. Operating as a band-pass filter, the coaxial filter 191 transmits the therapeutic microwaves and attenuates the MRI waves as shown in FIG. 34A.

[0226] A therapeutic system according to the sixteenth embodiment of the present invention will be described with reference to FIG. 34B. The sixteenth embodiment differs from the fourteenth embodiment (FIGS. 31 to 33), only in the operating characteristic of the coaxial filter 191. The coaxial filter 191 operates as a band-cut filter (BCF), not as a high-pass filter as in the fourteenth embodiment, and attenuates only the MRI microwaves having frequency f_2 . The coaxial filter 191 has a cut-off frequency having an upper-limit value f_{cH} and a lower-limit value f_{cL} . As can be seen from FIG. 34B, the values f_{cH} and f_{cL} , the frequency f_1 of the therapeutic microwaves, and the frequency f_2 of the MRI waves have the relationship of: $f_1 > f_{cH} > f_2 > f_{cL}$.

[0227] Since the coaxial filter 191 is a band-cut filter (BCF), it attenuates only microwaves of a specific band. Hence, the filter 191 generates heat only a little while operating and can be made small. The microwave therapy and the MR imaging can be performed at the same time by the use of a single filter, regardless of the frequency f_1 of the therapeutic microwaves. The filter 191 may be replaced by a waveguide that has been adjusted in size to have the cut-off frequency described above.

[0228] FIGS. 35 and 36 show a therapeutic system according to the seventeenth embodiment of the invention. The therapeutic system 1 according to the seventeenth embodiment differs from the fourteenth embodiment (FIGS. 31 to 33) in the following respects.

[0229] As shown in FIG. 35, a high-frequency power supply 204 is provided outside the MR inspection room 4, i.e. the magnetic shield room for use in MR imaging. The power supply 204 includes a high-frequency wave generator

of two-wire output type (not shown), such as an electrode knife apparatus. Two high-frequency wave relay cables **201** and **202** are connected at one end to the high-frequency wave generator arranged in the power supply **204**. The first cable **201** is connected at the other end to an active electrode (not shown) provided in the MR inspection room **4**. The second cable **202** is connected at the other end to a return electrode (not shown) provided in the MR inspection room **4**. A two-wire filter **203** is provided on the cables **201** and **202**. The filter **203** operates as a low-pass filter (LPF) having a threshold frequency f_c . The threshold frequency f_c is lower than the frequency f_1 of the therapeutic microwaves and higher than the frequency f_2 of the MRI microwaves, as is seen from FIG. 36. That is, $f_1 > f_c > f_2$. Thus, the coaxial filter **191** transmits the MRI microwaves and attenuates the therapeutic microwaves.

[0230] As described above, the cables **201** and **202** connects the two-wire high-frequency wave generator provided in the power supply **204** to the active electrode and return electrode, both provided in the MR inspection room **4**. Since the two-wire filter **203** is provided on the cables **201** and **202**, can remove noise, if any, in the MRI waves before the MRI microwaves are transmitted from the power supply **204** to the MR inspection room **4**, while attenuating the therapeutic microwaves. The MRI tomogram is therefore free from the influence of the noise in the MRI waves. This makes it possible to carry out microwave therapy and MR imaging at the same time.

[0231] A therapeutic system according to the eighteenth embodiment of the invention will be described with reference to FIG. 37A. The eighteenth embodiment differs from the seventeenth embodiment (FIGS. 35 and 36), only in the operating characteristic of the two-wire filter **203**. In the eighteenth embodiment, the two-wire filter **203** provided on the cables **201** and **202** operates as a band-pass filter (BPF), not as a low-pass filter as in the seventeenth embodiment. As can be understood from FIG. 37A, the filter **203** transmits the MRI microwaves having frequency f_2 and attenuates the therapeutic microwaves having frequencies similar to frequency f_1 .

[0232] Thanks to the use of a single filter, i.e., the two-wire filter **203** functioning as a band-pass filter, the microwave therapy and the MR imaging can be performed at the same time, regardless of the frequency f_2 of the MRI waves.

[0233] A therapeutic system according to the nineteenth embodiment of this invention will be described with reference to FIG. 37B. The nineteenth embodiment differs from the seventeenth embodiment (FIGS. 35 and 36), only in the operating characteristic of the two-wire filter **203**. In the nineteenth embodiment, the two-wire filter **203** provided on the cables **201** and **202** operates as a band-cut filter (BCF), not as a low-pass filter as in the seventeenth embodiment. As can be understood from FIG. 37B, the filter **203** attenuates only the therapeutic microwaves having frequency f_1 .

[0234] Thanks to the use of a single filter, i.e., the two-wire filter **203** functioning as a band-cut filter, the microwave therapy and the MR imaging can be performed at the same time, regardless of the frequency f_1 of the therapeutic microwaves. The two-wire filter **203** can remove noise, if any, in therapeutic microwaves which have harmonic components such as pulse-shaped components.

[0235] FIG. 38 shows a therapeutic system according to the twentieth embodiment of the present invention. This

system comprises a microwave applicator **15**, a diagnostic ultrasonic probe **212**, a coaxial cable **213**, a microwave generator **214**, and an ultrasonic imaging apparatus **215**. The microwave applicator **15** is used as a therapeutic applicator for applying therapeutic energy to an affected tissue. The diagnostic ultrasonic probe **212** is connected to the microwave applicator **15** and serves as observation means for detecting the position of the microwave applicator **15**. The coaxial cable **213** connects the applicator **15** to the microwave generator **214**. The diagnostic ultrasonic probe **212** is connected to the ultrasonic-wave imaging apparatus **215**.

[0236] The system further comprises a coaxial filter **216**, which is provided on the coaxial cable **213**. The coaxial filter **216** operates as a high-pass filter. Its threshold frequency is lower than the intermediate frequency of the therapeutic microwaves and higher than the ultrasonic waves used in the ultrasonic imaging apparatus **215**.

[0237] In the twentieth embodiment, the coaxial filter **216**, which operates as a high-pass filter, is provided on the coaxial cable **213** which connects the microwave applicator **15** to the microwave generator **214**. The filter **216** therefore removes noise which may adversely influence the ultrasonic imaging performed by the ultrasonic imaging apparatus **215**, without attenuating the therapeutic microwaves supplied from the microwave generator **214** to the microwave applicator **15**. Hence, the ultrasonic imaging apparatus **215** can generate a clear ultrasonic image even if the ultrasonic imaging and the microwave therapy are carried out at the same time, by means of the probe **212** and the applicator **15**, respectively.

[0238] The coaxial filter **216** may be replaced by a band-pass filter that has the operating characteristic shown in FIG. 34A, or by a band-cut filter that has the operating characteristic shown in FIG. 34B.

[0239] FIG. 39 shows a therapeutic system, which is the twenty-first embodiment of the present invention. This therapeutic system comprises a diagnostic ultrasonic probe **212**, an ultrasonic imaging apparatus **215**, a resectoscope **221**, and a two-wire high-frequency wave generator **224**. The resectoscope **221** is used as a therapeutic applicator for applying therapeutic energy to an affected tissue. The diagnostic ultrasonic probe **212** is similar to its counterpart of the twentieth embodiment (FIG. 38).

[0240] The resectoscope has a slender insertion section **222**, which can be inserted into a body cavity of a patient. The insertion section **222** contains a loop electrode **223**. A high-frequency output is supplied to the loop electrode **223** from the two-wire high-frequency wave generator **224**.

[0241] Two cables **225** and **226** are connected at one end to the high-frequency wave generator **224**. The loop electrode **223** provided in the resectoscope **221** is connected to the cable **225**. The high-frequency generator **224** incorporates a return electrode (not shown), which is connected to the cable **226**.

[0242] A two-wire filter **227** is provided on the cables **225** and **226**, which supply the therapeutic energy to the resectoscope **221** from the two-wire high-frequency wave generator **224**. The filter **227** operates as a low-pass filter having a threshold frequency that is lower than the frequency of the therapeutic high-frequency waves and higher than the frequency of the ultrasonic imaging waves.

[0243] To perform ultrasonic imaging and high-frequency wave therapy, the diagnostic ultrasonic probe 212 and the insertion section 222 of the resectoscope 221 are inserted into, for example, the rectum Hh and urethra Hi of the patient, respectively, as is illustrated in FIG. 39.

[0244] As indicated above, the two-wire filter 227 functioning as a low-pass filter is provided on the two cables 225 and 226 that supply the therapeutic energy from the generator 224 to the resectoscope 221. Hence, the filter 227 can remove noise in the therapeutic high-frequency waves, without attenuating the therapeutic waves similar to sine waves, before the loop electrode 223 approaches the diagnostic ultrasonic probe 212. As a result, the ultrasonic imaging apparatus 215 can generate a clear ultrasonic image even if the ultrasonic imaging and the high-frequency wave therapy are carried out at the same time, by means of the probe 212 and the applicator 15, respectively.

[0245] The twenty-first embodiment is not limited to a system, wherein a resectoscope is employed as therapeutic applicator. Rather, it may be applied to a system in which any other therapeutic applicator that applies high-frequency energy to accomplish therapy, while an ultrasonic imaging apparatus is operating.

[0246] FIG. 40 shows a therapeutic system according to the twenty-second embodiment of this invention. The twenty-second embodiment is different from the twenty-first embodiment (FIG. 39) in two respects only. First, a paracetic bipolar electrode 231 is used in place of the resectoscope 221. Secondly, an ultrasonic probe 212 for use in combination with a raparoscope. The twenty-second embodiment can achieve the same advantage as the twenty-first embodiment.

[0247] A therapeutic system according to the twenty-third embodiment of the invention will be described, with reference to FIG. 41. The twenty-third embodiment differs from the fourteenth embodiment (FIGS. 31 to 33) in the following respects.

[0248] A terminal board 242 is fitted in a sidewall of the MR inspection room 4, i.e. the magnetic shield room for use in MR imaging, and a coaxial noise filter 243 is mounted on the terminal board 242. The coaxial noise filter 243 is provided on a microwave relay cable 16 (i.e., a coaxial cable), which connects the microwave applicator 15 and the microwave generator (e.g., magnetron) which are provided in the MR inspection room 4 and the microwave oscillator 17, respectively. The filter 243 is either a band-pass filter or a high-pass filter, which transmits the MRI waves used in the MRI apparatus 3 to generate MR images.

[0249] As described above, the noise filter 243 is provided on the microwave relay cable 16. Therefore, the microwave therapy and the MRI imaging can be carried out at the same time, irrespective of the frequency of the microwaves generated by the microwave generator.

[0250] A therapeutic system, which is the twenty-fourth embodiment of the invention, will be described with reference to FIG. 42. The therapeutic applicator used in this embodiment is a resectoscope 221 having a loop electrode 223, as in the twenty-first embodiment (FIG. 39). And a diagnostic ultrasonic probe 212 is used as observation means for detecting the position of the resectoscope 221.

[0251] In the twenty-fourth embodiment, a terminal board 242 is fitted in a side wall of the MR inspection room 4 (i.e. the magnetic shield room for use in MR imaging), as in the twenty-third embodiment (FIG. 41). A two-wire noise filter 251 is mounted on the terminal board 242. The filter 251 is provided on two cables 225 and 226 for supplying therapeutic energy from a high-frequency generator 224, as in the twenty-first embodiment (FIG. 39). The filter 251 is either a band-pass filter or a high-pass filter, which transmits the MRI waves used in the MRI apparatus 3 to generate MR images.

[0252] As described above, the noise filter 251 is provided on the two cables 225 and 226. Therefore, the microwave therapy and the MRI imaging can be carried out at the same time, irrespective of the frequency of the output frequency of the high-frequency generator 224.

[0253] FIGS. 43 to 47 show a therapeutic system 261, which is the twenty-fifth embodiment of the present invention. FIG. 43 schematically depicts this therapeutic system 261. As shown in FIG. 43, the system 261 comprises an MRI apparatus 262 and a therapeutic apparatus 263. The MRI apparatus 262 comprises an MRI gantry 264 and an MRI controller 265, which are connected by an MRI signal cable 266. The therapeutic apparatus 263 comprises a therapeutic energy generator 268 and a therapeutic probe 270 (see FIG. 44). The therapeutic probe 270 is connected to the therapeutic energy generator 268 by a cable 269.

[0254] The MRI apparatus 262 further comprises an observation unit 271, which is provided between the MRI controller 265 and the therapeutic energy generator 268. The observation unit 271 is connected to the MRI controller 265 by a signal cable 272 and to the therapeutic energy generator 268 by a signal cable 273. In the therapeutic system 261, a doctor operates the therapeutic apparatus 263, performing therapy, while observing the MRI image generated by the MRI apparatus 262.

[0255] As shown in FIG. 46, the MRI controller 265 comprises an MRI control section 274 and an image signal output section 275. The input of the MRI control section 274 is connected to the MRI gantry 264 by the MRI signal cable 266. The output of the MRI control section 274 is connected to the image signal output section 275.

[0256] As FIG. 46 shows, the therapeutic energy generator 268 comprises a therapeutic energy control section 276, a therapeutic energy generating section 277, and a signal input/output section 278. The therapeutic energy generating section 277 is connected to the therapeutic probe 270 by the cable 269.

[0257] The observation unit 271 comprises a control section 279, a signal input/output section 280, an image signal input unit 281, a display section 282, a measuring-points setting section 283, a reference luminance setting means 284 and an indicator means 285. The signal input/output section 280, image signal input unit 281, display section 282, measuring-points setting section 283, reference luminance setting means 284 and indicator means 285 are connected to the control section 279. The image signal input unit 281 is connected to the image signal output section 275 of the MRI controller 265 by the signal cable 272. The signal input/output section 280 is connected to the signal input/output section 278 of the therapeutic energy generator 268

by the signal cable 273. The display section 282 incorporates a monitor 267 for displaying an MR image.

[0258] The measuring-points setting section 283 is connected to an input device (not shown) such as a keyboard, a mouse, a track ball, a touch pen, or the like. As the input device is operated, the section 283 sets four measuring points (a) to (d) in the MR image generated by the MRI apparatus 262, around the image H_j of the affected region as is illustrated in FIG. 44. Luminance is measured at the measuring points (a) to (d). The display section 282 of the observation unit 271 displays the luminances at these points (a) to (d), as is shown in FIG. 45.

[0259] The input device (e.g., keyboard, mouse, track ball, touch pen, or the like) is connected to the reference luminance setting means 284, too. As the input device is operated, the means 284 sets a reference luminance value L_s for each measuring point. When the luminances at all points (a) to (d) exceed the reference luminance values, the observation unit 271 outputs a therapy stop signal to the therapeutic energy generator 268, which stops generating therapeutic energy.

[0260] The therapeutic system 261, i.e., the twenty-fifth embodiment of the invention, will be described with reference to the flow chart of FIG. 47.

[0261] In Step S71, the MRI apparatus 262 is operated, generating an MRI image before the therapeutic probe 270 is operated to perform therapy. Then, in Step S72, the MRI controller 265 transfers an image signal to the observation unit 271. In Step S73, the display section 282 of the observation unit 271 displays the MR image generated by the MRI apparatus 262.

[0262] Thereafter, in Step S74, a doctor operates the input device (e.g., keyboard, mouse, track ball, touch pen, or the like) while observing the MR image displayed on the screen of the display section 282. The measuring-points setting section 283 of the observation unit 271 sets four measuring points (a) to (d) in the MR image, around the image H_j of the affected region as is illustrated in FIG. 44. In Step S75, the doctor operates the input device again, while observing the MRI image displayed on the screen of the display section 282. Therefore, the reference luminance setting means 284 sets a reference luminance value L_s for each measuring point.

[0263] Therapy is then started in Step S76. More specifically, the therapeutic energy generator 268 supplies a therapy start signal to the observation unit 271 in Step S77. In Step S78, the MRI apparatus 262 generates an MRI image. In Step S79, the MRI controller 265 transfers an image signal to the observation unit 271.

[0264] In Step S80, the luminance at each measuring point is measured and displayed as shown in FIG. 45. In Step S81, it is determined whether all luminances at the points (a) to (d) exceed the reference luminance values L_s, respectively. If NO, the operation returns to Step S78. If YES, the therapy is terminated in Step S82. In Step S83, the indicator means 285 of the observation unit 271 is operated, indicating that the therapy has been terminated.

[0265] As the therapy proceeds, the colors of the parts of the MR image, which are at the measuring points (a) to (d), change from white to black or vice versa, for example,

depending on the parameters which have been set. Hence, the colors of these parts of the MR image change to either black or white when the luminances at all measuring points (a) to (d) exceed the reference luminance values L_s, respectively.

[0266] In the twenty-fifth embodiment, the input device (e.g., keyboard, mouse, track ball, touch pen, or the like) is operated, setting four measuring points (a) to (d) in the MR image, around the image H_j of the affected region as is illustrated in FIG. 44. The input device is operated again, setting four reference luminance values L_s for the measuring points (a) to (d), respectively. When the luminances at all measuring points exceed the reference values L_s, respectively, the therapeutic energy generator 268 stops applying therapeutic energy to the affected region. Thus, the therapy is automatically terminated when the luminances at all measuring points exceed the reference values L_s. The influence of the therapy energy on the living tissues in the patient is therefore minimized. When the luminances at all measuring points exceed the reference values L_s, it is known that the therapy has been thoroughly achieved on the entire affected region. This is because the four measuring points (a) to (d) surround the image H_j of the affected region.

[0267] With the therapeutic system according to the twenty-fifth embodiment, it is possible to perform the MR imaging (i.e., providing an MRI tomogram by means of the MRI apparatus 262) and the therapy (i.e., applying therapy energy by means of the probe 270), either at the same time or alternately.

[0268] A therapeutic system according to the twenty-sixth embodiment of this invention will be described, with reference to the flow chart of FIG. 48. The twenty-sixth embodiment differs from the twenty-fifth embodiment (FIGS. 43 to 47) only in the steps of operation which are carried out after the completion of therapy.

[0269] In the twenty-sixth embodiment, Steps S71 to S83 are carried out in the same order as in the twenty-fifth embodiment (see the flow chart of FIG. 47). After the indicator means 285 informs, in Step S83, that the therapy should be terminated, the observation unit 271 supplies a therapy end signal to the therapeutic energy generator 268 in Step S84. In Step S85, the generator 268 stops applying therapeutic energy to the affected region, whereby the therapy is terminated. More precisely, the therapeutic probe 270 stops applying the energy in response to the therapy end signal. Alternatively, the therapy energy applied from the probe 270 may be decreased in response to the therapy end signal, thereby to terminate the therapy automatically.

[0270] In the twenty-sixth embodiment, the probe 270 stops applying the therapy energy or the therapy energy applied from the probe 270 is decreased when the affected region is thoroughly treated. In other words, the therapy is automatically terminated the moment the affected region is completely treated. The influence of the therapy energy on the living tissues in the patient is therefore minimized.

[0271] A therapeutic system according to the twenty-seventh embodiment of the invention will be described, with reference to FIGS. 49 and 50. This embodiment differs from the twenty-fifth embodiment (FIGS. 43 to 47) in that a luminance ratio setting means 291 is provided in the observation unit 271. The therapeutic system 261 is operated, as will be explained with reference to the flow chart of FIG. 50.

[0272] As can be understood from **FIGS. 47 and 50**, Steps **S71** to **S75** are performed in the same order as in the twenty-fifth embodiment. After the doctor operates the input device (e.g., keyboard, mouse, track ball, touch pen, or the like), thus setting four reference luminance values **Ls** for the measuring points (a) to (d), respectively, in Step **S75**, the operation goes to Step **S91**.

[0273] In Step **S91**, the doctor operates the input device again, whereby the luminance ratio setting means **291** sets four luminance ratios for the measuring points (a) to (d), respectively. Each of the luminance ratios, thus set, is the ratio of a maximum luminance to the reference luminance **Ls** set for that measuring point. The maximum luminance is a value experimentally obtained, which that part of the MR image has at the measuring point when the affected region is completely treated.

[0274] Thereafter, in Step **S76**, the therapy is started as in the twenty-fifth embodiment. Then, Steps **77** to **S80** are carried out in the same order as in the twenty-fifth embodiment. After the luminances at the measuring points (a) to (d) have been measured and displayed in Step **S80**, the operation goes to Step **S92**.

[0275] In Step **S92**, it is determined whether the ratio of the luminance at each measuring point to the reference luminance **Ls** set for the point has exceeded the luminance ratio set for the point in Step **S91**. If NO, the operation returns to Step **S78**. If YES in Step **S92**, the therapy is terminated in Step **S82**. In Step **S83**, the indicator means **285** of the observation unit **271** is operated, indicating that the therapy has been terminated.

[0276] The twenty-seventh embodiment is advantageous in that the affected region would not be treated excessively at all. This is because the therapy on the affected region is automatically terminated when it is determined that the ratio of the luminance at each measuring point to the reference luminance **Ls** set for the point has exceeded the luminance ratio set for the point.

[0277] In the twenty-seventh embodiment, a therapy end signal may be supplied to the therapeutic energy generator **268** as in the twenty-sixth embodiment (**FIG. 48**). In response to the therapy end signal, the generator **268** stops applying therapeutic energy to the affected region. Alternatively, the therapy energy applied from the probe **270** may be decreased in response to the therapy end signal.

[0278] A therapeutic system according to the twenty-eighth embodiment of the invention will be described, with reference to **FIG. 51**. The twenty-eighth embodiment differs from the twenty-fifth embodiment (**FIGS. 43 to 47**) in the operation prior to the therapy accomplished by the use of the therapeutic probe **270**.

[0279] As can be understood from **FIGS. 47 and 51**, Steps **S71** to **S73** are performed in the same order as in the twenty-fifth embodiment. After the display section **282** of the observation unit **271** displays the MR image in Step **S73**, the operation goes to Step **S101**. In Step **S101**, the MRI image displayed by the display section **282** is analyzed, thereby identifying the image **Hj** of the affected region and setting four measuring points (a) to (d) around the image **Hj** of the affected region. Then, in Step **S102**, the measuring-points setting section **283** sets additional measuring points around the image **Hj**, and the positions of the points (a) to

(d) automatically set are adjusted. Thereafter, the operation goes to Step **S75**. Steps **S75** to **S83** are performed in the same order as in the twenty-fifth embodiment.

[0280] The twenty-eighth embodiment is advantageous in that the MRI apparatus **261** and the therapeutic probe **270** can be operated easily at the same time. This is because the image **Hj** of the affected region is automatically identified by analyzing the MR image displayed by the display section **282**, and the measuring points (a) to (d) are then set around the image **Hj** of the affected region.

[0281] A therapeutic system according to the twenty-ninth embodiment of the invention will be described, with reference to **FIG. 52**. The twenty-ninth embodiment differs from the twenty-seventh embodiment (**FIGS. 49 to 50**) in the operation after the therapy accomplished by the use of the therapeutic probe **270**.

[0282] As can be understood from **FIGS. 50 and 52**, Steps **S71** to **S92** are performed in the same order as in the twenty-seventh embodiment. If it is determined in Step **S92** that the ratio of the luminance at each measuring point to the reference luminance **Ls** set for the point has exceeded the luminance ratio set for the point, the operation goes to Step **S111**.

[0283] In Step **S111**, the indicator means **285** of the observation unit **271** is operated, indicating that the therapy should be terminated. The operation then goes to Step **S81** that is identical to Step **S81** shown in the flow chart of **FIG. 47** that explains the operation of the twenty-fifth embodiment (**FIGS. 43 to 47**). In Step **S81**, it is determined whether all luminances at the points (a) to (d) exceed the reference luminance values **Ls**, respectively. If NO, the operation returns to Step **78**. If YES, the therapy is terminated in Step **S82**.

[0284] Then, in Step **S112**, the observation unit **271** supplies a therapy end signal to the therapeutic energy generator **268**. In Step **S113**, the generator **268** stops applying therapeutic energy to the affected region, whereby the therapy is terminated. More precisely, the therapeutic probe **270** stops applying the energy in response to the therapy end signal. Alternatively, the therapy energy applied from the probe **270** may be decreased in response to the therapy end signal, thereby to terminate the therapy automatically.

[0285] The twenty-ninth embodiment described above is advantageous in that the therapy is automatically terminated in safety. This is because the indicator means **285** is operated, indicating that the therapy should be terminated, when it is determined that the ratio of the luminance at each measuring point to the reference luminance **Ls** set for the point has exceeded the luminance ratio set for the point. Then, the therapeutic energy generator **268** stops applying therapeutic energy to the affected region.

[0286] **FIGS. 53 to 55** show a therapeutic system, which is the thirtieth embodiment of the present invention. The thirtieth embodiment differs from the twenty-fifth embodiment (**FIGS. 43 to 47**) in the following respects.

[0287] As shown in **FIG. 54**, the observation unit **271** has an additional component, i.e., a reference point setting means **301**. The reference point setting means **301** is designed to set a reference point **R** in the MR image generated by the MRI apparatus **262**, while the measuring-

points setting section **283** sets four measuring points (a) to (d). Furthermore, the reference luminance values **Ls** are not set for the four measuring points (a) to (d) as in the twenty-fifth embodiment. Instead, a luminance ratio setting means **302** sets ratio of each reference luminance value **Ls** to the reference luminance value for the reference point **R**.

[0288] As shown in **FIG. 53**, the reference point **R** is set in the MR image **Hk** of a region that surrounds the image **Hj** of the affected region and that is supposed to be not influenced by the therapeutic energy applied from the probe **270**. The therapeutic system is operated as will be explained below, with reference to the flow chart of **FIG. 55**.

[0289] As can be understood from **FIGS. 47 and 55**, Steps **S71** to **S74** are performed in the same order as in the twenty-fifth embodiment (**FIGS. 43 to 47**). After the four measuring points (a) to (d) have been set around the image **Hj** of the affected region as shown in **FIG. 53**, the operation goes to Step **S121**. In Step **S121**, the input device (e.g., keyboard, mouse, track ball, touch pen, or the like) is operated, whereby the reference point setting means **301** sets a reference point **R** in the image **Hk** as is illustrated in **FIG. 53**. In Step **S122**, the input device (not shown) is operated again, whereby the luminance ratio setting means **302** sets the ratios of the four reference luminance values **Ls** set for the measuring points (a) to (d) to the reference luminance value set for the reference point **R**.

[0290] Thereafter, in Step **S76**, the therapy is started in the same way as in the twenty-fifth embodiment. Steps **S76** to **S80** are carried out in the same order as in the twenty-fifth embodiment. After the luminances at the four measuring points (a) to (d) are measured and displayed in Step **S80**, the operation goes to Step **S123**.

[0291] In Step **S123**, it is determined whether all four luminance ratios set by the luminance ratio setting means **302** have exceeded a prescribed value or not. If **NO**, the operation returns to Step **S78**. If **YES**, the operation goes to Step **S82**, in which the therapy is terminated. In Step **S83**, the indicator means **285** informs that the therapy has been terminated.

[0292] The thirtieth embodiment is advantageous in that the termination of therapy is reliably recognized. This is because The reference point setting means **301** sets a reference point **R** in the MR image generated by the MRI apparatus **262**, and the luminance ratio setting means **302** sets the ratios of the four reference luminance values **Ls** to the reference luminance value set for the reference point **R**. Thus, the influence of individual differences or MRI parameters on the luminance at each measuring point can be compensated for.

[0293] **FIGS. 56 and 57** show a therapeutic system according to the thirty-first embodiment of the present invention. This embodiment differs from the thirtieth embodiment in the following respects.

[0294] As shown in **FIG. 56**, the observation unit **271** incorporates a memory means **311**, instead of the reference point setting means **301**. The memory means **311** is provided for storing the initial values of the luminances at the measuring points (a) to (d).

[0295] The operation of the thirty-first embodiment will be explained, with reference to the flow chart of **FIG. 57**.

[0296] As can be understood from **FIGS. 47 and 57**, Steps **S71** to **S75** are performed in the same order as in the twenty-fifth embodiment (**FIGS. 43 to 47**). After the reference luminance value **Ls** for the four measuring points (a) to (d) have been set in Step **S75**, the operation goes to Step **S131**. In Step **S131**, the initial luminance values **Ls** set for the points (a) to (d) are stored into the memory means **311**.

[0297] Then, the therapy is started in Steps **S76** in the same way as in the thirtieth embodiment. Steps **S77** to **S80** are carried out in the same order as in the thirtieth embodiment. After the luminances at the four measuring points (a) to (d) are measured and displayed in Step **S80**, the operation goes to Step **S132**. In Step **S132**, it is determined whether all four ratios of the luminances at the measuring points (a) to (d) to the initial values stored in the memory means **311** have exceeded a prescribed value or not. If **YES**, the operation goes to Step **S82**, in which the therapy is terminated. In this case, the indicator means **285** informs, in Step **S83**, that the therapy has been terminated. If **NO** in Step **S132**, the operation returns to Step **S78**, whereby Steps **S78**, **S79**, **S80** and **S132** are repeated.

[0298] In the thirty-first embodiment described above, the memory means **311** stores the initial luminance values **Ls** set for the points (a) to (d). The therapy is terminated when the ratios of the luminances at the points (a) to (d) set around the image **Hj** of the affected region, to the initial values stored in the memory means **311** have exceeded a prescribed value. Therefore, the thirty-first embodiment attains the same advantage as the thirtieth embodiment. In addition, the thirty-first embodiment can be used to perform therapy on an organ so small that the reference point **R** can hardly set in an MR image generated by the MRI apparatus **262**.

[0299] **FIGS. 58 and 59** show a therapeutic system according to the thirty-second embodiment of the present invention. This embodiment differs from the thirty-first embodiment in the following respects.

[0300] As shown in **FIG. 58**, the observation unit **271** incorporates a luminance-change rate setting means **321** and a luminance-change rate calculating means **322**, instead of the luminance ratio setting means **302**. Whether or not the therapy has should be terminated is determined in accordance with the luminance-change rates at the measuring points (a) to (d). The decision is not made in accordance with the luminances measured at the points (a) to (d) as in the thirty-first embodiment.

[0301] The operation of the thirty-second embodiment will be explained, with reference to the flow chart of **FIG. 59**. Steps **S71** to **S74** are carried out in the same order as in the twenty-fifth embodiment (**FIGS. 45 to 47**). After the four measuring points (a) to (d) have been set around the image **Hj** of the affected region, the operation goes to Step **S141**. In Step **S141**, the input device (e.g., keyboard, mouse, track ball, touch pen, or the like) is operated, whereby the luminance-change rate setting means **321** sets four luminance-change rates for the measuring points (a) to (d), respectively.

[0302] Thereafter, in Step **S76**, the therapy is started in the same way as in the twenty-fifth embodiment. Steps **S77** to **S80** are then performed in the same order as in the twenty-fifth embodiment. After the luminances at the four measuring points (a) to (d) are measured and displayed in Step **S80**, the operation goes to Step **S142**. In Step **S142**, the lumi-

nances at the points (a) to (d) are stored into the memory means 311. In Step S143, the luminance-change rate calculating means 322 calculates the luminance-change rates at the points (a) to (d). In Step S144, it is determined whether all luminance-change rates calculated are smaller than the four luminance-change rates that the luminance-change rate setting means 321 has set for the measuring points (a) to (d). If NO, the operation returns to Step S78. In this case, Steps S78 to S80 and Steps S141 to S143 are repeated. If YES in Step S144, the operation goes to Step S82, in which the therapy is terminated. In Step S83, the indicator means 285 informs that the therapy has been terminated.

[0303] In the thirty-second embodiment described above, whether the therapy should be terminated is determined in accordance with the luminance-change rates at the measuring points (a) to (d), not in accordance with the luminances measured at the points (a) to (d). In this regard, it should be noted that the luminance at any point in the image Hj of the affected region will not change once the affected region has been heated, becoming completely void of water. This is why the luminance-change rates at the measuring points (a) to (d) are monitored in the thirty-second embodiment. The thirty-second embodiment is advantageous in that it can be reliably determined whether the living tissues present in the affected region have perished.

[0304] FIGS. 60 to 63 show a therapeutic system, which is the thirty-third embodiment of this invention. The present embodiment differs from the thirty-second embodiment (FIGS. 58 and 59) in the following respects.

[0305] As shown in FIG. 60, the observation unit 271 incorporates a reference line setting means 331, instead of the measuring-points setting section 283. The reference-line setting means 331 is designed to set a reference line Lb in the MR image generated by the MRI apparatus 262, as illustrated in FIG. 62. The reference line Lb extends in a given direction from the energy-emission center O of the therapeutic probe 270, from which therapeutic energy is applied to the affected region Hj. A plurality of measuring points are set on the reference line Lb and spaced at regular intervals. Luminances at these points are measured.

[0306] The operation of the thirty-third embodiment will be described with reference to the flow chart of FIG. 61.

[0307] As shown in FIG. 61, Steps S71 to S73 are carried out in the same order as in the twenty-fifth embodiment (FIGS. 45 to 47). After the display section 282 of the observation unit 271 displays the MR image in Step S73, the operation goes to Step S151. In Step S151, the input device (e.g., keyboard, mouse, track ball, touch pen, or the like) is operated, whereby the reference-line setting means 331 sets a reference line Lb in the RM image generated by the MRI apparatus 262. In Step S152, the input device (not shown) is operated again, whereby the luminance-change rate setting means 321 sets a luminance-change rate for the reference line Lb.

[0308] Then, in Step S76, the therapy is started in the same way as in the twenty-fifth embodiment. Steps S77 to S79 are then performed in the same order as in the twenty-fifth embodiment. After the MRI controller 265 transfers an image signal to the observation unit 271 in Step S79, the operation goes to Step S153.

[0309] In Step S153, the luminances at the measuring points on the reference line Lb are measured and displayed.

Then, in Step S154, the luminances measured at these measuring points are stored into the memory means 311. In Step S155, the luminance-change rate calculating means 322 calculates the luminance-change rates at the measuring points.

[0310] Next, in Step S156, it is determined whether all luminance-change rates calculated for all measuring points are smaller than the four luminance-change rates that the means 321 has set for the measuring points. If NO, the operation returns to Step S78. If YES in Step S156, the operation goes to Step S82, in which the therapy is terminated. In Step S83, the indicator means 285 informs that the therapy has been terminated.

[0311] FIG. 63 shows how the luminance changes along the reference line Lb set in the MR image generated by the MRI apparatus 262, during the therapy accomplished by the use of the therapeutic probe 270. In FIG. 63, the distance from the therapeutic probe 270 is plotted on the X axis, and the luminance on the Y axis. While the probe 270 applies the therapeutic energy, the luminance distribution changes with time as is indicated by curves P1 to P5. As can be understood from FIG. 63, the luminance stops increasing once it reaches a specific value. The display section 282 of the observation unit 271 displays the curves P1 to P5. Alternatively, the display section 282 may display the luminance-change rates at some measuring points on the reference line Lb, in the form of such a bar graph as is shown in FIG. 39.

[0312] As mentioned above, a reference line Lb is set which extends in a given direction from the energy-emission center O of the therapeutic probe 270 applying therapeutic energy to the affected region Hj, and luminance-change rates at some measuring points automatically set on the reference line Lb are measured. On the basis of the luminance-change rates measured it is determined whether or not the therapy should be terminated.

[0313] As the therapeutic probe 270 applies the therapeutic energy to the affected region Hj, the temperature in the region Hj gradually rises. Once the region Hj has become completely void of water, there are no longer changes in the water content in the affected region Hj. In other words, the luminance at any measuring point no longer change, however much energy is applied to the affected region Hj. Thus, it is reliably determined that the therapy should be terminated, because luminance-change rates are measured at some measuring points which have been automatically set on the reference line Lb extending from the energy-emission center O of the therapeutic probe 270.

[0314] FIGS. 64 to 66 show a therapeutic system according to the thirty-fourth embodiment of the present invention. The thirty-fourth embodiment differs from the thirty-third embodiment (FIGS. 60 to 63) in the following respects.

[0315] As shown in FIG. 64, the observation unit 271 incorporates a reference point setting means 341 and a reference luminance setting means 284, instead of the reference line setting means 331 and the luminance-change rate setting means 321.

[0316] The operation of the therapeutic system, which is the thirty-fourth embodiment, will be explained with reference to the flow chart of FIG. 65.

[0317] Steps S71 to S73 are carried out in the same order as in the twenty-fifth embodiment (FIGS. 45 to 47) and as

is illustrated in the flow chart of **FIG. 47**. After the display section **282** of the observation unit **271** displays the MR image in Step **S73**, the operation goes to Step **S161**. In Step **S161**, the input device (e.g., keyboard, mouse, track ball, touch pen, or the like) is operated, whereby the reference point setting means **341** sets a reference point **X1** in the image of the affected region.

[0318] Thereafter, in Step **S76**, the therapy is started as in the twenty-fifth embodiment. Steps **S77** to **S80** are then performed in the same order as in the twenty-fifth embodiment. In Step **S80**, the luminance at the reference point **X1** is measured. In Step **S163**, it is determined whether or not the luminance at the reference point **X1** has exceeded the reference level **V1** set by the luminance setting means **284**. If NO, the operation returns to Step **S78**. If YES, the operation goes to Step **S82**, the operation goes to Step **S83**. In Step **S83**, the indicator means **285** of the observation unit **271** informs that the therapy has been terminated.

[0319] As the therapeutic probe **270** applies the therapeutic energy to the affected region **Hj** (i.e., living tissues), heat propagates like ripples, from the energy-emission center **O** in the RMI tomogram of the affected region **Hj**. Therefore, it can be confirmed how much the affected region **Hj** has been treated, by comparing the reference level **V1** set by the luminance setting means **284** with the luminance at the reference point **X1** which is at a certain distance from the energy-emission center **O**.

[0320] Moreover, the display section **282** of the observation unit **271** displays the relation between the luminance measured at the point set by the reference point setting means **341** and the distance between this point and the energy-emission center **O**, as is illustrated in **FIG. 66**. It is therefore easy for a doctor to visually understand how much the affected region **Hj** has been treated. If the relation is represented by a curve **P1**, indicating that the luminance at distance **X1** is higher than the reference level **V1**, the doctor recognizes that the therapy can be continued. On the other hand, if the relation is represented by a curve **P2**, indicating that the luminance at distance **X1** is lower than the reference level **V1**, the doctor understands that the therapy should be terminated.

[0321] Thus, the thirty-fourth embodiment is advantageous in that the doctor can visually understand how much the affected region **Hj** has been treated, merely by looking at the luminance-distance curve displayed by the display section **282** of the observation unit **271**.

[0322] **FIGS. 67** to **69** show a therapeutic system according to the thirty-fifth embodiment of the invention. The thirty-fifth embodiment differs from the twenty-fifth embodiment (**FIGS. 45** to **47**) in the following respects.

[0323] As shown in **FIG. 67**, an ultrasonic imaging apparatus **215** is provided, instead of the MRI apparatus **262**, for detecting the position of the therapeutic probe **270**. The ultrasonic imaging apparatus **215** is, for example, of the same type as the one used in the twenty-second embodiment (**FIG. 40**).

[0324] As shown in **FIG. 68**, the ultrasonic imaging apparatus **215** comprises an ultrasonic imaging section **351** and an image signal output section **352**. A diagnostic ultrasonic probe **212** is connected to the input of the ultrasonic imaging section **351**. The image signal input unit **281** of the

observation unit **271** is connected to the image signal output section **352** by the signal cable **353**.

[0325] The therapeutic system shown in **FIG. 67** is operated as will be described below, with reference to the flow chart of **FIG. 69**.

[0326] First, the diagnostic ultrasonic probe **212** generates an ultrasonic image in Step **S171**, prior to the therapy performed by means of the therapeutic probe **270**. In Step **S172**, the image signal representing the ultrasonic image is transferred from the ultrasonic imaging apparatus **215** to the observation unit **271**. In Step **S173**, the display section **282** of the observation unit **271** displays the ultrasonic image the ultrasonic probe **212** has generated.

[0327] Thereafter, in Step **S174**, the doctor operates the input device (e.g., keyboard, mouse, track ball, touch pen, or the like), while observing the ultrasonic image displayed on the screen of the display section **282** of the observation unit **271**. As a result, the measuring-points setting section **283** of the observation unit **271** sets four measuring points (a) to (d) in the ultrasonic image, around the image **Hj** of the affected region as is illustrated in **FIG. 44**. In Step **S175**, the doctor operates the input device again, while observing the ultrasonic image, setting four reference luminance values **Ls** for the measuring points (a) to (d), respectively.

[0328] In Step **S176**, the therapy is started. More precisely, the therapeutic energy generator **268** supplies a therapy start signal to the observation unit **271** in Step **S177**. In Step **S178**, the ultrasonic image the ultrasonic probe **212** applies ultrasonic waves, whereby the ultrasonic imaging apparatus **215** transfers an image signal to the observation unit **271**.

[0329] In Step **S180**, the luminances at the four measuring points (a) to (d) are monitored. In Step **S181**, it is determined whether the luminances have exceeded the reference values **Ls**, respectively. If NO, the operation returns to Step **S178**. If YES, the operation goes to Step **S182**, in which the therapy is terminated. Then, in Step **S183**, the indicator means **285** of the observation unit **271** informs that the therapy has been terminated.

[0330] In the thirty-fifth embodiment, the therapy is automatically terminated in the same way as in the twenty-fifth embodiment. The influence of the therapy energy on the living tissues in the patient is therefore minimized. Further, the affected region can be reliably treated in its entirety, because the therapy is terminated when the luminances exceed the reference luminances **Ls** at the four measuring points (a) to (d) set around the image **Hj** of the affected region.

[0331] In the thirty-fifth embodiment, the ultrasonic imaging apparatus **215** of the same type as the one incorporated in the twenty-second embodiment (**FIG. 40**) is used as an observation means for detecting the position of the therapeutic applicator. The ultrasonic imaging apparatus **215** can be used in the other embodiments, as well.

[0332] Utilizing a component or components of any other embodiment can modify each of the embodiments described above. For instance, in the therapeutic system according to the thirty-fifth embodiment (**FIGS. 67** to **69**), that incorporates the ultrasonic imaging apparatus **215**, the therapeutic energy generator **268** may be automatically turn on and off as in the twenty-sixth embodiment (**FIG. 48**).

[0333] The present invention is not limited to the embodiments described above. Various changes and modifications can be made, without departing the scope of the present invention.

[0334] Additional advantages and modifications will readily occur to those skilled in the art. Therefore, the invention in its broader aspects is not limited to the specific details and representative embodiments shown and described herein. Accordingly, various modifications may be made without departing from the spirit or scope of the general inventive concept as defined by the appended claims and their equivalents.

1. A therapeutic system comprising:

a therapeutic applicator adapted to be inserted into a body cavity, for applying therapeutic energy to treat living tissues present in the body cavity;

observation means for indicating a position which the therapeutic applicator takes in the body cavity; and

control means for controlling the therapeutic energy applied from the therapeutic applicator to the living tissues, on the basis of data representing the position which the therapeutic applicator takes in the body cavity.

2. A therapeutic system according to claim 1, wherein the observation means comprises image diagnostic apparatus capable of indicating the position of the therapeutic applicator, and the control means controls the therapeutic energy in accordance with a signal supplied from the image diagnostic apparatus.

3. A therapeutic system comprising:

an image diagnostic apparatus;

a therapeutic apparatus for applying therapeutic energy to an affected region; and

a control apparatus for supplying signals between the image diagnostic apparatus and the therapeutic apparatus.

4. A therapeutic system according to claim 3, wherein the control apparatus is designed to decrease an output of the therapeutic apparatus or inhibit the therapeutic apparatus from applying therapeutic energy, while the affected region is diagnosed by the use of the image diagnostic apparatus.

5. A therapeutic system according to claim 4, wherein the control apparatus is designed to cause the image diagnostic apparatus to display an image of the affected region for diagnostic purpose, after decreasing the output of the therapeutic apparatus or inhibiting the therapeutic apparatus from applying therapeutic energy.

6. A therapeutic system according to claim 3, wherein the control apparatus is designed to determine a rate at which the affected region is being treated, from changes in an image displayed by the image diagnostic apparatus, and to change various values set in the therapeutic apparatus in accordance with the rate thus determined.

7. A therapeutic system according to claim 3, wherein said image diagnostic apparatus comprises an MRI apparatus, and the control apparatus is designed to supply an MRI start signal and an MRI stop signal to the MRI apparatus.

8. A therapeutic system according to claim 7, wherein the control apparatus is designed to supply MRI parameters to the MRI apparatus.

9. A therapeutic system according to claim 7, wherein the control apparatus is designed to supply an MRI signal from the MRI apparatus.

10. A therapeutic system according to claim 3, wherein the control apparatus is designed to supply an output start signal, an output stop signal and a output-level setting signal to the therapeutic apparatus.

11. A therapeutic system according to claim 3, wherein said therapeutic apparatus has a therapeutic section adapted to contact living tissues, and the control apparatus is designed to supply a tissue-separating current to the living tissues to remove the tissues from the therapeutic section when the therapeutic apparatus stops applying the therapeutic energy.

12. A therapeutic system according to claim 3, wherein the image diagnostic apparatus comprises an MRI apparatus, the therapeutic apparatus has a therapeutic section adapted to contact living tissues, and the control apparatus is designed to decrease an output of the therapeutic apparatus or inhibit the therapeutic apparatus from applying therapeutic energy, while the affected region is diagnosed by the use of the image diagnostic apparatus, to cause the image diagnostic apparatus to display an image of the affected region for diagnostic purpose, after decreasing the output of the therapeutic apparatus or inhibiting the therapeutic apparatus from applying therapeutic energy, to determine a rate at which the affected region is being treated, from changes in an image displayed by the image diagnostic apparatus, and change various values set in the therapeutic apparatus in accordance with the rate thus determined, to supply an MRI start signal and an MRI stop signal to the MRI apparatus, to supply MRI parameters to the MRI apparatus, to supply an MRI signal from the MRI apparatus, to supply an output start signal, an output stop signal and a output-level setting signal to the therapeutic apparatus, and to supply a tissue-separating current to the living tissues to remove the tissues from the therapeutic section when the therapeutic apparatus stops applying the therapeutic energy.

13. A therapeutic system according to claim 12, wherein the therapeutic apparatus comprises a therapeutic applicator which is compatible with the MRI apparatus.

14. A therapeutic system comprising:

energy generating means for generating therapeutic energy;

a therapeutic applicator for applying the therapeutic energy generated by the energy generating means to treat living tissues;

tomogram generating means for generating a tomogram of an affected region;

an energy supplying path provided between the energy generating means and the therapeutic applicator;

a noise filter provided in the energy supplying path, for removing a frequency component that influences the tomogram generating means, from the therapeutic energy generated by the energy generating means.

15. A therapeutic system according to claim 14, wherein the energy generating means is a microwave generating apparatus

16. A therapeutic system according to claim 14, wherein the energy generating means is a high-frequency wave generating apparatus.

17. A therapeutic system according to claim 14, wherein the tomogram generating means is an MRI apparatus.

18. A therapeutic system according to claim 14, wherein the tomogram generating means is a n ultrasonic imaging apparatus.

19. An therapeutic system according to claim 14, wherein the noise filter is a band-pass filter which transmits waves having a main output frequency of the energy generating means.

20. A therapeutic system according to claim 14, wherein the noise filter is a band-cut filter which attenuates waves having an input frequency of the tomogram generating means.

21. A therapeutic system according to claim 14, wherein the noise filter a low-pass filter or a high-pass filter which transmits waves having a frequency lower than a main output frequency of the energy generating means and higher than an average of the main output frequency of the energy generating means and an input frequency of the tomogram generating means.

22. A therapeutic system according to claim 14, wherein the tomogram generating means comprises a magnetic shield room having an input section, and the noise filter is provided in the input section of the magnetic shield room.

23. A therapeutic system comprising:

energy generating means for generating therapeutic energy;

therapeutic means comprising a therapeutic electrode or a therapeutic applicator for applying the therapeutic energy from the energy generating means to living tissues present in an affected region, thereby to treat the living tissues, said therapeutic means having a plurality of position-indicating markers;

an image diagnostic apparatus having a display means for displaying a tomogram of the affected region; and

a control apparatus for detecting positions of the markers in the tomogram displayed by the display means and for controlling the energy generating means in accordance with the positions of the markers.

24. A therapeutic system according to claim 23, wherein the control apparatus causes the energy generating means to stop generating the therapeutic energy, when positional relation of the markers changes.

25. A therapeutic system according to claim 23, wherein the control apparatus causes the energy generating means to stop generating the therapeutic energy, when none of the markers is detected in the tomogram displayed by the display means.

26. A therapeutic system according to claim 23, wherein the control apparatus causes the energy generating means to stop generating the therapeutic energy, when an image signal representing a prescribed one of the markers changes.

27. A therapeutic system comprising:

energy generating means for generating therapeutic energy;

therapeutic means comprising a therapeutic electrode or a therapeutic applicator for applying the therapeutic energy from the energy generating means to living tissues present in an affected region, thereby to treat the living tissues, said therapeutic means having a plurality of position-indicating markers;

an image diagnostic apparatus having a display means for displaying a tomogram of the affected region;

drive means for moving the therapeutic means; and

a control unit for detecting the markers in the tomogram displayed by the display means and for controlling the energy generating means and the drive means in accordance with the positions of the markers.

28. A therapeutic system comprising:

energy generating means for generating therapeutic energy;

therapeutic means for applying therapeutic energy from the energy generating means to living tissues present in an affected region, thereby to treat the living tissues;

tomogram generating means for generating a tomogram of the affected region;

observation unit for setting measuring points or a reference line in the tomogram generated by the tomogram generating means and for determining how much the living tissues have been treated, from image data acquired at the measuring points or on the reference line.

29. A therapeutic system according to claim 28, wherein the observation unit has means for indicating how much the living tissues have been treated.

30. A therapeutic system according to claim 29, wherein the observation unit determines whether therapy should be terminated.

31. A therapeutic system according to claim 28, wherein the observation unit inhibits the energy generating means from generating the therapeutic energy or decreases the therapeutic energy generated by the energy generating means.

32. A therapeutic system according to claim 31, wherein the observation unit determines whether therapy should be terminated.

33. A therapeutic system according to claim 28, wherein the observation unit has manual setting means for setting the measuring points or the reference line when manually operated.

34. A therapeutic system according to claim 28, wherein the observation unit has automatic setting means for setting the measuring points or the reference line on the basis of tomogram data supplied from the tomogram generating means.

35. A therapeutic system according to claim 28, wherein the observation unit has means which uses, as image data values, the absolute values of luminances at the measuring points.

36. A therapeutic system according to claim 28, wherein the observation unit has means which sets a reference point in the tomogram and which uses, as image data values, the relative values of the luminances at the reference point and the measuring points.

37. A therapeutic system according to claim 28, wherein the observation unit has means which uses, as image data values, differences between the luminances measured at the measuring points before the therapeutic energy is applied and the luminances measured at the measuring points when the therapeutic energy is applied.

38. A therapeutic system according to claim 28, wherein the observation unit has means which uses, as image data values, the luminance-change rates measured at the measuring points.

39. A therapeutic system according to claim 28, wherein the observation unit is designed to determine that the image data values at all measuring points have reached threshold values, respectively.

40. A therapeutic system according to claim 28, wherein the observation unit is designed to set a plurality of measuring points in the tomogram and to determine that the image data values at all measuring points have reached threshold values set for the measuring points, respectively.

41. A therapeutic system according to claim 28, wherein the observation unit is designed to set a first group of measuring points and a second group of measuring points in the tomogram, to determine whether the image data values at the measuring points have reached threshold values, respectively, to determine and indicate that the image data values at the measuring points of the first group have reached the threshold values, and to inhibit the energy generating means from generating the therapeutic energy or decreases the therapeutic energy generated by the energy generating means, when determining that the image data values at the measuring points of the second group have reached the threshold values.

42. A therapeutic system according to claim 28, wherein the observation unit is designed to use, as image data values, the luminance-change rates measured at the measuring points.

43. A therapeutic system according to claim 28, wherein the observation unit is designed to set the measuring points by setting a reference line and distances from the reference line.

44. A therapeutic system comprising:

a therapeutic applicator adapted to be inserted into a body cavity, for applying therapeutic energy to treat living tissues present in the body cavity, said therapeutic applicator comprising a rod-shaped body and a conductor provided in the rod-shaped body and made of material having magnetic susceptibility of -10^{-3} to $+10^{-3}$; and

observation means for indicating a position which the therapeutic applicator takes in the body cavity.

45. A therapeutic system according to claim 44, wherein the therapeutic applicator has an MR marker made of

material which has magnetic susceptibility having an absolute value equal to or greater than magnetic susceptibility of the material of the rod-shaped body.

46. A therapeutic system according to claim 45, wherein the therapeutic applicator has a plurality of MR markers made of material which has magnetic susceptibility having an absolute value equal to or greater than magnetic susceptibility of the material of the rod-shaped body.

47. A therapeutic system according to claim 45, wherein the therapeutic applicator has an energy-applying section, and the MR marker is arranged on a distal portion of the energy-applying section.

48. A therapeutic system according to claim 45, wherein the therapeutic applicator has an energy-applying section, and the MR marker is arranged on a proximal portion of the energy-applying section.

49. A therapeutic system according to claim 46, wherein the therapeutic applicator has an energy-applying section, and the MR markers are arranged on a distal portion and proximal portion of the energy-applying section, respectively.

50. A therapeutic system according to claim 45, wherein the therapeutic applicator has an energy-applying section, and the MR marker is located at a distance of 10 mm or more from the energy-applying section in an axial direction thereof.

51. A method of controlling a therapeutic system comprising a therapeutic applicator adapted to be inserted into a body cavity, for applying therapeutic energy to treat living tissues present in the body cavity, and observation means for indicating a position which the therapeutic applicator takes in the body cavity, said method comprising the steps of:

generating an image of living tissues by the use of the observation means;

determining a position which the therapeutic applicator takes in the body cavity, from the image generated by the use of the observation means; and

controlling the therapeutic energy applied from the therapeutic applicator to the living tissues, on the basis of data representing the position which the therapeutic applicator determined.

* * * * *

专利名称(译)	治疗系统		
公开(公告)号	US20020016544A1	公开(公告)日	2002-02-07
申请号	US09/894723	申请日	2001-06-28
[标]申请(专利权)人(译)	奥林巴斯株式会社		
申请(专利权)人(译)	奥林巴斯光学CO.LTD.		
当前申请(专利权)人(译)	OLYMPUS CORPORATION		
[标]发明人	HAREYAMA NORIHIKO NAGASE TORU HATTA SHINJI		
发明人	HAREYAMA, NORIHIKO NAGASE, TORU HATTA, SHINJI		
IPC分类号	A61B18/12 A61B5/055 A61B6/12 A61B18/18 A61B19/00 A61N5/02		
CPC分类号	A61B5/055 A61B6/12 A61B18/18 A61B18/1815 A61B19/20 A61B19/201 A61B19/5244 A61B2019/5236 A61B2019/5276 A61B2019/5454 A61B34/20 A61B90/10 A61B90/11 A61B2090/374 A61B2090/378 A61B2090/3954		
优先权	1998077231 1998-03-25 JP		
其他公开文献	US7415301		
外部链接	Espacenet USPTO		

摘要(译)

一种治疗系统，包括用于治疗活组织的治疗施用器和用于确定施用器位置的观察单元。从施用器施加到活组织的治疗能量根据表示施用器位置的数据来控制，由观察单元确定。因此，即使同时使用涂抹器和观察单元（例如，MRI设备），也易于操作该系统。在使用治疗涂抹器期间，活组织的图像保持清晰。

