



US00RE46063E

(19) **United States**  
 (12) **Reissued Patent**  
**Regadas**

(10) **Patent Number:** **US RE46,063 E**  
 (45) **Date of Reissued Patent:** **Jul. 12, 2016**

(54) **POLYP REMOVAL DEVICE AND METHOD OF USE**

(71) Applicant: **Covidien LP**, Mansfield, MA (US)

(72) Inventor: **F. Sergio P. Regadas**, Fortaleza-Ceara (BR)

(73) Assignee: **COVIDIEN LP**, Mansfield, MA (US)

(21) Appl. No.: **14/561,461**

(22) Filed: **Dec. 5, 2014**

**Related U.S. Patent Documents**

Reissue of:

(64) Patent No.: **8,328,803**  
 Issued: **Dec. 11, 2012**  
 Appl. No.: **12/363,086**  
 Filed: **Jan. 30, 2009**

U.S. Applications:

(60) Provisional application No. 61/063,158, filed on Jan. 31, 2008.

(51) **Int. Cl.**  
**A61B 18/18** (2006.01)  
**A61B 17/24** (2006.01)  
**A61B 17/3205** (2006.01)  
**A61B 18/14** (2006.01)  
**A61B 17/221** (2006.01)

(Continued)

(52) **U.S. Cl.**  
 CPC ..... **A61B 17/32056** (2013.01); **A61B 18/14** (2013.01); **A61B 17/221** (2013.01); **A61B 17/24** (2013.01); **A61B 17/32** (2013.01); **A61B 18/18** (2013.01); **A61B 18/20** (2013.01); **A61B 2018/00345** (2013.01); **A61B 2018/00404** (2013.01); **A61B 2018/00482** (2013.01); **A61B 2018/00619** (2013.01); **A61B 2018/141** (2013.01); **A61B 2018/1407** (2013.01)

(58) **Field of Classification Search**

CPC ..... **A61B 18/00**; **A61B 2018/00571**;  
**A61B 2018/00607**

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

749,689 A 1/1904 Houghton  
 1,952,617 A 3/1934 Wappler

(Continued)

**FOREIGN PATENT DOCUMENTS**

DE 2415263 10/1975  
 DE 2415263 A1 10/1975

(Continued)

**OTHER PUBLICATIONS**

Japanese Office Action for Japanese Patent Application No. 2013-146277 dated Feb. 2, 2015.


(Continued)

*Primary Examiner* — Glenn K Dawson

(57) **ABSTRACT**

A device and system for removing tissue such as polyps is provided and includes a tubular member having proximal and distal ends, a snare portion operably extending from within the distal end of the tubular member and including first and second electrodes configured to treat tissue therebetween, the snare portion further including a cutting member for severing the treated tissue. The tissue removal device may further include a handle portion operatively extending from within the proximal end of the tubular member. The handle portion may be configured for operable engagement by a user and the cutting member may extend between distal ends of the first and second electrodes.

**14 Claims, 4 Drawing Sheets**

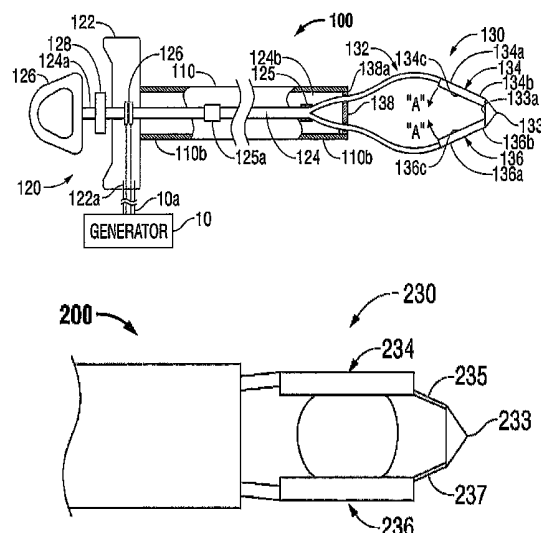

<i>A61B 17/32</i>	(2006.01)
<i>A61B 18/20</i>	(2006.01)
<i>A61B 18/00</i>	(2006.01)

## U.S. PATENT DOCUMENTS

1,963,636	A	6/1934	Wappler	
1,987,015	A	7/1934	Wappler	
2,002,559	A	5/1935	Wappler	
2,008,525	A	7/1935	Wappler	
2,054,149	A	9/1936	Charles .....	A61B 17/32056 606/113
2,442,966	A	6/1948	Wallace	
2,532,043	A	11/1950	Wallace	
3,149,633	A	9/1964	Zingale	
3,752,159	A	8/1973	Wappler	
3,856,015	A	12/1974	Iglesias	
4,011,872	A	3/1977	Komiya	
4,024,869	A	5/1977	Bonnet	
4,060,087	A	11/1977	Hiltebrandt et al.	
4,068,667	A	1/1978	Iglesias	
4,116,198	A	9/1978	Roos	
4,134,406	A	1/1979	Iglesias	
4,202,338	A	5/1980	Bitroff	
4,294,254	A	10/1981	Chamness	
4,311,143	A	1/1982	Komiya	
4,493,320	A	1/1985	Treat .....	A61B 18/14 606/47
4,503,855	A	3/1985	Maslanka	
4,718,419	A	1/1988	Okada	
4,733,662	A	3/1988	DeSatnick et al.	
4,905,691	A *	3/1990	Rydell .....	606/47
5,026,371	A	6/1991	Rydell et al.	
5,066,295	A	11/1991	Kozak et al.	
5,078,716	A	1/1992	Doll .....	606/47
5,192,280	A	3/1993	Parins	
5,197,964	A	3/1993	Parins	
5,207,686	A	5/1993	Dolgin	
5,290,284	A	3/1994	Adair	
5,318,564	A	6/1994	Eggers	
5,417,697	A	5/1995	Wilk et al.	
5,460,629	A	10/1995	Shlain et al.	
5,462,553	A	10/1995	Dolgin	
5,597,107	A	1/1997	Knodel et al.	
5,817,093	A *	10/1998	Williamson, IV et al. ....	606/50
5,971,994	A	10/1999	Fritzschn	
6,015,415	A	1/2000	Avellanet	
6,050,995	A *	4/2000	Durgin .....	606/47
6,071,283	A	6/2000	Nardella et al.	
6,152,922	A	11/2000	Ouchi	
6,235,026	B1	5/2001	Smith	
6,440,138	B1	8/2002	Reiley et al.	
6,517,539	B1	2/2003	Smith et al.	
6,730,097	B2	5/2004	Dennis	
6,743,228	B2	6/2004	Lee et al.	
6,773,432	B1	8/2004	Clayman et al.	
6,827,717	B2	12/2004	Brommersma et al.	
6,852,108	B2	2/2005	Barry et al.	
6,852,111	B1	2/2005	Lieber	
6,860,848	B2	3/2005	Wosnitza et al.	
6,972,017	B2	12/2005	Smith et al.	
7,008,420	B2	3/2006	Okada	
7,037,307	B2	5/2006	Dennis	
7,104,990	B2	9/2006	Jenkins et al.	
7,150,097	B2	12/2006	Sremcich et al.	
7,887,536	B2	2/2011	Johnson et al.	
8,016,827	B2	9/2011	Chojin	
8,114,122	B2	2/2012	Nau, Jr.	
8,133,254	B2	3/2012	Dumbauld et al.	
8,142,473	B2	3/2012	Cunningham	
8,162,965	B2	4/2012	Reschke et al.	
8,162,973	B2	4/2012	Cunningham	
8,197,479	B2	6/2012	Olson et al.	
8,226,650	B2	7/2012	Kerr	
8,251,994	B2	8/2012	McKenna et al.	

8,257,387	B2	9/2012	Cunningham	
8,277,446	B2	10/2012	Heard	
8,282,634	B2	10/2012	Cunningham et al.	
8,287,536	B2	10/2012	Mueller et al.	
8,303,582	B2	11/2012	Cunningham	
8,317,787	B2	11/2012	Hanna	
8,328,803	B2	12/2012	Regadas	
8,343,150	B2	1/2013	Artale	
8,357,159	B2	1/2013	Romero	
8,430,876	B2	4/2013	Kappus et al.	
8,439,911	B2	5/2013	Mueller	
8,469,956	B2	6/2013	McKenna et al.	
8,469,957	B2	6/2013	Roy	
8,486,107	B2	7/2013	Hinton	
8,535,312	B2	9/2013	Horner	
8,568,412	B2	10/2013	Brandt et al.	
8,623,017	B2	1/2014	Moses et al.	
8,632,539	B2	1/2014	Twomey et al.	
8,632,564	B2	1/2014	Cunningham	
8,636,761	B2	1/2014	Cunningham et al.	
8,679,115	B2	3/2014	Reschke	
8,795,274	B2	8/2014	Hanna	
2001/0009985	A1	7/2001	Durgin et al.	
2002/0013583	A1	1/2002	Camran et al.	
2002/0072739	A1	6/2002	Lee et al.	
2002/0151889	A1	10/2002	Swanson et al.	
2002/0165540	A1	11/2002	Bales et al.	
2003/0009166	A1	1/2003	Moutafis et al.	
2003/0040744	A1	2/2003	Latterell et al.	
2003/0109870	A1	6/2003	Lee et al.	
2003/0114850	A1	6/2003	McClurken et al.	
2003/0125731	A1	7/2003	Smith et al.	
2003/0144661	A1	7/2003	Brommersma et al.	
2003/0153909	A1	8/2003	Levinson	
2003/0176859	A1	9/2003	Levinson	
2003/0181906	A1	9/2003	Boebel et al.	
2003/0204188	A1	10/2003	Morrison et al.	
2003/0212389	A1	11/2003	Durgin et al.	
2003/0216731	A1	11/2003	Dennis	
2004/0064139	A1	4/2004	Yossepowitch	
2004/0106920	A1	6/2004	Jenkins et al.	
2004/0153059	A1	8/2004	Okada	
2004/0199159	A1	10/2004	Lee et al.	
2004/0220564	A1	11/2004	Ho et al.	
2005/0070889	A1	3/2005	Nobis et al.	
2005/0085808	A1	4/2005	Nakao	
2005/0096650	A1	5/2005	Ouchi	
2005/0119652	A1	6/2005	Vetter et al.	
2005/0131402	A1	6/2005	Ciarrocca et al.	
2005/0131403	A1	6/2005	Chang	
2005/0137591	A1	6/2005	Barry et al.	
2005/0171531	A1	8/2005	Eliachar et al.	
2005/0171532	A1	8/2005	Ciarrocca	
2005/0209590	A1	9/2005	Terakura	
2005/0222568	A1	10/2005	O'Sullivan et al.	
2005/0251134	A1	11/2005	Woloszko et al.	
2005/0283150	A1	12/2005	Moutafis et al.	
2006/0009759	A1	1/2006	Christian et al.	
2006/0030846	A1	2/2006	Buehlmann et al.	
2006/0036234	A1	2/2006	Durgin et al.	
2006/0052774	A1	3/2006	Garrison et al.	
2006/0178670	A1	8/2006	Woloszko et al.	
2007/0198011	A1	8/2007	Sugita	
2007/0270796	A2	11/2007	Girard et al.	
2008/0221587	A1*	9/2008	Schwartz .....	606/113
2010/0042143	A1	2/2010	Cunningham	
2010/0049187	A1	2/2010	Carlton et al.	
2010/0057081	A1	3/2010	Hanna	
2010/0063500	A1	3/2010	Muszala	
2010/0069903	A1	3/2010	Allen, IV et al.	
2010/0069953	A1	3/2010	Cunningham et al.	
2010/0076427	A1	3/2010	Heard	
2010/0076430	A1	3/2010	Romero	
2010/0076431	A1	3/2010	Allen, IV	
2010/0249769	A1	9/2010	Nau, Jr. et al.	
2010/0280511	A1	11/2010	Rachlin et al.	
2011/0034918	A1	2/2011	Reschke	

(56)

**References Cited**

## U.S. PATENT DOCUMENTS

2011/0054468 A1 3/2011 Dycus  
 2011/0054471 A1 3/2011 Gerhardt et al.  
 2011/0060335 A1 3/2011 Harper et al.

## FOREIGN PATENT DOCUMENTS

DE 25 14 501 A1 10/1976  
 DE 2514501 10/1976  
 DE 02514501 A1 10/1976  
 DE 2627679 1/1977  
 DE 2627679 A1 1/1977  
 DE 3423356 6/1986  
 DE 03423356 C2 6/1986  
 DE 3612646 4/1987  
 DE 03612646 A1 4/1987  
 DE 8712328 U1 2/1988  
 DE 8712328 3/1988  
 DE 4303882 8/1994  
 DE 04303882 C2 2/1995  
 DE 4403252 8/1995  
 DE 04403252 A1 8/1995  
 DE 19515914 7/1996  
 DE 19515914 C1 7/1996  
 DE 29616210 U1 11/1996  
 DE 29616210 1/1997  
 DE 19608716 4/1997  
 DE 19608716 C1 4/1997  
 DE 19751106 5/1998  
 DE 19751106 A1 5/1998  
 DE 19751108 5/1999  
 DE 19751108 A1 5/1999  
 DE 10045375 10/2002  
 DE 10045375 C2 10/2002  
 DE 19738457 1/2009  
 DE 19738457 B4 1/2009  
 EP 0 467 501 A 1/1992  
 EP 0467501 A1 1/1992  
 EP 1 159 926 A2 12/2001  
 EP 1159926 12/2001  
 EP 1301135 4/2003  
 EP 1645240 A2 4/2006  
 EP 1829494 A1 9/2007  
 GB 1490585 11/1977  
 GB 1 490 585 A 11/1997  
 JP 61-501068 9/1984  
 JP 65-502328 3/1992  
 JP 5-5106 1/1993  
 JP 5-40112 2/1993  
 JP 05-40112 2/1993  
 JP 06343644 12/1994  
 JP 06343644 A 12/1994  
 JP 07265328 10/1995  
 JP 07265328 A 10/1995  
 JP 08056955 3/1996  
 JP 08056955 A 3/1996  
 JP 08252263 10/1996  
 JP 08252263 A 10/1996  
 JP 09010223 1/1997  
 JP 09010223 A 1/1997  
 JP 10-014922 1/1998  
 JP 11-070124 5/1998  
 JP 2000-102545 9/1998  
 JP 11-070124 A 3/1999  
 JP 11244298 9/1999  
 JP 11244298 A 9/1999  
 JP 2000-102545 A 4/2000  
 JP 2000-342599 12/2000  
 JP 2000-350732 12/2000  
 JP 2000342599 A 12/2000  
 JP 2000350732 A 12/2000  
 JP 2001-008944 1/2001  
 JP 2001008944 A 1/2001  
 JP 2001-029356 2/2001  
 JP 2001029356 A 2/2001

JP 2001-128990 5/2001  
 JP 2001128990 A 5/2001  
 SU 401367 A1 10/1973  
 SU 401367 11/1974  
 WO 93/21845 11/1993  
 WO WO 93/21845 A 11/1993  
 WO WO 00/36986 6/2000  
 WO 0036986 A1 8/2000  
 WO 0154604 A1 8/2001  
 WO WO 01/54604 8/2001  
 WO 2004/073753 A2 9/2004  
 WO 2004/103156 A2 12/2004  
 WO 20051110264 A2 11/2005  
 WO WO 2005/110264 11/2005

## OTHER PUBLICATIONS

Michael Choti. "Abdominoperineal Resection with the LigaSure Vessel Sealing System and LigaSure Atlas 20 cm Open Instrument"; Innovations That Work, Jun. 2003.

E. David Crawford "Evaluation of a New Vessel Sealing Device in Urologic Cancer Surgery" Sales/Product Literature 2000.

Strasberg et al. "A Phase I Study of the LigaSure Vessel Sealing System in Hepatic Surgery" Section of HPB Surger, Washington University School of Medicine, St. Louis MO, Presented at AHPBA, Feb. 2001.

E. David Crawford "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Venous Complex" Sales/Product Literature 2000.

International Search Report and Written Opinion of the International Searching Authority mailed Jun. 16, 2009 issued by the European Patent Office in counterpart International Application No. PCT/US2009/032690 filed Jan. 30, 2009.

Paul G. Horgan, "A Novel Technique for Parenchymal Division During Hepatectomy" the American Journal of Surgery, vol. 181, No. 3, Apr. 2001 pp. 236-237.

European Search Report for EP 06006716.2 dated Aug. 16, 2006.

European Search Report for EP 07 014016 dated Feb. 12, 2008.

European Search Report for European Application No. EP 13184543.0 dated Nov. 7, 2013.

Canadian Office Action corresponding to Canadian Appln. No. 2,713,898 dated Oct. 26, 2015.

International Search Report and Written Opinion of the International Searching Authority mailed Jun. 16, 2009 issued by the European Patent Office in counterpart International Application No. PCT/US2009/032690 filed Jan. 30, 2009.

U.S. Appl. No. 12/176,679, filed Jul. 21, 2008.

U.S. Appl. No. 12/192,170, filed Aug. 15, 2008.

U.S. Appl. No. 12/192,189, filed Aug. 15, 2008.

U.S. Appl. No. 12/192,243, filed Aug. 15, 2008.

U.S. Appl. No. 12/195,624, filed Aug. 21, 2008.

U.S. Appl. No. 12/200,154, filed Aug. 28, 2008.

U.S. Appl. No. 12/200,246, filed Aug. 28, 2008.

U.S. Appl. No. 12/200,396, filed Aug. 28, 2008.

U.S. Appl. No. 12/200,526, filed Aug. 28, 2008.

U.S. Appl. No. 12/204,976, filed Sep. 5, 2008.

U.S. Appl. No. 12/210,598, filed Sep. 15, 2008.

U.S. Appl. No. 12/211,205, filed Sep. 16, 2008.

U.S. Appl. No. 12/233,157, filed Sep. 18, 2008.

U.S. Appl. No. 12/236,666, filed Sep. 24, 2008.

U.S. Appl. No. 12/237,515, filed Sep. 25, 2008.

U.S. Appl. No. 12/237,556, filed Sep. 25, 2008.

U.S. Appl. No. 12/237,582, filed Sep. 25, 2008.

U.S. Appl. No. 12/244,873, filed Oct. 3, 2008.

U.S. Appl. No. 12/246,553, filed Oct. 7, 2008.

U.S. Appl. No. 12/248,104, filed Oct. 9, 2008.

U.S. Appl. No. 12/248,115, filed Oct. 9, 2008.

U.S. Appl. No. 12/254,123, filed Oct. 20, 2008.

U.S. Appl. No. 12/331,643, filed Dec. 10, 2008.

U.S. Appl. No. 12/336,970, filed Dec. 17, 2008.

U.S. Appl. No. 12/352,942, filed Jan. 13, 2009.

U.S. Appl. No. 12/353,466, filed Jan. 14, 2009.

U.S. Appl. No. 12/353,470, filed Jan. 14, 2009.

U.S. Appl. No. 12/353,474, filed Jan. 14, 2009.

(56)

## References Cited

## OTHER PUBLICATIONS

- U.S. Appl. No. 12/353,086, filed Jan. 30, 2009.  
 U.S. Appl. No. 12/410,195, filed Mar. 24, 2009.  
 U.S. Appl. No. 12/411,542, filed Mar. 26, 2009.  
 U.S. Appl. No. 12/419,729, filed Apr. 7, 2009.  
 U.S. Appl. No. 12/429,533, filed Apr. 24, 2009.  
 U.S. Appl. No. 12/434,382, filed May 1, 2009.  
 U.S. Appl. No. 12/503,256, filed Jul. 15, 2009.  
 U.S. Appl. No. 12/508,052, filed Jul. 23, 2009.  
 U.S. Appl. No. 12/535,869, filed Aug. 5, 2009.  
 U.S. Appl. No. 12/543,831, filed Aug. 19, 2009.  
 U.S. Appl. No. 12/543,969, filed Aug. 19, 2009.  
 U.S. Appl. No. 12/548,031, filed Aug. 26, 2009.  
 U.S. Appl. No. 12/548,534, filed Aug. 27, 2009.  
 U.S. Appl. No. 12/548,566, filed Aug. 27, 2009.  
 U.S. Appl. No. 12/551,944, filed Sep. 1, 2009.  
 U.S. Appl. No. 12/553,509, filed Sep. 3, 2009.  
 U.S. Appl. No. 12/556,025, filed Sep. 9, 2009.  
 U.S. Appl. No. 12/556,407, filed Sep. 9, 2009.  
 U.S. Appl. No. 12/556,427, filed Sep. 9, 2009.  
 U.S. Appl. No. 12/556,796, filed Sep. 10, 2009.  
 U.S. Appl. No. 12/562,281, filed Sep. 18, 2009.  
 U.S. Appl. No. 12/565,281, filed Sep. 23, 2009.  
 U.S. Appl. No. 12/568,199, filed Sep. 28, 2009.  
 U.S. Appl. No. 12/568,282, filed Sep. 28, 2009.  
 U.S. Appl. No. 12/569,395, filed Sep. 29, 2009.  
 U.S. Appl. No. 12/569,710, filed Sep. 29, 2009.  
 U.S. Appl. No. 12/574,001, filed Oct. 6, 2009.  
 U.S. Appl. No. 12/574,292, filed Oct. 6, 2009.  
 U.S. Appl. No. 12/576,380, filed Oct. 9, 2009.  
 U.S. Appl. No. 12/607,191, filed Oct. 28, 2009.  
 Chung et al., "Clinical Experience of Sutureless Closed Hemorrhoidectomy with LigaSure" *Diseases of the Colon & Rectum* vol. 46, No. Jan. 1, 2003.  
 Carbonell et al., "Comparison of the Gyrus PlasmaKinetic Sealer and the Valleylab LigaSure Device in the Hemostasis of Small, Medium, and Large-Sized Arteries" *Carolinas Laparoscopic and Advanced Surgery Program, Carolinas Medical Center, Charlotte, NC*; Date: Aug. 2003.  
 Peterson et al., "Comparison of Healing Process Following Ligation with Sutures and Bipolar Vessel Sealing" *Surgical Technology International* (2001).  
 "Electrosurgery: A Historical Overview" *Innovations in Electrosurgery*; Sales/Product Literature; Dec. 31, 2000.  
 Johnson et al., "Evaluation of a Bipolar Electrothermal Vessel Sealing Device in Hemorrhoidectomy" *Sales/Product Literature*; Jan. 2004.  
 Johnson et al., "Evaluation of the LigaSure Vessel Sealing System in Hemorrhoidectomy" *American College of Surgeons (ACS) Clinica Congress Poster* (2000).  
 Muller et al., "Extended Left Hemicolectomy Using the LigaSure Vessel Sealing System" *Innovations That Work*, Sep. 1999.  
 Kennedy et al., "High-burst-strength, feedback-controlled bipolar vessel sealing" *Surgical Endoscopy* (1998) 12: 876-878.  
 Carus et al., "Initial Experience With the LigaSure Vessel Sealing System in Abdominal Surgery" *Innovations That Work*, Jun. 2002.  
 Heniford et al., "Initial Research and Clinical Results with an Electrothermal Bipolar Vessel Sealer" Oct. 1999.  
 Heniford et al., "Initial Results with an Electrothermal Bipolar Vessel Sealer" *Surgical Endoscopy* (2000) 15:799-801.  
 Herman et al., "Laparoscopic Intestinal Resection With the LigaSure Vessel Sealing System: A Case Report"; *Innovations That Work*, Feb. 2002.  
 Koyle et al., "Laparoscopic Palomo Varicocele Ligation in Children and Adolescents" *Pediatric Endosurgery & Innovative Techniques*, vol. 6, No. 1, 2002.  
 W. Scott Helton, "LigaSure Vessel Sealing System: Revolutionary Hemostasis Product for General Surgery"; *Sales/Product Literature* 1999.  
 LigaSure Vessel Sealing System, the Seal of Confidence in General, Gynecologic, Urologic, and Laparoscopic Surgery; *Sales/Product Literature*; Apr. 2002.  
 Joseph Ortenberg "LigaSure System Used in Laparoscopic 1st and 2nd Stage Orchiopexy" *Innovations That Work*, Nov. 2002.  
 Sigel et al., "The Mechanism of Blood Vessel Closure by High Frequency Electrocoagulation" *Surgery Gynecology & Obstetrics*, Oct. 1965 pp. 823-831.  
 Sampayan et al., "Multilayer Ultra-High Gradient Insulator Technology" *Discharges and Electrical Insulation in Vacuum*, 1998. Netherlands Aug. 17-21, 1998; vol. 2, pp. 740-743.  
 Paul G. Horgan, "A Novel Technique for Parenchymal Division During Hepatectomy" *The American Journal of Surgery*, vol. 181, No. 3, Apr. 2001 pp. 236-237.  
 Olsson et al., "Radical Cystectomy in Females" *Current Surgical Techniques in Urology*, vol. 14, Issue 3, 2001.  
 Palazzo et al., "Randomized clinical trial of Ligasure versus open haemorrhoidectomy" *British Journal of Surgery* 2002, 89, 154-157.  
 Levy et al., "Randomized Trial of Suture Versus Electrosurgical Bipolar Vessel Sealing in Vaginal Hysterectomy" *Obstetrics & Gynecology*, vol. 102, No. 1, Jul. 2003.  
 "Reducing Needlestick Injuries in the Operating Room" *Sales/Product Literature* 2001.  
 Bergdahl et al., "Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator" *J. Neurosurg*, vol. 75, Jul. 1991, pp. 148-151.  
 Sayfan et al., "Sutureless Closed Hemorrhoidectomy: A New Technique" *Annals of Surgery* vol. 234 No. 1 Jul. 2001; pp. 21-24.  
 Levy et al., "Update on Hysterectomy—New Technologies and Techniques" *OBG Management*, Feb. 2003.  
 Dulemba et al., "Use of a Bipolar Electrothermal Vessel Sealer in Laparoscopically Assisted Vaginal Hysterectomy" *Sales/Product Literature*; Jan. 2004.  
 Strasberg et al., "Use of a Bipolar Vessel-Sealing Device for Parenchymal Transection During Liver Surgery" *Journal of Gastrointestinal Surgery*, vol. 6, No. 4, Jul./Aug. 2002 pp. 569-574.  
 Sengupta et al., "Use of a Computer-Controlled Bipolar Diathermy System in Radical Prostatectomies and Other Open Urological Surgery" *ANZ Journal of Surgery* (2001) 71.9 pp. 538-540.  
 Rothenberg et al., "Use of the LigaSure Vessel Sealing System in Minimally Invasive Surgery in Children" *Int'l Pediatric Endosurgery Group (IPEG)* 2000.  
 Crawford et al., "Use of the LigaSure Vessel Sealing System in Urologic Cancer Surgery" *Grand Rounds in Urology* 1999 vol. 1 Issue 4 pp. 10-17.  
 Craig Johnson, "Use of the LigaSure Vessel Sealing System in Bloodless Hemorrhoidectomy" *Innovations That Work*, Mar. 2000.  
 Levy et al., "Use of a New Energy-based Vessel Ligation Device During Vaginal Hysterectomy" *Int'l Federation of Gynecology and Obstetrics (FIGO) World Congress* 1999.  
 Barbara Levy, "Use of a New Vessel Ligation Device During Vaginal Hysterectomy" *FIGO* 2000, Washington, D.C.  
 E. David Literature "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Venous Complex" *Sales/Product Literature* 2000.  
 Jarrett et al., "Use of the LigaSure Vessel Sealing System for Perihilar Vessels in Laparoscopic Nephrectomy" *Sales/Product Literature* 2000.  
 Crouch et al., "A Velocity-Dependent Model for Needle Insertion in Soft Tissue" *MICCAI* 2005; LNCS 3750 pp. 624-632, Dated: 2005.  
 McLellan et al., "Vessel Sealing for Hemostasis During Pelvic Surgery" *Int'l Federation of Gynecology and Obstetrics FIGO World Congress* 2000, Washington, D.C.  
 McLellan et al., "Vessel Sealing for Hemostasis During Gynecologic Surgery" *Sales/Product Literature* 1999.  
 Int'l Search Report EP 98944778.4 dated Oct. 31, 2000.  
 Int'l Search Report EP 98957771 dated Aug. 9, 2001.  
 Int'l Search Report EP 98958575.7 dated Sep. 20, 2002.  
 Int'l Search Report EP 04013772.1 dated Apr. 1, 2005.  
 Int'l Search Report EP 04027314.6 dated Mar. 10, 2005.  
 Int'l Search Report EP 04027479.7 dated Mar. 8, 2005.  
 Int'l Search Report EP 04027705.5 dated Feb. 3, 2005.  
 Int'l Search Report EP 04752343.6 dated Jul. 20, 2007.

(56)

**References Cited**

## OTHER PUBLICATIONS

- Int'l Search Report EP 05002671.5 dated Dec. 22, 2008.  
Int'l Search Report EP 05002674.9 dated Jan. 16, 2009.  
Int'l Search Report EP 05013463.4 dated Oct. 7, 2005.  
Int'l Search Report EP 05013895.7 dated Oct. 21, 2005.  
Int'l Search Report EP 05016399.7 dated Jan. 13, 2006.  
Int'l Search Report EP 05017281.6 dated Nov. 24, 2005.  
Int'l Search Report EP 05019130.3 dated Oct. 27, 2005.  
Int'l Search Report EP 05019429.9 dated May 6, 2008.  
Int'l Search Report EP 05020665.5 dated Feb. 27, 2006.  
Int'l Search Report EP 05020666.3 dated Feb. 27, 2006.  
Int'l Search Report EP 05021197.8 dated Feb. 20, 2006.  
Int'l Search Report EP 05021779.3 dated Feb. 2, 2006.  
Int'l Search Report EP 05021780.1 dated Feb. 23, 2006.  
Int'l Search Report EP 05021937.7 dated Jan. 23, 2006.  
Int'l Search Report--extended--EP 05021937.7 dated Mar. 15, 2006.  
Int'l Search Report EP 05023017.6 dated Feb. 24, 2006.  
Int'l Search Report EP 06002279.5 dated Mar. 30, 2006.  
Int'l Search Report EP 06005185.1 dated May 10, 2006.  
Int'l Search Report EP 06008716.2 dated Aug. 4, 2006.  
Int'l Search Report EP 06008515.6 dated Jan. 8, 2009.  
Int'l Search Report EP 06008779.8 dated Jul. 13, 2006.  
Int'l Search Report EP 06014461.5 dated Oct. 31, 2006.  
Int'l Search Report EP 06020574.7 dated Oct. 2, 2007.  
Int'l Search Report EP 06020583.8 dated Feb. 7, 2007.  
Int'l Search Report EP 06020584.6 dated Feb. 1, 2007.  
Int'l Search Report EP 06020756.0 dated Feb. 16, 2007.  
Int'l Search Report EP 06 024122.1 dated Apr. 16, 2007.  
Int'l Search Report EP 06024123.9 dated Mar. 6, 2007.  
Int'l Search Report EP 07 001480.8 dated Apr. 19, 2007.  
Int'l Search Report EP 07 001488.1 dated Jun. 5, 2007.  
Int'l Search Report EP 07 009026.1 dated Oct. 8, 2007.  
Int'l Search Report Extended--EP 07 009029.5 dated Jul. 20, 2007.  
Int'l Search Report EP 07 009321.6 dated Aug. 28, 2007.  
Int'l Search Report EP 07 010672.9 dated Oct. 16, 2007.  
Int'l Search Report EP 07 013779.9 dated Oct. 26, 2007.  
Int'l Search Report EP 07 014016 dated Jan. 28, 2008.  
Int'l Search Report EP 07 015191.5 dated Jan. 23, 2008.  
Int'l Search Report EP 07 015601.3 dated Jan. 4, 2008.  
Int'l Search Report EP 07 020283.3 dated Feb. 5, 2008.  
Int'l Search Report EP 07 021646.0 dated Mar. 20, 2008.  
Int'l Search Report EP 07 021646.0 dated Jul. 9, 2008.  
Int'l Search Report EP 07 021647.8 dated May 2, 2008.  
Int'l Search Report EP 08 002692.5 dated Dec. 12, 2008.  
Int'l Search Report EP 08 004655.0 dated Jun. 24, 2008.  
Int'l Search Report EP 08 006732.5 dated Jul. 29, 2008.  
Int'l Search Report EP 08 006917.2 dated Jul. 3, 2008.  
Int'l Search Report EP 08 016539.2 dated Jan. 8, 2009.  
Int'l Search Report EP 09 003813.4 dated Aug. 3, 2009.  
Int'l Search Report EP 09 004491.8 dated Sep. 9, 2009.  
Int'l Search Report EP 09 005575.7 dated Sep. 9, 2009.  
Int'l Search Report EP 09 152267.2 dated Jun. 15, 2009.  
Int'l Search Report EP 09 152898.4 dated Jun. 10, 2009.  
Int'l Search Report EP 09 154850.3 dated Jul. 20, 2009.  
Int'l Search Report EP 09 160476.9 dated Aug. 4, 2009.  
Int'l Search Report EP 09 164903.8 dated Aug. 21, 2009.  
Int'l Search Report PCT/US98/18640 dated Jan. 29, 1999.  
Int'l Search Report PCT/US98/23950 dated Jan. 14, 1999.  
Int'l Search Report PCT/US98/24281 dated Feb. 22, 1999.  
Int'l Search Report PCT/US99/24869 dated Feb. 3, 2000.  
Int'l Search Report PCT/US01/11218 dated Aug. 14, 2001.  
Int'l Search Report PCT/US01/11224 dated Nov. 13, 2001.  
Int'l Search Report PCT/US01/11340 dated Aug. 16, 2001.  
Int'l Search Report PCT/US01/11420 dated Oct. 16, 2001.  
Int'l Search Report PCT/US02/01890 dated Jul. 25, 2002.  
Int'l Search Report PCT/US02/11100 dated Jul. 16, 2002.  
Int'l Search Report PCT/US03/28534 dated Dec. 19, 2003.  
Int'l Search Report PCT/US04/03436 dated Mar. 3, 2005.  
Int'l Search Report PCT/US04/13273 dated Dec. 15, 2004.  
Int'l Search Report PCT/US04/15311 dated Jan. 12, 2005.  
Int'l Search Report PCT/US07/021438 dated Apr. 1, 2008.  
Int'l Search Report PCT/US07/021440 dated Apr. 8, 2008.  
Int'l Search Report PCT/US08/61498 dated Sep. 22, 2008.  
Int'l Search Report PCT/US09/032690 dated Jun. 16, 2009.

\* cited by examiner

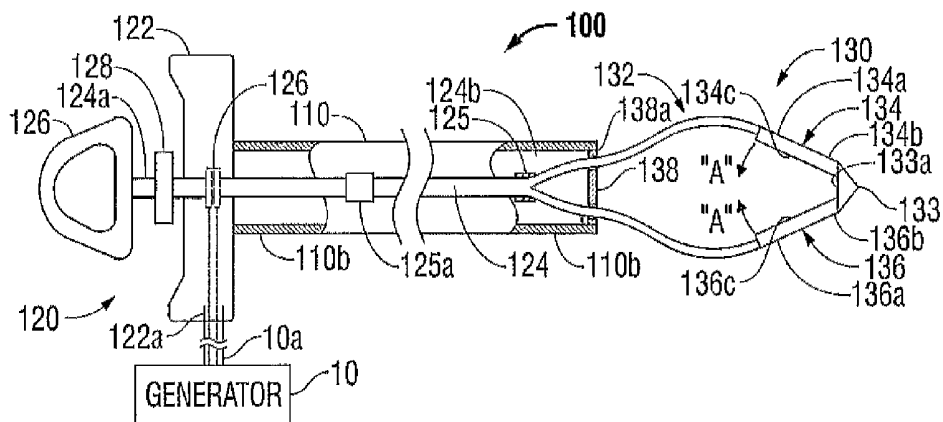


FIG. 1

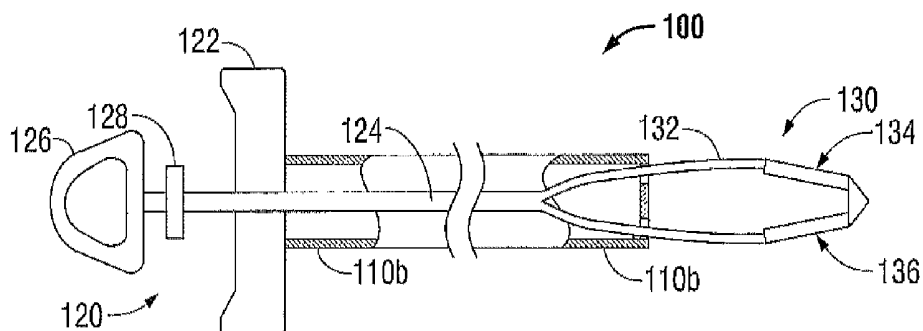


FIG. 2

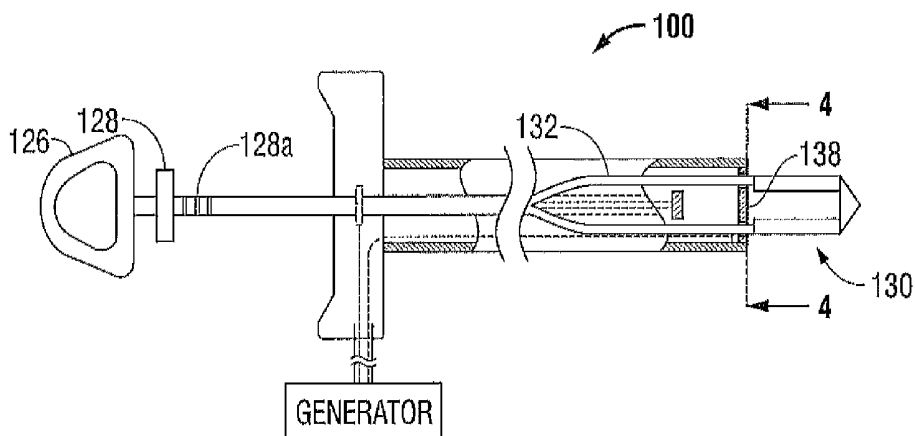


FIG. 3

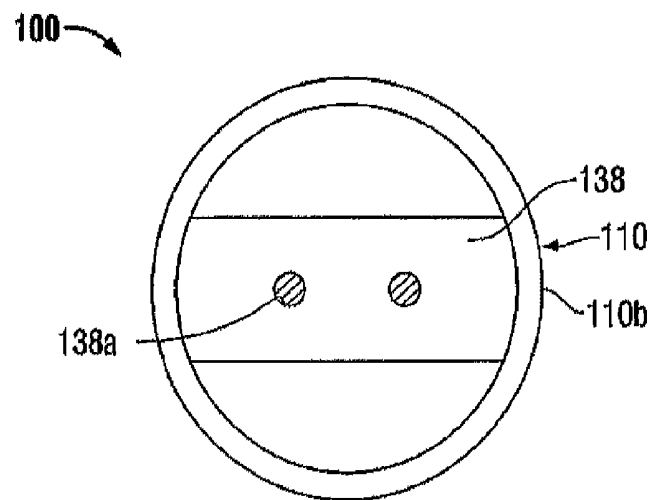


FIG. 4

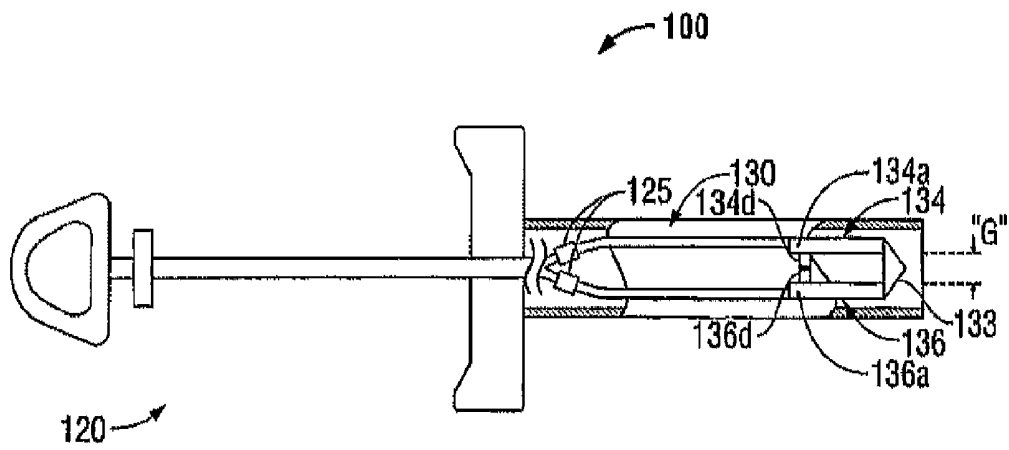


FIG. 5

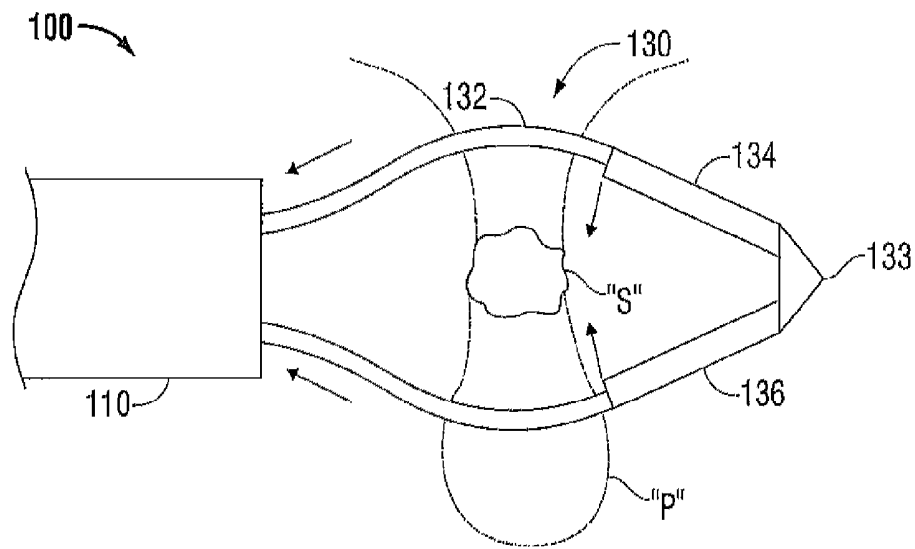


FIG. 6

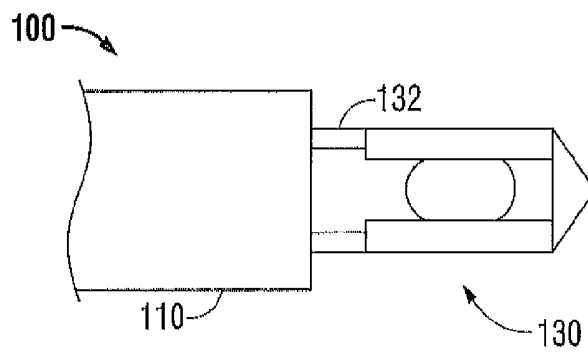


FIG. 7

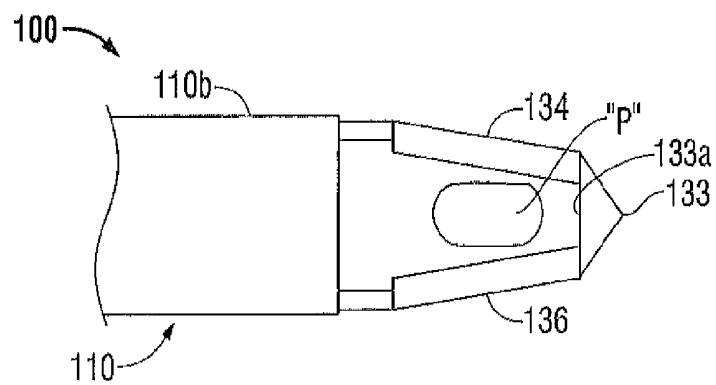


FIG. 8



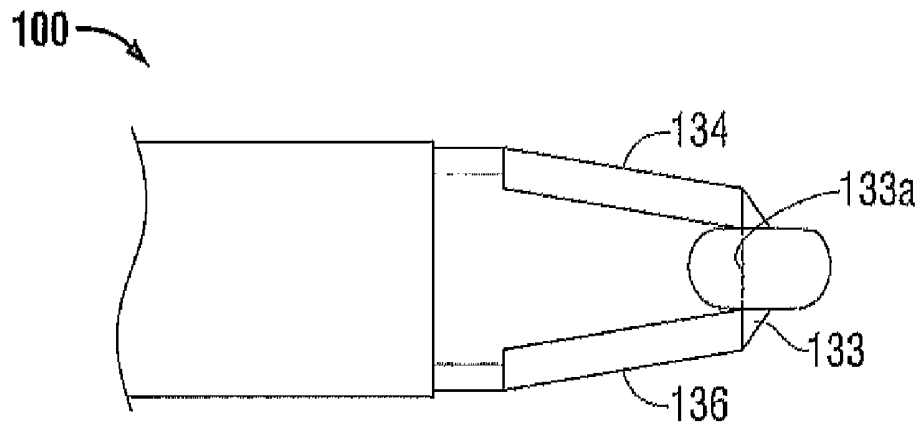


FIG. 9

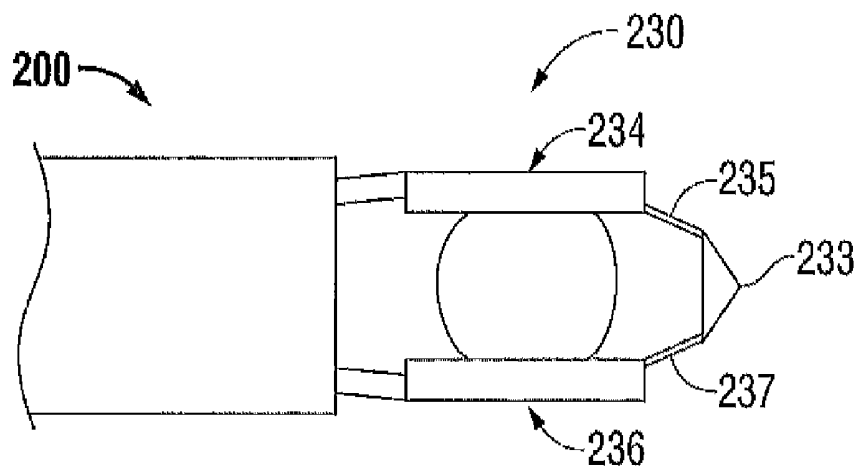


FIG. 10

## POLYP REMOVAL DEVICE AND METHOD OF USE

Matter enclosed in heavy brackets [ ] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue; a claim printed with strikethrough indicates that the claim was canceled, disclaimed, or held invalid by a prior post-patent action or proceeding.

### CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims the benefit of priority to U.S. Provisional Patent Application Ser. No. 61/063,158, titled "Endoscopic flexible loop for gastrointestinal polypectomy and mucosal resection using LigaSure™ sealing technology", by Wexner et al., filed Jan. 31, 2008, which is incorporated by reference herein.

### BACKGROUND

#### 1. Technical Field

The present disclosure relates to devices and methods for the removal of internal tissue and, more particularly, to snare-type devices including a pair of electrodes for treating tissue prior to excision.

#### 2. Background of Related Art

A polyp is an abnormal growth of tissue projecting from a mucous membrane. A polyp that is attached to the surface of the mucous membrane by a narrow elongated stalk is said to be pedunculated. If no stalk is present, the polyp is said to be sessile. Polyps are commonly found in the colon, stomach, nose, urinary bladder and uterus. Polyps may also form elsewhere in the body where mucous membranes exist, for example, the cervix and small intestine.

The surgical procedure for removing a polyp is generally referred to as a "polypectomy". Polypectomies are generally endoscopic or laparoscopic procedures performed through the oral or anal cavities. When the location of the polyp permits, the polypectomy may be performed as an open procedure. Conventional polypectomies are completed using various apparatus and techniques known in the art.

As noted above, there are two forms of polyps, sessile and pedunculated. The stalkless or sessile polyps are generally removed using electrical forceps. For example, the excess tissue projecting from the mucous membrane is cauterized and torn from the tissue wall. Pedunculated polyps, or those with stalks, tend to be larger with a greater blood supply. The size and shape of pedunculated polyps typically do not lend themselves to being removed using traditional forceps. Unlike sessile polyps, polyps with a stalk cannot simply be grasped in the jaw members of an electrosurgical forceps and be torn from the tissue wall. Instead, the polypectomy is performed using a surgical snare device.

Conventional snare devices are configured with a snare for looping over the distal end of a hanging polyp and tightening securely around the stalk of the polyp. By constricting the snare, and selectively applying energy to the snare, the device may cauterize or seal the polyp at the stalk as the polyp is severed from the tissue wall. Conventional snare devices may be configured for monopolar or bipolar use. Excising a polyp using a conventional snare device typically involves cutting or otherwise separating the polyp from the tissue wall as the

snare device is activated and constricted about the stalk of the polyp. In this manner, the polyp is cauterized as the snare passes through the tissue.

### SUMMARY

Disclosed is a device configured for removing polyps. In one embodiment, the polyp removal device includes a tubular member having proximal and distal ends, a snare portion operably extending from within the distal end of the tubular member and including first and second electrodes configured to seal tissue therebetween, the snare portion further including a cutting member for severing the sealed tissue. The polyp removal device may further include a handle portion operatively extending from within the proximal end of the tubular member. The handle portion may be configured for operable engagement by a user. The cutting member may extend between distal ends of the first and second electrodes.

The polyp removal device may be configured to grasp the stalk of a polyp between the first and second electrodes. The first and second electrodes may be hingedly attached to the cutting member. The snare portion may be configured to be retracted within the tubular member. The snare portion may be retracted within the tubular member upon retraction of the handle portion relative to the base portion.

A system including the polyp removal device may further include an electrosurgical generator. The electrodes may be electrically connected to the electrosurgical generator. The distal end of the tubular member may include a spacer member for preventing the first and second electrodes from contacting one another. Alternatively, at least one of the first and second electrodes may include a spacer mounted thereon for preventing contact between the first and second electrodes.

Also provided is a polyp removal device including a tubular member having proximal and distal ends, a handle portion operatively extending from the proximal end of the tubular member, and a snare portion slidably supported within the lumen of the tubular member and operably extending from the distal end of the tubular member, the snare portion including first and second electrodes operably mounted thereto for sealing tissue therebetween, wherein at least one of the first and second electrodes includes at least one spacer mounted thereon for preventing contact between the first and second electrodes. The snare portion of the polyp removal device may be retractable with the tubular member.

Additionally provided is a method of removing a polyp. The method includes the steps of providing a polyp removal device including, a tubular member having proximal and distal ends, a snare portion slidably supported within the lumen of the tubular member and operably extending from the distal end of the tubular member, the snare portion including first and second electrodes operably mounted thereto for sealing tissue therebetween, wherein at least one of the first and second electrodes includes at least one spacer mounted thereon for preventing contact between the first and second electrodes, extending the snare portion relative to the tubular member, looping the snare portion about a portion of a polyp, retracting the snare portion relative to the tubular member to capture the portion of the polyp between the first and second electrodes, and activating the first and second electrodes.

The method may further include the steps of partially advancing the snare portion relative to the tubular member, retracting the tubular member and the snare portion relative to the polyp and severing the polyp from surrounding tissue.

### BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate embodi-

ments of the present disclosure and, together with the detailed description of the embodiments given below, serve to explain the principles of the disclosure.

FIG. 1 is a partial cross-sectional, top plan view of a polyp removal device according to an embodiment of the present disclosure, shown in a first or extended position;

FIG. 2 is a partial cross-sectional top plan view of the polyp removal device of FIG. 1, shown in a partially retracted position;

FIG. 3 is a partial cross-sectional top plan view of the polyp removal device of FIG. 1, shown in a retracted position;

FIG. 4 is a cross-section end view of the polyp removal device of FIGS. 1-3 taken along line 4-4 of FIG. 3;

FIG. 5 is a partial cross-section top plan view of an alternative embodiment of a polyp removal device according to the present disclosure in a completely retracted position;

FIG. 6 is a partial top plan view of the distal end of the polyp removal device of FIGS. 1-4, in a first or extending position about a polyp;

FIG. 7 is a partial top plan view of the distal end of the polyp removal device of FIG. 6, in a retracted position about a polyp; and

FIG. 8 is a partial top plan view of the distal end of the polyp removal device of FIGS. 6 and 7, in a partially advanced position about a polyp;

FIG. 9 is a partial top plan view of the distal end of the polyp removal device of FIGS. 6-8, as the stalk of the polyp is being severed; and

FIG. 10 is a partial top plan view of another illustrative embodiment of a polyp removal device of the present disclosure, in a retracted position about a polyp.

#### DETAILED DESCRIPTION OF EMBODIMENTS

The foregoing summary, as well as the following detailed description will be better understood when read in conjunction with the appended figures. For the purpose of illustrating the present disclosure, various embodiments are shown. It is understood, however, that the present disclosure is not limited to the precise arrangement and instrumentalities shown.

As shown in the drawings and described throughout the following description, as is traditional when referring to relative positioning on an object, the term "proximal" refers to the end of the apparatus that is closer to the user and the term "distal" refers to the end of the apparatus that is further from the user.

Referring to FIGS. 1-4, an embodiment of the presently disclosed polyp removal device is shown therein and is generally designated as polyp removal device 100. Polyp removal device 100 includes an elongated tubular member 110, a handle portion 120 extending proximally from tubular member 110, and a snare portion or assembly 130 operably engaged with handle portion 120 and extending distally from within elongated tube 110. Polyp removal device 100 may be any suitable length and size for accessing various locations throughout the body. Device 100 may be configured for removal of suitable types of polyps of any size, or may be configured for general mucosal resection or removal of any suitable tissue mass. Preferably, polyp removal device 100 is configured for endoscopic, laparoscopic or transluminal insertion.

Referring initially to FIGS. 1-3, elongated tubular member 110 includes proximal and distal ends 110a, 110b. Proximal end 110a of tubular member 110 is operably coupled to handle portion 120. As will be described in further detail below, handle portion 120 may be integrally formed with tubular member 110. Alternatively, handle portion 120 may

be releasably secured to tubular member 110, or may instead be securely affixed to tubular member 110. Tubular member 110 may be flexible, semi-rigid, or rigid and may be constructed of metal, alloy, plastic, polymers, or any other suitable material. Distal end 110b of tubular member 110 is configured to slidably receive a proximal end of snare portion 130.

Although the following description of the polyp removal device 100 will be described in the form of a snare-type device, the aspects of the present disclosure may be modified for use with alternative handle configurations, including a pistol grip style device, mechanically and/or remotely actuated handles, other suitable types of devices or handle arrangements. As one example, polyp removal device 100 may be incorporated as a pistol grip style laparoscopic device like some of the LigaSure™ tissue fusion devices sold by Valleylab of Boulder, Colo.

Still referring to FIGS. 1-3, handle portion 120 of polyp removal device 100 includes a base 122 coupled to proximal end 110a of tubular member 110, a connector shaft 124 extending through base 122, and a handle 126 operably coupled to a proximal end 124a of connector shaft 124. In one embodiment, base 122 of handle portion 120 may be securely affixed to proximal end 110a of tubular member 110 using adhesive, bonding, mechanical fasteners, welding or other suitable methods. Alternatively, base 122 may be releasably connected to tubular member 110 using mechanical fasteners, threaded engagement, friction fitting, bayonet connections, or the like. In this manner, snare portion 130 may be removed and replaced through proximal end 110a of tubular member 110. Base 122 of handle portion 120 may instead be integrally formed with proximal end 110a of tubular member 110. Handle 126 is configured for operable engagement by a user. Handle 126 may be knurled or may include a coating for facilitating engagement by a user.

Base 122 of handle portion 120 is further configured for operable engagement with a generator 10. Base 122 defines a connection port 122a for receiving an electrical cord 10a extending from generator 10. Electrical cord 10a extends from connection port 122a through base 122 and is operably coupled to first and second electrodes 134, 136 of snare portion 130. Electrical cord 10a may be directly coupled to first and second electrodes 134, 136. Alternatively, electrical cord 10a may couple with a coupling member 123 mounted to shaft 124. In this manner, coupling member 123 electrically couples generator 10 with first and second electrodes 134, 136 along shaft 124. Generator 10 may include any suitable generator configured to selectively provide energy to electrodes 134, 136. For example, radiofrequency energy, either monopolar or bipolar may be provided to electrodes 134, 136. In other embodiments, ultrasonic, microwave, or laser energy may be provided. Depending on the energy modality utilized, snare 130 and/or electrodes 134, 136 may have to be reconfigured in order to handle the different types of energy.

In an embodiment where radiofrequency energy is utilized, to increase safety, bipolar radiofrequency energy is preferred because the energy will travel between first and second electrodes 134, 136 instead of between the snare 130 and some remote return pad. In one particular embodiment, generator 10 takes the form of a battery-powered generator that is integral with, or releasably coupled to, polyp removal device 100. In this example, electrical cord 10a is not needed. Generator 10 may also be configured to monitor the electrical properties of the tissue maintained between first and second electrodes 134, 136 and signal to the clinician when conditions have been met that are suitable for sealing of tissue.

Still referring to FIGS. 1-3, connector shaft 124 includes an elongated tubular shaft including proximal and distal ends 124a, 124b. Proximal end 124a is configured for operable engagement with handle 126. Handle 126 may be securely affixed, releasable coupled, or integrally formed with proximal end 124a of connector shaft 124. Handle portion 120 may further include a stop member 128 positioned about connector shaft 124 between base 122 and handle 126. Stop member 128 prevents complete retraction of connector shaft 124 past base 122. Proximal end 124a may be configured to securely retain stop member 128, or instead, may include grooves or indents 128a for selectively positioning stop member 128 thereabout. In this manner, adjustment of stop member 128 reduces or increases the amount of extension of snare portion 130. Alternatively, stop member 128 may be configured to selectively engage distal end 124a of connector shaft 124 through the incorporation of a mechanical fastener or the like (not shown). Distal end 124b of connector shaft 124 is operably coupled to snare portion 130. Distal end 124b may be permanently coupled, releasably coupled or integrally formed with snare portion 130.

Snare portion 130 includes a snare 132 formed of a loop of rigid or semi-rigid wire or flexible band. Snare 132 may be constructed of metal, polymer or other suitable material. In the illustrated embodiment, snare 132 is non-conductive; however, snare 132 may be conductive or partially conductive. Coupled to snare 132 in any suitable manner near a distal end 130b of snare portion 130 are first and second electrodes 134, 136. As discussed above, first and second electrodes 134, 136 are electrically coupled to generator 10 to receive electrosurgical energy therefrom. First and second electrodes 134, 136, which may be of any suitable construction, each include at least a tissue contacting surface 134c, 136c. In some embodiments, first and second electrodes 134, 136 are each formed from a tissue contacting surface 134c, 136c and an insulative body portion. Tissue contacting surfaces 134c, 136c may include any configuration suitable for treating tissue, including hatching, grooves and detents (not shown). In one embodiment, generator 10, first and second electrodes 134, 136, and tissue contacting surfaces 134c, 136c, are all configured for sealing tissue.

Positioned between first and second electrodes 134, 136 is a connection member 133. Distal ends 134b, 136b of first and second electrodes 134, 136, respectively, are coupled to connection member 133. First and second electrodes 134, 136 and connection member 133 are configured such that in a first or extended position, proximal ends 134a, 136a of first and second electrodes 134, 136, respectively, are substantially spaced from one another. As will be discussed in further detail below, this configuration opens snare 132 to facilitate the looping of snare 132 over a polyp "P" (FIG. 6) and the positioning of first and second electrodes 134, 136 about stalk "S" of polyp "P".

First and second electrodes 134, 136 and connection member 133 are further configured such that as proximal end 130a of snare portion 130 is retracted within distal end 110b of tubular member 110, proximal ends 134a, 136a of first and second electrodes 134, 136, respectively, are approximated towards each other, in the direction of arrows "A" (FIG. 1). In this manner, first and second electrodes 134, 136 and connection member 133 act like a jaw assembly, thereby compressing stalk "S" of polyp "P" between first and second electrodes 134, 136. To prevent first and second electrodes 134, 136 from contacting one another, distal end 110b of tubular member 110 may include a spacer member 138 through which snare 132 may extend. Spacer member 138 spans distal end 110b of tubular member 110 and includes a pair of apertures 138a

through which snare 132 is received. Apertures 138a are spaced such that upon retraction of proximal end 130a of snare portion 130 within tubular member 110, proximal end 134a, 136a of first and second electrodes 134, 136 are approximated towards one another. Apertures 138a are further configured to prevent first and second electrodes 134, 136 contacting one another. Release of proximal end 130a of snare portion 130 from within distal end 110b of tubular member 100 permits proximal ends 134a, 136a of first and second electrodes 134, 136 to approximate away from one another and eventual return to their initial position.

In an alternative embodiment, one or both of first and second electrodes 134, 136 may include one or more spacers 134d, 136d (FIG. 5) formed on respective proximal ends 134a, 136a. Spacers 134d, 136d are configured to prevent contact between first and second electrodes 134, 136.

Connection member 133 extends between first and second electrodes 134, 136 and is configured to maintain distal ends 134b, 136b of first and second electrodes 134, 136, in a spaced relationship throughout the tissue excising procedure. As described above, in a first or extended position, proximal ends 134a, 136a of first and second electrodes 134, 136 are maintained in a substantially spaced apart relationship. This configuration facilitates positioning of snare 132, and first and second electrodes 134, 136 in particular, about stalk "S" of a polyp "P" (FIG. 6). Distal ends 134b, 136b of first and second electrodes 134, 136 are coupled to connection member 133 in a manner that permits pivoting, hinging, or flexing of first and second electrodes 134, 136 relative to connection member 133 as snare 132 is constricted about stalk "S" of polyp "P". First and second electrodes 134, 136 and/or connection member 133 may be formed of flexible material, or may instead include a hinge mechanism or any other suitable configuration capable of permitting first and second electrodes 134, 136 to pivot, hinge, or flex relative to connection member 133. In the event that proximal ends 134a, 136a of first and second electrodes 134, 136 are approximated away from one another by the configuration of connection member 133, snare 132 may provide the spring force to maintain proximal ends 134a, 136a substantially spaced apart when polyp removal device 100 is in a first or extended position.

Connection member 133 further includes at least a first sharpened surface 133a. First sharpened surface 133a is formed between distal ends 134b, 136b of first and second electrodes 134, 136 and may be configured to sever stalk "S" of polyp "P" after proper sealing of the tissue. In addition, or alternatively, the outer surface of connection member 133 may be sharpened to facilitate excising of polyp "P".

Referring now to FIGS. 1-3 and 6-8, one embodiment of the operation of polyp removal device 100 will be described. Initially, distal end 110b of tubular member 110 is inserted into a patient. As discussed above, introduction of polyp removal device 100 may be accomplished through an endoscopic or laparoscopic port, or may be inserted transluminally through the mouth or anus. To facilitate insertion of tubular member 110 into the body, in one embodiment (FIG. 5), snare portion 130a is completely retracted within tubular member 110.

Once distal end 110b of tubular member 110 is positioned near a polyp "P" to be removed, snare portion 130 is extended distally by advancing handle 126 of handle portion 120 relative to base 122. The spring-like configuration between first and second electrodes 134, 136 and connection member 133 results in proximal ends 134a, 136a of first and second electrodes 134, 136 approximating away from each other as handle 126 is advanced and proximal end 130a of snare portion 130 is released from tubular member 110. The sepa-

rating of proximal ends **134a**, **136a** of first and second electrodes **134**, **136** opens snare **132** and facilitates positioning of snare **132** about stalk "S" of polyp "P". Once snare **132** is positioned such that stalk "S" is received between first and second electrodes **134**, **136**, handle **126** may be retracted or, in the alternative, tubular member **110** may be advanced to constrict snare **132** about stalk "S". As proximal end **130a** of snare portion **130** is received within distal end **110b** of tubular member **110** through spacer member **138**, proximal ends **134a**, **136a** of first and second electrodes **134**, **136** are approximated towards one another, thereby capturing stalk "S" of polyp "P" therebetween. Other methods of approximating first and second electrodes **134**, **136** towards one another are contemplated by the present invention. For example, another instrument separate from polyp removal device **100** may be utilized.

Continued retraction of snare portion **130** within tubular member **110** causes first and second electrodes **134**, **136** to compress stalk "S" of polyp "P". Once the clinician is satisfied stalk "S" is sufficiently received between first and second electrodes **134**, **136**, generator **10** may be activated to treat the tissue between first and second electrodes **134**, **136**. Alternatively, and as discussed above, generator **10** may include a system for monitoring the electrical properties of the tissue between first and second electrodes **134**, **136**. Once a predetermined condition has been satisfied, preferably, a condition suitable to promote tissue sealing, generator **10** signals to the clinician that the tissue is ready to be sealed, at which point, generator **10** may automatically provide electrosurgical energy to tissue contacting surfaces **134c**, **136c**, or the clinician may activate generator **10** to provide the energy to seal the tissue. Electrosurgical energy is provided to tissue contacting surfaces **134c**, **136c** until the tissue of stalk "S" is properly sealed. Electrosurgical energy may be provided at a range of frequencies, over a variable duration, and may be continuous or intermittent, depending of the type of tissue being treated and the thickness of the tissue. Furthermore, the monitoring function may include for a signal to denote that the sealing is finished and that severing of the polyp "P" may take place.

In some embodiments, in order to effectively seal larger vessels (or tissue) two predominant mechanical parameters should be accurately controlled—the pressure applied to the vessel (tissue) and the gap distance between the electrodes—both of which are affected by the thickness of the sealed vessel. More particularly, accurate application of pressure may be important to oppose the walls of the vessel; to reduce the tissue impedance to a low enough value that allows enough electrosurgical energy through the tissue; to overcome the forces of expansion during tissue heating; and to contribute to the end tissue thickness, which is an indication of a good seal. It has been determined that a typical fused vessel wall is preferably between 0.001 and 0.006 inches. Below this range, the seal may shred or tear and above this range the lumens may not be properly or effectively sealed.

With respect to smaller vessels, the pressure applied to the tissue tends to become less relevant, whereas the gap distance between the electrically conductive surfaces becomes more significant for effective sealing. In other words, the chances of the two electrically conductive surfaces touching during activation increases as vessels become smaller.

As mentioned above, at least one electrode, e.g., **134**, may include a stop member **134d** that limits the movement of the two opposing electrodes **134**, **136** relative to one another. Stop member **134d** may extend from the tissue contacting surface **134c** a predetermined distance according to the specific material properties (e.g., compressive strength, thermal

expansion, etc.) to yield a consistent and accurate gap distance "G" during sealing (FIG. 5). In one embodiment, the gap distance between opposing tissue contacting surfaces **134c**, **136c** during sealing ranges from about 0.001 inches to about 0.006 inches and, preferably, between about 0.002 and about 0.003 inches. The non-conductive stop members **134d**, **136d** may be molded onto electrodes **134**, **136** (e.g., overmolding, injection molding, etc.), stamped onto electrodes **134**, **136** or deposited (e.g., deposition) onto electrodes **134**, **136**. For example, one technique involves thermally spraying a ceramic material onto the surface of the electrodes **134**, **136** to form the stop members **134d**, **136d**, respectively. Several thermal spraying techniques are contemplated that involve depositing a broad range of heat resistant and insulative materials on various surfaces to create stop members **134d**, **136d** for controlling the gap distance between electrically conductive surfaces **134c**, **136c**.

It has also been found that the pressure range for assuring a consistent and effective seal may be between about 3 kg/cm<sup>2</sup> to about 16 kg/cm<sup>2</sup> and, preferably, within a working range of 7 kg/cm<sup>2</sup> to 13 kg/cm<sup>2</sup>. Manufacturing an instrument that is capable of providing a closure pressure within this working range has been shown, in some embodiments, to be effective for sealing arteries, tissues and other vascular bundles.

As can be appreciated, controlling the compressive force between first and second electrodes **134**, **136** as snare portion **130** is retracted may facilitate and assure consistent, uniform and accurate closure pressure about the tissue within the desired working pressure range of about 3 kg/cm<sup>2</sup> to about 16 kg/cm<sup>2</sup> and, preferably, about 7 kg/cm<sup>2</sup> to about 13 kg/cm<sup>2</sup>. By controlling the intensity, frequency and duration of the electrosurgical energy applied to the tissue, the user can either cauterize, coagulate/desiccate, seal and/or simply reduce or slow bleeding.

In one embodiment, by controlling the force applied to handle **126**, the resulting tension in snare portion **130** may be adjusted, which, in turn, regulates the overall pressure between electrodes **134**, **136** to within the above-identified desired sealing range. A sensor **125** may be employed to accomplish this purpose and may be mechanically coupled to handle portion **120** and/or snare portion **130**. A visual or audible indicator (not shown) may be operably coupled to handle portion **120**, snare portion **130** and/or sensor **125** to provide visual, audible or tactile feed back to the user to assure that the clamping pressure is within the desired range prior to activation of the instrument.

Alternatively, handle portion **120** may incorporate a spring mechanism **125a** configured to prevent excessive force being applied to snare portion **130**, thereby preventing overcompression of the tissue between first and second electrodes **134**, **136**. Spring mechanism **125a** may include a compression spring (not shown) that deforms once the force applied to handle **126** exceeds the force necessary to accomplish effective sealing between first and second electrodes **134**, **136**. In an alternative embodiment, snare portion **130** may instead be advanced and retracted through the rotation of handle **126**. In this manner, handle portion **120** may include a torque mechanism, e.g., torque wrench or the like, (not shown) which is precisely set to measure the torque (rotational force) applied to snare portion **130** so the closure pressure between electrodes **134**, **136** will fall within the desired pressure range.

Once the tissue of stalk "S" is sealed, handle **126** is partially advanced to extend a length of snare portion **130** from tubular member **110**, thereby approximating proximal ends **134a**, **136a** of first and second electrodes, respectively, away from each other and exposing sealed stalk "S" to first sharpened surface **133a** of connection member **133**. While main-

taining snare portion 130 relative to tubular member 110, tubular member 110 is retracted relative to polyp "P", thereby causing the engagement of stalk "S" with first sharpened surface 133a of connection member 133. Continued retraction of tubular member 110 causes the complete severing of stalk "S" (see FIG. 9).

When using polyp removal device 110, the likelihood of excessive bleeding is greatly reduced because the tissue is completely sealed prior to being cut. Using polyp removal device 110 further reduces the likelihood of creating an open wound that is susceptible to infection. In addition, the utilization of bipolar energy to seal a polyp or other tissue is safer than monopolar, e.g., because of less thermal and energy spread, thereby reducing the likelihood of perforations.

With reference now to FIG. 10, an alternative embodiment of the present disclosure is shown generally as polyp removal device 200. Polyp removal device 200 is substantially similar to polyp removal device 100 and will, therefore, only be described as relates to the differences therebetween. Snare portion 230 includes first and second electrodes 234, 236 and a connection member 233. Extending between first and second electrodes 234, 236 and connection member 233 are extension members 235, 237, respectively. Extension members 235, 237 permit first and second electrodes 234, 236 to be spaced further apart from one another in a second or sealing condition. In this manner, polyp removal device 200 may be used to excise larger polyps having a larger stalk.

Various changes in form, detail and operation of the polyp removal devices of the present disclosure may be made without departing from the spirit and scope of the present disclosure.

What is claimed is:

1. A tissue removal system comprising:
  - a tubular member having proximal and distal ends, *the tubular member defining a longitudinal axis between the proximal and distal ends thereof; and*
  - a snare portion operably extending from the distal end of the tubular member and including first and second electrodes configured to treat tissue therebetween, the snare portion further including a cutting member having a sharpened surface positioned between the first and second electrodes for severing the treated tissue, *the sharpened surface elongated in a direction transverse to the longitudinal axis of the tubular member, the first and second electrodes hingedly attached to the cutting member.*
2. The tissue removal system of claim 1, further comprising a handle portion operatively coupled to the proximal end of the tubular member.
3. The tissue removal system of claim 2, wherein the handle portion is configured for operable engagement by a user.
4. The tissue removal system of claim 1, wherein the cutting member is configured to only cut when pulled in a proximal direction.
5. The tissue removal system of claim 1, wherein the tissue is a polyp and the first and second electrodes are configured to grasp a stalk of a polyp.

[6. The tissue removal system of claim 2, wherein the first and second electrodes are hingedly attached to the cutting member.]

7. The tissue removal system of claim 1, wherein the snare portion is configured to be retracted within the tubular member.

8. The tissue removal system of claim 1, wherein the first and second electrodes are each formed from a tissue contacting surface and an insulative body portion.

9. The tissue removal system of claim 1, further including an electrosurgical generator.

10. The tissue removal system of claim 9, wherein the first and second electrodes are electrically coupled to the electrosurgical generator and the generator is configured to deliver energy to the first and second electrodes in a bipolar manner.

[11. The tissue removal system of claim 1, wherein the distal end of the tubular member includes a spacer member for preventing the first and second electrodes from contacting one another.]

12. The tissue removal system of claim 1, [wherein at least one of the first and second electrodes includes] *further including a spacer [member] mounted [thereon] on at least one of the first and second electrodes* for preventing contact between the first and second electrodes.

13. A tissue removal system comprising:  
a generator configured to generate and deliver energy to a tissue removal device, the tissue removal device comprising:

a tubular member having proximal and distal ends;  
a handle portion operatively extending from the proximal end of the tubular member; and

a snare portion slidably supported within the tubular member and configured to extend from the distal end of the tubular member, the snare portion including first and second electrodes operably mounted thereto for receiving energy from the generator for treating tissue therebetween;

a cutting member having a sharpened surface positioned between the first and second electrodes and configured to sever the treated tissue, *the first and second electrodes hingedly attached to the cutting member; and*

[wherein at least one of the first and second electrodes includes] at least one spacer [mounted thereon] *secured to a proximal portion of at least one of the first and second electrodes* for preventing contact between the first and second electrodes.

14. The tissue removal device of claim 13, wherein the snare portion is formed from a non-conductive material.

15. The tissue removal system of claim 13, wherein the energy is selected from the group consisting of radiofrequency, ultrasonic, microwave, and laser.

16. *The tissue removal system of claim 1, further including a spacer member disposed within, and secured to, the distal end of the tubular member to prevent the first and second electrodes from contacting one another.*

\* \* \* \* \*

专利名称(译)	息肉清除装置和使用方法		
公开(公告)号	<a href="#">USR46063</a>	公开(公告)日	2016-07-12
申请号	US14/561461	申请日	2014-12-05
[标]申请(专利权)人(译)	柯惠有限合伙公司		
申请(专利权)人(译)	COVIDIEN LP		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	REGADAS F SERGIO P		
发明人	REGADAS, F. SERGIO P.		
IPC分类号	A61B18/18 A61B17/24 A61B17/3205 A61B18/14 A61B17/221 A61B18/00 A61B18/20 A61B17/32		
优先权	61/063158 2008-01-31 US		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

提供了一种用于移除组织（例如息肉）的装置和系统，其包括具有近端和远端的管状构件，从管状构件的远端内可操作地延伸的圈套部分，并包括构造成在其间处理组织的第一和第二电极，圈套部分还包括用于切断处理过的组织的切割构件。组织去除装置还可包括手柄部分，其可操作地从管状构件的近端内延伸。手柄部分可以配置成可由使用者操作，并且切割构件可以在第一和第二电极的远端之间延伸。

