



(11) **EP 1 684 075 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
11.08.2010 Bulletin 2010/32

(51) Int Cl.:
G01N 33/569 (2006.01) G01N 33/53 (2006.01)
G01N 33/543 (2006.01)

(21) Application number: **06447013.1**

(22) Date of filing: **23.01.2006**

(54) **Method and reagent for classifying leukocytes in animal blood**

Verfahren und Reagenz zur Klassifizierung von Leukozyten in Tierblut

Procédé et réactif pour classifier les leucocytes dans le sang animal

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI SK TR

• **Hirayama, Hideki,**
Sysmex Corporation
Kobe-shi,
Hyogo 651-0073 (JP)

(30) Priority: **24.01.2005 JP 2005016035**

(74) Representative: **De Clercq, Ann G. Y. et al**
De Clercq & Partners cvba
Edgard Gevaertdreef 10 a
9830 Sint-Martens-Latem (BE)

(43) Date of publication of application:
26.07.2006 Bulletin 2006/30

(73) Proprietor: **SYSMEX CORPORATION**
Kobe-shi,
Hyogo 651-0073 (JP)

(56) References cited:
US-A- 4 485 175 US-A- 4 745 071
US-A- 5 763 280 US-A- 6 143 567

(72) Inventors:
• **Matsumoto, Hideaki,**
Sysmex Corporation
Kobe-shi,
Hyogo 651-0073 (JP)
• **Shiraishi, Junichi,**
Sysmex Corporation
Kobe-shi,
Hyogo 651-0073 (JP)

• **PEEBLES D ET AL: "Extended leukocyte parameters for hematology analyzers." ANNALS OF THE NEW YORK ACADEMY OF SCIENCES 1986, vol. 468, 1986, pages 104-112, XP009100510 ISSN: 0077-8923**

EP 1 684 075 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

5 1. Field of the Invention

[0001] The present invention relates to a method and reagent for classifying leukocytes in animal blood.

10 2. Description of the Related Art

[0002] In treatment or diagnosis of canine and feline diseases, blood examination is an essential examination. Information useful for treatment or diagnosis of leukemia, infections and allergic diseases is obtained in examination of leukocytes, and information useful for treatment and diagnosis of anemia is obtained in examination of hemoglobin.

15 **[0003]** The method of measuring human leukocytes has already been established. In the method, a lysing reagent is added to a human blood sample to lyse erythrocytes in the sample, and the remaining leukocytes are counted with a hemocytometer. By devising ingredients of the lysing reagent, it is possible not only to count total leukocytes, but also to classify the leukocytes into a plurality of sub-groups and count leukocytes in a specific sub-group (see, for example, U.S. Patent Nos. 4,346,018, 4,485,175 and 5,116,539 and Japanese Laid-Open Patent Application Publication Nos. H02-031162 and H03-020667). Alternatively, a plurality of aliquots are prepared from a blood sample, and different
20 lysing reagents are added to the respective aliquots, to measure specific sub-groups of leukocytes, and from the obtained results, the leukocytes can be classified into 5 sub-groups.

[0004] In measurement of hemoglobin, a cyan methemoglobin method is used as an international standard method. However, the cyan methemoglobin method makes use of a toxic cyan compound, thus making disposal of waste-fluid necessary. Therefore, in recent years, hemoglobin is also measured by a method of using no cyan compound; for
25 example, SLS hemoglobin method, methemoglobin method etc. (see, for example, U.S. Patent Nos. 5,250,437 and 5,968,832).

[0005] A hemocytometer for animal blood has been commercially available. In the hemocytometer, a reagent for human blood is used, and a program for analysis is altered to suit an animal species to be measured (see, for example,
30 U.S. Patent No. 6,391,263).

[0006] When a quaternary ammonium salt-containing lysing reagent for human blood is used to measure a canine or feline blood sample by an electric resistance detection method, the distribution of leukocyte sizes appears as a single peak, so the erythrocytes cannot be classified into a plurality of sub-groups (see, for example, WO 2002/014861, J. Anim. Clin. Med., 10(3) 129-134, 2001). This is because canine or feline leukocytes are fragile and sensitive to the quaternary ammonium salt as compared with human leukocytes.

35 **[0007]** To cope with this problem, WO 2002/014861 supra describes a method of measuring leukocytes by using the quaternary ammonium salt at a lower concentration than that for human blood (that is, the concentration of the salt in a solution measured for leukocytes is 1.5 to 4.5 g/L). It is described therein that according to this method, leukocytes in a blood sample such as a canine or feline sample can be classified into 3 sub-groups, that is, lymphocytes, "mixed cell group" composed mainly of monocytes, and granulocytes.

40 **[0008]** However, the method described in WO 2002/014861 supra cannot classify eosinophils into a sub-group by distinguishing them from other leukocytes. In examination of leukocytes, the number of eosinophils is information useful for diagnosis of allergic diseases and parasitosis. Particularly, canine and feline parasitosis is well known in the field of pet, and canine and feline allergic diseases are rapidly increasing in recent years. For diagnosis of allergic diseases and parasitosis for canine and feline, therefore, it is important that in blood examination, eosinophils be classified by
45 distinguishing them from other leukocytes.

[0009] When the present inventors compared a result obtained by the method described in WO 2002/014861 supra with a result obtained by a visual examination, the correlation therebetween was low.

SUMMARY OF THE INVENTION

50 **[0010]** The object of the present invention is to provide a method and reagent for classifying leukocytes contained in a canine or feline blood sample into 3 groups by distinguishing eosinophils from other leukocytes.

[0011] A first aspect of the present invention relates to a method for classifying leukocytes in animal blood, comprising the steps of: preparing a measurement sample by mixing a canine or feline blood sample with a lysing reagent, wherein erythrocytes are lysed and leukocytes are shrunk in the measurement sample; measuring data correlated with the size
55 of leukocytes in the measurement sample; and classifying the leukocytes, on the basis of the measured data, into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils.

5 [0012] A second aspect of the present invention relates to a lysing reagent for classifying leukocytes in a canine or feline blood sample into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils, comprising: a quaternary ammonium salt lysing erythrocytes and shrinking leukocytes in the blood sample, and an aqueous solvent dissolving the quaternary ammonium salt, wherein the concentration of the quaternary ammonium salt is a concentration satisfying the following conditions: (1) erythrocytes are sufficiently lysed, and (2) leukocytes are shrunk such that the leukocytes can be classified, on the basis of their size, into the first, second and third groups.

10 BRIEF DESCRIPTION OF THE DRAWINGS

[0013]

15 Fig. 1 shows the particle size distribution obtained by measuring a human blood sample with a lysing reagent 1 in Measurement Example 1.

Fig. 2 shows the particle size distribution obtained by measuring a dog blood sample with a lysing reagent 1 in Measurement Example 1.

Fig. 3 shows the particle size distribution obtained by measuring a cat blood sample with a lysing reagent 1 in Measurement Example 1.

20 Fig. 4 shows the particle size distribution obtained by measuring a dog blood sample with a lysing reagent 2 in Measurement Example 2.

Fig. 5 shows the particle size distribution obtained by measuring a dog blood sample with a lysing reagent 3 in Measurement Example 2.

Fig. 6 shows the particle size distribution obtained by measuring a dog blood sample with a lysing reagent 4 in Measurement Example 2.

25 Fig. 7 shows the particle size distribution obtained by measuring a dog blood sample with a lysing reagent 5 in Measurement Example 2.

Fig. 8 shows the particle size distribution obtained by measuring a dog blood sample with a lysing reagent 6 in Measurement Example 2.

30 Fig. 9 shows the particle size distribution obtained by measuring a cat blood sample with a lysing reagent 5 in Measurement Example 2.

Fig. 10 shows the particle size distribution obtained by measuring a cat blood sample with a lysing reagent 6 in Measurement Example 2.

Fig. 11 shows one example of the particle size distribution obtained by measuring a dog blood sample with a lysing reagent 7 in Measurement Example 3.

35 Fig. 12 shows the particle size distribution obtained by measuring a dog blood sample (dog 1) with a lysing reagent 7 in Measurement Example 3.

Fig. 13 shows the particle size distribution obtained by measuring a dog blood sample (dog 2) with a lysing reagent 7 in Measurement Example 3.

40 Fig. 14 shows the correlation of small cell ratio (SCR) obtained with a lysing reagent 7 with lymphocyte ratio obtained by a visual examination for a dog blood sample in Measurement Example 3.

Fig. 15 shows the correlation of small cell count (SCC) obtained with a lysing reagent 7 with lymphocyte count obtained by a visual examination for a dog blood sample in Measurement Example 3.

Fig. 16 shows the correlation of middle cell ratio (MCR) obtained with a lysing reagent 7 with neutrophil ratio obtained by a visual examination for a dog blood sample in Measurement Example 3.

45 Fig. 17 shows the correlation of middle cell ratio (MCR) obtained with a lysing reagent 7 with neutrophil ratio + monocyte ratio obtained by a visual examination for a dog blood sample in Measurement Example 3.

Fig. 18 shows the correlation of middle cell count (MCC) obtained with a lysing reagent 7 with the number of neutrophils + number of monocytes obtained by a visual examination for a dog blood sample in Measurement Example 3.

50 Fig. 19 shows the correlation of large cell ratio (LCR) obtained with a lysing reagent 7 with eosinophil ratio obtained by a visual examination for a dog blood sample in Measurement Example 3.

Fig. 20 shows the correlation of large cell ratio (LCR) obtained with a lysing reagent 7 with eosinophil ratio + monocyte ratio obtained by a visual examination for a dog blood sample in Measurement Example 3.

55 Fig. 21 shows the correlation of large cell count (LCC) obtained with a lysing reagent 7 with the number of eosinophils obtained by a visual examination for a dog blood sample in Measurement Example 3.

Fig. 22 shows one example of the particle size distribution obtained by measuring a cat blood sample with a lysing reagent 7 in Measurement Example 3.

Fig. 23 shows the particle size distribution obtained by measuring a cat blood sample (cat 1) with a lysing reagent

7 in Measurement Example 3.

Fig. 24 shows the particle size distribution obtained by measuring a cat blood sample (cat 2) with a lysing reagent 7 in Measurement Example 3.

5 Fig. 25 shows the correlation of small cell ratio (SCR) obtained with a lysing reagent 7 with lymphocyte ratio obtained by a visual examination for a cat blood sample in Measurement Example 3.

Fig. 26 shows the correlation of small cell count (SCC) obtained with a lysing reagent 7 with the number of lymphocytes obtained by a visual examination for a cat blood sample in Measurement Example 3.

Fig. 27 shows the correlation of middle cell ratio (MCR) obtained with a lysing reagent 7 with neutrophil ratio obtained by a visual examination for a cat blood sample in Measurement Example 3.

10 Fig. 28 shows the correlation of middle cell ratio (MCR) obtained with a lysing reagent 7 with neutrophil ratio + monocyte ratio obtained by a visual examination for a cat blood sample in Measurement Example 3.

Fig. 29 shows the correlation of middle cell count (MCC) obtained with a lysing reagent 7 with the number of neutrophils + number of monocytes obtained by a visual examination for a cat blood sample in Measurement Example 3.

15 Fig. 30 shows the correlation of large cell ratio (LCR) obtained with a lysing reagent 7 with eosinophil ratio obtained by a visual examination for a cat blood sample in Measurement Example 3.

Fig. 31 shows the correlation of large cell ratio (LCR) obtained with a lysing reagent 7 with eosinophil ratio + monocyte ratio obtained by a visual examination for a cat blood sample in Measurement Example 3.

20 Fig. 32 shows the correlation of large cell count (LCC) obtained with a lysing reagent 7 with the number of eosinophils obtained by a visual examination for a cat blood sample in Measurement Example 3.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

25 **[0014]** First, the present inventors measured human, canine and feline blood samples with a lysing reagent for human blood and then compared classification results of erythrocytes (Example 1). In the Example 1, a blood sample from dog was used as the canine blood sample, and a blood sample from a cat was used as a feline blood sample.

Example 1

30 **[0015]** On the basis of a description of U.S. Patent No. 5,968,832, the present inventors prepared a lysing reagent (lysing reagent 1) capable of classifying human leukocytes into 3 sub-groups, that is, lymphocytes, neutrophils and other leukocytes. The composition of the lysing reagent 1 is as follows:

Lysing reagent 1

35

[0016]

40

Lauryl trimethyl ammonium chloride	7.9 g/L (30 mM)
Stearyl trimethyl ammonium chloride	0.84 g/L (2.4 mM)
Sodium chloride	4.13 g
Succinic acid	3.0 g
EDTA-2K	2.5 g
Sodium hydroxide	1.55 g
Purified water	1 L
pH 5.3	

45

50 **[0017]** Using the lysing reagent 1, human, dog and cat blood samples were measured with an automatic hemocytometer pocH-100iV (Sysmex Corporation). In this hemocytometer, a blood sample is diluted with a diluent pocH-pack D (Sysmex Corporation) to prepare a sample diluted 500-fold. Then, one volume of the lysing reagent 1 is added to two volumes of the diluted sample to prepare a measurement sample. Thirteen seconds after the lysing reagent is added, leukocytes are counted for 6 seconds in a detector in an electric resistance system. In this example, the measured signal was transmitted from the detector via an RS-232C cable to a personal computer, and from the inputted signal, the count and the particle-size distribution were analyzed.

55 **[0018]** A smear was prepared from the blood sample used in measurement and then subjected to May-Grünwald-Giemsa staining, and the leukocytes were visually classified and counted.

[0019] Fig. 1 shows the particle size distribution obtained by measuring a human blood sample. Fig. 2 shows the

particle size distribution obtained by measuring a dog blood sample. Fig. 3 shows the particle size distribution obtained by measuring a cat blood sample. The correspondence between each sub-group on the particle size distribution and each sub-group of leukocytes can be confirmed by comparing data classified by the visual examination with data measured by the method of using the lysing reagent described above.

5 [0020] Similar to a description of U.S. Patent No. 5,968,832, a group containing lysed erythrocytes, a group containing lymphocytes, a group containing neutrophils, and a group containing other leukocytes appeared from the left to right in the particle size distribution in Fig. 1. In Figs. 2 and 3, on the other hand, a group of lysed erythrocytes and a group containing leukocytes appeared from the left to right. From Figs. 1 to 3, it was found that the lysing reagent 1 can classify human leukocytes into 3 sub-groups, but cannot classify dog or cat leukocytes into sub-groups. It was thus found that
10 when the lysing agent for human is used in classification of canine or feline leukocytes, it is difficult to classify the canine or feline leukocytes unlike human leukocytes.

[0021] In Fig. 1, eosinophils are not classified into an independent sub-group distinguished from other leukocytes. In blood examination of pets, especially canine and feline, however, classification of eosinophils by distinguishing them from other leukocytes is very important for diagnosis of allergic diseases and parasitosis, as described above.

15 [0022] Accordingly, the present inventors examined a lysing reagent for classifying canine and feline leukocytes, particularly a lysing reagent capable of classifying eosinophils into an independent sub-group distinguished from other leukocytes. In advancing this examination, the present inventors paid attention to a quaternary ammonium salt contained in the lysing reagent. As a result, they found a lysing reagent capable of classifying canine or feline leukocytes into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing
20 eosinophils.

[0023] The lysing reagent comprises a quaternary ammonium salt lysing erythrocytes and shrinking leukocytes in a blood sample and an aqueous solvent dissolving the quaternary ammonium salt. The concentration of the quaternary ammonium salt is a concentration satisfying the following conditions: The erythrocytes are sufficiently lysed; the leukocytes are shrunk such that the leukocytes can be classified on the basis of their size into 3 sub-groups, that is, a first
25 group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils.

[0024] Specifically, the concentration of the quaternary ammonium salt is preferably 1.5 mM or more in order to lyse erythrocytes sufficiently. For classifying leukocytes as described above, the concentration is preferably 20 mM or less, more preferably 14.5 mM or less.

30 [0025] As the quaternary ammonium salt, for example, an alkyl trimethyl ammonium salt having an alkyl group having a carbon number of 10 to 20 is used. The quaternary ammonium salt is preferably an alkyl trimethyl ammonium salt having an alkyl group having a carbon number of 12 to 18. The alkyl group includes a decane group, lauryl group, myristyl group, cetyl group, stearyl group etc.

35 [0026] As the number of carbon atoms in the alkyl group is increased, the power of the alkyl trimethyl ammonium salt to lyse erythrocytes and shrink leukocytes (hereinafter, abbreviated as lysis power) tends to increase. As the number of carbon atoms in the alkyl group is increased, the clouding point of the alkyl trimethyl ammonium salt tends to be lowered. Therefore, when one kind of alkyl trimethyl ammonium salt is used, inferior lysis of erythrocytes may occur, or leukocytes may be shrunk excessively, or precipitation may occur. For more evident classification of the sub-groups of leukocytes, it is preferable to combine a plurality of alkyl trimethyl ammonium salts in order to control the lysis power of
40 the lysing reagent as a whole. Such combination is preferably a combination of an alkyl trimethyl ammonium salt having an alkyl group containing fewer carbon atoms (first alkyl trimethyl ammonium salt) and an alkyl trimethyl ammonium salt having an alkyl group containing more carbon atoms (second alkyl trimethyl ammonium salt). Specifically, the first alkyl trimethyl ammonium salt includes a decane trimethyl ammonium salt and lauryl trimethyl ammonium salt, and the second alkyl trimethyl ammonium salt includes a cetyl trimethyl ammonium salt and stearyl trimethyl ammonium salt. The combination of the two is more preferably a combination of a lauryl trimethyl ammonium salt as the first alkyl trimethyl ammonium salt and a stearyl trimethyl ammonium salt as the second alkyl trimethyl ammonium salt.

45 [0027] When the two are combined, the concentration of the second alkyl trimethyl ammonium salt is preferably lower than the concentration of the first alkyl trimethyl ammonium salt. Specifically, the concentration of the lauryl trimethyl ammonium salt is preferably 20 mM or less, more preferably 8 to 20 mM. The concentration of the stearyl trimethyl ammonium salt is preferably 2 mM or less, more preferably 0.4 to 2 mM, most preferably 1 to 2 mM.

50 [0028] As the second alkyl trimethyl ammonium salt, a cetyl trimethyl ammonium salt can be used in place of the stearyl trimethyl ammonium salt. Because the lysis power of the alkyl trimethyl ammonium salt is increased as the number of carbon atoms in the alkyl group is increased, the lysis power of the cetyl trimethyl ammonium salt is lower than that of the stearyl trimethyl ammonium salt. It follows that when the cetyl trimethyl ammonium salt is used, the concentration thereof is preferably 3 mM or less, more preferably 1.5 to 3 mM.

55 [0029] A small amount of a myristyl trimethyl ammonium salt may further be combined with the combination described above. By doing so, the resulting lysing reagent can exhibit more stable lysis power on various samples. The concentration of the myristyl trimethyl ammonium salt is preferably 0.5 to 1.3 mM, more preferably 0.6 to 0.8 mM.

[0030] Further, a small amount of an alkyl dimethyl ethyl ammonium salt may be added to the lysing reagent. By doing so, a lysed erythrocyte can be shrunk more effectively. The alkyl dimethyl ethyl ammonium salt includes, for example, a cetyl dimethyl ethyl ammonium salt, and its concentration is preferably 0.4 to 1.1 mM, more preferably 0.5 to 0.8 mM.

[0031] Further addition of a nonionic surfactant having a Hydrophilic-Lipophilic-Balance (HLB) value of 17 to 20 to the lysing reagent is effective in obtaining a highly accurate particle size distribution by shrinking lysed erythrocytes and stabilizing shrunk leukocytes. Examples of the nonionic surfactant include polyoxyethylene cetyl ether, polyoxyethylene lauryl ether, polyoxyethylene oleyl ether, polyoxyethylene behenyl ether, polyoxyethylene nonyl phenyl ether and polyoxyethylene octyl phenyl ether, and the number of polyoxyethylene chains therein is preferably 20 to 100. The concentration of the nonionic surfactant is preferably 0.05 to 0.5 w/v%, more preferably 0.1 to 0.2 w/v%.

[0032] As a hemoglobin stabilizer, 5 to 30 mM nitrite salt, 5 to 30 mM nitrate salt, 5 to 50 mM alkyl trimethyl ammonium salt having an alkyl group having a carbon number 1 to 8 or 5 to 50 mM tetraalkyl ammonium salt having an alkyl group having a carbon number of 1 to 8 may be added to the lysing reagent. The alkyl group includes a methyl group, ethyl group, propyl group, butyl group, pentyl group, hexyl group, heptyl group and octyl group. Examples of the alkyl trimethyl ammonium salt and tetraalkyl ammonium salt include an ethyl trimethyl ammonium salt, octyl trimethyl ammonium salt, tetraethyl ammonium salt, tetrabutyl ammonium salt etc.

[0033] The above-mentioned aqueous solvent dissolving the quaternary salt includes water and buffers.

[0034] The osmotic pressure of the lysing reagent is kept preferably at 200 to 350 mmol/kg. The osmotic pressure can be regulated with an alkali metal salt such as sodium chloride or potassium chloride.

[0035] The lysing reagent is kept preferably at pH 4 to 9. For pH regulation, known buffers can be used.

[0036] By using the lysing reagent described above, canine and feline leukocytes can be classified and counted. In the method therefor, a canine or feline blood sample is first mixed with the lysing reagent to prepare a measurement sample. In this step, erythrocytes in this sample are lysed. On the other hand, leukocytes are shrunk to remain. Lysis of erythrocytes and shrinkage of leukocytes can occur simultaneously by regulating the type and concentration of the quaternary ammonium salt(s) contained in the lysing reagent, or can occur separately such that erythrocytes are first lysed and leukocytes are then shrunk or vice versa. It is not evident how leukocytes are shrunk, but it is estimated that by mixing a blood sample with the lysing reagent, the cell membrane of leukocyte in the sample is damaged thereby eluting the cytoplasm or baring the nucleus, through which the leukocytes are eventually shrunk. The size of the shrunk leukocytes varies depending on sub-group, so that depending on the size, the leukocytes can be classified into a sub-group and can be counted. Specifically, a lysing reagent is used which shrinks leukocytes such that the size of the leukocytes after shrinkage is made different among lymphocytes, neutrophils and monocytes, and eosinophils, whereby the leukocytes can be classified finally into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils. A measurement sample may be prepared by diluting the blood sample with a diluent, then adding the lysing reagent to the diluted blood sample, and reacting the mixture (for 11 to 15 seconds, for example). As the diluent, physiological saline or a buffer, pH 4 to 9, having an osmotic pressure of 200 to 350 mmol/kg can be used.

[0037] After the measurement sample is prepared as described above, data correlated with the size of leukocytes in the measurement sample are measured. On the basis of the measured data, the leukocytes are classified into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils. For example, when an electric resistance method is used in measurement, electric resistance can be mentioned as data correlated with the size of leukocytes. Specifically, the prepared measurement sample is sent to a detector in an electric resistance system in a measuring instrument. In the electric resistance method, the detector is provided with a pore, and both sides of the pore are provided with electrodes, respectively. Direct current is applied across the electrodes, and when a blood corpuscle is passed through the pore, the electric resistance varies in proportion to the volume of the blood corpuscle. This change in electric resistance is detected as a pulse signal, and a signal having pulse height higher than a predetermined level is counted as leukocyte. By converting the pulse height into volume and determining the frequency with which each pulse height is detected, the particle size distribution can be determined. In the determined particle size distribution, there appears a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils.

[0038] An optical method can also be used in measurement. In this case, the data correlated with the size of leukocytes includes forward scattered light. Specifically, a prepared measurement sample is sent to a detector in a measurement instrument. In the optical method, the detector is irradiated with light, and when a blood corpuscle is passed through the detector, forward scattered light corresponding to the size of the blood corpuscle is detected. On the basis of the intensity of this forward scattered light, the particle size distribution is determined, and leukocytes can be classified into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils.

[0039] The correspondence between each sub-group appearing on the particle size distribution and each sub-group of leukocytes can be confirmed by measuring a sample of each sub-group (for example, a sample of separated lymphocytes) separated from a blood sample, and determining the position of the sample in the particle size distribution.

EP 1 684 075 B1

Alternatively, the correspondence between each sub-group on the particle size distribution and each sub-group of leukocytes can be confirmed by preparing a smear of a blood sample and comparing data on leukocytes in the smear classified by the visual examination, with data on leukocytes measured by the method of using the lysing reagent described above. Further, a threshold value for dividing the respective sub-groups on the particle size distribution can be established in the position where the difference in the both data becomes minimum. Alternatively, a variable threshold value can be established wherein a valley of particle-size distribution is detected for each sample and the position of the valley is assumed as the threshold value.

[0040] By the method of classifying leukocytes with the lysing reagent described above, canine and feline leukocytes can be classified, on the basis of their size, into small leukocytes, middle leukocytes and large leukocytes. The small leukocytes contain lymphocytes, the middle leukocytes contain neutrophils and monocytes, and the large leukocytes contain eosinophils. Because the frequency with which basophils appear in blood is very low, which group basophils belong to is hardly specified, but it is estimated that basophils belong to the middle leukocytes.

[0041] The concentration of hemoglobin can be measured by measuring the absorbance of the above prepared measurement sample in the vicinity of 555 nm.

[0042] Hereinafter, measurement examples (Example 2 and Example 3) wherein canine and feline blood samples were measured with the lysing reagents described above are described in detail. In Example 2 and Example 3, a blood sample from dog was used as the canine blood sample, and a blood sample from a cat was used as a feline blood sample.

Example 2

[0043] Lysing reagents 2 to 6 having the same composition as in the lysing reagent 1 except for the concentrations and combination of the quaternary ammonium salts were prepared, and each lysing reagent was used to measure dog and cat blood samples. The quaternary ammonium salts used are as follows:

Alkyl trimethyl ammonium salts

- Decane trimethyl ammonium bromide (DTAB): number of carbon atoms in the alkyl group, 10
- Lauryl trimethyl ammonium chloride (LTAC): number of carbon atoms in the alkyl group, 12
- Myristyl trimethyl ammonium bromide (MTAB): number of carbon atoms in the alkyl group, 14
- Stearyl trimethyl ammonium chloride (STAC): number of carbon atoms in the alkyl group, 18

Alkyl dimethyl ethyl ammonium salt

- Cetyl dimethyl ethyl ammonium bromide (CDMEB): number of carbon atoms in the alkyl group, 16

[0044] The concentrations and combination of the quaternary ammonium salts in the lysing reagents 2 to 6 are as shown in Table 1.

Table 1

	Alkyl trimethyl ammonium salt (mM)				Alkyl dimethyl ethyl ammonium salt (mM)	Total concentration (mM)
	DTAB (C=10)	LTAC (C=12)	MTAB (C=14)	STAC (C=18)	CDMEB (C=16)	
Lysing reagent 2	0	18	0	1.44	0	19.44
Lysing reagent 3	0	15	0	1.2	0	16.2
Lysing reagent 4	0	15	1.2	0.48	1.06	17.74
Lysing reagent 5	12	0	0.6	1.2	0.53	14.33

EP 1 684 075 B1

(continued)

5	Alkyl trimethyl ammonium salt (mM)				Alkyl dimethyl ethyl ammonium salt (mM)	Total concentration (mM)	
	DTAB (C=10)	LTAC (C=12)	MTAB (C=14)	STAC (C=18)	CDMEB (C=16)		
10	Lysing reagent 6	0	9	0.6	1.44	0.53	11.57

[0045] Using the lysing reagents 2 to 6 shown in Table 1, dog blood samples were measured with an automatic hemocytometer poch-100iV (Sysmex Corporation). The measurement method was the same as in Example 1. In the same manner as in Example 1, smears were prepared from the blood samples used in measurement, and then subjected to May-Grünwald-Giemsa staining, and the leukocytes were visually classified and counted.

[0046] Fig. 4 shows the particle size distribution obtained by measuring a dog blood sample with the lysing reagent 2. Fig. 5 shows the particle size distribution obtained by measuring a dog blood sample with the lysing reagent 3. Fig. 6 shows the particle size distribution obtained by measuring a dog blood sample with the lysing reagent 4. Fig. 7 shows the particle size distribution obtained by measuring a dog blood sample with the lysing reagent 5. Fig. 8 shows the particle size distribution obtained by measuring a dog blood sample with the lysing reagent 6.

[0047] In any of the particle-size distributions in Figs. 4 to 8, three sub-groups of leukocytes (X, Y and Z) appeared. Comparison thereof with data classified by the visual examination revealed that the X is a group containing lymphocytes, the Y is a group containing neutrophils and monocytes, and the Z is a group containing eosinophils. When data on the respective sub-groups on the particle-size distribution are compared with data on the respective sub-groups obtained by the visual examination, high correlation was obtained particularly in Figs. 7 and 8.

[0048] From the forgoing, it was found that by using the lysing reagents 2 to 6, canine leukocytes can be classified into 3 sub-groups, that is, a group containing lymphocytes, a group containing neutrophils and monocytes, and a group containing eosinophils. It was also found that by using the lysing reagents 5 and 6, leukocytes can be classified more accurately.

[0049] Using the lysing reagents 5 and 6, cat blood samples were then measured in the same manner as for the dog blood samples. Fig. 9 shows the particle size distribution obtained by measuring a cat blood sample with the lysing reagent 5. Fig. 10 shows the particle size distribution obtained by measuring a cat blood sample with the lysing reagent 6.

[0050] In any of the particle-size distributions in Figs. 9 and 10, three sub-groups of leukocytes (X, Y and Z) appeared. Comparison thereof with data classified by the visual examination revealed that the X is a group containing lymphocytes, the Y is a group containing neutrophils and monocytes, and the Z is a group containing eosinophils.

[0051] From the forgoing, it was found that by using the lysing reagents 5 and 6, feline leukocytes similar to the canine leukocytes can be classified into 3 sub-groups, that is, a group containing lymphocytes, a group containing neutrophils and monocytes and a group containing eosinophils.

Example 3

[0052] Lysing reagent 7 having the following composition containing a nonionic surfactant was used to measure dog and cat blood samples. The nonionic surfactant contained in the lysing reagent 7 is Emulsit 9 (polyoxyethylene nonyl phenyl ether) that is a nonionic surfactant having an HLB of 17 to 20.

Lysing reagent 7

[0053]

Cation-AB	2.16 g
(Containing 23% stearyl trimethyl ammonium chloride, manufactured by Nippon Oil & Fats Co., Ltd.)	
Lauryl trimethyl ammonium chloride	2.39 g
Cetyl dimethyl ethyl ammonium bromide	0.2 g
Myristyl trimethyl ammonium bromide	0.2 g
Emulsit 9	1.0 g

EP 1 684 075 B1

(continued)

(Polyoxyethylene nonyl phenyl ether, manufactured by Dai-ichi Kogyo Seiyaku Co., Ltd.)

	Sodium chloride	4.13 g
5	Succinic acid	3.0 g
	EDTA-2K·2H ₂ O	2.5 g
	Sodium hydroxide	1.55 g
	Sodium nitrite	0.69 g
10	Purified water	1 L
	pH 5.3, osmotic pressure of 280 mmol/kg	

[0054] The lysing reagent 7 contains, as quaternary ammonium salts, 1.43 mM stearyl trimethyl ammonium chloride, 9 mM lauryl trimethyl ammonium chloride, 0.53 mM cetyl dimethyl ethyl ammonium bromide and 0.6 mM myristyl trimethyl ammonium bromide. Using the lysing reagent 7, 111 dog blood samples and 37 cat blood samples were measured with an automatic hemocytometer poch-100iV (Cysmex Corporation). The measurement method was the same as in Example 1. In the same manner as in Example 1, smears were prepared from the blood samples used in measurement, and then subjected to May-Grünwald-Giemsa staining, and the leukocytes were visually classified and counted.

20 <Dog blood sample>

[0055] One example of the particle size distribution measured in dog blood sample is shown in Fig. 11. In Fig. 11, the leftmost group is a group of lysed erythrocytes. Then, the first group (small leukocyte), the second group (middle leukocyte) and the third group (large leukocyte) appear in the order of small to large sizes.

25 **[0056]** Although the threshold value of each group varies slightly depending on the state of the particle-size distribution obtained, the threshold value was determined as follows: The threshold value between the group of lysed erythrocytes and the first group is in the vicinity of 48fl; the threshold value between the first and second groups is in the vicinity of 90fl; the threshold value between the second and third groups is set in the vicinity of 162fl; and the upper limit is set to 300fl.

30 **[0057]** Figs. 12 and 13 show the particle-size distributions of 2 samples (dogs 1 and 2) among the dog samples measured. In any of the distributions, similar to the distribution in Fig. 11, a group of lysed erythrocytes appeared in the leftmost position, and then the first group (small leukocyte), the second group (middle leukocyte) and the third group (large leukocyte) appeared in the order of small to large sizes.

35 **[0058]** Then, the data on the small, middle and large leukocytes appearing in the particle-size distributions in Figs. 12 and 13 were compared with data obtained by classifying and counting the leukocytes by the visual examination. The results are shown in Table 2.

Table 2

[0059]

	Classification of leukocytes with the lysing reagent 7			Classification of leukocytes by the visual examination			
	SCR (%)	MCR (%)	LCR (%)	Lymphocyte ratio (%)	Neutrophil ratio (%)	Monocyte ratio (%)	Eosinophil ratio (%)
45 Dog 1 (Fig. 12)	8.6	79.4	12.0	6	70	10	14
50 Dog 2 (Fig. 13)	13.1	57.9	29	10	63	0	27

[0060] In Table 2, SCR (%), MCR (%) and LCR (%) are values calculated on the basis of data on small leukocytes, middle leukocytes and large leukocytes appearing in the particle-size distributions in Figs. 12 and 13. SCR (%) is the ratio of the number of small leukocytes to the number of total leukocytes (small cell ratio (SCR)). MCR (%) is the ratio of the number of middle leukocytes to the number of total leukocytes (middle cell ratio (MCR)). LCR (%) is the ratio of the number of large leukocytes to the number of total leukocytes (large cell ratio (LCR)). On the other hand, lymphocyte ratio (%), neutrophil ratio (%), monocytes ratio (%) and eosinophil ratio (%) are values calculated on the basis of data obtained by classifying and counting leukocytes by the visual examination. Lymphocyte ratio (%) is the ratio of the

number of lymphocytes to the number of total leukocytes. Neutrophil ratio (%) is the ratio of the number of neutrophils to the number of total leukocytes. Monocyte ratio (%) is the ratio of the number of monocytes to the number of total leukocytes. Eosinophil ratio (%) is the ratio of the number of eosinophils to the number of total leukocytes.

[0061] From Table 2, it was found that the SCR value is close to the value of lymphocyte ratio. It was also found that the MCR is close to the total sum of monocyte ratio (%) and neutrophil ratio (%). It was further found that the LCR value is close to the value of eosinophil ratio.

[0062] Thus, the correlation of SCR with lymphocyte ratio obtained by the visual examination on dog blood samples (111 samples) was examined, and as a result, the correlation therebetween was better (Fig. 14). Accordingly, it is found that the small leukocyte group contains lymphocytes. The correlation of the number of small leukocytes (small cell count (SCC)) with the number of lymphocytes obtained by the visual examination was also better (Fig. 15).

[0063] Then, the correlation of MCR with neutrophil ratio obtained by the visual examination was examined (Fig. 16). Further, the correlation of MCR with neutrophil ratio + monocyte ratio obtained by the visual examination was examined (Fig. 17). The correlation in Fig. 17 was better as compared with Fig. 16. The correlation of the number of middle leukocytes (middle cell count (MCC)) with number of neutrophils + number of monocytes obtained by the visual examination was also better (Fig. 18).

[0064] Further, the correlation of LCR with eosinophil ratio obtained by the visual examination was examined (Fig. 19). Further, the correlation of LCR with eosinophil ratio + monocyte ratio obtained by the visual examination was examined (Fig. 20). The correlation in Fig. 19 was better as compared with Fig. 20. The correlation of the number of large leukocytes (large cell count (LCC)) with the number of eosinophils obtained by the visual examination was also better (Fig. 21).

[0065] In this example, a sample where basophils appeared was not found by the visual examination.

[0066] From the foregoing, it is found that the group of middle leukocytes contains neutrophils and monocytes, and the group of large leukocytes contains eosinophils.

<Cat blood sample>

[0067] One example of the particle size distribution measured in cat blood sample is shown in Fig. 22. In Fig. 22, the leftmost group is a group of lysed erythrocytes. Then, the first group (small leukocyte), the second group (middle leukocyte) and the third group (large leukocyte) appeared in the order of small to large sizes.

[0068] Although the threshold value of each group varies slightly depending on the state of the particle-size distribution obtained, the threshold value was determined as follows: The threshold value between the group of lysed erythrocytes and the first group is in the vicinity of 48fl; the threshold value between the first and second groups is in the vicinity of 96fl; the threshold value between the second and third groups is in the vicinity of 174fl; and the upper limit is 300fl.

[0069] Figs. 23 and 24 show the particle-size distributions of 2 samples (cats 1 and 2) among the cat samples measured. In any of the distributions, similar to the distribution in Fig. 22, a group of lysed erythrocytes appeared in the leftmost position, and then the first group (small leukocyte), the second group (middle leukocyte) and the third group (large leukocyte) appeared in the order of small to large sizes.

[0070] Then, the data on the small, middle and large leukocytes appearing in the particle-size distributions in Figs. 23 and 24 were compared with data obtained by classifying and counting the leukocytes by the visual examination. The results are shown in Table 3.

Table 3

	Classification of leukocytes with the lysing reagent 7			Classification of leukocytes by the visual examination			
	SCR (%)	MCR (%)	LCR (%)	Lymphocyte ratio (%)	Neutrophil ratio (%)	Monocyte ratio (%)	Eosinophil ratio (%)
Cat 1 (Fig. 23)	16.6	74.8	8.6	18	67	4	11
Cat 2 (Fig. 24)	44.7	42.3	13.0	39	40	5	16

[0071] In Table 3, SCR (%), MCR (%) and LCR (%) are values calculated on the basis of data on small leukocytes, middle leukocytes and large leukocytes appearing in the particle-size distributions in Figs. 23 and 24. SCR (%) is the ratio of the number of small leukocytes to the number of total leukocytes (small cell ratio (SCR)). MCR (%) is the ratio of the number of middle leukocytes to the number of total leukocytes (middle cell ratio (MCR)). LCR (%) is the ratio of

the number of large leukocytes to the number of total leukocytes (large cell ratio (LCR)). On the other hand, lymphocyte ratio (%), neutrophil ratio (%), monocytes ratio (%) and eosinophil ratio (%) are values calculated on the basis of data obtained by classifying and counting leukocytes by the visual examination. Lymphocyte ratio (%) is the ratio of the number of lymphocytes to the number of total leukocytes. Neutrophil ratio (%) is the ratio of the number of neutrophils to the number of total leukocytes. Monocyte ratio (%) is the ratio of the number of monocytes to the number of total leukocytes. Eosinophil ratio (%) is the ratio of the number of eosinophils to the number of total leukocytes.

[0072] From Table 3, it was found that the SCR value is close to the value of lymphocyte ratio. It was also found that the MCR is close to the total sum of monocyte ratio (%) and neutrophil ratio (%). It was further found that the LCR value is close to the value of eosinophil ratio.

[0073] Thus, the correlation of SCR with lymphocyte ratio obtained on cat blood samples (37 samples) by the visual examination was examined, and as a result, the correlation therebetween was better (Fig. 25). Accordingly, it is found that the small leukocyte group contains lymphocytes. The correlation of the number of small leukocytes (small cell count (SCC)) with the number of lymphocytes obtained by the visual examination was also better (Fig. 26).

[0074] Then, the correlation of MCR with neutrophil ratio obtained by the visual examination was examined (Fig. 27). Further, the correlation of MCR with neutrophil ratio + monocyte ratio obtained by the visual examination was examined (Fig. 28). The correlation in Fig. 28 was better as compared with Fig. 27. The correlation of the number of middle leukocytes (middle cell count (MCC)) with number of neutrophils + number of monocytes obtained by the visual examination was also better (Fig. 29).

[0075] Further, the correlation of LCR with neutrophil ratio obtained by the visual examination was examined (Fig. 30). Further, the correlation of LCR with eosinophil ratio + monocyte ratio obtained by the visual examination was examined (Fig. 31). The correlation in Fig. 30 was better as compared with Fig. 31. The correlation of the number of large leukocytes (large cell count (LCC)) with the number of eosinophils obtained by the visual examination was also better (Fig. 32).

[0076] In this example, a sample where basophils appeared was not found by the visual examination.

[0077] From the foregoing, it is found that the group of middle leukocytes contains neutrophils and monocytes, and the group of large leukocytes contains eosinophils.

<Hemoglobin concentration>

[0078] When dog blood samples and cat blood samples were measured for their hemoglobin concentrations with pocH-100iV by using the lysing reagent 7 and a conventional product Stomatorizer-WH (Sysmex Corporation), the correlation therebetween was better. It was thus confirmed that the hemoglobin concentration can be measured by the lysing reagent 7.

[0079] The method and reagent for classifying canine and feline leukocytes can give results of blood examination more accurately in more detail than conventional, thus enabling more suitable diagnosis and monitoring of therapy for canine and feline diseases including parasitosis and allergic diseases.

Claims

1. A method for classifying leukocytes in canine or feline blood into a first group containing lymphocytes, a second group containing neutrophils and monocytes, and a third group containing eosinophils, comprising the steps of:

preparing a measurement sample by mixing a canine or feline blood sample with a lysing reagent, wherein the lysing reagent comprises:

- a first alkyl trimethyl ammonium salt having a carbon number of 10 to 12;
- a second alkyl trimethyl ammonium salt having an alkyl group having a carbon number of 16 to 18; and
- an alkyl dimethyl ethyl ammonium salt,

wherein erythrocytes are lysed and leukocytes are shrunk in the measurement sample such that lymphocytes, neutrophils and monocytes, and eosinophils appear in the order of small to large sizes after shrinkage; measuring data correlated with the size of leukocytes in said measurement sample; and classifying the leukocytes, on the basis of said measured data, into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils.

2. The method according to claim 1, wherein the data correlated with the size of leukocytes in the measurement sample is electric resistance measured by an electric resistance method.

EP 1 684 075 B1

3. The method according to claim 1 or 2, wherein the concentration of the ammonium salt is 1.5 mM to 20 mM.
4. The method according to any one of claims 1 to 3, wherein the first alkyl trimethyl ammonium salt is selected from a lauryl trimethyl ammonium salt, and the second alkyl trimethyl ammonium salt is selected from the group consisting of a stearyl trimethyl ammonium salt and a cetyl trimethyl ammonium salt.
5. The method according to claim 4, wherein the concentration of the lauryl trimethyl ammonium salt is 8 to 20 mM, the concentration of the stearyl trimethyl ammonium salt is 0.4 to 2 mM, and the concentration of the cetyl trimethyl ammonium salt is 1.5 to 3 mM.
6. The method according to any one of claims 1 to 5, wherein the lysing reagent further comprises a myristyl trimethyl ammonium salt.
7. The method according to any of claims 1 to 6, wherein the lysing reagent further comprises a nonionic surfactant having a Hydrophilic-Lipophilic-Balance value of 17 to 20.
8. The method according to any of claims 1 to 7, wherein the pH value of the lysing reagent is 4 to 9.
9. A lysing reagent for classifying leukocytes in a canine or feline blood sample into a first group containing lymphocytes, a second group containing neutrophils and monocytes and a third group containing eosinophils, comprising:
- a first alkyl trimethyl ammonium salt having an alkyl group having a carbon number of 10 to 12;
 - a second alkyl trimethyl ammonium salt having an alkyl group having a carbon number of 16 to 18;
 - an alkyl dimethyl ethyl ammonium salt; and
 - an aqueous solvent dissolving said quaternary ammonium salt.
10. The reagent according to claim 9, wherein the concentration of the ammonium salts is 1.5 mM to 20 mM.
11. The reagent according to claim 9 or 10, wherein the first alkyl trimethyl ammonium salt is selected from a lauryl trimethyl ammonium salt, and the second alkyl trimethyl ammonium salt is selected from the group consisting of a stearyl trimethyl ammonium salt and a cetyl trimethyl ammonium salt.
12. The reagent according to claim 11, wherein the concentration of the lauryl trimethyl ammonium salt is 8 to 20 mM, the concentration of the stearyl trimethyl ammonium salt is 0.4 to 2 mM, and, the concentration of the cetyl trimethyl ammonium salt is 1.5 to 3 mM.
13. The reagent according to any of claims 9 to 12, which further comprises a nonionic surfactant having a Hydrophilic-Lipophilic-Balance value of 17 to 20.
14. The reagent according to any of claims 9 to 13, wherein the aqueous solvent is a buffer keeping the pH in the range of 4 to 9.

Patentansprüche

1. Verfahren zum Klassifizieren von Leukozyten in Hunde- oder Katzenblut in eine erste Gruppe, die Lymphozyten enthält, eine zweite Gruppe, die Neutrophile und Monozyten enthält, und eine dritte Gruppe, die Eosinophile enthält, umfassend die Schritte:
- Herstellen einer Messprobe durch Mischen einer Hunde- oder Katzenblutprobe mit einem Lyserreagenz, wobei das Lyserreagenz umfasst:
- ein erstes Alkyltrimethylammoniumsalz, das eine Anzahl der Kohlenstoffe von 10 bis 12 aufweist;
 - ein zweites Alkyltrimethylammoniumsalz, das eine Alkylgruppe enthält, die eine Anzahl der Kohlenstoffe von 16 bis 18 aufweist; und
 - ein Alkyldimethylethylammoniumsalz,

wobei die Erythrozyten in der Messprobe lysiert werden und die Leukozyten in der Messprobe schrumpfen,

EP 1 684 075 B1

derart, dass Lymphozyten, Neutrophile und Monozyten, und Eosinophile sich in der Reihenfolge von kleinen nach großen Größen nach dem Schrumpfen präsentieren;
Messen von Daten, die mit der Größe der Leukozyten in der Messprobe korreliert sind; und
Klassifizieren der Leukozyten auf der Basis der gemessenen Daten in eine erste Gruppe, die Leukozyten enthält,
eine zweite Gruppe, die Neutrophile und Monozyten enthält, und eine dritte Gruppe, die Eosinophile enthält.

2. Verfahren nach Anspruch 1, wobei die Daten, die mit der Größe der Leukozyten in der Messprobe korreliert sind, der elektrische Widerstand sind, gemessen durch ein Widerstandsmessverfahren.
3. Verfahren nach Anspruch 1 oder 2, wobei die Konzentration von dem Ammoniumsalz 1,5 mM bis 20 mM ist.
4. Verfahren nach einem der Ansprüche 1 bis 3, wobei das erste Alkyltrimethylammoniumsalz aus einem Lauryltrimethylammoniumsalz ausgewählt ist und das zweite Alkyltrimethylammoniumsalz aus der Gruppe ausgewählt ist, die aus einem Stearyltrimethylammoniumsalz und einem Cetyltrimethylammoniumsalz besteht.
5. Verfahren nach Anspruch 4, wobei die Konzentration von dem Lauryltrimethylammoniumsalz 8 bis 20 mM, die Konzentration von dem Stearyltrimethylammoniumsalz 0,4 bis 2 mM und die Konzentration von dem Cetyltrimethylammoniumsalz 1,5 bis 3 mM ist.
6. Verfahren nach einem der Ansprüche 1 bis 5, wobei das Lyseagens ferner ein Myristyltrimethylammoniumsalz umfasst.
7. Verfahren nach einem der Ansprüche 1 bis 6, wobei das Lyseagens ferner ein nichtionisches Tensid umfasst, das einen Wert für das Hydrophil-Lipophile-Gleichgewicht von 17 bis 20 aufweist.
8. Verfahren nach einem der Ansprüche 1 bis 7, wobei der pH-Wert von dem Lyseagens zwischen pH 4 bis 9 liegt.
9. Lyseagens zum Klassifizieren von Leukozyten in einer Hunde- oder Katzenblutprobe in eine erste Gruppe, die Lymphozyten enthält, eine zweite Gruppe, die Neutrophile und Monozyten enthält, und eine dritte Gruppe, die Eosinophile enthält, umfassend:
 - ein erstes Alkyltrimethylammoniumsalz, das eine Alkylgruppe enthält, die eine Anzahl der Kohlenstoffe von 10 bis 12 aufweist;
 - ein zweites Alkyltrimethylammoniumsalz, das eine Alkylgruppe enthält, die eine Anzahl der Kohlenstoffe von 16 bis 18 aufweist;
 - ein Alkyldimethylethylammoniumsalz; und
 - ein wässriges Lösemittel, welches das quaternäre Ammoniumsalz auflöst.
10. Reagens nach Anspruch 9, wobei die Konzentration von den Ammoniumsalzen 1,5 mM bis 20 mM ist.
11. Reagens nach einem der Ansprüche 9 oder 10, wobei das erste Alkyltrimethylammoniumsalz aus einem Lauryltrimethylammoniumsalz ausgewählt ist und das zweite Alkyltrimethylammoniumsalz aus der Gruppe ausgewählt ist, die aus einem Stearyltrimethylammoniumsalz und einem Cetyltrimethylammoniumsalz besteht.
12. Verfahren nach Anspruch 11, wobei die Konzentration von dem Lauryltrimethylammoniumsalz 8 bis 20 mM, die Konzentration von dem Stearyltrimethylammoniumsalz 0,4 bis 2 mM und die Konzentration von dem Cetyltrimethylammoniumsalz 1,5 bis 3 mM ist.
13. Reagens nach einem der Ansprüche 9 bis 12, das ferner ein nichtionisches Tensid umfasst, das einen Wert für das Hydrophil-Lipophile-Gleichgewicht von 17 bis 20 aufweist.
14. Reagens nach einem der Ansprüche 9 bis 13, wobei das wässrige Lösemittel ein Puffer ist, der den pH-Wert in dem Bereich von pH 4 bis 9 hält.

Revendications

1. Procédé de classification de leucocytes de sang canin ou félin en un premier groupe contenant des lymphocytes,

EP 1 684 075 B1

un deuxième groupe contenant des neutrophiles et des monocytes et un troisième groupe contenant des éosinophiles, qui comprend les étapes consistant à :

5 préparer un échantillon de mesure en mélangeant un échantillon de sang canin ou félin avec un réactif de lyse, le réactif de lyse comprenant :

- un premier sel d'alkyl triméthyl ammonium ayant un nombre d'atomes de carbone de 10 à 12,
- un second sel d'alkyl triméthyl ammonium ayant un groupe alkyle ayant un nombre d'atomes de carbone de 16 à 18 ; et
- 10 - un sel d'alkyl diméthyl éthyl ammonium,

les érythrocytes étant lysés et les leucocytes étant rétrécis dans l'échantillon de mesure, de manière à ce que les lymphocytes, les neutrophiles et les monocytes, et les éosinophiles apparaissent dans l'ordre des tailles croissantes après le rétrécissement ;

15 mesurer les données corrélées à la taille des leucocytes dans ledit échantillon de mesure ; et classifier les leucocytes, sur la base desdites données mesurées, en un premier groupe contenant des lymphocytes, un deuxième groupe contenant des neutrophiles et des monocytes et un troisième groupe contenant des éosinophiles.

20 **2.** Procédé selon la revendication 1, dans lequel les données corrélées à la taille des leucocytes dans l'échantillon de mesure sont la résistance électrique mesurée par un procédé de résistance électrique.

3. Procédé selon la revendication 1 ou 2, dans lequel la concentration en sel d'ammonium est comprise entre 1,5 mM et 20 mM.

25 **4.** Procédé selon l'une quelconque des revendications 1 à 3, dans lequel le premier sel d'alkyl triméthyl ammonium est choisi parmi un sel de lauryl triméthyl ammonium, et le deuxième sel d'alkyl triméthyl ammonium est choisi dans le groupe constitué par un sel de stéaryl triméthyl ammonium et un sel de cétyle triméthyl ammonium.

30 **5.** Procédé selon la revendication 4, dans lequel la concentration en sel de lauryl triméthyl ammonium est de 8 à 20 mM, la concentration en sel de stéaryl triméthyl ammonium est de 0,4 à 2 mM, et la concentration en sel de cétyle triméthyl ammonium est de 1,5 à 3 mM.

35 **6.** Procédé selon l'une quelconque des revendications 1 à 5, dans lequel le réactif de lyse comprend en outre un sel de myristyle triméthyl ammonium.

7. Procédé selon l'une quelconque des revendications 1 à 6, dans lequel le réactif de lyse comprend en outre un surfactant non ionique ayant une valeur de HLB de 17 à 20.

40 **8.** Procédé selon l'une quelconque des revendications 1 à 7, dans lequel la valeur de pH du réactif de lyse est de 4 à 9.

9. Réactif de lyse destiné à classifier les leucocytes dans un échantillon de sang canin ou félin en un premier groupe contenant des lymphocytes, un deuxième groupe contenant des neutrophiles et des monocytes et un troisième groupe contenant des éosinophiles, qui comprend :

- un premier sel d'alkyl triméthyl ammonium ayant un groupe alkyle ayant un nombre d'atomes de carbone de 10 à 12 ;
- un second sel d'alkyl triméthyl ammonium ayant un groupe alkyle ayant un nombre d'atomes de carbone de 16 à 18 ; et
- 50 - un sel d'alkyl diméthyl éthyl ammonium, et
- un solvant aqueux dissolvant ledit sel d'ammonium quaternaire.

10. Réactif selon la revendication 9, dans lequel la concentration en sels d'ammonium est de 1,5 mM à 20 mM.

55 **11.** Réactif selon la revendication 9 ou 10, dans lequel le premier sel d'alkyl triméthyl ammonium est choisi parmi un sel de lauryl triméthyl ammonium, et le deuxième sel d'alkyl triméthyl ammonium est choisi dans le groupe constitué par un sel de stéaryl triméthyl ammonium et un sel de cétyle triméthyl ammonium.

EP 1 684 075 B1

12. Réactif selon la revendication 11, dans lequel la concentration en sel de lauryl triméthyl ammonium est de 8 à 20 mM, la concentration en sel stéaryl triméthyl ammonium est de 0,4 à 2 mM et la concentration en sel de cétyle triméthyl ammonium est de 1,5 à 3 mM.

5 13. Réactif selon l'une quelconque des revendications 9 à 12, qui comprend en outre un surfactant non ionique ayant une valeur de HLB de 17 à 20.

14. Réactif selon l'une quelconque des revendications 9 à 13, dans lequel le solvant aqueux est un tampon permettant de maintenir le pH dans la plage de 4 à 9.

10

15

20

25

30

35

40

45

50

55

Fig. 1

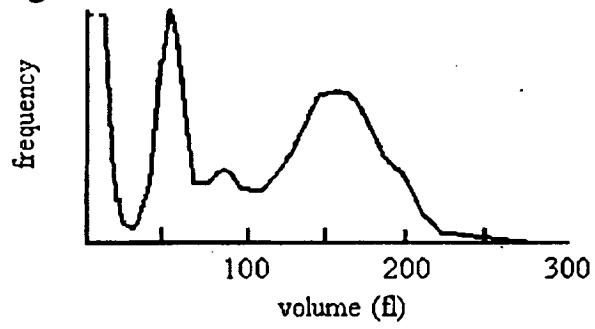


Fig. 2

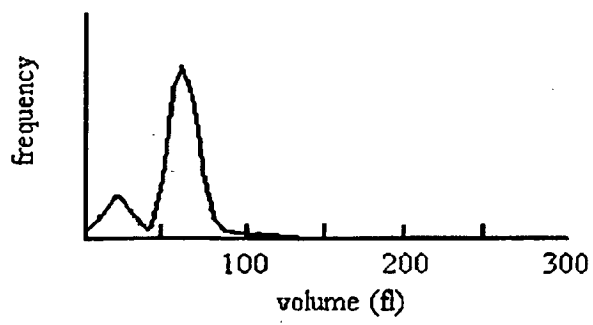


Fig. 3

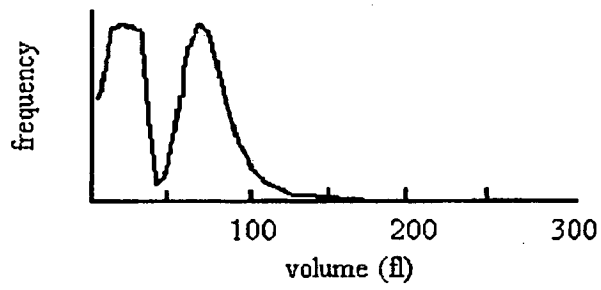


Fig. 4

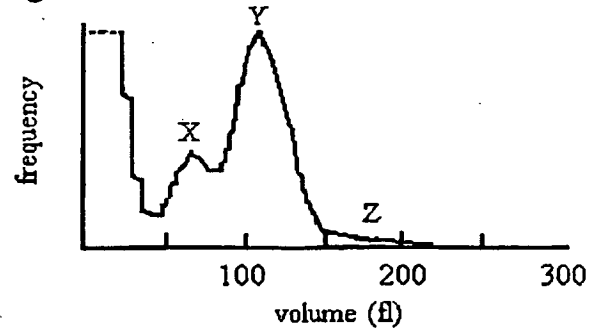


Fig. 5

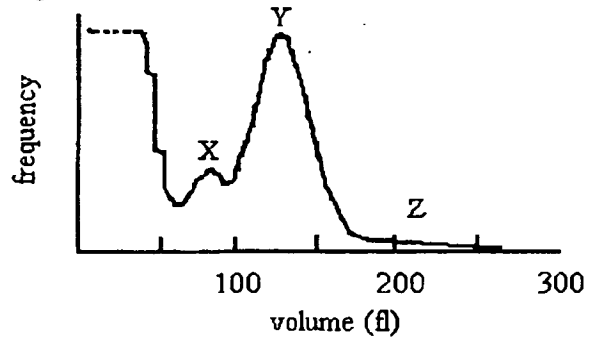


Fig. 6

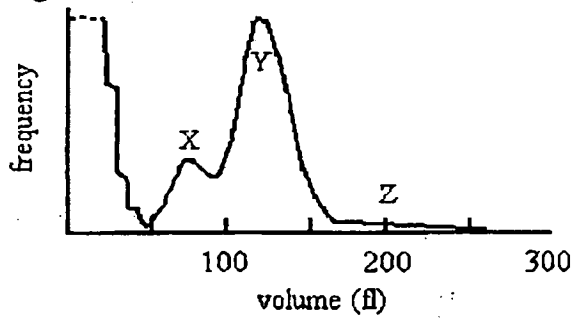


Fig. 7

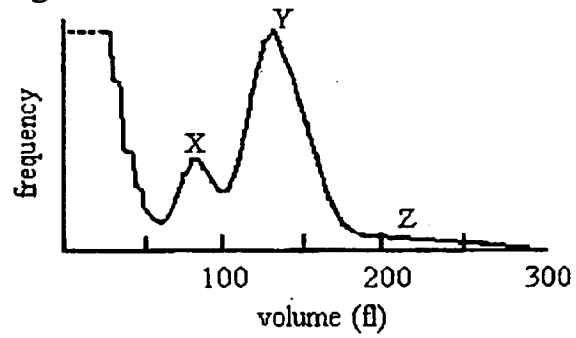


Fig. 8

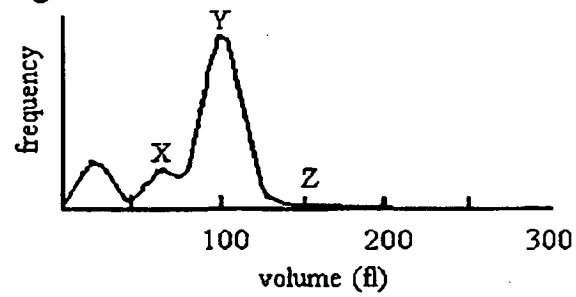


Fig. 9

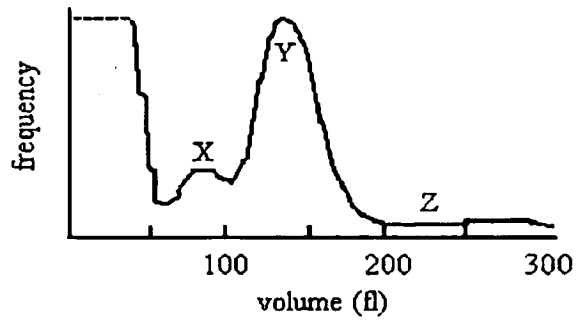


Fig. 10

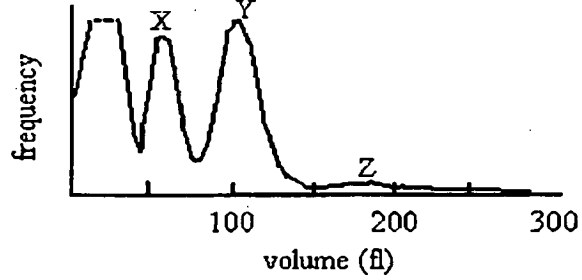


Fig. 11

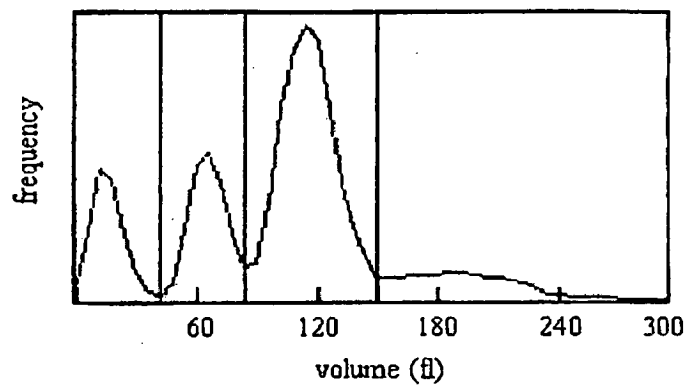


Fig. 12

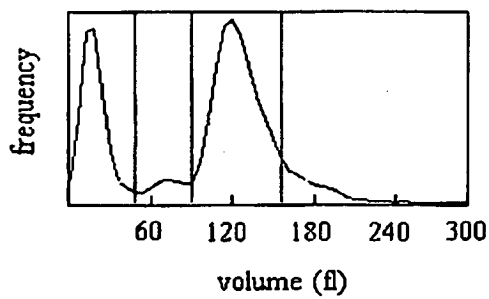


Fig. 13

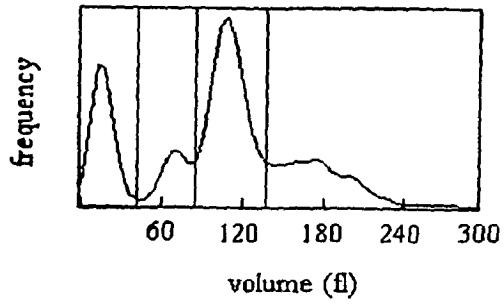


Fig. 14

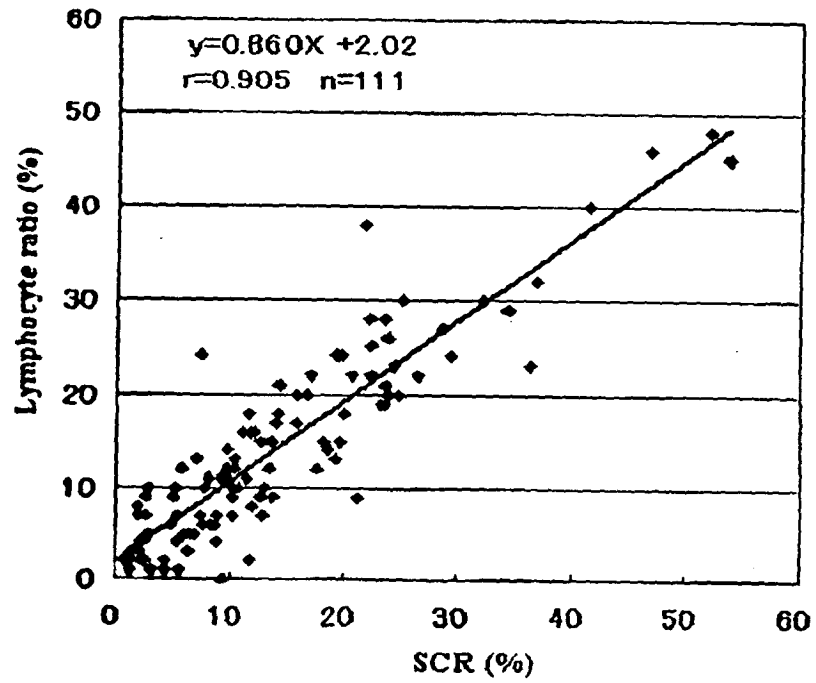


Fig. 15

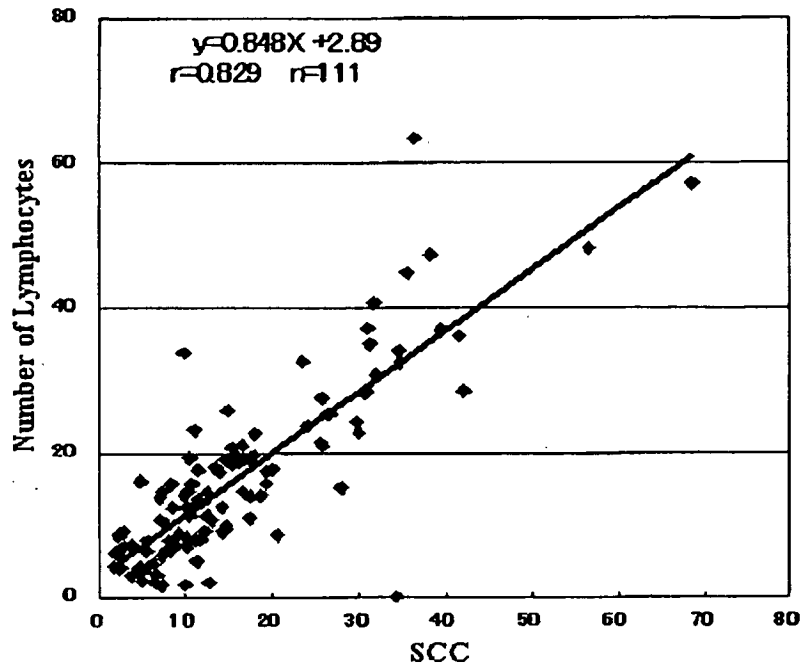


Fig. 16

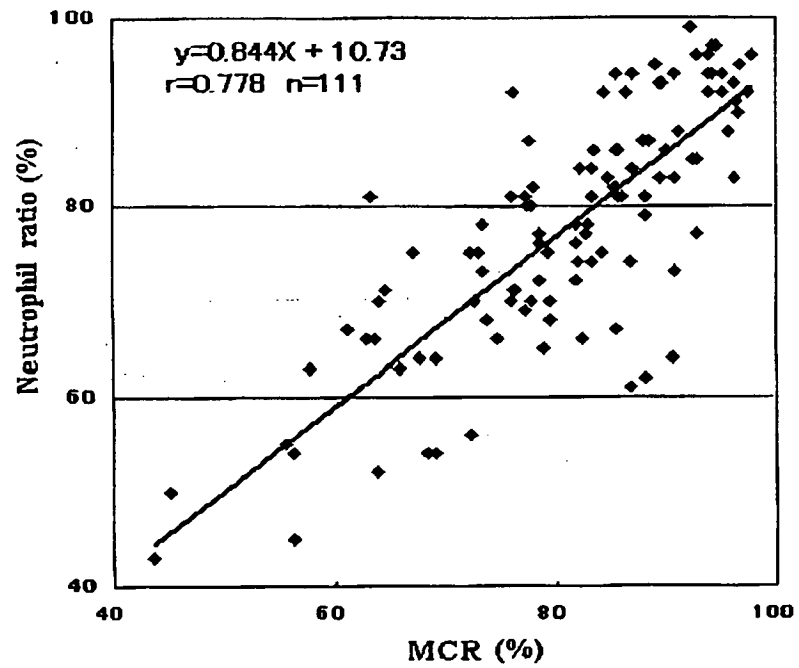


Fig. 17

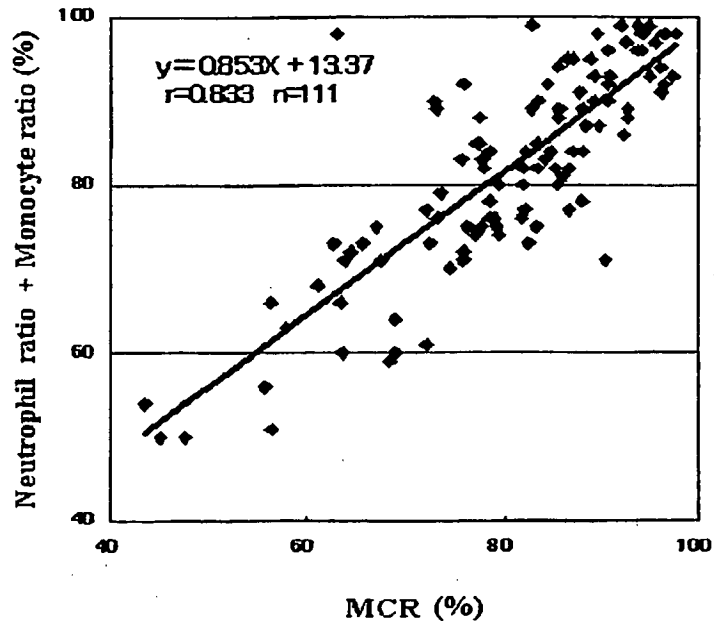


Fig. 18

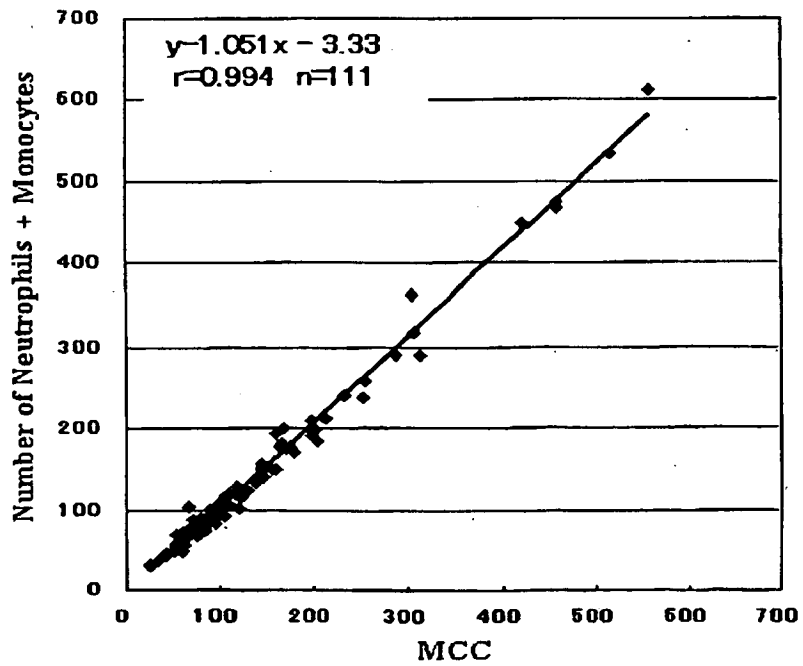


Fig. 19

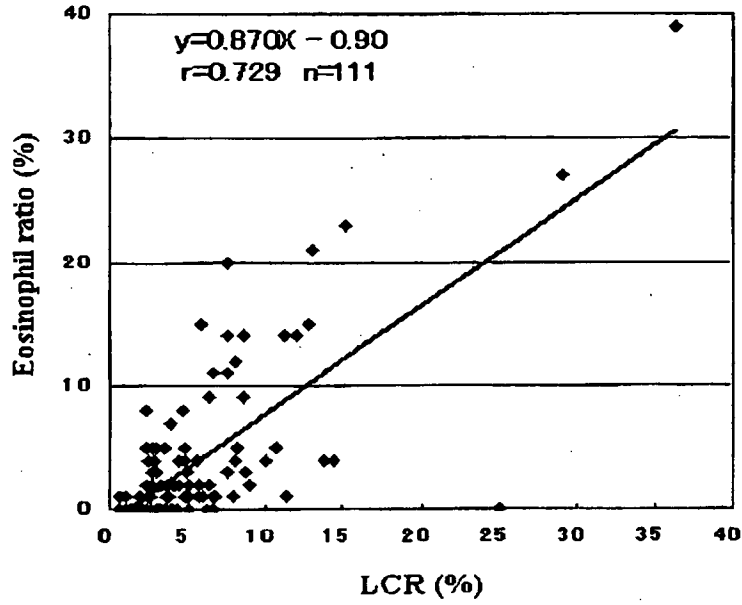


Fig. 20

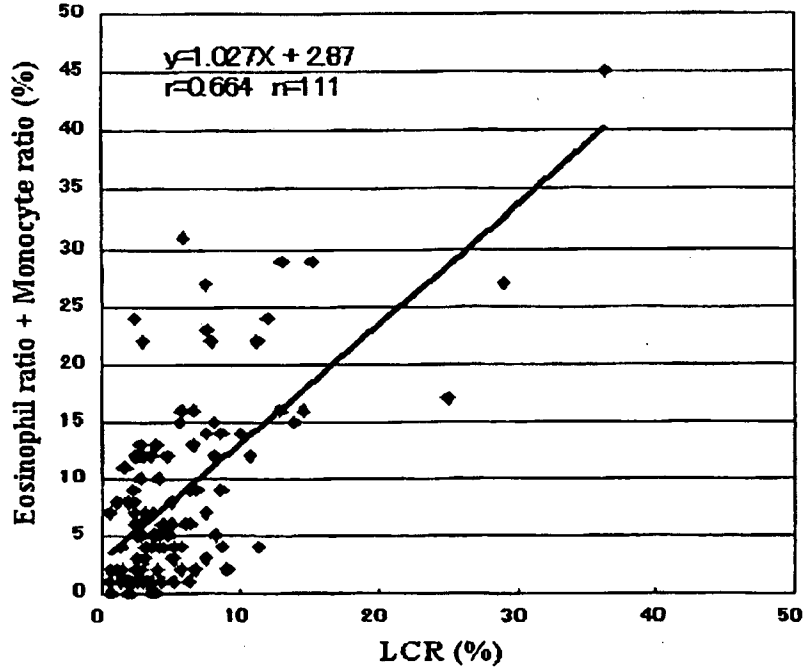


Fig. 21

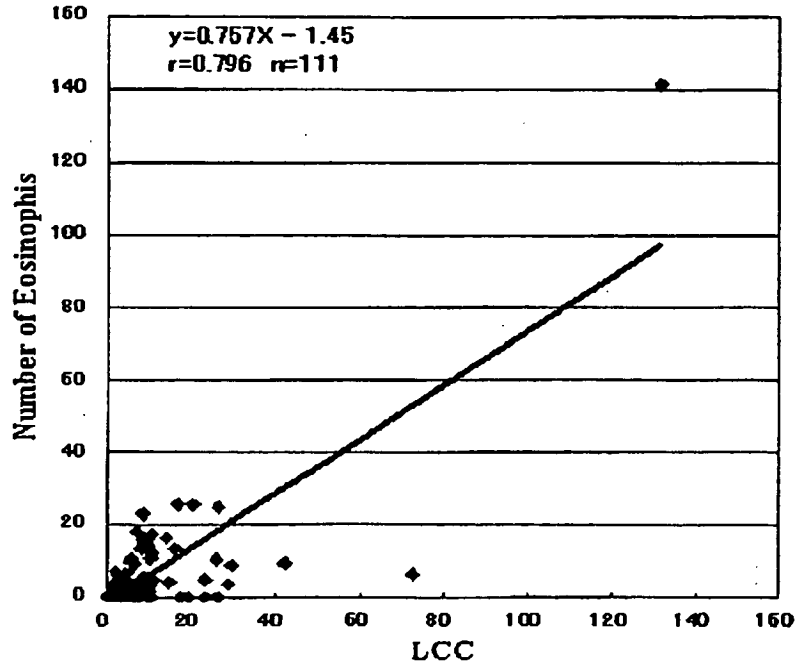


Fig. 22

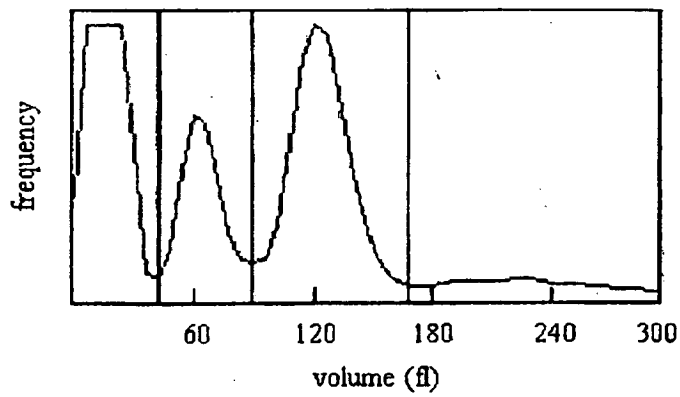


Fig. 23

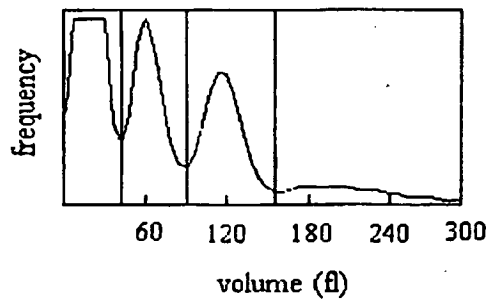


Fig. 24

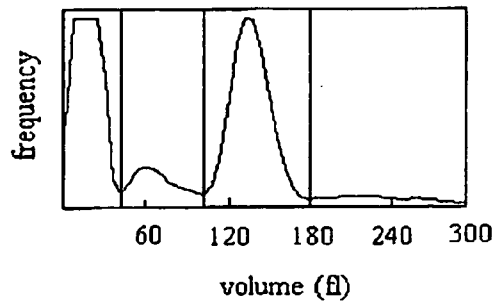


Fig. 25

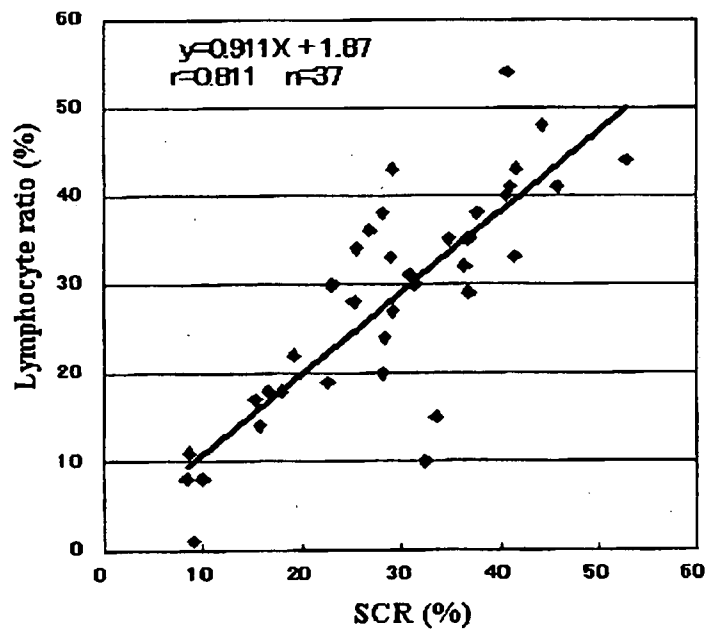


Fig. 26

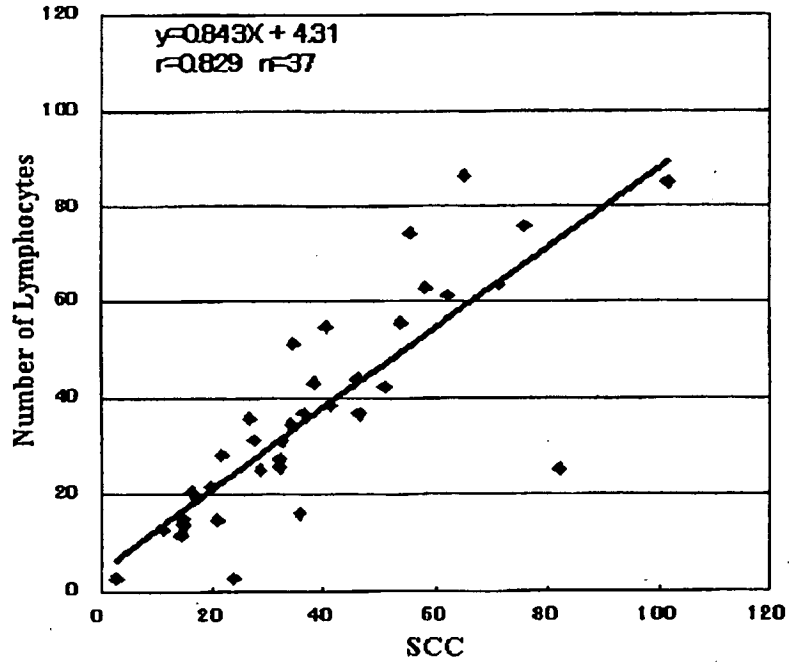


Fig. 27

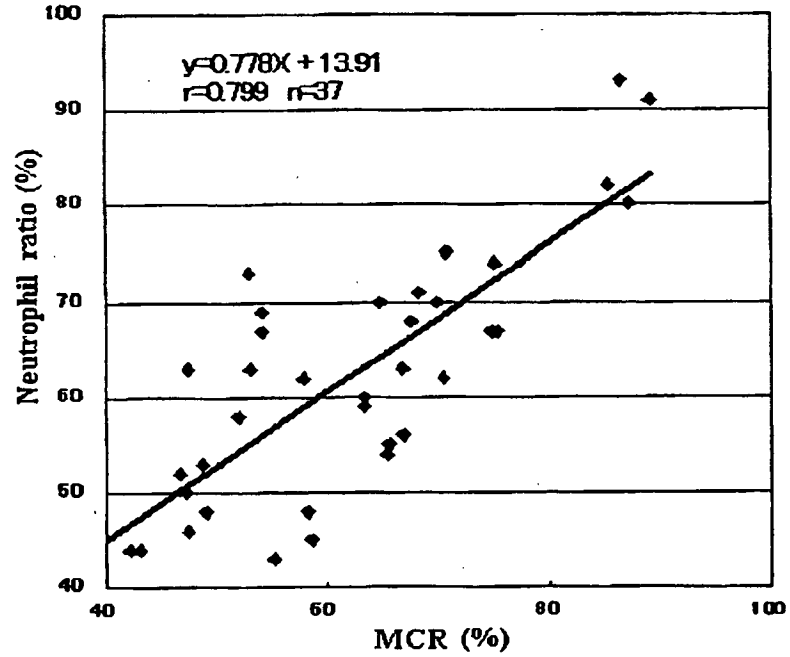


Fig. 28

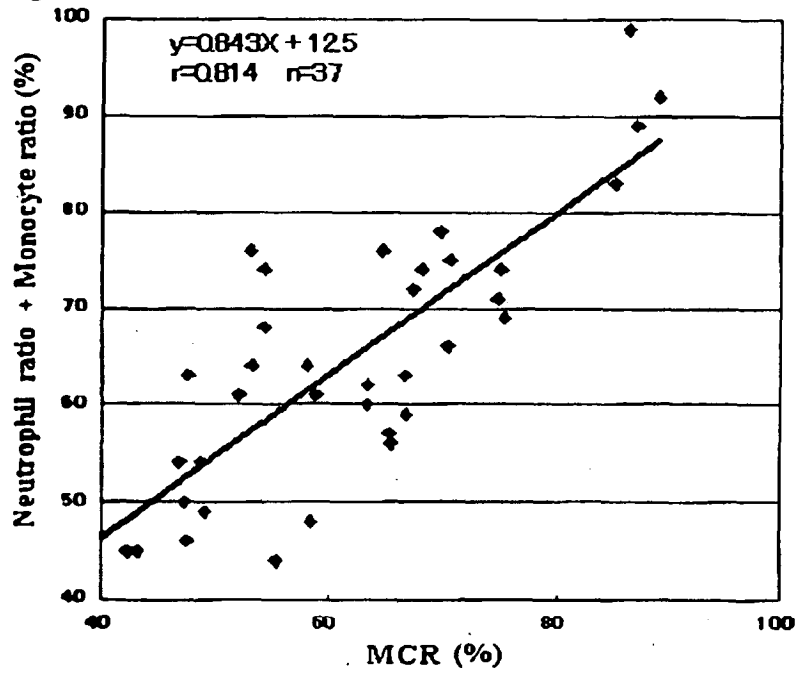


Fig. 29

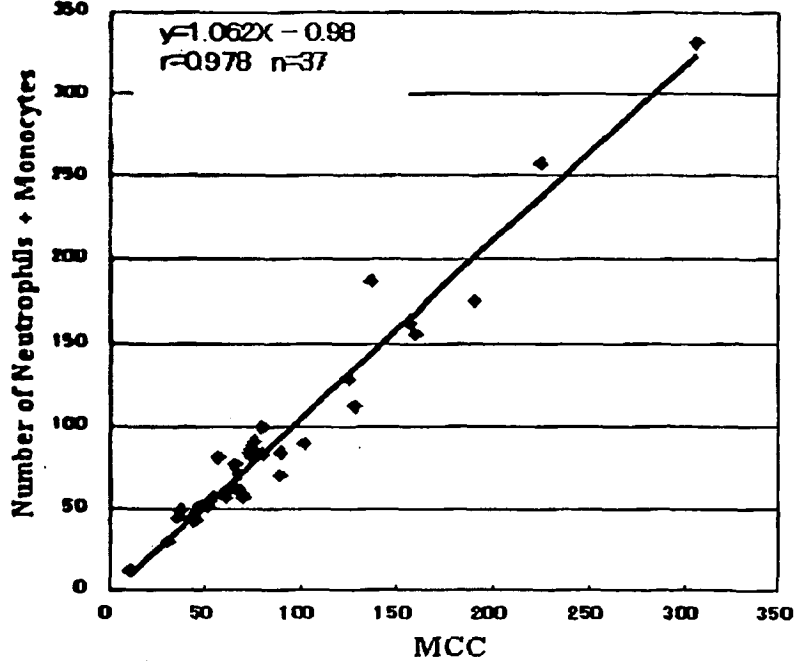


Fig. 30

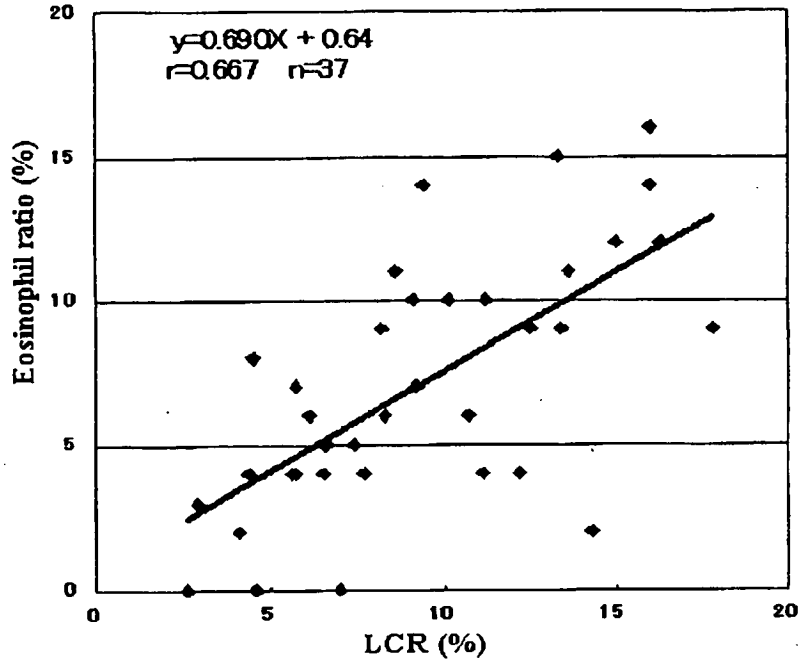


Fig. 31


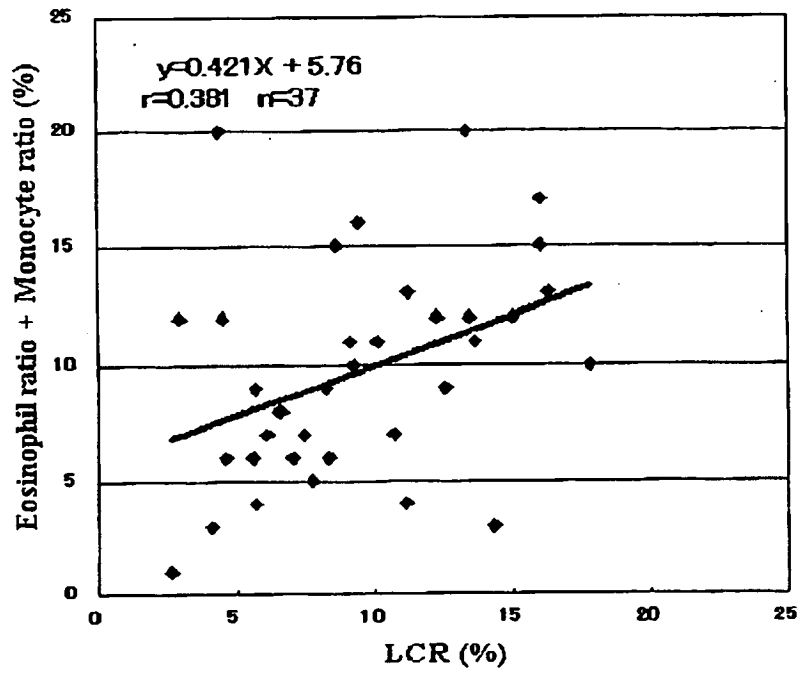


Fig. 32

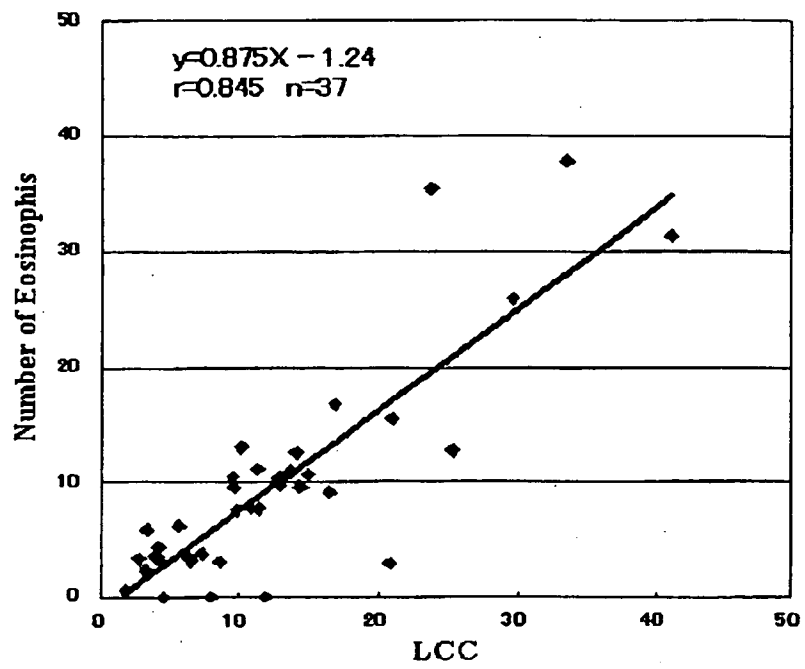

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 4346018 A [0003]
- US 4485175 A [0003]
- US 5116539 A [0003]
- JP H02031162 A [0003]
- JP H03020667 A [0003]
- US 5250437 A [0004]
- US 5968832 A [0004] [0015] [0020]
- US 6391263 B [0005]
- WO 2002014861 A [0006] [0007] [0008] [0009]

Non-patent literature cited in the description

- *J. Anim. Clin. Med*, 2001, vol. 10 (3), 129-134 [0006]

专利名称(译)	用于分类动物血液中白细胞的方法和试剂		
公开(公告)号	EP1684075B1	公开(公告)日	2010-08-11
申请号	EP2006447013	申请日	2006-01-23
[标]申请(专利权)人(译)	希森美康株式会社		
申请(专利权)人(译)	希森美康公司		
当前申请(专利权)人(译)	希森美康公司		
发明人	MATSUMOTO, HIDEAKI, SYSMEX CORPORATION SHIRAISHI, JUNICHI, SYSMEX CORPORATION HIRAYAMA, HIDEKI, SYSMEX CORPORATION		
IPC分类号	G01N33/569 G01N33/53 G01N33/543		
CPC分类号	G01N33/56972 Y10T436/10 Y10T436/101666 Y10T436/107497 Y10T436/25 Y10T436/25125		
优先权	2005016035 2005-01-24 JP		
其他公开文献	EP1684075A3 EP1684075A2		
外部链接	Espacenet		

摘要(译)

描述了一种用于对动物血液中的白细胞进行分类的方法。在该方法中，通过将犬或猫血液样品与裂解试剂混合来制备测量样品。在测量样品中裂解红细胞并使白细胞收缩。测量与测量样品中白细胞大小相关的数据。基于测量数据，白细胞被分类为含有淋巴细胞的第一组，含有嗜中性粒细胞和单核细胞的第二组和含有嗜酸性粒细胞的第三组。

