



(12) **EUROPEAN PATENT APPLICATION**
published in accordance with Art. 153(4) EPC

(43) Date of publication:
19.02.2020 Bulletin 2020/08

(21) Application number: **18784065.7**

(22) Date of filing: **13.04.2018**

(51) Int Cl.:
G01N 33/543 (2006.01) **G01N 33/553** (2006.01)
G01N 33/536 (2006.01) **G01N 33/569** (2006.01)
G01N 33/52 (2006.01)

(86) International application number:
PCT/KR2018/004313

(87) International publication number:
WO 2018/190664 (18.10.2018 Gazette 2018/42)

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
KH MA MD TN

(30) Priority: **13.04.2017 KR 20170047841**

(71) Applicant: **Cellemedy Co., Ltd**
Incheon 22011 (KR)

(72) Inventors:
• **LEE, Jeewon**
Seoul 06707 (KR)
• **KWON, Jeong-Hyeok**
Seongnam-si
Gyeonggi-do 13613 (KR)


(74) Representative: **Hutter, Anton et al**
Venner Shipley LLP
5 Stirling House
Stirling Road
The Surrey Research Park
Guildford GU2 7RF (GB)

(54) **ACCURATE, RAPID AND CONVENIENT SINGLE-STEP DISEASE DIAGNOSTIC METHOD USING SELF-AMPLIFICATION PRINCIPLE OF DETECTION SIGNAL**

(57) The present invention relates to a method of accurately, rapidly, and conveniently detecting a disease marker by linking immunodiagnostics and Au particle formation at the same time and, accordingly, realizing self-amplification of a detection signal and a kit thereof, more particularly, to a method of detecting a disease-specific marker using self-amplification of a detection signal and a kit thereof, the method including (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation. The method according to the present invention can diagnose a disease in a single step without any processes such as immobilization and washing processes that are generally accompanied in existing diagnosis methods such as ELISA; can short the time of a diagnostic test, which takes several hours or even several days, to about 10

minutes, thus being effectively used for diagnosis of diseases, in particular, of patients in an emergency; and can be confirmed by the naked eye without a separate analyzer, thus minimizing detection costs.

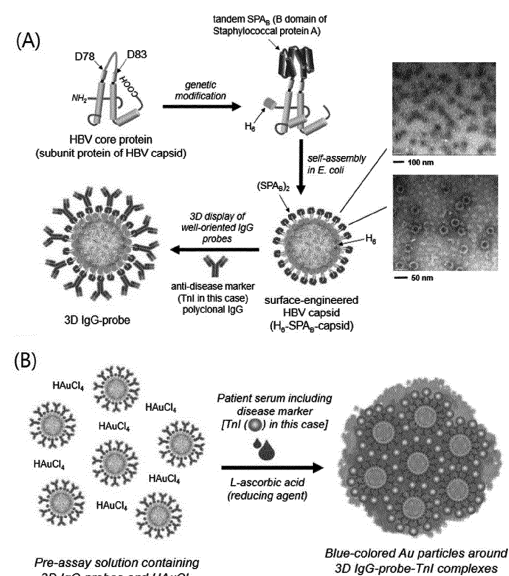Figure 1



Description

[Technical Field]

[0001] The present invention relates to a method of accurately, rapidly, and conveniently detecting a disease marker by linking immunodiagnostics and Au particle formation at the same time and, accordingly, realizing self-amplification of a detection signal and a kit therefor, more particularly, to a method of detecting a disease-specific marker using self-amplification of a detection signal and a kit therefor, the method including (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.

[Background Art]

[0002] In modern disease diagnosis, a diagnosis method having a rapid, accurate and simple procedure is most ideal. In addition, such rapid diagnosis is more important in patients with emergencies such as acute myocardial infarction. This rapid diagnosis is more important in patients with emergencies such as acute myocardial infarction. In the case of emergency patients, proper treatment according to rapid and accurate diagnosis is more important than the case of non-emergency patients because it is directly related to survival thereof.

[0003] In the field of clinical examination, the diagnosis of various diseases is performed using biological samples (blood, urine, etc.). As such a diagnosis method, various measurement methods have been developed and used. As representative methods of the measurement methods, there are biochemical assays using enzyme reactions and immunoassays using antigen-antibody reactions. Recently, it has been required to accurately measure components in biological samples. Accordingly, immunoassay methods using an antigen-antibody reaction with high specificity have been widely used.

[0004] Immunoassay methods utilize binding ability between an antigen and an antibody. Immunoassays are mainly used to analyze the presence of a specific antigen (or antibody)-a specific antibody (or antigen) in a sample. In particular, immunoassays are performed by flowing a sample on a specific antigen (or antibody) immobilized on a solid support (followed by washing), and then visualizing a bound antibody (or antigen) using various techniques.

[0005] In immunoassay methods, calibrators are generally used to determine (assign) the concentration of an unknown sample. In classical immunoassay, a set of calibrators is used, a calibration curve of a signal versus concentration is plotted, and the concentration of an unknown sample is determined by interpolation (Ibrahim A. Darwish, International Journal of Biomedical Science, Vol. 2 pp. 217-235, 2006).

[0006] Immunoassays can be classified into radioimmunoassay (RIA) in which signals are detected using radioisotopes, enzyme-linked immunosorbent assay (ELISA) or enzyme immunoassay (EIA) using signal amplification by an enzyme, a fluorescence antibody technique (FA) using fluorescence detection, chemiluminescence immunoassay (CLIA) using chemiluminescence, etc. according to the principle of detection and a method thereof. In addition, various classifications can be made according to use methods of labeling substances and substrate types.

[0007] ELISA can be greatly classified into direct ELISA, indirect ELISA, sandwich ELISA, and competitive ELISA.

[0008] Direct ELISA involves immobilizing an antigen on a 96-well plate, etc., and then injecting an enzyme-binding antibody thereto to cause an antigen-antibody reaction, followed by a washing process so as to measure the amount of a product converted from a substrate by the enzyme attached to the antibody. This method has the advantage of being faster than other ELISAs, but it is disadvantageous in that sensitivity is low, a specific antibody for each ELISA is required, it takes a long time, and costs are high.

[0009] Indirect ELISA involves immobilizing an antigen to a 96-well plate, and then treating with a primary antibody to induce an antigen-antibody reaction, followed by treating with an enzyme-bound secondary antibody so as to bind to an Fc domain of the primary antibody, followed by measuring the amount of a product converted from a substrate by the enzyme. This method has advantages such as high sensitivity, relative inexpensiveness, and the use of various types of primary antibodies, but it is disadvantageous in that the possibility of a false positive reaction due to cross-reaction between secondary antibodies is high, process steps are complicated, and it takes a long time.

[0010] Sandwich ELISA involves immobilizing a capture antibody capable of binding to an antigen to a 96-well plate, and then injecting a sample containing the antigen and injecting a detection antibody capable of binding another epitope of the antigen such that a sandwich structure of the capture antibody-antigen-detection antibody can be combined with an Fc domain of the detection antibody and, accordingly, an enzyme-bound secondary antibody can be detected. This method is advantageous in that a sample preparation step can be minimized and high sensitivity and accuracy are provided, but it is disadvantageous in that primary and secondary antibodies should be prepared to bind to different

epitopes of the antigen, it takes a long time, and costs are high.

[0011] Competitive ELISA involves injecting an antibody into a sample to induce an antigen-antibody reaction, and then injecting the antigen-antibody complex into an antigen-coated 96-well plate, followed by injecting an enzyme-bound secondary antibody to measure the amount of a product converted from a substrate. In the case of this method, the amount of a product converted by a secondary antibody is decreased with increasing amount of an antigen present in a sample. This method is advantageous in that a sample preparation step can be minimized, a wide range of antigen amounts can be measured, and even small epitopes, such as small molecules, can be detected, but it is disadvantageous in that it can be applied to diluted samples (Karichma Sha et al., British Journal of Hospital Medicine, Vol. 77, No. 7, 2016).

[0012] Electro-chemiluminescent (ECL) reaction is a chemiluminescence reaction occurring on a surface of an electrode induced by an electrochemical reaction. In particular, a conjugate of an antigen-antibody complex and ruthenium pyridine is excited by an electrochemical reaction in the presence of tripropylamine, and a redox reaction occurs to emit photons. The emitted photons may be collected by a photomultiplier tube. This process is repeatedly performed to generate photons, which amplifies optical signals. For electrochemiluminescence analysis, labels capable of binding to an antibody or antigen having a different chemical structure are generally used to produce a labeled antibody or antigen (Michael Vogesser et al., Ther. Drug Monit. Vol. 36, No. 5, pp. 640-650, 2014).

[0013] The ELISA method has advantages such as high sensitivity, a fast analysis speed, and easy automation, but it is disadvantageous in that several steps should be included and manufacturing costs of a labeled antibody or antigen are high. In the case of ruthenium pyridine, which is generally used, the properties thereof are greatly affected by an electrode material type, and there are disadvantages such as limited luminous efficiency and high costs.

[0014] To overcome the disadvantages, Korean Patent No. 10-1495665 has developed a fluorescence multiple immunoassay using a magnetic. However, this method also includes several steps, thereby taking a long time. Korean Patent No. 10-2014-0151305 has developed a method of increasing sensitivity by using protein particles such that an antigen is exposed while having correct orientation on a surface of the protein particles. However, this method also includes several steps and takes a long time. Accordingly, there is a need for an easy and rapid detection method.

[0015] Therefore, the present inventors have made diligent efforts to improve the disadvantages of existing immunoassay methods. As a result, the present inventors confirmed that, when Au particle formation using reduction of Au ions and an antigen-antibody immune response are simultaneously induced, a detection signal self-amplifies according to formation of aggregates of Au particles, which allows rapid detection of the presence or absence of a disease-specific marker, thus completing the present invention.

[0016] The above information described in this Background section is only provided to improve the understanding of the background of the present invention, and thus, information on prior art that is known to those of ordinary skill in the art may be excluded.

[Summary]

[0017] Therefore, the present invention has been made in view of the above problems, and it is one object of the present invention to provide a method of accurately, rapidly, and conveniently detecting a disease-specific marker in a single step using a self-amplification principle of a detection signal.

[0018] In accordance with an aspect of the present invention, the above and other objects can be accomplished by the provision of a method of detecting a disease-specific marker using self-amplification of a detection signal, the method including: (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.

[0019] In accordance with another aspect of the present invention, there is provided a method of detecting an antiviral antibody using self-amplification of a detection signal, the method including: (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antigen for detecting an antiviral antibody, free Au ions, and adsorbed Au ions are present, adding a sample, which contains an antiviral antibody binding specifically to the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of virus by a chromogenic reaction through the Au particle formation.

[0020] In accordance with another aspect of the present invention, there is provided a method of providing information for disease diagnosis using detection signal self-amplification, the method including: (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody

binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.

[0021] In accordance with yet another aspect of the present invention, there is provided a method of diagnosing a disease using detection signal self-amplification, the method including: (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.

[Description of Drawings]

[0022]

FIG. 1(A) illustrates a schematic diagram of protein particles for the diagnosis of acute myocardial infarction according to a method of the present invention and electron micrographs of the generated protein particles, and FIG. 1(B) is a schematic diagram illustrating a principle of the present invention, particularly a process in which Au particle formation and an antigen-antibody reaction simultaneously occur and thus a cluster is formed, so that rapid self-signal amplification occurs.

FIG. 2(A) illustrates one-step diagnosis results of serum of a patient with acute myocardial infarction and serum of a normal individual, and FIG. 2(B) illustrates experimental results showing that color changes in the sample of the patient with myocardial infarction are due to a difference in an absorbance of absorbing light at a specific wavelength, and an absorbance level difference between the patient and the normal individual at each time.

FIG. 3(A) illustrates experiment results of diagnose of serum of the same patient using an ELISA kit for detecting a marker, troponin I, for acute myocardial infarction, and FIG. 3(B) illustrates results (upper panel) obtained by additionally quantifying the amount of troponin I in the patient serum by ECLIA at the Green Cross diagnostic center and results (lower panel) of one-step diagnosis using the patient serum to investigate the possibility of quantification.

FIG. 4 illustrates TEM images of Au particle aggregates in an assay solution of a patient at each time zone.

FIG. 5(A) illustrates a simulation result of the principle that Au particle aggregates are formed, and FIG. 5(B) illustrates that absorbance increases in proportion to the size of an aggregate, particularly that the pattern wherein absorbance increases in proportion to the size of aggregate occurs at the same wavelength band.

FIG. 6 illustrates results of control experiments for investigating the principle of one-step diagnosis, particularly that complexes are generated when free Au ions are present and antigen-antibody complexes due to protein particles are formed, and thus, a chromogenic reaction occurs only in a patient (5).

FIG. 7 is a schematic diagram illustrating an interaction between Au ions and reducible peptides, an interaction between troponin I and protein particles in a patient sample, and how a signal self-amplification action due to the interactions occurs in this diagnosis.

FIG. 8 illustrates schematic diagrams of protein particles prepared to diagnose hepatitis C virus (HCV) according to the method of the present invention and electron micrographs of the protein particles.

FIG. 9 illustrates a schematic diagram illustrating a principle of detecting an HCV antibody present in a blood sample of a patient with hepatitis C according to the method of the present invention.

FIG. 10(A) illustrates test results of blood samples of a patient with hepatitis C and a normal individual according to the method of the present invention. FIG. 10(B) illustrates absorbances dependent upon antigen-antibody complex sizes in a patient with hepatitis C and absorbance changes dependent upon time. Particularly, it is illustrated that an absorbance increases at a specific wavelength of 588 nm over time, and clusters are formed in the shape shown in the TEM image. In addition, a box plot illustrates a difference in absorbances at each time of a normal individual group and a patient group.

FIG. 11(A) illustrates test results of blood samples of a patient with HIV and a normal individual according to the

method of the present invention, and FIG. 11(B) illustrates absorbances dependent upon antigen-antibody complex sizes and absorbance changes dependent upon time in a patient with HIV. Particularly, it is illustrated that absorbance increases at a specific wavelength of 588 nm over time, and clusters are formed in the shape shown in the TEM image. In addition, a box plot illustrates a difference in absorbances at each time of a normal individual group and a patient group.

In FIG. 12, a left panel illustrates test results of blood samples of a patient with HAV and a normal individual according to the method of the present invention, and a right panel illustrates antigen-antibody complex size-dependent absorbances and time-dependent absorbance changes in the patient with HAV. Particularly, it is illustrated that an absorbance increases at a specific wavelength of 574 nm over time.

FIG. 13 illustrates a test result of evaluating whether quantitative analysis of TnI in patient serum is reliable. (A) illustrates an absorbance measurement result of each standard serum 15 minutes after the start of diagnosis, (B) illustrates detection signal measurement results 20 minutes after the start of diagnosis, (C) illustrates detection signal measurement results 25 minutes after the start of diagnosis, and (D) illustrates detection signal measurement results 30 minutes after the start of diagnosis.

FIGS. 14 to 16 illustrate results of quantitative analysis performed using the ECLIA diagnostic device (model name: Roche E-170) of the Green Cross Medical Foundation. Particularly, FIG. 14 illustrates an analysis result of a normal individual sample (A), FIG. 15 illustrates an analysis result of a normal individual sample (B), and FIG. 16 illustrates an analysis result of a normal individual sample (C).

FIGS. 17 to 19 illustrate results of quantitative analysis performed using an ELISA diagnosis kit (E-EL-H0144) manufactured by Elascience. Particularly, FIG. 17 illustrates an analysis result of a normal individual sample (A), FIG. 18 illustrates an analysis result of a normal individual sample (B), and FIG. 19 illustrates an analysis result of a normal individual sample (C).

FIGS. 20 to 22 illustrate results of quantitative analysis performed using an ELISA diagnosis kit (abx050255) manufactured by Abbexa Ltd. Particularly, FIG. 20 illustrates an analysis result of a normal individual sample (A), FIG. 21 illustrates an analysis result of a normal individual sample (B), and FIG. 22 illustrates an analysis result of a normal individual sample (C).

FIGS. 23 to 25 illustrate results of quantitative analysis performed using an ELISA diagnosis kit (25-TR1HU-E01) manufactured by ALPCO. Particularly, FIG. 23 illustrates an analysis result of a normal individual sample (A), FIG. 24 illustrates an analysis result of a normal individual sample (B), and FIG. 25 illustrates an analysis result of a normal individual sample (C).

FIG. 26 illustrates quantification experiment results for evaluating the limit of detection (LOD) when diagnosing acute myocardial infarction using the method of the present invention.

FIG. 27 illustrates quantification experiment results for evaluating the limit of detection (LOD) when diagnosing hepatitis C using the method of the present invention.

FIG. 28 illustrates quantification experiment results for evaluating the limit of detection (LOD) when diagnosing AIDS using the method of the present invention.

[Detailed Description of Invention And Preferred Embodiments]

[0023] Unless otherwise defined, all terms including technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this inventive concept belongs. In general, nomenclature used in the present specification is well known and commonly used in the art.

[0024] The present invention has been made to confirm whether self-amplification of a detection signal according to an antigen-antibody immune response and Au particle formation due to reduction of Au ions occurs in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent, and thus, it is possible to detect a disease-specific marker.

[0025] According to the present invention, protein particles wherein a tag for gold ion adsorption and a tag for binding

an antibody Fc domain are exposed from a surface of a recombinant hepatitis B virus capsid (HBV-capsid)-derived core protein were prepared, and then an antibody capable of detecting a marker for acute myocardial infarction was attached to surfaces of the protein particles, and then an aqueous solution including the protein particles to which Au ions were absorbed was prepared. A marker for acute myocardial infarction and a reducing agent were added to the aqueous solution and, after 5 minutes, a chromogenic reaction was observed by the naked eye.

[0026] That is, according to an embodiment of the present invention, a hexa-histidine capable of adsorbing Au ions is expressed at an N-terminal of an HBV core protein, and a linker amino acid and a B domain of Staphylococcal Protein A capable of binding to an Fc domain of an antibody were bound to a loop portion, thereby preparing surface-modified recombinant HBV capsid protein particles (FIG. 1).

[0027] An antibody of troponin I (TnI) that is overexpressed in the case of acute myocardial infarction was bound to the protein particles to prepare protein particles in which an antibody was correctly oriented, and then a patient blood sample containing L-ascorbic acid (LAA) and TnI was injected thereto to induce an aggregation reaction (FIG. 1B). As a result, it was confirmed that, after 5 minutes, a chromogenic reaction observable by the naked eye occurred in the patient sample (FIG. 2).

[0028] Accordingly, in an aspect of the present invention, the present invention relates to a method of detecting a disease-specific marker using self-amplification of a detection signal, the method including (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.

[0029] The term "pre-assay solution" used in the present invention refers to a solution including an antibody (or an antigen) specifically binding to adsorbed Au ions, free Au ions, and an antigen (or an antibody) to be detected. The pre-assay solution may further include other buffers according to reaction conditions, particles from which amino acids adsorbing an antibody or an antigen and Au ions are exposed, and the like.

[0030] The term "assay solution" used in the present invention refers to a solution prepared by adding a sample and a reducing agent to the pre-assay solution. The sample may include an antigen or antibody to be detected.

[0031] The term "antibody" used in the present invention refers to an immunoglobulin selected from the group consisting of IgA, IgE, IgM, IgD, IgY and IgG. An antibody may specifically bind to a target antigen. An antibody is composed of two light chains and two heavy chains. Each of the chains is composed of a variable domain, an amino acid sequence of which is variable, and a constant domain, an amino acid sequence of which is constant. A site to which an antigen is bound is located at an end of a three-dimensional structure of a variable domain. The site is formed by a group of complementarity determining regions in which three light chains and three heavy chains are present. In a variable domain, the complementarity determining regions have highly variable amino acid sequences. Due to such high variability, an antibody specific to various antigens can be found. The scope of the present invention includes a complete antibody form and an antigen-binding fragment of the antibody molecule.

[0032] The term "single-chain Fv (ScFv, a single-chain fragment antibody or an antibody fragment)" used in the present invention refers to an antibody formed by connecting variable domains of a light chain and heavy chain to each other. As needed, a linker consisting of a peptide chain formed by connecting about 15 amino acids may be included. Here, ScFv may have a structure of a variable domain of a light chain-a linker-a variable domain of a heavy chain or a structure of a variable domain of a heavy chain-a linker-a variable domain of a light chain, and has antigen specificity the same as or similar to that of the original antibody.

[0033] A complete antibody includes two full-length light chains and two full-length heavy chains, and each of the light chains is connected to the heavy chain by a disulfide bond. A constant region of the heavy chain belongs to gamma (γ), mu (μ), alpha (α), delta (δ), and epsilon (ϵ) types and, as subclasses, includes gamma 1 (γ 1), gamma 2 (γ 2), gamma 3 (γ 3), gamma 4 (γ 4), alpha 1 (α 1) and alpha 2 (α 2). A constant region of the light chain belongs to kappa (κ) and lambda (λ) types.

[0034] An antigen-binding fragment of an antibody or an antibody fragment refers to a fragment having an antigen-binding function, and includes Fab, F(ab'), F(ab')₂, Fv, and the like. Fab among antibody fragments has variable domains of light and heavy chains, a constant region of a light chain, and a first constant region (CH1) of a heavy chain, and one antigen-binding site. Fab' is different from Fab in that Fab' has a hinge region wherein one or more cysteine residues are present at a C-terminal of a heavy chain CH1 domain. An antibody of F(ab')₂ is generated by a disulfide bond of cysteine residues at hinge regions of Fab'. Fv is a minimum antibody fragment only having a heavy-chain variable domain and a light-chain variable domain. Recombination techniques for producing Fv fragments are disclosed in PCT International Publication Nos. WO88/10649, WO88/106630, WO88/07085, WO88/07086, and WO88/09344. In the case of two-chain Fv, a heavy-chain variable domain and a light-chain variable domain are connected to each other by a non-covalent bond. In the case of single-chain Fv (scFv), a variable domain of a heavy chain and a variable domain of a light chain are connected to each other by a covalent bond through a peptide linker, or direct connection at a C-terminal is made,

thereby forming a dimer structure such as two-chain Fv. Such antibody fragments can be obtained using a protein hydrolase (for example, Fab can be obtained by restriction-digesting an entire antibody with papain, and a F(ab')₂ fragment can be obtained by digesting with pepsin) or using a gene recombination technique.

[0035] Examples of the antibody of the present invention include a monoclonal antibody, a multispecific antibody, a human antibody, a humanized antibody, a chimeric antibody, a single-chain Fvs (scFV), a single-chain antibody, a Fab fragment, a F(ab') fragment, disulfide-binding Fvs (sdFV), an anti-idiotypic (anti-Id) antibody, an epitope-binding fragment of the antibody, and the like, but the present invention is not limited thereto.

[0036] In the present invention, the adsorbed Au ions may be any one adsorbed to a material capable of adsorbing Au ions, preferably a material capable of being adsorbed to amino acids, more preferably a material capable of being adsorbed to an amino acid selected from the group consisting of histidine, lysine and arginine, but the present invention is not limited thereto.

[0037] In the present invention, the reducing agent may be any material capable of reducing Au ions into Au particles under reaction conditions of the present invention, preferably may be selected from the group consisting of ascorbic acid, imidazole, pyrazole, histamine, hydroxyl amine, citric acid, and sodium borohydride.

[0038] In the present invention, the sample may be selected from the group consisting of blood, plasma, serum, urine, saliva, oral mucosa, and saliva, but the present invention is not limited thereto.

[0039] In the present invention, the concentration of the Au ions (free Au ions + adsorbed Au ions) present in the pre-assay solution may be 1 mM to 10 mM, but the present invention is not limited thereto.

[0040] In the present invention, the concentration of the reducing agent present in the assay solution may be 0.005 M to 0.1 M, but the present invention is not limited thereto.

[0041] In the present invention, the amount of the sample may be 10 μ l to 30 μ l, but the present invention is not limited thereto.

[0042] In the present invention, when the concentration of the Au ions, the concentration of the reducing agent, and the amount of the sample are smaller than reference values, effective disease marker detection may not be performed. When the concentration of the Au ions, the concentration of the reducing agent, and the amount of the sample are greater than reference values, negative effects such as a false positive effect may be exhibited.

[0043] In the present invention, in the case of an antigen or antibody for detecting the disease-specific marker, the antigen or the antibody may be exposed from surfaces of protein particles. From the surfaces of the protein particles, a tag selected from the group consisting of histidine, lysine, and arginine capable of adsorbing Au ions may be further exposed.

[0044] In the present invention, an immune response of the antigen or antibody for detecting the disease-specific marker may occur on surfaces of protein particles. The tag may adsorb Au ions to induce aggregation of Au particles in the presence of a reducing agent.

[0045] In the present invention, the protein particles may be any particles formed by a self-assembly function of a protein, preferably may be selected from the group consisting of ferritin, ferritin-like proteins, magnetosome-constituting proteins, virus-constituting proteins (e.g. hepatitis B virus core protein, tobacco mosaic virus) DNA binding proteins (DPS), and proteasomes, but the present invention is not limited thereto. In the present invention, the virus-constituting proteins may be selected from the group consisting of capsid proteins of human hepatitis B virus.

[0046] In the present invention, the sizes of the protein particles may be 10 nm to 50 nm, but the present invention is not limited thereto.

[0047] In the present invention, in the case of the antibody for detecting a disease-specific marker exposed from surfaces of the protein particles, a domain capable of binding to an Fc domain of the antibody is exposed from surfaces of the protein particles, whereby the domain may bind to the antibody for detecting the disease-specific marker.

[0048] In the present invention, a domain capable of binding to the Fc domain of the antibody may be selected from the group consisting of B domain of Staphylococcal protein A and protein G, but the present invention is not limited thereto.

[0049] In the present invention, a domain capable of binding to the Fc domain of the antibody is exposed from surfaces of the protein particles. Such exposure may be further effectively made due to a linker protein.

[0050] In the present invention, the linker protein is not specifically limited so long as it is an amino acid capable of effectively exposing a domain, capable of binding to the Fc domain of the antibody, from surfaces of protein particles, and, preferably, may be G4SG4T or G4SG4.

[0051] In the present invention, the chromogenic reaction may more rapidly occur in a group, to which a sample of a patient is added, than a group to which a normal sample is added. In the patient group, the chromogenic reaction occurs within a minimum of 5 minutes to a maximum of 10 minutes. However, a reaction time may be changed according to reaction conditions.

[0052] In the present invention, the chromogenic reaction may be detected using any method of detecting changes in visible light and, preferably, may be detected by the naked eye or using a spectrophotometer, and an absorbance may be detected at 500 to 600 nm, but the present invention is not limited thereto.

[0053] In the present invention, by self-amplification of a detection signal, a small amount of disease marker is detected

and a resultant result is expressed by a color change that can be observed by the naked eye. Such self-amplification of a signal is caused by a phenomenon that Au ions dissolved in a solution for diagnosis are reduced into Au particles by a reducing agent. As the sizes of Au particles increase, a resultant color change is expressed as a signal that can be confirmed by the naked eye.

[0054] In the case of protein particles used in the present invention, hexa-histidine is fused to and expressed in monomers thereof. Here, since histidine amino acids have a property of binding with Au ions, Au ions bound to aggregates generated due to an antigen-antibody reaction react with a reducing agent, thereby being reduced into Au particles. The sizes of the Au particles increase as other Au ions are reduced, thereby forming larger Au particles. Such resultant aggregates are colored.

[0055] In the case of a normal individual serum, an antigen-antibody reaction does not occur. Accordingly, a generation speed of aggregates due to Au particles is low, whereby a time taken until a color is expressed is significantly slow. Through such color change, a patient may be distinguished from a normal individual.

[0056] In the present invention, whether a virus can be detected using self-amplification of a detection signal was also investigated.

[0057] That is, in another embodiment of the present invention, a method according to the present invention was used to detect a hepatitis C virus (HCV)-specific antibody from a patient with hepatitis C. First, 1) an expression vector with a H6-SPAB-HBVC capsid structure, 2) an expression vector with a H6-c33c(HCV epitope)-HBVC capsid structure and 3) an expression vector with a hFTN(human ferritin)-511p-c100p-c22p(HCV epitope)-H6 structure were respectively expressed in *Escherichia coli* to prepare three types of protein particles (FIG. 8). It was expected that protein particles prepared from the vector (1) include hexa-histidine and SPAB exposed from surfaces thereof, thereby binding with Au ions and an Fc domain of an antibody, and the vectors (2) and (3) include hepatitis C-specific epitopes exposed from surfaces thereof and thus bind with HCV-specific antibodies in a patient sample (FIG. 9).

[0058] It was confirmed that, when Au ions were adsorbed into an aqueous solution mixed with protein particles, and then a blood sample of a patient and a blood sample of a normal individual were respectively injected thereinto, clusters of protein particles and Au particles were formed and, thus, a blue chromogenic reaction occurred only in the patient blood sample (FIGS. 10 and 11).

[0059] Accordingly, in another aspect of the present invention, the present invention relates to a method of detecting an antiviral antibody using self-amplification of a detection signal, the method including (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antigen for detecting an antiviral antibody, free Au ions, and adsorbed Au ions are present, adding a sample, which contains an antiviral antibody binding specifically to the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a virus by a chromogenic reaction through the Au particle formation.

[0060] In the present invention, the term "antigen for virus detection" may be any virus protein specifically binding to an antibody capable of detecting a virus and may include, as well as a virus protein, any types of amino acids, such as virus peptides or epitopes, translated from virus genes.

[0061] In the present invention, the term "epitope" refers to a specific site binding to an antibody on an antigen molecule; or a conjugate of a T cell receptor (TCR) and a major tissue complex (MHC) and may be referred to as an antigenic determinant.

[0062] For example, hepatitis C virus (HCV) belongs to the Flaviviridae family causing non-A and non-B hepatitis. The HCV genome, which includes single-stranded RNA, expresses a polyprotein composed of about 3,010 amino acids (Choo et al., *Science*, 244:359-362, 1989). Polyprotein expressed by HCV is cut by host cell proteases and virus proteases into 10 functionally different proteins.

[0063] The HCV gene is composed of NH₂-C-E1-E2-p7-NS2-NS3-NS4A-NS4B-NS5A-NS5B-COOH (Steven Rosenberg, *J. Mol. Biol.*, 313:451-464, 2001). This protein is greatly classified into structural proteins including C (core), E1, E2 and p7; and non-structural proteins including NS2, NS3, NS4A, NS4B, NS5A, and NS5B.

[0064] C (core) protein of HCV is believed to be responsible for encapsidation of HCV genomic RNA and to play an important role in the development of hepatoma by regulating gene transcription, growth and proliferation of host cells. E1 and E2 are type-1 transmembrane proteins and virus envelope proteins, known to play important roles in cell infection. E1 protein had not attracted great attention in the past because it does not induce neutralizing antibodies. Recently, however, E1 protein was developed as a therapeutic vaccine by Innogenetics, Co. in Belgium, which is in the process of phase II clinical trial following successful phase I clinical trial with chimpanzees. It is encouraging that E1 protein can be effectively used for the treatment of 1b type HCV infection that has not been successfully treated by alpha-interferon.

[0065] E2 protein, which is a major envelope protein of a virus, has been known as a multi-functional protein which, in addition to structural roles, conjugates with the assumed cell receptor CD81, and it nullifies both the immune system of a host cell and interferon-mediated antiviral reaction, which leads to oncogenesis or autoimmune liver disease. Accordingly, E2 is recognized as a major antigen for the development of an HCV vaccine and a major target for the development of an anti-HCV drug. The function of P7 protein has not been known. NS2 protein is a part of a metallo-

protease, and NS3 harbors serine protease of HCV at its N-terminus and RNA helicase domain of its C-terminus.

[0066] NS4A is a cofactor of viral protease, and NS4B has been found to have a potential for tumorigenesis. NS5A was reported to function to endow HCV resistance against interferon and antiapoptosis. NS5B is known to act as a viral RNA-dependent RNA polymerase. It will be apparent to those skilled in the art that epitopes of such HCV constituent proteins may be used as a virus specific epitope of the present invention.

[0067] In the present invention, an antigen for detecting an antiviral (HCV) antibody present in the pre-assay solution may be selected from the group consisting of c22p, c33c, 5-1-1p, c100p, and a fused epitope of two or more thereof. The fused epitope may be selected from the group consisting of c22p-c33c, c22p-5-1-1p, c22p-c100p, c33c-5-1-1p, c33c-c100p, 5-1-1p-c100p and c22p-5-1-1p-c100p, but the present invention is not limited thereto.

[0068] The term "virus" used in the present invention refers to an obligatory intracellular parasite that has DNA or RNA as a nucleic acid, starts proliferation from the nucleic acid, does not proliferate through binary fission, and does not have an enzyme system required for ATP production.

[0069] The virus of the present invention includes a naked virus and an enveloped virus. Particularly, a virus according to an embodiment of the present invention may be an enveloped virus.

[0070] In the present invention, the enveloped virus may include, particularly, DNA viruses such as herpesvirus, poxvirus and hepadnavirus, and RNA viruses such as flavivirus, togavirus, coronavirus, hepatitis D, orthomyxovirus, paramyxovirus, rhabdovirus, bunyavirus, filovirus, human immunodeficiency virus (HIV), and retrovirus.

[0071] The orthomyxovirus includes influenza virus A, influenza virus B, influenza virus C, isavirus, thogotovirus and quaranjavirus genera.

[0072] The coronavirus includes alpha coronavirus, beta coronavirus, gamma coronavirus and delta coronavirus genera.

[0073] The paramyxovirus encompasses paramyxovirus, rubella virus, morbillivirus and pneumovirus genera.

[0074] The human immunodeficiency virus (HIV) genome consists of two positive single-stranded RNAs that encode nine viral gene factors. RNA is surrounded by a conical capsid consisting of about 2,000 virus proteins p24. The virus contains single-stranded RNA, nuclear capsid protein p7, and enzymes necessary for the formation of virion proteins (reverse transcriptase, proteinase, ribonuclease, integrase).

[0075] A substrate composed of a virus protein p17 surrounds the capsid again to preserve virions. The substrate is again surrounded by a viral membrane composed of phospholipid bilayers. The viral membrane is first formed when a new virus emerges from a host cell. The viral membrane being created is buried in a cell membrane of a host cell and consists of about 70 complex HIV proteins that protrude from a host cell's protein and a virus particle surface.

[0076] The complex HIV protein, known as Env, consists of a hat consisting of three glycoprotein120 molecules; and a stem, which anchors a protein structure to a viral membrane, consisting of three gp41 molecules. Glycoprotein conjugates are important at the start of an infection cycle, enabling a virus to attach and fuse to target cells. Two surface glycoproteins of a virus, particularly gp120, are known as subjects for future therapeutic agent and vaccine development.

[0077] Two TAT proteins (p16 and p14) are transcriptional transactivators for the LTR promoter acting by binding to the TAR RNA element. The TAR may also be processed into microRNAs that regulate the apoptosis genes ERCC1 and IER3. The Rev protein (p19) is involved in shuttling RNAs from the nucleus and the cytoplasm by binding to the RRE RNA element. The Vif protein (p23) prevents the action of APOBEC3G (a cellular protein that remove amines from DNA and RNA hybrids or interferes with Pol proteins). The Vpr protein (p14) arrests a host at G2/M and prevents cellular division thereof. The Nef protein (p27) down-regulates the MHC class I and class II molecules as well as CD4 (a major viral receptor) of T cells.

[0078] Nef also interacts with SH3 domains. The Vpu protein (p16) influences the release of new virus particles from infected cells. GAG gene expresses matrix proteins (MA, GAG p17), capsid proteins (CA, GAG p24), nucleic acid capsids (NC, GAG p7), etc., which are cores of viral particles. Pol gene contains an enzyme gene related to viral proliferation and is composed of an RT portion involved in reverse transcriptase expression of viral RNA, a PR responsible for protease, an integrase-related IN, etc.

[0079] In addition, TAT gene is known to express a regulator that activates the proliferation of a virus during an infection process, and, on the other hand, Nef gene is known to play a role in inhibiting the proliferation of a virus along with the LTR portion. The Long Term Repeat (LTR), in which the same nucleotide sequences are repeated, is attached to both ends of the entire HIV RNA. LTR sites act as switches that regulate the production of a new virus or can be triggered by proteins of HIV or host cells. The retroviral Psi element is involved in viral genome packaging and is recognized by gag and rev proteins. The SLIP element (TTTTTT) is known to be involved in the frameshift in the gag-pol reading frame required to make functional Pol. It will be apparent to those skilled in the art that an epitope of HIV can be used for the virus detection of the present invention.

[0080] In the present invention, the antigen for detecting an antiviral (HIV) antibody present in the pre-assay solution may be selected from the group consisting of gp41, p24 and gp100, but the present invention is not limited thereto.

[0081] DNA of the human papilloma virus (HPV) contains 8000 base pairs and is surrounded by a pentagonal capsid protein of the pentagon, not a lipid membrane. The capsid protein consists of two structural proteins, L1 and L2, which

are expressed later in a viral replication cycle. In the genome of all human papillomavirus (HPV), there are eight ORFs, and each ORF is divided into three functional sites. The functional sites consist of E1-E7 gene necessary for virus replication, L1-L2 gene expressing structural proteins constituting virions, and LCR gene regulating the replication and transcription of a virus.

[0082] E6 binds to p53 and promotes ubiquitination of p53, thereby inhibiting the function of p53 as a cancer tumor suppressor gene. It also induces the degradation of BAK, a pro-apoptotic protein. The activation of telomerase activates the cell cycle of host cells, and E7 interacts with retinoblastoma (RB) to degrade RB. Through this, E2F, a transcription promoter that has been inhibited by RB, is released. In addition, the cell cycle of the host cell is activated by the activation of cyclin E and cyclin A acting on the cell cycle S phase, and, when infected with the human papillomavirus through the activation of these genes, cervical cancer may be developed. However, the roles of other genes such as E1, E2, and E4 in HPV in cancer development processes, is still unknown.

[0083] L1 self-assembles to form pentameric capsomers. These capsomers form capsids through disulfide bonds with adjacent L1 molecules to package human papilloma virus DNA, and L2 is present in lesser amounts than L1, facilitating the packaging of the viral genome. In addition, human papillomaviruses are known to play an important role when penetrating new host cells.

[0084] Accordingly, in the present invention, the antigen for detecting an antiviral (HIV) antibody present in the pre-assay solution may be L1 or L2, but the present invention is not limited thereto.

[0085] Middle East Respiratory Syndrome Coronavirus (MERS-CoV), a type of coronavirus, was detected in samples collected from the lungs of a 60-year-old male with acute pneumonia and acute renal failure in Jidda, Saudi Arabia. MERS-CoV is a plus-sense, single stranded novel RNA beta coronavirus that is known to cause Middle East Respiratory Syndrome.

[0086] Accordingly, in the present invention, an antigen for detecting an antiviral (MERS-CoV) antibody present in the pre-assay solution may be a MERS-CoV surface protein, but the present invention is not limited thereto.

[0087] Hepatitis A virus (HAV) is classified into the genus Picornaviridae and the genus Hepatovirus, has no encapsulation, is a regular icosahedron, and has a particle size of 27 to 32 nm. The virion consists of three major structural polypeptides (VP1, VP2 and VP3).

[0088] Accordingly, in the present invention, an antigen for detecting an antiviral (HAV) antibody present in the pre-assay solution may be VP1, VP2, VP3 or an epitope prepared by extracting or connecting portions thereof, but the present invention is not limited thereto.

[0089] In the present invention, the adsorbed Au ions may be any one adsorbed to a material capable of adsorbing Au ions, preferably a material capable of being adsorbed to amino acids, more preferably a material capable of being adsorbed to an amino acid selected from the group consisting of histidine, lysine and arginine, but the present invention is not limited thereto.

[0090] In the present invention, the reducing agent may be any material capable of reducing Au ions into Au particles under reaction conditions of the present invention, preferably may be selected from the group consisting of ascorbic acid, imidazole, pyrazole, histamine, hydroxyl amine, citric acid, and sodium borohydride.

[0091] In the present invention, the sample may be selected from the group consisting of blood, plasma, serum, urine, saliva, oral mucosa, and saliva, but the present invention is not limited thereto.

[0092] In the present invention, the concentration of the Au ions (free Au ions + adsorbed Au ions) present in the pre-assay solution may be 1 mM to 10 mM, but the present invention is not limited thereto.

[0093] In the present invention, the concentration of the reducing agent present in the assay solution may be 0.005 M to 0.1 M, but the present invention is not limited thereto.

[0094] In the present invention, the amount of the sample may be 10 μ l to 30 μ l, but the present invention is not limited thereto.

[0095] In the present invention, when the concentration of the Au ions, the concentration of the reducing agent, and the amount of the sample are smaller than reference values, effect disease marker detection may not be performed. When the concentration of the Au ions, the concentration of the reducing agent, and the amount of the sample are greater than reference values, negative effects such as false positive effect may be exhibited.

[0096] In the present invention, the antigen for virus detection may be exposed from surfaces of protein particles. From the surfaces of the protein particles, a tag selected from the group consisting of histidine, lysine, and arginine capable of adsorbing Au ions may be further exposed.

[0097] In the present invention, an immune response of the antigen for virus detection may occur on surfaces of protein particles. The tag may adsorb Au ions to induce aggregation of Au particles in the presence of a reducing agent.

[0098] In the present invention, the protein particles may be any particles formed by a self-assembly function of a protein, preferably may be selected from the group consisting of ferritin, ferritin-like proteins, magnetosome-constituting proteins, virus-constituting proteins (e.g. hepatitis B virus core protein, tobacco mosaic virus) DNA binding proteins (DPS), and proteosome, but the present invention is not limited thereto. In the present invention, the virus-constituting proteins may be selected from the group consisting of capsid proteins of human hepatitis B virus.

[0099] In the present invention, the sizes of the protein particles may be 10 nm to 50 nm, but the present invention is not limited thereto.

[0100] In the present invention, by self-amplification of a detection signal, a small amount of antiviral antibody is detected and a resultant result is expressed by a color change that can be observed by the naked eye. Such self-amplification of a signal is caused by a phenomenon that Au ions dissolved in a solution for diagnosis are reduced into Au particles by a reducing agent. As the sizes of Au particles increase, a resultant color change is expressed as a signal that can be confirmed by the naked eye.

[0101] In the case of protein particles used in the present invention, hexa-histidine is fused to and expressed in monomers thereof. Here, since histidine amino acids have a property of binding with Au ions, Au ions bound to aggregates generated due to an antigen-antibody reaction react with a reducing agent, thereby being reduced into Au particles. The sizes of the Au particles increase as other Au ions are reduced, thereby forming larger Au particles. Such resultant aggregates are colored.

[0102] In the case of a normal individual serum, an antigen-antibody reaction does not occur. Accordingly, a generation speed of aggregates due to Au particles is low, whereby a time taken until a color is expressed is significantly slow. Through such a color change, a virus-bearing patient may be distinguished from a normal individual.

[0103] In the present invention, an antiviral antibody contained in a sample is exposed from surfaces of protein particles, thereby binding to a domain capable of binding to an Fc domain of the antibody.

[0104] In the present invention, a domain capable of binding to the Fc domain of the antibody may be selected from the group consisting of B domain of Staphylococcal protein A and protein G, but the present invention is not limited thereto.

[0105] In the present invention, a domain capable of binding to the Fc domain of the antibody may be bound to a linker protein exposed from surfaces of the protein particles.

[0106] In the present invention, the linker protein is not specifically limited so long as it is an amino acid capable of effectively exposing a domain, capable of binding to the Fc domain of the antibody, from surfaces of protein particles, and, preferably, may have an amino acid sequence such as G4SG4T or G4SG4.

[0107] In the present invention, the chromogenic reaction may more rapidly occur in a group, to which a sample of a patient is added, than a group to which a normal sample is added. In the patient group, the chromogenic reaction occurs within a minimum of 5 minutes to a maximum of 10 minutes. However, a reaction time may be changed according to reaction conditions.

[0108] In the present invention, the chromogenic reaction may be detected using any method of detecting changes in visible light and, preferably, may be detected by the naked eye or using a spectrophotometer, and an absorbance may be detected at 500 to 600 nm, but the present invention is not limited thereto.

[0109] Another aspect of the present invention relates to a method of providing information for disease diagnosis using self-amplification of a detection signal, the method including (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.

[0110] The present invention also relates to a disease diagnosis method using self-amplification of a detection signal, the method including (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.

[0111] In an embodiment of the present invention, an antibody binding specifically to Troponin I (TnI) was exposed to the protein particles of the present invention in a blood sample of a patient with acute myocardial infarction and a blood sample of a normal individual, and it was confirmed that a chromogenic reaction rapidly occurred in the patient blood sample (FIG. 2). That is, it is obvious to those of ordinary skill in the art that, when a disease-specific marker is detected according to the present invention, the disease may be diagnosed.

[0112] Accordingly, in the present invention, the disease may be acute myocardial infarction, but the present invention is not limited thereto.

[0113] In the present invention, when the disease is acute myocardial infarction, the disease-specific antibody may be an antibody specifically binding to troponin I, but the present invention is not limited thereto.

[0114] In the present invention, the disease may be hepatitis C, acquired immune deficiency syndrome (AIDS), or hepatitis A, but the present invention is not limited thereto.

[0115] In the present invention, when the disease is hepatitis C, the disease-specific antibody may be an antibody specifically binding to HCV and, when an antigen is exposed from surfaces of protein particles, may be selected from

the group consisting of c22p, c33c, 5-1-1p, and c100p of HCV and a fused epitope of two or more thereof. The fused epitope may be selected from the group consisting of c22p-c33c, c22p-5-1-1p, c22p-c100p, c33c-5-5-1p, c33c-c100p, 5-1-1p-c100p and c22p-5-1-1p-c100p, but the present invention is not limited thereto.

[0116] In the present invention, when the disease is AIDS, the disease-specific antibody may be an antibody binding specifically to HIV and, when an antigen is exposed from surfaces of protein particles, may be selected from the group consisting of gp41, p24 and gp100 of HIV, but the present invention is not limited thereto.

[0117] In the present invention, when the disease is hepatitis A, the disease-specific antibody may be an antibody specifically binding to HAV and, when an antigen is exposed from surfaces of protein particles, may be one or more epitopes selected from the group consisting of VP1, VP2, VP3 or an epitope prepared by extracting or connecting portions thereof, but the present invention is not limited thereto.

[0118] In the present invention, the disease may be cancer. The cancer may be selected from the group consisting of lung cancer, bronchial cancer, colorectal cancer, prostate cancer, breast cancer, pancreatic cancer, stomach cancer, ovarian cancer, bladder cancer, brain cancer, thyroid cancer, esophageal cancer, uterine cancer, liver cancer, kidney cancer, biliary cancer, glial cancer blastoma, and testicular cancer.

[0119] In the present invention, when the disease is cancer, the disease-specific antibody may be an antibody specifically binding to a tumor marker, but the present invention is not limited thereto.

[0120] In the present invention, the tumor marker may be as shown in Table 1 below for each cancer type, but the present invention is not limited thereto.

[Table 1]

Tumor marker for each carcinoma	
Carcinoma	Tumor markers
Brain, hard tumor	SCC
Lung cancer	SLX, NSE, SCO, ADH, ACTH
Liver cancer	AFP, PIVKA-II, ALP
Gastroduodenal cancer	CA19-9, CEA, AFP
Prostate cancer	PSA, PA
Testicular cancer	AFP, HCO, NSE
Thyroid cancer	CEA, Calcitonin, Thyroglobulin
Breast cancer	CA 15-3, CEA, CA549, TPA
Pancreatic cancer	CA19-9, Elastase I, CA50, Du-Pan-2, SPAN-1, KMO1, POA, PST
Colon cancer	CEA, NCC-ST-439
Uterine cancer	SCC, CEA, hCG
Ovarian cancer	CA125, CA72-4
Blood cancer	β -2-Microglobulin

[0121] In the present invention, when the disease is lymphoma or leukemia, the disease-specific antibody may be an antibody that specifically binds to CD20, CD30, CD33 or CD52, but the present invention is not limited thereto.

[0122] In the present invention, when the disease is breast cancer, colon cancer, lung cancer, or ovarian cancer, the disease-specific antibody may be an antibody specifically binding to EGFR, ERBB2, ERBB3, MET, IGF1R, EPHA3, TRAILR1, TRAILR2, FAP, Tenascin, EpCAM, CEA, gpA33, Mucin, TAG-72, CAIX, PSMA or a Folate-binding protein, but the present invention is not limited thereto.

[0123] In the present invention, the disease may be an infectious disease. The infectious disease may be selected from the group consisting of flu (influenza), smallpox, polio, foot and mouth disease, Ebola, measles, yellow fever, dengue fever, SARS, pneumonia, tuberculosis, cholera, typhoid, dysentery, diphtheria and Lyme disease, but the present invention is not limited thereto.

[0124] In the present invention, when the disease is influenza, the disease-specific antibody may be an antibody binding specifically to influenza virus, but the present invention is not limited thereto.

[0125] Influenza virus is a single stranded RNA virus belonging to Orthomyxoviridae, has two glycoprotein surface antigens, i.e., hemagglutinin and neuraminidase, and is classified into influenza A, B and C according to antigenicity.

Type A and B mainly cause epidemic outbreaks, type A is classified as a subtype according to the characteristics of HA (H1-H15) and NA (N1-N9), type B has no subtype. Accordingly, when the flu is diagnosed by the method of the present invention, the antibody used in the present invention may be an antibody specific to each influenza virus subtype, but the present invention is not limited thereto.

[0126] In the present invention, when the disease is polio, the disease-specific antibody may be an antibody specifically binding to a poliovirus, but the present invention is not limited thereto.

[0127] In the present invention, when the disease is Ebola, the disease-specific antibody may be an antibody specifically binding to an Ebola virus, but the present invention is not limited thereto. When the disease is measles, the disease-specific antibody may be an antibody specifically binding to a measles virus that is a type of paramyxovirus, but the present invention is not limited thereto. When the disease is yellow fever, the disease-specific antibody an antibody specifically binding to a yellow fever virus that belongs to the family Flavivirus, but the present invention is not limited thereto. When the disease is dengue fever, the disease-specific antibody may be an antibody specifically binding to a dengue virus, but the present invention is not limited thereto.

[0128] In the present invention, the disease may be an autoimmune disease. The autoimmune disease may be selected from the group consisting of rheumatoid arthritis, type 1 diabetes, Crohn's disease, ulcerative colitis, Behcet's disease, lupus, scleroderma, psoriasis and vitiligo, but the present invention is not limited thereto.

[0129] In the present invention, when the disease is Sjogren's syndrome, the disease-specific antibody may be an anti-Ro (Sjogren's syndrome A, SSA) antibody or an anti-La (Sjogren's syndrome B, SSB) antibody, but the present invention is not limited thereto.

[0130] In the present invention, when the disease is multiple sclerosis, the disease-specific antibody may be an anti-MOG antibody, an anti-myelin antibody or an anti-KIR4.1 antibody, but the present invention is not limited thereto.

[0131] In the present invention, when the disease is stroke, the disease-specific antibody may be an anti-NR2A/2B and metalloproteinase (MMP) antibody, an antinuclear antibody (ANA), an antiphospholipid antibody (APL), an anti-D-dimer antibody, an anti-S100 β antibody, an anti-B-type natriuretic peptide (BNP) antibody, or an anticardiolipin antibody (ACL), but the present invention is not limited thereto.

[0132] In the present invention, when the disease is cerebral hemorrhage, the disease-specific antibody may be anti-glial fibrillary acidic protein (GFAP) antibody, anti-asymmetric dimethylarginine (ADMA) antibody, or anti-D-dimer antibody, but the present invention is not limited thereto.

[0133] The present invention also relates to a disease diagnosis kit using self-amplification of a detection signal.

[0134] In the present invention, the kit may include a pre-assay solution containing an antigen or antibody for detecting a disease-specific marker, free Au ions, and adsorbed Au ions; and a reducing agent. Here, it is preferred to store the pre-assay solution and the reducing agent in different containers.

[0135] In the present invention, the kit may include an external package. The external package may include instructions for use of components thereof.

[0136] Hereinafter, the present invention will be described in more detail with reference to the following Examples. It will be apparent to those skilled in the art that the Examples are merely for concretely explaining the invention and therefore, there is no intent to limit the invention to the Examples.

Example 1. Preparation of expression vectors for synthesis of hFTN and HBV capsid protein particles

[0137] Expression vectors for manufacturing protein particles, H6-SPAB-capsid, H6-c33c-capsid, H6-gp41-capsid, H6-p24-capsid, hFTN-511p-c100p-c22p-H6, hFTN-ep1-H6, hFTN-ep2-H6, and hFTN-ep3-H6, were prepared according to schematic vector diagrams summarized in Table 1.

[0138] All of the prepared plasmid expression vectors were subjected to agarose gel-purification, and then total DNA sequences of each thereof were confirmed.

[0139] In particular, a PCR product required to prepare each of the expression vectors was produced using a primer set shown in Table 2, and then the resultant PCR product was sequentially inserted into a pT7-vector, thereby constituting an expression vector for expressing each protein particle type.

[0140] Vectors for expressing each of the protein particle type are as follows: pT7-H6-SPAB-capsid, pT7-H6-c33c-capsid, pT7-H6-gp41-capsid, pT7-H6-p24-capsid, pT7-hFTN-511p-c100p-c22p-H6, pT7-hFTN-ep1-H6 pT7-hFTN-ep2-H6 and pT7-hFTN-ep3-H6.

[Table 2]

Expression vector constructions for manufacturing protein particles	
Protein particles	Expression vectors
H ₆ -SPA _B -capsid	NH ₂ -NdeI-H ₆ -HBVC-(SPA _B) ₂ -HBVC-C/ai-COOH

(continued)

Expression vector constructions for manufacturing protein particles	
Protein particles	Expression vectors
H ₆ -c33c-capsid	NH ₂ - <i>Nde</i> I-H ₆ -HBVC-c33c-HBVC- <i>Cl</i> aI-COOH
H ₆ -gp41-capsid	NH ₂ - <i>Nde</i> I-H ₆ -HBVC-gp41-HBVC- <i>Cl</i> aI-COOH
H ₆ -p24-capsid	NH ₂ - <i>Nde</i> I-H ₆ -HBVC-p24-HBVC- <i>Cl</i> aI-COOH
hFTN-511p-c100p-c22p-H ₆	NH ₂ - <i>Nde</i> I-hFTN- <i>Xho</i> I-linker(G3SG3TG3SG3)-511p-c100p-c22p-H ₆ - <i>Hind</i> III-COOH
hFTN-ep1-H ₆	NH ₂ - <i>Nde</i> I-hFTN- <i>Xho</i> I-linker(G3SG3TG3SG3)-ep1-H ₆ - <i>Hind</i> III-COOH
hFTN-ep2-H ₆	NH ₂ - <i>Nde</i> I-hFTN- <i>Xho</i> I-linker(G3SG3TG3SG3)-ep2-H ₆ - <i>Hind</i> III-COOH
hFTN-ep3-H ₆	NH ₂ - <i>Nde</i> I-hFTN- <i>Xho</i> I-linker(G3SG3TG3SG3)-ep3-H ₆ - <i>Hind</i> III-COOH

[Table 3]

Primer sets for PCR to manufacture expression vectors	
Protein particles	Primers
H ₆ -SPA _B -capsid	5'primer: CTC GAG GCA CCG AAA GCT GAT AAC 3'primer: GGA TCC GTC AGC TTT TAG TGC TTG
H ₆ -c33c-capsid	5'primer: CTC GAG GCG GTG GAC TTT ATC CCT 3'primer: GGA TCC ACA CGT ATT GCA GTC TAT
H ₆ -gp41-capsid	5'primer: CTC GAG ATC CTG GCT GTG GAA CGC 3'primer: GGA TCC GAT CAA CTT TCC ACT AGC
H ₆ -p24-capsid	5'primer: CTC GAG CCG GAA GTA ATC CCG ATG 3'primer: GGA TCC TCC CAC TCC CTG ACA TGC

Example 2. Biosynthesis and separation purification of hFTN and HBV capsid protein particles

2-1. Biosynthesis of protein particles

[0141] E. coli strain BL21(DE3)[F-ompThsdSB (rB-mB-)] was transformed with each of the expression vectors manufactured according to Example 1, and ampicillin-resistant transformants were selected. The transformed E. coli were cultured in a flask (250 mL Erlenmeyer flask, 37°C, 150 rpm) containing 50 mL of a Luria-Bertani (LB) medium (containing 100 mg of L⁻¹ ampicillin).

[0142] When the turbidity (O.D 600) of the medium reached about 0.4 to 0.6, IPTG (Isopropyl-β-D-thiogalactopyranosid) (1.0 mM) was injected therein to induce expression of the recombinant gene. After culturing at 20°C for 12 to 16 hours, the cultured Escherichia coli was centrifuged at 4,500 rpm for 10 minutes to obtain a cell precipitate. The obtained cell precipitate was suspended in 5 ml of a lysis solution (10 mM Tris-HCl buffer, pH 7.5, 10 mM EDTA), and lysed using an ultrasonic crusher (Branson Ultrasonics Corp., Danbury, CT, USA), followed by centrifuging at 13,000 rpm for 10 minutes, followed by separating a supernatant from an insoluble aggregate. The separated supernatant was purified.

2-2. Purification of protein particles

[0143] To purify the fused protein particles, recombined by self-assembly, expressed in Example 2-1, the following three-step purification process was performed. First, 1) Ni^{2+} -NTA affinity chromatography using a combination between histidine fused to the recombined protein and nickel was performed, and then 2) the recombined protein was concentrated and a buffer of the concentrated protein was exchanged such that self-assembly of monomers occurred, and 3) sucrose gradient ultracentrifugation was performed to isolate only the self-assembled protein particles. A detailed description of each step follows.

1) Ni^{2+} -NTA affinity chromatography

[0144] To purify each of the recombined proteins, *Escherichia coli* cultured according to the aforementioned method was collected, and a cell pellet was resuspended in 5 mL of a lysis solution (pH 8.0, 50 mM sodium phosphate, 300 mM NaCl, 20 mM imidazole), followed by crushing the cells using an ultrasonic crusher. The crushed cell solution was centrifuged at 13,000 rpm for 10 minutes to isolate only a supernatant. Next, the recombined protein was separated using a Ni^{2+} -NTA column (Qiagen, Hilden, Germany) (washing buffer: pH 8.0, 50 mM sodium phosphate, 300 mM NaCl, 50 mM imidazole/elution buffer: pH 8.0, 50 mM sodium phosphate, 300 mM NaCl, 100 mM imidazole).

2) Concentration and buffer exchange

[0145] 3 ml of the recombined protein eluted through Ni^{2+} -NTA affinity chromatography was contained in an ultracentrifugal filter (Amicon Ultra 10K, Millipore, Billerica, MA), followed by centrifuging at 5,000 rpm until 1 ml of a solution remained on the column. The buffer of the protein particles was exchanged with a Tris-HCl (50 mM Tris-HCl, 500 mM NaCl, pH 7.0) buffer (in the case of hFTN particles, PBS buffer (2.7 mM KCl, 137 mM NaCl, 2 mM KH_2PO_4 , 10 mM Na_2HPO_4 , pH 7.4)) so that self-assembly of monomers occurred.

3) Sucrose-gradient high-speed centrifugation

[0146] To a Tris-HCl (50 mM Tris-HCl, 500 mM NaCl, pH 7.0) buffer (in the case of hFTN particles, a PBS buffer (2.7 mM KCl, 137 mM NaCl, 2 mM KH_2PO_4 , 10 mM Na_2HPO_4 , pH 7.4)), sucrose was added to each concentration, thereby preparing a solution including sucrose at a concentration of each of 60%, 50%, 40%, 30%, and 20%. Next, 2 ml of a sucrose solution at each concentration (60 to 20%) was added to a high-speed centrifuge tube (ultraclear 13.2 ml tube, Beckman) in a high-concentration order. After containing a solution, 1 ml of a recombined protein solution was finally added, followed by performing high-speed centrifugation at 24,000 rpm and 4°C for 16 hours (Ultracentrifuge L-90k, Beckman). After centrifugation, 40 to 50% of the sucrose solution was carefully removed, and the buffer of the recombined protein was replaced with a new buffer using an ultracentrifugal filter and a Tris-HCl buffer as described in step 2).

Example 3: Assembly verification of protein particles

[0147] To analyze the structure of the recombined protein particles prepared according to Example 2, the recombined protein particles were photographed using a transmission electron microscope (TEM). First, an unstained, purified protein sample was placed on a carbon-coated copper electron microscope grid, and then naturally dried. To obtain stained protein particle images, the electron microscope grid including the naturally dried sample was incubated together with a 2% (w/v) aqueous uranyl acetate solution at room temperature for 10 minutes, followed by washing with distilled water three to four times.

[0148] To obtain an image of aggregates in which Au particles were gathered, a sample of a color-changed assay solution used for diagnosis was placed on a grid and then naturally dried without a separate staining process.

[0149] Protein particles and Au particle aggregate were observed using an electron microscope, Philips Technai 120 kV. As results, it was confirmed that the respective protein particles were spherical and the respective Au particle aggregates were radial (FIGS. 1, 4, 8 and 11).

Example 4: One-step diagnosis using signal self-amplification

4-1. Disease-specific marker detection through antigen detection

[0150] In the case of acute myocardial infarction (AMI), 200 μL of a goat anti-TnI polyclonal IgG (cat. no. 70-XG82, Fitzgerald, Acton, MA, U.S.A) antibody at a concentration of 1 mg/ml was added to 800 μL of $\text{H}_6\text{-SPA}_\text{B}$ -capsid protein particles manufactured according to Example 2 and adjusted to a concentration of 1.25 mg/ml, followed by mixing at

4°C for 12 to 16 hours to be bound to each other.

[0151] To the protein particles to which the antibody has been fixed, 500 μL of 0.5% (w/v) Au^{3+} ion solution (HAuCl_4 (cat. no. 254169, Sigma Aldrich, St. Louis, MO, U.S.A.) was added, followed by mixing at 4°C for 12 to 16 hours to be bound to each other.

[0152] 60 μL of the solution (pre-assay solution) including the protein particles to which the antibody and the Au ions had been fixed was fed into each well of a 96-well plate (cat. no. 3599, Costar, NY, U.S.A.), and then 20 μL of a serum sample of a patient with AMI or a normal individual was added thereto. Soon after addition of the serum sample, 20 μL of 0.05 M L-ascorbic acid (cat. no. A7506, Sigma Aldrich, St. Louis, MO, U.S.A.), as a reducing agent, was added thereto to induce signal self-amplification. As a result, it was confirmed that a chromogenic reaction occurred in the well to which the patient serum sample had been added within 5 minutes (FIG. 2A).

[0153] In addition, it was confirmed that such a color change occurred due to a high absorbance at a wavelength band of 576 nm. In addition, an absorbance difference between the patient serum and the normal individual serum at the wavelength band was confirmed using a microplate reader (Infinite M200 Pro, TECAN, Zurich, Switzerland) (FIG. 2B).

4-2. Disease-specific marker detection through antibody detection

1) Human hepatitis C virus (HCV) diagnosis

[0154] In the case of HCV, 250 μL of H_6 -c33c-capsid protein particles at a concentration of 2.0 mg/ml and 250 μL of H_6 -hFTN-511p-c100p-c22p protein particles at a concentration of 1.0 mg/ml were added to 500 μL of H_6 -SPA_B-capsid protein particles at a concentration of 1.0 mg/ml manufactured according to Example 2, thereby preparing a protein particle mixture solution. Next, 500 μL of 0.5% Au^{3+} ion solution was added thereto, followed by mixing at 4°C for 12 to 16 hours to be bound to each other.

[0155] 60 μL of the prepared solution (pre-assay solution) was added to each well of a 96 well plate, and 20 μL of a serum sample of a patient with hepatitis C or a normal individual was added thereto. Soon after addition of the serum sample, 20 μL of 0.05 M L-ascorbic acid was added thereto to induce signal self-amplification. As a result, it was confirmed that a chromogenic reaction occurred in the well to which the patient serum sample had been added within 5 minutes (FIG. 10A).

[0156] In addition, it was confirmed that such a color change occurred due to a high absorbance at a wavelength band of 588 nm. In addition, an absorbance difference between the patient serum and the normal individual serum at the wavelength band was confirmed using a microplate reader (FIG. 10B).

2) Human immunodeficiency virus (HIV) diagnosis

[0157] In the case of HIV, an experimental procedure was the same as that in HCV, but the composition of a protein particle mixture solution was different. That is, 250 μL of H_6 -gp41-capsid protein particles at a concentration of 3.0 mg/ml and 250 μL of H_6 -p24-capsid protein particles at a concentration of 1.0 mg/ml were added to 500 μL of H_6 -SPA_B-capsid protein particles at a concentration of 1.0 mg/ml, thereby preparing a protein particle mixture solution. Next, 500 μL of 0.5% Au^{3+} ion solution was added thereto, followed by mixing at 4°C for 12 to 16 hours to be bound to each other.

[0158] 60 μL of the prepared solution (pre-assay solution) was added to each well of a 96 well plate, and 20 μL of a serum sample of a patient with HIV or a normal individual was added thereto. Soon after addition of the serum sample, 20 μL of 0.05 M L-ascorbic acid was added thereto to induce signal self-amplification. As a result, it was confirmed that a chromogenic reaction occurred in the well to which the patient serum sample had been added within 5 minutes (FIG. 11).

3) Human hepatitis A virus (HAV) diagnosis

[0159] In the case of HAV, 200 μL of hFTN-ep1- H_6 protein nanoparticles at a concentration of 2.0 mg/ml, 200 μL of hFTN-ep2- H_6 protein nanoparticles at a concentration of 2.0 mg/ml, and 200 μL of hFTN-ep3- H_6 protein nanoparticles at a concentration of 1.0 mg/ml were added to 600 μL of H_6 -SPAB-capsid protein particles at a concentration of 1.0 mg/ml manufactured according to Example 2, thereby preparing a protein particle mixture solution. Next, 600 μL of 0.5% Au^{3+} ion solution was added thereto, followed by mixing 4°C for 12 to 16 hours to be bound to each other.

[0160] 60 μL of the prepared solution (pre-assay solution) was added to each well of a 96 well plate, and 20 μL of a serum sample of a patient with hepatitis A or a normal individual was added thereto. Soon after addition of the serum sample, 20 μL of 0.05 M L-ascorbic acid was added thereto to induce signal self-amplification. As a result, it was confirmed that a chromogenic reaction occurred in the well to which the patient serum sample had been added within 5 minutes (FIG. 12).

Example 5: ELISA and ECLIA experiments using controls

[0161] A serum sample of a patient with AMI was subjected to ELISA and ECLIA, compared to controls. In ELISA, a kit (Abbexa, U.K., abx252868) having a detection limit of 12.5 pg/ml was used. In ECLIA, a kit having a detection limit of 0.16 ng/ml was used (Modular Analytics E170, Roche, Germany).

[0162] The same serum samples from 20 patients were used. From resultant experimental results, it was confirmed that one-step diagnosis using self-signal amplification was more sensitive, more rapid, and more accurate (FIG. 3)

Example 6: Au nanoaggregate model simulation experiment

[0163] In the one-step diagnosis experiment performed in Example 4, it was confirmed that a color rapidly turned blue in a patient. To investigate the cause of such a change, an finite difference time domain (FDTD) simulation experiment (Lumerical Solutions, ver. 8.15.736) was performed.

[0164] As a result of the simulation, a raspberry-shaped protein-metal complex as illustrated in FIG. 5A is formed. When the sizes of the aggregates were changed under the assumption that aggregates are formed in the form, a change in an absorption cross-sectional area was shown according to a wavelength in FIG. 5B. An absorption cross-sectional area was obtained by dividing the absorption power stored in a surrounding area including particles by the intensity of a light source.

[0165] In addition, in the case of the raspberry-shaped simulation model shown in FIG. 5A, it was confirmed that, as the sizes of aggregates increased, an absorbance increased in the same wavelength band rather than being separated into different wavelengths (FIG. 5B). This was confirmed as coinciding with an actual one-step diagnosis result.

Example 7: Control experiment for analyzing principle of one-step diagnosis experiment.

[0166] A control experiment was preformed to analyze the principle of one-step diagnosis. To perform a control experiment, Ni^{2+} , which is known to well bind histidine that is an amino acid binding to Au ions, was attached to histidine of protein particles. From the experimental results, it was confirmed whether binding between Au ions and histidine of protein particles affected this experiment, and the one-step diagnosis experiment was smoothly performed when the amount of gold ions freely present in a solution, as well as gold ions attached to protein particles, was a certain amount or more (FIGS. 6 and 7).

[0167] Experimental conditions of each number of FIG. 6 were as follows:

1: An experimental group to confirm whether, by simply treating with a Ni^{2+} solution, a patient serum, a normal individual serum, and a reducing agent, LAA, without any substance treatment, Ni^{2+} meets LAA, and thus, a color appeared while being reduced

2: A color change was measured by simply treating with an Au^{3+} (gold ions) solution, a patient serum, a normal individual serum, and a reducing agent, LAA, without any other substance treatment. As a result, it was confirmed that gold ions were reduced and turned blue while forming particles, regardless of the patient and the normal individual.

3: Only Au ions were attached to protein particles, and a patient serum, a normal individual serum, and a reducing agent were treated. As a result, since there were no free Au ions, there was no color change in the both serum samples.

4: An antibody was attached to protein particles, and then Au ions were attached thereto. Next, a patient serum, a normal individual serum, and a reducing agent were treated. To compare to the case 3 wherein there was no antibody, an experiment of binding an antibody was performed. As a result, it was confirmed that, since there were no free Au ions, color change did not occur.

5: As a result of reproducing an existing diagnosis method, it was confirmed that a color change occurred only in the patient serum.

6: To prevent Au ions from adhering to protein particles to which an antibody had been attached, the protein particles were previously treated with Ni^{2+} ions and free ions were present in the protein particles. These protein particles were treated with a patient serum, a normal individual serum, and a reducing agent. As a result, it was confirmed that reduction occurred due to the free ions, and thus, a color change occurred. However, it was confirmed that, since Au ions were absent in the protein particles to which the antibody had been attached, cluster formation was not facilitated, and thus, there was no difference between the normal individual serum and the patient serum.

Example 8: Confirmation of reliability of quantitative analysis using one-step diagnosis experiment and known diagnosis kit

8-1. Confirmation of possibility of quantitative analysis of one-step diagnosis method of present invention

[0168] A human serum-derived TnI standard sample (30-AT43, Fitzgerald, Acton, MA, U.S.A.) was respectively spiked to three types of normal individual serums, standard serum samples at different concentrations (0, 2, 5, 10, 20, 30 ng/ml) were prepared for each of the normal individual serums, and detection signals of the serums were detected as an absorbance at 576 nm at 15 minutes (FIG. 13A), 20 minutes (B), 25 minutes (C) and 30 minutes (D) after the start of diagnosis according to the method of Example 4.

[0169] As results, as shown in FIG. 13, it was confirmed that linear proportionalities of measured detection signal values were the best at 15 minutes and 20 minutes after the start of diagnosis. In addition, at 15 to 20 minutes after the start of diagnosis, it was confirmed that a disease was developed or not and quantitative analysis was possible.

8-2. Confirmation of possibility of quantitative analysis of known diagnosis kit

1) ECLIA diagnosis equipment provided by Green Cross Medical Foundation

[0170] Using an ECLIA diagnosis equipment (Roche E-170 model) provided by the Green Cross Medical Foundation, standard serum samples (normal individual sample A: FIG. 14, normal individual sample B: FIG. 15, normal individual sample C: FIG. 16) prepared according to Example 8-1 were subjected to quantitative analysis.

[0171] As results, as shown in FIGS. 14 to 16, it was confirmed that an exaggerated analysis result tended to be shown as the actual concentration of TnI increased, such a tendency increased at a concentration of 20 ng/ml or more, and variations between measured values also varied greatly for each sample.

2) ELISA diagnosis equipment manufactured by Elabscience

[0172] Using a diagnosis equipment (E-EL-H0144, Elabscience, 14780 Memorial Drive, Suite 216, Houston, Texas 77079, U.S.A.) manufactured by Elabscience, standard serum samples (normal individual sample A: FIG. 17, normal individual sample B: FIG. 18, normal individual sample C: FIG. 19) prepared according to Example 8-1 were subjected to quantitative analysis.

[0173] As results, as shown in FIGS. 17 to 19, it was confirmed that, contrary to the analysis results by the ECLIA diagnosis equipment, detection signals lower than actual concentrations were measured in all serum samples, and there was no deviation, but there was no reliable concentration interval.

3) ELISA diagnosis equipment manufactured by Abbexa

[0174] Using a diagnosis equipment (abx050255, Abbexa Ltd. Cambridge Science Park, Cambridge, CB4 0EY, U.K.) manufactured by Abbexa, standard serum samples (normal individual sample A: FIG. 20, normal individual sample B: FIG. 21, normal individual sample C: FIG. 22) prepared according to Example 8-1 were subjected to quantitative analysis.

[0175] As results, as shown in FIGS. 20 to 22, it was confirmed that, similar to the diagnosis results by the ELISA diagnosis equipment manufactured by Elabscience, detection signals lower than actual concentrations were measured, and there was no proportionality of measured signal measured values according to a concentration, whereby reliable quantitative analysis results were obtained.

4) ELISA diagnosis equipment manufactured by ALPCO

[0176] Using a diagnosis equipment (25-TR1HU-E01, ALPCO. 26-G Keewaydin Drive, Salem, NH 03079, U.S.A.) manufactured by ALPCO, standard serum samples (normal individual sample A: FIG. 23, normal individual sample B: FIG. 24, normal individual sample C: FIG. 25) prepared according to Example 8-1 were subjected to quantitative analysis.

[0177] As results, as shown in FIGS. 23 to 25, it was confirmed that detection signals closet to actual concentrations were measured, compared the two types of ELISA diagnosis kits, but deviations in the entire concentration range were not small, and a linear proportionality according to concentrations was not high, whereby reliable quantitative analysis results were not obtained.

Example 9: Confirmation of limit of detection (LOD) of one-step diagnosis method

9-1. Confirmation of LOD upon acute myocardial infarction diagnosis

[0178] A disease marker, Troponin I, in a concentration range of 0.002 to 2 ng/ml was spiked to a normal individual serum, thereby manufacturing a standard serum sample. The manufactured standard serum sample was subjected to the LOD measurement experiment of Example 4. A color changes in the sample in 96 well plate was confirmed and, simultaneously, an absorbance at 576 nm was measured.

[0179] As results, as shown in FIG. 26, it was confirmed that the LOD of TnI in the acute myocardial infarction diagnosis was present in a concentration range of at least 0.02 ng/ml (0.83 pM) and at most 0.2 ng/ml (8.3 pM). This was significantly low than the LOD (0.16 ng/ml) of the ECLIA-based diagnosis equipment.

9-2. Confirmation of LOD upon hepatitis C diagnosis

[0180] A disease marker, anti-HCV(c33c) IgG standard (LS-C103178, LifeSpan BioSciences, Inc., Seattle, WA, U.S.A.), in a concentration range of 0.001 to 10 ng/ml was spiked to a normal individual serum, thereby manufacturing a standard serum sample. The manufactured standard serum sample was subjected to the LOD measurement experiment of Example 4. A color changes in the sample in 96 well plate was confirmed and, simultaneously, an absorbance at 588 nm was measured.

[0181] As results, as shown in FIG. 27, it was confirmed that the LOD of the anti-HCV antibody in the hepatitis C diagnosis was present in a concentration range of at least 0.1 ng/ml (0.67 pM) and at most 1.0 ng/ml (6.7 pM). This was significantly low than the LOD (nM level) of the ELISA -based diagnosis equipment.

9-3. Confirmation of LOD upon AIDS diagnosis

[0182] A disease marker, anti-HIV(gp41) IgG standard (2509, ImmunoDX, LLC., Woburn, MA, U.S.A.), in a concentration range of 0.001 to 10 ng/ml was spiked to a normal individual serum, thereby manufacturing a standard serum sample. The manufactured standard serum sample was subjected to the LOD measurement experiment of Example 4. A color changes in the sample in 96 well plate was confirmed and, simultaneously, an absorbance at 555 nm was measured.

[0183] As results, as shown in FIG. 28, it was confirmed that the LOD of the anti-HIV antibody in AIDS was present in a concentration range of at least 0.1 ng/ml (0.67 pM) and at most 1.0 ng/ml (6.7 pM). This was significantly low than the LOD (nM level) of the ELISA -based diagnosis equipment.

[0184] As described above, specific portions of the present invention have been described in detail. Those skilled in the art will appreciate that these specific descriptions are merely preferred embodiments, and thus the scope of the present invention is not limited thereto. Therefore, the substantial scope of the present invention will be defined by the appended claims and their equivalents.

[Industrial Applicability]

[0185] A method of detecting a disease-specific marker according to the present invention can diagnose a disease in a single step without any processes such as immobilization and washing processes that are generally accompanied in existing diagnosis methods such as ELISA; can short the time of a diagnostic test, which takes several hours or even several days, to about 10 minutes, thus being effectively used for diagnosis of diseases, in particular, of patients in an emergency; and can be confirmed by the naked eye without a separate analyzer, thus minimizing detection costs.

Sequence List **Free Text**

[0186] Electronic File Attached.

EP 3 611 505 A1

<110> Korea University Research and Business Foundation
 <120> A Method for Accurate, Rapid, and Convenient One-Step-Diagnosis
 of Disease Based on Signal Self-Enhancement
 5 <130> PP-B2025
 <150> KR 10-2017-0047841
 <151> 2017-04-13
 10 <160> 16
 <170> KoPatentIn 3.0
 <210> 1
 15 <211> 24
 <212> DNA
 <213> Artificial Sequence
 <220>
 20 <223> H6-SPAB-capsid_F
 <400> 1
 ctcgaggcac cgaaagctga taac 24
 25 <210> 2
 <211> 24
 <212> DNA
 <213> Artificial Sequence
 30 <220>
 <223> H6-SPAB-capsid_R
 <400> 2
 35 ggatccgtca gcttttagtg cttg 24
 <210> 3
 <211> 24
 <212> DNA
 40 <213> Artificial Sequence
 <220>
 <223> H6-c33c-capsid_F
 45 <400> 3
 ctcgaggcgg tggactttat ccct 24
 <210> 4
 50 <211> 24
 <212> DNA
 <213> Artificial Sequence
 <220>
 55 <223> H6-c33c-capsid_R
 <400> 4

	ggatccacac gtattgcagt ctat	24
5	<210> 5 <211> 24 <212> DNA <213> Artificial Sequence	
10	<220> <223> H6-gp41-capsid_F	
15	<400> 5 ctcgagatcc tggctgtgga acgc	24
20	<210> 6 <211> 24 <212> DNA <213> Artificial Sequence	
25	<220> <223> H6-gp41-capsid_R	
30	<400> 6 ggatccgatc aactttccac tagc	24
35	<210> 7 <211> 24 <212> DNA <213> Artificial Sequence	
40	<220> <223> H6-p24-capsid_F	
45	<400> 7 ctcgagccgg aagtaatccc gatg	24
50	<210> 8 <211> 24 <212> DNA <213> Artificial Sequence	
55	<220> <223> H6-p24-capsid_R	
	<400> 8 ggatcctccc actccctgac atgc	24
	<210> 9 <211> 24 <212> DNA <213> Artificial Sequence	
	<220> <223> hFTN-511p-c100p-c22p-H6 _F	

	<400>	9	
		ctcgagatca tccccgatag ggaa	24
5	<210>	10	
	<211>	24	
	<212>	DNA	
	<213>	Artificial Sequence	
10	<220>		
	<223>	hFTN-511p-c100p-c22p-H6_R	
	<400>	10	
15		ggatccggaa gtcttcctag tcgc	24
	<210>	11	
	<211>	21	
	<212>	DNA	
20	<213>	Artificial Sequence	
	<220>		
	<223>	hFTN-ep1-H6_F	
25	<400>	11	
		ctcgaggaac ctttgagaac c	21
	<210>	12	
30	<211>	21	
	<212>	DNA	
	<213>	Artificial Sequence	
	<220>		
35	<223>	hFTN-ep1-H6_R	
	<400>	12	
		gaattctttc ctaggaggtg g	21
40	<210>	13	
	<211>	21	
	<212>	DNA	
	<213>	Artificial Sequence	
45	<220>		
	<223>	hFTN-ep2-H6_F	
	<400>	13	
50		ctcgagaaaa tcaatttggc a	21
	<210>	14	
	<211>	21	
	<212>	DNA	
55	<213>	Artificial Sequence	
	<220>		

<223> hFTN-ep2-H6_R

<400> 14

gaattcctga ctttcaattt t

21

<210> 15

<211> 21

<212> DNA

<213> Artificial Sequence

<220>

<223> hFTN-ep3-H6_F

<400> 15

catatgacga ccgcgtccac c

21

<210> 16

<211> 21

<212> DNA

<213> Artificial Sequence

<220>

<223> hFTN-ep3-H6_R

<400> 16

atcgatttag tgatggtgat g

21

Claims

1. A method of detecting a disease-specific marker using self-amplification of a detection signal, the method comprising: (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.
2. A method of detecting an antiviral antibody using self-amplification of a detection signal, the method comprising: (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antigen for detecting an antiviral antibody, free Au ions, and adsorbed Au ions are present, adding a sample, which contains an antiviral antibody binding specifically to the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of virus by a chromogenic reaction through the Au particle formation.
3. A method of providing information for disease diagnosis using self-amplification of a detection signal, the method comprising: (a) a step of simultaneously inducing an antigen-antibody immune response and an Au particle formation reaction by reduction of Au ions in an assay solution prepared by, to a pre-assay solution in which all of an antibody or antigen for detection of a disease-specific marker, free Au ions, and adsorbed Au ions are present, adding a sample, which contains a disease-specific antigen or antibody binding specifically to the antibody or the antigen, and a reducing agent; and (b) a step of confirming the presence or absence of a disease-specific marker by a chromogenic reaction through the Au particle formation.
4. The method according to any one of claims 1 to 3, wherein the adsorbed Au ions are adsorbed onto an amino acid

selected from the group consisting of histidine, lysine, and arginine.

- 5 5. The method according to any one of claims 1 to 3, wherein the reducing agent is selected from the group consisting of ascorbic acid, imidazole, pyrazole, histamine, hydroxyl amine, citric acid, and sodium borohydride.
- 6 6. The method according to any one of claims 1 to 3, wherein the sample is selected from the group consisting of blood, plasma, serum, urine, saliva, oral mucosa, and saliva.
- 10 7. The method according to any one of claims 1 to 3, wherein a concentration of the Au ions present in the pre-assay solution is 1 mM to 10 mM.
- 8 8. The method according to any one of claims 1 to 3, wherein a concentration of the reducing agent present in the assay solution is 0.005 M to 0.1 M.
- 15 9. The method according to any one of claims 1 to 3, wherein an amount of the sample is 10 μ l to 30 μ l.
- 10 10. The method according to claim 1 or 3, wherein the disease is selected from the group consisting of acute heart disease, human immunodeficiency syndrome, hepatitis C, Sjogren's syndrome, multiple sclerosis syndrome, hepatitis A, stroke, and cerebral hemorrhage.
- 20 11. The method according to any one of claims 1 to 3, wherein the chromogenic reaction occurs within at least 5 minutes to 10 minutes.
- 25 12. The method according to any one of claims 1 to 3, wherein the chromogenic reaction is confirmed by measuring an absorbance at 500 to 600 nm.
- 30 13. The method according to claim 1 or 3, wherein the antigen or antibody for detecting the disease-specific marker is exposed from surfaces of protein particles.
- 35 14. The method according to claim 13, wherein, from surfaces of the protein particles, a tag selected from the group consisting of histidine, lysine, and arginine that are capable of adsorbing Au ions is additionally exposed.
- 40 15. The method according to claim 13, wherein an immune response of the antigen or antibody for detecting the disease-specific marker occurs on surfaces of protein particles.
- 45 16. The method according to claim 14, wherein the tag adsorbs Au ions to induce aggregation of the Au particles in a presence of the reducing agent.
- 50 17. The method according to claim 2, wherein the antigen for virus detection is exposed from surfaces of protein particles.
- 55 18. The method according to claim 17, wherein, from surfaces of the protein particles, a tag selected from the group consisting of histidine, lysine, and arginine that are capable of adsorbing Au ions is additionally exposed.
19. The method according to claim 17, wherein an immune response of the antigen or antibody for virus detection occurs on surfaces of protein particles.
20. The method according to claim 18, wherein the tag adsorbs Au ions to induce aggregation of Au particles in a presence of the reducing agent.
21. The method according to claim 13, wherein the protein particles comprises a protein selected from the group consisting of ferritin, ferritin-like proteins, magnetosome-constituting proteins, virus-constituting proteins (e.g. hepatitis B virus core protein, tobacco mosaic virus), DPS (DNA binding protein), and proteasome.
22. The method according to claim 17, wherein the protein particles comprises a protein selected from the group consisting of ferritin, ferritin-like proteins, magnetosome-constituting proteins, virus-constituting proteins (e.g. hepatitis B virus core protein, tobacco mosaic virus), DPS (DNA binding protein), and proteasome.

Figure 1

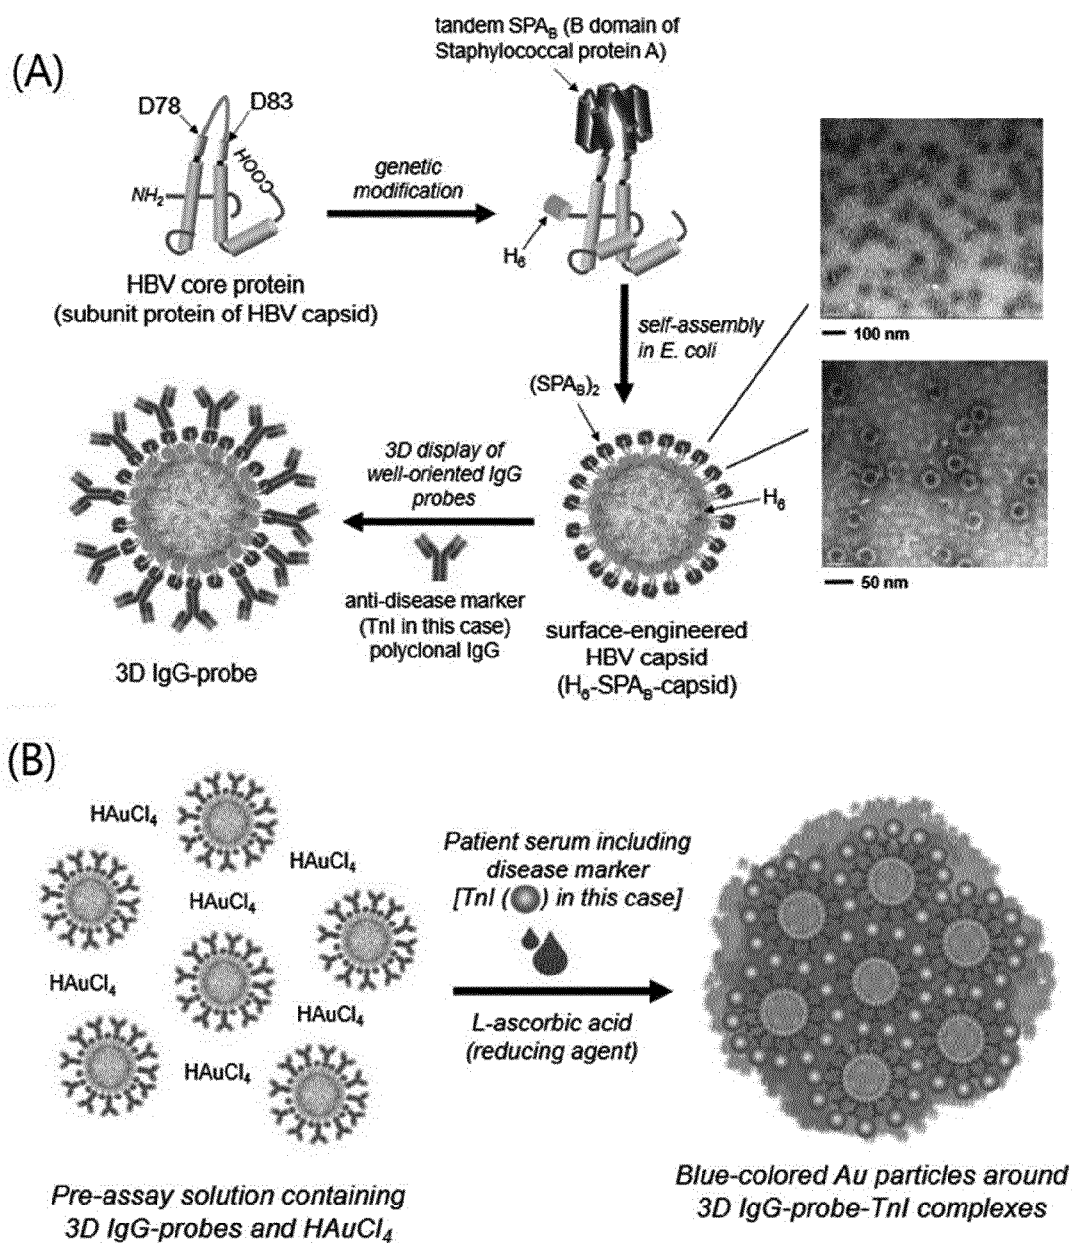


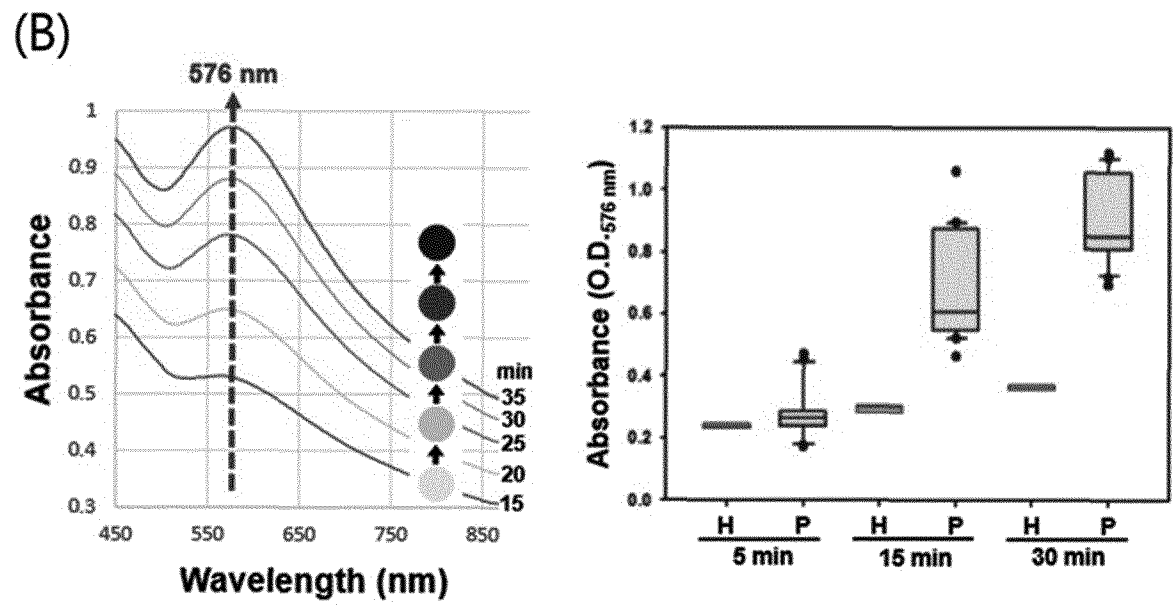
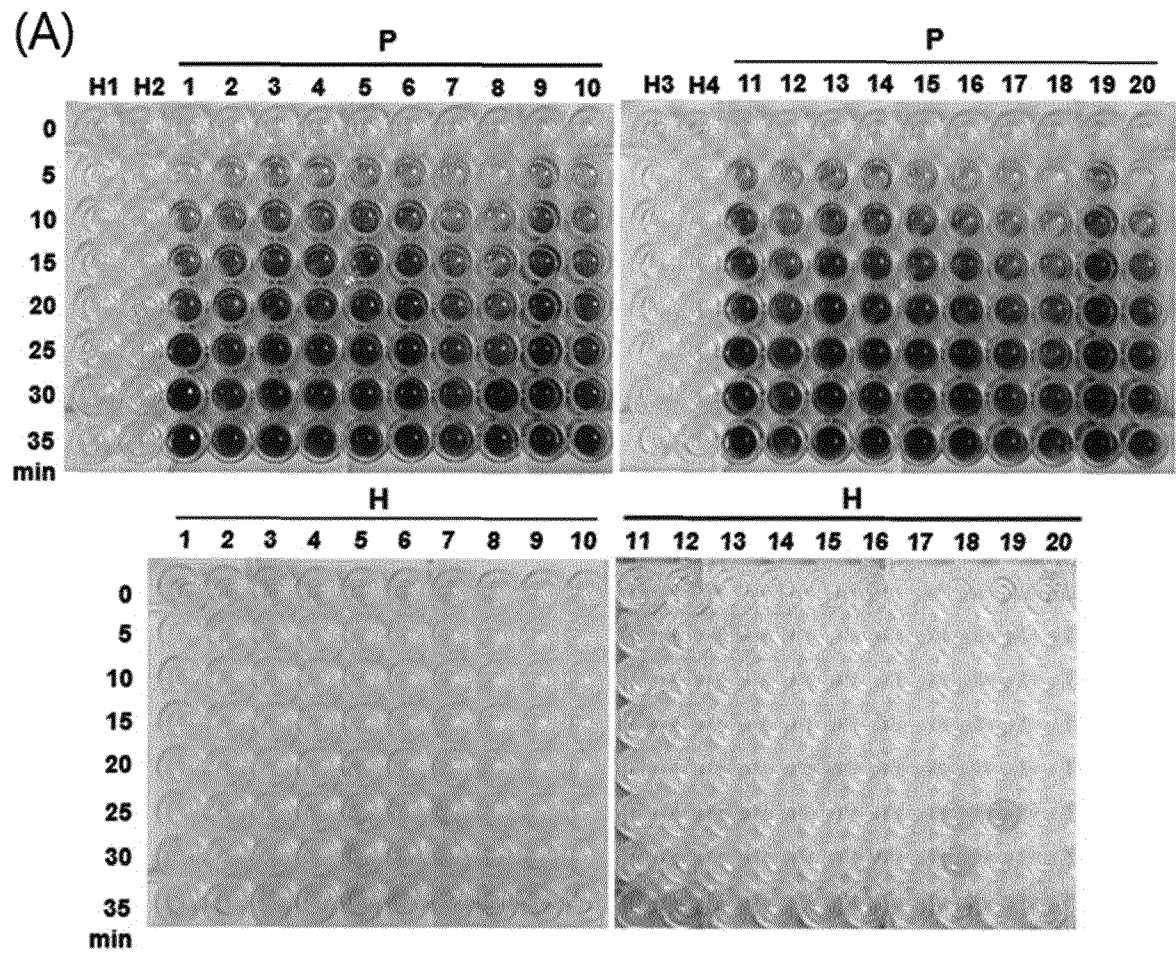
Figure 2

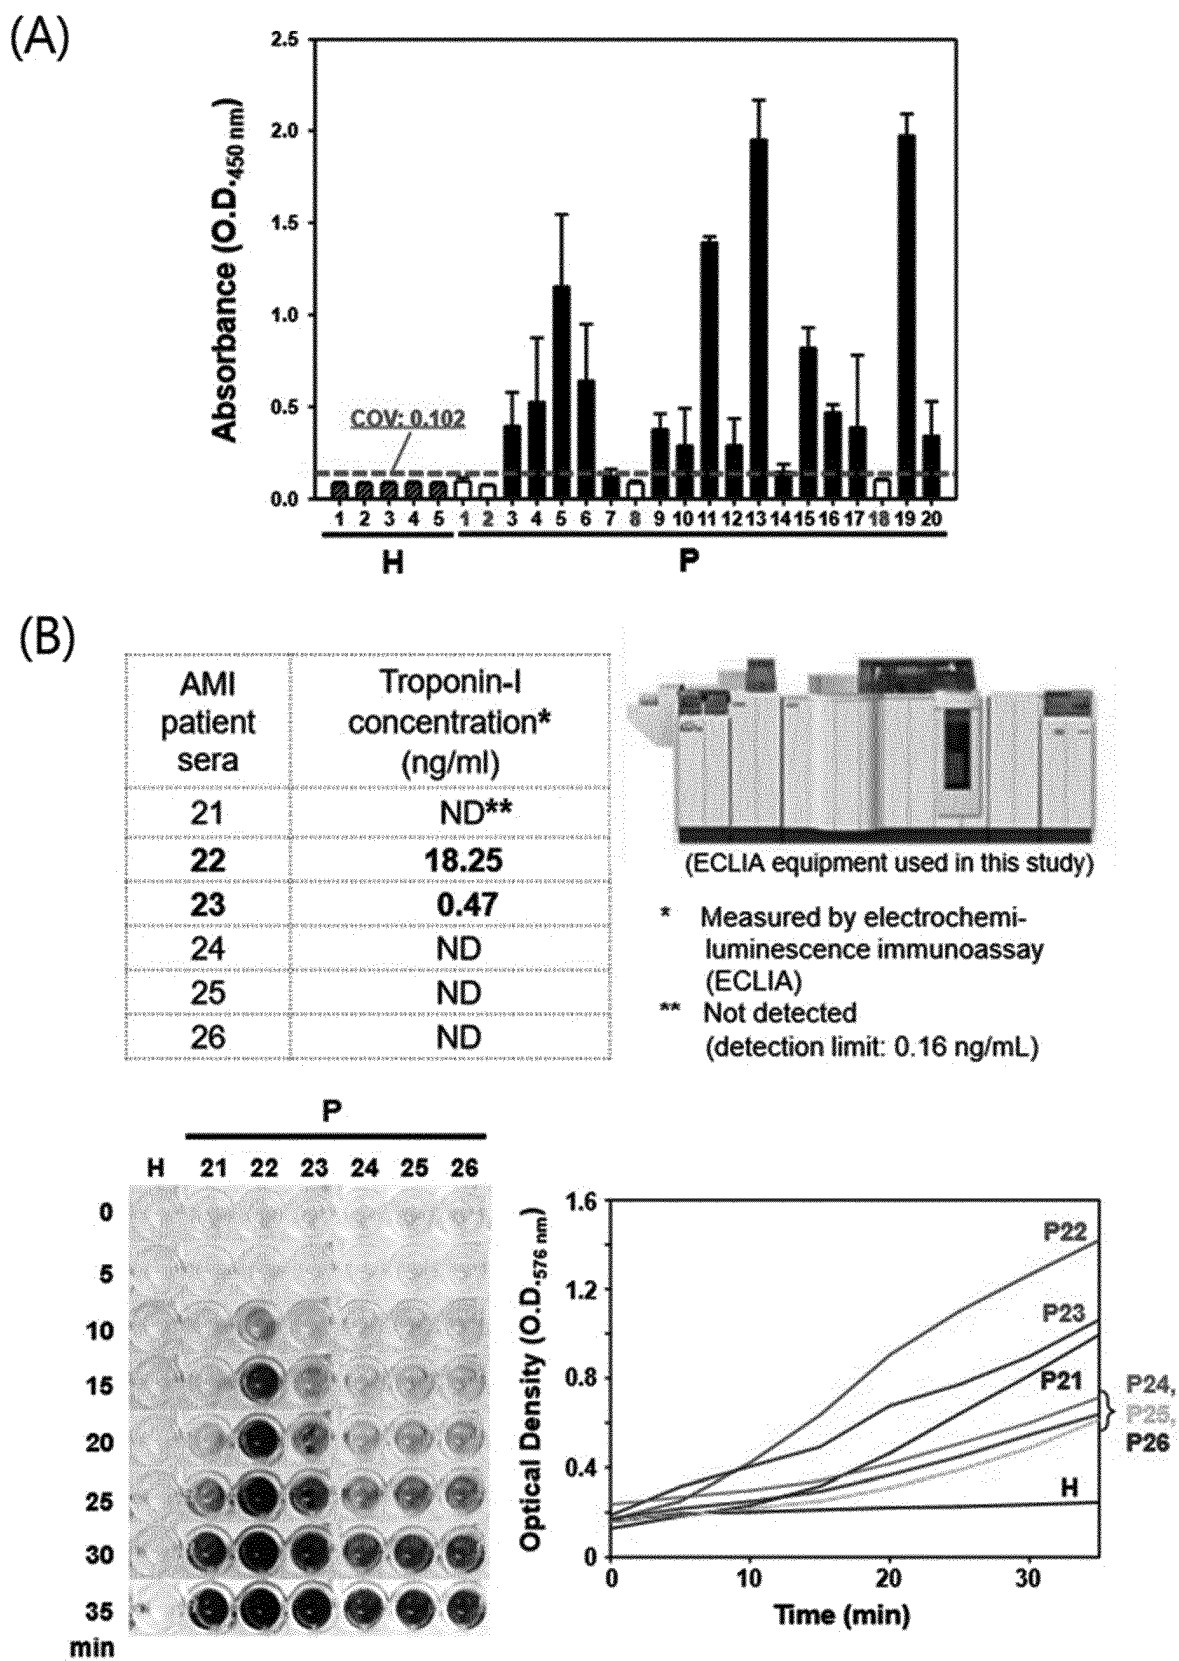
Figure 3


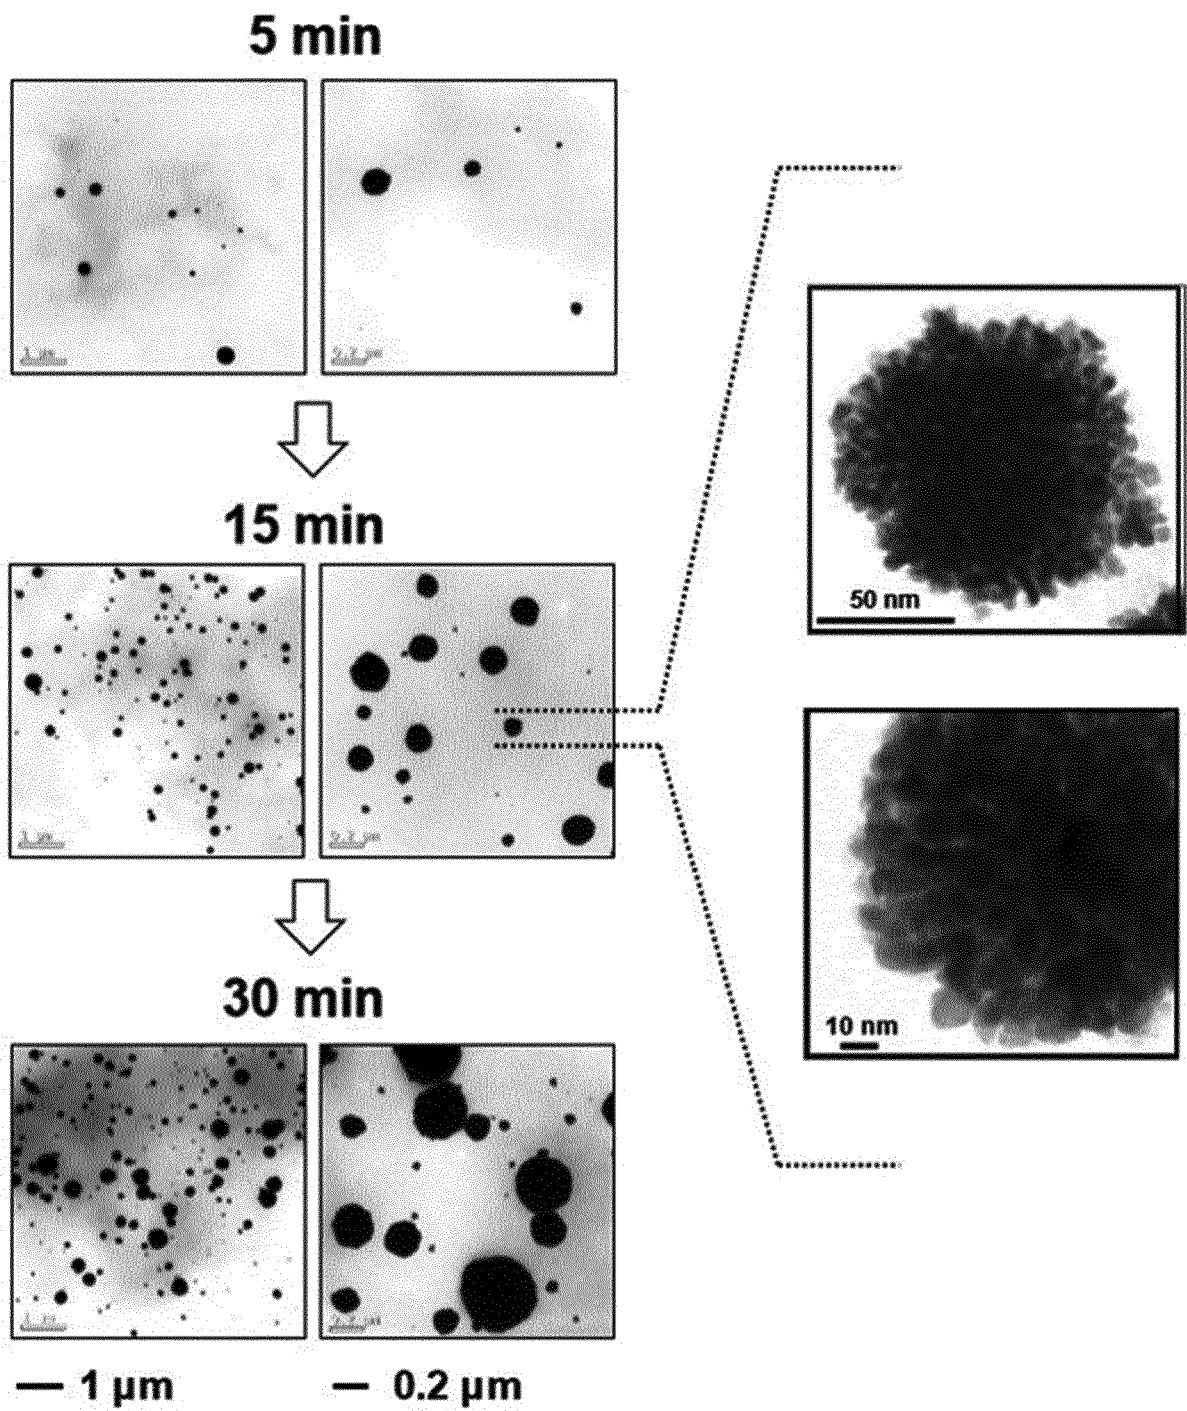
Figure 4

Figure 5

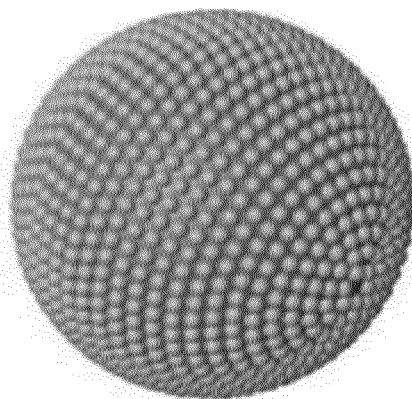(A)



(B)

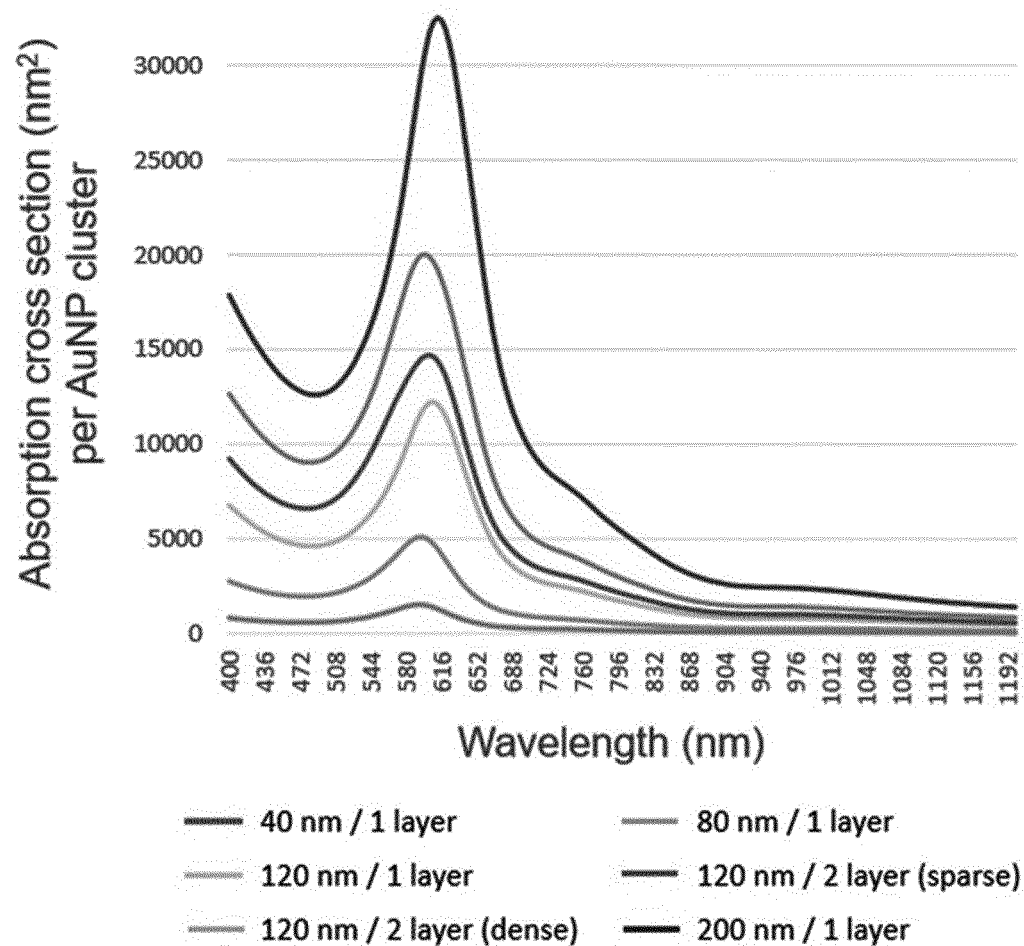


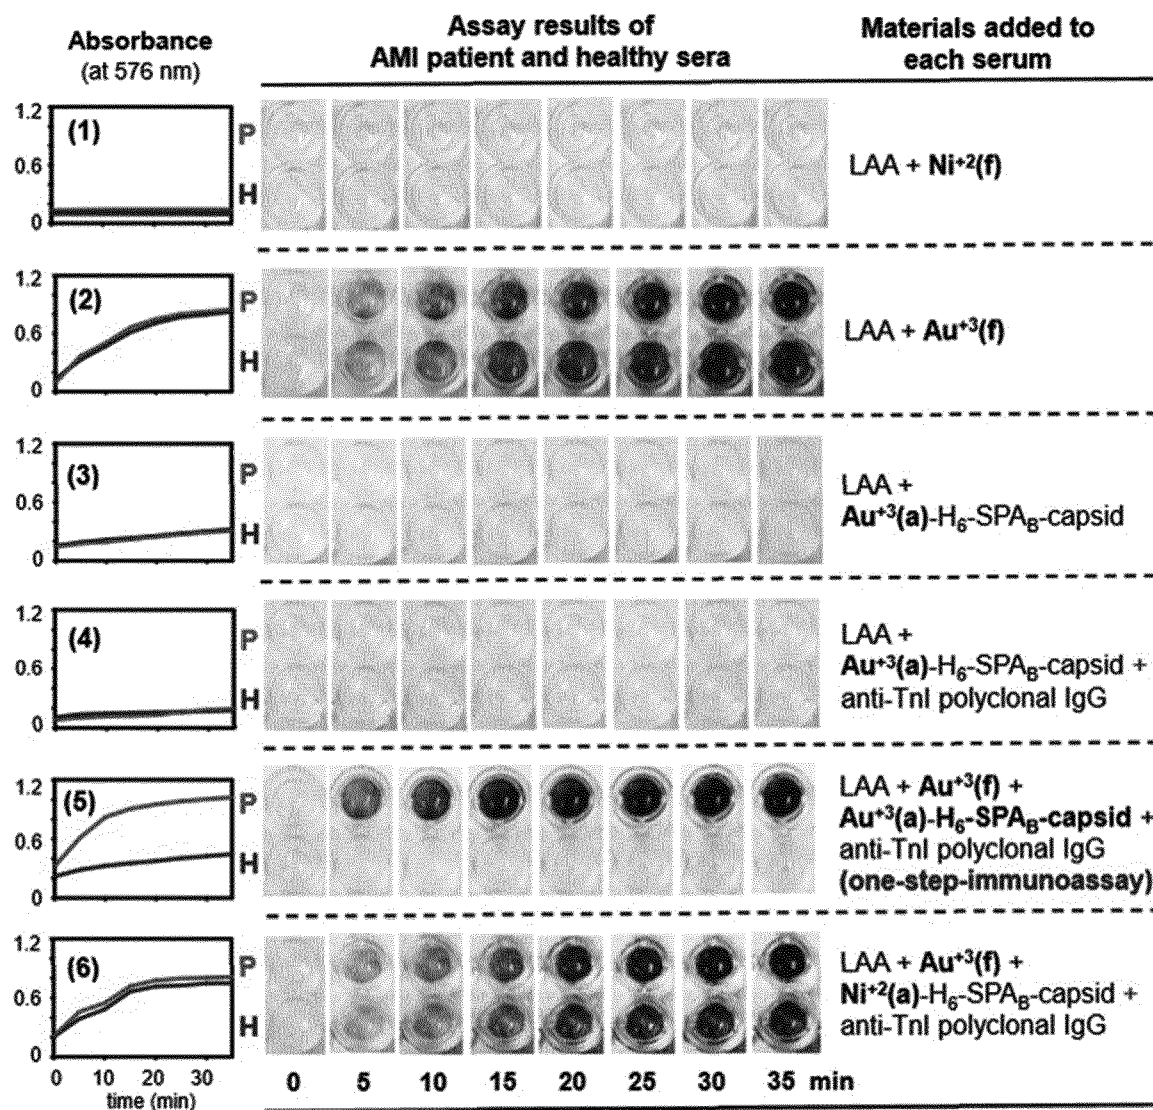
Figure 6

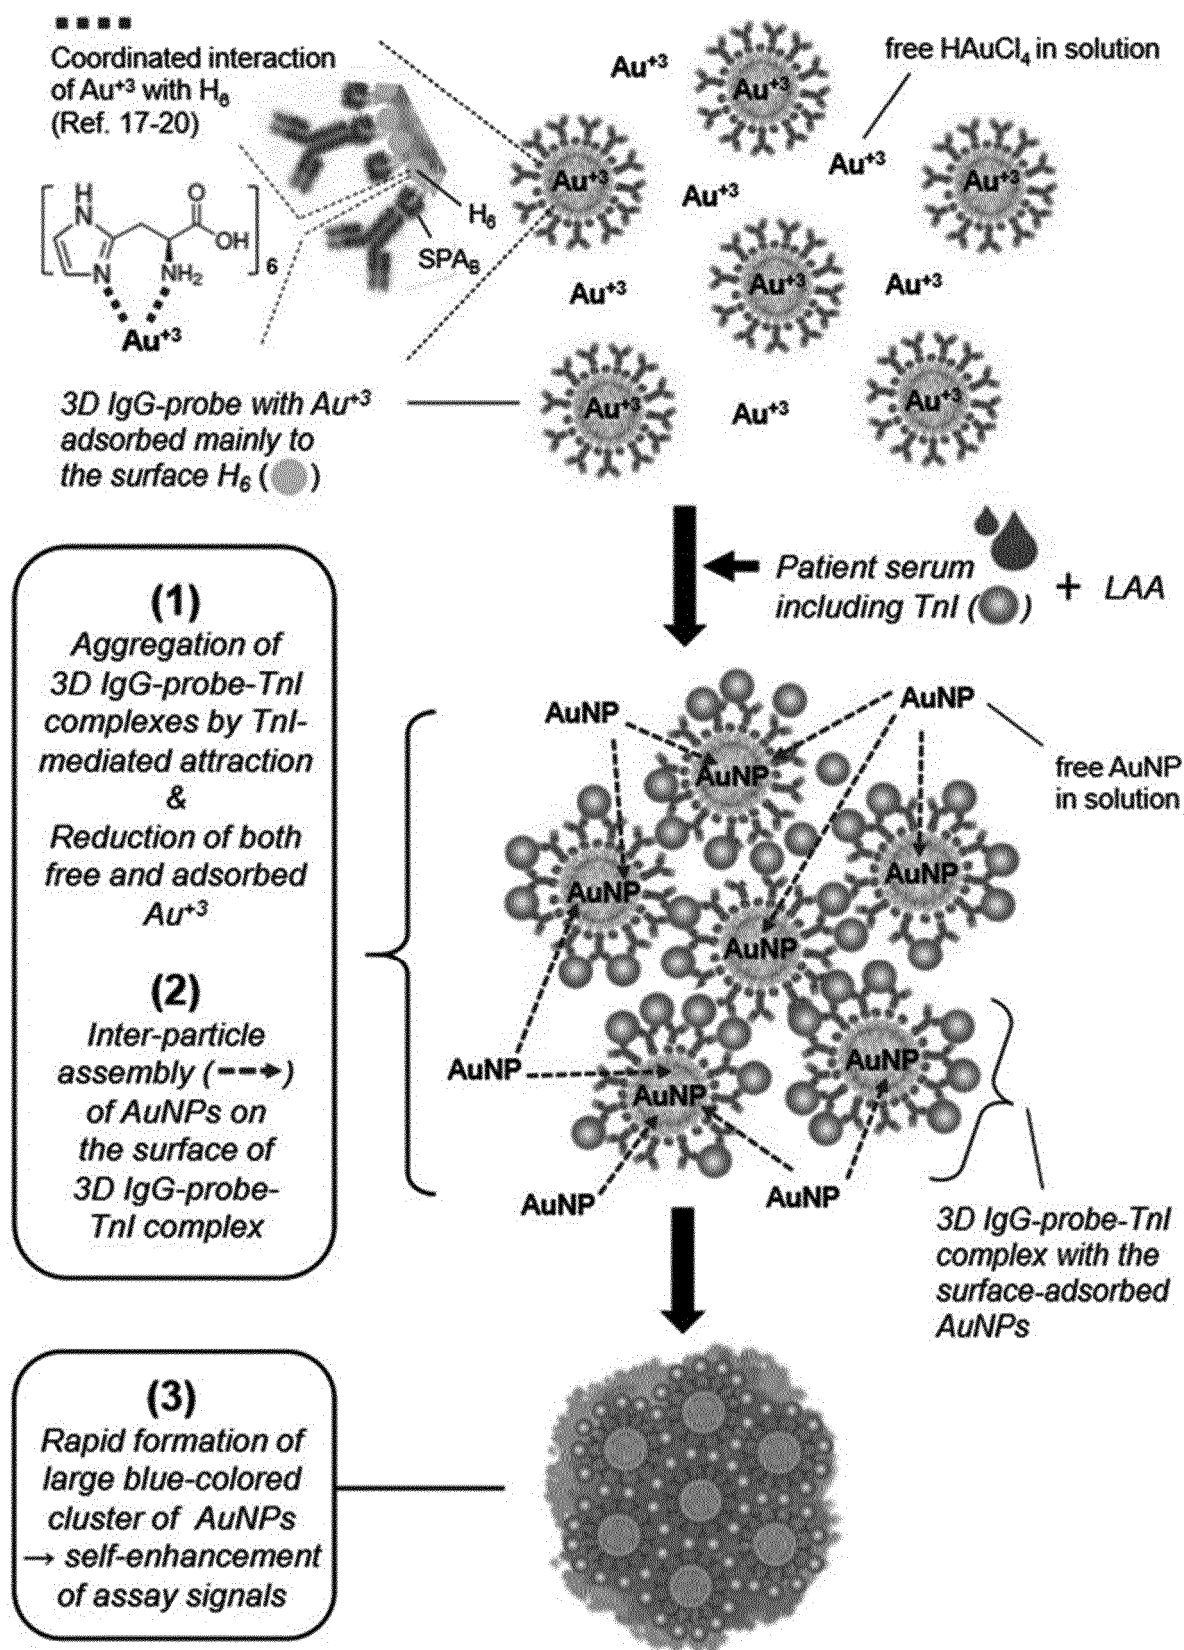
Figure 7

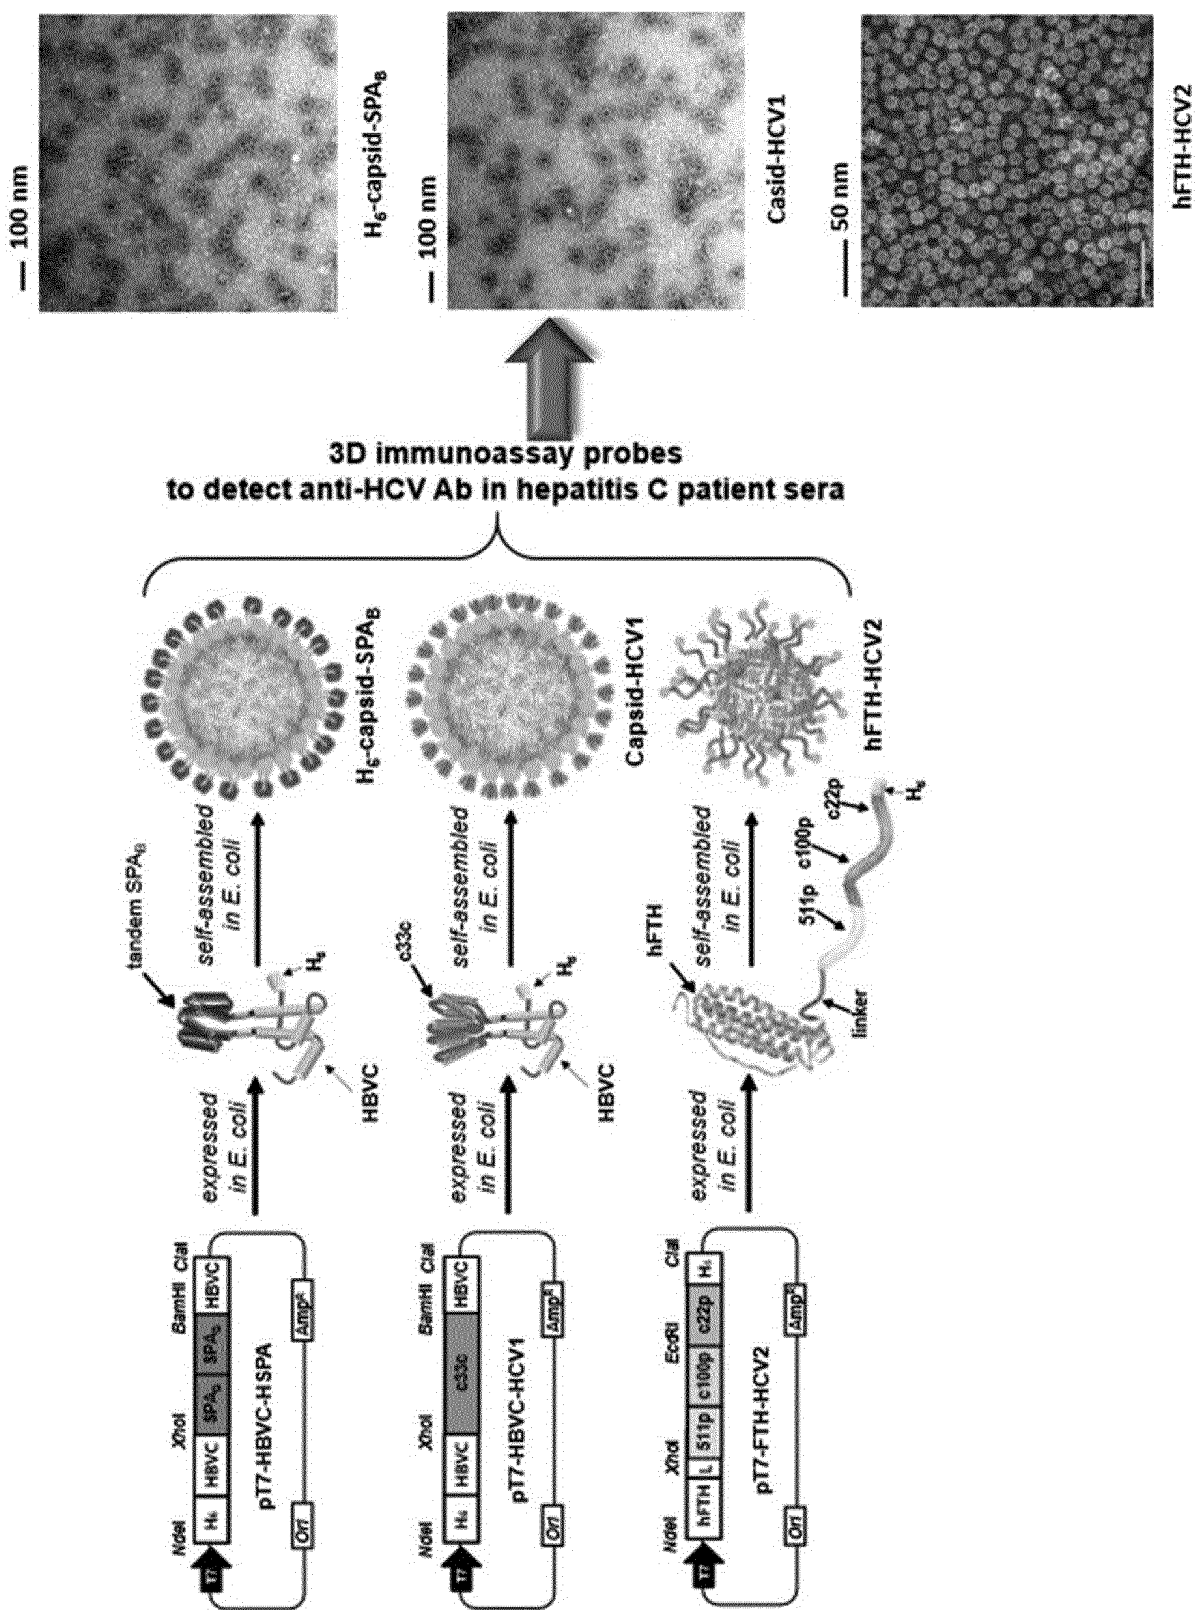
Figure 8

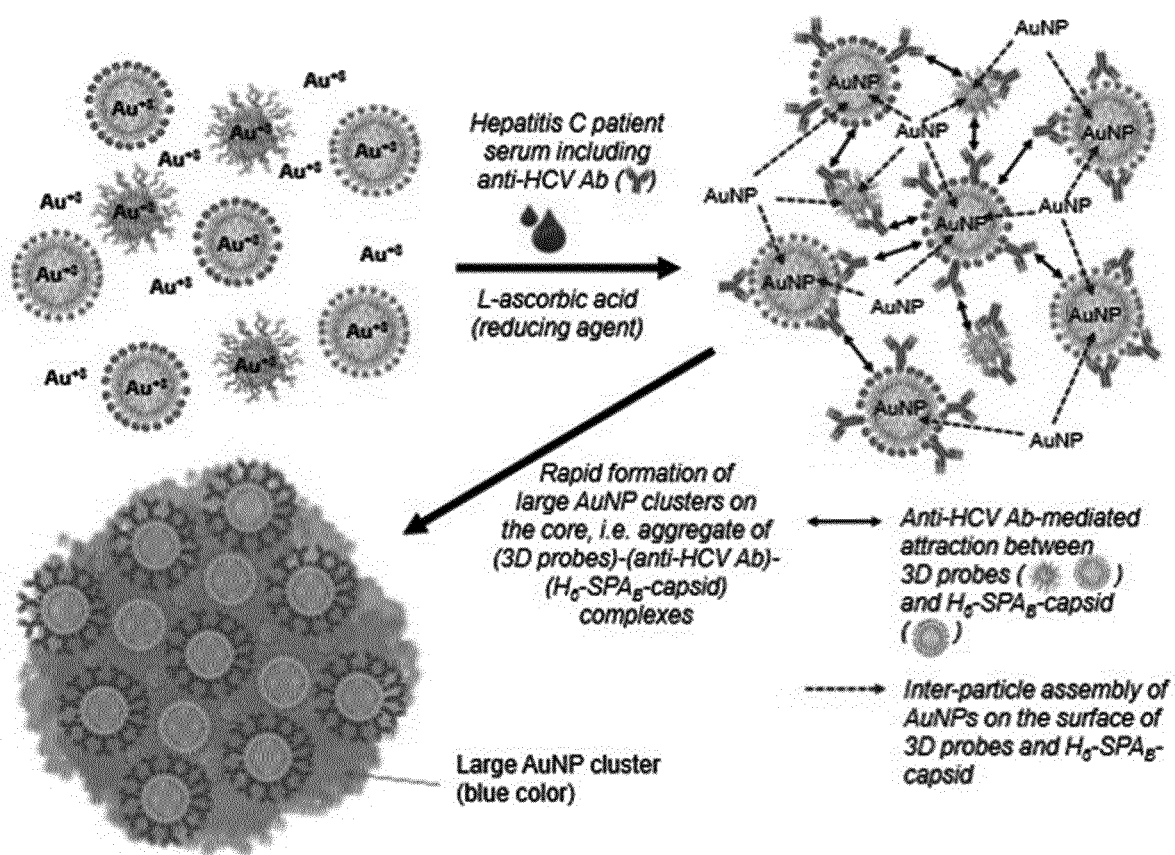
Figure 9

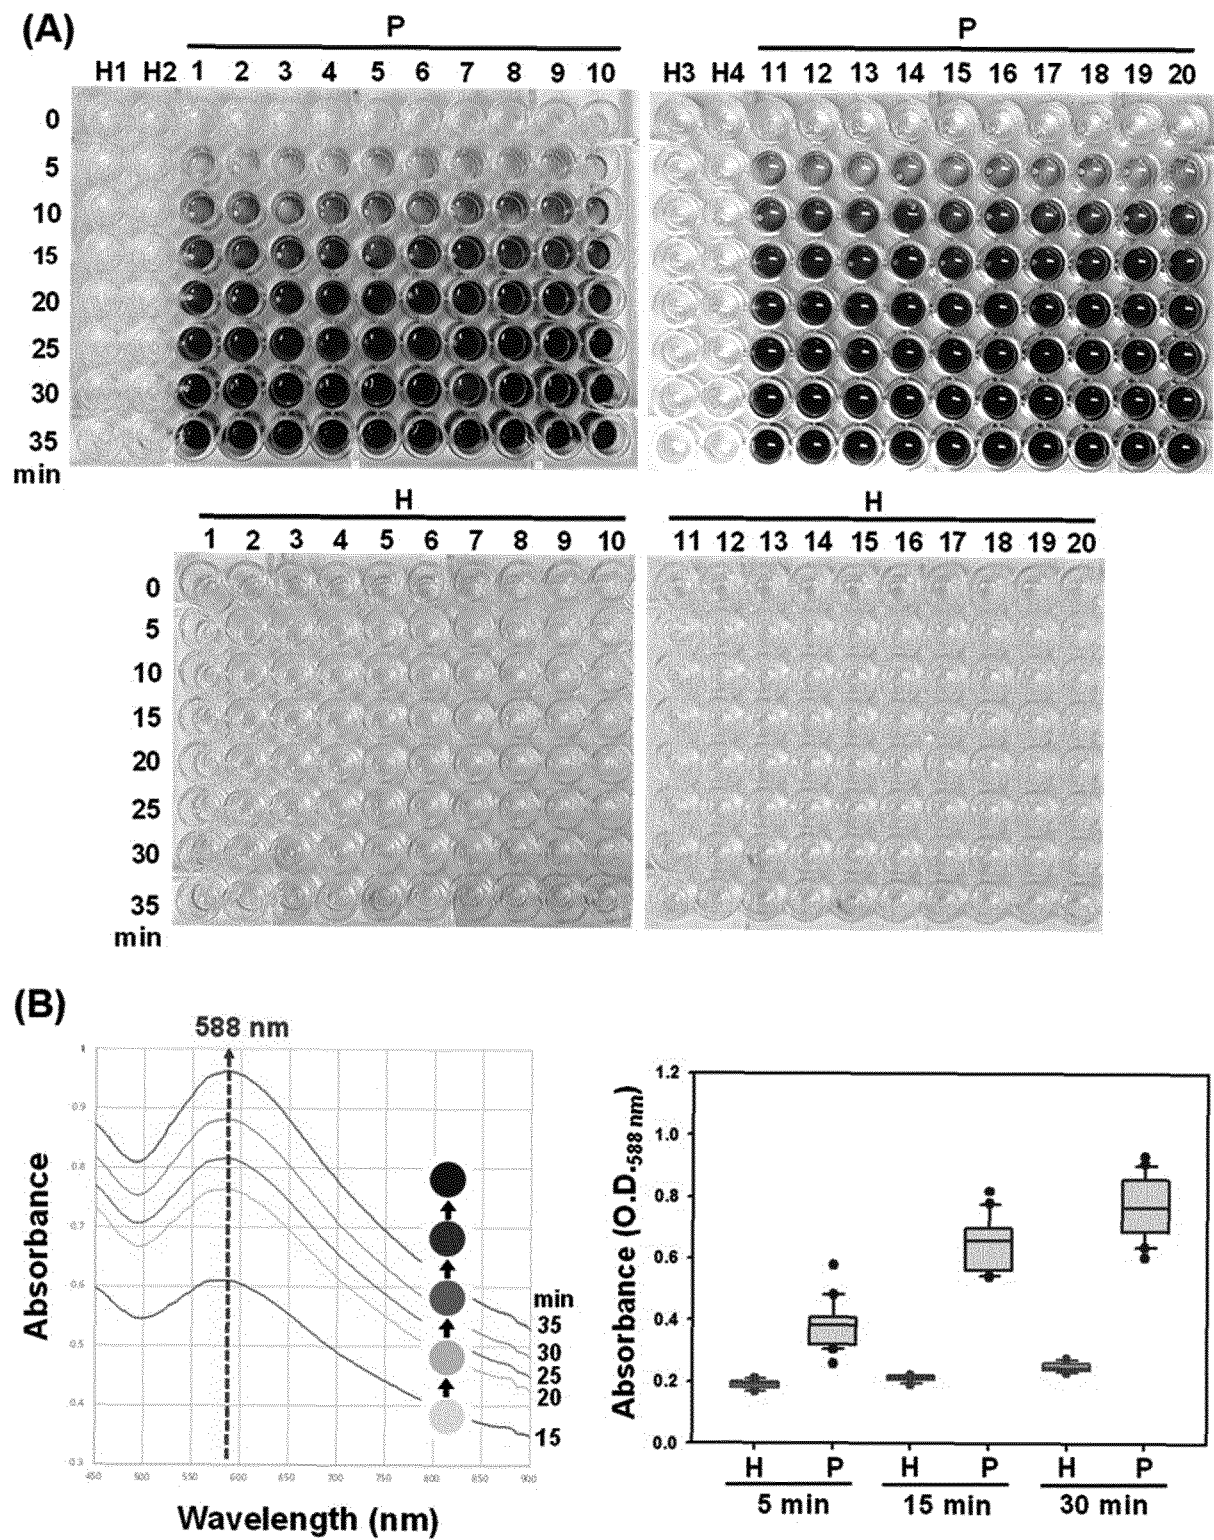
Figure 10

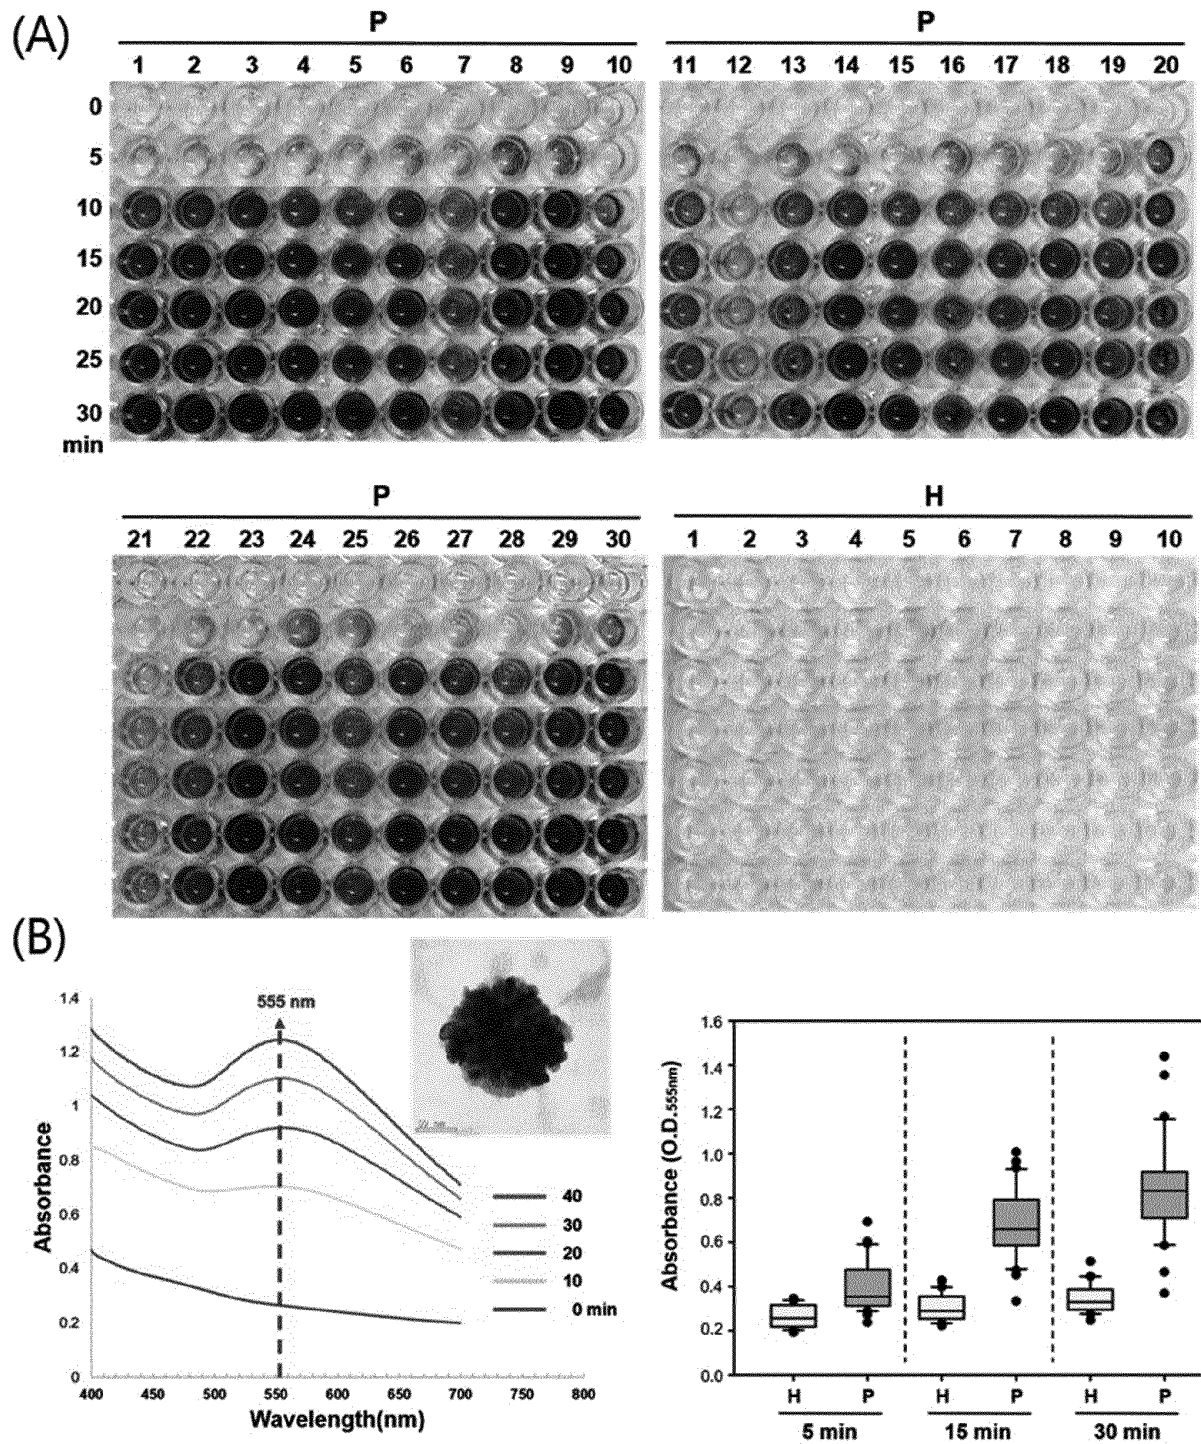
Figure 11

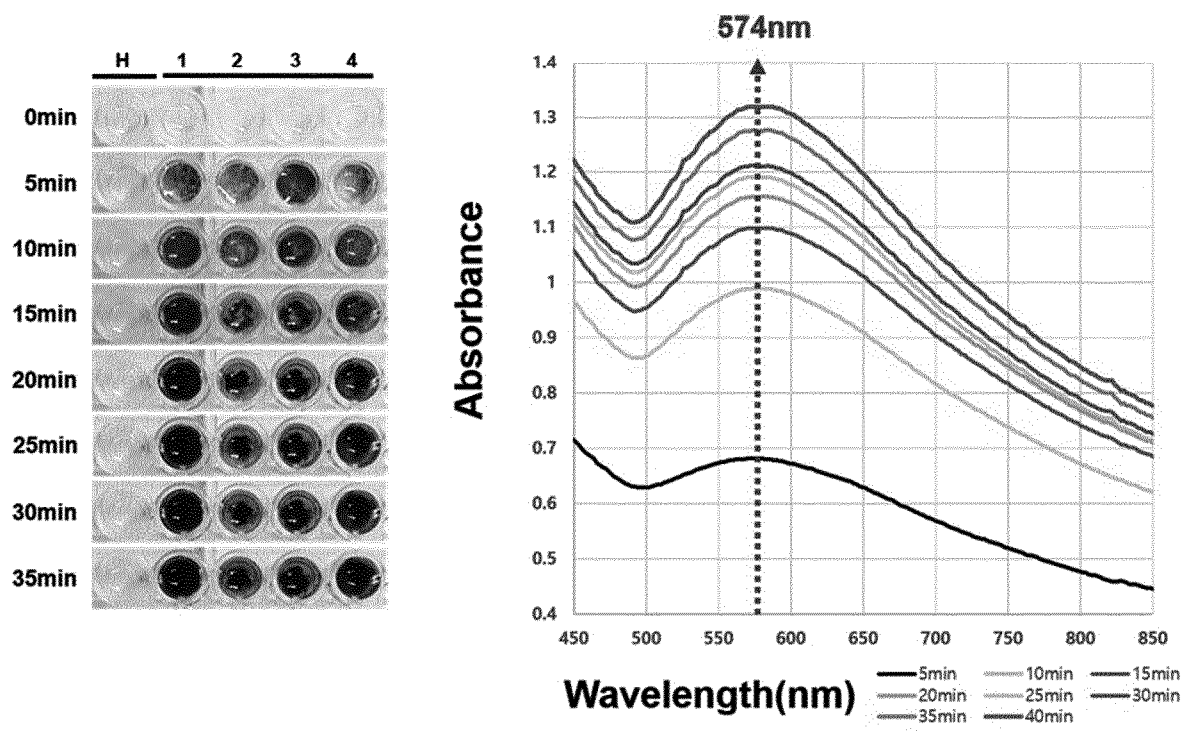
Figure 12

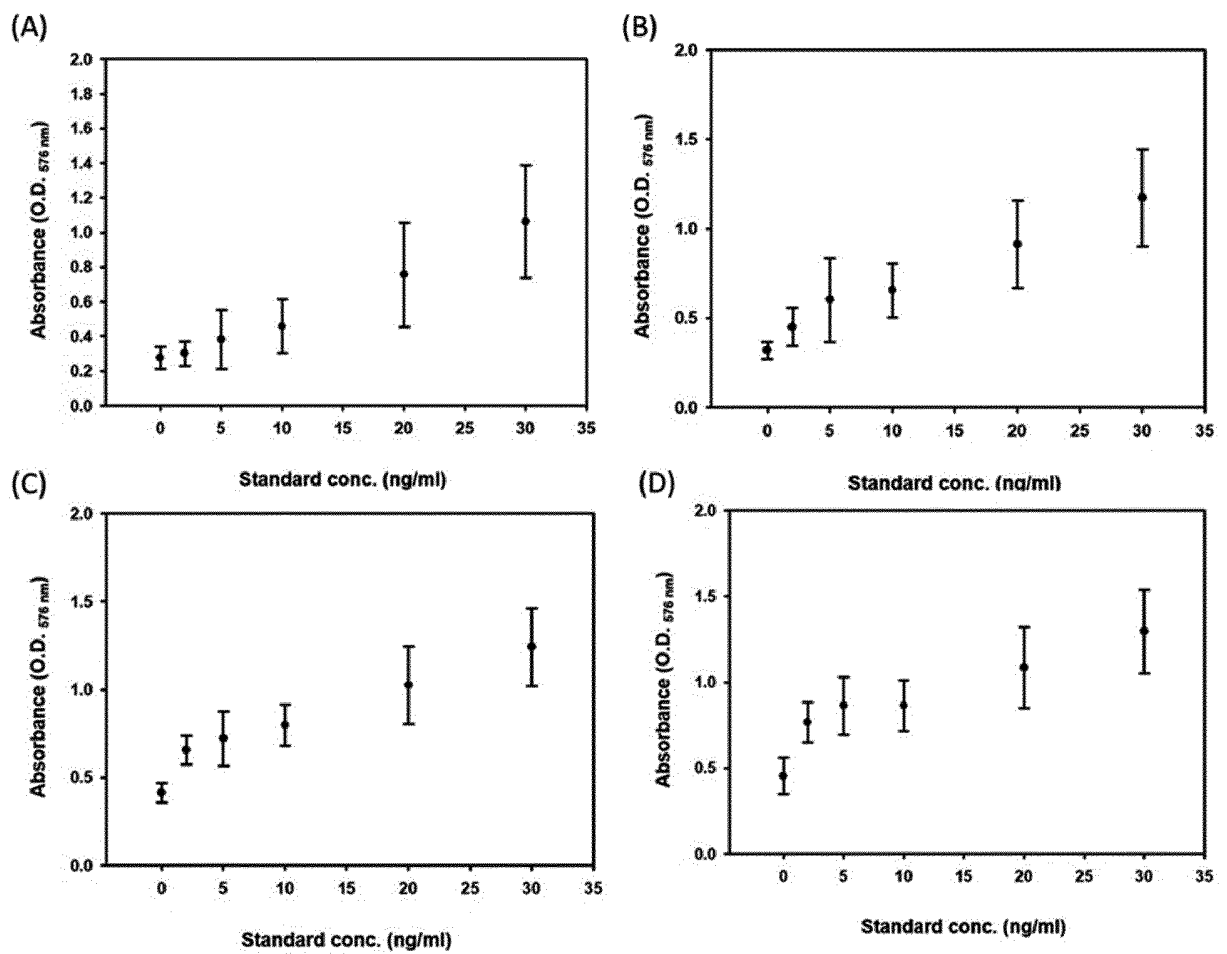
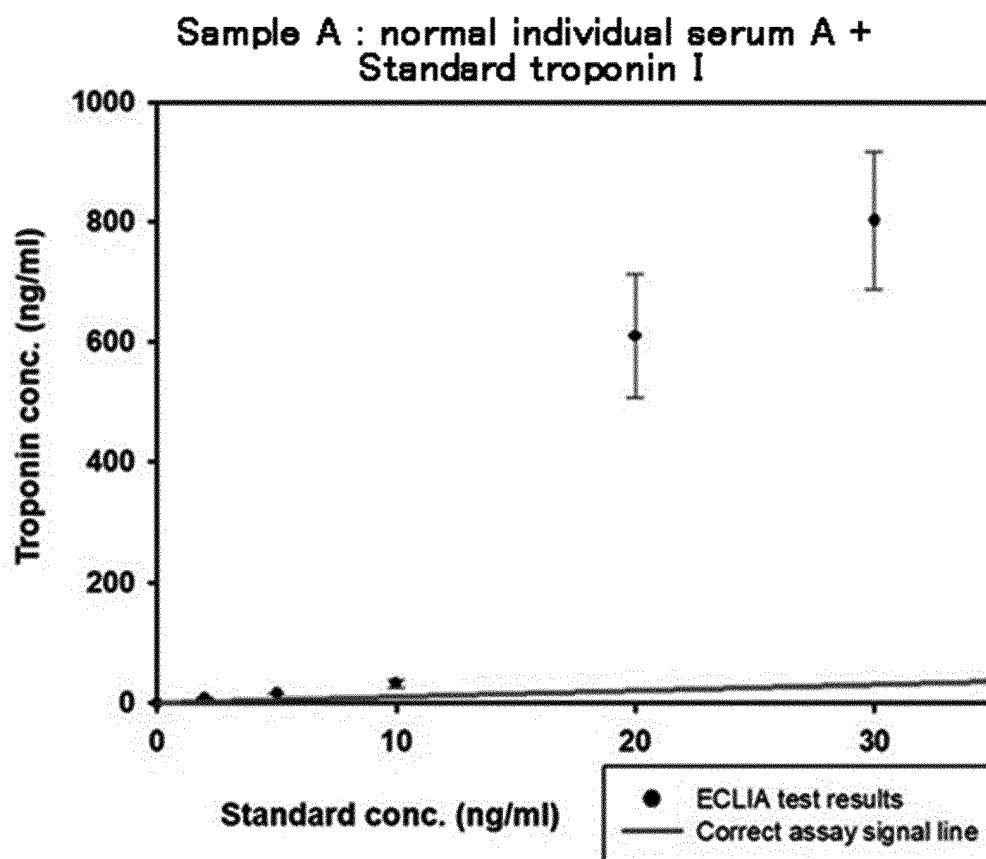
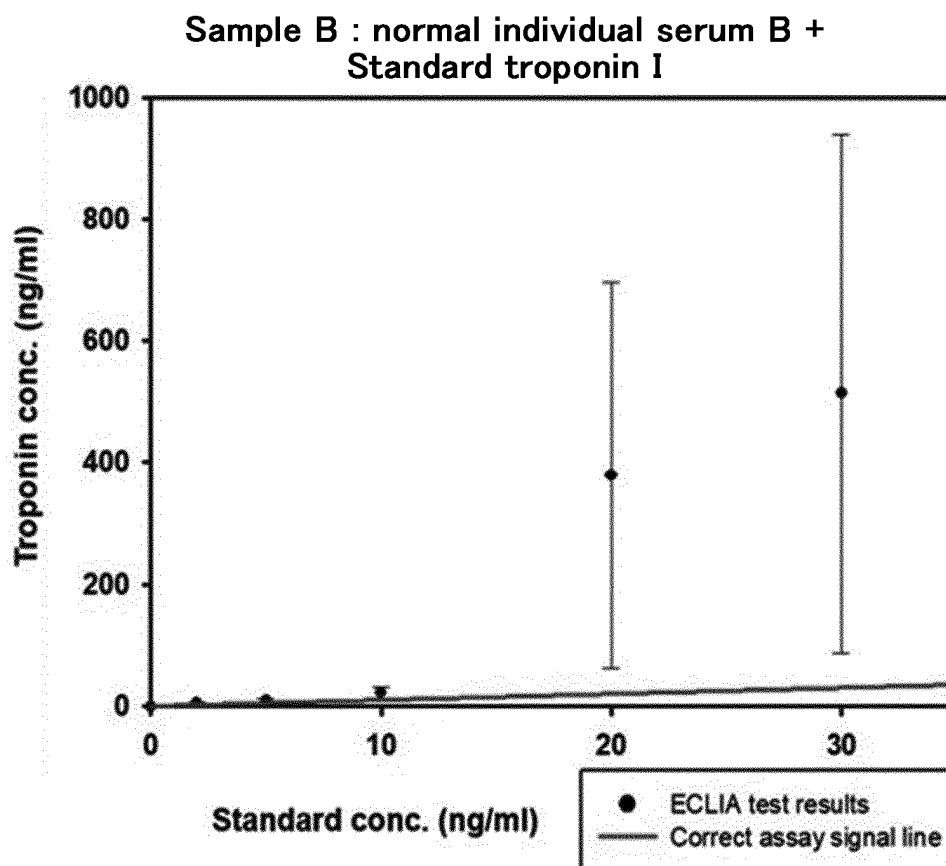
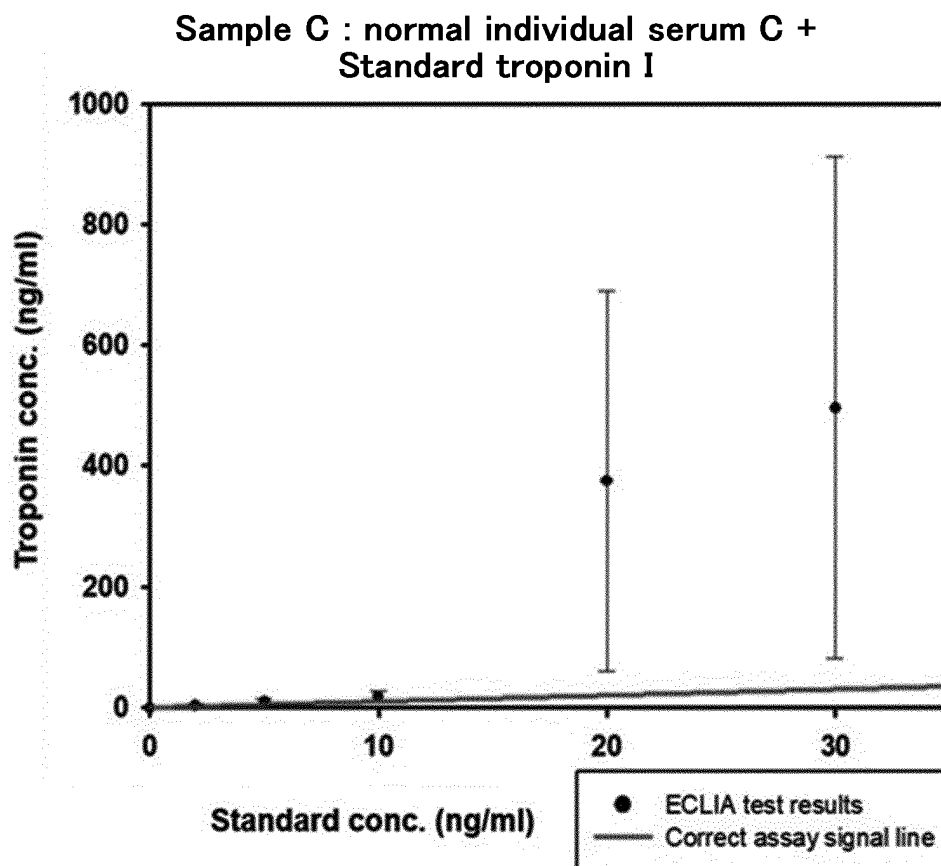
Figure 13

Figure 14

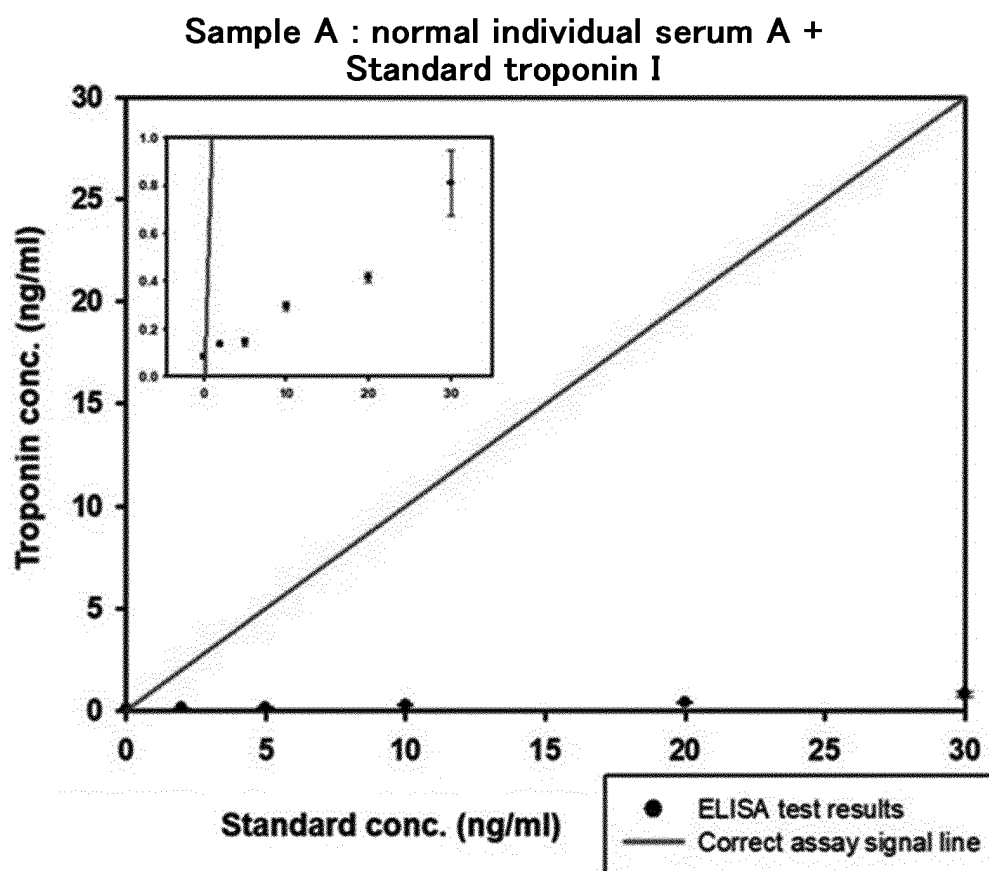
Standard conc.	ECLIA (Mean ± s.d.)
30 ng/ml	801.8 ± 115.0 ng/ml
20 ng/ml	609.8 ± 103.7 ng/ml
10 ng/ml	31.5 ± 6.2 ng/ml
5 ng/ml	14.7 ± 0.6 ng/ml
2 ng/ml	6.9 ± 0.7 ng/ml
0 ng/ml	< 0.16 ng/ml

Figure 15

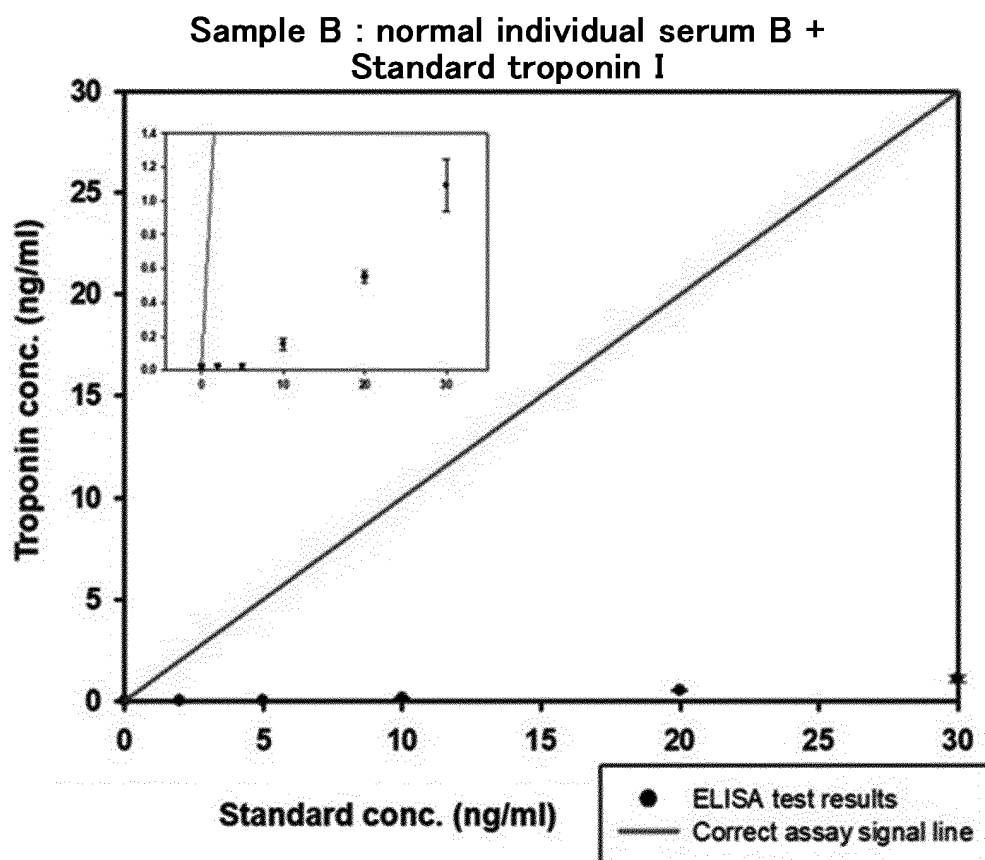
Standard conc.	ECLIA (Mean $\pm$ s.d.)
30 ng/ml	513.7 $\pm$ 425.8 ng/ml
20 ng/ml	378.7 $\pm$ 316.4 ng/ml
10 ng/ml	20.9 $\pm$ 9.3 ng/ml
5 ng/ml	9.6 $\pm$ 3.7 ng/ml
2 ng/ml	5.0 $\pm$ 1.9 ng/ml
0 ng/ml	< 0.16 ng/ml

Figure 16

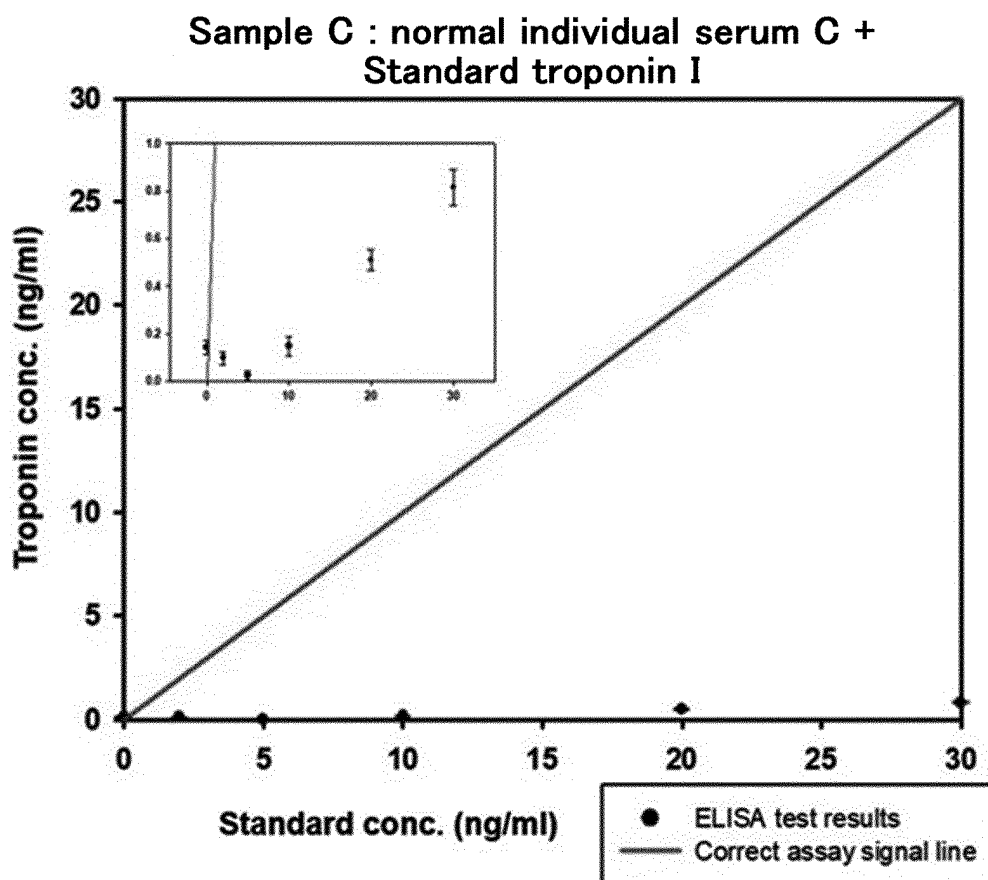
Standard conc.	ECLIA (Mean ± s.d.)
30 ng/ml	496.4 ± 414.9 ng/ml
20 ng/ml	375.0 ± 315.5 ng/ml
10 ng/ml	17.4 ± 9.6 ng/ml
5 ng/ml	9.0 ± 4.9 ng/ml
2 ng/ml	4.1 ± 2.2 ng/ml
0 ng/ml	< 0.16 ng/ml

Figure 17

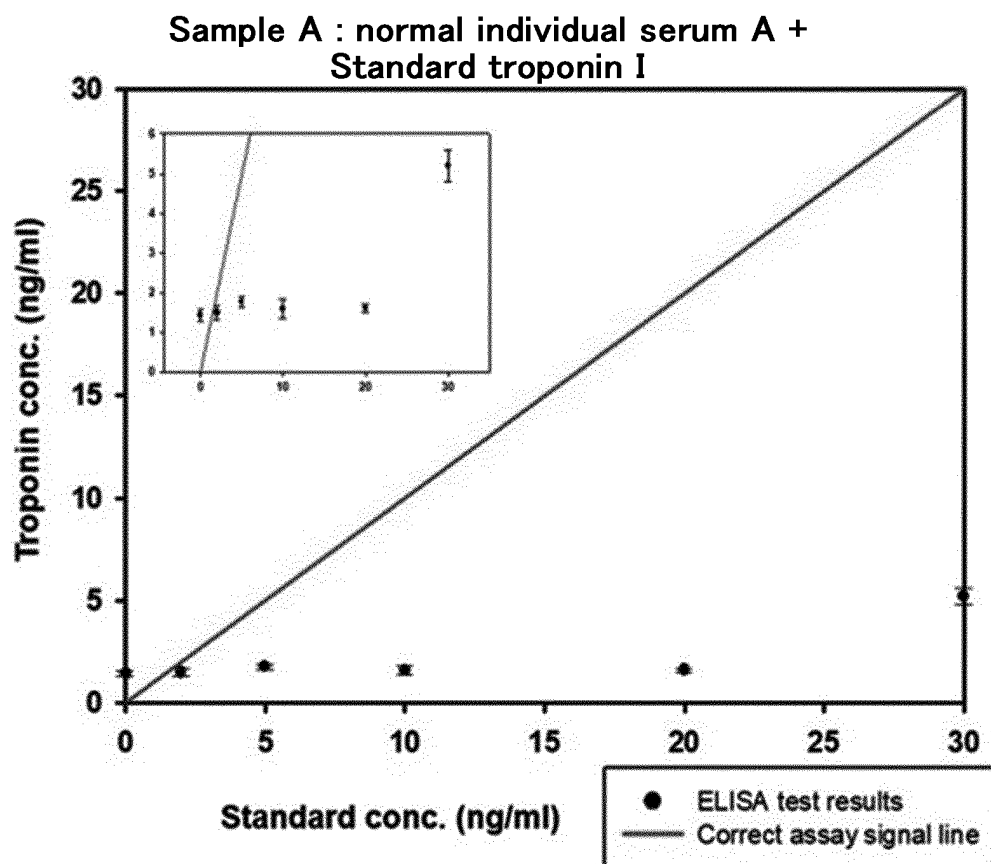
Standard conc.	ELISA (Mean $\pm$ s.d.)
30 ng/ml	0.81 $\pm$ 0.14 ng/ml
20 ng/ml	0.42 $\pm$ 0.02 ng/ml
10 ng/ml	0.30 $\pm$ 0.02 ng/ml
5 ng/ml	0.15 $\pm$ 0.02 ng/ml
2 ng/ml	0.14 $\pm$ 0.01 ng/ml
0 ng/ml	0.09 $\pm$ 0.01 ng/ml

Figure 18

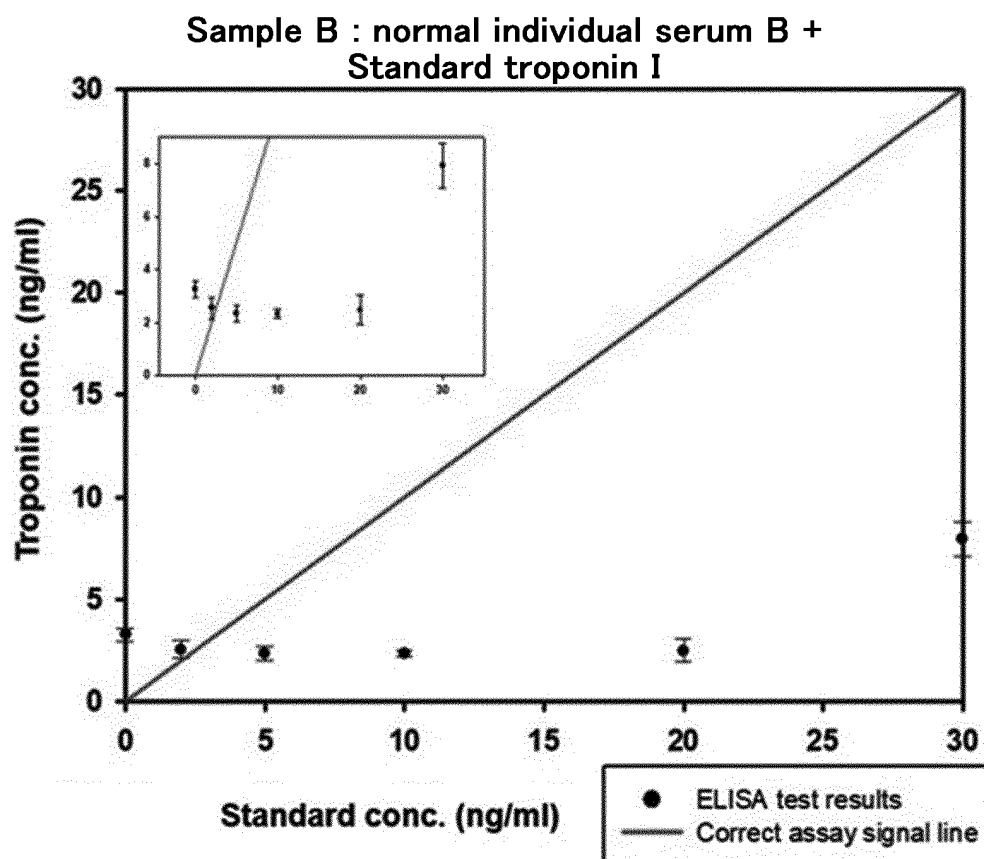
Standard conc.	ELISA (Mean $\pm$ s.d.)
30 ng/ml	1.09 $\pm$ 0.15 ng/ml
20 ng/ml	0.55 $\pm$ 0.04 ng/ml
10 ng/ml	0.15 $\pm$ 0.03 ng/ml
5 ng/ml	0.02 $\pm$ 0.01 ng/ml
2 ng/ml	0.02 $\pm$ 0.02 ng/ml
0 ng/ml	0.03 $\pm$ 0.01 ng/ml

Figure 19

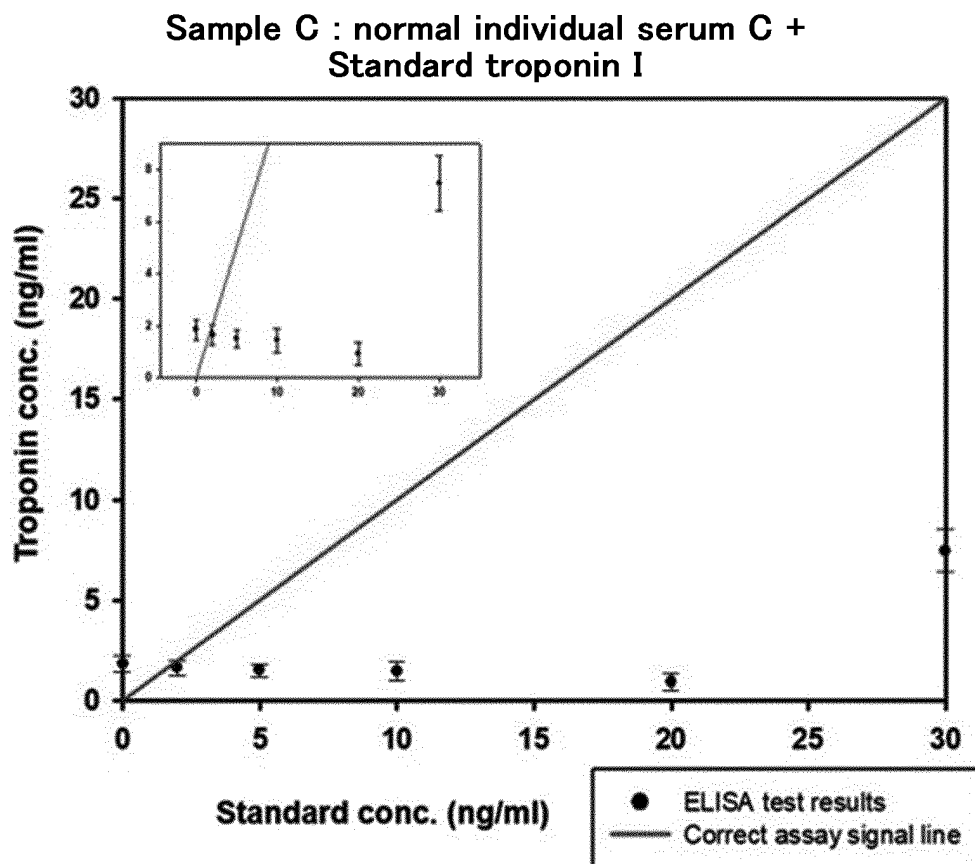
Standard conc.	ELISA (Mean $\pm$ s.d.)
30 ng/ml	0.81 $\pm$ 0.08 ng/ml
20 ng/ml	0.51 $\pm$ 0.04 ng/ml
10 ng/ml	0.15 $\pm$ 0.04 ng/ml
5 ng/ml	0.02 $\pm$ 0.02 ng/ml
2 ng/ml	0.10 $\pm$ 0.03 ng/ml
0 ng/ml	0.14 $\pm$ 0.03 ng/ml

Figure 20

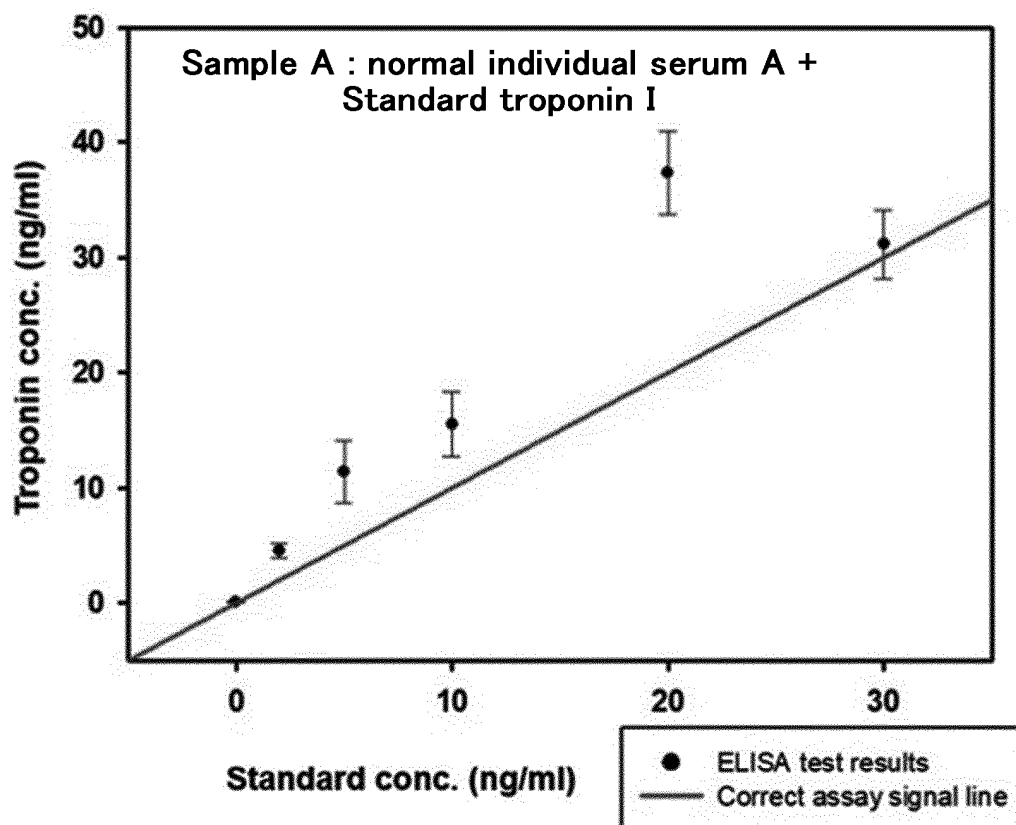
Standard conc.	ELISA (Mean $\pm$ s.d.)
30 ng/ml	5.19 $\pm$ 0.39 ng/ml
20 ng/ml	1.62 $\pm$ 0.09 ng/ml
10 ng/ml	1.59 $\pm$ 0.23 ng/ml
5 ng/ml	1.78 $\pm$ 0.12 ng/ml
2 ng/ml	1.50 $\pm$ 0.19 ng/ml
0 ng/ml	1.43 $\pm$ 0.14 ng/ml

Figure 21

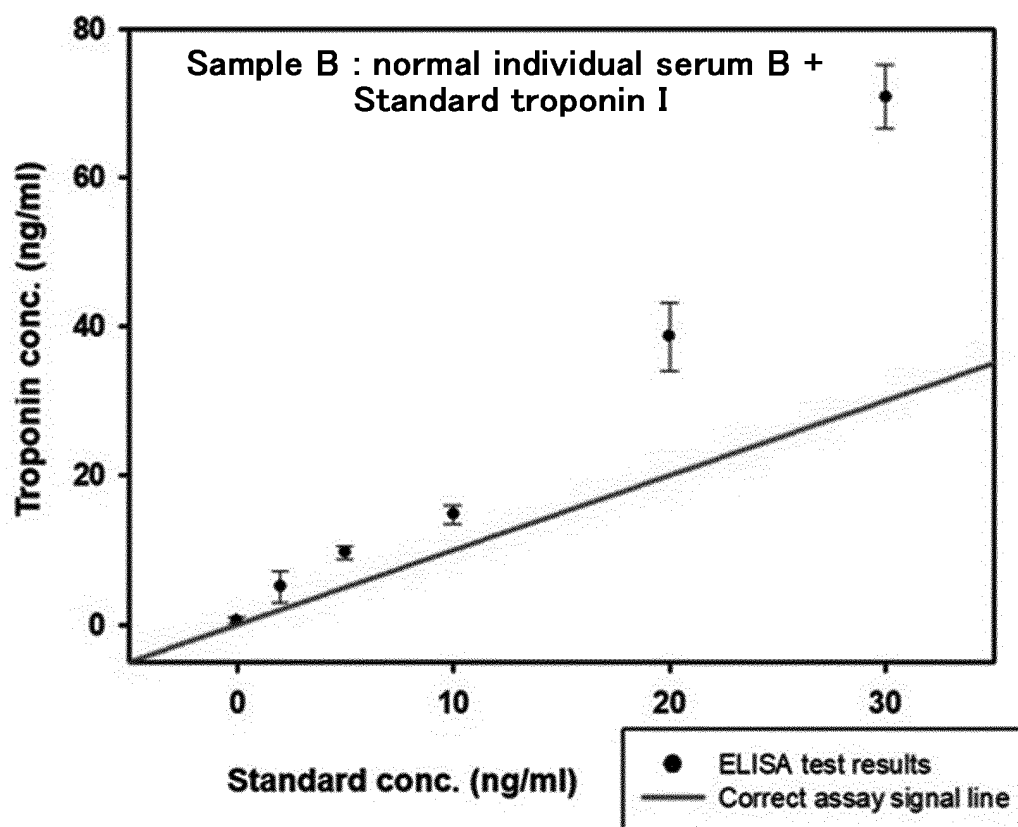
Standard conc.	ELISA (Mean $\pm$ s.d.)
30 ng/ml	7.95 $\pm$ 0.83 ng/ml
20 ng/ml	2.48 $\pm$ 0.55 ng/ml
10 ng/ml	2.33 $\pm$ 0.17 ng/ml
5 ng/ml	2.35 $\pm$ 0.32 ng/ml
2 ng/ml	2.55 $\pm$ 0.42 ng/ml
0 ng/ml	3.26 $\pm$ 0.30 ng/ml

Figure 22

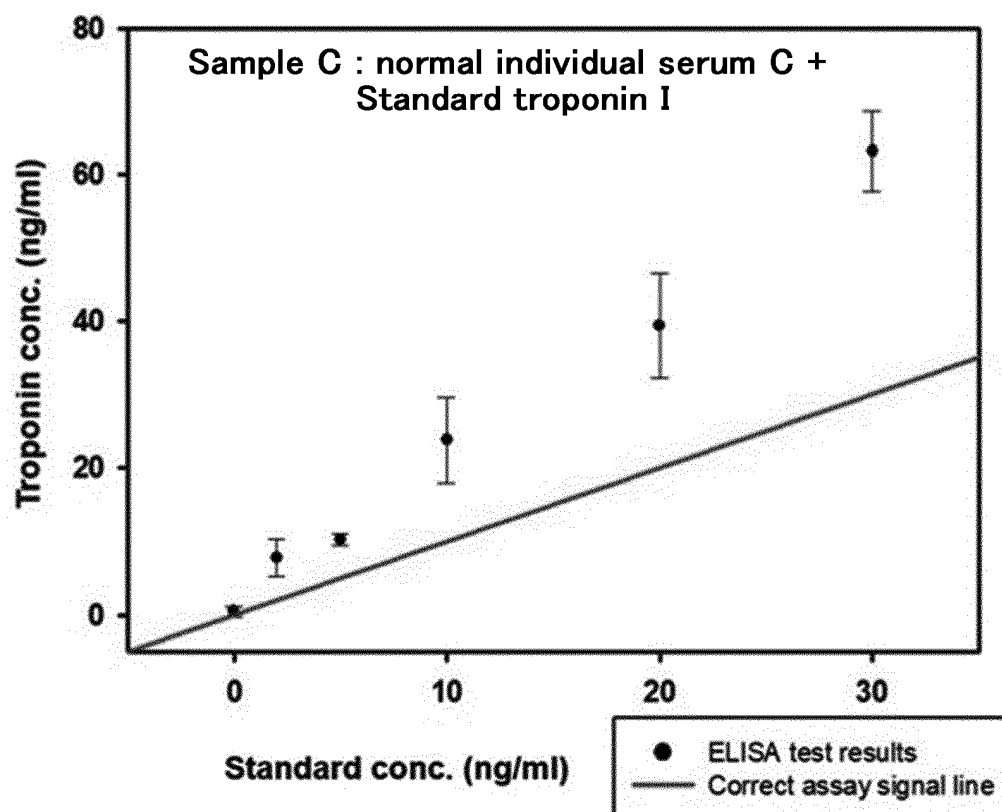
Standard conc.	ELISA (Mean $\pm$ s.d.)
30 ng/ml	7.46 $\pm$ 1.07 ng/ml
20 ng/ml	0.93 $\pm$ 0.44 ng/ml
10 ng/ml	1.45 $\pm$ 0.46 ng/ml
5 ng/ml	1.51 $\pm$ 0.32 ng/ml
2 ng/ml	1.65 $\pm$ 0.37 ng/ml
0 ng/ml	1.86 $\pm$ 0.39 ng/ml

Figure 23

Standard conc.	ELISA (Mean ± s.d.)
30 ng/ml	31.15 ± 2.96 ng/ml
20 ng/ml	37.32 ± 3.57 ng/ml
10 ng/ml	15.53 ± 2.78 ng/ml
5 ng/ml	11.41 ± 2.72 ng/ml
2 ng/ml	4.54 ± 0.61 ng/ml
0 ng/ml	0.06 ± 0.04 ng/ml

Figure 24

Standard conc.	ELISA (Mean ± s.d.)
30 ng/ml	70.81 ± 4.31 ng/ml
20 ng/ml	38.70 ± 4.58 ng/ml
10 ng/ml	14.84 ± 1.25 ng/ml
5 ng/ml	9.70 ± 0.86 ng/ml
2 ng/ml	5.11 ± 2.10 ng/ml
0 ng/ml	0.57 ± 0.51 ng/ml

Figure 25

Standard conc.	ELISA (Mean ± s.d.)
30 ng/ml	63.15 ± 5.51 ng/ml
20 ng/ml	39.36 ± 7.16 ng/ml
10 ng/ml	23.84 ± 5.85 ng/ml
5 ng/ml	10.24 ± 0.84 ng/ml
2 ng/ml	7.77 ± 2.58 ng/ml
0 ng/ml	0.51 ± 0.65 ng/ml

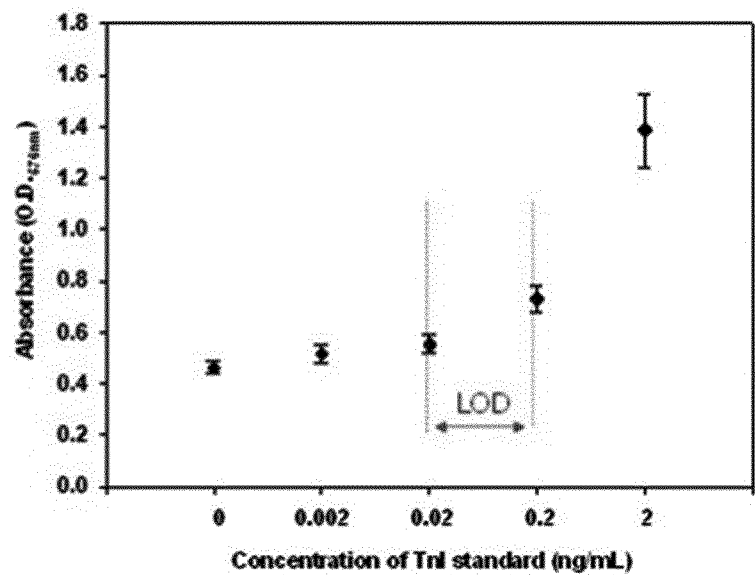
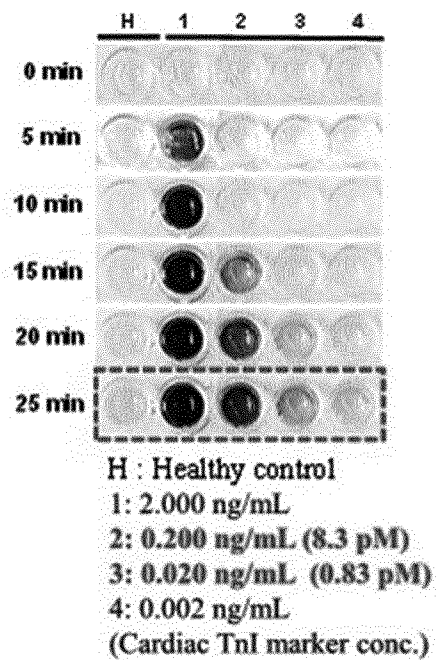
Figure 26

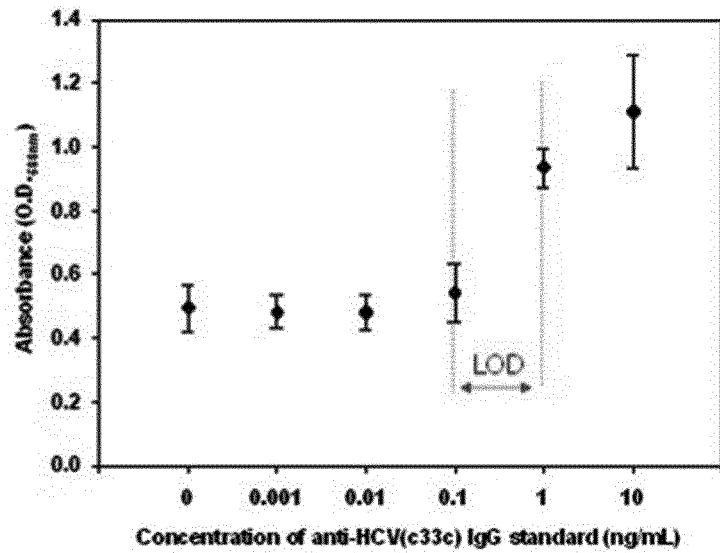
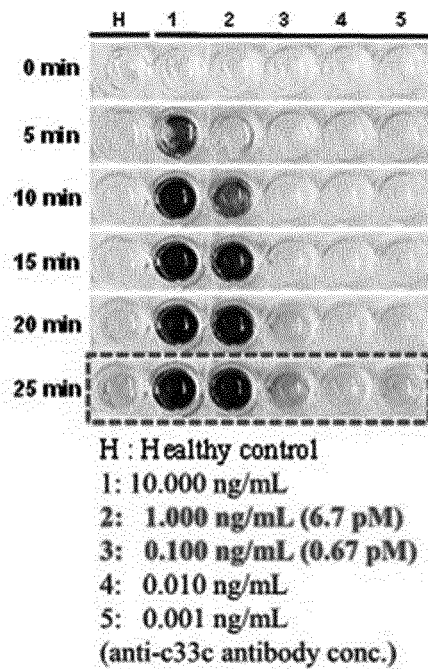
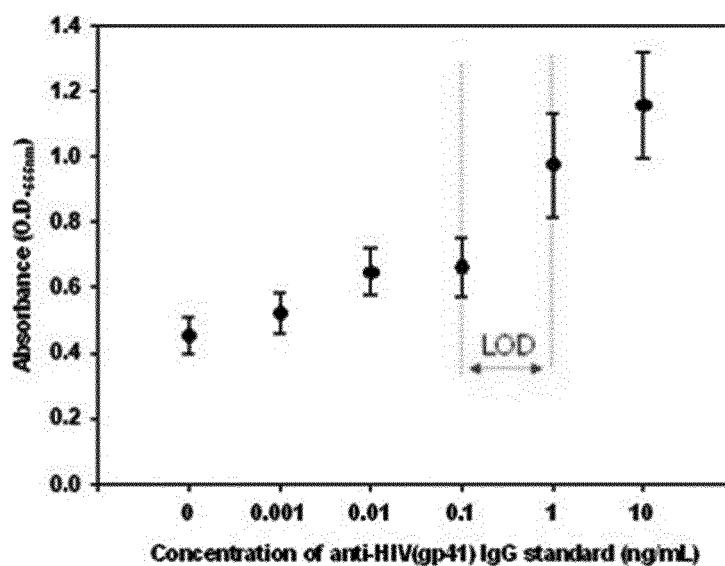
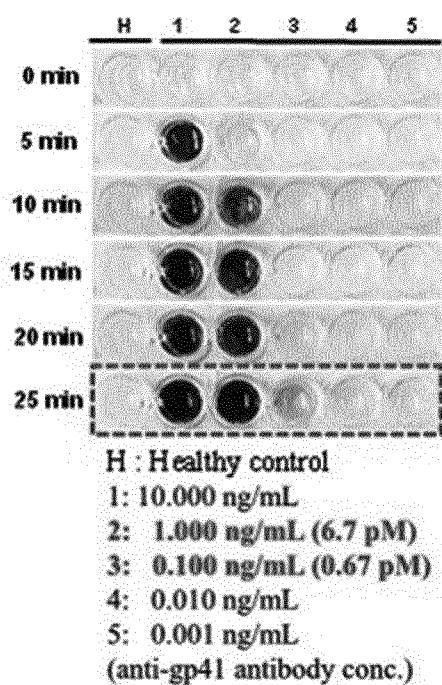
Figure 27

Figure 28

INTERNATIONAL SEARCH REPORT

International application No.

PCT/KR2018/004313

A. CLASSIFICATION OF SUBJECT MATTER

G01N 33/543(2006.01)i, G01N 33/553(2006.01)i, G01N 33/536(2006.01)i, G01N 33/569(2006.01)i, G01N 33/52(2006.01)i

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

G01N 33/543; C12N 15/63; C07K 19/00; B82Y 5/00; G01N 33/483; C12Q 1/26; G01N 33/53; G01N 33/50; G01N 33/553; G01N 33/536; G01N 33/569; G01N 33/52

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean Utility models and applications for Utility models: IPC as above

Japanese Utility models and applications for Utility models: IPC as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS (KIPO internal) & Keywords: gold ion, reduction, gold grain, gold adsorbed peptide, antigen, antibody, detection

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	KR 10-2016-0117688 A (ELECTRONICS AND TELECOMMUNICATIONS RESEARCH INSTITUTE) 11 October 2016 See paragraphs [0005], [0029]-[0036], [0055]-[0063]; claims 1-10; and figures 1a-4.	1-22
Y	KR 10-2010-0128550 A (INFOPIA CO., LTD.) 08 December 2010 See paragraphs [0018], [0019], [0041]; claims 1, 4; figures 1, 2.	1-22
Y	KR 10-2016-0061304 A (KOREA UNIVERSITY RESEARCH AND BUSINESS FOUNDATION) 31 May 2016 See paragraphs [0007], [0033]; and claims 5, 6.	4,13-22
A	KR 10-2011-0090347 A (KOREA UNIVERSITY RESEARCH AND BUSINESS FOUNDATION) 10 August 2011 See the entire document.	1-22
A	JP 2017-037014 A (IKEDA SHOKKEN KK. et al.) 16 February 2017 See the entire document.	1-22

☐ Further documents are listed in the continuation of Box C.
 ☒ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

20 AUGUST 2018 (20.08.2018)

Date of mailing of the international search report

03 SEPTEMBER 2018 (03.09.2018)

Name and mailing address of the ISA/KR


 Korean Intellectual Property Office
 Government Complex Daejeon Building 4, 189, Cheongsu-ro, Seo-gu,
 Daejeon, 35208, Republic of Korea
 Facsimile No. +82-42-481-8578

Authorized officer

Telephone No.

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.

PCT/KR2018/004313

Patent document cited in search report	Publication date	Patent family member	Publication date
KR 10-2016-0117688 A	11/10/2016	NONE	
KR 10-2010-0128550 A	08/12/2010	CN 102449482 A	09/05/2012
		CN 102449482 B	01/04/2015
		EP 2437058 A2	04/04/2012
		EP 2437058 B1	16/08/2017
		US 2012-0070822 A1	22/03/2012
		WO 2010-137807 A2	02/12/2010
		WO 2010-137807 A3	03/03/2011
KR 10-2016-0061304 A	31/05/2016	KR 10-1836921 B1	12/03/2018
		KR 10-2014-0133478 A	19/11/2014
		US 2016-0074511 A1	17/03/2016
		US 2018-0028833 A1	01/02/2018
		US 9814907 B2	14/11/2017
		WO 2014-182136 A1	13/11/2014
KR 10-2011-0090347 A	10/08/2011	NONE	
JP 2017-037014 A	16/02/2017	JP 2017-037015 A	16/02/2017
		WO 2017-026505 A1	16/02/2017

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- KR 101495665 [0014]
- KR 1020140151305 [0014]
- WO 8810649 A [0034]
- WO 88106630 PCT [0034]
- WO 8807085 PCT [0034]
- WO 8807086 PCT [0034]
- WO 8809344 PCT [0034]

Non-patent literature cited in the description

- **IBRAHIM A. DARWISH.** *International Journal of Biomedical Science*, 2006, vol. 2, 217-235 [0005]
- **KARICHMA SHA et al.** *British Journal of Hospital Medicine*, 2016, vol. 77 (7 [0011]
- **MICHAEL VOGESSER et al.** *Ther. Drug Monit.*, 2014, vol. 36 (5), 640-650 [0012]
- **CHOO et al.** *Science*, 1989, vol. 244, 359-362 [0062]
- **STEVEN ROSENBERG.** *J. Mol. Biol.*, 2001, vol. 313, 451-464 [0063]

专利名称(译)	借助检测信号的自我增强原理，一步一步实现精确，快速和实用的疾病诊断程序		
公开(公告)号	EP3611505A1	公开(公告)日	2020-02-19
申请号	EP2018784065	申请日	2018-04-13
[标]发明人	LEE JEEWON KWON JEONG HYEOK		
发明人	LEE, JEEWON KWON, JEONG-HYEOK		
IPC分类号	G01N33/543 G01N33/553 G01N33/536 G01N33/569 G01N33/52		
CPC分类号	G01N33/52 G01N33/536 G01N33/543 G01N33/553 G01N33/569 G01N33/54393 G01N33/56983 G01N33/56988 G01N33/6893		
代理机构(译)	HUTTER, ANTON		
优先权	1020170047841 2017-04-13 KR		
外部链接	Espacenet		

摘要(译)

本发明涉及通过同时链接免疫诊断和Au颗粒形成来准确，快速和方便地检测疾病标志物的方法，并因此实现检测信号的自扩增及其试剂盒，尤其涉及一种使用检测信号的自扩增来检测疾病特异性标志物的方法及其试剂盒，该方法包括 (a) 通过还原Au离子同时诱导抗原抗体免疫反应和Au颗粒形成反应的步骤 在由以下溶液制成的测定溶液中：向存在有助于检测疾病特异性标记物的所有抗体或抗原，游离Au离子和吸附的Au离子的所有预测定溶液中，添加样品，其中包含以下疾病：特异性抗原或与抗体或抗原特异性结合的抗体，以及还原剂； (b) 通过通过Au颗粒形成的显色反应来确认疾病特异性标志物的存在或不存在的步骤。 根据本发明的方法可以在单个步骤中诊断疾病，而无需诸如ELISA之类的现有诊断方法中通常伴随的诸如固定和清洗过程之类的任何过程。 可以将耗时数小时甚至数天的诊断测试时间缩短至约10分钟，从而有效地用于诊断疾病，尤其是紧急情况下的患者； 无需单独的分析仪即可通过肉眼确认，从而将检测成本降至最低。

Figure 1

