



US 20110028341A1

(19) **United States**

(12) **Patent Application Publication**
WANG et al.

(10) **Pub. No.: US 2011/0028341 A1**
(43) **Pub. Date: Feb. 3, 2011**

(54) **METHODS, DEVICES, AND SYSTEMS FOR CHEMILUMINESCENCE-BASED MICROFLUIDIC CELL COUNTING**

(75) Inventors: **Zuankai WANG**, Brooklyn, NY (US); **Sau Yin Chin**, Bronx, NY (US); **Samuel K. Sia**, New York, NY (US)

Correspondence Address:
MILES & STOCKBRIDGE PC
1751 PINNACLE DRIVE, SUITE 500
MCLEAN, VA 22102-3833 (US)

(73) Assignee: **The Trustees of Columbia University in the City of New York**, New York, NY (US)

(21) Appl. No.: **12/860,623**

(22) Filed: **Aug. 20, 2010**

Related U.S. Application Data

(63) Continuation-in-part of application No. 12/594,176, filed as application No. PCT/US08/68869 on Jun. 30, 2008.

(60) Provisional application No. 61/235,634, filed on Aug. 20, 2009, provisional application No. 60/947,345, filed on Jun. 29, 2007, provisional application No. 60/947,384, filed on Jun. 29, 2007.



Publication Classification

(51) **Int. Cl.**
C40B 30/04 (2006.01)
G01N 33/00 (2006.01)
C40B 60/12 (2006.01)
C12M 1/34 (2006.01)
G01N 33/543 (2006.01)
G01N 33/53 (2006.01)

(52) **U.S. Cl.** **506/9**; 422/73; 506/39; 435/287.2; 436/518; 435/7.24

(57) **ABSTRACT**

A chemiluminescence-based detection system and method for counting blood cells by capturing and isolating target blood cells flowing through a microfluidic chip and detecting light emitted by the captured target blood cells.

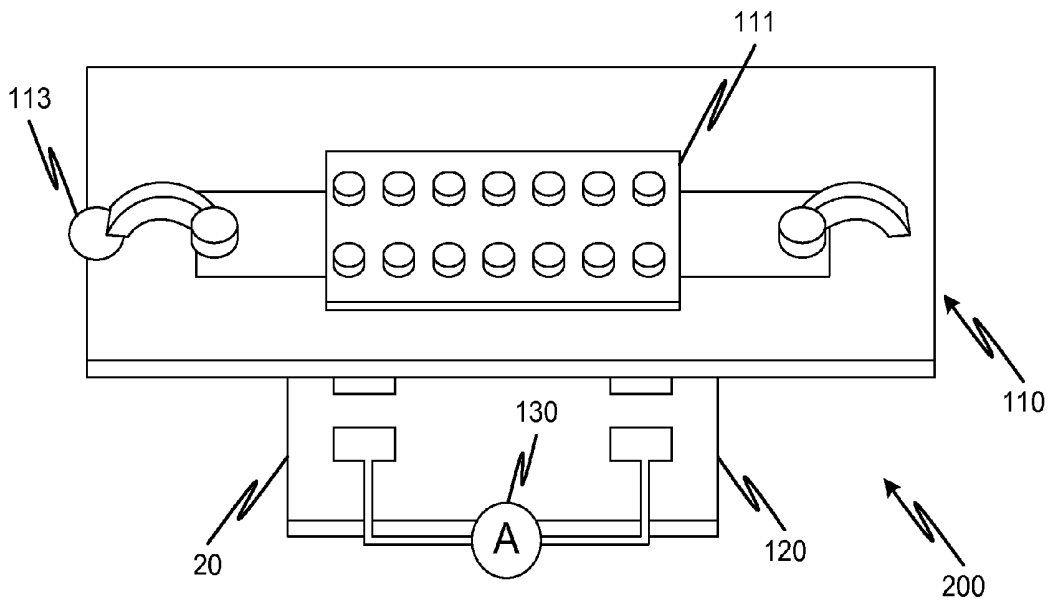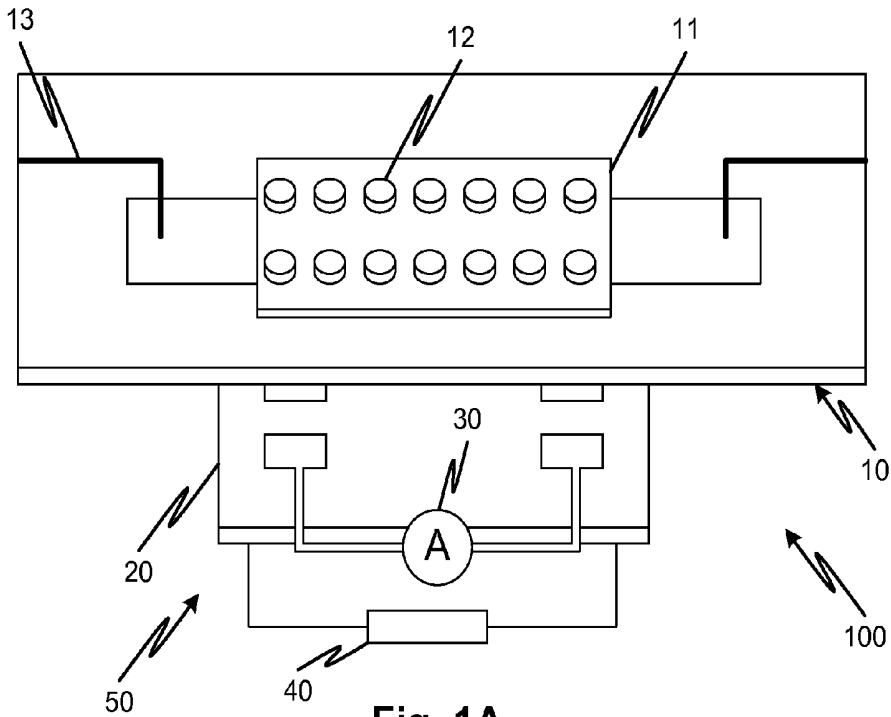

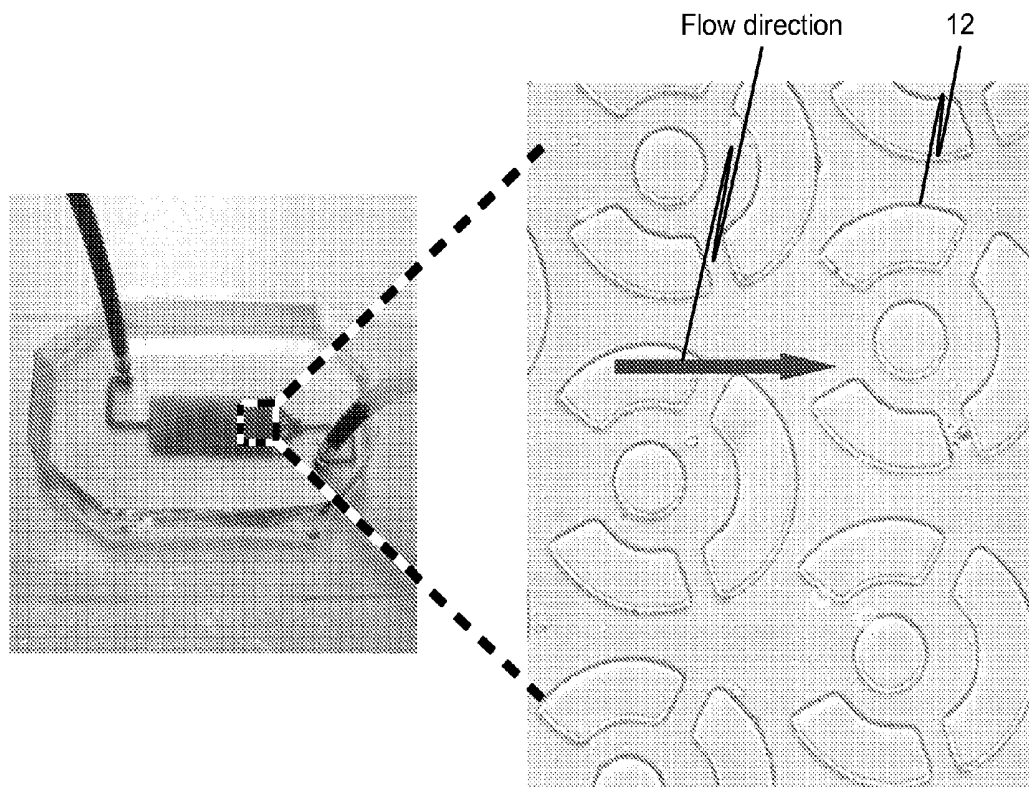


Fig. 1C

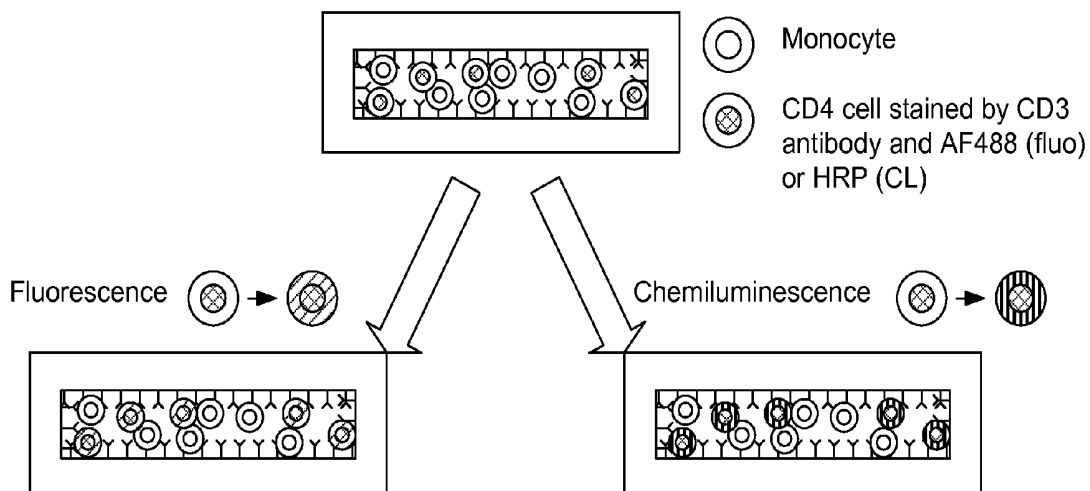


Fig. 2

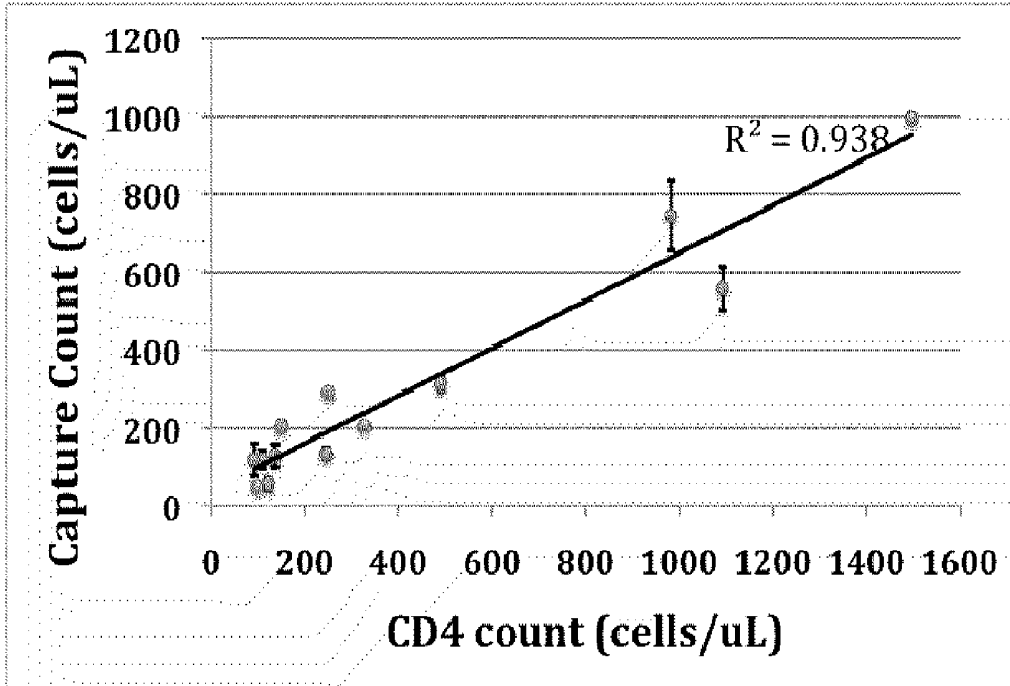


Fig. 3

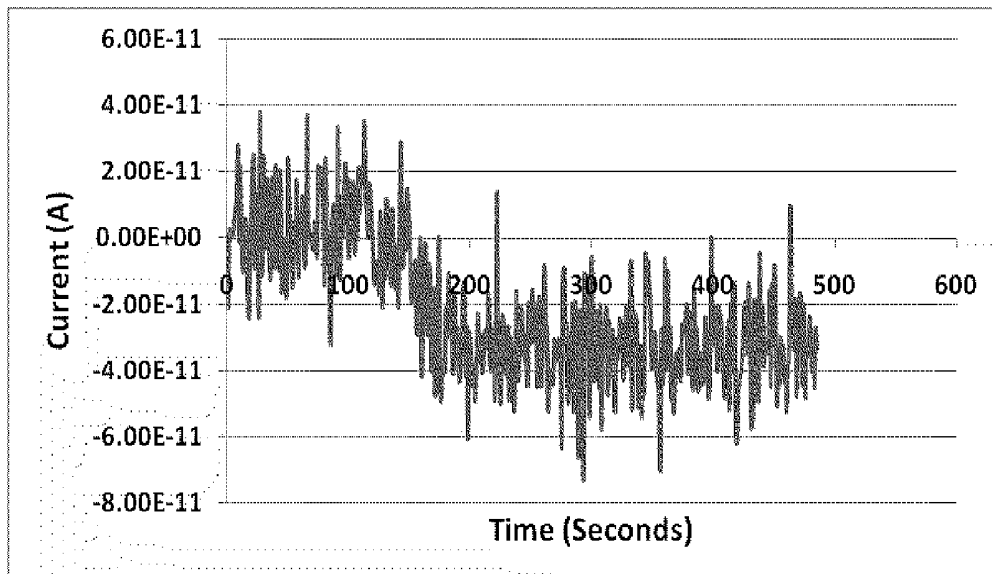


Fig. 4A

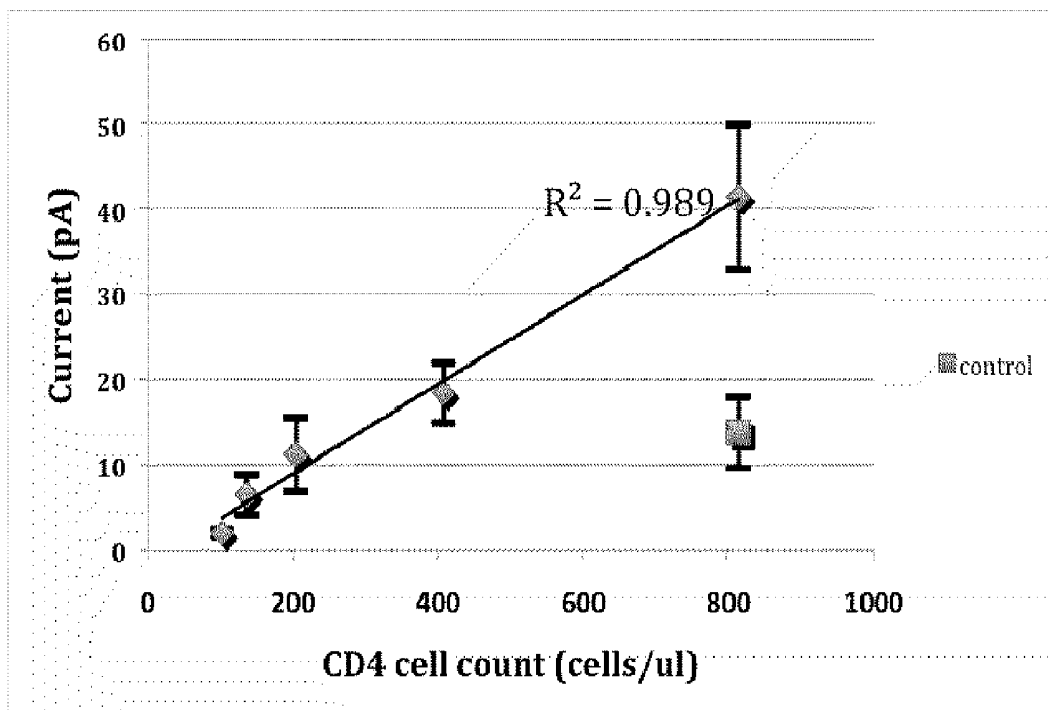


Fig. 4B

METHODS, DEVICES, AND SYSTEMS FOR CHEMILUMINESCENCE-BASED MICROFLUIDIC CELL COUNTING

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Provisional Application 61/235,634, filed on Aug. 20, 2009 and is a continuation-in-part of U.S. patent application Ser. No. 12/594,176, filed Sep. 30, 2009, which is a 371 of International Application No. PCT/US08/068869, filed Jun. 30, 2008, which claims the benefit of U.S. Provisional Application No. 60/947,345, filed Jun. 29, 2007, and U.S. Provisional Application No. 60/947,384, filed Jun. 29, 2007. All of the foregoing applications are hereby incorporated by reference as if set forth in their entireties herein.

BACKGROUND

[0002] Management of the human immunodeficiency virus/acquired immune deficiency syndrome (HIV/AIDS) pandemic is one of the biggest medical and clinical challenges, in both developed and developing countries. Globally, over 40 million people are now living with HIV. In the management of HIV-infected subjects, absolute counts of CD4+ T cells per micro-liter of blood have been proven to be an essential biological indicator for HIV staging and treatment decisions. The immune system needs CD4 cells to function properly. The more CD4 cells in circulation, the stronger the immune system. Clinically, a CD4 count below 200 cells per micro-liter of blood establishes the diagnosis of AIDS.

[0003] Currently, the gold standard for CD4 counting is through flow cytometry. High throughput flow cytometry may not be applicable in resource-poor settings due to its demanding technical requirements and expensive costs. However, availability of portable, cheap CD4 counting using advanced technologies would increase the efficiency and accessibility of CD4 monitoring, and produce a tremendous clinical impact via timely diagnosis of new AIDS patients.

SUMMARY OF THE INVENTION

[0004] The disclosed embodiments include methods, systems, devices, and articles which may provide for particle counting based on chemoluminescence. A useful application of the disclosed technology includes an integrated microfluidic-optical system to enumerate CD4 T-lymphocyte counts for HIV point of care testing at resource-poor settings. Features relating to portability and low power consumption are described.

BRIEF DESCRIPTION OF THE DRAWINGS

[0005] FIG. 1A is a schematic illustration of a target cell counting system according to an embodiment of the invention.

[0006] FIG. 1B is a schematic image of an integrated microfluidic-optical platform according to an embodiment of the invention.

[0007] FIG. 1C is an image of a microfluidic chip filled with blood, and a magnified image of a trapping mechanism according to an embodiment of the invention.

[0008] FIG. 2 is an illustration of a staining mechanism for excluding monocytes according to an embodiment of the invention.

[0009] FIG. 3 is a graph illustrating captured cells versus CD4 counts according to an embodiment of the invention.

[0010] FIG. 4A is a graph illustrating a transient current generated in a chemiluminescence detection process according to an embodiment of the invention.

[0011] FIG. 4B is a graph illustrating a photodetector current reading corresponding to different CD4 counts according to an embodiment of the invention.

DETAILED DESCRIPTION OF THE EMBODIMENTS

[0012] Referring to FIG. 1A, a portable integrated cell counting system 100 has a detecting module 50 positioned adjacent a microfluidic chip 10. The microfluidic chip 10 includes a flow chamber (capture chamber) 11 with a plurality of micro-channels and surface augmentations and/or a plurality of micro-trap arrays 12. The shape, size and position of the plurality of micro-channels and the plurality of micro-trap arrays are such that they collectively act as a trapping mechanism to capture and immobilize target blood cells flowing through the flow chamber 11. The trapped target cells are effectively captured and isolated from the other cells present in the blood sample flowing through the chamber 11. Whole blood, samples, washes, and reagent flowing through the microfluidic chip 10 enter the microfluidic chip through a plurality of tubes 13 and blood entry ports and spent fluids are recovered or disposed through sample exit ports (not shown). A pumping mechanism (not shown) can be employed to transfer the blood and any other samples to and from a sample source and through the microfluidic chip. The pumping mechanism can include a peristaltic pump, for example.

[0013] The detecting module 50 is positioned near the microfluidic chip 10 and adjacent the flow chamber 11 to efficiently detect and convert light emitted by the captured target blood cells. The flow chamber 11 includes a plurality of micro-channels and/or a plurality of arrayed passive hydrodynamic traps 12. The surfaces of the plurality of hydrodynamic traps (micro-traps trap arrays) 12 in the flow chamber 11 are immobilized with CD4+ antibody to allow for effective capture and isolation of CD4+ cells. The capture efficiency is over 80% from 3 μ L of whole blood and the non-specific binding is maintained at a low level ranging from 3% to 15%. The detecting module 50 includes a detector 20 with suitable optics and filtering to detect light emitted by the captured target blood cells, and a source-meter 30 to convert the detected light into an electrical signal. A processor 40, which may be integrated with the detector module 50, converts the electrical signals from the source-meter 30 into a cell count. The portable system 100 can further include a microcontroller (not shown) to control the pumping mechanism, the processor 40, the detecting module 50, as well as to control sample fluid flow through the microfluidic device and to display the target cell count. Inputs from a user may be provided by suitable actuators to allow a user to operate the system 100. A housing can also be provided to form a unitary portable system. When emitted light from the target cells is generated by chemiluminescence, the detector 20 can include a chemiluminescence (CL)-based photodetector amenable to use in the portable integrated system 100.

[0014] FIG. 1B illustrates a chemiluminescence (CL)-based detection system 200 to collect and achieve a digital reading of current (proportional to CD4+ count) using a silicon photodetector 120 and a source-meter 130 in an accurate and rapid manner. Using chemiluminescence detection cir-

cumvents a limitation of the fluorescence based detection which relies on external light sources. The chemiluminescence-based detection also enables the digital reading in a rapid and automatic manner without using complex image processing and has low instrumental requirements. The system **200** includes a microfluidic chip **110** measuring approximately 30 mm×5 mm. Hydrodynamic effects and antibody immobilization can be employed to capture the target cells (cells of interest) flowing through the flow chamber **111**. A hydrodynamic effect can be generated by allowing the hydrodynamic forces to transport target blood cells through the flow chamber **111** and the plurality of micro-channels and micro-trap arrays **112**. Whole blood enters and exits the flow chamber **111** through tubes **113** and is transported through the flow chamber **111** using a pumping mechanism (not shown). The shape and size of the micro-channels and the micro-trap arrays **112** allows for the simultaneous transportation and immobilization of the target cells. To selectively and accurately capture target CD4 cells, CD3 antibody immobilizations and/or surface antibody-antigen interaction can also be implemented for the cell capture. Additionally, to selectively isolate CD4+ cells from the whole blood flowing through, size-based exclusion may also be employed. This approach can effectively determine CD4 absolute counts below 200 cells/ μ L. The technical advantages, such as, the ability to have higher capture efficiency, sensitivity and the ability to offer a digital reading on a rapid and accurate manner make it attractive for point of care diagnostics.

[0015] In FIG. 1C the microfluidic chip **200** is shown filled with whole blood. A magnified image of the flow chamber (capture chamber) **111** with the plurality of micro-trap arrays **112** is also shown in FIG. 1C. The arrow indicates the direction of flow of the blood sample through the plurality of micro-trap arrays. The flow chamber **111** is approximately 10 mm×3.2 mm, and is about 45 μ m tall, and it contains hundreds of micro-trap arrays **112** to significantly increase the surface area for antibody immobilization. Each micro-trap in the array **112** is designed with a pillar surrounded by C-cups with a gap of about 17.5 μ m, for low non-specific binding (as shown in FIG. 1C). This space is larger than 3 μ m, which was reported for effective white blood cell isolation. The distance between each trap can be approximately 25 μ m and a shift of 88 μ m every three rows can be introduced in the array to lead to non-linear streamlines and thereby facilitating cell contact with trap surface.

[0016] Micro-electro-mechanical systems (MEMS) technology and microfluidics may be used to integrate fluidics, mechanics, optics, and electronics on a single chip in a point of care (POC) device. Microfluidic chips maximize cell capture efficiency while minimizing non-specific binding. The microfluidics may be designed to provide flow control with low shear rates which can accommodate cells that are very sensitive to shear stress. The microfluidic chips (**10**, **100**) may be fabricated using any suitable technique, for example, but not limited to, standard soft lithographic techniques. Using standard lithographic techniques, the chip **200** can be molded in Polydimethylsiloxane (PDMS) from a SU-8 master. One layer of 45 μ m thick SU-8 3050 can be spun onto a 3 inch silicon wafer, baked, and exposed under ultraviolet (UV) light to define a negative feature of the microfluidic chip in the resist. The PDMS can be cast on the SU-8 master and baked for 2 hours in an oven having a temperature of 70° C. The PDMS can then be peeled off the mold and holes for fluidic

connection can be punched. After this, PDMS chip can be bonded to glass after plasma treatment for 1 minute.

[0017] The microfluidic chips (**10**, **110**) can be modified for maximum CD4 antibody immobilization using a method in which, after the hydroxyl groups on PDMS surface were generated after plasma treatment, the chip is immediately treated with 4% (v/v) solution of 3-mercaptopropyl trimethoxysilane ethanol for 30 minutes at room temperature so that both the PDMS and glass will be functionalized. After surface silanization, the chip can be incubated with 0.01 μ mol/mL-1 GMBS (N- γ -maleimidobutyryloxysuccinimide) in ethanol for 15 minutes at room temperature. NeutrAvidin can be immobilized to GMBS by incubating the chip surfaces with 10 μ g/mL-1 NeutrAvidin solution in PBS overnight at 4° C. Afterward, 10 μ g/mL biotinylated anti-CD4 solution in PBS and 1% (w/v) BSA can be introduced to the microfluidic chip and incubated at room temperature for 15 minutes. Rinsing steps can be conducted after each step to remove unreacted molecules.

[0018] Monocyte contamination may also be reduced in both systems (**100**, **200**) based on flow control and/or double staining. This could be a significant consideration since the presence of monocytes could artificially contribute to the total CD4+ count.

[0019] FIG. 2 illustrates a staining mechanism for exclusion of monocyte contamination. Although monocytes might be captured on the chip, they will not be detected based on CD3 antibody staining. By coupling the captured cells to CD3 antibody conjugated with fluorophore or horseradish peroxidase (HRP), monocyte contamination exclusion may be achieved. CD3 antibody and a secondary antibody coupled with HRP may be employed to avoid staining monocytes so that monocyte contamination may be eliminated as a concern in the chemiluminescence-based detection system **200**.

[0020] For blood staining, whole blood was incubated with mouse, anti-human CD3 antibodies (Invitrogen) in PBS containing 1% BSA followed by goat, anti-mouse IgG conjugated with fluorophore (AF488). For chemiluminescence (CL) based detection, goat anti-mouse IgG conjugated with HRP was used instead of IgG-AF488. The concentrations of the primary and secondary antibodies and the reaction/incubation times were optimized. Alternatively, the staining step can be done on the chip. While CD4 antigens are expressed by monocytes as well, fluorophore or HRP will not be linked to monocytes, since monocytes are not subsets of a T cell. As a result, monocytes are excluded in the counting process, though some monocyte might be captured in the microfluidic chip, as shown in FIG. 2. Normal whole blood samples could be used in the staining process. Varying CD3+/CD4+ cell counts within the range of values typically encountered in both healthy and immunocompromised individuals could be simulated by diluting blood in a PBS solution with 1% (w/v) BSA using any available and appropriate diluting methods.

[0021] In order to identify optimal flow conditions for the microfluidic chips (**10**, **110**) fluorescence based detection can be conducted prior to cell detection. For this, after rinsing away unbound molecules in the treated microfluidic chip, stained blood is introduced into the chip and be left for incubation on the chip for 15 minutes. A red blood cell-lysis buffer can be flown through the flow chamber at 2 μ L/min for 10 minutes to lyse red blood cells. Subsequently, PBS containing 1% BSA (w/v) is flown through the microfluidic chip at 2 μ L/min for 15 minutes to rinse off unbound cells and quench the lysis buffer. In order to accurately count the CD4 cells (the

particle auto-fluorescence can lead to artificially high CD4 counts), cells can be counted under a microscope at high resolution and the phase-contrast images can be compared to fluorescence images obtained, to confirm the morphology of the cell.

[0022] In order to determine the efficiency of the system (100, 200) an estimation of the capture efficiency of the system (100, 200) can be measured by estimating a ratio of the captured cells in the flow chamber (11, 111) to a cell count based on flow cytometric detection. The net count in the flow chamber can be determined by subtracting non-specific binding from the whole count. The capture efficiency of the system (100, 200) is then estimated based on the ratio of captured CD3+CD4+ cells in the flow chamber to the count obtained via flow cytometry. Flow cytometry data can be collected on a Cyromics FC 500 system, for example, using any known cytometry technique and/or protocol. In a sample experiment, a correlation coefficient (CV) of 0.93 was obtained.

[0023] Because high flow rates will lead to the captured cell shearing off while low flow rates will result in low signals, the flow rate of the system can also be optimized to minimize non-specific binding, so that the capture efficiency becomes about 80% and the non-specific binding ranges from 3% to 15%. A flow rate of about 5 $\mu\text{L}/\text{min}$ was found to minimize non-specific binding. The capture efficiency can be verified based on a control experiment, in which blood samples are introduced into chips without antibody immobilized on their surfaces. In such a sample experiment, it was observed that over 70% CD4+ cells are captured on the trap surfaces. The nonspecific binding of other CD3 T cells can thus be defined as background noise. The net count in the flow chamber can be determined by subtracting background from the whole count.

[0024] In operation, the integrated system (100, 200) is first assembled by closely attaching the microfluidic chip (10, 110), which could be a PDMS microchip, for example, to a photodetector (12, 120), which could be a silicon photodetector with a 1000 ms gate time, for example, for maximum optical collection. The attaching of the microfluidic chip to the photodetector is done following the incubation of blood, lysing and the rinsing steps. Prior to the chemiluminescence-based detection, dark current can also be measured ensuring that the background noise is negligible.

[0025] After the target CD4 blood cells are captured and isolated through a combination of hydrodynamic effects and antibody immobilization in the capture chamber of the microfluidic chip, a mixture of hydrogen peroxide and luminol is injected into the microfluidic chip at a flow rate of about 5 $\mu\text{L}/\text{min}$. In the presence of a catalyst, which is conjugated on the captured CD4 cell surface, the excess energy associated with the reaction between hydrogen peroxide and luminol oxygen is liberated as photons, visible as blue light (i.e., chemiluminescent emission). The emitted blue light can be collected using the silicon photodiode (12, 120) (UV818, for example) and converted to photocurrent using a source-meter (13, 130). A transient signal can be collected over a period of about 5 minutes until a large, stable negative signal is observed (corresponding to the generation of stable light). Since only captured CD3+CD4+ cells are labeled with IgG-HRP, the measured current is proportional to the CD4 cell counts.

[0026] FIG. 3 illustrates a graph of data obtained using the integrated detection/counting systems as described in the embodiments of FIGS. 1A and 1B. The graph shows the

number of captured cells corresponding to the true cell counts of the blood samples introduced into the chip. The correlation coefficient between the assay and standard flow cytometry was found to be 0.938. The coefficient of variation was more than 30% at high cell counts, which might be caused by cell clumping at the high end. However, CD4 Lymphocyte counts to below 200 cells/ μL were measured with acceptable accuracy, indicating that the diagnostic criterion for the separation barrier between HIV and AIDS can be achieved with this approach.

[0027] FIG. 4A illustrates a graph of transient current generated in a chemiluminescent detection system, and the real-time collection of current signal obtained using the integrated systems as described in the embodiments of FIGS. 1A and 1B. A stable negative signal is not developed until after 180 seconds (in the system, positive currents indicate noise). A time-average value can be calculated as a true reading and based on this statistical analysis, a quantitative current signal can be extracted with a detection level of pico-Amperes (pA). Considering that the signal at high count can reach to several hundreds of pA, the system is able to offer a wide detection range, even at very low count, for example, tens of cells. Furthermore, the detection can be finished in several minutes, which is much faster than manual counting of individual cells under a microscope, for example.

[0028] FIG. 4B shows a photodetector reading in response to different CD3+/CD4+ cell counts introduced into a microfluidic chip of a system as described in the embodiments of FIGS. 1A and 1B. FIG. 4B shows a linear relationship between measured photocurrent and cell counts, where a higher current indicates a high cell count. In an exemplary detection operation, the assay had a coefficient of variation (CV) ranging from 18% to 38%. The high CV might have been caused by the variation associated with the experimental process. If current of 25 pA is taken as a cut-off data, the device displays a sensitivity of approximately 100%, a specificity of approximately 100%.

[0029] It is therefore, apparent that there is provided, in accordance with the present disclosure, systems, devices and methods for chemiluminescence-based microfluidic cell counting. In particular, the embodiments include an integrated, portable system that can address accurate CD4 capture, isolation, and exclusion of monocyte contamination, and rapid and automatic counting of CD4+ cells. The embodiments also include further variations including the following embodiments.

[0030] Various embodiments include a cell counter comprising a light-transparent trap incorporating an immobilizer to capture target cells flowing therethrough, and a luminance detector positioned adjacent the light-transparent trap to detect light emitted by target cells immobilized by the trap. The luminance detector generates an electrical signal corresponding to a quantity of light from trapped target cells. The cell counter can further include a processing device to convert the electrical signal to a target cell count. The counter may be provided with a kit having a stain and activator capable of, upon application to target cells, causing light to be generated selectively by the target cells such that when the trapped target cells so stained are in the trap, the luminance detector generates a signal.

[0031] Various embodiments include a portable system for counting particles in a sample fluid. The system comprises a flow chamber including a trapping mechanism configured to capture and isolate target particles flowing therethrough, the

trapping mechanism employing a hydrodynamic effect and an antibody immobilizer to capture and isolate the target particles, and a detecting device positioned adjacent the flow chamber and configured to detect light emitted by the trapped target particles. The detecting device is configured to generate a signal based on the detected light. The portable system further includes a processing device configured to convert said signal to a target particle count. The trapping mechanism can include a plurality of microfluidic channels with surface augmentations or a plurality of micro-trap arrays to generate said hydrodynamic effect. The system can further comprise a staining mechanism configured to stain the trapped target particles with incubated blood and an activating mechanism configured to apply an activator on the trapped target particles to generate emission of light from the trapped particles. The activating mechanism can activate fluorescence and/or chemiluminescence emission of light by the trapped target particles.

[0032] Various embodiments include an integrated blood cell counter comprising a microfluidic platform including a light-transparent trap incorporating an immobilizer to capture target blood cells flowing therethrough and a detecting system positioned adjacent said microfluidic platform to detect chemiluminescent light emitted by the captured target blood cells, and to output a blood cell count based on the detected light. The target blood cells can include CD4 blood cells. The light transparent trap can include a plurality of micro-channels with surface augmentations and the immobilizer can include an antibody or a surface antibody-antigen interaction.

[0033] Various embodiments include a chemiluminescence (CL) based detection method for counting blood cells, the method comprising capturing target blood cells flowing through an integrated microfluidic chip, the microfluidic chip including a plurality of micro-channels and an immobilizer to trap and isolate the target blood cells, generating chemiluminescence light emission from the captured target blood cells, detecting light emitted by the captured target blood cells, generating an electrical signal based on a quantity of light detected, and converting the electrical signal to a blood cell count.

[0034] Various embodiments include a method of counting particles in a sample fluid, the method comprising the step of capturing target particles flowing through a microfluidic platform, activating light emission by the captured target particles, detecting light emitted by the captured target particles, and converting a quantity of light detected to a particle count. The capturing of the target particles can employ a hydrodynamic effect and an antibody immobilization. The hydrodynamic effect can be achieved using a plurality of micro-trap arrays incorporated in the microfluidic platform.

[0035] In various embodiments the sample fluid includes blood and the target particles include CD4 blood cells. The counting method can further include staining the captured target particles before detecting the emitted light, and activating light emission by applying an activator on the captured target particles to activate one of a fluorescence emission and a chemiluminescence emission.

[0036] In various embodiments the activator includes hydrogen peroxide and luminol. In some embodiments the staining includes staining the captured target particles with incubated blood when the captured particles include CD4 blood cells.

[0037] Various embodiments include a method corresponding to the use of the above described devices and sys-

tems for counting CD4 cells. The trap may be a microfluidic channel having surface augmentation. The immobilization may be provided using antibodies. Captured cells may be coupled to CD3 antibody conjugated with either fluorophore or horseradish peroxidase (HRP). The luminance detector may include a silicon photodetector. The staining may be done by taking a sample of whole blood incubated with mouse, anti-human CD3 antibodies (Invitrogen) in PBS containing 1% BSA followed by goat, anti-mouse IgG conjugated with goat anti-mouse IgG conjugated with HRP. The staining step may be done on cells trapped in the trap.

[0038] Additional embodiments of traps, mechanisms for supplying fluid in a portable device, portable power sources, display elements and other embodiments that can be incorporated in chemiluminescent-based devices, methods, and system are described in U.S. patent application Ser. No. 12/594,176, filed Sep. 30, 2009, which is hereby incorporated by reference as if set forth in its entirety herein. For example, the incorporated application describes devices and methods for storing and delivering assay agents, pumps, control circuits, and other aspects that can readily be seen as applicable, in view of the present disclosure, to realize alternative and more detailed embodiments of a chemiluminescent-based device, systems, and methods.

[0039] Many alternatives, modifications, and variations are enabled by the present disclosure. Features of the disclosed embodiments can be combined, rearranged, omitted, etc. within the scope of the invention to produce additional embodiments.

[0040] Furthermore, certain features of the disclosed embodiments may sometimes be used to advantage without a corresponding use of other features. Accordingly, Applicant intends to embrace all such alternatives, modifications, equivalents, and variations that are within the spirit and scope of the present disclosure.

What is claimed is:

1. A portable system for counting particles in a sample fluid, comprising:

a flow chamber including a trapping mechanism configured to capture and isolate target particles flowing therethrough, the trapping mechanism employing a hydrodynamic effect and an antibody immobilizer to capture and isolate the target particles;

a detecting device positioned adjacent said flow chamber and configured to detect light emitted by said trapped target particles, the detecting device generating a signal based on the detected light; and

a processing device configured to convert said signal to a target particle count.

2. The system of claim 1, wherein the trapping mechanism includes a plurality of microfluidic channels with surface augmentations to generate said hydrodynamic effect or a plurality of micro-trap arrays to generate said hydrodynamic effect.

3. The system of claim 1, wherein the sample fluid includes blood and the target particles include blood cells and the antibody immobilizer includes a CD4+ antibody or the antibody immobilizer includes a surface antibody-antigen interaction.

4. The system of claim 1, further comprising a flow controller configured to control a flow rate of trapped target particles through the flow chamber at a predefined rate.

5. The system of claim 1, wherein the sample fluid includes blood and the target particles include CD4 blood cells and

wherein the CD4 blood cells are coupled to CD3 antibody conjugated with one of a fluorophore and horseradish peroxidase (HRP) to effectively control monocyte contamination or the CD4 blood cells are coupled to CD3 antibody and a secondary antibody conjugated with horseradish peroxidase (HRP) to effectively control monocyte contamination.

6. The system of claim 5, further comprising an activating mechanism configured to apply an activator on the trapped CD4 blood cells to generate emission of light from the trapped CD4 blood cells, wherein the activator includes hydrogen peroxide and luminol and wherein the blood is incubated with mouse, anti-human CD3 antibodies in PBS containing 1% BSA followed by goat, anti-mouse IgG conjugated with fluorophore to generate fluorescent light emission and wherein the blood is incubated with mouse, anti-human CD3 antibodies in PBS containing 1% BSA followed by goat, anti-mouse IgG conjugated with horseradish peroxidase (HRP) to generate chemiluminescent light emission.

7. The system of claim 1, wherein the detecting device includes a photodetector to detect chemiluminescent light emitted by the target cells and the flow chamber further comprises sample fluid entry and exit ports and tubes, the system further comprising a pump connected to establish sample fluid flow through the tubes and the sample flow chamber.

8. An integrated blood cell counter comprising:

a microfluidic platform including a light-transparent trap incorporating an immobilizer to capture target blood cells flowing therethrough; and

a detecting system positioned adjacent said microfluidic platform to detect light emitted by the captured target blood cells, the detecting system including an enclosure to block out all light and to output a blood cell count based on the detected light so as to be capable of detecting the auto-emission of light;

the detecting system including a photodetector configured to generate an electrical signal based on the detected light, and a processing device configured to convert said electrical signal to a blood cell count.

9. The counter of claim 8, wherein the target blood cells include CD4 blood cells.

10. The counter of claim 8, wherein the light transparent trap includes a plurality of micro-channels with surface augmentations and the immobilizer includes an antibody or the immobilizer includes a surface antibody-antigen interaction.

11. The counter of claim 9, further comprising a stain and activator device to stain the captured CD4 blood cells with incubated blood and to apply an activator on the trapped CD4 blood cells to generate emission of light from the captured CD4 blood cells, wherein the activator includes hydrogen peroxide and luminol.

12. The counter of claim 8, further comprising a flow controller to control a flow rate of the target blood cells through the microfluidic platform, wherein controlling the flow rate effectively controls monocyte contamination.

13. A method of counting particles in a sample fluid, the method comprising:

capturing target particles flowing through a microfluidic device, the microfluidic device including a plurality of micro-channels and an immobilizer to trap and isolate the target blood cells;

activating chemiluminescent light emission by the captured target particles and simultaneously blocking any sources of illumination from illuminating the target particles;

detecting light emitted by the captured target particles; and converting a quantity of light detected to a particle count.

14. The method of claim 13, wherein the capturing of the target particles employs a hydrodynamic effect and an antibody immobilization, wherein the hydrodynamic effect is achieved using a plurality of micro-trap arrays incorporated in the microfluidic platform and wherein the antibody immobilization further includes a surface antibody-antigen interaction.

15. The method of claim 13, wherein the sample fluid includes blood and the target particles include CD4 blood cells.

16. The method of claim 13, further comprising staining the captured target particles before detecting the emitted light.

17. The method of claim 16, wherein activating light emission includes applying an activator on the captured target particles to activate one of a fluorescence emission and a chemiluminescence emission.

18. The method of claim 17, wherein the activator includes hydrogen peroxide and luminol.

19. The method of claim 18, wherein staining includes staining the captured target particles with incubated blood when the captured particles include CD4 blood cells and wherein when blood is incubated with mouse, anti-human CD3 antibodies in PBS containing 1% BSA followed by goat, anti-mouse IgG conjugated with fluorophore, fluorescent light emission is generated, and when blood is incubated with mouse, anti-human CD3 antibodies in PBS containing 1% BSA followed by goat, anti-mouse IgG conjugated with horseradish peroxidase (HRP), chemiluminescent light emission is generated.

20. The method of claim 30, further comprising regulating monocyte contamination by one of controlling flow rate of the target cells through the microfluidic platform and double staining.

* * * * *

专利名称(译)	用于基于化学发光的微流体细胞计数的方法，装置和系统		
公开(公告)号	US20110028341A1	公开(公告)日	2011-02-03
申请号	US12/860623	申请日	2010-08-20
[标]申请(专利权)人(译)	纽约市哥伦比亚大学理事会		
申请(专利权)人(译)	哥伦比亚大学纽约市受托人		
当前申请(专利权)人(译)	哥伦比亚大学纽约市受托人		
[标]发明人	WANG ZUANKAI CHIN SAU YIN SIA SAMUEL K		
发明人	WANG, ZUANKAI CHIN, SAU YIN SIA, SAMUEL K.		
IPC分类号	C40B30/04 G01N33/00 C40B60/12 C12M1/34 G01N33/543 G01N33/53		
CPC分类号	G01N15/147 G01N15/1484 G01N33/54366 G01N2015/008 G01N2015/1486 Y10T436/2575 G01N2333/70514 B01L3/502761 B01L3/502746 B01L3/502707 G01N2333/7051		
优先权	61/235634 2009-08-20 US 60/947345 2007-06-29 US 60/947384 2007-06-29 US PCT/US2008/068869 2008-06-30 WO		
其他公开文献	US8921121		
外部链接	Espacenet USPTO		

摘要(译)

一种基于化学发光的检测系统和方法，用于通过捕获和分离流过微流体芯片的目标血细胞并检测由捕获的目标血细胞发射的光来计数血细胞。

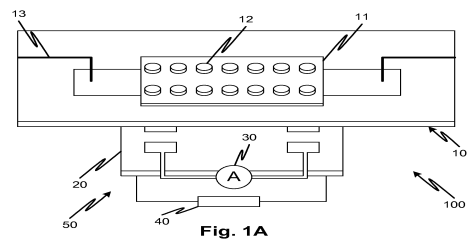


Fig. 1A

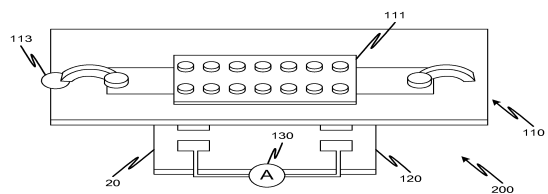


Fig. 1B