



(19) **United States**

(12) **Patent Application Publication**
Larson et al.

(10) **Pub. No.: US 2011/0053139 A1**
(43) **Pub. Date: Mar. 3, 2011**

(54) **DETECTION OF BIOAGENTS USING A SHEAR HORIZONTAL SURFACE ACOUSTIC WAVE BIOSENSOR**

(52) **U.S. Cl. 435/5; 422/69; 436/501; 435/7.2; 435/287.2**

(57) **ABSTRACT**

(76) Inventors: **Richard S. Larson**, Albuquerque, NM (US); **Brian Hjelle**, Placitas, NM (US); **Pam R. Hall**, Albuquerque, NM (US); **David C. Brown**, Albuquerque, NM (US); **Marco Bisoffi**, Albuquerque, NM (US); **Susan M. Brozik**, Albuquerque, NM (US); **Darren W. Branch**, Albuquerque, NM (US); **Thayne L. Edwards**, Albuquerque, NM (US); **David Wheeler**, Albuquerque, NM (US)

Viruses and other bioagents are of high medical and biodefense concern and their detection at concentrations well below the threshold necessary to cause health hazards continues to be a challenge with respect to sensitivity, specificity, and selectivity. Ideally, assays for accurate and real time detection of viral agents and other bioagents would not necessitate any pre-processing of the analyte, which would make them applicable for example to bodily fluids (blood, sputum) and man-made as well as naturally occurring bodies of water (pools, rivers). We describe herein a robust biosensor that combines the sensitivity of surface acoustic waves (SAW) generated at a frequency of 325 MHz with the specificity provided by antibodies and other ligands for the detection of viral agents. In preferred embodiments, a lithium tantalate based SAW transducer with silicon dioxide waveguide sensor platform featuring three test and one reference delay lines was used to adsorb antibodies directed against Coxsackie virus B4 or the negative-stranded category A bioagent Sin Nombre virus (SNV), a member of the genus Hantavirus, family Bunyaviridae, negative-stranded RNA viruses. Rapid detection (within seconds) of increasing concentrations of viral particles was linear over a range of order of magnitude for both viruses, although the sensor was approximately 50×10^4 -fold more sensitive for the detection of SNV. For both pathogens, the sensor's selectivity for its target was not compromised by the presence of confounding Herpes Simplex virus type 1. The biosensor was able to detect SNV at doses lower than the load of virus typically found in a human patient suffering from hantavirus cardiopulmonary syndrome (HCPS). Further, in a proof-of-principle real world application, the SAW biosensor was capable of selectively detecting SNV agents in complex solutions, such as naturally occurring bodies of water (river, sewage effluent) without analyte pre-processing.

(21) Appl. No.: **12/069,284**


(22) Filed: **Feb. 8, 2008**

Related U.S. Application Data

(60) Provisional application No. 60/900,416, filed on Feb. 9, 2007, provisional application No. 60/926,827, filed on Apr. 30, 2007, provisional application No. 61/009,656, filed on Dec. 31, 2007.

Publication Classification

(51) **Int. Cl.**
C12Q 1/70 (2006.01)
G01N 33/53 (2006.01)
C12M 1/34 (2006.01)

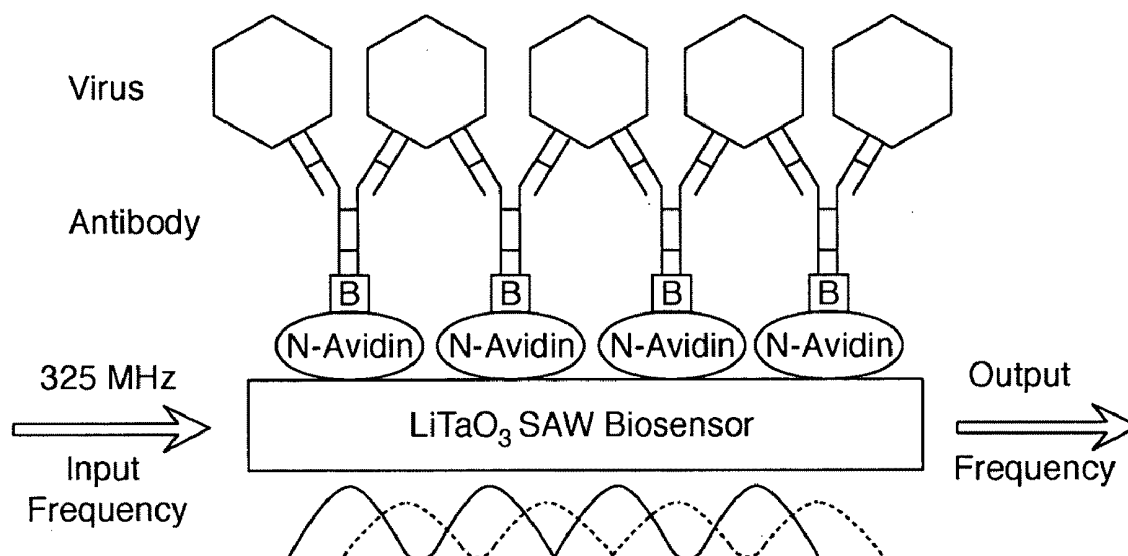

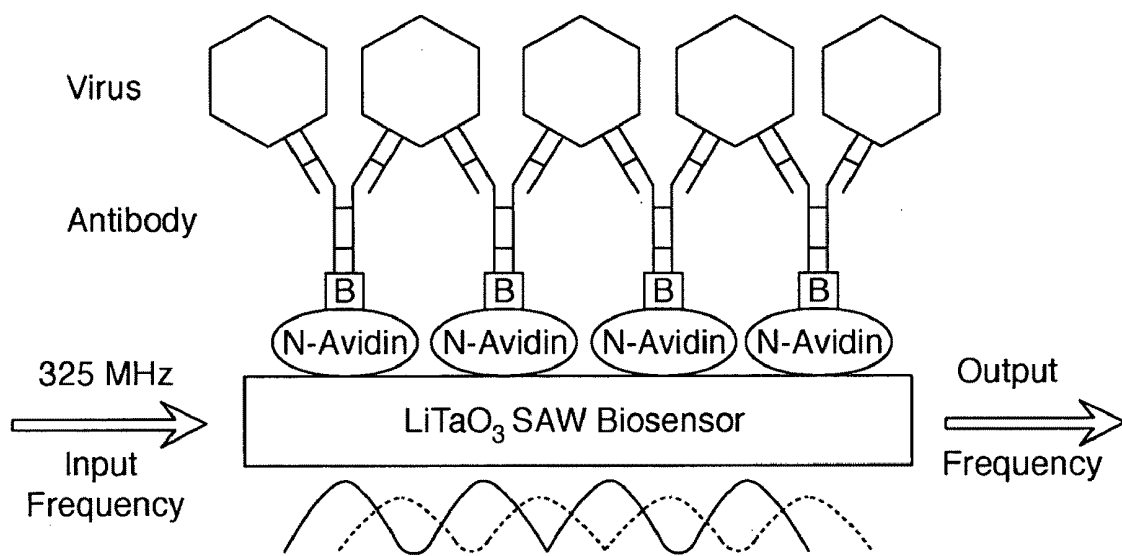


FIG. 1A

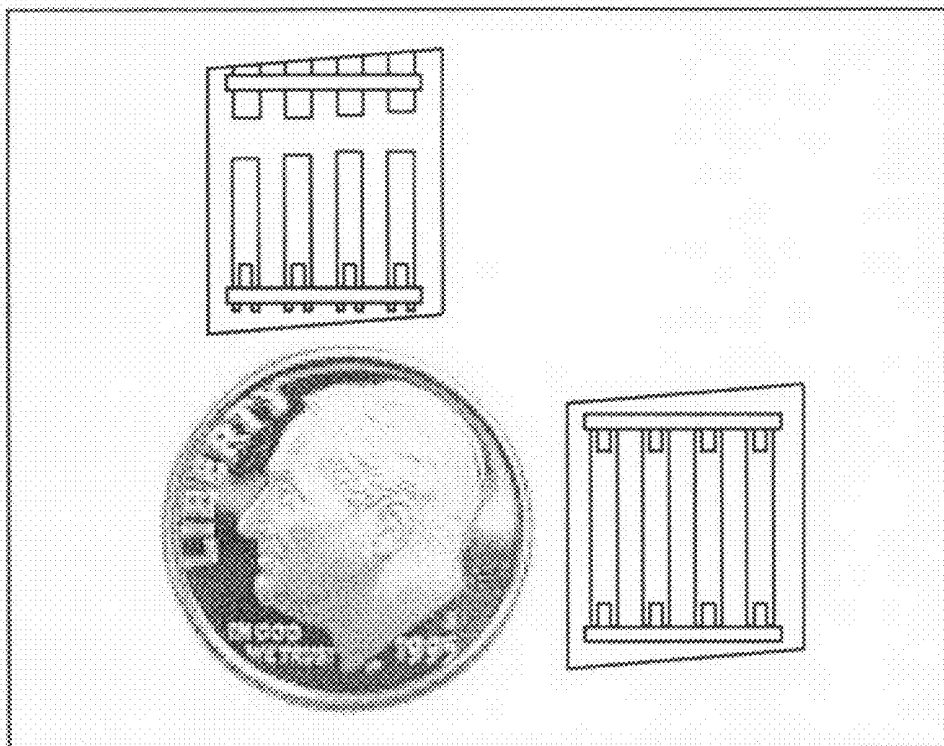


FIG. 1B

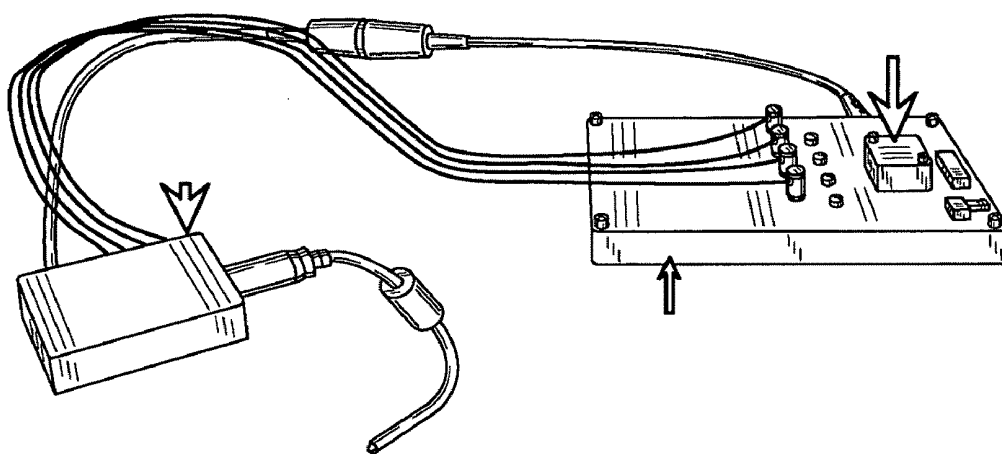


FIG. 1C

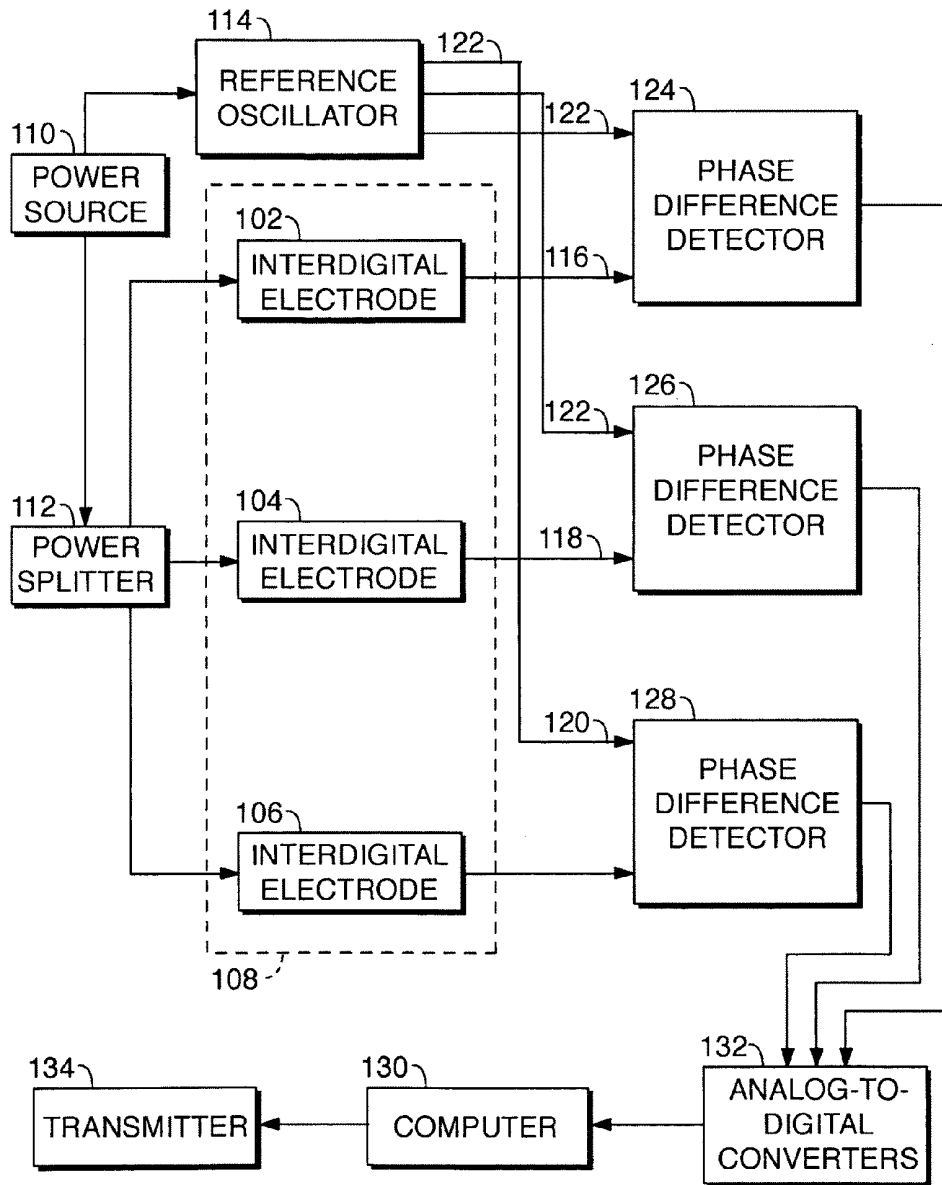


FIG. 1D

Figure 2

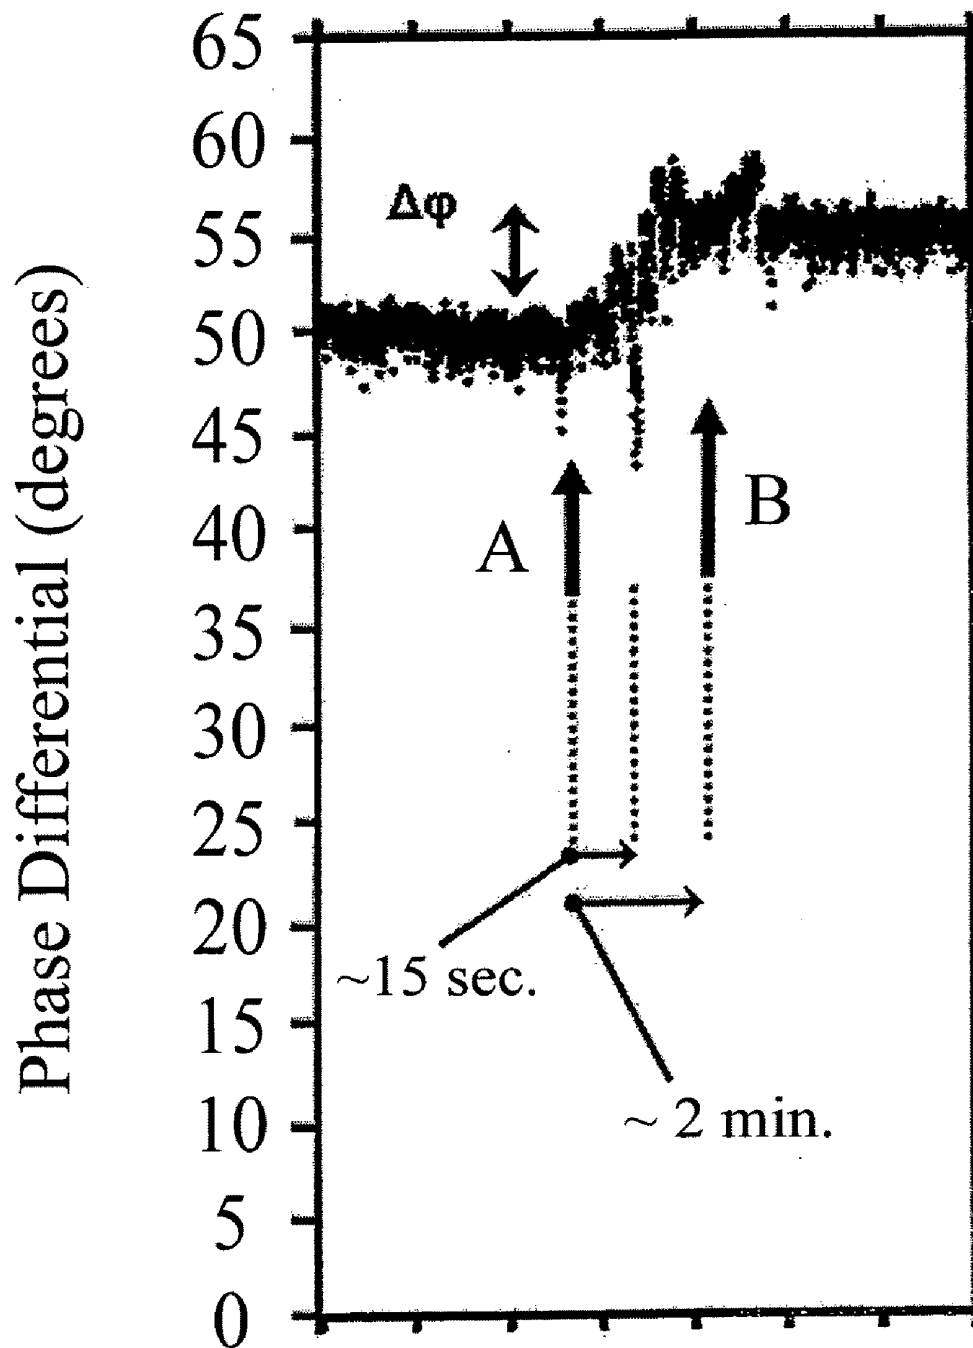


FIGURE 3


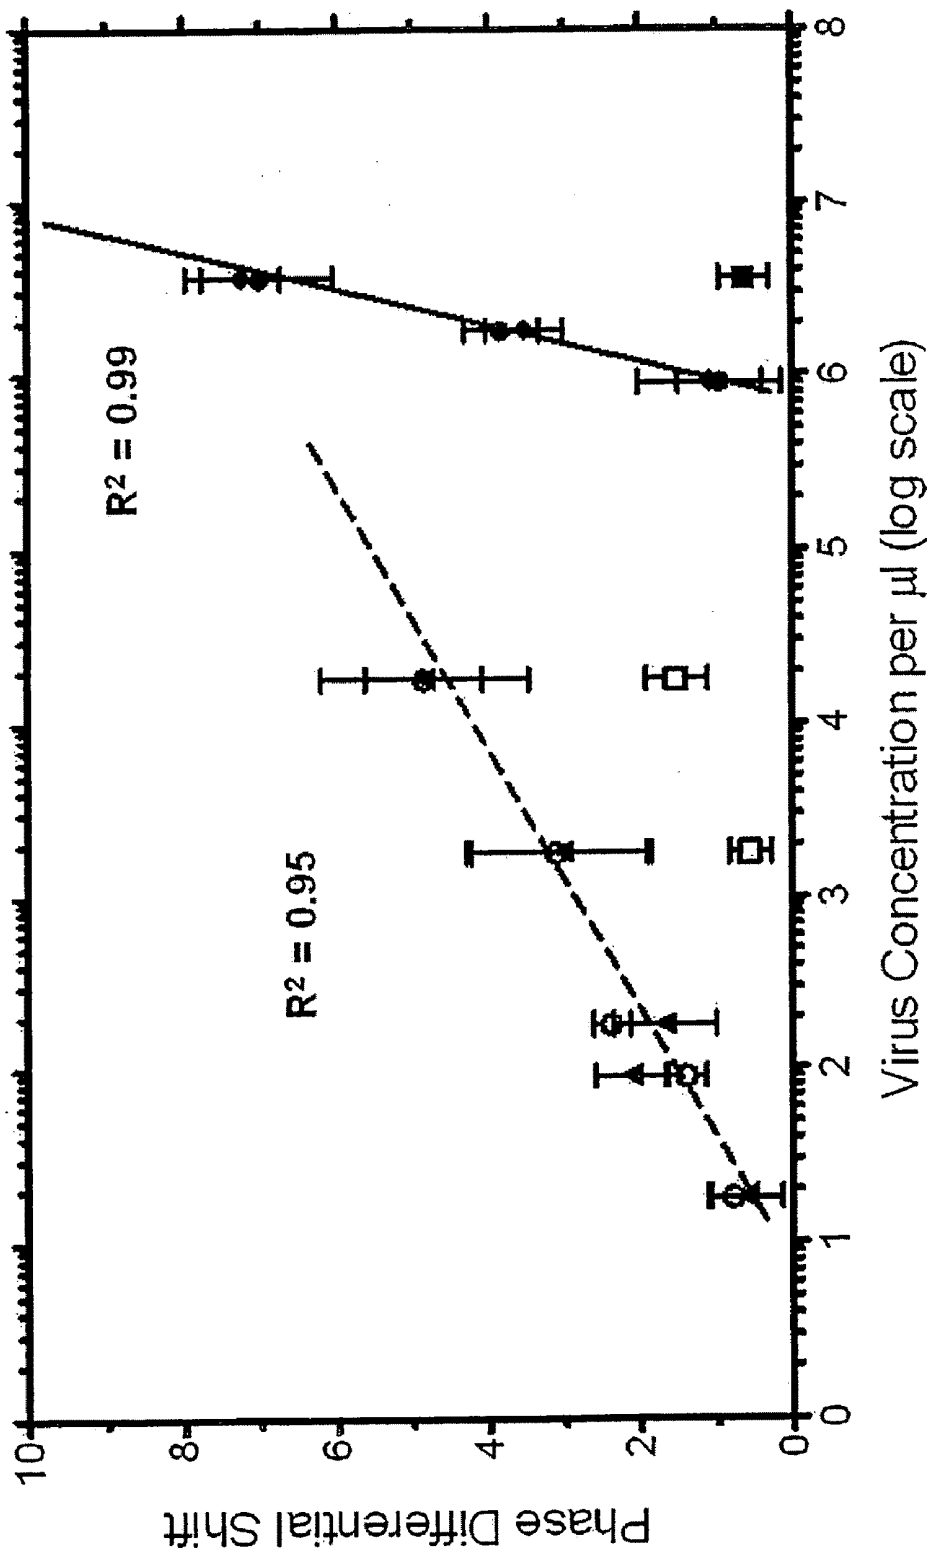


Figure 4

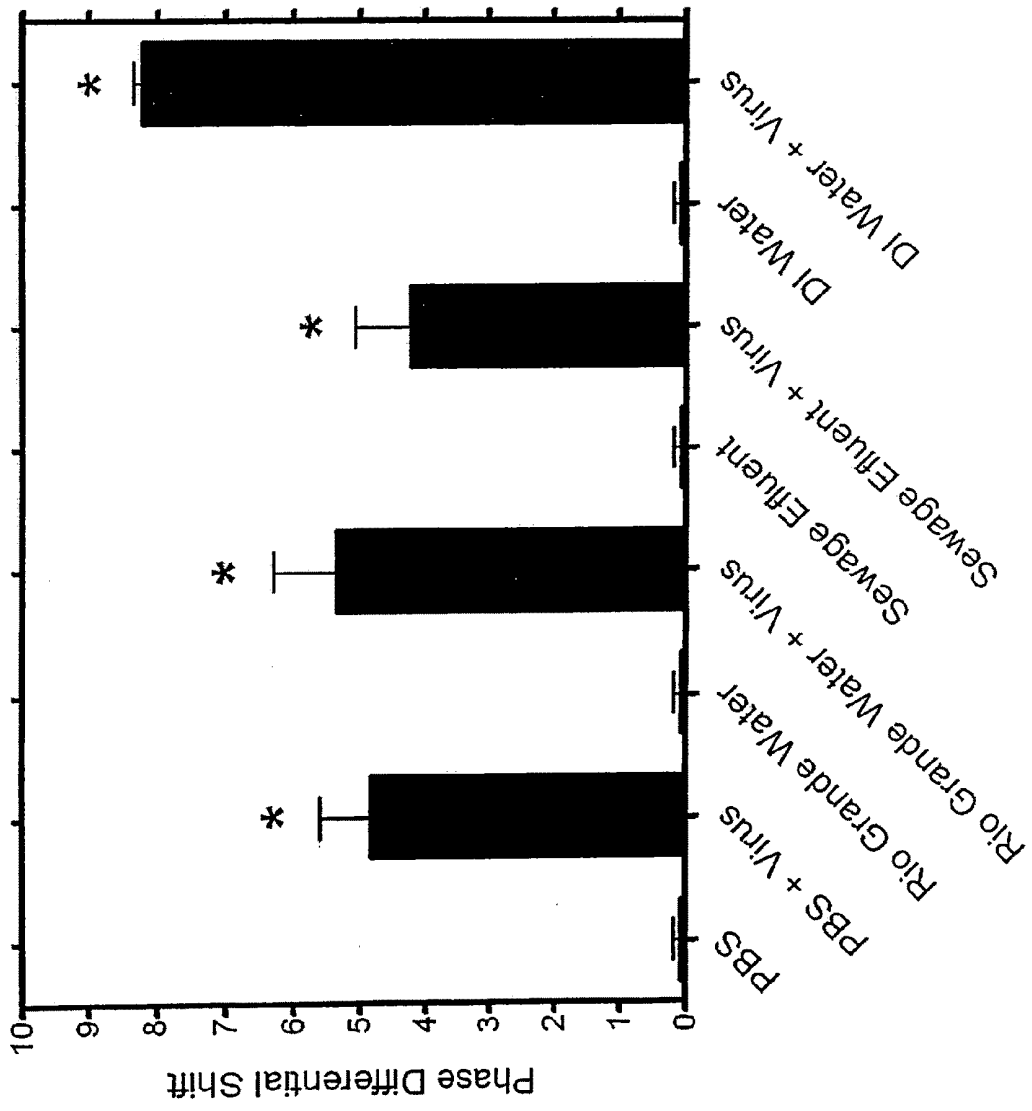

DETECTION OF BIOAGENTS USING A SHEAR HORIZONTAL SURFACE ACOUSTIC WAVE BIOSENSOR

RELATED APPLICATIONS

[0001] The present application claims the benefit of priority of U.S. provisional application Ser. No. 60/900,416, filed Feb. 9, 2007, Ser. No. 60/926,827, filed Apr. 30, 2007 and Ser. No. 61/009,656, filed Dec. 31, 2007, each of which applications is incorporated by reference in its entirety herein.

FIELD OF THE INVENTION

[0002] The present invention relates to the use of a shear horizontal surface acoustic wave biosensor adapted to detect a large number of biological or chemical agents, including viruses, virus fractions (membranes, biomarkers, etc.) and other microbes (prions, eukaryotic and prokaryotic cells, including fungus and bacteria) amino acid based biological agents including polypeptides, DNA and RNA, lipids (including glycosylated, phosphorylated, acetylated lipids) and synthetic chemicals, including nerve gas and other chemical agents. In the present invention, a piezoelectric material, in particular, a lithium tantalate (LiTaO_3) wafer is modified to provide on its surface at least one ligand and preferably, a plurality of ligands, which bind to one or more biological agents to be detected by the biosensor. In the present invention, a biosensor to which is bound a free (unbound) ligand, emits a characteristic wave which can be readily measured—and if the ligand becomes bound to a biological agent, the ligand-biological agent will produce a modified wave pattern which can be measured and result in the qualitative identification (including, in certain aspects, quantitative or concentration information) of the biological agent in a sample. The method and apparatus are adaptable to identify a large number of biological agents as otherwise described in detail herein.

Grant Support

[0003] This work was conducted with support from the National Science Foundation, grant number IIS-0434120, and from the National Institute of Allergy and Infectious Diseases, grant numbers UO1 AI56618 and UO1 AI054779.

BACKGROUND OF THE INVENTION

[0004] Recently, there has been a heightened interest in developing rapid and reliable methods of detection of microorganisms involved in bioterrorism, food poisoning, and clinical problems. Biosensors are devices under intense development to achieve these goals and a number of different types of transduction modes are currently investigated, including electrochemical, optical, thermal, and acoustic (Deisingh, 2004). Shear horizontal surface acoustic wave (SH-SAW) devices that are based on horizontally polarized surface shear waves (HPSSW) enable label-free, sensitive and cost-effective detection of biomolecules in real time and have been used for the detection of bacteria and viral DNA (Berkenpas et al., 2006; Branch and Brozik, 2004; Moll et al., 2007). A SAW device typically has a planar electrode structure consisting of a piezoelectric substrate containing interdigital transducers (IDTs) (Branch and Brozik, 2004). An often used substrate compound that meets many of the required conditions for successful HPSSW generation is lithium tantalate (LiTaO_3) (Branch and Brozik, 2004; Martin

et al., 2004). Applying an alternating voltage via the IDTs at high frequency (typically from 80 to 400 MHz), HPSSW are generated on the substrate. These HPSSW result in a specific resonance frequency that is characteristic for the substrate surface wave velocity. The frequency is sensitive to measurable changes on the sensor surface, for example caused by specific biological interactions.

BRIEF DESCRIPTION OF THE INVENTION

[0005] The present invention is directed to a biological ligand based biosensor comprising a biological ligand which is complexed (coated or tethered) directly or indirectly to the surface of a piezoelectric material of a biosensor apparatus which is combined to accommodate surface acoustic wave (SAW) technology.

[0006] The biosensor of the present invention has, complexed on its surface, any number of biological ligands, which are capable of binding to bioagents which are to be identified. The biological ligands may be chosen for their ability to bind a specific bioagent, or alternatively, to bind to a group or class of bioagents, depending upon common features which exist between the biological ligand which is tethered to the surface of the biosensor apparatus and the bioagent to be identified. The biological ligand may be amino acid based, such as a polypeptide (including modified polypeptides such as glycosylated polypeptides, multimeric polypeptides, including polypeptides which are multimerized by crosslinking devices, nanoparticles, etc., and antibodies), nucleic acid based (single stranded DNA, single stranded RNA, oligonucleotides, including modified oligonucleotides) or lipid based (including glycosylated lipid). The biological ligand is chosen to be specific for a given bioagent such that when a bioagent comes in contact with the ligand, the SAW associated with the biosensor reflects a change indicative of the binding of the bioagent to the ligand.

[0007] The present invention is based upon a biosensor apparatus featuring surface chemistries which are capable of transducing shear horizontal surface acoustic waves (SH-SAW) generated by piezoelectric materials, in particular, lithium tantalate (LiTaO_3), when connected to an electrical circuit at defined frequencies. The technology is manufactured onto wafers that can be sectioned into functional units (“chips”). These units can be applied to a SAW detection board featuring a fluidic housing and a connection of the chip via aluminum delay lines to an output interface with a computing device (e.g., a laptop computer or other computing device) for measurements of SAW. The biosensor apparatus is depicted in FIGS. 1a-d.

[0008] In a method of the present invention, a sample is presented to the ligand based biosensor as described above and a determination of the existence (binding) of a bioagent in the sample which is made by determining a change in a surface acoustic wave emanating from the biosensor which evidences the binding of the bioagent to the ligand.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] FIG. 1A is a diagram depicting an antibody based virus surface acoustic wave (SAW) biosensor in accordance with the present invention. The lithium tantalate (LiTaO_3) sensor surface was coated with NeutrAvidin Biotin Binding Protein (N-Avidin) and coupled to biotinylated [B] monoclonal anti-JVB antibody for Cocksackie virus. Anti-SNV-G1 glycoprotein scFv antibody for SNV detection was coupled

directly. Molecular interaction between virus and antibody elicits an acoustic wave leading to a change in the input frequency of 325 MHz.

[0010] FIG. 1B is a photographic plan view of a pair of substrates or sensor wafers with IDT electrodes disposed thereon for making SAW measurements, showing the sensor wafers in scale compared to a dime coin (10 US cents); four aluminum delay lines are visible; one serves as the reference and three as the test delay lines.

[0011] FIG. 1C is a photographic perspective view showing a SAW detection board (thin arrow) with the fluidic housing (thick arrow) and the output interface device (arrow head) to a laptop computer is shown.

[0012] FIG. 1D is a block diagram of a SAW measurement assembly for making SAW measurements in accordance with the present invention.

[0013] FIG. 2 is a graph showing a detected phase differential as a function of time during operation of a SAW sensor assembly in accordance with the present invention. More particularly, FIG. 2 is a representative SAW biosensor plot showing the response to 1.8×10^4 SNV particles per μl . Output was captured using a custom LabVIEW (National Instruments; website ni.com) program. The data is reported as phase differential mass shift $\Delta\phi$ (indicated by double-headed arrow) on the y-axis as a function of time on the x-axis, corresponding to the maximal difference between buffer-calibrated phase differential before addition of agent (arrow A at ~280 seconds) and after stabilization of signal (arrow B at ~420 seconds). Dotted lines indicate detection at ~15 seconds and maximal signal difference at ~2 minutes after addition of the agent. Single vertically oriented data points are visible as a function of time. See text for details.

[0014] FIG. 3 is a graph of phase differential shift as a function of virus concentration, depicting the detection of Cocksackie virus B4 and SNV using the SAW biosensor, in accordance with the present invention. Data was acquired as described in FIG. 2 and in the text. The plots show the shifts in phase differential (degrees) on the y-axis as a function of increasing viral particle concentrations (in virus/ μl) on the x-axis. Each data point represents an average of 2-5 measurements \pm standard errors. ●=Cocksackie virus B4; ◆=Cocksackie virus B4+HSV-1; ■=HSV-1 alone for the Cocksackie virus experiments; ▲=SNV; ○=SNV+HSV-1; □=HSV-1 alone for the SNV experiments. The solid and dotted lines represent the best fit models and coefficient correlations (R^2) for Cocksackie virus B4 (●) and SNV (▲), respectively.

[0015] FIG. 4 is a bar graph phase differential shift as a function of test solutions, showing detection of SNV in complex solutions using the SAW biosensor. SNV viral particles were spiked into distilled (DI) water, phosphate buffered saline (PBS), sewage effluent, or Rio Grande water for a final concentration of 1.8×10^4 viral particles/ μl . Data was acquired as described in FIG. 2 and in the text. The plots show the shifts in phase differential (degrees) on the y-axis as a function of solution input on the x-axis. Each data point represents an average of 2 measurements with \pm standard errors. Stars denote statistical significance ($p < 0.05$) over background (no virus) solutions using student's t-test.

DETAILED DESCRIPTION OF THE INVENTION

[0016] The following terms shall be used to describe the present invention. In instances where a term is not defined,

then the term shall be given its ordinary meaning as understood by those of ordinary skill within the context of its use.

[0017] The term "effective" is used to describe, within context, an amount of a component or compound used in the present invention in a manner consistent with its intended use.

[0018] The term "ligand" or "capture molecule" shall mean a biological compound comprising amino acids, DNA or RNA (polynucleotides or oligonucleotides), lipids or carbohydrates which may be complexed (coated or tethered) onto the surface of a piezoelectric material in a biosensor apparatus according to the present invention. Amino acid based ligands include antibodies (monoclonal or polyclonal) and fragments thereof (e.g. single chain Fab antibody fragments), polypeptides (at least 25 mer), oligopeptides (about 3 mer to about 25 mer or more), peptide multimers (palindromes, crosslinked multimeric peptides, nanoparticles, among others). DNA or RNA ligands are polynucleotides, oligonucleotides which may be single stranded DNA, single stranded RNA, oligonucleotides (phosphate backbone, etc.) and lipids, including glycosylated lipids and carbohydrates, including complex carbohydrates. Although the most common type of capture molecule is an antibody, other peptides such as receptors, enzymes, other proteins, including dendrimers (especially in the case of prions), nucleotides (polynucleotides and oligonucleotides), aptamers, primarily DNA molecules, but also stable RNA (preferably, single stranded) molecules may be used. In addition, lipids and carbohydrates (chitosan, lectins, among others) may be used as capture molecules, depending upon the nature of the bioagent to be detected.

[0019] The ligand may be designed and used to detect primary amino acid sequences, especially including biomarkers on cell or particle surfaces (including mutations, translocations, truncations and isoforms), posttranslational modifications, phosphorylations, glycosylation, non-peptide organics (nerve gasses, alkylating agents, other organic toxins), lipids, including glycosylated, phosphorylated or acetylated lipids, double stranded DNA or RNA (especially after denaturing) and single stranded DNA or RNA. The ligand may include a nucleocapsin protein capture DNA, as well as other capture DNA and RNA molecules (such as aptamers), among others.

[0020] Ligands may be broadly used and applied. Essentially any biological molecule capable of binding a bioagent as otherwise described herein finds use in the present invention. Exemplary ligands may be found throughout the literature and are numerous. An excellent directory which provides a large number of amino acid based ligands, especially monoclonal and polyclonal antibodies for use in the present invention is Linscott's directory of immunological and biological reagents, available at linscottsdirectory.com. DNA and RNA ligands (e.g., capture DNA/RNA) which bind to bioagents may be found throughout the literature. In applications of the present invention, depending upon the type and actual size of the ligand to be tethered to the biosensor, the number/concentration of ligands which are tethered to a biosensor ranges from 1 to about 100,000 or more per cm^2 , from 10 to about 50,000, about 50 to about 25,000, about 100 to about 20,000, about 500 to about 15,000 about 750 to about 12,500, about 1000 to about 10,000, about 1250 to about 7500, about

[0021] Exemplary ligands include monoclonal and polyclonal antibodies, including anti-Cocksackie virus monoclonal antibody (mouse IgG2a), anti-Sin Nombre virus (SNV) G1 glycoprotein (single chain Fv, scFv from phage display), anti-Herpes Simplex virus I (HSV-1) antibody (polyclonal), anti- $\alpha\text{v}\beta 3$ integrin antibody, anti-Interleukin-

12 (IL-12) monoclonal antibody (mouse IgG1), anti-Interleukin-6 (IL-6) polyclonal, among others; peptides, including 9 amino acid cyclic peptides from Sin Nombre Virus phage display as described in greater detail herein, 9 amino acid cyclic peptides from Andes virus phage display as described in greater detail herein, linear peptides including a 16 amino acid peptide from Dengue virus phage display; nucleic acids, including Sin Nombre virus-N(SNV-N) and SNV-M capture DNA (analyte is Sin Nombre virus (SNV) RNA) and BRCA1 capture DNA (single-stranded, 30 mer (base units in length)-analyte is BRCA1 DNA (single stranded-60 base units in length), among others.

[0022] The term “bioagents” or “analytes” used synonymously within context, shall mean viruses and their extracts, prions and their extracts, eucaryotic cells, fragments and extracts, prokaryotic cells (especially bacteria), fragments and extracts, prokaryotic spores, fragments and extracts, protein and peptide markers (biomarkers, especially biomarkers on cell surfaces), serum proteins, isolated proteins, synthetic chemicals, viral membranes, eukaryotic membranes, eukaryotic cell parts, including mitochondria and other organelles, prokaryotic membranes, DNA viruses (single and double stranded DNA viruses), RNA viruses (single and double stranded RNA viruses), point mutations (any organism), single nucleotide polymorphism (any organism), mRNA's, rTNAs, micro RNAs (from any organism). In preferred aspects of the invention, the bioagent or analyte is a virus or extract, a prion or a DNA or RNA molecule. Any virus for which a monoclonal or polyclonal antibody may be raised, for which a binding polypeptide is available or for which a capture DNA is available are particularly preferred bioagents or analytes for use in the present invention.

[0023] Exemplary viruses which may be viral bioagents in the present invention include animal, plant, fungal and bacterial viruses. Viral biogents which may be detected by the biosensors according to the present invention include those which impact animals, especially mammals, in particular humans, domestic animals and include, for example, Papovaviruses, e.g. polyoma virus and SV40; Poxviruses, e.g. vaccinia virus and variola (smallpox); Adenoviruses, e.g., human adenovirus; Herpesviruses, e.g. Human Herpes Simplex types I and II; Parvoviruses, e.g. adeno associated virus (AAV); Reoviruses, e.g., rotavirus and reovirus of humans; Picornaviruses, e.g. poliovirus; Togaviruses, including the alpha viruses (group A), e.g. Sindbis virus and Semliki forest virus (SFV) and the flaviviruses (group B), e.g. dengue virus, yellow fever virus and the St. Louis encephalitis virus; Retroviruses, e.g. HIV I and II, Rous sarcoma virus (RSV), and mouse leukemia viruses; Rhabdoviruses, e.g. vesicular stomatitis virus (VSV) and rabies virus; Paramyxoviruses, e.g. mumps virus, measles virus and Sendai virus; Arena viruses, e.g., lassa virus; Bunyaviruses, e.g., bunyawere (encephalitis); Coronaviruses, e.g. common cold, GI distress viruses, Orthomyxovirus, e.g., influenza; Caliciviruses, e.g., Norwalk virus, Hepatitis E virus; Filoviruses, e.g., ebola virus and Marburg virus; and Astroviruses, e.g. astrovirus, among others.

[0024] Bioagents such as Sin Nombre virus, influenza (especially H5N1 influenza), Herpes Simplex Virus (HSV1 and HSV-2), Cocksackie virus, Human immunodeficiency virus (I and II), Andes virus, Dengue virus, Papilloma, Epstein-Barr virus (mononucleosis), Variola (smallpox) and other pox viruses, West Nile virus, influenza (H5N1) find use as bioagents in the present invention.

[0025] A short list of animal viruses may be relevant bioagent targets for use in the present invention:

- [0026]** Reovirus
- [0027]** Rotavirus
- [0028]** Enterovirus
- [0029]** Rhinovirus
- [0030]** Hepatovirus
- [0031]** Cardiovirus
- [0032]** Aphthovirus
- [0033]** Parechovirus
- [0034]** Erbovirus
- [0035]** Kobuvirus
- [0036]** Teschovirus
- [0037]** Norwalk virus
- [0038]** Hepatitis E virus
- [0039]** Rubella virus
- [0040]** Lymphocytic choriomeningitis virus
- [0041]** HIV-1, HIV-2,
- [0042]** HTLV-I
- [0043]** Herpes Simplex Virus 1 and 2
- [0044]** Sin Nombre Virus
- [0045]** Cocksackie Virus
- [0046]** Dengue virus
- [0047]** Yellow fever virus
- [0048]** Hepatitis A virus
- [0049]** Hepatitis B virus
- [0050]** Hepatitis C virus
- [0051]** Influenzavirus A, B and C
- [0052]** Isavirus,
- [0053]** Thogotovirus
- [0054]** Measles virus
- [0055]** Mumps virus
- [0056]** Respiratory syncytial virus
- [0057]** California encephalitis virus
- [0058]** Hantavirus
- [0059]** Rabies virus
- [0060]** Ebola virus
- [0061]** Marburg virus
- [0062]** Corona virus
- [0063]** Astrovirus
- [0064]** Borna disease virus
- [0065]** Variola (smallpox virus)

[0066] Plant viruses also are relevant bioagents for use in the present invention. The present invention may be used to detect plant viruses, especially in agricultural applications.

[0067] Plant viruses, which may serve as bioagents (analytes) for the present include the following:

[0068] Geminiviruses e.g., bigeminivirus, monogeminivirus and bybriginivirus; Partitiviruses, e.g., alphacryptoviruses and betacryptoviruses; Potyvirus, e.g., bymoviruses and ipomoviruses; Bromoviruses, e.g. cucumoviruses and bromoviruses; Comoviruses, e.g. fabiviruses, neopoviruses and comoviruses; Rhabdoviruses, e.g., cytorhabdoviruses, nucleorhabdoviruses; Reoviruses, e.g., oryzaviruses and phytoreoviruses; Satellite viruses, e.g., satelliviruses; Tombusviruses, e.g., carmoviruses; Sequiviruses, e.g., sequiviruses and waikaviruses; among numerous others (see below).

Plant Virus Genuses, include the following:

- [0069]** Alfamoviruses: Bromoviridae
- [0070]** Alphacryptoviruses: Partitiviridae
- [0071]** Badnaviruses
- [0072]** Betacryptoviruses: Partitiviridae
- [0073]** Bigeminiviruses: Geminiviridae
- [0074]** Bromoviruses: Bromoviridae

- [0075] Bymoviruses: Potyviridae
- [0076] Capilloviruses
- [0077] Carlaviruses
- [0078] Carmoviruses: Tombusviridae
- [0079] Caulimoviruses
- [0080] Closteroviruses
- [0081] Comoviruses: Comoviridae
- [0082] Cucumoviruses: Bromoviridae
- [0083] Cytorhabdoviruses: Rhabdoviridae
- [0084] Dianthoviruses
- [0085] Enamoviruses
- [0086] Fabaviruses: Comoviridae
- [0087] Fijjiviruses: Reoviridae
- [0088] Furoviruses
- [0089] Hordeiviruses
- [0090] Hybrigeminiviruses: Geminiviridae
- [0091] Idaeoviruses
- [0092] Ilarviruses: Bromoviridae
- [0093] Ipomoviruses: Potyviridae
- [0094] Luteoviruses
- [0095] Machlomoviruses
- [0096] Macluraviruses
- [0097] Marafiviruses
- [0098] Monogeminiviruses: Geminiviridae
- [0099] Nanaviruses
- [0100] Necroviruses
- [0101] Nepoviruses: Comoviridae
- [0102] Nucleorhabdoviruses: Rhabdoviridae
- [0103] Oryzaviruses: Reoviridae
- [0104] Ourmiaviruses
- [0105] Phytoreoviruses: Reoviridae
- [0106] Potexviruses
- [0107] Potyvirus: Potyviridae
- [0108] Rymoviruses: Potyviridae
- [0109] Satellite RNAs
- [0110] Satelliviruses
- [0111] Sequiviruses: Sequiviridae
- [0112] Sobemoviruses
- [0113] Tenuiviruses
- [0114] Tobamoviruses
- [0115] Tobraviruses
- [0116] Tombusviruses: Tombusviridae
- [0117] Tospoviruses: Bunyaviridae
- [0118] Trichoviruses
- [0119] Tymoviruses
- [0120] Umbraviruses
- [0121] Unassigned potyvirus: Potyviridae
- [0122] Unassigned rhabdovirus: Rhabdoviridae
- [0123] Varicosaviruses
- [0124] Waikaviruses: Sequiviridae
- [0125] Ungrouped viruses

[0126] A much more complete list of viral bioagents which may be analytes in the present invention include, for example, those which are listed at: Virus Taxonomy, the Sixth Report of the International Committee on Taxonomy of Viruses (ICTV) 1995 See, the corresponding website: tulane.edu/~dmsander/WWW/335/VirusList.html, which is referenced herein.

[0127] Prions are another class of important bioagents which may be detected using the invention of the present application. Exemplary prions include Scrapie (Sheep and goats), transmissible mink encephalopathy (TME), chronic wasting disease (CWD) in mule deer and elk, bovine spongiform encephalopathy (BSE) cattle, feline spongiform encephalopathy (FSE) in cats, exotic ungulate encephalopa-

thy (EUE), Kuru in humans, Creutzfeldt-Jakob disease (CJD) in humans, Fatal familial insomnia (FFI) in humans and Gerstmann-Sträussler-Scheinker syndrome (GSS) in humans.

[0128] The present invention may be used to detect bioagents in a sample, such as viruses, prions, other microbes, biological mixtures of compositions and components, particles and their extracts, etc. as otherwise described herein. The present invention has utility in military applications, especially in field applications, in commercial applications, in agricultural applications and in research/medical applications (including the existence of air-borne infections in the lungs of a patient). The present invention may be used to detect bioagents in the atmosphere (air), in water supplies, including standing water, in soil samples, etc.

[0129] By way of example, the present invention is useful for detecting numerous interactions between ligand and bioagent, including, for example, interactions between receptor and agonist/antagonist, between peptide and other peptides (peptide-peptide interaction), between antibody (monoclonal and polyclonal) and epitope on the bioagent (biomarkers, basic protein sequence, etc.), between polynucleotides (Watson-Crick base pairing or hybridization), as well as any other chemical or physical interaction (e.g., Van der Waals interactions) which may specify the binding or interaction of a bioagent with the ligand.

[0130] The term "tethered" is used to describe the attachment of the biological ligand onto the surface of the biosensor. The ligands are attached to the biosensor in a manner so that the portion of the ligand which binds to the bioagent is exposed on the surface. The ligands may be attached to the surface of the biosensor (preferably, a lithium tantalate chip) directly or indirectly by any means available. Ligands which are used in the present invention are complexed (coated or tethered through covalent, ionic, hydrophobic or other types of bonding) with the surface of the biosensor. This may include employing covalent bonding between ligand and sensor surface; e.g., the use of diazonium chemistry to attach the ligand to the sensor surface or through use of silicone chemistry. Some employ non-covalent bonding such as self-assembled monolayers; other approaches combine both covalent binding and non-covalent binding such as streptavidin-biotin interactions, wherein the streptavidin molecule is non-covalently attached to the sensor surface, and the biotin molecule is covalent bonding to the ligand and the streptavidin and biotin molecules are covalently bound to each other. Additionally, the attachment of ligands to sensor surface may be made through the process of physisorption, which relies on Van der Waals forces to make non-covalent connections to the surface. Chemisorption, which uses covalent bonds, may also be used to attach or tether ligand to sensor surface. Simple adsorption may also be applicable to tether a ligand to the biosensor surface.

[0131] In certain applications, the surface of the piezoelectric material, a lithium tantalate wafer used in the present invention, is coated with a thin silicon dioxide surface or other surface which is created using standard methods such as sputtering techniques or more preferably, plasma enhanced chemical vapor deposition (PECVD) to produce a thin layer (about 500 Å to about 10,000 Å or more, in certain preferred aspects, about 5000 Å) as otherwise described herein. A ligand may be tethered to the silicon dioxide layer directly by covalent (chemisorption) or through non-covalent bonding (physisorption), or alternatively, the silicon dioxide layer may be further coated with a hydrophobic material (in certain

embodiments, hexamethyldisilazane, or other hydrophobic material such as a liquid/semi-liquid hydrocarbon such as petrolatum or mineral oil, including other silicone materials) to provide a surface which is amenable to adsorption of a ligand as otherwise described herein. The hydrophobic layer on the silicone dioxide layer may be modified (covalently or non-covalently) using a chemical linker such as a functional silane compound, as otherwise described herein, which can covalently bond a ligand directly or bond a further linker (a complex linker) such as a binder protein (e.g., NeutrAvidin binding protein) which can bond certain molecules/moieties (biotin) which can be complexed with the ligand to tether the ligand indirectly to the surface of the SAW biosensor.

[0132] The term “adsorption” refers to a process that occurs when a gas or liquid solute accumulates on the surface of a solid or a liquid (adsorbent), forming a molecular or atomic film (the adsorbate). Adsorption is operative in most natural physical, biological, and chemical systems, including the present invention. Similar to surface tension, adsorption is a consequence of surface energy. In a bulk material, all the bonding requirements (be they ionic, covalent or metallic) of the constituent atoms of the material are filled. But atoms on a clean surface experience a bond deficiency, because they are not wholly surrounded by other atoms. Thus, it is energetically favourable for them to bond with whatever happens to be available. The exact nature of the bonding depends on the details of the species involved, but the adsorbed material is generally classified as exhibiting physisorption or chemisorption.

[0133] The term “physisorption” is used to describe a physical adsorption process in which there are van der Waals forces of interaction between a surface (solid) and a liquid or air layer. Physical adsorption is a type of adsorption in which the adsorbate adheres to the surface only through Van der Waals (weak intermolecular) interactions, which are also responsible for the non-ideal behaviour of real gases. Physisorption is characterised by the following:

[0134] Low ambient temperature, always under the critical temperature of the adsorbate;

[0135] Type of interaction: Intermolecular forces (van der Waals forces);

[0136] Low enthalpy: $\Delta H < 20$ kJ/mol;

[0137] Adsorption takes place in multilayers;

[0138] Low activation energy;

[0139] The energy state of the adsorbate is not altered;

[0140] The process is reversible.

[0141] In the present invention an exemplary physisorption approach to tethering ligands to the biosensor involves creating a silicon dioxide (SiO_2) layer on the biosensor wafer. This is the waveguide layer and varies in thickness (ranges from less than about 500 Å to about 20,000 Å or more, about 1000 Å to about 10,000 Å, about 1500 Å to about 7,500 Å, about 2500 Å to about 6500 Å, about 4000 Å to 6000 Å, about 5000 Å), but is preferably about 5000 Å. Any method known in the art for depositing a silicon dioxide layer may be used, but a preferred approach utilizes plasma enhanced chemical vapor deposition (PECVD, Oerlikon Versaline, Switzerland) to provide the silicon dioxide layer. On top of the silicon dioxide layer a thin layer of a non-reactive liquid silicone material such as hexamethyldisilazane or other non-reactive, liquid alkyl silicone material such as an oligodialkylsiloxane, polydialkylsiloxane or other silicone, or a other non-reactive liquid may be used may be used.

[0142] The term “chemisorption” is used to describe a type of adsorption whereby a molecule adheres to a surface through the formation of a chemical bond, as opposed to the Van der Waals forces which cause physisorption. It is characterised by the following:

[0143] High temperatures;

[0144] Type of interaction: strong; covalent bond between adsorbate and surface;

[0145] High enthalpy: 50 kJ/mol $< \Delta H < 800$ kJ/mol

[0146] Adsorption takes place only in a monolayer.

[0147] High activation energy

[0148] Increase in electron density in the adsorbent-adsorbate interface.

[0149] Reversible generally at high temperature.

[0150] The main way in which chemisorption is used in the present invention is that a linker molecule which may contain at least one hydroxyl (especially, Si—OH) binding group or other binding group (to bind to the surface of the biosensor) and at least one group which can bind an amine group, a carboxyl group, a hydroxyl group or a phosphate group are used to chemically link or tether a ligand to the surface of the biosensor. Other approaches include providing a linker comprising an amine, hydroxyl, carboxyl or phosphate binding group which itself is non-covalently physisorbed to the biosensor surface to, for example, a non-covalently bonded silicone such as hexamethyldisilazane which is itself non-covalently complexed to the SiO_2 surface of the biosensor). Exemplary linkers for tethering a ligand to the biosensor include, for example, silanes containing reactive functional groups (“functional silane”), for example, 3-aminopropyltrimethoxysilane (amino group binding) and 3-glycidyloxypropyltriethoxysilane (carboxyl group binding), among others.

[0151] Several preferred approaches to tethering ligands may be taken in the present invention. These approaches may involve exclusively physisorption methods, chemisorption methods or combinations of physisorption and chemisorption methods. In a first physisorption method, a layer of silicon dioxide is produced on the surface of the biosensor using plasma enhanced chemical vapor deposition (PECVD) technology. Once the silicon dioxide layer is in place on the biosensor, a thin layer of hexamethyldisilazane (HMDS) or other inert silane is placed on the silicone dioxide layer. An antibody or peptide may be bonded (physisorbed) to the biosensor through the hexamethyldisilazane layer.

[0152] Alternatively, an antibody, peptide, fatty acid or carbohydrate may be bonded to a chemical linker (e.g. a functional silane) which is itself bonded (physisorbed) to a layer of hexamethyldisilazane (HMDS) and silicon dioxide to provide a tethered ligand on the biosensor of the present invention. This method combines both physisorption and chemisorption methods.

[0153] Still another approach for tethering a ligand to the biosensor of the present invention involves utilizing a linker protein, such as NeutrAvidin Binding Protein which itself binds to a biotinylated ligand, such as a peptide, amino acid or DNA molecule. In this aspect, the biosensor is first provided with a silicon dioxide layer to which is layered (physisorbed) a non-reactive silicone liquid, e.g., hexamethyldisilazane (HMDS). A thin layer of a functional silane, for example, 3-aminopropyltrimethoxysilane (amino group binding) and 3-glycidyloxypropyltriethoxysilane (carboxyl group binding), among others may be physisorbed to the hexamethylsilazane layer and the functional silane may be used to covalently link a binding protein (e.g. NeutrAvidin Binding

Protein) to the biosensor. The NeutrAvidin Binding Protein may then be used to bind any biotinylated ligand. Additional approaches, or variations on the above approaches to tether virtually any ligand to the biosensor of the present invention are well within the ordinary skill of the routineer.

[0154] The present invention is based on a biosensor apparatus featuring surface chemistries that are capable of transducing shear horizontal surface acoustic waves (SH-SAW) generated by piezoelectric materials such as lithium tantalate (LiTaO_3) when connected to an electrical circuit at defined frequencies. This technology is manufactured onto lithium tantalate wafers (or wafers from another piezoelectric material) that can be sectioned into functional units ("chips"). These units can be applied to a SAW detection board featuring a fluidic housing (described below) and a connection of the chip via aluminum delay lines to an output interface with a laptop computer for measurements of SAW. FIGS. 1B and 1C (attached) represent the functional unit. FIG. 1D is a block diagram of functional components of the ZAW measurement system.

[0155] As depicted in FIG. 1D, the components of the SH-SAW detector include three transducer elements **102**, **104**, **106** in the form of IDT electrodes disposed in a linear array on a substrate **108**. Electrodes **102**, **104**, **106** are connected at inputs to a power source **110** via a power splitter **112**. A reference oscillator **114** is provided, which may be used in part to generate the SH-SAW waves in the fluidic housing. As shown in FIG. 1B, reference oscillator **114** is disposed on the same substrate or chip as IDT electrodes **102**, **104**, **106**. IDT electrodes **102**, **104**, **106** are each connected on an output side via a respective delay line **116**, **118**, **120** to a respective phase difference detector **124**, **126**, **128** exemplarily in the form of an IQ demodulator. Phase difference detectors **122**, **124**, **126** also receive input from oscillator **114** via a reference line **122**. Phase difference detectors **122**, **124**, **126** are connected to a computer **130** via analog-to-digital converters **132**. Computer **128** may be programmed, inter cilia, to issue an alert signal via an output transmitter **134** upon detecting a disturbance in a standing wave indicating the presence of a target pathogen or toxic agent.

[0156] In FIG. 1B, the sensor wafer or substrate **108** is shown in scale compared to a dime coin (10 US cents); the four aluminum delay lines are visible; one line **122** serves as the reference and three others **116**, **118**, **120** (FIG. 1D) as the test delay lines. In FIG. 1C, the SAW detection board (thin arrow) with the fluidic housing (thick arrow) and the output interface device (arrow head) to a laptop computer is shown.

[0157] As described above, the surface of the sensor wafer can be complexed with ligands that are specific for any biological substance (for example, but not exclusively, a protein), free or as part of a larger complex (for example a virus, a spore, or a cell) for its detection when this substance, added in solution to the fluidic housing (the bioagent passes through small holes in the housing, which is permeable to the bioagent), is specifically recognized by its specific ligand on the surface of the sensor (see Claims below). Specific recognition (binding) results in a characteristic and quantifiable change of frequency that is captured using software applicable for such a purpose. The present invention is directed to the detection of biological entities, such as viruses and cells, of both prokaryotic and eukaryotic nature, as well as prions and molecules using ligands specific for surface molecules of these entities. Such ligands can be for example antibodies or peptides. FIG. 1A shows one such example, in which a biotinylated antibody

that is able to specifically recognize a virus is coupled to the LiTaO_3 surface of a SAW biosensor that has been coated with NeutrAvidin Biotin Binding Protein.

Preferred Embodiment

[0158] The following describes a preferred embodiment. The present invention is directed to the detection of viruses and other biological and chemical agents by SAW. In this embodiment, a Cocksackie virus, a member of the enterovirus family, which also includes polioviruses and hepatitis A virus (Palacios and Oberste, 2005) was the bioagent. Cocksackie virus infections are usually not of major health concern and possible fevers, headaches, and muscle aches typically self-dissolve after several days. Occasionally however, Cocksackie virus can cause serious infections, such as hand, foot and mouth disease, viral meningitis, encephalitis, myocarditis, and hepatitis, especially in newborns (Frydenberg and Starr, 2003; Tam, 2006). The primary objective is the Sin Nombre virus (SNV), a hantavirus member of the Bunyaviridae family of RNA viruses and a category A agent as defined by the National Institute of Allergy and Infectious Diseases (NIAID; website niaid.nih.gov) and other category A bioagents. SNV is transmitted by its reservoir host *Peromyscus maniculatus*, the deer mouse. Transmission happens by inhalation of aerosolized feces, urine, or saliva from the infected mice (Jay et al., 1997). The illness that ensues, hantavirus cardiopulmonary syndrome (HCPS), is characterized initially by mild flu-like symptoms, followed by rapid progression to respiratory distress, and can be fatal (Hjelle, 2002; Mertz et al., 2006). There is no established therapeutic regimen and treatment is only supportive. Preventive methods include attempts to minimize contact with the rodents since elimination of the virus is not realistic. Although human infections with hantaviruses are on the rare side, these agents have been classified by the Center of Disease Control (CDC) as potential agents for biologic terrorism due to their relative ease of production, the high susceptibility of large populations, and the limited treatment and vaccination strategies (Bronze et al., 2002).

[0159] In the present invention, the development and preliminary use of an SH-SAW biosensor able to detect category A viral agents operating at an input frequency of 325 MHz was a principal objective. Input frequencies may vary over a range of about 275 to 400 MHz, with 315-330 and 325 MHz being particularly useful. The present invention shows that the biosensor device of the present invention is sensitive and highly selective for its specific target. We also provide data in support of the biosensor's high reproducibility and its use in a real world scenario mimicking the exposure of an urban population to a viral agent, such as for example through the water system. The present invention indicates that this detection platform is highly versatile and robust and has significant medical or defense use.

2. Materials and Methods

2.1. Fabrication of the 325 MHz SH-SAW Sensor

[0160] Wafer preparation and lithographic deposition of IDT layer: The SH-SAW device was fabricated using metal evaporation and lift-off plasma enhanced chemical vapor deposition (PECVD), and reactive ion etching (RIE) techniques on a 36° y-cut, x-propagating lithium tantalate (LiTaO_3) crystal wafer of 510 μm thickness and 100 mm diameter. The wafer was cleaned in a barrel asher (PVA Tepla, Asslar, Germany) for 5 minutes, 600 Watts power and 900

mTorr of O₂, followed by dipping in 1 vol % hydrofluoric acid (HF) for 3 minutes, and rinsing in a cascade bath until the resistivity of the water was greater than 12 MOhm-cm followed by drying under N₂. The wafer layout was designed to include four IDT patterns with sets of transducers and delay lines. AZ2020 (AZ Electronic Materials, Branchburg, N.J., USA) negative-tone photoresist (PR) was applied using a spin coater with a Gyrset lid (Karl-Suss, Waterbury Center, Vt., USA) at 1300 and 3000 rpm/sec for 30 seconds each to achieve a thickness of 2.0 μm. The wafer was baked on a hotplate for 60 seconds at 110° C. and cooled to room temperature on a metal surface. Because of the pyroelectric nature of LiTaO₃ it was necessary to remove residual electric charge by dipping the wafer in de-ionized water and drying under N₂. The PR was exposed to i-line UV light at 365 nm for 6 seconds at 14 mW/cm². The wafer was re-baked on a hotplate at 110° C. for 60 seconds followed by a 1 minute developing time in a 300 MIF developer (AZ Electronic Materials) and rinsing in de-ionized water. The wafer was metallized with 5000 Å aluminum using an electron-beam evaporator (Temescal, Wilmington, Mass., USA). The deposition rate was 3 Å/sec for 500 Å and then 5 Å/sec for 4500 Å. The wafer was placed in an acetone bath to lift off the PR and excess aluminum. An acetone spray was used to remove the PR between the IDT fingers, followed by rinses in methanol, isopropyl alcohol, and de-ionized water. This procedure was repeated for the metallization of the ground plane, buss lines, and contact pads.

[0161] Deposition of the waveguide layer and final preparation: A 5000 Å silicon dioxide (SiO₂) film was deposited onto the entire wafer using PECVD (Oerlikon Versaline, Pfaeffikon, Switzerland) at 150° C. for 410 seconds. The oxide was coated with hexamethyldisilazane (HMDS) in a vacuum oven at 100° C. for 30 minutes. AZ4330 positive-tone PR (AZ Electronic Materials) was spin coated onto the wafer at 2000 rpm and 3000 rpm/sec for 30 seconds each. The wafer was baked on a hotplate at 90° C. for 90 seconds, exposed for 48 seconds at 20 mW/cm² (at 400 nm), and developed in a 300 MIF developer for 3 minutes. A photoresist mask was used to "open" the SiO₂ and expose the electrical contact pads. The SiO₂ was etched by RIE (Oerlikon Versaline) for 1500 seconds (p=40 mT, CHF₃=45 sccm, O₂=5 sccm, P=125 watts, DC bias=712 volts). The wafer was diced using a resinoid dicing blade. The PR was removed from the individual die by rinsing in acetone, methanol, and isopropanol.

2.2. Virus Production and Preparation

[0162] Viral work was conducted in Biosafety Level 2 (Coxsackie virus B4) or Level 3 (SNV) facilities at the University of New Mexico School of Medicine. The JVB strain of Coxsackie virus B4 was purchased from ATCC (Manassas, Va., USA). Buffalo Green Monkey Kidney (BGMK) cells were purchased from Diagnostic Hybrids, Inc. (Athens, Ohio, USA). BGMK cells were grown to confluency in DMEM, 2 mM L-glutamine, 10 mM HEPES, 26.8 mM sodium bicarbonate, and 10% fetal bovine serum. After removal of culture media, BGMK cells were inoculated with Coxsackie virus B4 for 1 hour at room temperature and grown in a serum free media, Opti PRO SFM (GIBCO, Grand Island, N.Y., USA) supplemented with 4 mM L-glutamine. Upon reaching 100% cytopathic effect (CPE), the media was centrifuged in a sealed rotor for 5 minutes at 3000 rpm and the supernatant was stored at -20° C. The viral titer was determined by serial dilution and growth in BGMK cells. The virus was inactivated

with 2.0 Mrads of gamma radiation using a Gammacell 40 (Atomic Energy of Canada, Ltd., Kanata, Ontario, Canada) and concentrated by lyophilization and resuspension in distilled water.

[0163] SNV particles were purified from the supernatant of VeroE6 monkey kidney cells (ATCC) infected with SNV at a multiplicity of infection of 0.1 for 1 hour. After 9 days the media was subjected to ultracentrifugation using Optiprep density gradients in phosphate buffered saline (PBS) (Axis-Shield, Norton, Mass.) and the isolated virus was inactivated by UV. The amount of SNV particles was quantified by determining the SNV nucleocapsid (SNV-N) protein concentration (not shown). SNV particle number was calculated based on the following parameters pertaining to the SNV-N protein: SNV-N has a mass of 50 kD; thus 1 mol (6.02×10²³)=50,000 grams; thus one SNV-N protein=8.3×10⁻¹¹ nanograms. There are ~10⁵ SNV-N proteins per SNV particle; thus 8.3×10⁻⁶ nanograms of SNV-N=one SNV particle. Using these calculations, 1 nanogram of SNV-N protein corresponds to ~120,000 SNV particles. Purified Herpes Simplex virus type 1 (HSV-1) was a kind gift of Dr. Stephen Young at TriCore Laboratories (Albuquerque, N. Mex., USA).

2.3. Preparation of Antibodies and Adsorption to the SAW Biosensor

[0164] The IgG2a isotype monoclonal antibody (mAb) directed against the JVB strain of Coxsackie virus B4 was produced by the 204-4 hybridoma cell line (ATCC). The mAb was labeled with biotin using the EZ-Link NHS-PEO Solid Phase Biotinylation Kit and Spin Column featuring the SwellGel Disk technology (Pierce, Rockford Ill., USA). The mAb was added to the gel at 2 mg/ml for 10 minutes followed by incubation in NHS-PEO4-Biotin for 30 minutes at room temperature and column spinning. The biotin labeled antibody was eluted from the column with 0.2 M Imidazole in PBS. Single chain Fv antibodies (scFv) directed against SNV have been previously selected from a phage antibody library, and are specific for the SNV-G1 glycoprotein exerting no cross-reactivity with glycoproteins from other hantaviruses (Velappan et al., 2007). These scFv antibodies were left unmodified and directly adsorbed to the biosensor.

[0165] The SAW devices were cleaned in acetone, methanol, and isopropanol, then treated by ultrasonication in 95% ethanol, rinsed in distilled water, followed by exposure to UV-ozone for 10 minutes in a UVOCS UV-Ozone cleaner (UVOCS Inc., Montgomeryville, Pa., USA). For the antibody directed against the Coxsackie virus B4, the oxide layer of the test delay lines of the SAW device were coated in a non-covalent physisorption process with 0.25 mg/ml of NeutrAvidin Biotin Binding Protein (Pierce) in PBS for 30 minutes at room temperature. The device was washed 3 times with PBS and 1 time with distilled water, and dried using nitrogen. The biotin labeled 204-4 mAb was adsorbed to the NeutrAvidin Biotin Binding Protein at 0.25 mg/ml in PBS for 30 minutes at room temperature. For the detection of SNV, anti-SNV-G1 scFv at 0.25 mg/ml was directly adsorbed to the SAW device for 30 minutes at room temperature. After coating with the antibodies, the biosensor devices were washed 3 times with PBS and 1 time with distilled water, followed by nitrogen drying.

2.4. SAW detection of Coxsackie and SNV

[0166] For display and acquisition of the digitized voltage data from the sensor platform, a custom LabVIEW (National Instruments; website ni.com) program was developed. The

data from each of the delay lines were acquired simultaneously and the voltage information was converted back to the phase. Data from the reference line were subtracted from the data from the test lines for each time point measured and continuously saved to disk in spreadsheet format. The data for the quantitative measurements of viral detection presented in this study refer to the phase differential mass shift ($\Delta\phi$) and are displayed on a graph as a function of time of acquisition. Multiple data points per time are recorded during this process. The SAW device was assembled in a static cell with a 325 MHz input frequency from a power supply. The chamber (fluidic housing) was covered with 0.4 ml of PBS or medium and the phase differential was stabilized for at least 100 seconds. 0.1 ml of solution was removed and replaced with 0.1 ml of virus containing solution. Virus was typically detected within ~15 seconds as observed by an elevation of the signal $\Delta\phi$ (in degrees on the y-axis) along the time plot (x-axis). The detection run was allowed to reach stabilization of the phase differential, typically after ~2 minutes. The virus containing solution can be removed and the run can be continued with 0.4 ml of PBS until stabilization. $\Delta\phi$ can either be measured at stabilization after agent injection or after removal of the agent and re-stabilization in buffer. A detailed description of the former process is given in the legend for FIG. 2.

2.5. Statistics

[0167] All phase differential mass shift ($\Delta\phi$) data points were generated in at least duplicate and sometimes up to five tests. Data is presented as average \pm standard errors (SE). The statistical difference between groups of average measurements of phase differential mass shifts $\Delta\phi$ were determined using the students t-test. $P < 0.05$ was considered to be statistically significant.

3. Results

[0168] 3.1. Initial testing of the SAW detector

[0169] The major objective of this study was to couple the characteristics of SAW with the selectivity of antibodies to detect viruses of high medical and bio-warfare importance. FIG. 1A depicts the overall schematic concept of our device. FIG. 1B shows the miniature size of the wafer sensors, i.e. approximately 15 by 20 mm, featuring 4 delay lines, of which one is used as the reference line, while the others are used as test lines. FIG. 1C shows the SAW detection board with the fluidic housing (containing the wafer) and the output interface device to a laptop computer. The sealed fluidic housing connected the IDTs to the electrical input/output system of the static cell; a power supply provided an input frequency of 325 MHz. The phase differential mass shift $\Delta\phi$ (expressed in degrees) was captured on the laptop computer using a custom LabVIEW program.

[0170] Viral detection was performed by immobilizing antibodies onto the sensor. The test delay lines were either directly coated with unlabeled antibodies (for SNV) or with NeutrAvidin Biotin Binding Protein followed by biotinylated antibodies (for Coxsackie virus B4). FIG. 2 represents a typical phase differential plot generated by exposing the sensor to 1.8×10^4 SNV particles per μl . The plot shows the PBS buffer calibrated surface at ~50 degrees, injection of the virus containing solution at ~280 seconds (measured on the x-axis), and maximal signal at ~420 seconds (~2 minutes after agent injection). Detection was evident at ~15 seconds after ad-

tion of the agent and resulted in an overall $\Delta\phi$ of ~5 degrees (measured on the y-axis). Thus, $\Delta\phi$ can be measured shortly after agent injection and the overall process can be performed within minutes. All subsequent data for the quantitative measurements of viral detection refer to the change in $\Delta\phi$ as described in FIG. 2.

3.2. Quantitative and Selective Detection of Coxsackie B4 and Sin Nombre Virus (SNV)

[0171] The SAW biosensor was used in a series of experiments for the detection of Coxsackie virus B4 particles (FIG. 3). Increasing concentrations of viral particles ranging from 9×10^5 to 3.6×10^6 viruses per μl were analyzed as described in FIG. 2. $\Delta\phi$ was recorded for each concentration and resulted in a dose-dependent increase with $\Delta\phi$ values ranging from 0.95 ± 0.54 to 6.99 ± 0.96 (FIG. 3; data set to the right). There was a linear relationship between viral load and $\Delta\phi$ for this range of viral particles with a correlation coefficient R^2 of 0.99. To determine the selectivity of the biosensor for its target in the presence of a confounding agent, the experiments were repeated using admixtures of Coxsackie B4 and HSV-1 viruses. HSV-1 was spiked into the Coxsackie virus preparations at equal final concentrations as for Coxsackie B4 and the previous experiments were repeated. HSV-1 did not affect the selectivity for Coxsackie B4, yielding similar $\Delta\phi$ values ranging from 1.09 ± 0.66 to 7.24 ± 0.36 . The relationship between viral load and $\Delta\phi$ remained linear with a correlation coefficient R^2 of 0.98. In these spiking experiments, where HSV-1 was used as a confounding agent, the $\Delta\phi$ for HSV-1 at a concentration of $3.6 \times 10^6/\mu\text{l}$ was 0.64 ± 0.33 , indicating that the biosensor did not detect HSV-1.

[0172] Next, we used the SAW biosensor to detect an agent of high medical concern, i.e. SNV, a member of the hantavirus genus of the family Bunyaviridae and an NIH-designated bioagent of category A (Bronze et al., 2002). Concentrations of 1.8×10^1 to 1.8×10^4 viral particles per μl resulted in $\Delta\phi$ of 0.63 ± 0.49 to 4.85 ± 0.77 (FIG. 3; data set to the left). The measured values displayed variation with some overlap as shown by their standard deviations. This can be attributed mainly to factors related to microfabrication reproducibility for the current sensor system. Our studies indicate that sensitivity is a function of the absolute thickness of the silicon dioxide waveguide. We have determined that thickness variations of 5% lead to a ~8% alterations in detection sensitivities (data not shown). However, our calculated waveguide variations for the current sensors are approximately 1-2%, which is unlikely to contribute to the observed experimental variation. In addition, variations in the lithographic process which guides the geometry of the IDTs on our sensors can influence their sensitivity. We are currently gathering data to quantify this potential problem and may change the process from contact to projection lithography. Nevertheless, the data means resulted in a linear relationship between viral load and $\Delta\phi$ for this range of viral particles with a correlation coefficient R^2 of 0.95. Similar to the experiments with Coxsackie virus, the selectivity of the SAW biosensor for SNV was not diminished by the presence of confounding HSV-1 at equal concentrations. The corresponding $\Delta\phi$ ranged from 0.78 ± 0.30 to 4.83 ± 1.36 and the relationship between viral load and $\Delta\phi$ remained linear with a correlation coefficient R^2 of 0.97. For this set of experiments, the biosensor was marginally sensitive to HSV-1 alone, resulting in $\Delta\phi$ values of 0.56 ± 0.27 and of 1.51 ± 0.40 for viral concentrations of $1.8 \times 10^3/\mu\text{l}$ and $1.8 \times 10^4/\mu\text{l}$, respectively.

[0173] Based on the lowest concentrations tested for both viral agents, which in both cases yielded $\Delta\phi$ above values obtained with HSV-1, the sensitivity for the antibody directed against SNV was approximately 50×10^4 -fold greater compared to the sensitivity of the antibody directed against Coxsackie B4 virus. The slopes for the detection of Coxsackie virus and SNV were markedly different (FIG. 3). This could be due to multiple factors including the deposition efficiency and corresponding site density of the capturing agents coated on the biosensor surface, in this case the anti-Coxsackie B4 and anti-SNV antibodies, which determines the number of binding sites available to specific viral ligands, in this case the Coxsackie B4 JVB epitope and the SNV-G1 glycoprotein. Similarly, differences in sensitivity can be explained by its dependence on the affinity between an antibody and its corresponding antigen. This leaves room for the development of better immunological tools with higher sensitivities. Accordingly, we are currently employing phage display to identify high affinity protein-peptide interactions to increase the sensitivity for viral particles.

3.3. Virus Detection in Complex Solutions

[0174] The SAW biosensor was applied to a real world scenario which could mimic the exposure of an urban population to a viral agent, such as for example through the water system. In these proof-of-principle experiments, SNV particles were spiked into 0.4 ml of either the sewage effluent water of the City of Albuquerque N. Mex., water taken from the Rio Grande River in Albuquerque, or distilled water or PBS as controls at a final concentration of 1.8×10^4 virus/ μ l. As shown in FIG. 4, all of the control solutions lacking viral particles showed similar background levels of $\Delta\phi$ in the order of 0.1. The SAW biosensor showed the highest sensitivity when the viral particles were spiked into distilled water, displaying a $\Delta\phi$ of 8.21 ± 0.11 degrees ($\sim 82 \times$ over background). The $\Delta\phi$ for virus spiked into PBS, Rio Grande River water, and sewage effluent water were similar, i.e. 4.85 ± 0.77 , 5.36 ± 0.93 , and 4.22 ± 0.84 , respectively, corresponding to $\sim 48 \times$, $54 \times$, and $42 \times$ fold differences over background, respectively. The $\Delta\phi$ values of all virus spiked solutions were significantly ($p < 0.05$) higher than their background solutions without virus, as determined by simple students t-test. In addition, these experiments in complex solutions collectively indicate a high re-usability of the sensor resulting in reproducible data. The data in FIG. 4 represent duplicate experiments using regenerated sensors after treatment with organic solvents, ultrasound, and UV-ozone. Nevertheless, multiple antibody re-coating and re-testing procedures led to $\Delta\phi$ measurements for the specific target within standard errors of $\sim 13\%$ of the mean.

4. Discussion

[0175] Antibody based detection by SAW has previously been reported for cellular microorganisms, such as bacteria. We recently reported on a 103 MHz operated SAW sensor to detect bacterial spores of *Bacillus thuringiensis*, a pathogen simulant for *Bacillus anthracis*, at or below inhalational infectious levels (Branch and Brozik, 2004). In that study we developed suitable chemistries to orient the antibodies on the sensor using protein G on two different waveguide materials, i.e. polyimide and polystyrene. We found that polyimide had a lower mass detection limit leading to highly selective bacterial detection as shown by the absence of binding to the

control agent *Bacillus subtilis*. Similarly, Berkenpas and colleagues recently described a SAW biosensor that was coated with a polyclonal antibody specific for the toxigenic *Escherichia coli* O157:H7 bacterium which causes hemorrhagic colitis and hemolytic uremic syndrome (Berkenpas et al., 2006). These authors reported $\Delta\phi$ responses of approximately 14 degrees representing a 7-fold difference over background control antibodies against trinitrophenyl (TNP) hapten.

[0176] In contrast, detection of viral and other agents by antibody coupled SAW is largely absent from the literature. In one of the few published studies Tamarin and colleagues developed a SAW sensor similar to the one presented here, and used it to study physical parameters of specific binding between antibodies and M13 bacteriophages (Tamarin et al., 2003). In addition, Tassew and Thompson reported on the detection of the human immunodeficiency virus (HIV) type 1 Tat protein using immobilized trans-activation-responsive RNA elements and various Tat peptide fragments (Tassew and Thompson, 2003). Thus, our study represents a contribution to the field of specific detection of viral agents by the SAW technology based on protein interactions (antibodies).

[0177] Collectively, our experiments using Coxsackie B4 and SNV indicate a high sensitivity and selectivity of the SAW detector for its targets. Importantly, selectivity was not compromised by the presence of confounding and related factors, such as other viruses, indicating the potential use of this device for the specific detection in complex solutions. In a previous study we have used quantitative (real time) reverse transcriptase polymerase chain reaction (RT-PCR) specific for the S segment of SNV RNA to determine viral copy number in bodily fluids, such as blood plasma and tracheal aspirates (Xiao et al., 2006). Assay sensitivity was ~ 5000 RNA copies (corresponding to viral particles) per ml, but the material to be tested had to be processed. Pre-processing of analyte is also necessary for other established techniques, including enzyme linked immunosorbent assay (ELISA) and surface plasmon resonance (SPR). Furthermore, SPR technology is still relatively costly and not amenable to a portable format. In contrast, our SAW platform allows detection of viral bioagents without pre-processing of the analyte, and can be developed into a portable field application. The SAW biosensor was able to detect at least 7000 SNV particles. Although the minimal infectious dose of SNV necessary to establish a successful human infection remains unknown, this number is substantially lower than the dosage found in hantavirus infected humans suffering from HCPS (Xiao et al., 2006).

[0178] An important and novel finding of this study is the detector's application to a real world scenario using water obtained from the sewage system and from a river of an urban area. This is a real world possibility for planned or accidental bioagent distribution and can lead to mass exposure within the population, which in turn can lead to an extensive health crisis (Bronze et al., 2002; www.cdc.gov). Naturally occurring water bodies, such as rivers are admittedly very complex solutions containing perhaps millions of different organic and inorganic molecules. It is thus noteworthy that our antibody-coated biosensor was able with high selectivity to detect the correct agent against this complex background. While the likelihood of detection in a large body of water could be increased by concentration strategies, such a procedure would compromise two important strengths and advantages of the current system, i.e. the hand-held, portable nature, and the absence of analyte pre-processing. In addition, it remains

to be shown whether a flow-through set-up that continuously monitors dilute samples vs. the static set-up reported here would increase the representative power of the analyzed sample. In a static setting changes in phase differential due to the added agent and buffer are accumulating, while in a flow-through setting the sensor would return back to the original phase differential of the carrier buffer, as the sample passes through the sensor. Comparisons between these approaches are currently under investigation in our laboratory.

[0179] Together, these data, and the results which are presented in Table 1, below, indicate that the sensor of the present invention may be used under field conditions and warrant further efforts into the development of inexpensive portable devices for field operation. This includes a hand-held battery operated and self-contained version of the present invention.

5. Further Examples

[0180] The following ligands (presented in Table 1) have been successfully adsorbed to the SAW biosensor and the corresponding analysis using the biosensor/SAW technology as described above have been successfully implemented. The analytes (Table 1) were detected selectively, partially in the presence of confounding agents (agents which are provided to make it more difficult to evidence binding and analysis by the present invention).

[0181] Importantly, the analytes were rapidly detected in real-time and in complete absence of any pre-processing steps.

Methods of Tethering Ligand to SAW Biosensor

[0182] The surface of the SAW biosensor can be prepared for ligand binding using the following different procedures/methods which are applicable to different ligands as listed in the Table. The sequential steps are generally described for each Method (also, see above), and the letters are listed in the third column (under "Adsorption Mode") for the correspond-

ing ligands. The following coats are deposited onto the lithium tantalate (LiTaO₃) surface.

Method A

- [0183] 1. A layer of silicon dioxide is etched/deposited onto the surface of the lithium tantalate surface. This is the waveguide layer and is ~5000 Å thick.
2. A thin layer of hexamethyldisilazane (HMDS) is deposited onto the surface of the silicon dioxide.
3. Ligand is deposited onto the HMDS layer non-covalently.

Method B

- [0184] 1. A layer of silicon dioxide is etched/deposited onto the surface of the lithium tantalate surface. This is the waveguide layer and is ~5000 Å thick.
2. A thin layer of hexamethyldisilazane (HMDS) is deposited onto the surface of the silicon dioxide.
3. A thin layer of 3-aminopropyltrimethoxy silane (amino group binding) or 3-cycloxypropyltriethoxy silane (carboxyl group binding) as a functional silane is deposited onto the HMDS layer.
4. Ligand is bound to the functional group (amine or carboxyl group) of the silane covalently.

Method C

- [0185] 1. A layer of silicon dioxide is etched/deposited onto the surface of the lithium tantalate surface. This is the waveguide layer and is ~5000 Å thick.
2. A thin layer of hexamethyldisilazane (HMDS) is deposited onto the surface of the silicon dioxide.
3. A thin layer of 3-aminopropyltrimethoxy silane (amino group binding) or 3-cycloxypropyltriethoxy silane (carboxyl group binding) as a functional silane is deposited onto the HMDS layer.
4. A thin layer of NeutrAvidin Binding Protein (0.25 mg/ml-range of 0.05 mg/ml to 1 mg/ml, about 0.1 mg/ml to about 0.75 mg/ml, about) in phosphate buffered saline is layered onto the layer of functional silane. A covalent linkage between the protein and functional silane results.
5. Ligand is bound to the functional group (amine or carboxyl group) of the silane covalently.

TABLE 1

Ligand	Analyte (recognized by ligand)	Adsorption Mode
Antibodies		
Anti-Coxsackie virus monoclonal antibody (mouse IgG2a)	Coxsackie virus B4 (JVB strain)	Methods A, B, Method C (if ligand biotinylated)
Anti-Sin Nombre virus (SNV) G1 glycoprotein (single chain Fv, scFv from phage display)	Sin Nombre virus (SNV)	Methods A, B, Method C (if ligand biotinylated)
Anti-Herpes Simplex virus 1 (HSV-1) antibody (polyclonal)	Herpes Simplex virus 1 (HSV-1)	Methods A, B, Method C (if ligand biotinylated)
Anti-avβ3 integrin antibody	avβ3 integrin	Methods A, B, Method C (if ligand biotinylated)
Anti-Interleukin-12 (IL-12) monoclonal antibody (mouse IgG1)	Human Interleukin-12 (IL-12)	Methods A, B, Method C (if ligand biotinylated)

TABLE 1-continued

Ligand	Analyte (recognized by ligand)	Adsorption Mode
Anti-Interleukin-6 (IL-6) polyclonal antibody (goat IgG)	Human Interleukin-6 (IL-6)	Methods A, B, Method C (if ligand biotinylated)
Peptides		
18 different peptides (cyclic, 9 amino acids; from phage display)	Sin Nombre virus (SNV)	Methods A, B, Method C (if ligand biotinylated)
18 different peptides (cyclic, 9 amino acids; from phage display)		
1) JC-1 = CLVRNLAWC SEQ ID No 1		
2) JC-2 = CSASTESLC SEQ ID No 2		
3) JC-3 = CQTTNWNTC SEQ ID No 3		
4) JC-4 = CKSFTTTRC SEQ ID No 4		
5) JC-5 = CAEPNSHRC SEQ ID No 5		
6) G1-0 = CKQTTNRNC SEQ ID No 6		
7) G1-1 = CQATTARNC SEQ ID No 7		
8) CSAGAPEFC SEQ ID No 8		
9) CTQSGLLSC SEQ ID No 9		
10) CKSFTTTRC SEQ ID No 10		
11) CTYPYPKFC SEQ ID No 11		
12) CKSTFSPNC SEQ ID No 12		
13) CTSAAVHMC SEQ ID 13		
14) CQPHLPWHC SEQ ID 14		
15) CQWPGQSGC SEQ ID No 15		
16) CNSSSPTAC SEQ ID No 16		
17) CHQLMQNLC SEQ ID No 17		
18) CIQSGLLS SEQ ID No 18		
10 different peptides (cyclic, 9 amino acids; from phage display)	Andes virus	Methods A, B, Method C (if ligand biotinylated)
1) C5-1 CPKLHPGGC SEQ ID No 19		
2) C5-2 CPMSQNPTC SEQ ID No 20		
3) C5-3 CTVGPTTRC SEQ ID No 21		
4) B9-1 CPSNVNNIC SEQ ID No 22		
5) B9-2 CMQSAAAHC SEQ ID No 23		
6) B9-3 CNSHSPVHC SEQ ID No 24		
7) B9-4 CKSLGSSQC SEQ ID No 25		
8) B9-5 CPAASHPRC SEQ ID No 26		
9) B9-6 CEKLHTASC SEQ ID No 27		
10) B9-7 CSLHSHKGC SEQ ID No 28		
1 peptide (linear, 16 amino acids; from phage display)	Dengue virus	Methods A, B, Method C (if ligand biotinylated)
DTRACDVIALLCHLNT SEQ ID No 29		
Nucleic Acids		
(a) SNV-N (nucleocapsin protein) Capture DNA	Sin Nombre virus (SNV) RNA	Method C
1) CCCTAGAGATGCTGCATTGGCACTAA SEQ ID No 30		
2) TTACAGGTTGATGAGTCAAAGTTAGT SEQ ID NO 31		
3) TTACAGGTTGATGAGTCAAAGTTAGTGATATTGAGGACC SEQ ID NO 32		
(b) SNV-M (glycoprotein) Capture DNA		
1) CCTGATCAAAAATGGACAAGGTTAATGAGAATAGCTGGGC SEQ ID No 33		
2) TTTTCATGCTCACATTATTCTACAGAAT SEQ ID No 34		
3) TTTTCATGCTCACATTATTCTACAGAATCAAAATTCAAAGT SEQ ID No 35		
Biotinylated BRCA1 capture DNA (single-stranded; 30 bases)	BRCA1 DNA (single-stranded; 60 bases)	Method C
5'-CCTGGATAATGGGTTTATGAAAAACACTTT SEQ ID No 36		

Physisorption = Direct adsorption on silicon dioxide

Silane = 3-aminopropyltrimethoxy silane

NAB = NeutrAvidin Binding Protein

6. Conclusions

[0186] Detection of biological agents and their products in the context of bio-warfare, human health and agricultural production are important tasks with a current sense of urgency. Applications include the detection of agents and

their products in the environment after planned or accidental distribution into the soil or water bodies, such as swimming pools, rivers, aquifers, and the sewage system, especially in highly urbanized areas. Another application is the detection of agents and markers thereof in human fluids and tissues for

the correct diagnosis and treatment stratification of patients. Towards this end, we have developed a SAW biosensor that is capable of rapidly detecting viral agents with high selectivity and sensitivity for at least two different targets, i.e. Coxsackie B4 virus and the category A bioagent SNV. Our detector combines the sensitivity of surface acoustics with the selectivity of antibody-antigen recognition and offers a highly versatile platform for the detection of other viral agents and their products. Further, the results obtained in this study emphasize the possibility for future, more refined developments and applications of portable SAW based technology in the fields of viral medicine and environmental surveillance.

REFERENCES

- [0187] Berkenpas, E., Millard, P., Pereira da Cunha, M., 2006. *Biosens. Bioelectron.* 21, 2255-62.
- [0188] Branch, D. W., Brozik, S. M., 2004. *Biosens. Bioelectron.* 19, 849-59.
- [0189] Bronze, M. S., Huycke, M. M., Machado, L. J., Voskuhl, G. W., Greenfield, R. A., 2002. *Am. J. Med. Sci.* 323, 316-25.
- [0190] Deisingh, A. K., Thompson, M., 2004. *Can. J. Microbiol.* 50, 69-77.
- [0191] Frydenberg, A., Starr, M., 2003. *Aust. Fam. Physician.* 32, 594-5.
- [0192] Hjelle, B., 2002. *Expert Rev. Vaccines.* 1, 373-84.
- [0193] Jay, M., Ascher, M. S., Chomel, B. B., Madon, M., Sesline, D., Enge, B. A., Hjelle, B., Ksiazek, T. G., Rollin, P. E., Kass, P. H., Reilly, K., 1997. *Emerg. Infect. Dis.* 3, 183-90.
- [0194] Martin, F., Newton, M. I., McHale, G., Melzak, K. A., Gizeli, E., 2004. *Biosens. Bioelectron.* 19, 627-32.
- [0195] Mertz, G. J., Hjelle, B., Crowley, M., Iwamoto, G., Tomicic, V., Vial, P. A., 2006. *Curr. Opin. Infect. Dis.* 19, 437-42.
- [0196] Moll, N., Pascal, E., Dinh, D. H., Pillot, J. P., Bennetau, B., Rebière, D., Moynet, D., Mas, Y., Mossalayi, D., Pistré, J., Déjous C., 2007. *Biosens. Bioelectron.* 22, 2145-50.
- [0197] Palacios, G., Oberste, M. S., 2005. *J. Neurovirol.* 11, 424-33.
- [0198] Tam, P. E., 2006. *Viral Immunol.* 19, 133-46.
- [0199] Tamarin, O., Comeau, S., Déjous, C., Moynet, D., Rebière, D., Bezian, J., Pistré, J., 2003. *Biosens. Bioelectron.* 18, 755-63.
- [0200] Tassew, N., Thompson, M., 2003. *Org. Biomol. Chem.* 1, 3268-70.
- [0201] Velappan, N., Martinez, J. S., Valero, R., Chasteen, L., Ponce, L., Bondu-Hawkins, V., Kelly, C., Pavlik, P., Hjelle, B., Bradbury, A. R., 2007. *J. Immunol. Methods.* 321, 60-9.
- [0202] Xiao, R., Yang, S., Koster, F., Ye, C., Stidley, C., Hjelle, B., 2006. *J. Infect. Dis.* 194, 1403-.

SEQUENCE LISTING

<160> NUMBER OF SEQ ID NOS: 36

<210> SEQ ID NO 1
 <211> LENGTH: 9
 <212> TYPE: PRT
 <213> ORGANISM: Artificial Sequence
 <220> FEATURE:
 <223> OTHER INFORMATION: Synthetic Peptide

<400> SEQUENCE: 1

Cys Leu Val Arg Asn Leu Ala Trp Cys
 1 5

<210> SEQ ID NO 2
 <211> LENGTH: 9
 <212> TYPE: PRT
 <213> ORGANISM: Artificial Sequence
 <220> FEATURE:
 <223> OTHER INFORMATION: Synthetic Peptide

<400> SEQUENCE: 2

Cys Ser Ala Ser Thr Glu Ser Leu Cys
 1 5

<210> SEQ ID NO 3
 <211> LENGTH: 9
 <212> TYPE: PRT
 <213> ORGANISM: Artificial Sequence
 <220> FEATURE:
 <223> OTHER INFORMATION: Synthetic Peptide

<400> SEQUENCE: 3

Cys Gln Thr Thr Asn Trp Asn Thr Cys

-continued

1 5

<210> SEQ ID NO 4
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic Peptide

<400> SEQUENCE: 4

Cys Lys Ser Phe Thr Thr Thr Arg Cys
1 5

<210> SEQ ID NO 5
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 5

Cys Ala Glu Pro Asn Ser His Arg Cys
1 5

<210> SEQ ID NO 6
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 6

Cys Lys Gln Thr Thr Asn Arg Asn Cys
1 5

<210> SEQ ID NO 7
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 7

Cys Gln Ala Thr Thr Ala Arg Asn Cys
1 5

<210> SEQ ID NO 8
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 8

Cys Ser Ala Gly Ala Pro Glu Phe Cys
1 5

<210> SEQ ID NO 9
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 9

-continued

Cys Thr Gln Ser Gly Leu Leu Ser Cys
1 5

<210> SEQ ID NO 10
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 10

Cys Lys Ser Phe Thr Thr Thr Arg Cys
1 5

<210> SEQ ID NO 11
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 11

Cys Thr Tyr Pro Tyr Pro Lys Phe Cys
1 5

<210> SEQ ID NO 12
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 12

Cys Lys Ser Thr Phe Ser Pro Asn Cys
1 5

<210> SEQ ID NO 13
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 13

Cys Thr Ser Ala Ala Val His Met Cys
1 5

<210> SEQ ID NO 14
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 14

Cys Gln Pro His Leu Pro Trp His Cys
1 5

<210> SEQ ID NO 15
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

-continued

<400> SEQUENCE: 15

Cys Gln Trp Pro Gly Gln Ser Gly Cys
1 5

<210> SEQ ID NO 16

<211> LENGTH: 9

<212> TYPE: PRT

<213> ORGANISM: Artificial Sequence

<220> FEATURE:

<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 16

Cys Asn Ser Ser Ser Pro Thr Ala Cys
1 5

<210> SEQ ID NO 17

<211> LENGTH: 9

<212> TYPE: PRT

<213> ORGANISM: Artificial Sequence

<220> FEATURE:

<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 17

Cys His Gln Leu Met Gln Asn Leu Cys
1 5

<210> SEQ ID NO 18

<211> LENGTH: 8

<212> TYPE: PRT

<213> ORGANISM: Artificial Sequence

<220> FEATURE:

<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 18

Cys Ile Gln Ser Gly Leu Leu Ser
1 5

<210> SEQ ID NO 19

<211> LENGTH: 9

<212> TYPE: PRT

<213> ORGANISM: Artificial Sequence

<220> FEATURE:

<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 19

Cys Pro Lys Leu His Pro Gly Gly Cys
1 5

<210> SEQ ID NO 20

<211> LENGTH: 9

<212> TYPE: PRT

<213> ORGANISM: Artificial Sequence

<220> FEATURE:

<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 20

Cys Pro Met Ser Gln Asn Pro Thr Cys
1 5

<210> SEQ ID NO 21

<211> LENGTH: 9

<212> TYPE: PRT

<213> ORGANISM: Artificial Sequence

-continued

<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 21

Cys Thr Val Gly Pro Thr Arg Ser Cys
1 5

<210> SEQ ID NO 22
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 22

Cys Pro Ser Asn Val Asn Asn Ile Cys
1 5

<210> SEQ ID NO 23
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 23

Cys Met Gln Ser Ala Ala Ala His Cys
1 5

<210> SEQ ID NO 24
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 24

Cys Asn Ser His Ser Pro Val His Cys
1 5

<210> SEQ ID NO 25
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 25

Cys Lys Ser Leu Gly Ser Ser Gln Cys
1 5

<210> SEQ ID NO 26
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 26

Cys Pro Ala Ala Ser His Pro Arg Cys
1 5

<210> SEQ ID NO 27
<211> LENGTH: 9

-continued

```

<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 27

Cys Glu Lys Leu His Thr Ala Ser Cys
1           5

<210> SEQ ID NO 28
<211> LENGTH: 9
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 28

Cys Ser Leu His Ser His Lys Gly Cys
1           5

<210> SEQ ID NO 29
<211> LENGTH: 16
<212> TYPE: PRT
<213> ORGANISM: Artificial Sequence
<220> FEATURE:
<223> OTHER INFORMATION: Synthetic peptide

<400> SEQUENCE: 29

Asp Thr Arg Ala Cys Asp Val Ile Ala Leu Leu Cys His Leu Asn Thr
1           5           10          15

<210> SEQ ID NO 30
<211> LENGTH: 27
<212> TYPE: DNA
<213> ORGANISM: Sin Nombre hantavirus

<400> SEQUENCE: 30

ccctagagat gctgcattgg caactaa                27

<210> SEQ ID NO 31
<211> LENGTH: 27
<212> TYPE: DNA
<213> ORGANISM: Sin Nombre hantavirus

<400> SEQUENCE: 31

ttacaggttg atgagtcaaa agttagt                27

<210> SEQ ID NO 32
<211> LENGTH: 40
<212> TYPE: DNA
<213> ORGANISM: Sin Nombre hantavirus

<400> SEQUENCE: 32

ttacaggttg atgagtcaaa agttagtgat attgaggacc    40

<210> SEQ ID NO 33
<211> LENGTH: 40
<212> TYPE: DNA
<213> ORGANISM: Sin Nombre hantavirus

<400> SEQUENCE: 33

cctgatcaaa atggacaagg ttaaatgaga atagctgggc    40

```

-continued

<210> SEQ ID NO 34
 <211> LENGTH: 27
 <212> TYPE: DNA
 <213> ORGANISM: Sin Nombre hantavirus

<400> SEQUENCE: 34

tttcatgctc acattattct acagaat

27

<210> SEQ ID NO 35
 <211> LENGTH: 40
 <212> TYPE: DNA
 <213> ORGANISM: Sin Nombre hantavirus

<400> SEQUENCE: 35

tttcatgctc acattattct acagaatcaa aattcaaagt

40

<210> SEQ ID NO 36
 <211> LENGTH: 30
 <212> TYPE: DNA
 <213> ORGANISM: Sin Nombre hantavirus

<400> SEQUENCE: 36

cctggataat gggtttatga aaaacacttt

30

1. A ligand based biosensor comprising a biological ligand complexed, directly or indirectly to a surface of a piezoelectric material, said piezoelectric material being operably connected to an electric circuit capable of producing surface acoustic waves on the surface of the piezoelectric material to detect the binding of a bioagent or analyte to said ligand based biosensor.

2. The biosensor according to claim 1 wherein said biological ligand is a polypeptide, a DNA or RNA molecule, a lipid or carbohydrate.

3. The biosensor according to claim 1 wherein said piezoelectric material is lithium tantalate (LiTaO_3).

4. The biosensor according to claim 1 wherein said ligand is an antibody.

5. The biosensor according to claim 4 wherein said antibody is a monoclonal antibody.

6. The biosensor according to claim 4 wherein said antibody is a polyclonal antibody.

7. The biosensor according to claim 1 wherein said ligand is a polypeptide.

8. The biosensor according to claim 1 wherein said ligand is a polynucleotide.

9. The biosensor according to claim 8 wherein said ligand is a DNA molecule.

10. The biosensor according to claim 8 wherein said ligand is a RNA molecule.

11. The biosensor according to claim 1 wherein said ligand is a lipid or a carbohydrate.

12. The biosensor according to claim 1 wherein said ligand is covalently linked to said piezoelectric material.

13. The biosensor according to claim 1 wherein said ligand is non-covalently linked to said piezoelectric material.

14. The biosensor according to claim 1 wherein said bioagent or analyte is selected from the group consisting of viruses and their extracts, prions and their extracts, eucaryotic cells, fragments and extracts, prokaryotic cells, fragments

and extracts, prokaryotic spores, fragments and extracts, protein and peptide markers, serum proteins, isolated proteins, synthetic chemicals, viral membranes, eukaryotic membranes, eukaryotic cell parts, including mitochondria and other organelles, prokaryotic membranes, DNA viruses (single and double stranded DNA viruses), RNA viruses (single and double stranded RNA viruses), point mutations (any organism), single nucleotide polymorphism (any organism), mRNA's, rINAs or a micro RNA.

15. The biosensor according to claim 14 wherein said bioagent is a single or double stranded DNA virus.

16. The biosensor according to claim 14 wherein said bioagent is a single or double stranded DNA molecule.

17. A method of identifying the presence of a bioagent in a sample with the ligand based biosensor according to claim 1, said method comprising establishing a surface acoustic wave on the surface of said piezoelectric material comprising a ligand which binds to said bioagent, exposing said surface to a sample suspected of containing said bioagent and then determining whether the sample contains a suspect bioactive agent if the wave at the surface of said piezoelectric material evidences a change consisting with the binding of said bioactive agent.

18. The method according to claim 17 wherein said sample is an environmental or human sample.

19. The method according to claim 18 wherein said human sample is blood, serum, plasma, urine, sputum or fecal matter.

20. The method according to claim 17 wherein said surface acoustic wave has a specific resonance frequency ranging from 80 to 400 Mhz.

21. The method according to claim 17 wherein said surface acoustic wave has a specific resonance frequency of about 325 Mhz.

22. The method according to claim 17 wherein said bioagent or analyte is selected from the group consisting of viruses

and their extracts, prions and their extracts, eucaryotic cells, fragments and extracts, prokaryotic cells, fragments and extracts, prokaryotic spores, fragments and extracts, protein and peptide markers, serum proteins, isolated proteins, synthetic chemicals, viral membranes, eukaryotic membranes, eukaryotic cell parts, including mitochondria and other organelles, prokaryotic membranes, DNA viruses (single and double stranded DNA viruses), RNA viruses (single and double stranded RNA viruses), point mutations (any organism), single nucleotide polymorphism (any organism), mRNA's, rTNA's or a micro RNA.

23. A ligand based biosensor comprising a lithium tantalate material and at least one biological ligand complexed, directly or indirectly to the surface of said material, said material further comprising at least two delay lines wherein at least one of said delay lines is a reference delay line which produces a surface acoustic wave at the surface of the biosensor and at least one of said delay lines is a test delay line which measures the frequency of the acoustic wave at the surface of the biosensor to detect the binding of a bioagent or analyte to said ligand.

24-46. (canceled)

47. A biosensor comprising: a housing; at least one first transducer disposed in said housing for generating surface acoustic waves in a fluid disposed in said housing in contact with said first transducer; a plurality of second transducers disposed in said housing for detecting said surface acoustic waves, said fluid also being disposed in contact with said second transducers; a biological ligand complexed, directly or indirectly at least to a surface disposed in said housing so as to be in contact with said fluid; an electric circuit operatively linked to said first transducer and said second transducers for operating said first transducer to generate said surface

acoustic waves at a predetermined frequency and for monitoring signals from said second transducers to detect changes in said surface acoustic waves owing to a binding of a bioagent or analyte to said ligand, thereby detecting the presence of said bioagent or analyte.

48. The biosensor defined in claim **47** wherein said first transducer and said second transducers are inter-digital electrodes disposed on said surface in said housing, at least said second transducers being connected to respective output delay lines.

49. The biosensor defined in claim **47** wherein said surface is a surface of a substrate made at least in part of piezoelectric material.

50. A method of identifying a bioagent, comprising: providing a housing having a surface to which a ligand is directly or indirectly complexed; generating a surface acoustic wave in a fluid disposed in said housing in contact with said surface; exposing the fluid in said housing to a sample containing a bioagent which binds to said ligand; automatically monitoring the surface acoustic wave after the exposing of said fluid to said sample; and detecting a change in said surface acoustic wave thereby determining a binding of said bioagent to said ligand and according the presence of said bioagent in said sample.

51. The method defined in claim **50** wherein the generating of said surface acoustic wave comprises transmitting a signal to a first inter-digital electrode disposed in said housing in contact with said fluid.

52. The method defined in claim **50** wherein the monitoring of the surface acoustic wave comprises operating a plurality of inter-digital electrodes in contact with said fluid.

* * * * *

专利名称(译)	使用剪切水平表面声波生物传感器检测生物试剂		
公开(公告)号	US20110053139A1	公开(公告)日	2011-03-03
申请号	US12/069284	申请日	2008-02-08
[标]申请(专利权)人(译)	LARSON RICHARD小号 HJELLE BRIAN HALL PAM R BROWN DAVID C BISOFFI MARCO BROZIK SUSAN中号 BRANCH DARREN W EDWARDS THAYNE大号 惠勒DAVID		
申请(专利权)人(译)	LARSON RICHARD小号 HJELLE BRIAN HALL PAM R BROWN DAVID C BISOFFI MARCO BROZIK SUSAN中号 BRANCH DARREN W EDWARDS THAYNE大号 惠勒DAVID		
当前申请(专利权)人(译)	LARSON RICHARD小号 HJELLE BRIAN HALL PAM R BROWN DAVID C BISOFFI MARCO BROZIK SUSAN中号 BRANCH DARREN W EDWARDS THAYNE大号 惠勒DAVID		
[标]发明人	LARSON RICHARD S HJELLE BRIAN HALL PAM R BROWN DAVID C BISOFFI MARCO BROZIK SUSAN M BRANCH DARREN W EDWARDS THAYNE L WHEELER DAVID		
发明人	LARSON, RICHARD S. HJELLE, BRIAN HALL, PAM R. BROWN, DAVID C. BISOFFI, MARCO BROZIK, SUSAN M. BRANCH, DARREN W. EDWARDS, THAYNE L. WHEELER, DAVID		

IPC分类号	C12Q1/70 G01N33/53 C12M1/34
CPC分类号	C12Q1/6825 G01N33/54373 G01N29/032 G01N33/553 G01N2291/0422
优先权	61/009656 2007-12-31 US 60/900416 2007-02-09 US 60/926827 2007-04-30 US
其他公开文献	US8709791
外部链接	Espacenet USPTO

摘要(译)

病毒和其他生物制剂具有很高的医学和生物防御性，并且在远低于引起健康危害所必需的阈值的浓度下进行检测仍然是敏感性，特异性和选择性方面的挑战。理想情况下，用于准确和实时检测病毒剂和其他生物剂的测定法不需要对分析物进行任何预处理，这将使它们适用于例如体液（血液，痰液）和人造以及自然发生的体液。水体（池塘，河流）。我们在此描述了一种稳健的生物传感器，其结合了在325MHz频率下产生的表面声波（SAW）的灵敏度与由抗体和其他配体提供的用于检测病毒剂的特异性。在优选的实施案中，使用具有三个测试和一个参考延迟线的二氧化硅波导传感器平台的基于钽酸锂的SAW换能器来吸附针对的抗体。柯萨奇病毒B4或负链A类生物制剂Sin Nombre病毒（SNV），汉坦病毒属，布尼亚病毒科，负链RNA病毒的成员。对于两种病毒，增加浓度的病毒颗粒的快速检测（在几秒内）在线性范围内是线性的，尽管传感器对于SNV的检测灵敏度大约高 50×10^4 倍。对于这两种病原体，传感器对其靶标的选择性不会因混杂的1型单纯疱疹病毒的存在而受到影响。

生物传感器能够以低于通常在患有汉坦病毒心肺综合征的人类患者中发现的病毒载量的剂量检测SNV。（HCPS）。此外，在原理验证现实世界应用中，SAW生物传感器能够选择性地检测复杂溶液中的SNV试剂，例如天然存在的水体（河流，污水流出物），而无需分析物预处理。

